

System Check_2450MHz

DUT: D2450V2 - SN736

Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1

Medium: HSL_2450_220829 Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.82$ S/m; $\epsilon_r = 38.4$


Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7692; ConvF(8.41, 8.41, 8.41); Calibrated: 2021-11-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2021-11-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.0.2.83
- UID: , 0--

Pin=50mW/Area Scan (40.0 mm x 96.0 mm): Measurement Grid: 10.0 mm x 12.0 mm
SAR(1g) = 2.36 W/kg; SAR (10g) = 1.13 W/kg;

Pin=50mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5mm
Power Drift = -0.01 dB
SAR (1g) = 2.44 W/kg; SAR (8g) = 1.28 W/kg; SAR (10g) = 1.17 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 80.6 %

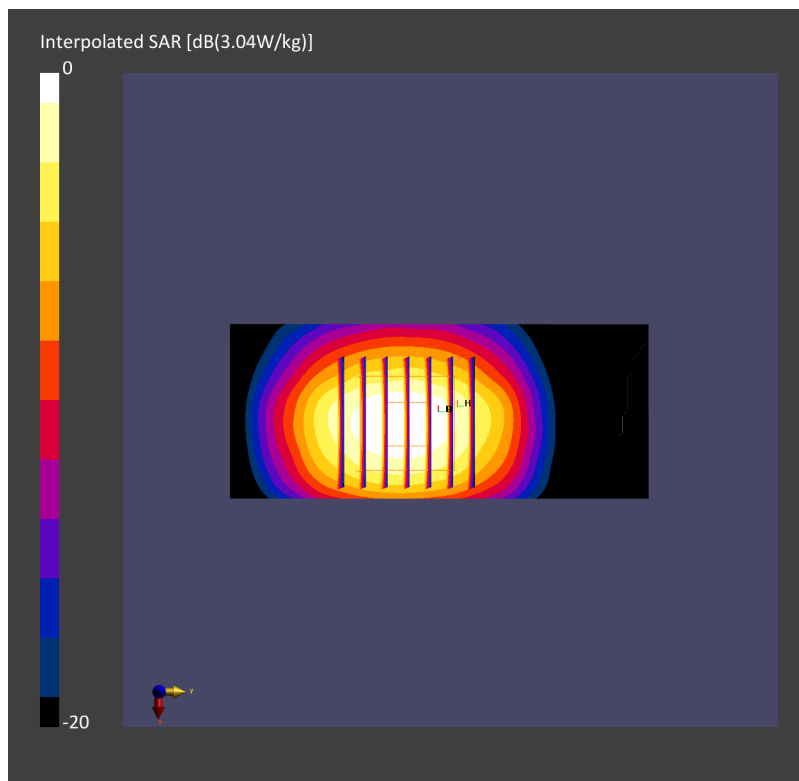

System Check_5250MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5250.0 MHz; Duty Cycle: 1:1

Medium: HSL_5G_220829 Medium parameters used: $f= 5250.0$ MHz; $\sigma= 4.67$ S/m; $\epsilon_r = 35.6$


Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7692; ConvF(5.45, 5.45, 5.45); Calibrated: 2021-11-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2021-11-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.0.2.83
- UID: , 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR(1g) = 3.45 W/kg; SAR (10g) = 1.02 W/kg;

Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4mm
Power Drift = -0.01 dB
SAR (1g) = 3.62 W/kg; SAR (8g) = 1.23 W/kg; SAR (10g) = 1.05 W/kg
Smallest distance from peaks to all points 3 dB below = 7.5 mm
Ratio of SAR at M2 to SAR at M1 = 65.4 %

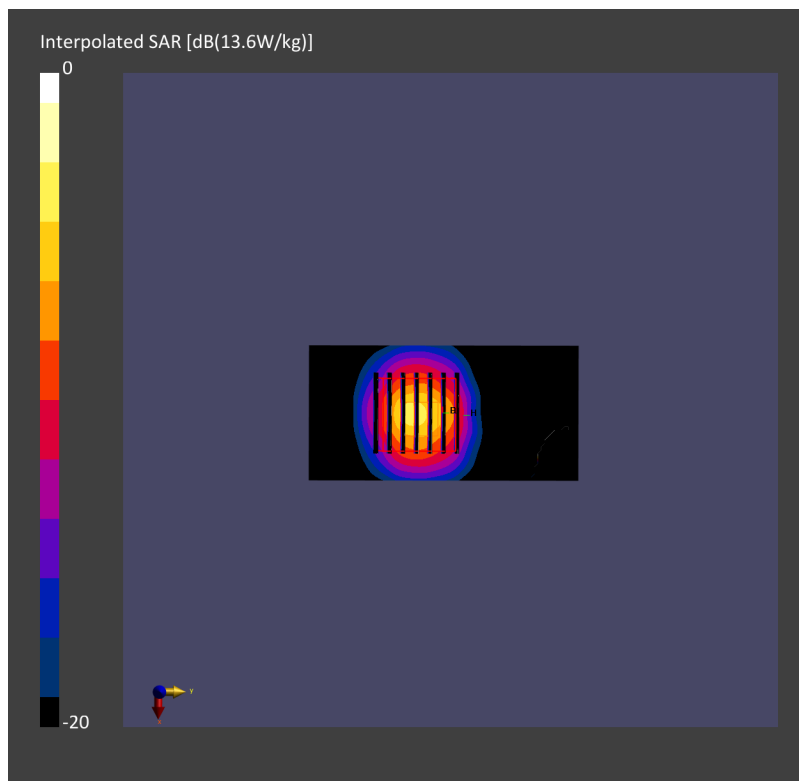

System Check_5600MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5600.0 MHz; Duty Cycle: 1:1

Medium: HSL_5G_220829 Medium parameters used: $f= 5600.0$ MHz; $\sigma= 5.06$ S/m; $\epsilon_r = 35.0$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7692; ConvF(4.75, 4.75, 4.75); Calibrated: 2021-11-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2021-11-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.0.2.83
- UID: , 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR(1g) = 3.72 W/kg; SAR (10g) = 1.07 W/kg;


Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4mm

Power Drift = -0.01 dB

SAR (1g) = 3.97 W/kg; SAR (8g) = 1.32 W/kg; SAR (10g) = 1.13 W/kg

Smallest distance from peaks to all points 3 dB below = 7.5 mm

Ratio of SAR at M2 to SAR at M1 = 62.5 %

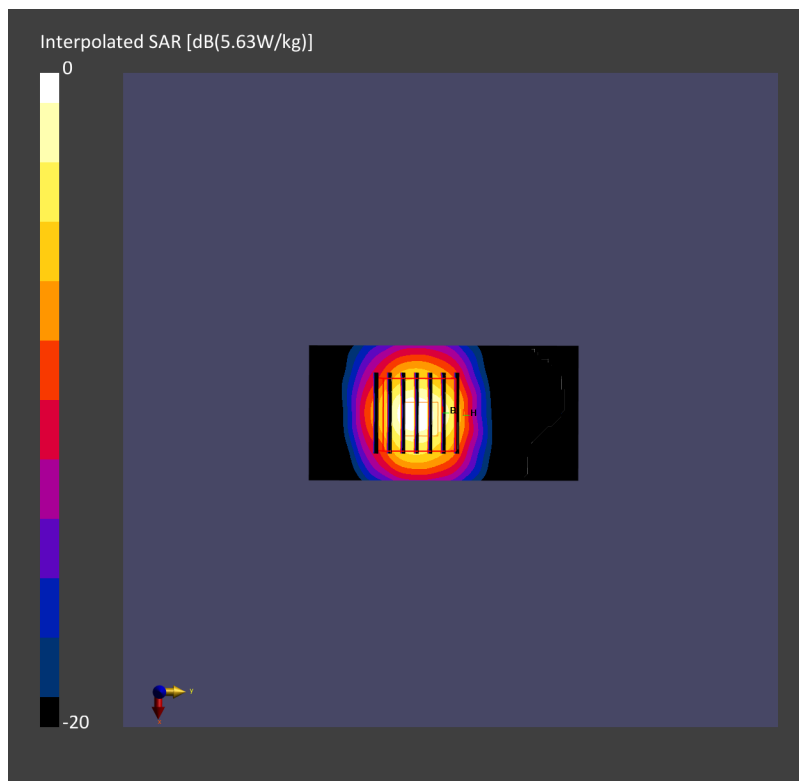

System Check_5750MHz

DUT: D5GHzV2 - SN1171

Communication System: CW; Frequency: 5750.0 MHz; Duty Cycle: 1:1
Medium: HSL_5G_220829 Medium parameters used: $f= 5750.0$ MHz; $\sigma= 5.25$ S/m; $\epsilon_r = 34.7$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7692; ConvF(5.0, 5.0, 5.0); Calibrated: 2021-11-03
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1694; Calibrated: 2021-11-03
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2156; Section: Flat
- Measurement Software: 16.0.2.83
- UID: , 0--

Pin=50mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR(1g) = 3.49 W/kg; SAR (10g) = 1.01 W/kg;

Pin=50mW/Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4mm
Power Drift = -0.00 dB
SAR (1g) = 3.70 W/kg; SAR (8g) = 1.23 W/kg; SAR (10g) = 1.06 W/kg
Smallest distance from peaks to all points 3 dB below = 7.4 mm
Ratio of SAR at M2 to SAR at M1 = 61.1 %

