

Test Laboratory: Compliance Certification Services

System Performance Check - D1450V2

DUT: Dipole; Type: D1450V2; Serial: 1020

Communication System: System Check Signal - CW; Frequency: 1450 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 1450$ MHz; $\sigma = 1.36$ mho/m; $\epsilon_r = 52.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Room Ambient Temperature: 25.0 deg. C; Liquid Temperature: 24.0 deg. C

DASY4 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Probe: EX3DV3 - SN3531; ConvF(9.33, 9.33, 9.33); Calibrated: 4/23/2008
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 11/16/2007
- Phantom: Flat Phantom ELI4.0; Type: QDOVA001BA; Serial: SN:XXXX
- Measurement SW: DASY4, V4.7 Build 71; Postprocessing SW: SEMCAD, V1.8 Build 184

d=10mm; Pin=250mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 8.50 mW/g


d=10mm; Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm

Reference Value = 84.2 V/m; Power Drift = -0.151 dB

Peak SAR (extrapolated) = 12.3 W/kg

SAR(1 g) = 7.16 mW/g; SAR(10 g) = 4.02 mW/g

Maximum value of SAR (measured) = 9.34 mW/g

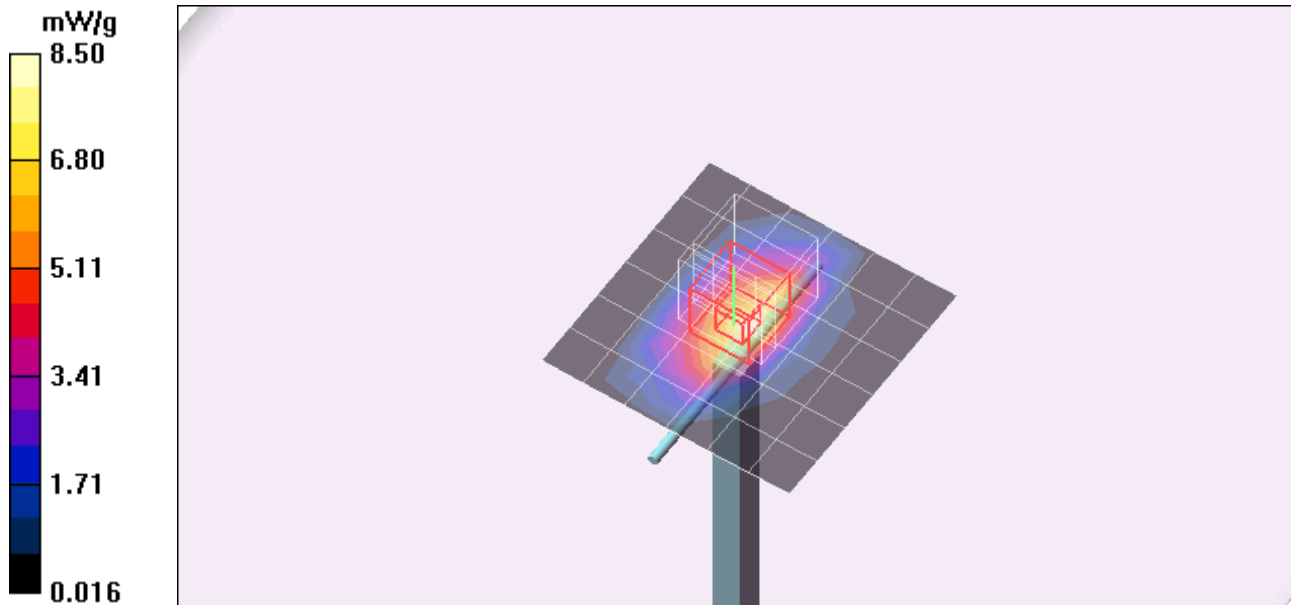

Test Laboratory: Compliance Certification Services

System Performance Check - D1450V2

DUT: Dipole; Type: D1450V2; Serial: 1020

Communication System: System Check Signal - CW; Frequency: 1450 MHz;Duty Cycle: 1:1

d=10mm; Pin=250mW/Z Scan (1x1x34): Measurement grid: dx=20mm, dy=20mm, dz=3mm
Maximum value of SAR (measured) = 9.01 mW/g

