

APPENDIX

11. Photographs of Test Setup

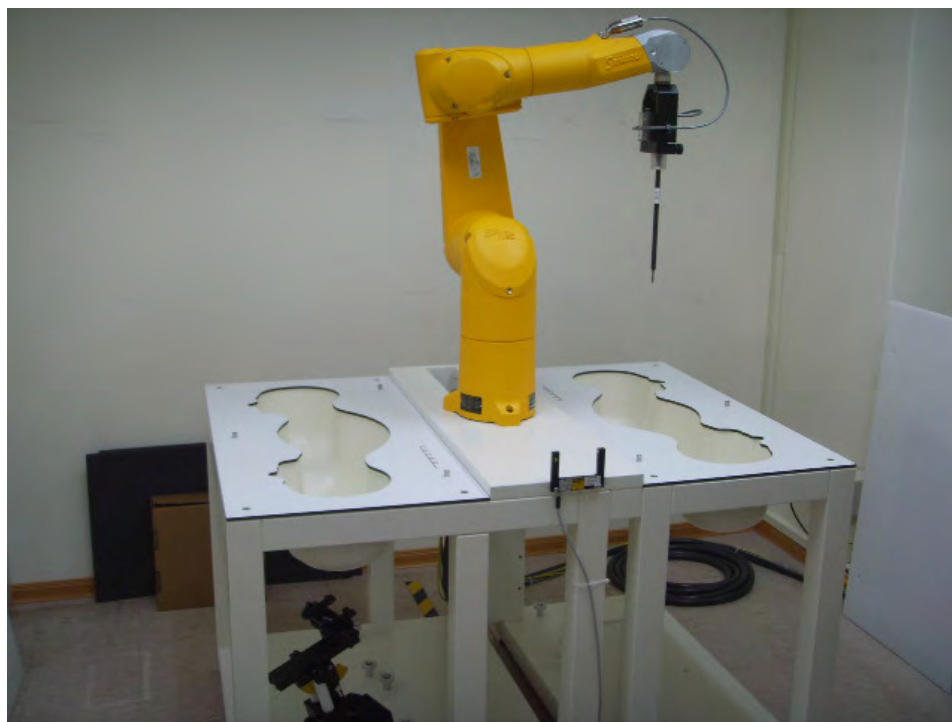


Fig.1 Photograph of the SAR measurement system

Photograph of the Tissue Simulant Fluid Liquid Depth

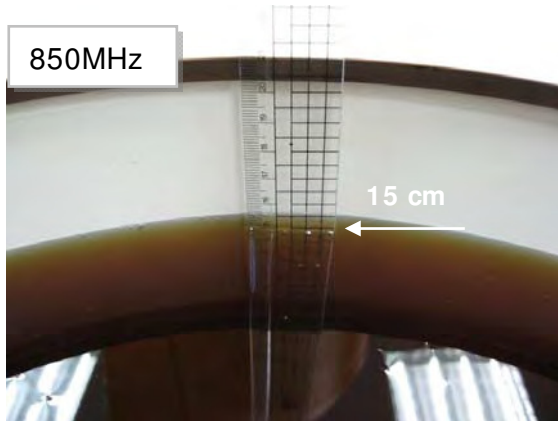


Fig.2.1

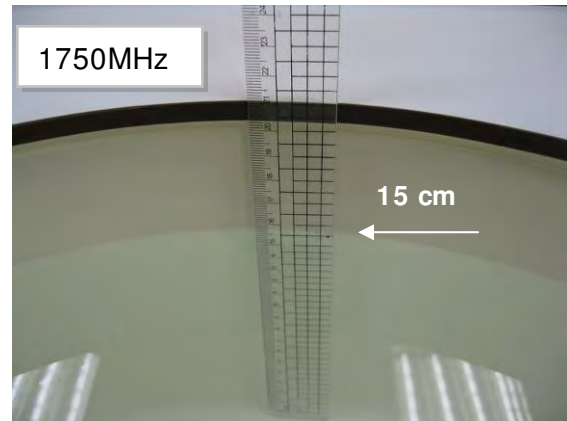


Fig.2.2

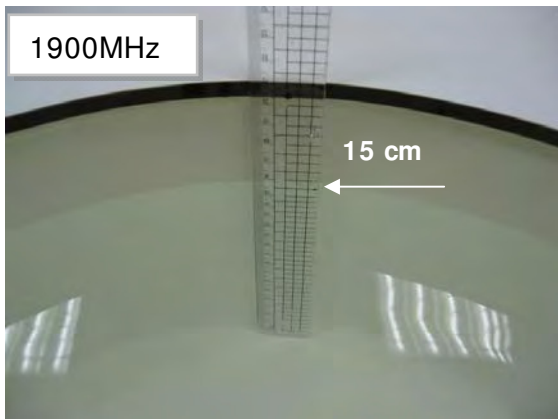


Fig.2.3

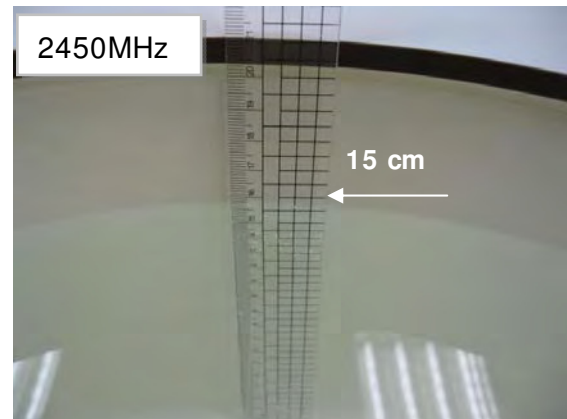


Fig.2.4

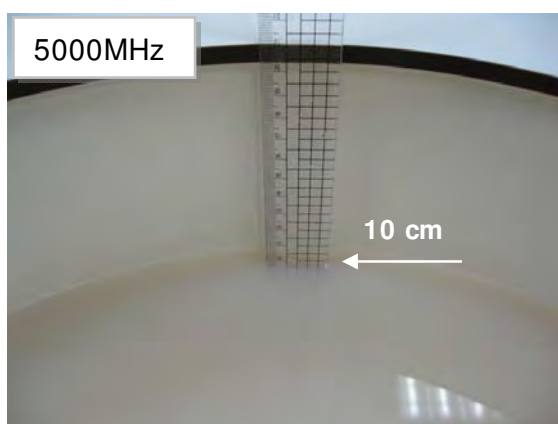


Fig.2.5

Body - distance between flat phantom and EUT is 0 mm

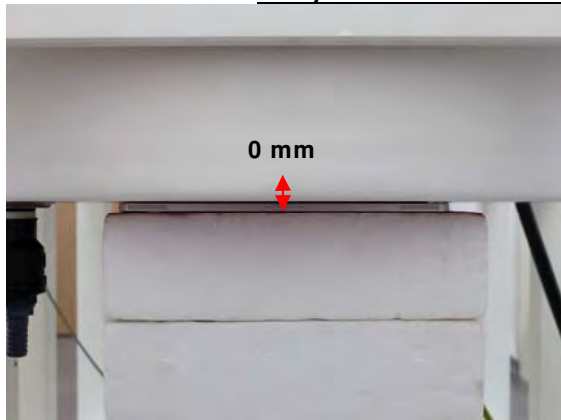


Fig.3 EUT Back side to flat phantom


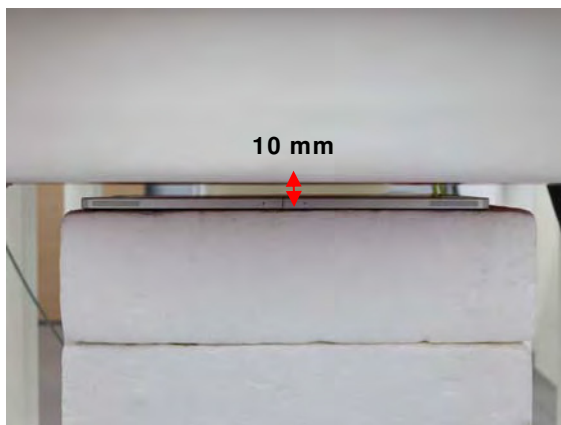


Fig.4 EUT Back side (10mm) to flat phantom



Fig.5 EUT Bottom side to flat phantom

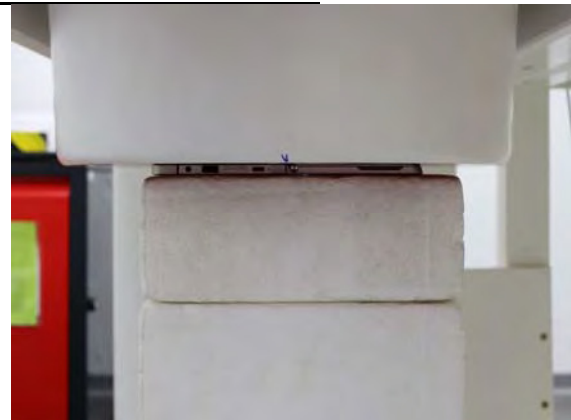

Body - distance between flat phantom and EUT is 0 mm

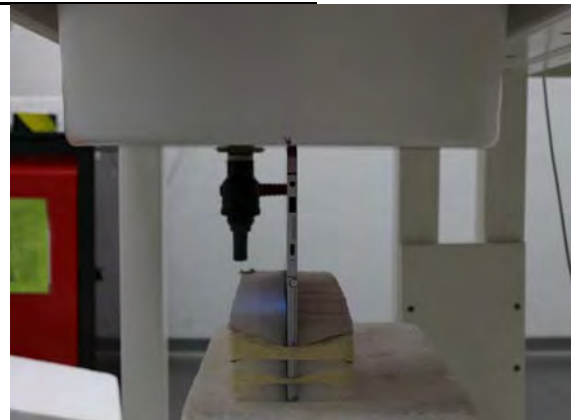
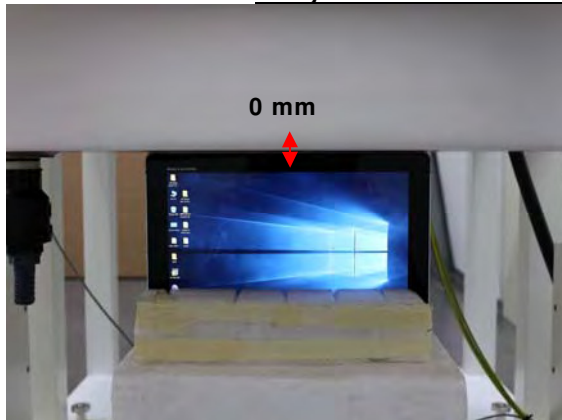


Fig.6 EUT Top side to flat phantom

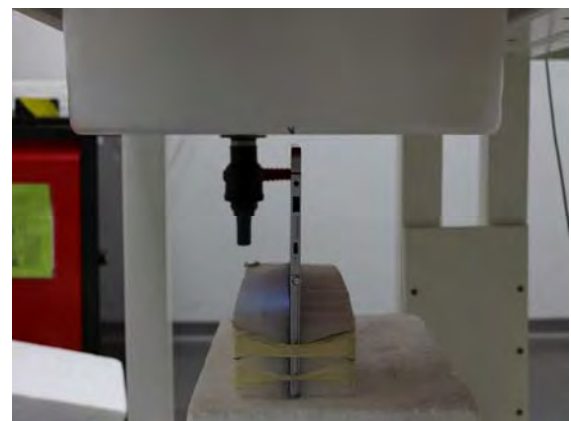
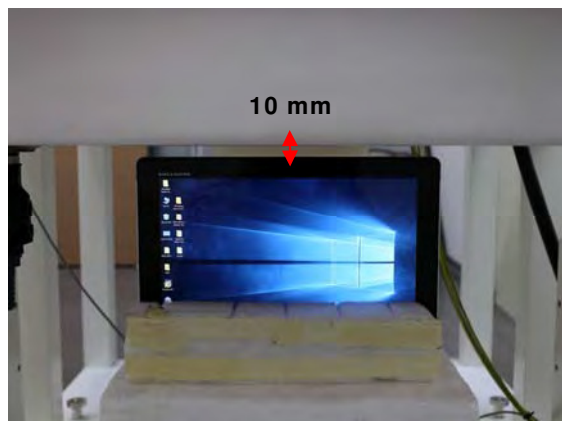


Fig.7 EUT Top side (10mm) to flat phantom

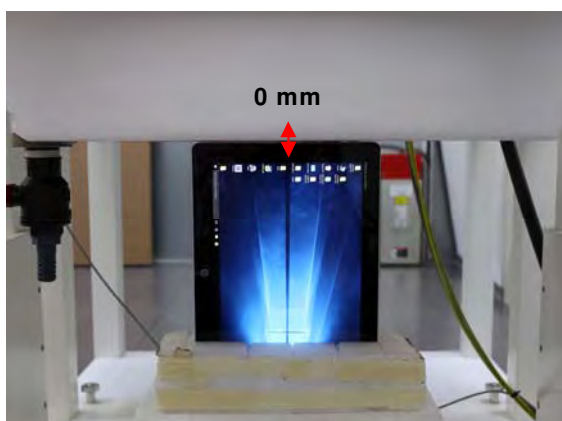


Fig.8 EUT Left side to flat phantom

Body - distance between flat phantom and EUT is 0 mm

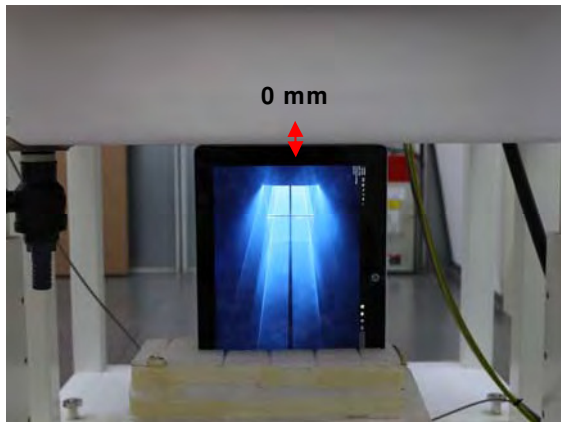


Fig.9 EUT Right side to flat phantom

12. Photographs of the EUT



Fig.10 Front view of EUT



Fig.11 Back view of EUT

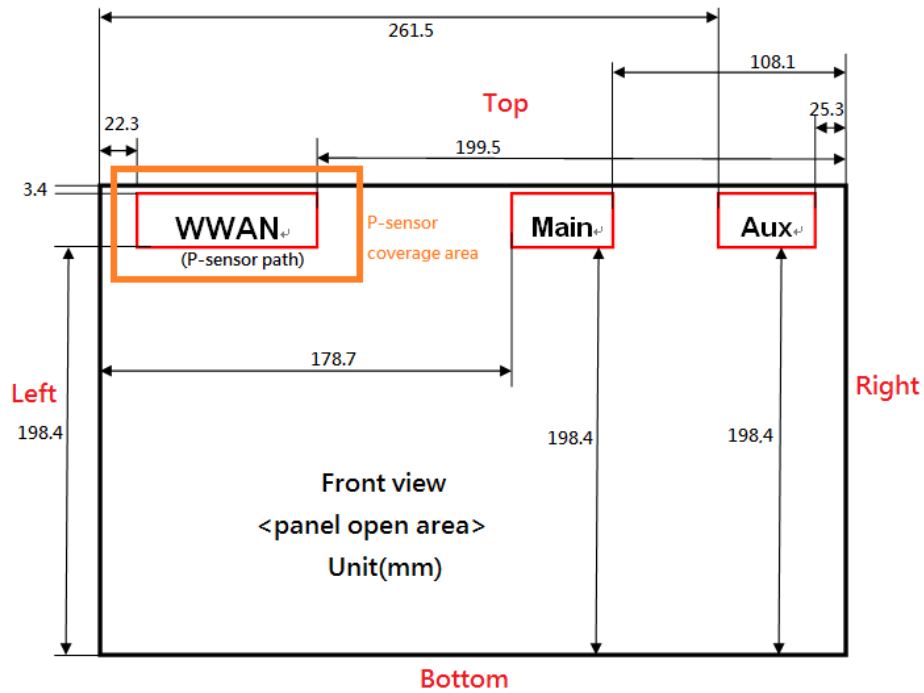


Fig.12 Antenna position of EUT (Front view)

- End of Report -