

**APPENDIX B: SAR DIPOLE VERIFICATION PLOTS**

# ELEMENT

**DUT: Dipole 750.0 MHz; Type: D750V3 - SN1034**

Communication System: UID: 0, CW; Frequency: 750.0 MHz

Medium: 750 Head; Medium parameters used:

f = 750.0 MHz; cond = 0.917 S/m; perm = 41.2; density = 1000 kg/m<sup>3</sup>

Phantom Section: Flat; Space: 15 mm

Test Date: 06/12/2023; Ambient Temp: 21.0°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7421; ConvF:(9.33,9.33,9.33); Calibrated: 2023-03-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn604; Calibrated: 2023-03-15

Phantom: Twin-SAM V8.0; Serial: 2070

Measurement SW: DASY Module SAR V16.2.0.1425

## 750 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.66 W/kg

**SAR(1 g) = 1.71 W/kg; SAR(10 g) = 1.13 W/kg**

Deviation (1 g) = -1.04%; Deviation (10 g) = 0.71%

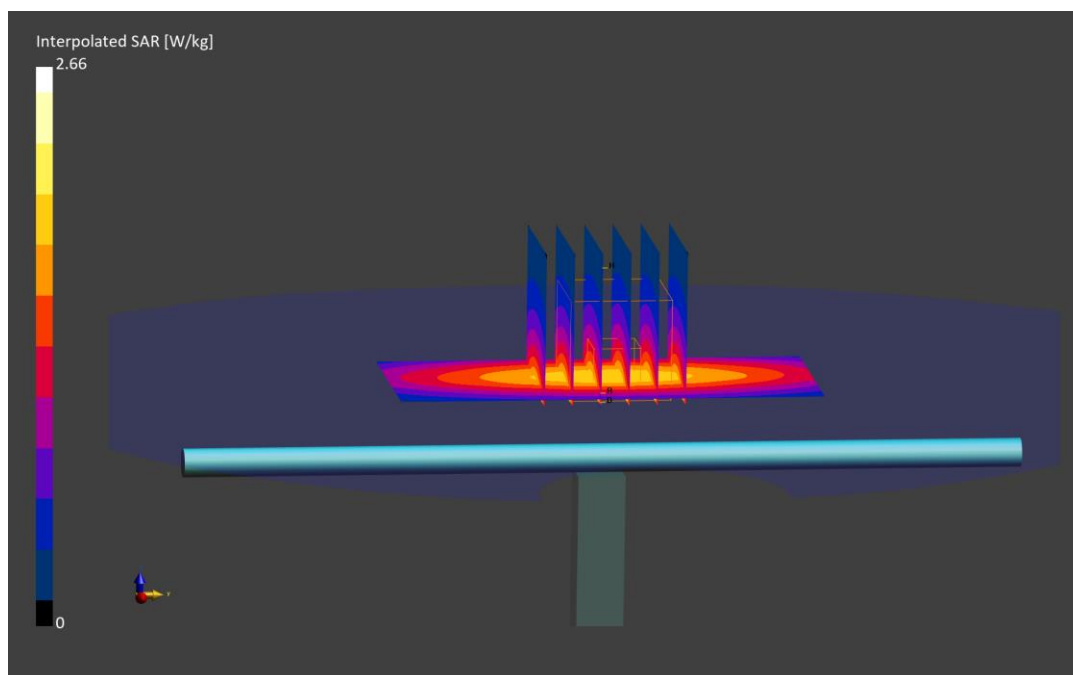

# ELEMENT

**DUT: Dipole 750.0 MHz; Type: D750V3 - SN1034**

Communication System: UID: 0, CW; Frequency: 750.0 MHz  
Medium: 750 Head; Medium parameters used:  
f = 750.0 MHz; cond = 0.874 S/m; perm = 40.3; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 06/14/2023; Ambient Temp: 22.0°C; Tissue Temp: 22.1°C

Probe: EX3DV4 - SN7421; ConvF:(9.33,9.33,9.33); Calibrated: 2023-03-16  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn604; Calibrated: 2023-03-15  
Phantom: Twin-SAM V8.0; Serial: 2070  
Measurement SW: DASY Module SAR V16.2.0.1425

## 750 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.50 W/kg

**SAR(1 g) = 1.63 W/kg; SAR(10 g) = 1.09 W/kg**

Deviation (1 g) = -5.67%; Deviation (10 g) = -2.85%

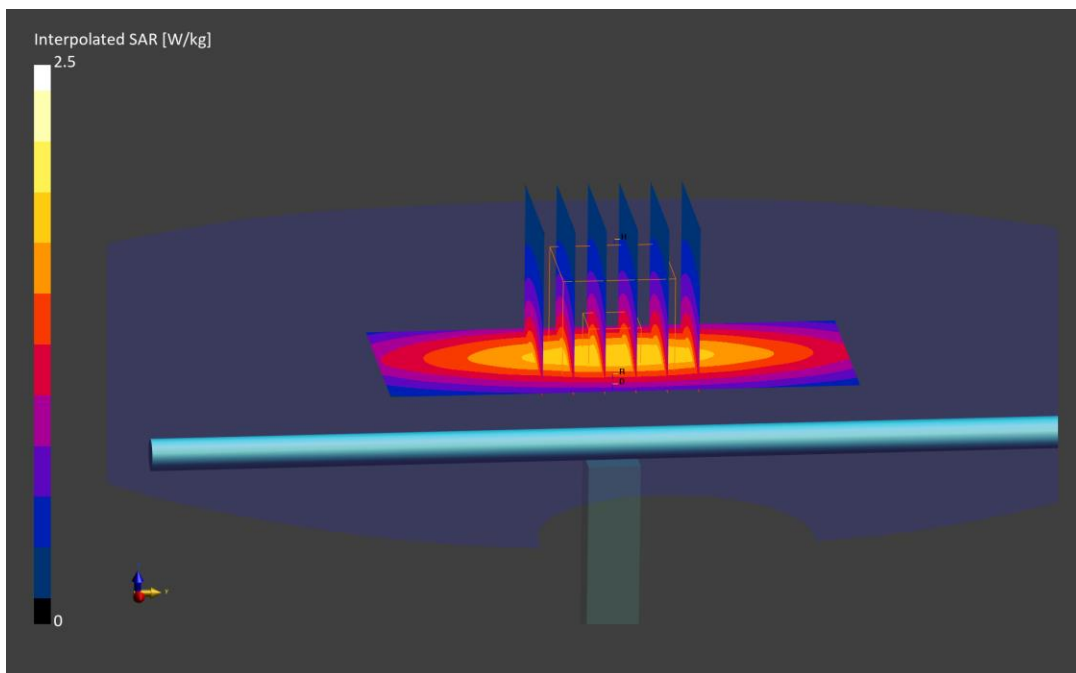

# ELEMENT

**DUT: Dipole 750.0 MHz; Type: D750V3 - SN1097**

Communication System: UID: 0, CW; Frequency: 750.0 MHz  
Medium: 750 Head; Medium parameters used:  
f = 750.0 MHz; cond = 0.870 S/m; perm = 41.0; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 06/21/2023; Ambient Temp: 21.4°C; Tissue Temp: 23.0°C

Probe: EX3DV4 - SN7421; ConvF:(9.33,9.33,9.33); Calibrated: 2023-03-16  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn604; Calibrated: 2023-03-15  
Phantom: Twin-SAM V8.0; Serial: 2070  
Measurement SW: DASY Module SAR V16.2.0.1425

## 750 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.60 W/kg

**SAR(1 g) = 1.68 W/kg; SAR(10 g) = 1.11 W/kg**

Deviation (1 g) = 2.31%; Deviation (10 g) = 3.93%;

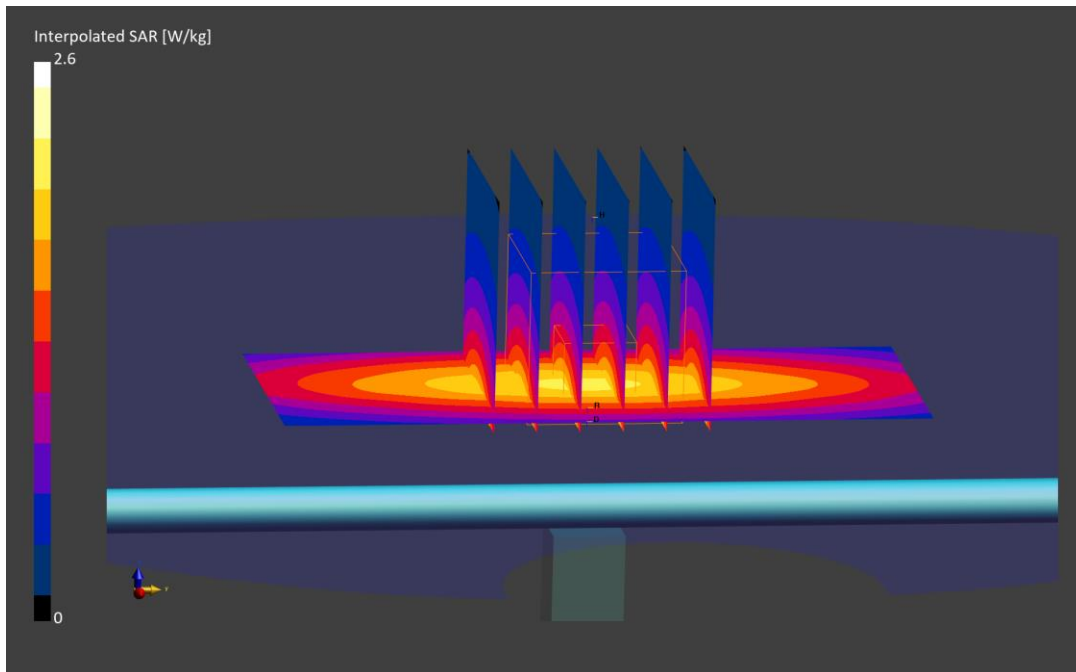

# ELEMENT

**DUT: Dipole 835.0 MHz; Type: D835V2 - SN460**

Communication System: UID: 0, CW; Frequency: 835.0 MHz  
Medium: 835 Head; Medium parameters used:  
f = 835.0 MHz; cond = 0.926 S/m; perm = 41.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 06/21/2023; Ambient Temp: 21.7°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7490; ConvF:(10.06,10.06,10.06); Calibrated: 2022-12-09  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1644; Calibrated: 2022-12-13  
Phantom: Twin-SAM V8.0; Serial: 2034  
Measurement SW: DASY Module SAR V16.2.0.1425

## 835 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.06 W/kg

**SAR(1 g) = 1.96 W/kg; SAR(10 g) = 1.29 W/kg**

Deviation (1 g) = 0.82%; Deviation (10 g) = 1.74%;

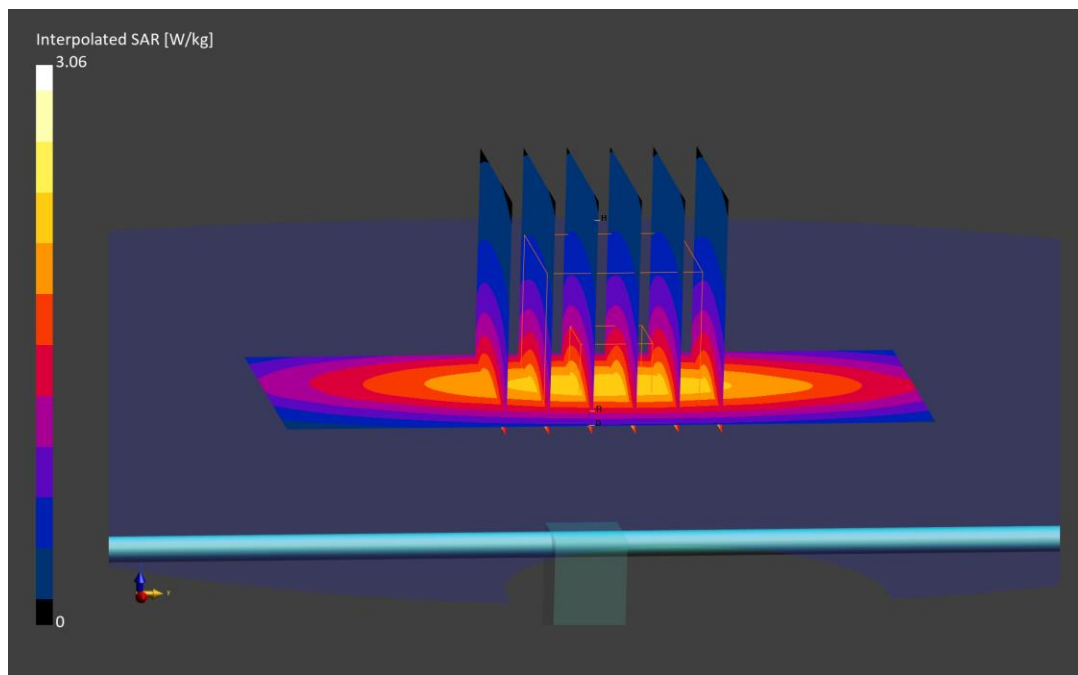

# ELEMENT

**DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d040**

Communication System: UID: 0, CW; Frequency: 835.0 MHz  
Medium: 835 Head; Medium parameters used:  
f = 835.0 MHz; cond = 0.933 S/m; perm = 41.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 06/28/2023; Ambient Temp: 22.0°C; Tissue Temp: 22.6°C

Probe: EX3DV4 - SN7490; ConvF:(10.06,10.06,10.06); Calibrated: 2022-12-09  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1644; Calibrated: 2022-12-13  
Phantom: Twin-SAM V8.0; Serial: 2034  
Measurement SW: DASY Module SAR V16.2.0.1425

## 835 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.09 W/kg

**SAR(1 g) = 1.99 W/kg; SAR(10 g) = 1.31 W/kg**

Deviation (1 g) = 1.63%; Deviation (10 g) = 2.66%;

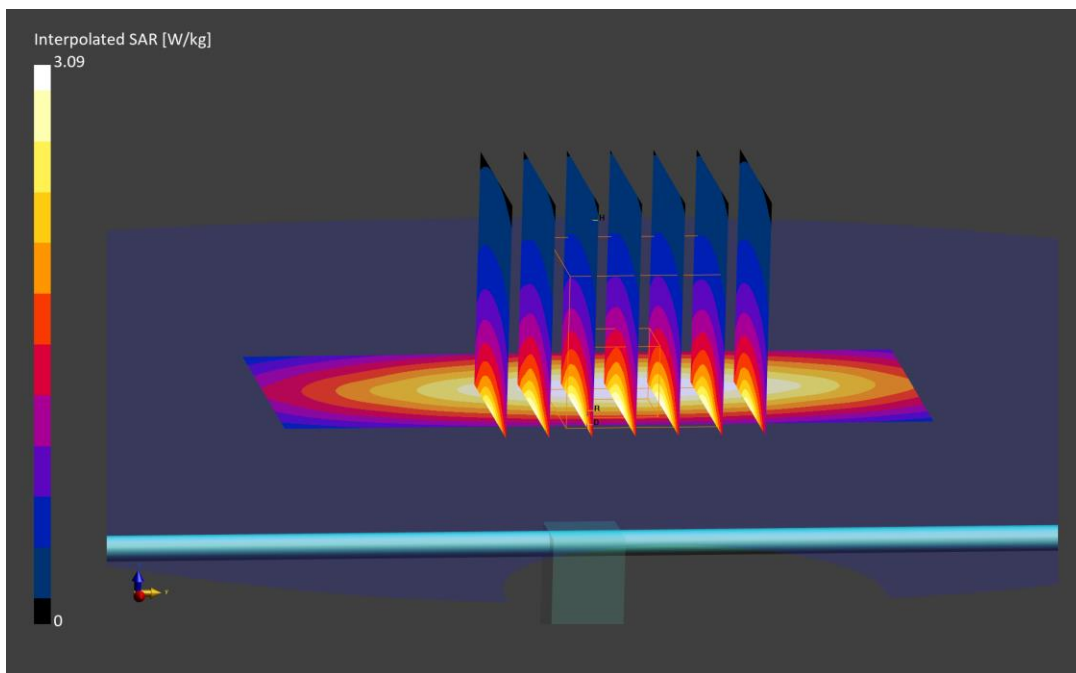

# ELEMENT

**DUT: Dipole 835.0 MHz; Type: D835V2 - SN460**

Communication System: UID: 0, CW; Frequency: 835.0 MHz  
Medium: 835 Head; Medium parameters used:  
f = 835.0 MHz; cond = 0.915 S/m; perm = 40.1; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 07/04/2023; Ambient Temp: 20.1°C; Tissue Temp: 20.8°C

Probe: EX3DV4 - SN3746; ConvF:(9.1,9.1,9.1); Calibrated: 2022-11-14  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1237; Calibrated: 2022-11-14  
Phantom: Twin-SAM V8.0; Serial: 2029  
Measurement SW: DASY Module SAR V16.2.0.1425

## 835 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.23 W/kg

**SAR(1 g) = 2.07 W/kg; SAR(10 g) = 1.36 W/kg**

Deviation (1 g) = 6.48%; Deviation (10 g) = 7.26%;

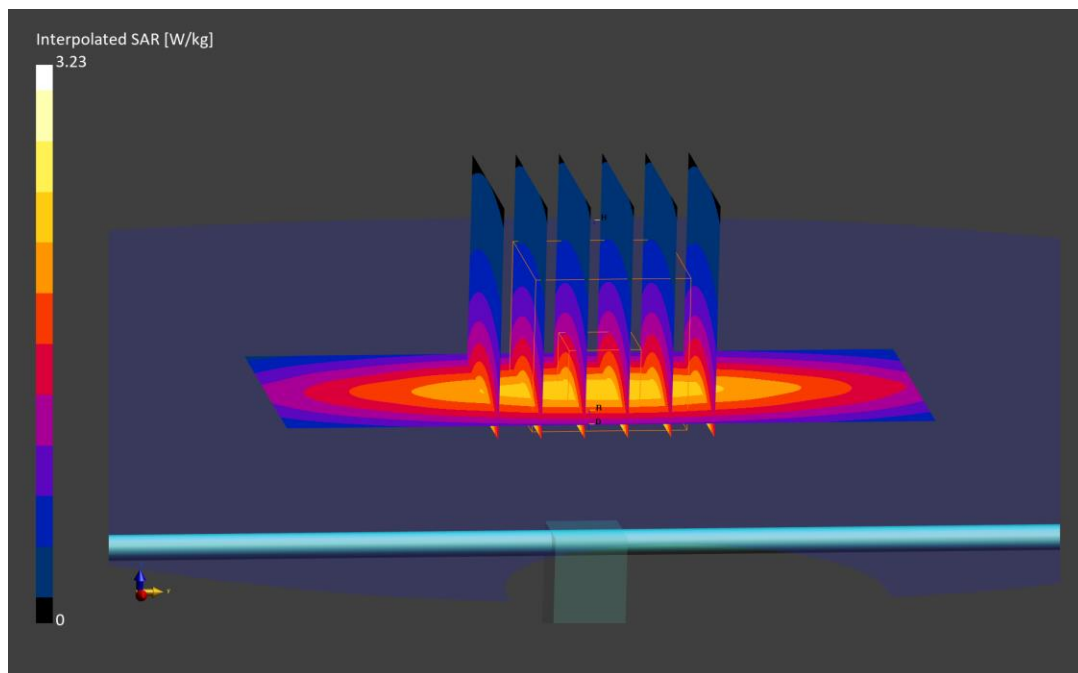

# ELEMENT

**DUT: Dipole 835.0 MHz; Type: D835V2 - SN460**

Communication System: UID: 0, CW; Frequency: 835.0 MHz  
Medium: 835 Head; Medium parameters used:  
f = 835.0 MHz; cond = 0.922 S/m; perm = 41.1; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 15 mm

Test Date: 07/06/2023; Ambient Temp: 20.9°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN3746; ConvF:(9.1,9.1,9.1); Calibrated: 2022-11-14  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1237; Calibrated: 2022-11-14  
Phantom: Twin-SAM V8.0; Serial: 2029  
Measurement SW: DASY Module SAR V16.2.0.1425

## 835 MHz System Verification at 23 dBm (200 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.16 W/kg

**SAR(1 g) = 2.02 W/kg; SAR(10 g) = 1.32 W/kg**

Deviation (1 g) = 3.91%; Deviation (10 g) = 4.10%;

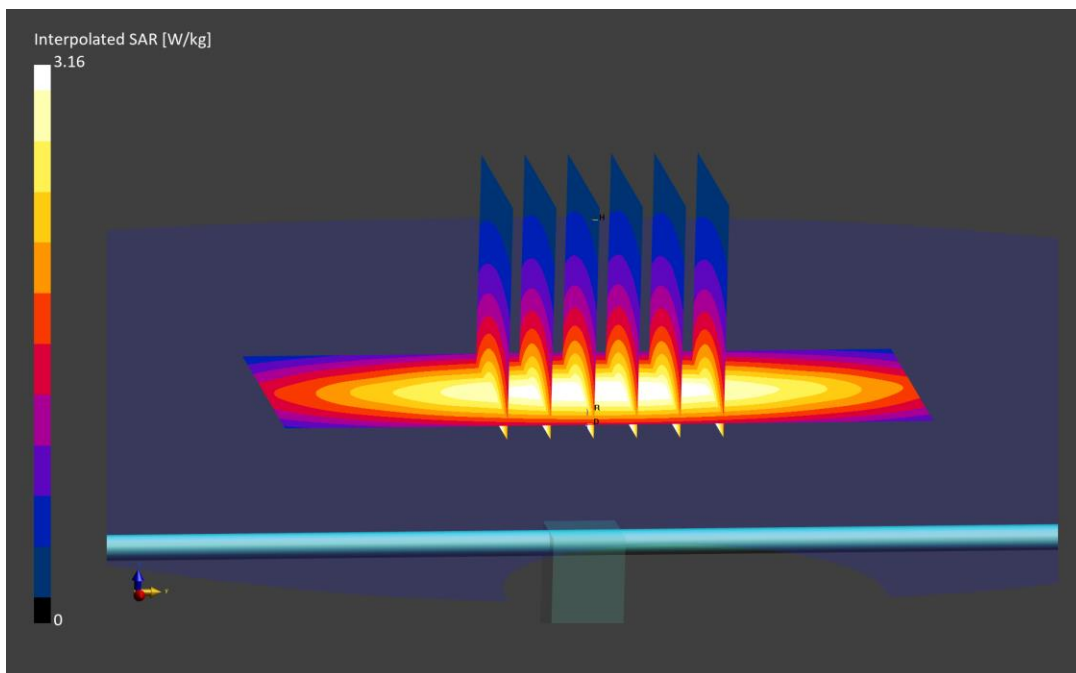



# ELEMENT

**DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1083**

Communication System: UID: 0, CW; Frequency: 1750.0 MHz  
Medium: 1750 Head; Medium parameters used:  
f = 1750.0 MHz; cond = 1.41 S/m; perm = 39.1; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/16/2023; Ambient Temp: 22.0°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN3746; ConvF:(7.98,7.98,7.98); Calibrated: 2022-11-14  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1237; Calibrated: 2022-11-14  
Phantom: Twin-SAM V8.0; Serial: 2029  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1750 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.09 W/kg

**SAR(1 g) = 3.70 W/kg; SAR(10 g) = 1.93 W/kg**

Deviation (1 g) = 1.37%; Deviation (10 g) = 0.52%;

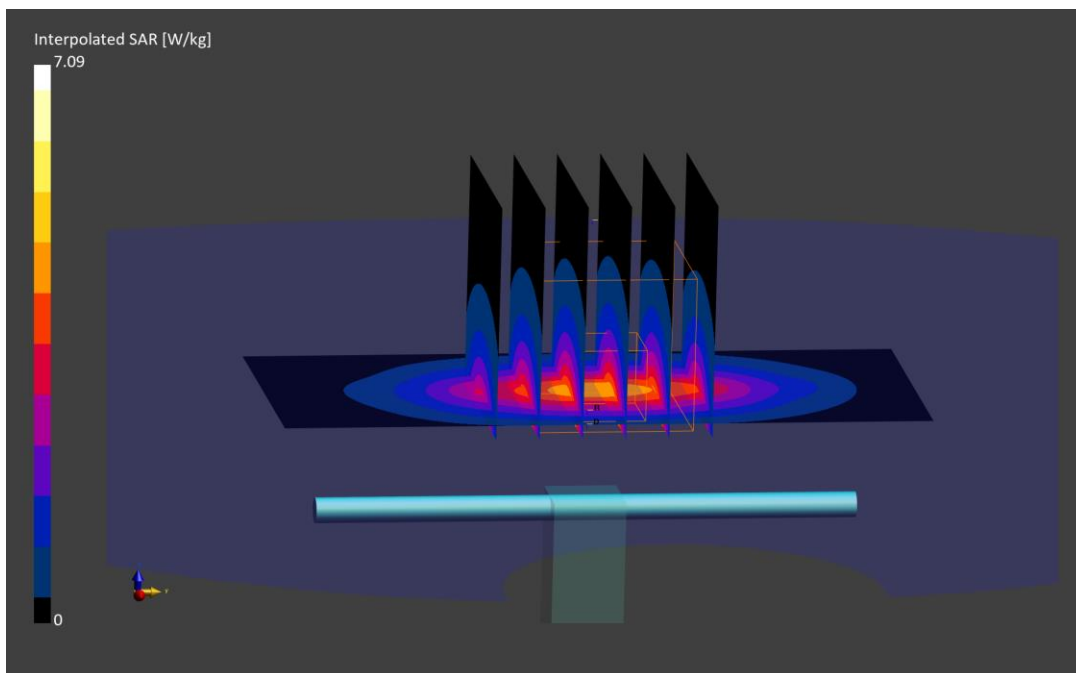

# ELEMENT

**DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1104**

Communication System: UID: 0, CW; Frequency: 1750.0 MHz  
Medium: 1750 Head; Medium parameters used:  
f = 1750.0 MHz; cond = 1.41 S/m; perm = 38.6; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/19/2023; Ambient Temp: 20.5°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN3746; ConvF:(7.98,7.98,7.98); Calibrated: 2022-11-14  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1237; Calibrated: 2022-11-14  
Phantom: Twin-SAM V8.0; Serial: 2029  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1750 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.88 W/kg

**SAR(1 g) = 3.56 W/kg; SAR(10 g) = 1.85 W/kg**

Deviation (1 g) = -0.28%; Deviation (10 g) = -1.60%;

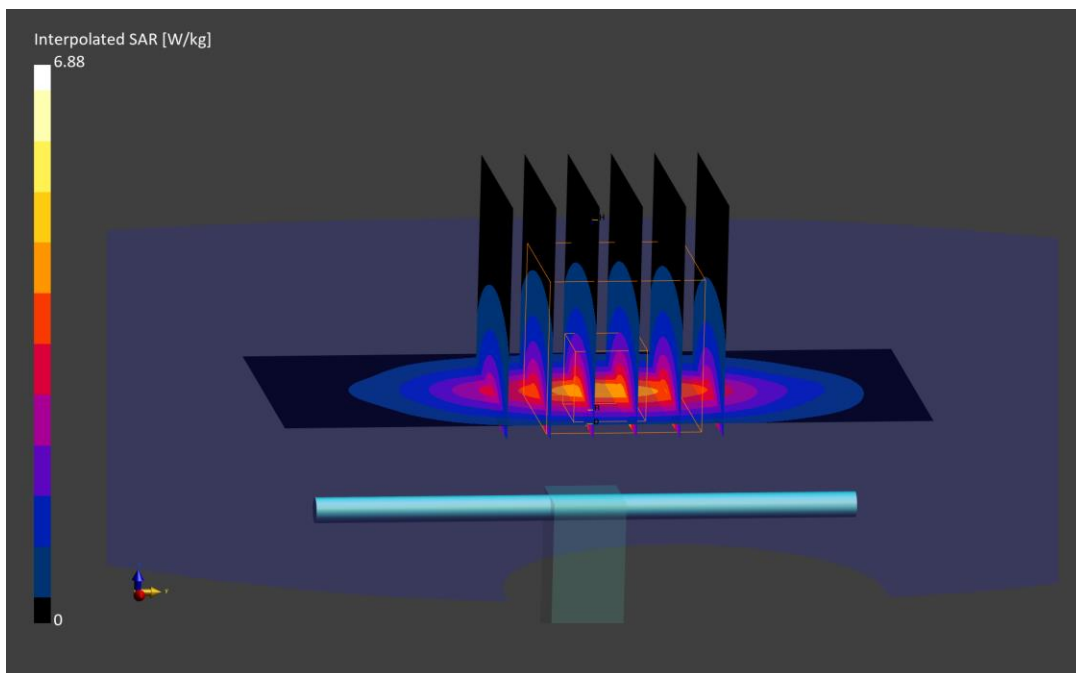

# ELEMENT

**DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1104**

Communication System: UID: 0, CW; Frequency: 1750.0 MHz  
Medium: 1750 Head; Medium parameters used:  
f = 1750.0 MHz; cond = 1.32 S/m; perm = 40.6; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/28/2023; Ambient Temp: 20.7°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7421; ConvF:(7.79,7.79,7.79); Calibrated: 2023-03-16  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn604; Calibrated: 2023-03-15  
Phantom: Twin-SAM V8.0; Serial: 2070  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1750 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.54 W/kg

**SAR(1 g) = 3.53 W/kg; SAR(10 g) = 1.89 W/kg**

Deviation (1 g) = -1.12%; Deviation (10 g) = 0.53%;

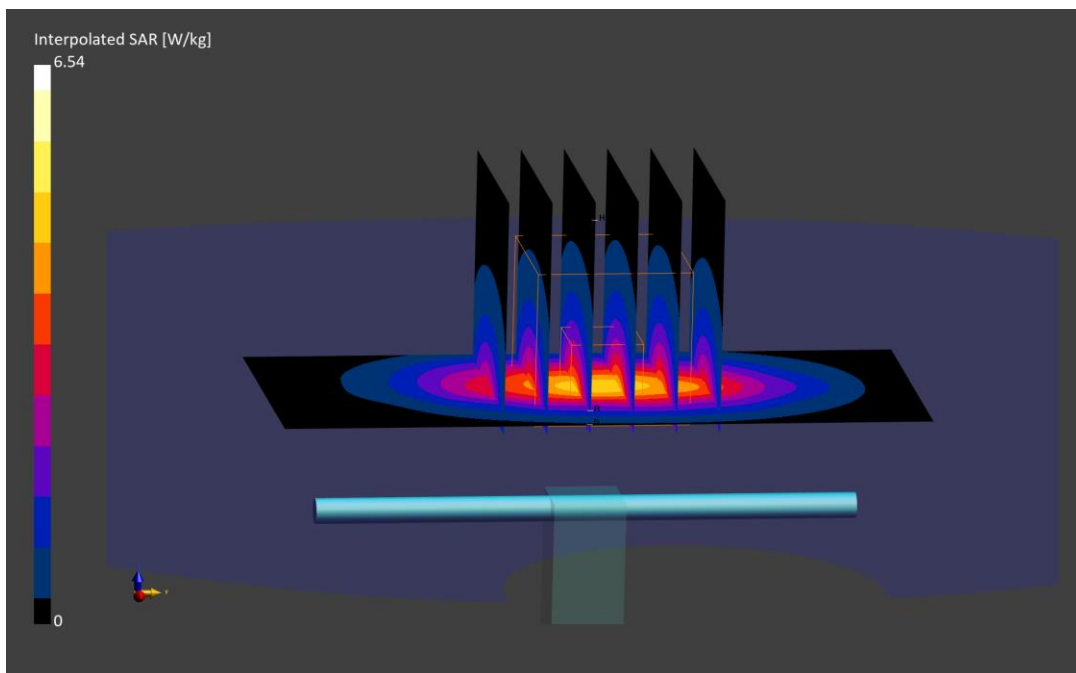

# ELEMENT

**DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d030**

Communication System: UID: 0, CW; Frequency: 1900.0 MHz  
Medium: 1900 Head; Medium parameters used:  
f = 1900.0 MHz; cond = 1.40 S/m; perm = 39.7; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/14/2023; Ambient Temp: 21.7°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7490; ConvF:(8.27,8.27,8.27); Calibrated: 2022-12-09  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1644; Calibrated: 2022-12-13  
Phantom: Twin-SAM V8.0; Serial: 2034  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1900 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.40 W/kg

**SAR(1 g) = 3.99 W/kg; SAR(10 g) = 2.11 W/kg**

Deviation (1 g) = 0.25%; Deviation (10 g) = 3.43%;

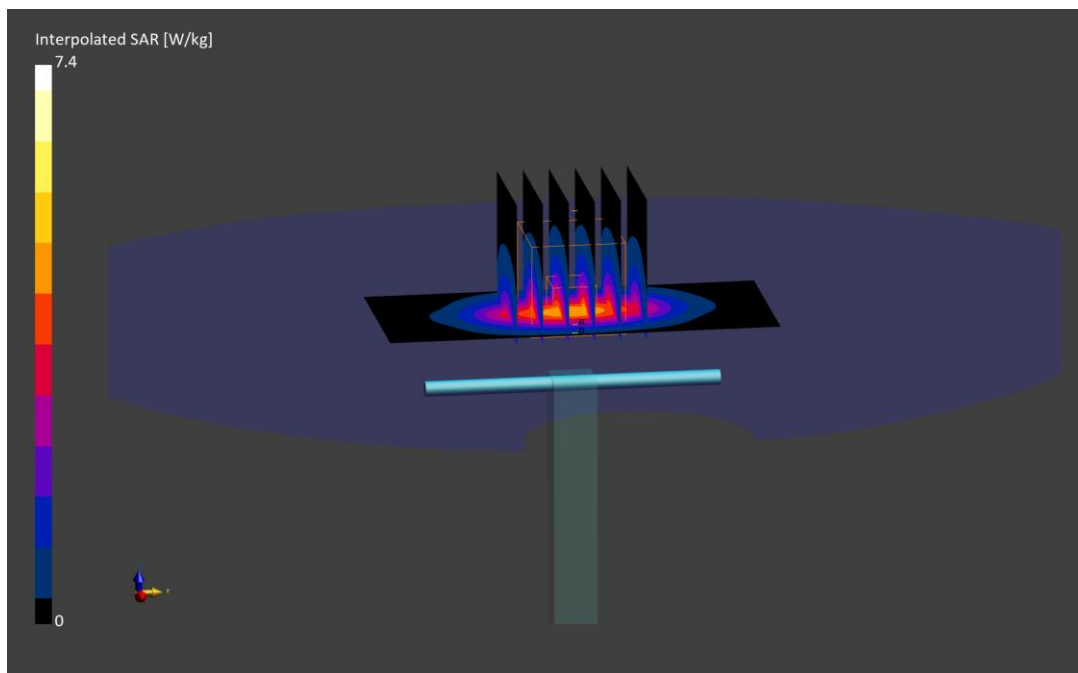

# ELEMENT

**DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d181**

Communication System: UID: 0, CW; Frequency: 1900.0 MHz  
Medium: 1900 Head; Medium parameters used:  
f = 1900.0 MHz; cond = 1.37 S/m; perm = 40.0; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/19/2023; Ambient Temp: 21.7°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7490; ConvF:(8.27,8.27,8.27); Calibrated: 2022-12-09  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1644; Calibrated: 2022-12-13  
Phantom: Twin-SAM V8.0; Serial: 2034  
Measurement SW: DASY Module SAR V16.2.0.1425

## 1900 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 90.0):** Measurement grid: dx=10.0 mm, dy=15.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.72 W/kg

**SAR(1 g) = 4.18 W/kg; SAR(10 g) = 2.20 W/kg**

Deviation (1 g) = 4.24%; Deviation (10 g) = 5.77%;

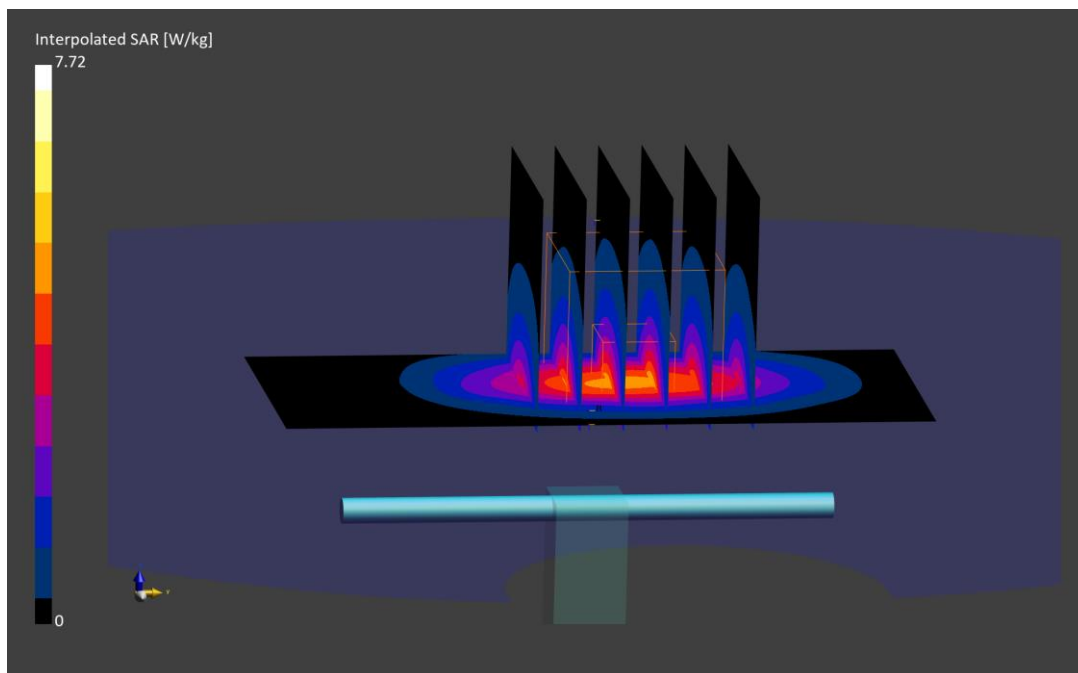

# ELEMENT

**DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921**

Communication System: UID: 0, CW; Frequency: 2450.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2450.0 MHz; cond = 1.86 S/m; perm = 40.2; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/06/2023; Ambient Temp: 21.1 °C; Tissue Temp: 21.1 °C

Probe: EX3DV4 - SN7308; ConvF:(7.91,7.91,7.91); Calibrated: 2023-02-13  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn467; Calibrated: 2023-02-15  
Phantom: Twin-SAM V4.0; Serial: 1275  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2450 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.2 W/kg

**SAR(1 g) = 5.30 W/kg; SAR(10 g) = 2.46 W/kg**

Deviation (1 g) = -2.21%; Deviation (10 g) = -3.53%;

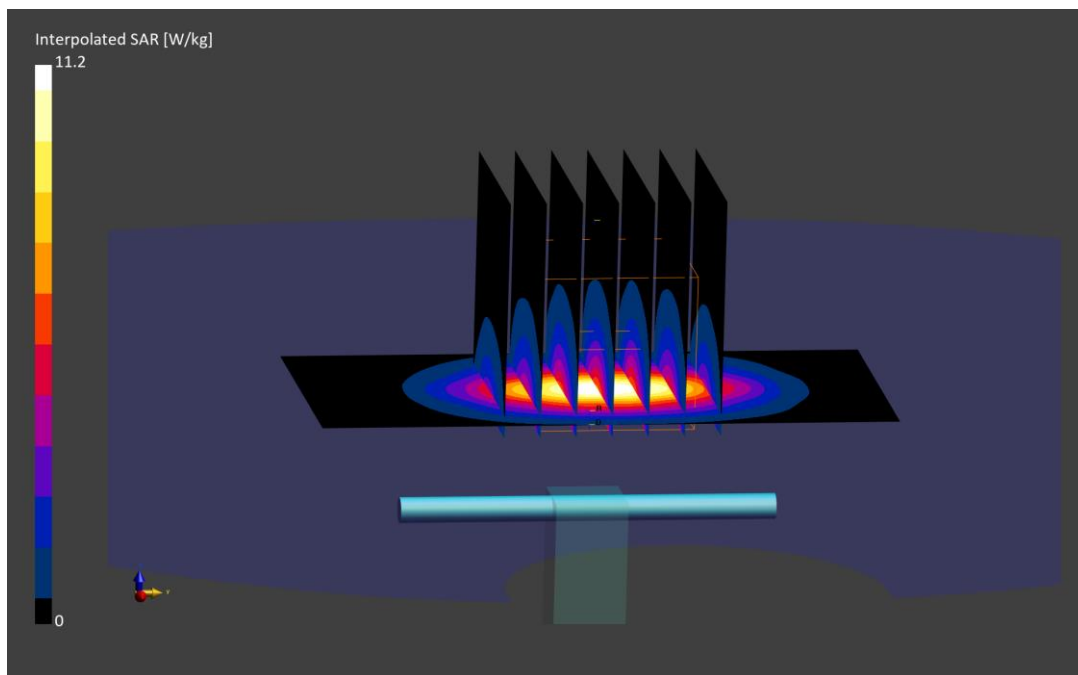

# ELEMENT

**DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921**

Communication System: UID: 0, CW; Frequency: 2450.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2450.0 MHz; cond = 1.88 S/m; perm = 39.7; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/14/2023; Ambient Temp: 21.1°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN7308; ConvF:(7.91,7.91,7.91); Calibrated: 2023-02-13  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn467; Calibrated: 2023-02-15  
Phantom: Twin-SAM V4.0; Serial: 1275  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2450 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.6 W/kg

**SAR(1 g) = 5.20 W/kg; SAR(10 g) = 2.42 W/kg**

Deviation (1 g) = -4.06%; Deviation (10 g) = -5.10%;

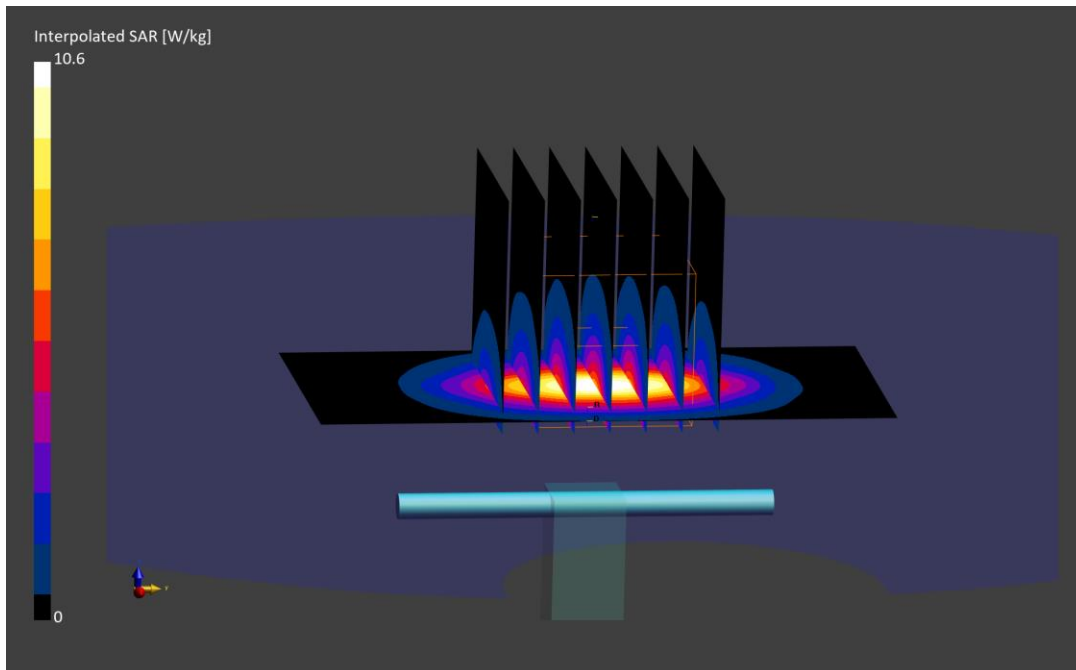

# ELEMENT

**DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921**

Communication System: UID: 0, CW; Frequency: 2450.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2450.0 MHz; cond = 1.87 S/m; perm = 39.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/16/2023; Ambient Temp: 21.9°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7308; ConvF:(7.91,7.91,7.91); Calibrated: 2023-02-13  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn467; Calibrated: 2023-02-15  
Phantom: Twin-SAM V4.0; Serial: 1275  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2450 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.2 W/kg

**SAR(1 g) = 5.51 W/kg; SAR(10 g) = 2.56 W/kg**

Deviation (1 g) = 1.66%; Deviation (10 g) = 0.39%;

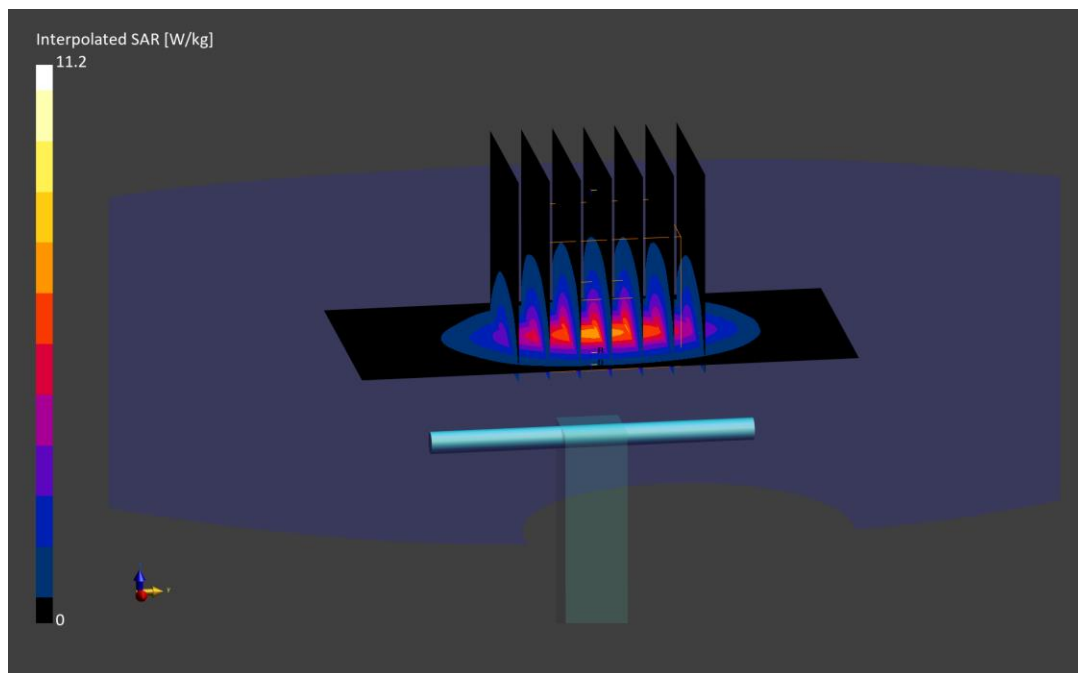



# ELEMENT

**DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921**

Communication System: UID: 0, CW; Frequency: 2450.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2450.0 MHz; cond = 1.77 S/m; perm = 39.8; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/28/2023; Ambient Temp: 22.9°C; Tissue Temp: 20.9°C

Probe: EX3DV4 - SN7308; ConvF:(7.91,7.91,7.91); Calibrated: 2023-02-13  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn467; Calibrated: 2023-02-15  
Phantom: Twin-SAM V4.0; Serial: 1275  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2450 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.2 W/kg

**SAR(1 g) = 5.15 W/kg; SAR(10 g) = 2.45 W/kg**

Deviation (1 g) = -4.98%; Deviation (10 g) = -3.92%;

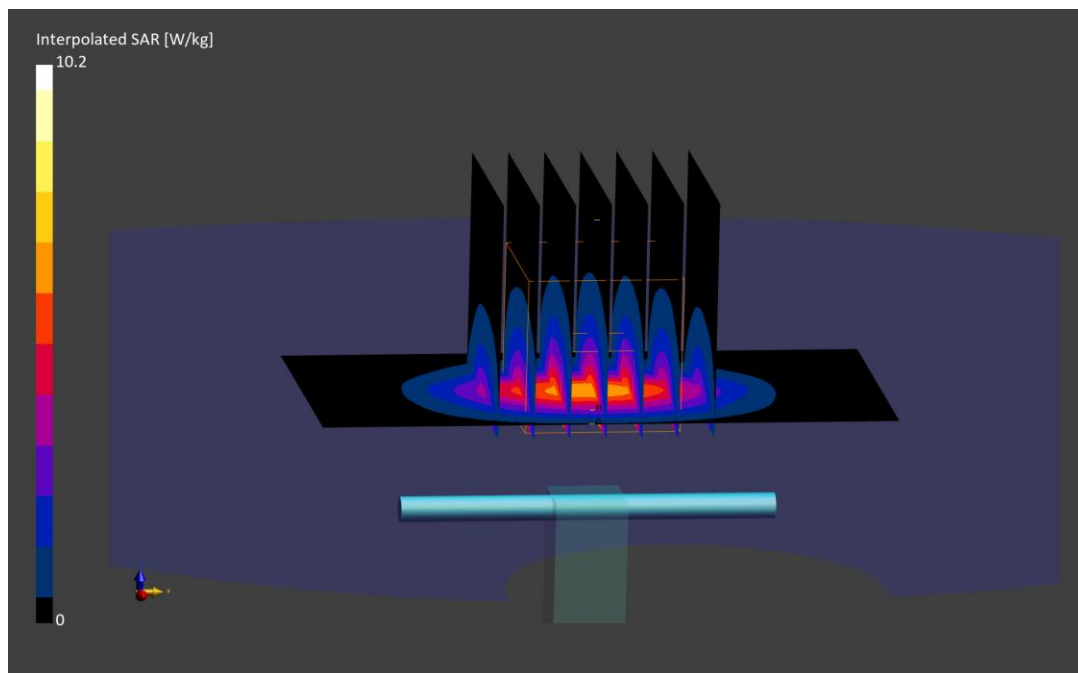

# ELEMENT

**DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921**

Communication System: UID: 0, CW; Frequency: 2450.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2450.0 MHz; cond = 1.76 S/m; perm = 39.5; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/28/2023; Ambient Temp: 21.4°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7532; ConvF:(7.88,7.88,7.88); Calibrated: 2023-04-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn501; Calibrated: 2023-04-14  
Phantom: Twin-SAM V8.0; Serial: 2067  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2450 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.4 W/kg

**SAR(1 g) = 5.49 W/kg; SAR(10 g) = 2.59 W/kg**

Deviation (1 g) = 1.29%; Deviation (10 g) = 1.57%;

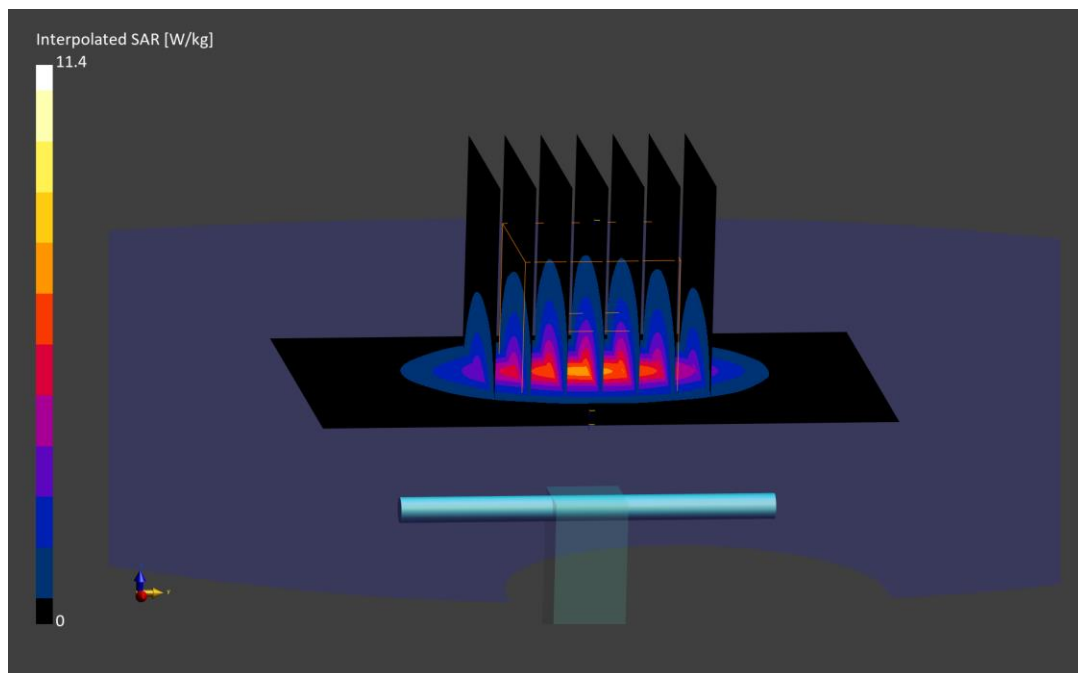

# ELEMENT

**DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921**

Communication System: UID: 0, CW; Frequency: 2450.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2450.0 MHz; cond = 1.76 S/m; perm = 40.6; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 07/04/2023; Ambient Temp: 20.0°C; Tissue Temp: 20.1°C

Probe: EX3DV4 - SN7532; ConvF:(7.88,7.88,7.88); Calibrated: 2023-04-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn501; Calibrated: 2023-04-14  
Phantom: Twin-SAM V8.0; Serial: 2067  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2450 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.2 W/kg

**SAR(1 g) = 5.35 W/kg; SAR(10 g) = 2.52 W/kg**

Deviation (1 g) = -1.29%; Deviation (10 g) = -1.18%;

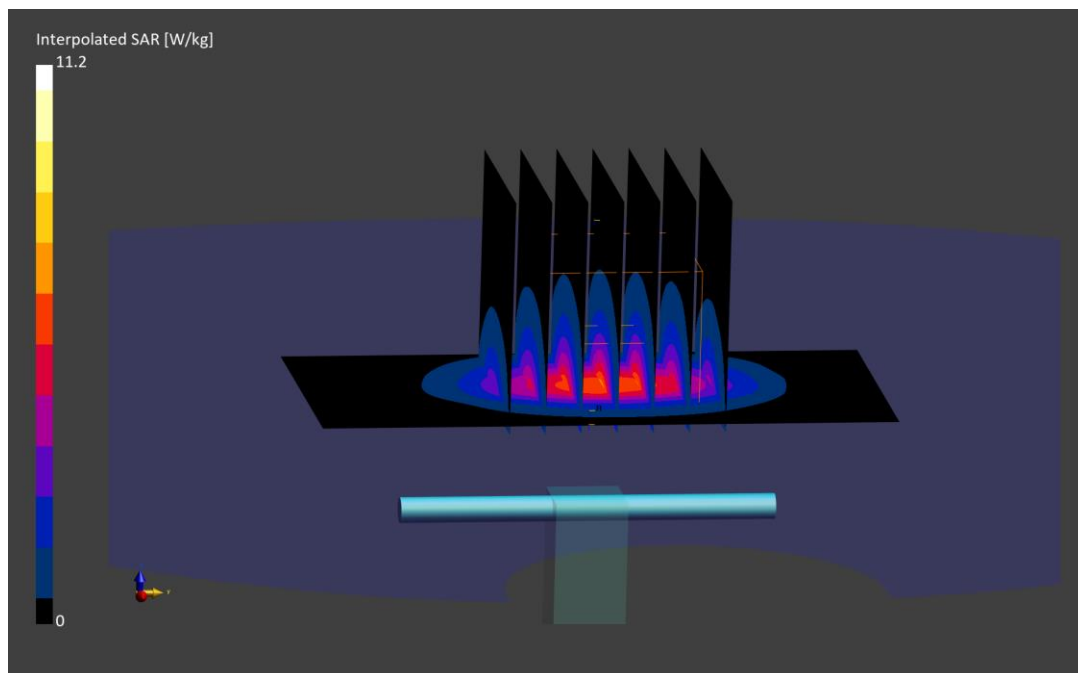

# ELEMENT

**DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1069**

Communication System: UID: 0, CW; Frequency: 2600.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2600.0 MHz; cond = 1.99 S/m; perm = 39.9; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/06/2023; Ambient Temp: 21.1°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7308; ConvF:(7.74,7.74,7.74); Calibrated: 2023-02-13  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn467; Calibrated: 2023-02-15  
Phantom: Twin-SAM V4.0; Serial: 1275  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2600 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.9 W/kg

**SAR(1 g) = 5.63 W/kg; SAR(10 g) = 2.54 W/kg**

Deviation (1 g) = 1.26%; Deviation (10 g) = 2.01%;

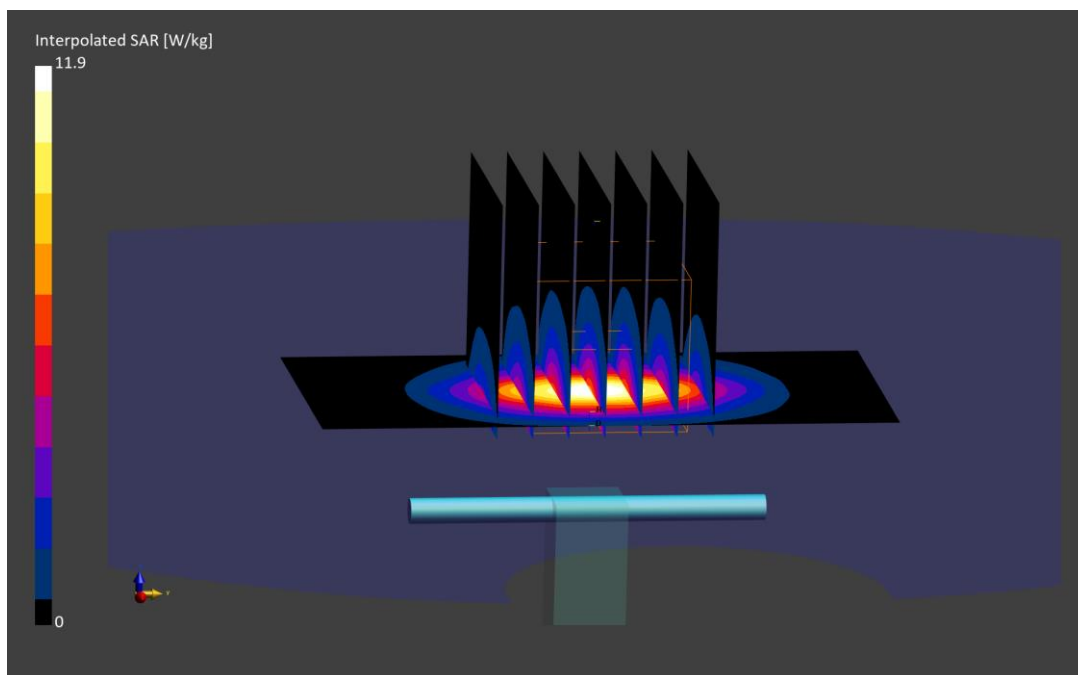

# ELEMENT

**DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1069**

Communication System: UID: 0, CW; Frequency: 2600.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2600.0 MHz; cond = 2.00 S/m; perm = 39.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/14/2023; Ambient Temp: 21.1 °C; Tissue Temp: 21.2 °C

Probe: EX3DV4 - SN7308; ConvF:(7.74,7.74,7.74); Calibrated: 2023-02-13  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn467; Calibrated: 2023-02-15  
Phantom: Twin-SAM V4.0; Serial: 1275  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2600 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.0 W/kg

**SAR(1 g) = 5.78 W/kg; SAR(10 g) = 2.60 W/kg**

Deviation (1 g) = 3.96%; Deviation (10 g) = 4.42%;

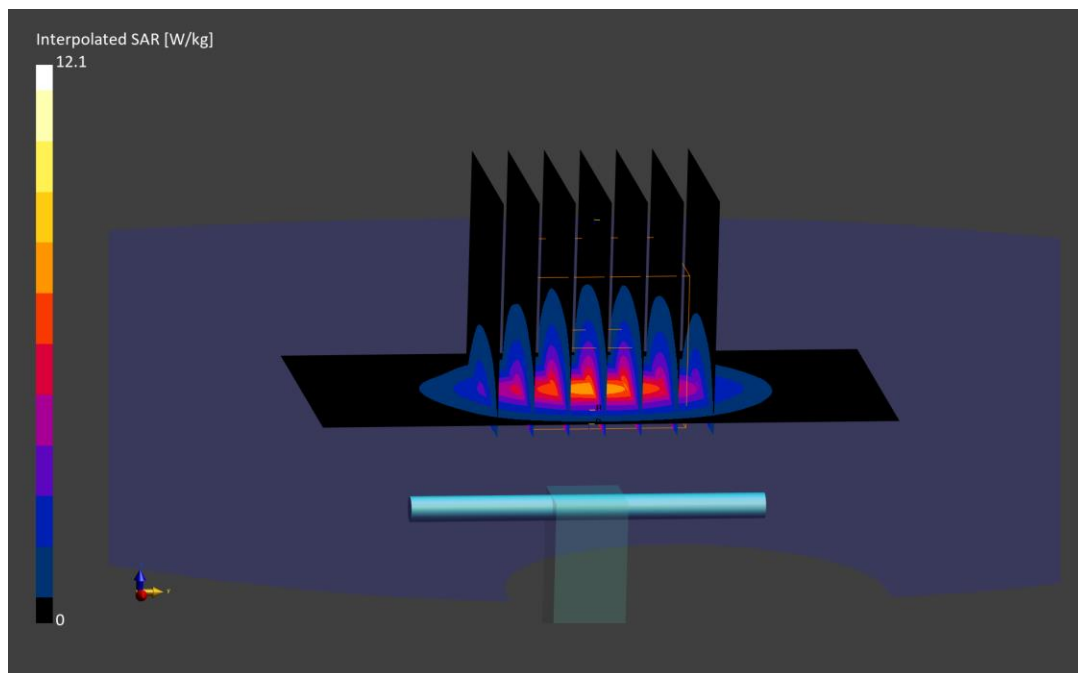

# ELEMENT

**DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1069**

Communication System: UID: 0, CW; Frequency: 2600.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2600.0 MHz; cond = 1.89 S/m; perm = 39.3; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/28/2023; Ambient Temp: 21.4°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7532; ConvF:(7.53,7.53,7.53); Calibrated: 2023-04-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn501; Calibrated: 2023-04-14  
Phantom: Twin-SAM V8.0; Serial: 2067  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2600 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.1 W/kg

**SAR(1 g) = 5.35 W/kg; SAR(10 g) = 2.46 W/kg**

Deviation (1 g) = -3.78%; Deviation (10 g) = -1.20%;

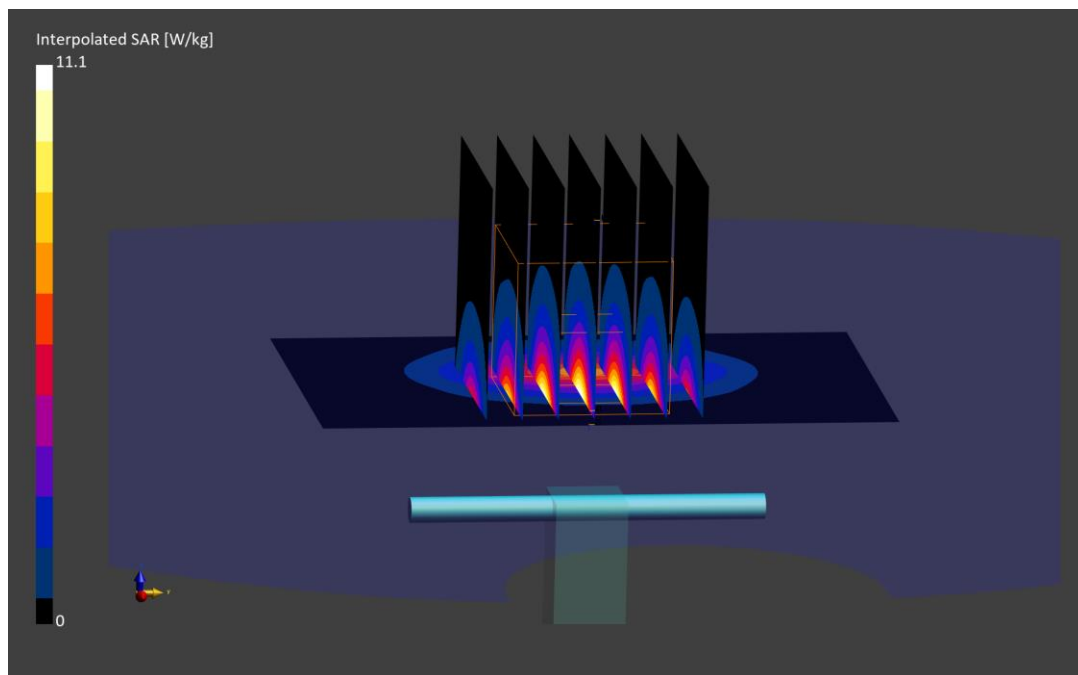

# ELEMENT

**DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1068**

Communication System: UID: 0, CW; Frequency: 2600.0 MHz  
Medium: 2450 Head; Medium parameters used:  
f = 2600.0 MHz; cond = 1.88 S/m; perm = 40.4; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 07/04/2023; Ambient Temp: 20.0°C; Tissue Temp: 20.1°C

Probe: EX3DV4 - SN7532; ConvF:(7.53,7.53,7.53); Calibrated: 2023-04-18  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn501; Calibrated: 2023-04-14  
Phantom: Twin-SAM V8.0; Serial: 2067  
Measurement SW: DASY Module SAR V16.2.0.1425

## 2600 MHz System Verification at 20 dBm (100 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (30.0 x 30.0 x 30.0):** Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.6 W/kg

**SAR(1 g) = 5.44 W/kg; SAR(10 g) = 2.47 W/kg**

Deviation (1 g) = -3.72%; Deviation (10 g) = -2.76%;

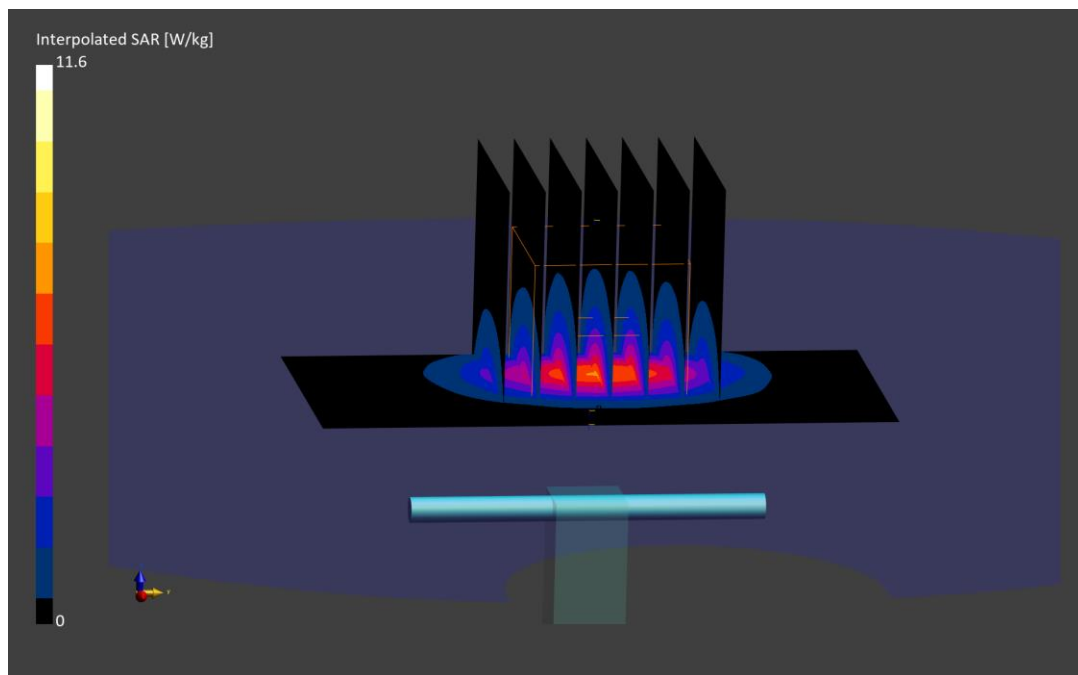

# ELEMENT

**DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1066**

Communication System: UID: 0, CW; Frequency: 5250.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5250.0 MHz; cond = 4.73 S/m; perm = 36.7; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/08/2023; Ambient Temp: 20.7°C; Tissue Temp: 20.8°C

Probe: EX3DV4 - SN7420; ConvF:(5.22,5.22,5.22); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5250 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.2 W/kg

**SAR(1 g) = 3.99 W/kg; SAR(10 g) = 1.12 W/kg**

Deviation (1 g) = -0.62%; Deviation (10 g) = -3.03%;

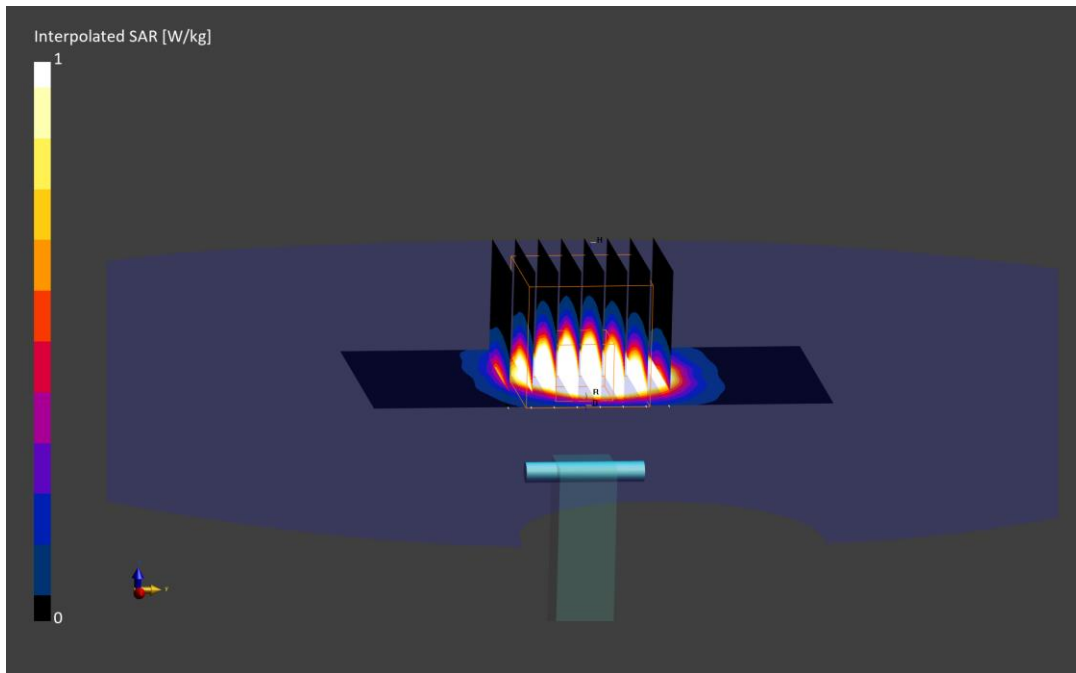



# ELEMENT

**DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1123**

Communication System: UID: 0, CW; Frequency: 5250.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5250.0 MHz; cond = 4.73 S/m; perm = 35.2; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/19/2023; Ambient Temp: 22.0°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7420; ConvF:(5.22,5.22,5.22); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5250 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.8 W/kg

**SAR(1 g) = 4.04 W/kg; SAR(10 g) = 1.14 W/kg**

Deviation (1 g) = 0.37%; Deviation (10 g) = -0.44%;

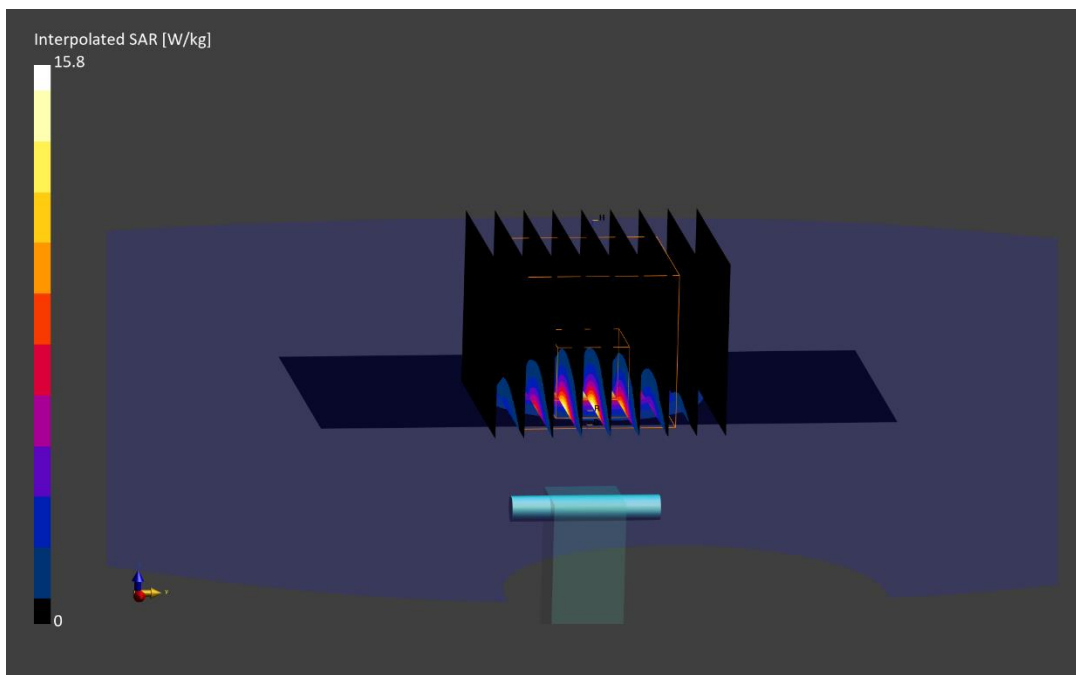

# ELEMENT

**DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1123**

Communication System: UID: 0, CW; Frequency: 5250.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5250.0 MHz; cond = 4.49 S/m; perm = 35.6; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 07/18/2023; Ambient Temp: 22.5°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7420; ConvF:(5.22,5.22,5.22); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5250 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.6 W/kg

**SAR(1 g) = 3.85 W/kg; SAR(10 g) = 1.10 W/kg**

Deviation (1 g) = -4.35%; Deviation (10 g) = -3.93%;

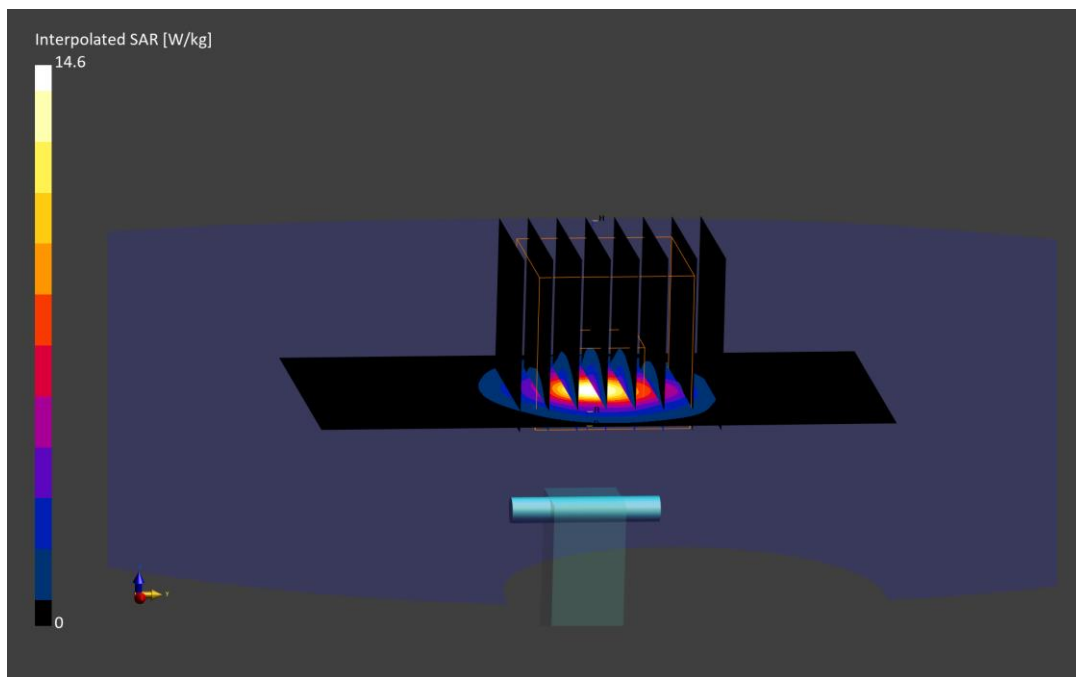

# ELEMENT

**DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1066**

Communication System: UID: 0, CW; Frequency: 5600.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5600.0 MHz; cond = 5.14 S/m; perm = 36.1; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/08/2023; Ambient Temp: 20.7°C; Tissue Temp: 20.8°C

Probe: EX3DV4 - SN7420; ConvF:(4.63,4.63,4.63); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5600 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.2 W/kg

**SAR(1 g) = 3.94 W/kg; SAR(10 g) = 1.11 W/kg**

Deviation (1 g) = -6.08%; Deviation (10 g) = -7.88%;

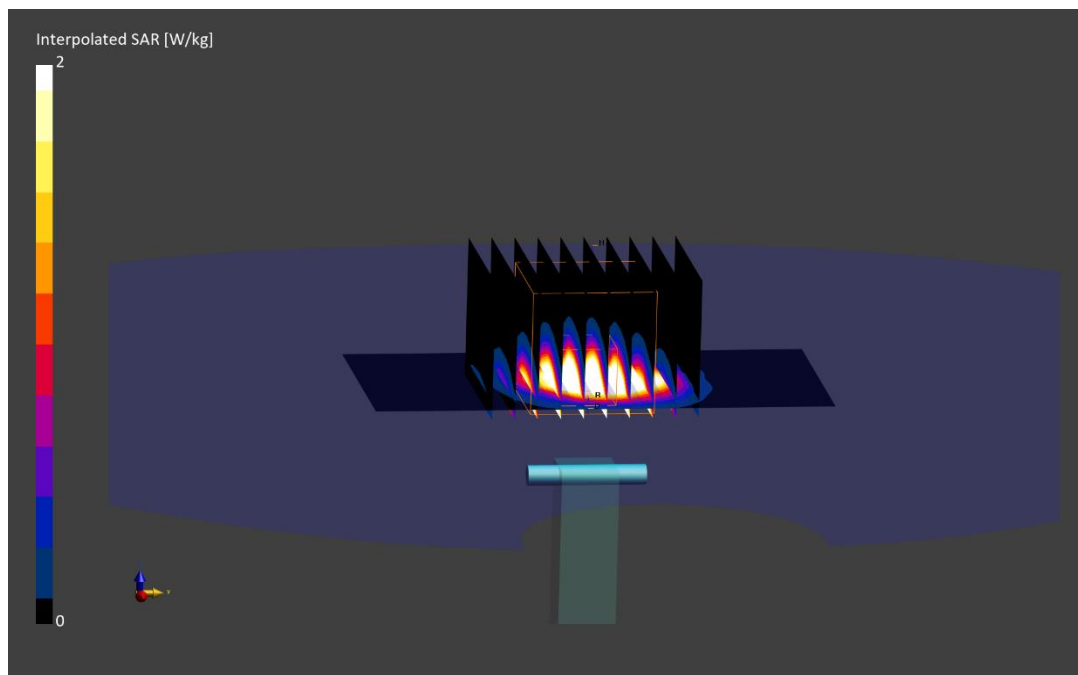

# ELEMENT

**DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1123**

Communication System: UID: 0, CW; Frequency: 5600.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5600.0 MHz; cond = 5.12 S/m; perm = 34.5; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/19/2023; Ambient Temp: 22.0°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7420; ConvF:(4.63,4.63,4.63); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5600 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.9 W/kg

**SAR(1 g) = 4.28 W/kg; SAR(10 g) = 1.20 W/kg**

Deviation (1 g) = 2.27%; Deviation (10 g) = 1.27%;

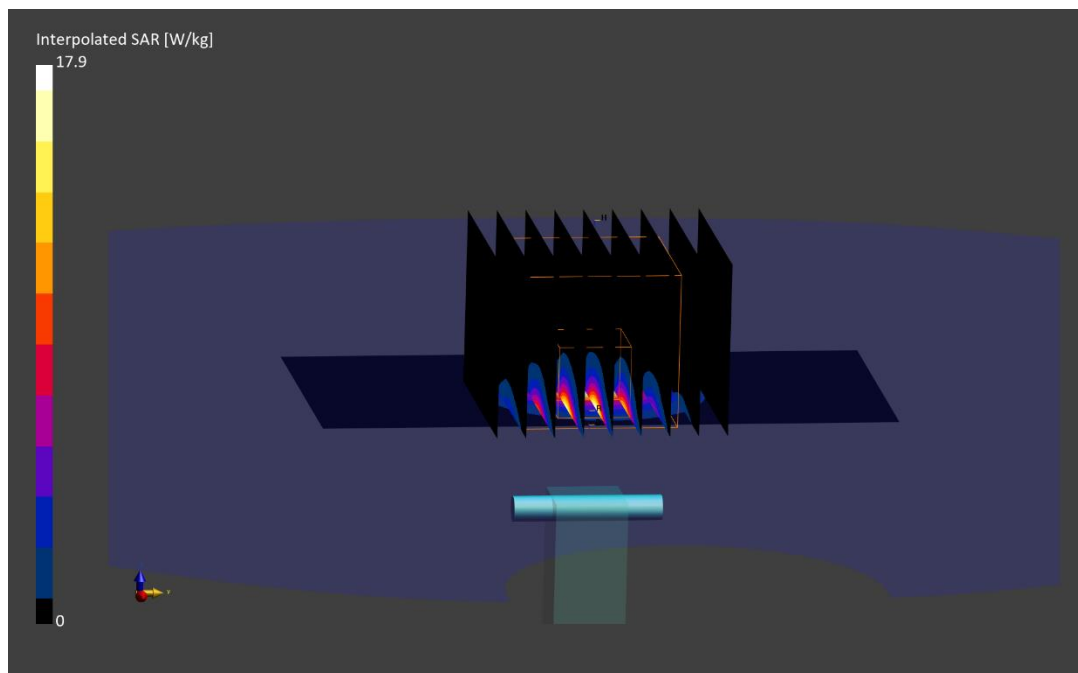

# ELEMENT

**DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1123**

Communication System: UID: 0, CW; Frequency: 5600.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5600.0 MHz; cond = 4.87 S/m; perm = 35.0; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 07/18/2023; Ambient Temp: 22.5°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7420; ConvF:(4.63,4.63,4.63); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5600 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.0 W/kg

**SAR(1 g) = 4.26 W/kg; SAR(10 g) = 1.21 W/kg**

Deviation (1 g) = 1.79%; Deviation (10 g) = 2.11%;

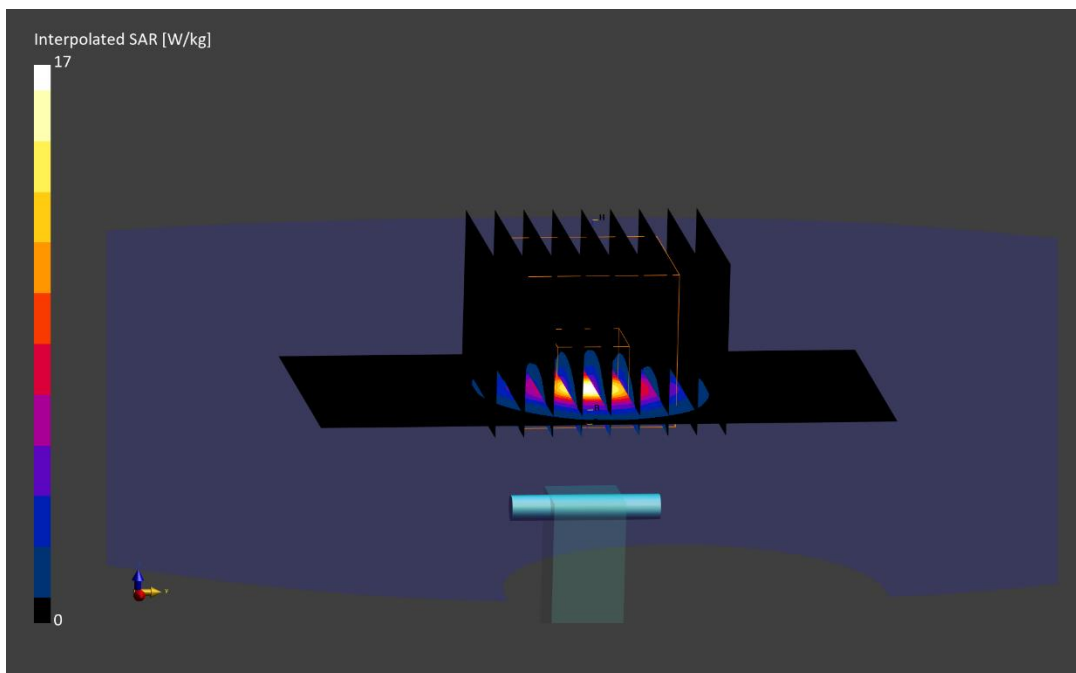

# ELEMENT

**DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1066**

Communication System: UID: 0, CW; Frequency: 5750.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5750.0 MHz; cond = 5.32 S/m; perm = 35.8; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/08/2023; Ambient Temp: 20.7°C; Tissue Temp: 20.8°C

Probe: EX3DV4 - SN7420; ConvF:(4.8,4.8,4.8); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5750 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.1 W/kg

**SAR(1 g) = 3.79 W/kg; SAR(10 g) = 1.06 W/kg**

Deviation (1 g) = -4.65%; Deviation (10 g) = -6.19%;

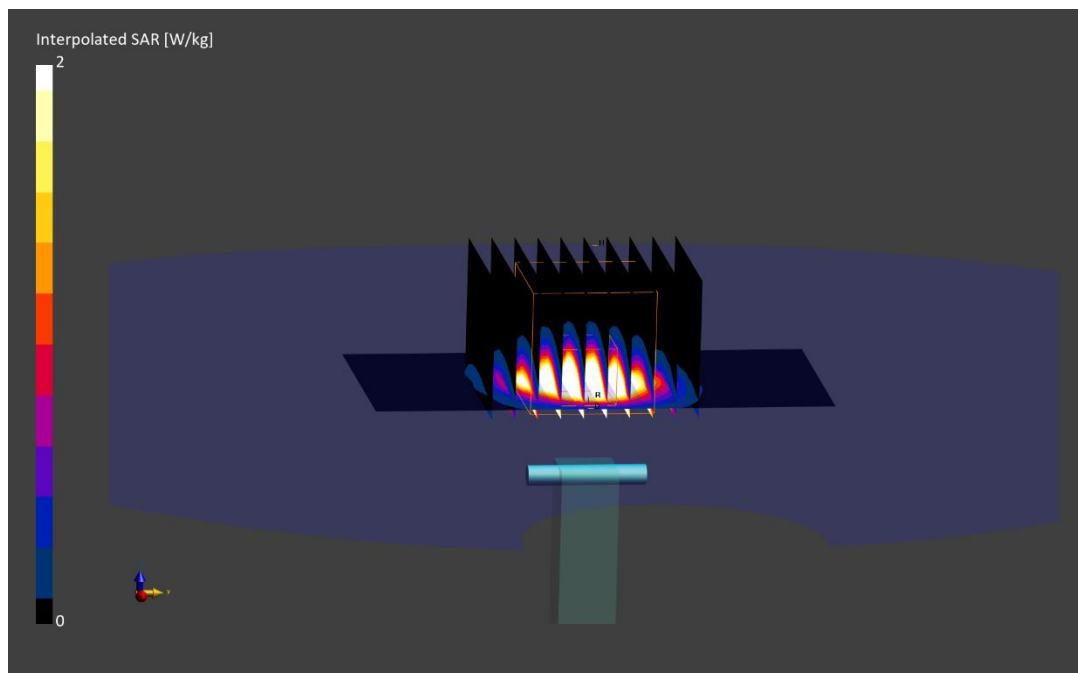

# ELEMENT

**DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1123**

Communication System: UID: 0, CW; Frequency: 5750.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5750.0 MHz; cond = 5.31 S/m; perm = 34.2; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 06/19/2023; Ambient Temp: 22.0°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7420; ConvF:(4.8,4.8,4.8); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5750 MHz System Verification at 17 dBm (50 mW)


**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.5 W/kg

**SAR(1 g) = 3.83 W/kg; SAR(10 g) = 1.08 W/kg**

Deviation (1 g) = -4.84%; Deviation (10 g) = -4.85%;

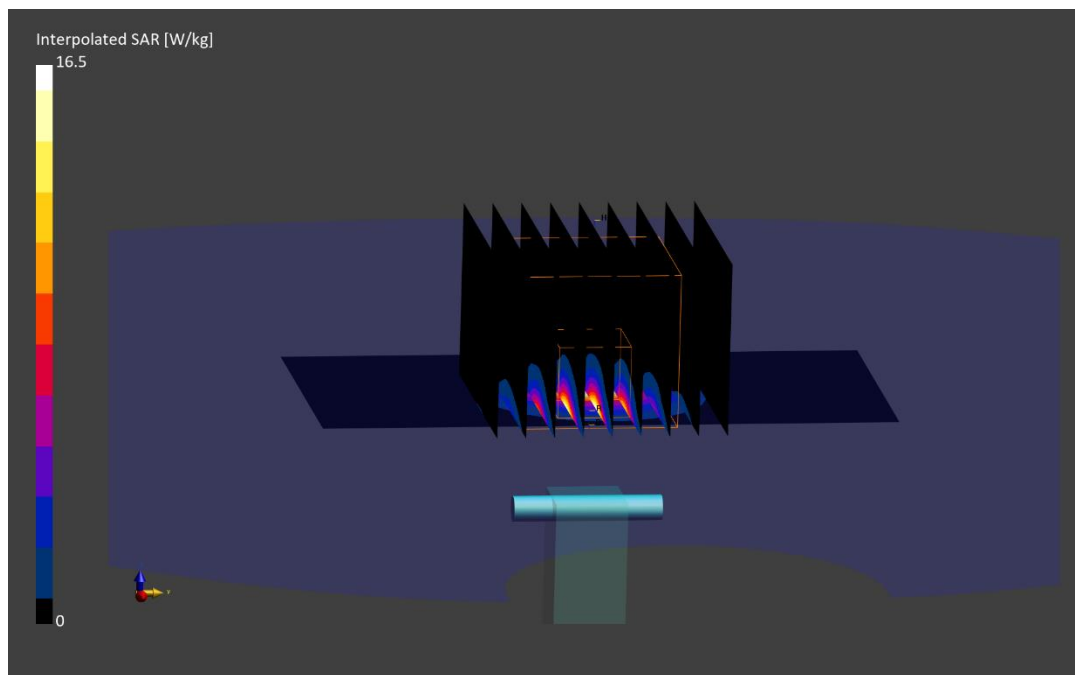

# ELEMENT

**DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1123**

Communication System: UID: 0, CW; Frequency: 5750.0 MHz  
Medium: 5200-5800 Head; Medium parameters used:  
f = 5750.0 MHz; cond = 5.05 S/m; perm = 34.8; density = 1000 kg/m<sup>3</sup>  
Phantom Section: Flat; Space: 10 mm

Test Date: 07/18/2023; Ambient Temp: 22.5°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7420; ConvF:(4.8,4.8,4.8); Calibrated: 2022-10-20  
Sensor-Surface: 1.4mm (VMS + 6p)  
Electronics: DAE4 Sn1333; Calibrated: 2022-10-13  
Phantom: Twin-SAM V8.0; Serial: 1736  
Measurement SW: DASY Module SAR V16.2.0.1425

## 5750 MHz System Verification at 17 dBm (50 mW)

**Area Scan (40.0 x 80.0):** Measurement grid: dx=10.0 mm, dy=10.0 mm

**Zoom Scan (22.0 x 22.0 x 22.0):** Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.0 W/kg

**SAR(1 g) = 3.81 W/kg; SAR(10 g) = 1.08 W/kg**

Deviation (1 g) = -5.34%; Deviation (10 g) = -4.85%;

