

### HAC-RF Emission System Check

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4041; ConvF(1, 1, 1) @ 835 MHz; Calibrated: 3/22/2021
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1352; Calibrated: 11/17/2020
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

### Dipole E-Field measurement 835MHz/835 MHz/Hearing Aid Compatibility Test at 15mm distance (41x361x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 120.6 V/m; Power Drift = 0.06 dB


Applied MIF = 0.00 dB

RF audio interference level = 41.12 dBV/m

Emission category: **M3**

MIF scaled E-field

Grid 1 <b>M3</b> 40.86 dBV/m	Grid 2 <b>M3</b> 41.12 dBV/m	Grid 3 <b>M3</b> 41.04 dBV/m
Grid 4 <b>M4</b> 35.61 dBV/m	Grid 5 <b>M4</b> 35.88 dBV/m	Grid 6 <b>M4</b> 35.86 dBV/m
Grid 7 <b>M3</b> 40.46 dBV/m	Grid 8 <b>M3</b> 40.94 dBV/m	Grid 9 <b>M3</b> 40.9 dBV/m

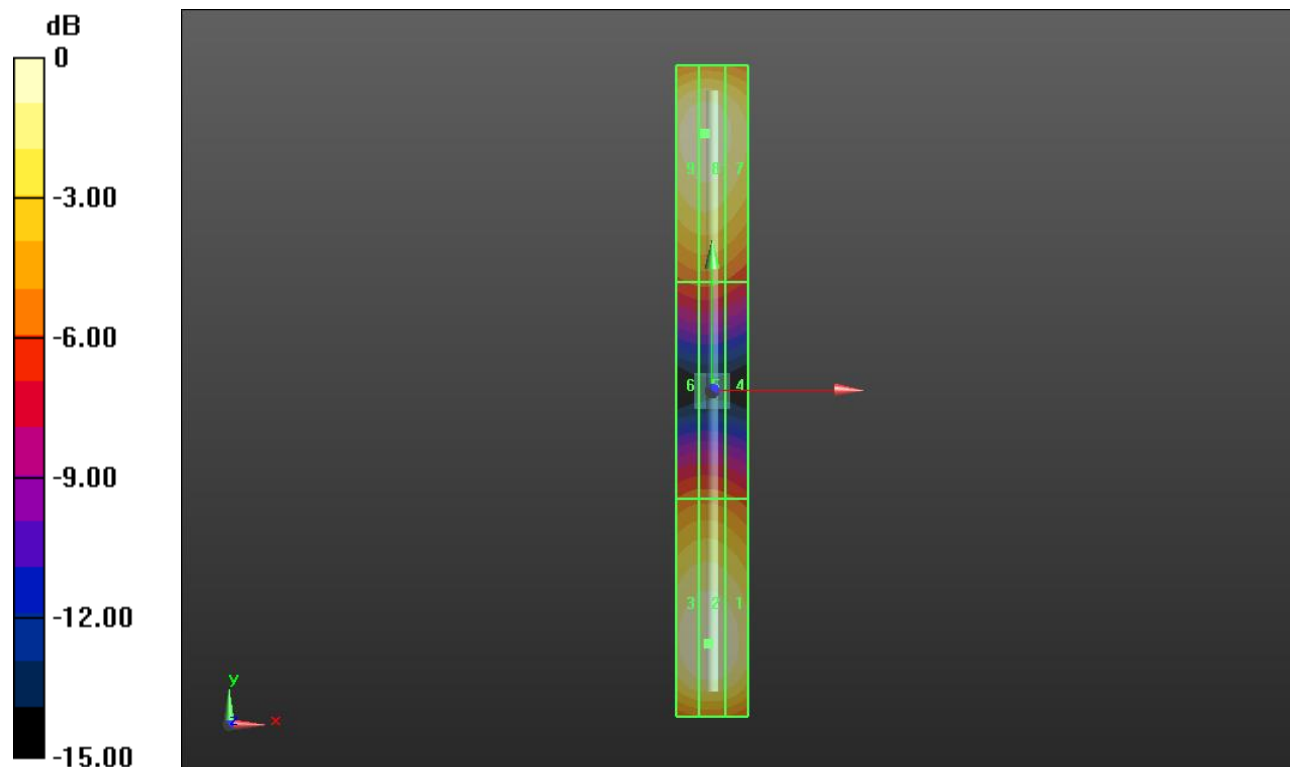

0 dB = 113.8 V/m = 41.12 dBV/m

### HAC-RF Emission System Check

Communication System: UID 0, CW; Frequency: 1880 MHz; Duty Cycle: 1:1  
 Phantom section: RF Section  
 DASY5 Configuration:  
 - Probe: EF3DV3 - SN4041; ConvF(1, 1, 1) @ 1880 MHz; Calibrated: 3/22/2021  
 - Sensor-Surface: (Fix Surface)  
 - Electronics: DAE4 Sn1352; Calibrated: 11/17/2020  
 - Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB  
 - Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

### Dipole E-Field Measurement 1880MHz/1880 MHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1):

Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 132.0 V/m; Power Drift = 0.02 dB


Applied MIF = 0.00 dB

RF audio interference level = 38.39 dBV/m

Emission category: **M2**

MIF scaled E-field

Grid 1 <b>M2</b> 37.62 dBV/m	Grid 2 <b>M2</b> 38 dBV/m	Grid 3 <b>M2</b> 37.98 dBV/m
Grid 4 <b>M3</b> 34.14 dBV/m	Grid 5 <b>M3</b> 34.41 dBV/m	Grid 6 <b>M3</b> 34.4 dBV/m
Grid 7 <b>M2</b> 37.93 dBV/m	Grid 8 <b>M2</b> 38.39 dBV/m	Grid 9 <b>M2</b> 38.35 dBV/m

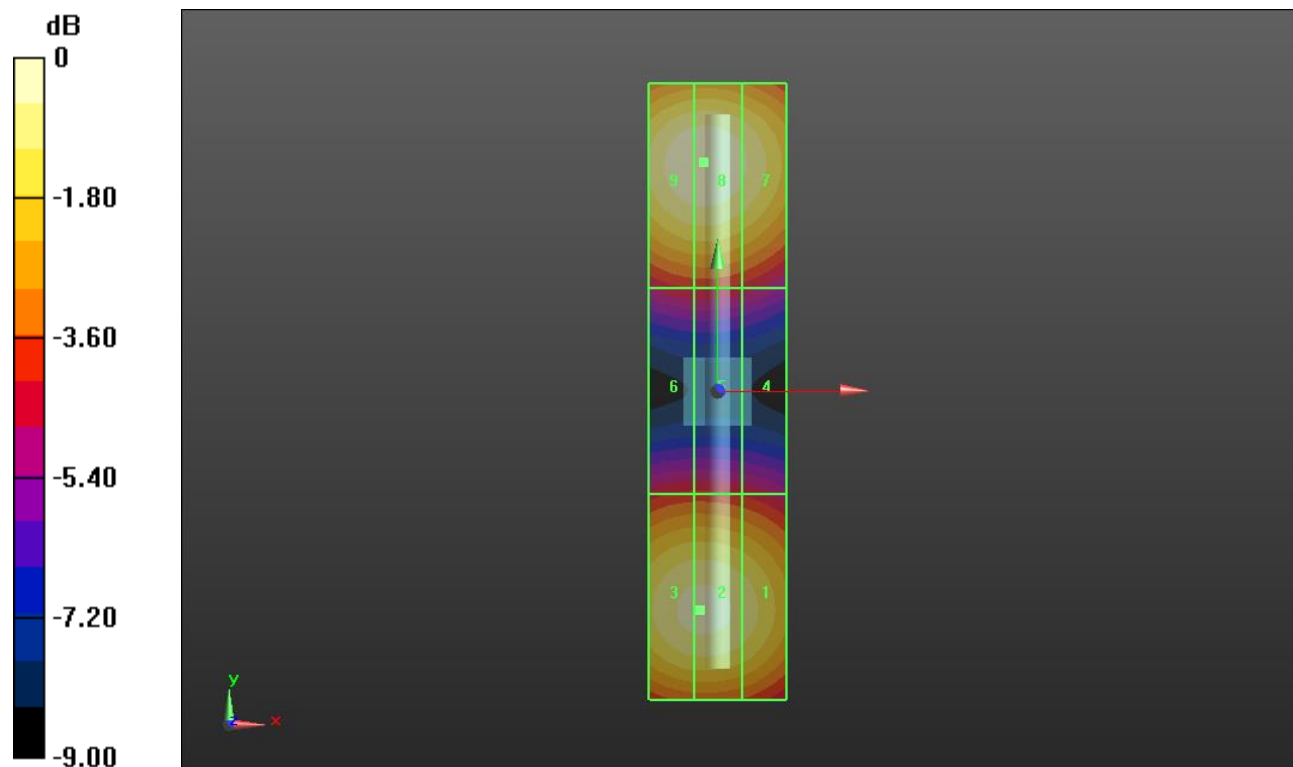

0 dB = 83.07 V/m = 38.39 dBV/m

### HAC-RF Emission System Check

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1  
 Phantom section: RF Section  
 DASY5 Configuration:  
 - Probe: EF3DV3 - SN4041; ConvF(1, 1, 1) @ 835 MHz; Calibrated: 3/22/2021  
 - Sensor-Surface: (Fix Surface)  
 - Electronics: DAE4 Sn1352; Calibrated: 11/17/2020  
 - Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB  
 - Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)


### Dipole E-Field measurement 835MHz/835 MHz/Hearing Aid Compatibility Test at 15mm distance (41x361x1):

Interpolated grid: dx=0.5000 mm, dy=0.5000 mm  
 Device Reference Point: 0, 0, -6.3 mm  
 Reference Value = 124.9 V/m; Power Drift = 0.03 dB  
 Applied MIF = 0.00 dB  
 RF audio interference level = 41.32 dBV/m

Emission category: **M3**

MIF scaled E-field

Grid 1 <b>M3</b> 40.9 dBV/m	Grid 2 <b>M3</b> 41.17 dBV/m	Grid 3 <b>M3</b> 41.1 dBV/m
Grid 4 <b>M4</b> 35.83 dBV/m	Grid 5 <b>M4</b> 36.12 dBV/m	Grid 6 <b>M4</b> 36.09 dBV/m
Grid 7 <b>M3</b> 40.81 dBV/m	Grid 8 <b>M3</b> 41.32 dBV/m	Grid 9 <b>M3</b> 41.29 dBV/m

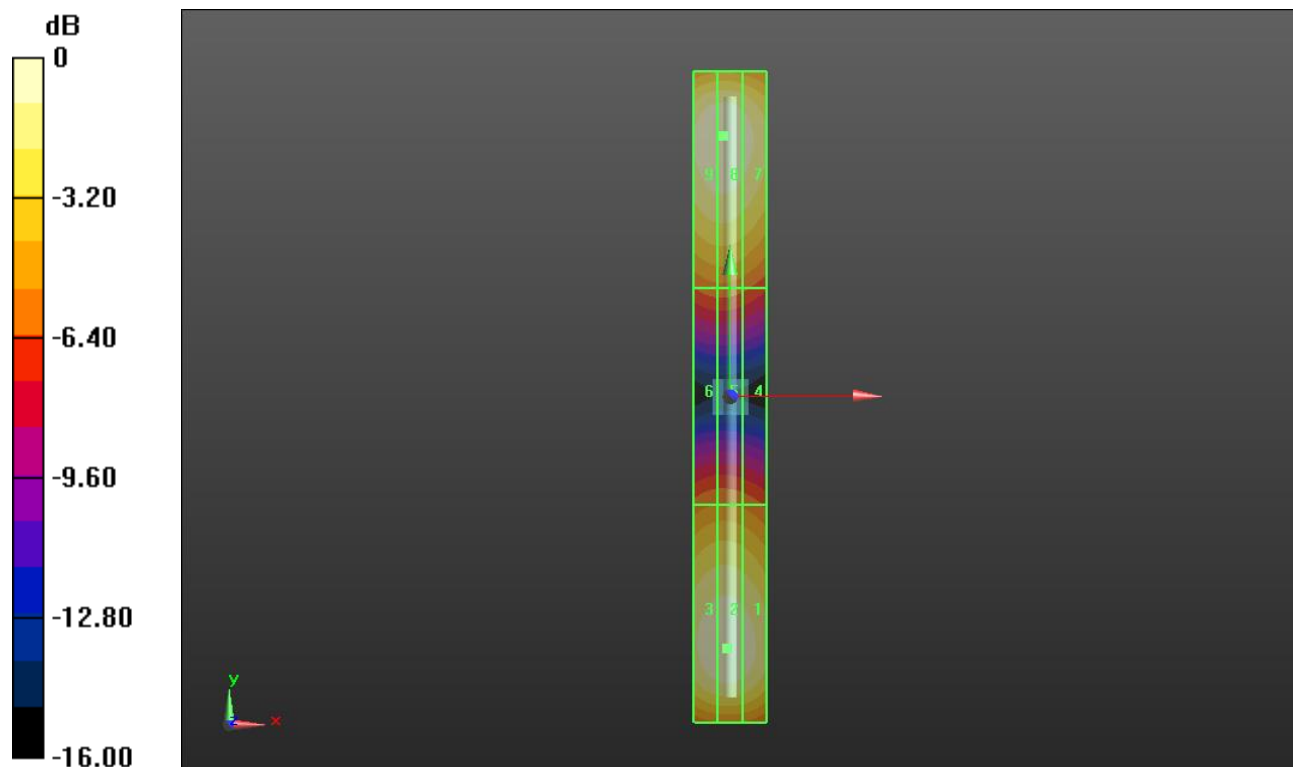

0 dB = 116.4 V/m = 41.32 dBV/m

### HAC-RF Emission System Check

Communication System: UID 0, CW; Frequency: 1880 MHz; Duty Cycle: 1:1  
 Phantom section: RF Section  
 DASY5 Configuration:  
 - Probe: EF3DV3 - SN4041; ConvF(1, 1, 1) @ 1880 MHz; Calibrated: 3/22/2021  
 - Sensor-Surface: (Fix Surface)  
 - Electronics: DAE4 Sn1352; Calibrated: 11/17/2020  
 - Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB  
 - Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

### Dipole E-Field Measurement 1880MHz/1880 MHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1):

Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 137.9 V/m; Power Drift = 0.03 dB


Applied MIF = 0.00 dB

RF audio interference level = 38.54 dBV/m

Emission category: **M2**

MIF scaled E-field

Grid 1 <b>M2</b> 37.57 dBV/m	Grid 2 <b>M2</b> 37.93 dBV/m	Grid 3 <b>M2</b> 37.9 dBV/m
Grid 4 <b>M3</b> 34.26 dBV/m	Grid 5 <b>M3</b> 34.54 dBV/m	Grid 6 <b>M3</b> 34.53 dBV/m
Grid 7 <b>M2</b> 37.97 dBV/m	Grid 8 <b>M2</b> 38.54 dBV/m	Grid 9 <b>M2</b> 38.53 dBV/m

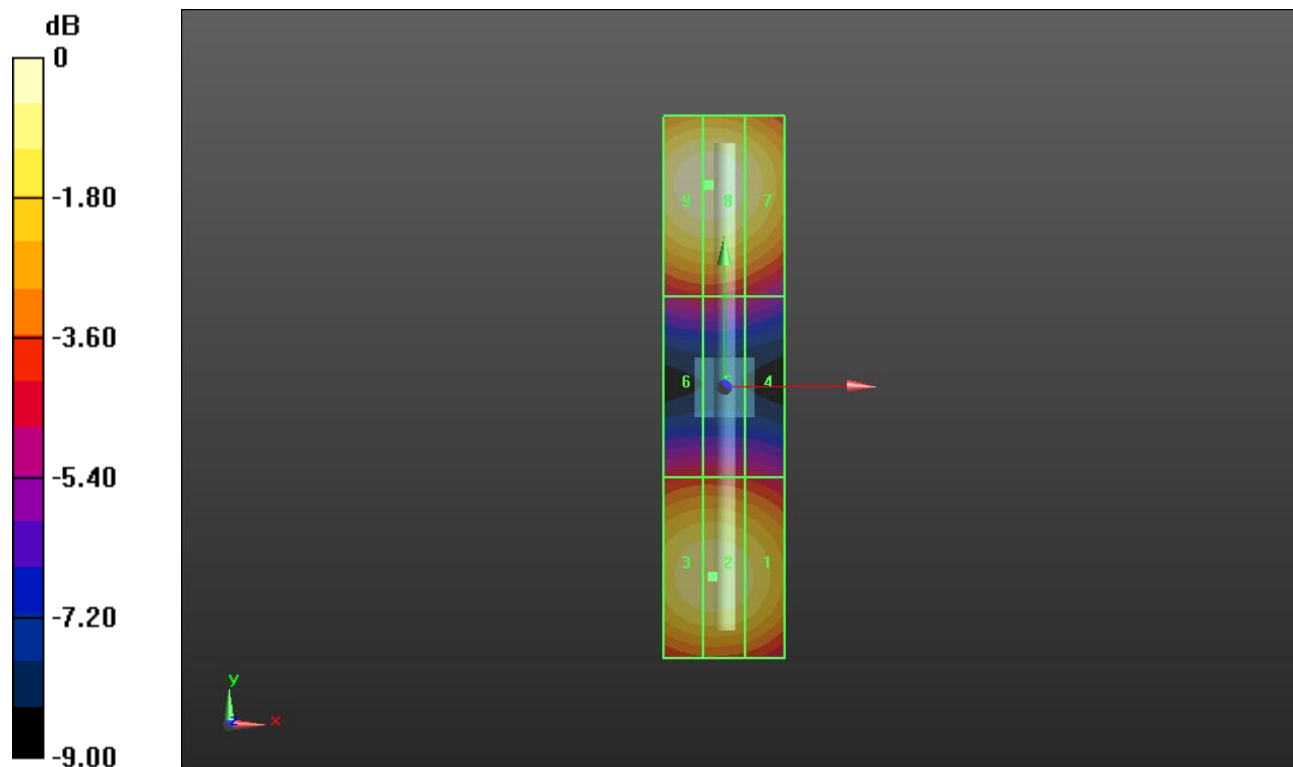

0 dB = 84.57 V/m = 38.54 dBV/m

### HAC-RF Emission System Check

Communication System: UID 0, CW (0); Frequency: 2450 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 2450 MHz; Calibrated: 7/22/2020
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1377; Calibrated: 9/10/2020
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

### Dipole E-Field Measurement 2450MHz/2450 MHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 73.83 V/m; Power Drift = 0.06 dB


Applied MIF = 0.00 dB

RF audio interference level = 39.27 dBV/m

Emission category: **M2**

MIF scaled E-field

Grid 1 <b>M2</b> <b>39.03 dBV/m</b>	Grid 2 <b>M2</b> <b>39.27 dBV/m</b>	Grid 3 <b>M2</b> <b>39.18 dBV/m</b>
Grid 4 <b>M2</b> <b>37.96 dBV/m</b>	Grid 5 <b>M2</b> <b>38.17 dBV/m</b>	Grid 6 <b>M2</b> <b>38.14 dBV/m</b>
Grid 7 <b>M2</b> <b>38.68 dBV/m</b>	Grid 8 <b>M2</b> <b>38.95 dBV/m</b>	Grid 9 <b>M2</b> <b>38.82 dBV/m</b>

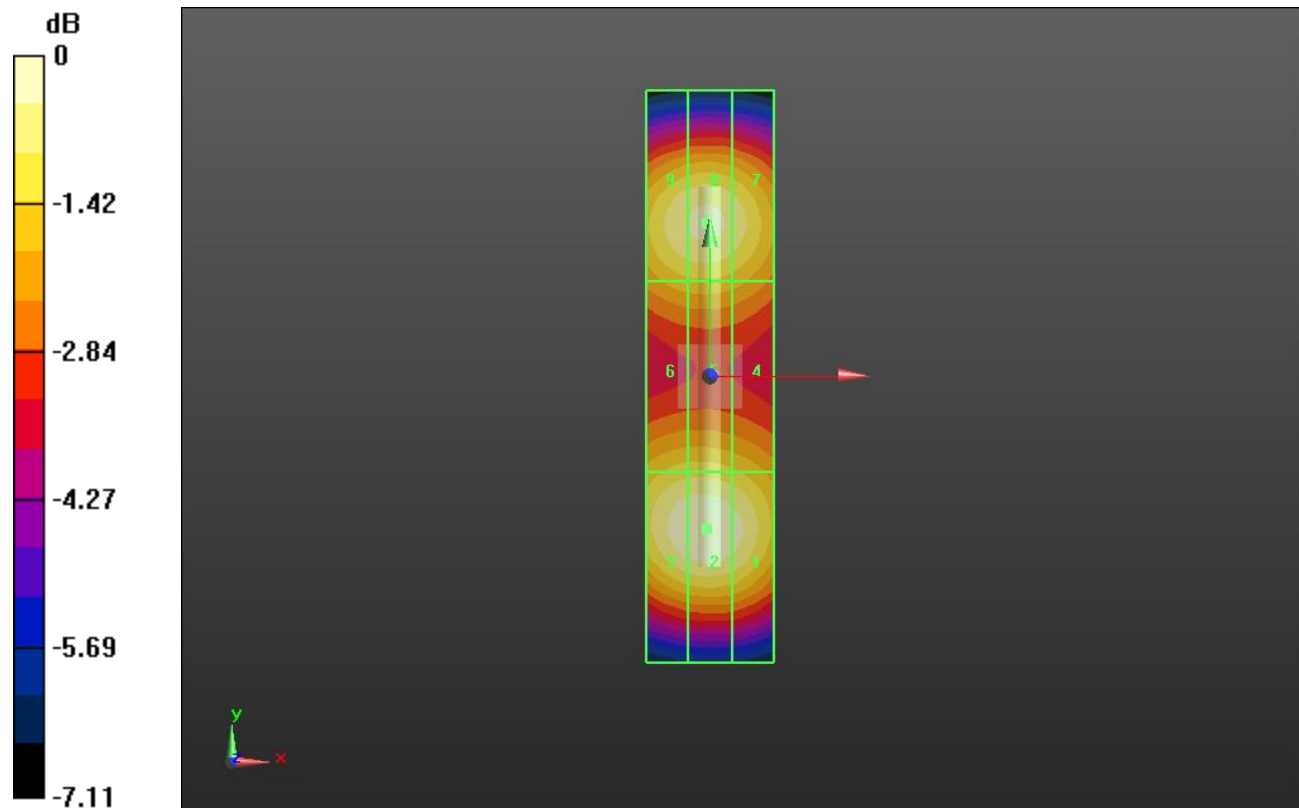

0 dB = 91.93 V/m = 39.27 dBV/m

## HAC-RF Emission System Check

Communication System: UID 0, CW (0); Frequency: 5500 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 5500 MHz; Calibrated: 7/22/2020
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1377; Calibrated: 9/10/2020
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

## Dipole E-Field Measurement 5.5GHz/5.5GHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1):

Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 23.25 V/m; Power Drift = 0.06 dB


Applied MIF = 0.00 dB

RF audio interference level = 40.54 dBV/m

Emission category: **M1**

MIF scaled E-field

Grid 1 <b>M2</b> <b>38.85 dBV/m</b>	Grid 2 <b>M2</b> <b>39 dBV/m</b>	Grid 3 <b>M2</b> <b>38.81 dBV/m</b>
Grid 4 <b>M1</b> <b>40.41 dBV/m</b>	Grid 5 <b>M1</b> <b>40.54 dBV/m</b>	Grid 6 <b>M1</b> <b>40.24 dBV/m</b>
Grid 7 <b>M2</b> <b>38.73 dBV/m</b>	Grid 8 <b>M2</b> <b>38.91 dBV/m</b>	Grid 9 <b>M2</b> <b>38.65 dBV/m</b>

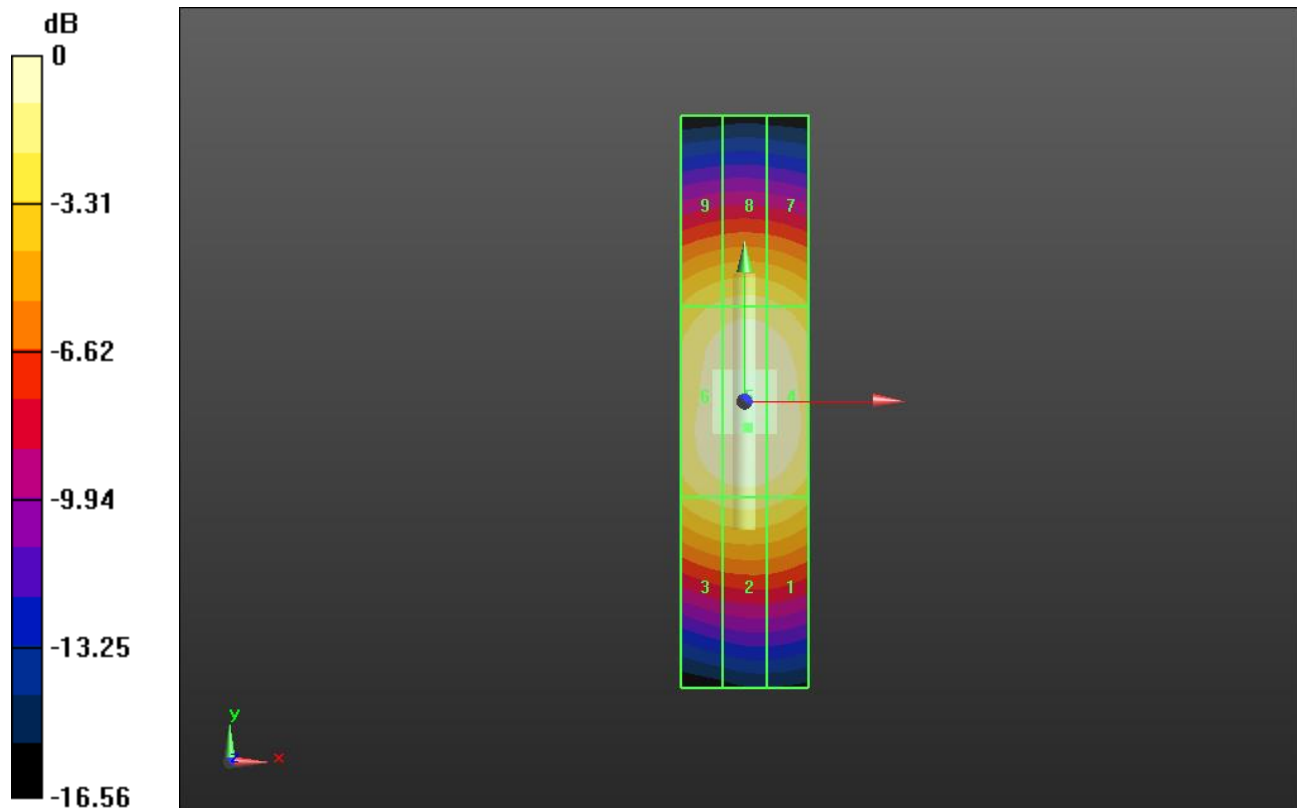

0 dB = 106.4 V/m = 40.54 dBV/m

### HAC-RF Emission System Check

Communication System: UID 0, CW (0); Frequency: 2600 MHz; Duty Cycle: 1:1  
 Phantom section: RF Section  
 DASY5 Configuration:  
 - Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 2600 MHz; Calibrated: 7/22/2020  
 - Sensor-Surface: (Fix Surface)  
 - Electronics: DAE4 Sn1377; Calibrated: 9/10/2020  
 - Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB  
 - Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)


### Dipole E-Field Measurement 2600MHz/2600 MHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1):

Interpolated grid: dx=0.5000 mm, dy=0.5000 mm  
 Device Reference Point: 0, 0, -6.3 mm  
 Reference Value = 70.00 V/m; Power Drift = 0.04 dB  
 Applied MIF = 0.00 dB  
 RF audio interference level = 39.23 dBV/m

Emission category: **M2**

MIF scaled E-field

Grid 1 <b>M2</b> <b>38.93 dBV/m</b>	Grid 2 <b>M2</b> <b>39.2 dBV/m</b>	Grid 3 <b>M2</b> <b>39.14 dBV/m</b>
Grid 4 <b>M2</b> <b>38.33 dBV/m</b>	Grid 5 <b>M2</b> <b>38.55 dBV/m</b>	Grid 6 <b>M2</b> <b>38.52 dBV/m</b>
Grid 7 <b>M2</b> <b>38.88 dBV/m</b>	Grid 8 <b>M2</b> <b>39.23 dBV/m</b>	Grid 9 <b>M2</b> <b>39.17 dBV/m</b>

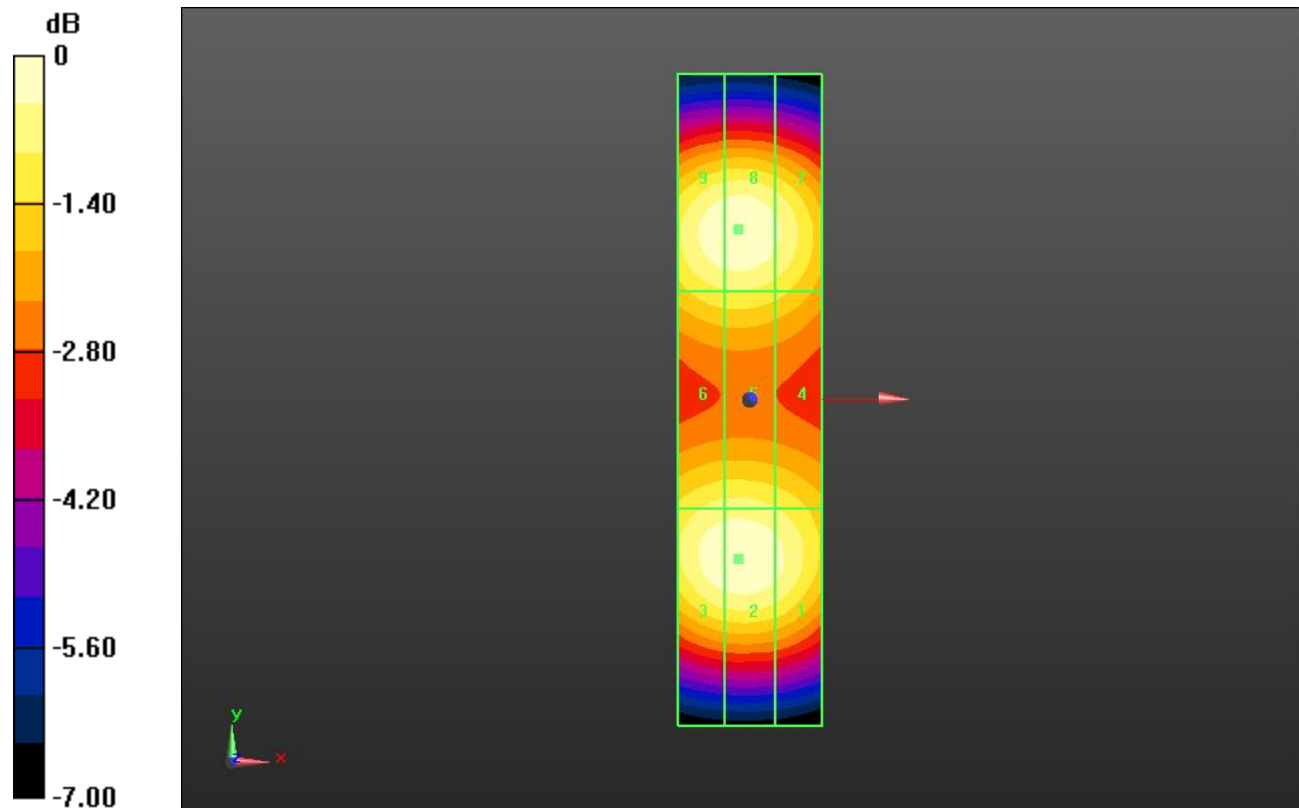

0 dB = 91.56 V/m = 39.23 dBV/m

### HAC-RF Emission System Check

Communication System: UID 0, CW (0); Frequency: 3500 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 3500 MHz; Calibrated: 7/22/2020
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1377; Calibrated: 9/10/2020
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

### Dipole E-Field Measurement 3500MHz/3500 MHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1):

Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 37.39 V/m; Power Drift = -0.01 dB


Applied MIF = 0.00 dB

RF audio interference level = 39.12 dBV/m

Emission category: **M2**

MIF scaled E-field

Grid 1 <b>M2</b> <b>38.58 dBV/m</b>	Grid 2 <b>M2</b> <b>38.85 dBV/m</b>	Grid 3 <b>M2</b> <b>38.82 dBV/m</b>
Grid 4 <b>M2</b> <b>38.77 dBV/m</b>	Grid 5 <b>M2</b> <b>39.1 dBV/m</b>	Grid 6 <b>M2</b> <b>39.05 dBV/m</b>
Grid 7 <b>M2</b> <b>38.77 dBV/m</b>	Grid 8 <b>M2</b> <b>39.12 dBV/m</b>	Grid 9 <b>M2</b> <b>39.06 dBV/m</b>

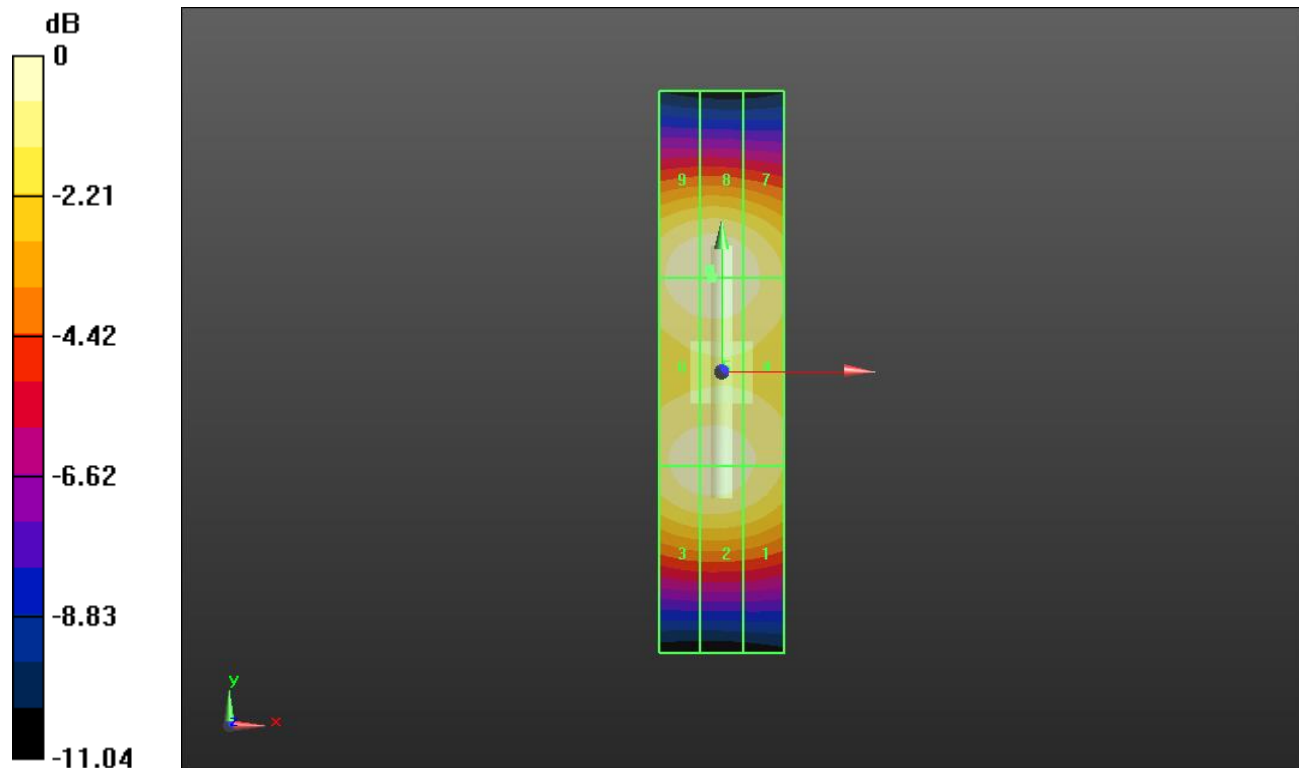

0 dB = 90.37 V/m = 39.12 dBV/m



## HAC-RF Emission System Check

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 835 MHz; Calibrated: 7/22/2020

- Sensor-Surface: (Fix Surface)

- Electronics: DAE4 Sn1377; Calibrated: 9/10/2020

- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB

- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

### Dipole E-Field measurement 835MHz/835 MHz/Hearing Aid Compatibility Test at 15mm distance (41x361x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 134.3 V/m; Power Drift = 0.01 dB


Applied MIF = 0.00 dB

RF audio interference level = 42.02 dBV/m

Emission category: **M3**

MIF scaled E-field

Grid 1 <b>M3</b> 41.16 dBV/m	Grid 2 <b>M3</b> 41.55 dBV/m	Grid 3 <b>M3</b> 41.5 dBV/m
Grid 4 <b>M4</b> 36.04 dBV/m	Grid 5 <b>M4</b> 36.44 dBV/m	Grid 6 <b>M4</b> 36.43 dBV/m
Grid 7 <b>M3</b> 41.54 dBV/m	Grid 8 <b>M3</b> 42.02 dBV/m	Grid 9 <b>M3</b> 42 dBV/m

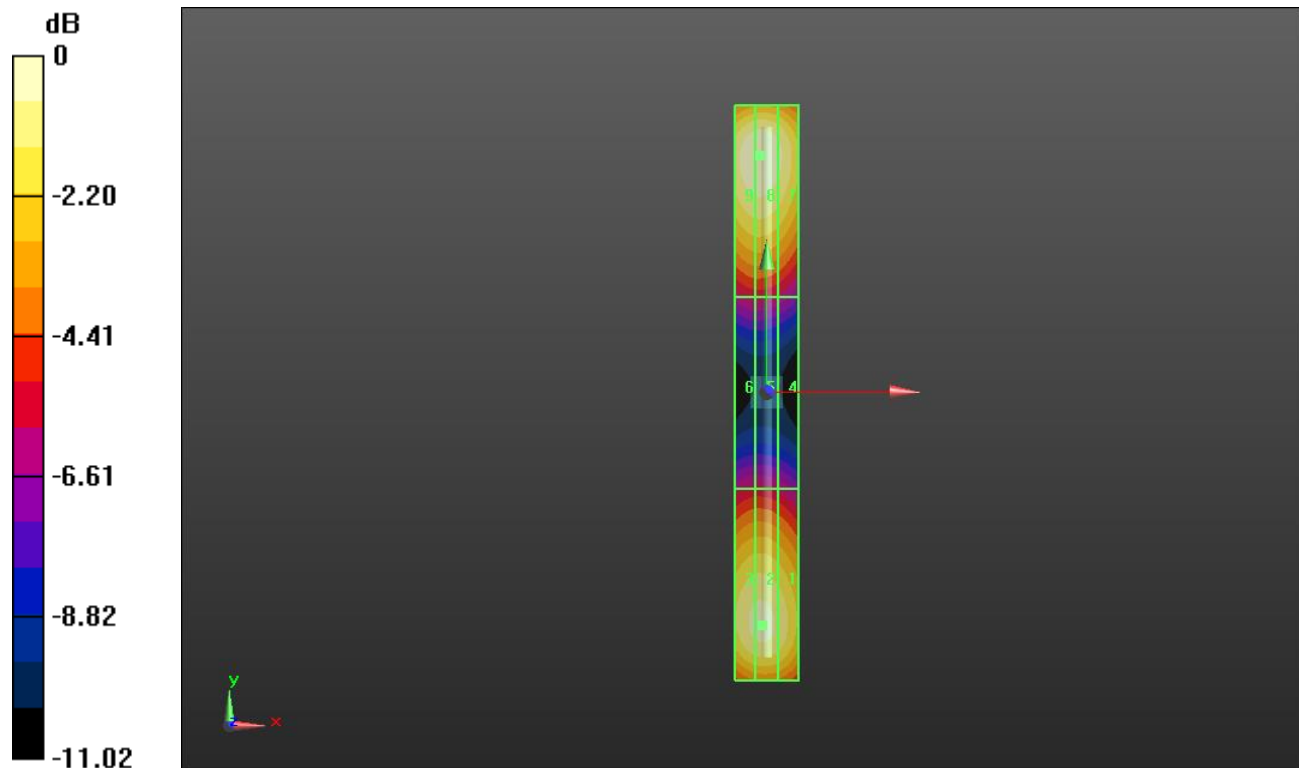

0 dB = 126.2 V/m = 42.02 dBV/m

### HAC-RF Emission System Check

Communication System: UID 0, CW; Frequency: 1880 MHz; Duty Cycle: 1:1  
 Phantom section: RF Section  
 DASY5 Configuration:  
 - Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 1880 MHz; Calibrated: 7/22/2020  
 - Sensor-Surface: (Fix Surface)  
 - Electronics: DAE4 Sn1377; Calibrated: 9/10/2020  
 - Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB  
 - Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

### Dipole E-Field Measurement 1880MHz/1880 MHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1):

Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 156.5 V/m; Power Drift = -0.01 dB


Applied MIF = 0.00 dB

RF audio interference level = 39.46 dBV/m

Emission category: **M2**

MIF scaled E-field

Grid 1 <b>M2</b> <b>39 dBV/m</b>	Grid 2 <b>M2</b> <b>39.35 dBV/m</b>	Grid 3 <b>M2</b> <b>39.32 dBV/m</b>
Grid 4 <b>M2</b> <b>36.21 dBV/m</b>	Grid 5 <b>M2</b> <b>36.42 dBV/m</b>	Grid 6 <b>M2</b> <b>36.42 dBV/m</b>
Grid 7 <b>M2</b> <b>38.98 dBV/m</b>	Grid 8 <b>M2</b> <b>39.46 dBV/m</b>	Grid 9 <b>M2</b> <b>39.44 dBV/m</b>

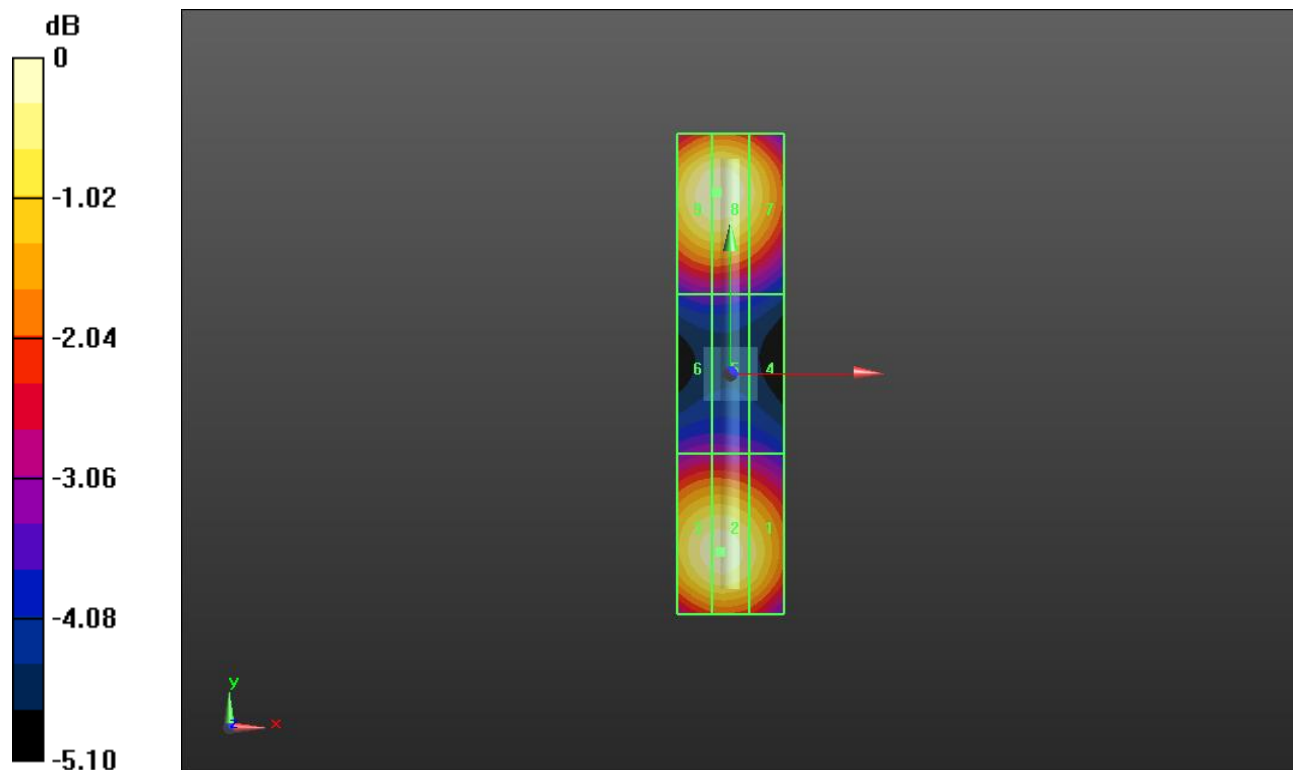

0 dB = 93.97 V/m = 39.46 dBV/m

### HAC-RF Emission System Check

Communication System: UID 0, CW (0); Frequency: 2450 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 2450 MHz; Calibrated: 7/22/2020
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1377; Calibrated: 9/10/2020
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

### Dipole E-Field Measurement 2450MHz/2450 MHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 76.17 V/m; Power Drift = 0.01 dB


Applied MIF = 0.00 dB

RF audio interference level = 39.29 dBV/m

Emission category: **M2**

MIF scaled E-field

Grid 1 <b>M2</b> <b>38.73 dBV/m</b>	Grid 2 <b>M2</b> <b>39.09 dBV/m</b>	Grid 3 <b>M2</b> <b>39.06 dBV/m</b>
Grid 4 <b>M2</b> <b>37.78 dBV/m</b>	Grid 5 <b>M2</b> <b>38.07 dBV/m</b>	Grid 6 <b>M2</b> <b>38.06 dBV/m</b>
Grid 7 <b>M2</b> <b>38.88 dBV/m</b>	Grid 8 <b>M2</b> <b>39.29 dBV/m</b>	Grid 9 <b>M2</b> <b>39.24 dBV/m</b>

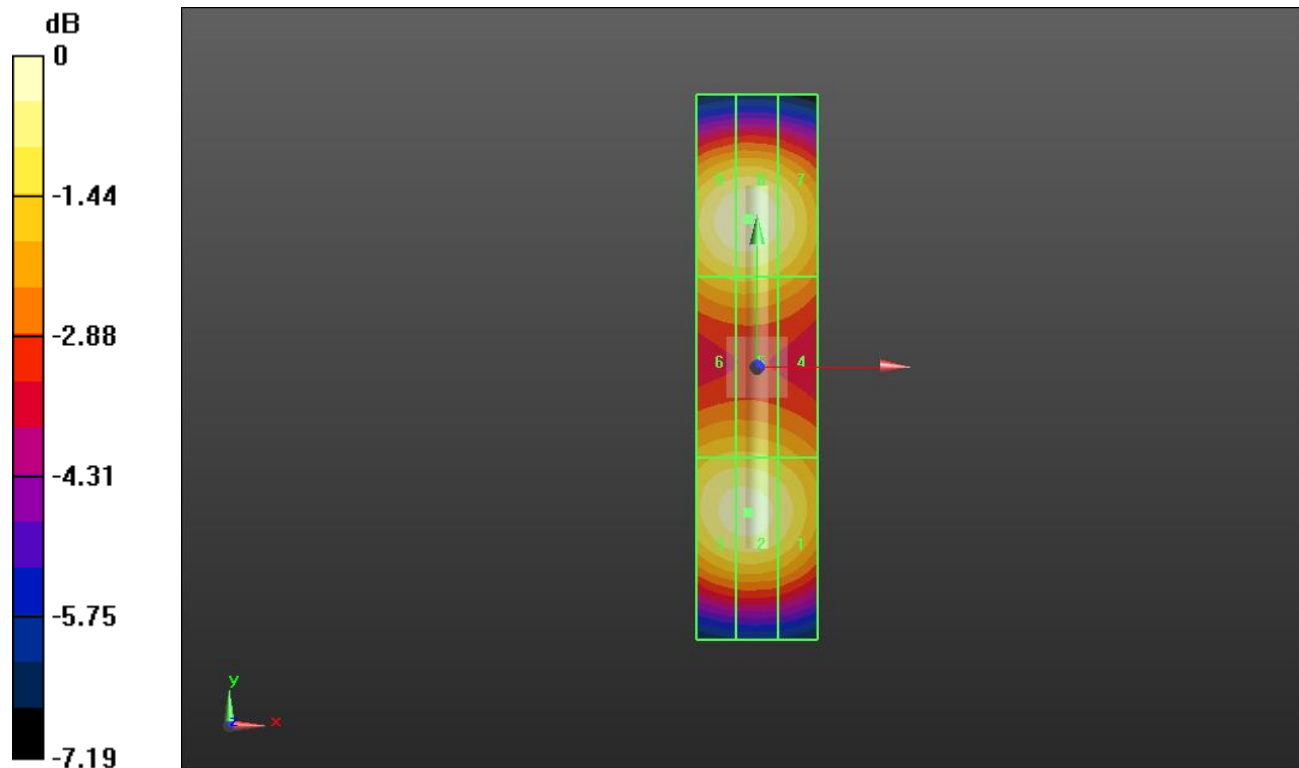

0 dB = 92.18 V/m = 39.29 dBV/m

## HAC-RF Emission System Check

Communication System: UID 0, CW (0); Frequency: 5500 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 5500 MHz; Calibrated: 7/22/2020
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1377; Calibrated: 9/10/2020
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

## Dipole E-Field Measurement 5.5GHz/5.5GHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 23.80 V/m; Power Drift = 0.04 dB


Applied MIF = 0.00 dB

RF audio interference level = 40.50 dBV/m

Emission category: **M1**

MIF scaled E-field

Grid 1 <b>M2</b> <b>38.67 dBV/m</b>	Grid 2 <b>M2</b> <b>38.93 dBV/m</b>	Grid 3 <b>M2</b> <b>38.83 dBV/m</b>
Grid 4 <b>M1</b> <b>40.27 dBV/m</b>	Grid 5 <b>M1</b> <b>40.5 dBV/m</b>	Grid 6 <b>M1</b> <b>40.32 dBV/m</b>
Grid 7 <b>M2</b> <b>38.59 dBV/m</b>	Grid 8 <b>M2</b> <b>38.9 dBV/m</b>	Grid 9 <b>M2</b> <b>38.75 dBV/m</b>

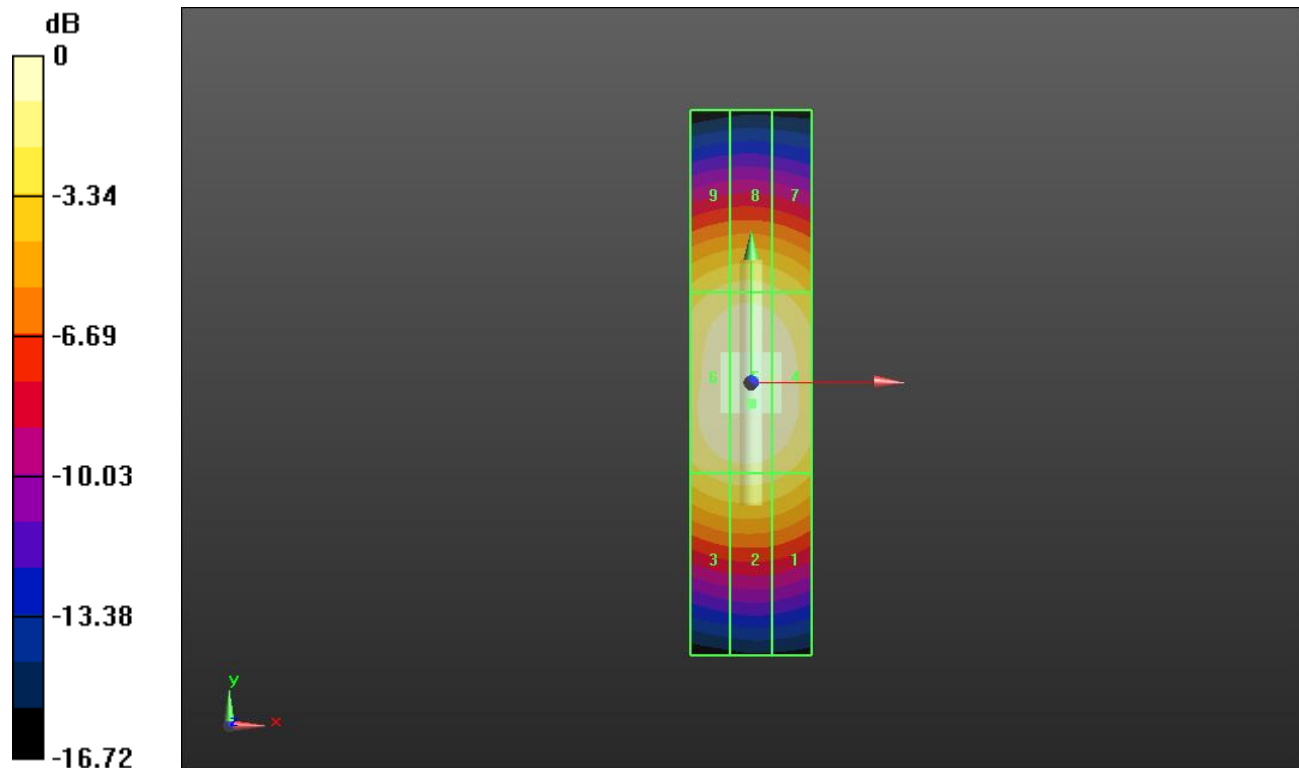

0 dB = 105.9 V/m = 40.50 dBV/m

### HAC-RF Emission System Check

Communication System: UID 0, CW (0); Frequency: 2450 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 2450 MHz; Calibrated: 7/22/2020
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1377; Calibrated: 9/10/2020
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

### Dipole E-Field Measurement 2450MHz/2450 MHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 75.58 V/m; Power Drift = 0.05 dB



Applied MIF = 0.00 dB

RF audio interference level = 39.25 dBV/m

Emission category: **M2**

MIF scaled E-field

Grid 1 <b>M2</b> <b>38.89 dBV/m</b>	Grid 2 <b>M2</b> <b>39.25 dBV/m</b>	Grid 3 <b>M2</b> <b>39.23 dBV/m</b>
Grid 4 <b>M2</b> <b>37.94 dBV/m</b>	Grid 5 <b>M2</b> <b>38.23 dBV/m</b>	Grid 6 <b>M2</b> <b>38.23 dBV/m</b>
Grid 7 <b>M2</b> <b>38.5 dBV/m</b>	Grid 8 <b>M2</b> <b>38.88 dBV/m</b>	Grid 9 <b>M2</b> <b>38.83 dBV/m</b>

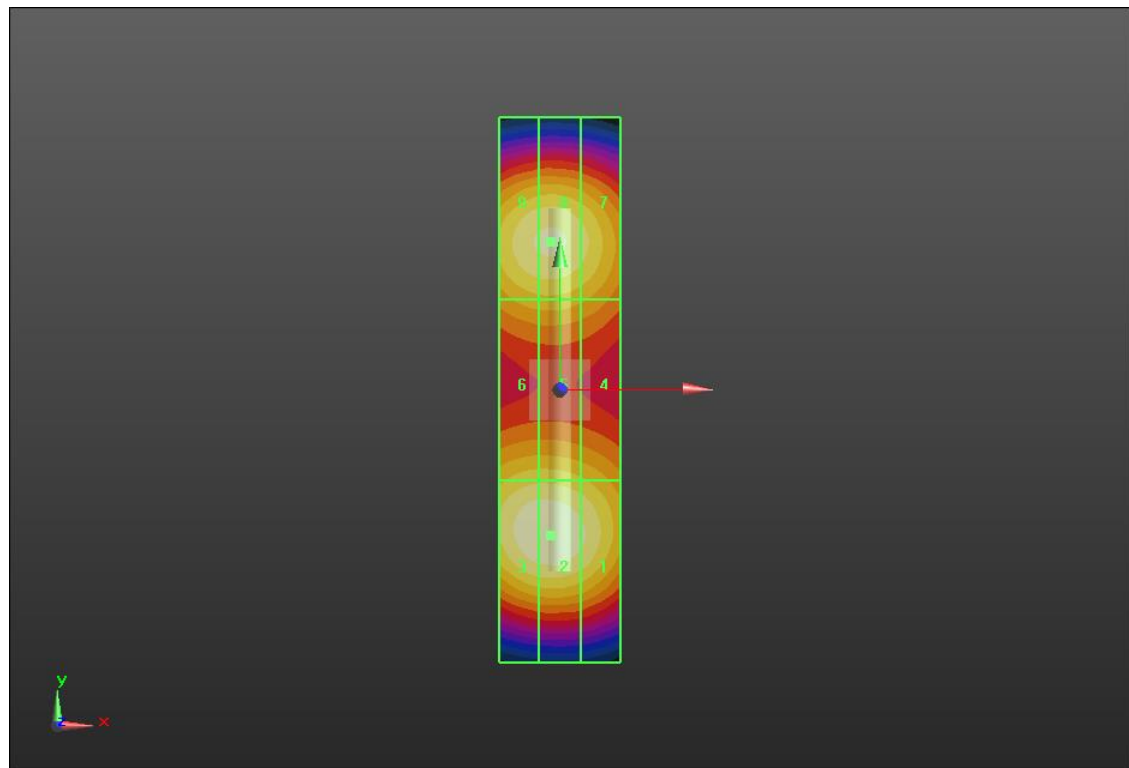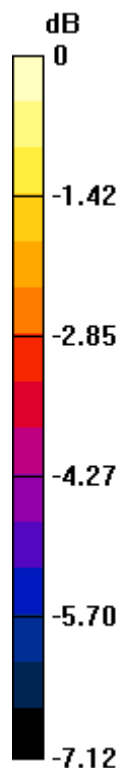

0 dB = 91.77 V/m = 39.25 dBV/m

### HAC-RF Emission System Check

Communication System: UID 0, CW (0); Frequency: 5500 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 5500 MHz; Calibrated: 7/22/2020
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1377; Calibrated: 9/10/2020
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

### Dipole E-Field Measurement 5.5GHz/5.5GHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 24.15 V/m; Power Drift = 0.06 dB


Applied MIF = 0.00 dB

RF audio interference level = 40.56 dBV/m

Emission category: **M1**

MIF scaled E-field

Grid 1 <b>M2</b> <b>38.7 dBV/m</b>	Grid 2 <b>M2</b> <b>38.95 dBV/m</b>	Grid 3 <b>M2</b> <b>38.85 dBV/m</b>
Grid 4 <b>M1</b> <b>40.33 dBV/m</b>	Grid 5 <b>M1</b> <b>40.56 dBV/m</b>	Grid 6 <b>M1</b> <b>40.38 dBV/m</b>
Grid 7 <b>M2</b> <b>38.7 dBV/m</b>	Grid 8 <b>M2</b> <b>39 dBV/m</b>	Grid 9 <b>M2</b> <b>38.85 dBV/m</b>

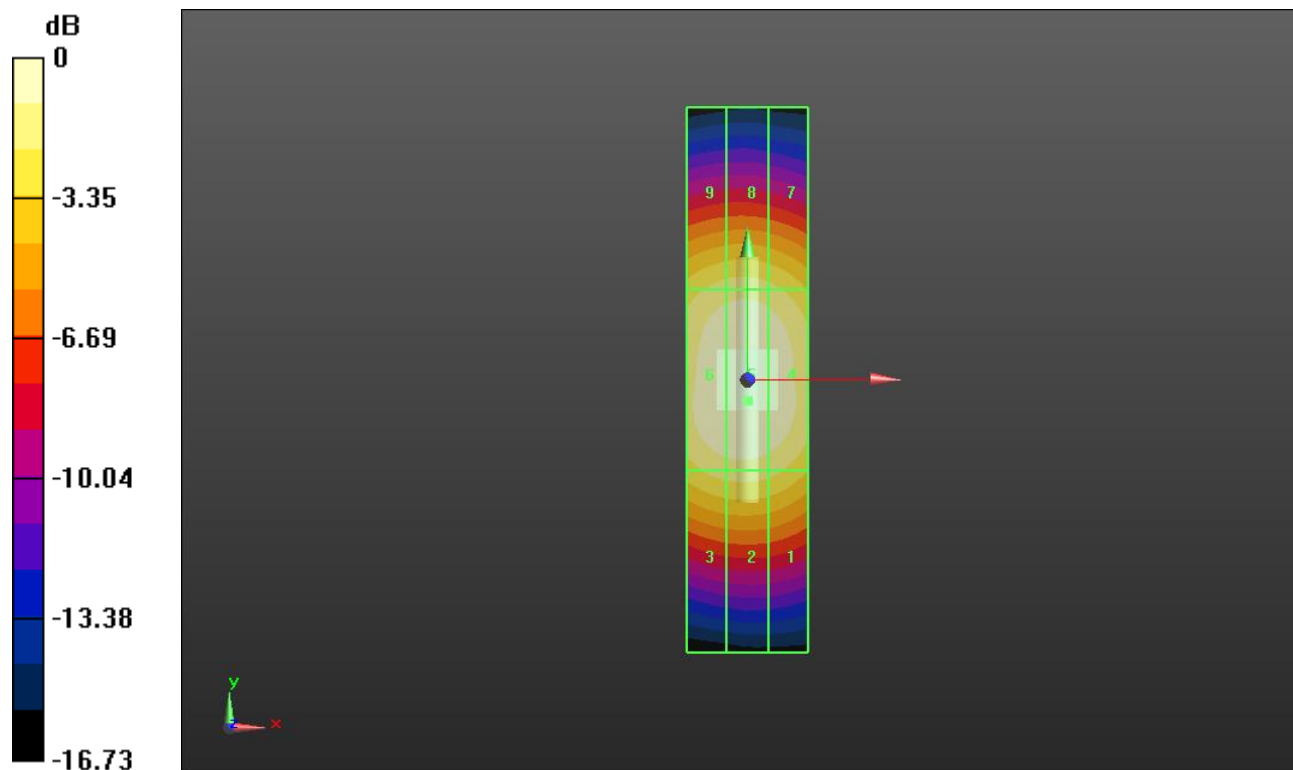

0 dB = 106.6 V/m = 40.56 dBV/m