

APPENDIX B: SAR DIPOLE VERIFICATION PLOTS

ELEMENT

DUT: Dipole 13.0 MHz; Type: CLA-13 - SN1004

Communication System: UID: 0, CW; Frequency: 13.0 MHz
Medium: 30 Head; Medium parameters used:
f = 13.0 MHz; cond = 0.727 S/m; perm = 53.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 0 mm

Test Date: 02/14/2024; Ambient Temp: 22.6°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7360; ConvF:(17.98,17.98,17.98); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (All points)
Electronics: DAE4 Sn534; Calibrated: 2023-03-15
Phantom: ELI V6.0; Serial: 2044
Measurement SW: DASY Module SAR V16.2.0.1425

13.0 MHz System Verification at 30.0 dBm (1000 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 1.10 W/kg

SAR(1 g) = 0.552 W/kg

Deviation (1 g) = -4.50%

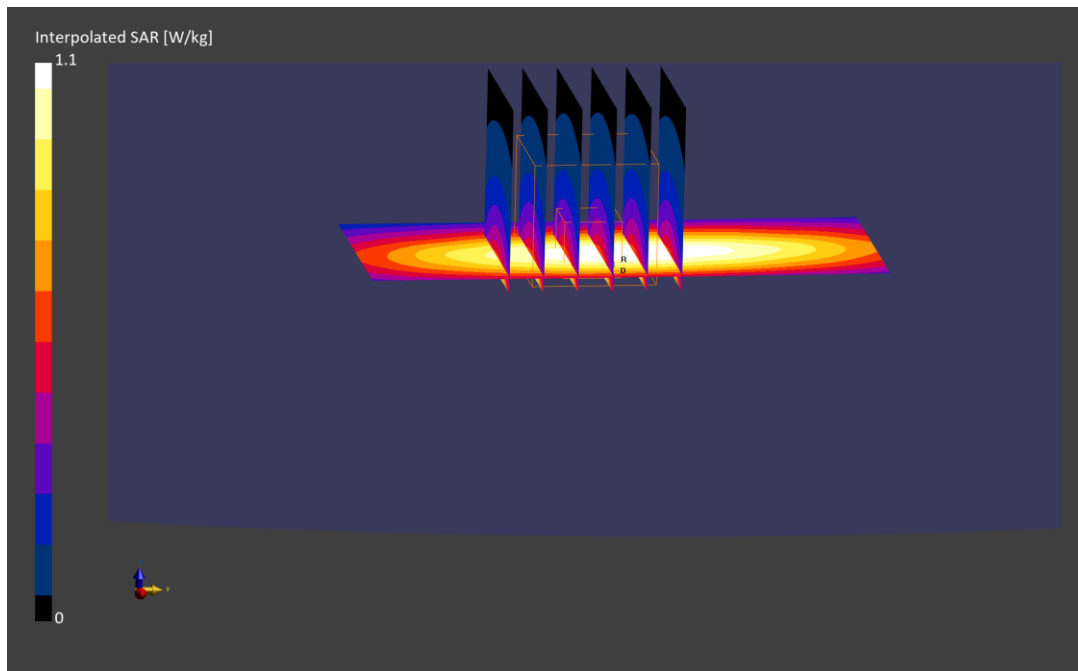

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1097

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.869 S/m; perm = 43.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/12/2024; Ambient Temp: 21.2°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN3949; ConvF:(10.55,10.55,10.55); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.66 W/kg

SAR(1 g) = 1.72 W/kg

Deviation (1 g) = 3.99%

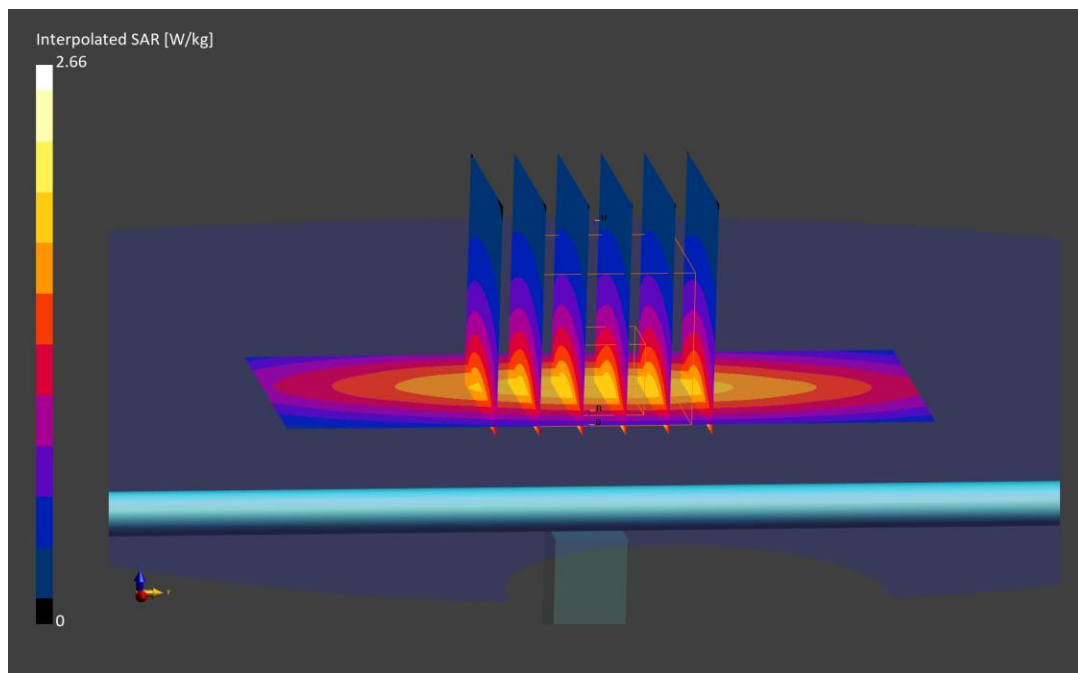

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1057

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.909 S/m; perm = 40.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/12/2024; Ambient Temp: 23.1°C; Tissue Temp: 23.4°C

Probe: EX3DV4 - SN7357; ConvF:(9.9,9.9,9.9); Calibrated: 2023-04-13
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1582; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 1866
Measurement SW: DASY Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.52 W/kg

SAR(1 g) = 1.69 W/kg

Deviation (1 g) = -0.71%

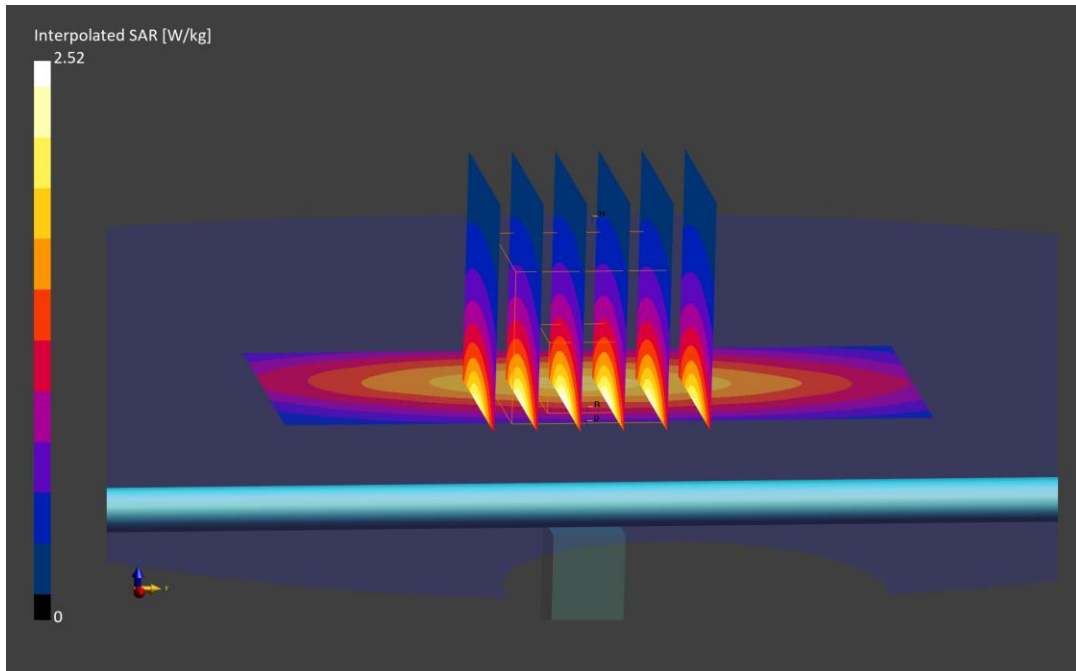

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1057

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.879 S/m; perm = 41.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/14/2024; Ambient Temp: 22.9°C; Tissue Temp: 23.0°C

Probe: EX3DV4 - SN7357; ConvF:(9.9,9.9,9.9); Calibrated: 2023-04-13
Sensor-Surface: 1.4mm (All points)
Electronics: DAE4 Sn1582; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 1866
Measurement SW: DASY Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.39 W/kg

SAR(1 g) = 1.65 W/kg

Deviation (1 g) = -3.06%

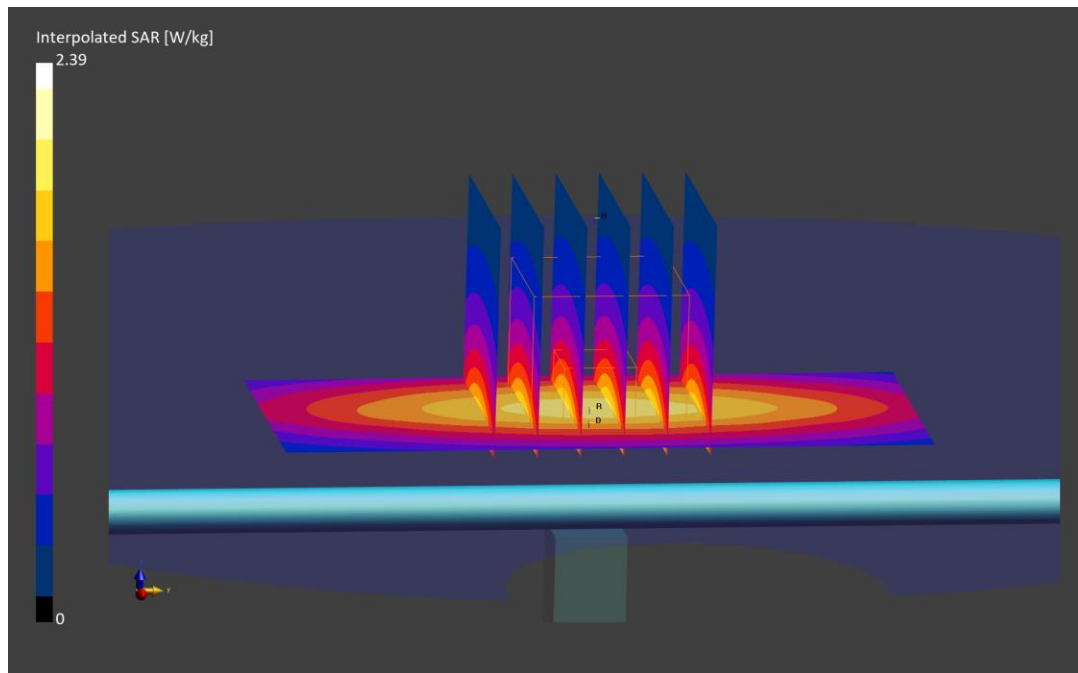

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1097

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.877 S/m; perm = 42.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/16/2024; Ambient Temp: 21.1°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN3949; ConvF:(10.55,10.55,10.55); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.53 W/kg

SAR(1 g) = 1.62 W/kg

Deviation (1 g) = -2.06%

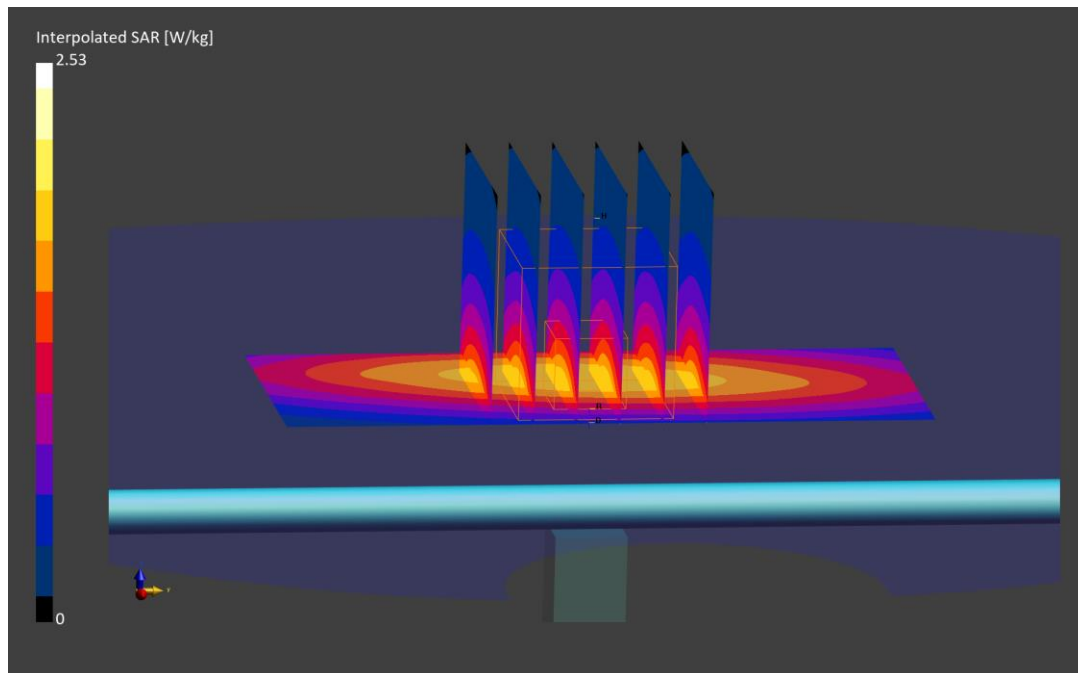

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1057

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.880 S/m; perm = 40.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/16/2024; Ambient Temp: 21.5°C; Tissue Temp: 23.4°C

Probe: EX3DV4 - SN7357; ConvF:(9.9,9.9,9.9); Calibrated: 2023-04-13
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1582; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 1866
Measurement SW: DASY Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.51 W/kg

SAR(1 g) = 1.73 W/kg

Deviation (1 g) = 1.65%

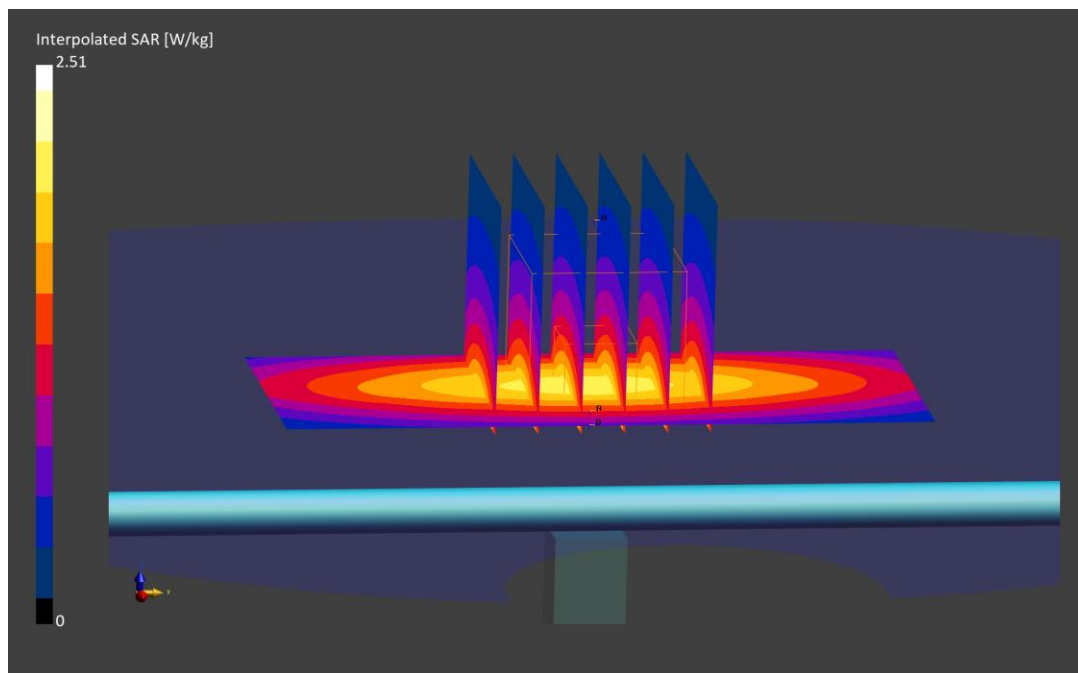

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1057

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.879 S/m; perm = 41.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 02/09/2024; Ambient Temp: 20.9°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN7357; ConvF:(9.9,9.9,9.9); Calibrated: 2023-04-13
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1582; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 1866
Measurement SW: DASYS Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.43 W/kg

SAR(1 g) = 1.63 W/kg

Deviation (1 g) = -4.23%

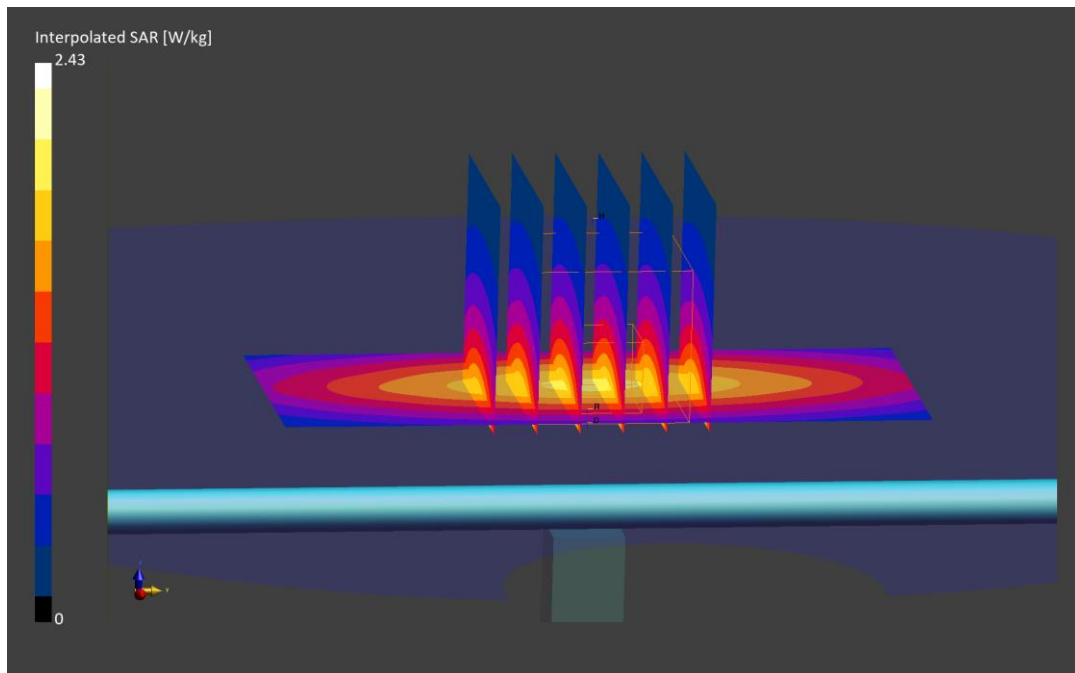

ELEMENT

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d108

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Head; Medium parameters used:
f = 835.0 MHz; cond = 0.888 S/m; perm = 40.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/16/2024; Ambient Temp: 20.6°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7416; ConvF:(9.73,9.73,9.73); Calibrated: 2023-05-08
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn701; Calibrated: 2023-05-11
Phantom: Twin-SAM V8.0; Serial: 2029
Measurement SW: DASY Module SAR V16.2.0.1425

835.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.86 W/kg

SAR(1 g) = 1.85 W/kg

Deviation (1 g) = -5.61%

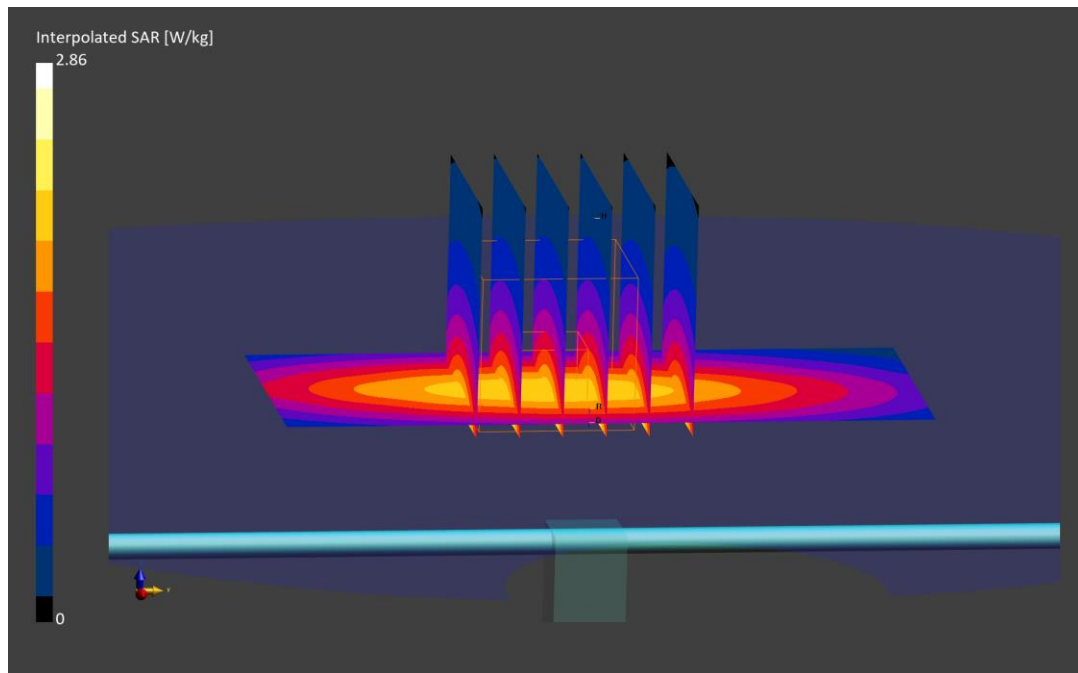

ELEMENT

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d040

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Head; Medium parameters used:
f = 835.0 MHz; cond = 0.894 S/m; perm = 41.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/18/2024; Ambient Temp: 20.5°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7416; ConvF:(9.73,9.73,9.73); Calibrated: 2023-05-08
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn701; Calibrated: 2023-05-11
Phantom: Twin-SAM V8.0; Serial: 2029
Measurement SW: DASY Module SAR V16.2.0.1425

835.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.98 W/kg

SAR(1 g) = 1.90 W/kg

Deviation (1 g) = -2.96%

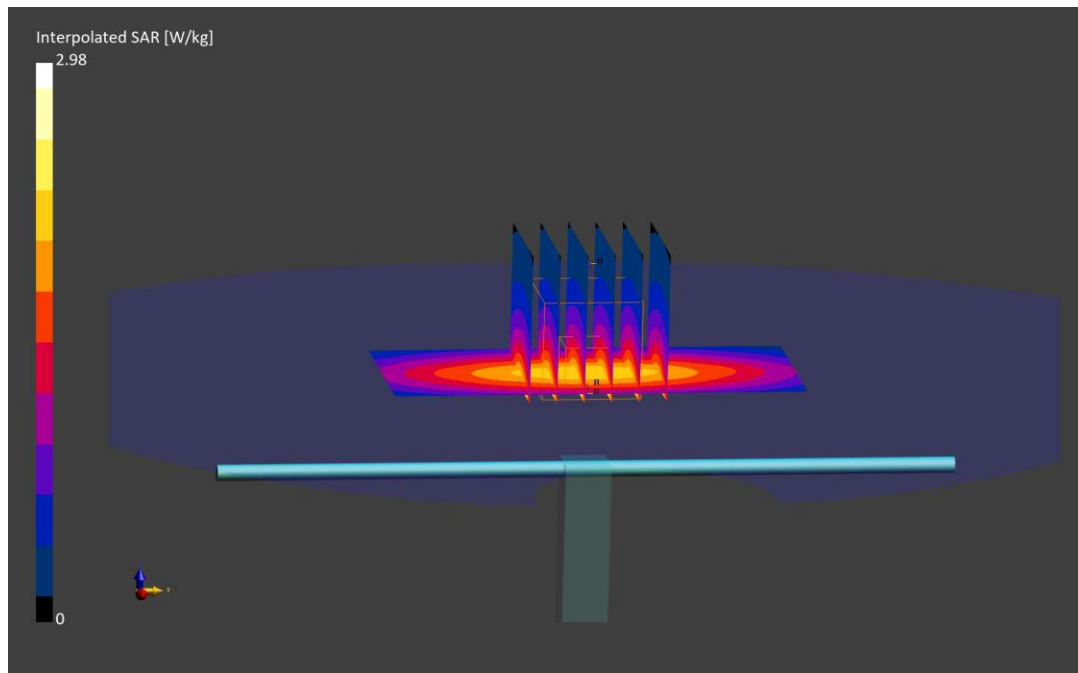

ELEMENT

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d108

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Head; Medium parameters used:
f = 835.0 MHz; cond = 0.900 S/m; perm = 41.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/20/2024; Ambient Temp: 22.3°C; Tissue Temp: 19.7°C

Probe: EX3DV4 - SN7416; ConvF:(9.73,9.73,9.73); Calibrated: 2023-05-08
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn701; Calibrated: 2023-05-11
Phantom: Twin-SAM V8.0; Serial: 2029
Measurement SW: DASY Module SAR V16.2.0.1425

835.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.95 W/kg

SAR(1 g) = 1.88 W/kg

Deviation (1 g) = -3.98%

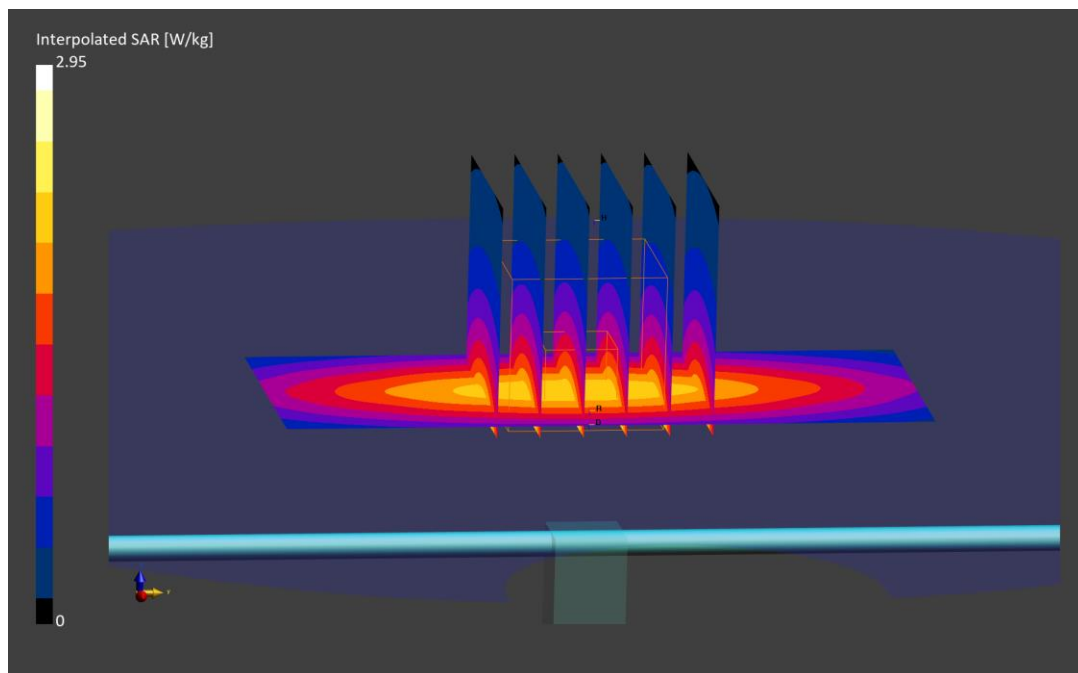

ELEMENT

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d040

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Head; Medium parameters used:
f = 835.0 MHz; cond = 0.900 S/m; perm = 41.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/21/2024; Ambient Temp: 21.2°C; Tissue Temp: 20.3°C

Probe: EX3DV4 - SN7416; ConvF:(9.73,9.73,9.73); Calibrated: 2023-05-08
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn701; Calibrated: 2023-05-11
Phantom: Twin-SAM V8.0; Serial: 2029
Measurement SW: DASY Module SAR V16.2.0.1425

835.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.07 W/kg

SAR(1 g) = 1.96 W/kg

Deviation (1 g) = 0.10%

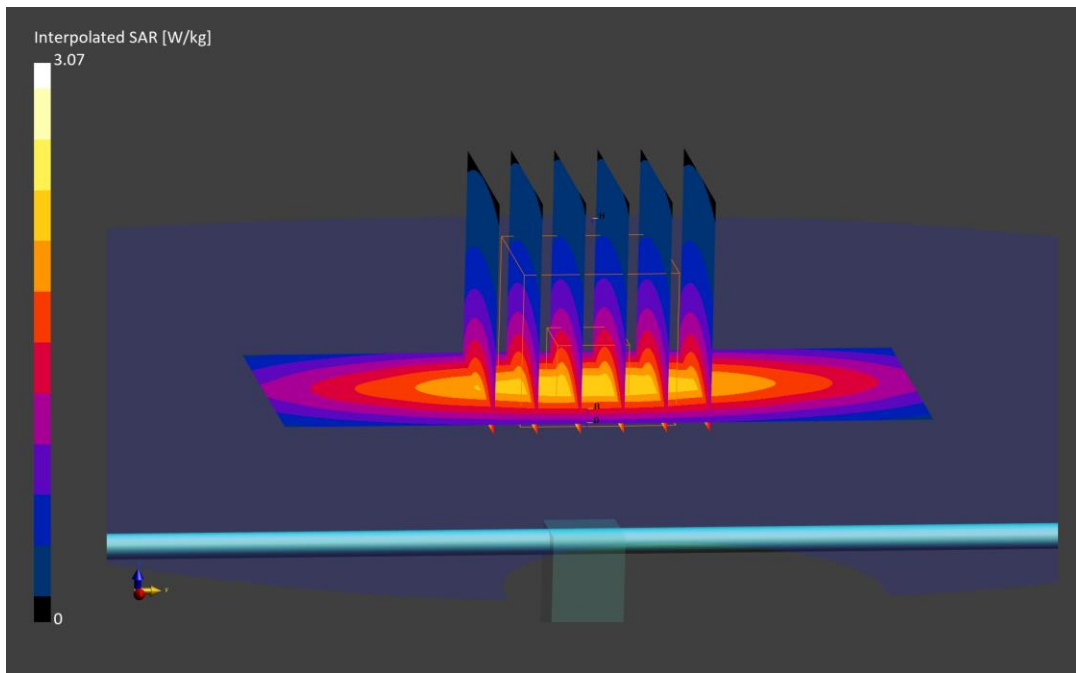

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1040

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.38 S/m; perm = 38.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/09/2024; Ambient Temp: 20.3°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN7360; ConvF:(9.15,9.15,9.15); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn534; Calibrated: 2023-03-15
Phantom: Twin-SAM V4.0; Serial: 1447
Measurement SW: DASY Module SAR V16.2.0.1425

1750.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.26 W/kg

SAR(1 g) = 3.70 W/kg

Deviation (1 g) = 1.65%

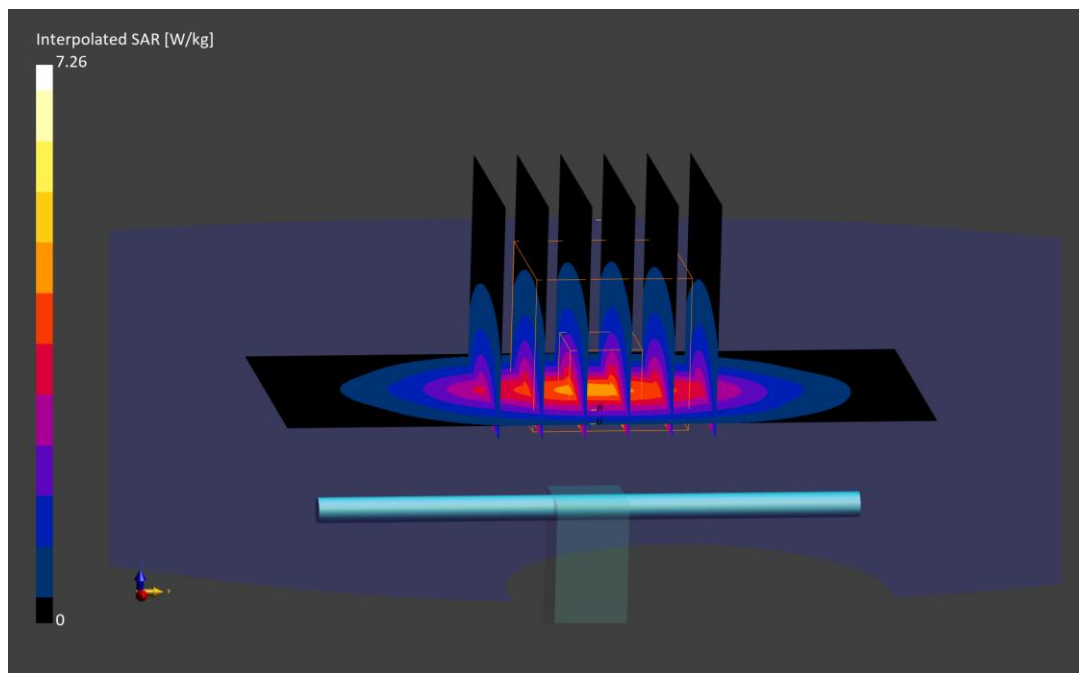

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1083

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.38 S/m; perm = 38.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/11/2024; Ambient Temp: 22.0°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7360; ConvF:(9.15,9.15,9.15); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn534; Calibrated: 2023-03-15
Phantom: Twin-SAM V4.0; Serial: 1447
Measurement SW: DASY Module SAR V16.2.0.1425

1750.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.57 W/kg

SAR(1 g) = 3.40 W/kg

Deviation (1 g) = -6.85%

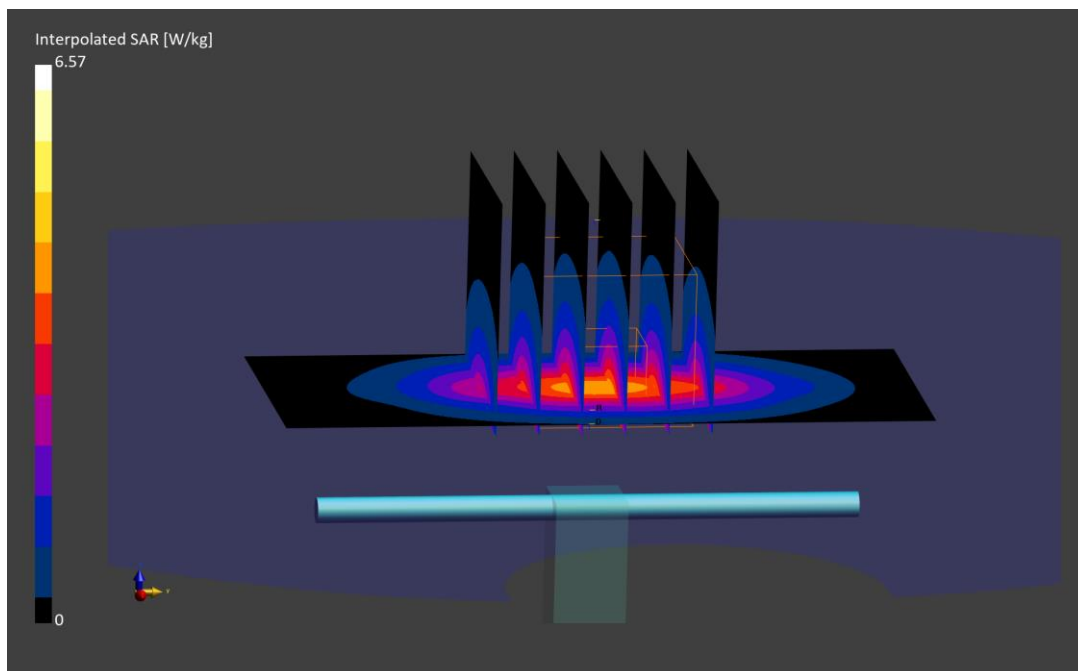

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1040

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.39 S/m; perm = 38.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/14/2024; Ambient Temp: 21.3°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN7639; ConvF:(8.98,8.98,8.98); Calibrated: 2023-11-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1403; Calibrated: 2023-11-14
Phantom: Twin-SAM V8.0; Serial: 2034
Measurement SW: DASY Module SAR V16.2.0.1425

1750.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.92 W/kg

SAR(1 g) = 3.76 W/kg

Deviation (1 g) = 3.30%

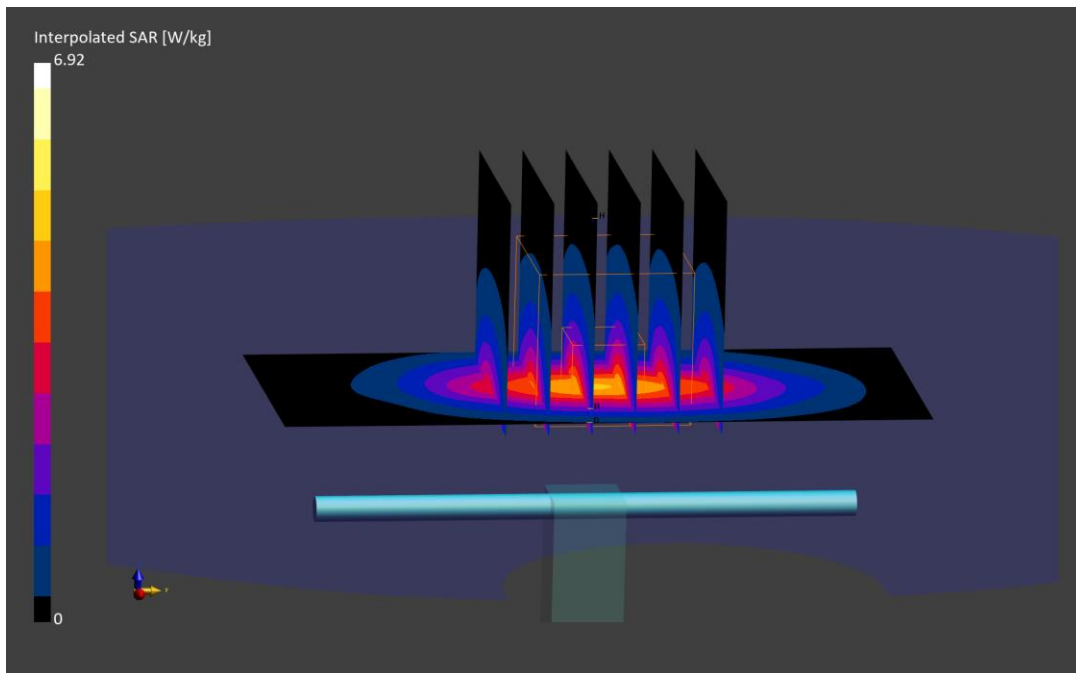

ELEMENT

DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d030

Communication System: UID: 0, CW; Frequency: 1900.0 MHz
Medium: 1900 Head; Medium parameters used:
f = 1900.0 MHz; cond = 1.42 S/m; perm = 38.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/12/2024; Ambient Temp: 19.1°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7668; ConvF:(8.0,8.0,8.0); Calibrated: 2023-08-10
Sensor-Surface: 1.4mm (All points)
Electronics: DAE4 Sn1681; Calibrated: 2023-09-12
Phantom: Twin-SAM V5.0 ; Serial: 1692
Measurement SW: DASY Module SAR V16.2.0.1425

1900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.90 W/kg

SAR(1 g) = 3.96 W/kg

Deviation (1 g) = -0.50%

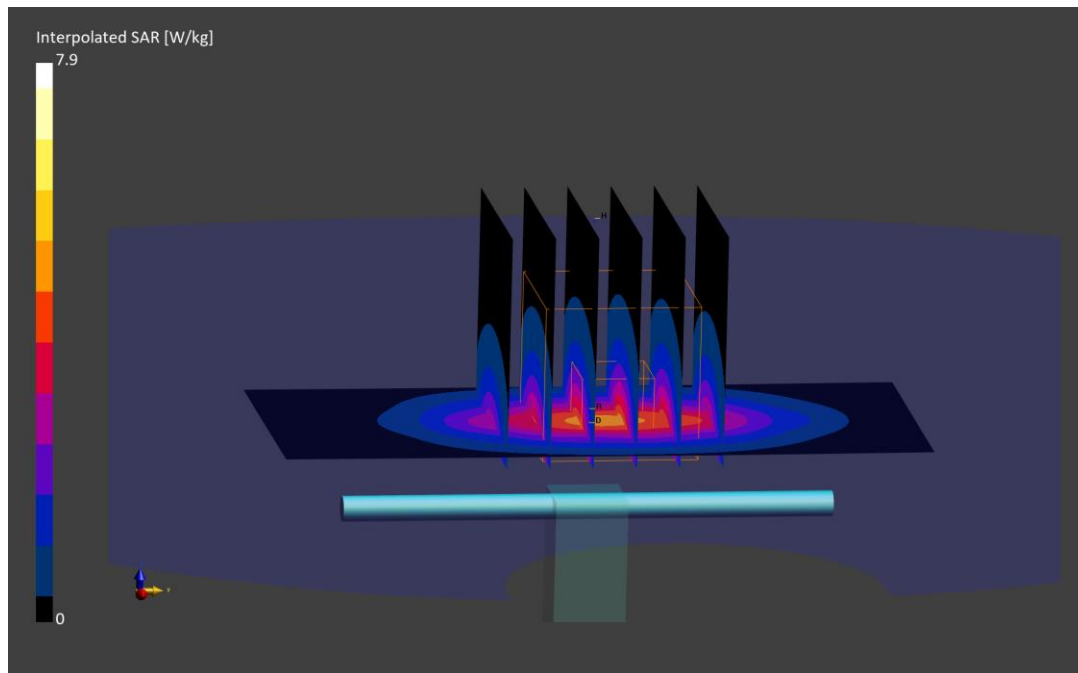

ELEMENT

DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d030

Communication System: UID: 0, CW; Frequency: 1900.0 MHz
Medium: 1900 Head; Medium parameters used:
f = 1900.0 MHz; cond = 1.44 S/m; perm = 38.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/16/2024; Ambient Temp: 20.7°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7668; ConvF:(8.0,8.0,8.0); Calibrated: 2023-08-10
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2023-09-12
Phantom: Twin-SAM V5.0 ; Serial: 1692
Measurement SW: DASY Module SAR V16.2.0.1425

1900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.55 W/kg

SAR(1 g) = 3.76 W/kg

Deviation (1 g) = -5.53%

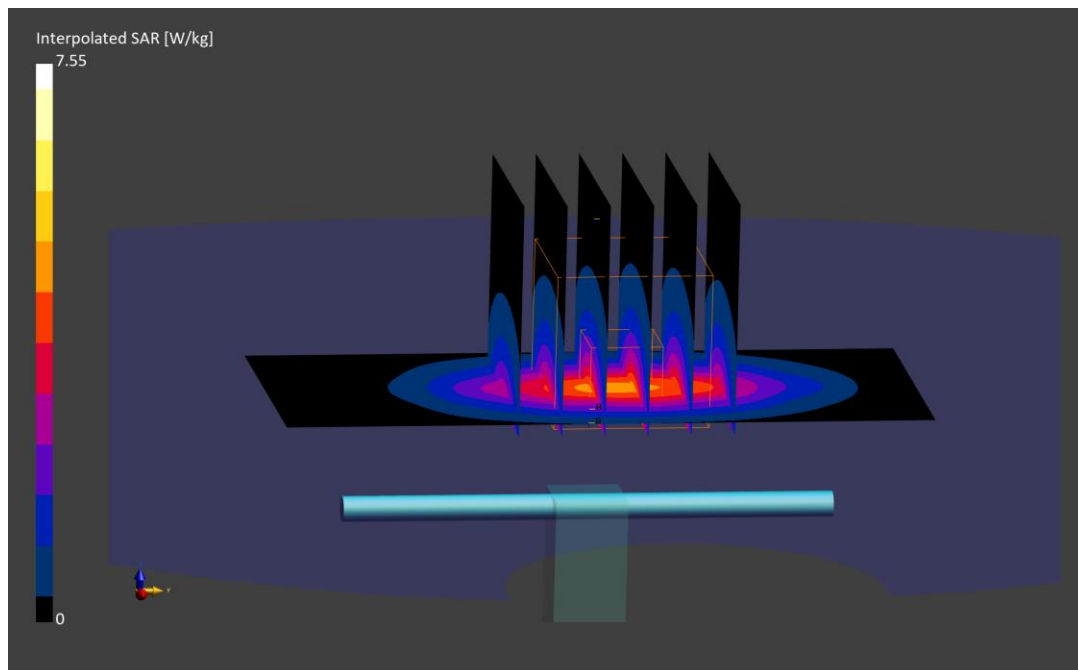

ELEMENT

DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d030

Communication System: UID: 0, CW; Frequency: 1900.0 MHz
Medium: 1900 Head; Medium parameters used:
f = 1900.0 MHz; cond = 1.41 S/m; perm = 38.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/18/2024; Ambient Temp: 21.7°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7668; ConvF:(8.0,8.0,8.0); Calibrated: 2023-08-10
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2023-09-12
Phantom: Twin-SAM V5.0 ; Serial: 1692
Measurement SW: DASY Module SAR V16.2.0.1425

1900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.37 W/kg

SAR(1 g) = 3.71 W/kg

Deviation (1 g) = -6.78%

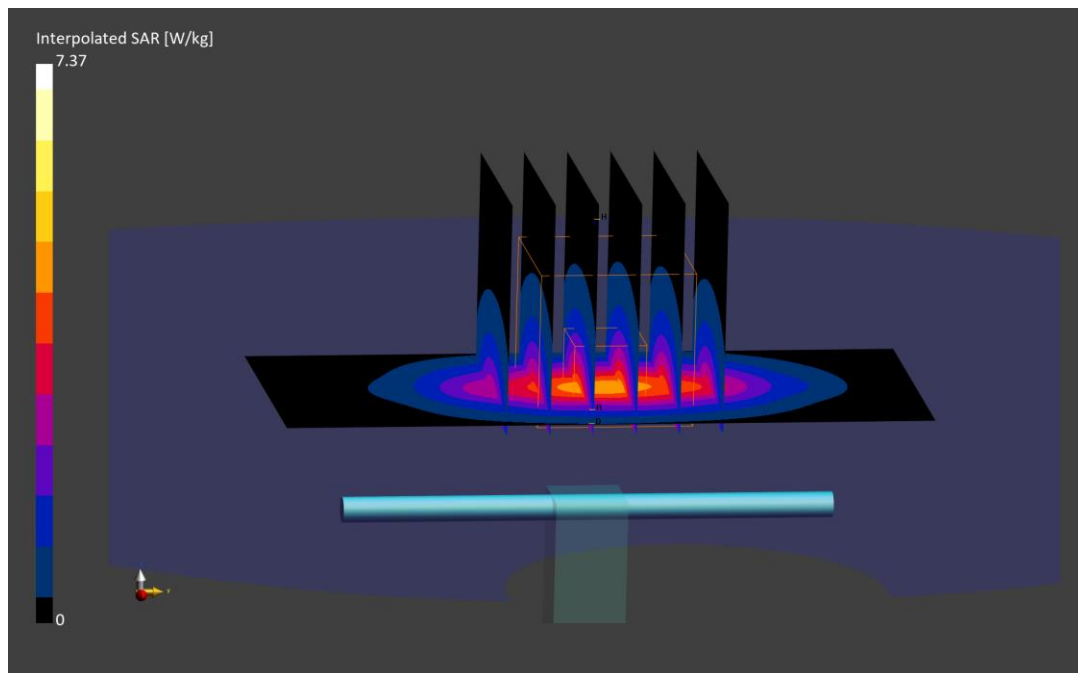

ELEMENT

DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1038

Communication System: UID: 0, CW; Frequency: 2300.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2300.0 MHz; cond = 1.65 S/m; perm = 40.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/10/2024; Ambient Temp: 20.8°C; Tissue Temp: 19.1°C

Probe: EX3DV4 - SN7421; ConvF:(7.61,7.61,7.61); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn604; Calibrated: 2023-03-15
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASYS Module SAR V16.2.0.1425

2300.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.2 W/kg

SAR(1 g) = 5.07 W/kg

Deviation (1 g) = 4.32%

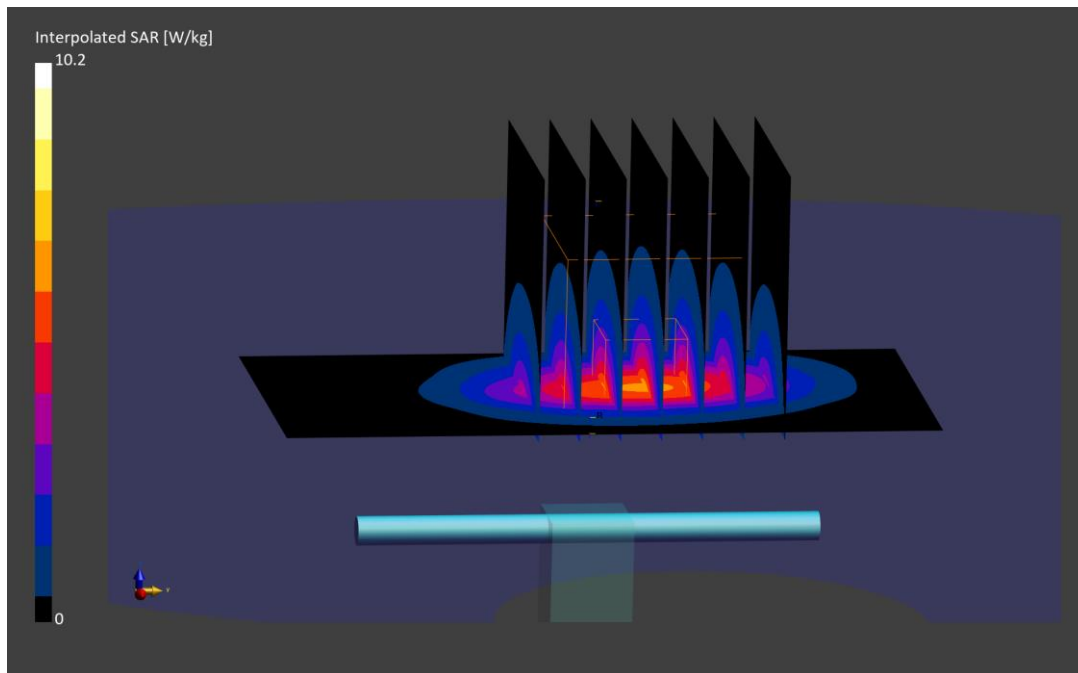

ELEMENT

DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1038

Communication System: UID: 0, CW; Frequency: 2300.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2300.0 MHz; cond = 1.64 S/m; perm = 41.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/12/2024; Ambient Temp: 20.8°C; Tissue Temp: 19.7°C

Probe: EX3DV4 - SN7421; ConvF:(7.61,7.61,7.61); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn604; Calibrated: 2023-03-15
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.0.1425

2300.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.1 W/kg

SAR(1 g) = 5.08 W/kg

Deviation (1 g) = 4.53%

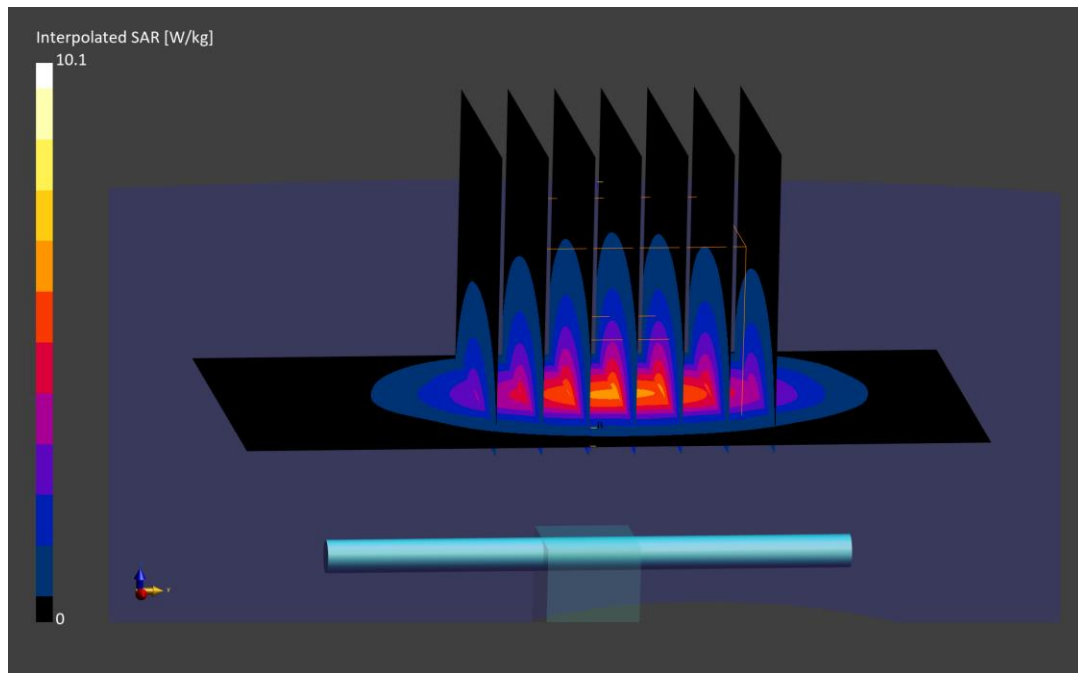

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.76 S/m; perm = 40.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/12/2024; Ambient Temp: 20.8°C; Tissue Temp: 19.7°C

Probe: EX3DV4 - SN7421; ConvF:(7.45,7.45,7.45); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn604; Calibrated: 2023-03-15
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.0.1425

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.6 W/kg

SAR(1 g) = 5.12 W/kg

Deviation (1 g) = -5.54%

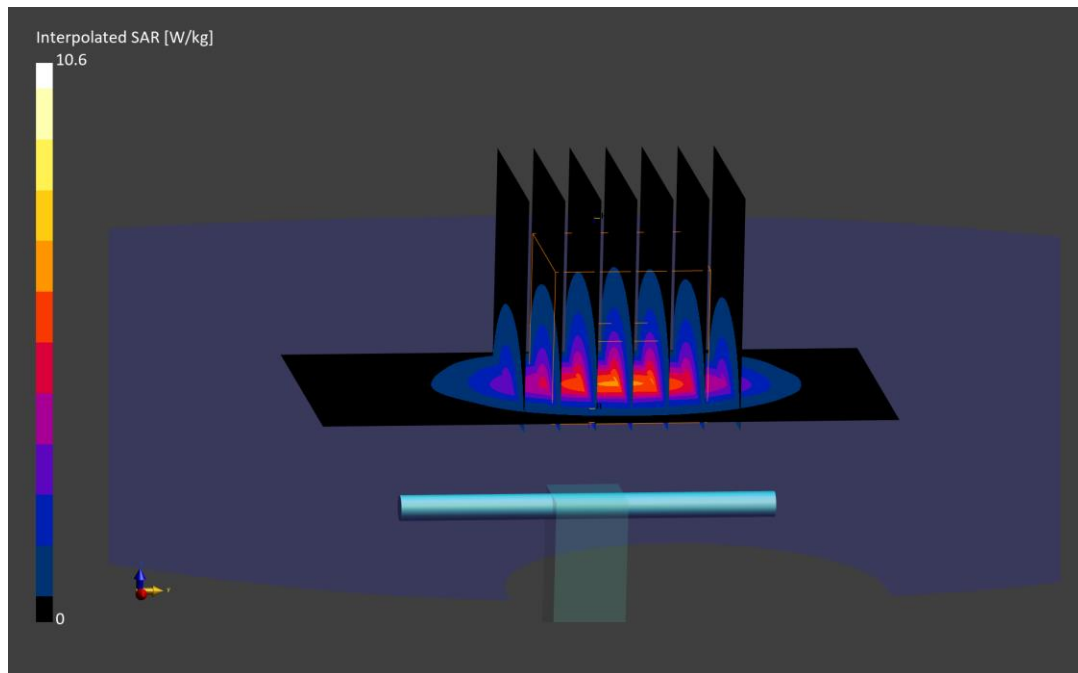

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN855

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.83 S/m; perm = 38.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/21/2024; Ambient Temp: 21.5°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN7532; ConvF:(7.88,7.88,7.88); Calibrated: 2023-04-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn501; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 2067
Measurement SW: DASY Module SAR V16.2.0.1425

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.5 W/kg

SAR(1 g) = 5.08 W/kg

Deviation (1 g) = -3.05%

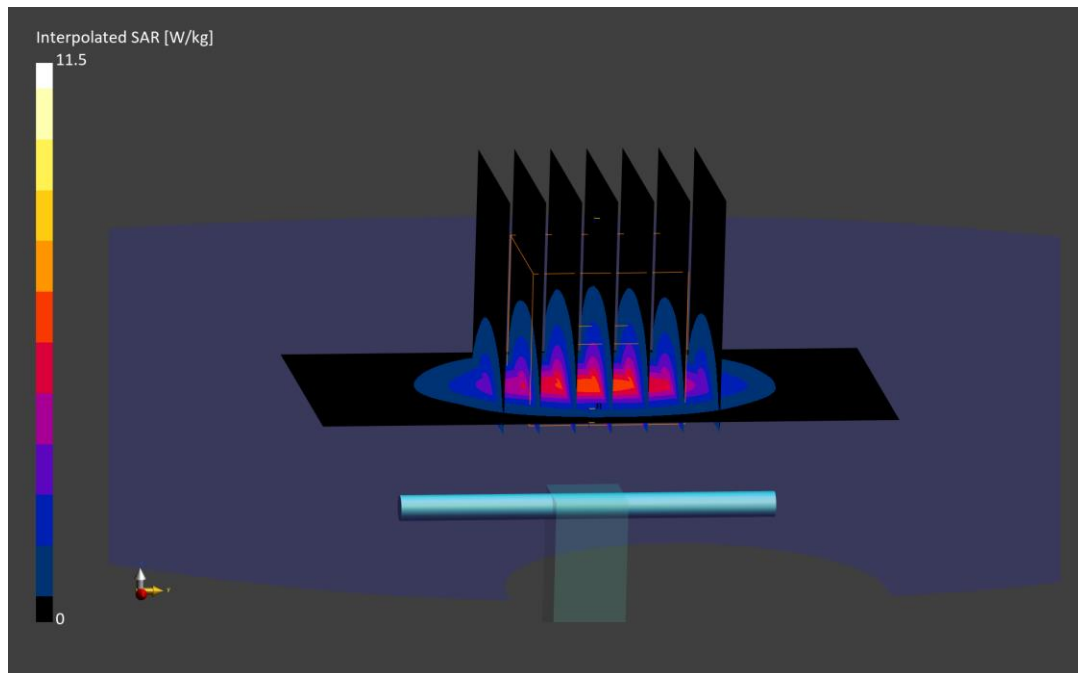

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.85 S/m; perm = 39.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2024; Ambient Temp: 21.0°C; Tissue Temp: 23.0°C

Probe: EX3DV4 - SN7546; ConvF:(7.29,7.29,7.29); Calibrated: 2023-04-14
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1402; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0 ; Serial: 1935
Measurement SW: DASY Module SAR V16.2.0.1425

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.2 W/kg

SAR(1 g) = 5.13 W/kg

Deviation (1 g) = -2.47%

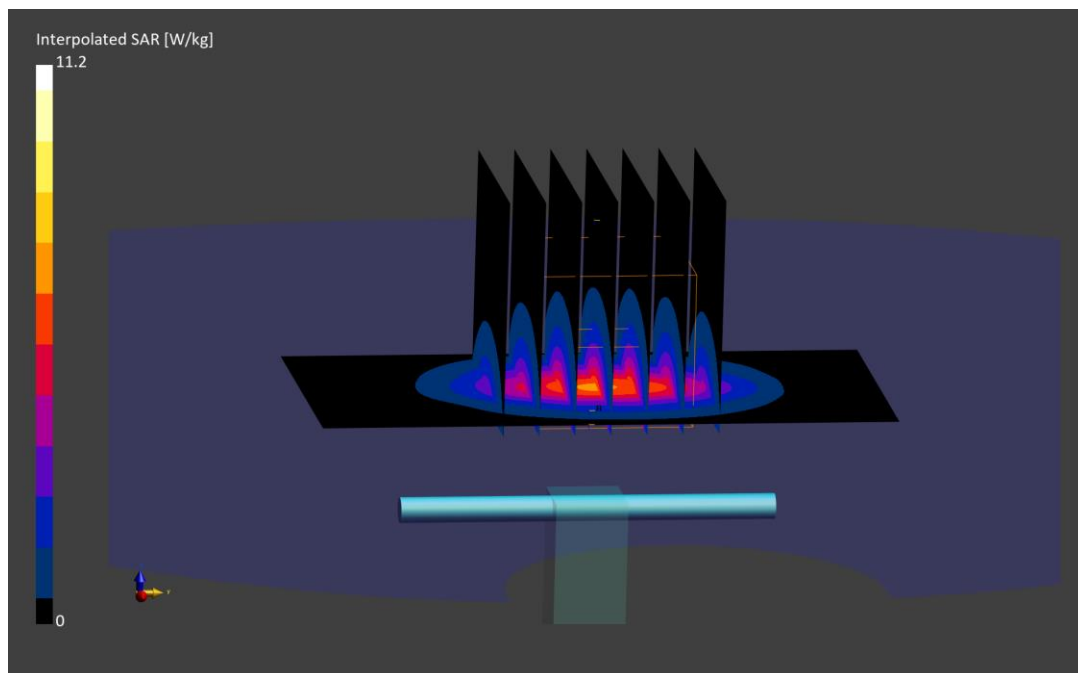

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.77 S/m; perm = 39.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 02/01/2024; Ambient Temp: 20.6°C; Tissue Temp: 19.6°C

Probe: EX3DV4 - SN7421; ConvF:(7.45,7.45,7.45); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn604; Calibrated: 2023-03-15
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.0.1425

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.8 W/kg

SAR(1 g) = 5.13 W/kg

Deviation (1 g) = -5.35%

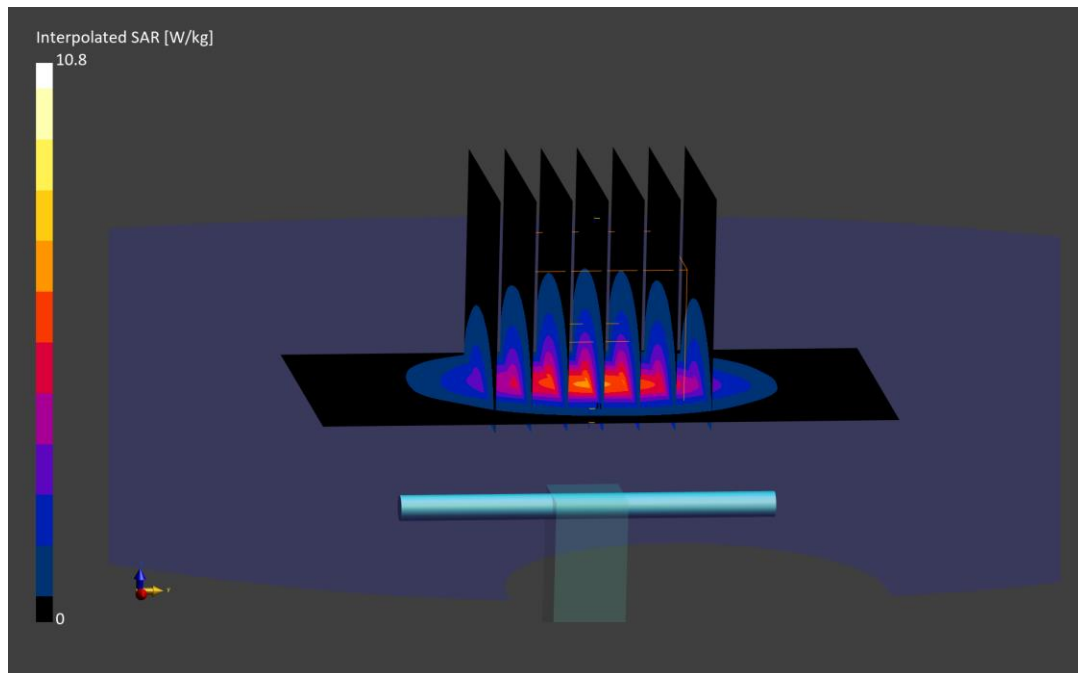

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.87 S/m; perm = 40.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 03/07/2024; Ambient Temp: 22.0°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7639; ConvF:(8.36,8.36,8.36); Calibrated: 2023-11-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1403; Calibrated: 2023-11-14
Phantom: Twin-SAM V8.0; Serial: 2034
Measurement SW: DASY Module SAR V16.2.0.1425

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.4 W/kg

SAR(1 g) = 5.16 W/kg

Deviation (1 g) = -1.90%

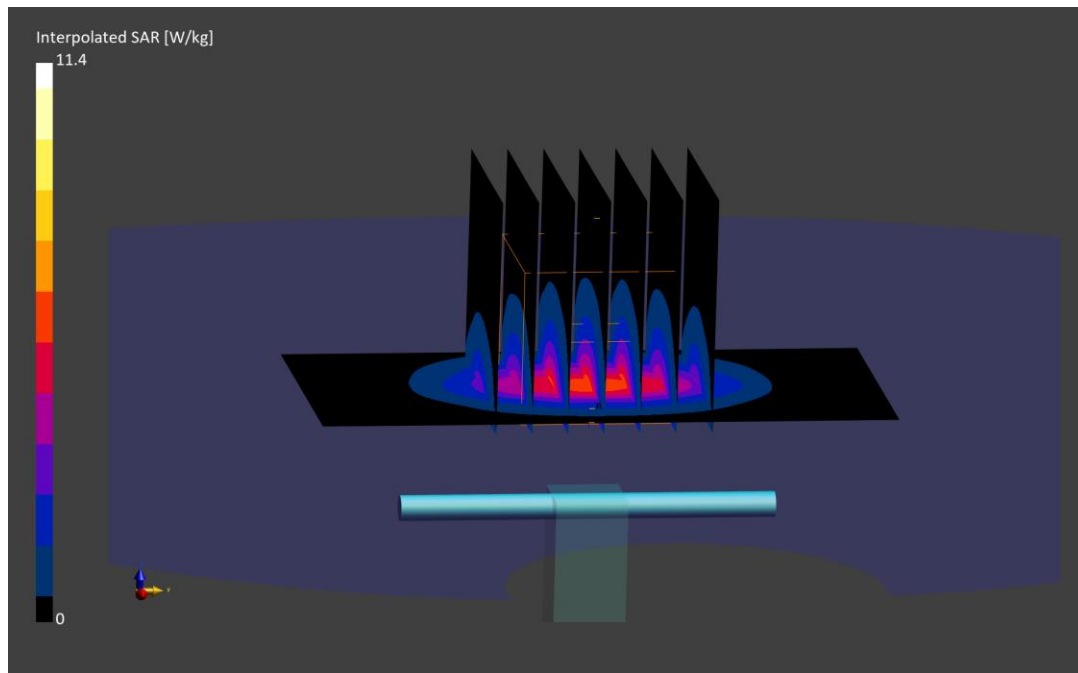

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1068

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 2.04 S/m; perm = 37.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/18/2024; Ambient Temp: 21.1°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7532; ConvF:(7.53,7.53,7.53); Calibrated: 2023-04-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn501; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 2067
Measurement SW: DASY Module SAR V16.2.0.1425

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 13.3 W/kg

SAR(1 g) = 5.74 W/kg

Deviation (1 g) = 1.59%

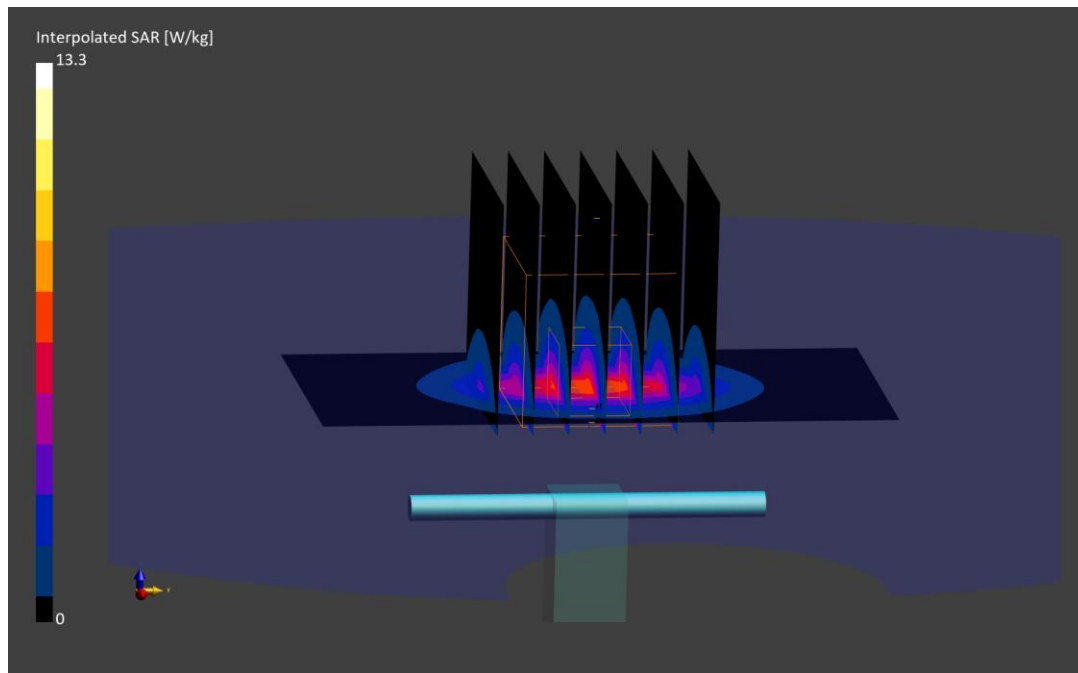

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1068

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 2.01 S/m; perm = 37.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/21/2024; Ambient Temp: 21.5°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN7532; ConvF:(7.53,7.53,7.53); Calibrated: 2023-04-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn501; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 2067
Measurement SW: DASY Module SAR V16.2.0.1425

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.9 W/kg

SAR(1 g) = 5.53 W/kg

Deviation (1 g) = -2.12%

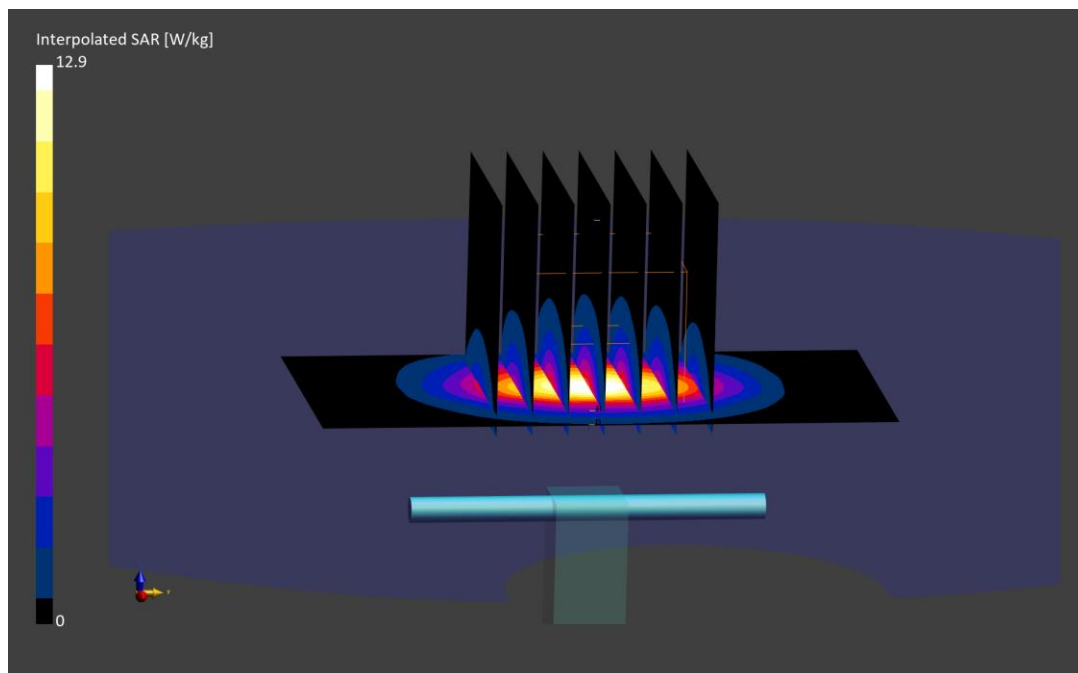

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1042

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 2.03 S/m; perm = 39.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2024; Ambient Temp: 21.0°C; Tissue Temp: 23.0°C

Probe: EX3DV4 - SN7546; ConvF:(7.08,7.08,7.08); Calibrated: 2023-04-14
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1402; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0 ; Serial: 1935
Measurement SW: DASY Module SAR V16.2.0.1425

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 13.2 W/kg

SAR(1 g) = 5.81 W/kg

Deviation (1 g) = 4.12%

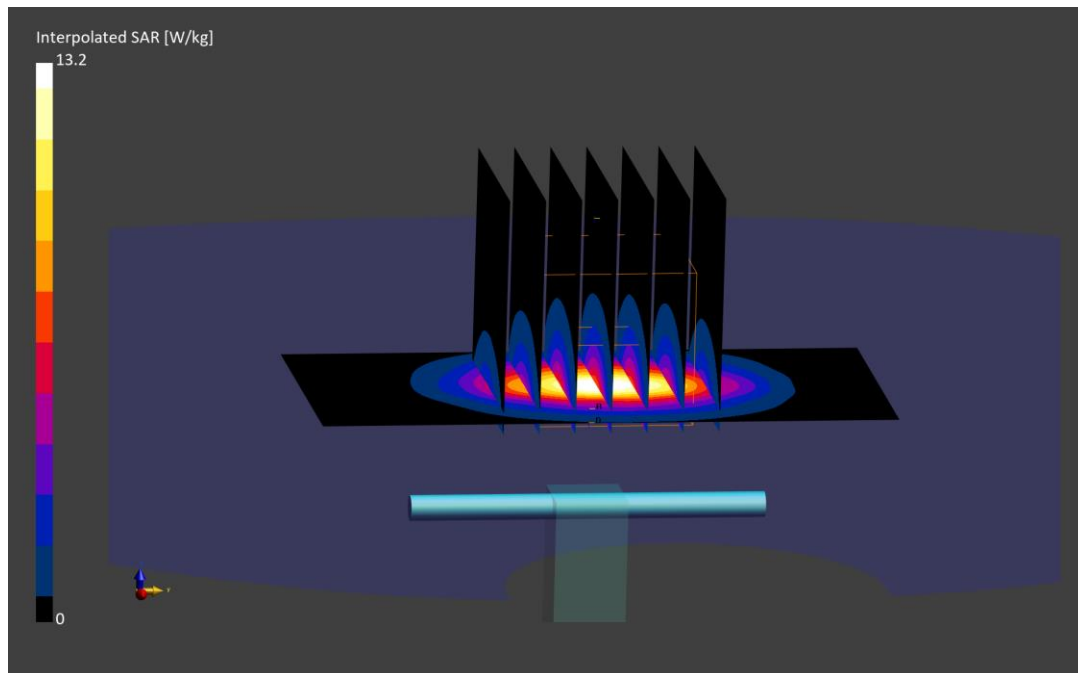

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1126

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 2.94 S/m; perm = 38.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/14/2024; Ambient Temp: 20.9°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7638; ConvF:(7.02,7.02,7.02); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1408; Calibrated: 2023-03-13
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.0.1425

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.2 W/kg

SAR(1 g) = 6.94 W/kg

Deviation (1 g) = 3.58%

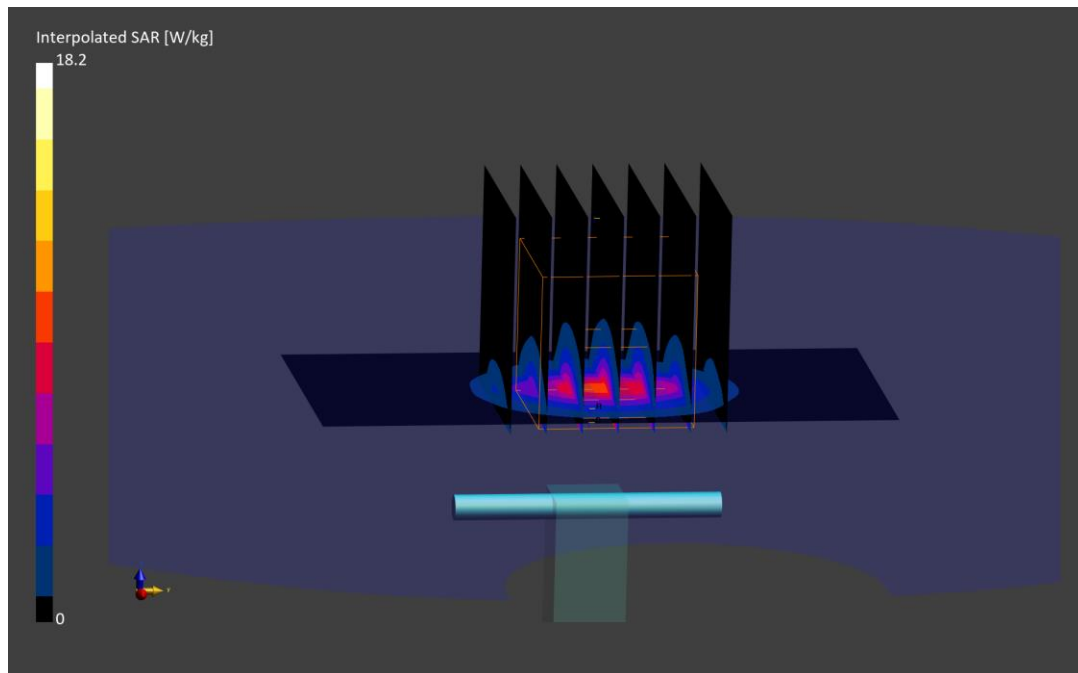

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1126

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 3.03 S/m; perm = 36.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/22/2024; Ambient Temp: 24.0°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7782; ConvF:(6.19,6.19,6.19); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.9 W/kg

SAR(1 g) = 6.53 W/kg

Deviation (1 g) = -2.54%

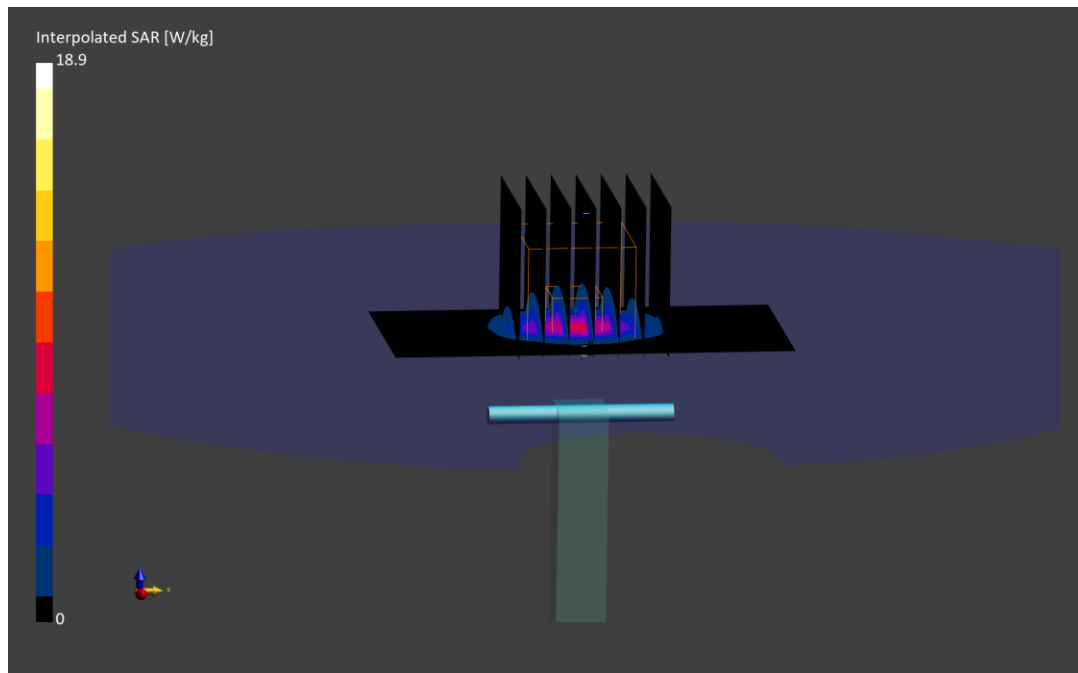

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1055

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 2.99 S/m; perm = 38.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2024; Ambient Temp: 21.3°C; Tissue Temp: 20.9°C

Probe: EX3DV4 - SN7638; ConvF:(7.02,7.02,7.02); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1408; Calibrated: 2023-03-13
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.0.1425

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.3 W/kg

SAR(1 g) = 6.92 W/kg

Deviation (1 g) = 4.85%

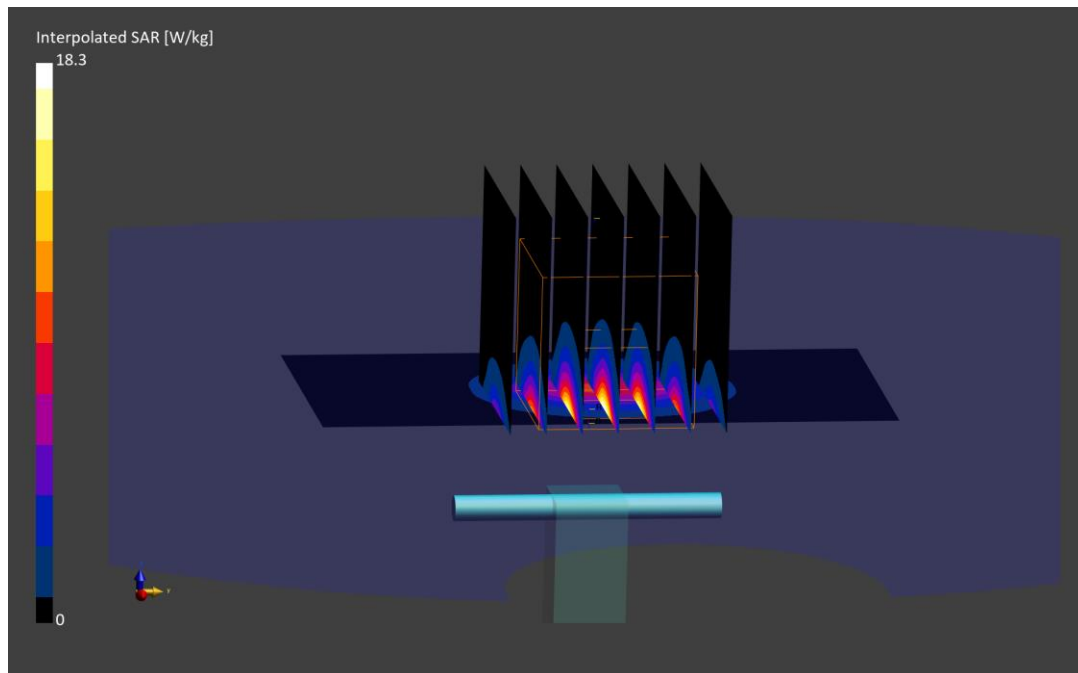

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1126

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 3.04 S/m; perm = 36.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2024; Ambient Temp: 21.6°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7782; ConvF:(6.19,6.19,6.19); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 19.4 W/kg

SAR(1 g) = 6.76 W/kg

Deviation (1 g) = 0.90%

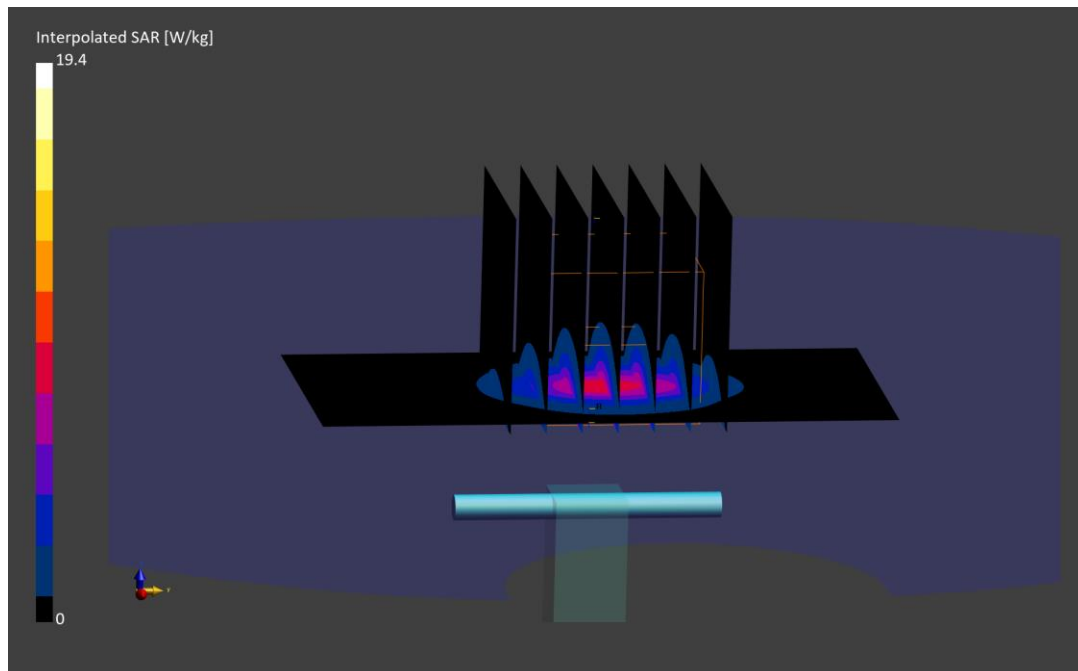

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1002

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.12 S/m; perm = 38.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/14/2024; Ambient Temp: 20.9°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7638; ConvF:(6.99,6.99,6.99); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1408; Calibrated: 2023-03-13
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.0.1425

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.1 W/kg

SAR(1 g) = 6.67 W/kg

Deviation (1 g) = -1.77%

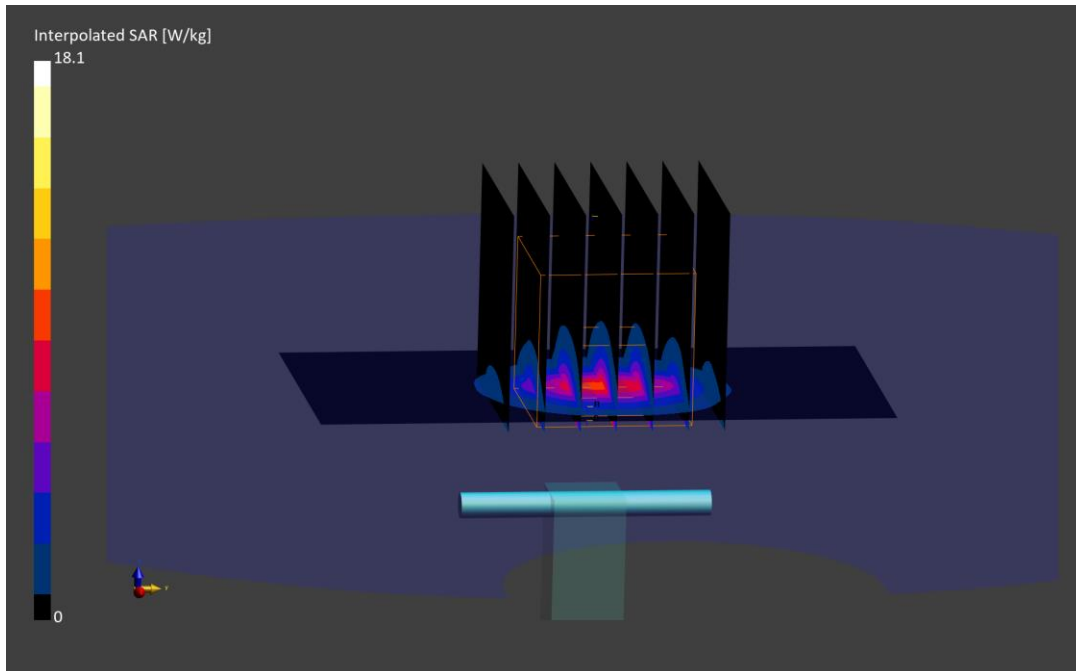

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1097

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.19 S/m; perm = 36.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/22/2024; Ambient Temp: 24.0°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7782; ConvF:(6.18,6.18,6.18); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 21.1 W/kg

SAR(1 g) = 7.12 W/kg

Deviation (1 g) = 4.55%

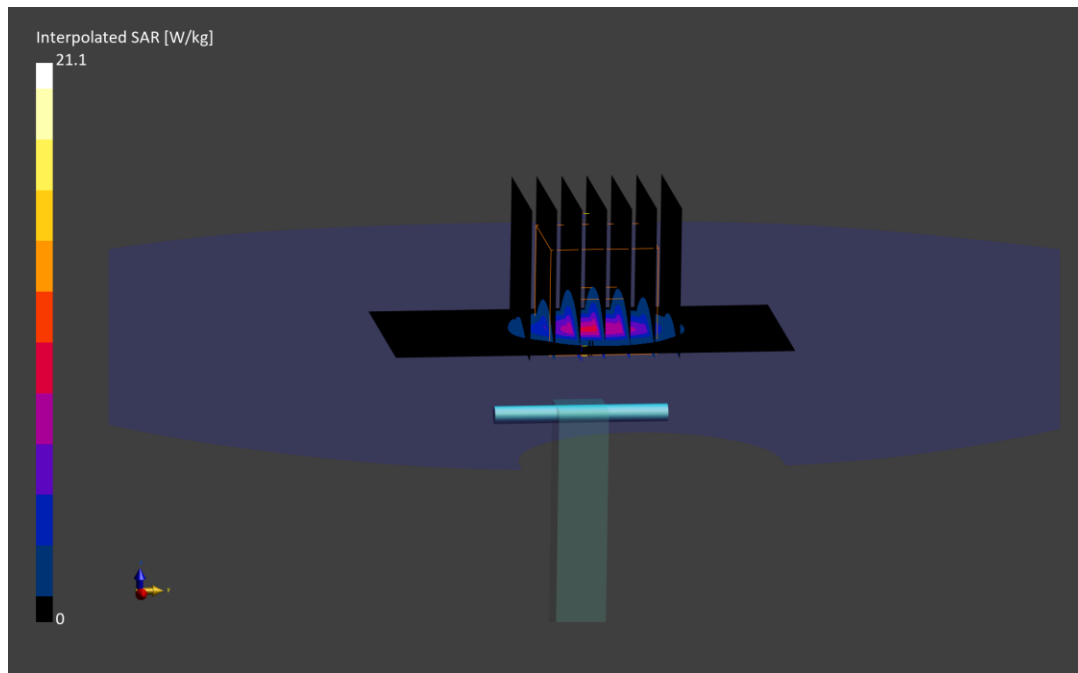

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1002

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.15 S/m; perm = 38.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2024; Ambient Temp: 21.3°C; Tissue Temp: 20.9°C

Probe: EX3DV4 - SN7638; ConvF:(6.99,6.99,6.99); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1408; Calibrated: 2023-03-13
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.0.1425

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.5 W/kg

SAR(1 g) = 6.80 W/kg

Deviation (1 g) = 0.15%

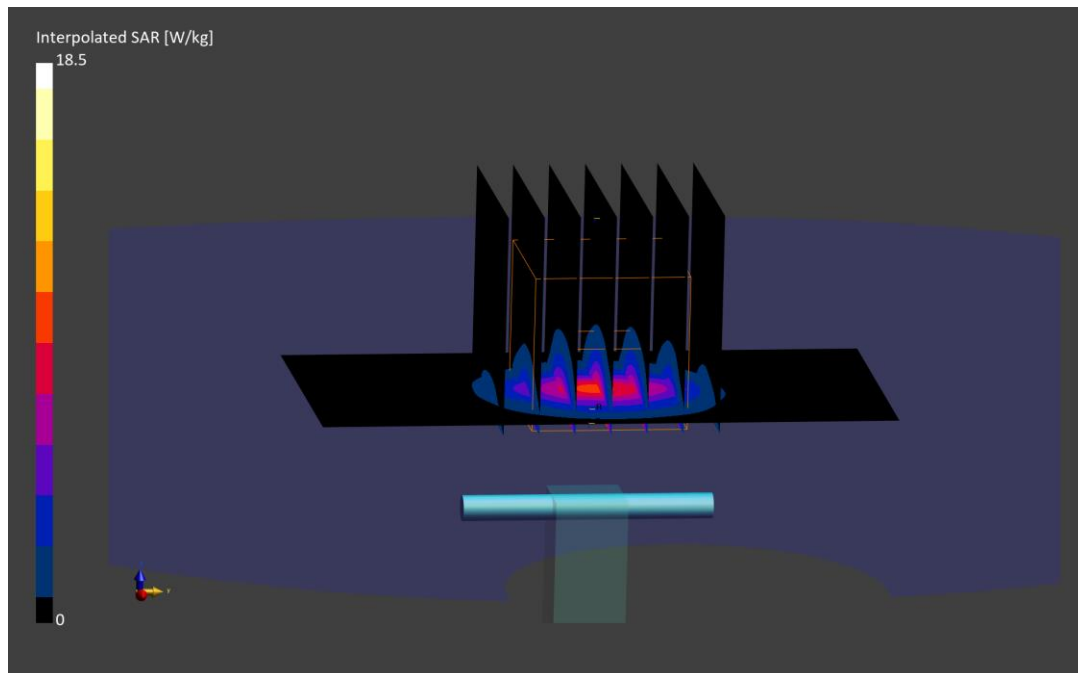

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1097

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.19 S/m; perm = 36.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2024; Ambient Temp: 21.6°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7782; ConvF:(6.18,6.18,6.18); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 21.2 W/kg

SAR(1 g) = 7.22 W/kg

Deviation (1 g) = 6.02%

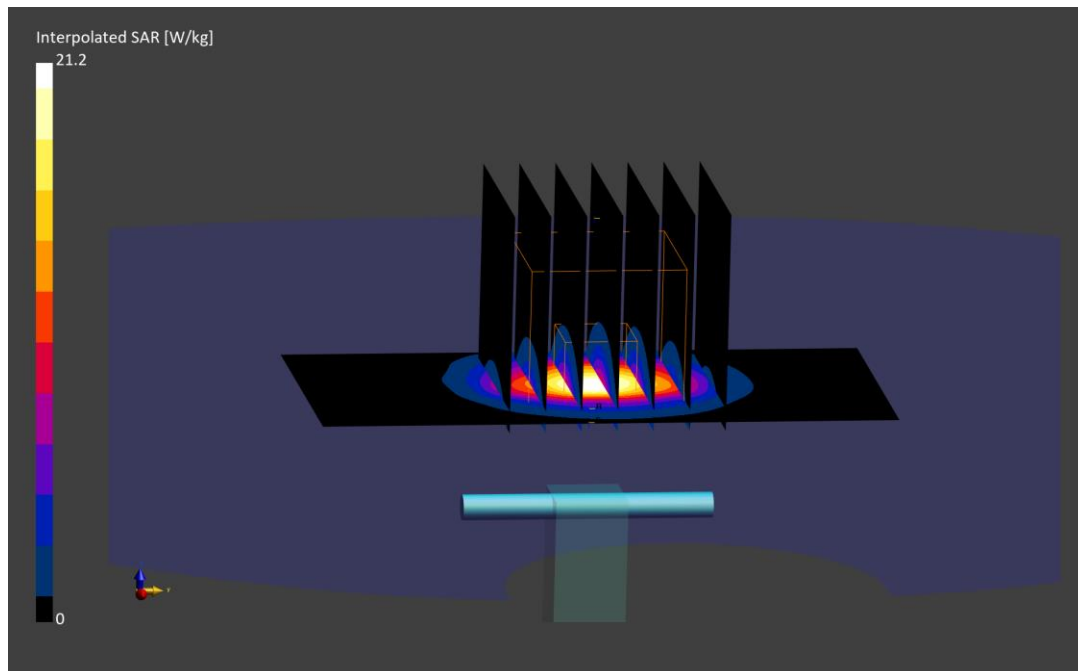

ELEMENT

DUT: Dipole 3900.0 MHz; Type: D3900V2 - SN1073

Communication System: UID: 0, CW; Frequency: 3900.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3900.0 MHz; cond = 3.35 S/m; perm = 36.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/22/2024; Ambient Temp: 24.0°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7782; ConvF:(5.65,5.65,5.65); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 20.1 W/kg

SAR(1 g) = 6.82 W/kg

Deviation (1 g) = -2.15%

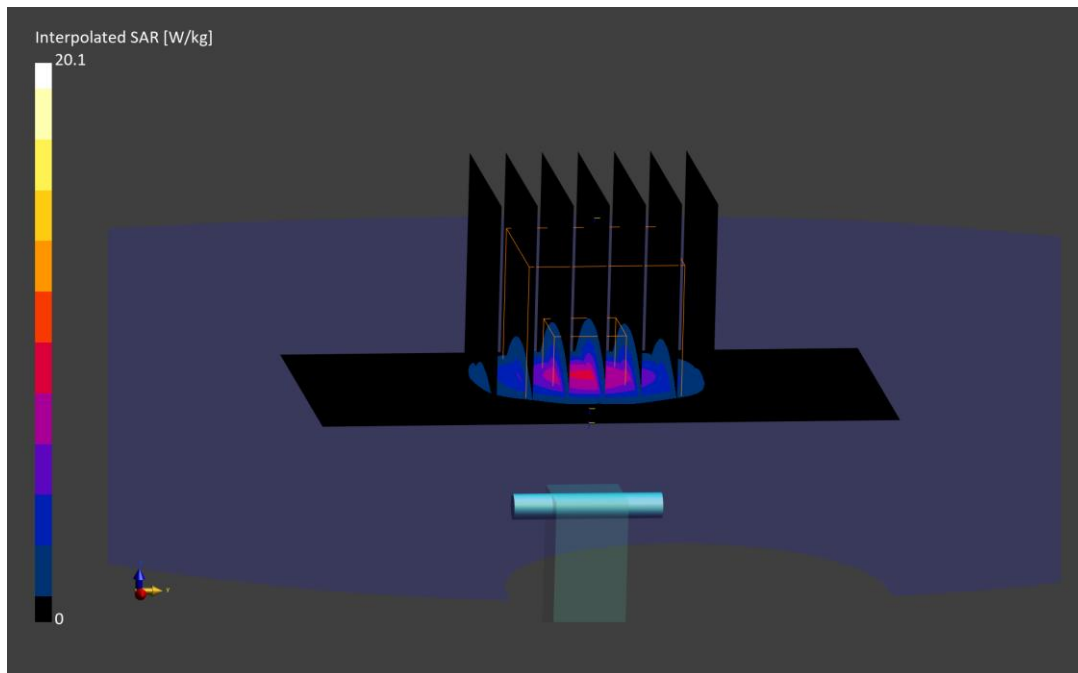

ELEMENT

DUT: Dipole 3900.0 MHz; Type: D3900V2 - SN1073

Communication System: UID: 0, CW; Frequency: 3900.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3900.0 MHz; cond = 3.33 S/m; perm = 37.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2024; Ambient Temp: 21.3°C; Tissue Temp: 20.9°C

Probe: EX3DV4 - SN7638; ConvF:(6.92,6.92,6.92); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1408; Calibrated: 2023-03-13
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.0.1425

3900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 20.7 W/kg

SAR(1 g) = 7.06 W/kg

Deviation (1 g) = 1.29%

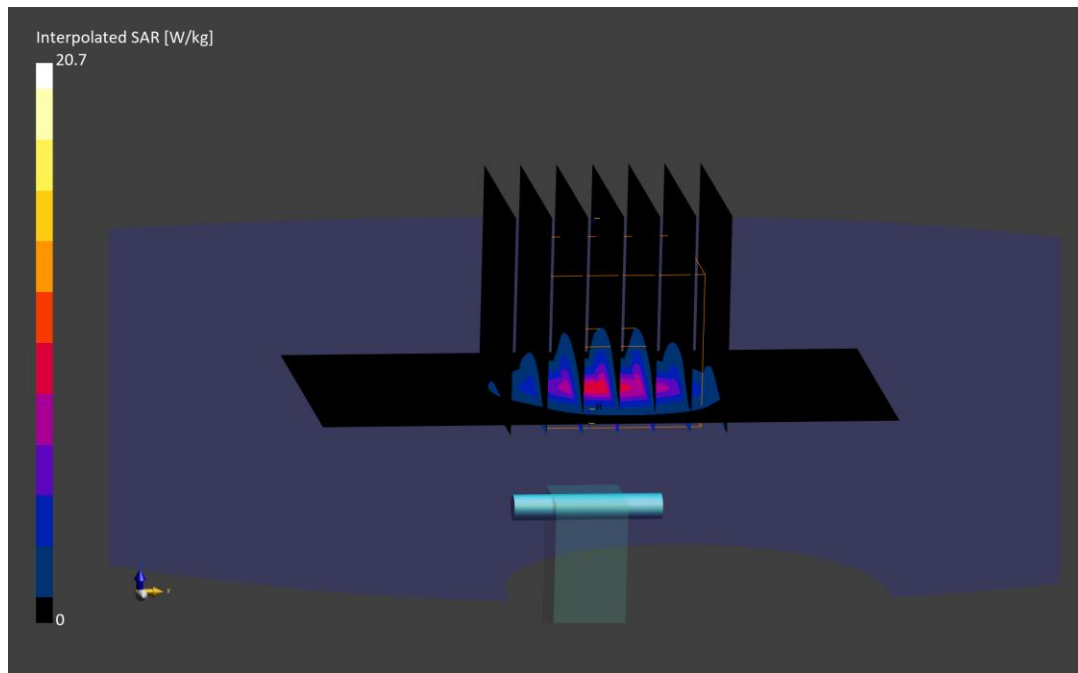

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5250.0 MHz; cond = 4.52 S/m; perm = 35.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2024; Ambient Temp: 22.3°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN3949; ConvF:(5.74,5.74,5.74); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.0.1425

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.8 W/kg

SAR(1 g) = 4.18 W/kg

Deviation (1 g) = 3.85%

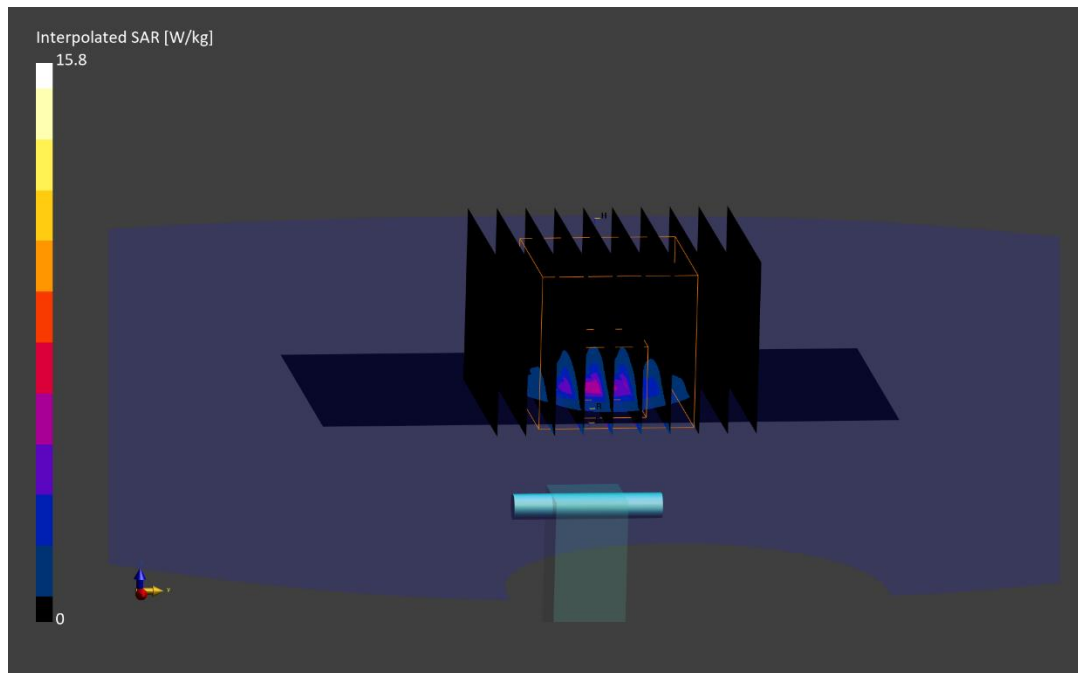

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5250.0 MHz; cond = 4.51 S/m; perm = 35.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 02/13/2024; Ambient Temp: 20.8°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN3746; ConvF:(5.12,5.12,5.12); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.2.0.1425

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.9 W/kg

SAR(1 g) = 4.03 W/kg

Deviation (1 g) = 0.12%

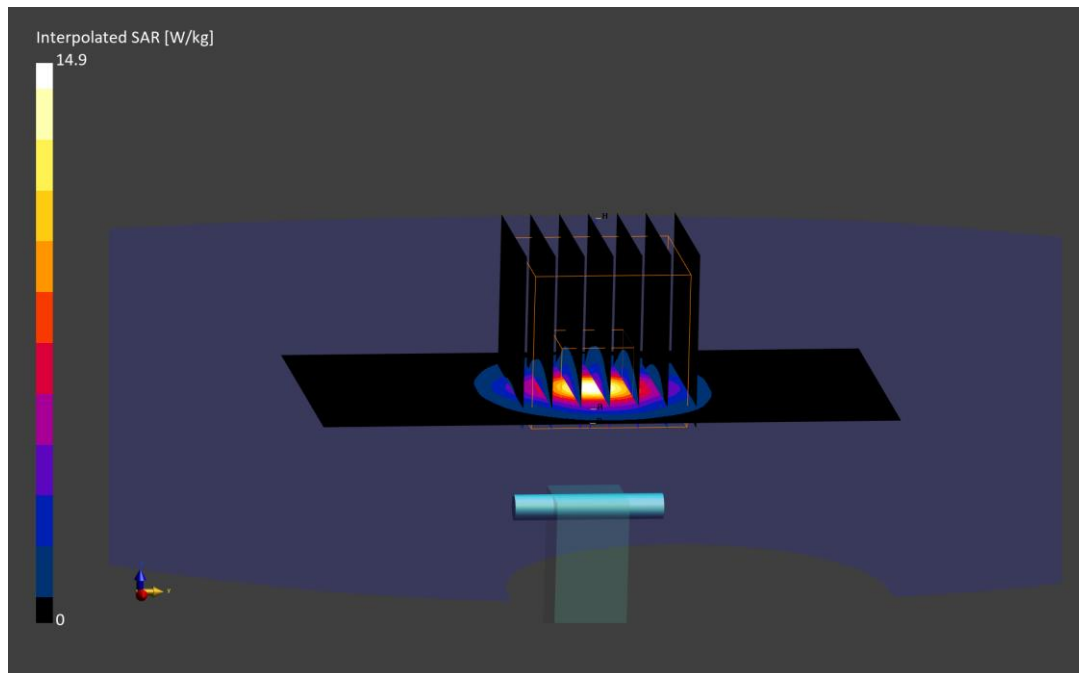

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5600.0 MHz; cond = 4.91 S/m; perm = 35.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2024; Ambient Temp: 22.3°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN3949; ConvF:(5.11,5.11,5.11); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.0.1425

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.3 W/kg

SAR(1 g) = 3.97 W/kg

Deviation (1 g) = -5.14%

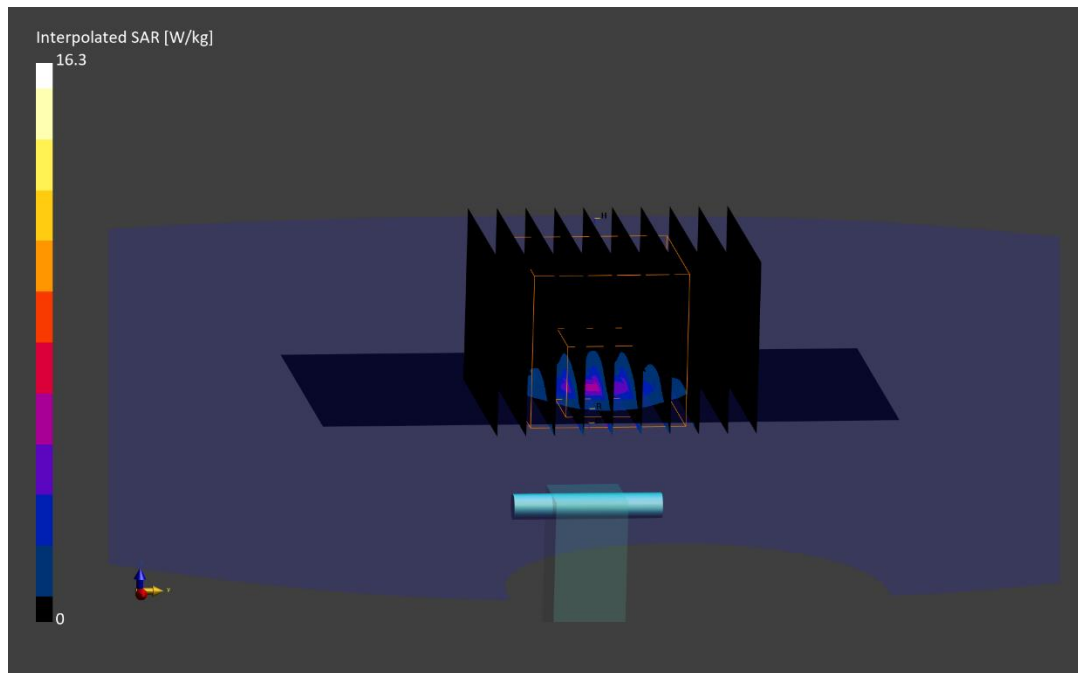

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5600.0 MHz; cond = 4.91 S/m; perm = 34.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 02/13/2024; Ambient Temp: 20.8°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN3746; ConvF:(4.45,4.45,4.45); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.2.0.1425

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.6 W/kg

SAR(1 g) = 4.40 W/kg

Deviation (1 g) = 5.14%

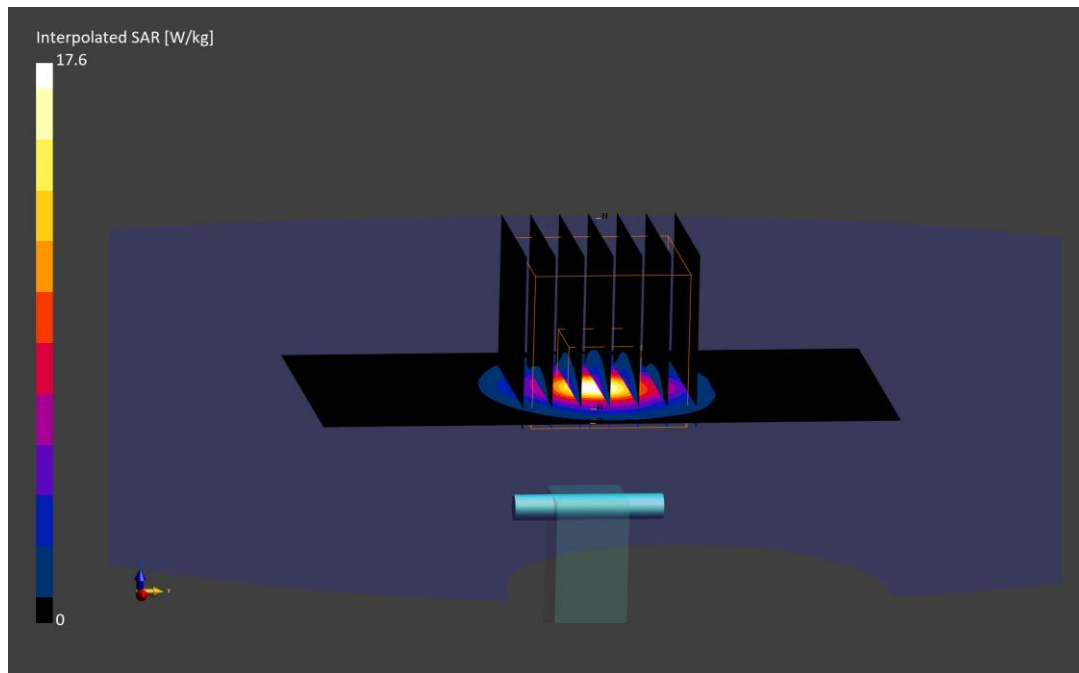

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5750.0 MHz; cond = 5.09 S/m; perm = 35.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2024; Ambient Temp: 22.3°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN3949; ConvF:(5.31,5.31,5.31); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.0.1425

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.6 W/kg

SAR(1 g) = 3.97 W/kg

Deviation (1 g) = -1.37%

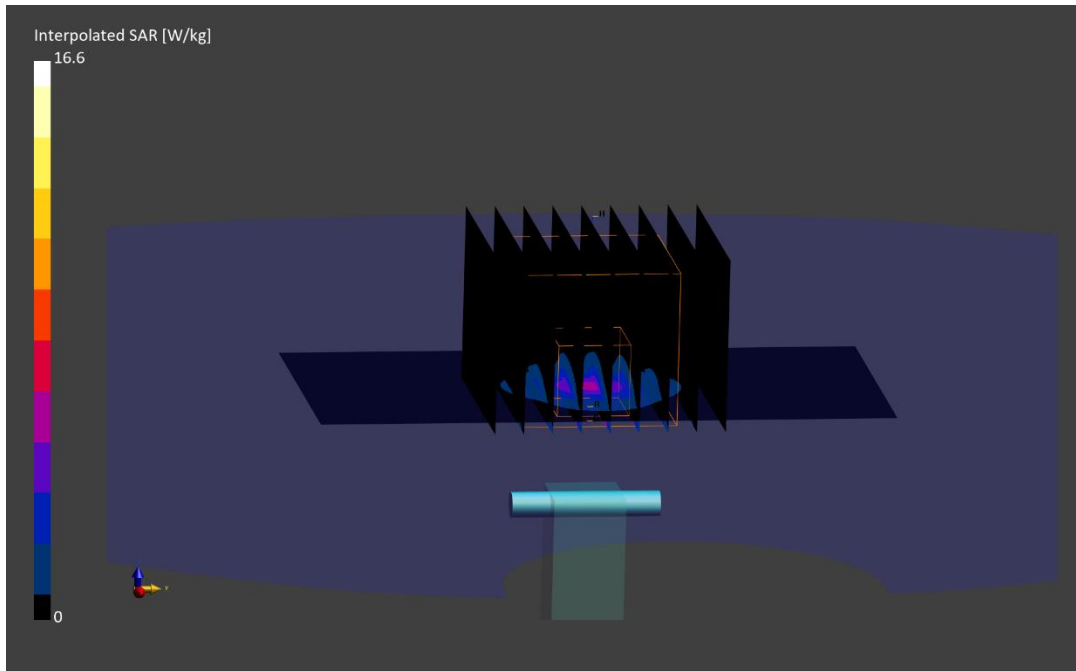

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5750.0 MHz; cond = 5.08 S/m; perm = 34.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 02/13/2024; Ambient Temp: 20.8°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN3746; ConvF:(4.59,4.59,4.59); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.2.0.1425

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.9 W/kg

SAR(1 g) = 4.13 W/kg

Deviation (1 g) = 2.61%

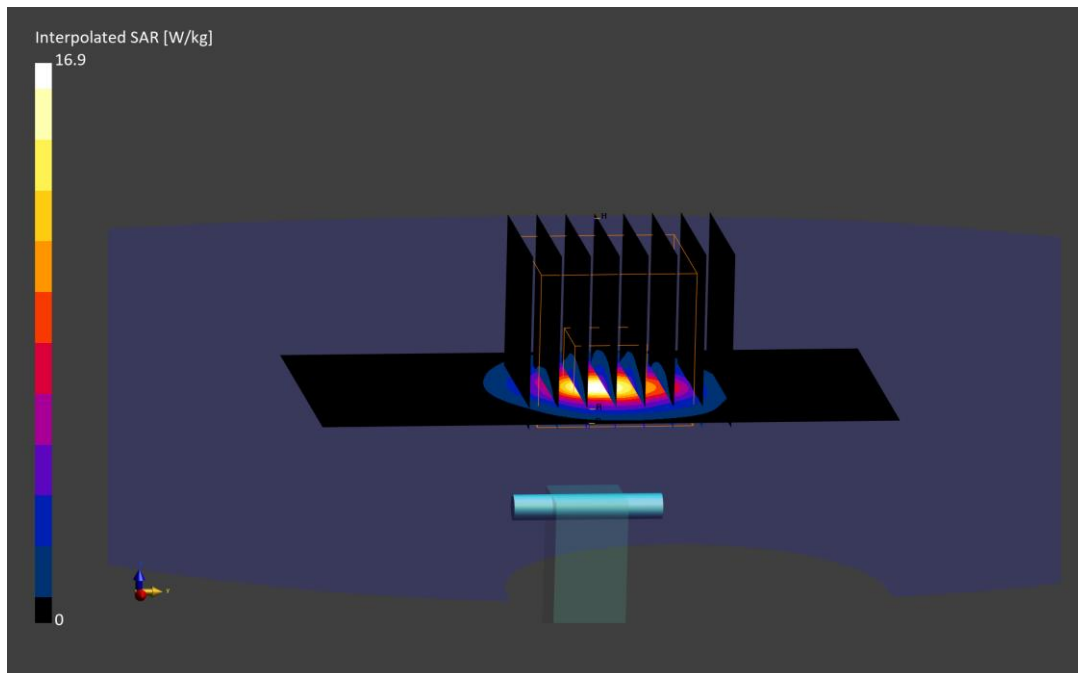

ELEMENT

DUT: Dipole 5800.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5800.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5800.0 MHz; cond = 5.14 S/m; perm = 34.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/28/2024; Ambient Temp: 22.3°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN3949; ConvF:(5.21,5.21,5.21); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.0.1425

5800.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.2 W/kg

SAR(1 g) = 3.79 W/kg

Deviation (1 g) = -5.84%

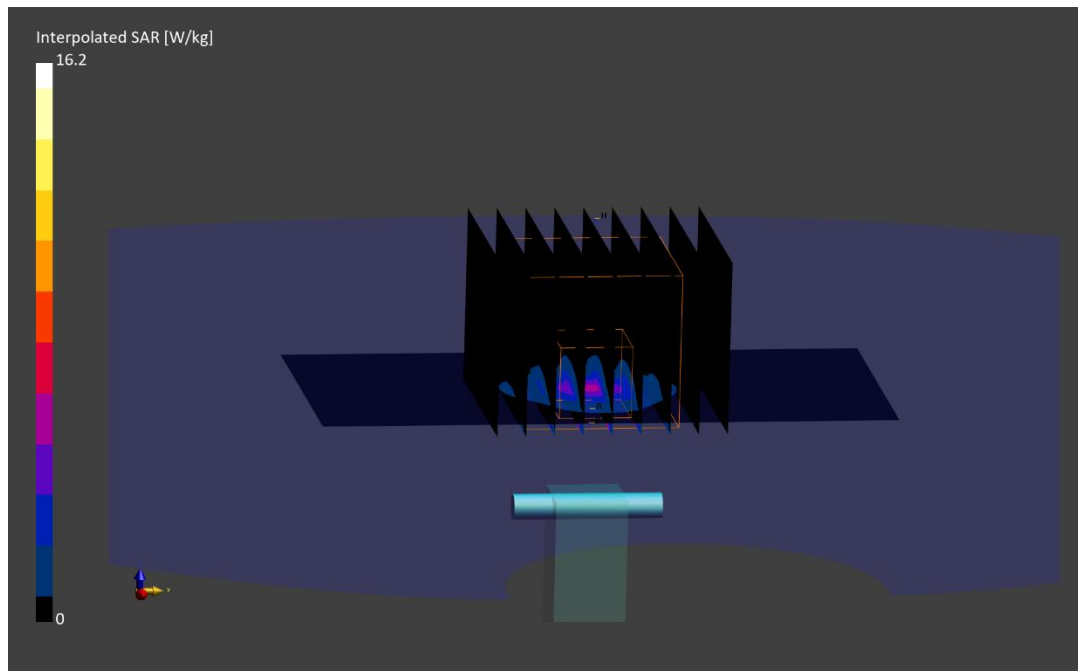

ELEMENT

DUT: Dipole 5800.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5800.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5800.0 MHz; cond = 5.14 S/m; perm = 34.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 02/13/2024; Ambient Temp: 20.8°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN3746; ConvF:(4.5,4.5,4.5); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.2.0.1425

5800.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.7 W/kg

SAR(1 g) = 4.06 W/kg

Deviation (1 g) = 0.87%

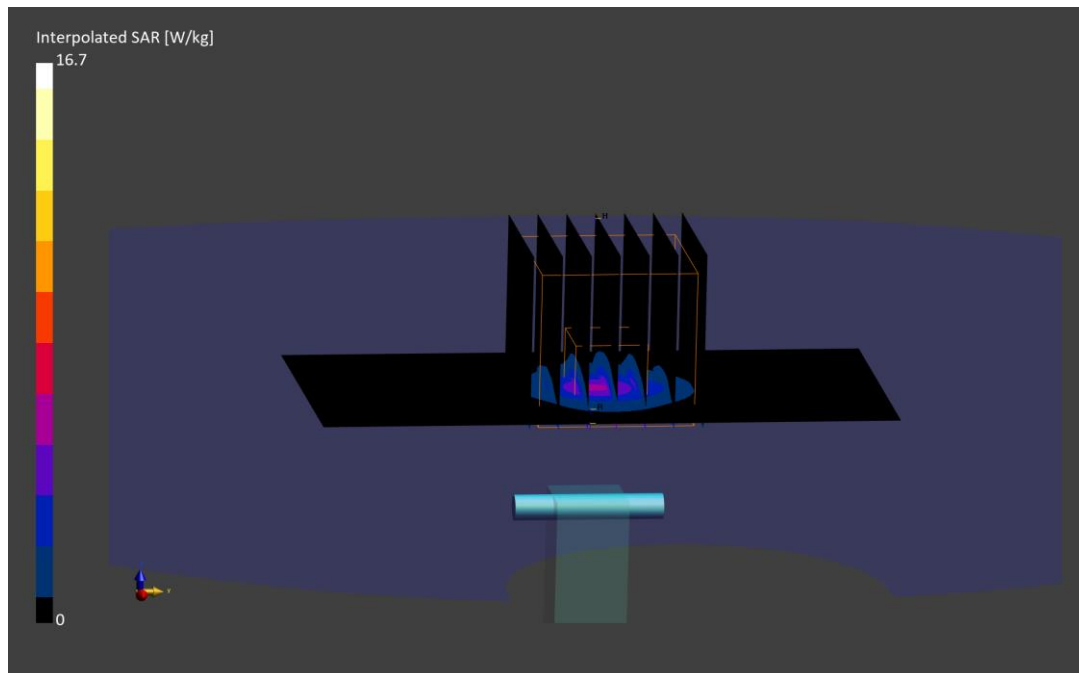

ELEMENT

DUT: Dipole 6500.000 MHz; Type: D6.5GHzV2 - SN1019

Communication System: UID: 0, CW; Frequency: 6500.000 MHz
Medium: 6000 Head; Medium parameters used:
f = 6500 MHz; cond = 5.97 S/m; perm = 33.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 5 mm

Test Date: 01/08/2024; Ambient Temp: 21.5°C; Tissue Temp: 19.0°C

Probe: EX3DV4 - SN7420; ConvF:(5.21,5.12,5.28); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1333; Calibrated: 2023-10-18
Phantom: Twin-SAM V4.0 ; Serial: 1275
Measurement SW: DASY Module SAR V16.2.4.2524

6500.0 MHz System Verification at 14.0 dBm (25 mW)


Area Scan (51.0 x 85.0): Measurement grid: dx=8.5 mm, dy=8.5 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=3.4 mm, dy=3.4 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 49.1 W/kg

SAR(1 g) = 7.76 W/kg

Deviation (1 g) = 5.94%

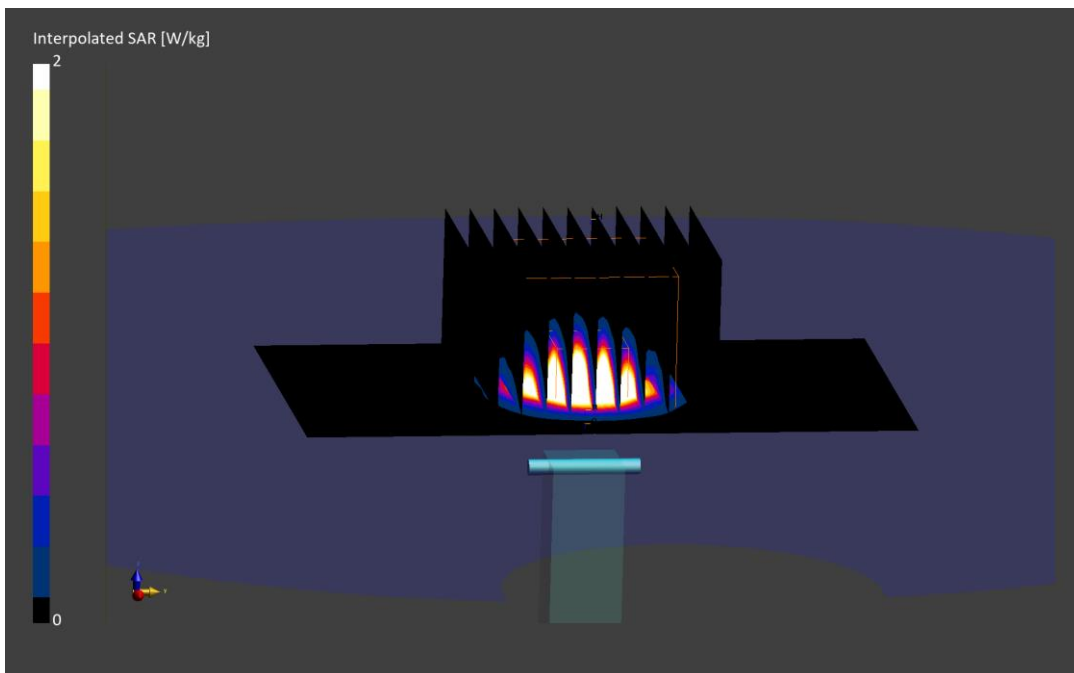

Date: 01/29/2024

10 GHz System Verification

Device Under Test Properties

DUT	Serial Number
10 GHz Verification Source	1002

Exposure Conditions

Phantom Section	Position	Test Distance [mm]	Band	Frequency [MHz]
5G	FRONT	10.00	Validation band	10000.0

Hardware Setup

Probe, Calibration Date	DAE, Calibration Date
EUmmWV3 - SN9407, 10/09/2023	DAE4 - SN793, 10/18/2023

Software Setup

Software	Software Version
cDASY6 Module mmWave	3.2.0.1840

Scans Setup

Scan Type	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [lambda]	0.25 x 0.25
Sensor Surface [mm]	10.0

Measurement Results

Scan Type	5G Scan
Avg. Area [cm ²]	4.00
pS _{tot} avg [W/m ²]	56.3
pS _n avg [W/m ²]	56.2
E _{peak} [V/m]	153
Deviation [dB] pS _{tot}	0.25
Deviation [dB] pS _n	0.27

