

APPENDIX B: SAR DIPOLE VERIFICATION PLOTS

ELEMENT

DUT: Dipole 13.0 MHz; Type: CLA-13 - SN1004

Communication System: UID: 0, CW; Frequency: 13.0 MHz
Medium: 30 Head; Medium parameters used:
 $f = 13.0$ MHz; $\text{cond} = 0.725$ S/m; $\text{perm} = 53.3$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 0 mm

Test Date: 01/02/2024; Ambient Temp: 21.2°C; Tissue Temp: 20.8°C

Probe: EX3DV4 - SN7360; ConvF:(17.98,17.98,17.98); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (All points)
Electronics: DAE4 Sn534; Calibrated: 2023-03-15
Phantom: ELI V6.0; Serial: 2044
Measurement SW: DASY Module SAR V16.2.0.1425

13.0 MHz System Verification at 30.0 dBm (1000 mW)


Area Scan (40.0 x 90.0): Measurement grid: $dx=10.0$ mm, $dy=15.0$ mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: $dx=6.0$ mm, $dy=6.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 1.13 W/kg

SAR(1 g) = 0.574 W/kg

Deviation (1 g) = -0.69%

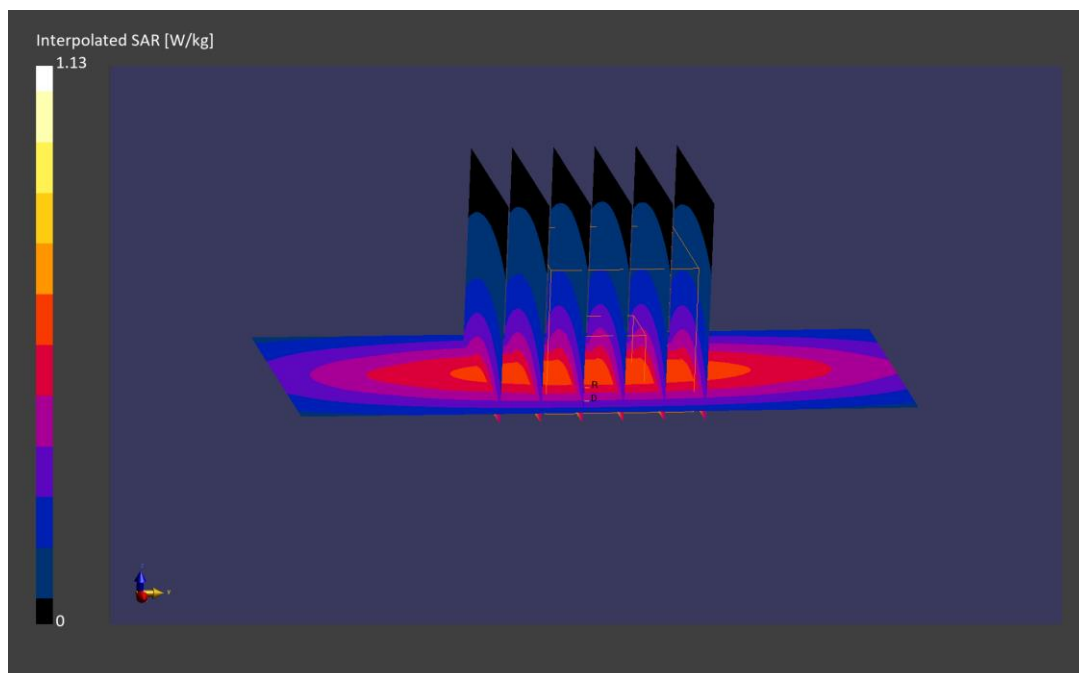

ELEMENT

DUT: Dipole 750.000 MHz; Type: D750V3 - SN1097

Communication System: UID: 0, CW; Frequency: 750.000 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.903 S/m; perm = 40.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 12/10/2023; Ambient Temp: 19.7°C; Tissue Temp: 24.3°C

Probe: EX3DV4 - SN3949; ConvF:(10.55,10.55,10.55); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.75 W/kg

SAR(1 g) = 1.75 W/kg

Deviation (1 g) = 5.80%

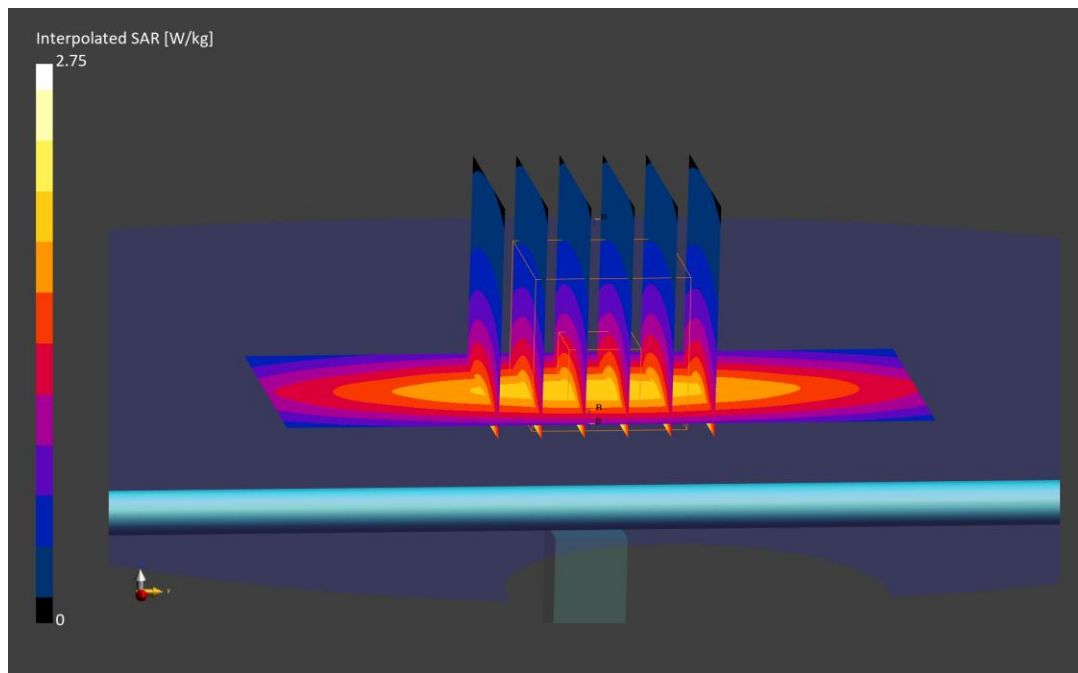

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1034

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.907 S/m; perm = 40.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 12/12/2023; Ambient Temp: 22.5°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN3949; ConvF:(10.55,10.55,10.55); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.82 W/kg

SAR(1 g) = 1.79 W/kg

Deviation (1 g) = 3.59%

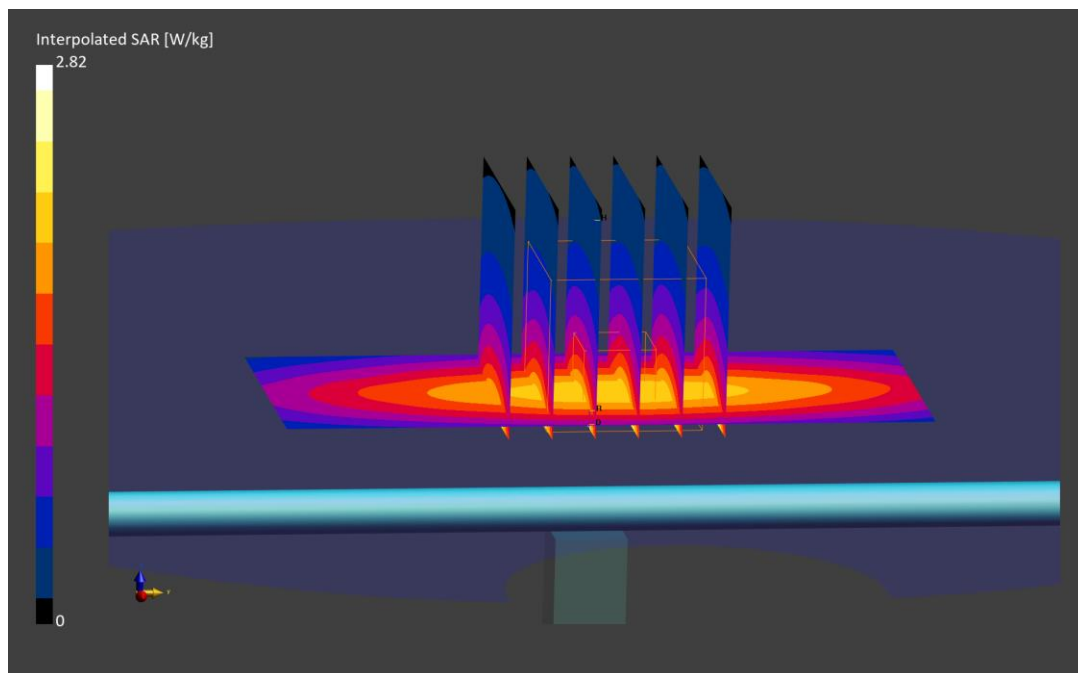

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1034

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.873 S/m; perm = 40.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 12/16/2023; Ambient Temp: 21.3°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN3949; ConvF:(10.55,10.55,10.55); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.74 W/kg

SAR(1 g) = 1.75 W/kg

Deviation (1 g) = 1.27%

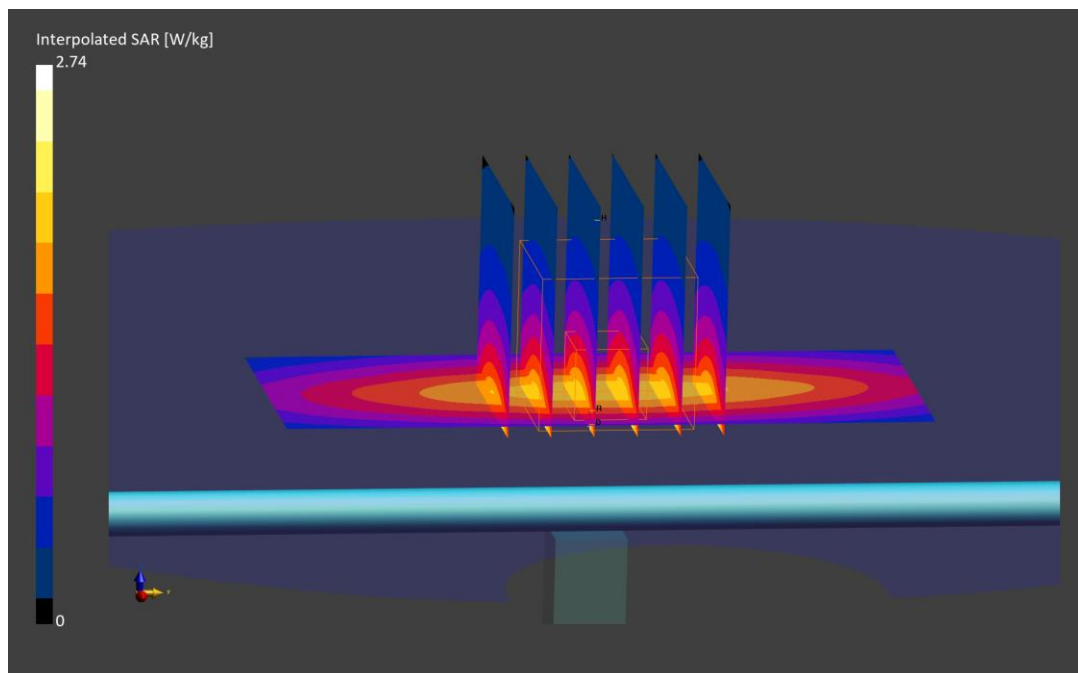

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1034

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.885 S/m; perm = 41.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 12/18/2023; Ambient Temp: 22.7°C; Tissue Temp: 22.2°C

Probe: EX3DV4 - SN3949; ConvF:(10.55,10.55,10.55); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASYS Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.93 W/kg

SAR(1 g) = 1.81 W/kg

Deviation (1 g) = 4.75%

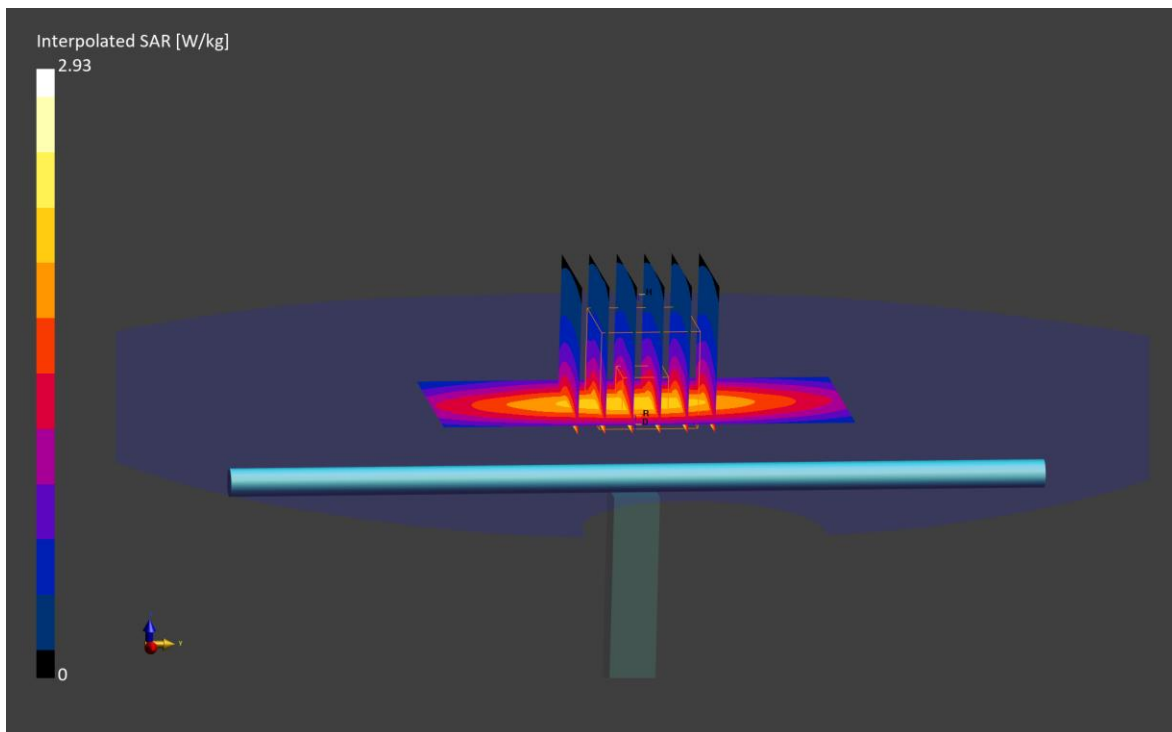

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1057

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.894 S/m; perm = 42.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 12/22/2023; Ambient Temp: 21.8°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN7682; ConvF:(11.36,11.36,11.36); Calibrated: 2023-05-11
Sensor-Surface: 1.4mm (All points)
Electronics: DAE4 Sn1683; Calibrated: 2023-05-11
Phantom: Twin-SAM V4.0; Serial: 1598
Measurement SW: DASY Module SAR V16.2.0.1425

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.68 W/kg

SAR(1 g) = 1.73 W/kg

Deviation (1 g) = 1.65%

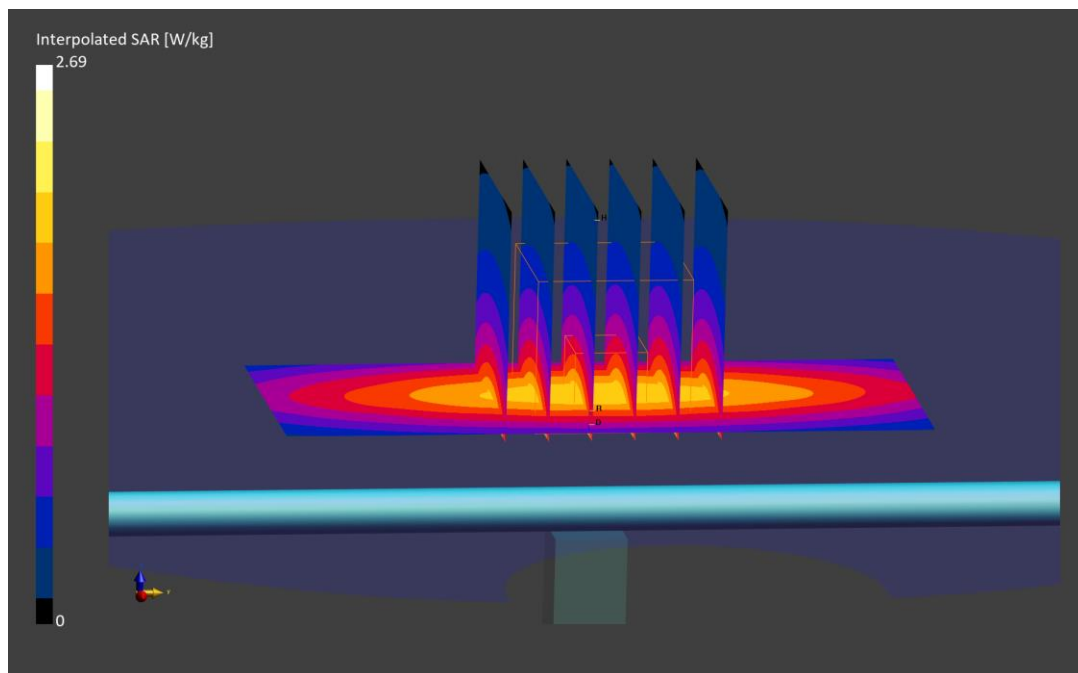

ELEMENT

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d040

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Head; Medium parameters used:
f = 835.0 MHz; cond = 0.891 S/m; perm = 40.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 12/11/2023; Ambient Temp: 19.6°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7416; ConvF:(9.73,9.73,9.73); Calibrated: 2023-05-08
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn701; Calibrated: 2023-05-11
Phantom: Twin-SAM V8.0; Serial: 2029
Measurement SW: DASY Module SAR V16.2.0.1425

835.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.92 W/kg

SAR(1 g) = 1.85 W/kg

Deviation (1 g) = -5.52%

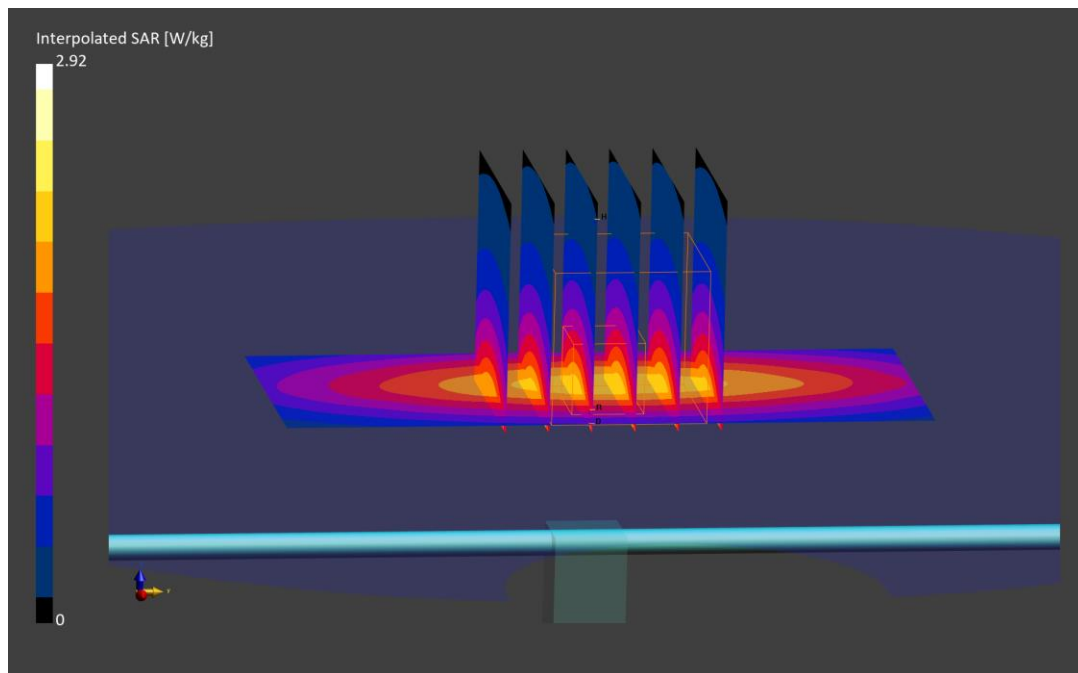

ELEMENT

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d040

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Head; Medium parameters used:
f = 835.0 MHz; cond = 0.922 S/m; perm = 41.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 12/13/2023; Ambient Temp: 20.9°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7416; ConvF:(9.73,9.73,9.73); Calibrated: 2023-05-08
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn701; Calibrated: 2023-05-11
Phantom: Twin-SAM V8.0; Serial: 2029
Measurement SW: DASY Module SAR V16.2.0.1425

835.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.98 W/kg

SAR(1 g) = 1.91 W/kg

Deviation (1 g) = -2.45%

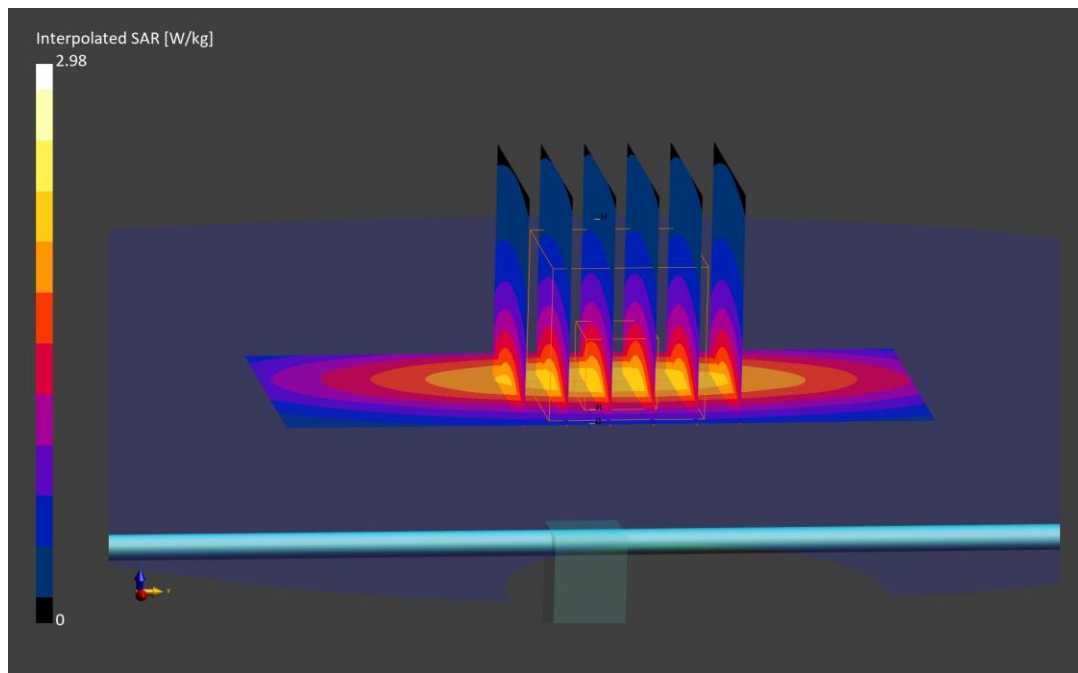

ELEMENT

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d040

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Head; Medium parameters used:
f = 835.0 MHz; cond = 0.906 S/m; perm = 41.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 12/15/2023; Ambient Temp: 20.6°C; Tissue Temp: 20.2°C

Probe: EX3DV4 - SN7416; ConvF:(9.73,9.73,9.73); Calibrated: 2023-05-08
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn701; Calibrated: 2023-05-11
Phantom: Twin-SAM V8.0; Serial: 2029
Measurement SW: DASY Module SAR V16.2.0.1425

835.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.85 W/kg

SAR(1 g) = 1.82 W/kg

Deviation (1 g) = -7.05%

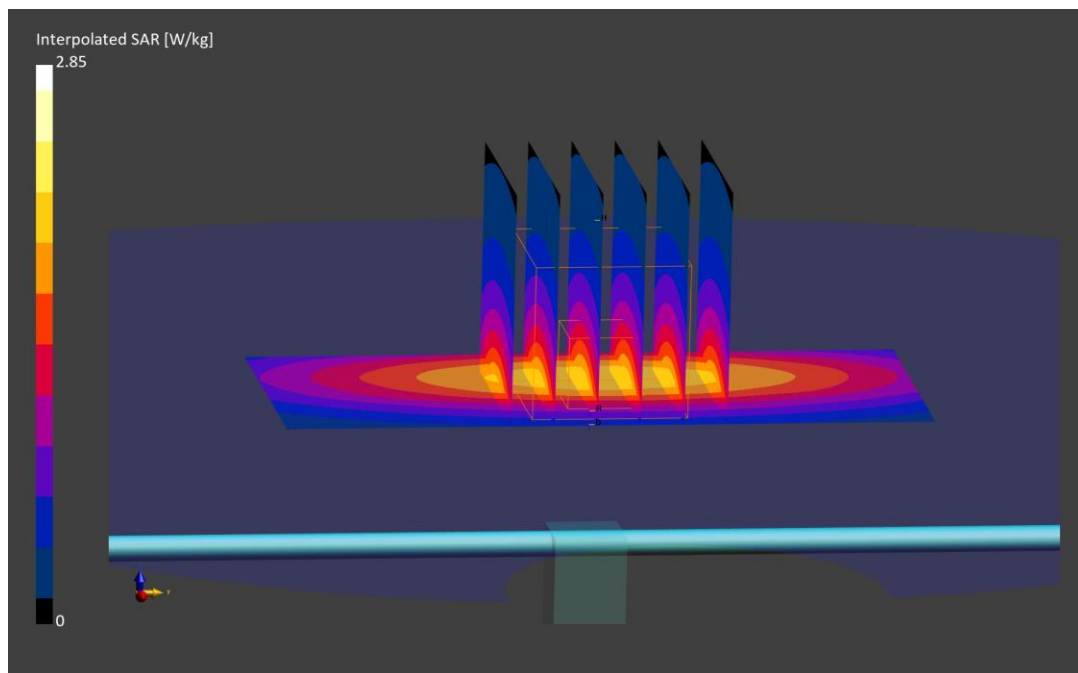

ELEMENT

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d040

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Head; Medium parameters used:
f = 835.0 MHz; cond = 0.916 S/m; perm = 40.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 01/31/2024; Ambient Temp: 20.9°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7416; ConvF:(9.73,9.73,9.73); Calibrated: 2023-05-08
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn701; Calibrated: 2023-05-11
Phantom: Twin-SAM V8.0; Serial: 2029
Measurement SW: DASY Module SAR V16.2.0.1425

835.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.98 W/kg

SAR(1 g) = 1.87 W/kg

Deviation (1 g) = -4.49%

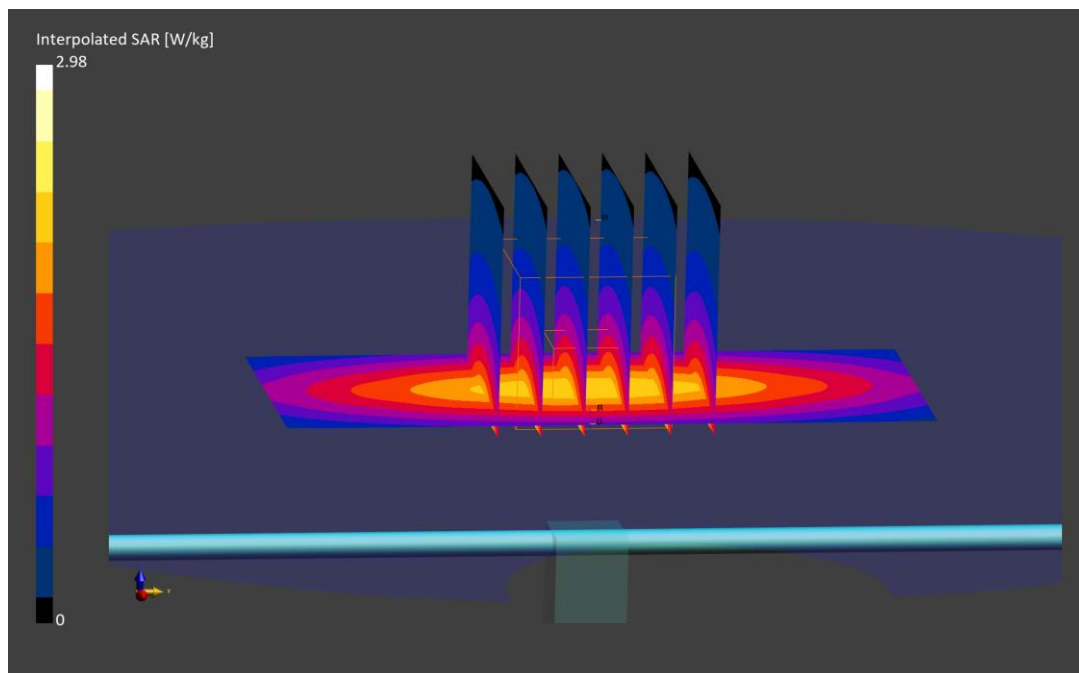

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1083

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.38 S/m; perm = 38.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/12/2023; Ambient Temp: 21.6°C; Tissue Temp: 19.7°C

Probe: EX3DV4 - SN7360; ConvF:(9.15,9.15,9.15); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn534; Calibrated: 2023-03-15
Phantom: Twin-SAM V4.0; Serial: 1447
Measurement SW: DASY Module SAR V16.2.0.1425

1750.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.76 W/kg

SAR(1 g) = 3.49 W/kg

Deviation (1 g) = -4.38%

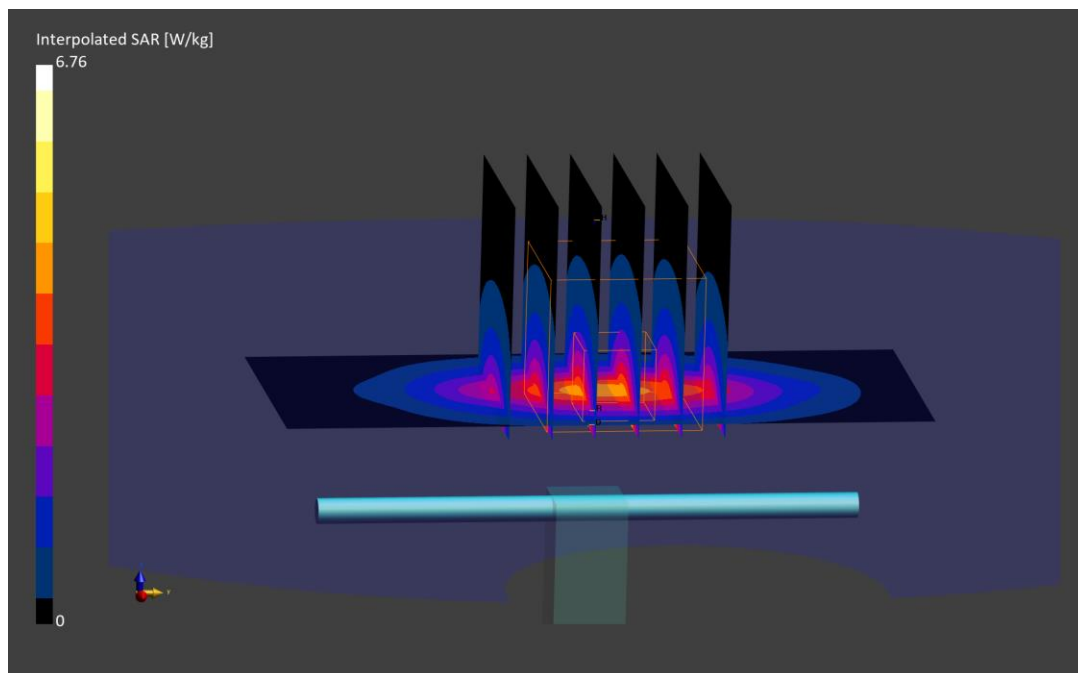

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1040

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.33 S/m; perm = 39.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test date: 12/12/2023; Ambient Temp: 23.7°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7639; ConvF:(8.98,8.98,8.98); Calibrated: 2023-11-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1403; Calibrated: 2023-11-14
Phantom: Twin-SAM V8.0; Serial: 2034
Measurement SW: DASY Module SAR V16.2.0.1425

1750.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.40 W/kg

SAR(1 g) = 3.52 W/kg

Deviation (1 g) = -3.30%

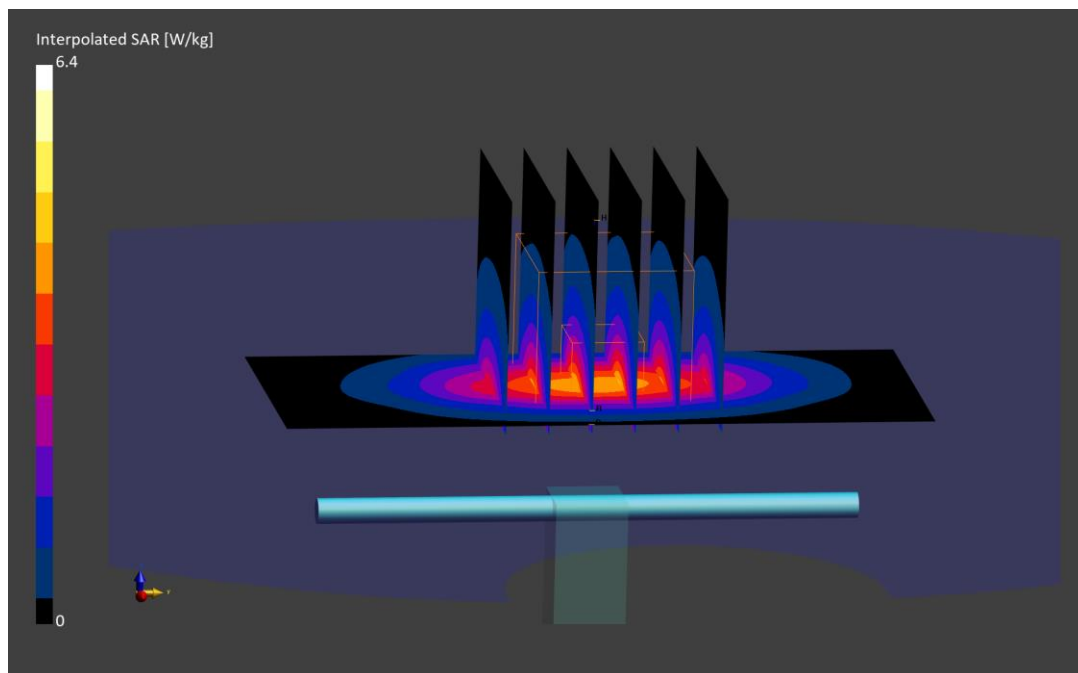

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1083

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.37 S/m; perm = 38.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/14/2023; Ambient Temp: 22.1°C; Tissue Temp: 19.5°C

Probe: EX3DV4 - SN7360; ConvF:(9.15,9.15,9.15); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn534; Calibrated: 2023-03-15
Phantom: Twin-SAM V4.0; Serial: 1447
Measurement SW: DASY Module SAR V16.2.0.1425

1750.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.78 W/kg

SAR(1 g) = 3.51 W/kg

Deviation (1 g) = -3.84%

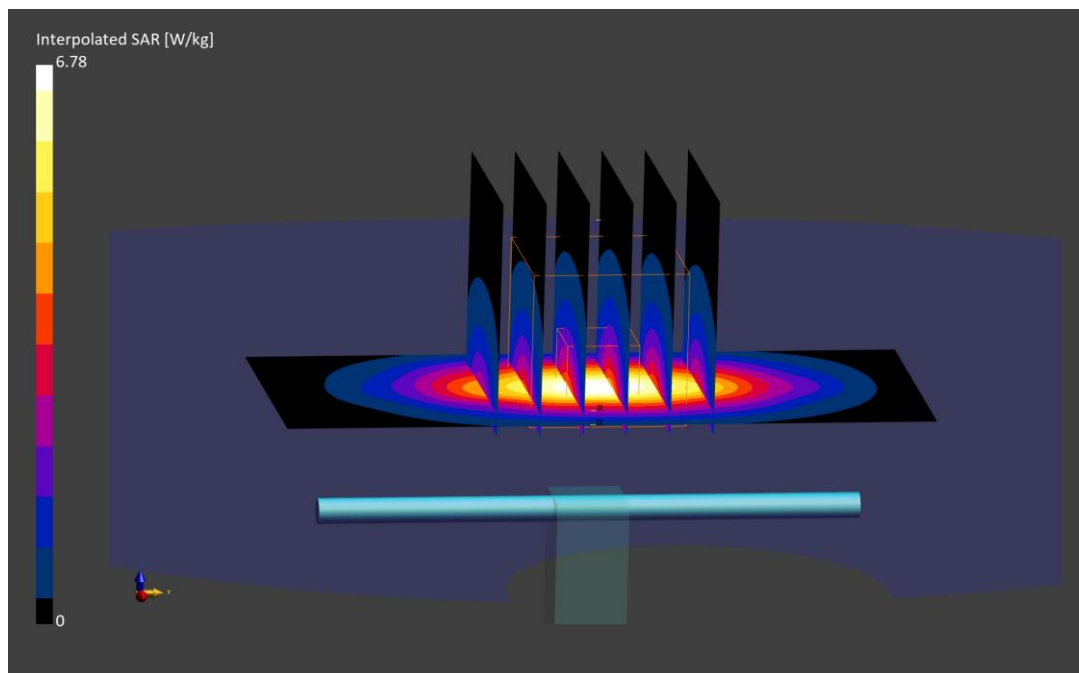

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1040

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.36 S/m; perm = 38.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 01/10/2024; Ambient Temp: 20.8°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7639; ConvF:(8.98,8.98,8.98); Calibrated: 2023-11-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1403; Calibrated: 2023-11-14
Phantom: Twin-SAM V8.0; Serial: 2034
Measurement SW: DASY Module SAR V16.2.0.1425

1750.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.39 W/kg

SAR(1 g) = 3.44 W/kg

Deviation (1 g) = -5.49%

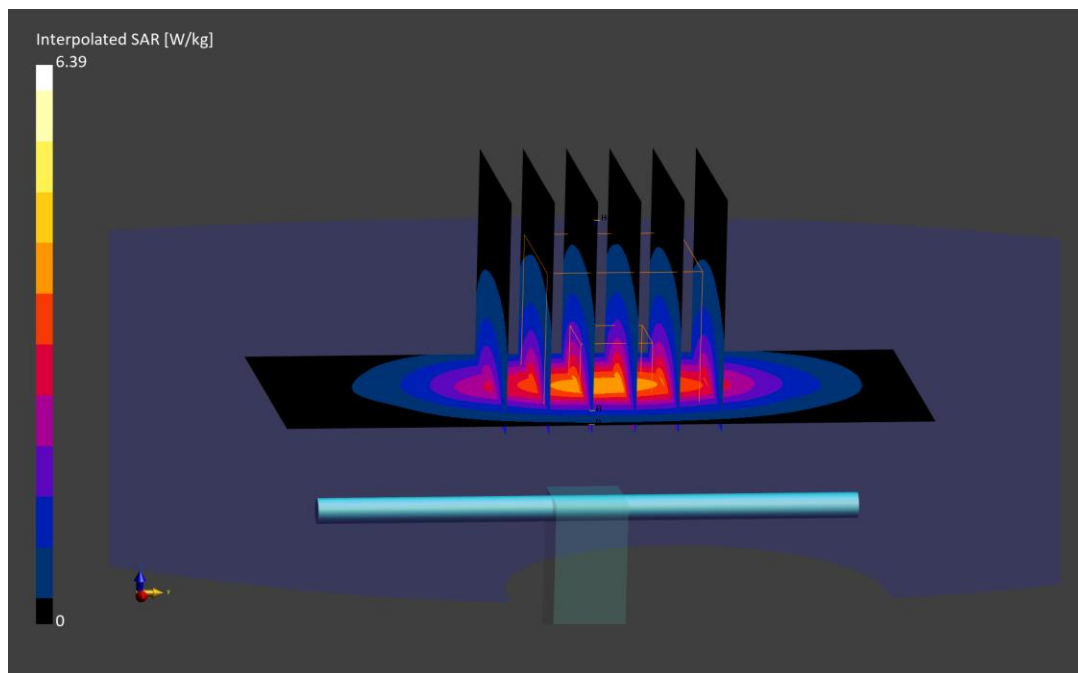

ELEMENT

DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d030

Communication System: UID: 0, CW; Frequency: 1900.0 MHz
Medium: 1900 Head; Medium parameters used:
f = 1900.0 MHz; cond = 1.42 S/m; perm = 38.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/16/2023; Ambient Temp: 20.1°C; Tissue Temp: 19.5°C

Probe: EX3DV4 - SN7357; ConvF:(8.3,8.3,8.3); Calibrated: 2023-04-13
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1582; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 1866
Measurement SW: DASY Module SAR V16.2.0.1425

1900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 8.12 W/kg

SAR(1 g) = 4.17 W/kg

Deviation (1 g) = 4.77%

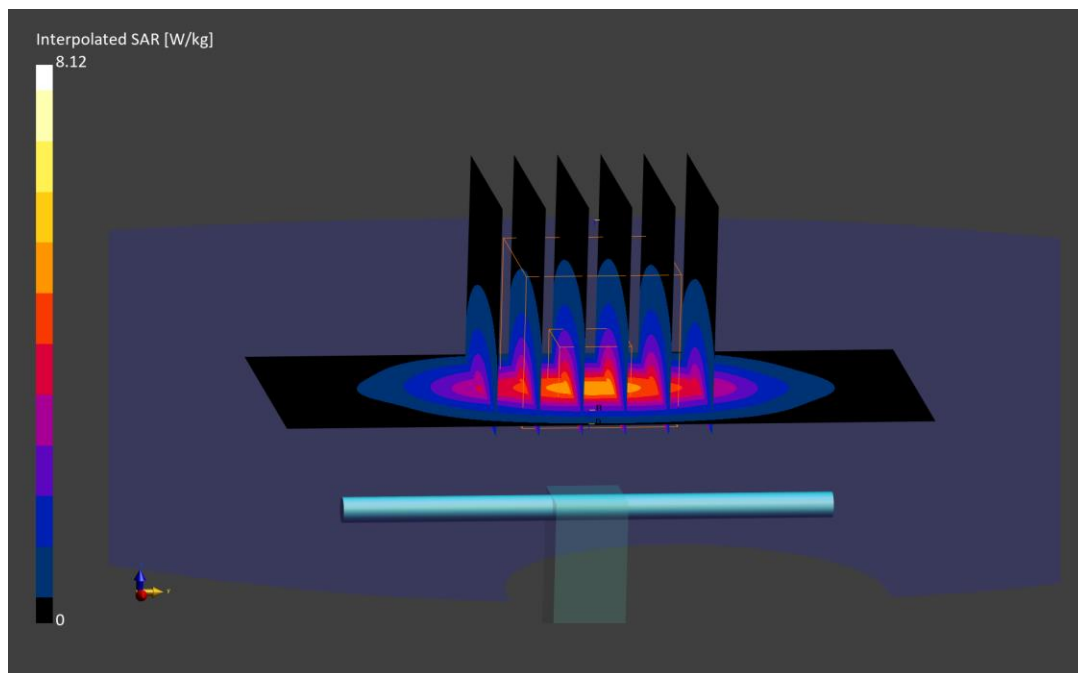

ELEMENT

DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d030

Communication System: UID: 0, CW; Frequency: 1900.0 MHz
Medium: 1900 Head; Medium parameters used:
f = 1900.0 MHz; cond = 1.43 S/m; perm = 38.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/18/2023; Ambient Temp: 21.8°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7357; ConvF:(8.3,8.3,8.3); Calibrated: 2023-04-13
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1582; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 1866
Measurement SW: DASY Module SAR V16.2.0.1425


1900.0 MHz System Verification at 20.0 dBm (100 mW)

Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5
Peak SAR (extrapolated) = 7.67 W/kg

SAR(1 g) = 3.92 W/kg

Deviation (1 g) = -1.51%

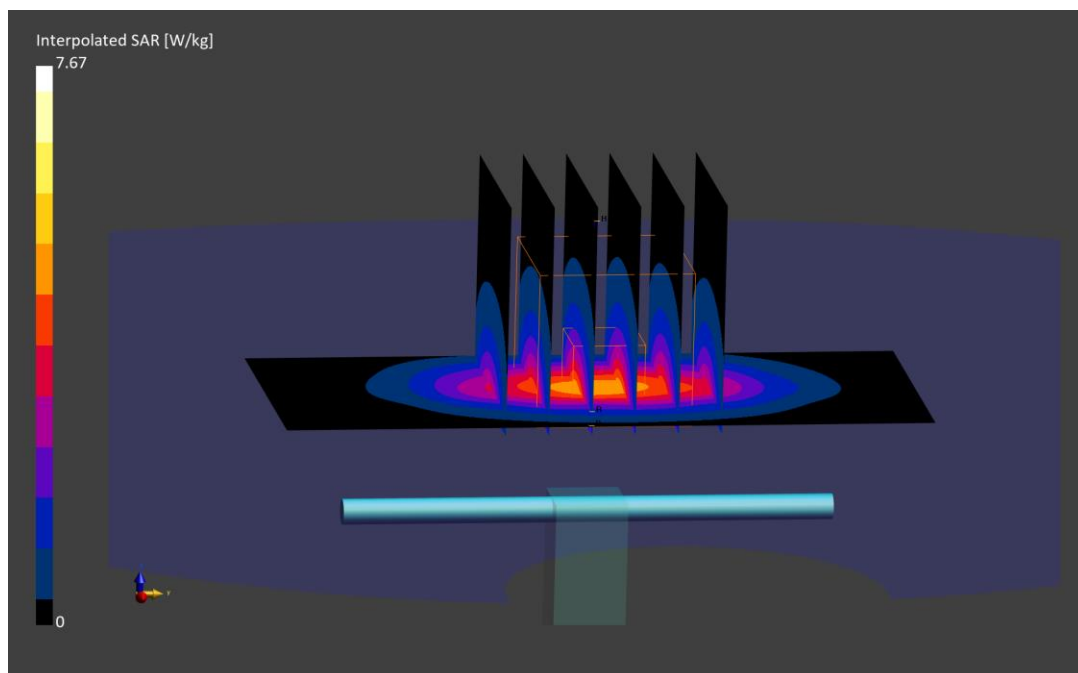

ELEMENT

DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1038

Communication System: UID: 0, CW; Frequency: 2300.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2300.0 MHz; cond = 1.66 S/m; perm = 41.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/13/2023; Ambient Temp: 20.3°C; Tissue Temp: 19.2°C

Probe: EX3DV4 - SN7532; ConvF:(8.2,8.2,8.2); Calibrated: 2023-04-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn501; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 2067
Measurement SW: DASY Module SAR V16.2.0.1425

2300.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.97 W/kg

SAR(1 g) = 4.88 W/kg

Deviation (1 g) = 0.41%

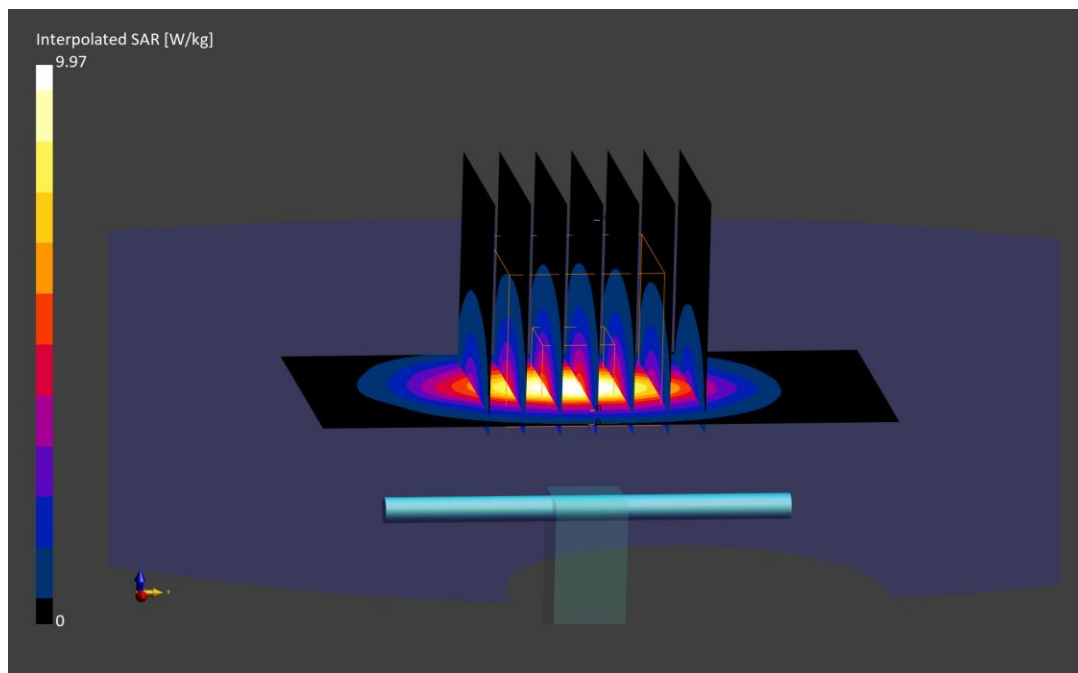

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.74 S/m; perm = 39.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/13/2023; Ambient Temp: 20.3°C; Tissue Temp: 19.7°C

Probe: EX3DV4 - SN7421; ConvF:(7.45,7.45,7.45); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn604; Calibrated: 2023-03-15
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.0.1425

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.3 W/kg

SAR(1 g) = 5.42 W/kg

Deviation (1 g) = 0.00%

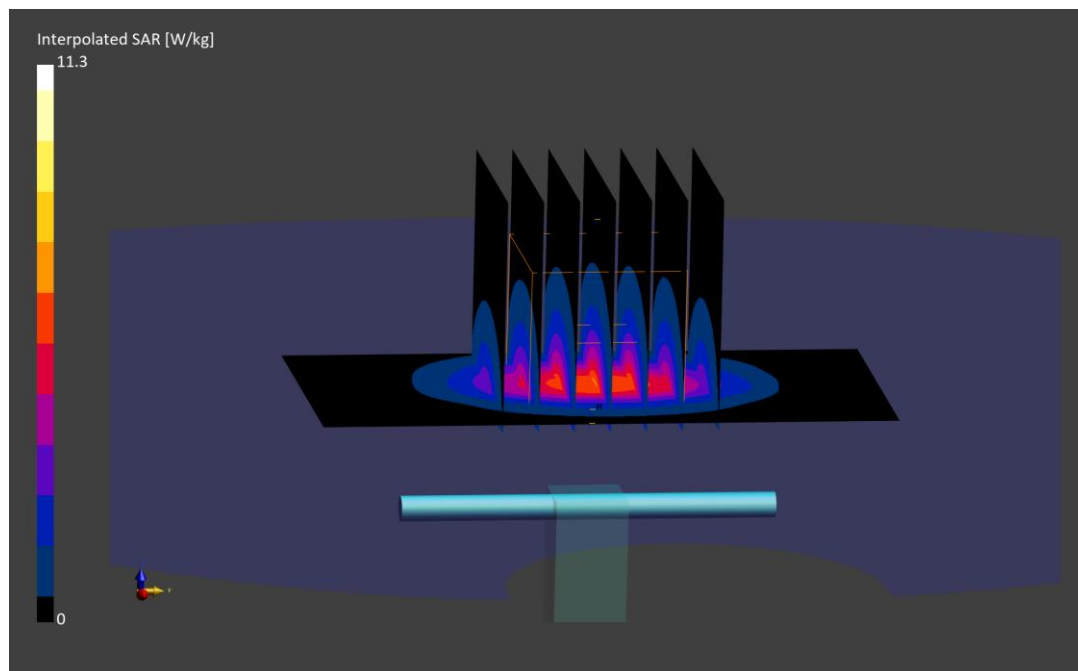

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.77 S/m; perm = 40.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/15/2023; Ambient Temp: 20.9°C; Tissue Temp: 19.1°C

Probe: EX3DV4 - SN7421; ConvF:(7.45,7.45,7.45); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn604; Calibrated: 2023-03-15
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.0.1425

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.4 W/kg

SAR(1 g) = 5.10 W/kg

Deviation (1 g) = -5.90%

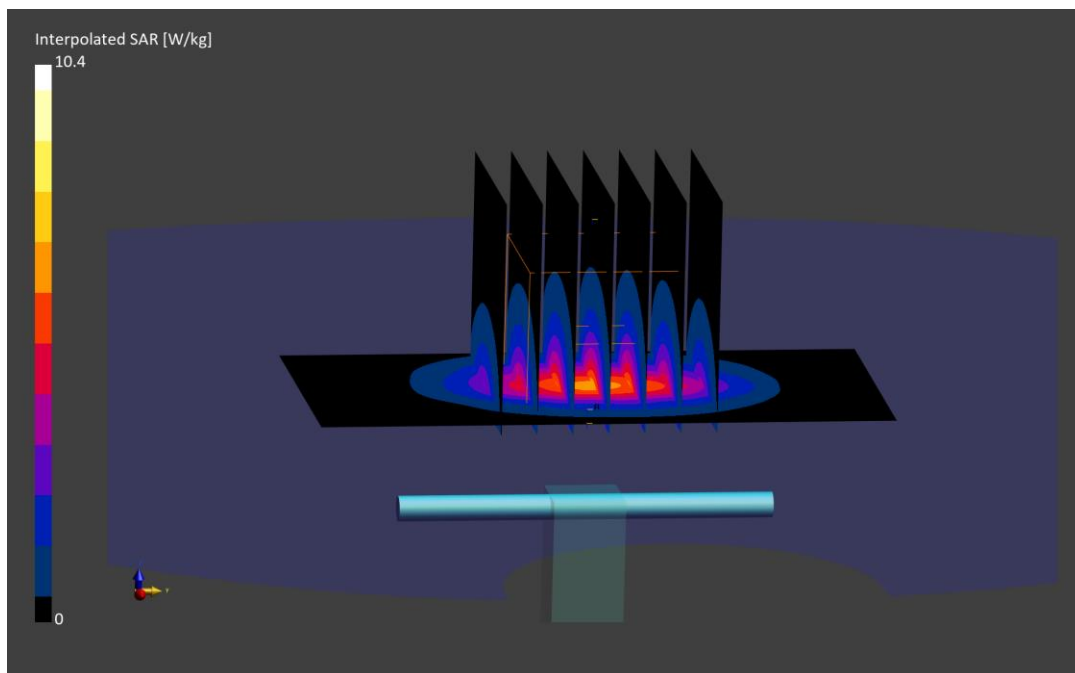

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.85 S/m; perm = 39.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/22/2023; Ambient Temp: 20.8°C; Tissue Temp: 22.0°C

Probe: EX3DV4 - SN7532; ConvF:(7.88,7.88,7.88); Calibrated: 2023-04-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn501; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 2067
Measurement SW: DASY Module SAR V16.2.0.1425

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.8 W/kg

SAR(1 g) = 5.26 W/kg

Deviation (1 g) = -2.95%

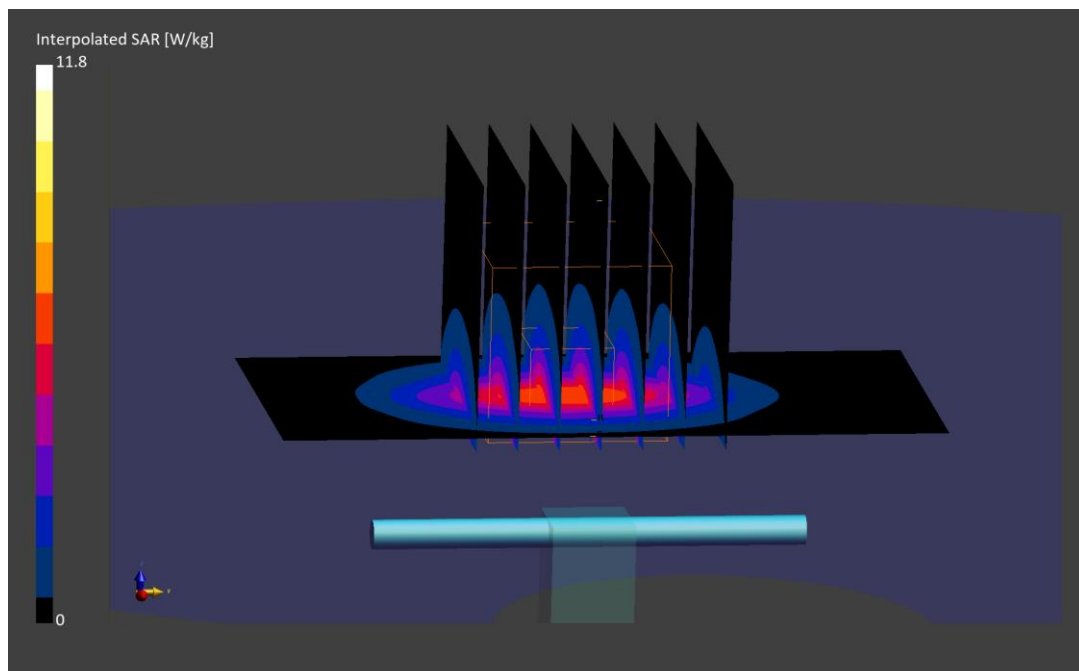

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.87 S/m; perm = 38.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/26/2023; Ambient Temp: 22.5°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN7546; ConvF:(7.29,7.29,7.29); Calibrated: 2023-04-14
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1402; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 1935
Measurement SW: DASY Module SAR V16.2.0.1425

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.8 W/kg

SAR(1 g) = 5.42 W/kg

Deviation (1 g) = 3.04%

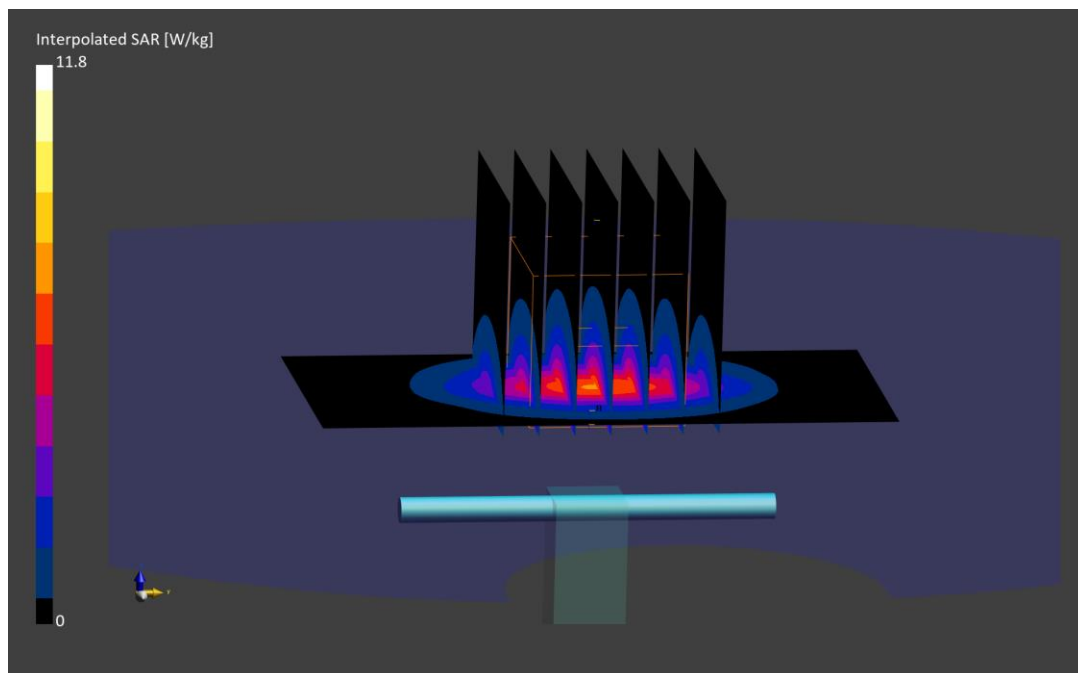

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921

Communication System: UID: 0, CW; Frequency: 2450.0 MHz

Medium: 2450 Head; Medium parameters used:

f = 2450.0 MHz; cond = 1.78 S/m; perm = 40.5; density = 1000 kg/m³

Phantom Section: Flat; Space: 10 mm

Test Date: 02/21/2024; Ambient Temp: 21.5°C; Tissue Temp: 19.9°C

Probe: EX3DV4 - SN7421; ConvF:(7.45,7.45,7.45); Calibrated: 2023-03-16

Sensor-Surface: 1.4mm (VMS + 6p)

Electronics: DAE4 Sn604; Calibrated: 2023-03-15

Phantom: Twin-SAM V8.0; Serial: 2070

Measurement SW: DASY Module SAR V16.2.0.1425

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.2 W/kg

SAR(1 g) = 5.37 W/kg

Deviation (1 g) = -0.92%

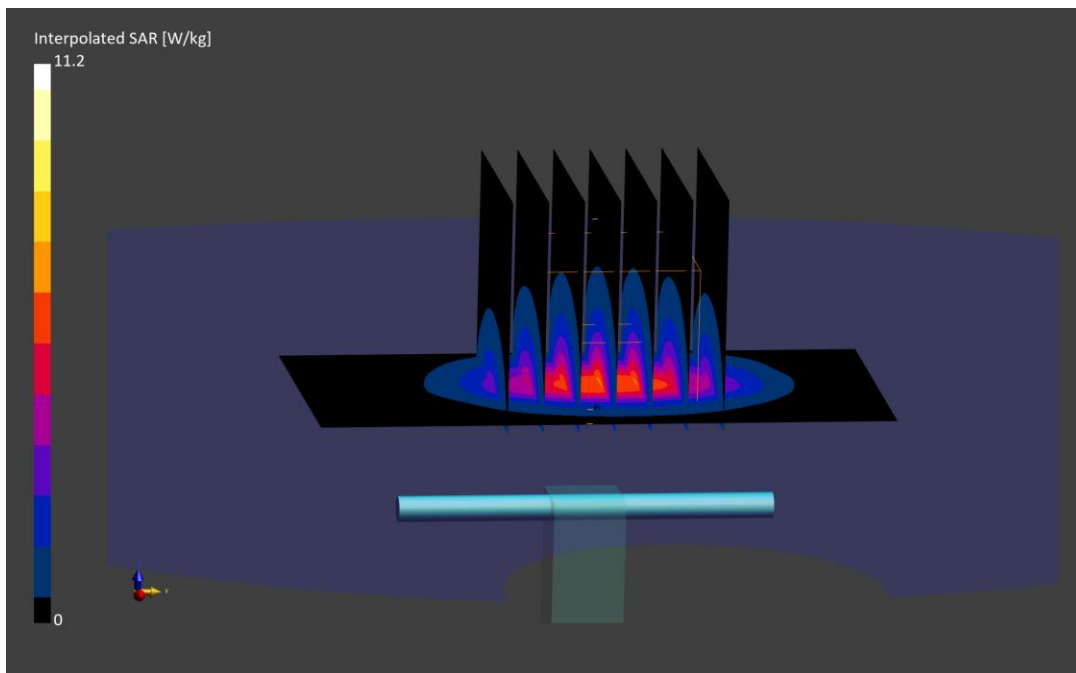

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1042

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 2.03 S/m; perm = 37.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/20/2023; Ambient Temp: 23.5°C; Tissue Temp: 22.6°C

Probe: EX3DV4 - SN7546; ConvF:(7.08,7.08,7.08); Calibrated: 2023-04-14
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1402; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 1935
Measurement SW: DASY Module SAR V16.2.0.1425

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.7 W/kg

SAR(1 g) = 5.59 W/kg

Deviation (1 g) = 0.18%

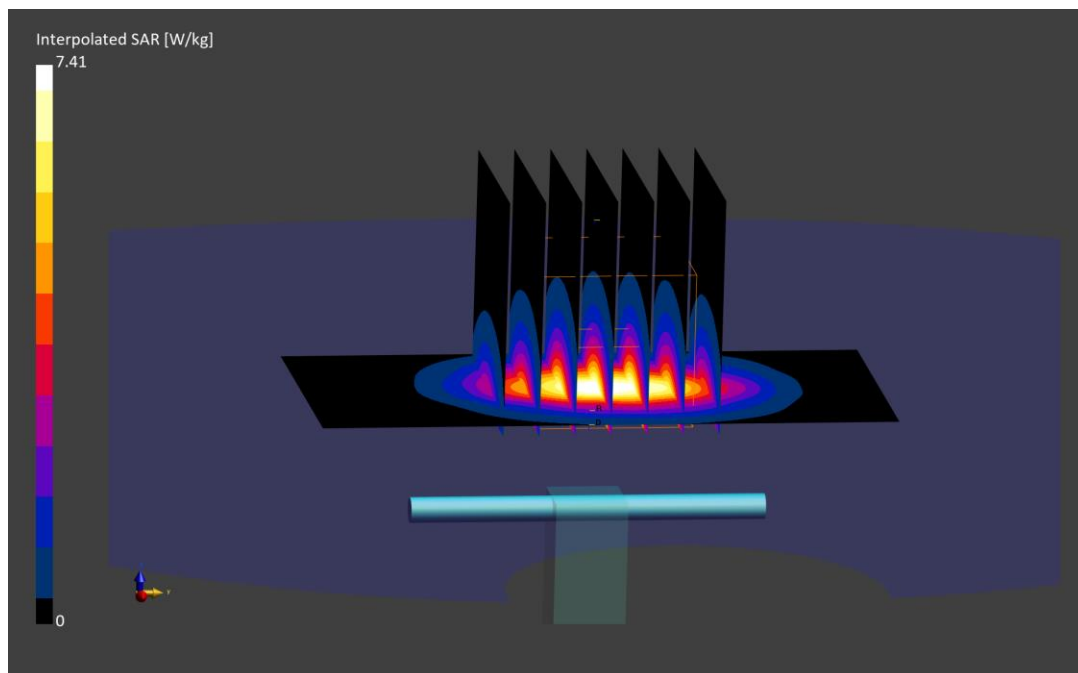

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1068

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 2.03 S/m; perm = 38.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/22/2023; Ambient Temp: 20.8°C; Tissue Temp: 22.0°C

Probe: EX3DV4 - SN7532; ConvF:(7.53,7.53,7.53); Calibrated: 2023-04-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn501; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 2067
Measurement SW: DASY Module SAR V16.2.0.1425

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.8 W/kg

SAR(1 g) = 5.58 W/kg

Deviation (1 g) = -1.24%

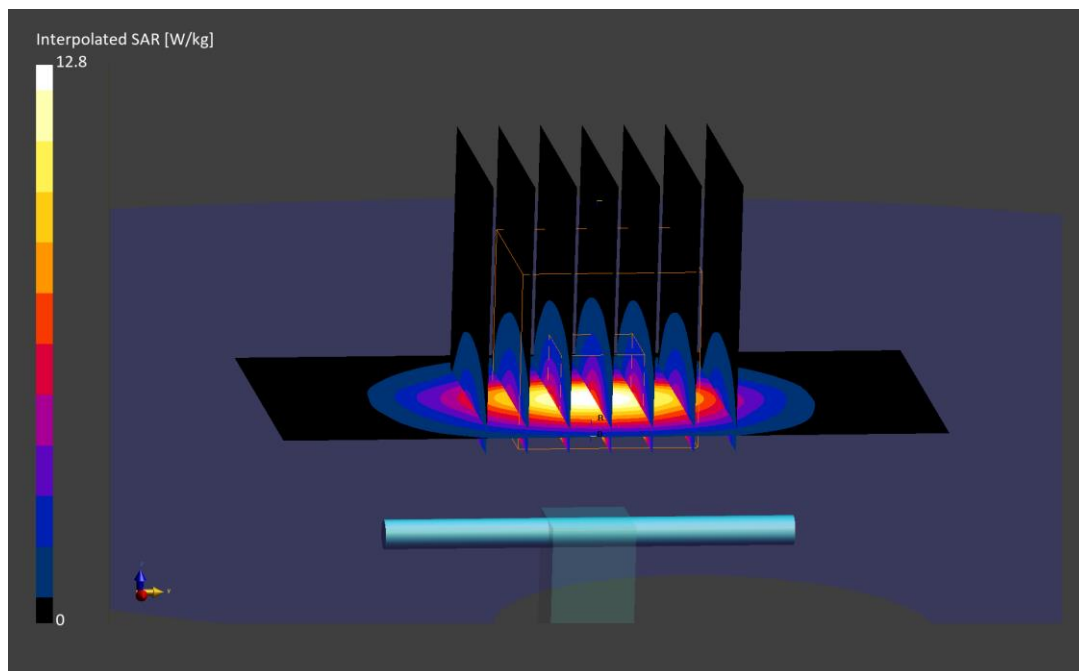

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1042

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 2.04 S/m; perm = 37.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/26/2023; Ambient Temp: 22.5°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN7546; ConvF:(7.08,7.08,7.08); Calibrated: 2023-04-14
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1402; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 1935
Measurement SW: DASY Module SAR V16.2.0.1425

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 13.2 W/kg

SAR(1 g) = 5.83 W/kg

Deviation (1 g) = 4.48%

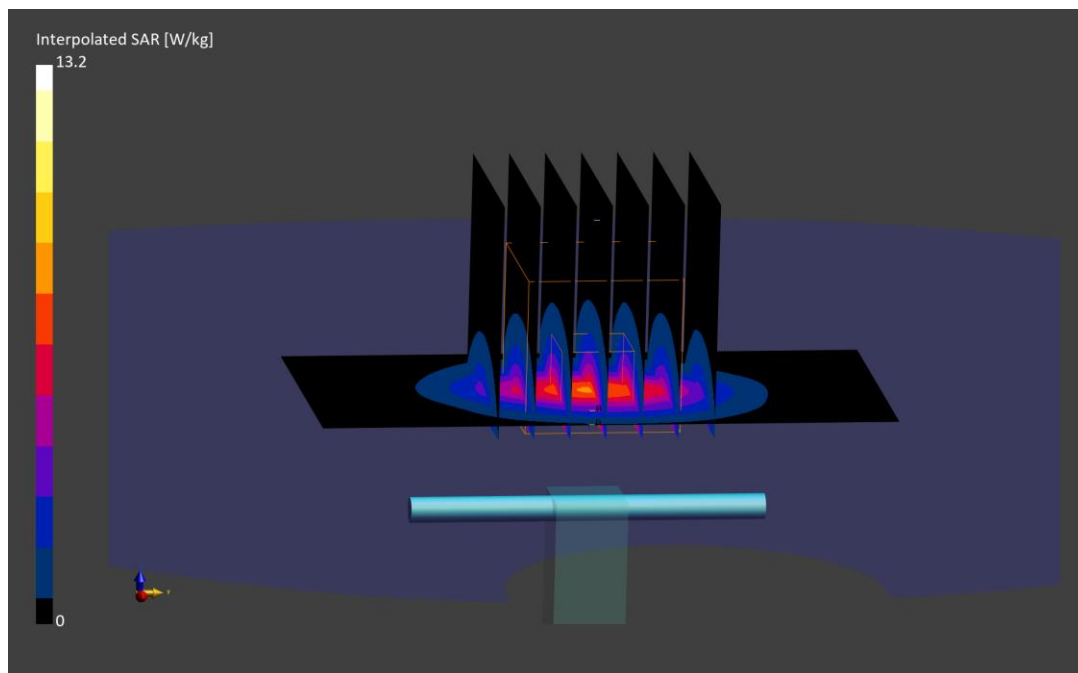

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1068

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 2.04 S/m; perm = 37.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 03/02/2024; Ambient Temp: 21.2°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7532; ConvF:(7.53,7.53,7.53); Calibrated: 2023-04-18
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn501; Calibrated: 2023-04-14
Phantom: Twin-SAM V8.0; Serial: 2067
Measurement SW: DASY Module SAR V16.2.0.1425

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 13.2 W/kg

SAR(1 g) = 5.67 W/kg

Deviation (1 g) = 0.35%

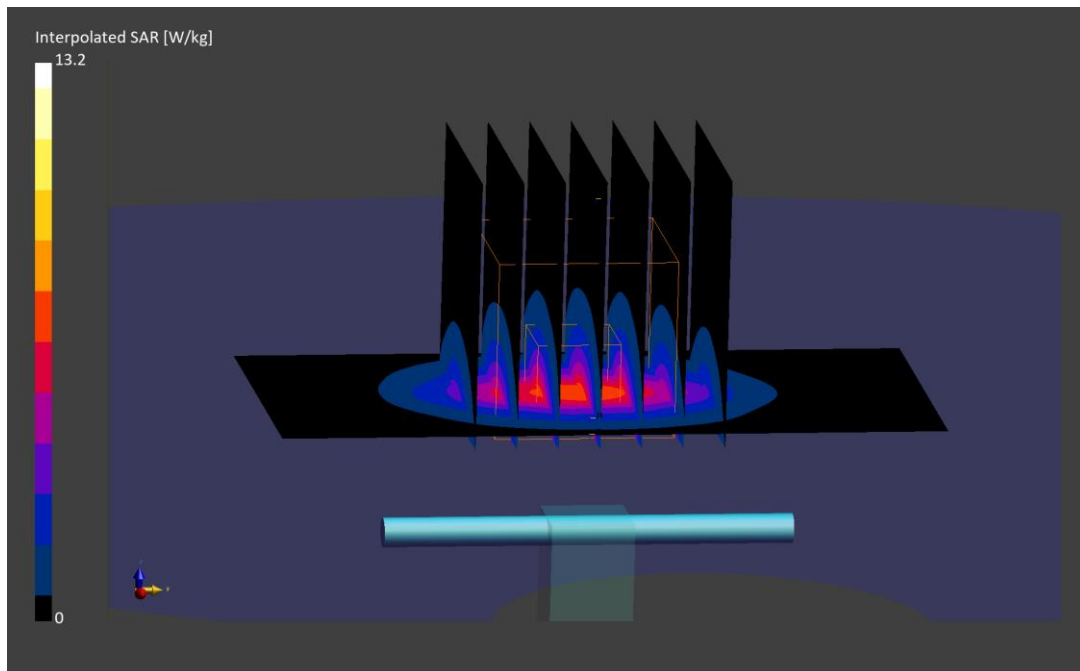

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1126

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 2.96 S/m; perm = 36.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/10/2023; Ambient Temp: 21.0°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN7782; ConvF:(6.19,6.19,6.19); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 19.4 W/kg

SAR(1 g) = 6.66 W/kg

Deviation (1 g) = -0.60%

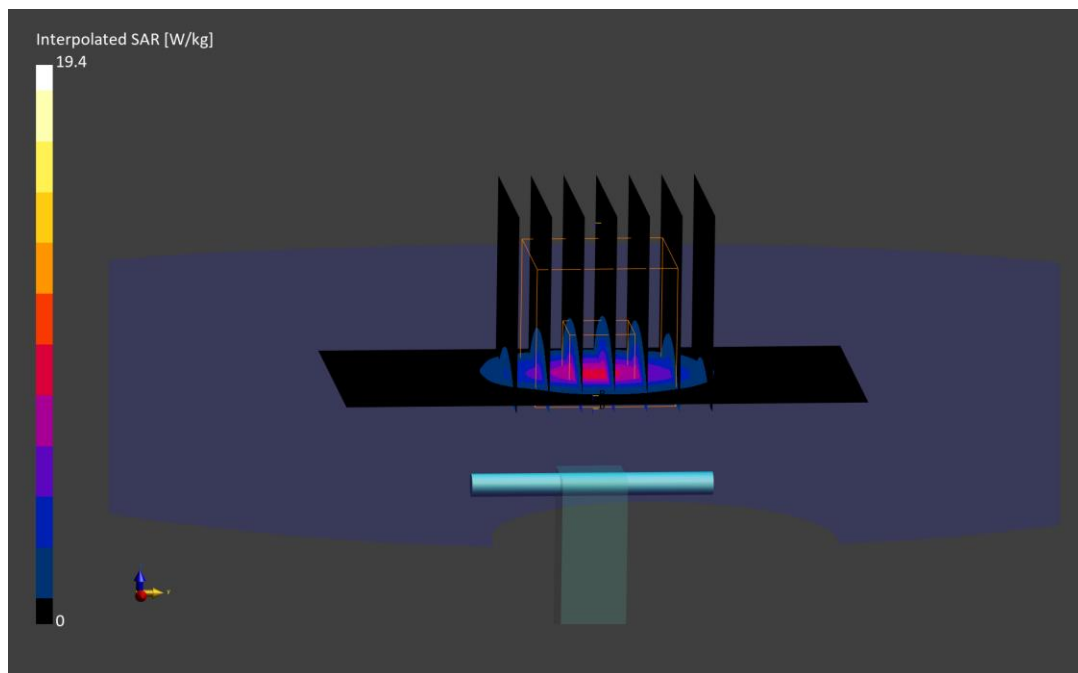

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1126

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 2.86 S/m; perm = 38.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/12/2023; Ambient Temp: 20.3°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7638; ConvF:(7.02,7.02,7.02); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1408; Calibrated: 2023-03-13
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.0.1425

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.5 W/kg

SAR(1 g) = 7.02 W/kg

Deviation (1 g) = 4.78%

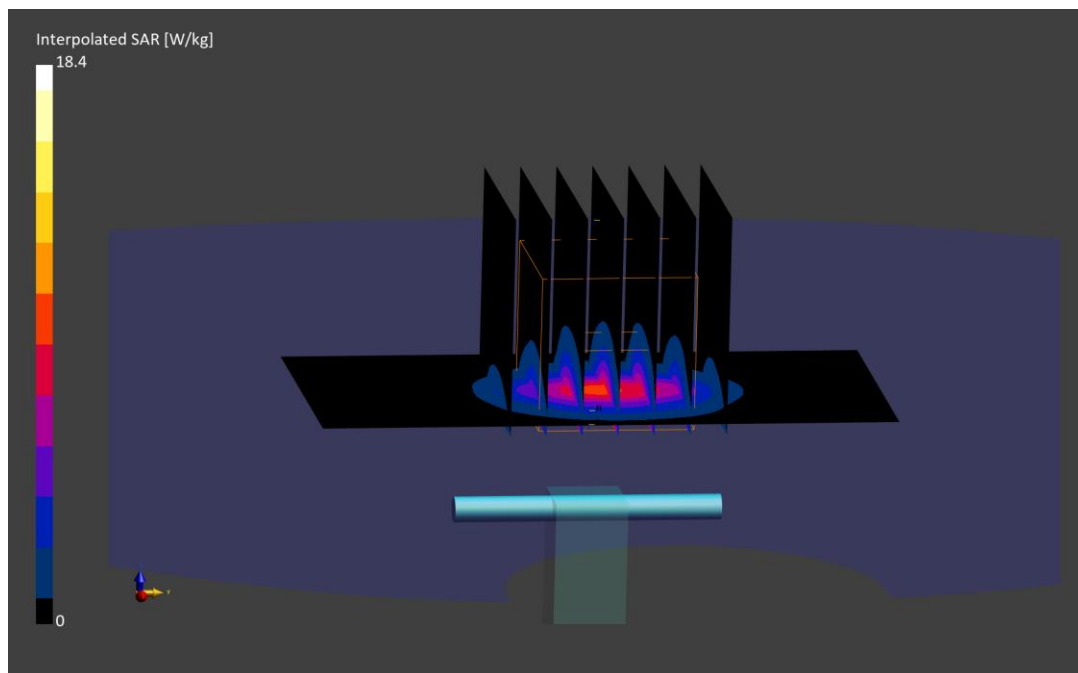

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1055

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 2.91 S/m; perm = 38.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/18/2023; Ambient Temp: 20.7°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7638; ConvF:(7.02,7.02,7.02); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1408; Calibrated: 2023-03-13
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.0.1425

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.7 W/kg

SAR(1 g) = 6.91 W/kg

Deviation (1 g) = 4.70%

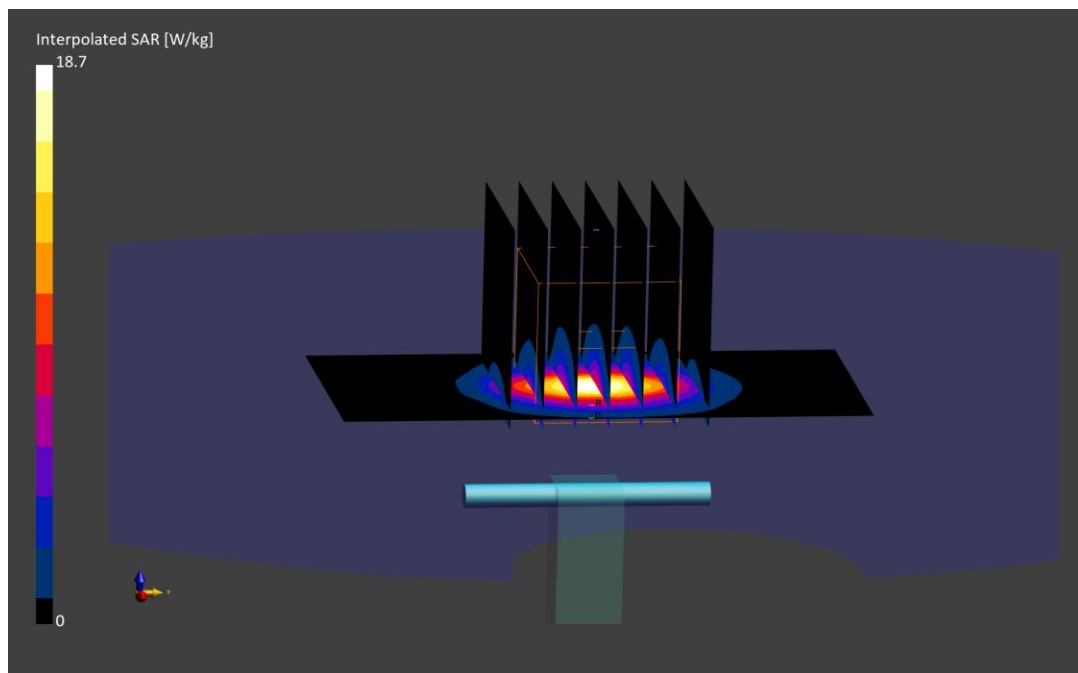

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1126

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 3.05 S/m; perm = 36.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/19/2023; Ambient Temp: 23.2°C; Tissue Temp: 22.2°C

Probe: EX3DV4 - SN7782; ConvF:(6.19,6.19,6.19); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 20.2 W/kg

SAR(1 g) = 7.10 W/kg

Deviation (1 g) = 5.97%

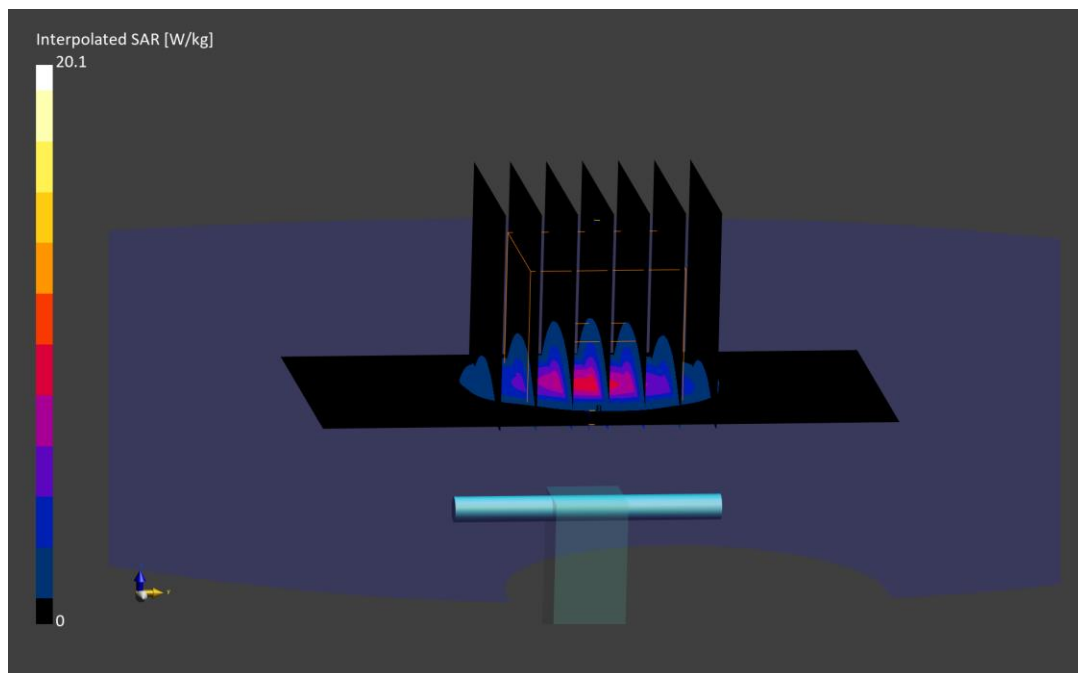

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1097

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.11 S/m; perm = 36.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/10/2023; Ambient Temp: 21.0°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN7782; ConvF:(6.18,6.18,6.18); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 20.3 W/kg

SAR(1 g) = 6.82 W/kg

Deviation (1 g) = 0.15%

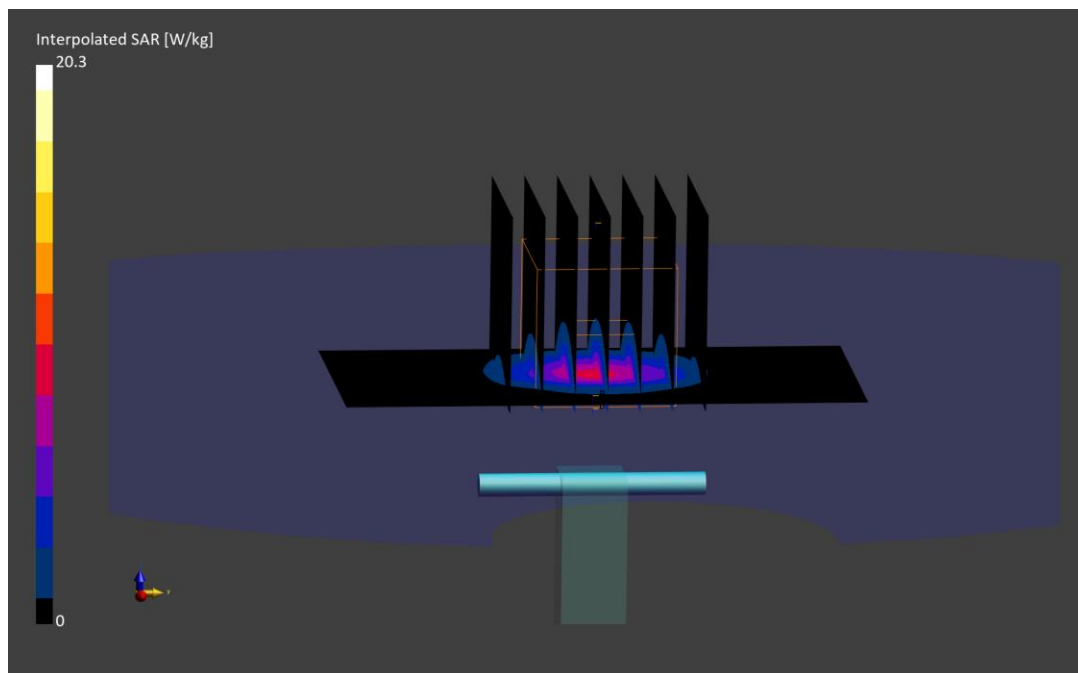

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1097

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.02 S/m; perm = 37.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/12/2023; Ambient Temp: 20.3°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7638; ConvF:(6.99,6.99,6.99); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1408; Calibrated: 2023-03-13
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASYS Module SAR V16.2.0.1425

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 17.4 W/kg

SAR(1 g) = 6.36 W/kg

Deviation (1 g) = -6.61%

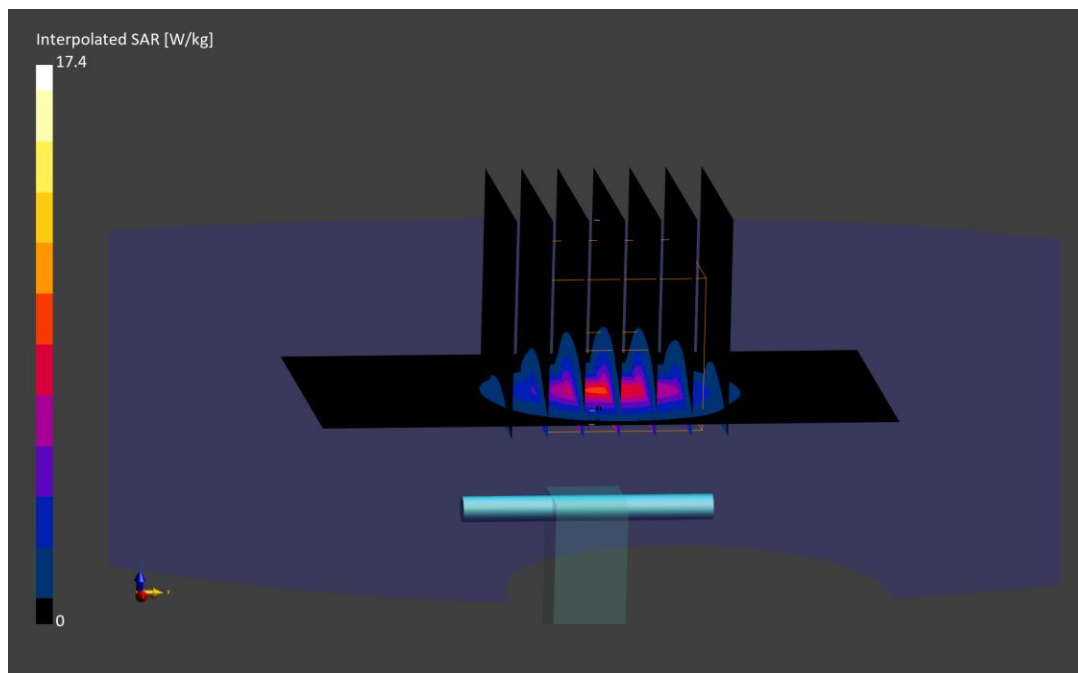

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1002

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.07 S/m; perm = 38.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/18/2023; Ambient Temp: 20.7°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7638; ConvF:(6.99,6.99,6.99); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1408; Calibrated: 2023-03-13
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.0.1425

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.6 W/kg

SAR(1 g) = 6.65 W/kg

Deviation (1 g) = -2.06%

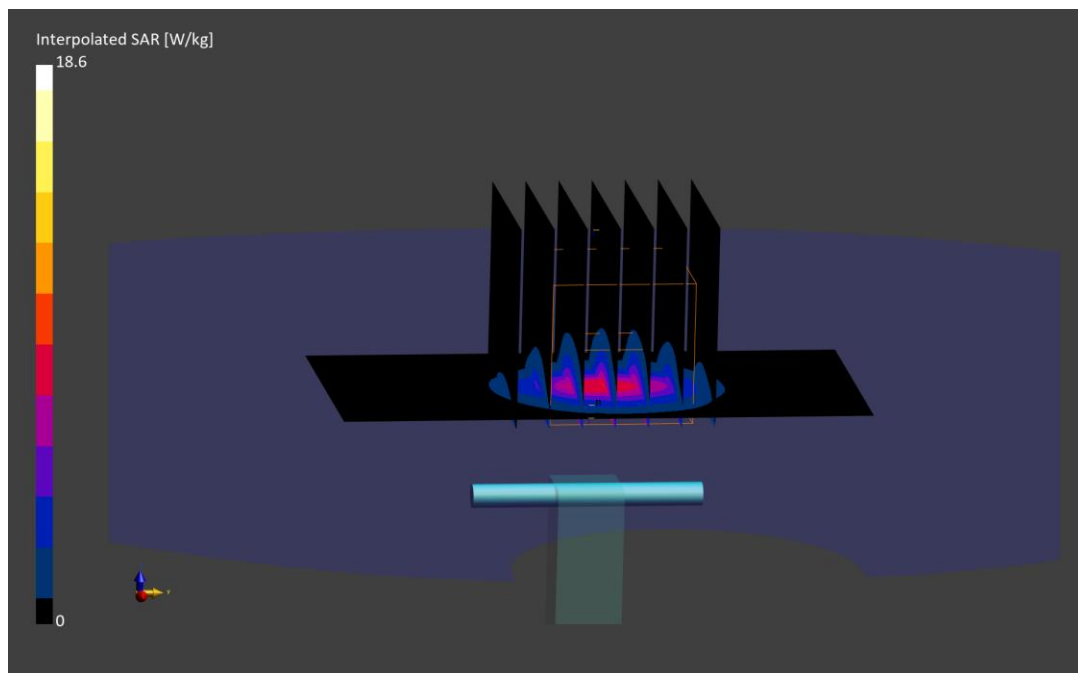

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1097

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.22 S/m; perm = 36.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/19/2023; Ambient Temp: 23.2°C; Tissue Temp: 22.2°C

Probe: EX3DV4 - SN7782; ConvF:(6.18,6.18,6.18); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 20.7 W/kg

SAR(1 g) = 7.02 W/kg

Deviation (1 g) = 3.08%

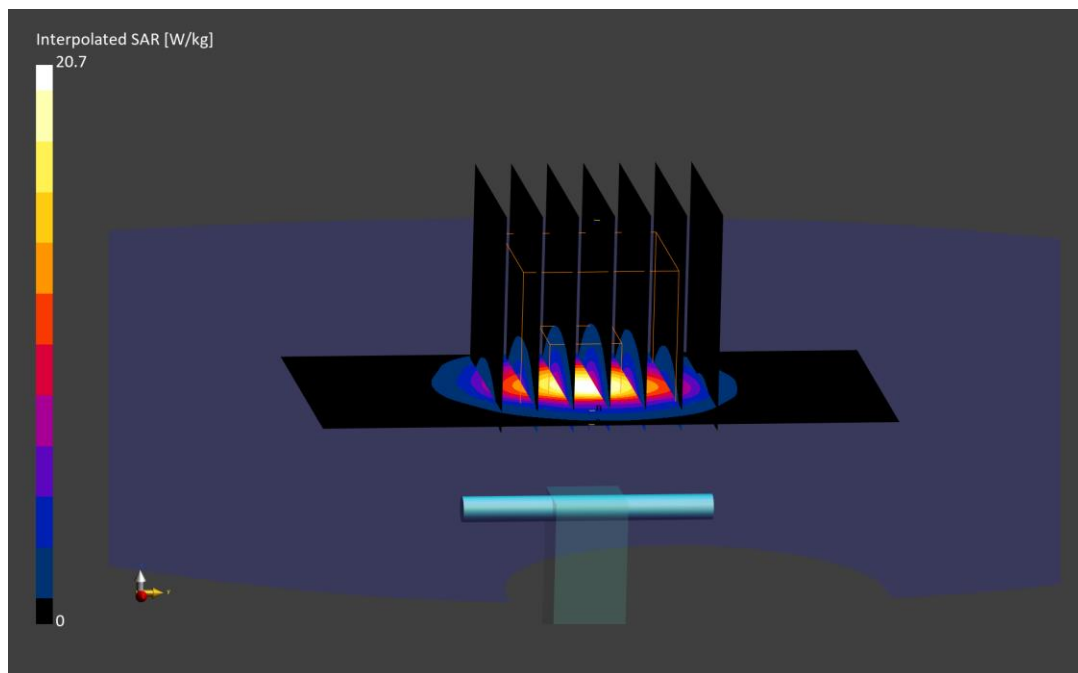

ELEMENT

DUT: Dipole 3900.0 MHz; Type: D3900V2 - SN1073

Communication System: UID: 0, CW; Frequency: 3900.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3900.0 MHz; cond = 3.28 S/m; perm = 36.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/10/2023; Ambient Temp: 21.0°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN7782; ConvF:(5.65,5.65,5.65); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.0.1425

3900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 21.7 W/kg

SAR(1 g) = 7.48 W/kg

Deviation (1 g) = 7.32%

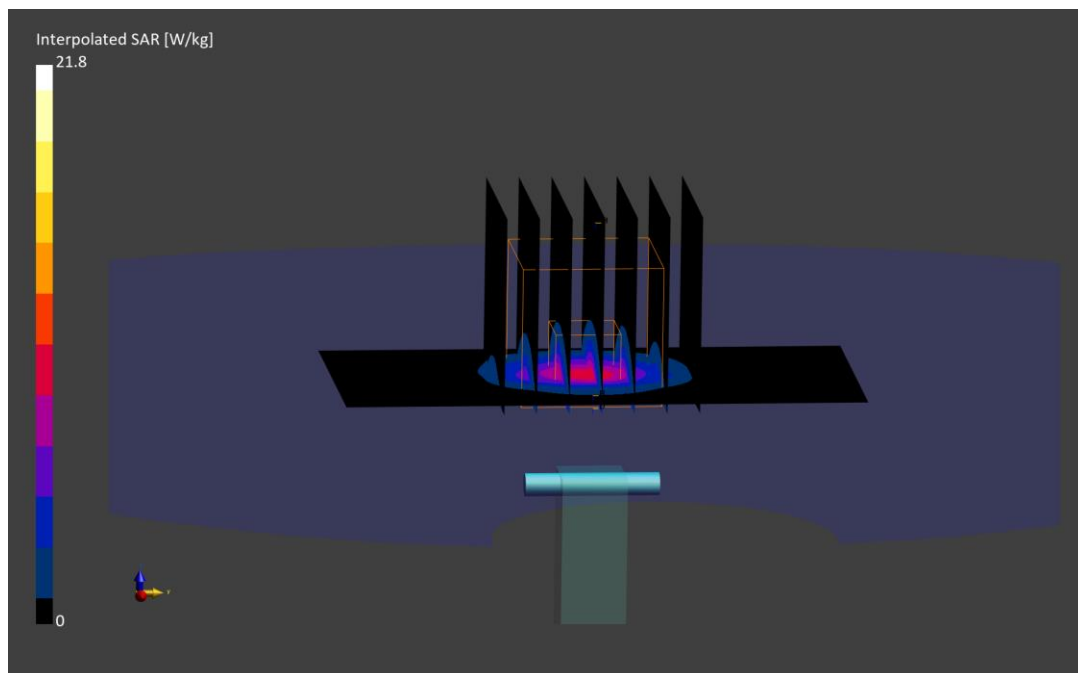

ELEMENT

DUT: Dipole 3900.0 MHz; Type: D3900V2 - SN1073

Communication System: UID: 0, CW; Frequency: 3900.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3900.0 MHz; cond = 3.20 S/m; perm = 37.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/12/2023; Ambient Temp: 20.3°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7638; ConvF:(6.92,6.92,6.92); Calibrated: 2023-03-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1408; Calibrated: 2023-03-13
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.0.1425

3900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 19.5 W/kg

SAR(1 g) = 6.71 W/kg

Deviation (1 g) = -3.73%

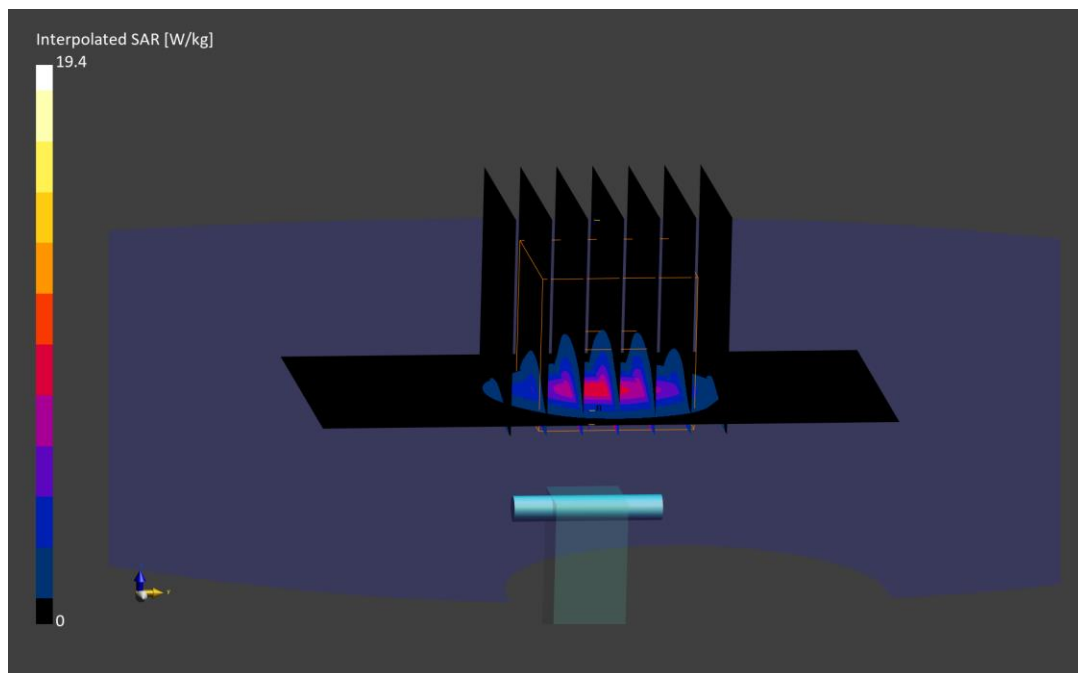

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5250.0 MHz; cond = 4.50 S/m; perm = 35.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/14/2023; Ambient Temp: 20.4°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN3746; ConvF:(5.12,5.12,5.12); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.2.0.1425

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.2 W/kg

SAR(1 g) = 3.74 W/kg

Deviation (1 g) = -7.08%

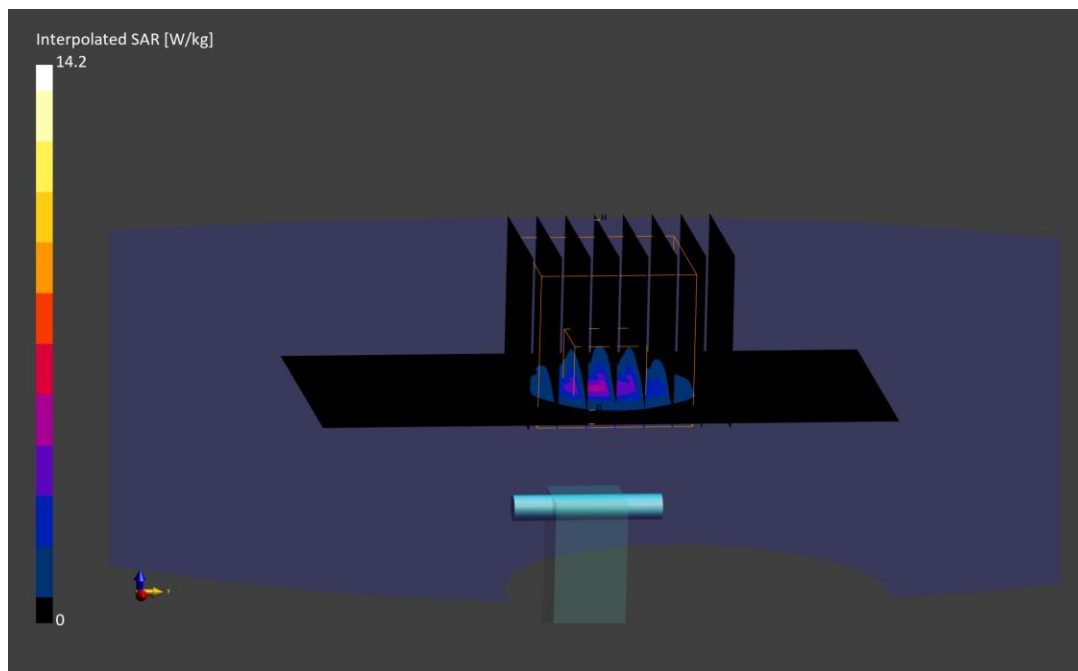

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5250.0 MHz; cond = 4.65 S/m; perm = 35.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/26/2023; Ambient Temp: 21.1°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN3949; ConvF:(5.74,5.74,5.74); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.0.1425

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.2 W/kg

SAR(1 g) = 3.95 W/kg

Deviation (1 g) = -1.86%

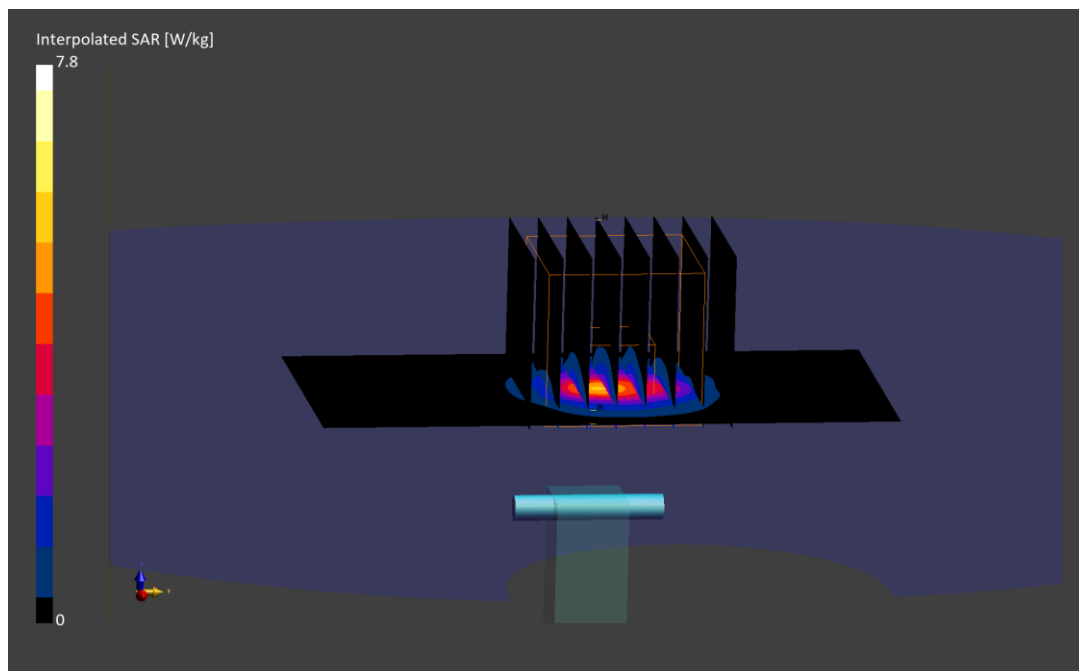

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5600.0 MHz; cond = 4.89 S/m; perm = 34.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/14/2023; Ambient Temp: 20.4°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN3746; ConvF:(4.45,4.45,4.45); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.2.0.1425

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.3 W/kg

SAR(1 g) = 3.94 W/kg

Deviation (1 g) = -5.85%

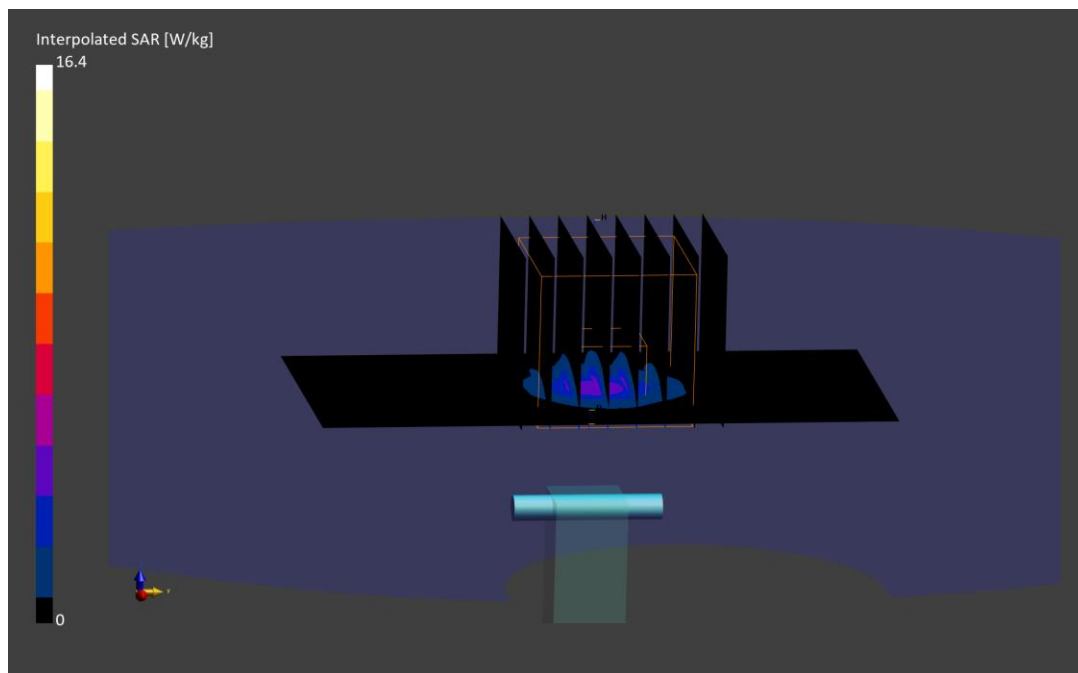

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5600.0 MHz; cond = 5.05 S/m; perm = 35.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/26/2023; Ambient Temp: 21.1°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN3949; ConvF:(5.11,5.11,5.11); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.0.1425

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.5 W/kg

SAR(1 g) = 3.99 W/kg

Deviation (1 g) = -4.66%

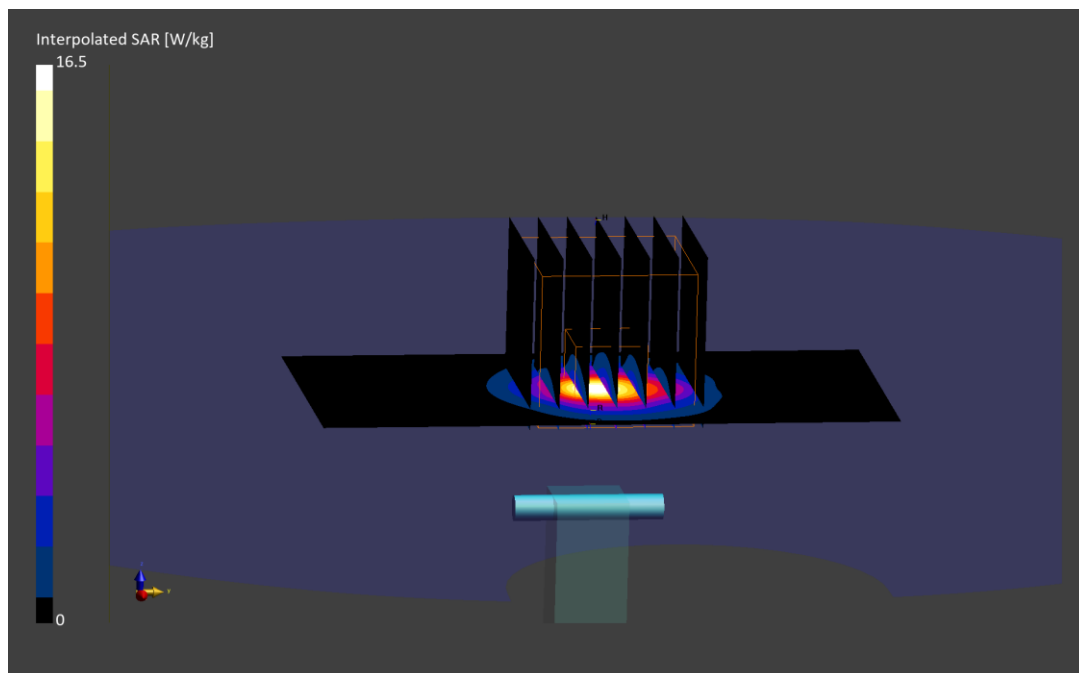

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5750.0 MHz; cond = 5.06 S/m; perm = 34.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/14/2023; Ambient Temp: 20.4°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN3746; ConvF:(4.59,4.59,4.59); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.2.0.1425

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.0 W/kg

SAR(1 g) = 3.95 W/kg

Deviation (1 g) = -1.86%

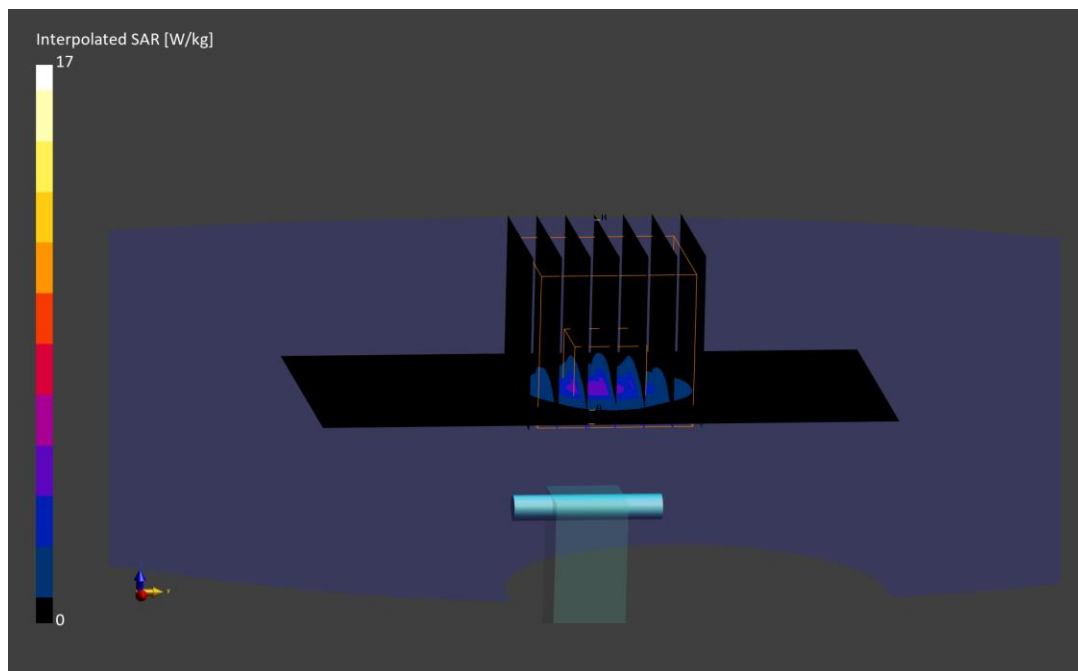

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5750.0 MHz; cond = 5.23 S/m; perm = 34.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/26/2023; Ambient Temp: 21.1°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN3949; ConvF:(5.31,5.31,5.31); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASy Module SAR V16.2.0.1425

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.3 W/kg

SAR(1 g) = 3.87 W/kg

Deviation (1 g) = -3.85%

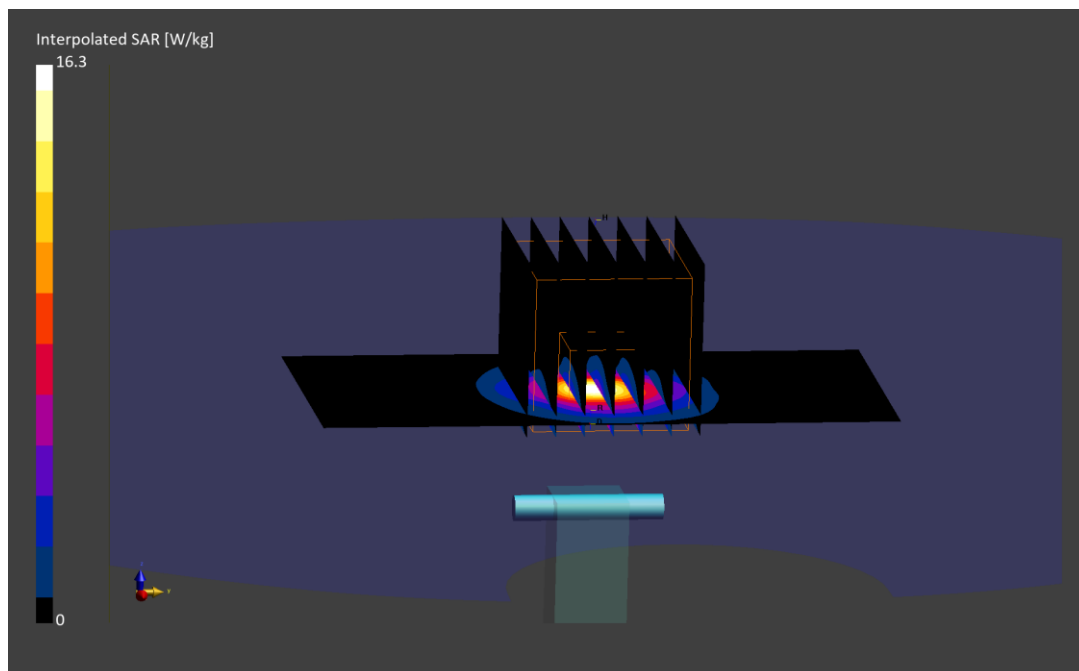

ELEMENT

DUT: Dipole 5800.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5800.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5800.0 MHz; cond = 5.10 S/m; perm = 33.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/14/2023; Ambient Temp: 20.4°C; Tissue Temp: 19.3°C

Probe: EX3DV4 - SN3746; ConvF:(4.5,4.5,4.5); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.2.0.1425

5800.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.5 W/kg

SAR(1 g) = 3.81 W/kg

Deviation (1 g) = -5.34%

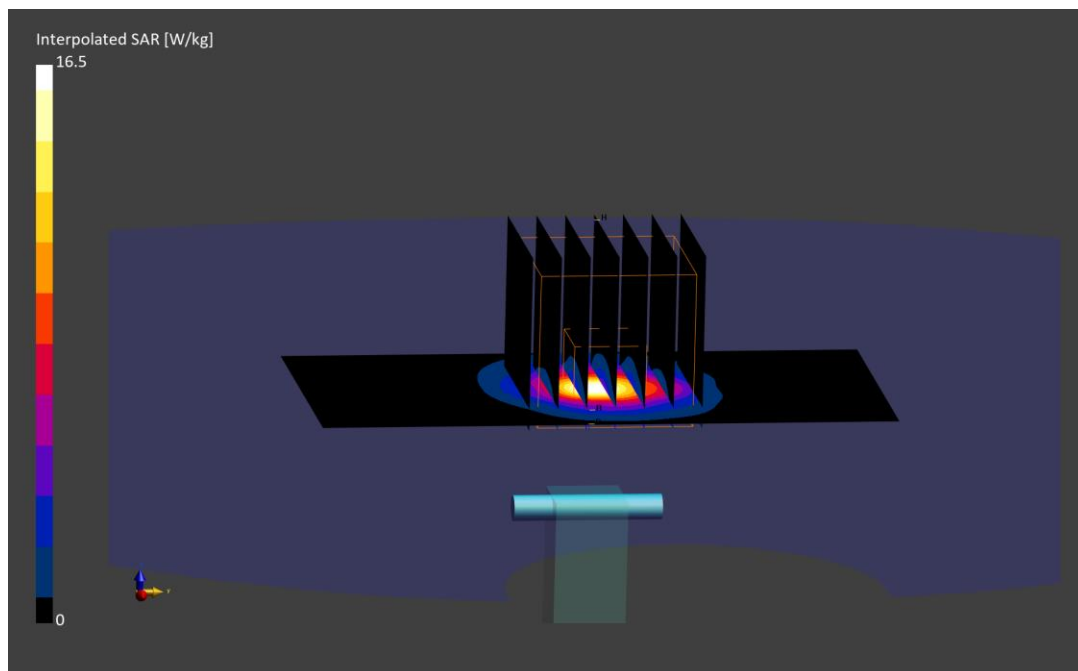

ELEMENT

DUT: Dipole 5800.0 MHz; Type: D5GHzV2 - SN1123

Communication System: UID: 0, CW; Frequency: 5800.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5800.0 MHz; cond = 5.29 S/m; perm = 34.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 12/26/2023; Ambient Temp: 21.1°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN3949; ConvF:(5.21,5.21,5.21); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.0.1425

5800.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.3 W/kg

SAR(1 g) = 3.99 W/kg

Deviation (1 g) = -0.87%

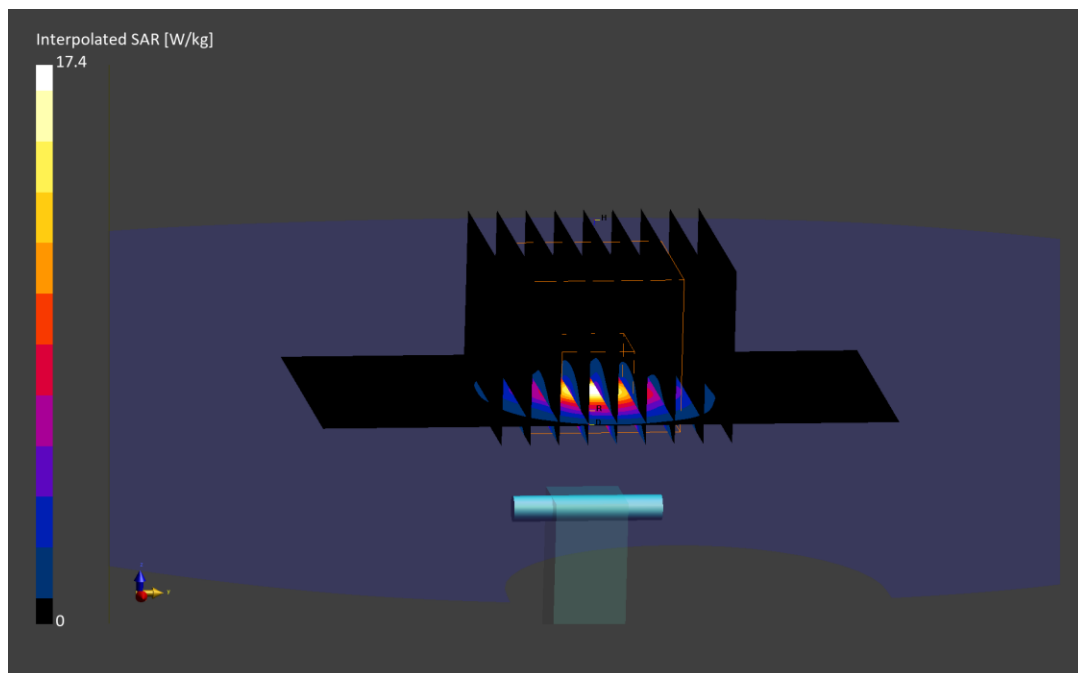

ELEMENT

DUT: Dipole 6500.0 MHz; Type: D6.5GHzV2 - SN1019

Communication System: UID: 0, CW; Frequency: 6500.0 MHz
Medium: 6000 Head; Medium parameters used:
f = 6500.0 MHz; cond = 6.05 S/m; perm = 35.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 5 mm

Test Date: 12/15/2023; Ambient Temp: 21.3°C; Tissue Temp: 20.3°C

Probe: EX3DV4 - SN7682; ConvF:(5.5,5.5,5.5); Calibrated: 2023-05-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1683; Calibrated: 2023-05-11
Phantom: Twin-SAM V4.0; Serial: 1598
Measurement SW: DASY Module SAR V16.2.0.1425

6500.0 MHz System Verification at 14.0 dBm (25 mW)


Area Scan (51.0 x 85.0): Measurement grid: dx=8.5 mm, dy=8.5 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=3.4 mm, dy=3.4 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 46.3 W/kg

SAR (1 g) = 7.74 W/kg; APD (4 cm²) = 35.2 W/m²

Deviation (1 g) = 5.67%; Deviation (4 cm²) = 6.67%

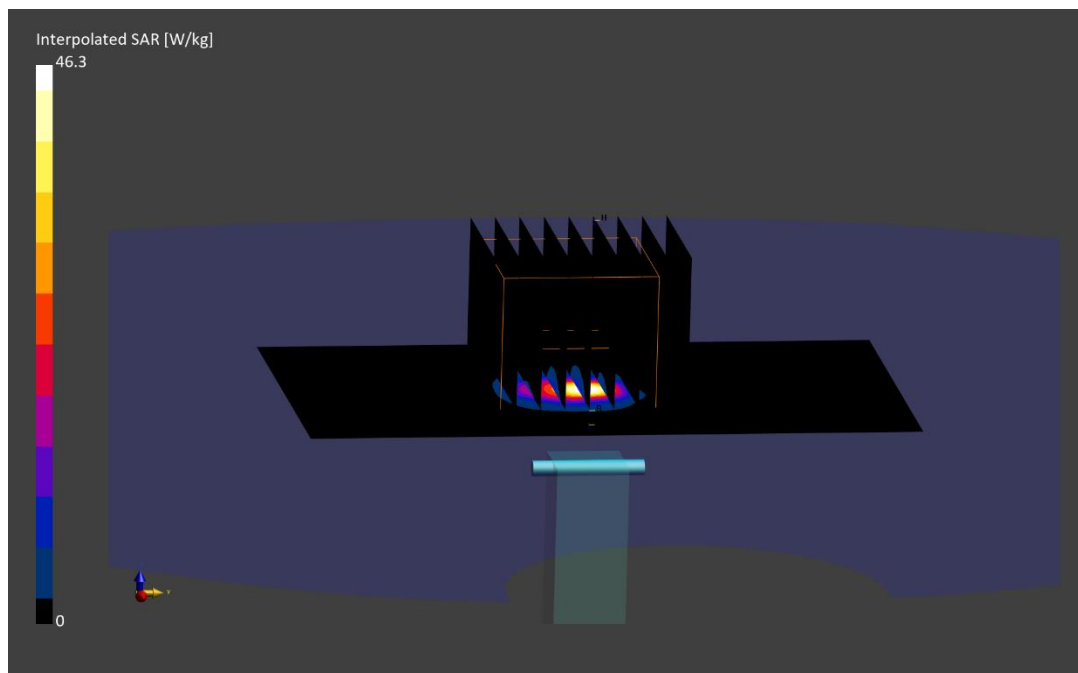

Date: 12/13/2023

10 GHz System Verification

Device Under Test Properties

DUT	Serial Number
10 GHz Verification Source	1006

Exposure Conditions

Phantom Section	Position	Test Distance [mm]	Band	Frequency [MHz]
5G	FRONT	10.00	Validation band	10000.0

Hardware Setup

Probe, Calibration Date	DAE, Calibration Date
EUmmWV4 - SN9523, 01/16/2023	DAE4 - SN793, 10/18/2023

Software Setup


Software	Software Version
cDASY6 Module mmWave	3.2.0.1840

Scans Setup


Scan Type	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [lambda]	0.25 x 0.25
Sensor Surface [mm]	10.0

Measurement Results

Scan Type	5G Scan
Avg. Area [cm ²]	4.00
pS _{tot} avg [W/m ²]	54.3
pS _n avg [W/m ²]	54.1
E _{peak} [V/m]	150
Deviation [dB] pS _{tot}	-0.35
Deviation [dB] pS _n	-0.34

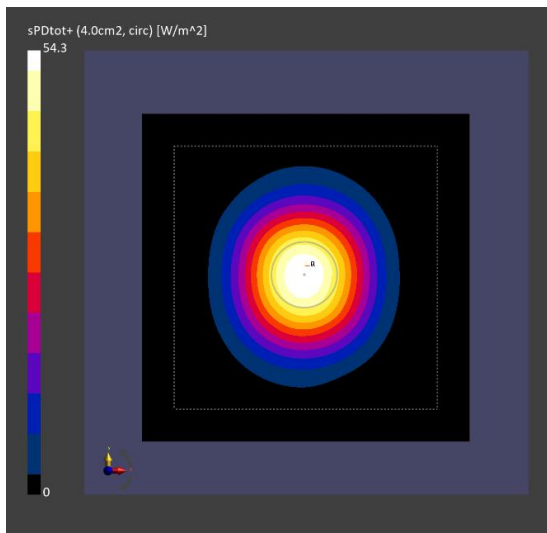

10 GHz System Verification

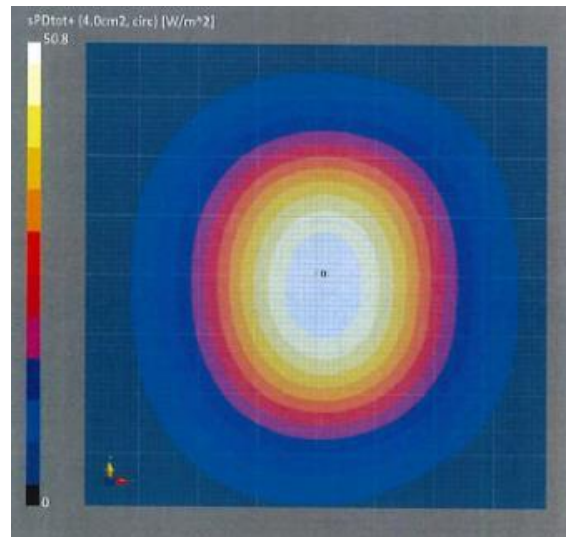

Calibration Certificate