

APPENDIX B: SAR DIPOLE VERIFICATION PLOTS

ELEMENT

DUT: Dipole 13.0 MHz; Type: CLA-13 - SN1004

Communication System: UID: 0, CW; Frequency: 13.0 MHz
Medium: 30 Head; Medium parameters used:
f = 13.0 MHz; cond = 0.722 S/m; perm = 52.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 0 mm

Test Date: 6/22/2024; Ambient Temp: 21.0°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN3746; ConvF:(16.19,16.19,16.19); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (All points)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: ELI V6.0; Serial: 2003
Measurement SW: DASYS Module SAR V16.2.4.2524

13.0 MHz System Verification at 30.0 dBm (1000 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 1.19 W/kg

SAR(1 g) = 0.590 W/kg

Deviation (1 g) = 2.08%

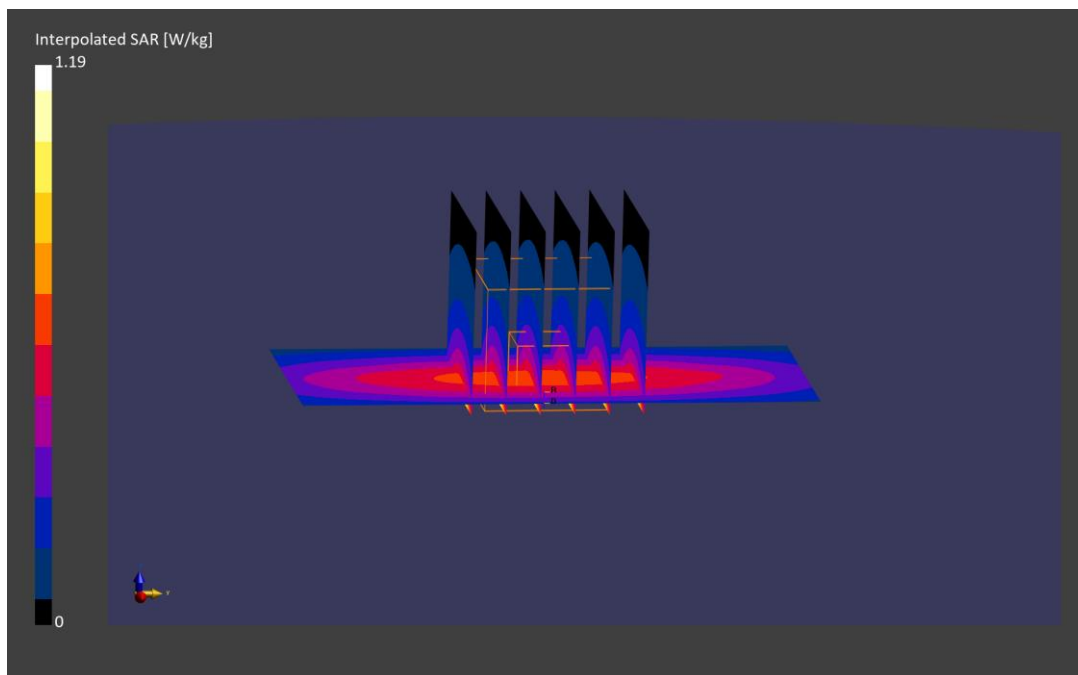

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1057

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.927 S/m; perm = 43.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 05/28/2024; Ambient Temp: 21.5°C; Tissue Temp: 20.8°C

Probe: EX3DV4 - SN3949; ConvF:(10.55,10.55,10.55); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.4.2524

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.62 W/kg

SAR(1 g) = 1.68 W/kg

Deviation (1 g) = -1.29%

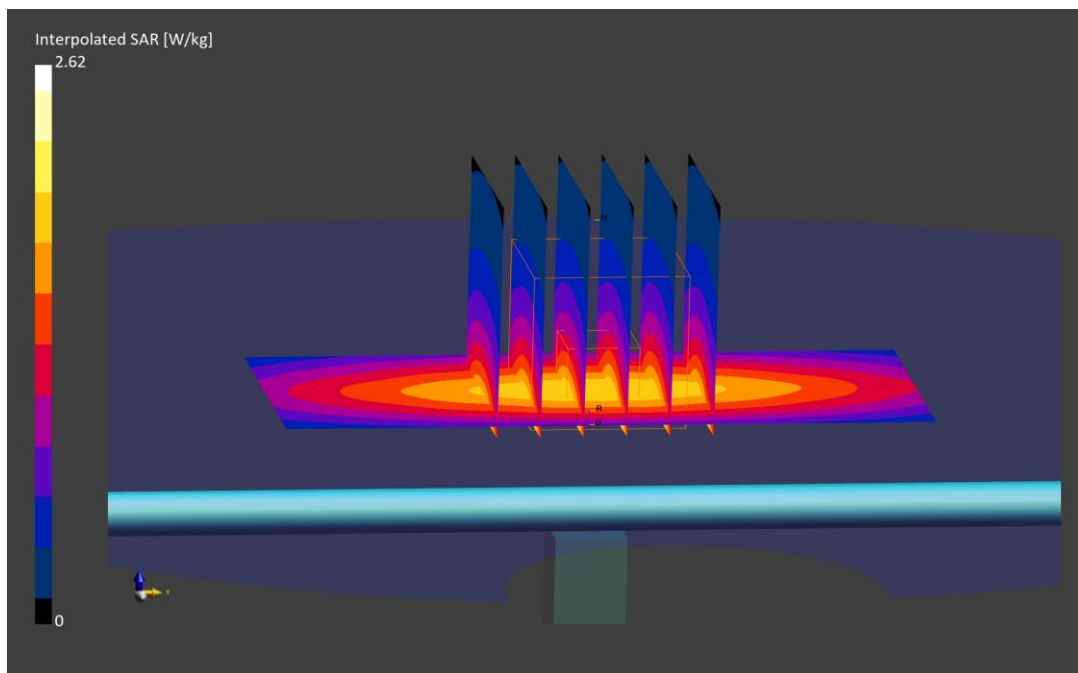

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1097

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.895 S/m; perm = 43.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 05/30/2024; Ambient Temp: 22.0°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN3949; ConvF:(10.55,10.55,10.55); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.4.2524

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.66 W/kg

SAR(1 g) = 1.72 W/kg

Deviation (1 g) = 3.99%

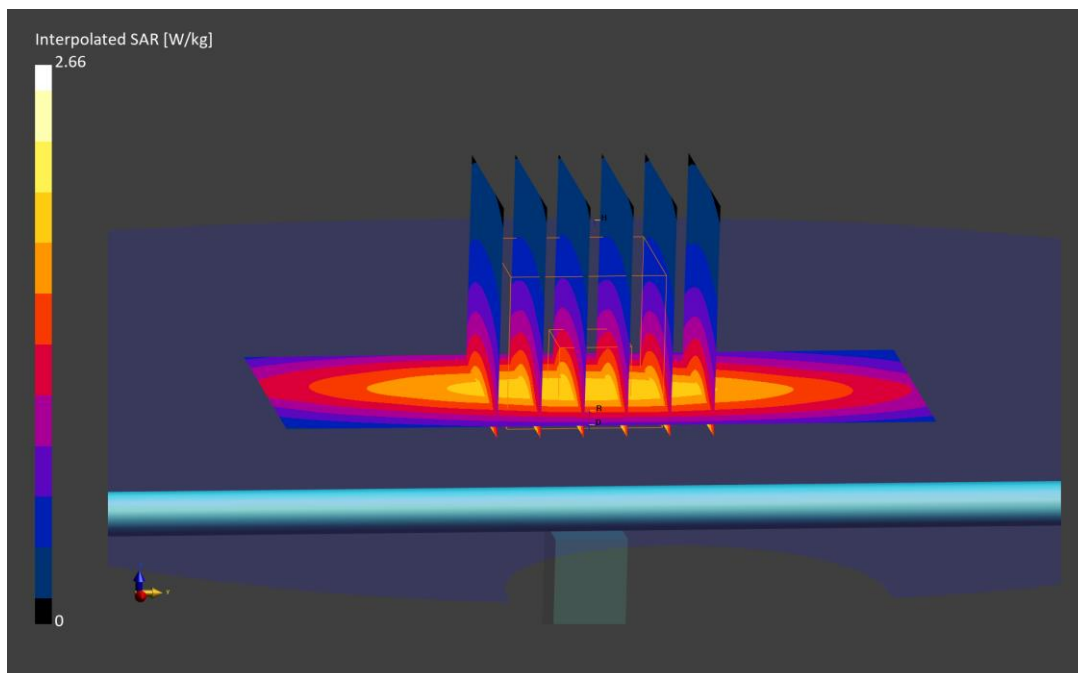

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1097

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.893 S/m; perm = 41.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 06/03/2024; Ambient Temp: 22.4°C; Tissue Temp: 22.0°C

Probe: EX3DV4 - SN3949; ConvF:(10.55,10.55,10.55); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.4.2524

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.72 W/kg

SAR(1 g) = 1.74 W/kg

Deviation (1 g) = 5.20%

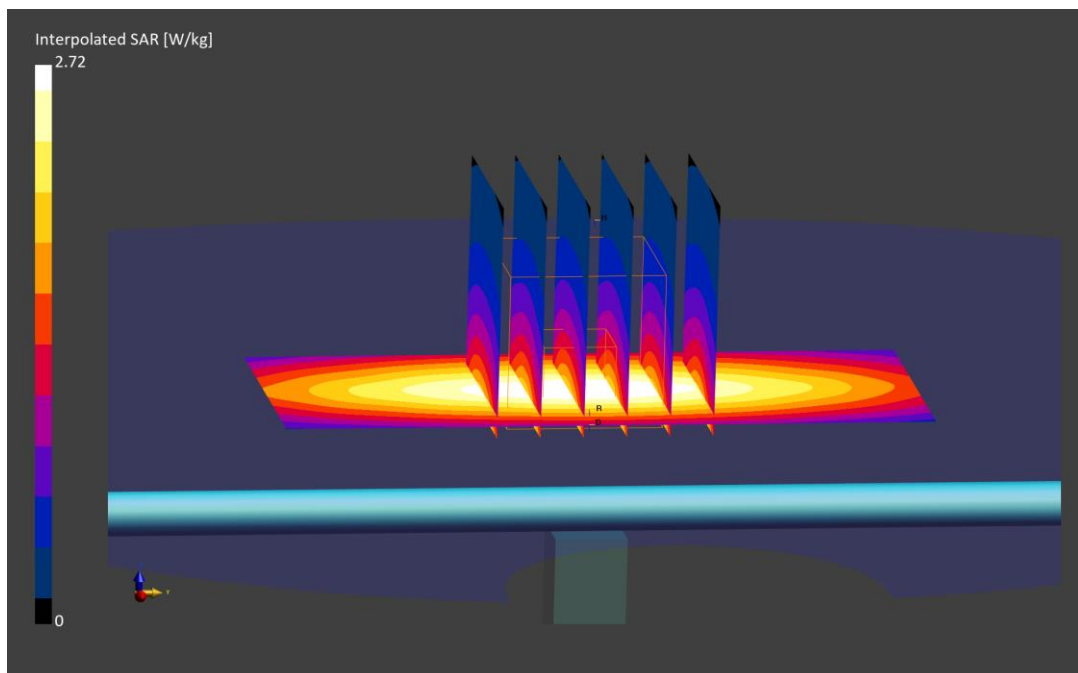

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1097

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.910 S/m; perm = 43.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 06/10/2024; Ambient Temp: 21.5°C; Tissue Temp: 23.0°C

Probe: EX3DV4 - SN3949; ConvF:(10.55,10.55,10.55); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.4.2524

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.62 W/kg

SAR(1 g) = 1.68 W/kg

Deviation (1 g) = 1.57%

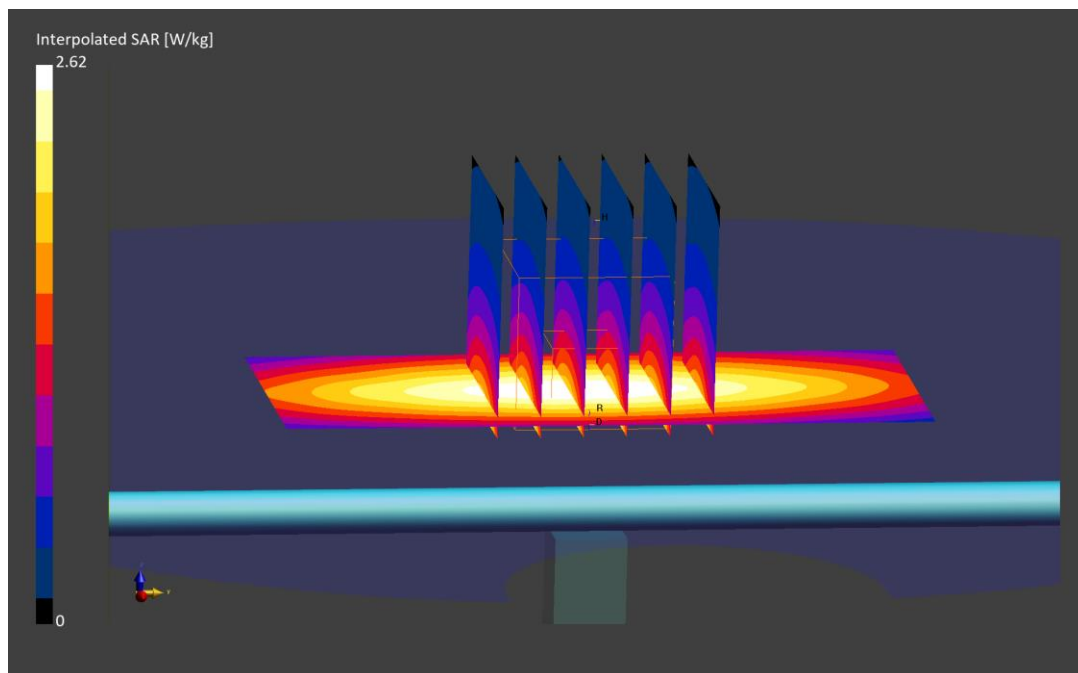

ELEMENT

DUT: Dipole 750.0 MHz; Type: D750V3 - SN1097

Communication System: UID: 0, CW; Frequency: 750.0 MHz
Medium: 750 Head; Medium parameters used:
f = 750.0 MHz; cond = 0.919 S/m; perm = 43.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 06/12/2024; Ambient Temp: 21.6°C; Tissue Temp: 22.7°C

Probe: EX3DV4 - SN3949; ConvF:(10.55,10.55,10.55); Calibrated: 2023-10-02
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1684; Calibrated: 2023-09-12
Phantom: Twin-SAM V8.0; Serial: 1736
Measurement SW: DASY Module SAR V16.2.4.2524

750.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 2.72 W/kg

SAR(1 g) = 1.73 W/kg

Deviation (1 g) = 4.59%

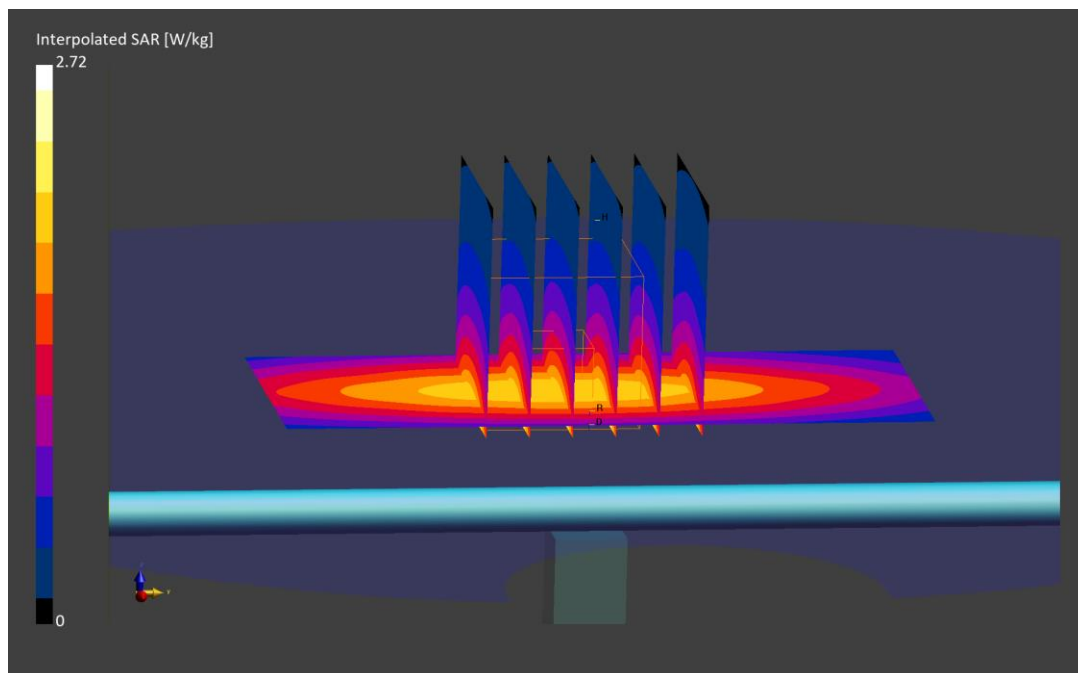

ELEMENT

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d108

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Head; Medium parameters used:
f = 835.0 MHz; cond = 0.910 S/m; perm = 39.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 05/20/2024; Ambient Temp: 20.5°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7668; ConvF:(9.05,9.05,9.05); Calibrated: 2023-08-10
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2023-09-12
Phantom: Twin-SAM V5.0; Serial: 1692
Measurement SW: DASY Module SAR V16.2.4.2524

835.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.24 W/kg

SAR(1 g) = 2.04 W/kg

Deviation (1 g) = 4.08%

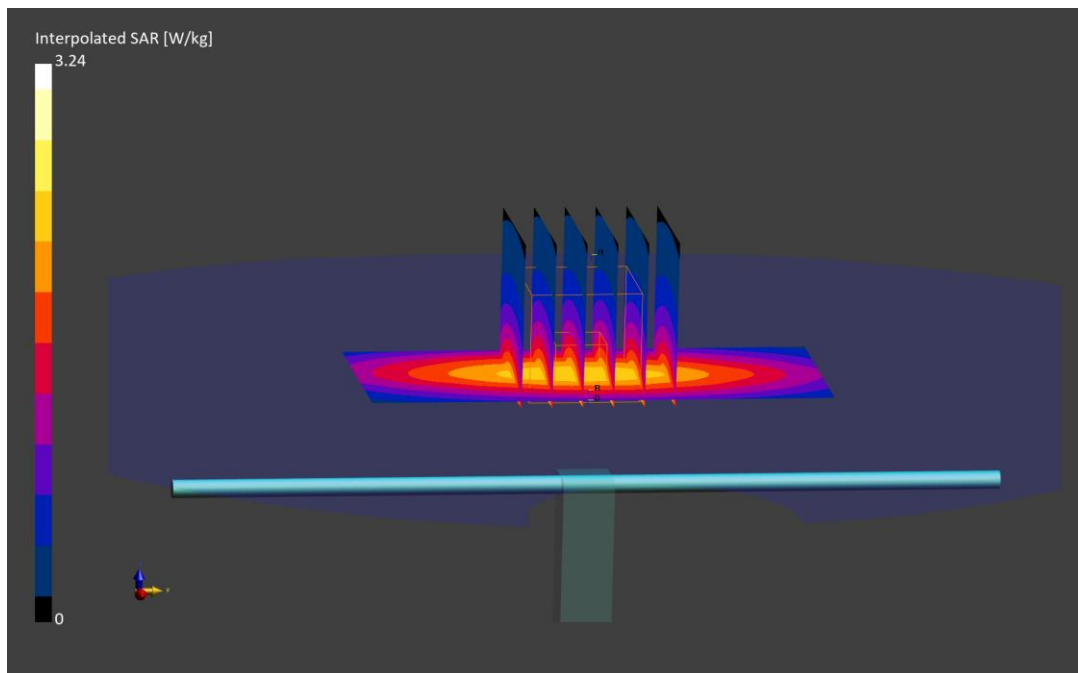

ELEMENT

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d108

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Head; Medium parameters used:
f = 835.0 MHz; cond = 0.885 S/m; perm = 39.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 05/22/2024; Ambient Temp: 22.4°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7668; ConvF:(9.05,9.05,9.05); Calibrated: 2023-08-10
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1681; Calibrated: 2023-09-12
Phantom: Twin-SAM V5.0; Serial: 1692
Measurement SW: DASY Module SAR V16.2.4.2524

835.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.34 W/kg

SAR(1 g) = 2.09 W/kg

Deviation (1 g) = 6.63%

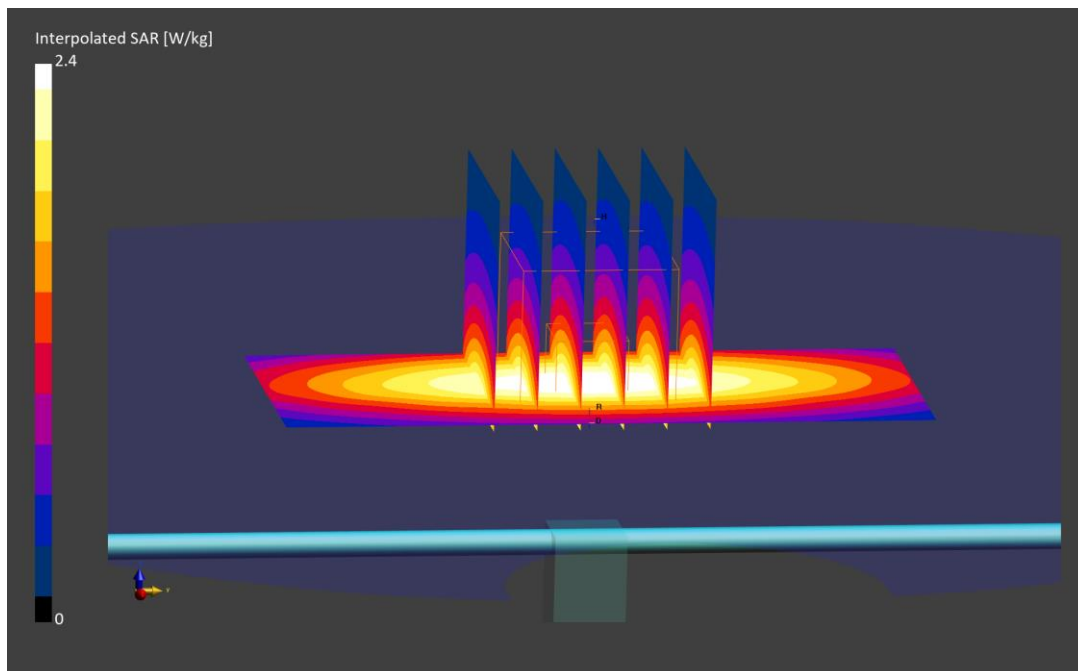

ELEMENT

DUT: Dipole 835.0 MHz; Type: D835V2 - SN4d108

Communication System: UID: 0, CW; Frequency: 835.0 MHz
Medium: 835 Head; Medium parameters used:
f = 835.0 MHz; cond = 0.887 S/m; perm = 40.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 15 mm

Test Date: 06/03/2024; Ambient Temp: 21.0°C; Tissue Temp: 19.6°C

Probe: EX3DV4 - SN7668; ConvF:(9.05,9.05,9.05); Calibrated: 2023-08-10
Sensor-Surface: 1.4mm (All points)
Electronics: DAE4 Sn1681; Calibrated: 2023-09-12
Phantom: Twin-SAM V5.0; Serial: 1692
Measurement SW: DASY Module SAR V16.2.4.2524

835.0 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 3.17 W/kg

SAR(1 g) = 2.01 W/kg

Deviation (1 g) = 2.55%

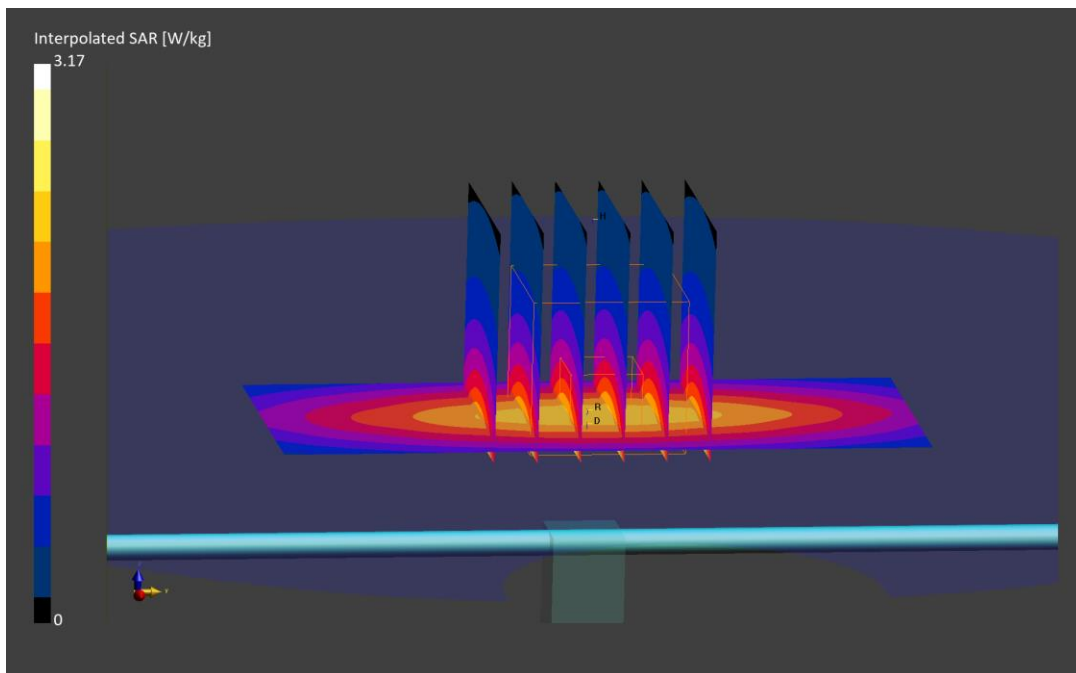

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1083

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.38 S/m; perm = 39.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/23/2024; Ambient Temp: 23.2°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7421; ConvF:(8.13,8.13,8.13); Calibrated: 2024-03-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn604; Calibrated: 2024-03-06
Phantom: Twin-SAM V8.0; Serial: 2067
Measurement SW: DASY Module SAR V16.2.4.2524

1750.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.07 W/kg

SAR(1 g) = 3.82 W/kg

Deviation (1 g) = 4.66%

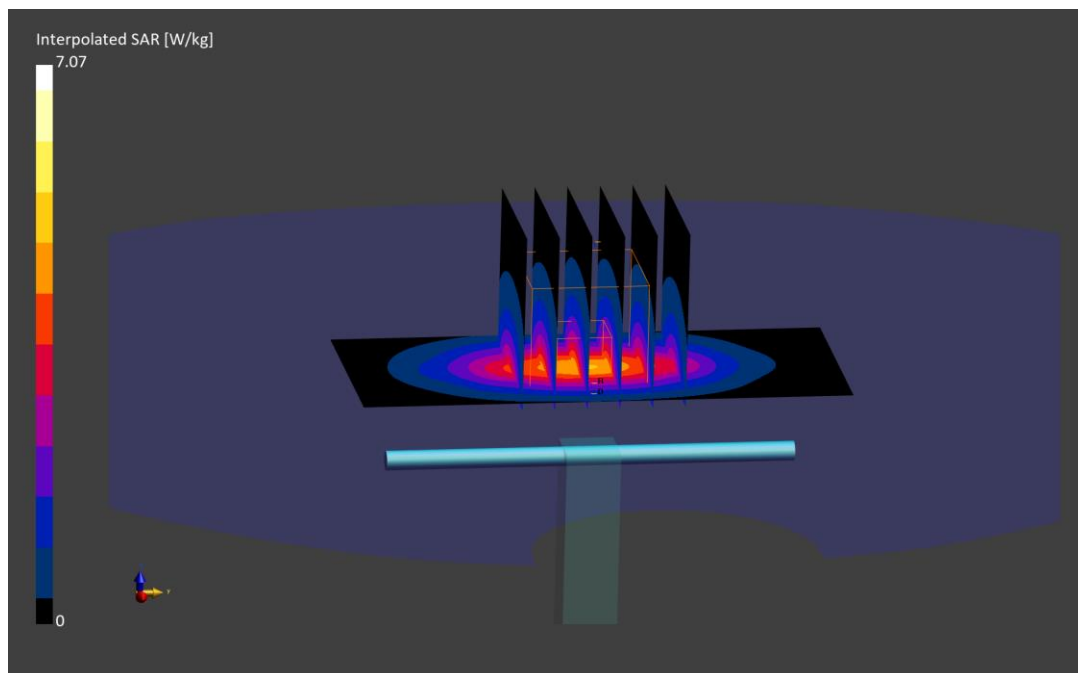

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1104

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.36 S/m; perm = 39.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/30/2024; Ambient Temp: 21.2°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN7421; ConvF:(8.13,8.13,8.13); Calibrated: 2024-03-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn604; Calibrated: 2024-03-06
Phantom: Twin-SAM V8.0; Serial: 2067
Measurement SW: DASY Module SAR V16.2.4.2524

1750.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.13 W/kg

SAR(1 g) = 3.79 W/kg

Deviation (1 g) = 6.46%

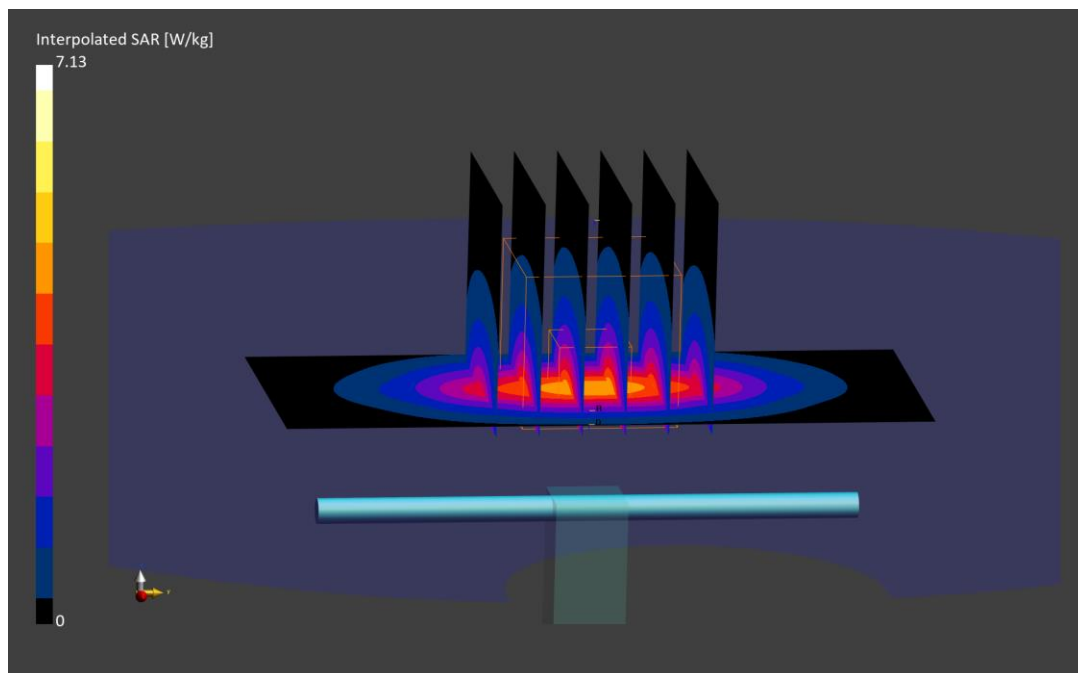

ELEMENT

DUT: Dipole 1750.0 MHz; Type: D1750V2 - SN1104

Communication System: UID: 0, CW; Frequency: 1750.0 MHz
Medium: 1750 Head; Medium parameters used:
f = 1750.0 MHz; cond = 1.35 S/m; perm = 38.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/05/2024; Ambient Temp: 20.8°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7421; ConvF:(8.13,8.13,8.13); Calibrated: 2024-03-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn604; Calibrated: 2024-03-06
Phantom: Twin-SAM V8.0; Serial: 2067
Measurement SW: DASY Module SAR V16.2.4.2524

1750.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 6.74 W/kg

SAR(1 g) = 3.65 W/kg

Deviation (1 g) = 2.53%

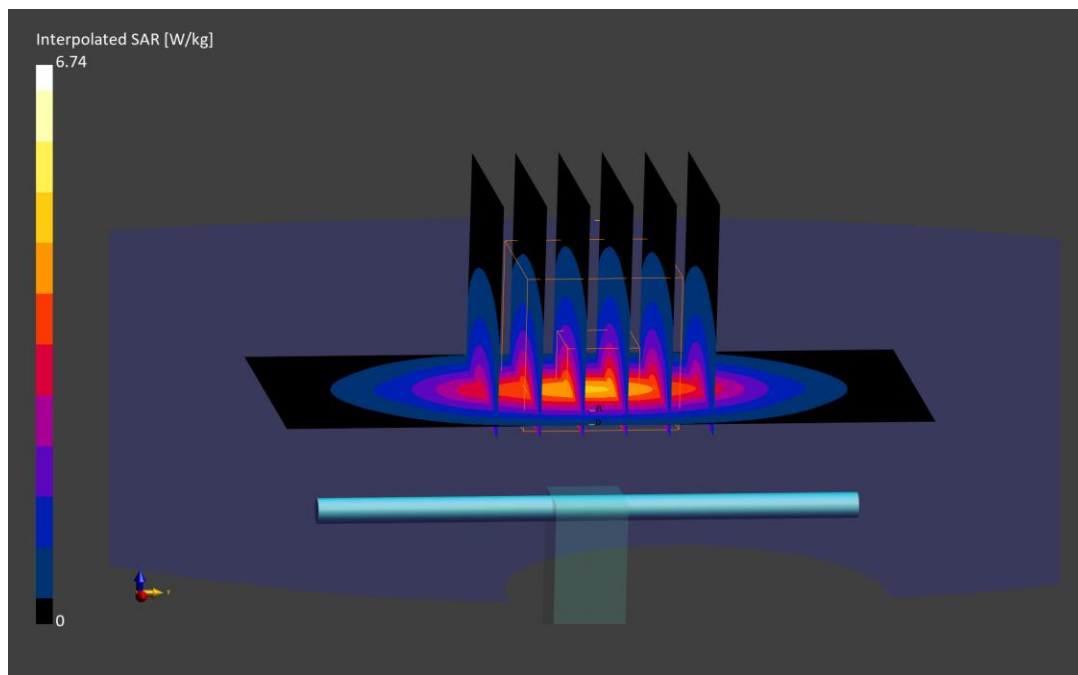

ELEMENT

DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d180

Communication System: UID: 0, CW; Frequency: 1900.0 MHz
Medium: 1900 Head; Medium parameters used:
f = 1900.0 MHz; cond = 1.44 S/m; perm = 39.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/28/2024; Ambient Temp: 21.8°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7639; ConvF:(8.53,8.53,8.53); Calibrated: 2023-11-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1403; Calibrated: 2023-11-14
Phantom: Twin-SAM V8.0; Serial: 2034
Measurement SW: DASY Module SAR V16.2.4.2524

1900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.65 W/kg

SAR(1 g) = 4.04 W/kg

Deviation (1 g) = 3.06%

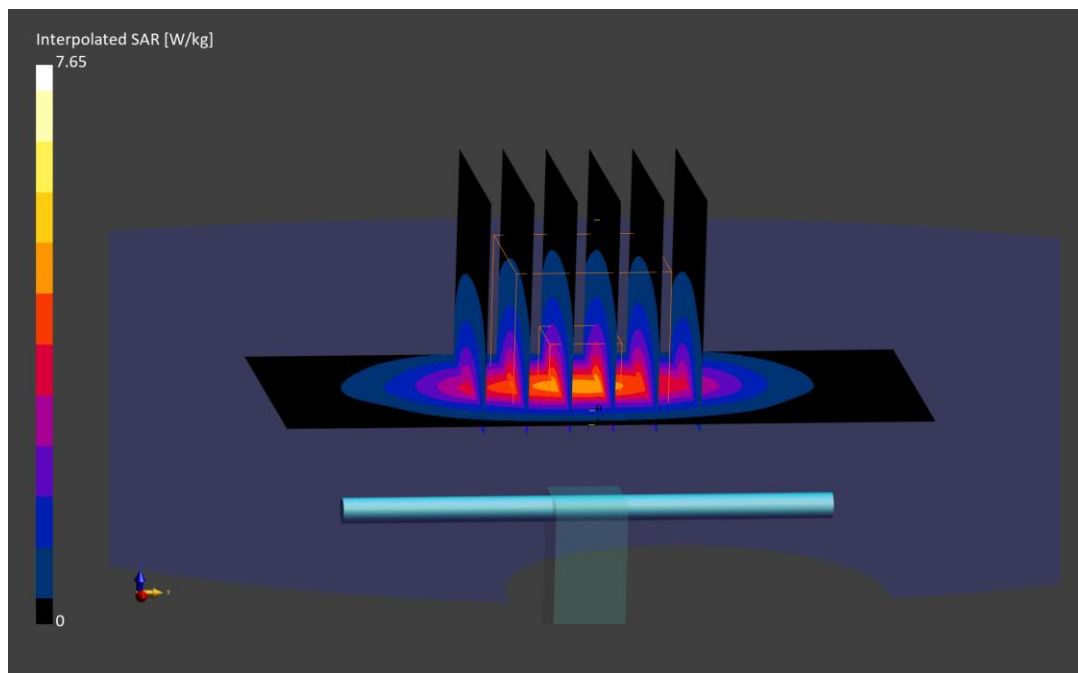

ELEMENT

DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d180

Communication System: UID: 0, CW; Frequency: 1900.0 MHz
Medium: 1900 Head; Medium parameters used:
f = 1900.0 MHz; cond = 1.44 S/m; perm = 39.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/30/2024; Ambient Temp: 22.6°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7639; ConvF:(8.53,8.53,8.53); Calibrated: 2023-11-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1403; Calibrated: 2023-11-14
Phantom: Twin-SAM V8.0; Serial: 2034
Measurement SW: DASY Module SAR V16.2.4.2524

1900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: dx=10.0 mm, dy=15.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=6.0 mm, dy=6.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.97 W/kg

SAR(1 g) = 4.17 W/kg

Deviation (1 g) = 6.38%

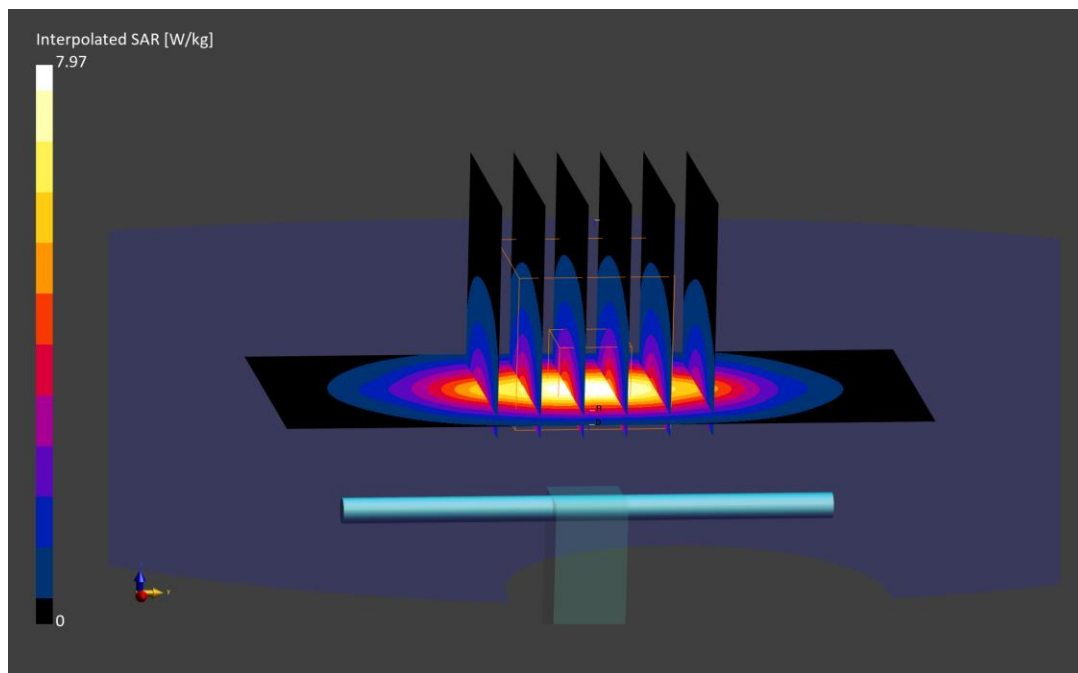

ELEMENT

DUT: Dipole 1900.0 MHz; Type: D1900V2 - SN5d180

Communication System: UID: 0, CW; Frequency: 1900.0 MHz
Medium: 1900 Head; Medium parameters used:
 $f = 1900.0$ MHz; $\text{cond} = 1.43$ S/m; $\text{perm} = 38.3$; $\text{density} = 1000$ kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/05/2024; Ambient Temp: 22.1°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7639; ConvF:(8.53,8.53,8.53); Calibrated: 2023-11-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1403; Calibrated: 2023-11-14
Phantom: Twin-SAM V8.0; Serial: 2034
Measurement SW: DASY Module SAR V16.2.4.2524

1900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 90.0): Measurement grid: $dx=10.0$ mm, $dy=15.0$ mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: $dx=6.0$ mm, $dy=6.0$ mm, $dz=1.5$ mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 7.67 W/kg

SAR(1 g) = 4.06 W/kg

Deviation (1 g) = 3.57%

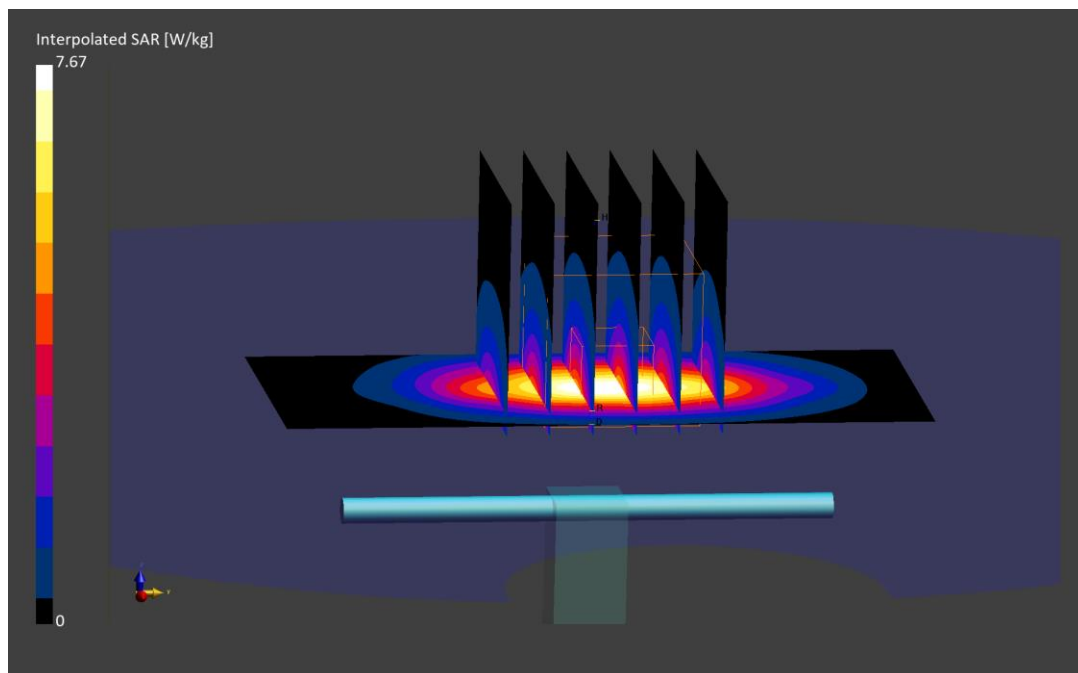

ELEMENT

DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1064

Communication System: UID: 0, CW; Frequency: 2300.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2300.0 MHz; cond = 1.61 S/m; perm = 38.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/28/2024; Ambient Temp: 21.5°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7682; ConvF:(8.0,7.85,8.33); Calibrated: 2024-05-13
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1683; Calibrated: 2024-05-08
Phantom: Twin-SAM V8.0; Serial: 1866
Measurement SW: DASY Module SAR V16.2.4.2524

2300.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.44 W/kg

SAR(1 g) = 4.73 W/kg

Deviation (1 g) = -4.06%

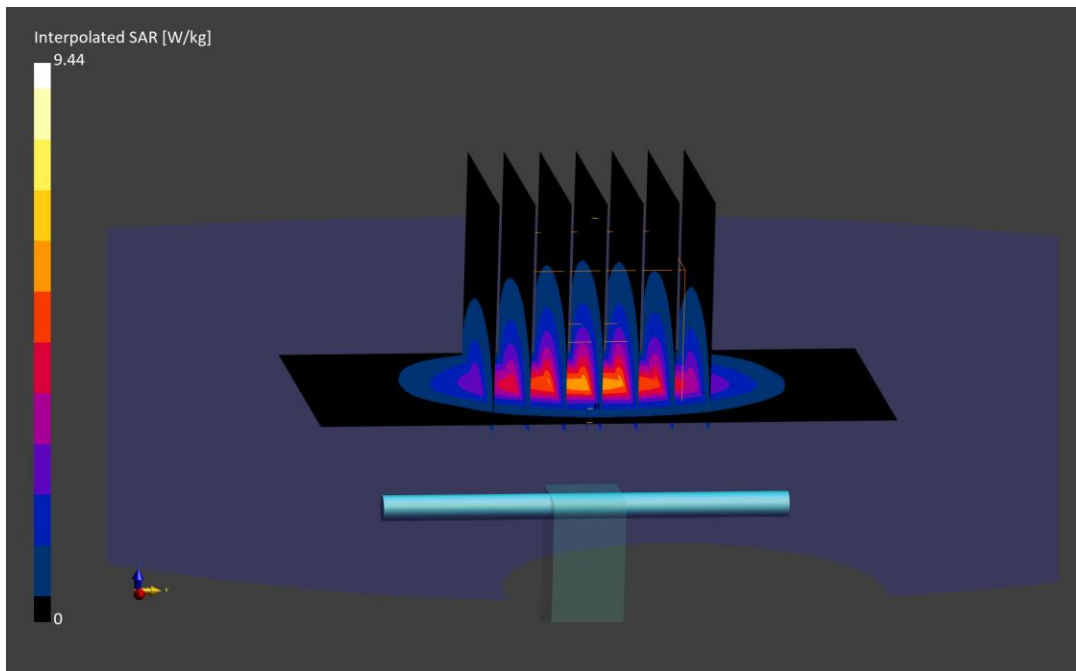

ELEMENT

DUT: Dipole 2300.0 MHz; Type: D2300V2 - SN1064

Communication System: UID: 0, CW; Frequency: 2300.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2300.0 MHz; cond = 1.63 S/m; perm = 38.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/30/2024; Ambient Temp: 22.8°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN7682; ConvF:(8.0,7.85,8.33); Calibrated: 2024-05-13
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1683; Calibrated: 2024-05-08
Phantom: Twin-SAM V8.0; Serial: 1866
Measurement SW: DASY Module SAR V16.2.4.2524

2300.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 9.04 W/kg

SAR(1 g) = 4.59 W/kg

Deviation (1 g) = -6.90%

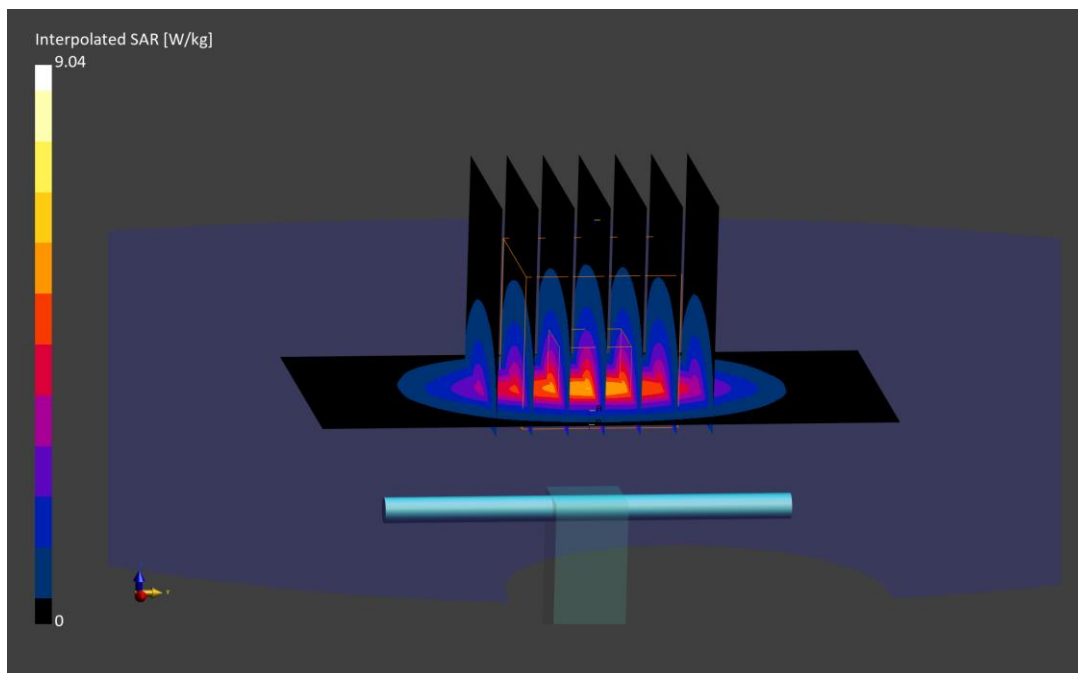

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.83 S/m; perm = 40.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/22/2024; Ambient Temp: 22.0°C; Tissue Temp: 23.0°C

Probe: EX3DV4 - SN7499; ConvF:(7.13,7.46,7.69); Calibrated: 2024-01-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; Calibrated: 2023-12-07
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.4.2524

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.0 W/kg

SAR(1 g) = 5.32 W/kg

Deviation (1 g) = -1.85%

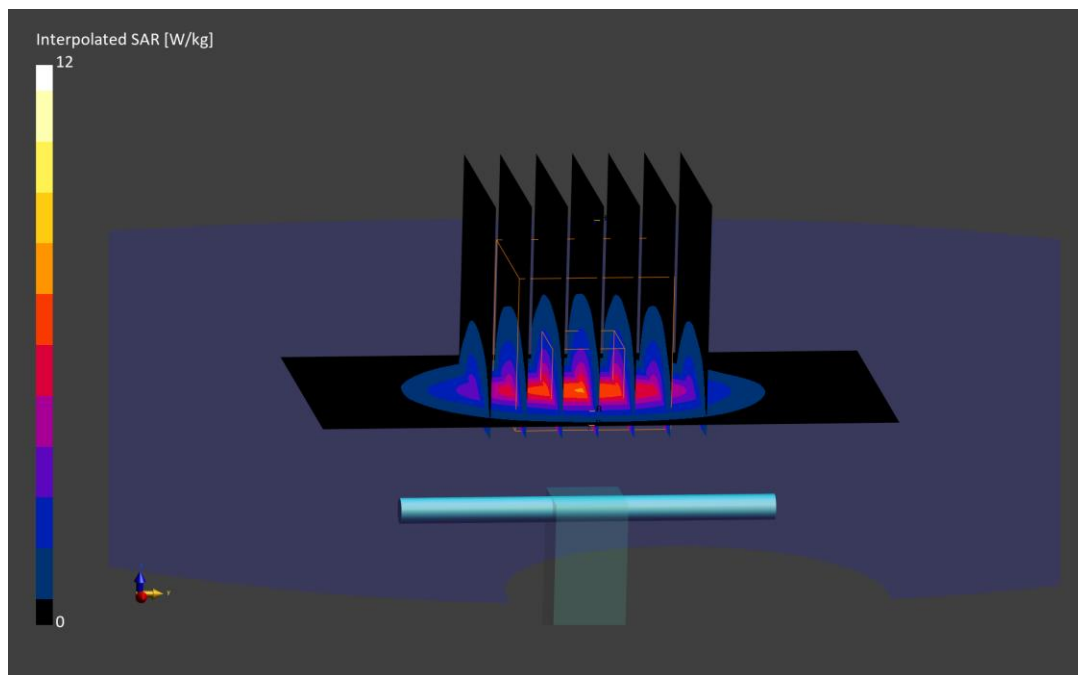

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN921

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.85 S/m; perm = 39.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/30/2024; Ambient Temp: 21.5°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN7499; ConvF:(7.13,7.46,7.69); Calibrated: 2024-01-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; Calibrated: 2023-12-07
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.4.2524

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.7 W/kg

SAR(1 g) = 5.24 W/kg

Deviation (1 g) = -3.32%

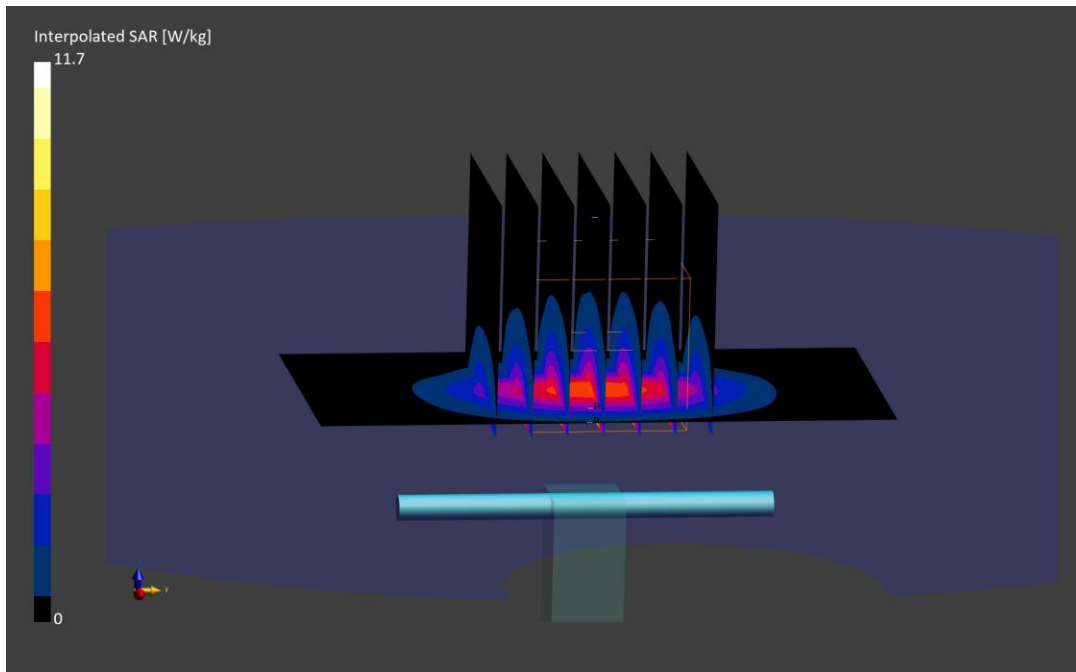

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.86 S/m; perm = 38.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/01/2024; Ambient Temp: 21.5°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN7638; ConvF:(7.38,7.72,7.8); Calibrated: 2024-03-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1408; Calibrated: 2024-03-06
Phantom: Twin-SAM V8.0; Serial: 1935
Measurement SW: DASY Module SAR V16.2.4.2524

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 11.6 W/kg

SAR(1 g) = 5.33 W/kg

Deviation (1 g) = 1.33%

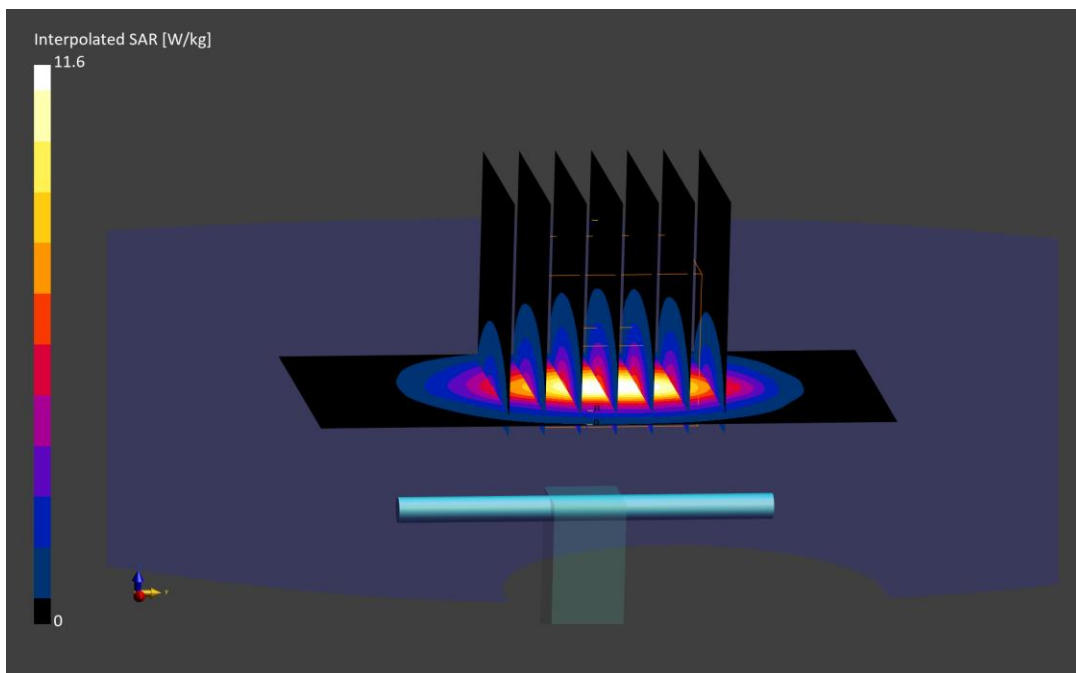

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.85 S/m; perm = 39.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/03/2024; Ambient Temp: 22.0°C; Tissue Temp: 22.7°C

Probe: EX3DV4 - SN7499; ConvF:(7.13,7.46,7.69); 2024-01-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; 2023-12-07
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.4.2524

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.0 W/kg

SAR(1 g) = 5.37 W/kg;

Deviation (1 g) = 2.09%;

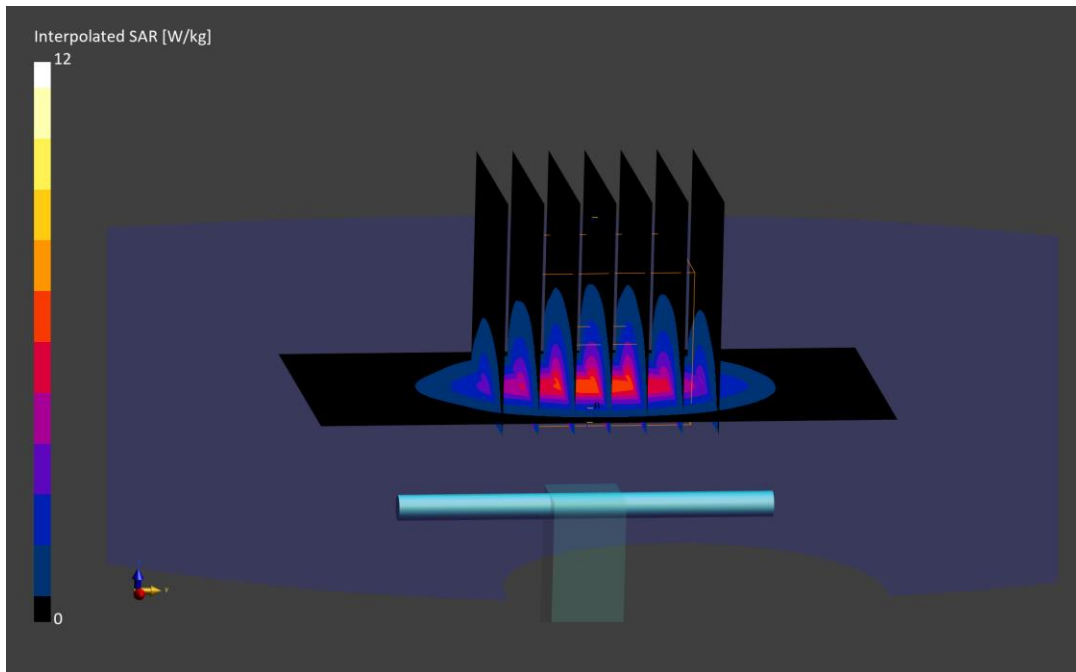

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.74 S/m; perm = 39.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/12/2024; Ambient Temp: 21.5°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN7682; ConvF:(7.87,7.72,8.18); Calibrated: 2024-05-13
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1683; Calibrated: 2024-05-08
Phantom: Twin-SAM V8.0; Serial: 1917
Measurement SW: DASY Module SAR V16.2.4.2524

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 10.1 W/kg

SAR(1 g) = 5.05 W/kg

Deviation (1 g) = -3.99%

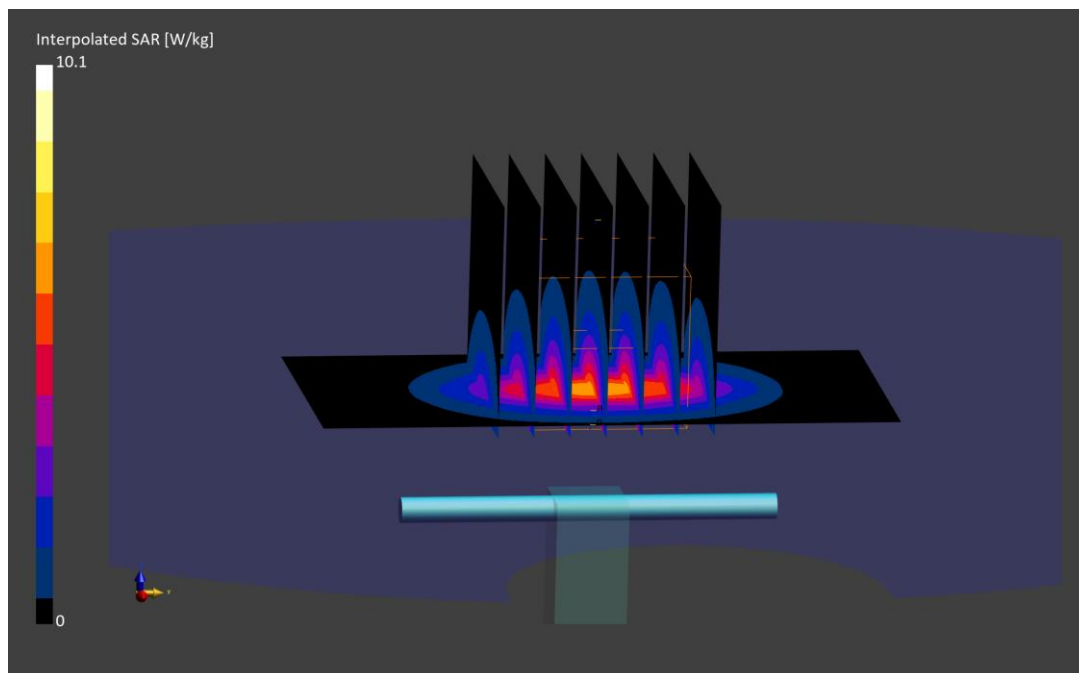

ELEMENT

DUT: Dipole 2450.0 MHz; Type: D2450V2 - SN750

Communication System: UID: 0, CW; Frequency: 2450.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2450.0 MHz; cond = 1.86 S/m; perm = 38.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/26/2024; Ambient Temp: 20.8°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN7499; ConvF:(7.13,7.46,7.69); 2024-01-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; 2023-12-07
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.4.2524

2450.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.2 W/kg

SAR(1 g) = 5.33 W/kg;

Deviation (1 g) = 1.33%;

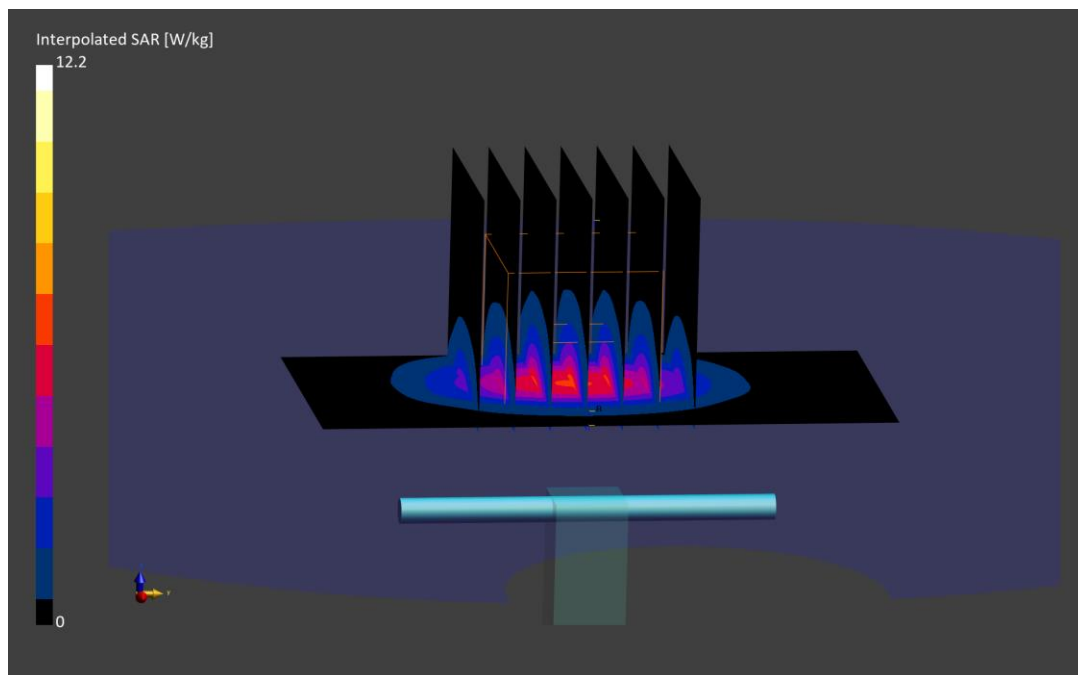

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1068

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 2.03 S/m; perm = 39.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/30/2024; Ambient Temp: 21.5°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN7499; ConvF:(7.24,7.57,7.85); Calibrated: 2024-01-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; Calibrated: 2023-12-07
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.4.2524

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 13.3 W/kg

SAR(1 g) = 5.51 W/kg

Deviation (1 g) = -2.48%

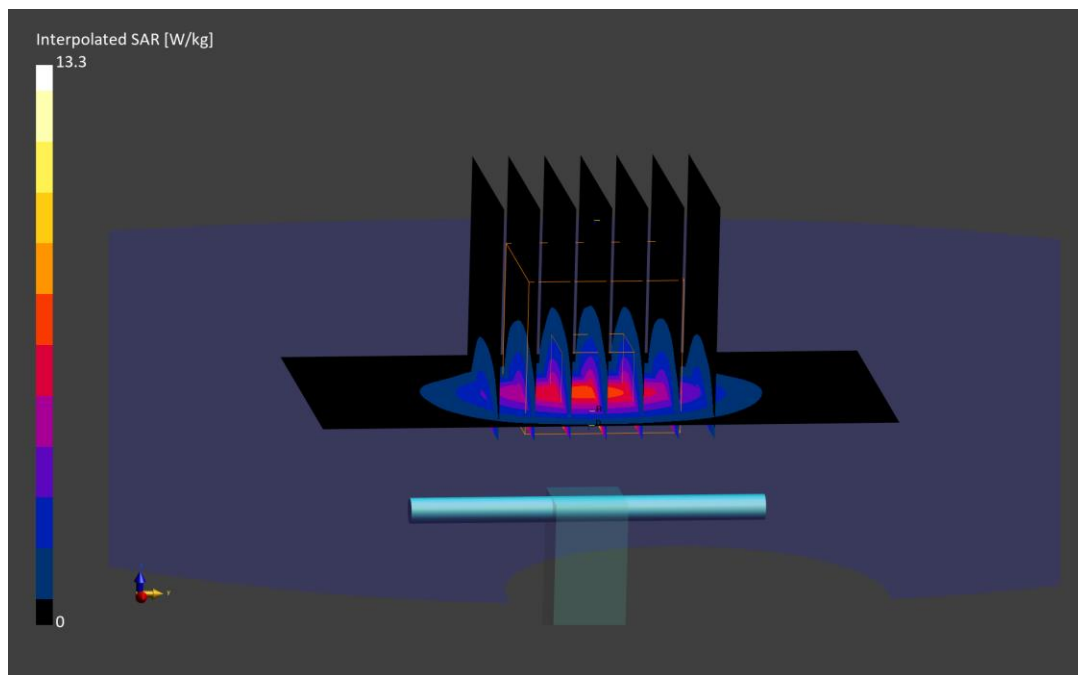

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1042

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 2.03 S/m; perm = 37.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/01/2024; Ambient Temp: 21.5°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN7638; ConvF:(7.26,7.51,7.65); Calibrated: 2024-03-11
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1408; Calibrated: 2024-03-06
Phantom: Twin-SAM V8.0; Serial: 1935
Measurement SW: DASY Module SAR V16.2.4.2524

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.7 W/kg

SAR(1 g) = 5.64 W/kg

Deviation (1 g) = 1.08%

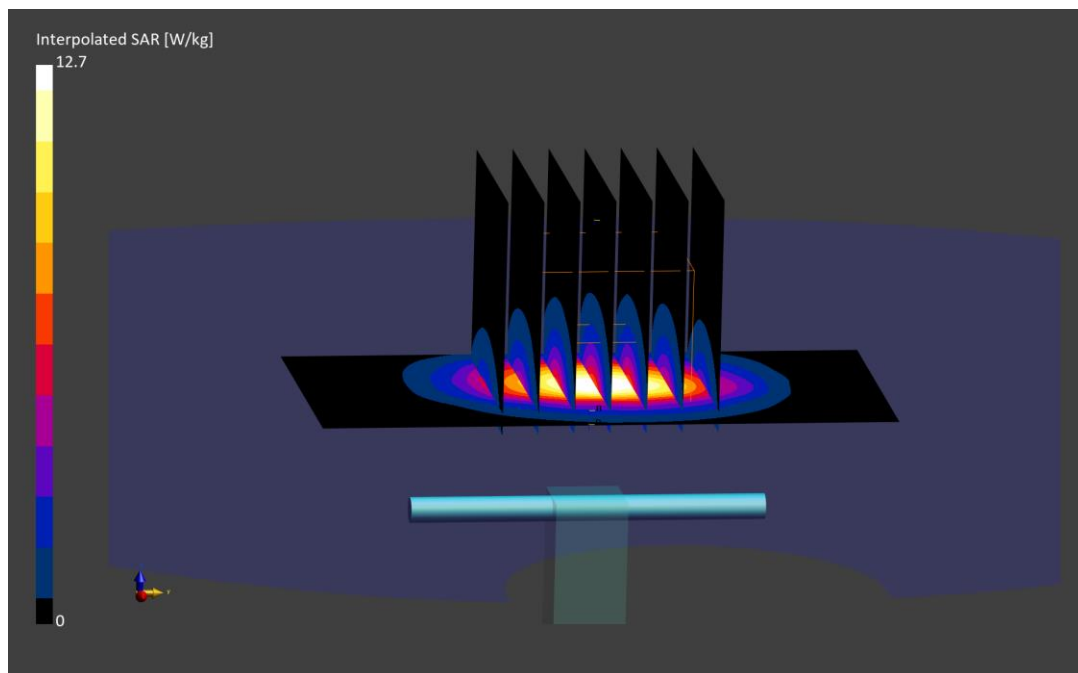

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1042

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 2.02 S/m; perm = 38.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/03/2024; Ambient Temp: 22.0°C; Tissue Temp: 22.7°C

Probe: EX3DV4 - SN7499; ConvF:(7.24,7.57,7.85); Calibrated: 2024-01-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; Calibrated: 2023-12-07
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.4.2524

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 12.7 W/kg

SAR(1 g) = 5.34 W/kg

Deviation (1 g) = -4.30%

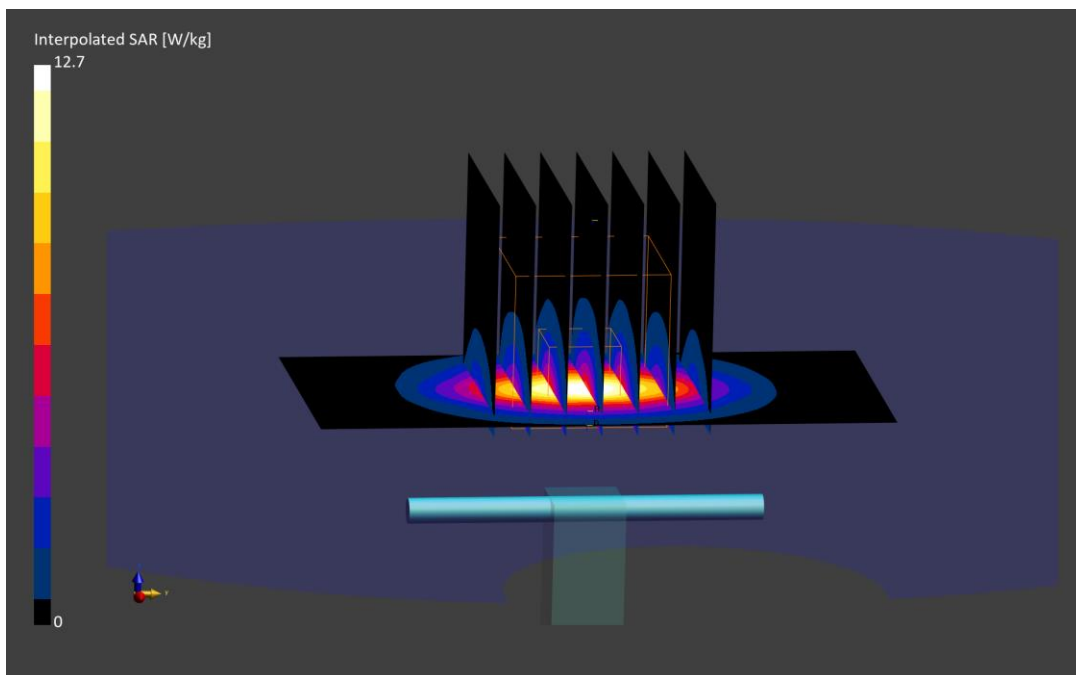

ELEMENT

DUT: Dipole 2600.0 MHz; Type: D2600V2 - SN1042

Communication System: UID: 0, CW; Frequency: 2600.0 MHz
Medium: 2450 Head; Medium parameters used:
f = 2600.0 MHz; cond = 2.04 S/m; perm = 37.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/26/2024; Ambient Temp: 20.8°C; Tissue Temp: 22.4°C

Probe: EX3DV4 - SN7499; ConvF:(7.24,7.57,7.85); Calibrated: 2024-01-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; Calibrated: 2023-12-07
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.4.2524

2600.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (30.0 x 30.0 x 30.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.5 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 13.2 W/kg

SAR(1 g) = 5.56 W/kg

Deviation (1 g) = -0.36%

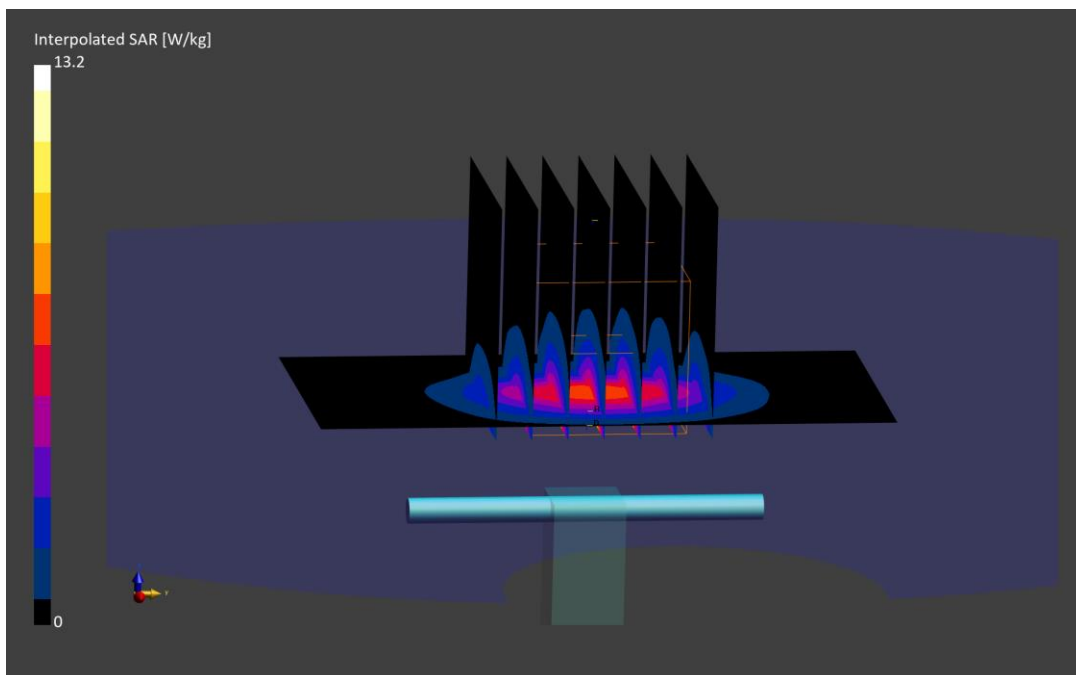

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1126

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 2.95 S/m; perm = 38.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/26/2024; Ambient Temp: 21.1°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7782; ConvF:(6.19,6.19,6.19); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.4.2524

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.1 W/kg

SAR(1 g) = 6.45 W/kg

Deviation (1 g) = -3.73%

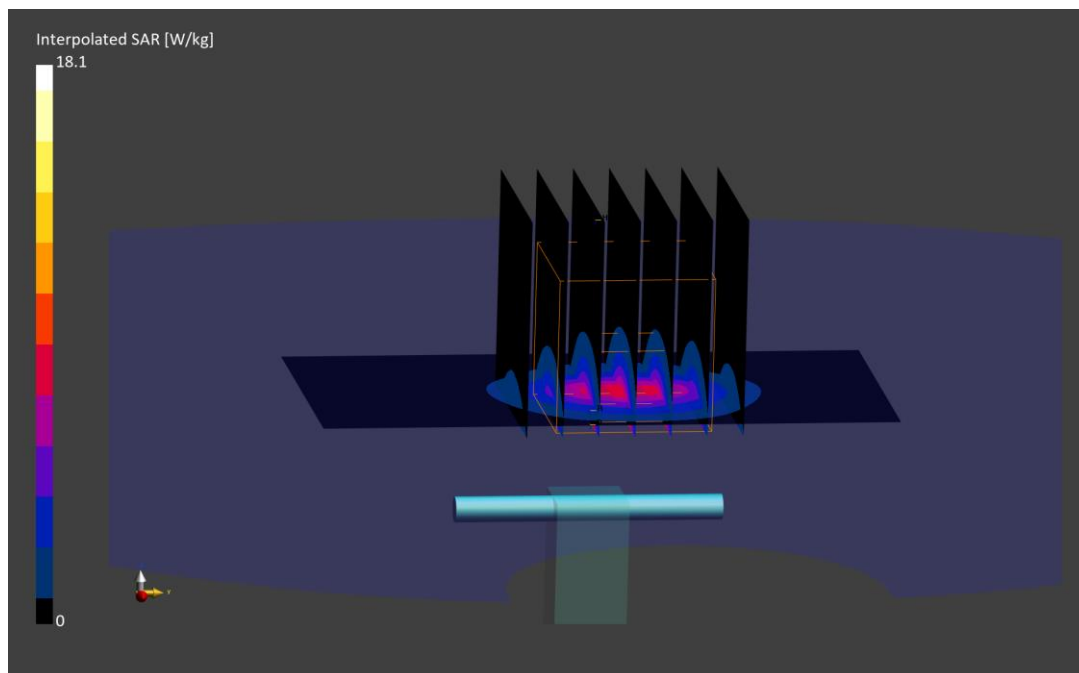

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1126

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 3.01 S/m; perm = 39.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/29/2024; Ambient Temp: 22.1°C; Tissue Temp: 22.0°C

Probe: EX3DV4 - SN7782; ConvF:(6.19,6.19,6.19); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.4.2524

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.7 W/kg

SAR(1 g) = 6.66 W/kg

Deviation (1 g) = -0.60%

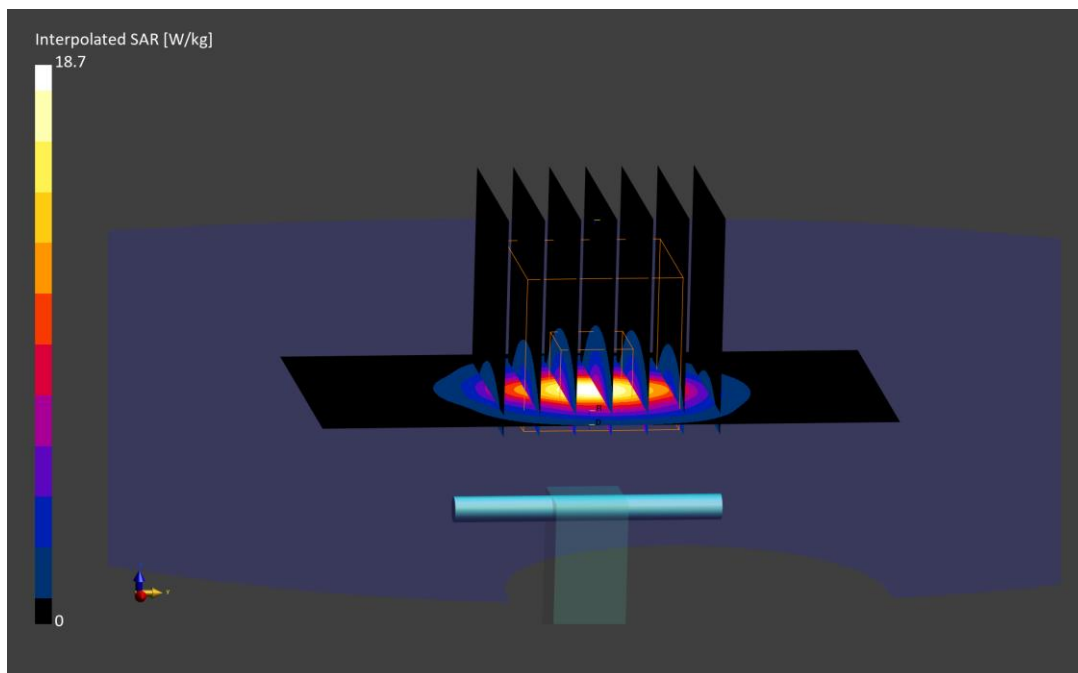

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1055

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 3.03 S/m; perm = 39.4; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/10/2024; Ambient Temp: 21.8°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7782; ConvF:(6.19,6.19,6.19); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.4.2524

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 19.8 W/kg

SAR(1 g) = 7.08 W/kg

Deviation (1 g) = 7.27%

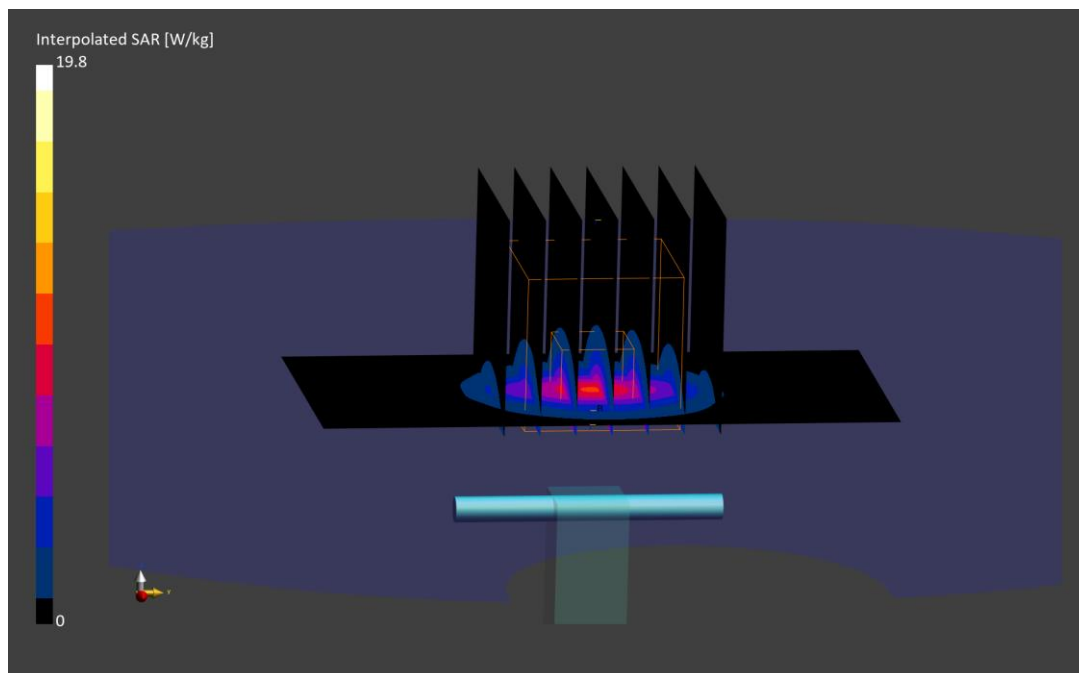

ELEMENT

DUT: Dipole 3500.0 MHz; Type: D3500V2 - SN1055

Communication System: UID: 0, CW; Frequency: 3500.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3500.0 MHz; cond = 2.92 S/m; perm = 38.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/31/2024; Ambient Temp: 20.3°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7499; ConvF:(6.64,6.95,7.18); 2024-01-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; 2023-12-07
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.4.2524

3500.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.4 W/kg

SAR(1 g) = 6.68 W/kg

Deviation (1 g) = 1.21%

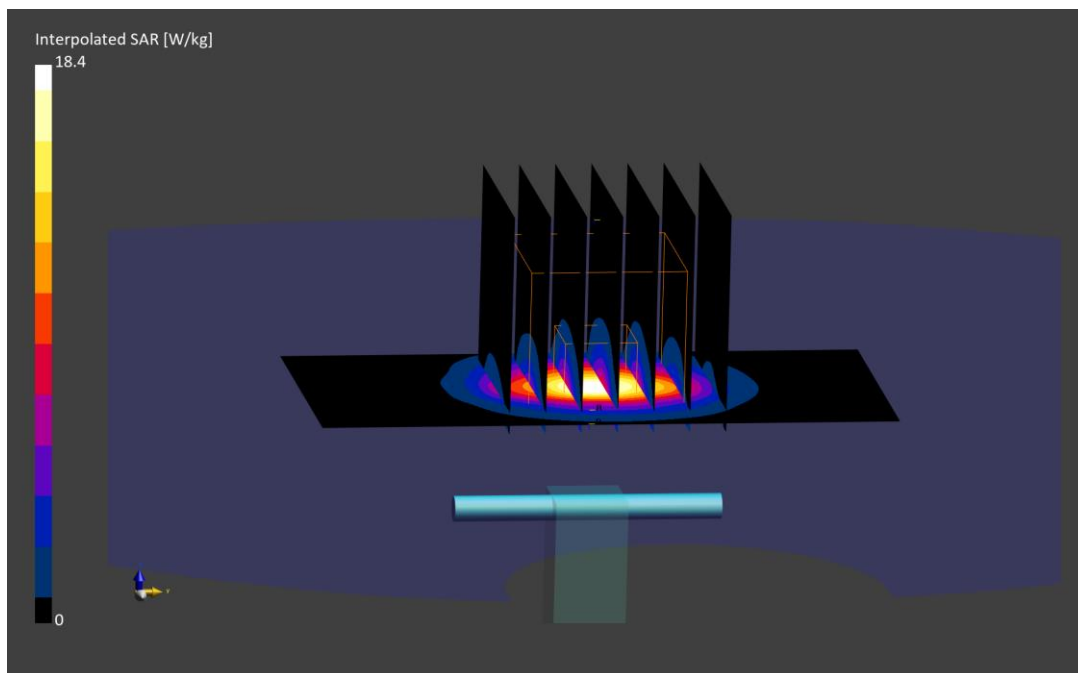

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1097

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.11 S/m; perm = 38.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/26/2024; Ambient Temp: 21.1°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7782; ConvF:(6.18,6.18,6.18); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.4.2524

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 19.3 W/kg

SAR(1 g) = 6.62 W/kg

Deviation (1 g) = -2.79%

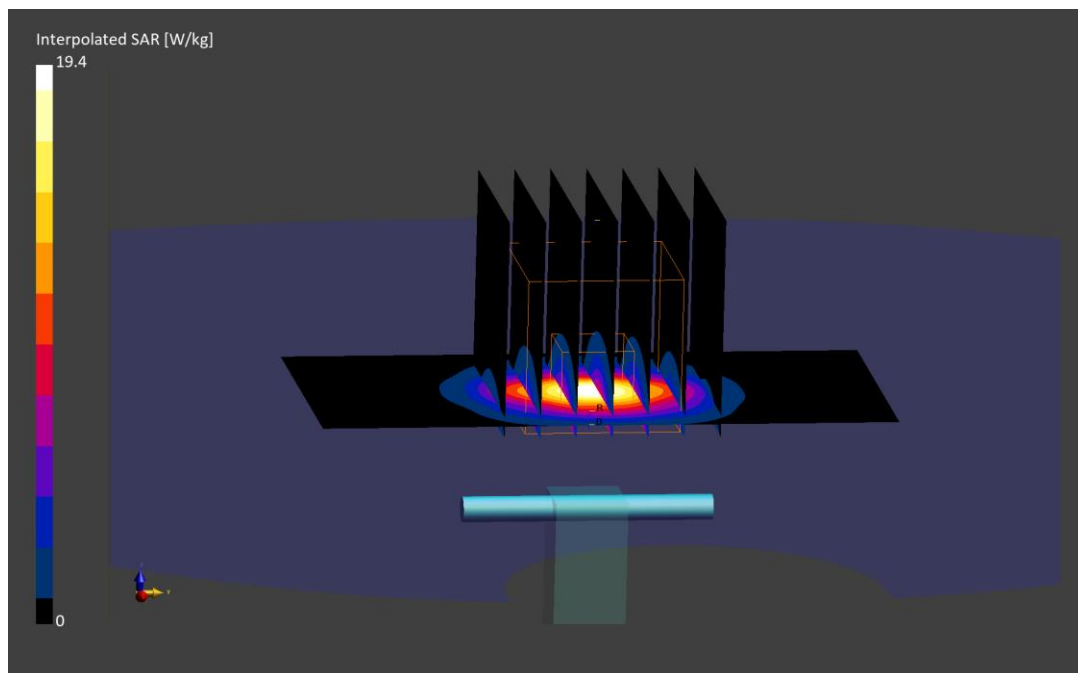

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1097

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.18 S/m; perm = 39.5; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/29/2024; Ambient Temp: 22.1°C; Tissue Temp: 22.0°C

Probe: EX3DV4 - SN7782; ConvF:(6.18,6.18,6.18); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.4.2524

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 19.2 W/kg

SAR(1 g) = 6.58 W/kg

Deviation (1 g) = -3.38%

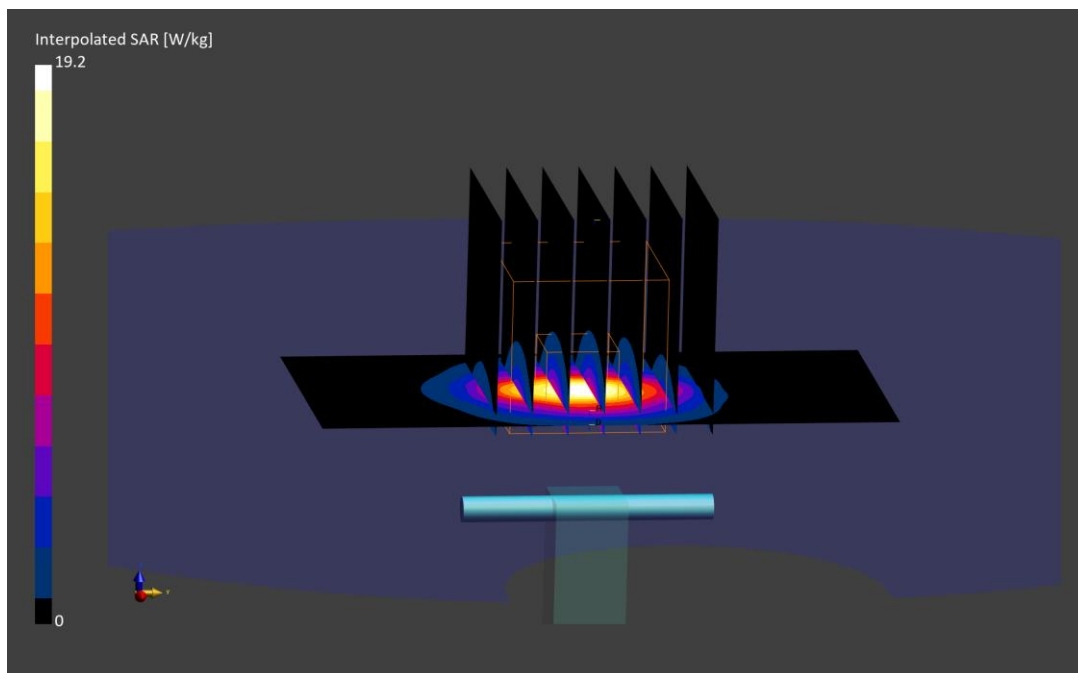

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1002

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.20 S/m; perm = 39.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/10/2024; Ambient Temp: 21.8°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7782; ConvF:(6.18,6.18,6.18); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.4.2524

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 20.4 W/kg

SAR(1 g) = 7.00 W/kg

Deviation (1 g) = 3.09%

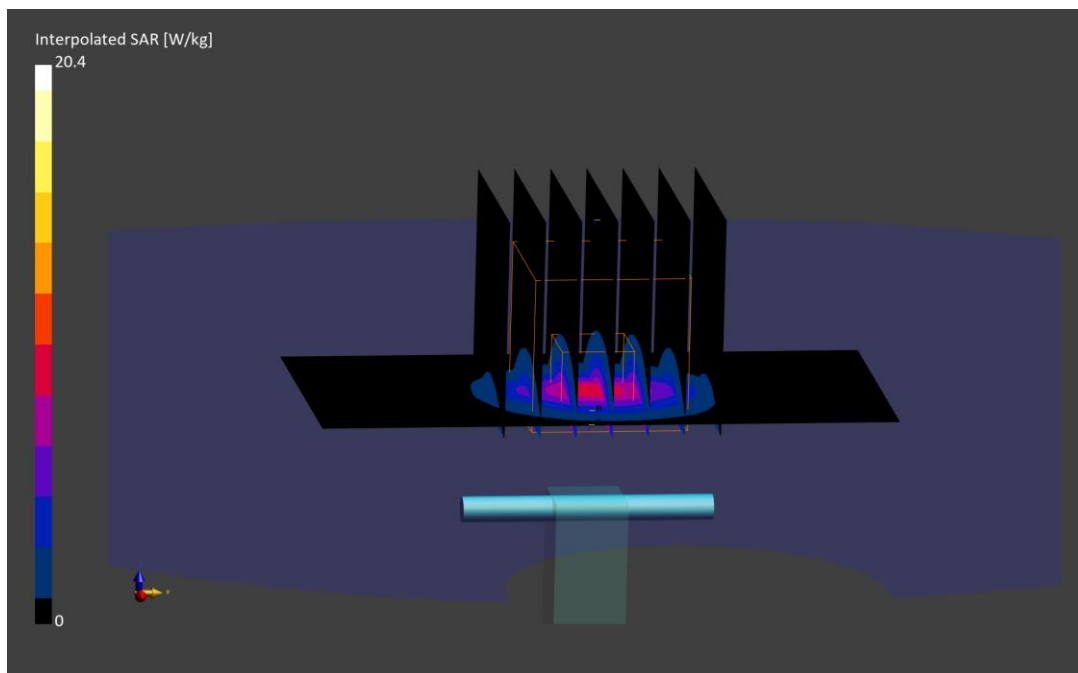

ELEMENT

DUT: Dipole 3700.0 MHz; Type: D3700V2 - SN1002

Communication System: UID: 0, CW; Frequency: 3700.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3700.0 MHz; cond = 3.09 S/m; perm = 38.3; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/31/2024; Ambient Temp: 20.3°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7499; ConvF:(6.65,6.97,7.2); Calibrated: 2024-01-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; Calibrated: 2023-12-07
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.4.2524

3700.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 18.3 W/kg

SAR(1 g) = 6.54 W/kg

Deviation (1 g) = -3.68%

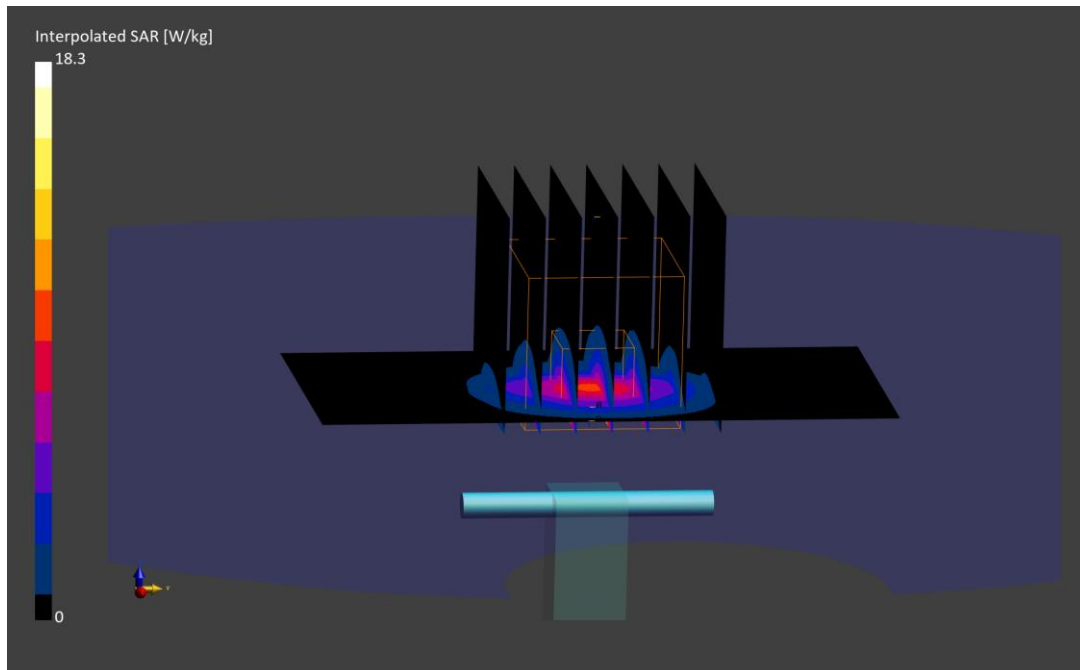

ELEMENT

DUT: Dipole 3900.0 MHz; Type: D3900V2 - SN1073

Communication System: UID: 0, CW; Frequency: 3900.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3900.0 MHz; cond = 3.27 S/m; perm = 38.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/26/2024; Ambient Temp: 21.1°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7782; ConvF:(5.65,5.65,5.65); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.4.2524

3900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 19.7 W/kg

SAR(1 g) = 6.83 W/kg

Deviation (1 g) = -2.01%

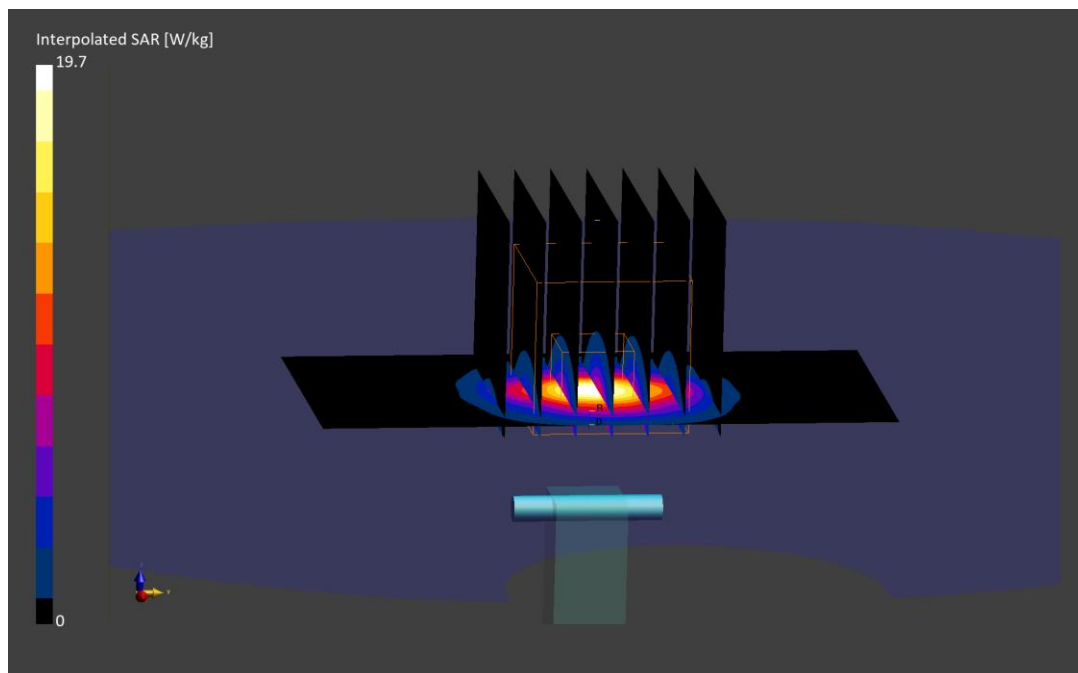

ELEMENT

DUT: Dipole 3900.0 MHz; Type: D3900V2 - SN1073

Communication System: UID: 0, CW; Frequency: 3900.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3900.0 MHz; cond = 3.35 S/m; perm = 39.2; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 05/29/2024; Ambient Temp: 22.1°C; Tissue Temp: 22.0°C

Probe: EX3DV4 - SN7782; ConvF:(5.65,5.65,5.65); Calibrated: 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; Calibrated: 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.4.2524

3900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 20.0 W/kg

SAR(1 g) = 6.88 W/kg

Deviation (1 g) = -1.29%

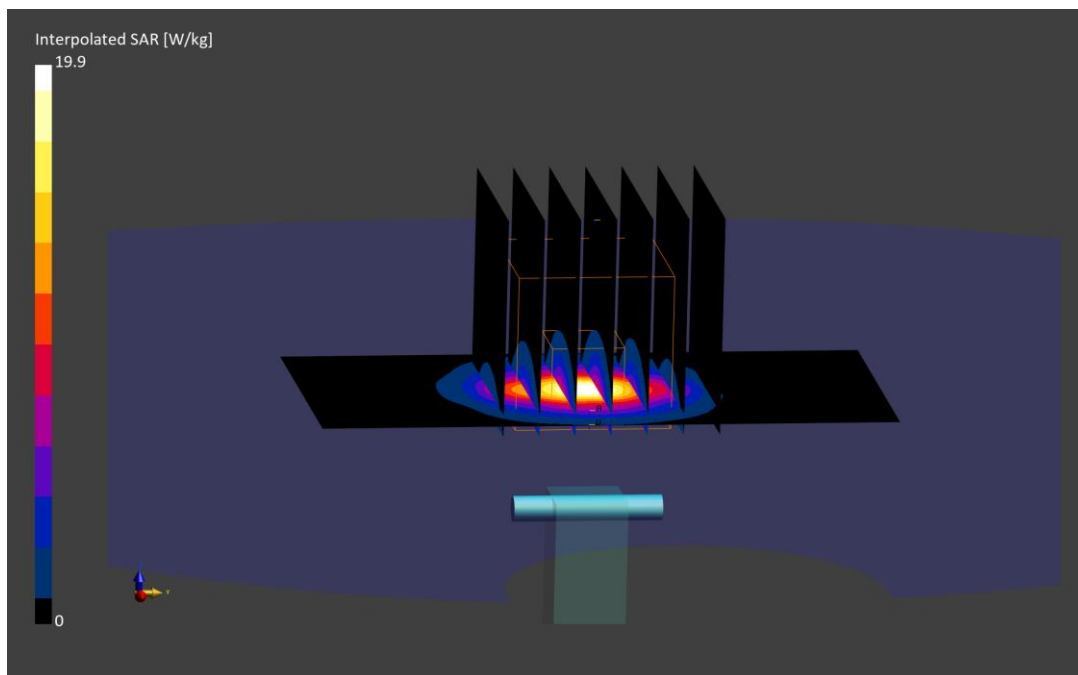

ELEMENT

DUT: Dipole 3900.0 MHz; Type: D3900V2 - SN1062

Communication System: UID: 0, CW; Frequency: 3900.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3900.0 MHz; cond = 3.38 S/m; perm = 38.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/10/2024; Ambient Temp: 21.8°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7782; ConvF:(5.65,5.65,5.65); 2023-09-12
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1646; 2023-09-08
Phantom: Twin-SAM V8.0; Serial: 1944
Measurement SW: DASY Module SAR V16.2.4.2524

3900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 21.0 W/kg

SAR(1 g) = 7.26 W/kg

Deviation (1 g) = 5.37%

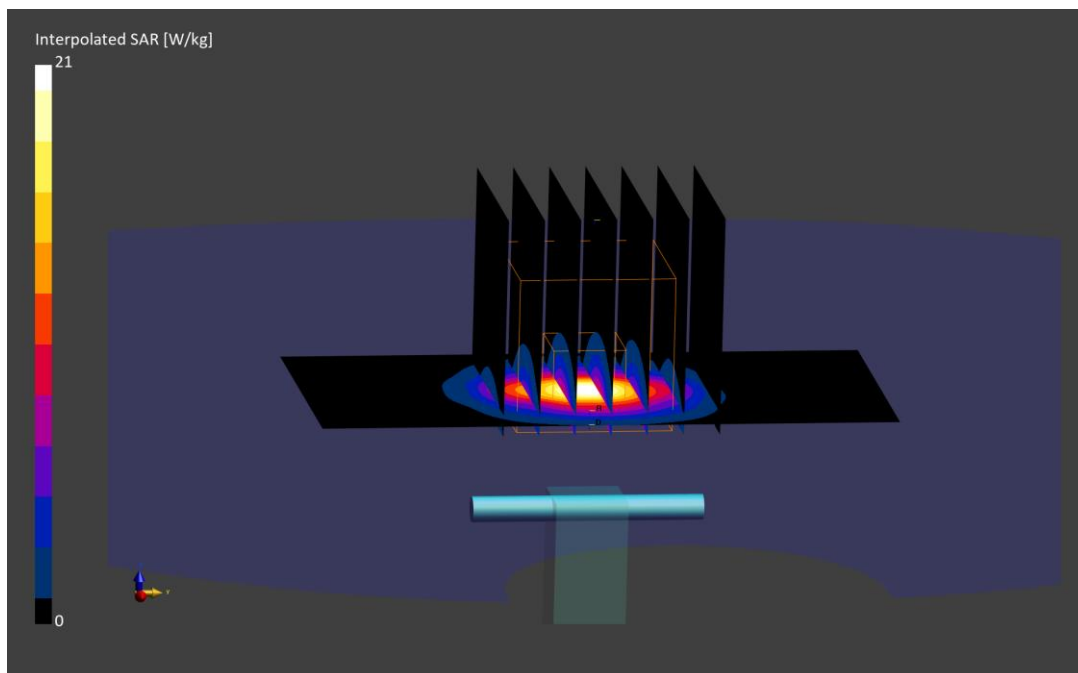

ELEMENT

DUT: Dipole 3900.0 MHz; Type: D3900V2 - SN1062

Communication System: UID: 0, CW; Frequency: 3900.0 MHz
Medium: 3600 Head; Medium parameters used:
f = 3900.0 MHz; cond = 3.27 S/m; perm = 38.0; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 07/31/2024; Ambient Temp: 20.3°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7499; ConvF:(6.47,6.78,6.99); 2024-01-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1644; 2023-12-07
Phantom: Twin-SAM V8.0; Serial: 1357
Measurement SW: DASY Module SAR V16.2.4.2524

3900.0 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (28.0 x 28.0 x 28.0): Measurement grid: dx=5.0 mm, dy=5.0 mm, dz=1.4 mm; Graded Ratio: 1.5

Peak SAR (extrapolated) = 21.4 W/kg

SAR(1 g) = 6.96 W/kg

Deviation (1 g) = 1.02%

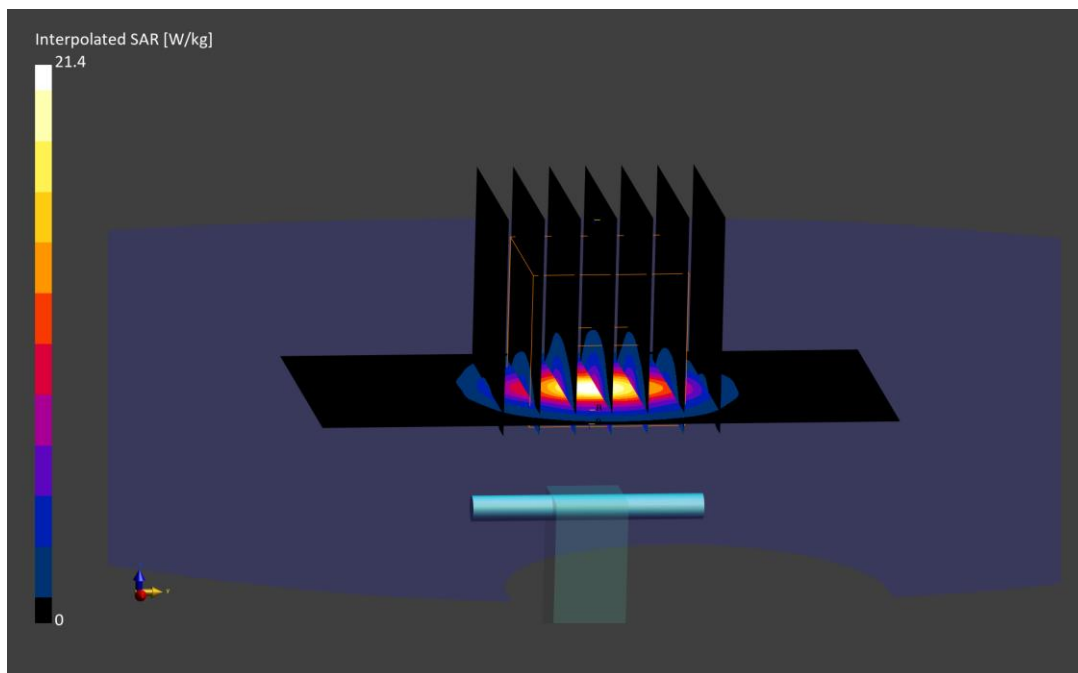

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5250.0 MHz; cond = 4.49 S/m; perm = 37.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/03/2024; Ambient Temp: 20.1°C; Tissue Temp: 19.1°C

Probe: EX3DV4 - SN3746; ConvF:(5.12,5.12,5.12); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.2.4.2524

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.4 W/kg

SAR(1 g) = 4.13 W/kg

Deviation (1 g) = 2.86%

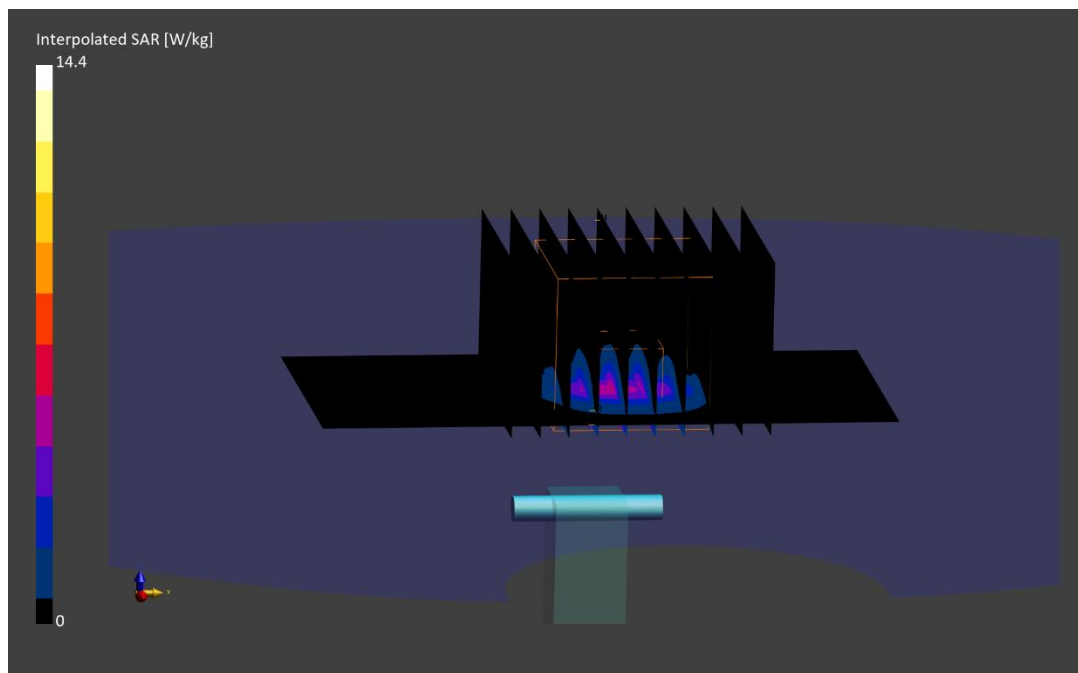

ELEMENT

DUT: Dipole 5250.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5250.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5250.0 MHz; cond = 4.56 S/m; perm = 34.6; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/27/2024; Ambient Temp: 20.8°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7427; ConvF:(4.73,5.26,5.35); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5250.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.9 W/kg

SAR(1 g) = 3.80 W/kg

Deviation (1 g) = -5.35%

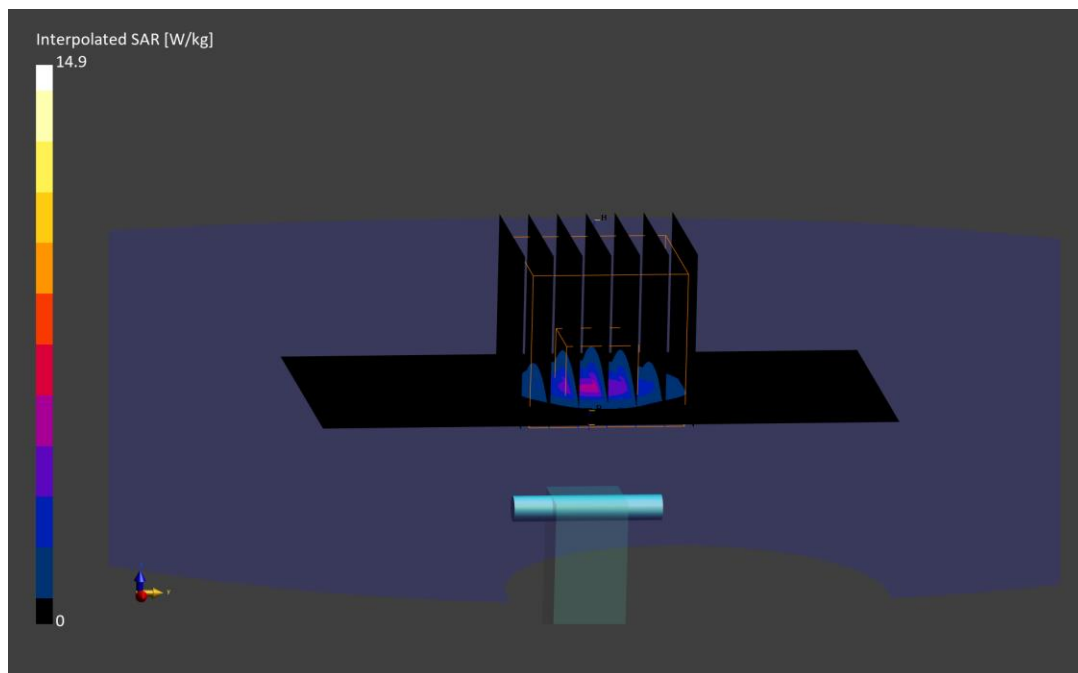

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5600.0 MHz; cond = 4.89 S/m; perm = 37.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/03/2024; Ambient Temp: 20.1°C; Tissue Temp: 19.1°C

Probe: EX3DV4 - SN3746; ConvF:(4.45,4.45,4.45); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.2.4.2524

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.4 W/kg

SAR(1 g) = 4.37 W/kg

Deviation (1 g) = 4.17%

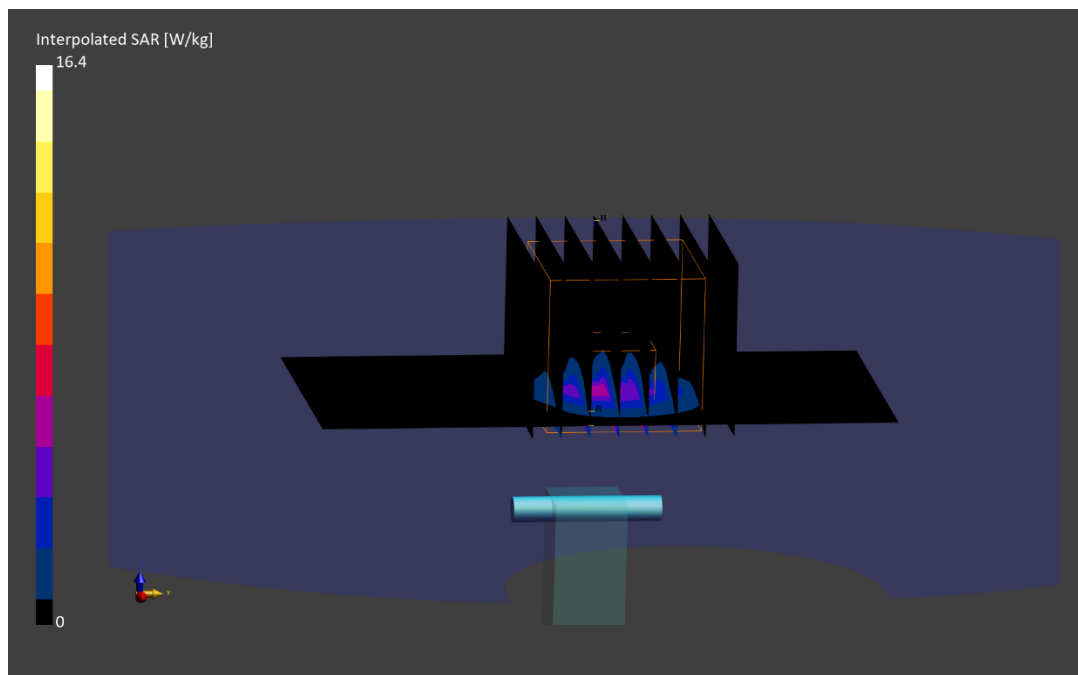

ELEMENT

DUT: Dipole 5600.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5600.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5600.0 MHz; cond = 4.93 S/m; perm = 34.1; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/27/2024; Ambient Temp: 20.8°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7427; ConvF:(4.18,4.62,4.72); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5600.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.1 W/kg

SAR(1 g) = 4.12 W/kg

Deviation (1 g) = -1.79%

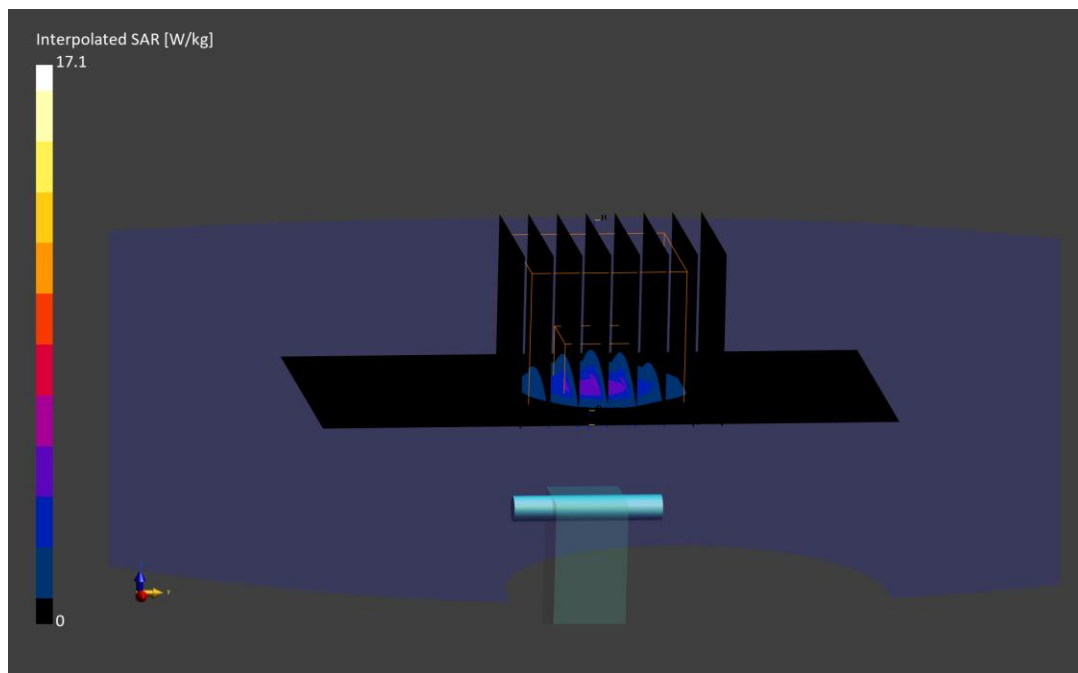

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5750.0 MHz; cond = 5.07 S/m; perm = 36.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/03/2024; Ambient Temp: 20.1°C; Tissue Temp: 19.1°C

Probe: EX3DV4 - SN3746; ConvF:(4.59,4.59,4.59); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.2.4.2524

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.2 W/kg

SAR(1 g) = 4.23 W/kg

Deviation (1 g) = 6.42%

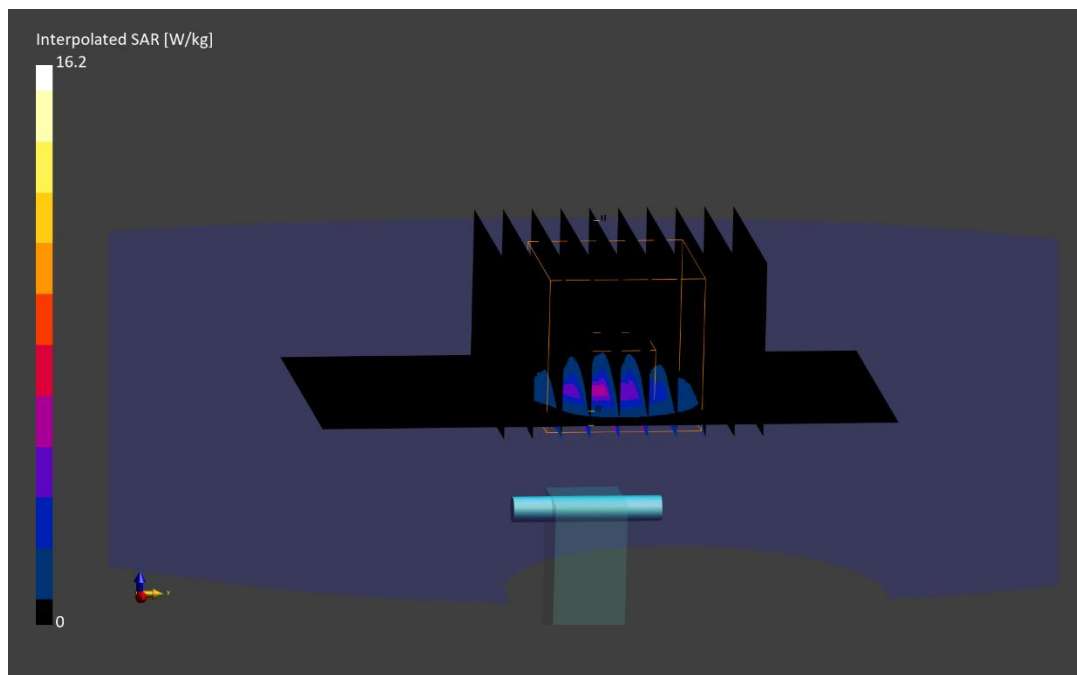

ELEMENT

DUT: Dipole 5750.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5750.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5750.0 MHz; cond = 5.10 S/m; perm = 33.8; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/27/2024; Ambient Temp: 20.8°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7427; ConvF:(4.35,4.78,4.93); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5750.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 16.2 W/kg

SAR(1 g) = 3.80 W/kg

Deviation (1 g) = -4.40%

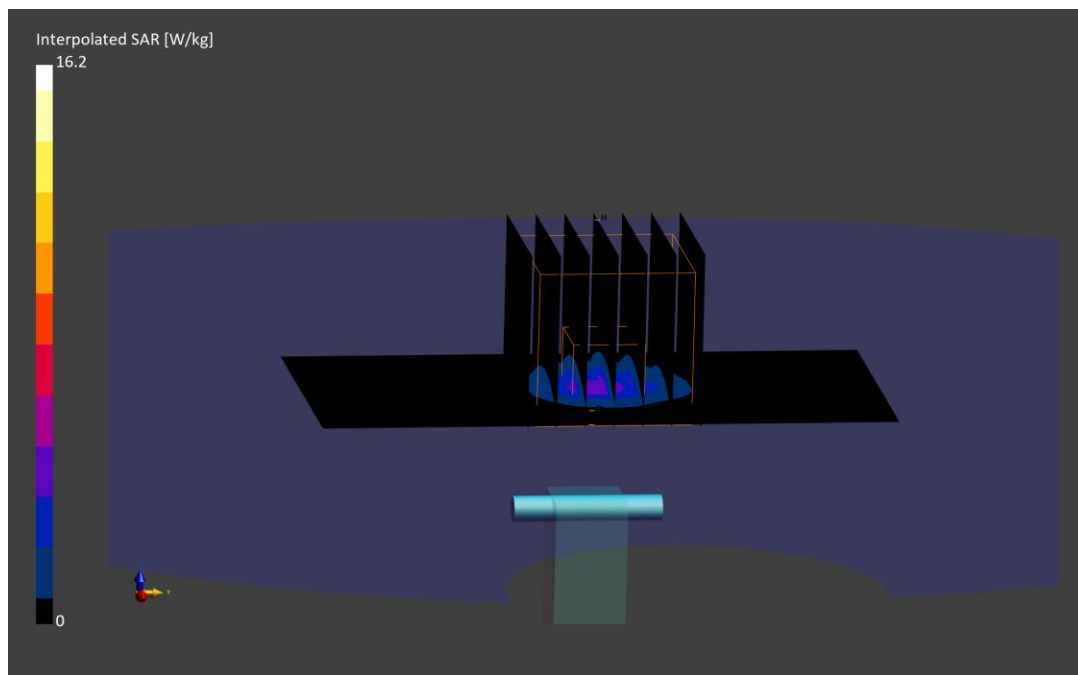

ELEMENT

DUT: Dipole 5850.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5850.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5850.0 MHz; cond = 5.18 S/m; perm = 36.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/03/2024; Ambient Temp: 20.1°C; Tissue Temp: 19.1°C

Probe: EX3DV4 - SN3746; ConvF:(4.5,4.5,4.5); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1237; Calibrated: 2023-10-18
Phantom: Twin-SAM V8.0; Serial: 2027
Measurement SW: DASY Module SAR V16.2.4.2524

5850.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.0 W/kg

SAR(1 g) = 4.32 W/kg

Deviation (1 g) = 5.11%

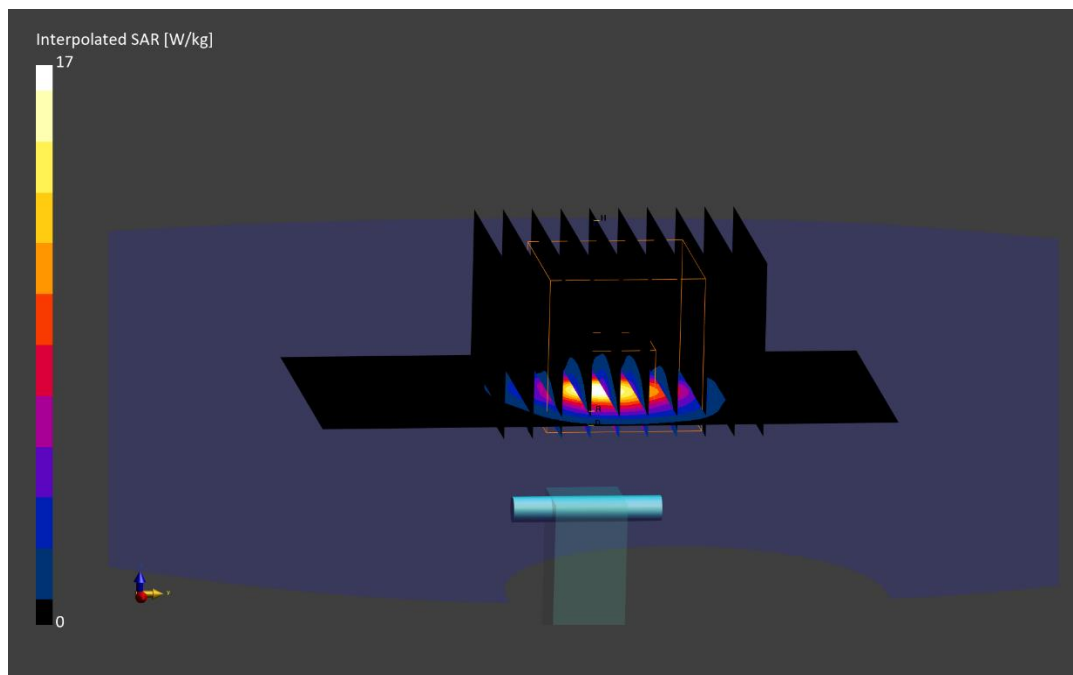

ELEMENT

DUT: Dipole 5850.0 MHz; Type: D5GHzV2 - SN1066

Communication System: UID: 0, CW; Frequency: 5850.0 MHz
Medium: 5200-5800 Head; Medium parameters used:
f = 5850.0 MHz; cond = 5.20 S/m; perm = 33.7; density = 1000 kg/m³
Phantom Section: Flat; Space: 10 mm

Test Date: 06/27/2024; Ambient Temp: 20.8°C; Tissue Temp: 19.8°C

Probe: EX3DV4 - SN7427; ConvF:(4.04,4.57,4.63); Calibrated: 2024-02-09
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn467; Calibrated: 2024-02-09
Phantom: Twin-SAM V8.0; Serial: 2070
Measurement SW: DASY Module SAR V16.2.4.2524

5850.0 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (40.0 x 80.0): Measurement grid: dx=10.0 mm, dy=10.0 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=4.0 mm, dy=4.0 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.0 W/kg

SAR(1 g) = 3.96 W/kg

Deviation (1 g) = -3.65%

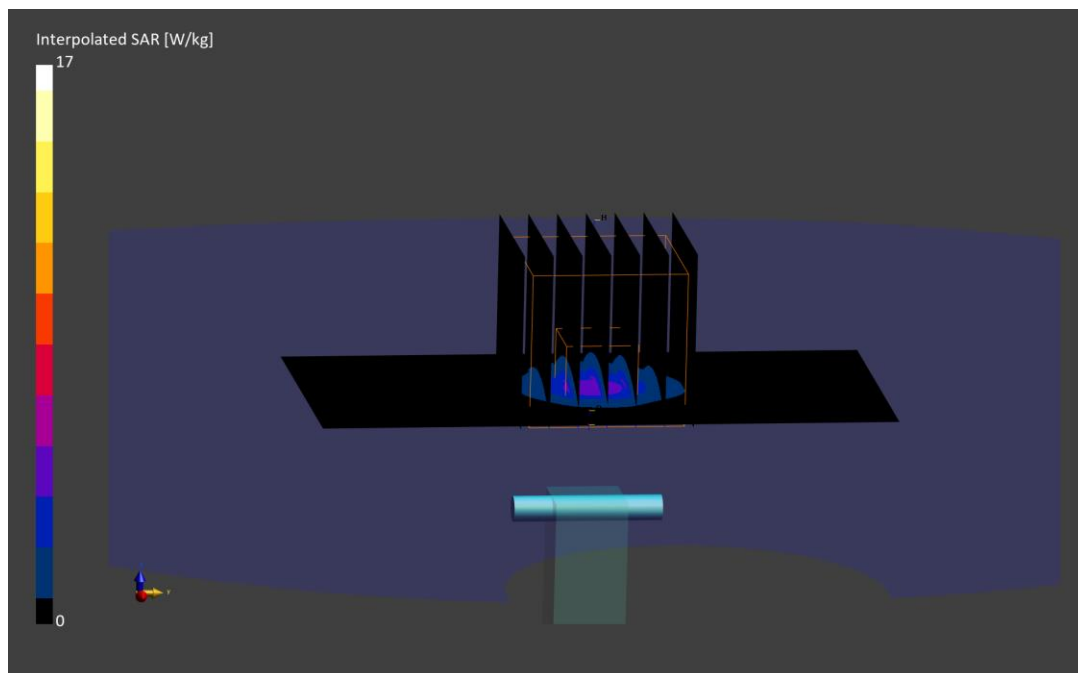

ELEMENT

DUT: Dipole 6500.0 MHz; Type: D6.5GHzV2 - SN1019

Communication System: UID: 0, CW; Frequency: 6500.0 MHz
Medium: 6000 Head; Medium parameters used:
f = 6500.0 MHz; cond = 5.92 S/m; perm = 34.9; density = 1000 kg/m³
Phantom Section: Flat; Space: 5 mm

Test Date: 05/28/2024; Ambient Temp: 21.3°C; Tissue Temp: 20.0°C

Probe: EX3DV4 - SN7420; ConvF:(5.21,5.12,5.28); Calibrated: 2023-10-16
Sensor-Surface: 1.4mm (VMS + 6p)
Electronics: DAE4 Sn1333; Calibrated: 2023-10-18
Phantom: Twin-SAM V4.0; Serial: 1275
Measurement SW: DASY Module SAR V16.2.4.2524

6500.0 MHz System Verification at 14.0 dBm (25 mW)


Area Scan (51.0 x 85.0): Measurement grid: dx=8.5 mm, dy=8.5 mm

Zoom Scan (22.0 x 22.0 x 22.0): Measurement grid: dx=3.4 mm, dy=3.4 mm, dz=1.4 mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 43.5 W/kg

SAR(1 g) = 7.10 W/kg; APD (4 cm²) = 31.8 W/m²

Deviation (1 g) = -3.07%; Deviation (APD) = -3.64%

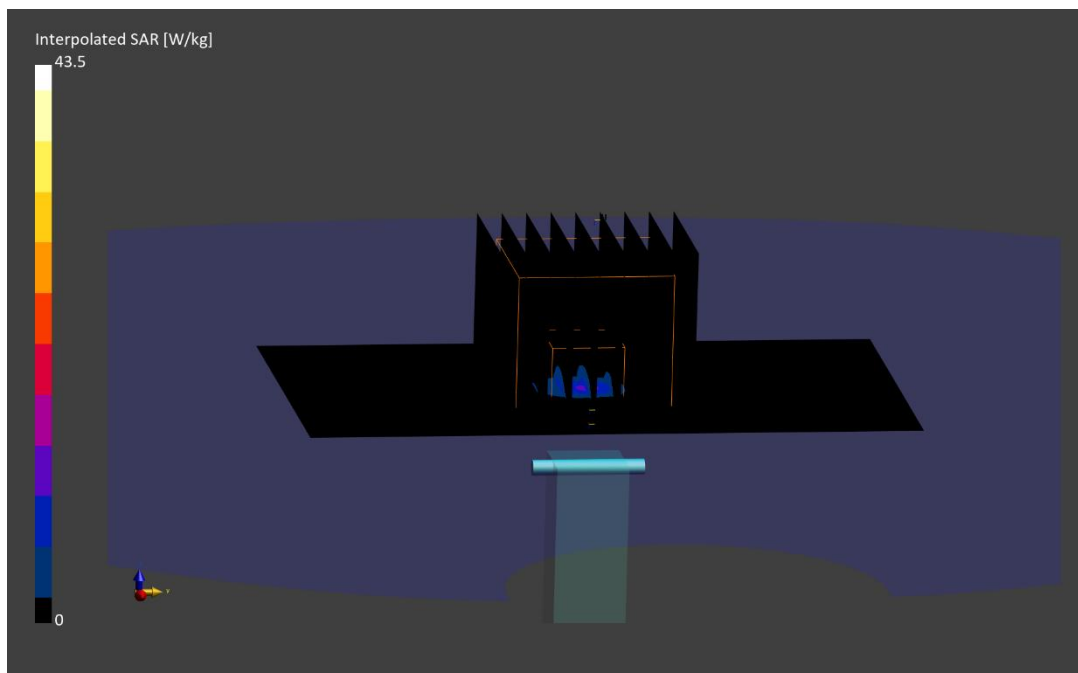

Date: 05/22/2024

10 GHz System Verification

Device Under Test Properties

DUT	Serial Number
10 GHz Verification Source	1006

Exposure Conditions

Phantom Section	Position	Test Distance [mm]	Band	Frequency [MHz]
5G	FRONT	10.00		10000.0

Hardware Setup

Probe, Calibration Date	DAE, Calibration Date
EUmmWV3 - SN9407, 10/09/2023	DAE4 - SN793, 10/18/2023

Software Setup


Software	Software Version
cDASY6 Module mmWave	3.2.0.1840

Scans Setup


Scan Type	5G Scan
Grid Extents [mm]	60.0 x 60.0
Grid Steps [lambda]	0.25 x 0.25
Sensor Surface [mm]	10.0

Measurement Results

Scan Type	5G Scan
Avg. Area [cm ²]	4.00
pS _{tot} avg [W/m ²]	54.4
pS _n avg [W/m ²]	54.3
E _{peak} [V/m]	150
Power Drift [dB]	0.01

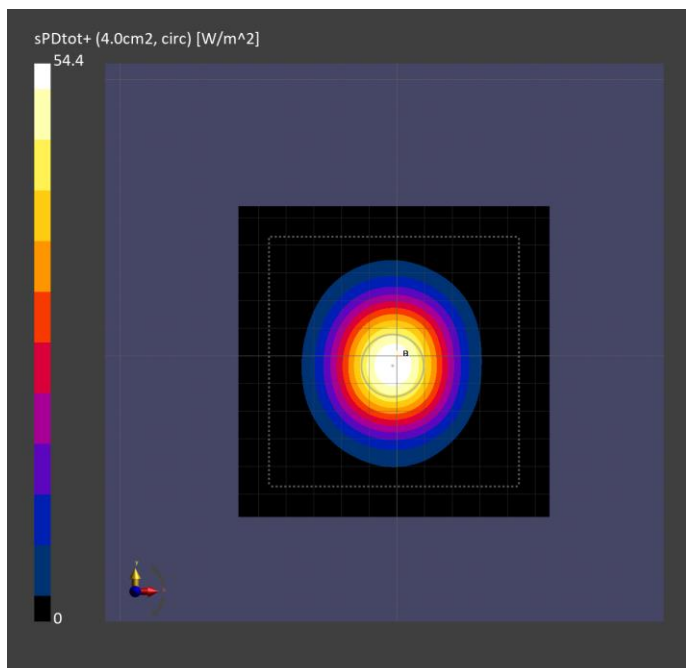

10 GHz System Verification

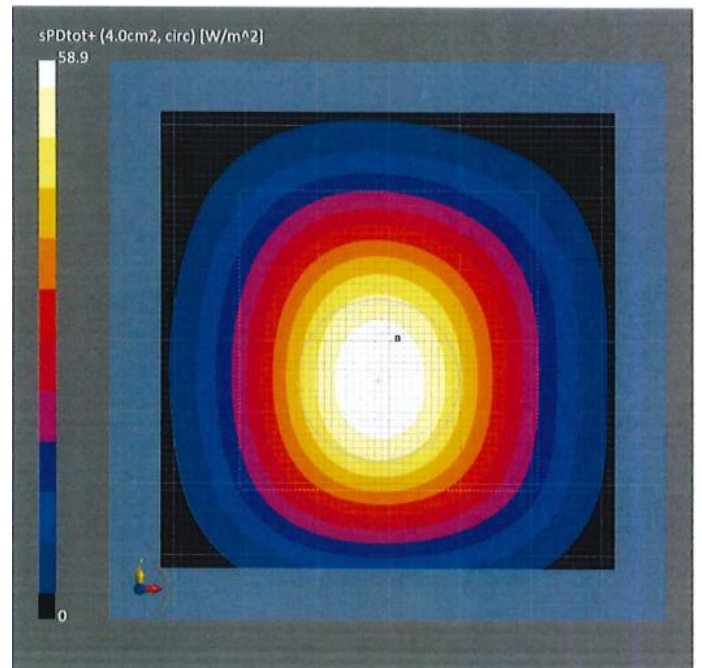

Calibration Certificate