

HAC-RF Emission System Check

Communication System: UID 0, CW (0); Frequency: 5500 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 5500 MHz; Calibrated: 8/13/2021
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1434; Calibrated: 11/11/2021
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7495)

Dipole E-Field Measurement 5.5GHz/5.5GHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 25.52 V/m; Power Drift = -0.03 dB


Applied MIF = 0.00 dB

RF audio interference level = 40.34 dBV/m

Emission category: M1

MIF scaled E-field

Grid 1 M2 38.27 dBV/m	Grid 2 M2 38.55 dBV/m	Grid 3 M2 38.39 dBV/m
Grid 4 M1 40.11 dBV/m	Grid 5 M1 40.34 dBV/m	Grid 6 M1 40.12 dBV/m
Grid 7 M2 38.7 dBV/m	Grid 8 M2 38.97 dBV/m	Grid 9 M2 38.73 dBV/m

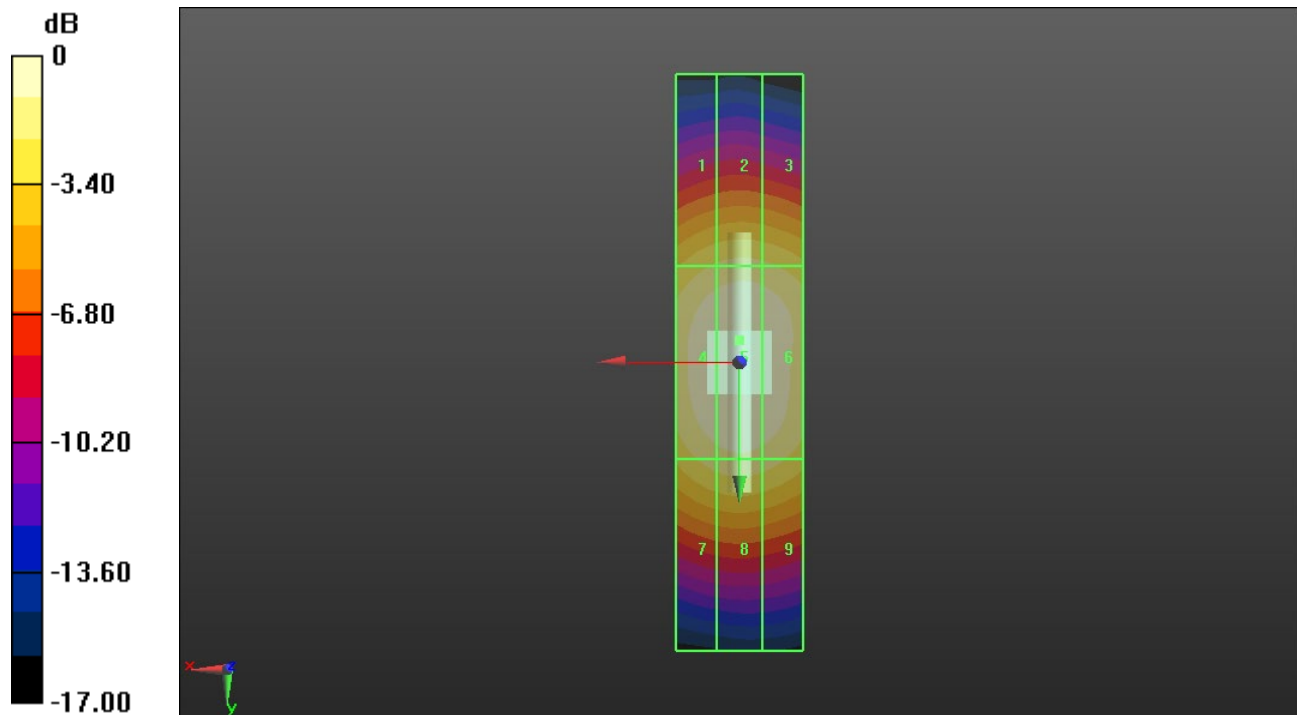

0 dB = 104.0 V/m = 40.34 dBV/m

HAC-RF Emission System Check

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 835 MHz; Calibrated: 8/13/2021

- Sensor-Surface: (Fix Surface)

- Electronics: DAE4 Sn1434; Calibrated: 11/11/2021

- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB

- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7495)

Dipole E-Field measurement 835MHz/835 MHz/Hearing Aid Compatibility Test at 15mm distance (41x361x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 125.0 V/m; Power Drift = 0.00 dB


Applied MIF = 0.00 dB

RF audio interference level = 41.51 dBV/m

Emission category: M3

MIF scaled E-field

Grid 1 M3 41.17 dBV/m	Grid 2 M3 41.51 dBV/m	Grid 3 M3 41.42 dBV/m
Grid 4 M4 36.05 dBV/m	Grid 5 M4 36.38 dBV/m	Grid 6 M4 36.36 dBV/m
Grid 7 M3 40.64 dBV/m	Grid 8 M3 41.2 dBV/m	Grid 9 M3 41.2 dBV/m

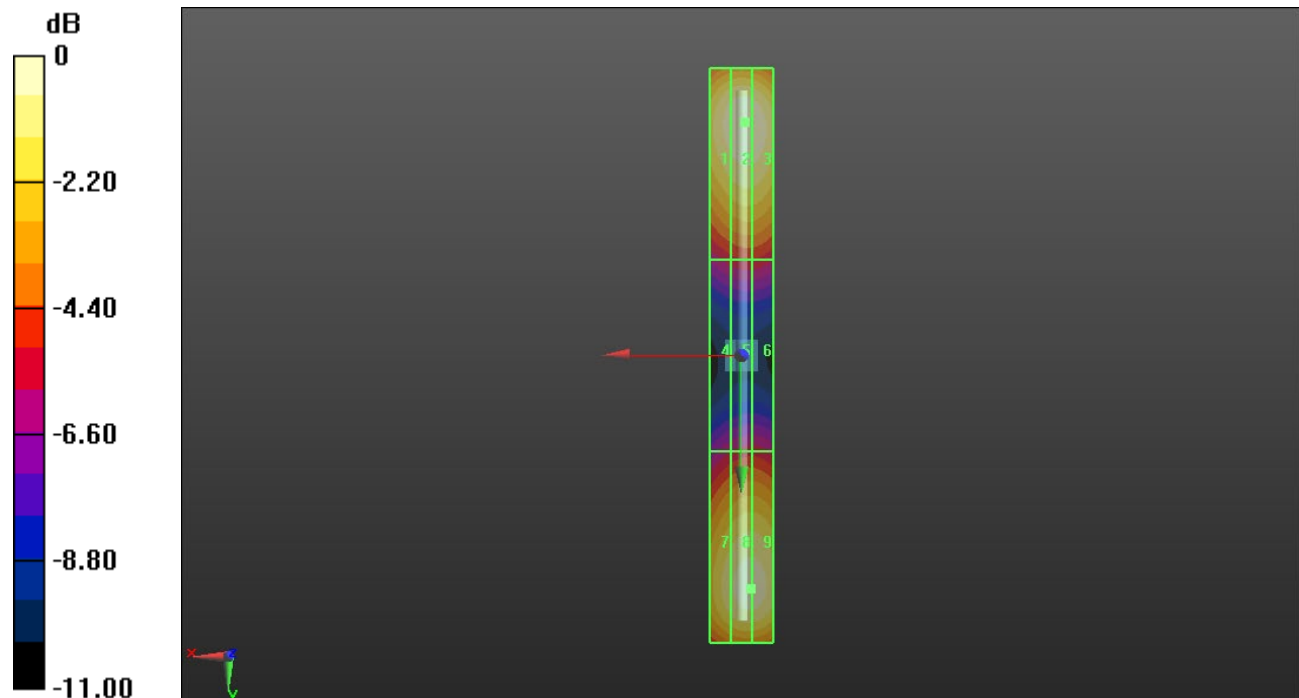

0 dB = 119.0 V/m = 41.51 dBV/m

HAC-RF Emission System Check

Communication System: UID 0, CW; Frequency: 1880 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 1880 MHz; Calibrated: 8/13/2021
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1434; Calibrated: 11/11/2021
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7495)

Dipole E-Field Measurement 1880MHz/1880 MHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 146.3 V/m; Power Drift = 0.01 dB


Applied MIF = 0.00 dB

RF audio interference level = 39.30 dBV/m

Emission category: M2

MIF scaled E-field

Grid 1 M2 38.86 dBV/m	Grid 2 M2 39.3 dBV/m	Grid 3 M2 39.27 dBV/m
Grid 4 M2 36.16 dBV/m	Grid 5 M2 36.43 dBV/m	Grid 6 M2 36.43 dBV/m
Grid 7 M2 38.52 dBV/m	Grid 8 M2 38.93 dBV/m	Grid 9 M2 38.91 dBV/m

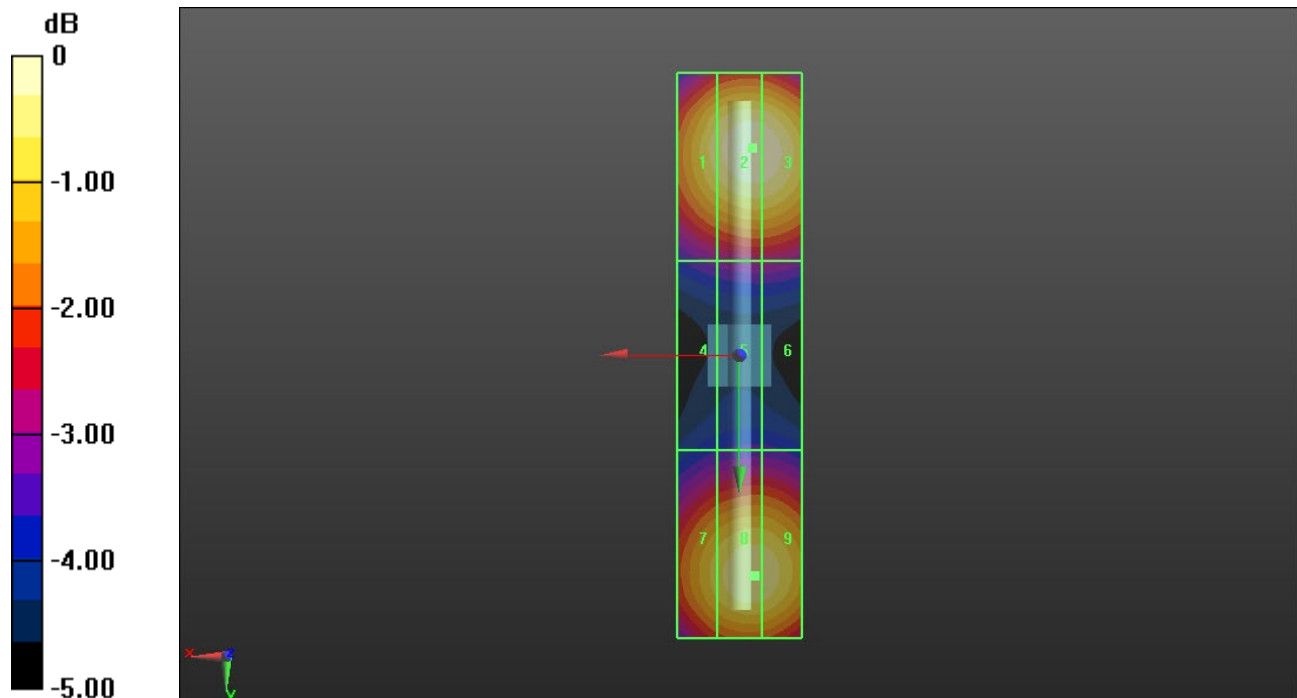

0 dB = 92.21 V/m = 39.30 dBV/m

HAC-RF Emission System Check

Communication System: UID 0, CW (0); Frequency: 2450 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 2450 MHz; Calibrated: 8/13/2021
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1434; Calibrated: 11/11/2021
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7495)

Dipole E-Field Measurement 2450MHz/2450 MHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 76.77 V/m; Power Drift = 0.02 dB



Applied MIF = 0.00 dB

RF audio interference level = 39.22 dBV/m

Emission category: M2

MIF scaled E-field

Grid 1 M2 38.86 dBV/m	Grid 2 M2 39.22 dBV/m	Grid 3 M2 39.17 dBV/m
Grid 4 M2 37.85 dBV/m	Grid 5 M2 38.09 dBV/m	Grid 6 M2 38.08 dBV/m
Grid 7 M2 38.74 dBV/m	Grid 8 M2 39.09 dBV/m	Grid 9 M2 39.04 dBV/m

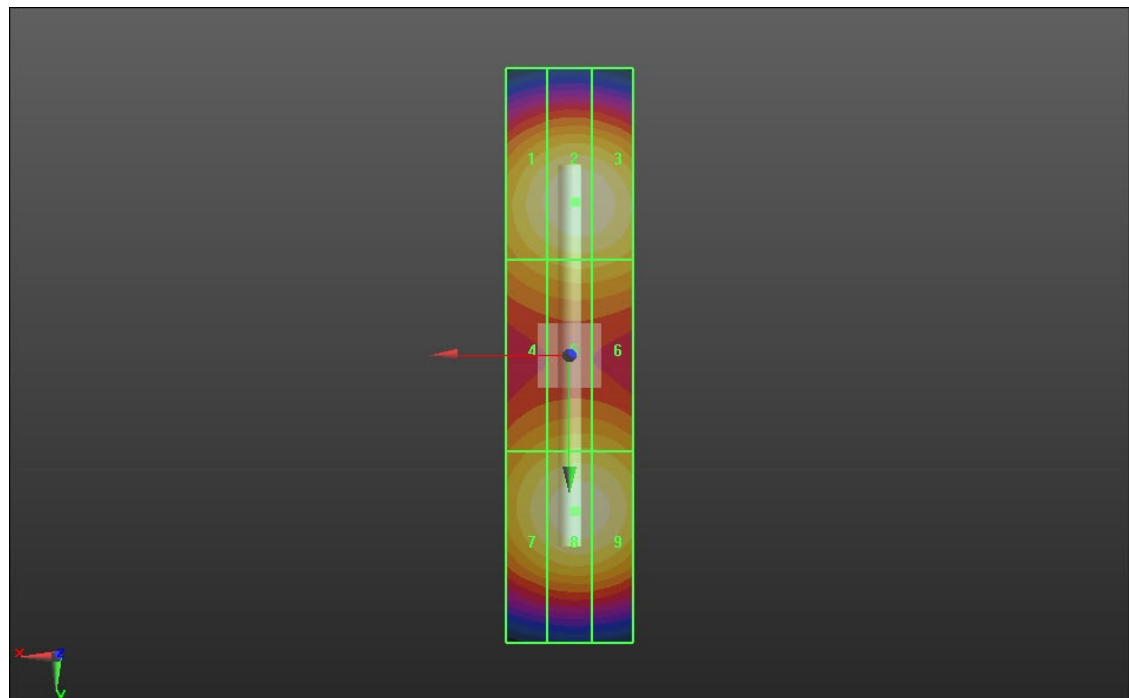

0 dB = 91.39 V/m = 39.22 dBV/m

HAC-RF Emission System Check

Communication System: UID 0, CW (0); Frequency: 2600 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 2600 MHz; Calibrated: 8/13/2021
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1434; Calibrated: 11/11/2021
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7495)

Dipole E-Field Measurement 2600MHz/2600 MHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 68.17 V/m; Power Drift = 0.02 dB



Applied MIF = 0.00 dB

RF audio interference level = 39.19 dBV/m

Emission category: M2

MIF scaled E-field

Grid 1 M2 38.71 dBV/m	Grid 2 M2 39.04 dBV/m	Grid 3 M2 38.99 dBV/m
Grid 4 M2 38.1 dBV/m	Grid 5 M2 38.34 dBV/m	Grid 6 M2 38.33 dBV/m
Grid 7 M2 38.8 dBV/m	Grid 8 M2 39.19 dBV/m	Grid 9 M2 39.16 dBV/m

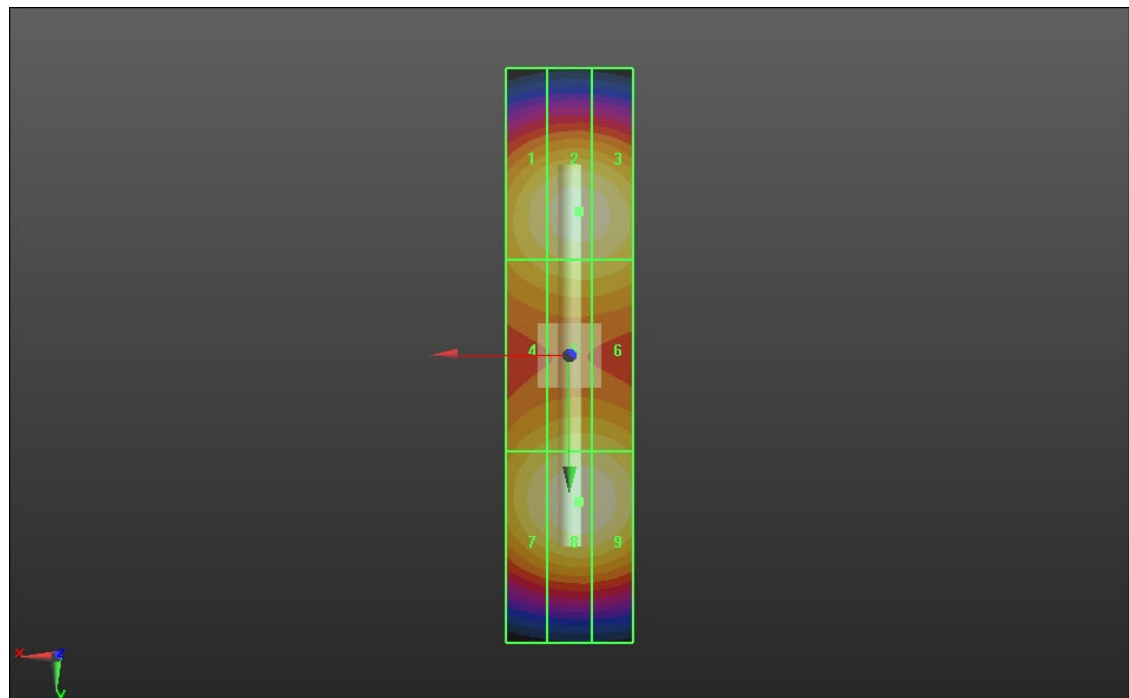

0 dB = 91.15 V/m = 39.20 dBV/m

HAC-RF Emission System Check

Communication System: UID 0, CW (0); Frequency: 3500 MHz; Duty Cycle: 1:1

Phantom section: RF Section

DASY5 Configuration:

- Probe: EF3DV3 - SN4028; ConvF(1, 1, 1) @ 3500 MHz; Calibrated: 8/13/2021
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1434; Calibrated: 11/11/2021
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BB
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7495)

Dipole E-Field Measurement 3500MHz/3500 MHz/Hearing Aid Compatibility Test at 15mm distance (41x181x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 36.83 V/m; Power Drift = 0.02 dB


Applied MIF = 0.00 dB

RF audio interference level = 38.99 dBV/m

Emission category: M2

MIF scaled E-field

Grid 1 M2 38.57 dBV/m	Grid 2 M2 38.87 dBV/m	Grid 3 M2 38.85 dBV/m
Grid 4 M2 38.71 dBV/m	Grid 5 M2 38.99 dBV/m	Grid 6 M2 38.92 dBV/m
Grid 7 M2 38.71 dBV/m	Grid 8 M2 38.99 dBV/m	Grid 9 M2 38.93 dBV/m

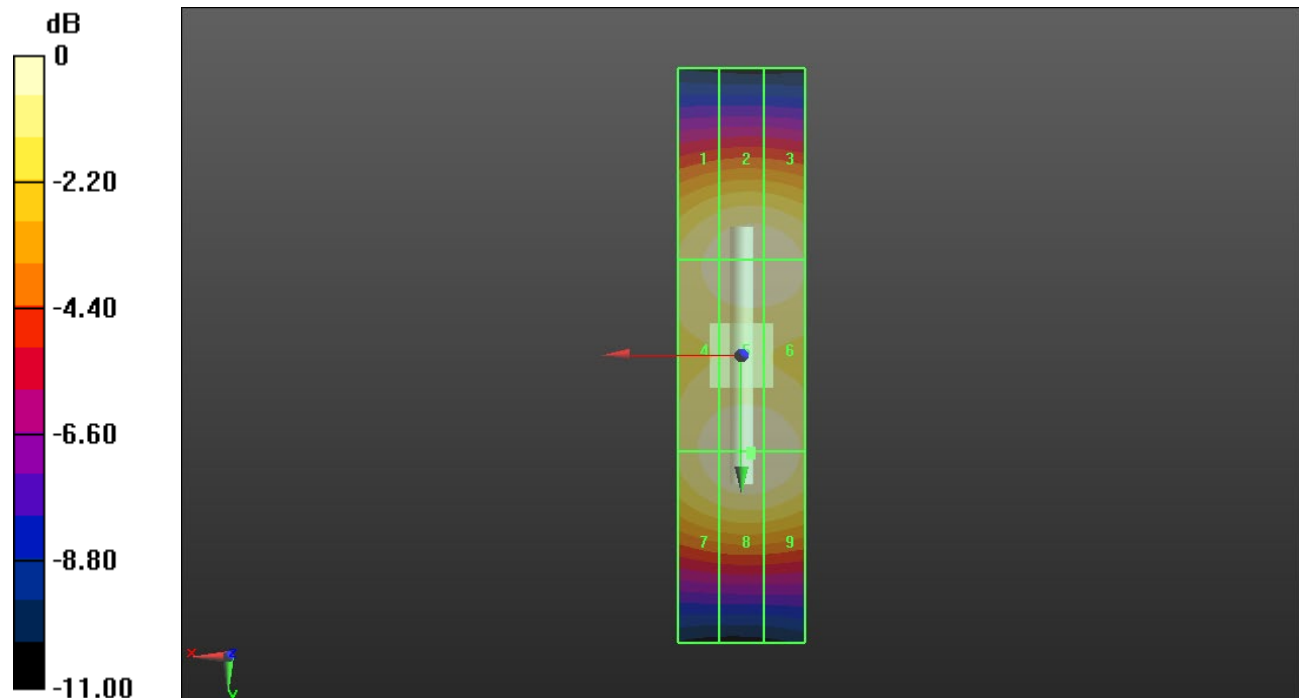

0 dB = 89.04 V/m = 38.99 dBV/m