

Client **EMC Technologies**

**CALIBRATION CERTIFICATE**

Object(s) **D300V2 - SN:1005**

Calibration procedure(s) **QA CAL-15.v2  
 Calibration procedure for dipole validation kits below 800 MHz**

Calibration date: **November 27, 2003**



Condition of the calibrated item **In Tolerance (according to the specific calibration document)**

This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

Calibration Equipment used (M&TE critical for calibration)

Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM E4419B	GB41293874	2-Apr-03 (METAS, No 252-0250)	Apr-04
Power sensor E4412A	MY41495277	2-Apr-03 (METAS, No 252-0250)	Apr-04
Reference 20 dB Attenuator	SN: 5086 (20b)	3-Apr-03 (METAS No. 251-0340)	Apr-04
Fluke Process Calibrator Type 702	SN: 6295803	8-Sep-03 (Sintrel SCS No. E-030020)	Sep-04
Power sensor HP 8481A	MY41092180	18-Sep-02 (SPEAG, in house check Nov-03)	In house check: Nov 05
RF generator HP 8684C	US3642U01700	4-Aug-99 (SPEAG, in house check Aug-02)	In house check: Aug-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-03)	In house check: Nov 05

	Name	Function	Signature
Calibrated by:	Katja Pokovic	Laboratory Director	
Approved by:	Fin Bornholt	R&D Director	

Date issued: November 28, 2003

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

# DASY

## Dipole Validation Kit

Type: D300V2

Serial: 1005

Manufactured: September 2, 2003  
Calibrated: November 27, 2003



## 1. Measurement Conditions

The measurements were performed in the 6mm thick flat phantom filled with head simulating liquid of the following electrical parameters at 300 MHz:

Relative Dielectricity	45.8	± 5%
Conductivity	0.89 mho/m	± 5%

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 8.75 at 300 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center of the flat phantom and the dipole was oriented parallel to the longer side of the phantom. The standard measuring distance was 15mm from dipole center to the liquid surface including the 6mm thick phantom shell. The included distance spacer was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was 398 mW ± 3 %. The results are normalized to 1W input power.

## 2. SAR Measurement with DASY System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the advanced extrapolation are:

averaged over 1 cm <sup>3</sup> (1 g) of tissue:	2.94 mW/g ± 20.7 % (k=2) <sup>1</sup>
averaged over 10 cm <sup>3</sup> (10 g) of tissue:	1.95 mW/g ± 20.2 % (k=2) <sup>1</sup>

---

<sup>1</sup> validation uncertainty



Test Laboratory: SPEAG, Zurich, Switzerland  
File Name: [D300\\_SN1005\\_SN1507\\_H300\\_271103.da4](#)

**DUT: Dipole 300 MHz; Type: D300V2; Serial: D300V2 - SN:1005**  
**Program Name: System Performance Check at 300 MHz**

Communication System: CW; Frequency: 300 MHz; Duty Cycle: 1:1  
Medium: HSL300 ( $\sigma = 0.89$  mho/m,  $\epsilon_r = 45.81$ ,  $\rho = 1000$  kg/m<sup>3</sup>)  
Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1507-Y2003; ConvF(8.75, 8.75, 8.75); Calibrated: 2/24/2002
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 1001; Calibrated: 9/30/2003
- Phantom: Flat Phantom 4.4; Type: Flat Phantom 4.4; Serial: TP:1002
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.8 Build 59

**d=15mm, Pin=26dBm/Area Scan (121x171x1):** Measurement grid: dx=15mm, dy=15mm

Reference Value = 37.6 V/m

Power Drift = 0.006 dB

Maximum value of SAR = 1.23 mW/g

**d=15mm, Pin=26dBm/Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 1.78 W/kg

SAR(1 g) = 1.17 mW/g; SAR(10 g) = 0.777 mW/g

Reference Value = 37.6 V/m

Power Drift = 0.006 dB

Maximum value of SAR = 1.24 mW/g

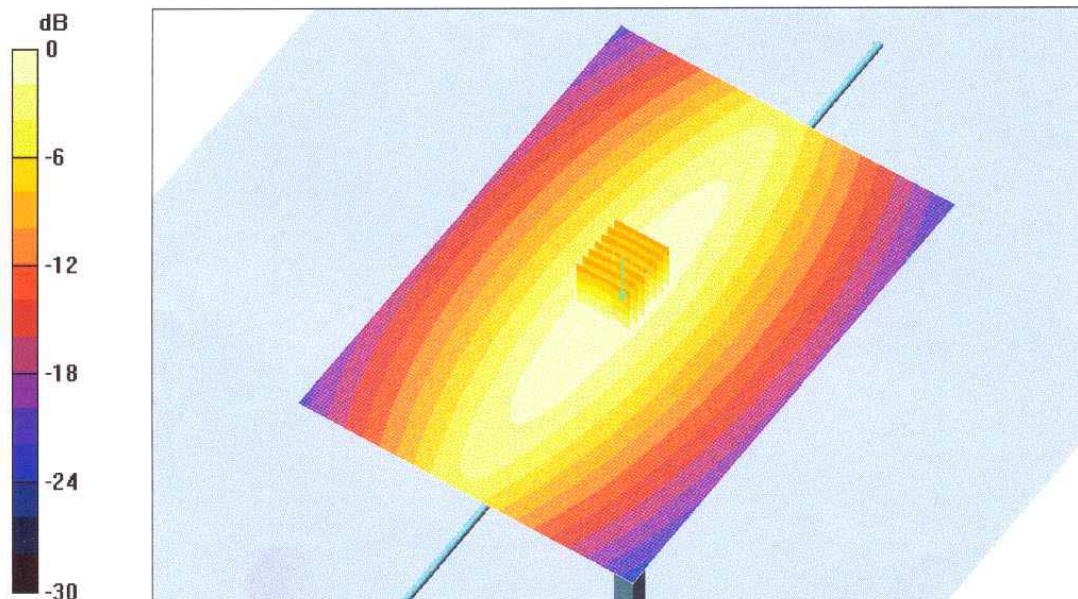

0 dB = 1.24mW/g

1005


27 Nov 2003 21:15:33

CH1 S11 1 U FS 1: 53.418  $\mu$  -9.0293  $\mu$  58.755 pF 300.000 000 MHz

Del

Cor


↑

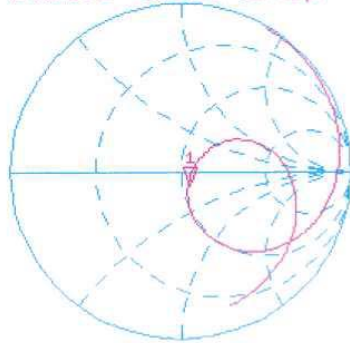

CH2 S11 LOG 2.5 dB/REF -20 dB 1: -20.629 dB 300.000 000 MHz

Cor

↑

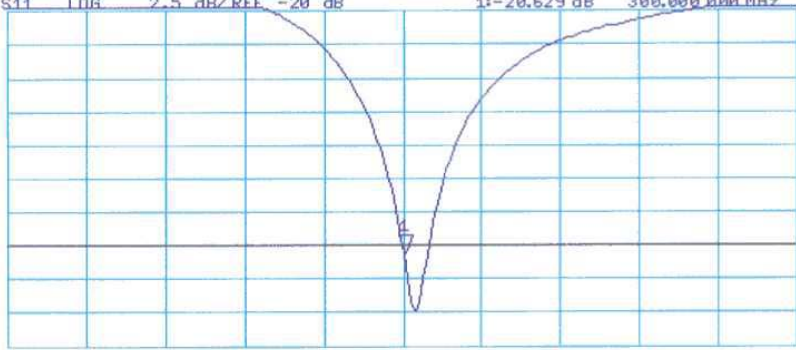

CENTER 300.000 000 MHz

SPAN 400.000 000 MHz