

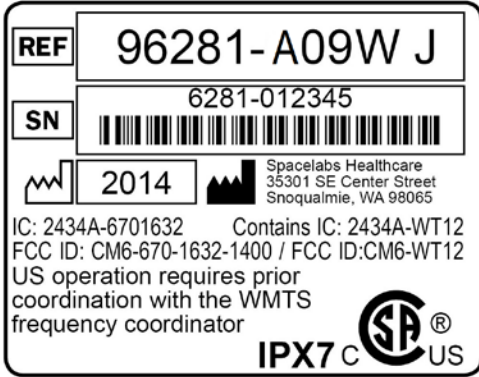



General arrangement of labels on the 96281. See next figure for the five variants in this application.


96281 Medical Telemetry Transmitter - Exhibit for review by NWEMC




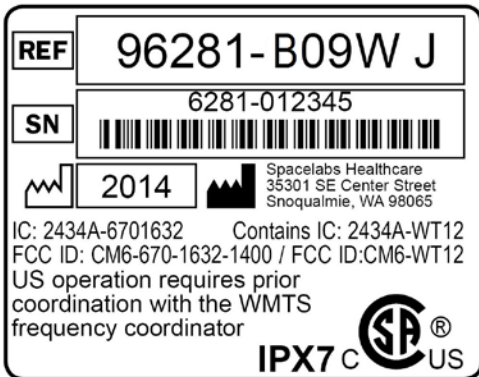
REF: 96281-A09N J
 SN: 6281-012345
 2014
 Spacelabs Healthcare
 35301 SE Center Street
 Snoqualmie, WA 98065
 IC: 2434A-6701632 Contains IC: 2434A-WT12
 FCC ID: CM6-670-1632-1400 / FCC ID:CM6-WT12
 US operation requires prior
 coordination with the WMTS
 frequency coordinator
 IPX7 C  US

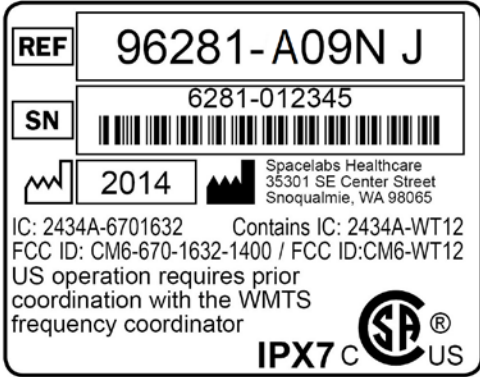


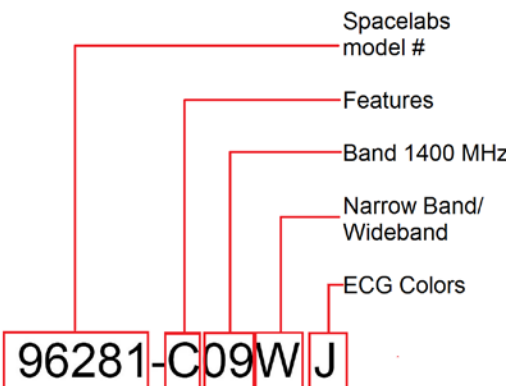
REF: 96281-A09W J
 SN: 6281-012345
 2014
 Spacelabs Healthcare
 35301 SE Center Street
 Snoqualmie, WA 98065
 IC: 2434A-6701632 Contains IC: 2434A-WT12
 FCC ID: CM6-670-1632-1400 / FCC ID:CM6-WT12
 US operation requires prior
 coordination with the WMTS
 frequency coordinator
 IPX7 C  US

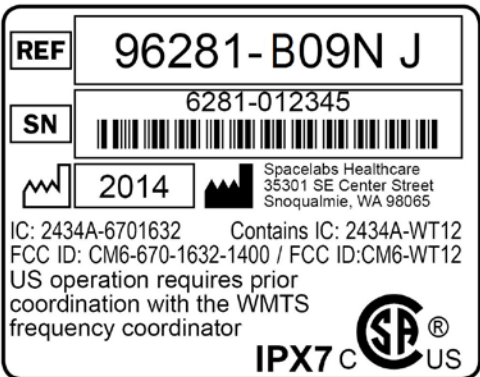

REF: 96281-B09N J
 SN: 6281-012345
 2014
 Spacelabs Healthcare
 35301 SE Center Street
 Snoqualmie, WA 98065
 IC: 2434A-6701632 Contains IC: 2434A-WT12
 FCC ID: CM6-670-1632-1400 / FCC ID:CM6-WT12
 US operation requires prior
 coordination with the WMTS
 frequency coordinator
 IPX7 C  US





REF: 96281-B09W J
 SN: 6281-012345
 2014
 Spacelabs Healthcare
 35301 SE Center Street
 Snoqualmie, WA 98065
 IC: 2434A-6701632 Contains IC: 2434A-WT12
 FCC ID: CM6-670-1632-1400 / FCC ID:CM6-WT12
 US operation requires prior
 coordination with the WMTS
 frequency coordinator
 IPX7 C  US



96281-C09W J

- Spacelabs model #
- Features
- Band 1400 MHz
- Narrow Band/
Wideband
- ECG Colors

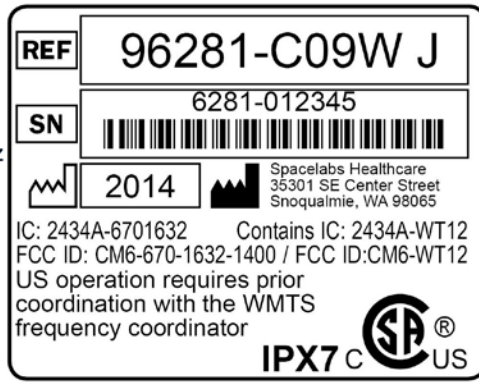

REF: 96281-C09W J
 SN: 6281-012345
 2014
 Spacelabs Healthcare
 35301 SE Center Street
 Snoqualmie, WA 98065
 IC: 2434A-6701632 Contains IC: 2434A-WT12
 FCC ID: CM6-670-1632-1400 / FCC ID:CM6-WT12
 US operation requires prior
 coordination with the WMTS
 frequency coordinator
 IPX7 C  US

Model number / technical label - showing the five model-option codes in this application.