


EXHIBIT E – Spurious Radiated Emissions Data

FCC ID CM676A90343-04

Northwest EMC, Inc., Radiated and Conducted Emissions Data Sheets						Rev 3.3 10/09/99
EUT: 90347 configuration		Serial Number: 343-001201 (602)		Job Number: SPAC0246	Date: 08/23/00	
Manufacturer: Spacelabs		Test Engineer: Jim Theabolt		Job Site: SU02		
Customer Reference Number:		Software: Application Specific		Power:		
Comments: 9VDC, patient leads shorted, R7 = 4.99K ohm.						
<i>James Theabolt</i>				Temperature (°C): 22		% Humidity: 57
Test System						
See system details						
Test Equipment						
AAI	AQB	APA	ABD	ALH	ADD	


FCC Part 15.242c (3 Meter Limit)

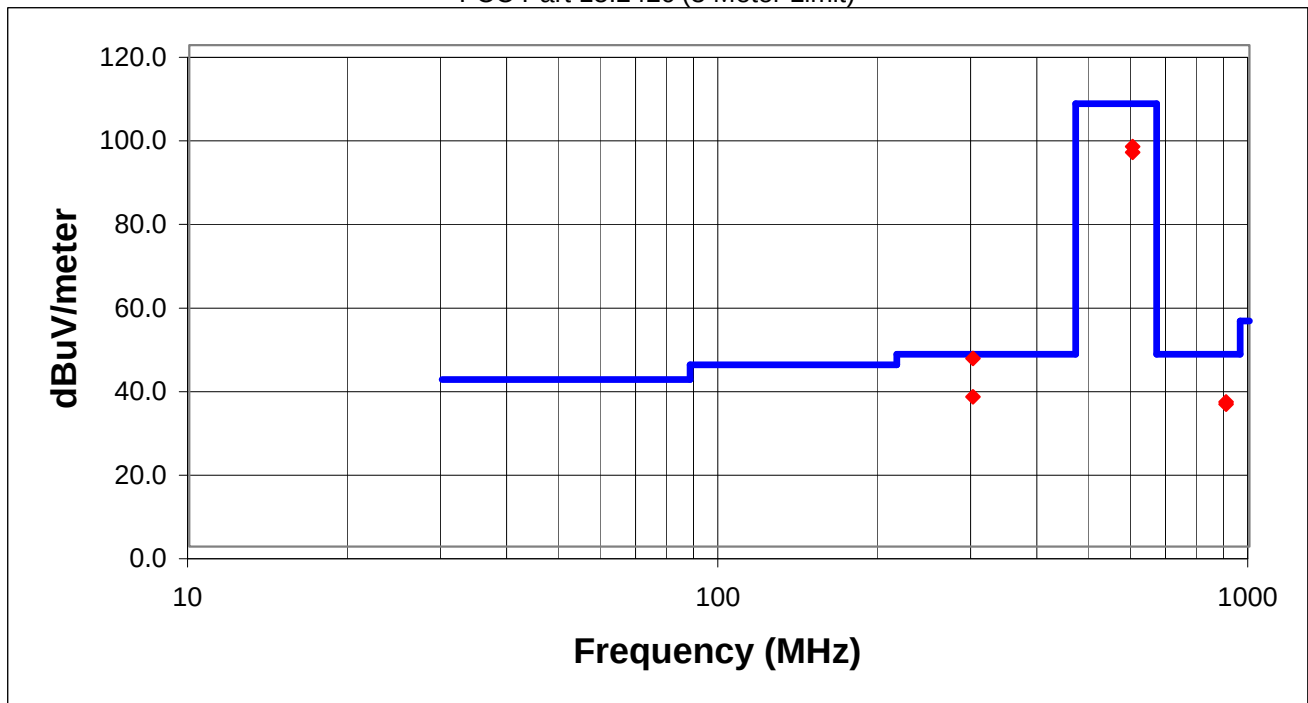


Frequency (MHz)	Meter Reading (dBuV)	Detector	Antenna Factor (dB/m)	Antenna Polarity	Preamp Gain (dB)	Cable Loss (dB)	Table Azimuth (degrees)	Antenna Height (meters)	Adjusted Level (dBuV/m)	Spec. Limit (dBuV/m)	Margin (dB)
301.020	58.2	QP	18.1	HBLG	34.8	3.5	50.0	1.3	45.0	46.0	-1.0
301.003	52.0	QP	15.1	VLPA	34.8	3.5	90.0	1.4	35.8	46.0	-10.2
602.064	106.0	QP	19.0	HLPA	34.7	5.4	60.0	1.6	95.7	106.0	-10.3
903.041	39.7	QP	22.8	HLPA	34.2	6.3	60.0	1.0	34.6	46.0	-11.4
602.038	104.6	QP	19.0	VLPA	34.7	5.4	70.0	1.7	94.3	106.0	-11.7
903.037	39.1	QP	22.8	VLPA	34.2	6.3	95.0	1.0	34.0	46.0	-12.0

Northwest EMC, Inc., Radiated and Conducted Emissions Data Sheets						Rev 3.3 10/09/99
EUT: 90343		Serial Number: 343-001239 (620)		Job Number: SPAC0246		Date: 08/23/00
Manufacturer: Spacelabs		Test Engineer: Jim Theabolt		Job Site: SU02		
Customer Reference Number:		Software: Application Specific		Power:		
Comments: 9VDC, patient leads shorted						
				Temperature (°C): 22		% Humidity: 54
Test System						
See system details						
Test Equipment						
AAI	AQB	APA	ABD	ALH	ADD	


FCC Part 15.242c (3 Meter Limit)

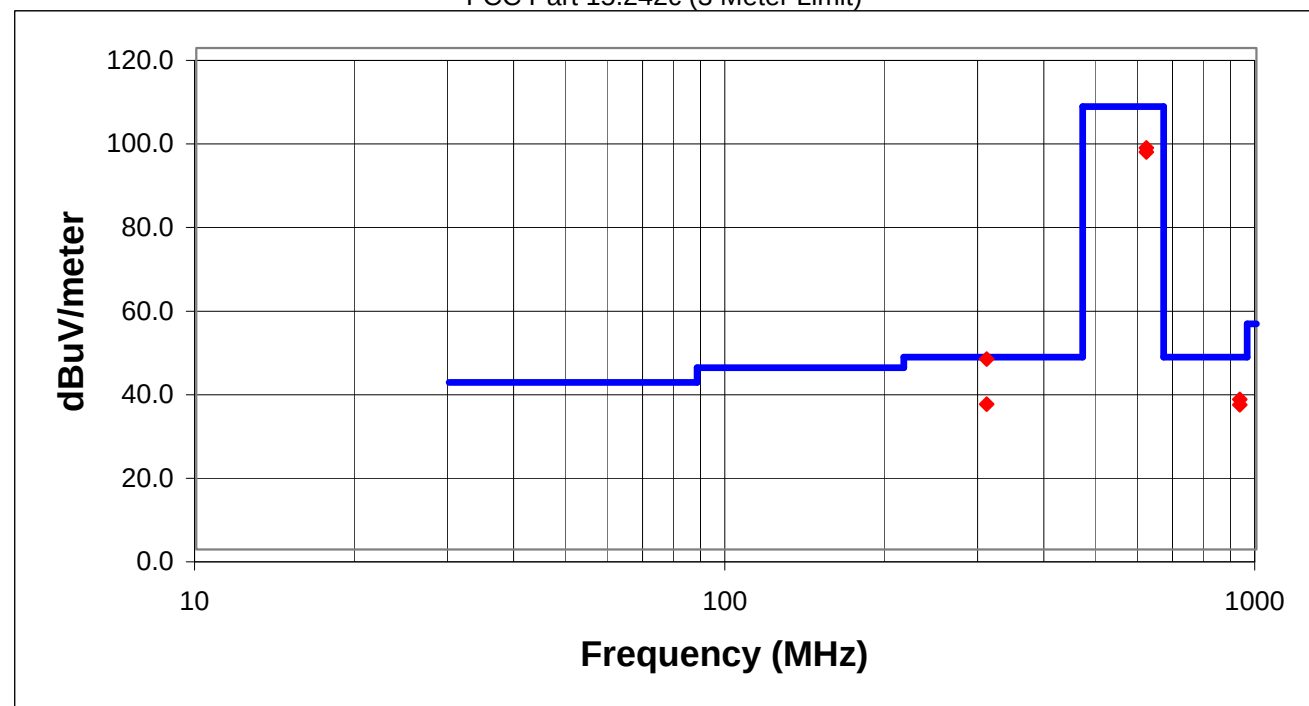

Frequency (MHz)	Meter Reading (dBuV)	Detector	Antenna Factor (dB/m)	Antenna Polarity	Preamp Gain (dB)	Cable Loss (dB)	Table Azimuth (degrees)	Antenna Height (meters)	Adjusted Level (dBuV/m)	Spec. Limit (dBuV/m)	Margin (dB)
309.975	58.4	QP	18.4	HBLG	34.8	3.6	310.0	1.1	45.6	46.0	-0.4
619.949	106.1	QP	19.2	HLPA	34.7	5.5	290.0	1.3	96.1	106.0	-9.9
929.912	40.2	PK	23.2	VLPA	34.0	6.5	275.0	1.0	35.9	46.0	-10.1
619.952	105.1	QP	19.2	VLPA	34.7	5.5	240.0	1.3	95.1	106.0	-10.9
309.959	51.1	QP	14.9	VLPA	34.8	3.6	260.0	1.2	34.8	46.0	-11.2
929.911	38.9	PK	23.2	HLPA	34.0	6.5	280.0	1.0	34.6	46.0	-11.4

Northwest EMC, Inc., Radiated and Conducted Emissions Data Sheets						Rev 3.3 10/09/99
EUT: 90347 Configuration		Serial Number: 347-001337 (611)		Job Number: SPAC0246		Date: 08/23/00
Manufacturer: Spacelabs		Test Engineer: Jim Theabolt		Job Site: SU02		
Customer Reference Number:		Software: Application Specific		Power:		
Comments: 9VDC, patient leads shorted						
				Temperature (°C): 22		% Humidity: 54
Test System						
See system details						
Test Equipment						
AAI	AQB	APA	ABD	ALH	ADD	


FCC Part 15.242c (3 Meter Limit)

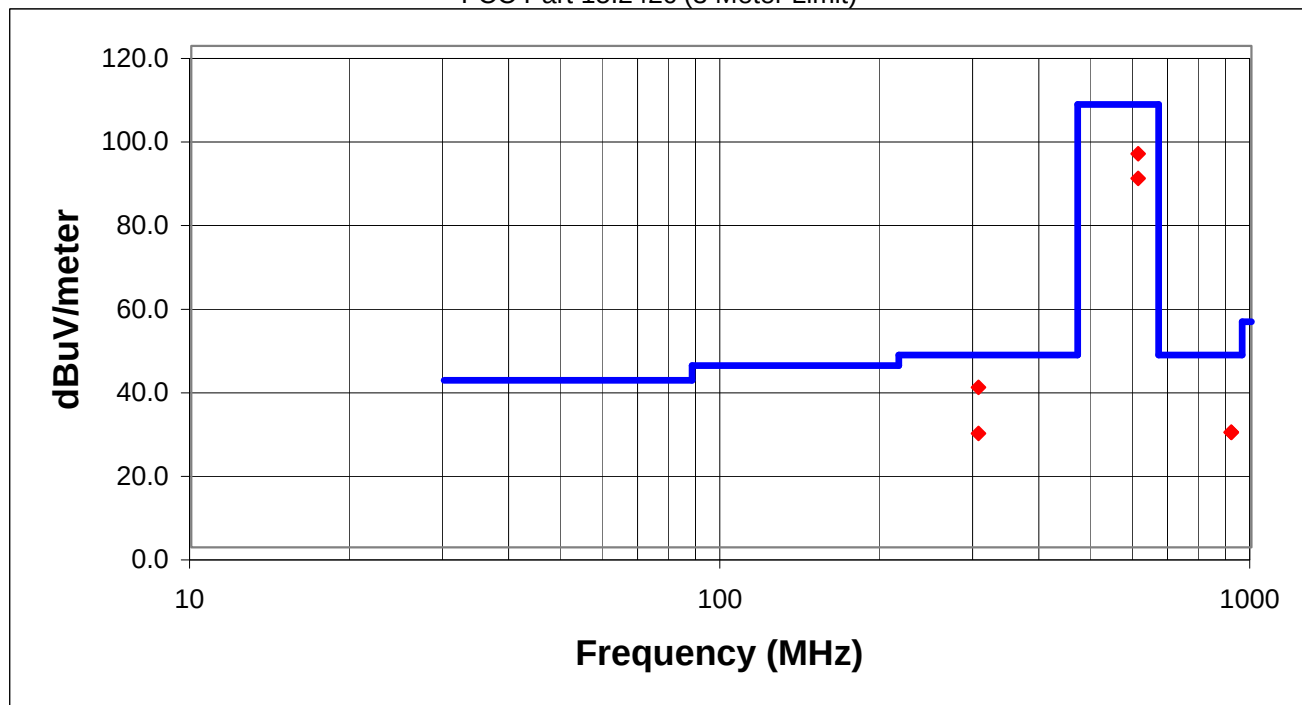

Frequency (MHz)	Meter Reading (dBuV)	Detector	Antenna Factor (dB/m)	Antenna Polarity	Preamplifier Gain (dB)	Cable Loss (dB)	Table Azimuth (degrees)	Antenna Height (meters)	Adjusted Level (dBuV/m)	Spec. Limit (dBuV/m)	Margin (dB)
305.496	54.6	QP	15.0	HLPA	34.8	3.5	220.0	1.0	38.3	46.0	-7.7
611.029	104.4	QP	19.1	HLPA	34.7	5.4	240.0	1.2	94.2	106.0	-11.8
611.030	98.5	QP	19.1	VLPA	34.7	5.4	285.0	1.1	88.3	106.0	-17.7
916.548	32.3	QP	23.0	VLPA	34.1	6.4	60.0	1.2	27.6	46.0	-18.4
916.548	32.2	QP	23.0	HLPA	34.1	6.4	30.0	1.0	27.5	46.0	-18.5
305.498	43.5	QP	15.0	VLPA	34.8	3.5	270.0	1.1	27.2	46.0	-18.8

Northwest EMC, Inc., Radiated and Conducted Emissions Data Sheets						Rev 3.3 10/09/99
EUT: 90343 Configuration		Serial Number: 343-001201 (602)		Job Number: SPAC0246	Date: 08/23/00	
Manufacturer: Spacelabs		Test Engineer: Jim Theabolt		Job Site: SU02		
Customer Reference Number:		Software: Application Specific		Power:		
Comments:	9VDC, patient leads shorted, R7 = 6.98K ohm resistor.					
<i>James Theabolt</i>				Temperature (°C): 22		% Humidity: 50
Test System						
See system details						
Test Equipment						
AAI	AQB	APA	ABD	ALH	ADD	


FCC Part 15.242c (3 Meter Limit)

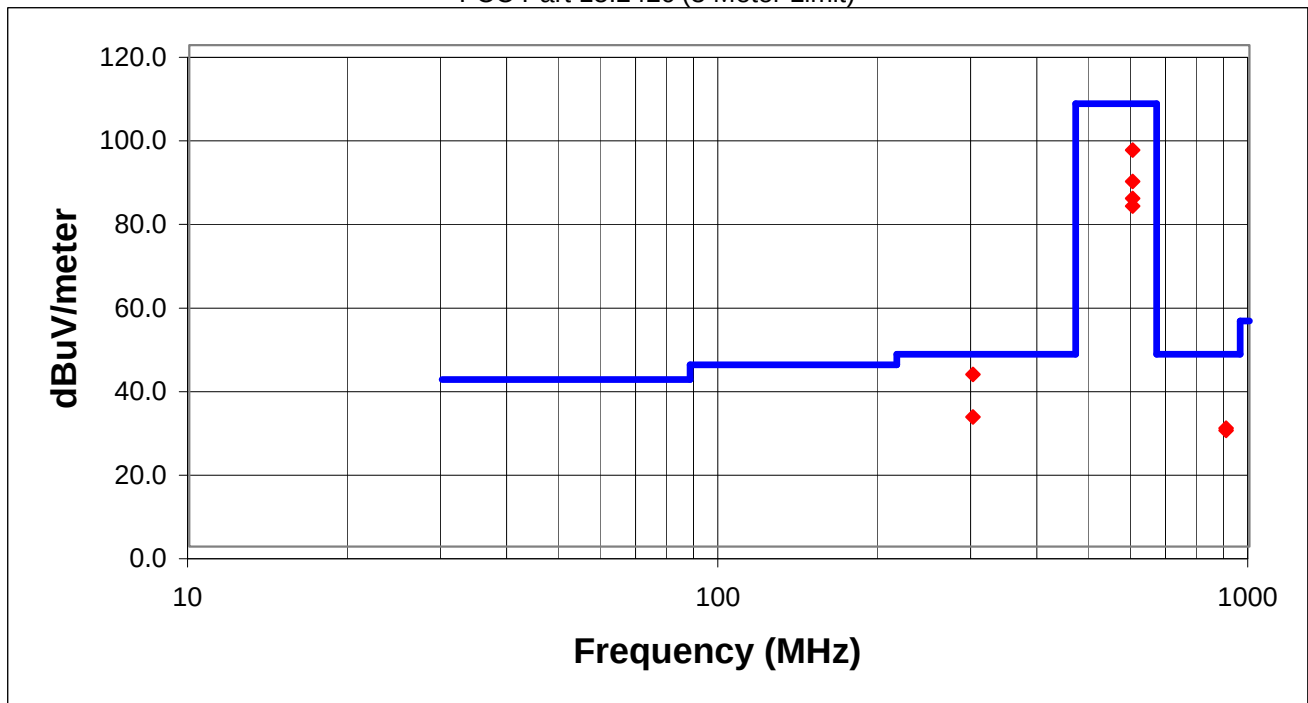

Frequency (MHz)	Meter Reading (dBuV)	Detector	Antenna Factor (dB/m)	Antenna Polarity	Preamplifier Gain (dB)	Cable Loss (dB)	Table Azimuth (degrees)	Antenna Height (meters)	Adjusted Level (dBuV/m)	Spec. Limit (dBuV/m)	Margin (dB)
300.999	57.4	QP	15.1	HLPA	34.8	3.5	35.0	1.1	41.2	46.0	-4.8
602.040	105.2	QP	19.0	HLPA	34.7	5.4	65.0	1.2	94.9	106.0	-11.1
301.008	47.2	QP	15.1	VLPA	34.8	3.5	75.0	1.2	31.0	46.0	-15.0
903.054	33.5	QP	22.8	VLPA	34.2	6.3	95.0	1.3	28.4	46.0	-17.6
903.054	32.9	QP	22.8	HLPA	34.2	6.3	175.0	1.1	27.8	46.0	-18.2
602.074	97.6	QP	19.0	VLPA	34.7	5.4	90.0	1.3	87.3	106.0	-18.7
602.038	93.6	QP	19.0	HLPA	34.7	5.4	250.0	1.1	83.3	106.0	-22.7
602.038	91.8	QP	19.0	VLPA	34.7	5.4	240.0	1.3	81.5	106.0	-24.5

Northwest EMC, Inc., Radiated and Conducted Emissions Data Sheets						Rev 3.3 10/09/99
EUT: 90343 Configuration		Serial Number: 347-001337 (611)		Job Number: SPAC0246	Date: 08/23/00	
Manufacturer: Spacelabs		Test Engineer: Jim Theabolt		Job Site: SU02		
Customer Reference Number:		Software: Application Specific		Power:		
Comments:	9VDC, patient leads shorted					
<i>James Theabolt</i>				Temperature (°C): 22	% Humidity: 50	
Test System						
See system details						
Test Equipment						
AAI	AQB	APA	ABD	ALH	ADD	


FCC Part 15.242c (3 Meter Limit)

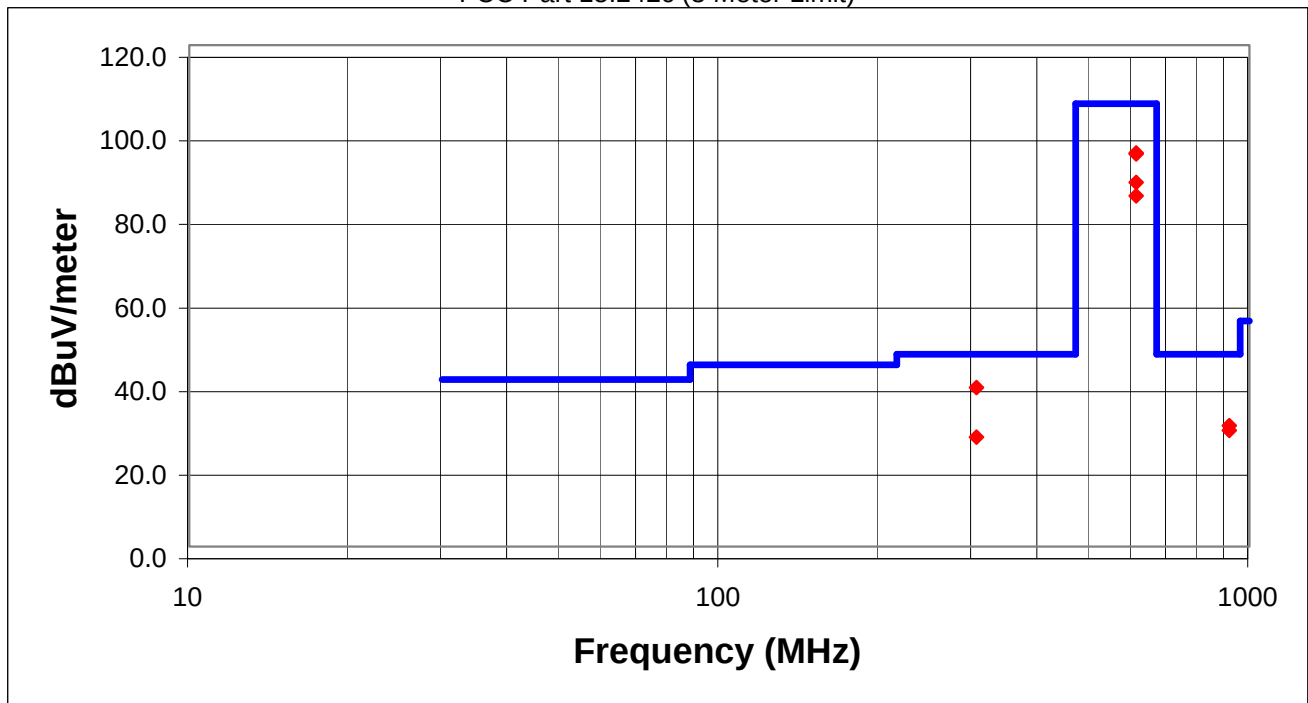

Frequency (MHz)	Meter Reading (dBuV)	Detector	Antenna Factor (dB/m)	Antenna Polarity	Preamplifier Gain (dB)	Cable Loss (dB)	Table Azimuth (degrees)	Antenna Height (meters)	Adjusted Level (dBuV/m)	Spec. Limit (dBuV/m)	Margin (dB)
305.501	54.3	QP	15.0	HLP	34.8	3.5	35.0	1.1	38.0	46.0	-8.0
611.035	104.4	QP	19.1	HLP	34.7	5.4	60.0	1.1	94.2	106.0	-11.8
611.035	104.1	QP	19.1	VLPA	34.7	5.4	270.0	1.0	93.9	106.0	-12.1
916.540	33.6	QP	23.0	VLPA	34.1	6.4	240.0	1.4	28.9	46.0	-17.1
916.540	32.5	QP	23.0	HLP	34.1	6.4	240.0	1.0	27.8	46.0	-18.2
611.070	97.3	QP	19.1	HLP	34.7	5.4	215.0	1.3	87.1	106.0	-18.9
305.517	42.5	QP	15.0	VLPA	34.8	3.5	215.0	1.2	26.2	46.0	-19.8
611.016	94.1	QP	19.1	VLPA	34.7	5.4	265.0	1.2	83.9	106.0	-22.1

Northwest EMC, Inc., Radiated and Conducted Emissions Data Sheets						Rev 3.3 10/09/99
EUT: 90347 Configuration		Serial Number: 343-001239 (620)		Job Number: SPAC0246	Date: 08/23/00	
Manufacturer: Spacelabs		Test Engineer: Jim Theabolt		Job Site: SU02		
Customer Reference Number:		Software: Application Specific		Power:		
Comments:	9VDC, patient leads shorted, R7 = 4.99K ohm resistor.					
<i>James Theabolt</i>				Temperature (°C): 22		% Humidity: 50
Test System						
See system details						
Test Equipment						
AAI	AQB	APA	ABD	ALH	ADD	


FCC Part 15.242c (3 Meter Limit)

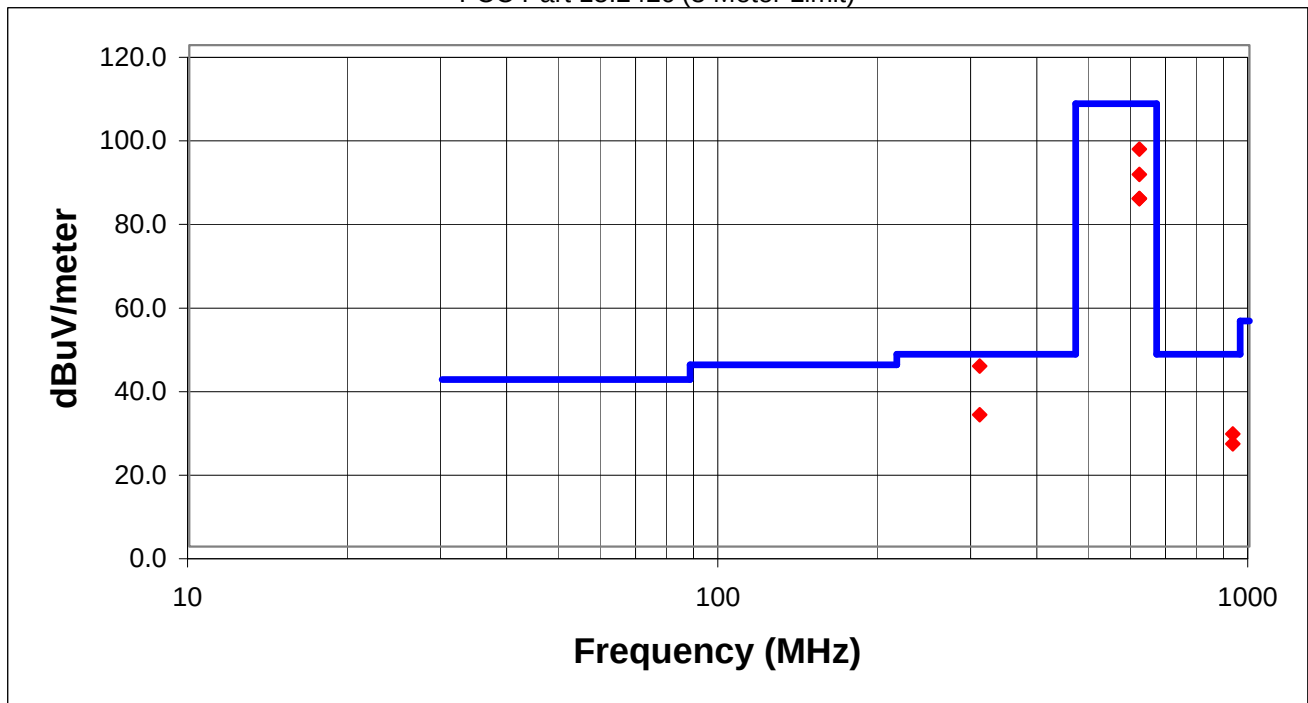

Frequency (MHz)	Meter Reading (dBuV)	Detector	Antenna Factor (dB/m)	Antenna Polarity	Preamplifier Gain (dB)	Cable Loss (dB)	Table Azimuth (degrees)	Antenna Height (meters)	Adjusted Level (dBuV/m)	Spec. Limit (dBuV/m)	Margin (dB)
309.975	59.5	QP	14.9	HLPA	34.8	3.6	320.0	1.0	43.2	46.0	-2.8
619.950	105.1	QP	19.2	HLPA	34.7	5.5	300.0	1.3	95.1	106.0	-10.9
309.958	47.8	QP	14.9	VLPA	34.8	3.6	245.0	1.2	31.5	46.0	-14.5
619.951	99.1	QP	19.2	VLPA	34.7	5.5	240.0	1.0	89.1	106.0	-16.9
929.913	31.3	PK	23.2	HLPA	34.0	6.5	60.0	1.0	27.0	46.0	-19.0
929.912	28.9	PK	23.2	VLPA	34.0	6.5	110.0	1.0	24.6	46.0	-21.4
619.923	93.4	QP	19.2	VLPA	34.7	5.5	285.0	1.2	83.4	106.0	-22.7
619.951	93.3	QP	19.2	HLPA	34.7	5.5	150.0	1.6	83.3	106.0	-22.7

Northwest EMC, Inc., Radiated and Conducted Emissions Data Sheets				Rev 3.3 10/09/99
EUT: 90343 Configuration		Serial Number: 343-001239 (620)	Job Number: SPAC0246	Date: 08/23/00
Manufacturer: Spacelabs		Test Engineer: Jim Theabolt	Job Site: SU01	
Customer Reference Number:		Software: Application Specific	Power:	
Comments:	9VDC, patient leads shorted			
			Temperature (°C): 21	% Humidity: 50
Test System				
See system details				
Test Equipment				
AAN	APL	AHF		


FCC Class B Radiated Specification Limit (3 meter)

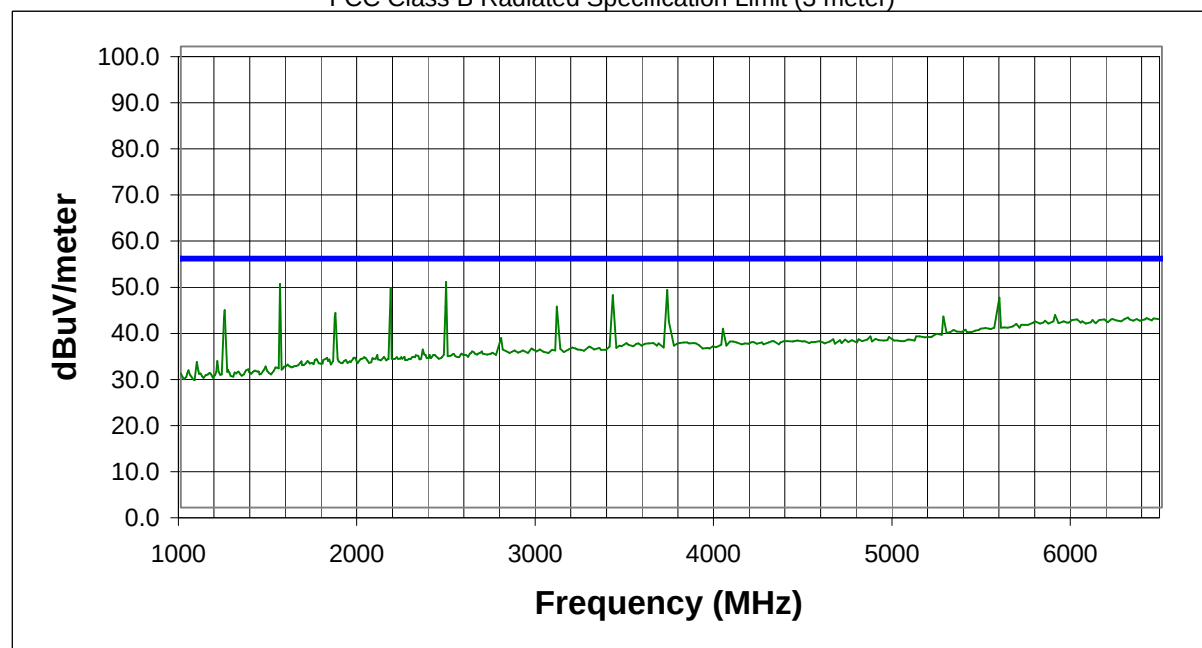

Frequency (MHz)	Meter Reading (dBuV)	Antenna Polarity	Correction Factor (dB/m)	Adjusted Level (dBuV/meter)	Specification Limit (dBuV/meter)	Margin (dB)
2487.500	58.6	Hor.	-9.7	48.9	54.0	-5.1
1556.750	61.3	Ver.	-12.8	48.5	54.0	-5.5
2177.250	58.0	Ver.	-10.4	47.6	54.0	-6.4
3726.000	53.4	Ver.	-6.2	47.2	54.0	-6.8
3422.000	53.0	Hor.	-6.9	46.1	54.0	-7.9
5588.000	46.9	Ver.	-1.4	45.5	54.0	-8.5
3108.500	51.2	Hor.	-7.6	43.6	54.0	-10.4
1246.500	57.5	Hor.	-14.7	42.8	54.0	-11.2
1867.000	53.2	Ver.	-11.0	42.2	54.0	-11.8
5901.500	42.2	Ver.	-0.4	41.8	54.0	-12.2
5274.500	44.1	Ver.	-2.7	41.4	54.0	-12.6
6310.000	41.0	Hor.	0.2	41.2	54.0	-12.8
6414.500	40.9	Ver.	0.2	41.1	54.0	-12.9
6452.500	40.8	Hor.	0.2	41.0	54.0	-13.0
6291.000	40.7	Hor.	0.2	40.9	54.0	-13.1
6357.500	40.7	Hor.	0.2	40.9	54.0	-13.1
6224.500	40.8	Ver.	0.1	40.9	54.0	-13.1
6481.000	40.6	Ver.	0.3	40.9	54.0	-13.1
6025.000	40.8	Ver.	0.0	40.8	54.0	-13.2
6177.000	40.8	Hor.	0.0	40.8	54.0	-13.2

Northwest EMC, Inc., Radiated and Conducted Emissions Data Sheets				Rev 3.3 10/09/99
EUT: 90347 Configuration		Serial Number: 343-001201 (602)	Job Number: SPAC0246	Date: 08/23/00
Manufacturer: Spacelabs		Test Engineer: Jim Theabolt	Job Site: SU01	
Customer Reference Number:		Software: Application Specific	Power:	
Comments:	9VDC, patient leads shorted, R7 = 4.99K ohm resistor.			
			Temperature (°C): 21	% Humidity: 50
Test System				
See system details				
Test Equipment				
AAN	APL	AHF		


FCC Class B Radiated Specification Limit (3 meter)

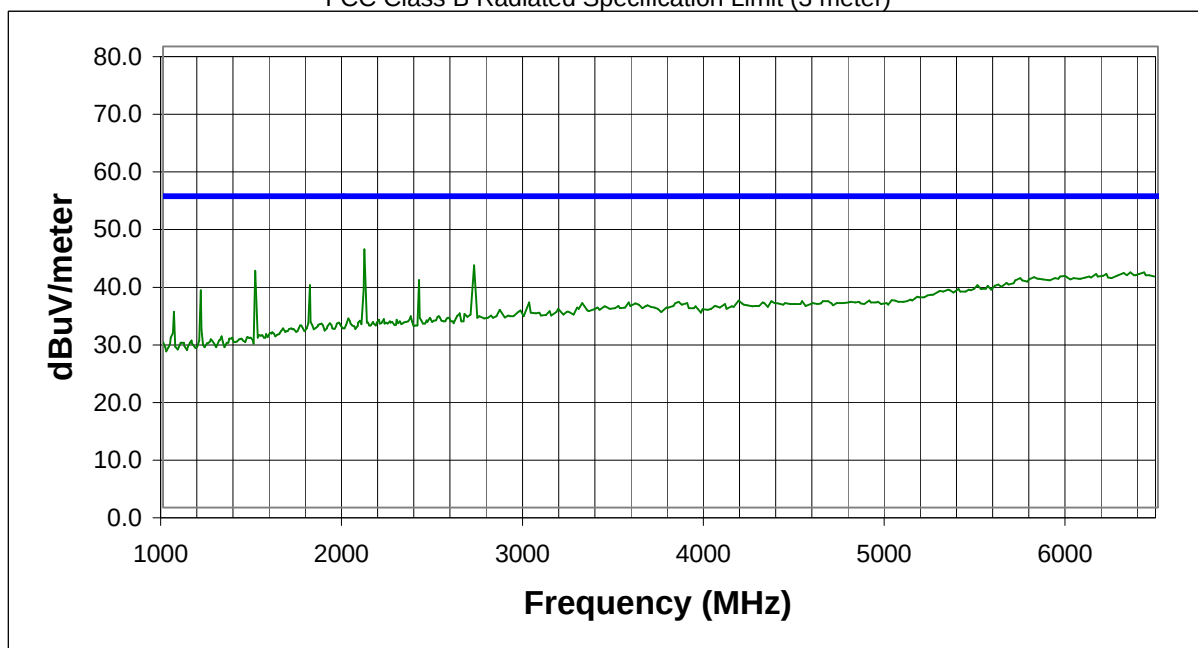

Frequency (MHz)	Meter Reading (dBuV)	Antenna Polarity	Correction Factor (dB/m)	Adjusted Level (dBuV/meter)	Specification Limit (dBuV/meter)	Margin (dB)
2113.500	55.2	Ver.	-10.4	44.8	54.0	-9.2
2719.000	50.8	Ver.	-8.8	42.0	54.0	-12.0
1510.000	54.3	Ver.	-13.2	41.1	54.0	-12.9
6424.000	40.6	Ver.	0.2	40.8	54.0	-13.2
6348.000	40.6	Hor.	0.2	40.8	54.0	-13.2
6395.500	40.3	Ver.	0.2	40.5	54.0	-13.5
6158.000	40.5	Hor.	0.0	40.5	54.0	-13.5
6215.000	40.4	Ver.	0.1	40.5	54.0	-13.5
6452.500	40.1	Ver.	0.2	40.3	54.0	-13.7
6281.500	40.2	Hor.	0.1	40.3	54.0	-13.7
5987.000	40.2	Hor.	0.0	40.2	54.0	-13.8
6196.000	40.1	Hor.	0.1	40.2	54.0	-13.8
5958.500	40.3	Ver.	-0.2	40.1	54.0	-13.9
6490.500	39.8	Ver.	0.3	40.1	54.0	-13.9
5816.000	40.6	Hor.	-0.6	40.0	54.0	-14.0
6034.500	39.8	Ver.	0.0	39.8	54.0	-14.2
5740.000	40.7	Hor.	-0.9	39.8	54.0	-14.2
5835.000	40.3	Hor.	-0.6	39.7	54.0	-14.3
5892.000	39.9	Ver.	-0.4	39.5	54.0	-14.5
2415.250	49.4	Ver.	-9.9	39.5	54.0	-14.5

Northwest EMC, Inc., Radiated and Conducted Emissions Data Sheets				Rev 3.3 10/09/99
EUT: 90343 Configuration		Serial Number: 347-001337 (611)	Job Number: SPAC0246	Date: 08/23/00
Manufacturer: Spacelabs		Test Engineer: Jim Theabolt	Job Site: SU01	
Customer Reference Number:		Software: Application Specific	Power:	
Comments:	9VDC, patient leads shorted			
			Temperature (°C): 21	% Humidity: 50
Test System				
See system details				
Test Equipment				
AAN	APL	AHF		


FCC Class B Radiated Specification Limit (3 meter)

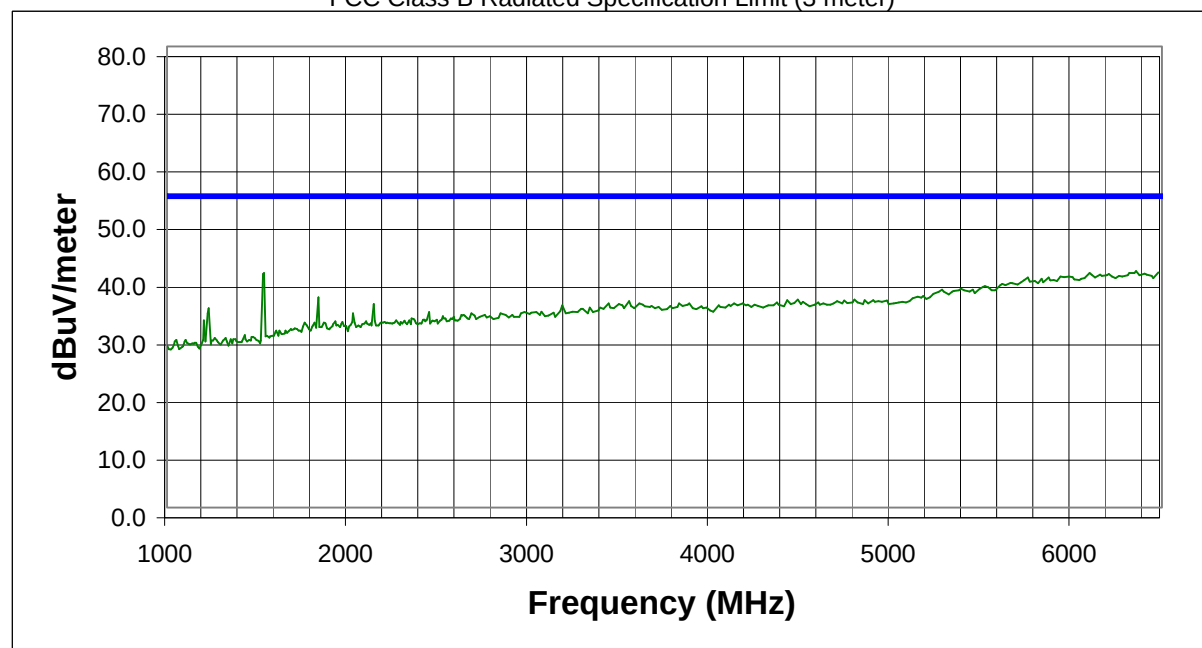

Frequency (MHz)	Meter Reading (dBuV)	Antenna Polarity	Correction Factor (dB/m)	Adjusted Level (dBuV/meter)	Specification Limit (dBuV/meter)	Margin (dB)
6357.500	40.8	Hor.	0.2	41.0	54.0	-13.0
6481.000	40.5	Hor.	0.3	40.8	54.0	-13.2
6319.500	40.5	Hor.	0.2	40.7	54.0	-13.3
1535.500	53.7	Ver.	-13.0	40.7	54.0	-13.3
6101.000	40.6	Ver.	0.1	40.7	54.0	-13.3
6405.000	40.4	Ver.	0.2	40.6	54.0	-13.4
6205.500	40.4	Hor.	0.1	40.5	54.0	-13.5
6158.000	40.4	Hor.	0.0	40.4	54.0	-13.6
5939.500	40.4	Hor.	-0.3	40.1	54.0	-13.9
5987.000	40.1	Hor.	0.0	40.1	54.0	-13.9
5873.000	40.3	Hor.	-0.4	39.9	54.0	-14.1
5759.000	40.7	Ver.	-0.8	39.9	54.0	-14.1
6053.500	39.7	Hor.	0.0	39.7	54.0	-14.3
5901.500	39.9	Ver.	-0.4	39.5	54.0	-14.5
5721.000	40.1	Hor.	-1.0	39.1	54.0	-14.9
5664.000	40.1	Ver.	-1.1	39.0	54.0	-15.0
5616.500	40.1	Hor.	-1.3	38.8	54.0	-15.2
5521.500	40.0	Ver.	-1.6	38.4	54.0	-15.6
5550.000	39.7	Ver.	-1.5	38.2	54.0	-15.8
5388.500	40.3	Ver.	-2.3	38.0	54.0	-16.0

Northwest EMC, Inc., Radiated and Conducted Emissions Data Sheets				Rev 3.3 10/09/99
EUT: 90347 Configuration		Serial Number: 347-001239 (620)	Job Number: SPAC0246	Date: 08/23/00
Manufacturer: Spacelabs		Test Engineer: Jim Theabolt	Job Site: SU01	
Customer Reference Number:		Software: Application Specific	Power:	
Comments:	9VDC, patient leads shorted			
			Temperature (°C): 21	% Humidity: 50
Test System				
See system details				
Test Equipment				
AAN	APL	AHF		


FCC Class B Radiated Specification Limit (3 meter)

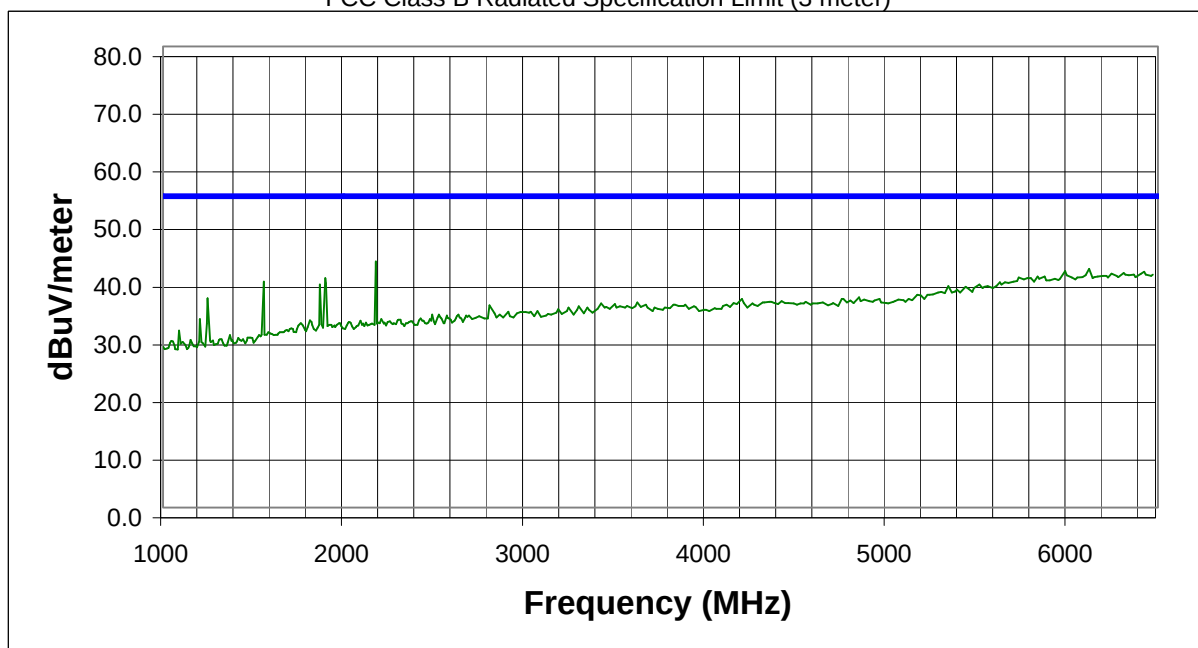

Frequency (MHz)	Meter Reading (dBuV)	Antenna Polarity	Correction Factor (dB/m)	Adjusted Level (dBuV/meter)	Specification Limit (dBuV/meter)	Margin (dB)
2177.250	53.1	Ver.	-10.4	42.7	54.0	-11.3
6120.000	41.3	Ver.	0.1	41.4	54.0	-12.6
5987.000	41.0	Hor.	0.0	41.0	54.0	-13.0
6424.000	40.7	Hor.	0.2	40.9	54.0	-13.1
6310.000	40.5	Hor.	0.2	40.7	54.0	-13.3
6243.500	40.5	Hor.	0.1	40.6	54.0	-13.4
6367.000	40.2	Ver.	0.2	40.4	54.0	-13.6
6471.500	40.2	Ver.	0.2	40.4	54.0	-13.6
6101.000	40.2	Ver.	0.1	40.3	54.0	-13.7
6272.000	40.1	Ver.	0.1	40.2	54.0	-13.8
6196.000	40.1	Hor.	0.1	40.2	54.0	-13.8
5835.000	40.7	Ver.	-0.6	40.1	54.0	-13.9
6490.500	39.7	Ver.	0.3	40.0	54.0	-14.0
6025.000	39.9	Ver.	0.0	39.9	54.0	-14.1
5730.500	40.9	Ver.	-1.0	39.9	54.0	-14.1
1896.750	50.8	Ver.	-11.0	39.8	54.0	-14.2
5778.000	40.6	Hor.	-0.8	39.8	54.0	-14.2
5930.000	40.0	Hor.	-0.3	39.7	54.0	-14.3
1556.750	52.0	Ver.	-12.8	39.2	54.0	-14.8
5654.500	40.2	Ver.	-1.1	39.1	54.0	-14.9

Northwest EMC, Inc., Radiated and Conducted Emissions Data Sheets				Rev 3.3 10/09/99
EUT: 90343 Configuration		Serial Number: 343-001201 (602)	Job Number: SPAC0246	Date: 08/23/00
Manufacturer: Spacelabs		Test Engineer: Jim Theabolt	Job Site: SU01	
Customer Reference Number:		Software: Application Specific	Power:	
Comments:	9VDC, Patient leads shorted, R7 = 6.98K ohm resistor.			
			Temperature (°C): 21	% Humidity: 50
Test System				
See system details				
Test Equipment				
AAN	APL	AHF		

FCC Class B Radiated Specification Limit (3 meter)

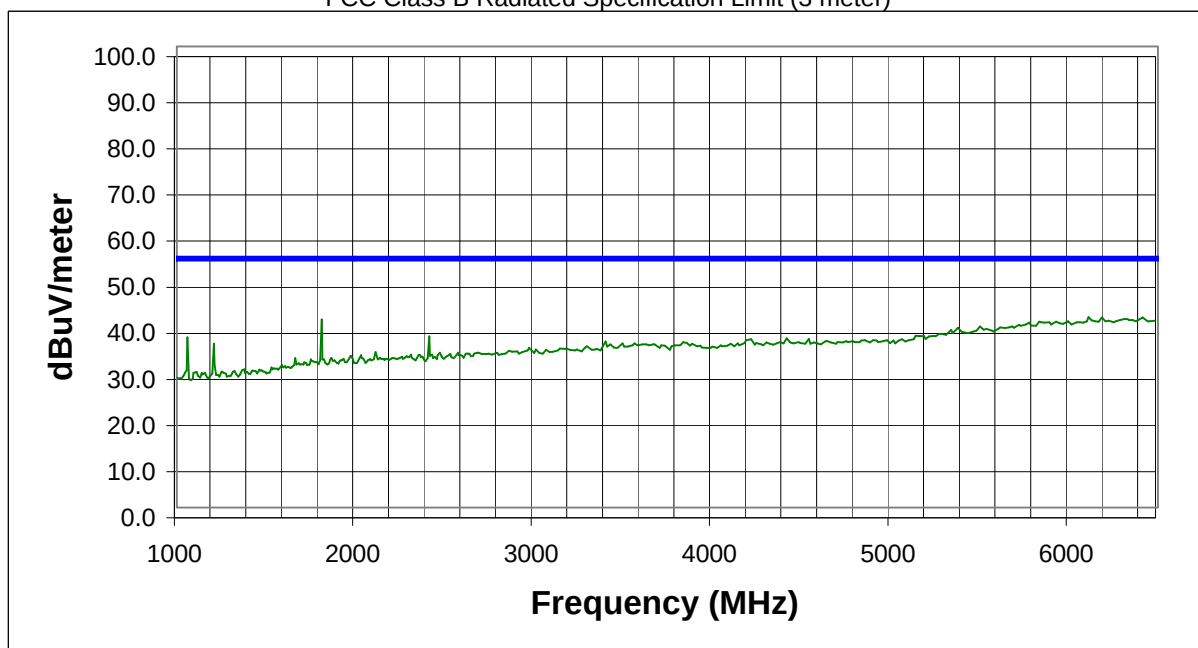

Frequency (MHz)	Meter Reading (dBuV)	Antenna Polarity	Correction Factor (dB/m)	Adjusted Level (dBuV/meter)	Specification Limit (dBuV/meter)	Margin (dB)
6110.500	41.2	Hor.	0.1	41.3	54.0	-12.7
6414.500	41.0	Ver.	0.2	41.2	54.0	-12.8
6186.500	41.1	Hor.	0.1	41.2	54.0	-12.8
6490.500	40.9	Ver.	0.3	41.2	54.0	-12.8
6310.000	40.7	Ver.	0.2	40.9	54.0	-13.1
1811.750	52.0	Ver.	-11.2	40.8	54.0	-13.2
6395.500	40.6	Ver.	0.2	40.8	54.0	-13.2
6281.500	40.5	Ver.	0.1	40.6	54.0	-13.4
6129.500	40.6	Hor.	0.0	40.6	54.0	-13.4
6224.500	40.4	Hor.	0.1	40.5	54.0	-13.5
5996.500	40.4	Ver.	0.0	40.4	54.0	-13.6
5835.000	40.9	Hor.	-0.6	40.3	54.0	-13.7
5930.000	40.6	Hor.	-0.3	40.3	54.0	-13.7
6044.000	40.2	Hor.	0.0	40.2	54.0	-13.8
5892.000	40.6	Hor.	-0.4	40.2	54.0	-13.8
5778.000	40.9	Hor.	-0.8	40.1	54.0	-13.9
5721.000	40.6	Hor.	-1.0	39.6	54.0	-14.4
5683.000	40.3	Hor.	-1.0	39.3	54.0	-14.7
5502.500	41.0	Hor.	-1.7	39.3	54.0	-14.7
5616.500	40.4	Hor.	-1.3	39.1	54.0	-14.9

Northwest EMC, Inc.

Version 98.9, feb. 2000

Equipment Tested: 90347 Configuration

Serial Number: 347-001337 (611)

Manufacturer: Spacelabs


Job Number: SPAC0246

Date/Time: 08-23-2000 13:05:15 Run #1

Tested By: Jim Theabolt, SU01

Test Distance: 3 meters

9VDC, patient leads shorted, C45 = 1pf, R76 & R77 = 0 ohm resistor, R78 = 120 ohm fb, R70 & L9 = 300 ohm fb.

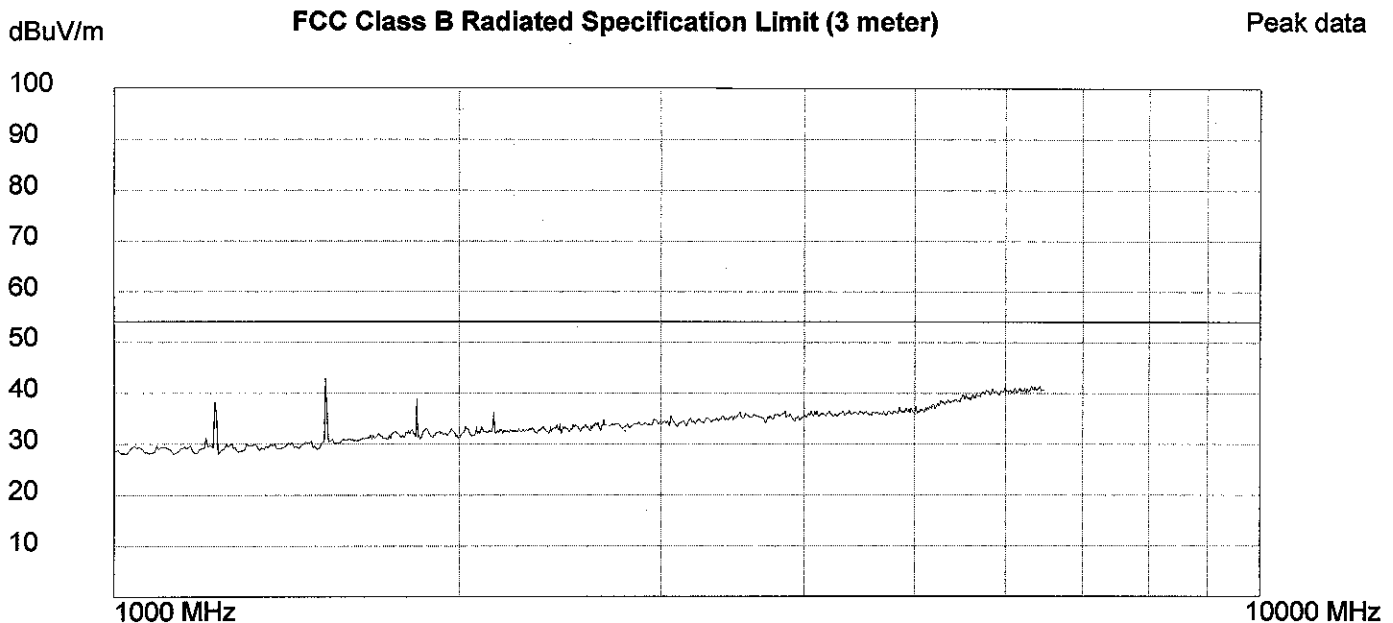

Frequency (MHz)	Meter Reading (dBuV)	Antenna Factor (dB/m)	Antenna Horizontal Vertical	Preamp Gain (dB)	Cable Loss (dB)	Chamber Correction (dB)	Adjusted Level (dBuV/m)	Spec Limit (dBuV/m)	Compared To Limit (dB)
1531.250	56.0	26.9	Ver.	41.0	1.1	0.0	43.0	54.0	-11.0
6424.000	41.3	35.8	Ver.	39.8	4.2	0.0	41.5	54.0	-12.5
6319.500	41.3	35.9	Ver.	39.8	4.1	0.0	41.5	54.0	-12.5
6357.500	41.2	35.9	Hor.	39.8	4.1	0.0	41.4	54.0	-12.6
6177.000	41.2	35.9	Ver.	39.9	4.0	0.0	41.2	54.0	-12.8
5987.000	41.0	36.0	Hor.	40.0	4.0	0.0	41.0	54.0	-13.0
6234.000	40.9	35.9	Hor.	39.9	4.1	0.0	41.0	54.0	-13.0
6262.500	40.9	35.9	Hor.	39.9	4.1	0.0	41.0	54.0	-13.0
6110.500	40.9	36.0	Ver.	39.9	4.0	0.0	41.0	54.0	-13.0
5844.500	41.6	35.8	Ver.	40.3	3.9	0.0	41.0	54.0	-13.0
6452.500	40.6	35.8	Hor.	39.8	4.2	0.0	40.8	54.0	-13.2
5768.500	41.5	35.8	Ver.	40.4	3.8	0.0	40.7	54.0	-13.3
5949.000	40.8	36.0	Ver.	40.1	3.9	0.0	40.6	54.0	-13.4
6481.000	40.3	35.8	Ver.	39.7	4.2	0.0	40.6	54.0	-13.4
6025.000	40.6	36.0	Ver.	40.0	4.0	0.0	40.6	54.0	-13.4
5882.500	40.9	35.9	Hor.	40.2	3.9	0.0	40.5	54.0	-13.5
5797.000	41.0	35.8	Hor.	40.3	3.9	0.0	40.4	54.0	-13.6
5730.500	41.3	35.7	Ver.	40.5	3.8	0.0	40.3	54.0	-13.7
5654.500	40.9	35.7	Hor.	40.6	3.8	0.0	39.8	54.0	-14.2
5540.500	41.4	35.5	Hor.	40.8	3.7	0.0	39.8	54.0	-14.2

Jim Theabolt