

Appendix C

Phantom Description

Schmid & Partner Engineering AG

е a g s р

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 info@speag.com, http://www.speag.com

Certificate of Conformity / First Article Inspection

Item	Oval Flat Phantom ELI 5.0
Type No	QD OVA 002 A
Series No	1108 and higher
Manufacturer	Untersee Composites
	Knebelstrasse 8, CH-8268 Mannenbach, Switzerland

Tests

Complete tests were made on the prototype units QD OVA 001 A, pre-series units QD OVA 001 B as well as on some series units QD OVA 001 B. Some tests are made on all series units QD OVA 002 A.

Test	Requirement	Details	Units tested
Shape	Internal dimensions, depth and sagging are compatible with standards	Bottom elliptical 600 x 400 mm, Depth 190 mm, dimension compliant with [1] for f > 375 MHz	Prototypes
Material thickness	Bottom: 2.0mm +/- 0.2mm	dimension compliant with [3] for f > 800 MHz	all
Material parameters	rel. permittivity 2 – 5, loss tangent ≤ 0.05, at f ≤ 6 GHz	rel. permittivity 3.5 +/- 0.5 loss tangent ≤ 0.05	Material samples
Material resistivity	Compatibility with tissue simulating liquids .	Compatible with SPEAG liquids. **	Phantoms, Material sample
Sagging	Sagging of the flat section in tolerance when filled with tissue simulating liquid.	within tolerance for filling height up to 155 mm	Prototypes, samples

Note: Compatibility restrictions apply certain liquid components mentioned in the standard.

containing e.g. DGBE, DGMHE or Triton X-100. Observe technical note on material compatibility

Standards

OET Bulletin 65, Supplement C, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields", Edition 01-01
 IEEE 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific

- Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques, December 2003
- [3] IEC 62209-1 ed1.0, "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures - Part 1: Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close
- proximity to the ear (frequency range of 300 MHz to 3 GHz)", 2005-02-18 [4] IEC 62209-2 ed1.0, "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures - Part 2: Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", 2010-03-30

Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of body-worn SAR measurements and system performance checks as specified in [1 - 4] and further standards.

Date 25.7.2011

Signature / Stamp

speag Schmid & Partner-Engineering/AG Zeugbarestrasse 43, 8004 Zeich, Smithiand Phone/441 44/255 9708, Few-444 64 44 59779

Doc No 881 - QD OVA 002 A - A

1 (1) Page

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號



System Validation from Original Equipment Supplier

Engineering AG eughausstrasse 43, 8004 Zuric	h, Switzerland		Servizio svizzero di taratura
Accredited by the Swiss Accredita The Swiss Accreditation Service Multilateral Agreement for the re	is one of the signatori	es to the EA n certificates	Accreditation No.: SCS 0108
Client SGS		Certificate No.	D2450V2-727_Apr23
Taoyuan City, Taiwar	1	ostitute rio.	D2450V2-727_Apr23
CALIBRATION C	ERTIFICAT	E	
Object	D2450V2 - SN:7	27	
	SENGULE ONLY		
Calibration procedure(s)	QA CAL-05.v12		
- and an proceeding(b)		edure for SAR Validation Sources	hetwoon 0.7.3 CHz
		addre for onit validation Sources	between 0.7-3 GHZ
Calibration date:	April 25, 2023		
	April 20, 2020		
The measurements and the uncert	taintles with confidence p	robability are given on the following pages an	d are part of the certificate.
I ne measurements and the uncert	taintles with confidence p red in the closed laborato	robability are given on the following pages an ry facility: environment temperature (22 \pm 3)°C	d are part of the certificate.
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TI	taintles with confidence p red in the closed laborato	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C	d are part of the certificate. 3 and humidity < 70%.
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power meter NRP2	taintles with contidence p ad in the closed laborato E critical for calibration)	robability are given on the following pages an	d are part of the certificate. 2 and humidity < 70%, Scheduled Calibration
Ine measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power meter NRP2	taintles with contidence p red in the closed laborato E critical for calibration)	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.)	d are part of the certificate. 2 and humidity < 70%, Scheduled Calibration Mar-24
All calibrations have been conduct Calibration Equipment used (M&TI 2rimary Standards 2rower meter NRP2 2rower sensor NRP-Z91 2rower sensor NRP-Z91	tainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805)	d are part of the certificate. 2 and humidity < 70%, Scheduled Calibration
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power meter NRP2 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator	atainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103934 (20k)	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power meter NRP-29 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination	Iainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 103242 SN: 103242 SN: 103242 SN: 103242	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804)	d are part of the certificate. 2 and humidity < 70%. <u>Scheduled Calibration</u> Mar-24 Mar-24 Mar-24
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power smoth NRP-2 Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Altenuator Type-N mismatch combination Paterence Probe EX3DV4	alinties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 103244 SN: 103244 SN: 103245 SN: 31494394 (20k) SN: 3149 SN: 3149	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 30-Mar-23 (No. 217-03604/03805) 30-Mar-23 (No. 217-03605) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Primary Standards Prover sensor NRP-29 Power sensor NRP-291 Power sensor NRP-291 Peterence 20 dB Attenuator Type-N mismatch combination Paterence Probe EX3DV4	Iainties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 103242 SN: 103242 SN: 103242 SN: 103242	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C <u>Cal Date (Certificate No.)</u> 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power meter NRP2 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4	alinties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 103244 SN: 103244 SN: 103245 SN: 31494394 (20k) SN: 3149 SN: 3149	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C Cal Date (Certificata No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. EX3-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards 20wer meter NRP: 2 20wer sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismach combination Reterence Probe EX3DV4 3AE4 Secondary Standards	alinties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 103244 SN: 103245 SN: 103245 SN: 103245 SN: 19324 (20k) SN: 310982 / 66327 SN: 7349 SN: 601	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Jan-24 Scheduled Check
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Fype-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B	atinties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 103244 SN: 103244 SN: 103244 SN: 303244 SN: 30982 / 06327 SN: 7349 SN: 601 ID #	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 30-Mar-24 (No. 217-03810) 30-Mar-22 (No. 217-03810) 30-Ddt-14 (In house) 30-Odt-14 (In house)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power meter NRP-2 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismach combination Reterence Probe EX3DV4 DAE4 Secondary Standards Power sensor HP 8481A Power sensor HP 8481A	alinties with confidence p ed in the closed laborato E critical for calibration) ID # SN: 104776 SN: 103244 SN: 103244 SN: BH9394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Jec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24 In house check: Oct-24
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Paterence 20 dB Attenuator Fype-N mismatch combination Paterence Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A Power sensor HP 8481A Power Resor H& 8481A	ad in the closed laborato ed in the closed laborato E critical for calibration) ID # SN: 104776 SN: 103244 SN: 5H:9394 (20k) SN: 310982 / 06827 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: MY1093315 SN: 10972	Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-24 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-25 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-26 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-27 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-28 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-28 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-29 (No. DAE4-601_Dec22) 30-Mar-23 (No. 217-03805) 30-Mar-14 (In house check Oct-22) 30-Oct-15 (In house check Oct-22)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24 In house check: Oct-24 In house check: Oct-24
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A Power sensor HP 8481A Pig egenrator R&S SMT-06	atinties with confidence p ad in the closed laborato E critical lor calibration) ID # SN: 103244 SN: 103244 SN: 103244 SN: 30424 SN: 30425 SN: 30455 SN: 30455 SN: 30455 SN: 30455 SN: 304555 SN: 304555 SN: 3	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 213-7349_Jan23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Jan-24 Jec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24 In house check: Oct-24
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E44198 Power meter E44198 Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer Agilent E8358A	ad in the closed laborato ed in the closed laborato E critical for calibration) ID # SN: 104776 SN: 103244 SN: 5H:9394 (20k) SN: 310982 / 06827 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: MY1093315 SN: 10972	Cal Date (Certificate No.) 20-date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03804) 10-Jan-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Dt-14 (In house check Ot-22) Check Date (In house check Ot-22) 07-0ct-15 (In house check Ot-22) 07-0ct-15 (In house check Ot-22) 07-0ct-15 (In house check Ot-22)	d are part of the certificate. 2 and humidity < 70%. 3 Scheduled Calibration 4 Mar-24 4 Mar-24 4 Mar-24 4 Mar-24 4 Mar-24 5 Mar-2
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power sensor NRP-291 Power meter E44198 Power meter E44198 Power sensor HP 8481A Power Sensor PR 8481A Power 9481A Power 9481A	In the closed laborato ID # ID # SN: 103244 SN: 103728 SN: US41080477	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-13 (In house check Oct-22) 07-Oct-15 (In house check Oct-22) 07-Oct-15 (In house check Oct-22) 15-Jan-15 (In house check Oct-22) 31-Mar-14 (In house check Oct-22)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Jan-24
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E44198 Power meter E44198 Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer Agilent E8358A	Iainties with confidence p ad in the closed laborato E critical for calibration) ID # SN: 103244 SN: 103244 SN: 103244 SN: 310982 / 06827 SN: 601 ID # SN: 601 SN: US37282783 SN: W1403315 SN: 103272 SN: US41080477 Name	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 10-Jan-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-0380) 30-Oct-14 (In house check Oct-22) Check Date (In house check Oct-22) 07-Oct-15 (In house check Oct-22) 15-Jun-15 (In house check Oct-22) 31-Mar-14 (In house check Oct-22) Function	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24
The measurements and the uncert All calibration Equipment used (M&TI Calibration Equipment used (M&TI Primary Standards Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Altenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power sensor HP 8481A Power sensor PB 8481A	Iainties with confidence p ad in the closed laborato ID # SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 310982 / 06327 SN: 601 ID # SN: 601 SN: US37292783 SN: US41080477 Name Michael Weber	robability are given on the following pages an ry facility: environment temperature (22 ± 3)*C Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03804) 30-Oct-14 (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22) 31-Mar-14 (in house check Oct-22) Function Laboratory Technician	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24
	Iainties with confidence p ad in the closed laborato E critical for calibration) ID # SN: 103244 SN: 103244 SN: 103244 SN: 310982 / 06827 SN: 601 ID # SN: 601 SN: US37282783 SN: W1403315 SN: 103272 SN: US41080477 Name	robability are given on the following pages an ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 10-Jan-23 (No. 217-03809) 30-Mar-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-0380) 30-Oct-14 (In house check Oct-22) Check Date (In house check Oct-22) 07-Oct-15 (In house check Oct-22) 15-Jun-15 (In house check Oct-22) 31-Mar-14 (In house check Oct-22) Function	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Jan-24
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Power sensor NRP-291 Power sensor Probe EX3DV4 DAE4 Secondary Standards Power sensor HP 8481A Power sensor HP 8481A Power sensor HP 8481A Power sensor HP 8481A Pennetar E4198 Power sensor HP 8481A Power sensor HP 8481A Pennetar F44198 Power sensor HP 8481A Panetar Patha Patha Panetar Patha Patha Panetar Patha Patha Panetar Patha Patha Panetar Panetar Patha Panetar Panetar Panet	Iainties with confidence p ad in the closed laborato ID # SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 103244 SN: 310982 / 06327 SN: 601 ID # SN: 601 SN: US37292783 SN: US41080477 Name Michael Weber	robability are given on the following pages an ry facility: environment temperature (22 ± 3)*C Cal Date (Certificate No.) 30-Mar-23 (No. 217-03804/03805) 30-Mar-23 (No. 217-03804) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 30-Mar-23 (No. 217-03805) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03810) 10-Jan-23 (No. 217-03804) 30-Oct-14 (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22) 31-Mar-14 (in house check Oct-22) Function Laboratory Technician	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Mar-24 Mar-24 Mar-24 Mar-24 Mar-24 Jan-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

t (886-2) 2299-3279

Unless otherwise stated the results shown in this test report reter only to the sample(s) lested and such sample(s) are retained to 90 days only. Mir#JSfabity i, Lt&Bateger and the company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fulleest extent of the law. prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號



Report No. : TESA2309000534EN Page: 3 of 15

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

S

C

S

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

- Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020. b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The source is mounted in a touch configuration below the center marking of the flat phantom.
- Return Loss: This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized; SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-727 Apr23

Page 2 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



Report No. : TESA2309000534EN Page: 4 of 15

Measurement Conditions

DASY system configuration, as far as not given on page	1
--	---

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.7 ± 6 %	1.86 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	àna.	

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.6 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	53.1 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured	condition 250 mW input power	6.28 W/kg

Certificate No: D2450V2-727_Apr23

Page 3 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

Unless other was baled une solute of the state and the state report refer only to the sample(s) lessed and state and provide the sample(s) lessed and state prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



Report No. : TESA2309000534EN Page: 5 of 15

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	55.0 Ω + 2.1 jΩ
Return Loss	- 25.8 dB

General Antenna Parameters and Design

1.148 ns	Electrical Delay (one direction)	1.148 ns
----------	----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still constrained to be Stendard. according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG	

Certificate No: D2450V2-727_Apr23

Page 4 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488

www.sqs.com.tw



Report No. : TESA2309000534EN Page: 6 of 15

DASY5 Validation Report for Head TSL

Test Laboratory: SPEAG, Zurich, Switzerland

Date: 25.04.2023

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:727


Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz; $\sigma = 1.86$ S/m; $\epsilon_r = 37.7$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(7.88, 7.88, 7.88) @ 2450 MHz; Calibrated: 10.01.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 19.12.2022
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 118.5 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 27.1 W/kgSAR(1 g) = 13.6 W/kg; SAR(10 g) = 6.28 W/kg Smallest distance from peaks to all points 3 dB below = 9 mm Ratio of SAR at M2 to SAR at M1 = 50.2%Maximum value of SAR (measured) = 22.5 W/kg



0 dB = 22.5 W/kg = 13.52 dBW/kg

Certificate No: D2450V2-727_Apr23

Page 5 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.


除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



Impedance Measurement Plot for Head TSL

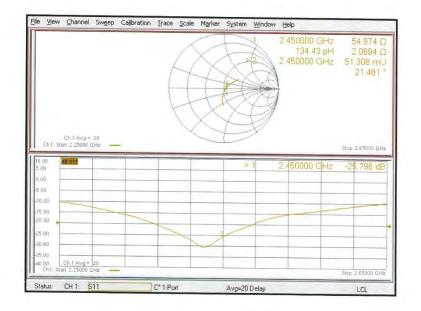

Certificate No: D2450V2-727_Apr23

Page 6 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

t (886-2) 2299-3279 台灣檢驗科技股份有限公司

f (886-2) 2298-0488

www.sgs.com.tw



Report No. : TESA2309000534EN Page: 8 of 15

		The and the second	Swiss Calibration Service
Accredited by the Swiss Accredita The Swiss Accreditation Service Multilateral Agreement for the re	is one of the signatori		Accreditation No.: SCS 0108
Client SGS Taoyuan City, Ta	iwan	Certificate No.	D5GHzV2-1349_Mar23
CALIBRATION C	ERTIFICAT	E	
Object	D5GHzV2 - SN:"	1349	
Calibration procedure(s)	QA CAL-22,v7		
	Calibration Proce	edure for SAR Validation Sources	between 3-10 GHz
Calibration date:	March 20, 2023		
All calibrations have been conduct	ed in the closed laborator	onal standards, which realize the physical unit robability are given on the following pages and ry facility: environment temperature (22 ± 3) °C	d are part of the certificate.
Il calibrations have been conduct	ed in the closed laborator	robability are given on the following pages and ry facility: environment temperature $(22 \pm 3)^{\circ}C$	d are part of the certificate.
Il calibrations have been conduct calibration Equipment used (M&TI rimary Standards	ed in the closed laborator	robability are given on the following pages and ry facility: environment temperature (22 ± 3)*C Cal Date (Certificate No.)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration
Il calibrations have been conduct alibration Equipment used (M&TI rimary Standards ower meter NRP	ed in the closed laborator E critical for calibration)	robability are given on the following pages and ry facility: environment temperature $(22 \pm 3)^{\circ}C$	d are part of the certificate.
Il calibrations have been conduct alibration Equipment used (M&TI rimary Standards ower meter NRP- ower sensor NRP-291 ower sensor NRP-291	ed in the closed laborator E critical for calibration) ID # SN: 104778	robability are given on the following pages and ry facility: environment temperature (22 ± 3)*C Cal Date (Certificate No.) D4-Apr-22 (No. 217-03525/03524)	d are part of the cartificate.
II calibrations have been conduct calibration Equipment used (M&TI rimary Standards ower meter NRP- ower sensor NRP-291 over sensor NRP-291 eference 20 dB Attenuator	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k)	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03524)	d are part of the certificate.
Il calibrations have been conduct Calibration Equipment used (M&TI trimary Standards Tower meter NRP tower sensor NRP-291 tower sensor NRP-291 teference 20 dB Attenuator ype-N mismatch combination	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 310384 (20k) SN: 310382 / 06327	Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03528)	d are part of the certificate.
II calibrations have been conduct calibration Equipment used (M&TI rimary Standards over meter NRP over sensor NRP-291 over sensor NRP-291 deference 20 dB Attenuator ype-N mismatch combination eference Probe EX3DV4	ed in the closed laboration E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 8149394 (20k) SN: 3503 SN: 3503	Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03528) 07-Mar-23 (No. EX3-3005_Mar23) 04-Apr-23 (No. 217-03528)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24
II calibrations have been conduct calibration Equipment used (M&TI rimary Standards over meter NRP over sensor NRP-291 over sensor NRP-291 deference 20 dB Attenuator ype-N mismatch combination eference Probe EX3DV4	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 310384 (20k) SN: 310382 / 06327	Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03528)	d are part of the cartificate.
All calibrations have been conduct Calibration Equipment used (M&TI trimary Standards Tower meter NRP Tower sensor NRP-Z91 Tower sensor NRP-Z91 Geference 20 dB Attenuator type-N mismatch combination teference Probe EX3DV4 IAE4	ed in the closed laboration E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 8149394 (20k) SN: 3503 SN: 3503	Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03528) 07-Mar-23 (No. EX3-3005_Mar23) 04-Apr-23 (No. 217-03528)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24
All calibrations have been conduct Calibration Equipment used (M&TI trimary Standards Tower sensor NRP-291 Cover sensor NRP-291 Reference 20 dB Attenuator ype-N mismatch combination teference Probe EX3DV4 VAE4 econdary Standards over meter E4419B	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 8H9394 (20k) SN: 310982 / 06327 SN: 3503 SN: 601	Cal Date (Certificate No.) D4-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03528) 07-Mar-23 (No. EX3-3503_Mar23) 19-Dec-22 (No. DAE4-601_Dec22)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24 Dec-23
Il calibrations have been conduct Salibration Equipment used (M&TI trimary Standards Tower meter NRP Tower sensor NRP-Z91 tower sensor NRP-Z91 teference 20 dB Attenuator ype-N mismatch combination teference Probe EX3DV4 iyAE4 econdary Standards ower meter E44198 ower sensor HP 8481A	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 104778 SN: 103244 SN: 310982 (06327 SN: 3503 SN: 3601 ID #	Cal Date (Certificate No.) Gal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03528) 07-Mar-23 (No. EX3-3005_Mar23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24 Dec-23 Scheduled Check
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Prower meter NRP Prower sensor NRP-291 Yower sensor NRP-291 Reference 20 dB Attenuator ype-N mismatch combination Reference Probe EX3DV4 VAE4 Recondary Standards Yower sensor HP 8481A Yower sensor HP 8481A	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 104778 SN: 103244 SN: 310982 (06327 SN: 3503 SN: 601 ID # ID # SN: 0539512475 SN: US37292783 SN: W41093315	Cal Date (Certificate No.) Gal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 07-Mar-23 (No. EX3-3005_Mar23) 19-Dec-22 (No. 216-03528) 07-Ch-15 (in house check Oct-22) Check Date (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24 Dec-23 Scheduled Check In house check: Oct-24
All calibrations have been conduct Calibration Equipment used (M&TI trimary Standards Tower sensor NRP-291 telerence 20 dB Attenuator ype-N mismatch combination telerence Probe EX3DV4 WAE4 econdary Standards ower sensor HP 8481A ower sensor HP 8481A F generator R&S SMT-06	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 8H3944 (20k) SN: 310882 / 06327 SN: 3038 SN: 6B39512475 SN: 6B39512475 SN: US37282783 SN: W141093115 SN: 10972	Cal Date (Certificate No.) Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03528) 07-Mar-32 (No. EX3-3503) Mar23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24
All calibrations have been conduct Calibration Equipment used (M&TI trimary Standards Tower sensor NRP-291 telerence 20 dB Attenuator ype-N mismatch combination telerence Probe EX3DV4 WAE4 econdary Standards ower sensor HP 8481A ower sensor HP 8481A F generator R&S SMT-06	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 104778 SN: 103244 SN: 310982 (06327 SN: 3503 SN: 601 ID # ID # SN: 0539512475 SN: US37292783 SN: W41093315	Cal Date (Certificate No.) Gal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 07-Mar-23 (No. EX3-3005_Mar23) 19-Dec-22 (No. 216-03528) 07-Ch-15 (in house check Oct-22) Check Date (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24 In house check: Oct-24 In house check: Oct-24
All calibrations have been conduct Calibration Equipment used (M&TI trimary Standards Tower sensor NRP-291 telerence 20 dB Attenuator ype-N mismatch combination telerence Probe EX3DV4 WAE4 econdary Standards ower sensor HP 8481A ower sensor HP 8481A F generator R&S SMT-06	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 8H3944 (20k) SN: 310882 / 06327 SN: 3038 SN: 6B39512475 SN: 6B39512475 SN: US37282783 SN: W141093115 SN: 10972	Cal Date (Certificate No.) Gal Date (Certificate No.) G4-Apr-22 (No. 217-03525/03524) G4-Apr-22 (No. 217-03525/03524) G4-Apr-22 (No. 217-03525) G4-Apr-22 (No. 217-03525) G4-Apr-22 (No. 217-03525) G4-Apr-22 (No. 217-03527) G4-Apr-22 (No. 217-03527) G4-Apr-22 (No. 217-03528) O7-Mar-23 (No. EX3-3305_Mar23) 19-Dec-22 (No. 217-03527) O7-Mar-23 (No. EX3-3305_Mar23) 19-Dec-22 (No. 217-03527) O7-Mar-13 (In house check Oct-22) Check Date (in house) 30-0ct-14 (In house check Oct-22) O7-Oct-15 (In house check Oct-22) O7-Oct-15 (In house check Oct-22) 15-Jun-15 (In house check Oct-22) 31-Mar-14 (In house check Oct-22)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24
All calibrations have been conduct Calibration Equipment used (M&TI trimary Standards Yower meter NRP Yower sensor NRP-291 telerence 20 dB Attenuator ype-N mismatch combination telerence 20 dB Attenuator ype-N mismatch combination telerence Probe EX3DV4 WAE4 econdary Standards ower meter E4419B ower sensor HP 8481A ower sensor HP 8481A F generator R&S SMT-06 etwork Analyzer Agilent E8358A	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 104778 SN: 03244 SN: 30345 SN: 8H9394 (20k) SN: 310982 (06327 SN: 3503 SN: 601 ID # ID # SN: 639512475 SN: US3722783 SN: 10972 SN: US41080477	Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03526) 04-Apr-22 (No. 217-03528) 07-Mar-32 (No. EX3-3030, Mar23) 19-Dec-22 (No. EX4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22) 31-Mar-14 (in house check Oct-22)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24
All calibrations have been conduct Calibration Equipment used (M&TI trimary Standards Yower meter NRP Yower sensor NRP-291 telerence 20 dB Attenuator ype-N mismatch combination telerence 20 dB Attenuator ype-N mismatch combination telerence Probe EX3DV4 WAE4 econdary Standards ower meter E4419B ower sensor HP 8481A ower sensor HP 8481A F generator R&S SMT-06 etwork Analyzer Agilent E8358A	ed in the closed laborator E critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 8H394 (20k) SN: 310882 / 06327 SN: 310882 / 06327 SN: 503 SN: 603 SN: 603 SN: 603 SN: 6039512475 SN: US37292783 SN: WY4109315 SN: 109972 SN: US41080477 Name	Cal Date (Certificate No.) Gal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03527) 04-Apr-22 (No. 217-03528) 07-Mar-23 (No. EX3-3030_Mar23) 19-Dec-22 (No. DAE4-601_Dec22) Check Date (in house) 30-0ct-14 (in house check Oct-22) 07-0ct-15 (in house check Oct-22) 07-0ct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22) 31-Mar-14 (in house check Oct-22)	d are part of the certificate. 2 and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24
All calibrations have been conduct Calibration Equipment used (M&TI Primary Standards Power meter NRP Power sensor NRP-291 Reference 20 dB Attenuator ype-N mismatch combination Reference 20 dB Attenuator ype-N mismatch combination Reference Probe EX3DV4 WAE4 Recondary Standards Power sensor HP 8481A rower sensor HP 8481A rower sensor HP 8481A rower sensor HP 8481A rower sensor HP 8481A regenerator R&S SMT-06 letwork Analyzer Agilent E8358A salibrated by:	ed in the closed laborator E critical for calibration) 1D # SN: 104778 SN: 103244 SN: 103245 SN: 8H394 (20k) SN: 31082 / 06327 SN: 30820 SN: 6B39512475 SN: US37202783 SN: W74103315 SN: US37202783 SN: US37202783 SN: US372072 SN: US41080477 Name Michael Weber	Cal Date (Certificate No.) Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03526) 07-Mar-32 (No. EX3-3030, Mar23) 19-Dec-22 (No. EX3-3030, Mar23) 09-Or-L15 (in house check Oct-22) Check Date (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 31-Mar-14 (in house check Oct-22) Function Laboratory Technician	d are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24
All calibrations have been conduct Calibration Equipment used (M&TI trimary Standards Tower meter NRP Tower sensor NRP-291 telerence 20 dB Attenuator ype-N mismatch combination telerence 20 dB Attenuator ype-N mismatch combination telerence Probe EX3DV4 WAE4 econdary Standards ower meter E4419B ower sensor HP 8481A ower sensor HP 8481A Figenerator R&S SMT-06 etwork Analyzer Agilent E8358A alibrated by:	ed in the closed laborator E critical for calibration) 1D # SN: 104778 SN: 103244 SN: 103245 SN: 8H394 (20k) SN: 310882 / 06327 SN: 310882 / 06327 SN: 6B39512475 SN: 6B39512475 SN: 6B39512475 SN: US37292783 SN: 4W1400315 SN: 109972 SN: US41080477 Name	Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03526) 04-Apr-22 (No. 217-03528) 07-Mar-32 (No. EX3-3030, Mar23) 19-Dec-22 (No. EX4-601_Dec22) Check Date (in house) 30-Oct-14 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 15-Jun-15 (in house check Oct-22) 31-Mar-14 (in house check Oct-22)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24
	ed in the closed laborator E critical for calibration) 1D # SN: 104778 SN: 103244 SN: 103245 SN: 8H394 (20k) SN: 31082 / 06327 SN: 30820 SN: 6B39512475 SN: US37202783 SN: W74100315 SN: US37202783 SN: US37202783 SN: US372072 SN: US41080477 Name Michael Weber	Cal Date (Certificate No.) Cal Date (Certificate No.) 04-Apr-22 (No. 217-03525/03524) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03525) 04-Apr-22 (No. 217-03526) 07-Mar-32 (No. EX3-3030, Mar23) 19-Dec-22 (No. EX3-3030, Mar23) 09-Or-L15 (in house check Oct-22) Check Date (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 07-Oct-15 (in house check Oct-22) 31-Mar-14 (in house check Oct-22) Function Laboratory Technician	d are part of the certificate. and humidity < 70%. Scheduled Calibration Apr-23 Apr-23 Apr-23 Apr-23 Apr-23 Mar-24 Dec-23 Scheduled Check In house check: Oct-24 In house check: Oct-24 I

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

t (886-2) 2299-3279

Unless otherwise stated the results shown in this test report reter only to the sample(s) lested and such sample(s) are retained to 90 days only. Mir#JSfabity i, Lt&Bateger and the company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fulleest extent of the law. prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號



Report No. : TESA2309000534EN Page: 9 of 15

Calibration Laboratory of Schmid & Partner Engineering AG aughausstrasse 43, 8004 Zurich, Switzerland Zeugh



Schweizerischer Kalibrierdienst S Service suisse d'étalonnag Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

C

S

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary: TSL ConvF N/A

not applicable or not measured

tissue simulating liquid sensitivity in TSL / NORM x,y,z

- Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
 - b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The source is mounted in a touch configuration below the center marking of the flat phantom.
- Return Loss: This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D5GHzV2-1349 Mar23

Page 2 of 8

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



Report No. : TESA2309000534EN Page: 10 of 15

Measurement Conditions

DASY system configuration, as far as not given on page 1

DASY Version	DASY52	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5250 MHz ± 1 MHz 5600 MHz ± 1 MHz 5750 MHz ± 1 MHz	

Head TSL parameters at 5250 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.71 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.8 ± 6 %	4.71 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL at 5250 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.04 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	80.4 W/kg ± 19.9 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.30 W/kg

Head TSL parameters at 5600 MHz

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22,0 ± 0.2) °C	35.6 ± 6 %	5.09 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL at 5600 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	83.1 W/kg ± 19.9 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured	condition 100 mW input power	2.36 W/kg

Certificate No: D5GHzV2-1349_Mar23

Page 3 of 8

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

t (886-2) 2299-3279

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號



Report No. : TESA2309000534EN Page: 11 of 15

Head TSL parameters at 5750 MHz The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.4	5.22 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.4 ± 6 %	5.21 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		1.000

SAR result with Head TSL at 5750 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	81.4 W/kg ± 19.9 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured	condition 100 mW input power	2.32 W/kg

Certificate No: D5GHzV2-1349_Mar23

Page 4 of 8

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留的天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents subject to Terms and Conditions for Electronic Documents at <u>http://www.sgs.com.tw/Terms-and-Conditions</u>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

t (886-2) 2299-3279 台灣檢驗科技股份有限公司

f (886-2) 2298-0488

www.sgs.com.tw



Report No. : TESA2309000534EN Page: 12 of 15

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL at 5250 MHz

Impedance, transformed to feed point	48.4 Ω - 1.8 jΩ
Return Loss	- 32.1 dB

Antenna Parameters with Head TSL at 5600 MHz

Impedance, transformed to feed point	51.2 Ω + 2.5 jΩ	
Return Loss	- 31.3 dB	

Antenna Parameters with Head TSL at 5750 MHz

Impedance, transformed to feed point	53.3 Ω + 4.6 jΩ	
Return Loss	- 25.1 dB	-

General Antenna Parameters and Design

Electrical Delay (one direction)	1.198 ns	-

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still recording to the Standard according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
	OFEAG

Certificate No: D5GHzV2-1349_Mar23

Page 5 of 8

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號



Report No. : TESA2309000534EN Page: 13 of 15

Date: 20.03.2023

DASY5 Validation Report for Head TSL

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN:1349

Communication System: UID 0 - CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN3503; ConvF(5.5, 5.5, 5.5) @ 5250 MHz, ConvF(5.1, 5.1, 5.1) @ 5600 MHz, . ConvF(5.08, 5.08, 5.08) @ 5750 MHz; Calibrated: 07.03.2023
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 19,12,2022
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5250 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 74.15 V/m; Power Drift = -0.02 dB Peak SAR (extrapolated) = 27.5 W/kg SAR(1 g) = 8.04 W/kg; SAR(10 g) = 2.3 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mmRatio of SAR at M2 to SAR at M1 = 70.7%Maximum value of SAR (measured) = 18.3 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 73.50 V/m; Power Drift = -0.02 dBPeak SAR (extrapolated) = 30.7 W/kgSAR(1 g) = 8.3 W/kg; SAR(10 g) = 2.36 W/kgSmallest distance from peaks to all points 3 dB below = 7.4 mm Ratio of SAR at M2 to SAR at M1 = 68.1% Maximum value of SAR (measured) = 19.6 W/kg

Certificate No: D5GHzV2-1349_Mar23

Page 6 of 8

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law


No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



Report No. : TESA2309000534EN Page: 14 of 15

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5750 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 70.65 V/m; Power Drift = -0.02 dB Peak SAR (extrapolated) = 31.7 W/kg SAR(1 g) = 8.14 W/kg; SAR(10 g) = 2.32 W/kg Smallest distance from peaks to all points 3 dB below = 7.4 mm Ratio of SAR at M2 to SAR at M1 = 66.4%Maximum value of SAR (measured) = 19.6 W/kg

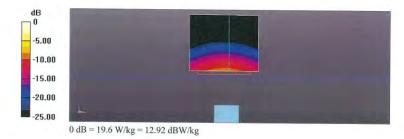

Certificate No: D5GHzV2-1349_Mar23

Page 7 of 8

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.


除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



Impedance Measurement Plot for Head TSL

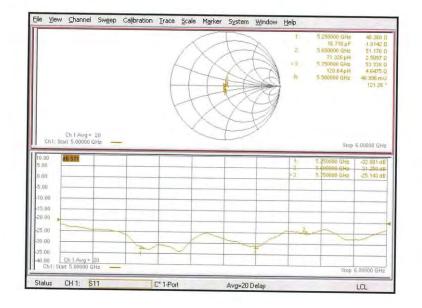

Certificate No: D5GHzV2-1349_Mar23

Page 8 of 8

- End of report -

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com.tw/Terms-and-Conditions and for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com.tw/Terms-and-Conditions. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

t (886-2) 2299-3279 台灣檢驗科技股份有限公司

f (886-2) 2298-0488

www.sgs.com.tw