

ROHDE & SCHWARZ FSP · SPECTRUM ANALYZER · 9 kHz ... 40 GHz


Nemko

Liberty Labs CAN
Serial 100032
Rev. 08/05/2017
Rev. 08/05/2016
Model SM 04444

1164.4391.40

PRESET
CAL
SETUP
HCOPI

FSP

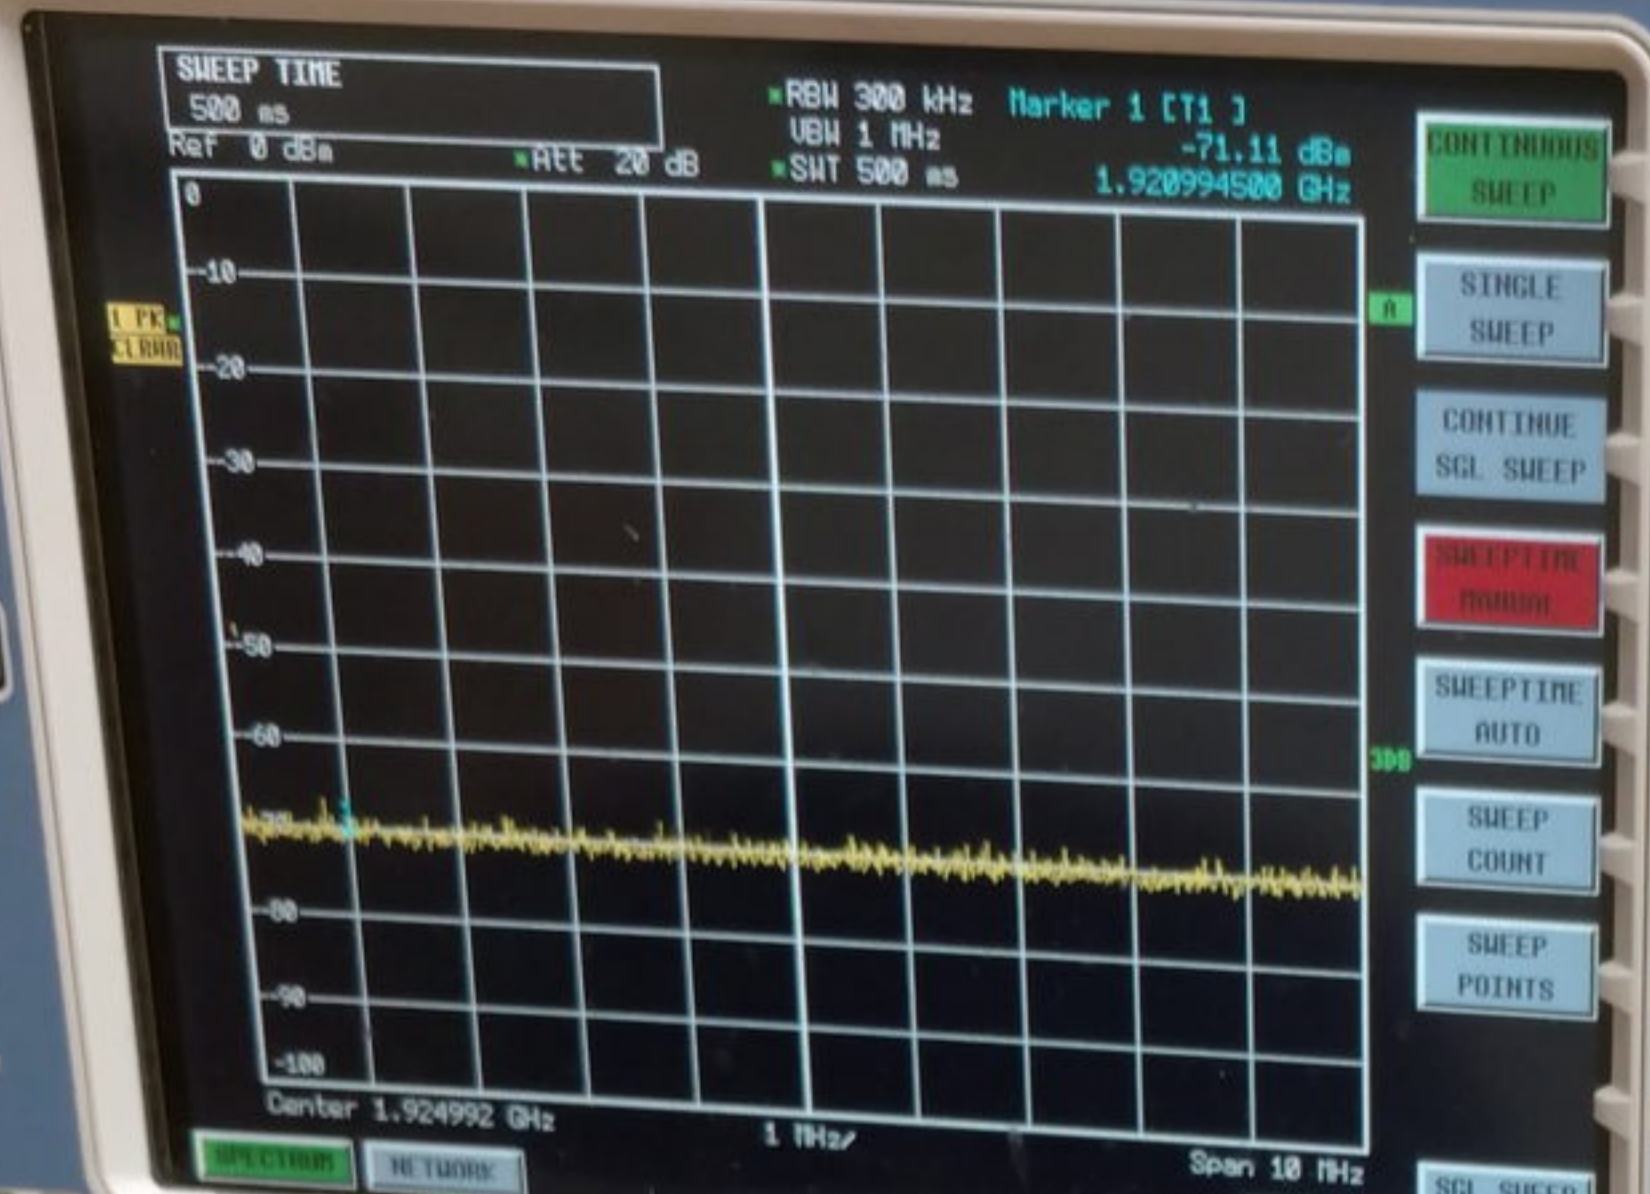

CONTINUOUS SWEEP
SINGLE SWEEP
CONTINUE SGL SWEEP
SWEEP TIME MANUAL
SWEEP TIME AUTO
SWEEP COUNT
SWEEP POINTS
SGL SWEEP DISP OFF

CONTROL: FREQ, SPAN, AMPT, MKR, MKR →, MKR FCTN

DATA: 7, 8, 9, 4, 5, 6, 1, 2, 3, 0, ., -, Hz dBm, kHz dB, MHz dBm, GHz dBm

SWEEP: BW, SWEEP, MEAS, TRIG

VARIATION: [Knob]

AF OUTPUT, GEN OUTPUT 50 Ω, PROBE POWER, EXT MIXER, LO OUT / IF IN, IF IN, RF INPUT 50 Ω, KEYBOARD

TRACE, LINES, DISP, FILE



153

