



DS-7100 (type7141) Rear Side

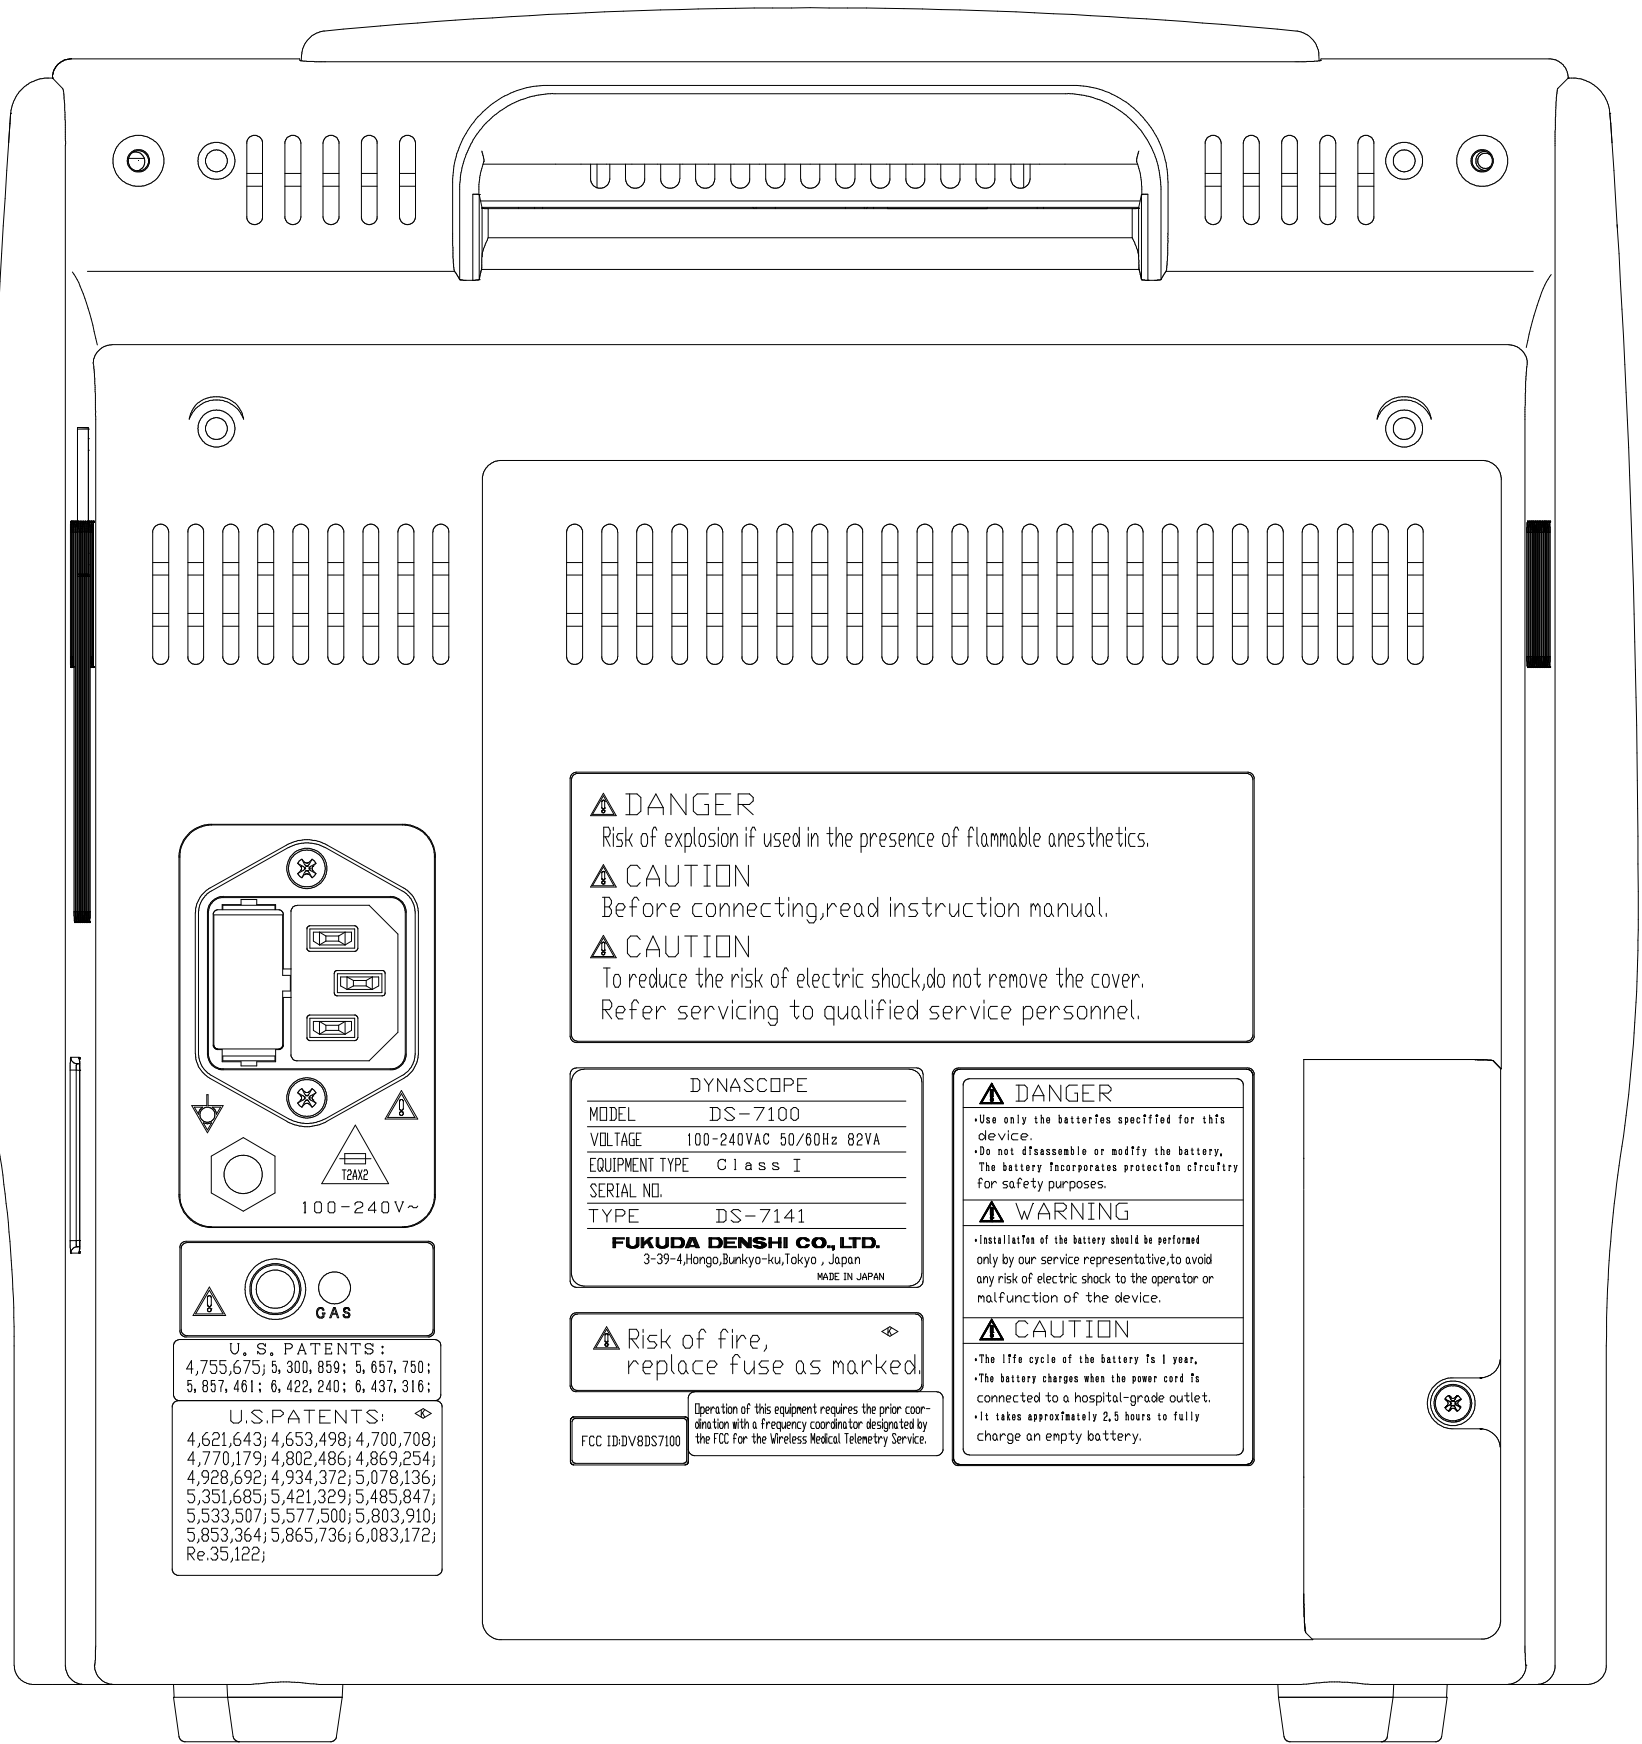

⚠ DANGER
Risk of explosion if used in the presence of flammable anesthetics.

⚠ CAUTION
Before connecting, read instruction manual.

⚠ CAUTION
To reduce the risk of electric shock, do not remove the cover.
Refer servicing to qualified service personnel.

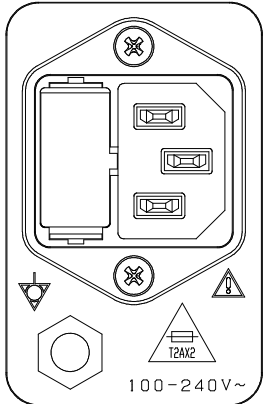

⚠ GAS

U. S. PATENTS:
4,755,675; 5,300,859; 5,657,750;
5,857,461; 6,422,240; 6,437,316;

U.S.PATENTS:
4,621,643; 4,653,498; 4,700,708;
4,770,179; 4,802,486; 4,869,254;
4,928,692; 4,934,372; 5,078,136;
5,351,685; 5,421,329; 5,485,847;
5,533,507; 5,577,500; 5,803,910;
5,853,364; 5,865,736; 6,083,172;
Re.35,122;

DYNASCOPE
MODEL DS-7100
VOLTAGE 100-240VAC 50/60Hz 82VA
EQUIPMENT TYPE Class I
SERIAL NO.
TYPE DS-7141
FUKUDA DENSHI CO., LTD.
3-39-4, Hongo, Bunkyo-ku, Tokyo, Japan
MADE IN JAPAN

⚠ DANGER
-Use only the batteries specified for this device.
-Do not disassemble or modify the battery. The battery incorporates protection circuitry for safety purposes.

⚠ WARNING
-Installation of the battery should be performed only by our service representative, to avoid any risk of electric shock to the operator or malfunction of the device.

⚠ CAUTION
-The life cycle of the battery is 1 year.
-The battery charges when the power cord is connected to a hospital-grade outlet.
-It takes approximately 2.5 hours to fully charge an empty battery.

⚠ Risk of fire, replace fuse as marked.

Operation of this equipment requires the prior coordination with a frequency coordinator designated by the FCC for the Wireless Medical Telemetry Service.
FCC ID: DV8DS7100