


• Labeling

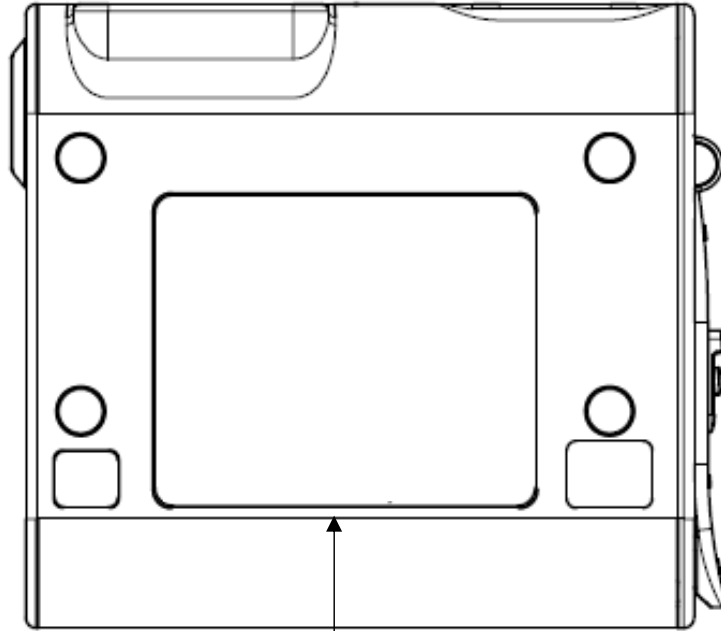

<b>ECG &amp; Respiration Transmitter</b> ◆	
<b>MODEL</b> LX-8100	<b>IPX5/IPX8</b>
<b>VOLTAGE</b> LR6 x 1	
<b>EQUIPMENT TYPE</b> INT	
<b>[SN]</b>	
<b>TYPE</b> LX-8100(G)   ID FA	<b>CERTIFIED</b> SAFETY NS E467008
<b>FCC ID</b> DV8LX8100G	
<small>ANSI/AAMI ES80601-1 (2005) + AMD 1 (2012)</small>	
<small>MEDICAL - PATIENT-MONITORING EQUIPMENT</small>	
<b>Fukuda Denshi Co.,Ltd.</b>	
<small>3-39-4 Hongo, Bunkyo-ku, Tokyo, Japan    MADE IN JAPAN</small>	