


Appendix A. Test Setup Photos

The equipment under test was placed on a wooden desk inside of shield room. The isotropic field probe was used to measure the field strength for 6 EUT surfaces, and during measurement a separation of 20cm for position A and B, 15cm for position C, D, E and F are maintained between EUT surface and the center of the field probe.



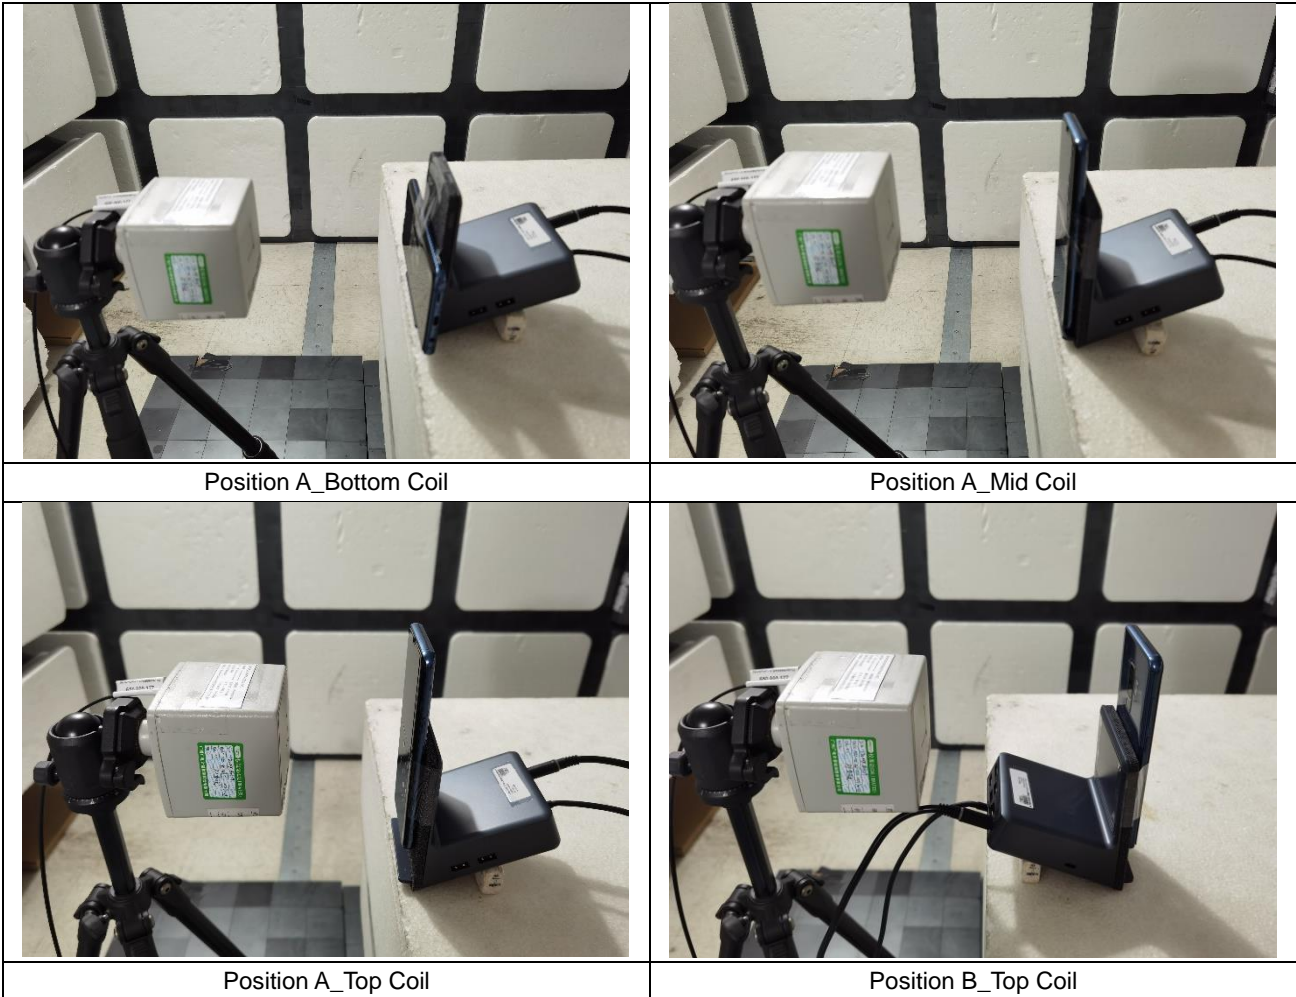

Position C_Top Coil



Position D_Top Coil



Position E_Top Coil



Position F_Top Coil