



SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

## Appendix A SAR Plots



## SAR Test Report

Operator : Chen  
 Validation Date : 19-Apr-2009  
 Measurement Date : 19-Apr-2009  
 Starting Time : 19-Apr-2009 10:56:49 AM  
 End Time : 19-Apr-2009 11:10:54 AM  
 Scanning Time : 845 secs

Product Data  
 Device Name : Dell\_Tahiti\_Hitachi  
 Serial No. : N/A  
 Type : Other  
 Model : Latitude D510  
 Frequency : 2450.00 MHz  
 Max. Transmit Pwr : 0.05 W  
 Drift Time : 0 min(s)  
 Length : 100 mm  
 Width : 150 mm  
 Depth : 30.4 mm  
 Antenna Type : Internal  
 Power Drift-Start : 0.112  
 Power Drift-Finish: 0.117  
 Power Drift (%) : 4.464

Phantom Data  
 Name : APREL-Uni  
 Type : Uni-Phantom  
 Size : 280 x 280 x 200  
 Serial No. : User Define  
 Location : Center  
 Description : User Define Data

Tissue Data  
 Type : BODY  
 Serial No. : 2450  
 Frequency : 2450 MHz  
 Calibration Date : 19-Apr-2005  
 Temperature : 21 °C  
 Ambient Temp. : 22 °C  
 Humidity : 50 RH%  
 Epsilon : 54.12 F/m  
 Sigma : 2.01 S/m  
 Density : 1000 kg/cu. m


Probe Data  
 Name : APREL Probe 212  
 Model : E020  
 Type : E-Field Triangle  
 Serial No. : 212  
 Calibration Date : 27-Dec-2004  
 Frequency : 2450 MHz  
 Duty Cycle Factor: 1  
 Conversion Factor: 5  
 Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
 Compression Point: 95 mV  
 Offset : 1.56

Measurement Data

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 21 °C  
 Ambient Temp. : 22°C  
 Set-up Date : 19-Apr-2009  
 Set-up Time : 10:54:11 AM

Other Data

DUT Position : Touch  
 Separation : 0  
 Channel : Low - 2412

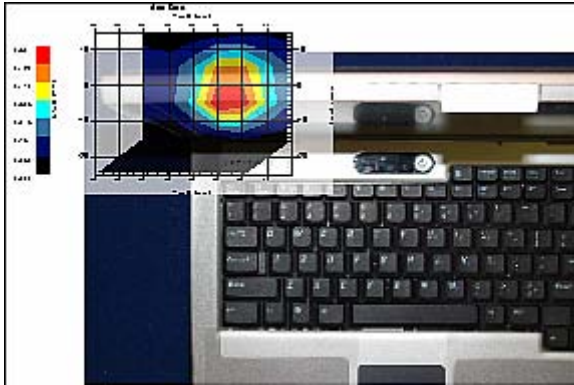

1 gram SAR value : 0.458 W/kg  
 Zoom Scan Peak SAR : 0.900






SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

**Exposure Assessment Measurement Uncertainty**

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	$c_i^1$ (1-g)	$c_i^1$ (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)^{1/2}$	$(1-cp)^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	13.4	rectangular	$\sqrt{3}$	1	1	0.0	0.0
Phantom and Setup							
Phantom Uncertainty (shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity (target)	5.0	rectangular	$\sqrt{3}$	0.7	0.5	2.0	1.4
Liquid Conductivity (meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity (target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.7	0.6
Liquid Permittivity (meas.)	5.4	rectangular	$\sqrt{3}$	0.6	0.5	1.9	1.6
Combined Uncertainty		RSS				9.3	9.1
Combined Uncertainty (coverage factor=2)		Normal (k=2)				18.6	18.2



SAR-Z Axis  
at Hotspot x:-2.9 y:-41.9

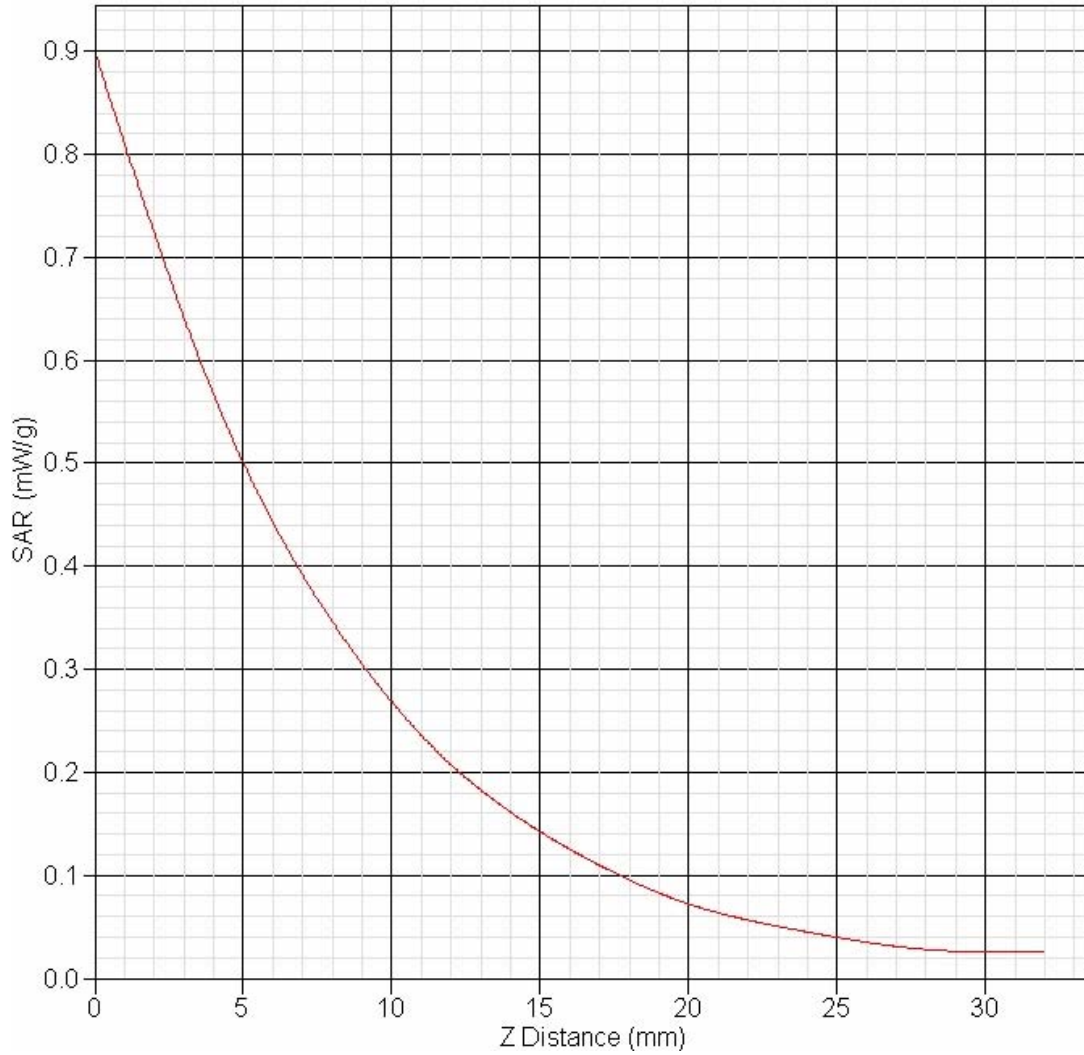

## SAR Test Report

Operator : Chen  
 Validation Date : 19-Apr-2009  
 Measurement Date : 19-Apr-2009  
 Starting Time : 19-Apr-2009 11:57:48 AM  
 End Time : 19-Apr-2009 12:11:47 PM  
 Scanning Time : 839 secs

Product Data  
 Device Name : Dell\_Tahiti\_Hitachi  
 Serial No. : N/A  
 Type : Other  
 Model : Latitude D510  
 Frequency : 2450.00 MHz  
 Max. Transmit Pwr : 0.05 W  
 Drift Time : 0 min(s)  
 Length : 100 mm  
 Width : 150 mm  
 Depth : 30.4 mm  
 Antenna Type : Internal  
 Power Drift-Start : 0.100  
 Power Drift-Finish: 0.099  
 Power Drift (%) : -1.000

Phantom Data  
 Name : APREL-Uni  
 Type : Uni-Phantom  
 Size : 280 x 280 x 200  
 Serial No. : User Define  
 Location : Center  
 Description : User Define Data

Tissue Data  
 Type : BODY  
 Serial No. : 2450  
 Frequency : 2450 MHz  
 Calibration Date : 19-Apr-2005  
 Temperature : 21 °C  
 Ambient Temp. : 22 °C  
 Humidity : 50 RH%  
 Epsilon : 54.12 F/m  
 Sigma : 2.01 S/m  
 Density : 1000 kg/cu. m

Probe Data  
 Name : APREL Probe 212  
 Model : E020  
 Type : E-Field Triangle  
 Serial No. : 212  
 Calibration Date : 27-Dec-2004  
 Frequency : 2450 MHz  
 Duty Cycle Factor: 1  
 Conversion Factor: 5  
 Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
 Compression Point: 95 mV  
 Offset : 1.56




Measurement Data

Crest Factor : 1  
Scan Type : Complete  
Tissue Temp. : 21 °C  
Ambient Temp. : 22°C  
Set-up Date : 19-Apr-2009  
Set-up Time : 10:54:11 AM

Other Data

DUT Position : Touch  
Separation : 0  
Channel : Low - 2412

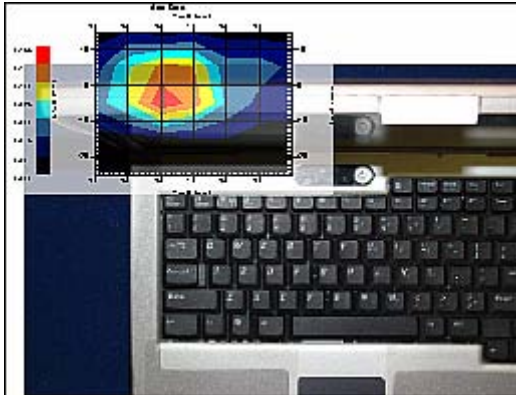

1 gram SAR value : 0.125 W/kg  
Zoom Scan Peak SAR : 0.270





SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training


**Exposure Assessment Measurement Uncertainty**

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	$c_i^{-1}$ (1-g)	$c_i^{-1}$ (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)^{1/2}$	$(1-cp)^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	-57.1	rectangular	$\sqrt{3}$	1	1	0.0	0.0
Phantom and Setup							
Phantom Uncertainty (shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity (target)	5.0	rectangular	$\sqrt{3}$	0.7	0.5	2.0	1.4
Liquid Conductivity (meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity (target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.7	0.6
Liquid Permittivity (meas.)	5.4	rectangular	$\sqrt{3}$	0.6	0.5	1.9	1.6
Combined Uncertainty		RSS				9.3	9.1
Combined Uncertainty (coverage factor=2)		Normal (k=2)				18.6	18.2





SAR-Z Axis  
at Hotspot x:5.1 y:-41.9

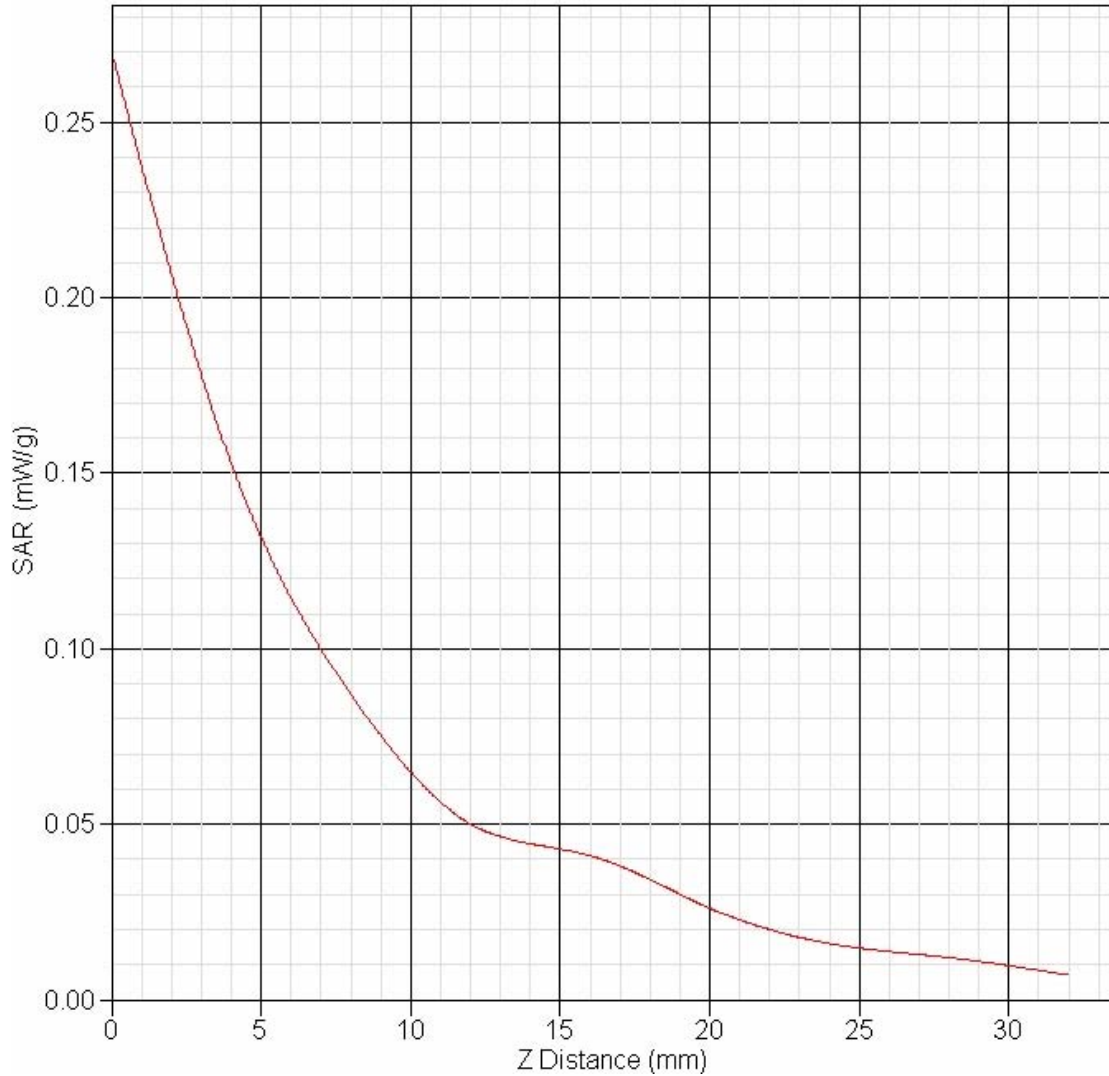

## SAR Test Report

Operator : Chen  
 Validation Date : 19-Apr-2009  
 Measurement Date : 19-Apr-2009  
 Starting Time : 19-Apr-2009 11:40:54 AM  
 End Time : 19-Apr-2009 11:54:53 AM  
 Scanning Time : 839 secs

Product Data  
 Device Name : Dell\_Tahiti\_Hitachi  
 Serial No. : N/A  
 Type : Other  
 Model : Latitude D510  
 Frequency : 2450.00 MHz  
 Max. Transmit Pwr : 0.05 W  
 Drift Time : 0 min(s)  
 Length : 100 mm  
 Width : 150 mm  
 Depth : 30.4 mm  
 Antenna Type : Internal  
 Power Drift-Start : 0.122  
 Power Drift-Finish: 0.125  
 Power Drift (%) : 3.107

Phantom Data  
 Name : APREL-Uni  
 Type : Uni-Phantom  
 Size : 280 x 280 x 200  
 Serial No. : User Define  
 Location : Center  
 Description : User Define Data

Tissue Data  
 Type : BODY  
 Serial No. : 2450  
 Frequency : 2450 MHz  
 Calibration Date : 19-Apr-2005  
 Temperature : 21 °C  
 Ambient Temp. : 22 °C  
 Humidity : 50 RH%  
 Epsilon : 54.12 F/m  
 Sigma : 2.01 S/m  
 Density : 1000 kg/cu. m


Probe Data  
 Name : APREL Probe 212  
 Model : E020  
 Type : E-Field Triangle  
 Serial No. : 212  
 Calibration Date : 27-Dec-2004  
 Frequency : 2450 MHz  
 Duty Cycle Factor: 1  
 Conversion Factor: 5  
 Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
 Compression Point: 95 mV  
 Offset : 1.56

Measurement Data

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 21 °C  
 Ambient Temp. : 22°C  
 Set-up Date : 19-Apr-2009  
 Set-up Time : 10:54:11 AM

Other Data

DUT Position : Touch  
 Separation : 0  
 Channel : Mid - 2437

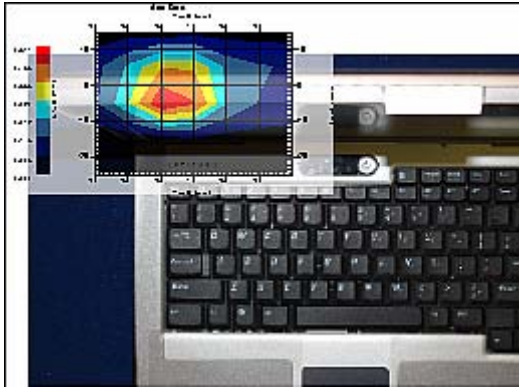

1 gram SAR value : 0.431 W/kg  
 Zoom Scan Peak SAR : 0.880




**Exposure Assessment Measurement Uncertainty**

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	$c_i^{-1}$ (1-g)	$c_i^{-1}$ (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)^{1/2}$	$(1-cp)^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	3.1	rectangular	$\sqrt{3}$	1	1	0.0	0.0
Phantom and Setup							
Phantom Uncertainty (shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity (target)	5.0	rectangular	$\sqrt{3}$	0.7	0.5	2.0	1.4
Liquid Conductivity (meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity (target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.7	0.6
Liquid Permittivity (meas.)	5.4	rectangular	$\sqrt{3}$	0.6	0.5	1.9	1.6
Combined Uncertainty		RSS				9.3	9.1
Combined Uncertainty (coverage factor=2)		Normal (k=2)				18.6	18.2



### SAR-Z Axis at Hotspot x:-2.9 y:-49.9

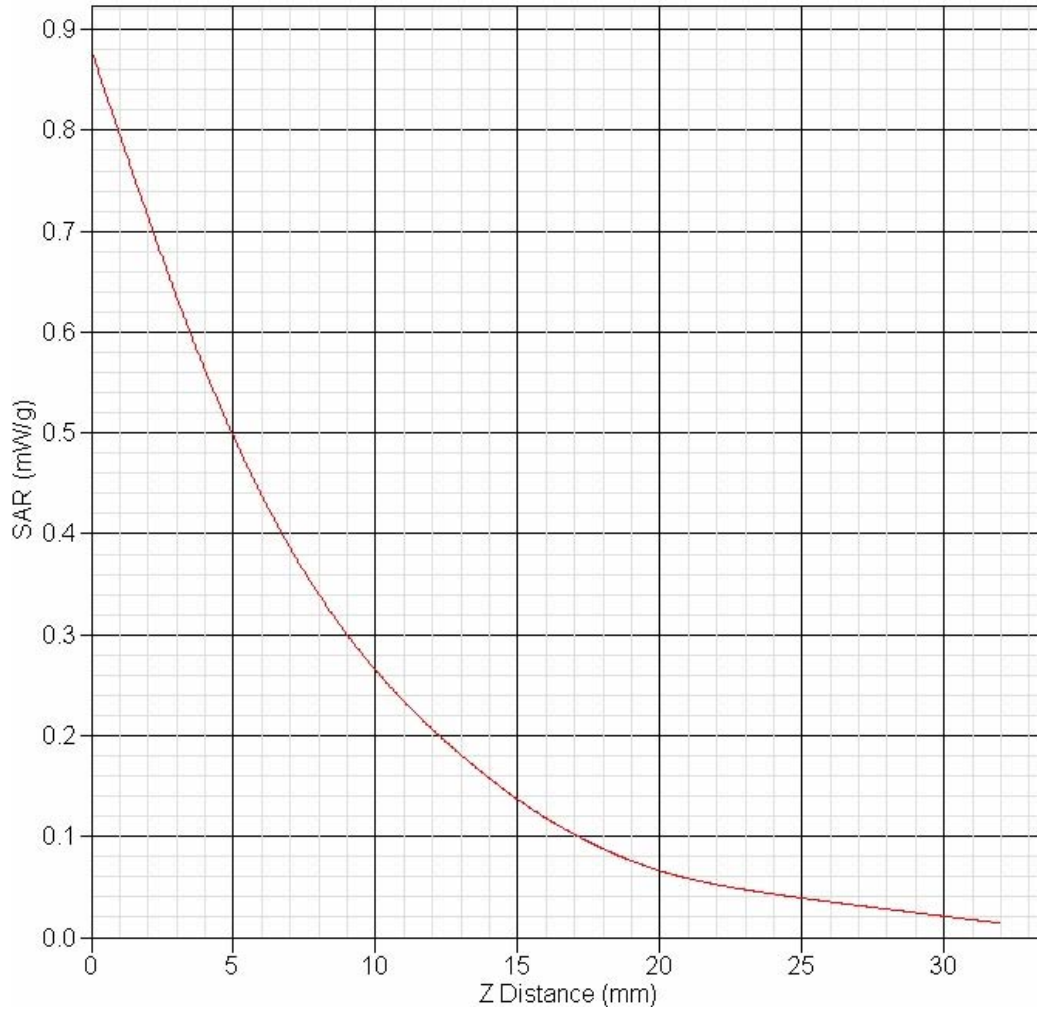



## SAR Test Report

Operator : Chen  
 Validation Date : 19-Apr-2009  
 Measurement Date : 19-Apr-2009  
 Starting Time : 19-Apr-2009 12:13:55 PM  
 End Time : 19-Apr-2009 12:27:54 PM  
 Scanning Time : 839 secs

Product Data  
 Device Name : Dell\_Tahiti\_Hitachi  
 Serial No. : N/A  
 Type : Other  
 Model : Latitude D510  
 Frequency : 2450.00 MHz  
 Max. Transmit Pwr : 0.05 W  
 Drift Time : 0 min(s)  
 Length : 100 mm  
 Width : 150 mm  
 Depth : 30.4 mm  
 Antenna Type : Internal  
 Power Drift-Start : 0.100  
 Power Drift-Finish: 0.098  
 Power Drift (%) : -2.000

Phantom Data  
 Name : APREL-Uni  
 Type : Uni-Phantom  
 Size : 280 x 280 x 200  
 Serial No. : User Define  
 Location : Center  
 Description : User Define Data

Tissue Data  
 Type : BODY  
 Serial No. : 2450  
 Frequency : 2450 MHz  
 Calibration Date : 19-Apr-2005  
 Temperature : 21 °C  
 Ambient Temp. : 22 °C  
 Humidity : 50 RH%  
 Epsilon : 54.12 F/m  
 Sigma : 2.01 S/m  
 Density : 1000 kg/cu. m

Probe Data  
 Name : APREL Probe 212  
 Model : E020  
 Type : E-Field Triangle  
 Serial No. : 212  
 Calibration Date : 27-Dec-2004  
 Frequency : 2450 MHz  
 Duty Cycle Factor: 1  
 Conversion Factor: 5  
 Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
 Compression Point: 95 mV  
 Offset : 1.56




Measurement Data

Crest Factor : 1  
Scan Type : Complete  
Tissue Temp. : 21 °C  
Ambient Temp. : 22°C  
Set-up Date : 19-Apr-2009  
Set-up Time : 10:54:11 AM

Other Data

DUT Position : Touch  
Separation : 0  
Channel : Mid - 2437

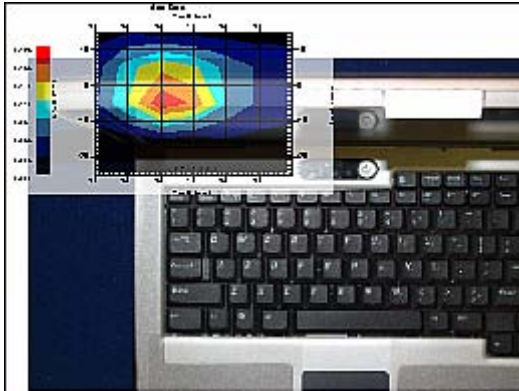

1 gram SAR value : 0.156 W/kg  
Zoom Scan Peak SAR : 0.300






SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

**Exposure Assessment Measurement Uncertainty**

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	$c_i^1$ (1-g)	$c_i^1$ (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)^{1/2}$	$(1-cp)^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	-60.2	rectangular	$\sqrt{3}$	1	1	0.0	0.0
Phantom and Setup							
Phantom Uncertainty (shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity (target)	5.0	rectangular	$\sqrt{3}$	0.7	0.5	2.0	1.4
Liquid Conductivity (meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity (target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.7	0.6
Liquid Permittivity (meas.)	5.4	rectangular	$\sqrt{3}$	0.6	0.5	1.9	1.6
Combined Uncertainty		RSS				9.3	9.1
Combined Uncertainty (coverage factor=2)		Normal (k=2)				18.6	18.2



### SAR-Z Axis at Hotspot x=-2.9 y=-49.9

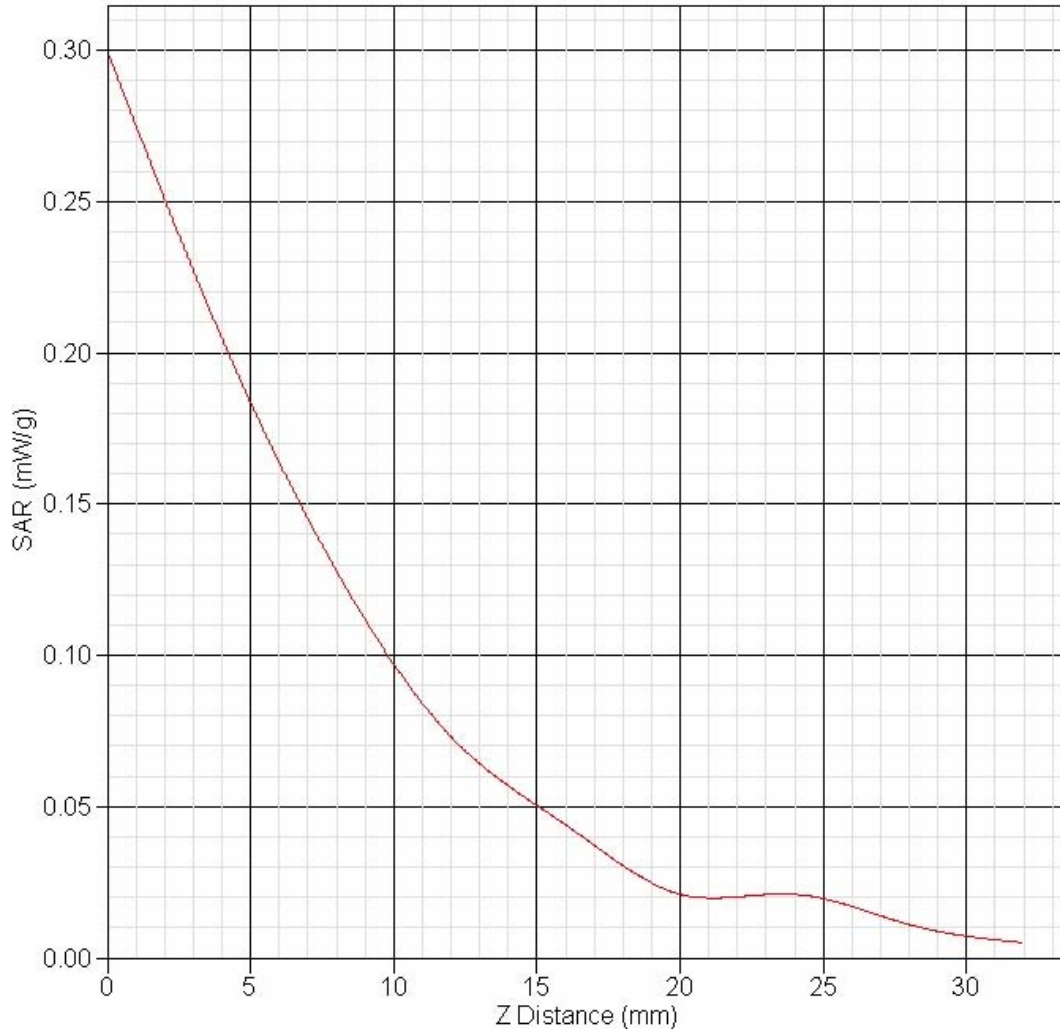

## SAR Test Report

Operator : Chen  
 Validation Date : 19-Apr-2009  
 Measurement Date : 19-Apr-2009  
 Starting Time : 19-Apr-2009 11:20:26 AM  
 End Time : 19-Apr-2009 11:34:27 AM  
 Scanning Time : 841 secs

Product Data  
 Device Name : Dell\_Tahiti\_Hitachi  
 Serial No. : N/A  
 Type : Other  
 Model : Latitude D510  
 Frequency : 2450.00 MHz  
 Max. Transmit Pwr : 0.05 W  
 Drift Time : 0 min(s)  
 Length : 100 mm  
 Width : 150 mm  
 Depth : 30.4 mm  
 Antenna Type : Internal  
 Power Drift-Start : 0.115  
 Power Drift-Finish: 0.110  
 Power Drift (%) : -4.348

Phantom Data  
 Name : APREL-Uni  
 Type : Uni-Phantom  
 Size : 280 x 280 x 200  
 Serial No. : User Define  
 Location : Center  
 Description : User Define Data

Tissue Data  
 Type : BODY  
 Serial No. : 2450  
 Frequency : 2450 MHz  
 Calibration Date : 19-Apr-2005  
 Temperature : 21 °C  
 Ambient Temp. : 22 °C  
 Humidity : 50 RH%  
 Epsilon : 54.12 F/m  
 Sigma : 2.01 S/m  
 Density : 1000 kg/cu. m


Probe Data  
 Name : APREL Probe 212  
 Model : E020  
 Type : E-Field Triangle  
 Serial No. : 212  
 Calibration Date : 27-Dec-2004  
 Frequency : 2450 MHz  
 Duty Cycle Factor: 1  
 Conversion Factor: 5  
 Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
 Compression Point: 95 mV  
 Offset : 1.56

Measurement Data

Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 21 °C  
 Ambient Temp. : 22°C  
 Set-up Date : 19-Apr-2009  
 Set-up Time : 10:54:11 AM

Other Data

DUT Position : Touch  
 Separation : 0  
 Channel : High - 2462

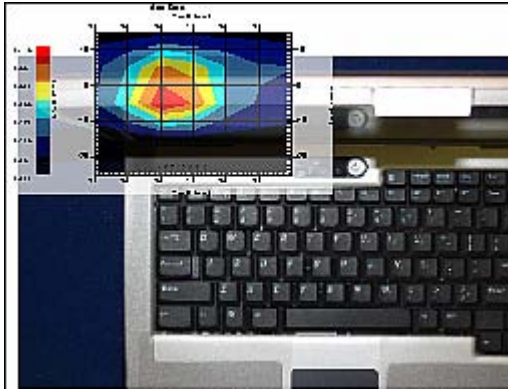

1 gram SAR value : 0.354 W/kg  
 Zoom Scan Peak SAR : 0.720





SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

**Exposure Assessment Measurement Uncertainty**


Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	$c_i^1$ (1-g)	$c_i^1$ (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)^{1/2}$	$(1-cp)^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	-11.3	rectangular	$\sqrt{3}$	1	1	0.0	0.0
Phantom and Setup							
Phantom Uncertainty (shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity (target)	5.0	rectangular	$\sqrt{3}$	0.7	0.5	2.0	1.4
Liquid Conductivity (meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity (target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.7	0.6
Liquid Permittivity (meas.)	5.4	rectangular	$\sqrt{3}$	0.6	0.5	1.9	1.6
Combined Uncertainty		RSS				9.3	9.1
Combined Uncertainty (coverage factor=2)		Normal (k=2)				18.6	18.2





### SAR-Z Axis

at Hotspot x:5.1 y:-49.9

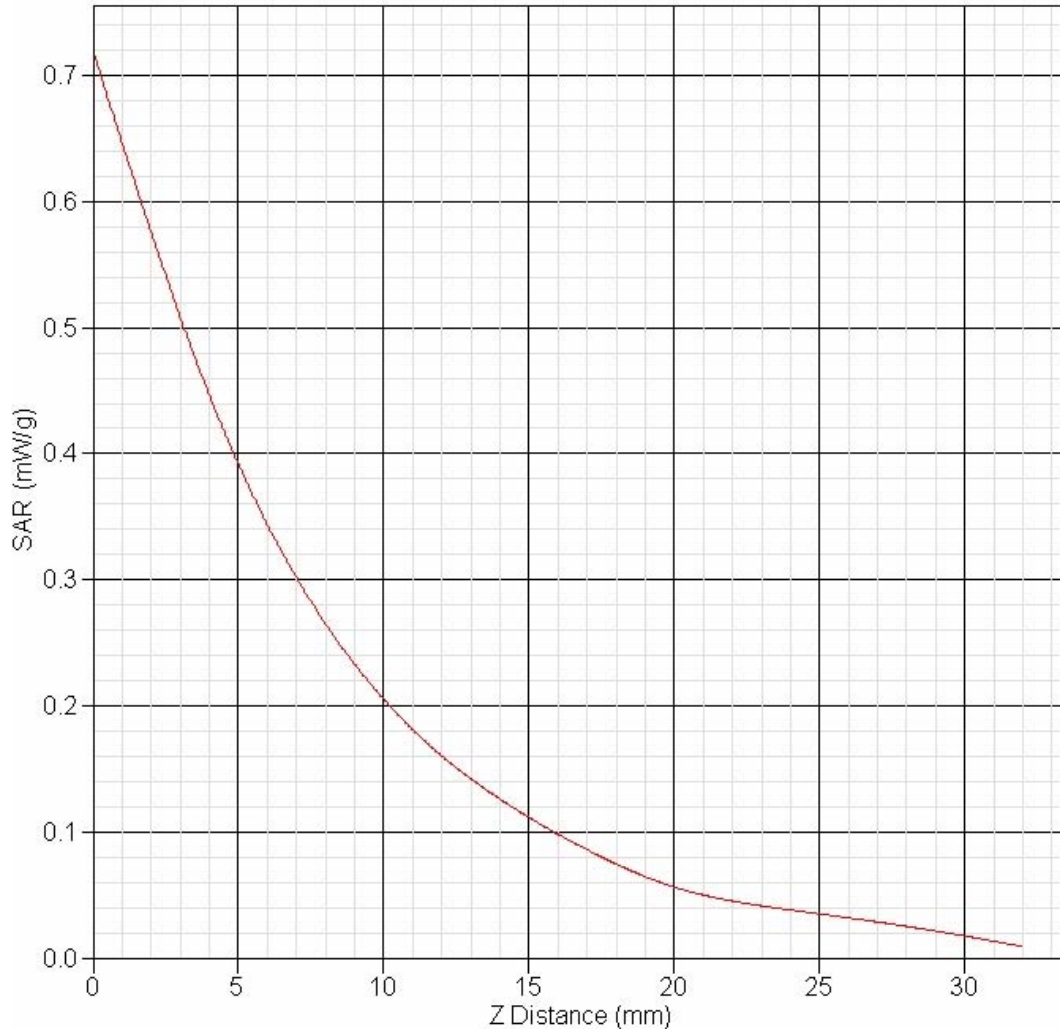

## SAR Test Report

Operator : Chen  
 Validation Date : 19-Apr-2009  
 Measurement Date : 19-Apr-2009  
 Starting Time : 19-Apr-2009 01:21:20 PM  
 End Time : 19-Apr-2009 01:35:19 PM  
 Scanning Time : 839 secs

Product Data  
 Device Name : Dell\_Tahiti\_Hitachi  
 Serial No. : N/A  
 Type : Other  
 Model : Latitude D510  
 Frequency : 2450.00 MHz  
 Max. Transmit Pwr : 0.05 W  
 Drift Time : 0 min(s)  
 Length : 100 mm  
 Width : 150 mm  
 Depth : 30.4 mm  
 Antenna Type : Internal  
 Power Drift-Start : 0.100  
 Power Drift-Finish: 0.097  
 Power Drift (%) : -3.000

Phantom Data  
 Name : APREL-Uni  
 Type : Uni-Phantom  
 Size : 280 x 280 x 200  
 Serial No. : User Define  
 Location : Center  
 Description : User Define Data

Tissue Data  
 Type : BODY  
 Serial No. : 2450  
 Frequency : 2450 MHz  
 Calibration Date : 19-Apr-2005  
 Temperature : 21 °C  
 Ambient Temp. : 22 °C  
 Humidity : 50 RH%  
 Epsilon : 54.12 F/m  
 Sigma : 2.01 S/m  
 Density : 1000 kg/cu. m


Probe Data  
 Name : APREL Probe 212  
 Model : E020  
 Type : E-Field Triangle  
 Serial No. : 212  
 Calibration Date : 27-Dec-2004  
 Frequency : 2450 MHz  
 Duty Cycle Factor: 1  
 Conversion Factor: 5  
 Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
 Compression Point: 95 mV  
 Offset : 1.56

Measurement Data

Crest Factor : 1  
Scan Type : Complete  
Tissue Temp. : 21 °C  
Ambient Temp. : 22°C  
Set-up Date : 19-Apr-2009  
Set-up Time : 10:54:11 AM

Other Data

DUT Position : Touch  
Separation : 0  
Channel : High - 2462

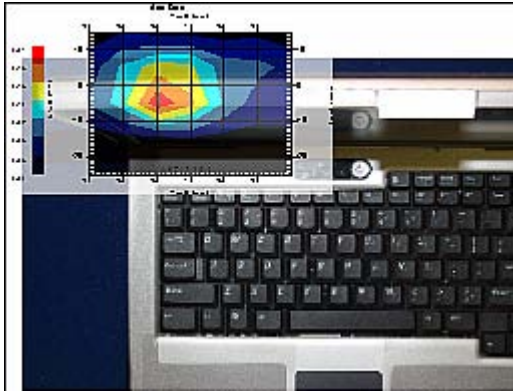

1 gram SAR value : 0.154 W/kg  
Zoom Scan Peak SAR : 0.310






SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

**Exposure Assessment Measurement Uncertainty**

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	$c_i^1$ (1-g)	$c_i^1$ (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)^{1/2}$	$(1-cp)^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	-61.5	rectangular	$\sqrt{3}$	1	1	0.0	0.0
Phantom and Setup							
Phantom Uncertainty (shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity (target)	5.0	rectangular	$\sqrt{3}$	0.7	0.5	2.0	1.4
Liquid Conductivity (meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity (target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.7	0.6
Liquid Permittivity (meas.)	5.4	rectangular	$\sqrt{3}$	0.6	0.5	1.9	1.6
Combined Uncertainty		RSS				9.3	9.1
Combined Uncertainty (coverage factor=2)		Normal (k=2)				18.6	18.2



### SAR-Z Axis at Hotspot x:-2.9 y:-49.9

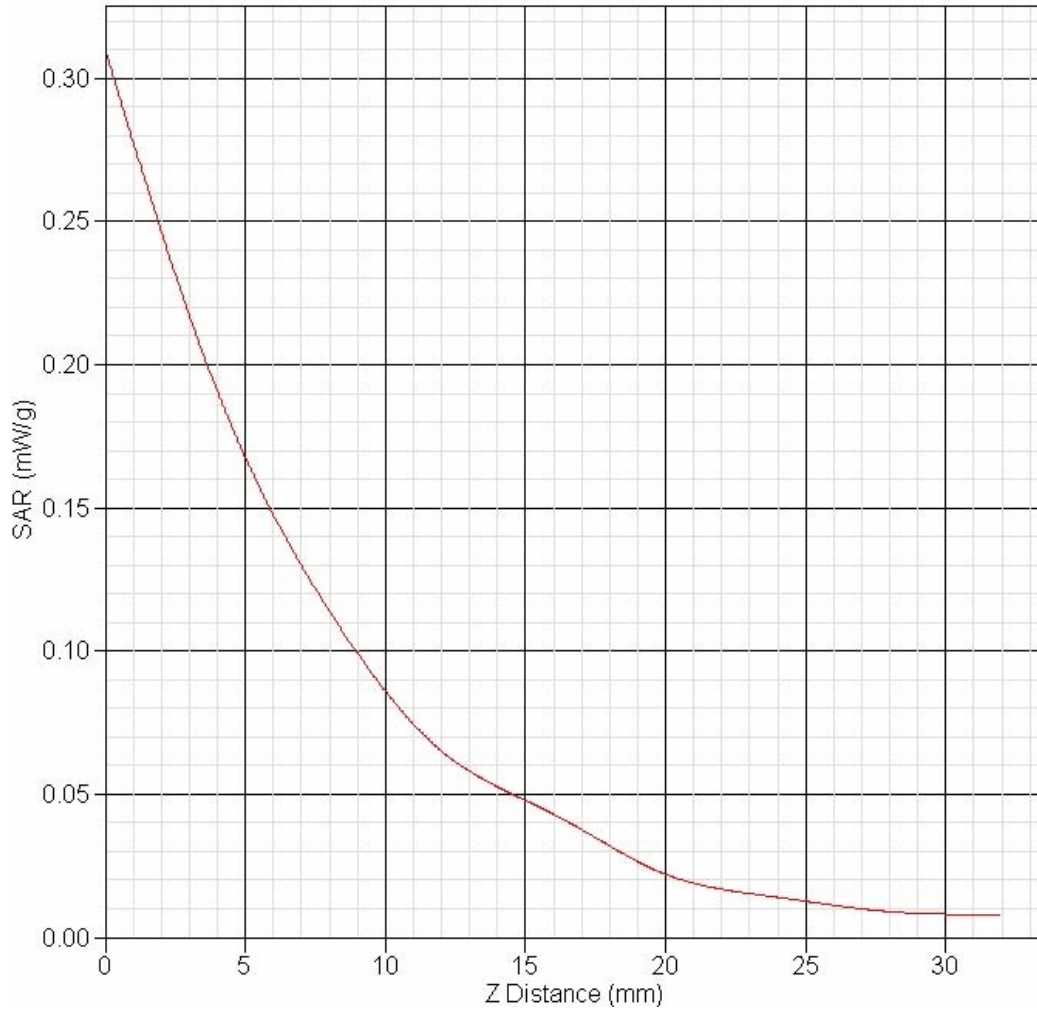



## SAR Test Report

Operator : Chen  
 Validation Date : 20-Apr-2009  
 Measurement Date : 20-Apr-2009  
 Starting Time : 20-Apr-2009 01:45:13 PM  
 End Time : 20-Apr-2009 01:58:18 PM  
 Scanning Time : 785 secs

Product Data  
 Device Name : Dell\_Tahiti\_Hitachi  
 Serial No. : N/A  
 Type : Other  
 Model : Latitude D510  
 Frequency : 2450.00 MHz  
 Max. Transmit Pwr : 0.05 W  
 Drift Time : 0 min(s)  
 Length : 150 mm  
 Width : 120 mm  
 Depth : 30.4 mm  
 Antenna Type : Internal  
 Power Drift-Start : 0.100  
 Power Drift-Finish: 0.098  
 Power Drift (%) : -2.503

Phantom Data  
 Name : APREL-Uni  
 Type : Uni-Phantom  
 Size : 280 x 280 x 200  
 Serial No. : User Define  
 Location : Center  
 Description : User Define Data


Tissue Data  
 Type : BODY  
 Serial No. : 2450  
 Frequency : 2450 MHz  
 Calibration Date : 20-Apr-2005  
 Temperature : 21 °C  
 Ambient Temp. : 22 °C  
 Humidity : 50 RH%  
 Epsilon : 54.12 F/m  
 Sigma : 2.01 S/m  
 Density : 1000 kg/cu. m

Probe Data  
 Name : APREL Probe 212  
 Model : E020  
 Type : E-Field Triangle  
 Serial No. : 212  
 Calibration Date : 27-Dec-2004  
 Frequency : 2450 MHz  
 Duty Cycle Factor: 1  
 Conversion Factor: 5  
 Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
 Compression Point: 95 mV  
 Offset : 1.56



Measurement Data  
 Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 21 °C  
 Ambient Temp. : 22°C  
 Set-up Date : 19-Apr-2009  
 Set-up Time : 10:54:11 AM

Other Data  
 DUT Position : Touch  
 Separation : 0  
 Channel : Mid - 2437

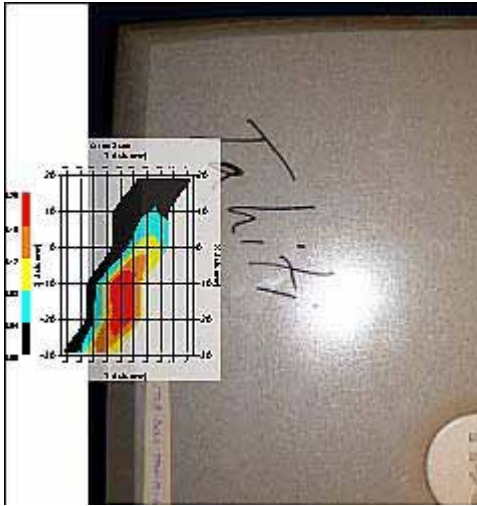

1 gram SAR value : 0.185 W/kg  
 Zoom Scan Peak SAR : 0.360






SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

**Exposure Assessment Measurement Uncertainty**

Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	$c_i^1$ (1-g)	$c_i^1$ (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)^{1/2}$	$(1-cp)^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	-92.5	rectangular	$\sqrt{3}$	1	1	0.0	0.0
Phantom and Setup							
Phantom Uncertainty (shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity (target)	5.0	rectangular	$\sqrt{3}$	0.7	0.5	2.0	1.4
Liquid Conductivity (meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity (target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.7	0.6
Liquid Permittivity (meas.)	5.4	rectangular	$\sqrt{3}$	0.6	0.5	1.9	1.6
Combined Uncertainty		RSS				9.3	9.1
Combined Uncertainty (coverage factor=2)		Normal (k=2)				18.6	18.2



### SAR-Z Axis at Hotspot x:12.1 y:-72.9

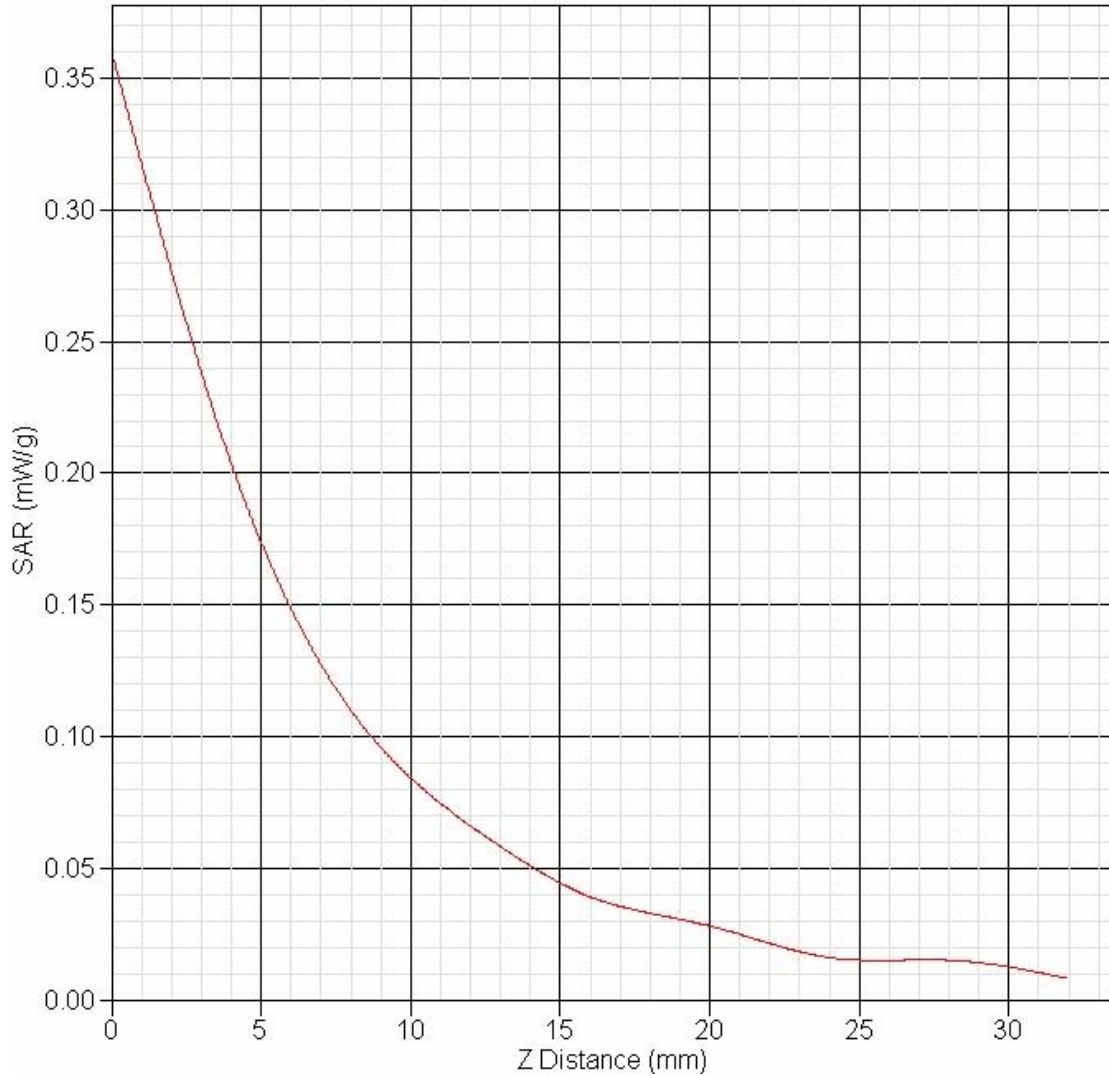

## SAR Test Report

Operator : Chen  
 Validation Date : 20-Apr-2009  
 Measurement Date : 20-Apr-2009  
 Starting Time : 20-Apr-2009 02:20:33 PM  
 End Time : 20-Apr-2009 02:33:38 PM  
 Scanning Time : 785 secs

Product Data  
 Device Name : Dell\_Tahiti\_Hitachi  
 Serial No. : N/A  
 Type : Other  
 Model : Latitude D510  
 Frequency : 2450.00 MHz  
 Max. Transmit Pwr : 0.05 W  
 Drift Time : 0 min(s)  
 Length : 150 mm  
 Width : 120 mm  
 Depth : 30.4 mm  
 Antenna Type : Internal  
 Power Drift-Start : 0.100  
 Power Drift-Finish: 0.104  
 Power Drift (%) : 4.000


Phantom Data  
 Name : APREL-Uni  
 Type : Uni-Phantom  
 Size : 280 x 280 x 200  
 Serial No. : User Define  
 Location : Center  
 Description : User Define Data

Tissue Data  
 Type : BODY  
 Serial No. : 2450  
 Frequency : 2450 MHz  
 Calibration Date : 20-Apr-2005  
 Temperature : 21 °C  
 Ambient Temp. : 22 °C  
 Humidity : 50 RH%  
 Epsilon : 54.12 F/m  
 Sigma : 2.01 S/m  
 Density : 1000 kg/cu. m

Probe Data  
 Name : APREL Probe 212  
 Model : E020  
 Type : E-Field Triangle  
 Serial No. : 212  
 Calibration Date : 27-Dec-2004  
 Frequency : 2450 MHz  
 Duty Cycle Factor: 1  
 Conversion Factor: 5  
 Probe Sensitivity: 1.20 1.20 1.20  $\mu\text{V}/(\text{V}/\text{m})^2$   
 Compression Point: 95 mV  
 Offset : 1.56

Measurement Data  
 Crest Factor : 1  
 Scan Type : Complete  
 Tissue Temp. : 21 °C  
 Ambient Temp. : 22°C  
 Set-up Date : 19-Apr-2009  
 Set-up Time : 10:54:11 AM

Other Data  
 DUT Position : Touch  
 Separation : 0  
 Channel : Low - 2412

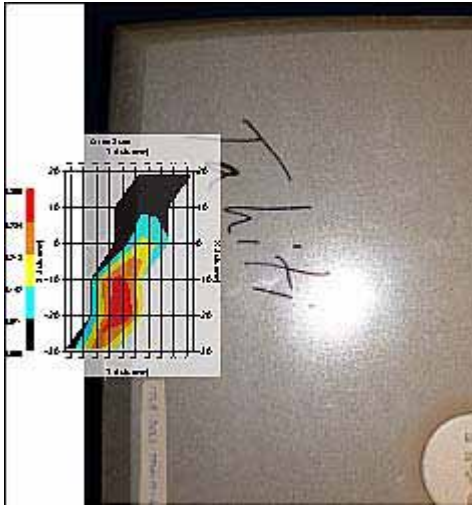

1 gram SAR value : 0.328 W/kg  
 Zoom Scan Peak SAR : 0.670







SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

**Exposure Assessment Measurement Uncertainty**


Source of Uncertainty	Tolerance Value	Probability Distribution	Divisor	$c_i^{-1}$ (1-g)	$c_i^{-1}$ (10-g)	Standard Uncertainty (1-g)	Standard Uncertainty (10-g)
Measurement System							
Probe Calibration	3.5	normal	1	1	1	3.5	3.5
Axial Isotropy	3.7	rectangular	$\sqrt{3}$	$(1-cp)^{1/2}$	$(1-cp)^{1/2}$	1.5	1.5
Hemispherical Isotropy	10.9	rectangular	$\sqrt{3}$	$\sqrt{cp}$	$\sqrt{cp}$	4.4	4.4
Boundary Effect	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Linearity	4.7	rectangular	$\sqrt{3}$	1	1	2.7	2.7
Detection Limit	1.0	rectangular	$\sqrt{3}$	1	1	0.6	0.6
Readout Electronics	1.0	normal	1	1	1	1.0	1.0
Response Time	0.8	rectangular	$\sqrt{3}$	1	1	0.5	0.5
Integration Time	1.7	rectangular	$\sqrt{3}$	1	1	1.0	1.0
RF Ambient Condition	3.0	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Probe Positioner Mech.	0.4	rectangular	$\sqrt{3}$	1	1	0.2	0.2
Restriction							
Probe Positioning with respect to Phantom Shell	2.9	rectangular	$\sqrt{3}$	1	1	1.7	1.7
Extrapolation and Integration	3.7	rectangular	$\sqrt{3}$	1	1	2.1	2.1
Test Sample Positioning	4.0	normal	1	1	1	4.0	4.0
Device Holder Uncertainty	2.0	normal	1	1	1	2.0	2.0
Drift of Output Power	-95.9	rectangular	$\sqrt{3}$	1	1	0.0	0.0
Phantom and Setup							
Phantom Uncertainty (shape & thickness tolerance)	3.4	rectangular	$\sqrt{3}$	1	1	2.0	2.0
Liquid Conductivity (target)	5.0	rectangular	$\sqrt{3}$	0.7	0.5	2.0	1.4
Liquid Conductivity (meas.)	0.2	rectangular	$\sqrt{3}$	0.7	0.5	0.1	0.1
Liquid Permittivity (target)	2.0	rectangular	$\sqrt{3}$	0.6	0.5	0.7	0.6
Liquid Permittivity (meas.)	5.4	rectangular	$\sqrt{3}$	0.6	0.5	1.9	1.6
Combined Uncertainty		RSS				9.3	9.1
Combined Uncertainty (coverage factor=2)		Normal (k=2)				18.6	18.2





## SAR-Z Axis

at Hotspot x:20.1 y:-74.9

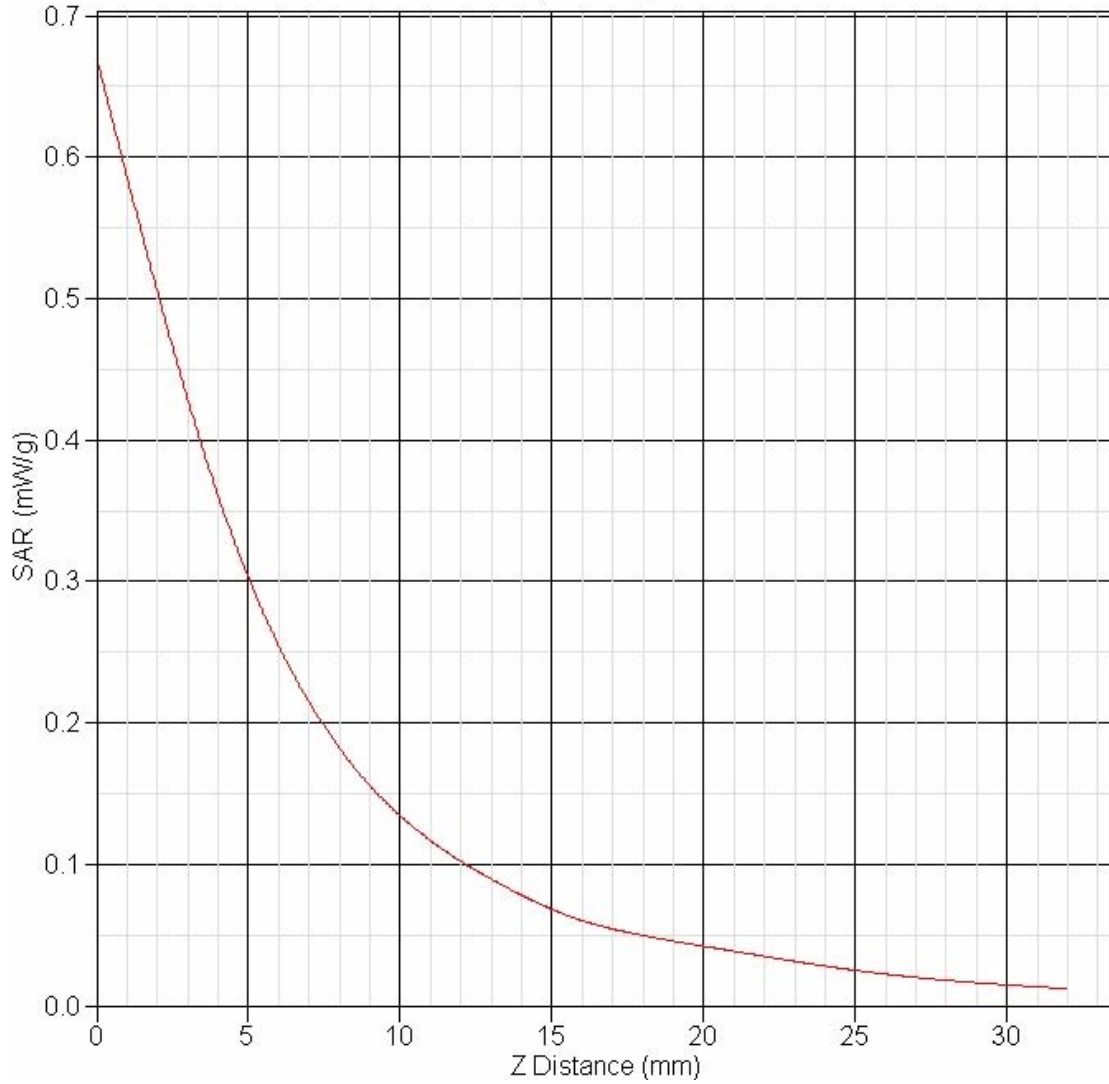



SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

## Appendix B Probe Calibration Certificate





SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

**NCL CALIBRATION LABORATORIES**

Calibration File No.: CP-469

Client.: APREL

**CERTIFICATE OF CALIBRATION**

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5800 MHz

Manufacturer: APREL Laboratories

Model No.: E-020

Serial No.: 212

Body Calibration

Calibration Procedure: SSI/DRB-TP-D01-032-E020-V2

Project No: Internal

Calibrated: 27<sup>th</sup> December 2004

Released on: 27<sup>th</sup> December 2004

This Calibration Certificate is Incomplete Unless Accompanied with the Calibration Results Summary

Released By: \_\_\_\_\_

**NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161



## Introduction

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-020 212.

## References

SSI/DRB-TP-D01-032-E020-V2 E-Field Probe Calibration Procedure  
 IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
 SSI-TP-011 Tissue Calibration Procedure

## Conditions

Probe 212 was a new probe taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 22 °C +/- 0.5°C  
**Temperature of the Tissue:** 21 °C +/- 0.5°C

## Calibration Results Summary

<b>Probe Type:</b>	E-Field Probe E-020
<b>Serial Number:</b>	212
<b>Frequency:</b>	2450 MHz
<b>Sensor Offset:</b>	1.56 mm
<b>Sensor Length:</b>	2.5 mm
<b>Tip Enclosure:</b>	Ertalyte*
<b>Tip Diameter:</b>	5 mm
<b>Tip Length:</b>	60 mm
<b>Total Length:</b>	290 mm

\*Resistive to recommended tissue recipes per IEEE-1528

#### Sensitivity in Air

<b>Channel X:</b>	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Y:</b>	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Z:</b>	$1.2 \mu\text{V}/(\text{V}/\text{m})^2$
<b>Diode Compression Point:</b>	95 mV

#### Sensitivity in Body Tissue



**Frequency:** 2450 MHz

**Epsilon:** 50.6 (+/-5%)      **Sigma:** 2.01 S/m (+/-10%)

**ConvF****Channel X:** 5.0**Channel Y:** 5.0**Channel Z:** 5.0

Tissue sensitivity values were calculated using the load impedance of the APREL Laboratories Daq-Paq.

**Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.4mm.


**Spatial Resolution:**

The measured probe tip diameter is 5 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.



**Receiving Pattern 2450 MHz (Air)**



Receiving Pattern Probe s/n 212 24500MHz

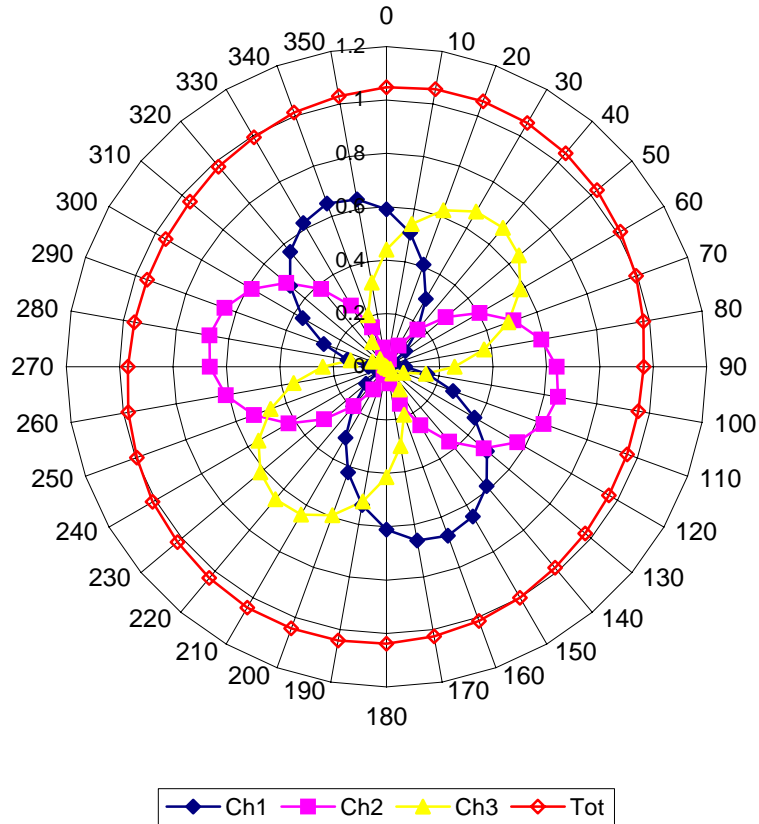


## Isotropy Error 2450 MHz (Air)

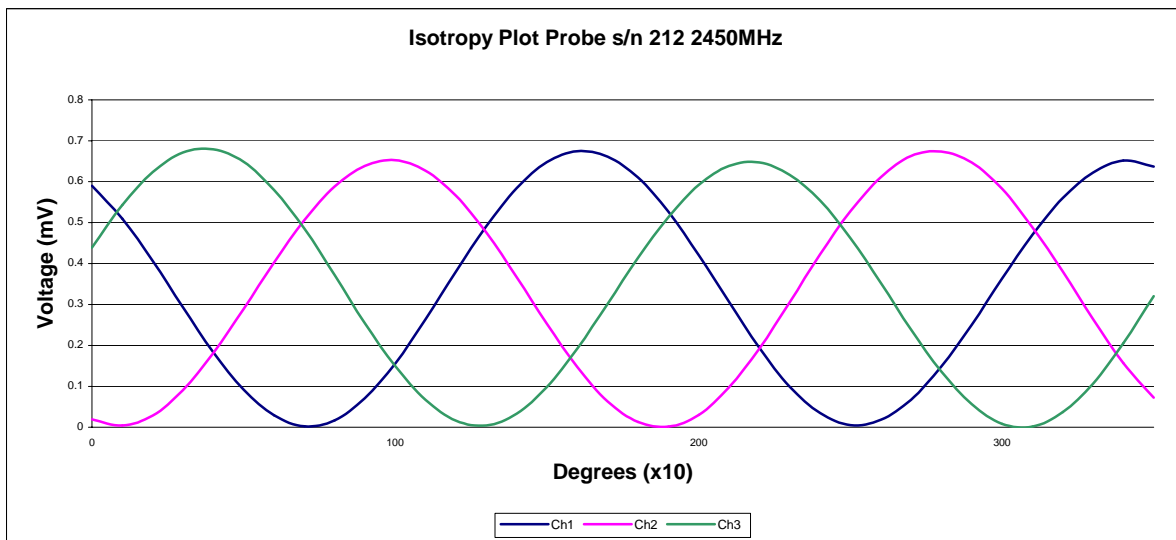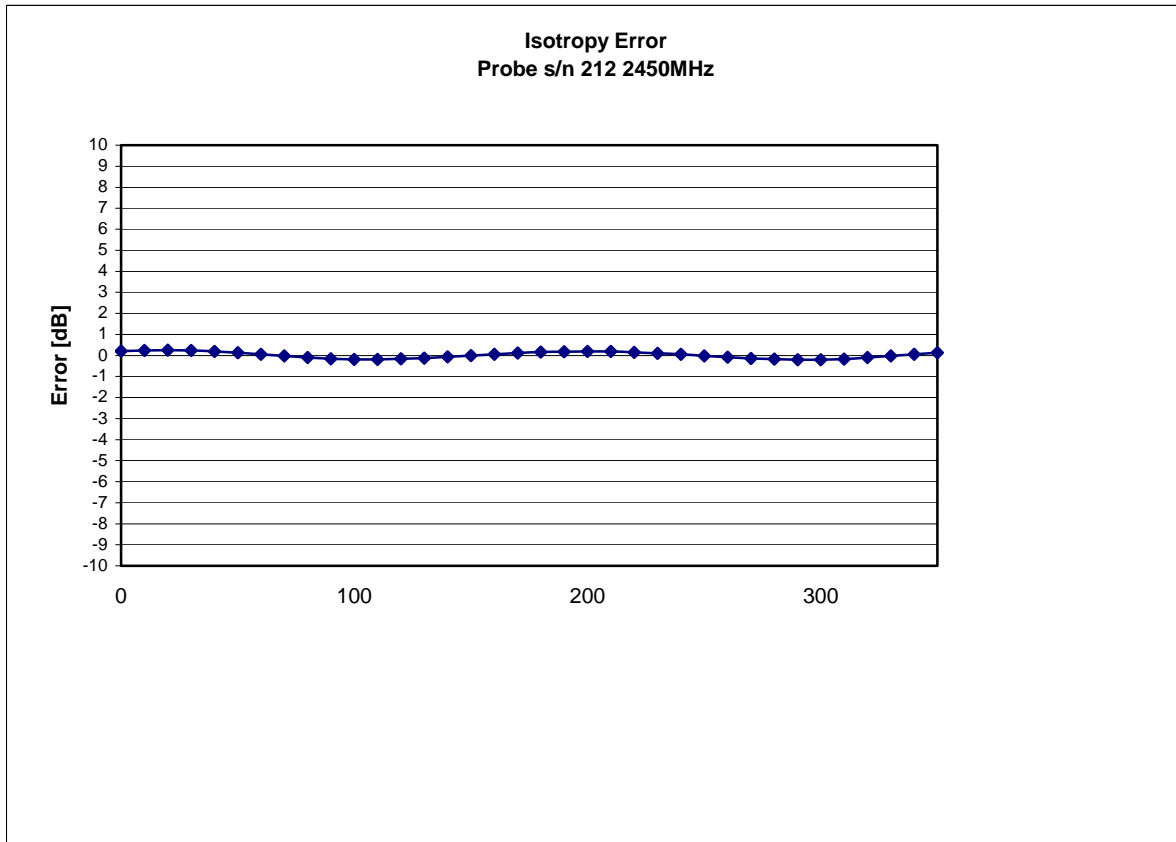

**Isotropy:** 0.10 dB




## Dynamic Range

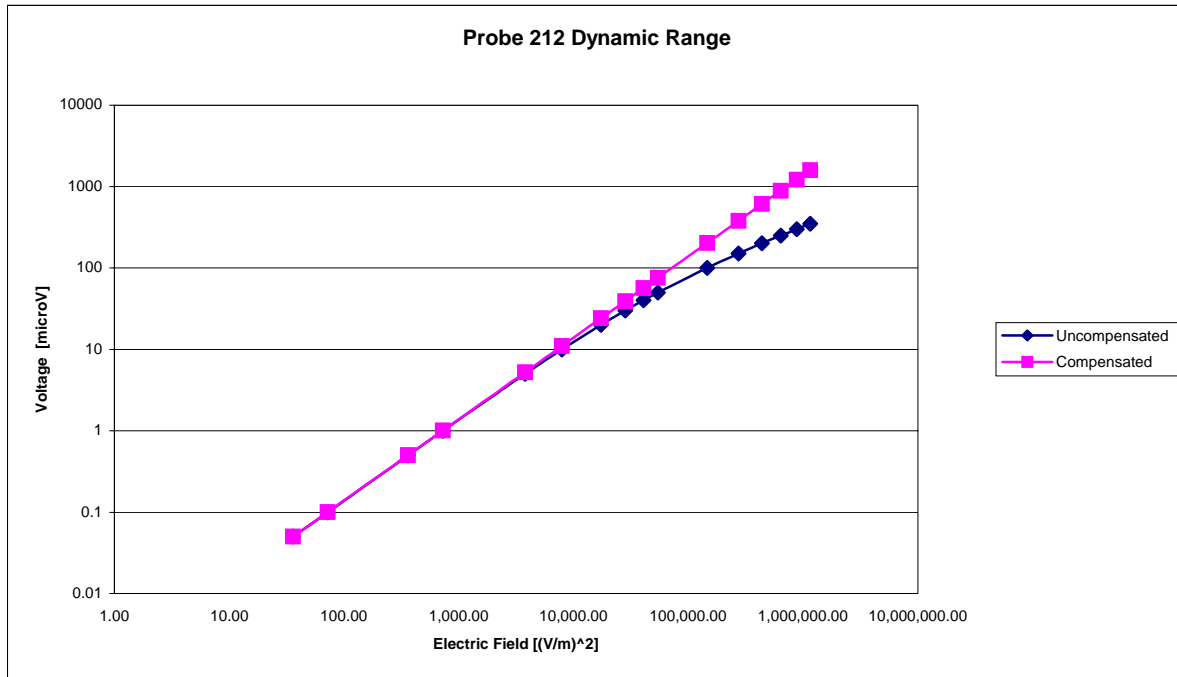

## Video Bandwidth

### Probe Frequency Characteristics

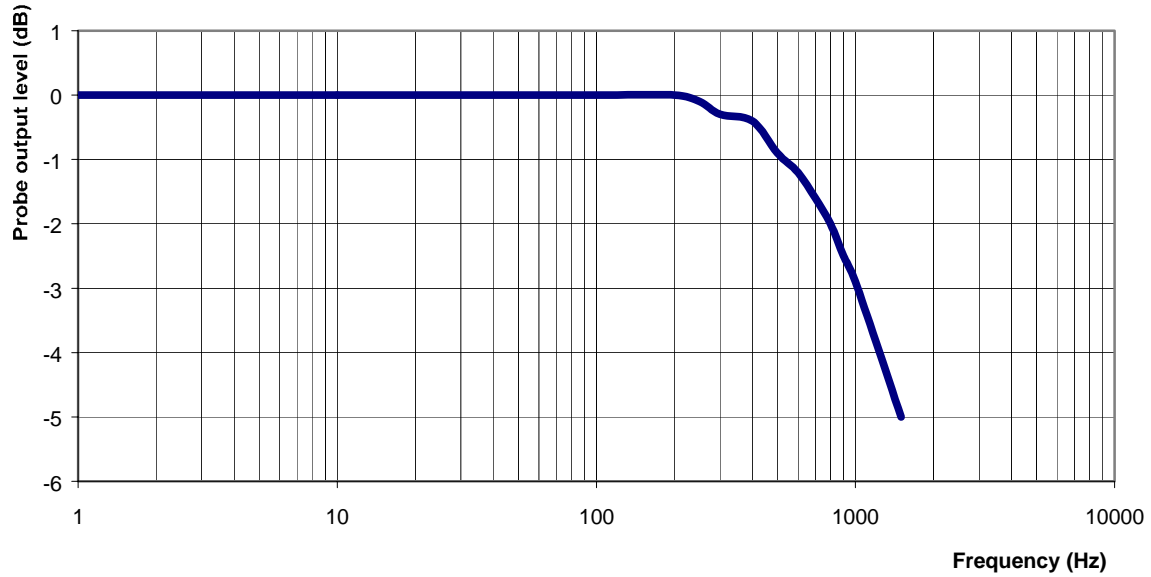

Video Bandwidth at 500 Hz      1 dB  
Video Bandwidth at 1.02 KHz:   3 dB



## Conversion Factor Uncertainty Assessment

**Frequency:** 2450MHz

**Epsilon:** 50.6 (+/-5%)      **Sigma:** 2.01 S/m (+/-10%)

### ConvF

**Channel X:** 5.0    7%(K=2)

**Channel Y:** 5.0    7%(K=2)

**Channel Z:** 5.0    7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 MΩ.

### Boundary Effect:

For a distance of 2.4mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.



SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

## Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2004.







SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

## Appendix C Dipole Calibration Certificate





SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

**NCL CALIBRATION LABORATORIES**

Calibration File No: DC-0265  
Project Number: Internal

**CERTIFICATE OF CALIBRATION**

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

APREL Validation Dipole

Manufacturer: APREL Laboratories  
Part number: D-2450-S-1  
Frequency: 2.45 GHz  
Serial No: ALCD-10

Customer: APREL

Calibrated: 14 November 2003  
Released on: 15 November 2003

Released By: \_\_\_\_\_

**NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161



## Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

### Mechanical Dimensions


**Length:** 51.7 mm  
**Height:** 30.8 mm

### Electrical Specification

**SWR:** 1.181U  
**Return Loss:** -21.4 dB  
**Impedance:** 46.175

### System Validation Results

Frequency	1 Gram	10 Gram	Peak
2.45 GHz	52.45	22.91	102.91

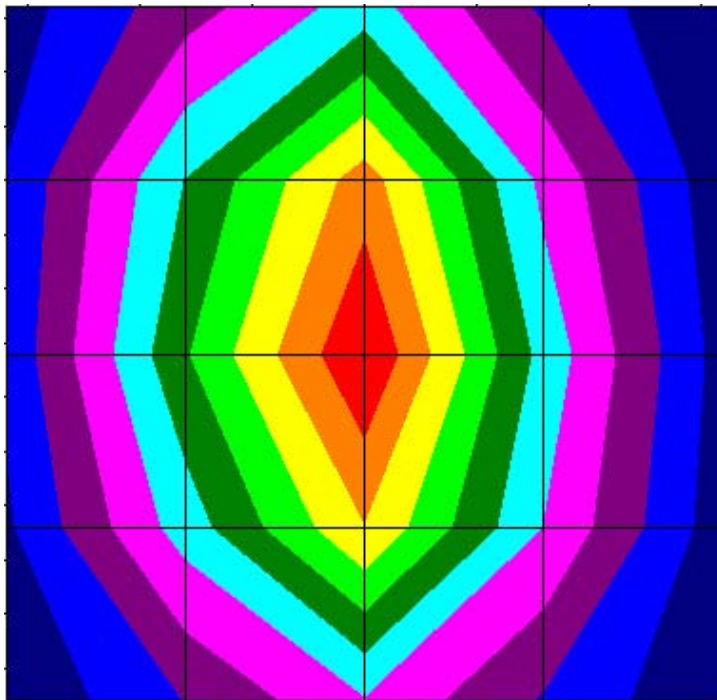

## Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018. The results contained within this report are for Validation Dipole ALCD-10 at 2.45 GHz. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the IEEE mechanical specification. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALIDX-500, along with the APREL Reference E-010 130 MHz to 26 GHz E-Field Probe Serial Number 163.

## References

SSI-TP-018 Dipole Calibration Procedure  
 SSI-TP-016 Tissue Calibration Procedure  
 IEEE 1528 *DRAFT* "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

## Conditions

Dipole ALCD-10 was a new Dipole taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 24 °C +/- 0.5°C  
**Temperature of the Tissue:** 20 °C +/- 0.5°C

## Dipole Calibration Results

### Mechanical Verification

IEEE Length	IEEE Height	Measured Length	Measured Height
51.5 mm	30.4 mm	51.7 mm	30.8 mm

### Tissue Validation

Head Tissue 2450 MHz	Measured
Dielectric constant, $\epsilon_r$	39.2
Conductivity, $\sigma$ [S/m]	1.82
Tissue Conversion Factor,	4.61



## Electrical Calibration


Test	Result	IEEE Value
S11 R/L	-21.4	-21 dB
SWR	1.181U	-
Impedance	46.175 Ω	

The Following Graphs are the results as displayed on the Vector Network Analyzer.

### S11 Parameter Return Loss

S11 FORWARD REFLECTION

LOG MAGNITUDE      REF=0.000 dB      10.000 dB/DIV

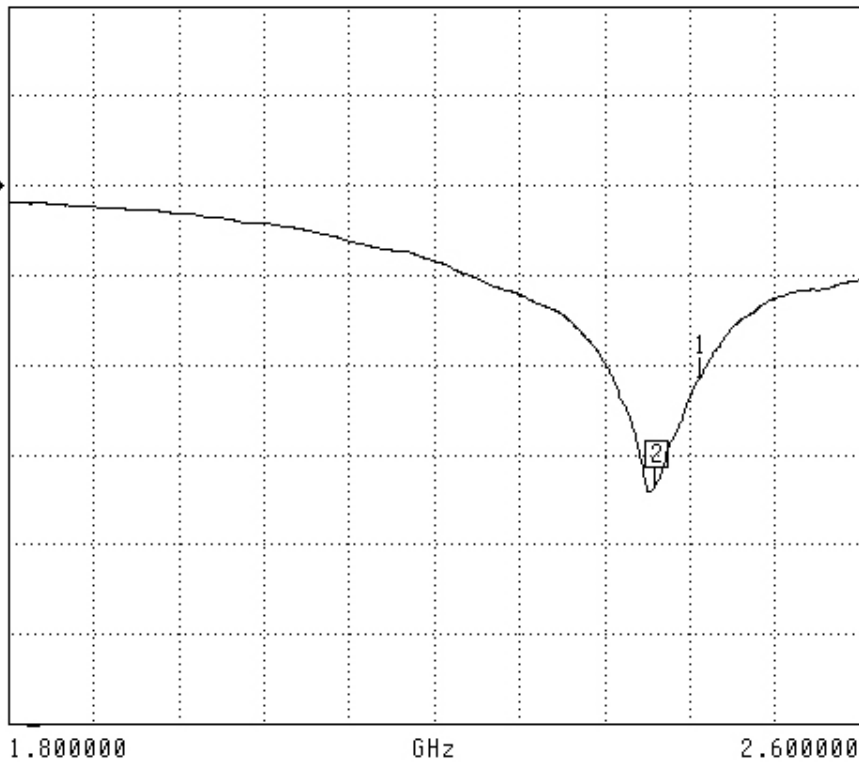

CH 1 - S11  
REFERENCE PLANE  
5.1160 mm

MARKER 2  
2.408000 GHz  
-33.566 dB

MARKER TO MAX  
▶ MARKER TO MIN  
**1** 2.450000 GHz  
-21.377 dB

MARKER READOUT  
FUNCTIONS






## SWR

S11 FORWARD REFLECTION

SWR

REF=1.000 U

5.000 U/DIV

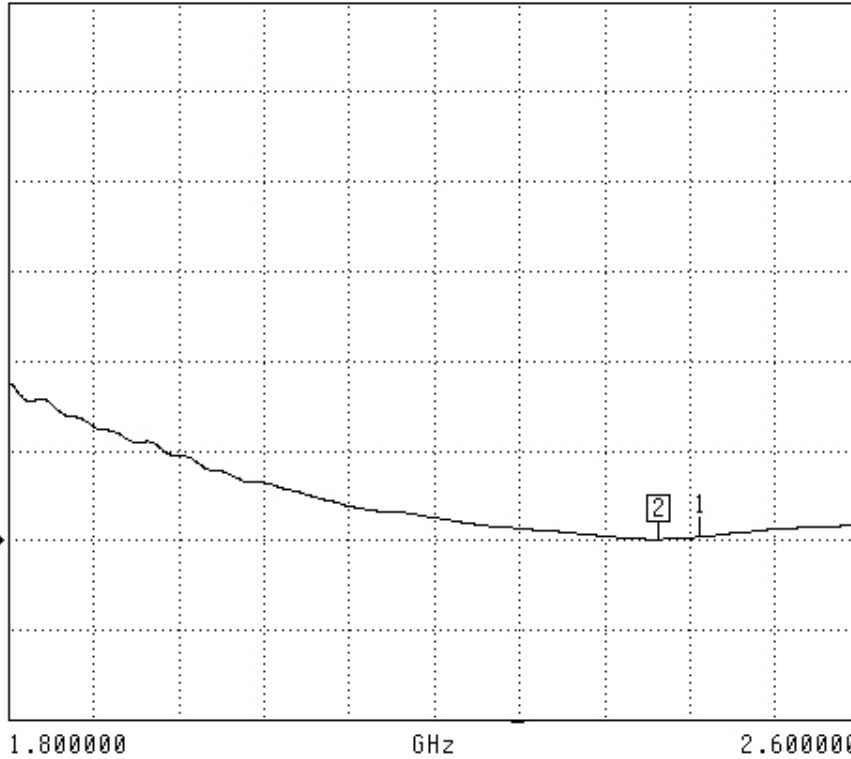

CH 1 - S11  
REFERENCE PLANE  
5.1160 mm

MARKER 2  
2.411000 GHz  
1.049 U


MARKER TO MAX  
▶ MARKER TO MIN  
**1** 2.450000 GHz  
1.181 U

MARKER READOUT  
FUNCTIONS



## Smith Chart Dipole Impedance

S11 FORWARD REFLECTION  
IMPEDANCE

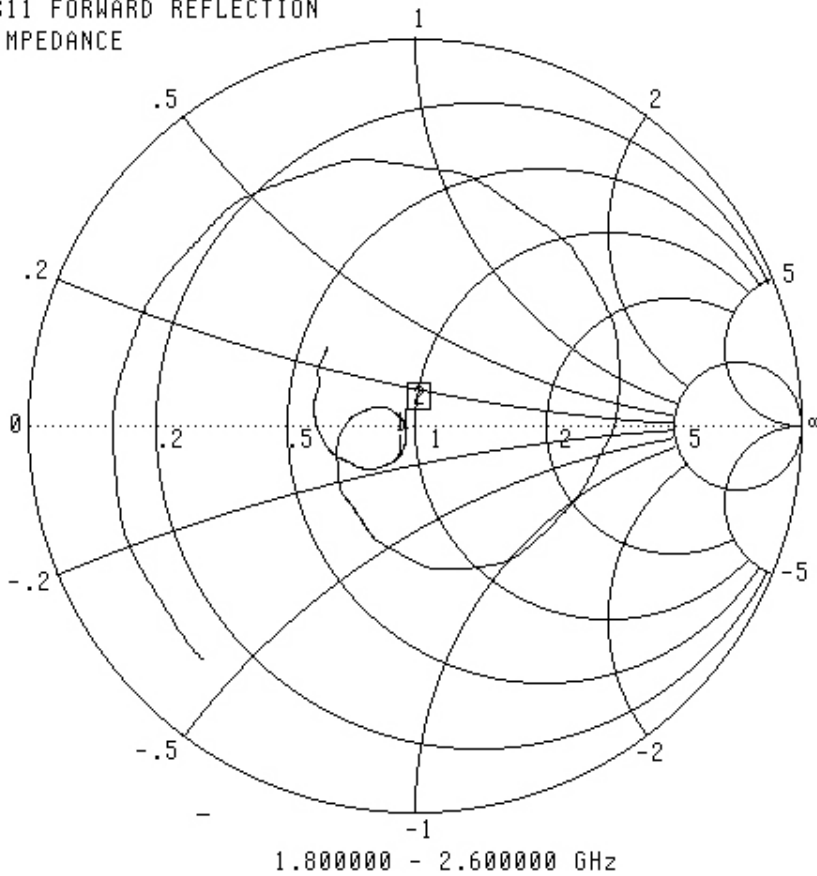

CH 1 - S11  
REFERENCE PLANE  
5.1160 mm

MARKER 2  
2.411000 GHz  
48.080 Ω  
-1.171 jΩ

MARKER TO MAX  
▶ MARKER TO MIN

**1** 2.450000 GHz  
46.175 Ω  
-7.199 jΩ


MARKER READOUT  
FUNCTIONS



## System Validation Results Using the Electrically Calibrated Dipole

Frequency	1 Gram	10 Gram	Peak Above Feed Point
2.45 GHz	52.45	22.91	102.91

The following Graphic Plot is the splined measurement result for the course scan.

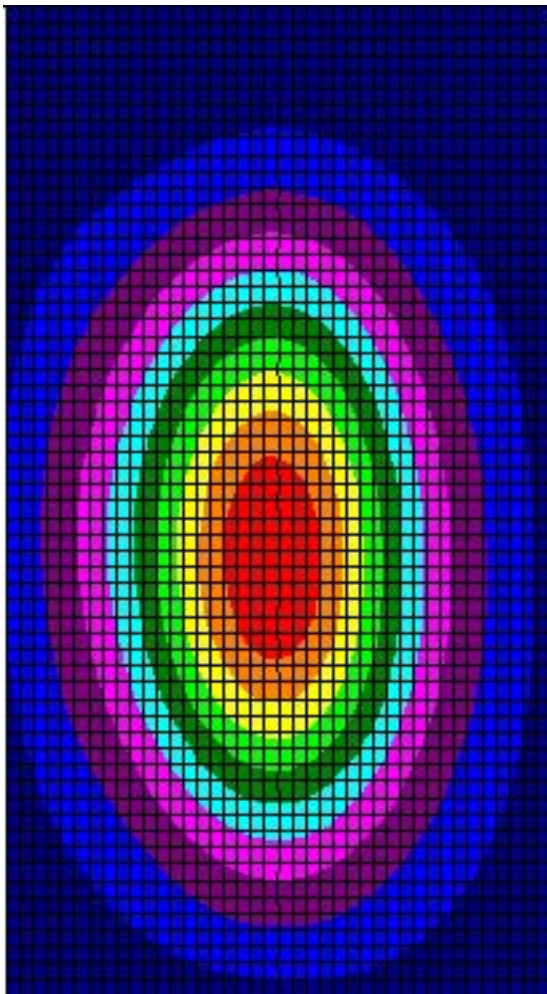



SAR & HAC Instruments for Wireless • Consulting • Research • Standards • Compliance • Training

## Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2004.

