Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client EMC Technologies

Certificate No: D5GHzV2-1008_Dec07

Object	D5GHzV2 - SN:	1008	
Calibration procedure(s)	QA CAL-22.v1 Calibration proce	dure for dipole validation kits between	en 3-6 GHz
Calibration date:	December 07, 20	007	
Condition of the calibrated item	In Tolerance		
Calibration Equipment used (M&	TE critical for calibration)	y facility: environment temperature (22 ± 3)°C and	
Calibration Equipment used (M& Primary Standards	TE critical for calibration)	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Calibration Equipment used (M& Primary Standards Power meter EPM-442A	TE critical for calibration) ID # GB37480704	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736)	Scheduled Calibration Oct-08
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	ID # GB37480704 US37292783	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736)	Scheduled Calibration Oct-08 Oct-08
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	ID # GB37480704 US37292783 SN: S5072.1 (20g)	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718)	Scheduled Calibration Oct-08
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe EX3DV4	ID # GB37480704 US37292783	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736)	Scheduled Calibration Oct-08 Oct-08 Aug-08
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe EX3DV4 DAE4	ID # GB37480704 US37292783 SN: S5072.1 (20g) SN: 3503	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718) 9-Mar-07 (SPEAG, No. EX3-3503_Mar07)	Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-08
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe EX3DV4 DAE4	ID # GB37480704 US37292783 SN: S5072.1 (20g) SN: 3503 SN 601 ID # 100005	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718) 9-Mar-07 (SPEAG, No. EX3-3503_Mar07) 30-Jan-07 (SPEAG, No. DAE4-601_Jan07) Check Date (in house) 4-Aug-99 (SPEAG, in house check Oct-07)	Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-08 Jan-08 Scheduled Check In house check: Oct-09
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E	ID # GB37480704 US37292783 SN: S5072.1 (20g) SN: 3503 SN 601 ID # 100005 US37390585 S4206	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718) 9-Mar-07 (SPEAG, No. EX3-3503_Mar07) 30-Jan-07 (SPEAG, No. DAE4-601_Jan07) Check Date (in house) 4-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07)	Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-08 Jan-08 Scheduled Check In house check: Oct-09 In house check: Oct-08
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E Power meter E4419B	ID # GB37480704 US37292783 SN: S5072.1 (20g) SN: 3503 SN 601 ID # 100005	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718) 9-Mar-07 (SPEAG, No. EX3-3503_Mar07) 30-Jan-07 (SPEAG, No. DAE4-601_Jan07) Check Date (in house) 4-Aug-99 (SPEAG, in house check Oct-07)	Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-08 Jan-08 Scheduled Check In house check: Oct-09
	ID # GB37480704 US37292783 SN: S5072.1 (20g) SN: 3503 SN 601 ID # 100005 US37390585 S4206 GB43310788	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 9-Mar-07 (SPEAG, No. EX3-3503_Mar07) 30-Jan-07 (SPEAG, No. DAE4-601_Jan07) Check Date (in house) 4-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 13-Aug-03 (SPEAG, in house check Oct-07)	Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-08 Jan-08 Scheduled Check In house check: Oct-09 In house check: Oct-08 In house check: Oct-08
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E Power meter E4419B	ID # GB37480704 US37292783 SN: S5072.1 (20g) SN: 3503 SN 601 ID # 100005 US37390585 S4206 GB43310788	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 9-Mar-07 (SPEAG, No. EX3-3503_Mar07) 30-Jan-07 (SPEAG, No. DAE4-601_Jan07) Check Date (in house) 4-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 13-Aug-03 (SPEAG, in house check Oct-07)	Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-08 Jan-08 Scheduled Check In house check: Oct-09 In house check: Oct-08 In house check: Oct-08
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E Power meter E4419B	ID # GB37480704 US37292783 SN: S5072.1 (20g) SN: 3503 SN 601 ID # 100005 US37390585 S4206 GB43310788 MY41093315	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No 217-00718) 9-Mar-07 (SPEAG, No. EX3-3503_Mar07) 30-Jan-07 (SPEAG, No. DAE4-601_Jan07) Check Date (in house) 4-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 13-Aug-03 (SPEAG, in house check Oct-07) 10-Aug-03 (SPEAG, in house check Oct-07)	Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-08 Jan-08 Scheduled Check In house check: Oct-09 In house check: Oct-08 In house check: Oct-08 In house check: Oct-08

Certificate No: D5GHzV2-1008_Dec07

Page 1 of 8





Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC Std 62209 Part 2, "Evaluation of Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices in the Frequency Range of 30 MHz to 6 GHz: Human models, Instrumentation, and Procedures"; Part 2: "Procedure to determine the Specific Absorption Rate (SAR) for including accessories and multiple transmitters", Draft Version 0.9, December 2004
- b) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

c) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
 No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D5GHzV2-1008_Dec07 Page 2 of 8





Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Area Scan resolution	dx, dy = 10 mm	
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 2.5 mm	
Frequency	5200 MHz ± 1 MHz 5500 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Head TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.0 ± 6 %	4.51 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C		-

SAR result with Head TSL at 5200 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	100 mW input power	7.76 mW/g
SAR normalized	normalized to 1W	77.6 mW/g
SAR for nominal Head TSL parameters ¹	normalized to 1W	77.6 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.19 mW/g
SAR normalized	normalized to 1W	21.9 mW/g
SAR for nominal Head TSL parameters ¹	normalized to 1W	21.8 mW / g ± 19.5 % (k=2)

Certificate No: D5GHzV2-1008_Dec07

Page 3 of 8





Head TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.5 ± 6 %	4.81 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C		

SAR result with Head TSL at 5500 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	100 mW input power	7.98 mW / g
SAR normalized	normalized to 1W	79.8 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	79.7 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.23 mW / g
SAR normalized	normalized to 1W	22.3 mW/g
SAR for nominal Head TSL parameters ¹	normalized to 1W	22.2 mW / g ± 19.5 % (k=2)

Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.02 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C		

SAR result with Head TSL at 5800 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	100 mW input power	7.63 mW / g
SAR normalized	normalized to 1W	76.3 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	75.7 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.12 mW / g
SAR normalized	normalized to 1W	21.2 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	21.0 mW / g ± 19.5 % (k=2)

Certificate No: D5GHzV2-1008_Dec07 Page 4 of 8





¹ Correction to nominal TSL parameters according to c), chapter "SAR Sensitivities"

Appendix

Antenna Parameters with Head TSL at 5200 MHz

Impedance, transformed to feed point	53.2 Ω - 13.5 jΩ	
Return Loss	-17.5 dB	

Antenna Parameters with Head TSL at 5500 MHz

Impedance, transformed to feed point	46.8 Ω - 5.3 jΩ
Return Loss	-24.0 dB

Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	55.2 Ω + 5.1 jΩ	
Return Loss	-23.2 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.200 ns	
----------------------------------	----------	--

After long term use with 40 W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	August 28, 2003









DASY4 Validation Report for Head TSL

Date/Time: 07.12.2007 13:06:45

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1008

Communication System: CW-5GHz; Frequency: 5200 MHz Frequency: 5500 MHz Frequency: 5800 MHz;

Duty Cycle: 1:1

Medium: HSL 5800 MHz;

Medium parameters used: f = 5200 MHz; $\sigma = 4.51$ mho/m; $\epsilon_r = 36$; $\rho = 1000$ kg/m³ Medium parameters used: f = 5500 MHz; $\sigma = 4.81$ mho/m; $\epsilon_r = 35.5$; $\rho = 1000$ kg/m³ Medium parameters used: f = 5800 MHz; $\sigma = 5.02$ mho/m; $\epsilon_r = 34.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: EX3DV4 SN3503; ConvF(5.56, 5.56, 5.56) ConvF(5.2, 5.2, 5.2) ConvF(4.97, 4.97, 4.97); Calibrated: 09.03.2007
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.01.2007
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA;;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

d=10mm, Pin=100mW, f=5200 MHz/Area Scan (91x91x1):

Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 17.1 mW/g

d=10mm, Pin=100mW, f=5200 MHz/Zoom Scan (8x8x10), dist=2mm (8x8x10)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2.5mm Reference Value = 47.9 V/m; Power Drift = 0.021 dB

Peak SAR (extrapolated) = 28.5 W/kg

SAR(1 g) = 7.76 mW/g; SAR(10 g) = 2.19 mW/g

Maximum value of SAR (measured) = 15.2 mW/g

d=10mm, Pin=100mW, f=5500 MHz/Zoom Scan (8x8x10), dist=2mm 2 (8x8x10)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 46.9 V/m; Power Drift = 0.049 dB

Peak SAR (extrapolated) = 31.5 W/kg

SAR(1 g) = 7.98 mW/g; SAR(10 g) = 2.23 mW/g

Maximum value of SAR (measured) = 16.1 mW/g

d=10mm, Pin=100mW, f=5800 MHz/Zoom Scan (8x8x10), dist=2mm (8x8x10)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 44.6 V/m; Power Drift = 0.080 dB

Peak SAR (extrapolated) = 31.8 W/kg

SAR(1 g) = 7.63 mW/g; SAR(10 g) = 2.12 mW/g


Maximum value of SAR (measured) = 15.8 mW/g

Certificate No: D5GHzV2-1008_Dec07

Page 6 of 8





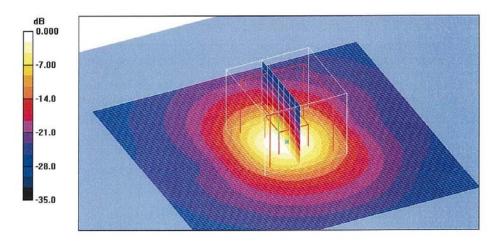


0~dB=15.8mW/g

Certificate No: D5GHzV2-1008_Dec07





Impedance Measurement Plot for Head TSL

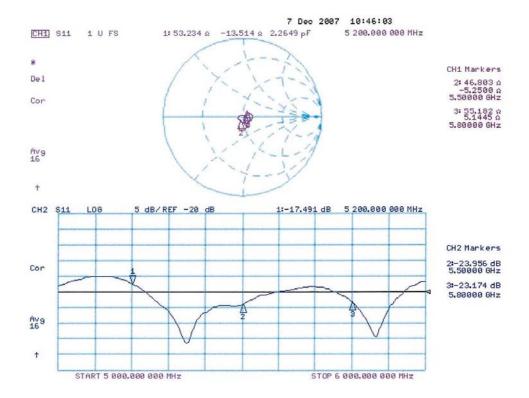

Certificate No: D5GHzV2-1008_Dec07





