

APPENDIX

11. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement system

Photograph of the tissue simulant fluid liquid depth (Body)

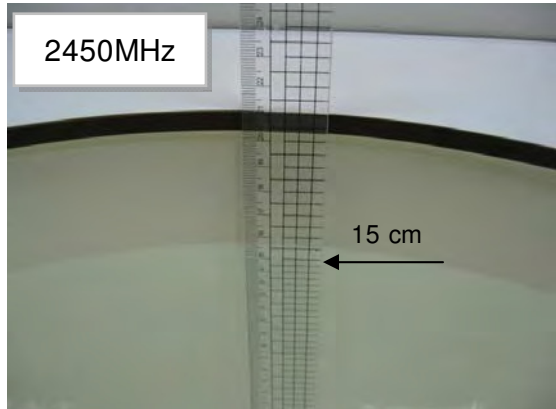


Fig.2.1

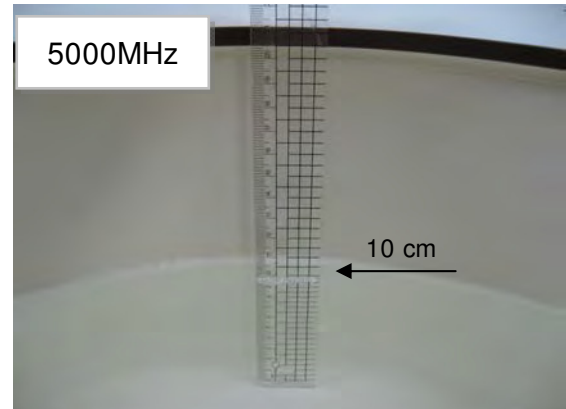


Fig.2.2

Body - distance between flat phantom and EUT is 0 mm

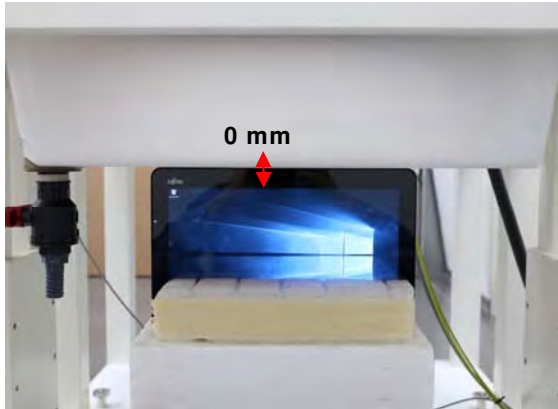


Fig.3 EUT Top side to flat phantom



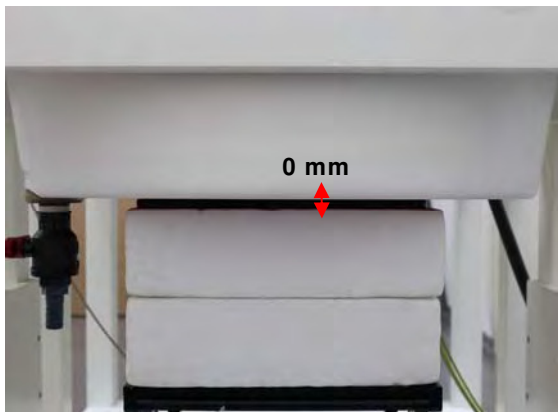


Fig.4 EUT Back side to flat phantom



Fig.5 EUT Right side to flat phantom

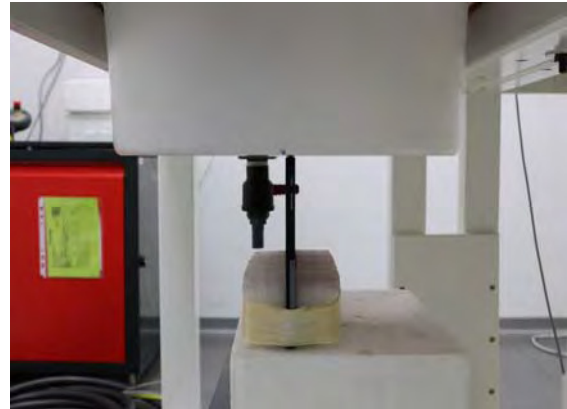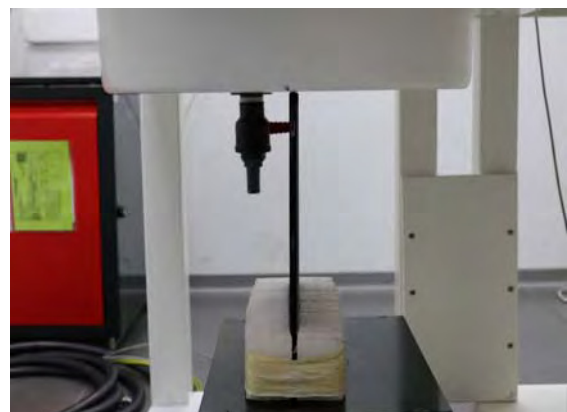

Body - distance between flat phantom and EUT is 0 mm

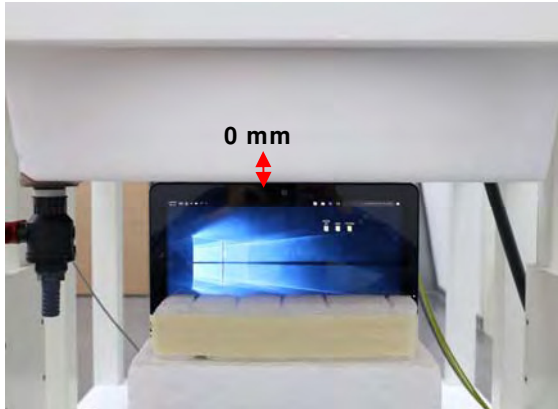


Fig.6 EUT Bottom side to flat phantom

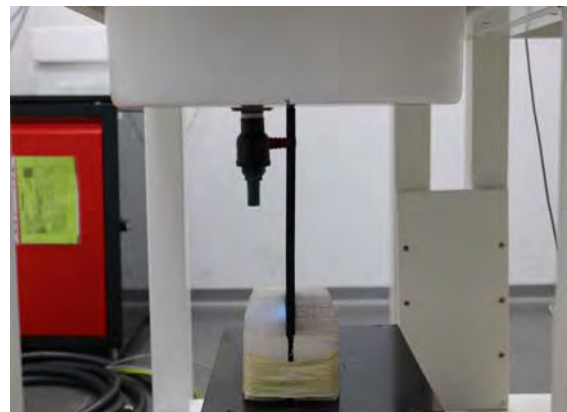
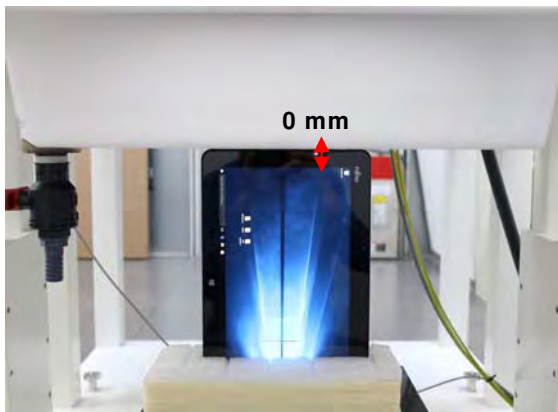


Fig.7 EUT Left side to flat phantom

12. Photographs of the EUT



Fig.8 Front view of EUT



Fig.9 Back view of EUT

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.
除非另有說明，此報告結果僅對測試之樣品負責，同時此樣品僅保留90天。本報告未經本公司書面許可，不可部份複製。

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at

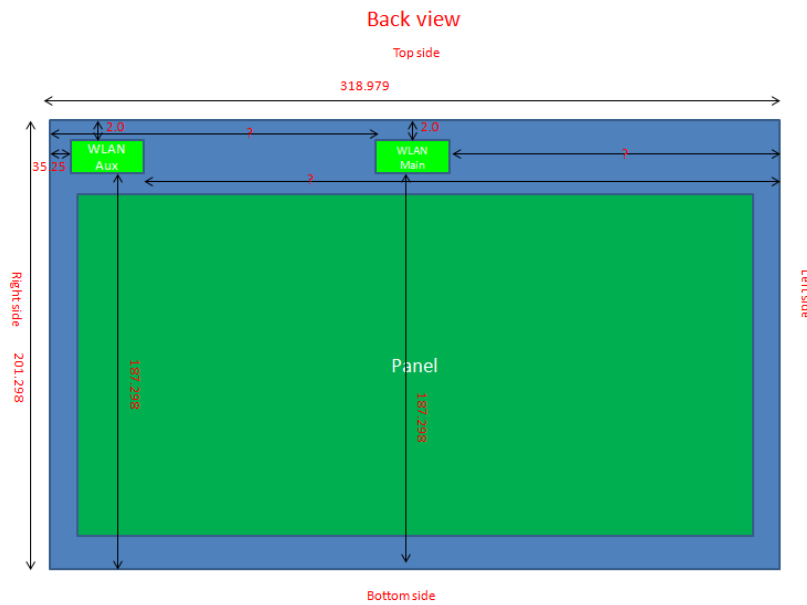


Fig.10 Antenna position of EUT (Back view)

- End of Report -