


## APPENDIX

### 11. Photographs of Test Setup




**Fig.1 Photograph of the SAR measurement system**

**Photograph of the tissue simulant fluid liquid depth (Body)**

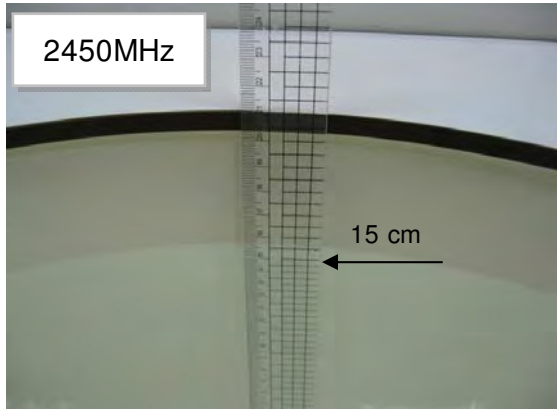

**Fig.2.1**


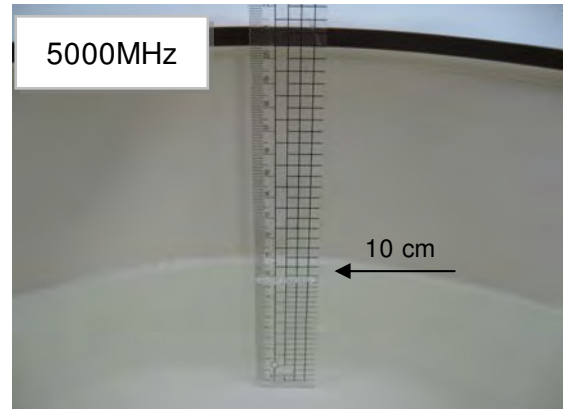


**Fig.2.2**

**Body - distance between flat phantom and EUT is 0 mm**




**Fig.3 EUT Top side to flat phantom**

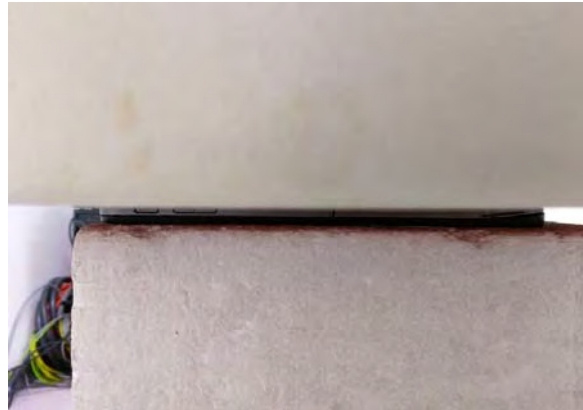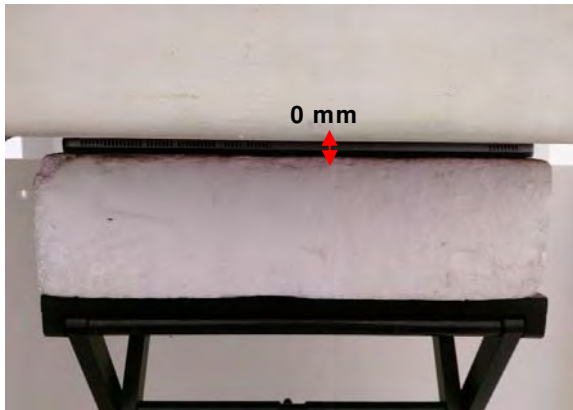

**Fig.4 EUT Back side to flat phantom**

## 12. Photographs of the EUT

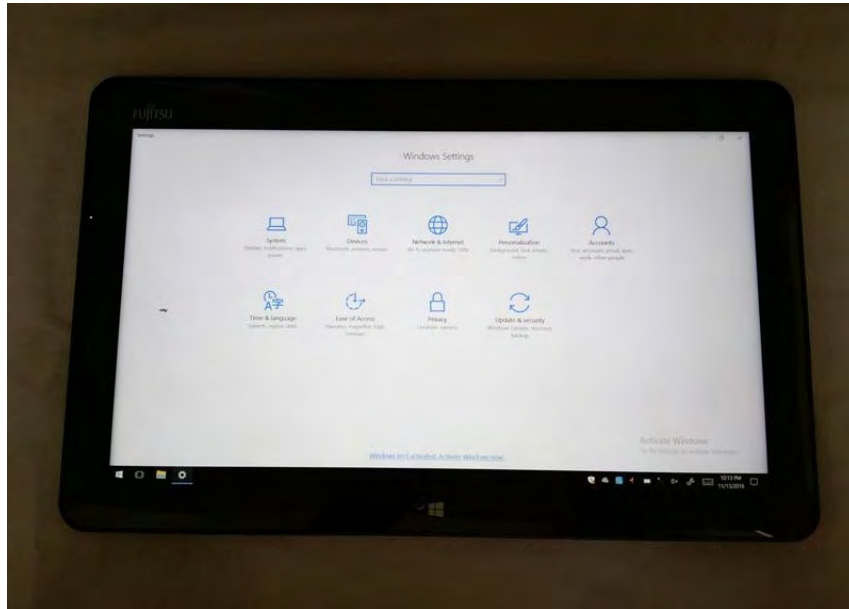

**Fig.5 Front view of EUT**



**Fig.6 Back view of EUT**

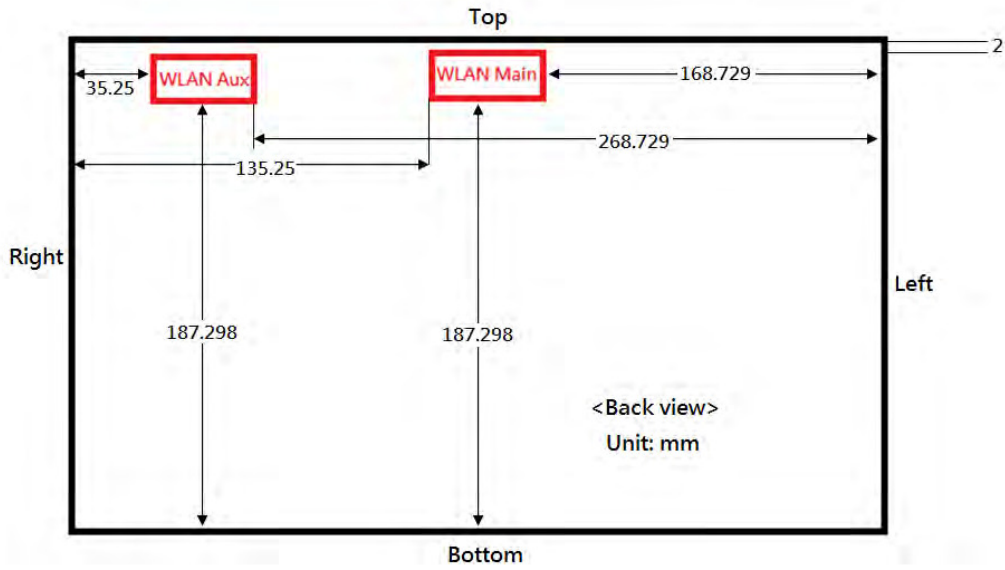


Fig.7 Antenna position of EUT (Back view)

- End of Report -