



## NCL CALIBRATION LABORATORIES

Calibration File No.: C-P-0256m

# CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the **NCL CALIBRATION LABORATORIES** by qualified personnel following recognized procedures and using transfer standards traceable to NRC/NIST.

Equipment: Miniature Isotropic RF Probe 5.8 GHz

Manufacturer: APREL Laboratories

Model No.: E-010

Serial No.: 163

Calibration Procedure: SSI/DRB-TP-D01-032

Project No: Probe Cal Internal

Calibrated: May 8<sup>th</sup> 2002

Recalibration required: may 7<sup>th</sup> 2003

Released on: May 8<sup>th</sup> 2002

Released By: \_\_\_\_\_

**NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY  
NEPEAN, ONTARIO  
CANADA K2R 1E6

Division of APREL Lab.  
TEL: (613) 820-4988  
FAX: (613) 820-4161

## **Introduction**

This Calibration Report reproduces the results of the calibration performed in line with the SSI/DRB-TP-D01-032m E-Field Probe Calibration Procedure. The results contained within this report are for APREL E-Field Probe E-010 163.

## **References**

SSI/DRB-TP-D01-032m E-Field Probe Calibration Procedure  
IEEE P-1528 *DRAFT* "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"  
FCC Supplement C Edition 01-01  
SSI-TP-014 Tissue Calibration Procedure

## **Conditions**

Probe 163 was a new probe taken from stock prior to calibration.

**Ambient Temperature of the Laboratory:** 23 °C +/- 0.5°C  
**Temperature of the Tissue:** 22 °C +/- 0.5°C

## Calibration Results Summary

<b>Probe Type:</b>	E-Field Probe E-010
<b>Serial Number:</b>	163
<b>Frequency:</b>	5.8 GHz
<b>Sensor Offset:</b>	2.4 mm
<b>Sensor Length:</b>	2.5 mm
<b>Tip Enclosure:</b>	Glass*
<b>Tip Diameter:</b>	7 mm
<b>Tip Length:</b>	40 mm
<b>Total Length:</b>	290 mm

\*Resistive to recommended tissue recipes per IEEE-P1528

## Sensitivity in Air

<b>Channel X:</b>	0.58 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Y:</b>	0.58 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Channel Z:</b>	0.58 $\mu\text{V}/(\text{V}/\text{m})^2$
<b>Diode Compression Point:</b>	76 mV

## **Sensitivity in Muscle Tissue**

**Frequency:** 5.8 GHz

**Epsilon:** 48.2 (+/-10%)      **Sigma:** 6.0 S/m (+/-10%)

### **ConvF**

**Channel X:** 2.5

**Channel Y:** 2.5

**Channel Z:** 2.5

Tissue sensitivity values were calculated using a load impedance of 5 M $\Omega$ .


### **Boundary Effect:**

Uncertainty resulting from the boundary effect is less than 2% for the distance between the tip of the probe and the tissue boundary, when less than 2.6mm.



### **Spatial Resolution:**

The measured probe tip diameter is 7 mm (+/- 0.01 mm) and therefore meets the requirements of SSI/DRB-TP-D01-032 for spatial resolution.


### Receiving Pattern 5.8 GHz (Air)

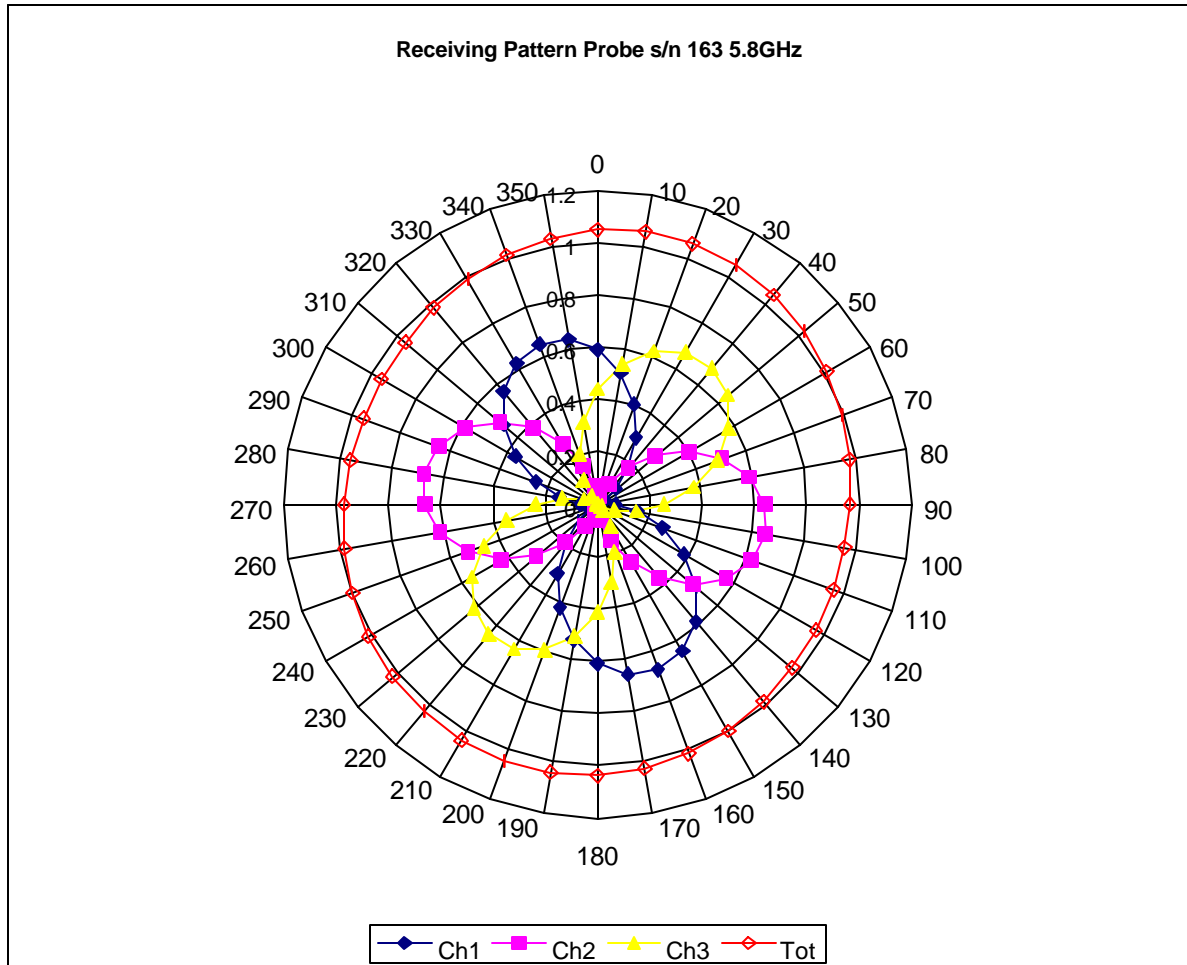

### Isotropy Error 5.8 GHz (Air)

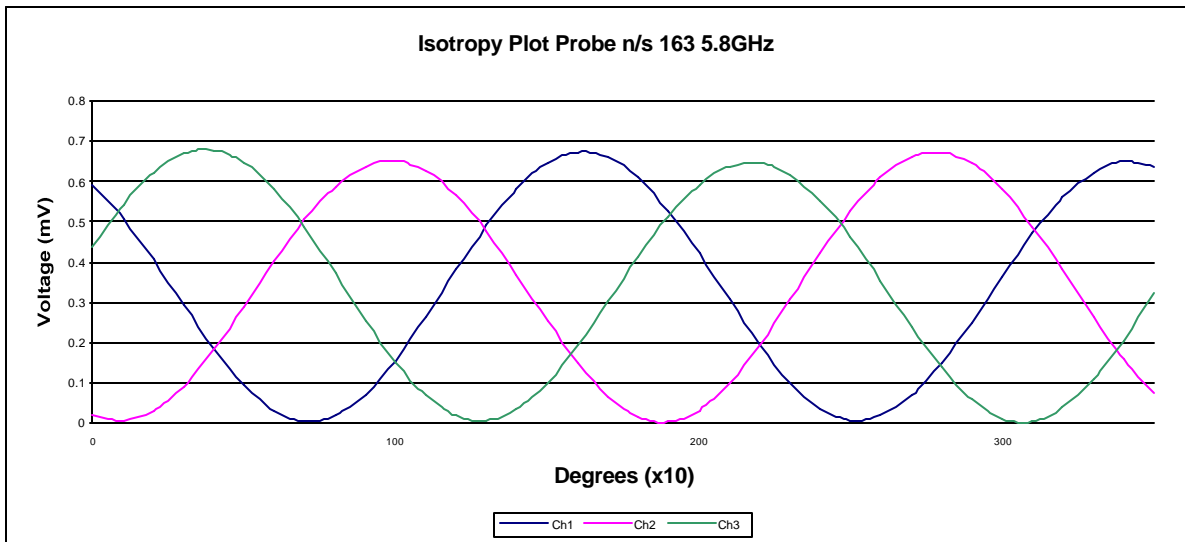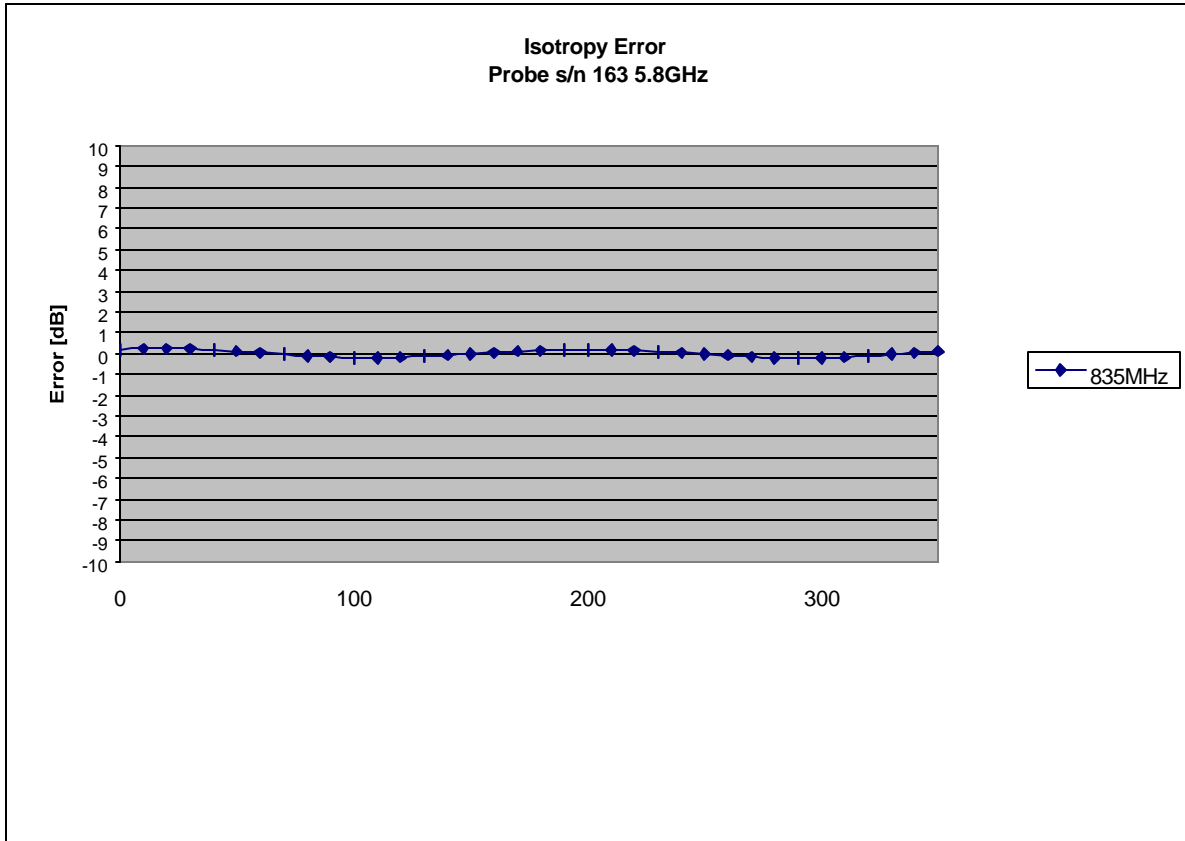


## Dynamic Range

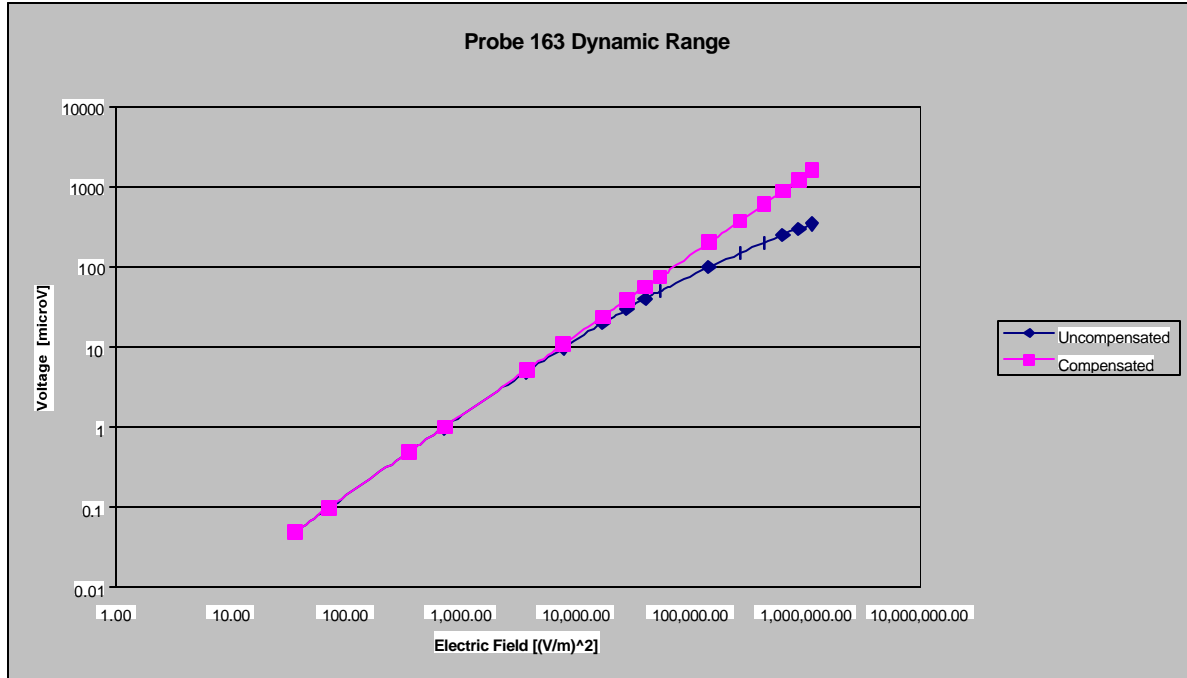

## Video Bandwidth

**Probe Frequency Characteristics**

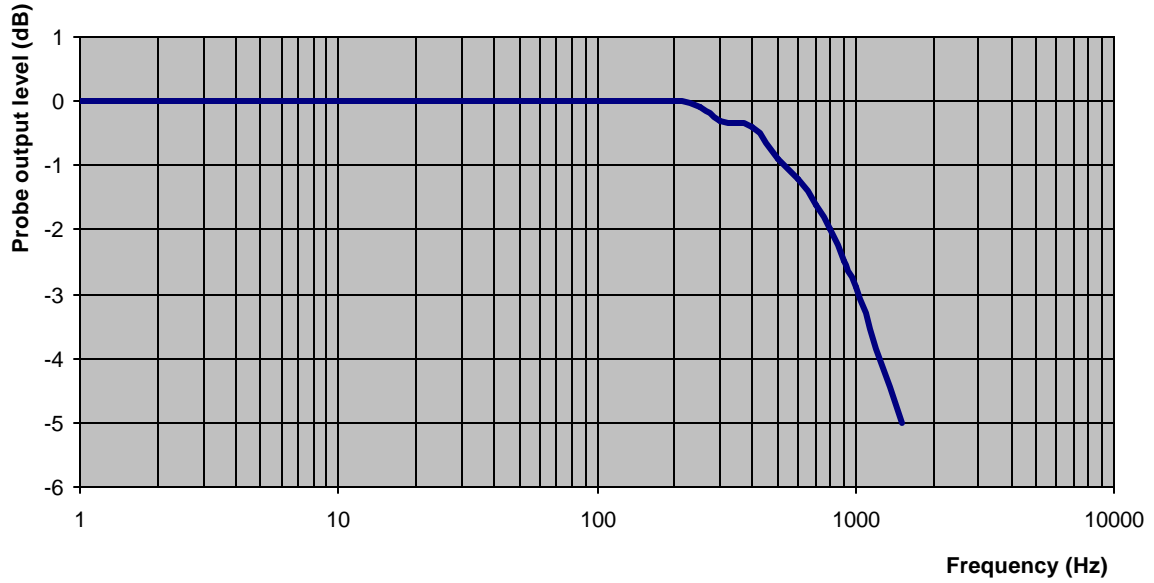

**Video Bandwidth at 500 Hz**                      1 dB  
**Video Bandwidth at 1.02 KHz:**                3 dB



## **Conversion Factor Uncertainty Assessment**

**Frequency:** 5.8 GHz  
**Epsilon:** 48.2 (+/-10%)      **Sigma:** 6.0 S/m (+/-10%)

### **ConvF**

**Channel X:** 2.5      7%(K=2)  
**Channel Y:** 2.5      7%(K=2)  
**Channel Z:** 2.5      7%(K=2)

To minimize the uncertainty calculation all tissue sensitivity values were calculated using a load impedance of 5 M $\Omega$ .

### **Boundary Effect:**

For a distance of 2.6mm the evaluated uncertainty (increase in the probe sensitivity) is less than 2%.

## **Test Equipment**

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List May 2002