

# A Test Lab Techno Corp.

Changan Lab : No. 140 -1, Changan Street, Bade City, Taoyuan County, Taiwan R.O.C.

Tel: 886-3-271-0188 / Fax: 886-3-271-0190

## SAR EVALUATION REPORT



Test Report No.	:	1001FS18
Applicant	:	VTech Telecommunications Ltd.
EUT Type	:	1.9GHz DECT 6.0 Cordless Phone
FCC ID	:	EW780-7446-00
Trade Name	:	AT&T
Model Number	:	TL32200
Dates of Test	:	Jan. 21, 2010
Test Environment	:	Ambient Temperature : 22 $\pm$ 2 $^{\circ}$ C
		Relative Humidity:40 - 70 %
Test Specification	:	Standard C95.1-2005
		IEEE Std. 1528-2003
		2.1093;FCC/OET Bulletin 65 Supplement C [July 2001]
Max. SAR	:	0.01500 W/kg Head SAR
		0.03300 W/kg Body SAR
Test Lab Location	:	Chang-an Lab



- 1. The test operations have to be performed with cautious behavior, the test results are as attached.
- 2. The test results are under chamber environment of A Test Lab Techno Corp. A Test Lab Techno Corp. does not assume responsibility for any conclusions and generalizations drawn from the test results with regard to other specimens or samples.
- 3. The measurement report has to be written approval of A Test Lab Techno Corp. It may only be reproduced or published in full. This report shall not be reproduced except in full, without the written approval of A Test Lab Techno Corp. The test results in the report only apply to the tested sample.

20100129 Sam Chuang

Sam Chuang Approve Signer

Alex Wu Testing Engineer

20100129



## Contents

1. Description of Equipment Under Test (EUT)	3
2. Introduction	4
3. SAR Definition	4
4. SAR Measurement Setup	5
5. System Components	7
6. Test Equipment List	15
7. Tissue Simulating Liquids	16
8. Measurement Process	20
9. Measurement Uncertainty	26
10. SAR Test Results Summary	28
11. Conclusion	32
12. References	32
Appendix A - System Performance Check	33
Appendix B - SAR Measurement Data	35
Appendix C - Calibration	40



## 1. <u>Description of Equipment Under Test (EUT)</u>

Applicant	:	VTech Telecommunications Ltd.		
Applicant Address	•	23/F, Tai Ping Industrial Centre, Block 1,		
Applicant Address	•			
		57 Ting Kok Road, Tai Po, Hong Kong		
Manufacturer :		Dongguan VTech Satellite Equipment Co.Ltd		
Manufacturer Address	:	VTech Science Park, Xia Ling Bei Management		
		Zone, Liaobu, Dongguan, Guangdong, China		
EUT Type	:	1.9GHz DECT 6.0 Cordless Phone		
FCC ID	:	EW780-7446-00		
Trade Name	:	AT&T		
Model Number	:	TL32200		
Battery Type	:	Ni-MH Battery (2.4V , 400mAh )		
Test Device	:	Production Unit		
Tx Frequency :		1921.536 -1928.448 MHz ( UPCS )		
Max. RF Conducted Power		0.103W (20.14dBm ) UPCS		
Max. SAR Measurement		0.01500 W/kg UPCS Head SAR		
		0.03300 W/kg UPCS Body SAR		
HW Version	:	NA		
SW Version	:	NA		
Antenna Type	:	Fixed Type		
Antenna Gain	:	0dBi		
Device Category	:	Portable		
RF Exposure Environment	:	General Population / Uncontrolled		
Battery Option	:	Standard		
Application Type	:	Certification		

This wireless portable device has been shown to be capable of compliance for localized specific absorption rate (SAR) for uncontrolled environment / general population exposure limits specified in Standard C95.1-2005 and had been tested in accordance with the measurement procedures specified in IEEE Std. 1528-2003.



## 2. <u>Introduction</u>

The A Test Lab Techno Corp. has performed measurements of the maximum potential exposure to the user of **VTech Telecommunications Ltd. Trade Name : AT&T Model(s) : TL32200.** The test procedures, as described in American National Standards, Institute C95.1 - 2005[1], FCC/OET Bulletin 65 Supplement C [July 2001] were employed and they specify the maximum exposure limit of 1.6mW/g as averaged over any 1 gram of tissue for portable devices being used within 20cm between user and EUT in the uncontrolled environment. A description of the product and operating configuration, detailed summary of the test results, methodology and procedures used in the equipment used are included within this test report.

## 3. <u>SAR Definition</u>

Specific Absorption Rate (SAR) is defined as the time derivative (rate) of the incremental energy (dw) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density (P). It is also defined as the rate of RF energy absorption per unit mass at a point in an absorbing body.

#### SAR Mathematical Equation

SAR = 
$$\frac{d}{dt}\left(\frac{dw}{dm}\right) = \frac{d}{dt}\left(\frac{dw}{\rho dv}\right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

$$SAR = \frac{\sigma E^2}{\rho}$$

Where :

 $\sigma$  = conductivity of the tissue (S/m)

 $\rho$  = mass density of the tissue (kg/m<sup>3</sup>)

E = RMS electric field strength (V/m)

\*Note :

The primary factors that control rate of energy absorption were found to be the wavelength of the incident field in relations to the dimensions and geometry of the irradiated organism, the orientation of the organism in relation to the polarity of field vectors, the presence of reflecting surfaces, and whether conductive contact is made by the organism with a ground plane [2]



## 4. <u>SAR Measurement Setup</u>

These measurements were performed with the automated near-field scanning system DASY4 from Schmid & Partner Engineering AG (SPEAG). The system is based on a high precision robot (working range greater than 0.9m) which positions the probes with a positional repeatability of better than  $\pm$  0.025mm. Special E- and H-field probes have been developed for measurements close to material discontinuity, the sensors of which are directly loaded with a Schottky diode and connected via highly resistive lines (length = 300mm) to the data acquisition unit.

A cell controller system contains the power supply, robot controller, teaches pendant (Joystick) and remote control, and is used to drive the robot motors. The Measurement Server is based on a PC/104 CPU board with a 166MHz low-power Pentium, 32MB chipdisk and 64MB RAM. The necessary circuits for communication with either the DAE4 electronic box as well as the 16-bit AD-converter system for optical detection and digital I/O interface are contained on the DASY4 I/O-board, which is directly connected to the PC/104 bus of the CPU board. The PC consists of the Intel Pentium 4 2.4GHz computer with Windows XP system and SAR Measurement Software DASY4, Post Processor SEMCAD, monitor, mouse, and keyboard. The Staubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection...etc. is connected to the Electro-optical converter (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the Measurement Server.

The DAE4 (or DAE3) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe mounting device includes two different sensor systems for frontal and sidewise probe contacts. They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built in VME-bus computer. The system is described in detail in [3].



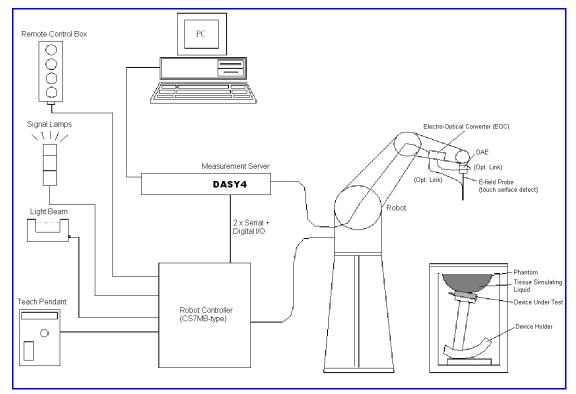


Figure 1. SAR Lab Test Measurement Setup



## 5. <u>System Components</u>

#### 5.1 DASY4 E-Field Probe System

The SAR measurements were conducted with the dosimetric probe ES3DV3 or ET3DV6 (manufactured by SPEAG), designed in the classical triangular configuration [3] and optimized for dosimetric evaluation. The probes is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multi-fiber line ending at the front of the probe tip. It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY4 software reads the reflection during a software approach and looks for the maximum using a 2nd order fitting. The approach is stopped when reaching the maximum.



### 5.1.1 E-Field Probe Specification

Construction	Symmetrical design with triangular core
	Built-in optical fiber for surface detection
	System
	Built-in shielding against static charges
	PEEK enclosure material
	(resistant to organic solvents, e.q., glycol)
Calibration	In air from 10 MHz to 2.5 GHz
	In brain and muscle simulating tissue at
	frequencies of 1900MHz and 2000MHz
	(accuracy ±8%)
	Calibration for other liquids and frequencies upon
	request
Frequency	10 MHz to > 6 GHz; Linearity: $\pm 0.2 \text{ dB}$
	(30 MHz to 3 GHz)
Directivity	± 0.2 dB in brain tissue
	(rotation around probe axis)
	± 0.4 dB in brain tissue
	(rotation normal probe axis)
Dynamic Range	5 $\mu$ W/g to > 100mW/g; Linearity: ±0.2dB
Surface Detection	$\pm$ 0.2 mm repeatability in air and clear liquids
	over diffuse reflecting surface(ET3DV6 only)
Dimensions	Overall length: 330mm
	Tip length: 16mm
	Body diameter: 12mm
	Tip diameter: 6.8mm
	Distance from probe tip to dipole centers: 2.7mm
Application	General dosimetry up to 3GHz
	Compliance tests of mobile phones
	Fast automatic scanning in arbitrary phantoms

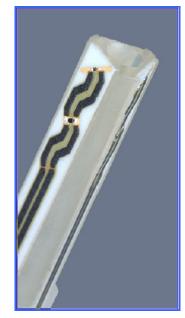


Figure 2. E-field Probe



Figure 3. Probe setup on robot



#### 5.1.2 E-Field Probe Calibration

Each probe is calibrated according to a dosimetric assessment procedure described in (4) with accuracy better than  $\pm$  10%. The spherical isotropy was evaluated with the procedure described in (5) and found to be better than  $\pm$  0.25dB. The sensitivity parameters (NormX, NormY, and NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested.

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies bellow 1GHz, and in a wave guide above 1GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees.

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium correlates to temperature rise in a dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

SAR = 
$$C \frac{\Delta T}{\Delta t}$$

Where :

 $\Delta t$  = Exposure time (30 seconds),

**C** = Heat capacity of tissue (brain or muscle),

 $\Delta T$  = Temperature increase due to RF exposure.

Or SAR = 
$$\frac{|E|^2 \sigma}{\rho}$$

Where :

**σ** = Simulated tissue conductivity,

 $\boldsymbol{\rho}$  = Tissue density (kg/m<sup>3</sup>).



## 5.2 Data Acquisition Electronic (DAE) System

#### **Cell Controller**

Processor :	Intel Pentium 4
Clock Speed :	2.4GHz
Operating System :	Windows XP Professional

#### **Data Converter**

Features :	Signal Amplifier, multiplexer, A/D converter, and control logic
Software :	DASY4 v4.7 (Build 80) & SEMCAD v1.8 (Build 186)
Connecting Lines :	Optical downlink for data and status info
	Optical uplink for commands and clock

#### 5.3 Robot

Positioner :	Stäubli Unimation Corp. Robot Model: RX90L
Repeatability :	±0.025 mm
No. of Axis :	6

#### 5.4 Measurement Server

Processor :	PC/104 with a 166MHz low-power Pentium
I/O-board:	Link to DAE4 (or DAE3)
	16-bit A/D converter for surface detection system
	Digital I/O interface
	Serial link to robot
	Direct emergency stop output for robot



#### 5.5 Device Holder for Transmitters

In combination with the SAM Twin Phantom V4.0, the Mounting Device (POM) enables the rotation of the mounted transmitter in spherical coordinates whereby the rotation points is the ear opening. The devices can be easily, accurately, and repeat ably positioned according to the IEEE SCC34-SC2 and CENELEC specifications. The device holder can be locked at different phantom locations (left head, right head, and flat phantom).

\* Note: A simulating human hand is not used due to the complex anatomical and geometrical structure of the hand that may produced infinite number of configurations [6]. To produce the worst-case condition (the hand absorbs antenna output power), the hand is omitted during the tests.

Larger DUT cannot be tested using this device holder. Instead a support of bigger polystyrene cubes and thin polystyrene plates is used to position the DUT in all relevant positions to find and measure spots with maximum SAR values. Therefore those devices are normally only tested at the flat part of the SAM.



Figure 4. Device Holder

#### 5.6 Phantom - SAM v4.0

The shell corresponds to the specifications of the Specific Anthropomorphic Mannequin (SAM) phantom defined in IEEE 1528-200X, EN 62209-1 and IEC 62209. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents evaporation of the liquid. Reference markings on the phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points with the robot.



Figure 5. SAM Twin Phantom

Shell Thickness	2 ± 0.2 mm	
Filling Volume	Approx. 25 liters	
Dimensions	810×1000×500 mm (H×L×W)	

Table 1. Specification of SAM v4.0



#### 5.7 Data Storage and Evaluation

#### 5.7.1 Data Storage

The DASY4 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension .DA4. The postprocessing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

#### 5.7.2 Data Evaluation

The DASY4 post processing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software :

Probe parameters :	- Sensitivity	Normi, ai0, ai1, ai2
	- Conversion factor	ConvFi
	- Diode compression point	dcpi
Device parameters :	- Frequency	f
	- Crest factor	cf
Media parameters :	- Conductivity	σ
	- Density	ρ

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY components. In the direct measuring mode of the multimeter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.



The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as :

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with  $V_i$  = compensated signal of channel *i* (*i* = x, y, z)

 $U_i$  = input signal of channel *i* (*i* = x, y, z)

*cf* = crest factor of exciting field (DASY parameter)

*dcp*<sub>i</sub> = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated :

E-field probes :

$$E_i = \sqrt{\frac{V_i}{Norm_i \cdot ConvF}}$$

H-field probes : 
$$H_i = \sqrt{V_i} \cdot \frac{a_{i0} + a_{i1}f + a_{i2}f^2}{f}$$

with  $V_i$  = compensated signal of channel *i* (*i* = x, y, z)

*Norm*<sub>i</sub> = sensor sensitivity of channel i (i = x, y, z)

 $\mu$  V/(V/m)<sup>2</sup> for E-field Probes

*ConvF* = sensitivity enhancement in solution

 $a_{ij}$  = sensor sensitivity factors for H-field probes

f = carrier frequency [GHz]

 $E_i$  = electric field strength of channel *i* in V/m

Hi = magnetic field strength of channel *i* in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude) :

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$



The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with SAR = local specific absorption rate in mW/g

 $E_{tot}$  = total field strength in V/m

 $\sigma$  = conductivity in [mho/m] or [Siemens/m]

 $\rho$  = equivalent tissue density in g/cm<sup>3</sup>

**\*Note**: That the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$
 or  $P_{pwe} = \frac{H_{tot}^2}{37.7}$ 

with  $P_{pwe}$  = equivalent power density of a plane wave in mW/cm<sup>2</sup>

 $E_{tot}$  = total electric field strength in V/m

 $H_{tot}$  = total magnetic field strength in A/m



## 6. <u>Test Equipment List</u>

Manufacture		True (Medel		Calibration		
r	Name of Equipment	Type/Model	Serial Number	Last Cal.	Due Date	
SPEAG	Dosimetric E-Field Probe	ES3DV3	3071	Jun. 22, 2009	Jun. 22, 2010	
SPEAG	1900MHz System Validation Kit	D1900V2	5d111	Jul. 14, 2009	Jul. 14, 2010	
SPEAG	Data Acquisition Electronics	DAE4	541	Feb. 10, 2009	Feb. 10, 2010	
SPEAG	Measurement Server	SE UMS 001 BA	1021	N	CR	
SPEAG	Device Holder	N/A	N/A	N	CR	
SPEAG	Phantom	SAM V4.0	1009	N	CR	
SPEAG	Robot	Staubli RX90L	F00/589B1/A/01	N	CR	
SPEAG	Software	DASY4 V4.7 Build 80	N/A	NCR		
SPEAG	Software	SEMCAD V1.8 Build 186	N/A	NCR		
R&S	Wireless Communication Test Set	CMU200	109369	Jul. 29, 2009	Jul. 29, 2011	
Agilent	Wireless Communication Test Set	E5515C	GB47020167	May 25, 2009	May 25, 2011	
Agilent	ENA Series Network Analyzer	E5071B	MY42402996	Nov. 04, 2009	Nov. 04, 2010	
Agilent	Dielectric Probe Kit	85070C	US99360094	N	CR	
R&S	Power Sensor	NRP-Z22	100179	May 17, 2009	May 17, 2010	
Agilent	Signal Generator	E8257D	MY44320425	NCR		
Agilent	Dual Directional Coupler	778D	50334	NCR		
Mini-Circuits	Power Amplifier	ZHL-42W-SMA	D111103#5	NCR		
Mini-Circuits	Power Amplifier	ZVE-8G-SMA	D042005 671800514	NCR		

#### Table 2. Test Equipment List



## 7. <u>Tissue Simulating Liquids</u>

The mixture is calibrated to obtain proper dielectric constant (permittivity) and conductivity of the tissue. The dielectric parameters of the liquids were verified prior to the SAR evaluation using an 85070C Dielectric Probe Kit and an E5071B Network Analyzer.

#### IEEE SCC-34/SC-2 in 1528 recommended Tissue Dielectric Parameters

The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 in 1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in human head. Other head and body tissue parameters that have not been specified in 1528 are derived from the tissue dielectric parameters computed from the 4-Cole-Cole equation and extrapolated according to the head parameter specified in 1528.

Target Frequency	He	ad	Body		
(MHz)	٤r	<b>σ</b> (S/m)	٤r	<b>σ</b> (S/m)	
150	52.3	0.76	61.9	0.80	
300	45.3	0.87	58.2	0.92	
450	43.5	0.87	56.7	0.94	
835	41.5	0.90	55.2	0.97	
900	41.5	0.97	55.0	1.05	
915	41.5	0.98	55.0	1.06	
1450	40.5	1.20	54.0	1.30	
1610	40.3	1.29	53.8	1.40	
1800 - 2000	40.0	1.40	53.3	1.52	
2450	39.2	1.80	52.7	1.95	
3000	38.5	2.40	52.0	2.73	
5800	35.3	5.27	48.2	6.00	
( $\boldsymbol{\epsilon}_r$ = relative permittivity, $\boldsymbol{\sigma}$ = conductivity and $\boldsymbol{\rho}$ = 1000 kg/m <sup>3</sup> )					

Table 3.	Tissue dielectric parameters for head and body phantoms
----------	---



#### 7.1 Ingredients

The following ingredients are used:

- Water: deionized water (pure H<sub>2</sub>0), resistivity  $\geq$  16 M  $\Omega$  -as basis for the liquid
- Sugar: refied white sugar (typically 99.7 % sucrose, available as crystal sugar in food shops)
   -to reduce relative permittivity
- Salt: pure NaCl -to increase conductivity
- Cellulose: Hydroxyethyl-cellulose, medium viscosity (75-125 mPa.s, 2% in water, 20<sup>°</sup>C), CAS # 54290 -to increase viscosity and to keep sugar in solution.
- Preservative: Preventol D-7 Bayer AG, D-51368 Leverkusen, CAS # 55965-84-9 -to prevent the spread of bacteria and molds
- DGBE: Diethylenglycol-monobuthyl ether (DGBE), Fluka Chemie GmbH, CAS # 112-34-5 -to reduce relative permittivity

#### 7.2 Recipes

The following tables give the recipes for tissue simulating liquids to be used in different frequency bands.

Note: The goal dielectric parameters (at 22  $\,^\circ C)$  must be achieved within a tolerance of  $\pm 5\%$  for  $\epsilon\,$  and  $\pm 5\%$  for  $\sigma$  .

Liquid type	HSL 1950-B				
Ingredient	Weight (g)	Weight (%)			
Water	554.12	55.41			
DGBE	445.08	44.51			
Salt	0.80	0.08			
Total amount	1,000.00	100.00			
Goal dielectric parameters					
Frequency [MHz]	1950	2000			
Relative Permittivity	40.0	40.0			
Conductivity [S/m]	1.40	1.40			

Liquid type	MSL 1	950-В
Ingredient	Weight (g)	Weight (%)
Water	697.94	69.79
DGBE	300.03	30.00
Salt	2.03	0.20
Total amount	1,000.00	99.99
Goal dielectric parameters		
Frequency [MHz]	1950	2000
Relative Permittivity	53.3	53.3
Conductivity [S/m]	1.52	1.52



## 7.3 Liquid Confirmation

## 7.3.1 Parameters

Liquid Ver	Liquid Verify											
Ambient Temperature : 22 $\pm$ 2 °C ; Relative Humidity : 40 -70%												
Liquid Type	Frequency	Temp (°C)	Parameters	Target Value	Measured Value	Deviation (%)	Limit (%)	Measured Date				
		22.0	٤r	40.0	38.52	-3.70 %	± 5 %	lan 01 0010				
	1850MHz	22.0	σ	1.40	1.34	-4.29 %	±5%	Jan. 21, 2010				
1900MHz	10001411-	22.0	٤r	40.0	38.40	-4.00 %	±5%	lan 01 0010				
Head	1900MHz	22.0	σ	1.40	1.39	-0.71 %	±5%	Jan. 21, 2010				
	1950MHz		٤r	40.0	38.18	-4.55 %	±5%	lon 21 2010				
	1950IVIFIZ			22.0	σ	1.40	1.44	2.86 %	±5%	Jan. 21, 2010		
	1050141-	22.0	٤r	53.3	51.72	-2.96 %	±5%	lan 01 0010				
	1850MHz	22.0	σ	1.52	1.45	-4.61 %	±5%	Jan. 21, 2010				
1900MHz	40001411-	00.0	٤r	53.3	51.60	-3.19 %	±5%	lan 01 0010				
Body	1900MHz	1900101612	1900101612		I SUUIVIHZ	22.0	σ	1.52	1.50	-1.32 %	±5%	Jan. 21, 2010
			22.0	٤r	53.3	51.41	-3.55 %	±5%	lan 01 0010			
	1950MHz	22.0	σ	1.52	1.55	1.97 %	±5%	Jan. 21, 2010				
	Table 4.	Measure	d Tissue diel	ectric pa	rameters for	head and bo	dy phanto	ms				



## 7.3.2 Liquid Depth

The liquid level was during measurement 15cm  $\pm$ 0.5cm.

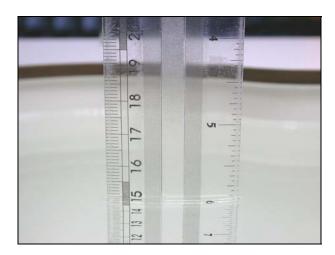


Figure 6. Head-Tissue-Simulating-Liquid




Figure 7. Body-Tissue-Simulating-Liquid



## 8. <u>Measurement Process</u>

#### 8.1 Device and Test Conditions

The Test Device was provided by **VTech Telecommunications Ltd.** for this evaluation. The spatial peak SAR values were assessed for the middle channel defined by UPCS (Ch2 = 1924.992MHz) systems. The antenna(s), battery and accessories shall be those specified by the manufacturer. The battery shall be fully charged before each measurement and there shall be no external connections.

Usage	Operates with normal mode by client					
Distance between an the joint and the liqui	For head, EUT left head, right head, to phantom 2mm separation. For Body, EUT back to phantom 2mm separation.					
Simulating human He	Head a	Head and Body				
EUT Battery		Fully-charged with Ni-MH batteries.				
Conducted power Channe		el	Frequency MHz	Before SAR Test (dBm)	After SAR Test (dBm)	
	Middle Channel - 2		1924.992	20.14	20.12	

#### 8.2 System Performance Check

#### 8.2.1 Symmetric Dipoles for System Validation Construction

Symmetrical dipole with I/4 balun enables measurement of feed point impedance with NWA matched for use near flat phantoms filled with brain simulating solutions Includes distance holder and tripod adaptor Calibration Calibrated SAR value for specified position and input power at the flat phantom in brain simulating solutions.

Frequency 900, 1800, 1900 MHz

**Return Loss** > 20 dB at specified validation position

Power Capability > 100 W (f < 1GHz); > 40 W (f > 1GHz)

#### Options

Dipoles for other frequencies or solutions and other calibration conditions are available upon request

#### Dimensions

D900V2 : Dipole length 149 mm; overall height 330 mm D1800V2 : Dipole length 72 mm; overall height 300 mm D1900V2 : dipole length 62 mm; overall height 300 mm



Figure 8. Validation Kit Page 20 of 63




#### 8.2.2 Validation

Prior to the assessment, the system validation kit was used to test whether the system was operating within its specifications of  $\pm$  7%. The validation was performed at 1900MHz.

Validation kit		Mixture Type	SAR <sub>1g</sub> [mW/g]		SAR₁₀g [mW/g]		Date of Calibration	
D1900V2 – SN5d111		Head	42.0		21.96		Jul. 14, 2009	
D1900V2 -		Body 4		42.8		.44	Jul. 14, 2009	
Frequency (MHz)	Power			Drift (dB)		rence ntage	Date	
(101112)		(mW/g)	(mW/g)	(ub)	1g	10g		
1900	250mW	10.5	5.51	0.100	0.0 %	0.4 %	lon 21 2010	
(Head)	Normalize to 1 Watt	42.0	22.04	0.100	0.0 %	0.4 %	Jan. 21, 2010	
1900	250mW	10.5	5.54	0.018	-1.9 %	-1.2 %	Jan. 21, 2010	
(Body)	Normalize to 1 Watt	42.0	22.16	0.010	-1.3 %	-1.2 70	Jan. 21, 2010	


Detail results see Appendix A.



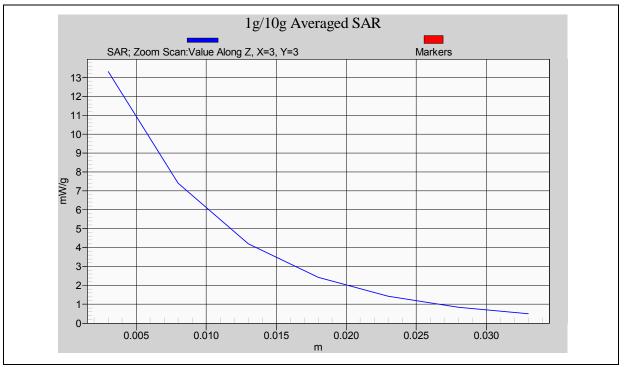

#### Z-axis Plot of System Performance Check

Head-Tissue-Simulating-Liquid 1900MHz

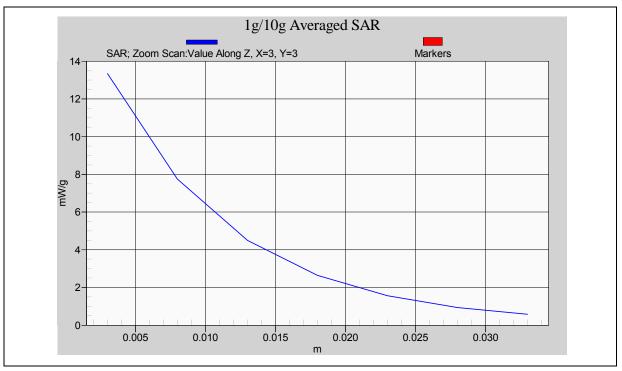



Test Report No : 1001FS18 ©2010 A Test Lab Techno Corp.



#### 8.3 Dosimetric Assessment Setup

#### 8.3.1 Body Test Position

#### **Body - Worn Configuration**

Body - Worn operating configurations should be tested with the belt-clips and holsters attached to the device and positioned against a flat phantom in normal use configurations. Devices with a headset output should be tested with a headset connected to the device.

Body - Worn accessories may not always be supplied or available as options for some devices that are intended to be authorized for body-worn use. A separation distance of 15 mm between the back of the device and a flat phantom is recommended for testing body-worn SAR compliance under such circumstances.

For this test :

- The EUT is placed into the holster/belt clip and the holster is positioned against the surface of the phantom in a normal operating position.
- Since this EUT doesn't supply any body-worn accessory to the end user, a distance of 2 mm was tested to confirm the necessary "minimum SAR separation distance". (\*Note : This distance includes the 2 mm phantom shell thickness.)



#### 8.3.2 Measurement Procedures

#### The evaluation was performed with the following procedures :

- Surface Check : A surface checks job gathers data used with optical surface detection. It determines the distance from the phantom surface where the reflection from the optical detector has its peak. Any following measurement jobs using optical surface detection will then rely on this value. The surface check performs its search a specified number of times, so that the repeatability can be verified. The probe tip distance is 1.3mm to phantom inner surface during scans.
- **Reference :** The reference job measures the field at a specified reference position, at 4 mm from the selected section's grid reference point.
- Area Scan : The area scan is used as a fast scan in two dimensions to find the area of high field values, before doing a finer measurement around the hot spot. The sophisticated interpolation routines can find the maximum locations even in relatively coarse grids. When an area scan has measured all reachable points, it computes the field maxima found in the scanned area, within a range of the global maximum. Any following zoom scan within the same procedure will then perform fine scans around these maxima. The area covered the entire dimension of the EUT and the horizontal grid spacing was 15 mm × 15 mm.
- Zoom Scan : Zoom scans are used to assess the highest averaged SAR for cubic averaging volumes with 1 g and 10 g of simulated tissue. The zoom scan measures 7 x 7 x 9 points in a 30 x 30 x 24 mm cube whose base faces are centered around the maxima returned from a preceding area scan within the same procedure.
- **Drift :** The drift job measures the field at the same location as the most recent reference job within the same procedure, with the same settings. The drift measurement gives the field difference in dB from the last reference measurement. Several drift measurements are possible for each reference measurement. This allows monitoring of the power drift of the device in the batch process. If the value changed by more than 5%, the evaluation was repeated.



#### 8.4 Spatial Peak SAR Evaluation

The DASY4 software includes all numerical procedures necessary to evaluate the spatial peak SAR values. Based on the Draft: SCC-34, SC-2, WG-2 - Computational Dosimetry, IEEE P1529/D0.0 (Draft Recommended Practice for Determining the Spatial-Peak Specific Absorption Rate (SAR) Associated with the Use of Wireless Handsets - Computational Techniques), a new algorithm has been implemented. The spatial-peak SAR can be computed over any required mass.

The base for the evaluation is a "cube" measurement in a volume of ( 30 x 30 x 24 mm<sup>3</sup>) ( 7 x 7 x 9 points). The measured volume must include the 1g and 10g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan. If the 10g cube or both cubes are not entirely inside the measured volumes, the system issues a warning regarding the evaluated spatial peak values within the Postprocessing engine (SEMCAD). This means that if the measured volume is shifted, higher values might be possible. To get the correct values you can use a finer measurement grid for the area scan. In complicated field distributions, a large grid spacing for the area scan might miss some details and give an incorrectly interpolated peak location.

The entire evaluation of the spatial peak values is performed within the Postprocessing engine (SEMCAD). The system always gives the maximum values for the 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into three stages:

#### Interpolation and Extrapolation

The probe is calibrated at the center of the dipole sensors which is located 1 to 2.7mm away from the probe tip. During measurements, the probe stops shortly above the phantom surface, depending on the probe and the surface detecting system. Both distances are included as parameters in the probe configuration file. The software always knows exactly how far away the measured point is from the surface. As the probe cannot directly measure at the surface, the values between the deepest measured point and the surface must be extrapolated.

In DASY4, the choice of the coordinate system defining the location of the measurement points has no influence on the uncertainty of the interpolation, Maxima Search and SAR extrapolation routines. The interpolation, Maxima Search and extrapolation routines are all based on the modified Quadratic Shepard's method [7].



## 9. <u>Measurement Uncertainty</u>

Measurement uncertainties in SAR measurements are difficult to quantify due to several variables including biological, physiological, and environmental. However, we estimate the measurement uncertainties in SAR to be less than  $\pm 22.4 \%$  [8].

According to Std. C95.3[9], the overall uncertainties are difficult to assess and will vary with the type of meter and usage situation. However, accuracy's of  $\pm 1$  to 3 dB can be expected in practice, with greater uncertainties in near-field situations and at higher frequencies (shorter wavelengths), or areas where large reflecting objects are present. Under optimum measurement conditions, SAR measurement uncertainties of at least  $\pm 2$ dB can be expected.

According to CENELEC [10], typical worst-case uncertainty of field measurements is  $\pm 5$  dB. For well-defined modulation characteristics the uncertainty can be reduced to  $\pm 3$  dB.



Uncertainty Component	Uncertainty Value	Probability Distribution	Divisor	с <sub>і</sub> (1g)	с <sub>і</sub> (10g)	Standard Uncertainty ±1% ( 1-g )	Standard Uncertainty ±1% (10-g)	V <sub>i</sub> or V <sub>eff</sub>
Measurement System								
Probe Calibration ( <i>k</i> =1)	4.8	Normal	1	1	1	4.8	4.8	∞
Axial Isotropy	4.7	Rectangular	$\sqrt{3}$	$\sqrt{0.5}$	$\sqrt{0.5}$	1.9	1.9	8
Hemispherical Isotropy	9.6	Rectangular	$\sqrt{3}$	$\sqrt{0.5}$	$\sqrt{0.5}$	3.9	3.9	8
Boundary Effect	0.8	Rectangular	$\sqrt{3}$	1	1	0.5	0.5	8
Linearity	4.7	Rectangular	$\sqrt{3}$	1	1	2.7	2.7	8
System Detection Limit	1.0	Rectangular	$\sqrt{3}$	1	1	0.6	0.6	∞
Readout Electronics	1.0	Normal	1	1	1	1.0	1.0	8
Response Time	1.0	Rectangular	$\sqrt{3}$	1	1	0.6	0.6	8
Integration Time	1.9	Rectangular	$\sqrt{3}$	1	1	1.1	1.1	8
RF Ambient Conditions	3.0	Rectangular	$\sqrt{3}$	1	1	1.7	1.7	8
Probe Positioner Mechanical Tolerance	1.4	Rectangular	$\sqrt{3}$	1	1	0.8	0.8	∞
Probe Positioning with respect to Phantom Shell	2.9	Rectangular	$\sqrt{3}$	1	1	1.7	1.7	8
Extrapolation, interpolation and integration Algorithms for Max. SAR Evaluation	4.5	Rectangular	$\sqrt{3}$	1	1	2.6	2.6	∞
Test sample Related								
Test sample Positioning	2.9	Normal	1	1	1	2.9	2.9	145
Device Holder Uncertainty	3.6	Normal	1	1	1	3.6	3.6	5
Output Power Variation - SAR drift measurement	5.0	Rectangular	$\sqrt{3}$	1	1	2.9	2.9	∞
Phantom and Tissue Paramet	ers		_		-			
Phantom Uncertainty ( shape and thickness tolerances)	4.0	Rectangular	$\sqrt{3}$	1	1	2.3	2.3	∞
Liquid Conductivity - deviation from target values	5.0	Rectangular	$\sqrt{3}$	0.64	0.43	1.8	1.2	∞
Liquid Conductivity - measurement uncertainty	5.0	Normal	1	0.64	0.43	3.2	2.2	8
Liquid Permittivity - deviation from target values	5.0	Rectangular	$\sqrt{3}$	0.6	0.49	1.7	1.4	8
Liquid Permittivity - measurement uncertainty	5.0	Normal	1	0.6	0.49	3.0	2.5	8
Combined standard uncertair	nty	RSS				11.2	10.7	388
Expanded uncertainty (95% CONFIDENCE LEVEL)		<i>k</i> =2				22.4	21.5	

Table 5. Uncertainty Budget of DASY



## 10. SAR Test Results Summary


#### 10.1 UPCS Head SAR

		e(℃): <u>22</u>	± 2	Re	lative HUMID	40 - 70		
	kture Typ	e: <u>HS</u>	L1950		uid Temperat pth of liquid (	22.0 15		
Measurement : Crest Factor : 24				Pro	obe S/N:	-	3	071
Freque MHz	ency CH	Battery	Phantom Position	Accessory	SAR₁g [mW/g]	Power Drift [dB]	Amb. Temp.	Remark
1924.992	сн 2	Ni-MH	Right-Cheek	N/A	0.01400	0.050	22.0	_
1924.992	2	Ni-MH	Right-Tilted	N/A	0.00827	0.049	22.0	-
1924.992	2	Ni-MH	Left-Cheek	N/A	0.01500	0.100	22.0	-
1924.992	2	Ni-MH	Left-Tilted	N/A	0.00982	0.148	22.0	-
Unc	Std. C95.1-2005 - Safety Limit Spatial Peak Uncontrolled Exposure/General Population					1.6 W/kg ( Averaged ov		n

Detail results see Appendix B.





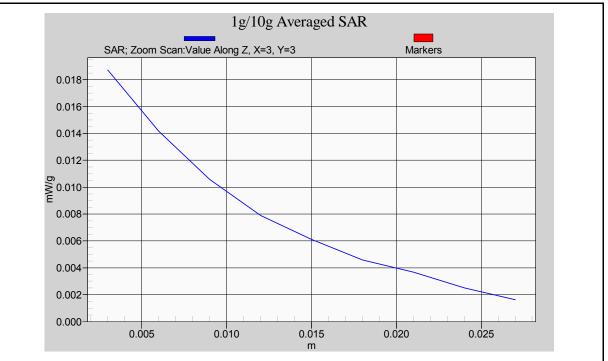


Head SAR Measurement \_ Left Cheek CH2



### 10.2 UPCS Body SAR\_ 2mm separation

Ambient Ter (°C	nperature	e 22	± 2	Re	lative HUMID	40 - 70				
Liquid: Mix	ture Typ	e: MSL	: MSL1950 Liquid Temperature (°C) : Depth of liquid (cm) :					<u>22.0</u> 15		
Measurement :         Probe S/N :         3071										
Freque	ency	Battery	Phantom	Accessory	SAR <sub>1g</sub>	Power Drift	Amb.	Remark		
Freque MHz	ency CH	Battery	Phantom Position	Accessory	SAR <sub>1g</sub> [mW/g]	Power Drift [dB]	Amb. Temp.	Remark		
	-	Battery Ni-MH		Accessory N/A				Remark -		

Detail results see Appendix B.

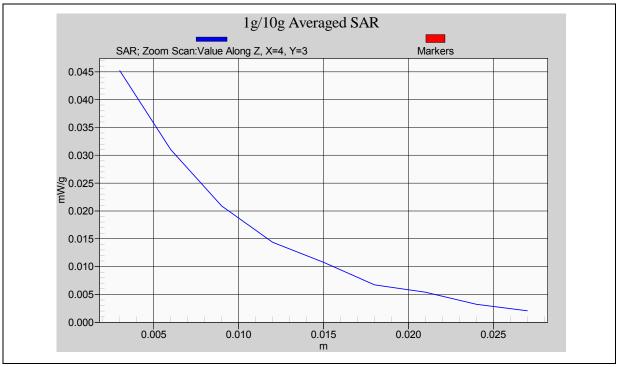

#### **Z-axis Plot of SAR Measurement**

Body SAR Measurement \_ Back to Phantom 2mm separation \_CH2



#### 10.3 Std. C95.1-2005 RF Exposure Limit

Human Exposure	Population Uncontrolled Exposure ( W/kg ) or (mW/g)	Occupational Controlled Exposure ( W/kg ) or (mW/g)
Spatial Peak SAR* (head)	1.60	8.00
Spatial Peak SAR** (Whole Body)	0.08	0.40
Spatial Peak SAR*** (Partial-Body)	1.60	8.00
Spatial Peak SAR**** (Hands / Feet / Ankle / Wrist )	4.00	20.00

Table 6. Safety Limits for Partial Body Exposure

#### Notes :

- The Spatial Peak value of the SAR averaged over any 1 gram of tissue.
   (defined as a tissue volume in the shape of a cube ) and over the appropriate averaging time.
- \*\* The Spatial Average value of the SAR averaged over the whole body.
- \*\*\* The Spatial Average value of the SAR averaged over the partial body.
- \*\*\*\* The Spatial Peak value of the SAR averaged over any 10 grams of tissue.( defined as a tissue volume in the shape of a cube ) and over the appropriate averaging time.

**Population** / **Uncontrolled Environments** : are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure.

*Occupational / Controlled Environments* : are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation).



## 11. <u>Conclusion</u>

The SAR test values found for the portable mobile phone **VTech Telecommunications Ltd. Trade Name : AT&T Model(s) : TL32200** is below the maximum recommended level of 1.6 W/kg (mW/g).

## 12. <u>References</u>

- [1] Std. C95.1-2005, "American National Standard safety levels with respect to human exposure to radio frequency electromagnetic fields, 300KHz to 100GHz", New York.
- [2] NCRP, National Council on Radiation Protection and Measurements, "*Biological Effects and Exposure Criteria for Radio frequency Electromagnetic Fields*", NCRP report NO. 86, 1986.
- [3] T. Schmid, O. Egger, and N. Kuster, "Automatic E-field scanning system for dosimetric assessments", IEEE Transactions on Microwave Theory and Techniques, vol. 44, pp, 105-113, Jan. 1996.
- [4] K. Poković, T. Schmid, and N. Kuster, "Robust setup for precise calibration of E-field probes in tissue simulating liquids at mobile communications frequency", in ICECOM'97, Dubrovnik, October 15-17, 1997, pp.120-124.
- [5] K. Poković, T. Schmid, and N. Kuster, "*E-field probe with improved isotropy in brain simulating liquids*", in Proceedings of the ELMAR, Zadar, Croatia, 23-25 June, 1996, pp.172-175.
- [6] N. Kuster, and Q. Balzano, "Energy absorption mechanism by biological bodies in the near field of dipole antennas above 300MHz", IEEE Transaction on Vehicular Technology, vol. 41, no. 1, Feb. 1992, pp. 17-23.
- [7] Robert J. Renka, "Multivariate Interpolation Of Large Sets Of Scattered Data", University of North Texas ACM Transactions on Mathematical Software, vol. 14, no. 2, June 1988, pp. 139-148.
- [8] N. Kuster, R. Kastle, T. Schmid, Dosimetric evaluation of mobile communications equipment with known precision, IEEE Transaction on Communications, vol. E80-B, no. 5, May 1997, pp. 645-652.
- [9] Std. C95.3-1991, "IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic Fields – RF and Microwave, New York: IEEE, Aug. 1992.
- [10] CENELEC CLC/SC111B, European Prestandard (prENV 50166-2), *Human Exposure to Electromagnetic Fields High-frequency*: 10KHz-300GHz, Jan. 1995.



## Appendix A - System Performance Check

See following Attached Pages for System Performance Check.

Test Laboratory: A Test Lab Techno Corp. Date/Time: 2010/1/21 AM 08:52:08

#### System Performance Check at 1900MHz\_20100121\_Head

#### DUT: Dipole D1900V2\_SN5d111; Type: D1900V2; Serial: D1900V2 - SN:5d111

Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium parameters used: f = 1900 MHz;  $\sigma$  = 1.39 mho/m;  $\varepsilon_r$  = 38.4;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:


- Probe: ES3DV3 SN3071; ConvF(4.63, 4.63, 4.63); Calibrated: 2009/6/22
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn541; Calibrated: 2009/2/10
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

#### System Performance Check at 1900MHz/Area Scan (91x91x1):

Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 13.3 mW/g

#### System Performance Check at 1900MHz/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mmReference Value = 101.3 V/m; Power Drift = 0.100 dB Peak SAR (extrapolated) = 19.0 W/kg SAR(1 g) = 10.5 mW/g; SAR(10 g) = 5.51 mW/g Maximum value of SAR (measured) = 13.3 mW/g

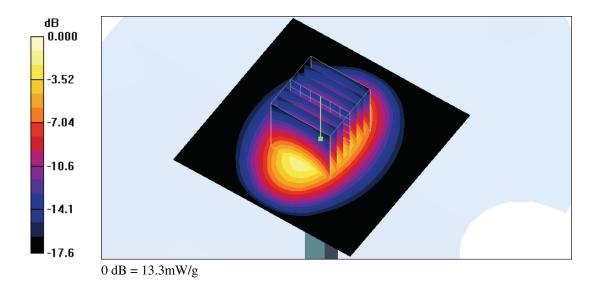



Test Laboratory: A Test Lab Techno Corp. Date/Time: 2010/1/21 PM 03:26:14

#### System Performance Check at 1900MHz\_20100121\_Body

#### DUT: Dipole D1900V2\_SN5d111; Type: D1900V2; Serial: D1900V2 - SN:5d111

Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium parameters used: f = 1900 MHz;  $\sigma$  = 1.5 mho/m;  $\varepsilon_r$  = 51.6;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:


- Probe: ES3DV3 SN3071; ConvF(4.26, 4.26, 4.26); Calibrated: 2009/6/22
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn541; Calibrated: 2009/2/10
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

#### System Performance Check at 1900MHz/Area Scan (91x91x1):

Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 13.4 mW/g

#### System Performance Check at 1900MHz/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 98.5 V/m; Power Drift = 0.018 dB Peak SAR (extrapolated) = 18.3 W/kg SAR(1 g) = 10.5 mW/g; SAR(10 g) = 5.54 mW/gMaximum value of SAR (measured) = 13.3 mW/g

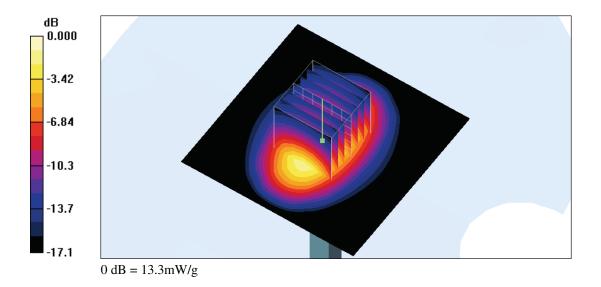



#### Appendix B - SAR Measurement Data

See following Attached Pages for SAR Measurement Data.

Test Laboratory: A Test Lab Techno Corp. Date/Time: 2010/1/21 PM 01:13:18

#### **RC\_DECT CH2**

#### DUT: TL32200; Type: DECT Cordless Phone; FCC ID: EW780-7446-00

Communication System: DECT; Frequency: 1924.992 MHz;Duty Cycle: 1:24 Medium parameters used: f = 1924.992 MHz;  $\sigma = 1.41$  mho/m;  $\varepsilon_r = 38.2$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Right Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:


- Probe: ES3DV3 SN3071; ConvF(4.53, 4.53, 4.53); Calibrated: 2009/6/22
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn541; Calibrated: 2009/2/10
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

#### Right Cheek/Area Scan (91x211x1):

Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.020 mW/g

#### Right Cheek/Zoom Scan (7x7x9)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=3mm Reference Value = 3.28 V/m; Power Drift = 0.050 dB Peak SAR (extrapolated) = 0.026 W/kg SAR(1 g) = 0.014 mW/g; SAR(10 g) = 0.00762 mW/g Maximum value of SAR (measured) = 0.018 mW/g

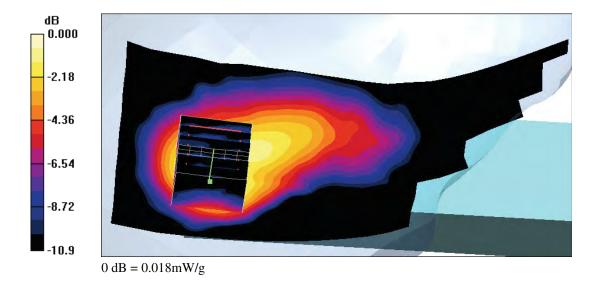



Test Laboratory: A Test Lab Techno Corp. Date/Time: 2010/1/21 PM 02:15:08

#### RT\_DECT CH2

#### DUT: TL32200; Type: DECT Cordless Phone; FCC ID: EW780-7446-00

Communication System: DECT; Frequency: 1924.992 MHz;Duty Cycle: 1:24 Medium parameters used: f = 1924.992 MHz;  $\sigma = 1.41$  mho/m;  $\varepsilon_r = 38.2$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Right Section Measurement Standard: DASY4 (High Precision Assessment)

#### DASY4 Configuration:


- Probe: ES3DV3 SN3071; ConvF(4.53, 4.53, 4.53); Calibrated: 2009/6/22
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn541; Calibrated: 2009/2/10
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

#### **Right Tilted/Area Scan (91x211x1):**

Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.011 mW/g

#### **Right Tilted/Zoom Scan (7x7x9)/Cube 0:**

Measurement grid: dx=5mm, dy=5mm, dz=3mm Reference Value = 2.37 V/m; Power Drift = 0.049 dB Peak SAR (extrapolated) = 0.023 W/kg SAR(1 g) = 0.00827 mW/g; SAR(10 g) = 0.00467 mW/g Maximum value of SAR (measured) = 0.010 mW/g

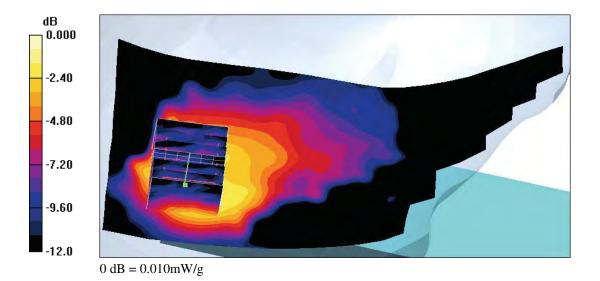



Test Laboratory: A Test Lab Techno Corp. Date/Time: 2010/1/21 AM 11:59:51

### LC\_DECT CH2

### DUT: TL32200; Type: DECT Cordless Phone; FCC ID: EW780-7446-00

Communication System: DECT; Frequency: 1924.992 MHz;Duty Cycle: 1:24 Medium parameters used: f = 1924.992 MHz;  $\sigma = 1.41$  mho/m;  $\varepsilon_r = 38.2$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Left Section Measurement Standard: DASY4 (High Precision Assessment)

### DASY4 Configuration:


- Probe: ES3DV3 SN3071; ConvF(4.53, 4.53, 4.53); Calibrated: 2009/6/22
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn541; Calibrated: 2009/2/10
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

### Left Cheek/Area Scan (91x211x1):

Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.019 mW/g

### Left Cheek/Zoom Scan (7x7x9)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=3mm Reference Value = 3.64 V/m; Power Drift = 0.100 dB Peak SAR (extrapolated) = 0.023 W/kg SAR(1 g) = 0.015 mW/g; SAR(10 g) = 0.00914 mW/g Maximum value of SAR (measured) = 0.019 mW/g

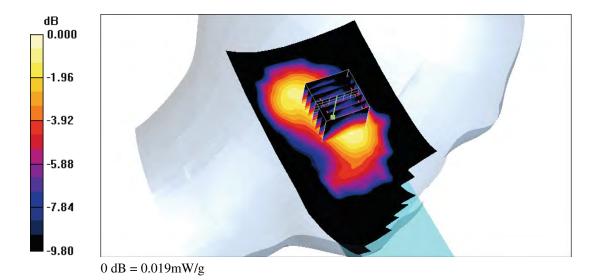



Test Laboratory: A Test Lab Techno Corp. Date/Time: 2010/1/21 PM 12:34:35

## LT\_DECT CH2

### DUT: TL32200; Type: DECT Cordless Phone; FCC ID: EW780-7446-00

Communication System: DECT; Frequency: 1924.992 MHz;Duty Cycle: 1:24 Medium parameters used: f = 1924.992 MHz;  $\sigma = 1.41$  mho/m;  $\varepsilon_r = 38.2$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Left Section Measurement Standard: DASY4 (High Precision Assessment)

### DASY4 Configuration:


- Probe: ES3DV3 SN3071; ConvF(4.53, 4.53, 4.53); Calibrated: 2009/6/22
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn541; Calibrated: 2009/2/10
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

### Left Tilted/Area Scan (91x211x1):

Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.013 mW/g

### Left Tilted/Zoom Scan (7x7x9)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=3mm Reference Value = 2.87 V/m; Power Drift = 0.148 dB Peak SAR (extrapolated) = 0.015 W/kg SAR(1 g) = 0.00982 mW/g; SAR(10 g) = 0.00546 mW/g Maximum value of SAR (measured) = 0.012 mW/g

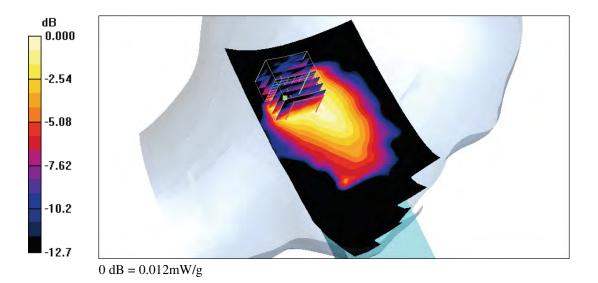



Test Laboratory: A Test Lab Techno Corp. Date/Time: 2010/1/21 PM 04:08:46

### Flat\_DECT CH2

### DUT: TL32200; Type: DECT Cordless Phone; FCC ID: EW780-7446-00

Communication System: DECT; Frequency: 1924.992 MHz;Duty Cycle: 1:24 Medium parameters used: f = 1924.992 MHz;  $\sigma = 1.53$  mho/m;  $\varepsilon_r = 51.4$ ;  $\rho = 1000$  kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

### DASY4 Configuration:


- Probe: ES3DV3 SN3071; ConvF(4.32, 4.32, 4.32); Calibrated: 2009/6/22
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn541; Calibrated: 2009/2/10
- Phantom: SAM 12; Type: SAM v4.0; Serial: TP:1009
- Measurement SW: DASY4, V4.7 Build 80; Postprocessing SW: SEMCAD, V1.8 Build 186

### Flat/Area Scan (111x221x1):

Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 0.050 mW/g

### Flat/Zoom Scan (7x7x9)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=3mmReference Value = 3.91 V/m; Power Drift = 0.143 dB Peak SAR (extrapolated) = 0.063 W/kg SAR(1 g) = 0.033 mW/g; SAR(10 g) = 0.016 mW/g Maximum value of SAR (measured) = 0.045 mW/g

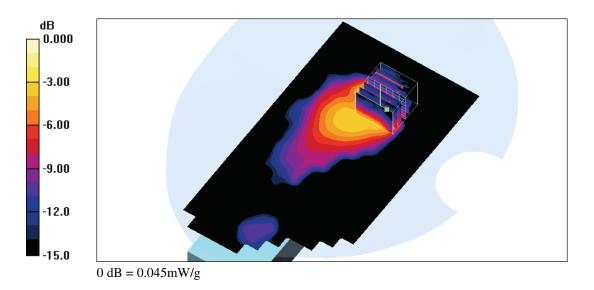



# Appendix C - Calibration

All of the instruments Calibration information are listed below.

- Dipole \_ D1900V2 SN:5d111 Calibration No.D1900V2-5d111\_Jul09
- Probe \_ ES3DV3 SN:3071 Calibration No.ES3-3071\_Jun09
- DAE \_ DAE4 SN:541 Calibration No.DAE4-541\_ Feb09



ATL (Auden)

Client



SNISS SP Z Prories S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage

Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Certificate No: D1900V2-5d111\_Jul09

Object	D1900V2 - SN: 5	d111	
Calibration procedure(s)	QA CAL-05.v7 Calibration proce	dure for dipole validation kits	
Calibration date:	July 14, 2009		
Condition of the calibrated item	In Tolerance		
The measurements and the unce	rtainties with confidence p	onal standards, which realize the physical units robability are given on the following pages and by facility: environment temperature $(22 \pm 3)^{\circ}$ C a	are part of the certificate.
rimary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2	ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601	Cal Date (Calibrated by, Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 31-Mar-09 (No. 217-01025) 31-Mar-09 (No. 217-01029) 30-Apr-09 (No. ES3-3025_Apr09) 07-Mar-09 (No. DAE4-601_Mar09)	Scheduled Calibration Oct-09 Mar-10 Mar-10 Apr-10 Mar-10 Mar-10
Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4	GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025	08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 31-Mar-09 (No. 217-01025) 31-Mar-09 (No. 217-01029) 30-Apr-09 (No. ES3-3025_Apr09)	Oct-09 Oct-09 Mar-10 Mar-10 Apr-10
Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601	08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 31-Mar-09 (No. 217-01025) 31-Mar-09 (No. 217-01029) 30-Apr-09 (No. ES3-3025_Apr09) 07-Mar-09 (No. DAE4-601_Mar09)	Oct-09 Oct-09 Mar-10 Mar-10 Apr-10 Mar-10
Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 100005	08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 31-Mar-09 (No. 217-01025) 31-Mar-09 (No. 217-01029) 30-Apr-09 (No. ES3-3025_Apr09) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07)	Oct-09 Oct-09 Mar-10 Mar-10 Apr-10 Mar-10 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09
Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 100005 US37390585 S4206	08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 31-Mar-09 (No. 217-01025) 31-Mar-09 (No. 217-01029) 30-Apr-09 (No. ES3-3025_Apr09) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08)	Oct-09 Oct-09 Mar-10 Mar-10 Apr-10 Mar-10 Scheduled Check In house check: Oct-09 In house check: Oct-09
Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by: Approved by:	GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name	08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 31-Mar-09 (No. 217-01025) 31-Mar-09 (No. 217-01029) 30-Apr-09 (No. ES3-3025_Apr09) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08) Function	Oct-09 Oct-09 Mar-10 Mar-10 Apr-10 Mar-10 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09 Signature

Certificate No: D1900V2-5d111\_Jul09

Page 1 of 9







S Schweizerischer Kalibrierdienst
 Service suisse d'étalonnage
 Servizio svizzero di taratura
 S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

### Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

### Additional Documentation:

d) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D1900V2-5d111\_Jul09

Page 2 of 9



### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V5.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.9 ± 6 %	1.43 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C		

### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	condition	
SAR measured	250 mW input power	10.5 mW / g
SAR normalized	normalized to 1W	42.0 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	41.7 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.49 mW / g
SAR normalized	normalized to 1W	22.0 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	21.9 mW / g ± 16.5 % (k=2)

<sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D1900V2-5d111\_Jul09

Page 3 of 9



### **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.5 ± 6 %	1.55 mho/m ± 6 %
Body TSL temperature during test	(21.1 ± 0.2) °C		

### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.7 mW / g
SAR normalized	normalized to 1W	42.8 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	42.4 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.61 mW / g
SAR normalized	normalized to 1W	22.4 mW / g
SAR for nominal Body TSL parameters <sup>2</sup>	normalized to 1W	22.3 mW / g ± 16.5 % (k=2)

<sup>2</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D1900V2-5d111\_Jul09

Page 4 of 9



### Appendix

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.1 Ω + 4.8 jΩ	
Return Loss	- 26.3 dB	

### Antenna Parameters with Body TSL

Impedance, transformed to feed point	45.3 Ω + 6.4 jΩ	
Return Loss	- 21.6 dB	

### **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.200 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	March 28, 2008

Certificate No: D1900V2-5d111\_Jul09

Page 5 of 9



### **DASY5 Validation Report for Head TSL**

Date/Time: 07.07.2009 15:32:44

Test Laboratory: SPEAG, Zurich, Switzerland

### DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d111


Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1 Medium: HSL U11 BB Medium parameters used: f = 1900 MHz;  $\sigma$  = 1.43 mho/m;  $\epsilon_r$  = 40.9;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC)

DASY5 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.88, 4.88, 4.88); Calibrated: 30.04.2009
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.4 Build 45

# Pin = 250 mW; dip = 10 mm, scan at 3.0 mm/Zoom Scan (dist=3.0 mm, probe 0deg) (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 95.7 V/m; Power Drift = 0.109 dB Peak SAR (extrapolated) = 19.1 W/kg SAR(1 g) = 10.5 mW/g; SAR(10 g) = 5.49 mW/g Maximum value of SAR (measured) = 13.1 mW/g

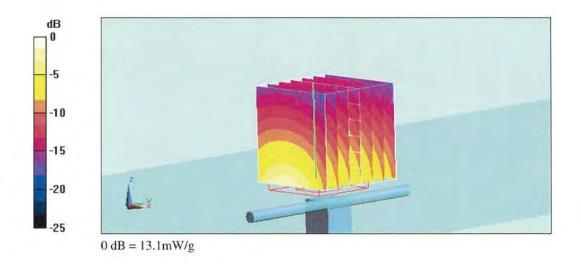

Certificate No: D1900V2-5d111\_Jul09

Page 6 of 9



### 7 Jul 2009 11:05:12 CHI S11 1 U FS 2: 51.117 Ω 4.7969 Ω 401.81 pH 1 900.000 000 MHz \* CH1 Markers De 1 1:43.670 Ω -13.871 Ω 1.80000 GHz Cor Av9 16 t 2:-26.257 dB 1 900.000 000 MHz CH2 \$11 LOG 5 dB/REF -20 dB CH2 Markers 1:-15.863 dB 1.80000 GHz Cor 1 Avg 16 1 STOP 2 100.000 000 MHz START 1 600.000 000 MHz

### Impedance Measurement Plot for Head TSL

Certificate No: D1900V2-5d111\_Jul09

Page 7 of 9



### **DASY5 Validation Report for Body TSL**

Date/Time: 14.07.2009 16:37:13

Test Laboratory: SPEAG, Zurich, Switzerland

### DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d111


Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1 Medium: MSL U10 BB Medium parameters used: f = 1900 MHz;  $\sigma$  = 1.55 mho/m;  $\varepsilon_r$  = 53.6;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC)

DASY5 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.46, 4.46, 4.46); Calibrated: 30.04.2009
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.4 Build 45

# Pin = 250 mW; dip = 10 mm, scan at 3.0mm/Zoom Scan (dist=3.0mm, probe 0deg) (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mmReference Value = 97.2 V/m; Power Drift = -0.00871 dB Peak SAR (extrapolated) = 18.8 W/kg SAR(1 g) = 10.7 mW/g; SAR(10 g) = 5.61 mW/g Maximum value of SAR (measured) = 13.5 mW/g

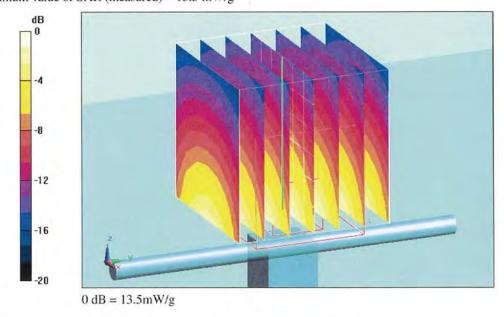

Certificate No: D1900V2-5d111\_Jul09

Page 8 of 9



# 14 Jul 2009 11:50:17 CHI S11 1 U FS 1:45.289 a 6.3691 a 533.52 pH 1 900.000 000 MHz \* De 1 C4 Av9 16 1 CH2 \$11 L06 5 dB/REF -20 dB 1:-21.622 dB 1 900.000 000 MHz De 1 CA Av9 1 CENTER 1 900.000 000 MHz SPAN 400.000 000 MHz

### Impedance Measurement Plot for Body TSL

Certificate No: D1900V2-5d111\_Jul09

Page 9 of 9





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage С Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Auden Client

Certificate No: ES3-3071\_Jun09

Accreditation No.: SCS 108

S

Object	ES3DV3 - SN:3071					
Calibration procedure(s)		and QA CAL-23.v3 edure for dosimetric E-field probe	S			
Calibration date:	June 22, 2009					
Condition of the calibrated item	In Tolerance					
The measurements and the unce All calibrations have been conduc	rtainties with confidence	tional standards, which realize the physical uni probability are given on the following pages an ory facility: environment temperature (22 ± 3)°C	d are part of the certificate			
Calibration Equipment used (M&	IE critical for calibration)					
	IE critical for calibration)	Cal Date (Certificate No.)	Scheduled Calibration			
Primary Standards		Cal Date (Certificate No.) 1-Apr-09 (No. 217-01030)	Scheduled Calibration			
Primary Standards Power meter E4419B	ID #					
Primary Standards Power meter E4419B Power sensor E4412A	ID # GB41293874	1-Apr-09 (No. 217-01030)	Apr-10			
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A	ID # GB41293874 MY41495277 MY41498087	1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030)	Apr-10 Apr-10			
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator	ID # GB41293874 MY41495277	1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030)	Apr-10 Apr-10 Apr-10			
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c)	1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026)	Apr-10 Apr-10 Apr-10 Mar-10 Mar-10			
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5056 (20b)	1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028)	Apr-10 Apr-10 Apr-10 Mar-10 Mar-10			
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b)	1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027)	Apr-10 Apr-10 Apr-10 Mar-10 Mar-10 Mar-10			
Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	10 # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S50586 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: 3013 SN: 660	1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 2-Jan-09 (No. ES3-3013_Jan09) 9-Sep-08 (No. DAE4-660_Sep08)	Apr-10 Apr-10 Apr-10 Mar-10 Mar-10 Jan-10 Sep-09			
Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: 660 ID #	1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 2-Jan-09 (No. 233-3013_Jan09) 9-Sep-08 (No. DAE4-660_Sep08) Check Date (in house)	Apr-10 Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Jan-10 Sep-09 Scheduled Check			
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	10 # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S50586 (20b) SN: S5129 (30b) SN: S5129 (30b) SN: 3013 SN: 660	1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 2-Jan-09 (No. ES3-3013_Jan09) 9-Sep-08 (No. DAE4-660_Sep08)	Apr-10 Apr-10 Apr-10 Mar-10 Mar-10 Jan-10 Sep-09			
Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700	1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 2-Jan-09 (No. 253-3013_Jan09) 9-Sep-08 (No. DAE4-660_Sep08) Check Date (in house) 4-Aug-99 (in house check Oct-07)	Apr-10 Apr-10 Apr-10 Mar-10 Mar-10 Jan-10 Jan-10 Sep-09 Scheduled Check In house check: Oct-09 In house check: Oct-09			
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5026 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700 US37390585	1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 2-Jan-09 (No. ES3-3013_Jan09) 9-Sep-08 (No. DAE4-660_Sep08) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08)	Apr-10 Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Jan-10 Sep-09 Scheduled Check In house check: Oct-09			
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700 US37390585 Name	1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 2-Jan-09 (No. 2S3-3313_Jan09) 9-Sep-08 (No. DAE4-660_Sep08) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08) Function	Apr-10 Apr-10 Apr-10 Mar-10 Mar-10 Jan-10 Jan-10 Sep-09 Scheduled Check In house check: Oct-09 In house check: Oct-09			





SWIS

BR

S Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura S swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

### Glossary:

TSL NORMx,y,z ConvF DCP Polarization φ Polarization θ tissue simulating liquid sensitivity in free space sensitivity in TSL / NORMx,y,z diode compression point φ rotation around probe axis θ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., θ = 0 is normal to probe axis

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

#### Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization θ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z \* frequency\_response (see Frequency Response Chart). This
  linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of
  the frequency response is included in the stated uncertainty of ConvF.
- DCPx, y, z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ES3-3071\_Jun09

Page 2 of 9



June 22, 2009

# Probe ES3DV3

# SN:3071

Manufactured: Last calibrated: Repaired: Recalibrated: December 14, 2004 July 23, 2008 June 8, 2009 June 22, 2009

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: ES3-3071\_Jun09

Page 3 of 9



June 22, 2009

# DASY - Parameters of Probe: ES3DV3 SN:3071

Sensitivity in Free Space<sup>A</sup>

Diode Compression<sup>B</sup>

NormX	1.30 ± 10.1%	$\mu V/(V/m)^2$	DCP X	94 mV
NormY	1.25 ± 10.1%	$\mu V/(V/m)^2$	DCP Y	93 mV
NormZ	1.00 ± 10.1%	$\mu V/(V/m)^2$	DCP Z	94 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

### **Boundary Effect**

TSL		

TSL

900 MHz Typical SAR gradient: 5 % per mm

Sensor Center	to Phanto	om Surface Distance	3.0 mm	4.0 mm
SAR <sub>be</sub> [%]	Withou	t Correction Algorithm	10.3	5.9
SAR <sub>be</sub> [%]	With C	orrection Algorithm	0.9	0.5
175	50 MHz	Typical SAR gradient: 10 %	6 per mm	

Sensor Cente	r to Phantom Surface Distance	3.0 mm	4.0 mm
SAR <sub>be</sub> [%]	Without Correction Algorithm	9.0	5.2
SAR <sub>be</sub> [%]	With Correction Algorithm	0.8	0.5

### Sensor Offset

Probe Tip to Sensor Center

2.0 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 8)

<sup>8</sup> Numerical linearization parameter: uncertainty not required.

Certificate No: ES3-3071\_Jun09


Page 4 of 9



June 22, 2009



(TEM-Cell:ifi110 EXX, Waveguide: R22)

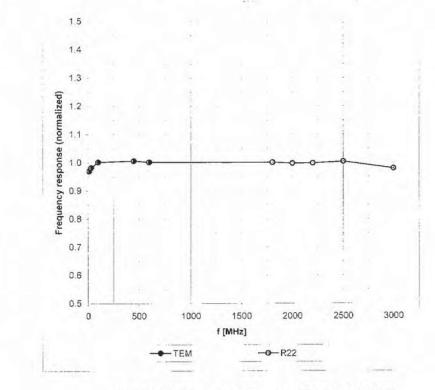


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: ES3-3071\_Jun09

Page 5 of 9



June 22, 2009

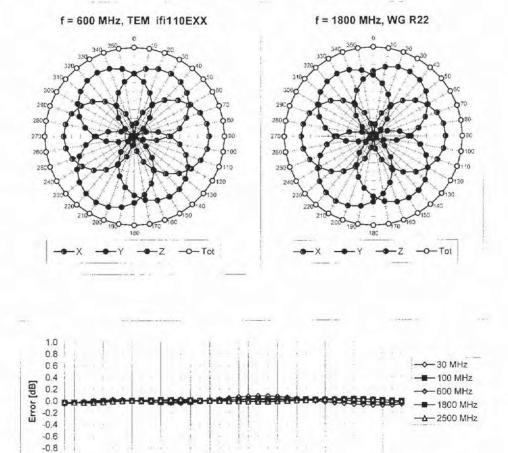

# Receiving Pattern ( $\phi$ ), $\vartheta = 0^{\circ}$

Certificate No: ES3-3071\_Jun09

-1.0 0

60

120

Page 6 of 9

180

¢ [°]

240


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

300



June 22, 2009



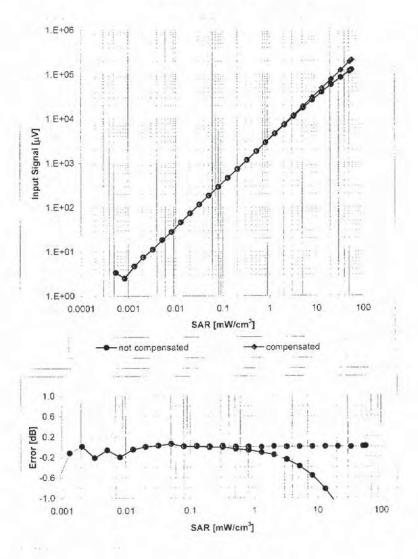


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: ES3-3071\_Jun09


Page 7 of 9



June 22, 2009



# **Conversion Factor Assessment**



f [MHz]	Validity [MHz] <sup>C</sup>	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
835	± 50 / ± 100	Head	41.5 ± 5%	0.90 ± 5%	0.99	1.07	5.58 ± 11.0% (k=2)
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.89	1.10	5.41 ± 11.0% (k=2)
1750	± 50 / ± 100	Head	40.1 ± 5%	1.37 ± 5%	0.48	1.50	4.82 ± 11.0% (k=2)
1900	± 50/± 100	Head	40.0 ± 5%	1.40 ± 5%	0.48	1.52	4.63 ± 11.0% (k=2)
2000	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.51	1.47	4.53 ± 11.0% (k=2)
2450	± 50/±100	Head	39.2 ± 5%	1.80 ± 5%	0.51	1.58	4.13 ± 11.0% (k=2)
835	± 50 / ± 100	Body	55.2 ± 5%	0.97 ± 5%	0.95	1.12	5.59 ± 11.0% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.99	1.09	5.44 ± 11.0% (k=2)
1750	± 50 / ± 100	Body	53.4 ± 5%	1.49 ± 5%	0.34	2.03	4.48 ± 11.0% (k=2)
1900	± 50/±100	Body	53.3 ± 5%	1.52 ± 5%	0.29	2.64	4.26 ± 11.0% (k=2)
2000	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.34	2.25	4.32 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.92	1.12	4.00 ± 11.0% (k=2)

<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Certificate No: ES3-3071\_Jun09


Page 8 of 9



June 22, 2009

# Deviation from Isotropy in HSL

Error (¢, 3), f = 900 MHz

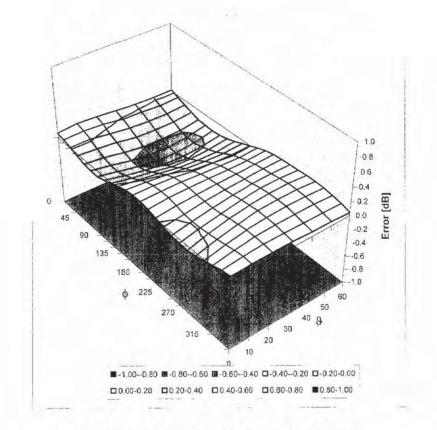

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ES3-3071\_Jun09

Page 9 of 9





SWISS S CHUBRAT С s

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Certificate No: DAE4-541\_Feb09

ATL (Auden)		Certificate	
ALIBRATION C	ERTIFICATE		
Dbject	DAE4 - SD 000 D	04 BJ - SN: 541	
Calibration procedure(s)	QA CAL-06.v12 Calibration proceed	dure for the data acquisition e	electronics (DAE)
Calibration date:	February 10, 2009	9	
Condition of the calibrated item	In Tolerance		
The measurements and the uncer All calibrations have been conduc	rtainties with confidence protection the closed laboratory	onal standards, which realize the physica obability are given on the following page y facility: environment temperature (22 ±	s and are part of the certificate.
Calibration Equipment used (M&T	E critical for calibration)		
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
rimary Standards luke Process Calibrator Type 70	ID # 02 SN: 6295803	30-Sep-08 (No: 7673)	Sep-09
Primary Standards Iuke Process Calibrator Type 70	ID #		
Primary Standards Fluke Process Calibrator Type 70 Keithley Multimeter Type 2001	ID # 02 SN: 6295803	30-Sep-08 (No: 7673)	Sep-09
Primary Standards Fluke Process Calibrator Type 70 Keithley Multimeter Type 2001 Secondary Standards	ID # 2 SN: 6295803 SN: 0810278	30-Sep-08 (No: 7673) 30-Sep-08 (No: 7670) Check Date (in house)	Sep-09 Sep-09
Primary Standards Fluke Process Calibrator Type 70 Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ID # 2 SN: 6295803 SN: 0810278 ID #	30-Sep-08 (No: 7673) 30-Sep-08 (No: 7670) Check Date (in house)	Sep-09 Sep-09 Scheduled Check In house check: Jun-09 Signature
Primary Standards Fluke Process Calibrator Type 70 Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ID #           I2         SN: 6295803           SN: 0810278           ID #           SE UMS 006 AB 1004	30-Sep-08 (No: 7673) 30-Sep-08 (No: 7670) Check Date (in house) 06-Jun-08 (in house check) Function	Sep-09 Sep-09 Scheduled Check In house check: Jun-09 Signature
Primary Standards Fluke Process Calibrator Type 70 Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ID #           I2         SN: 6295803           SN: 0810278           ID #           SE UMS 006 AB 1004	30-Sep-08 (No: 7673) 30-Sep-08 (No: 7670) Check Date (in house) 06-Jun-08 (in house check) Function	Sep-09 Sep-09 Scheduled Check In house check: Jun-09
Primary Standards Fluke Process Calibrator Type 70 Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ID #           I2         SN: 6295803           SN: 0810278           ID #           SE UMS 006 AB 1004           Name           Daniel Hess	30-Sep-08 (No: 7673) 30-Sep-08 (No: 7670) Check Date (in house) 06-Jun-08 (in house check) Function Techniclan	Sep-09 Sep-09 Scheduled Check In house check: Jun-09 Signature





GNISS C. C. Z. Pr/BRIATI

S

С

S

Schweizerischer Kalibrierdienst Service sulsse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

### Glossary

DAE Connector angle data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

### Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a
  result from the performance test and require no uncertainty.
  - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
  - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
  - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
  - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - Input resistance: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - *Power consumption:* Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-541\_Feb09

Page 2 of 5



# DC Voltage Measurement

A/D - Converter Reso	olution nominal			
High Range:	1LSB =	6.1µV,	full range =	-100+300 mV
Low Range:	1LSB =	61nV ,	· · · · · ·	-1+3mV
DASY measurement	parameters: Aut	o Zero Time:	3 sec; Measuring	time: 3 sec

Calibration Factors	X	Y	Z
High Range	404.590 ± 0.1% (k=2)	$404.475 \pm 0.1\%$ (k=2)	404.230 ± 0.1% (k=2)
Low Range	3.96369 ± 0.7% (k=2)	$3.95198 \pm 0.7\%$ (k=2)	$3.96911 \pm 0.7\%$ (k=2)

### **Connector Angle**

Connector Angle to be used in DASY system	290 ° ± 1 °
Connector Angle to be used in DACT system	

Certificate No: DAE4-541\_Feb09

Page 3 of 5



### Appendix

### 1. DC Voltage Linearity

High Range	Input (µV)	Reading (µV)	Error (%)
Channel X + Input	200000	200000	0.00
Channel X + Input	20000	20006.58	0.03
Channel X - Input	20000	-19998.29	-0.01
Channel Y + Input	200000	200000.1	0.00
Channel Y + Input	20000	20000.17	0.00
Channel Y - Input	20000	-20003.10	0.02
Channel Z + Input	200000	200000.1	0.00
Channel Z + Input	20000	20004.44	0.02
Channel Z - Input	20000	-19998.76	-0.01

Low Range	Input (µV)	Reading (µV)	Error (%)
Channel X + Input	2000	2000.1	0.00
Channel X + Input	200	199.81	-0.09
Channel X - Input	200	-200.41	0.20
Channel Y + Input	2000	2000.1	0.00
Channel Y + Input	200	199.52	-0.24
Channel Y - Input	200	-200.54	0.27
Channel Z + Input	2000	2000.1	0.00
Channel Z + Input	200	199.17	-0.42
Channel Z - Input	200	-201.07	0.53

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	11.35	10.66
	- 200	-10.12	-10.20
Channel Y	200	1.63	1.34
	- 200	-2.00	-2.45
Channel Z	200	1.36	0.91
	- 200	-1.75	-2.09

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (μV)
Channel X	200	-	3.55	-0.09
Channel Y	200	0.32	-	5.22
Channel Z	200	-0.36	0.33	(1-1)

Certificate No: DAE4-541\_Feb09

Page 4 of 5



### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15992	15779
Channel Y	15779	15842
Channel Z	15970	16928

### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input  $10 M \Omega$ 

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	-0.06	-0.79	0.84	0.26
Channel Y	-0.72	-1.57	0.26	0.32
Channel Z	-0.95	-2.45	0.17	0.33

### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

### 7. Input Resistance

	Zeroing (MOhm)	Measuring (MOhm)
Channel X	0.2000	198.8
Channel Y	0.2000	202.2
Channel Z	0.2000	202.5

#### 8. Low Battery Alarm Voltage (verified during pre test)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

### 9. Power Consumption (verified during pre test)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.0	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE4-541\_Feb09

Page 5 of 5