

SAR EVALUATION REPORT

For

BUFFALO INC.

4-15, Shibata Hondori, Minami-ku,
Nagoya, 457-8520, Japan

FCC ID: FDI-09102036-0
MODEL: WLI-CB-AG300N

This Report Concerns: <input checked="" type="checkbox"/> Original Report		Product Name: 802.11 a/b/g/n-draft Client Card Bus
Test Engineer:	Eric Hong <i>HONG</i>	
Report No.:	R0610232-SAR	
Report Date:	2006-11-27	
Reviewed By:	Daniel Deng <i>[Signature]</i>	
Prepared By: (HW)	Bay Area Compliance Laboratories Corp. 1274 Anvilwood Ave. Sunnyvale, CA 94089, USA Tel: (408) 732-9162 Fax: (408) 732 9164	

Note: This test report is for the customer shown above and their specific product only. It may not be duplicated or used in part without prior written consent from Bay Area Compliance Laboratories Corp. This report **must not** be used by the customer to claim product certification, approval, or endorsement by NVLAP or any agency of the U.S. Government.

DECLARATION OF COMPLIANCE SAR EVALUATION


Rule Part(s):	FCC §2.1093 & IEEE 1528:2003
Test Procedure(s):	FCC OET Bulletin 65 Supplement C & IEEE 1528
Device Type:	Wireless Notebook Adapter
Model:	WLI-CB-AG300N
Modulation:	802.11a/b/g/n
TX Frequency Range:	2412-2462 MHz 2422/2452 MHz 5180 -5240 MHz 5190/5230 MHz 5260-5320 MHz 5270/5310 MHz
Max. Combined Conducted Power :	(2.4 GHz) 11 Mbps for 802.11b 20 MHz – 21.86 dBm (2.4 GHz) 11 Mbps for 802.11b 40 MHz – 20.80 dBm (2.4 GHz) 54 Mbps for 802.11g 20 MHz – 21.86 dBm (2.4 GHz) 54 Mbps for 802.11g 40 MHz – 19.59 dBm (2.4 GHz) MCS 11 for 802.11n HT 20 – 21.67 dBm (2.4 GHz) MCS 15 for 802.11n HT 40 – 21.68 dBm (5 GHz) 52W 9 Mbps for 802.11a 20 MHz – 16.94 dBm (5 GHz) 52W 9 Mbps for 802.11a 40 MHz – 16.84 dBm (5 GHz) 52W MCS 0 for 802.11n HT 20 – 16.88 dBm (5 GHz) 52W MCS 0 for 802.11n HT 40 – 16.94 dBm (5 GHz) 53W 9 Mbps for 802.11a 20 MHz – 21.50 dBm (5 GHz) 53W 9 Mbps for 802.11a 40 MHz – 20.43 dBm (5 GHz) 53W MCS 0 for 802.11n HT 20 – 21.46 dBm (5 GHz) 53W MCS 0 for 802.11n HT 40 – 21.35 dBm
Antenna Type(s):	Integral Antenna
Measured SAR Value:	(2.4 GHz) 11 Mbps for 802.11b 20 MHz – 0.851 mw/g (2.4 GHz) 11 Mbps for 802.11b 40 MHz – 0.545 mw/g (2.4 GHz) 54 Mbps for 802.11g 20 MHz – 0.853 mw/g (2.4 GHz) 54 Mbps for 802.11g 40 MHz – 0.542 mw/g (2.4 GHz) MCS 11 for 802.11n HT 20 – 0.717 mw/g (2.4 GHz) MCS 15 for 802.11n HT 40 – 0.788 mw/g (5 GHz) W52 9 Mbps for 802.11a 20 MHz – 0.395 mw/g (5 GHz) W52 9 Mbps for 802.11a 40 MHz – 0.259 mw/g (5 GHz) W52 MCS 0 for 802.11n HT 20 – 0.309 mw/g (5 GHz) W52 MCS 0 for 802.11n HT 40 – 0.381 mw/g (5 GHz) W53 9 Mbps for 802.11a 20 MHz – 0.351 mw/g (5 GHz) W53 9 Mbps for 802.11a 40 MHz – 0.266 mw/g (5 GHz) W53 MCS 0 for 802.11n HT 20 – 0.315 mw/g (5 GHz) W53 MCS 0 for 802.11n HT 40 – 0.363 mw/g
<p>BACL Corp. declares under its sole responsibility that this wireless portable device has been determined to be in compliance for localized specific absorption rate (SAR) for uncontrolled exposure and general population exposure limits specified in FCC OET Bulletin 65 Supplement C and has been tested in accordance with the measurement procedures specified in ANSI C95.3:2002 & IEEE 1528.</p> <p>All measurements reported herein were performed under my supervision and believed to be accurate to the best of my knowledge. I further attest for the completeness of these measurements and vouch for the qualifications any and all personnel performing such measurements.</p> <p style="text-align: center;">The results and statements contained in this report pertain only to the device(s) evaluated.</p>	
<p><u>/signature/</u></p> <p style="text-align: center; font-size: 2em;"><i>Hong</i></p> <p>Eric Hong</p> <p>Bay Area Compliance Laboratories Corp.</p>	

TABLE OF CONTENTS

REFERENCE, STANDARDS, AND GUIDELINES..... 4
 SAR LIMITS 5
EUT DESCRIPTION..... 6
 EUT PHOTO 6
DESCRIPTION OF TEST SYSTEM..... 7
 TEST FACILITY 7
 MEASUREMENT SYSTEM DIAGRAM..... 9
 SYSTEM COMPONENTS 10
TESTING EQUIPMENT 18
 EQUIPMENTS LIST & CALIBRATION INFO 18
SAR MEASUREMENT SYSTEM VERIFICATION..... 19
 SYSTEM ACCURACY VERIFICATION 19
EUT TEST STRATEGY AND METHODOLOGY 20
 SAR EVALUATION PROCEDURE 20
CONCLUSION 21
 SAR BODY & HEAD WORST-CASE TEST DATA 21
APPENDIX A – MEASUREMENT UNCERTAINTY..... 27
APPENDIX B – PROBE CALIBRATION CERTIFICATES 29
APPENDIX C – DIPOLE CALIBRATION CERTIFICATES..... 49
APPENDIX D - TEST SYSTEM VERIFICATIONS SCANS 69
 LIQUID MEASUREMENT RESULT..... 69
APPENDIX E - EUT SCANS..... 74
APPENDIX F – CONDUCTED OUTPUT POWER MEASUREMENT..... 128
 PROVISION APPLICABLE 128
 TEST PROCEDURE..... 128
 TEST EQUIPMENT..... 128
 TEST RESULTS 128
APPENDIX G – EUT TEST POSITION PHOTOS..... 130
 EUT WITH ACER LAPTOP BACK TOUCHING TO THE FLAT PHANTOM FRONT VIEW 130
 EUT WITH IBM LAPTOP BACK TOUCHING TO THE FLAT PHANTOM FRONT VIEW 130
 EUT WITH SONY LAPTOP BACK TOUCHING TO THE FLAT PHANTOM FRONT VIEW 131
APPENDIX H– EUT PHOTO 132
 EUT – FRONT VIEW 132
 EUT – REAR VIEW 132
 EUT – PORT VIEW..... 133
 EUT – COMPONENT VIEW 1 133
 EUT – COMPONENT VIEW 2 134
 EUT – COMPONENT VIEW 3 134
APPENDIX I - INFORMATIVE REFERENCES 135
APPENDIX J– SPEAG EQUIPMENT EVALUATION REPORT 136

REFERENCE, STANDARDS, AND GUIDELINES

FCC:

The Report and Order requires routine SAR evaluation prior to equipment authorization of portable transmitter devices, including portable telephones. For consumer products, the applicable limit is 1.6 mw/g as recommended by the ANSI/IEEE standard C95.1-1992 [6] for an uncontrolled environment (Paragraph 65). According to the Supplement C of OET Bulletin 65 "Evaluating Compliance with FCC Guide-lines for Human Exposure to Radio frequency Electromagnetic Fields", released on Jun 29, 2001 by the FCC, the device should be evaluated at maximum output power (radiated from the antenna) under "worst-case" conditions for normal or intended use, incorporating normal antenna operating positions, device peak performance frequencies and positions for maximum RF energy coupling.

This report describes the methodology and results of experiments performed on wireless data terminal. The objective was to determine if there is RF radiation and if radiation is found, what is the extent of radiation with respect to safety limits. SAR (Specific Absorption Rate) is the measure of RF exposure determined by the amount of RF energy absorbed by human body (or its parts) – to determine how the RF energy couples to the body or head which is a primary health concern for body worn devices. The limit below which the exposure to RF is considered safe by regulatory bodies in North America is 1.6 mw/g average over 1 gram of tissue mass.

CE:

The order requires routine SAR evaluation prior to equipment authorization of portable transmitter devices, including portable telephones. For consumer products, the applicable limit is 2 mw/g as recommended by the EN50360 for an uncontrolled environment. According to the Standard, the device should be evaluated at maximum output power (radiated from the antenna) under "worst-case" conditions for normal or intended use, incorporating normal antenna operating positions, device peak performance frequencies and positions for maximum RF energy coupling.

This report describes the methodology and results of experiments performed on wireless data terminal. The objective was to determine if there is RF radiation and if radiation is found, what is the extent of radiation with respect to safety limits. SAR (Specific Absorption Rate) is the measure of RF exposure determined by the amount of RF energy absorbed by human body (or its parts) – to determine how the RF energy couples to the body or head which is a primary health concern for body worn devices. The limit below which the exposure to RF is considered safe by regulatory bodies in Europe is 2 mw/g average over 10 gram of tissue mass.

The test configurations were laid out on a specially designed test fixture to ensure the reproducibility of measurements. Each configuration was scanned for SAR. Analysis of each scan was carried out to characterize the above effects in the device.

There was no SAR of any concern measured on the device for any of the investigated configurations.

SAR Limits

FCC Limit (1g tissue)

EXPOSURE LIMITS	SAR (W/kg)	
	(General Population / Uncontrolled Exposure Environment)	(Occupational / Controlled Exposure Environment)
Spatial Average (averaged over the whole body)	0.08	0.4
Spatial Peak (averaged over any 1 g of tissue)	1.60	8.0
Spatial Peak (hands/wrists/feet/ankles averaged over 10 g)	4.0	20.0

CE Limit (10g tissue)

EXPOSURE LIMITS	SAR (W/kg)	
	(General Population / Uncontrolled Exposure Environment)	(Occupational / Controlled Exposure Environment)
Spatial Average (averaged over the whole body)	0.08	0.4
Spatial Peak (averaged over any 1 g of tissue)	2.0	10
Spatial Peak (hands/wrists/feet/ankles averaged over 10 g)	4.0	20.0

Population/Uncontrolled Environments are defined as locations where there is the exposure of individual who have no knowledge or control of their exposure.

Occupational/Controlled Environments are defined as locations where there is exposure that may be incurred by people who are aware of the potential for exposure (i.e. as a result of employment or occupation).

General Population/Uncontrolled environments Spatial Peak limit 1.6 W/kg (FCC) & 2 W/kg (CE) applied to the EUT.

EUT DESCRIPTION

This BACL measurement and test report has been prepared on behalf of *Buffalo Inc.*'s product, *FCC ID: FDI-09102036-0*, model number: *WLI-CB-AG300N* or the "EUT" as referred to in this report is an *Air Station Nfiniti High Speed Mode Wireless Notebook Adapter* designed to connect to the PCII or PCIII slot commonly found in notebook style PCs. It also features Buffalo's exclusive Air Station One-Touch Secure System (AOSS) technology, which enables user to setup secure wireless connections to an AOSS-enabled Router. The EUT features 32-Bit card bus technology and 270 Mbps wireless data capability.

This network adapter supports IEEE 802.11a, 802.11b, 802.11g and 802.11n (1.0 Draft) wireless networks. This allows a notebook computer to access the Internet, e-mail, video and transfer files etc. wirelessly.

* *The test data gathered are from a production sample which is provided by the manufacturer with the serial number: NK-3763.*

EUT Photo



Additional EUT photos in Exhibit C

Mechanical Description

The *Buffalo Inc.* product, model number: *WLI-CB-AG300N* measures approximately 122 mm (L) x 54 mm (W) x 4.3 mm (H). The EUT operates at the frequency range of 2412– 2462 MHz (802.11b/g/n) and 5180-5240 MHz (802.11a/n).

DESCRIPTION OF TEST SYSTEM

These measurements were performed with the automated near-field scanning system DASY4 from Schmid & Partner Engineering AG (SPEAG) which is the fourth generation of the system shown in the figure hereinafter:



The system is based on a high precision robot (working range greater than 0.9m), which positions the probes with a positional repeatability of better than $\pm 0.02\text{mm}$. Special E- and H-field probes have been developed for measurements close to material discontinuity, the sensors of which are directly loaded with a Schottky diode and connected via highly resistive lines to the data acquisition unit.

The SAR measurements were conducted with the dosimetric probe ET3DV6 SN: 1604 (manufactured by SPEAG), designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe has been calibrated according to the procedure with accuracy of better than $\pm 10\%$. The spherical isotropy was evaluated with the procedure and found to be better than $\pm 0.25\text{dB}$.

Test Facility

The Test site used by BACL Corp. to collect emissions measurement data is located at it's facility in Sunnyvale, California, USA.

Test site at BACL has been fully described in reports submitted to the Federal Communication Commission (FCC) and Voluntary Control Council for Interference (VCCI). The details of these reports has been found to be in compliance with the requirements of Section 2.948 of the FCC Rules on February 11 and December 10, 1997 and Article 8 of the VCCI regulations on December 25, 1997. The facility also complies with the radiated and AC line conducted test site criteria set forth in ANSI C63.4-2003.

The Federal Communications Commission and Voluntary Control Council for Interference have the reports on file and is listed under FCC registration number: 90464 and VCCI Registration No.: C-1298 and R-1234. The test site has been approved by the FCC and VCCI for public use and is listed in the FCC Public Access Link (PAL) database.

Additionally, BACL is a National Institute of Standards and Technology (NIST) accredited laboratory, under the National Voluntary Laboratory Accredited Program (Lab Code 200167-0). The current scope of accreditations can be found at <http://ts.nist.gov/ts/htdocs/210/214/scopes/2001670.htm>


The phantom used was the Generic Twin Phantom. The ear was simulated as a spacer of 4 mm thickness between the earpiece of the phone and the tissue simulating liquid. The Tissue simulation liquid used for each test is in according with the FCC OET65 supplement C as listed below.

Ingredients (% by weight)	Frequency (MHz)									
	450		835		915		1900		2450	
Tissue Type	Head	Body	Head	Body	Head	Body	Head	Body	Head	Body
Water	38.56	51.16	41.45	52.4	41.05	56.0	54.9	40.4	62.7	73.2
Salt (NaCl)	3.95	1.49	1.45	1.4	1.35	0.76	0.18	0.5	0.5	0.04
Sugar	56.32	46.78	56.0	45.0	56.5	41.76	0.0	58.0	0.0	0.0
HEC	0.98	0.52	1.0	1.0	1.0	1.21	0.0	1.0	0.0	0.0
Bactericide	0.19	0.05	0.1	0.1	0.1	0.27	0.0	0.1	0.0	0.0
Triton X-100	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	36.8	0.0
DGBE	0.0	0.0	0.0	0.0	0.0	0.0	44.92	0.0	0.0	26.7
Dielectric Constant	43.42	58.0	42.54	56.1	42.0	56.8	39.9	54.0	39.8	52.5
Conductivity (S/m)	0.85	0.83	0.91	0.95	1.0	1.07	1.42	1.45	1.88	1.78

IEEE SCC-34/SC-2 P1528 Recommended Tissue Dielectric Parameters

Frequency (MHz)	Head		Body	
	ϵ_r	σ (S/m)	ϵ_r	σ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800-2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00

Measurement System Diagram

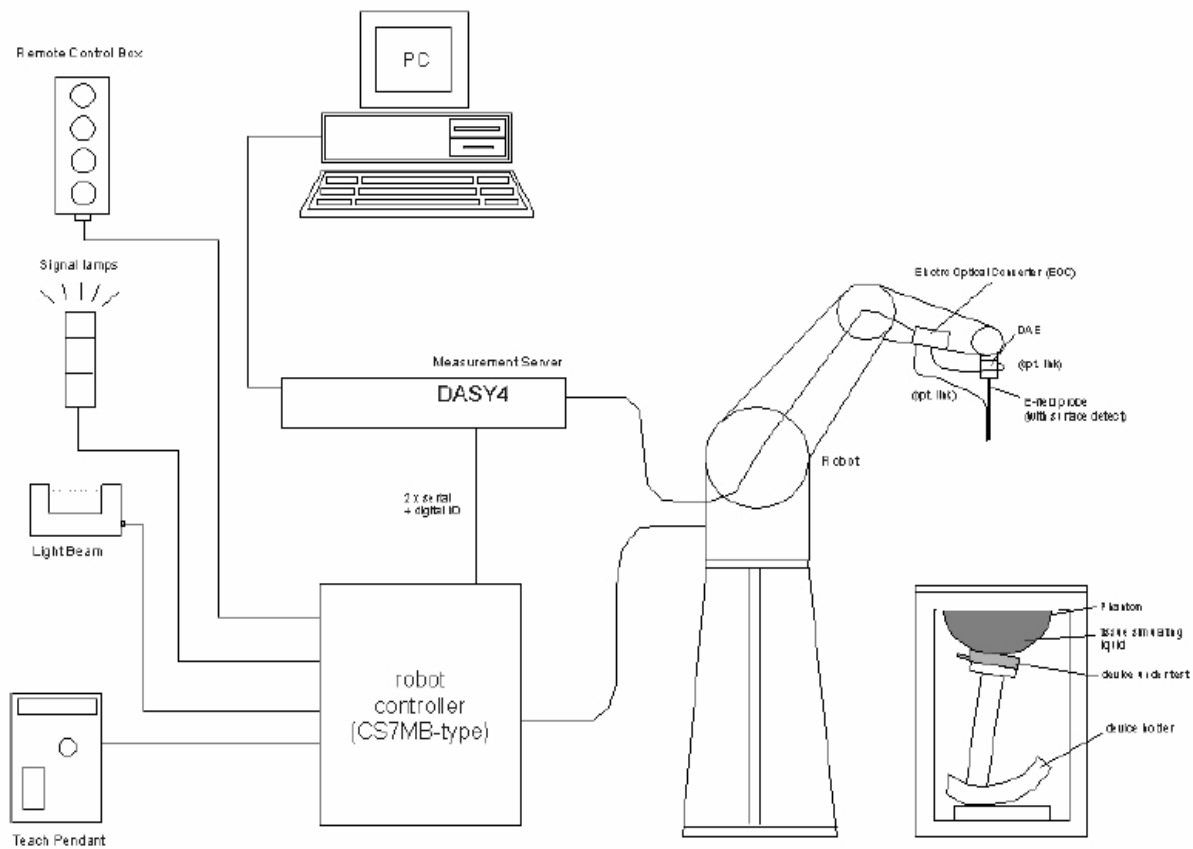

The DASY4 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Stäubli RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A Data Acquisition Electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-Optical Converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows 2000 or Windows XP.

- DASY4 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM twin phantom enabling testing left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing to validate the proper functioning of the system.

System Components

- DASY4 Measurement Server
- Data Acquisition Electronics
- Probes
- Light Beam Unit
- Medium
- SAM Twin Phantom
- Device Holder for SAM Twin Phantom
- System Validation Kits
- Robot

DASY4 Measurement Server

The DASY4 measurement server is based on a PC/104 CPU board with a 166MHz low-power Pentium, 32MB chip disk and 64MB RAM. The necessary circuits for communication with either the DAE4 (or DAE3) electronic box as well as the 16-bit AD-converter system for optical detection and digital I/O interface are contained on the DASY4 I/O-board, which is directly connected to the PC/104 bus of the CPU board.



The measurement server performs all real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operation. The PC-operating system cannot interfere with these time critical processes. All connections are supervised by a watchdog, and disconnection of any of the cables to the measurement server will automatically disarm the robot and disable all program-controlled robot movements. Furthermore, the measurement server is equipped with two expansion slots which are reserved for future applications. Please note that the expansion slots do not have a standardized pinout and therefore only the expansion cards provided by SPEAG can be inserted. Expansion cards from any other supplier could seriously damage the measurement server.

Data Acquisition Electronics

The data acquisition electronics DAE3 consists of a highly sensitive electrometer grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.



Probes

The DASY system can support many different probe types.


Dosimetric Probes: These probes are specially designed and calibrated for use in liquids with high permittivities. They should not be used in air, since the spherical isotropy in air is poor (± 2 dB). The dosimetric probes have special calibrations in various liquids at different frequencies.

Free Space Probes: These are electric and magnetic field probes specially designed for measurements in free space. The z-sensor is aligned to the probe axis and the rotation angle of the x-sensor is specified. This allows the DASY system to automatically align the probe to the measurement grid for field component measurement. The free space probes are generally not calibrated in liquid. (The H-field probes can be used in liquids without any change of parameters.)

Temperature Probes: Small and sensitive temperature probes for general use. They use a completely different parameter set and different evaluation procedures. Temperature rise features allow direct SAR evaluations with these probes.

ET3DV6 Probe Specification


Construction Symmetrical design with triangular core
 Built-in optical fiber for surface detection System
 Built-in shielding against static charges
 Calibration In air from 10 MHz to 2.5 GHz
 In brain and muscle simulating tissue at
 Frequencies of 450 MHz, 900 MHz and
 1.8 GHz (accuracy $\pm 8\%$)
 Frequency 10 MHz to > 6 GHz; Linearity: ± 0.2 dB
 (30 MHz to 3 GHz)
 Directivity ± 0.2 dB in brain tissue (rotation around
 probe axis)
 ± 0.4 dB in brain tissue (rotation normal probe axis)
 Dynamic 5 mw/g to > 100 mw/g;
 Range Linearity: ± 0.2 dB
 Surface ± 0.2 mm repeatability in air and clear liquids
 Detection over diffuse reflecting surfaces.
 Dimensions Overall length: 330 mm
 Tip length: 16 mm

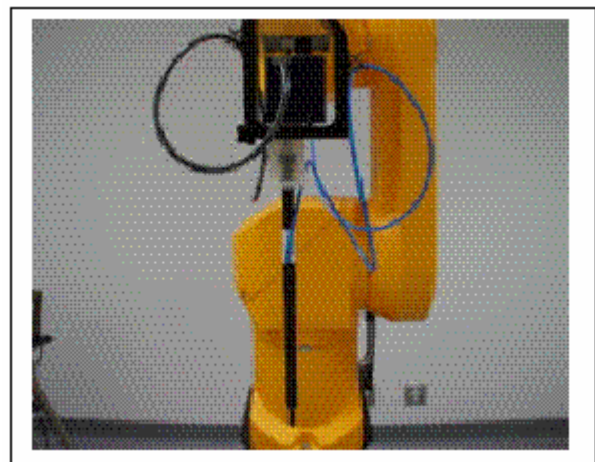

Photograph of the probe

Body diameter: 12 mm
 Tip diameter: 6.8 mm
 Distance from probe tip to dipole centers: 2.7 mm
 Application General dosimetric up to 3 GHz
 Compliance tests of mobile phones
 Fast automatic scanning in arbitrary phantoms

The SAR measurements were conducted with the dosimetric probe ET3DV6 designed in the classical triangular configuration and optimized for dosimetric evaluation. The probe is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multi-fiber line ending at the front of the probe tip. It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY3 software reads the reflection during a software approach and looks for the maximum using a 2nd order fitting. The approach is stopped when reaching the maximum.

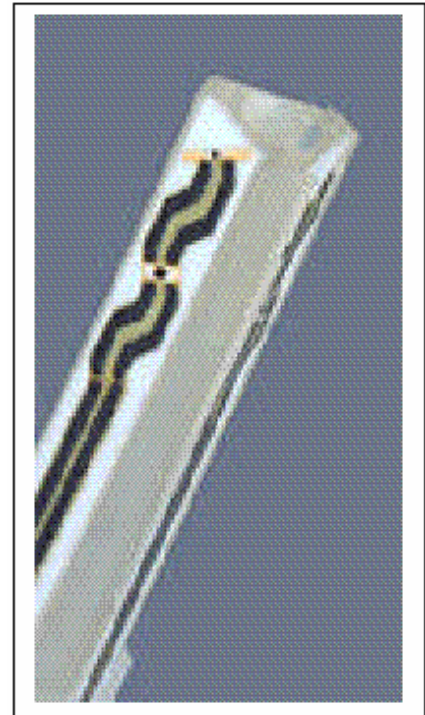

**Inside view of
ET3DV6 E-field Probe**

E-Field Probe Calibration Process

Each probe is calibrated according to a dosimetric assessment procedure described in [6] with accuracy better than +/- 10%. The spherical isotropy was evaluated with the procedure described in [7] and found to be better than +/-0.25dB. The sensitivity parameters (NormX, NormY, NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested.

The free space E-field from amplified probe outputs is determined in a test chamber. This is performed in a TEM cell for frequencies below 1 GHz, and in a waveguide above 1 GHz for free space. For the free space calibration, the probe is placed in the volumetric center of the cavity and at the proper orientation with the field. The probe is then rotated 360 degrees.

E-field temperature correlation calibration is performed in a flat phantom filled with the appropriate simulated brain tissue. The measured free space E-field in the medium correlates to temperature rise in dielectric medium. For temperature correlation calibration a RF transparent thermistor-based temperature probe is used in conjunction with the E-field probe.

Data Evaluation

The DASY4 post-processing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe parameters: - Sensitivity	Normi, ai0, ai1, ai2
- Conversion factor	ConvFi
- Diode compression point	dcpi

Device parameters: - Frequency	f
- Crest factor	cf
Media parameters: - Conductivity	σ
- Density	ρ

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASYS components. In the direct measuring mode of the multi-meter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

With V_i = compensated signal of channel i (i = x, y, z)
 U_i = input signal of channel i (i = x, y, z)
 cf = crest factor of exciting field (DASY parameter)
 dcp_i = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

$$\text{E - fieldprobes : } E_i = \sqrt{\frac{V_i}{\text{Norm}_i \cdot \text{ConvF}}}$$

$$\text{H - fieldprobes : } H_i = \sqrt{V_i} \cdot \frac{a_{i0} + a_{i1}f + a_{i2}f^2}{f}$$

With V_i = compensated signal of channel i (i = x, y, z)
 Norm_i = sensor sensitivity of channel i (i = x, y, z)
 $\mu\text{V}/(\text{V/m})^2$ for E-field probes
 ConvF = sensitivity enhancement in solution
 a_{ij} = sensor sensitivity factors for H-field probes
 f = carrier frequency [GHz]
 E_i = electric field strength of channel i in V/m
 H_i = diode compression point (DASY parameter)

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1'000}$$

With SAR = local specific absorption rate in mW/g
 E_{tot} = total field strength in V/m
 σ = conductivity in [mho/m] or [Siemens/m]
 ρ = equivalent tissue density in g/cm³

Note that the density is normally set to 1, to account for actual brain density rather than the density of the simulation liquid.

Light Beam Unit

The light beam switch allows automatic "tooling" of the probe. During the process, the actual position of the probe tip with respect to the robot arm is measured, as well as the probe length and the horizontal probe offset. The software then corrects all movements, so that the robot coordinates are valid for the probe tip. The repeatability of this process is better than 0.1 mm. If a position has been taught with an aligned probe, the same position will be reached with another aligned probe within 0.1 mm, even if the other probe has different dimensions. During probe rotations, the probe tip will keep its actual position.

Medium

Parameters

The parameters of the tissue simulating liquid strongly influence the SAR in the liquid. The parameters for the different frequencies are defined in the corresponding compliance standards (e.g., EN 50361, IEEE 1528-2003).

Parameter measurements

Several measurement systems are available for measuring the dielectric parameters of liquids:

- The open coax test method (e.g., HP85070 dielectric probe kit) is easy to use, but has only moderate accuracy. It is calibrated with open, short, and deionized water and the calibrations a critical process.
- The transmission line method (e.g., model 1500T from DAMASKOS, INC.) measures the transmission and reflection in a liquid filled high precision line. It needs standard two port calibration and is probably more accurate than the open coax method.
- The reflection line method measures the reflection in a liquid filled shorted precision lined, the method is not suitable for these liquids because of its low sensitivity.
- The slotted line method scans the field magnitude and phase along a liquid filled line. The evaluation is straight forward and only needs a simple response calibration. The method is very accurate, but can only be used in high loss liquids and at frequencies above 100 to 200MHz. Cleaning the line can be tedious.

SAM Twin Phantom

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- Left hand
- Right hand
- Flat phantom

The phantom table comes in two sizes: A 100 x 50 x 85 cm (L x W x H) table for use with free standing robots (DASY4 professional system option) or as a second phantom and a 100 x 75 x 85 cm(L x W x H) table with reinforcements for table mounted robots (DASY4 compact system option) .

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. Only one device holder is necessary if two phantoms are used (e.g., for different liquids) A white cover is provided to tap the phantom during o_-periods to prevent water evaporation and changes in the liquid parameters. Free space scans of devices on the cover are possible. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.


The phantom can be used with the following tissue simulating liquids:

- Water-sugar based liquids can be left permanently in the phantom. Always cover the liquid if the system is not used, otherwise the parameters will change due to water evaporation.
- Glycol based liquids should be used with care. As glycol is a softener for most plastics, the liquid should be taken out of the phantom and the phantom should be dried when the system is not used (desirable at least once a week).
- Do not use other organic solvents without previously testing the phantom resistiveness.



Device Holder for SAM Twin Phantom

The SAR in the phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source in 5mm distance, a positioning uncertainty of $\pm 0.5\text{mm}$ would produce a SAR uncertainty of $\pm 20\%$. An accurate device positioning is therefore crucial for accurate and repeatable measurements. The positions, in which the devices must be measured, are defined by the standards. The DASY device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation centers for both scales are the ear reference point (ERP). Thus the device needs no repositioning when changing the angles.

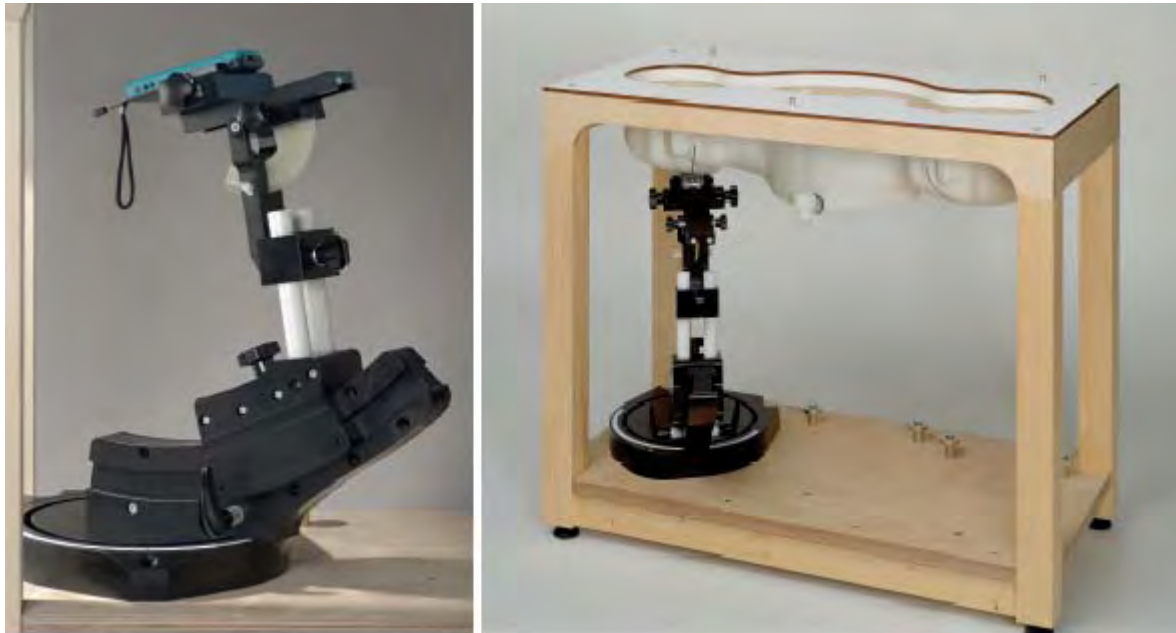

The DASY device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity $\epsilon_r=3$ and loss tangent $\tan \delta=0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.

System Validation Kits

Each DASY system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY software, enable the user to conduct the system performance check and system validation. For that purpose a well defined SAR distribution in the flat section of the SAM twin phantom is produced.

System validation kit includes a dipole, tripod holder to fix it underneath the flat phantom and a corresponding distance holder. Dipoles are available for the variety of frequencies between 300MHz and 6 GHz (dipoles for other frequencies or media and other calibration conditions are available upon request).

The dipoles are highly symmetric and matched at the center frequency for the specified liquid and distance to the flat phantom (or flat section of the SAM-twin phantom). The accurate distance between the liquid surface and the dipole center is achieved with a distance holder that snaps on the dipole.

Robot

The DASY4 system uses the high precision industrial robots RX60L, RX90 and RX90L, as well as the RX60BL and RX90BL types out of the newer series from Stäubli SA (France). The RX robot series offers many features that are important for our application:

- High precision (repeatability 0.02mm)
- High reliability (industrial design)
- Low maintenance costs (virtually maintenance-free due to direct drive gears; no belt drives)
- Jerk-free straight movements (brushless synchrony motors; no stepper motors)
- Low ELF interference (the closed metallic construction shields against motor control fields)

For the newly delivered DASY4 systems as well as for the older DASY3 systems delivered since 1999, the CS7MB robot controller version from Stäubli is used. Previously delivered systems have either a CS7 or CS7M controller; the differences to the CS7MB are mainly in the hardware, but some procedures in the robot software from Stäubli are also not completely the same. The following descriptions about robot hard- and software correspond to CS7MB controller with software version 13.1 (edit S5). The actual commands, procedures and configurations, also including details in hardware, might differ if an older robot controller is in use. In this case please also refer to the Stäubli manuals for further information.



TESTING EQUIPMENT

Equipments List & Calibration Info

Type / Model	Calibration Due Date	S/N:
DASY4 Professional Dosimetric System	N/A	N/A
Robot RX60L	N/A	CS7MBSP / 467
Robot Controller	N/A	F01/5J72A1/A/01
Dell Computer Demension 3000	N/A	N/A
SPEAG EDC3	N/A	N/A
SPEAG DAE3	2006-10-18*	456
DASY4 Measurement Server	N/A	1176
Probe, SAR Sensor EX3DV4	2007-04-20	3576
SPEAG E-Field Probe ET3DV6	2007-05-02	1604
Antenna, Dipole, D5100V2	2007-05-03	1001
Antenna Dipole D-2450-S-1	2007-08-28	BCL-141
SPEAG Generic Twin Phantom	N/A	N/A
SPEAG Light Alignment Sensor	N/A	278
Brain Equivalent Matter (2450MHz)	N/A	N/A
Muscle Equivalent Matter (2450MHz)	N/A	N/A
Brain Equivalent Matter (5GHz)	N/A	N/A
Muscle Equivalent Matter (5GHz)	N/A	N/A
Robot Table	N/A	N/A
Phone Holder	N/A	N/A
Phantom Cover	N/A	N/A
Agilent, Spectrum Analyzer 8565EC	2007-11-06	2240A01930
Microwave Amp. 8349A	N/A	2644A02662
Power Meter Agilent E4419B	2007-09-13	MY4121511
Power Sensor Agilent E4412A	2007-10-12	MY41497252
Agilent, Wireless Communications Test Set 8960 Series 10	2007-08-08	E5515C
Dielectric Probe Kit HP85070A	N/A	US99360201
HP, Microwave Frequency Counter 5342A	2006-12-12	2232A06383
Amplifier, ST181-20	N/A	E012-0101
Antenna, Horn SAS-200/571	2007-04-20	A052704

**Please see SPEAG Evaluation Report featured the Appendix of this test report for verification of calibration succeeding the listed due date.*

SAR MEASUREMENT SYSTEM VERIFICATION

System Accuracy Verification

Prior to the assessment, the system validation kit was used to test whether the system was operating within its specifications of $\pm 10\%$. The validation results are tabulated below. And also the corresponding SAR plot is attached as well in the SAR plots files.

IEEE P1528 recommended reference value for head

Frequency (MHz)	1 g SAR	10 g SAR	Local SAR at surface (above feed point)	Local SAR at surface (v=2cm offset from feed point)
300	3.0	2.0	4.4	2.1
450	4.9	3.3	7.2	3.2
835	9.5	6.2	14.1	4.9
900	10.8	6.9	16.4	5.4
1450	29.0	16.0	50.2	6.5
1800	38.1	19.8	69.5	6.8
1900	39.7	20.5	72.1	6.6
2000	41.1	21.1	74.6	6.5
2450	52.4	24.0	104.2	7.7
3000	63.8	25.7	140.2	9.5

Validation Dipole SAR Reference Test Result for Body (2450 MHz)

Validation Measurement	SAR @ 0.025mW Input averaged over 1g	SAR @ 1W Input averaged over 1g	SAR @ 0.025mW Input averaged over 10g	SAR @ 1W Input averaged over 10g
Test 1	14.2	56.80	6.33	25.32
Test 2	14.3	57.20	6.34	25.36
Test 3	14.2	56.80	6.33	25.32
Test 4	14.1	56.40	6.32	25.28
Test 5	14.3	57.20	6.33	25.32
Test 6	14.0	56.00	6.31	25.24
Test 7	14.2	56.80	6.33	25.32
Test 8	14.2	56.80	6.33	25.32
Test 9	14.4	57.60	6.34	25.36
Test 10	14.2	56.80	6.32	25.28
Average	14.21	56.84	6.32	25.31

Reference SAR Values for 5GHz

f (GHz)	Head Tissue			Body Tissue		
	SAR 1g	SAR 10g	SAR peak	SAR 1g	SAR 10g	SAR peak
5.0	72.9	20.7	285.6	68.1	19.2	260.3
5.1	74.6	21.1	297.5	78.8	19.6	272.3
5.2	76.5	21.6	310.3	71.8	20.1	284.7
5.5	83.3	23.4	349.4	79.1	22.0	326.3
5.8	78.0	21.9	340.9	74.1	20.5	324.7

EUT TEST STRATEGY AND METHODOLOGY

SAR Evaluation Procedure

The evaluation was performed with the following procedure:

Step 1: Measurement of the SAR value at a fixed location above the ear point or central position was used as a reference value for assessing the power drop.

Step 2: The SAR distribution at the exposed side of the head was measured at a distance of 3.9 mm from the inner surface of the shell. The area covered the entire dimension of the head or EUT and the horizontal grid spacing was 20 mm x 20 mm. Based on these data, the area of the maximum absorption was determined by spline interpolation.

Step 3: Around this point, a volume of 32 mm x 32 mm x 34 mm was assessed by measuring 5 x 5 x 7 points. On the basis of this data set, the spatial peak SAR value was evaluated under the following procedure:

1. The data at the surface were extrapolated, since the center of the dipoles is 2.7 mm away from the tip of the probe and the distance between the surface and the lowest measuring point is 1.2 mm. The extrapolation was based on a least square algorithm [11]. A polynomial of the fourth order was calculated through the points in z-axes. This polynomial was then used to evaluate the points between the surface and the probe tip.
2. The maximum interpolated value was searched with a straightforward algorithm. Around this maximum the SAR values averaged over the spatial volumes (1 g or 10 g) were computed by the 3D-Spline interpolation algorithm. The 3D-Spline is composed of three one dimensional splines with the "Not a knot"-condition (in x, y and z-directions) [11], [12]. The volume was integrated with the trapezoidal-algorithm. One thousand points (10 x 10 x 10) were interpolated to calculate the average.
3. All neighboring volumes were evaluated until no neighboring volume with a higher average value was found.

Step 4: Re-measurement of the SAR value at the same location as in Step 1. If the value changed by more than 5%, the evaluation was repeated.

CONCLUSION

This page summarizes the results of the performed dosimetric evaluation. The plots with the corresponding SAR distributions, which reveal information about the location of the maximum SAR with respect to the device, could be found in Appendix E.

SAR Body & Head Worst-Case Test Data

Environmental Conditions

Ambient Temperature:	21° C
Relative Humidity:	52%
ATM Pressure:	1016 mbar

* Testing was performed by Eric Hong on 2006-11-7, 2006-11-8 and 2006-11-9 for 2.4GHz.

11 Mbps for 802.11b 20 MHz

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	2437	153.5	Body	Flat	none	0.851	1.6	1
Acer	Back touching to the flat phantom	2412	145.2	Body	Flat	none	0.785	1.6	2
Acer	Back touching to the flat phantom	2462	146.6	Body	Flat	none	0.749	1.6	3
IBM	Back touching to the flat phantom	2437	153.5	Body	Flat	none	0.836	1.6	4
IBM	Back touching to the flat phantom	2412	145.2	Body	Flat	none	0.696	1.6	5
IBM	Back touching to the flat phantom	2462	146.6	Body	Flat	none	0.661	1.6	6
Sony	Back touching to the flat phantom	2437	153.5	Body	Flat	none	0.816	1.6	7
Sony	Back touching to the flat phantom	2412	145.2	Body	Flat	none	0.733	1.6	8
Sony	Back touching to the flat phantom	2462	146.6	Body	Flat	none	0.705	1.6	9

11 Mbps for 802.11b 40 MHz

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	2452	120.2	Body	Flat	none	0.545	1.6	10
IBM	Back touching to the flat phantom	2452	120.2	Body	Flat	none	0.444	1.6	11
Sony	Back touching to the flat phantom	2452	120.2	Body	Flat	none	0.453	1.6	12

54 Mbps for 802.11g 20 MHz

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	2437	153.5	Body	Flat	none	0.829	1.6	13
Acer	Back touching to the flat phantom	2412	113.2	Body	Flat	none	0.461	1.6	14
Acer	Back touching to the flat phantom	2462	78.3	Body	Flat	none	0.402	1.6	15
IBM	Back touching to the flat phantom	2437	153.5	Body	Flat	none	0.853	1.6	16
IBM	Back touching to the flat phantom	2412	113.2	Body	Flat	none	0.576	1.6	17
IBM	Back touching to the flat phantom	2462	78.3	Body	Flat	none	0.459	1.6	18
Sony	Back touching to the flat phantom	2437	153.5	Body	Flat	none	0.848	1.6	19
Sony	Back touching to the flat phantom	2412	113.2	Body	Flat	none	0.528	1.6	20
Sony	Back touching to the flat phantom	2462	78.3	Body	Flat	none	0.408	1.6	21

54 Mbps for 802.11g 40 MHz

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	2437	91	Body	Flat	none	0.542	1.6	22
IBM	Back touching to the flat phantom	2437	91	Body	Flat	none	0.513	1.6	23
Sony	Back touching to the flat phantom	2437	91	Body	Flat	none	0.475	1.6	24

MCS11 for 802.11n HT20

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	2437	146.9	Body	Flat	none	0.702	1.6	25
IBM	Back touching to the flat phantom	2437	146.9	Body	Flat	none	0.717	1.6	26
Sony	Back touching to the flat phantom	2437	146.9	Body	Flat	none	0.694	1.6	27

MCS15 for 802.11n HT40

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	2437	147.2	Body	Flat	none	0.786	1.6	28
IBM	Back touching to the flat phantom	2437	147.2	Body	Flat	none	0.685	1.6	29
Sony	Back touching to the flat phantom	2437	147.2	Body	Flat	none	0.788	1.6	30

* Testing was performed by Eric Hong from 2006-11-10 & 2006-11-13 & 2006-11-14 for 5 GHz

W52 9Mbps for 802.11a 20 MHz (5180-5240MHz)

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	5220	49.4	Body	Flat	none	0.260	1.6	31
IBM	Back touching to the flat phantom	5220	49.4	Body	Flat	none	0.395	1.6	32
Sony	Back touching to the flat phantom	5220	49.4	Body	Flat	none	0.184	1.6	33

W52 9Mbps for 802.11a 40 MHz (5190/5230MHz)

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	5230	48.3	Body	Flat	none	0.259	1.6	34
IBM	Back touching to the flat phantom	5230	48.3	Body	Flat	none	0.177	1.6	35
Sony	Back touching to the flat phantom	5230	48.3	Body	Flat	none	0.185	1.6	36

W52 MCS0 for 802.11n HT20 (5180-5240MHz)

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	5180	48.8	Body	Flat	none	0.309	1.6	37
IBM	Back touching to the flat phantom	5180	48.8	Body	Flat	none	0.270	1.6	38
Sony	Back touching to the flat phantom	5180	48.8	Body	Flat	none	0.297	1.6	39

W52 MCS0 for 802.11n HT40 (5190/5230MHz)

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	5230	49.4	Body	Flat	none	0.234	1.6	40
IBM	Back touching to the flat phantom	5230	49.4	Body	Flat	none	0.381	1.6	41
Sony	Back touching to the flat phantom	5230	49.4	Body	Flat	none	0.221	1.6	42

W53 9Mbps for 802.11a 20 MHz (5260-5320MHz)

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	5260	141.3	Body	Flat	none	0.275	1.6	43
IBM	Back touching to the flat phantom	5260	141.3	Body	Flat	none	0.351	1.6	44
Sony	Back touching to the flat phantom	5260	141.3	Body	Flat	none	0.206	1.6	45

W53 9Mbps for 802.11a 40 MHz (5270/5310MHz)

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	5270	110.4	Body	Flat	none	0.266	1.6	46
IBM	Back touching to the flat phantom	5270	110.4	Body	Flat	none	0.205	1.6	47
Sony	Back touching to the flat phantom	5270	110.4	Body	Flat	none	0.218	1.6	48

W53 MCS0 for 802.11n HT20 (5260-5320MHz)

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	5260	140	Body	Flat	none	0.315	1.6	49
IBM	Back touching to the flat phantom	5260	140	Body	Flat	none	0.282	1.6	50
Sony	Back touching to the flat phantom	5260	140	Body	Flat	none	0.293	1.6	51

W53 MCS0 for 802.11n HT40 (5270/5310MHz)

Laptop	EUT position	Frequency (MHz)	Conducted Power (mW)	Liquid	Phantom	Notes / Accessories	Measured (mW/g) (1 g)	Limit (mW/g)	Plot #
Acer	Back touching to the flat phantom	5270	136.5	Body	Flat	none	0.245	1.6	52
IBM	Back touching to the flat phantom	5270	136.5	Body	Flat	none	0.363	1.6	53
Sony	Back touching to the flat phantom	5270	136.5	Body	Flat	none	0.236	1.6	54

APPENDIX A – MEASUREMENT UNCERTAINTY

The uncertainty budget has been determined for the DASY4 measurement system and is given in the following Table.

DASY4 Uncertainty Budget According to IEEE 1528 [1]								
Error Description	Uncertainty value	Prob. Dist.	Div.	(c_i) 1g	(c_i) 10g	Std. Unc. (1g)	Std. Unc. (10g)	(e_i) e_{eff}
Measurement System								
Probe Calibration	±5.9%	N	1	1	1	±5.9%	±5.9%	∞
Axial Isotropy	±4.7%	R	$\sqrt{3}$	0.7	0.7	±1.9%	±1.9%	∞
Hemispherical Isotropy	±9.6%	R	$\sqrt{3}$	0.7	0.7	±3.9%	±3.9%	∞
Boundary Effects	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	∞
Linearity	±4.7%	R	$\sqrt{3}$	1	1	±2.7%	±2.7%	∞
System Detection Limits	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	∞
Readout Electronics	±0.3%	N	1	1	1	±0.3%	±0.3%	∞
Response Time	±0.8%	R	$\sqrt{3}$	1	1	±0.5%	±0.5%	∞
Integration Time	±2.6%	R	$\sqrt{3}$	1	1	±1.5%	±1.5%	∞
RF Ambient Conditions	±3.0%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%	∞
Probe Positioner	±0.4%	R	$\sqrt{3}$	1	1	±0.2%	±0.2%	∞
Probe Positioning	±2.9%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%	∞
Max. SAR Eval.	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	∞
Test Sample Related								
Device Positioning	±2.9%	N	1	1	1	±2.9%	±2.9%	145
Device Holder	±3.6%	N	1	1	1	±3.6%	±3.6%	5
Power Drift	±5.0%	R	$\sqrt{3}$	1	1	±2.9%	±2.9%	∞
Phantom and Setup								
Phantom Uncertainty	±4.0%	R	$\sqrt{3}$	1	1	±2.3%	±2.3%	∞
Liquid Conductivity (target)	±5.0%	R	$\sqrt{3}$	0.64	0.43	±1.8%	±1.2%	∞
Liquid Conductivity (meas.)	±2.5%	N	1	0.64	0.43	±1.6%	±1.1%	∞
Liquid Permittivity (target)	±5.0%	R	$\sqrt{3}$	0.6	0.49	±1.7%	±1.4%	∞
Liquid Permittivity (meas.)	±2.5%	N	1	0.6	0.49	±1.5%	±1.2%	∞
Combined Std. Uncertainty						±10.8%	±10.6%	330
Expanded STD Uncertainty						±21.6%	±21.1%	

DASY4 Uncertainty Budget

According to CENELEC EN 50361 [2]

Error Description	Uncertainty value	Prob. Dist.	Div.	(c_i) 1g	(c_i) 10g	Std. Unc. (1g)	Std. Unc. (10g)	(v_i) v_{eff}
Measurement Equipment								
Probe Calibration	±5.9%	N	1	1	1	±5.9%	±5.9%	∞
Axial Isotropy	±4.7%	R	$\sqrt{3}$	0.7	0.7	±1.9%	±1.9%	∞
Spherical Isotropy	±9.6%	R	$\sqrt{3}$	0.7	0.7	±3.9%	±3.9%	∞
Probe Linearity	±4.7%	R	$\sqrt{3}$	1	1	±2.7%	±2.7%	∞
Detection Limit	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	∞
Boundary Effects	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	∞
Readout Electronics	±0.3%	N	1	1	1	±0.3%	±0.3%	∞
Response Time	±0.8%	N	1	1	1	±0.8%	±0.8%	∞
Noise	±0%	N	1	1	1	±0%	±0%	∞
Integration Time	±2.6%	N	1	1	1	±2.6%	±2.6%	∞
Mechanical Constraints								
Scanning System	±0.4%	R	$\sqrt{3}$	1	1	±0.2%	±0.2%	∞
Phantom Shell	±4.0%	R	$\sqrt{3}$	1	1	±2.3%	±2.3%	∞
Probe Positioning	±2.9%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%	∞
Device Positioning	±2.9%	N	1	1	1	±2.9%	±2.9%	145
Physical Parameters								
Liquid Conductivity (target)	±5.0%	R	$\sqrt{3}$	0.7	0.5	±2.0%	±1.4%	∞
Liquid Conductivity (meas.)	±4.3%	R	$\sqrt{3}$	0.7	0.5	±1.7%	±1.2%	∞
Liquid Permittivity (target)	±5.0%	R	$\sqrt{3}$	0.6	0.5	±1.7%	±1.4%	∞
Liquid Permittivity (meas.)	±4.3%	R	$\sqrt{3}$	0.6	0.5	±1.5%	±1.2%	∞
Power Drift	±5.0%	R	$\sqrt{3}$	1	1	±2.9%	±2.9%	∞
RF Ambient Conditions	±3.0%	R	$\sqrt{3}$	1	1	±1.7%	±1.7%	∞
Post-Processing								
Extrap. and Integration	±1.0%	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	∞
Combined Std. Uncertainty						± 10.9%	± 10.6%	18125
Expanded Std. Uncertainty						±21.7%	±12.1%	

APPENDIX B – PROBE CALIBRATION CERTIFICATES

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Bay Area**

Certificate No: **ET3-1604_May06**

CALIBRATION CERTIFICATE

Object **ET3DV6 - SN: 1604**

Calibration procedure(s) **QA CAL-01.v5 and QA CAL-12.v4
Calibration procedure for dosimetric E-field probes**

Calibration date: **May 2, 2006**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293674	5-Apr-06 (METAS, No. 251-00557)	Apr-07
Power sensor E4412A	MY41495277	5-Apr-06 (METAS, No. 251-00557)	Apr-07
Power sensor E4412A	MY41498087	5-Apr-06 (METAS, No. 251-00557)	Apr-07
Reference 3 dB Attenuator	SN: S5054 (3c)	11-Aug-05 (METAS, No. 251-00499)	Aug-06
Reference 20 dB Attenuator	SN: S5086 (20b)	4-Apr-06 (METAS, No. 251-00558)	Apr-07
Reference 30 dB Attenuator	SN: S5129 (30b)	11-Aug-05 (METAS, No. 251-00500)	Aug-06
Reference Probe ES3DV2	SN: 3013	2-Jan-06 (SPEAG, No. ES3-3013_Jan06)	Jan-07
DAE4	SN: 654	2-Feb-06 (SPEAG, No. DAE4-654_Feb06)	Feb-07

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Nov-05)	in house check: Nov-07
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-05)	in house check: Nov 06

	Name	Function	Signature
Calibrated by:	Katja Pokovic	Technical Manager	
Approved by:	Niels Kuster	Quality Manager	

Issued: May 3, 2006

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
Polarization φ	φ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not effect the E^2 -field uncertainty inside TSL (see below *ConvF*).
- NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * *ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

ET3DV6 SN:1604

May 2, 2006

Probe ET3DV6

SN:1604

Manufactured:	July 30, 2001
Last calibrated:	March 18, 2005
Recalibrated:	May 2, 2006

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

ET3DV6 SN:1604

May 2, 2006

DASY - Parameters of Probe: ET3DV6 SN:1604**Sensitivity in Free Space^A****Diode Compression^B**

NormX	1.87 ± 10.1%	$\mu\text{V}/(\text{V}/\text{m})^2$	DCP X	93 mV
NormY	1.80 ± 10.1%	$\mu\text{V}/(\text{V}/\text{m})^2$	DCP Y	93 mV
NormZ	1.91 ± 10.1%	$\mu\text{V}/(\text{V}/\text{m})^2$	DCP Z	93 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

Boundary Effect**TSL 900 MHz Typical SAR gradient: 5 % per mm**

Sensor Center to Phantom Surface Distance		3.7 mm	4.7 mm
SAR _{be} [%]	Without Correction Algorithm	7.9	4.1
SAR _{be} [%]	With Correction Algorithm	0.1	0.2

TSL 1810 MHz Typical SAR gradient: 10 % per mm

Sensor Center to Phantom Surface Distance		3.7 mm	4.7 mm
SAR _{be} [%]	Without Correction Algorithm	7.0	4.1
SAR _{be} [%]	With Correction Algorithm	0.1	0.3

Sensor OffsetProbe Tip to Sensor Center **2.7 mm**

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.


^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 8).^B Numerical linearization parameter: uncertainty not required.

ET3DV6 SN:1604

May 2, 2006

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)



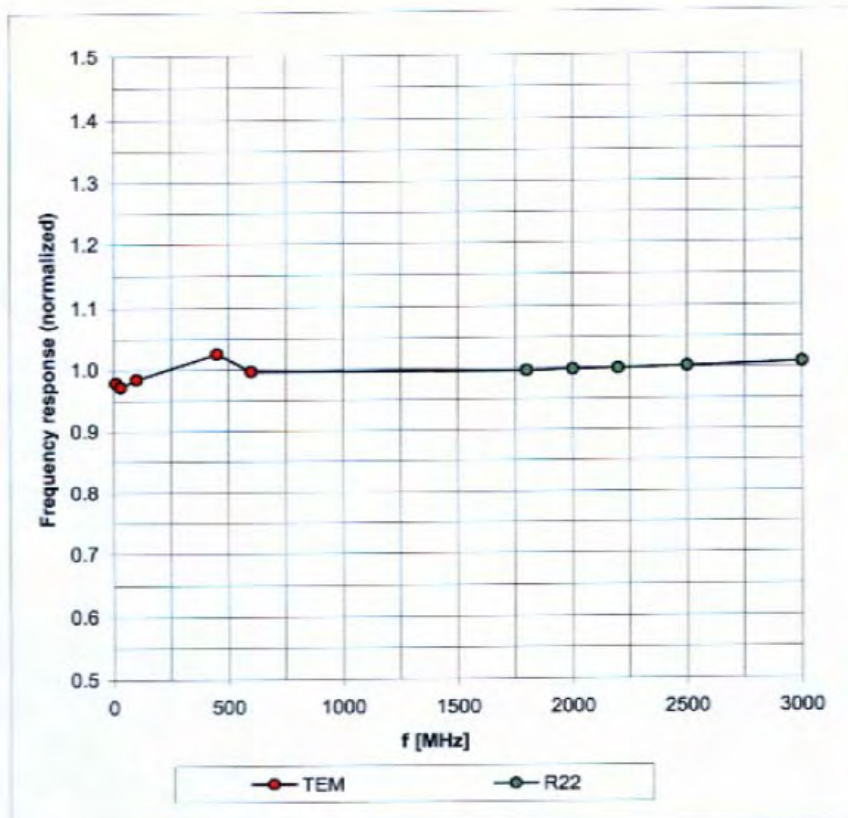


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

ET3DV6 SN:1604

May 2, 2006

Receiving Pattern (ϕ), $\theta = 0^\circ$

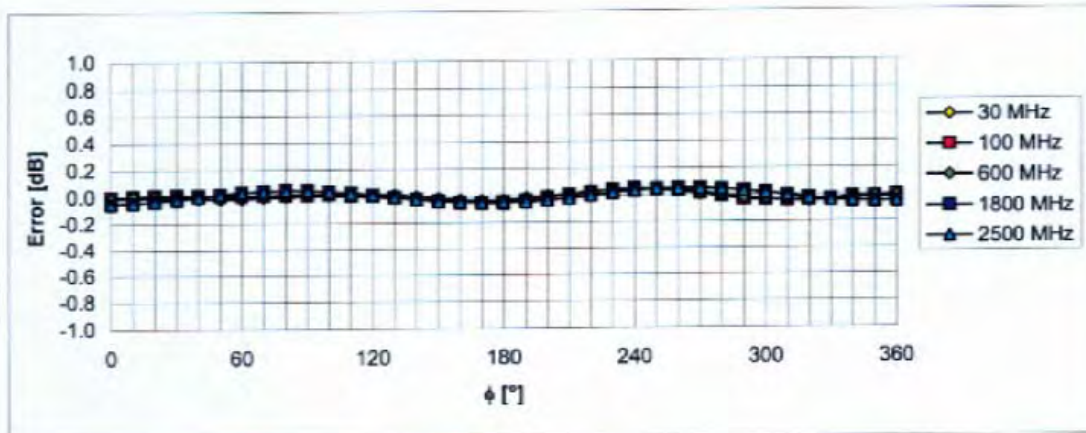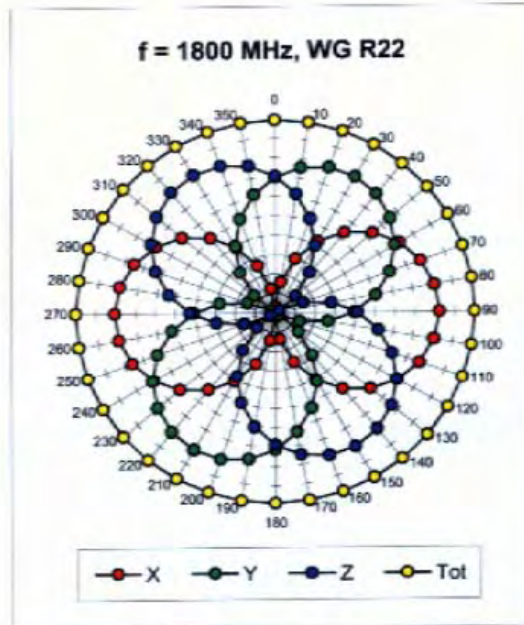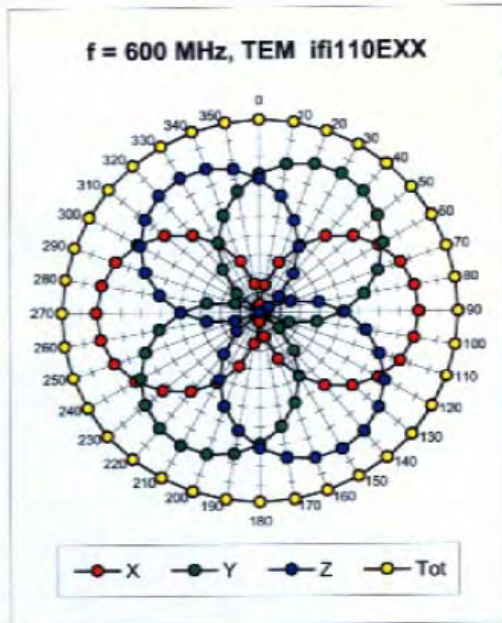


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

ET3DV6 SN:1604

May 2, 2006

Dynamic Range $f(\text{SAR}_{\text{head}})$ (Waveguide R22, $f = 1800 \text{ MHz}$)


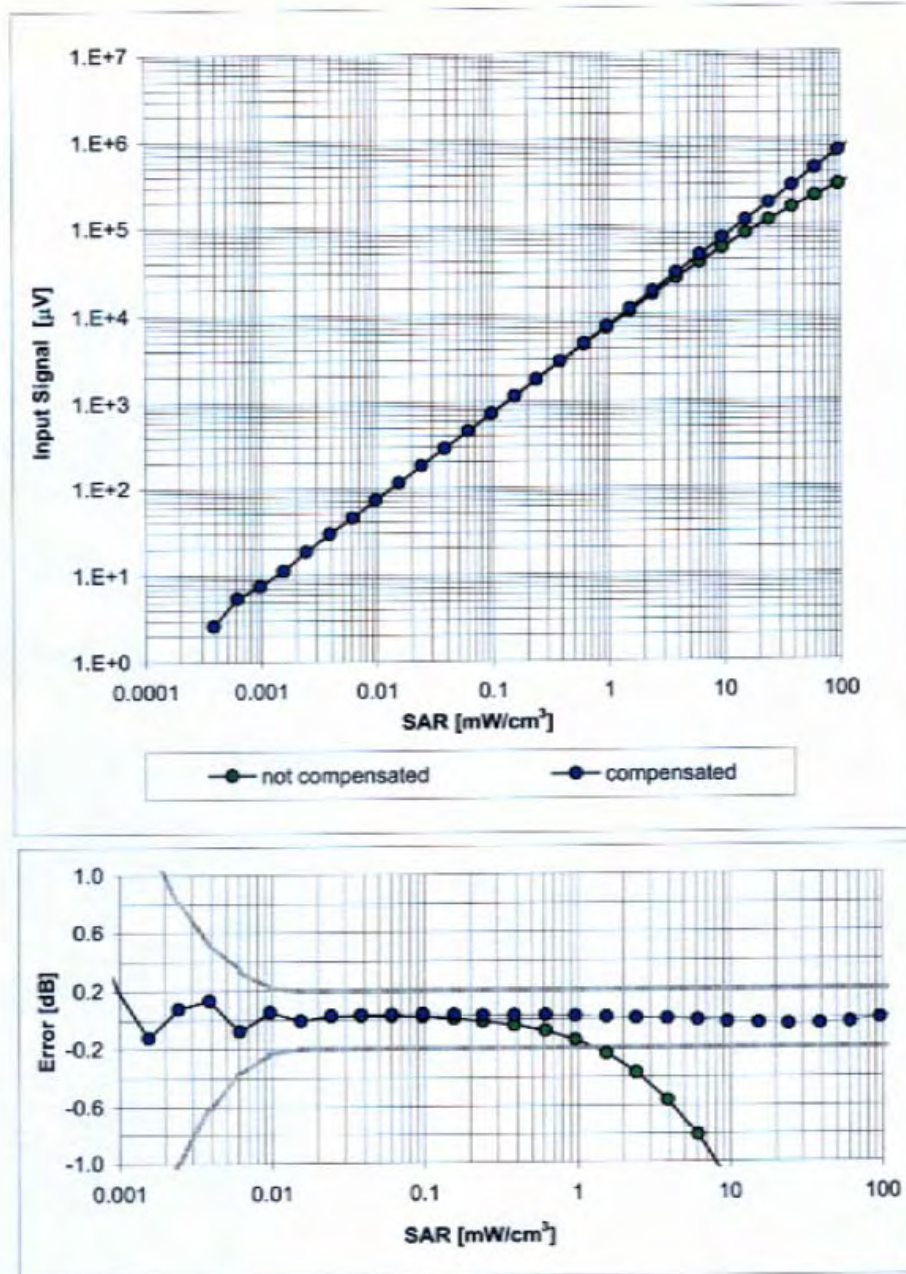


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

ET3DV6 SN:1604

May 2, 2006

Conversion Factor Assessment

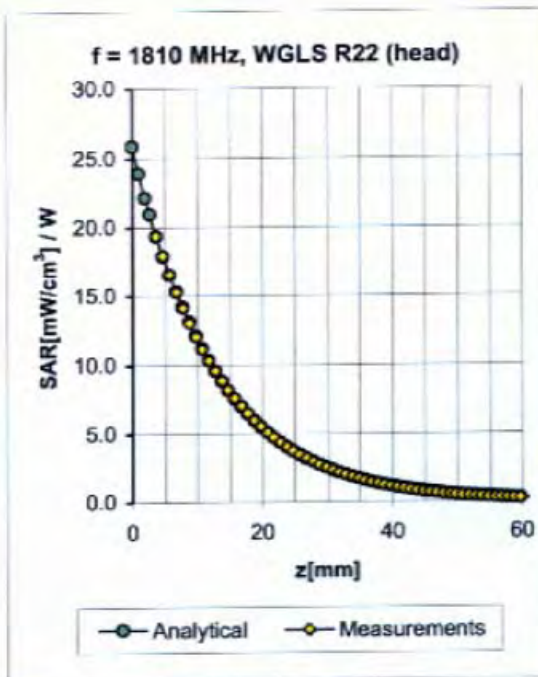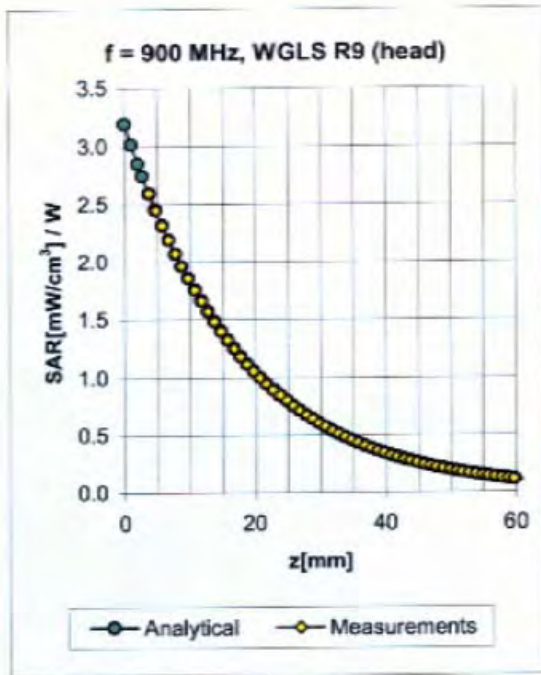

f [MHz]	Validity [MHz] ^c	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
450	± 50 / ± 100	Head	43.5 ± 5%	0.87 ± 5%	0.26	2.94	7.14 ± 13.3% (k=2)
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.56	1.81	6.60 ± 11.0% (k=2)
1810	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.50	2.59	5.29 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1.80 ± 5%	0.68	1.85	4.60 ± 11.8% (k=2)
450	± 50 / ± 100	Body	56.7 ± 5%	0.94 ± 5%	0.25	4.44	7.42 ± 13.3% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.47	2.08	6.27 ± 11.0% (k=2)
1810	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.56	2.66	4.88 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.66	1.95	4.27 ± 11.8% (k=2)


^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

ET3DV6 SN:1604

May 2, 2006

Deviation from Isotropy in HSL

Error (ϕ , θ), $f = 900$ MHz

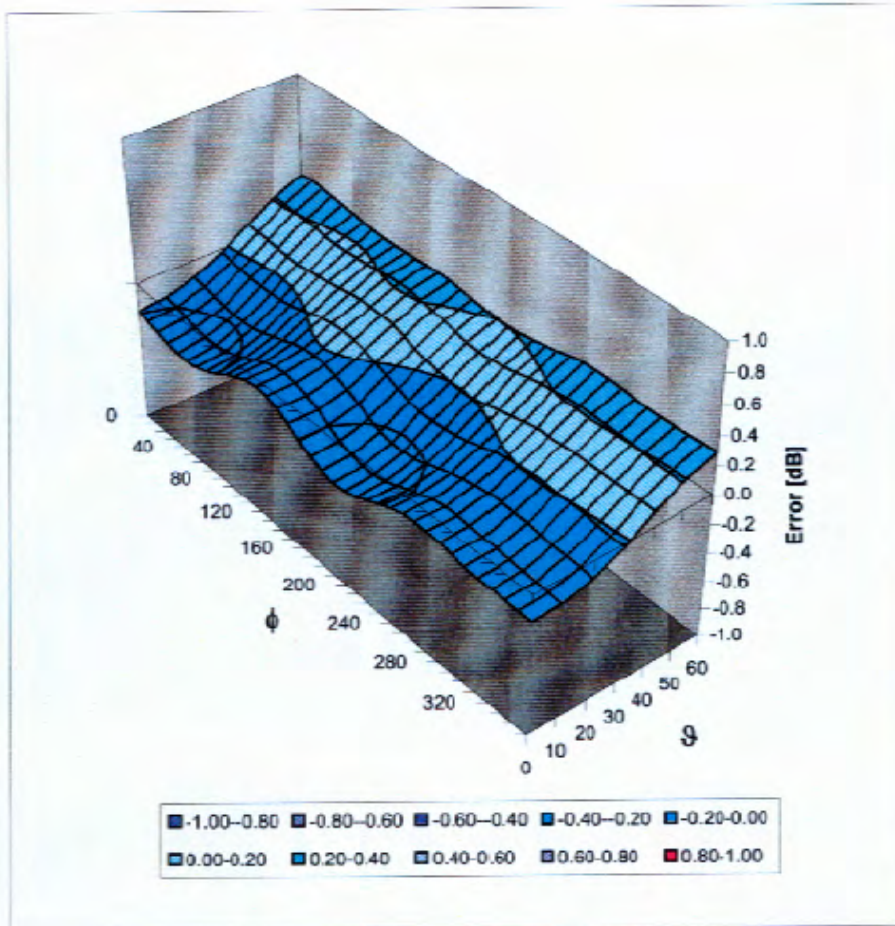

Uncertainty of Spherical Isotropy Assessment: $\pm 2.6\%$ ($k=2$)

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **BACL**

Certificate No: **EX3-3756_Apr06**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3576**

Calibration procedure(s) **QA CAL-01.v5 and QA CAL-14.v3
Calibration procedure for dosimetric E-field probes**

Calibration date: **April 20, 2006**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	5-Apr-06 (METAS, No. 251-00557)	Apr-07
Power sensor E4412A	MY41495277	5-Apr-06 (METAS, No. 251-00557)	Apr-07
Power sensor E4412A	MY41498087	5-Apr-06 (METAS, No. 251-00557)	Apr-07
Reference 3 dB Attenuator	SN: S5054 (3c)	11-Aug-05 (METAS, No. 251-00499)	Aug-06
Reference 20 dB Attenuator	SN: S5086 (20b)	4-Apr-06 (METAS, No. 251-00558)	Apr-07
Reference 30 dB Attenuator	SN: S5129 (30b)	11-Aug-05 (METAS, No. 251-00500)	Aug-06
Reference Probe ES3DV2	SN: 3013	2-Jan-06 (SPEAG, No. ES3-3013_Jan06)	Jan-07
DAE4	SN: 654	2-Feb-06 (SPEAG, No. DAE4-654_Feb06)	Feb-07
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Nov-05)	In house check: Nov-07
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-05)	In house check: Nov 06

	Name	Function	Signature
Calibrated by:	Katja Pokovic	Technical Manager	
Approved by:	Niels Kuster	Quality Manager	

Issued: April 20, 2006

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
Polarization φ	φ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not effect the E²-field uncertainty inside TSL (see below *ConvF*).
- NORM(f)_{x,y,z} = NORM_{x,y,z} * frequency_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to **NORM_{x,y,z} * ConvF** whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

EX3DV4 SN:3576

April 20, 2006

Probe EX3DV4

SN:3576

Manufactured:	November 4, 2005
Calibrated:	April 20, 2006

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

EX3DV4 SN:3576

April 20, 2006

DASY - Parameters of Probe: EX3DV4 SN:3576

Sensitivity in Free Space^A

Diode Compression^B

NormX	0.438 ± 10.1%	$\mu V/(V/m)^2$	DCP X	93 mV
NormY	0.439 ± 10.1%	$\mu V/(V/m)^2$	DCP Y	93 mV
NormZ	0.386 ± 10.1%	$\mu V/(V/m)^2$	DCP Z	93 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

Boundary Effect

TSL 900 MHz Typical SAR gradient: 5 % per mm

Sensor Center to Phantom Surface Distance		2.0 mm	3.0 mm
SAR _{be} [%]	Without Correction Algorithm	3.1	1.1
SAR _{be} [%]	With Correction Algorithm	0.2	0.4

TSL 1810 MHz Typical SAR gradient: 10 % per mm

Sensor Center to Phantom Surface Distance		2.0 mm	3.0 mm
SAR _{be} [%]	Without Correction Algorithm	2.5	1.1
SAR _{be} [%]	With Correction Algorithm	0.2	0.4

Sensor Offset

Probe Tip to Sensor Center **1.0 mm**

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 8).


^B Numerical linearization parameter: uncertainty not required.

EX3DV4 SN:3576

April 20, 2006

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)



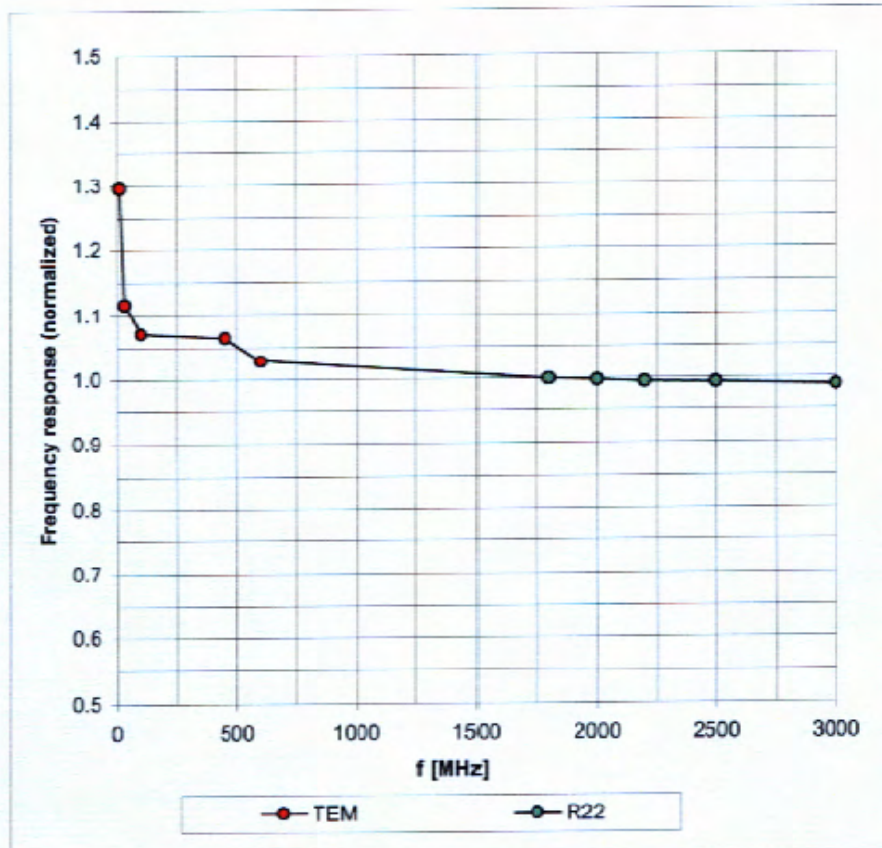


Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

EX3DV4 SN:3576

April 20, 2006

Receiving Pattern (ϕ), $\theta = 0^\circ$

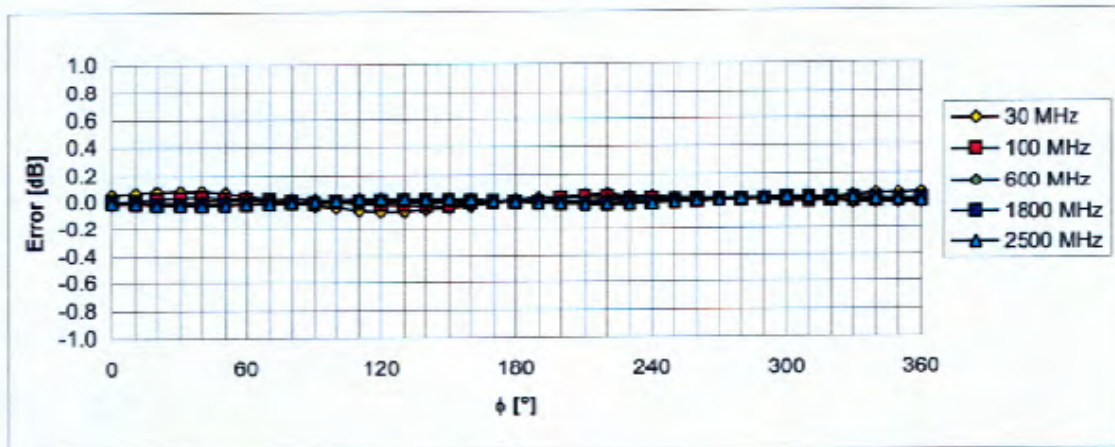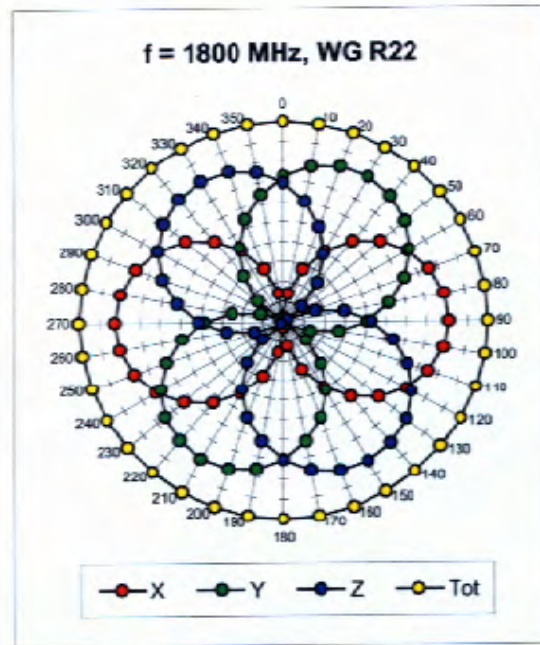
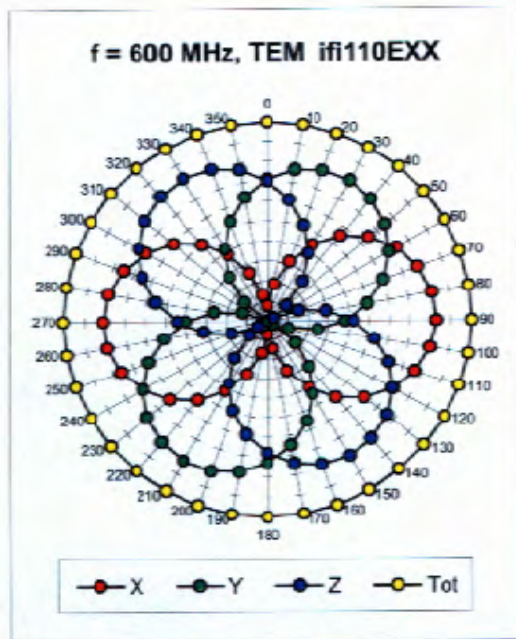


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

EX3DV4 SN:3576

April 20, 2006

Dynamic Range $f(\text{SAR}_{\text{head}})$ (Waveguide R22, $f = 1800 \text{ MHz}$)

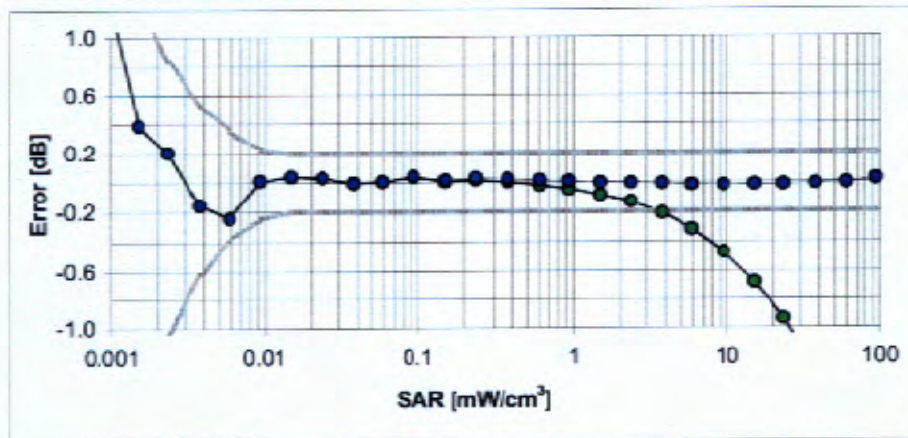
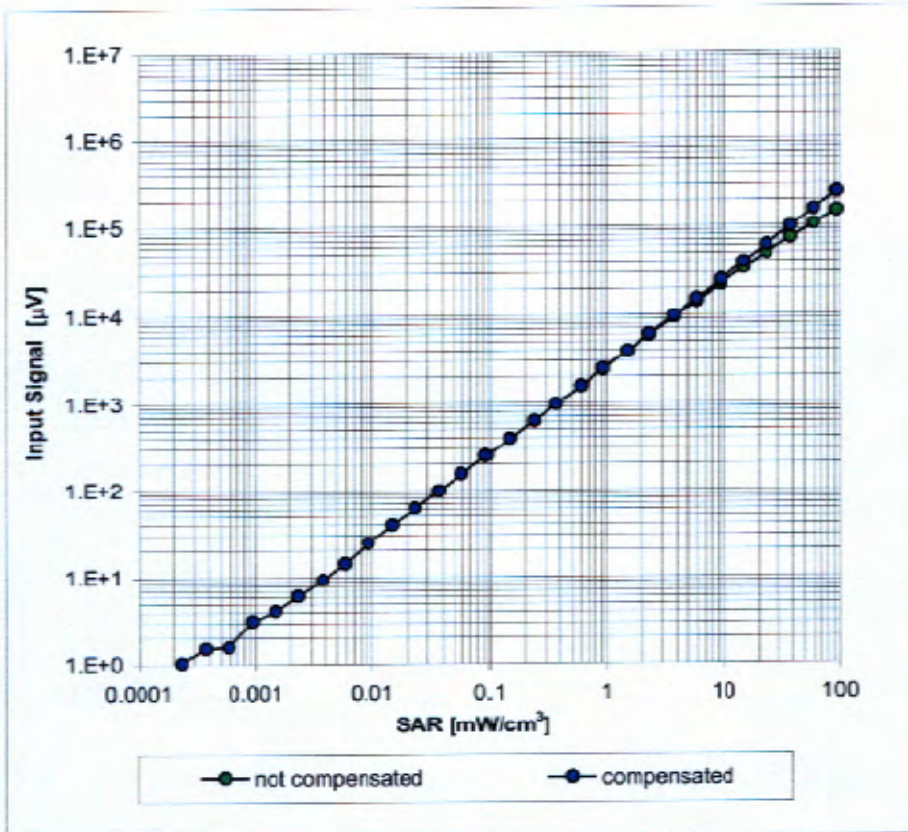


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

EX3DV4 SN:3576

April 20, 2006

Conversion Factor Assessment

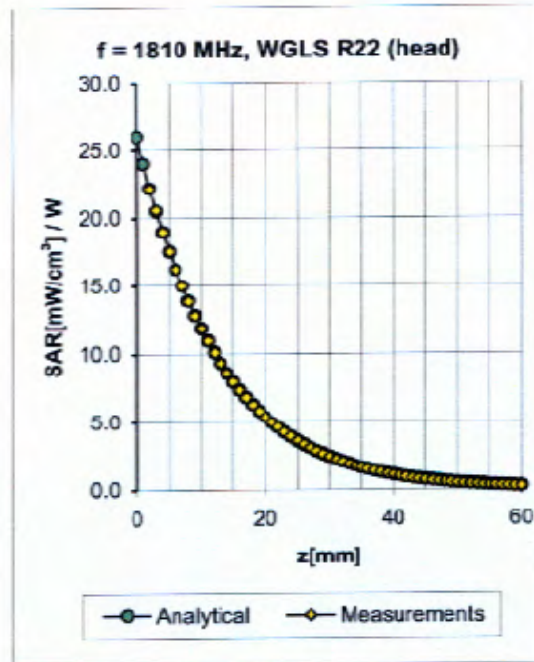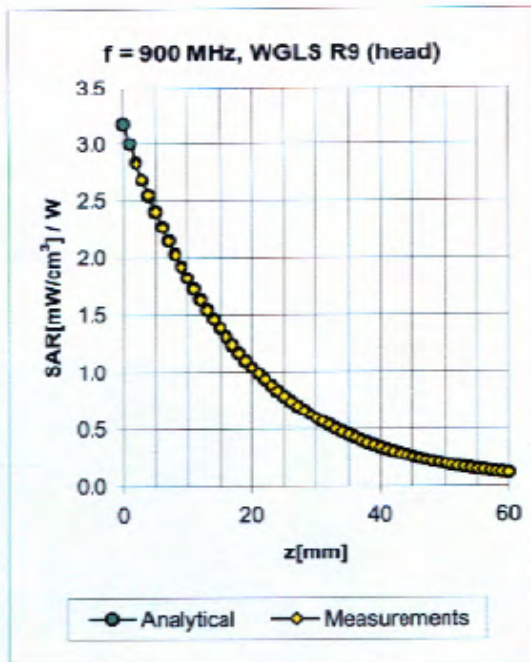

f [MHz]	Validity [MHz] ^c	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.77	0.63	8.12 ± 11.0% (k=2)
1810	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.27	1.14	7.29 ± 11.0% (k=2)
5500	± 50 / ± 100	Head	35.6 ± 5%	4.96 ± 5%	0.35	1.75	4.06 ± 13.1% (k=2)
5800	± 50 / ± 100	Head	35.3 ± 5%	5.27 ± 5%	0.32	1.75	3.89 ± 13.1% (k=2)
5500	± 50 / ± 100	Body	48.6 ± 5%	5.65 ± 5%	0.35	1.80	3.74 ± 13.1% (k=2)
5800	± 50 / ± 100	Body	48.2 ± 5%	6.00 ± 5%	0.32	1.80	3.85 ± 13.1% (k=2)


^c The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

EX3DV4 SN:3576

April 20, 2006

Deviation from Isotropy in HSL

Error (ϕ , θ), $f = 900$ MHz

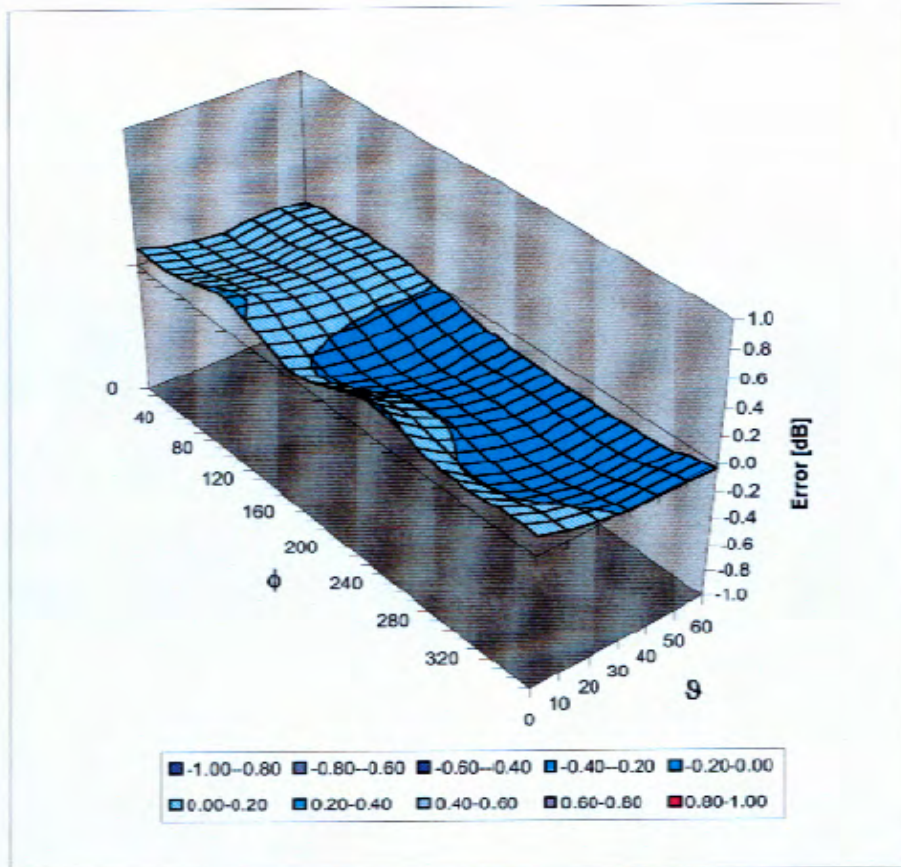


Uncertainty of Spherical Isotropy Assessment: $\pm 2.6\%$ ($k=2$)

Conversion Factor Assessment for EX3DV4 SN: 3576 for 5MHz

TSL: Body


Frequency	ConvF Uncertainty
5180	3.62
5260	3.65
5500	3.74
5800	3.85

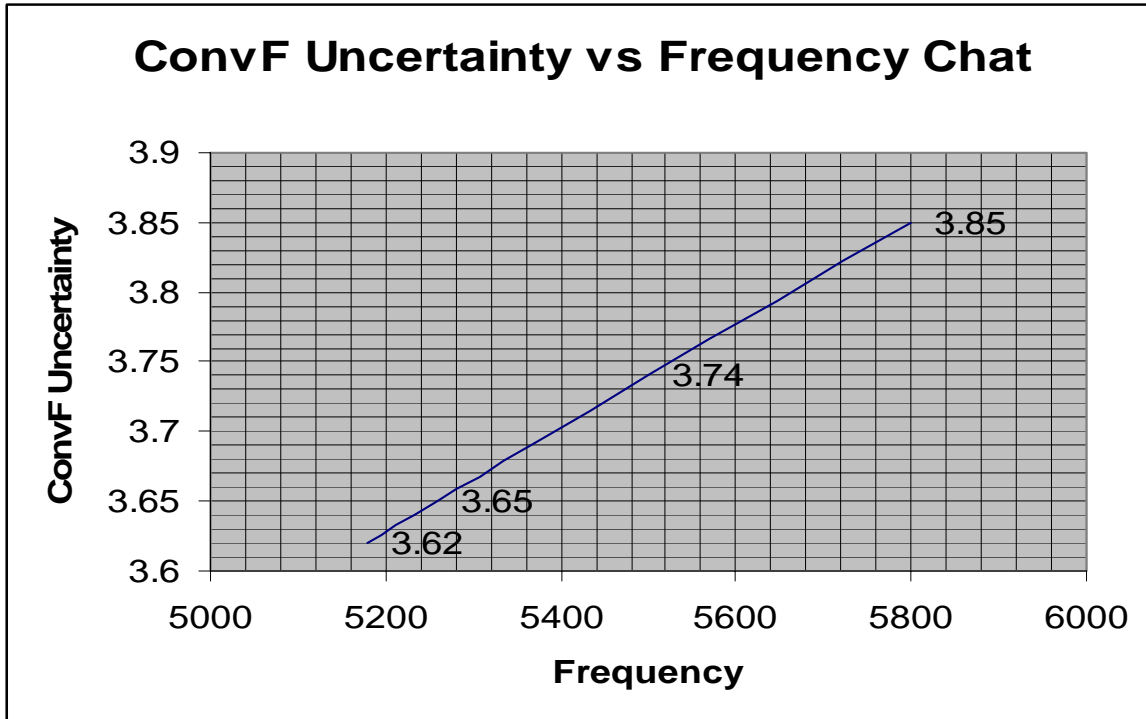

Conversion Factor Assessment for EX3DV4 SN: 3576 for 5MHz

TSL: Head

Frequency	ConvF Uncertainty
5180	4.24
5260	4.19
5500	4.06
5800	3.89

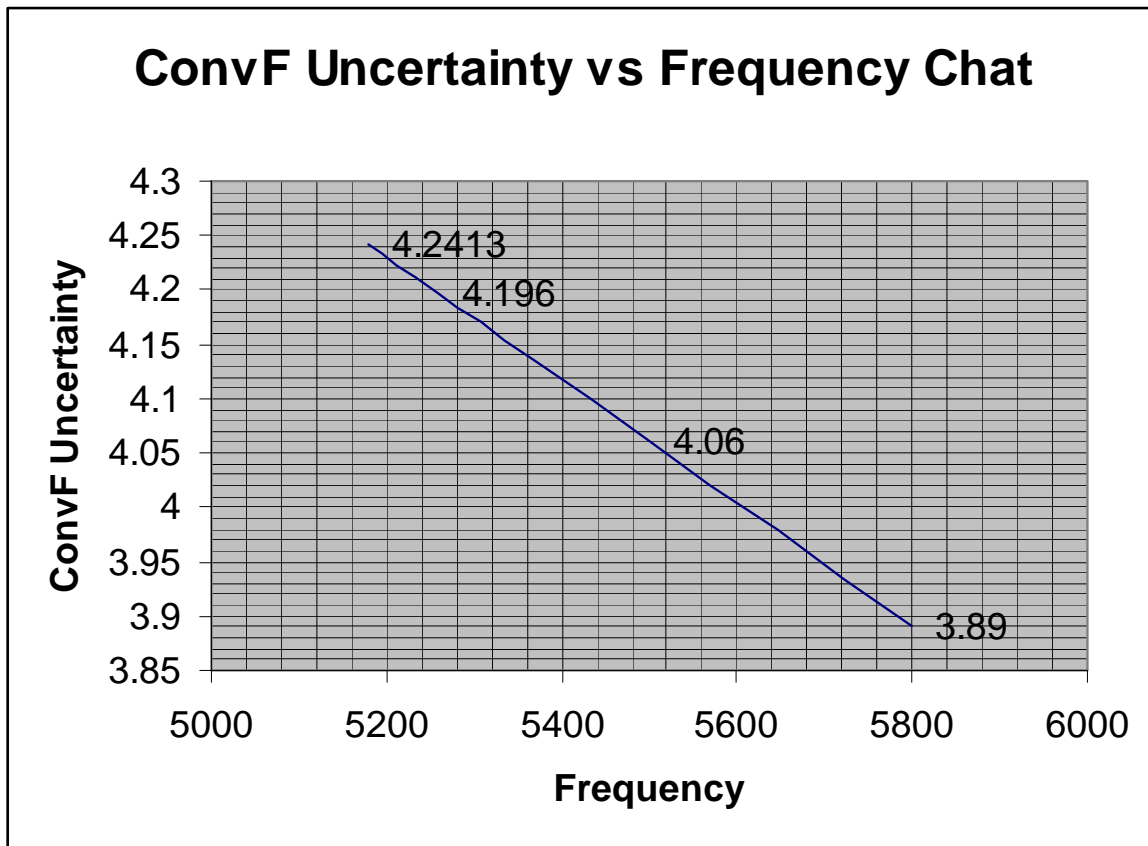

APPENDIX C – DIPOLE CALIBRATION CERTIFICATES**NCL CALIBRATION LABORATORIES**

Calibration File No: DC-713
Project Number: BACL-CAL-D-2450-5249

CERTIFICATE OF CALIBRATION

It is certified that the equipment identified below has been calibrated in the
NCL CALIBRATION LABORATORIES by qualified personnel following recognized
procedures and using transfer standards traceable to NRC/NIST.


BACL Validation Dipole

Manufacturer: APREL Laboratories
Part number: D-2450-S-1
Frequency: 2450 MHz
Serial No: BCL-141

Customer: Bay Area Compliance Laboratory

Calibrated: 28th August 2006
Released on: 28th August 2006

Released By: _____

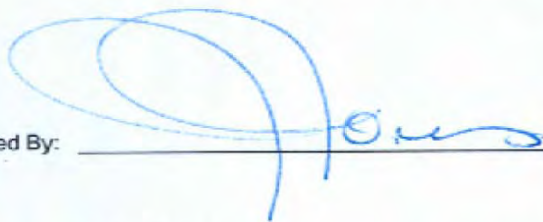**NCL CALIBRATION LABORATORIES**

51 SPECTRUM WAY
NEPEAN, ONTARIO
CANADA K2R 1E6

Division of APREL Lab.
TEL: (613) 820-4988
FAX: (613) 820-4162

NCL Calibration Laboratories

Division of APREL Laboratories.


Conditions

Dipole BCL-141 was received from customer in good condition for re-calibration, SMA connector required cleaning prior to calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C

Temperature of the Tissue: 21 °C +/- 0.5°C

We the undersigned attest that to the best of our knowledge the calibration of this device has been accurately conducted and that all information contained within this report has been reviewed for accuracy.

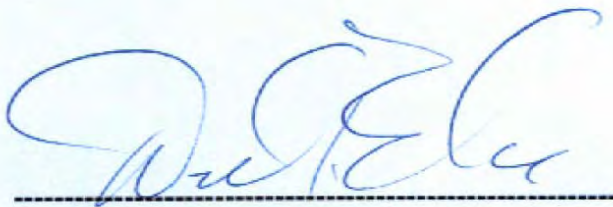

D. Brooks
Member of Engineering Staff
(Calibration Engineer)

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories

Division of APREL Laboratories.

Calibration Results Summary

The following results relate the Calibrated Dipole and should be used as a quick reference for the user.

Mechanical Dimensions


Length: 51.5 mm
Height: 30.4 mm

Electrical Specification

SWR: 1.095 U to 1.397 U
Return Loss: -26.77 dB to -15.52 dB
Impedance: 47.81 Ω to 63.37 Ω

System Validation Results

Frequency	1 Gram	10 Gram	Peak
2450 MHz	5.31	2.44	10.18

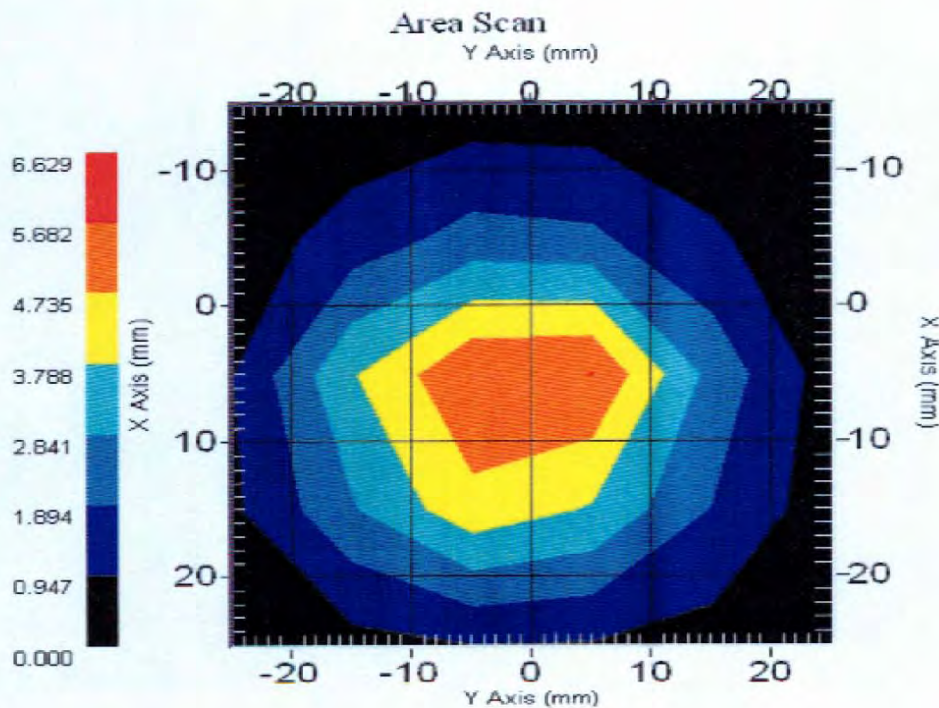

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories

Division of APREL Laboratories.

Introduction

This Calibration Report has been produced in line with the SSI Dipole Calibration Procedure SSI-TP-018-ALSAS. The results contained within this report are for Validation Dipole BCL-141. The calibration routine consisted of a three-step process. Step 1 was a mechanical verification of the dipole to ensure that it meets the mechanical specifications. Step 2 was an Electrical Calibration for the Validation Dipole, where the SWR, Impedance, and the Return loss were assessed. Step 3 involved a System Validation using the ALSAS-10U, along with APREL E-020 130 MHz to 26 GHz E-Field Probe Serial Number 212.

References

SSI-TP-018-ALSAS Dipole Calibration Procedure
SSI-TP-016 Tissue Calibration Procedure
IEEE 1528 "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques"

Conditions

Dipole BCL-141 was received from customer in good condition for re-calibration, SMA connector required cleaning prior to calibration.

Ambient Temperature of the Laboratory: 22 °C +/- 0.5°C
Temperature of the Tissue: 20 °C +/- 0.5°C

This page has been reviewed for content and attested to by signature within this document.

4

NCL Calibration Laboratories

Division of APREL Laboratories.

Dipole Calibration Results

Mechanical Verification

APREL Length	APREL Height	Measured Length	Measured Height
51.5 mm	30.4 mm	51.6 mm	30.5 mm

Tissue Validation

Head Tissue 2450 MHz	Measured
Dielectric constant, ϵ_r	39.2
Conductivity, σ [S/m]	1.80

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories


Division of APREL Laboratories.

Electrical Calibration

Test	Result
S11 R/L	-26.77 dB to -15.52 dB
SWR	1.095 U to 1.397 U
Impedance	47.81 Ω to 63.37 Ω

The Following Graphs are the results as displayed on the Vector Network Analyzer.

S11 Parameter Return Loss

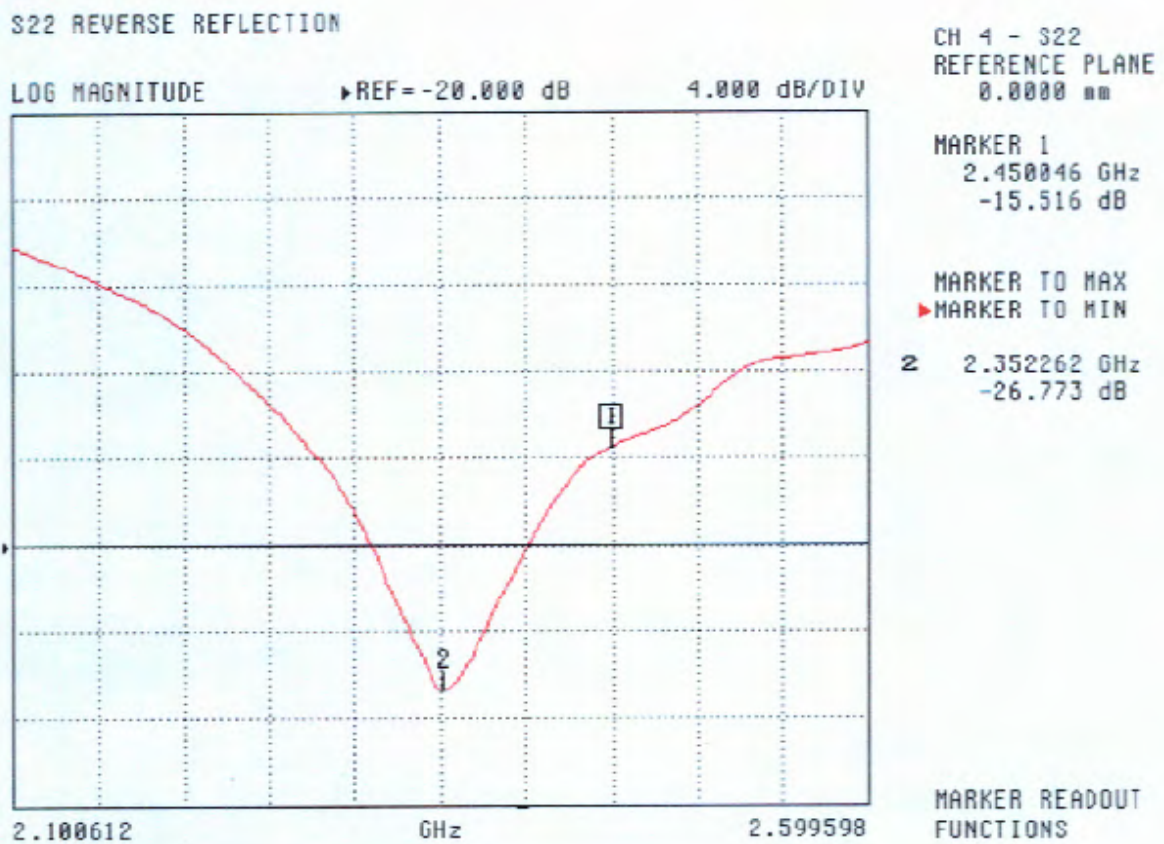

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories

Division of APREL Laboratories.


SWR

S22 REVERSE REFLECTION

SWR

REF=500.000 mU

400.000 mU/DIV

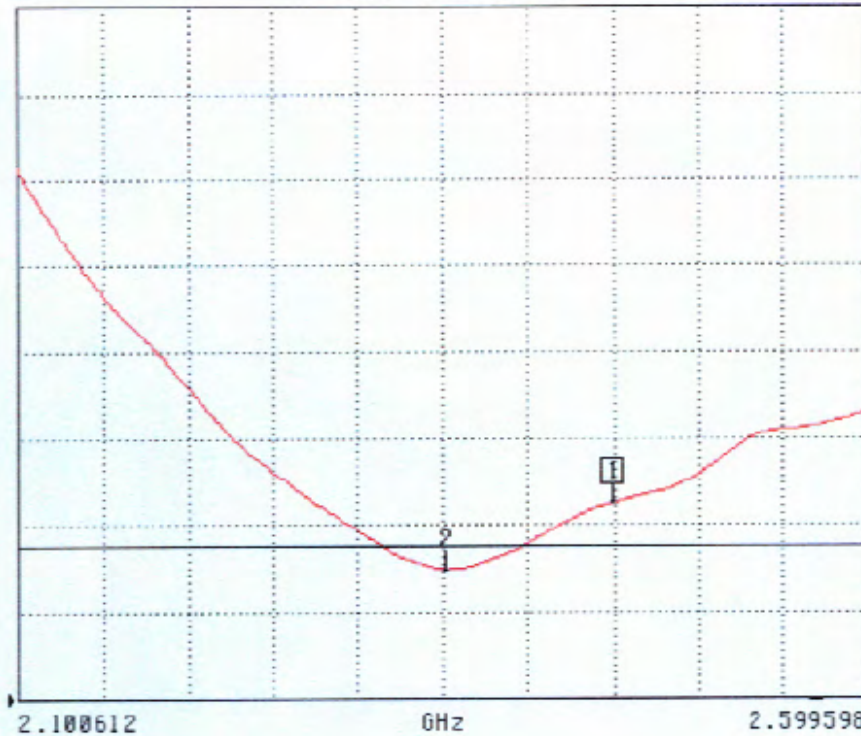

CH 4 - S22
REFERENCE PLANE
0.0000 mm

MARKER 1
2.450046 GHz
1.397 U

MARKER TO MAX
▶ MARKER TO MIN
2 2.352262 GHz
1.095 U

MARKER READOUT
FUNCTIONS


This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories

Division of APREL Laboratories.

Smith Chart Dipole Impedance

S22 REVERSE REFLECTION
IMPEDANCE

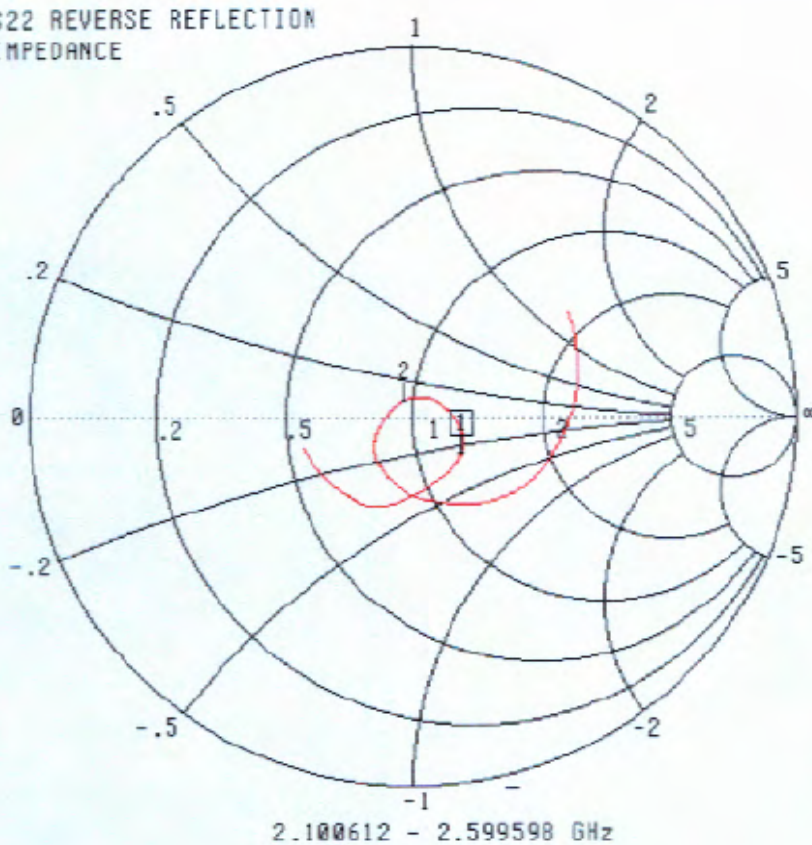

CH 4 - S22
REFERENCE PLANE
0.0000 mm

MARKER 1
2.450046 GHz
63.373 Ω
-13.350 j Ω

MARKER TO MAX
▶ MARKER TO MIN
2 2.352262 GHz
47.808 Ω
3.861 j Ω

MARKER READOUT
FUNCTIONS


This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories

Division of APREL Laboratories.

System Validation Results Using the Electrically Calibrated Dipole

Head Tissue Frequency	1 Gram	10 Gram	Peak Above Feed Point
2450 MHz	5.31	2.44	10.18

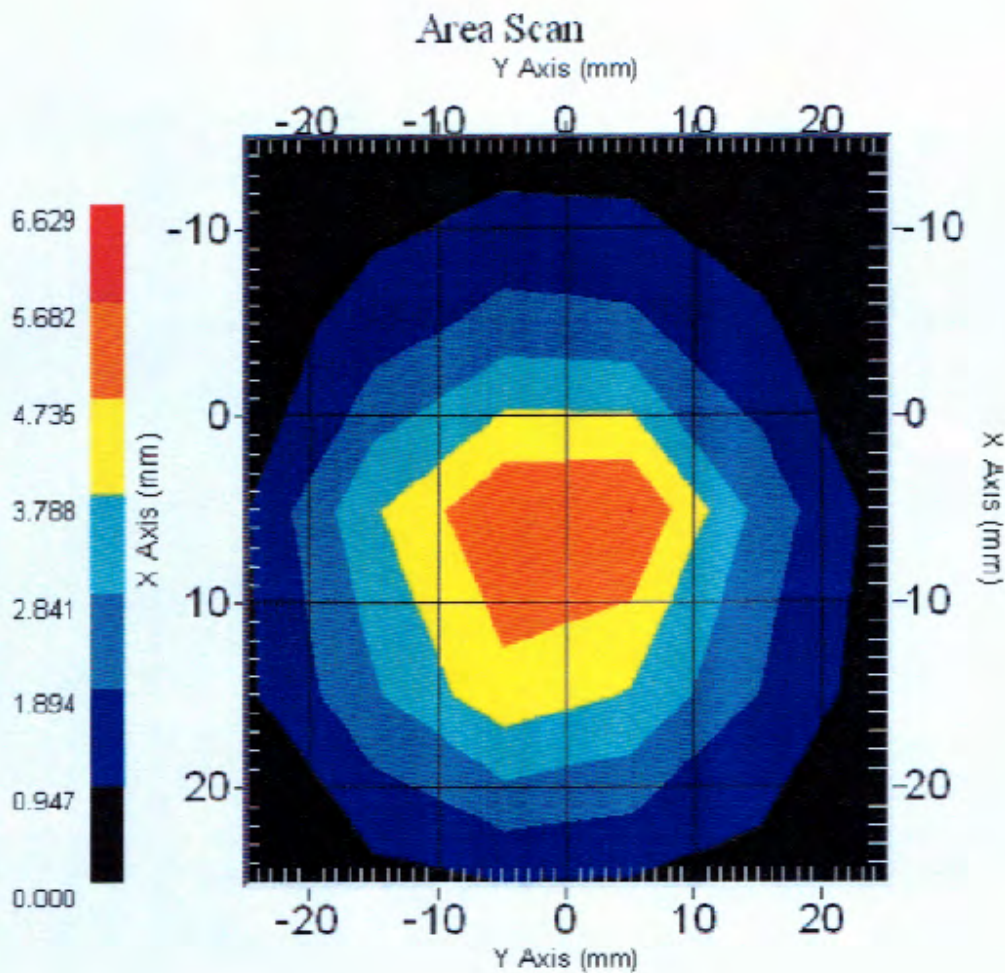

This page has been reviewed for content and attested to by signature within this document.

NCL Calibration Laboratories

Division of APREL Laboratories.

Test Equipment

The test equipment used during Probe Calibration, manufacturer, model number and, current calibration status are listed and located on the main APREL server R:\NCL\Calibration Equipment\Instrument List

This page has been reviewed for content and attested to by signature within this document.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Bay Area**

Certificate No: **D5GHZV2-1001_May06**

CALIBRATION CERTIFICATE

Object **D5100V2 - SN: 1001**

Calibration procedure(s) **QA CAL-22.v1
Calibration procedure for dipole validation kits between 3-6 GHz**

Calibration date: **May 3, 2006**

Condition of the calibrated item **In Tolerance**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	5-Apr-06 (METAS, No. 251-00557)	Apr-07
Power sensor E4412A	MY41495277	5-Apr-06 (METAS, No. 251-00557)	Apr-07
Power sensor E4412A	MY41498087	5-Apr-06 (METAS, No. 251-00557)	Apr-07
Reference 20 dB Attenuator	SN: S5086 (20b)	4-Apr-06 (METAS, No. 251-00556)	Apr-07
Reference 10 dB Attenuator	SN: 5047.2 (10r)	11-Aug-05 (METAS, No 251-00488)	Aug-06
Reference Probe EX3DV4	SN: 3503	19-Mar-05 (SPEAG, No. EX3-3503_Mar06)	Mar-07
DAE4	SN: 601	15-Dec-05 (SPEAG, No. DAE4-601_Dec05)	Dec-06

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	4-Aug-99 (SPEAG, in house check Nov-05)	In house check: Nov-07
Network Analyzer HP 8753E	US37390565 S4206	18-Oct-01 (SPEAG, in house check Nov-05)	In house check: Nov 06

Calibrated by:	Name Marcel Fehr	Function Laboratory Technician	Signature
----------------	----------------------------	--	---------------

Approved by:	Name Katja Pokovic	Technical Manager Technical Manager	Signature
--------------	------------------------------	---	---------------

Issued: May 4, 2006

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL tissue simulating liquid
ConvF sensitivity in TSL / NORM x,y,z
N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC Std 62209 Part 2, "Evaluation of Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices in the Frequency Range of 30 MHz to 6 GHz: Human models, Instrumentation, and Procedures"; Part 2: "Procedure to determine the Specific Absorption Rate (SAR) for including accessories and multiple transmitters", Draft Version 0.9, December 2004
- b) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- c) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Area Scan resolution	dx, dy = 10 mm	
Zoom Scan Resolution	dx, dy = 4.3 mm, dz = 3 mm	
Frequency	5500 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Head TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.6	4.95 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.1 ± 6 %	4.80 mho/m ± 6 %
Head TSL temperature during test	(21.7 ± 0.2) °C	---	---

SAR result with Head TSL at 5500 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	250 mW input power	21.3 mW / g
SAR normalized	normalized to 1W	85.2 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	84.7 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.00 mW / g
SAR normalized	normalized to 1W	24.0 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	23.8 mW / g ± 19.5 % (k=2)

¹ Correction to nominal TSL parameters according to c), chapter "SAR Sensitivities"

Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.6 ± 6 %	5.09 mho/m ± 6 %
Head TSL temperature during test	(22.2 ± 0.2) °C	---	---

SAR result with Head TSL at 5800 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	250 mW input power	20.7 mW / g
SAR normalized	normalized to 1W	82.8 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	82.2 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.80 mW / g
SAR normalized	normalized to 1W	23.2 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	23.0 mW / g ± 19.5 % (k=2)

Body TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.6	5.56 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.4 ± 6 %	5.50 mho/m ± 6 %
Body TSL temperature during test	(22.2 ± 0.2) °C	---	---

SAR result with Body TSL at 5500 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	condition	
SAR measured	250 mW input power	19.7 mW / g
SAR normalized	normalized to 1W	78.8 mW / g
SAR for nominal Body TSL parameters ¹	normalized to 1W	78.6 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.54 mW / g
SAR normalized	normalized to 1W	22.2 mW / g
SAR for nominal Body TSL parameters ¹	normalized to 1W	22.1 mW / g ± 19.5 % (k=2)

Body TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.2	6.00 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.8 ± 6 %	5.88 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C	—	—

SAR result with Body TSL at 5800 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	condition	
SAR measured	250 mW input power	18.0 mW / g
SAR normalized	normalized to 1W	72.0 mW / g
SAR for nominal Body TSL parameters ¹	normalized to 1W	71.8 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.04 mW / g
SAR normalized	normalized to 1W	20.2 mW / g
SAR for nominal Body TSL parameters ¹	normalized to 1W	20.1 mW / g ± 19.5 % (k=2)

Appendix

Antenna Parameters with Head TSL at 5500 MHz

Impedance, transformed to feed point	50.4 Ω - 1.4 j Ω
Return Loss	-36.7 dB

Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	54.9 Ω + 1.6 j Ω
Return Loss	-26.1 dB

Antenna Parameters with Body TSL at 5500 MHz

Impedance, transformed to feed point	49.8 Ω - 0.7 j Ω
Return Loss	-42.7 dB

Antenna Parameters with Body TSL at 5800 MHz

Impedance, transformed to feed point	55.8 Ω + 3.2 j Ω
Return Loss	-24.1 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.203 ns
----------------------------------	----------

After long term use with 40 W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	April 2, 2003

DASY4 Validation Report for Head TSL

Date/Time: 02.05.2006 15:01:43

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHz; Serial: D5100V2 - SN:1001

Communication System: CW-5GHz, Frequency: 5500 MHz Frequency: 5800 MHz; Duty Cycle: 1:1
 Medium: HSL 5800 MHz;
 Medium parameters used: $f = 5500$ MHz; $\sigma = 4.8$ mho/m; $\epsilon_r = 35.1$; $\rho = 1000$ kg/m³ Medium parameters
 used: $f = 5800$ MHz; $\sigma = 5.08$ mho/m; $\epsilon_r = 34.6$; $\rho = 1000$ kg/m³
 Phantom section: Flat Section
 Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.18, 5.18, 5.18)ConvF(5.02, 5.02, 5.02); Calibrated: 18.03.2006
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 15.12.2005
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.7 Build 21; Postprocessing SW: SEMCAD, V1.8 Build 165

d=10mm, Pin=250mW, f=5500 MHz/Area Scan (91x91x1): Measurement grid: dx=dy=10mm
 Maximum value of SAR (interpolated) = 44.1 mW/g

d=10mm, Pin=250mW, f=5500 MHz/Zoom Scan (8x8x8), dist=2mm 2 (8x8x8)/Cube 0:
 Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm
 Reference Value = 79.1 V/m; Power Drift = 0.048 dB
 Peak SAR (extrapolated) = 84.3 W/kg
SAR(1 g) = 21.3 mW/g; SAR(10 g) = 6 mW/g
 Maximum value of SAR (measured) = 41.2 mW/g


d=10mm, Pin=250mW, f=5800 MHz/Zoom Scan (8x8x8), dist=2mm (8x8x8)/Cube 0:
 Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm
 Reference Value = 75.5 V/m; Power Drift = 0.144 dB
 Peak SAR (extrapolated) = 86.2 W/kg
SAR(1 g) = 20.7 mW/g; SAR(10 g) = 5.8 mW/g
 Maximum value of SAR (measured) = 43.3 mW/g

Impedance Measurement Plot for Head TSL

2 May 2006 11:10:37


CHI S11 1 U FS 1: 49.063 Ω -13.175 Ω 2.4159 pF 5 000.000 000 MHz

*
Del
Cor
Avg
16
†

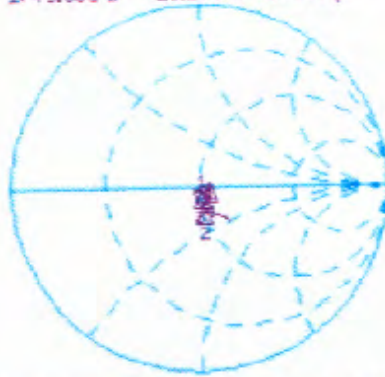

CH1 Markers
2: 50.549 Ω
-10.248 Ω
5.20000 GHz
3: 50.354 Ω
-1.4160 Ω
5.50000 GHz
4: 54.930 Ω
1.3742 Ω
5.80000 GHz

CH2 S11 LOG 5 dB/REF -20 dB 1: -17.578 dB 5 000.000 000 MHz

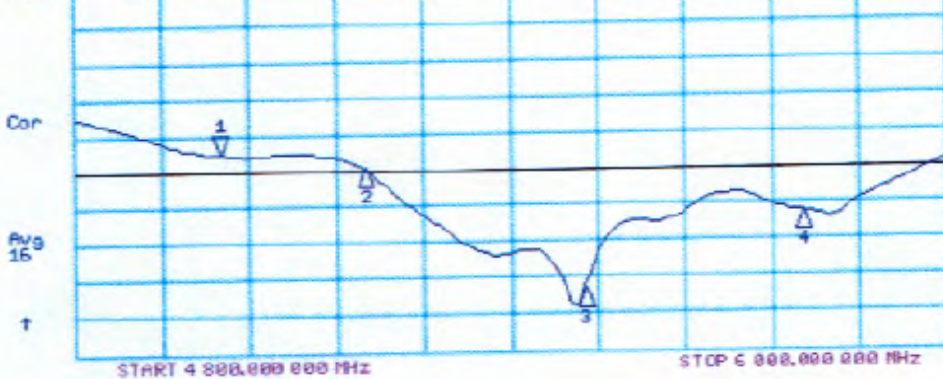

CH2 Markers
2: -19.867 dB
5.20000 GHz
3: -36.729 dB
5.50000 GHz
4: -25.124 dB
5.80000 GHz

DASY4 Validation Report for Body TSL

Date/Time: 03.05.2006 12:55:54

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHz; Serial: D5100V2 - SN:1001

Communication System: CW-5GHz; Frequency: 5500 MHz Frequency: 5800 MHz; Duty Cycle: 1:1

Medium: MSL U10 BB;

Medium parameters used: $f = 5500$ MHz; $\sigma = 5.5$ mho/m; $\epsilon_r = 48.4$; $\rho = 1000$ kg/m³ Medium parameters used: $f = 5800$ MHz; $\sigma = 5.88$ mho/m; $\epsilon_r = 47.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:


- Probe: EX3DV4 - SN3503; ConvF(4.67, 4.67, 4.67)ConvF(4.72, 4.72, 4.72); Calibrated: 18.03.2006
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 15.12.2005
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.7 Build 21; Postprocessing SW: SEMCAD, V1.8 Build 165

d=10mm, Pin=250mW, f=5500 MHz/Area Scan (91x91x1): Measurement grid: dx=dy=10mm
 Maximum value of SAR (interpolated) = 43.5 mW/g

d=10mm, Pin=250mW, f=5500 MHz/Zoom Scan (8x8x8), dist=2mm (8x8x8)/Cube 0:
 Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm
 Reference Value = 77.5 V/m; Power Drift = 0.074 dB
 Peak SAR (extrapolated) = 72.4 W/kg
SAR(1 g) = 19.7 mW/g; SAR(10 g) = 5.54 mW/g
 Maximum value of SAR (measured) = 37.5 mW/g

d=10mm, Pin=250mW, f=5800 MHz/Zoom Scan (8x8x8), dist=2mm (8x8x8)/Cube 0:
 Measurement grid: dx=4.3mm, dy=4.3mm, dz=3mm
 Reference Value = 73.3 V/m; Power Drift = 0.010 dB
 Peak SAR (extrapolated) = 70.9 W/kg
SAR(1 g) = 18 mW/g; SAR(10 g) = 5.04 mW/g
 Maximum value of SAR (measured) = 35.1 mW/g

Impedance Measurement Plot for Body TSL

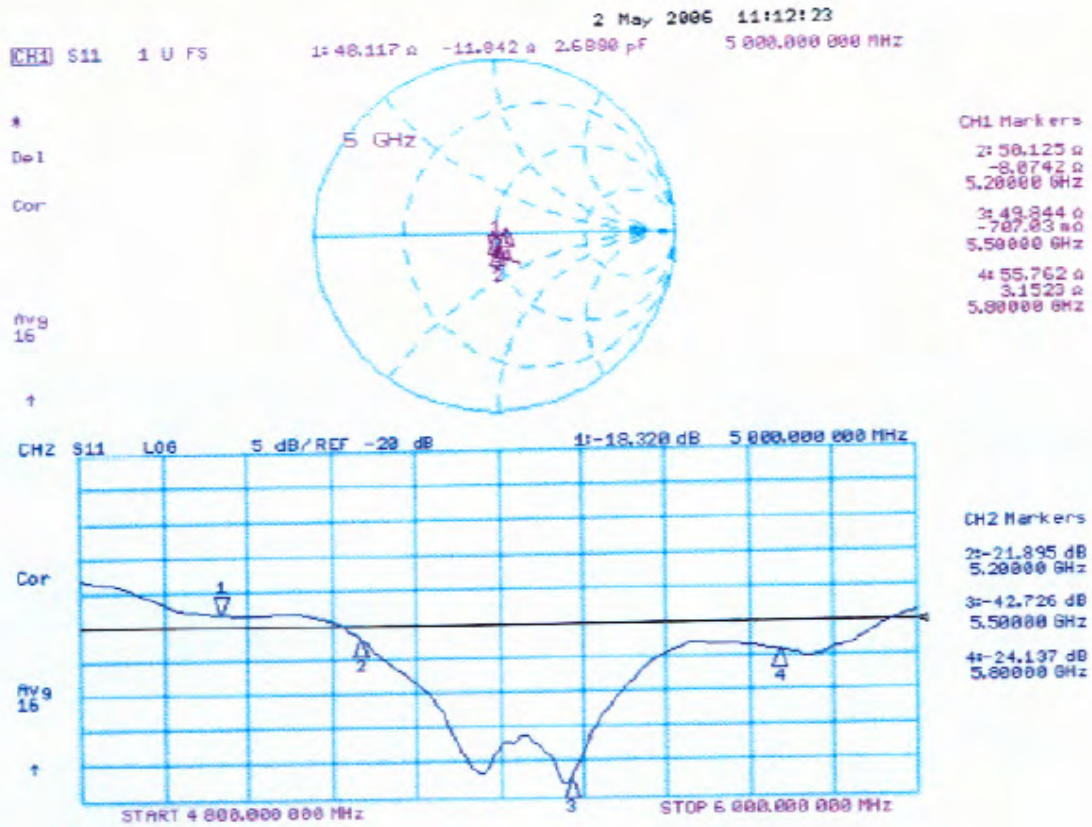

APPENDIX D - TEST SYSTEM VERIFICATIONS SCANS

Liquid Measurement Result

2006-11-7 & 2006-11-8 & 2006-11-9

Stimulant	Freq [MHz]	Parameters	Liquid Temp [°C]	Target Value	Measured Value	Deviation [%]	Limits [%]
Head	2450	ϵ	22	39.2	39.1	-0.26	± 5
		σ	22	1.80	1.81	0.56	± 5
		1g SAR	22	52.4	51.7	-1.34	± 10
Body	2450	ϵ	21	52.7	52.5	-0.38	± 5
		σ	21	1.95	1.96	0.51	± 5
		1g SAR	21	56.84	56.74	-0.18	± 10

ϵ_r = relative permittivity, σ = conductivity and $\rho=1000\text{kg/m}^3$

2006-11-10 & 2006-11-13 & 2006-11-14

Stimulant	Freq [MHz]	Parameters	Liquid Temp [°C]	Target Value	Measured Value	Deviation [%]	Limits [%]
Head	5800	ϵ_r	22.0	35.3	36.27	2.75	± 5
		σ	22.0	5.27	5.26	-0.19	± 5
		1g SAR	22.0	76.5	76.8	0.39	± 10
Body	5800	ϵ_r	22.0	48.2	47.4	-1.66	± 5
		σ	22.0	6.0	6.05	0.83	± 5
		1g SAR	22.0	74.27	75.16	1.20	± 10

ϵ_r = relative permittivity, σ = conductivity and $\rho=1000\text{kg/m}^3$

Test Laboratory: Bay Area Compliance Laboratories Corp. (BACL)

System Performance Check for Head

EUT: Dipole Antenna 2450 MHz; Type: D-2450-S-1; Serial Number: BCL-141

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
 Medium parameters used: $f = 2450$ MHz; $\sigma = 1.81$ mho/m; $\epsilon_r = 39.1$; $\rho = 1000$ kg/m³
 Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 – s/n: 1604; ConvF(4.60, 4.60, 4.60); Calibrated: 2006-05-02
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 s/n: 456; calibrated: 2005-10-18
- Phantom: SAM with CRP; Type: Twin SAM; s/n: TP-1032
- Measurement SW: DASY4, V4.6 Build 23; Post processing SW: SEMCAD, V1.8 Build 161

System Performance Check for Head, 1W/Area Scan (81x101x1): Measurement grid: dx=10mm, dy=10mm
 Maximum value of SAR (interpolated) = 55.2 mW/g

System Performance Check for Head, 1W/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 195.2 V/m; Power Drift = 0.000 dB

Peak SAR (extrapolated) = 104.9 W/kg

SAR(1 g) = 51.7 mW/g; SAR(10 g) = 23.5 mW/g

Maximum value of SAR (measured) = 54.6 mW/g

