

Test Laboratory: The name of your organization

D835V2SN4d002_033104

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d002

Ambient temperature = 23.0 deg. C; Liquid temperature = 22.0 deg. C

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 835$ MHz; $\sigma = 0.917$ mho/m; $\epsilon_r = 42$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 - SN3021; ConvF(6.5, 6.5, 6.5); Calibrated: 7/29/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 12/23/2003
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DASY4, V4.2 Build 37; Postprocessing SW: SEMCAD, V1.8 Build 109

d=15mm, Pin=250mW/Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Reference Value = 55.5 V/m; Power Drift = -0.0 dB

Maximum value of SAR (measured) = 2.75 mW/g


d=15mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm

Reference Value = 55.5 V/m; Power Drift = -0.0 dB

Maximum value of SAR (measured) = 2.74 mW/g

Peak SAR (extrapolated) = 3.85 W/kg

SAR(1 g) = 2.55 mW/g; SAR(10 g) = 1.65 mW/g

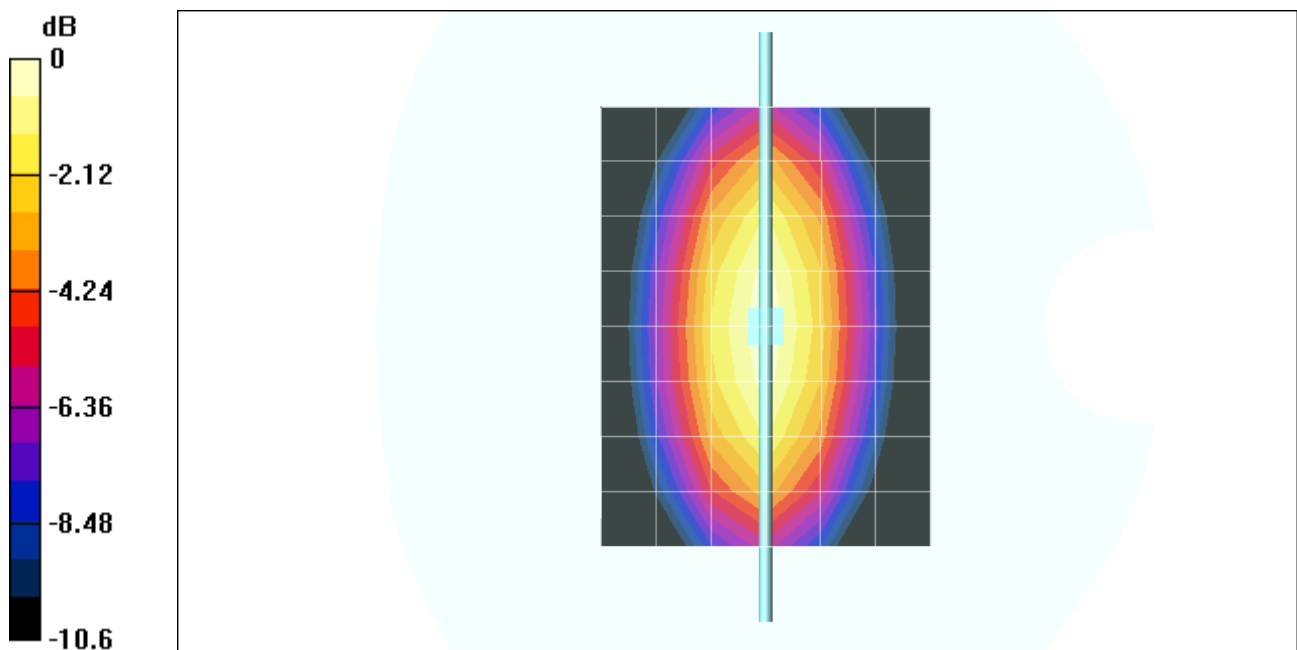

0 dB = 2.74mW/g

Test Laboratory: The name of your organization

D835V2SN4d002_033104

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d002


DASY4 Configuration:

- Probe: ES3DV2 - SN3021; ConvF(6.5, 6.5, 6.5); Calibrated: 7/29/2003
- Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE3 Sn500; Calibrated: 12/23/2003
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DASY4, V4.2 Build 37; Postprocessing SW: SEMCAD, V1.8 Build 109

d=15mm, Pin=250mW/Z Scan (1x1x51): Measurement grid: dx=20mm, dy=20mm, dz=2mm

Reference Value = 55.5 V/m; Power Drift = -0.0 dB

Maximum value of SAR (measured) = 2.3 mW/g

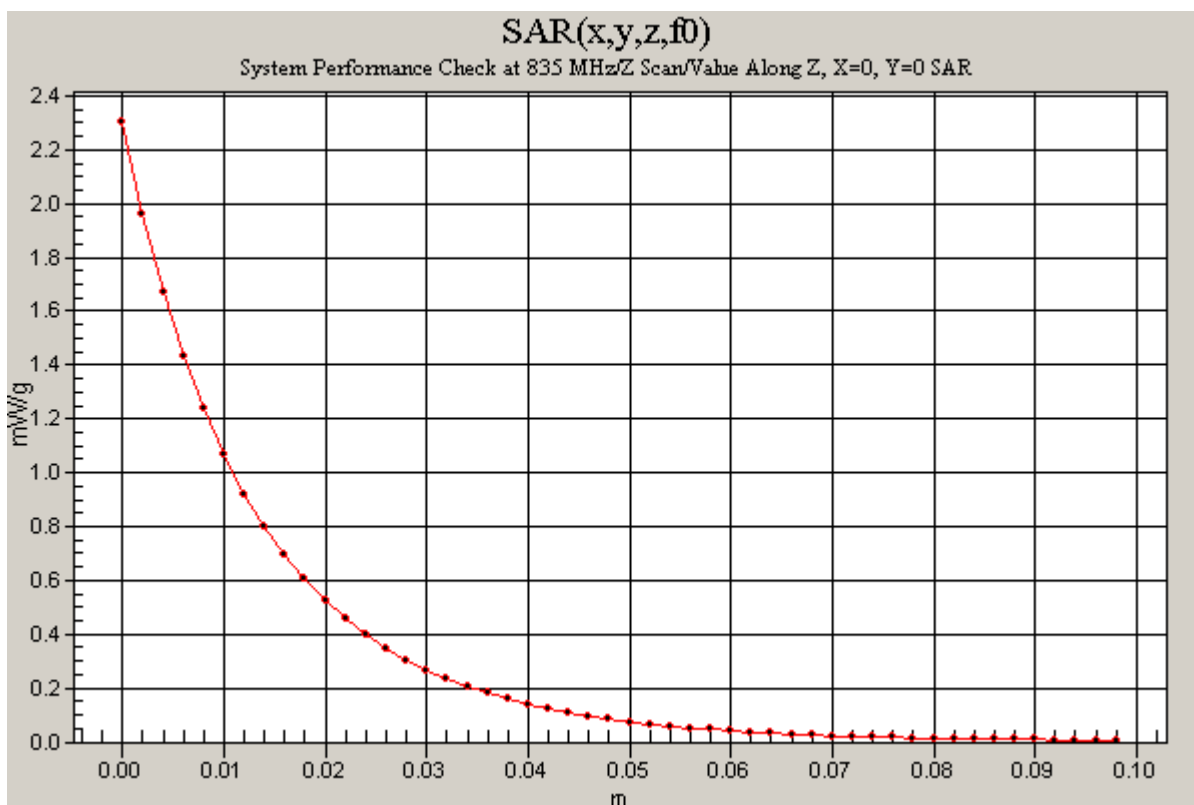

Test Laboratory: The name of your organization

D835V2SN4d002_040104

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d002

Ambient temperature = 23.0 deg. C; Liquid temperature = 22.0 deg. C

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 835$ MHz; $\sigma = 0.912$ mho/m; $\epsilon_r = 41.5$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DAS4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 - SN3021; ConvF(6.5, 6.5, 6.5); Calibrated: 7/29/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn500; Calibrated: 12/23/2003
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DAS4, V4.2 Build 37; Postprocessing SW: SEMCAD, V1.8 Build 109

d=15mm, Pin=250mW/Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Reference Value = 55.1 V/m; Power Drift = -0.0 dB

Maximum value of SAR (measured) = 2.73 mW/g


d=15mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm

Reference Value = 55.1 V/m; Power Drift = -0.0 dB

Maximum value of SAR (measured) = 2.72 mW/g

Peak SAR (extrapolated) = 3.8 W/kg

SAR(1 g) = 2.5 mW/g; SAR(10 g) = 1.62 mW/g

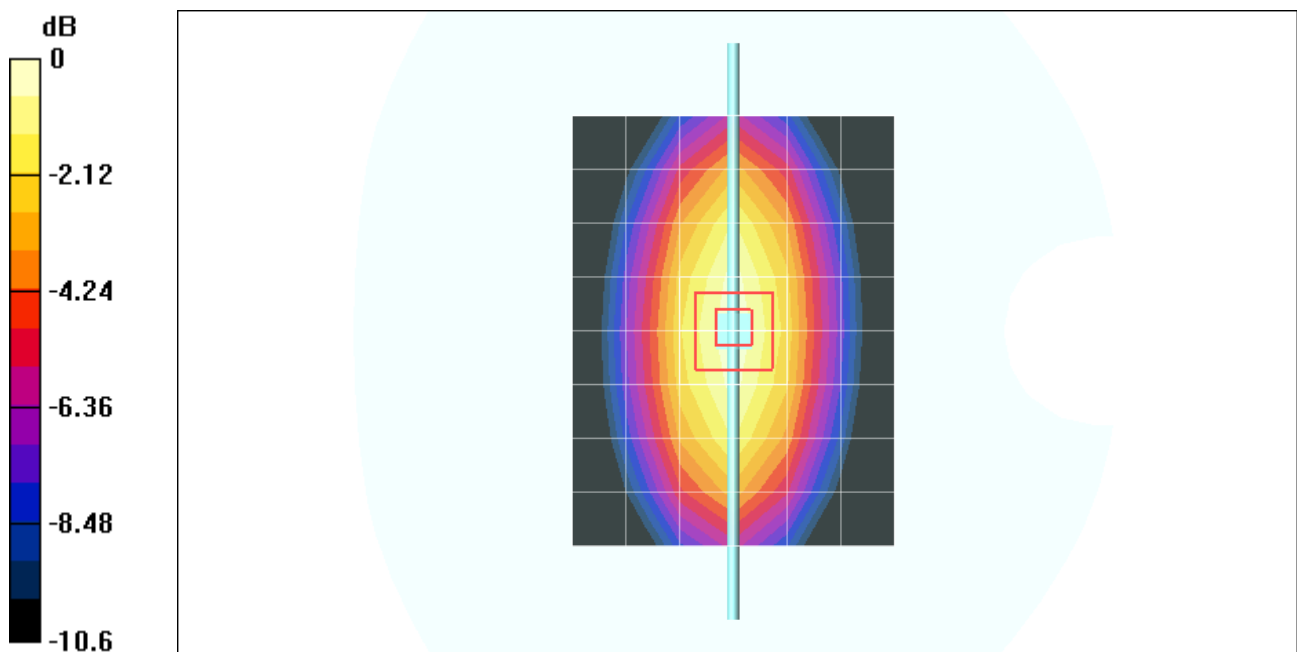

0 dB = 2.72mW/g

Test Laboratory: The name of your organization

D835V2SN4d002_040104

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d002

DASY4 Configuration:

- Probe: ES3DV2 - SN3021; ConvF(6.5, 6.5, 6.5); Calibrated: 7/29/2003
- Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE3 Sn500; Calibrated: 12/23/2003
- Phantom: SAM 2; Type: SAM 2; Serial: 1050
- Measurement SW: DASY4, V4.2 Build 37; Postprocessing SW: SEMCAD, V1.8 Build 109

d=15mm, Pin=250mW/Z Scan (1x1x51): Measurement grid: dx=20mm, dy=20mm, dz=2mm

Reference Value = 55.1 V/m; Power Drift = -0.0 dB

Maximum value of SAR (measured) = 2.27 mW/g

