

Test Laboratory: Compliance Certification Services

File Name: [D900V2_108.da4](#)

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN:xxx
Program: System Performance Check at 900 MHz
Ambient Temperature: 24.5 deg C; Liquid Temperature: 23 deg C

Communication System: CW; Frequency: 900 MHz; Duty Cycle: 1:1
 Medium: Head 900 MHz ($\sigma = 0.96401$ mho/m, $\epsilon_r = 41.1443$, $\rho = 1000$ kg/m³)
 Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(7.1, 7.1, 7.1); Calibrated: 2/7/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

d=15mm, Pin=250mW/Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

d=15mm, Pin=250mW/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm


Peak SAR (extrapolated) = 3.99 W/kg

SAR(1 g) = 2.71 mW/g; SAR(10 g) = 1.73 mW/g

Reference Value = 56.9 V/m

Power Drift = -0.02 dB

Maximum value of SAR = 2.86 mW/g

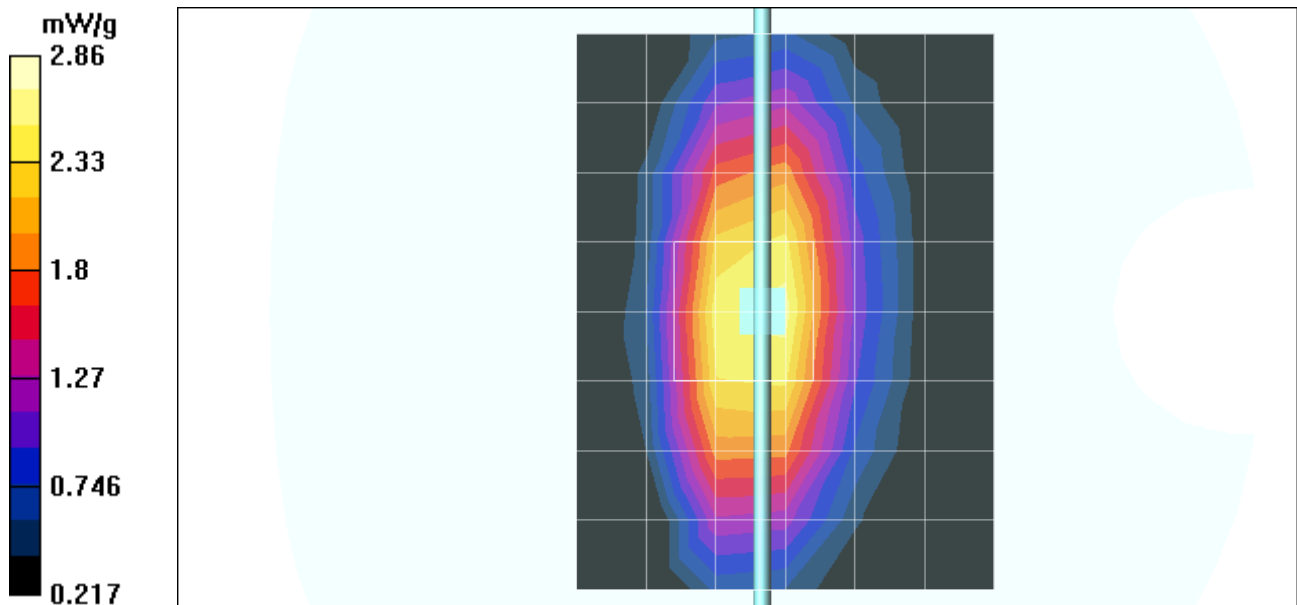

Test Laboratory: Compliance Certification Services

File Name: [D900V2_108.da4](#)

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN:xxx
Program: System Performance Check at 900 MHz

Communication System: CW; Frequency: 900 MHz; Duty Cycle: 1:1

Medium: Head 900 MHz ($\sigma = 0.96401$ mho/m, $\epsilon_r = 41.1443$, $\rho = 1000$ kg/m³)

Phantom section: Flat Section

DASY4 Configuration:


- Probe: ET3DV6 - SN1577; ConvF(7.1, 7.1, 7.1); Calibrated: 2/7/2003
- Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

d=15mm, Pin=250mW/Z Scan (1x1x61): Measurement grid: dx=20mm, dy=20mm, dz=2mm

Reference Value = 56.9 V/m

Power Drift = -0.01 dB

Maximum value of SAR = 1.73 mW/g

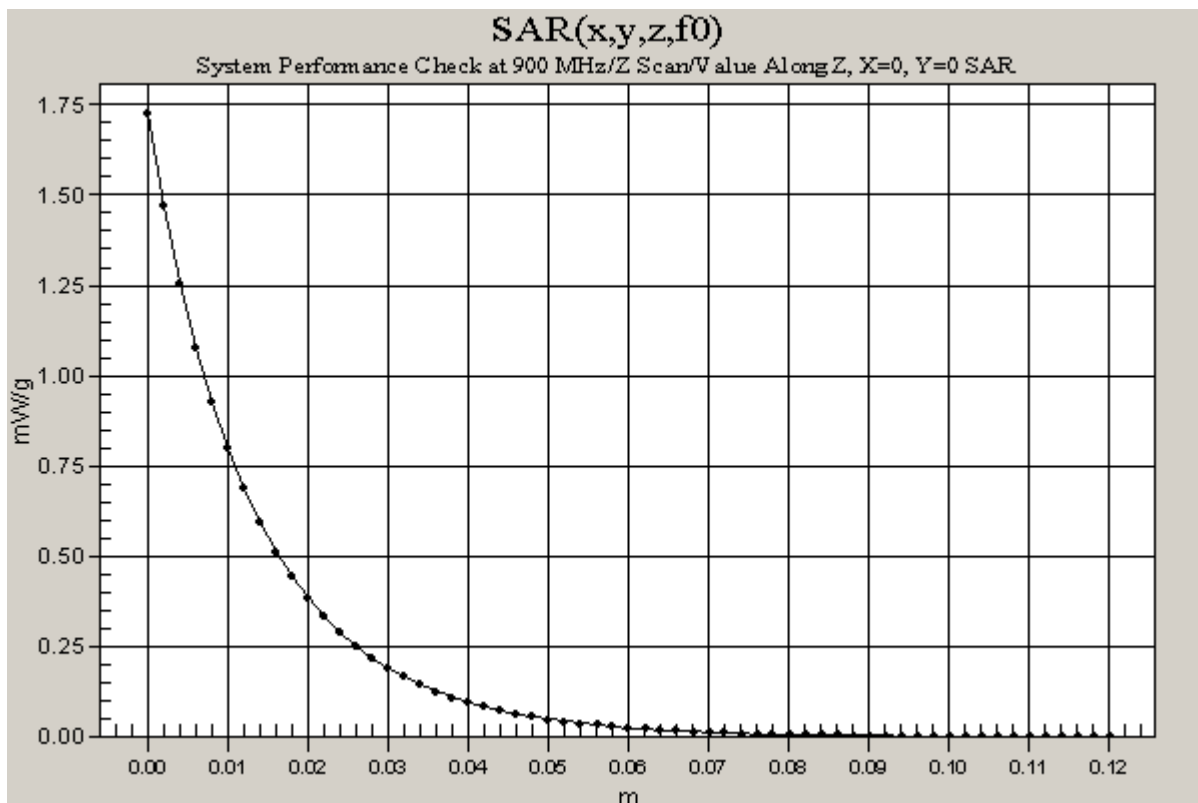

Test Laboratory: Compliance Certification Services

File Name: [D900V2_108.da4](#)

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN:xxx
Program: System Performance Check at 900 MHz
Ambient Temperature: 24.5 deg C; Liquid Temperature: 23.0 deg C

Communication System: CW; Frequency: 900 MHz; Duty Cycle: 1:1
 Medium: Head 900 MHz ($\sigma = 0.9766$ mho/m, $\epsilon_r = 41.1693$, $\rho = 1000$ kg/m³)
 Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(7.1, 7.1, 7.1); Calibrated: 2/7/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

d=15mm, Pin=250mW/Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

d=15mm, Pin=250mW/Zoom Scan (5x5x7) (5x5x7)/Cube 0: Measurement grid: dx=7.5mm, dy=7.5mm, dz=5mm


Peak SAR (extrapolated) = 4.16 W/kg

SAR(1 g) = 2.83 mW/g; SAR(10 g) = 1.81 mW/g

Reference Value = 58.4 V/m

Power Drift = -0.03 dB

Maximum value of SAR = 3.03 mW/g

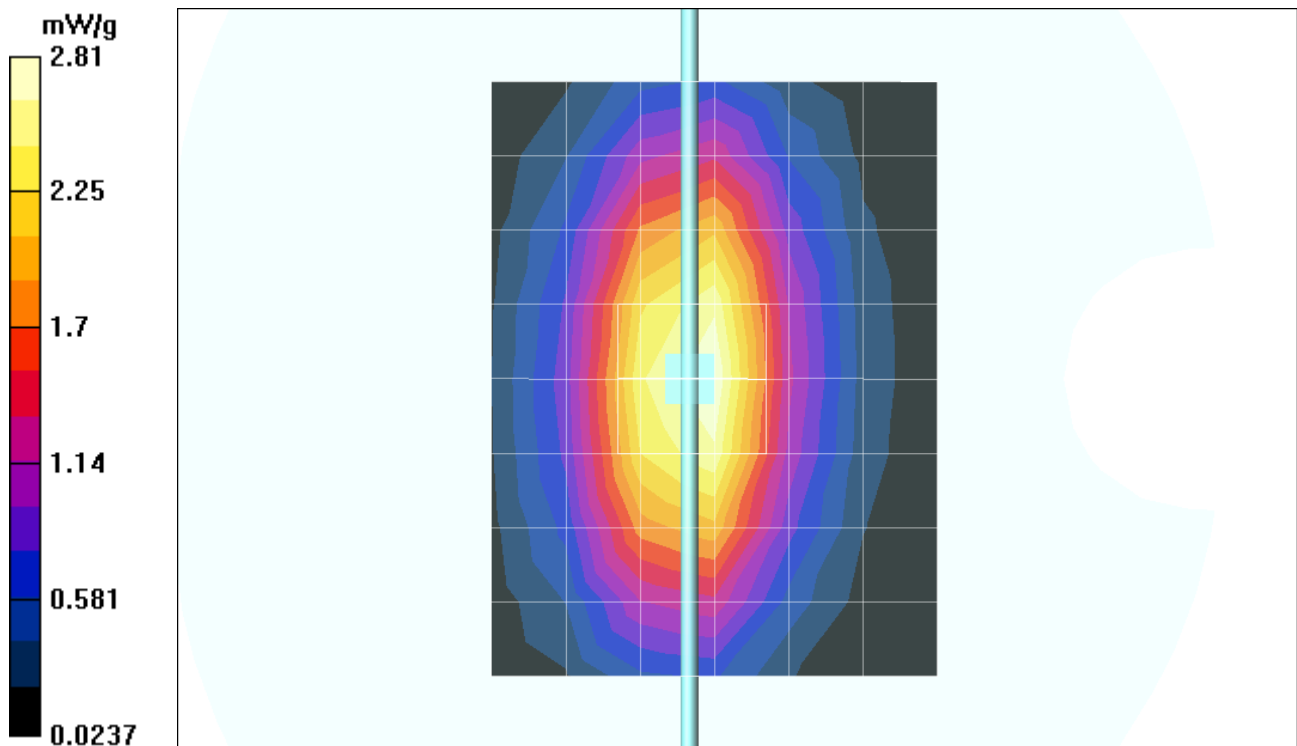

Test Laboratory: Compliance Certification Services

File Name: [D900V2_108.da4](#)

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN:xxx
Program: System Performance Check at 900 MHz

Communication System: CW; Frequency: 900 MHz; Duty Cycle: 1:1

Medium: Head 900 MHz ($\sigma = 0.9766$ mho/m, $\epsilon_r = 41.1693$, $\rho = 1000$ kg/m³)

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(7.1, 7.1, 7.1); Calibrated: 2/7/2003
- Sensor-Surface: 0mm (Fix Surface)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 1; Type: SAM 1; Serial: 1185
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

d=15mm, Pin=250mW/Z Scan (1x1x51): Measurement grid: dx=20mm, dy=20mm, dz=2mm

Reference Value = 58.4 V/m

Power Drift = -0.04 dB

Maximum value of SAR = 1.67 mW/g

