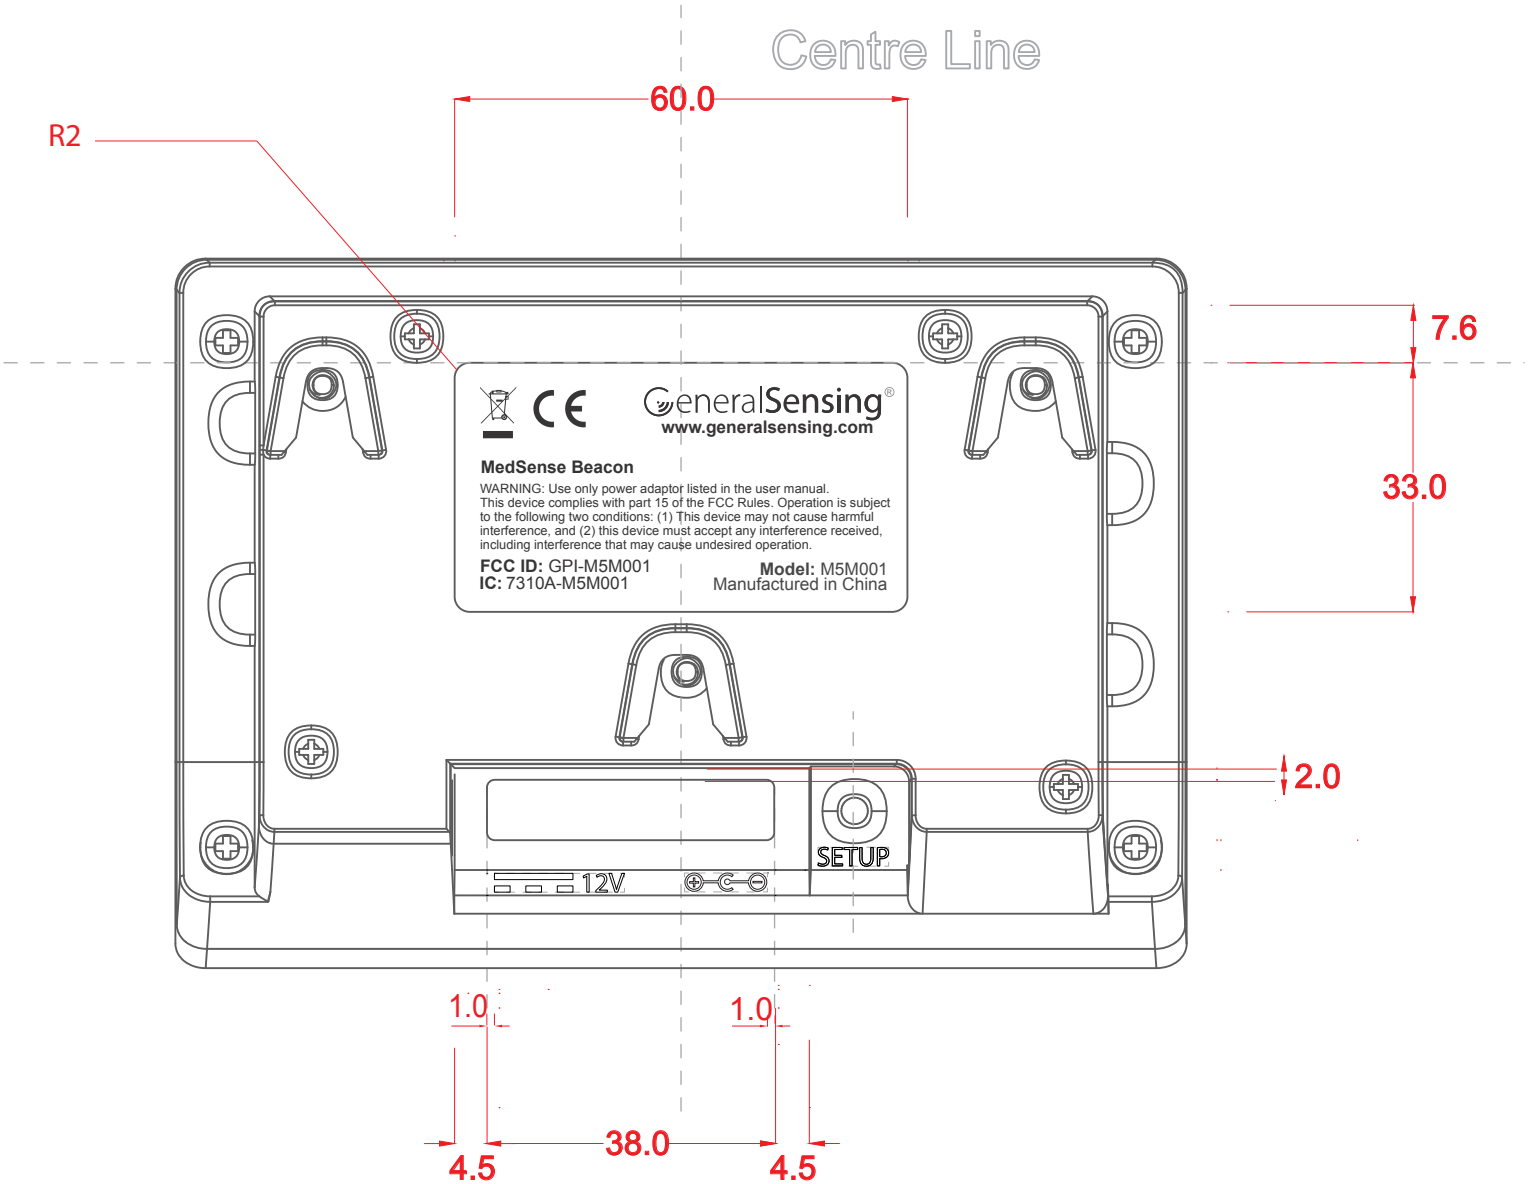
Centre Line
60.0
R2
7.6
33.0
2.0
GeneralSensing®
www.generalsensing.com
MedSense Beacon
WARNING: Use only power adaptor listed in the user manual.
This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.
FCC ID: GPI-M5M001
IC: 7310A-M5M001
Model: M5M001
Manufactured in China
SETUP
12V
1.0
1.0
4.5
38.0
4.5