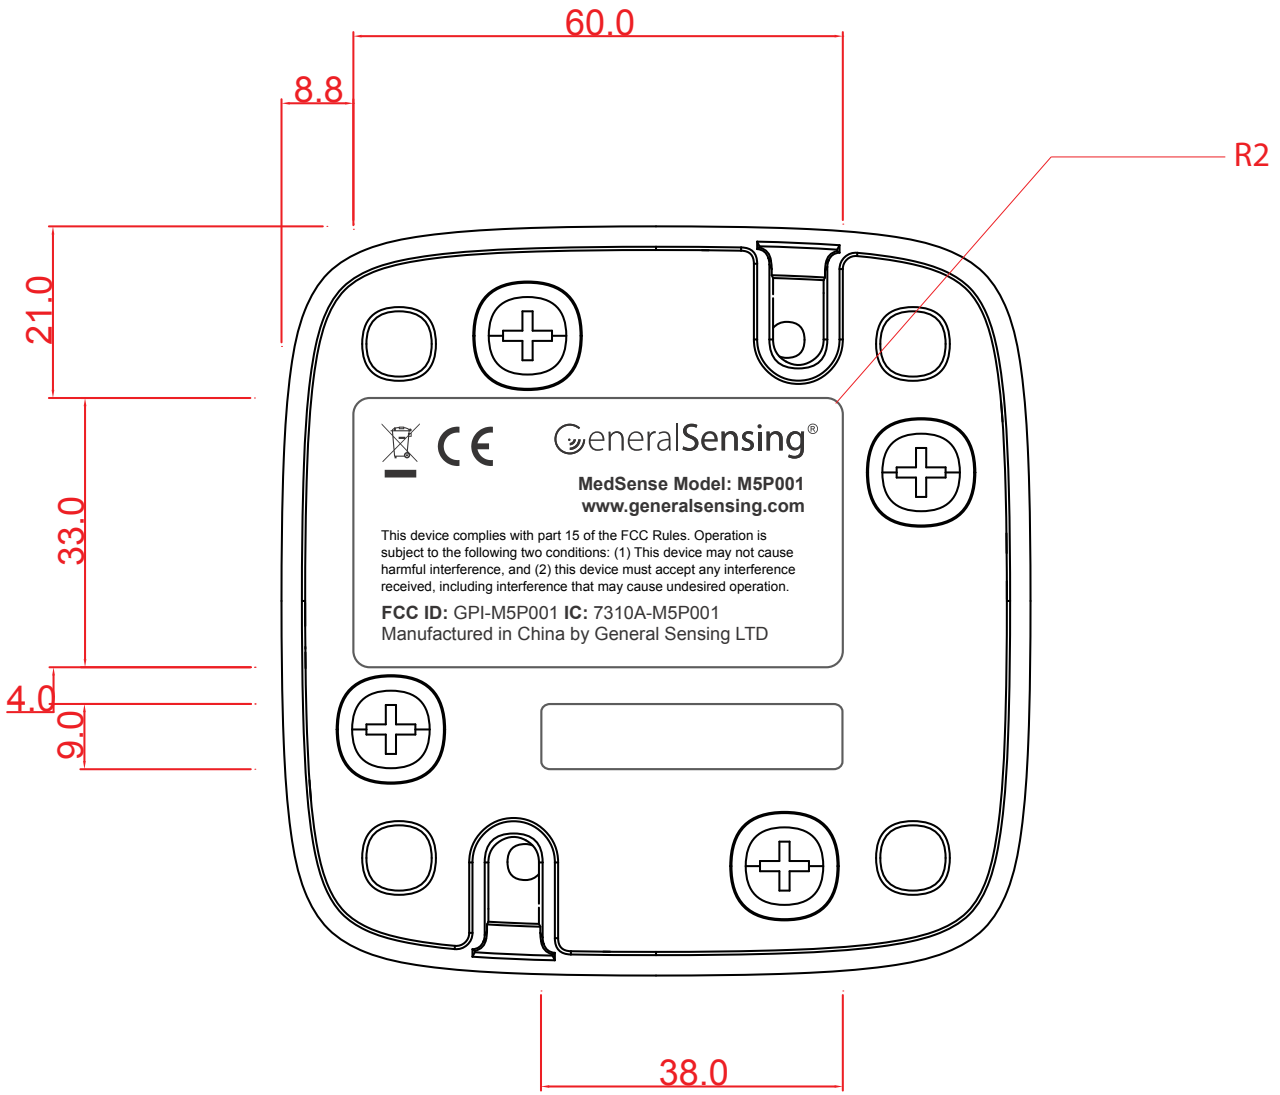
60.0
8.8
R2
21.0
33.0
4.0
9.0
38.0
GeneralSensing®
MedSense Model: M5P001
www.generalsensing.com
This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.
FCC ID: GPI-M5P001 IC: 7310A-M5P001
Manufactured in China by General Sensing LTD