

Calibration Certificate


Dosimetric E-Field Probe

Type:	ET3DV6
Serial Number:	1578
Place of Calibration:	Zurich
Date of Calibration:	February 22, 2002
Calibration Interval:	12 months


Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:



Approved by:



Probe ET3DV6

SN:1578

Manufactured:	April 6, 2001
Last calibration:	April 20, 2001
Recalibrated:	February 22, 2002

Calibrated for System DASY3

DASY3 - Parameters of Probe: ET3DV6 SN:1578

Sensitivity in Free Space

NormX	1.72 $\mu\text{V}/(\text{V}/\text{m})^2$
NormY	1.83 $\mu\text{V}/(\text{V}/\text{m})^2$
NormZ	1.68 $\mu\text{V}/(\text{V}/\text{m})^2$

Diode Compression

DCP X	99	mV
DCP Y	99	mV
DCP Z	99	mV

Sensitivity in Tissue Simulating Liquid

Head	900 MHz	$\epsilon_r = 41.5 \pm 5\%$	$\sigma = 0.97 \pm 5\%$ mho/m
Head	835 MHz	$\epsilon_r = 41.5 \pm 5\%$	$\sigma = 0.90 \pm 5\%$ mho/m
ConvF X	7.0 $\pm 9.5\%$ (k=2)		Boundary effect:
ConvF Y	7.0 $\pm 9.5\%$ (k=2)		Alpha 0.33
ConvF Z	7.0 $\pm 9.5\%$ (k=2)		Depth 2.34
Head	1800 MHz	$\epsilon_r = 40.0 \pm 5\%$	$\sigma = 1.40 \pm 5\%$ mho/m
Head	1900 MHz	$\epsilon_r = 40.0 \pm 5\%$	$\sigma = 1.40 \pm 5\%$ mho/m
ConvF X	5.5 $\pm 9.5\%$ (k=2)		Boundary effect:
ConvF Y	5.5 $\pm 9.5\%$ (k=2)		Alpha 0.47
ConvF Z	5.5 $\pm 9.5\%$ (k=2)		Depth 2.20

Boundary Effect


Head	900 MHz	Typical SAR gradient: 5 % per mm	
	Probe Tip to Boundary	1 mm	2 mm
	SAR _{be} [%] Without Correction Algorithm	7.6	4.3
	SAR _{be} [%] With Correction Algorithm	0.2	0.4
Head	1800 MHz	Typical SAR gradient: 10 % per mm	
	Probe Tip to Boundary	1 mm	2 mm
	SAR _{be} [%] Without Correction Algorithm	9.5	6.3
	SAR _{be} [%] With Correction Algorithm	0.2	0.3

Sensor Offset


Probe Tip to Sensor Center	2.7	mm
Optical Surface Detection	1.5 \pm 0.2	mm

Receiving Pattern (ϕ), $\theta = 0^\circ$


f = 30 MHz, TEM cell ifi110

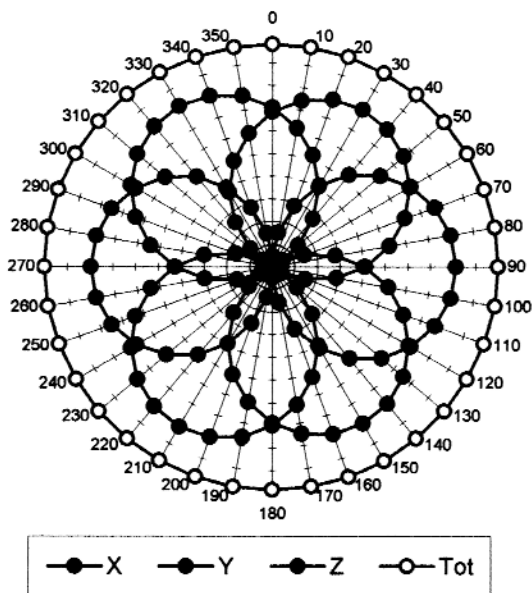


f = 100 MHz, TEM cell ifi110


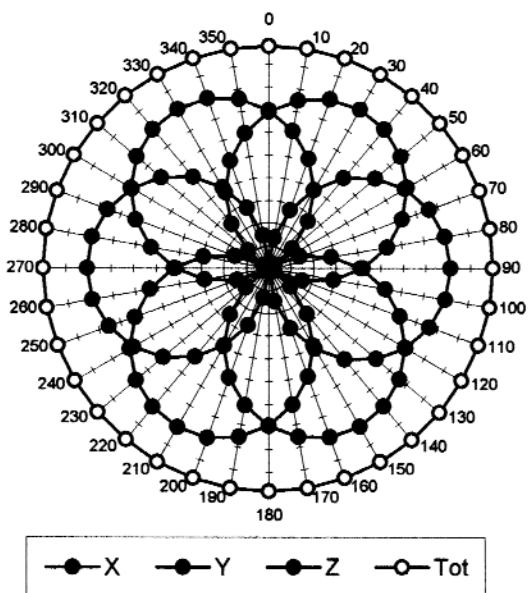


f = 300 MHz, TEM cell ifi110

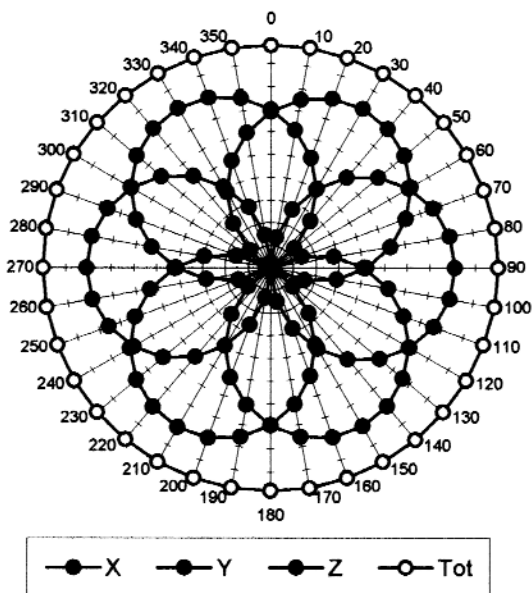


f = 900 MHz, TEM cell ifi110

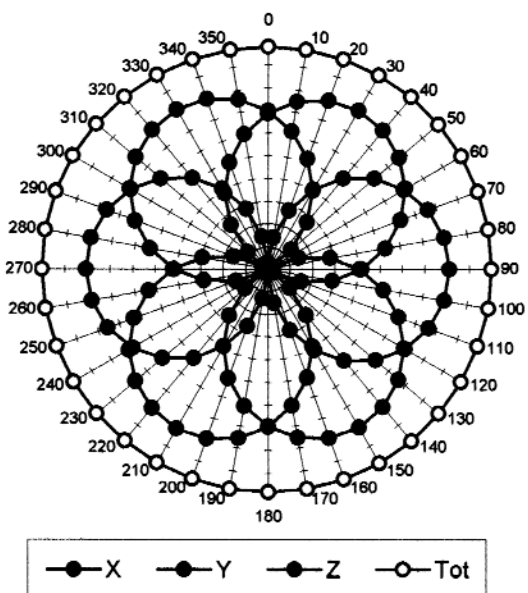

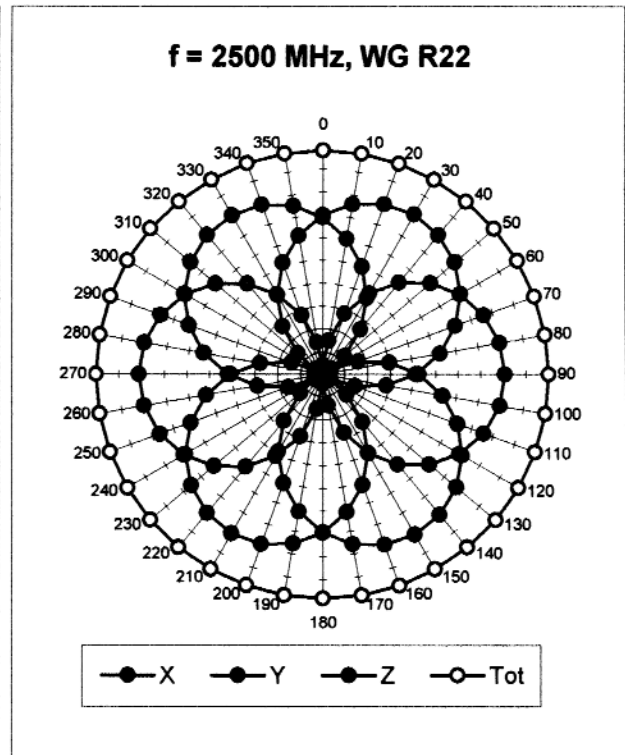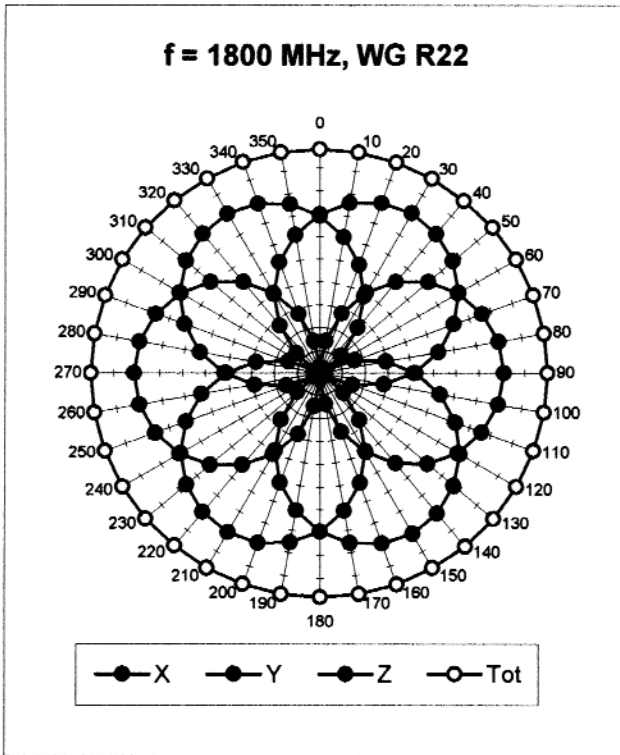


Isotropy Error (ϕ), $\theta = 0^\circ$


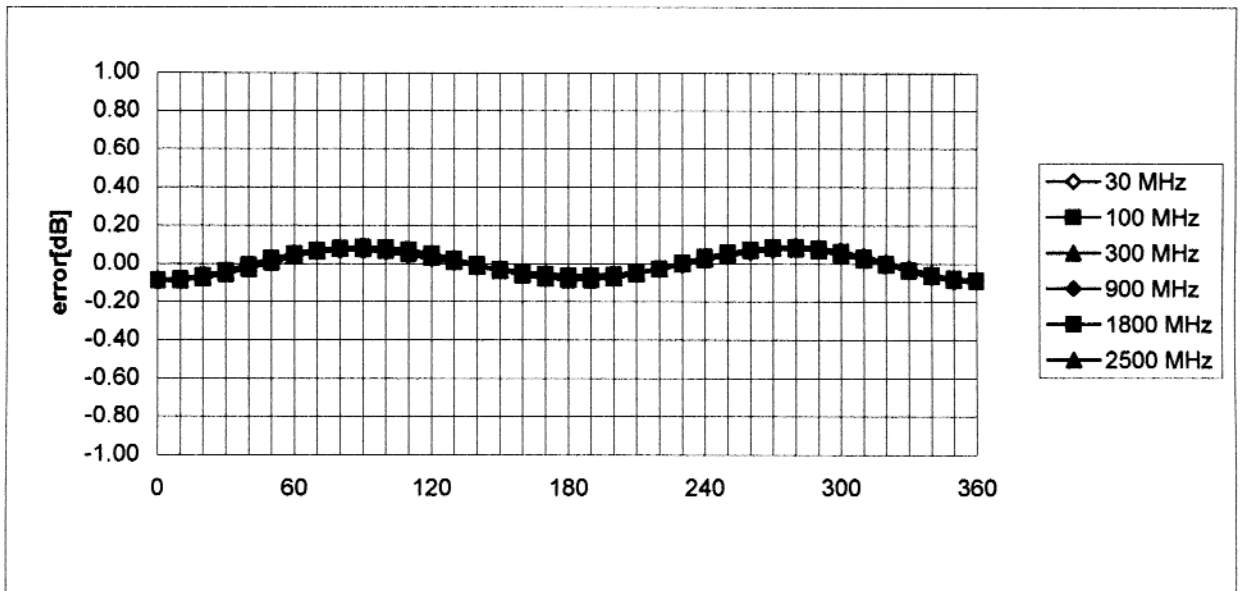


Frequency Response of E-Field



(TEM-Cell:ifi110, Waveguide R22)

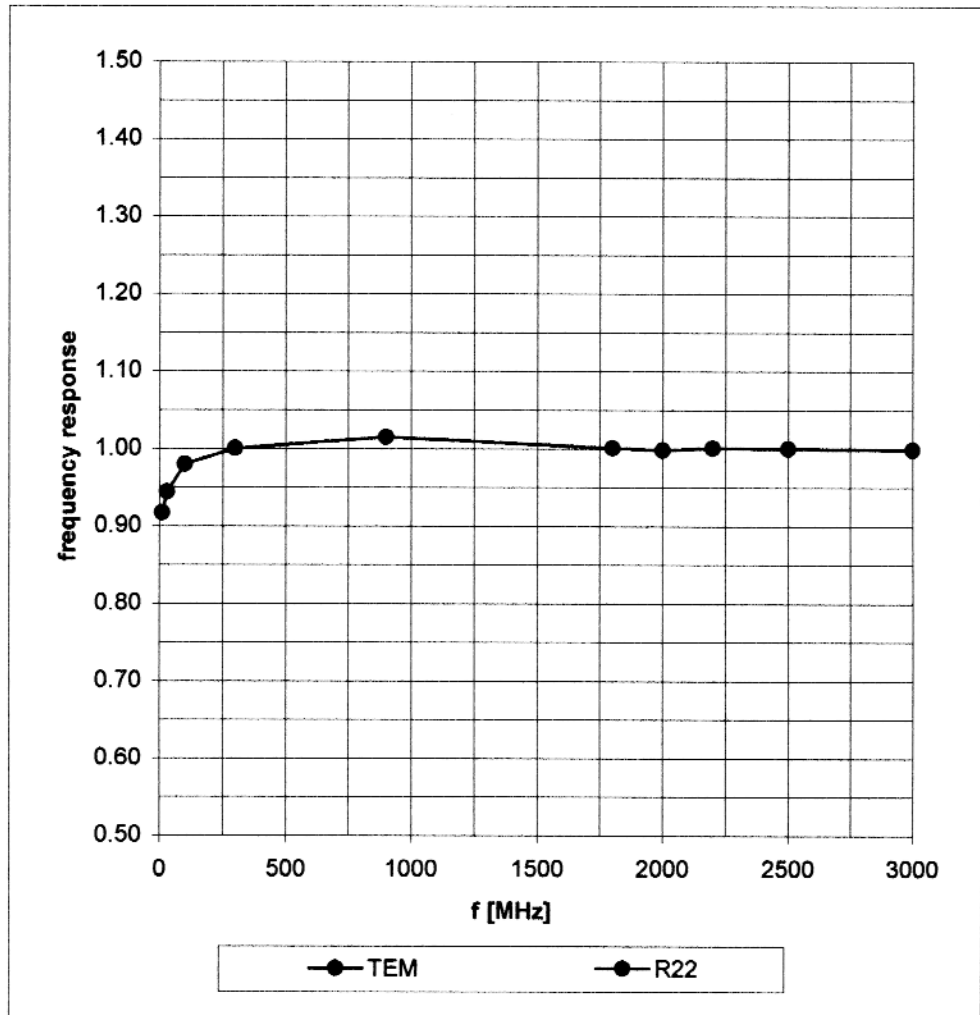

Dynamic Range f(SAR_{brain}) (Waveguide R22)

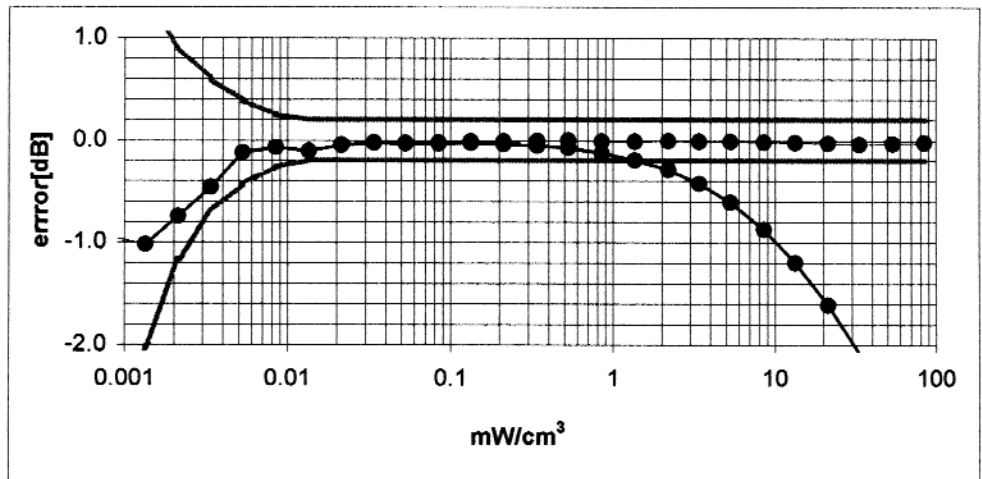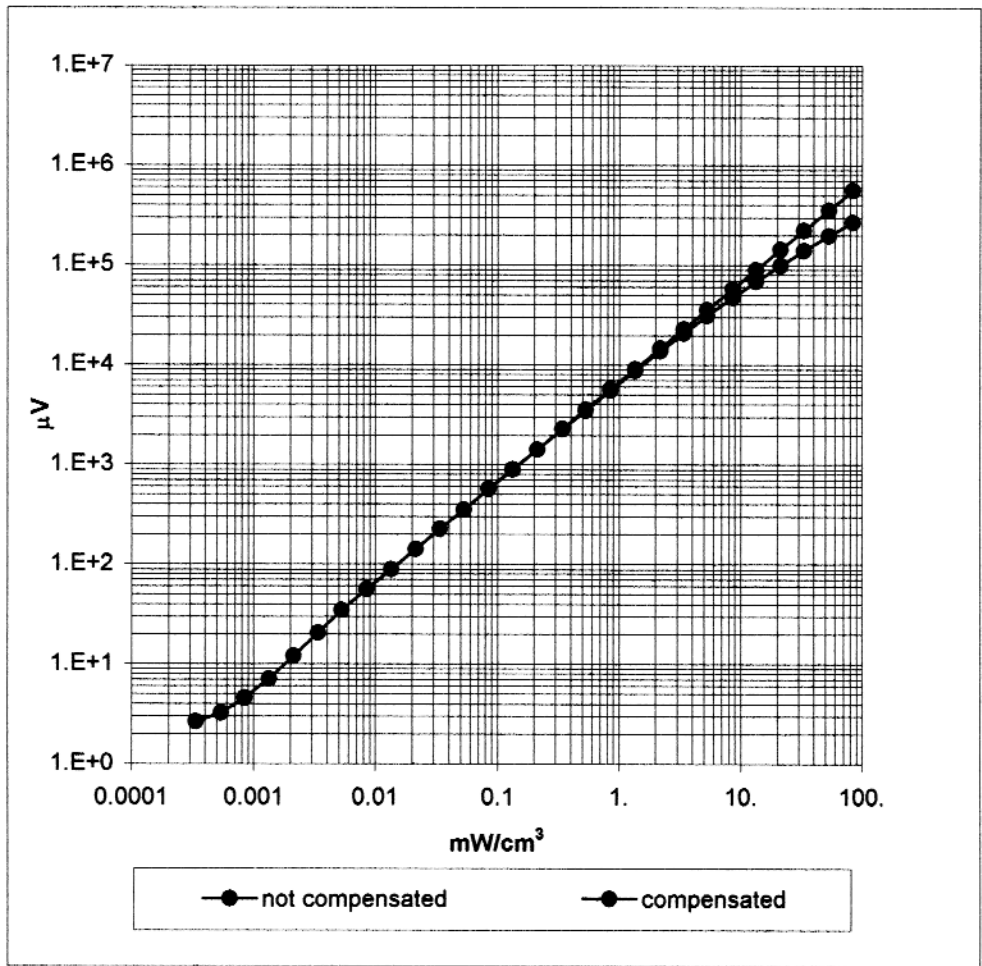


Conversion Factor Assessment

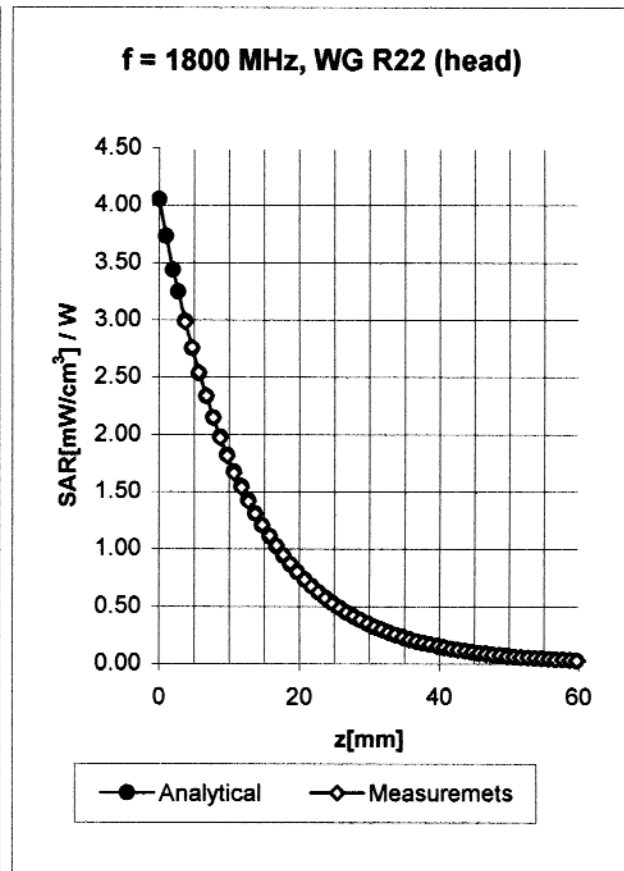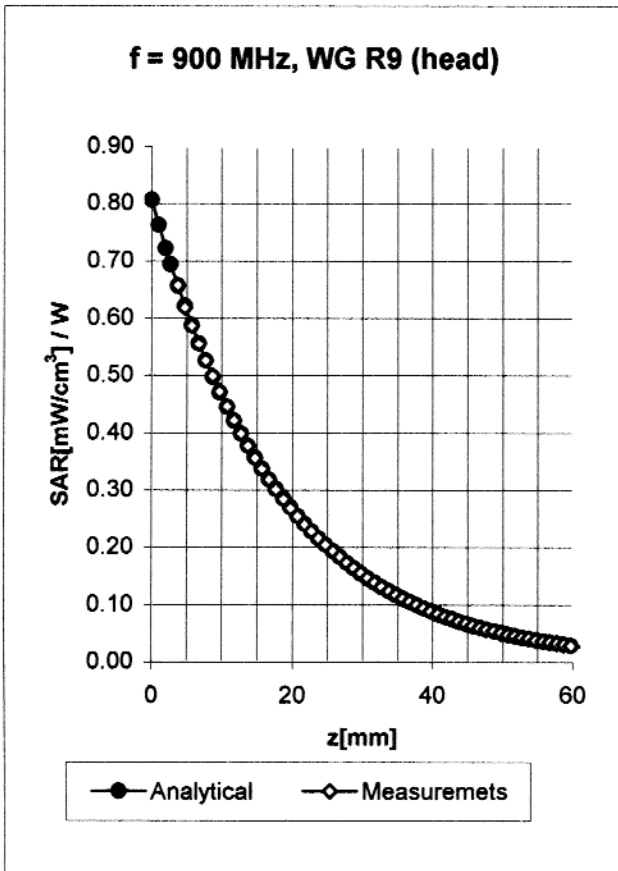

Head	900 MHz	$\epsilon_r = 41.5 \pm 5\%$	$\sigma = 0.97 \pm 5\%$ mho/m
Head	835 MHz	$\epsilon_r = 41.5 \pm 5\%$	$\sigma = 0.90 \pm 5\%$ mho/m
	ConvF X	7.0 $\pm 9.5\%$ (k=2)	Boundary effect:
	ConvF Y	7.0 $\pm 9.5\%$ (k=2)	Alpha 0.33
	ConvF Z	7.0 $\pm 9.5\%$ (k=2)	Depth 2.34
Head	1800 MHz	$\epsilon_r = 40.0 \pm 5\%$	$\sigma = 1.40 \pm 5\%$ mho/m
Head	1900 MHz	$\epsilon_r = 40.0 \pm 5\%$	$\sigma = 1.40 \pm 5\%$ mho/m
	ConvF X	5.5 $\pm 9.5\%$ (k=2)	Boundary effect:
	ConvF Y	5.5 $\pm 9.5\%$ (k=2)	Alpha 0.47
	ConvF Z	5.5 $\pm 9.5\%$ (k=2)	Depth 2.20


Conversion Factor Assessment

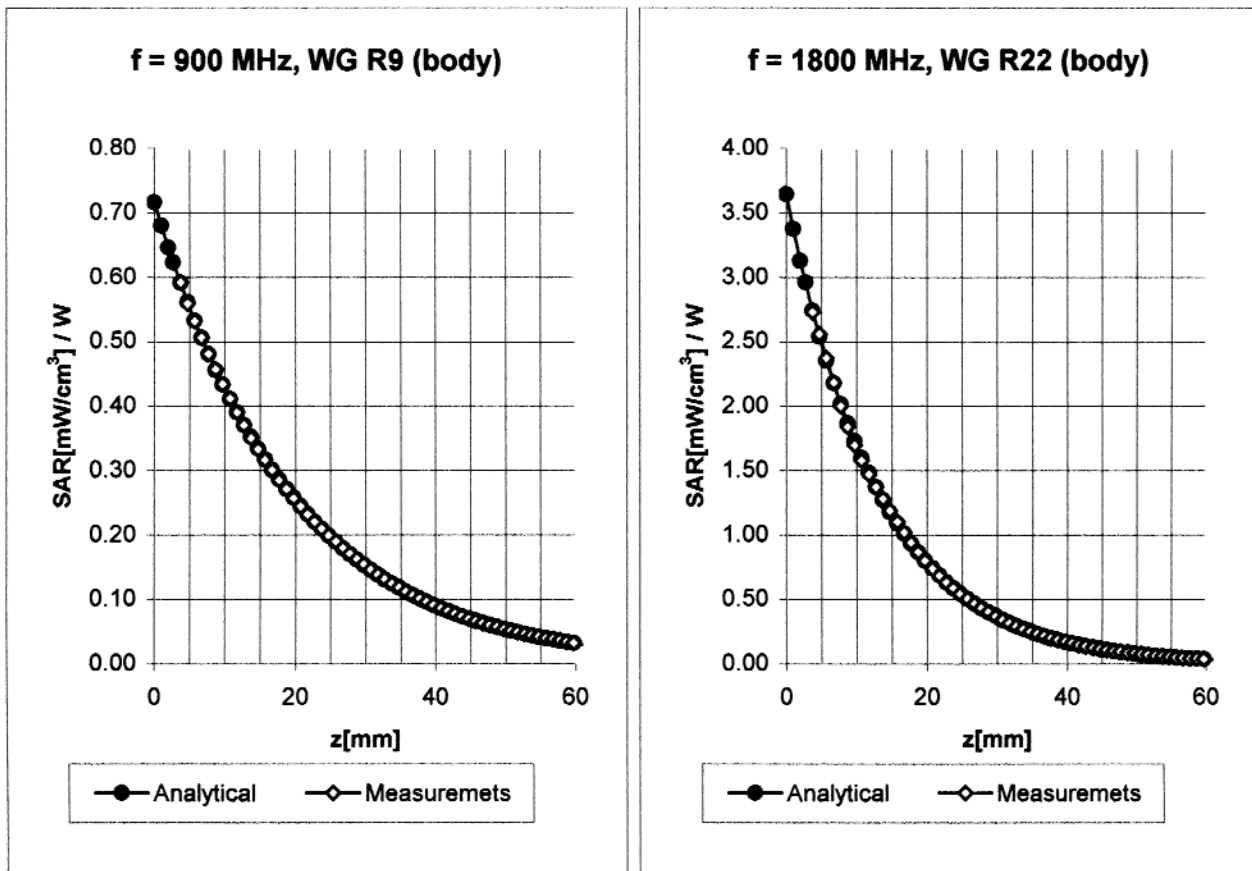

Body	900 MHz	$\epsilon_r = 55.0 \pm 5\%$	$\sigma = 1.05 \pm 5\% \text{ mho/m}$
Body	835 MHz	$\epsilon_r = 55.2 \pm 5\%$	$\sigma = 0.97 \pm 5\% \text{ mho/m}$
	ConvF X	6.7 $\pm 9.5\%$ (k=2)	Boundary effect:
	ConvF Y	6.7 $\pm 9.5\%$ (k=2)	Alpha 0.29
	ConvF Z	6.7 $\pm 9.5\%$ (k=2)	Depth 2.76
Body	1800 MHz	$\epsilon_r = 53.3 \pm 5\%$	$\sigma = 1.52 \pm 5\% \text{ mho/m}$
Body	1900 MHz	$\epsilon_r = 53.3 \pm 5\%$	$\sigma = 1.52 \pm 5\% \text{ mho/m}$
	ConvF X	5.1 $\pm 9.5\%$ (k=2)	Boundary effect:
	ConvF Y	5.1 $\pm 9.5\%$ (k=2)	Alpha 0.58
	ConvF Z	5.1 $\pm 9.5\%$ (k=2)	Depth 2.19

Deviation from Isotropy in HSL

Error (θ, ϕ), $f = 900$ MHz

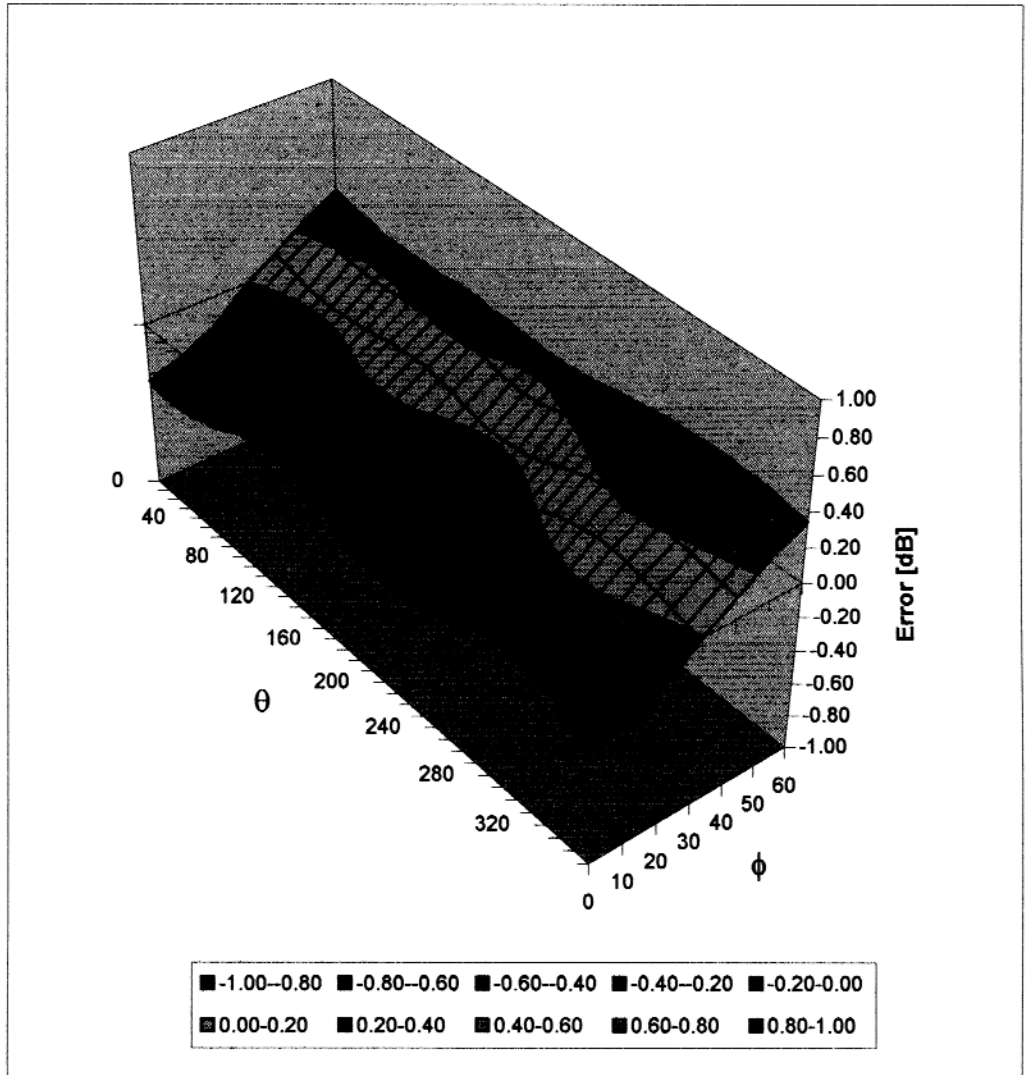

Additional Conversion Factors for Dosimetric E-Field Probe

Type:

ET3DV6

Serial Number:

1578

Place of Assessment:

Zurich

Date of Assessment:

February 25, 2002

Probe Calibration Date:

February 22, 2002

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:

Johnie Katz

Dosimetric E-Field Probe ET3DV6 SN:1578

Conversion factor (\pm standard deviation)

450 MHz ConvF **8.0 \pm 8%**

$\epsilon_r = 43.5$ $\sigma = 0.87$ mho/m (head tissue)

450 MHz ConvF **8.1 \pm 8%**

$\epsilon_r = 56.7$ $\sigma = 0.94$ mho/m (body tissue)

2450 MHz ConvF **4.5 \pm 8%**

$\epsilon_r = 39.2$ $\sigma = 1.80$ mho/m (head tissue)

2450 MHz ConvF **4.1 \pm 8%**

$\epsilon_r = 52.7$ $\sigma = 1.95$ mho/m (body tissue)
