
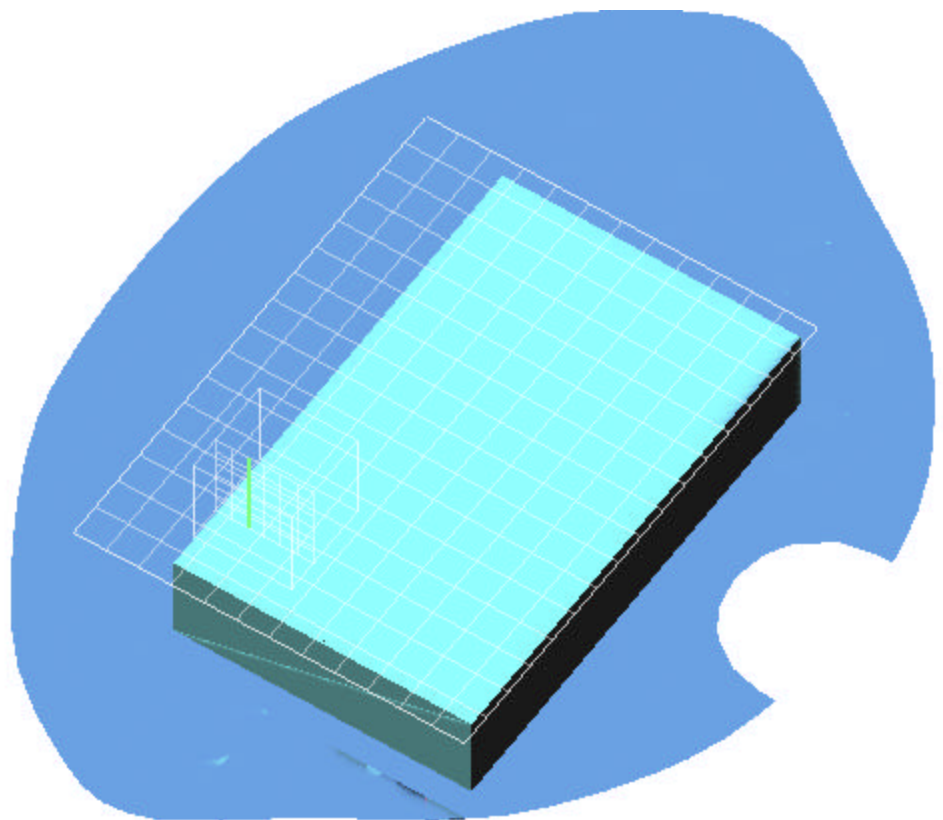


Test Laboratory: Compliance Certification Services  
File Name: 1L-CH\_0.28 mW.da4

### EUT Setup Configuration 1 (Back side)

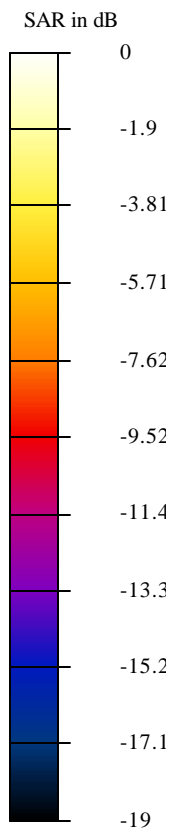

Test Laboratory: Compliance Certification Services  
File Name: 1L-CH\_0.28 mW.da4

**DUT: Symbol Type & Serial Number: ViewPoint Telepack 2.4**  
**Program: EUT Setup Configuration 1; Air temp 25 deg C & Liquid temp 23.5 deg C**

Communication System: FHSS; Frequency: 2402 MHz; Duty Cycle: 1:1  
Medium: Muscle 2450 MHz ( $\sigma = 1.9613$  mho/m,  $\epsilon = 50.45$ ,  $\rho = 1000$  kg/m<sup>3</sup>)  
Phantom section: FlatSection

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(4.7, 4.7, 4.7); Calibrated: 2/7/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 2 - TP:1050
- Software: DASY4, V4.0 Build 51

**Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm



Reference Value = 7.42 V/m

Peak SAR = 0.64 mW/g

SAR(1 g) = 0.28 mW/g; SAR(10 g) = 0.145 mW/g

Power Drift = 0.09 dB

**Area Scan (13x17x1):** Measurement grid: dx=10mm, dy=10mm

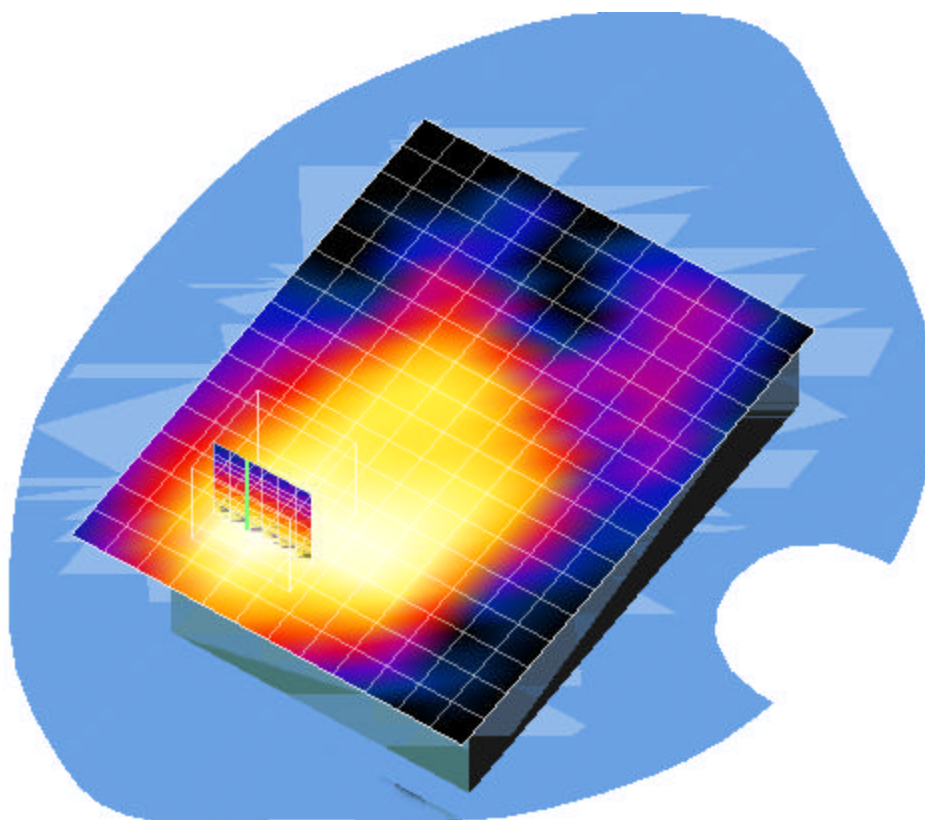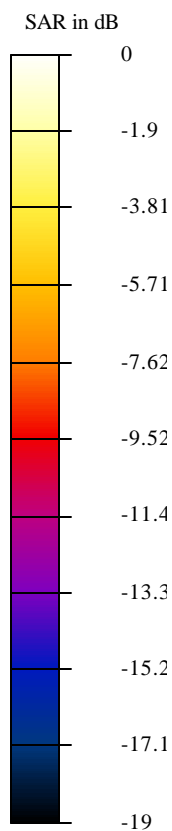

Test Laboratory: Compliance Certification Services

File Name: 2M-CH\_0.239 mW.da4

**DUT: Symbol Type & Serial Number: ViewPoint Telepack 2.4**

**Program: EUT Setup Configuration 1; Air temp 25 deg C & Liquid temp 23.5 deg C**

Communication System: FHSS; Frequency: 2440 MHz; Duty Cycle: 1:1

Medium: Muscle 2450 MHz ( $\sigma = 1.9613$  mho/m,  $\epsilon = 50.45$ ,  $\rho = 1000$  kg/m<sup>3</sup>)

Phantom section: FlatSection

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(4.7, 4.7, 4.7); Calibrated: 2/7/2003

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE3 Sn427; Calibrated: 2/4/2003

- Phantom: SAM 2 - TP:1050

- Software: DASY4, V4.0 Build 51

**Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm



Reference Value = 7.55 V/m

Peak SAR = 0.575 mW/g

SAR(1 g) = 0.239 mW/g; SAR(10 g) = 0.118 mW/g

Power Drift = -0.07 dB

**Area Scan (13x17x1):** Measurement grid: dx=10mm, dy=10mm

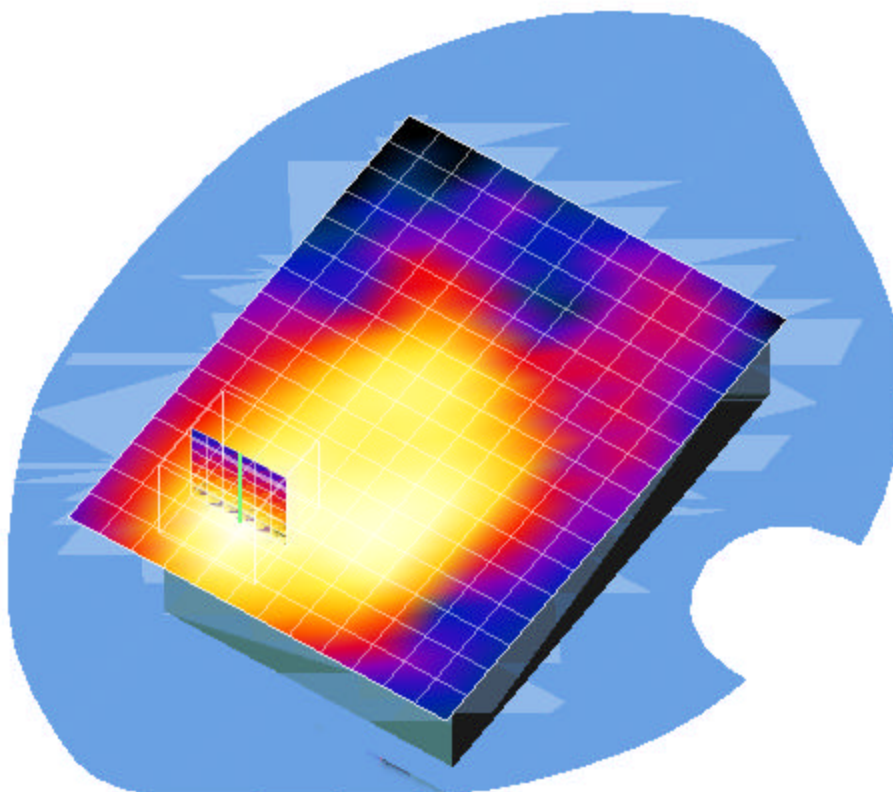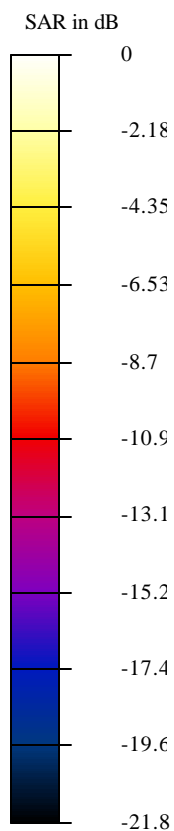

Test Laboratory: Compliance Certification Services

File Name: 2M-CH\_0.189 mW.da4

**DUT: Symbol Type & Serial Number: ViewPoint Telepack 2.4**

**Program: EUT Setup Configuration 1; Air temp 25 deg C & Liquid temp 23.5 deg C**

Communication System: FHSS; Frequency: 2440 MHz; Duty Cycle: 1:1

Medium: Muscle 2450 MHz ( $\sigma = 1.9613$  mho/m,  $\epsilon = 50.45$ ,  $\rho = 1000$  kg/m<sup>3</sup>)

Phantom section: FlatSection

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(4.7, 4.7, 4.7); Calibrated: 2/7/2003

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE3 Sn427; Calibrated: 2/4/2003

- Phantom: SAM 2 - TP:1050

- Software: DASY4, V4.0 Build 51

**Zoom Scan (7x7x7)/Cube 1:** Measurement grid: dx=5mm, dy=5mm



Reference Value = 7.55 V/m

Peak SAR = 0.563 mW/g

SAR(1 g) = 0.189 mW/g; SAR(10 g) = 0.11 mW/g

Power Drift = -0.07 dB

**Area Scan (13x17x1):** Measurement grid: dx=10mm, dy=10mm

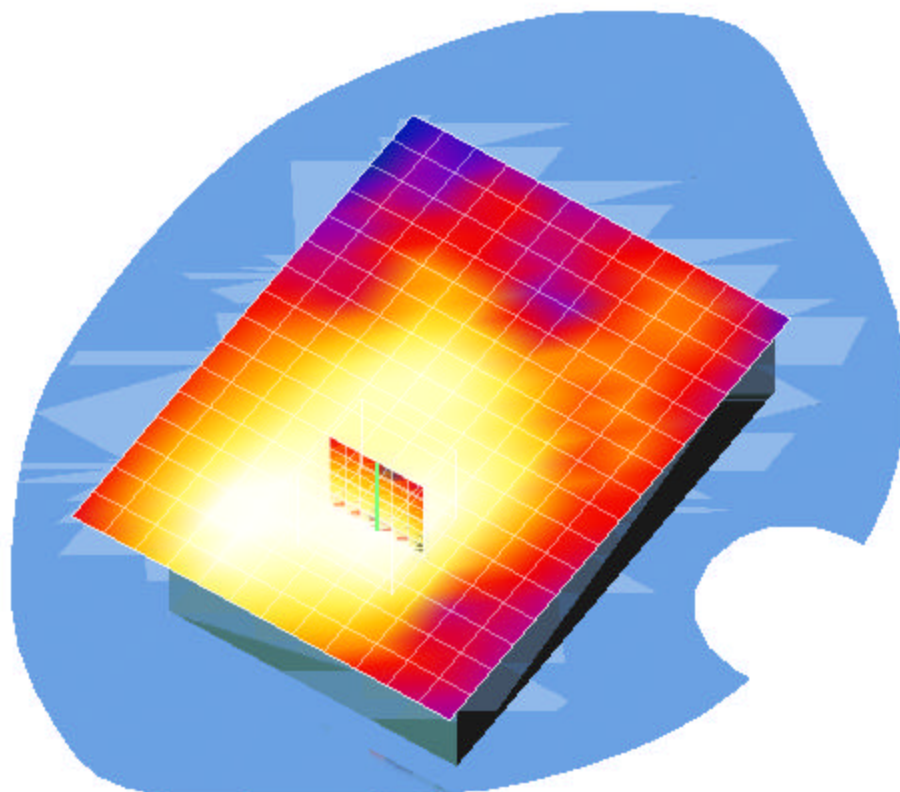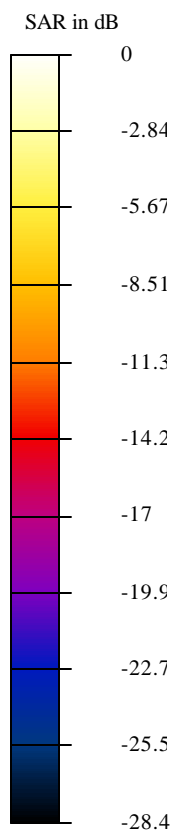

Test Laboratory: Compliance Certification Services  
File Name: 3H-CH\_0.197 mW.da4

**DUT: Symbol Type & Serial Number: ViewPoint Telepack 2.4**  
**Program: EUT Setup Configuration 1; Air temp 25 deg C & Liquid temp 23.5 deg C**

Communication System: FHSS; Frequency: 2480 MHz; Duty Cycle: 1:1  
Medium: Muscle 2450 MHz ( $\sigma = 1.9613$  mho/m,  $\epsilon = 50.45$ ,  $\rho = 1000$  kg/m<sup>3</sup>)  
Phantom section: FlatSection

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(4.7, 4.7, 4.7); Calibrated: 2/7/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 2 - TP:1050
- Software: DASY4, V4.0 Build 51

**Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm


Reference Value = 7.44 V/m

Peak SAR = 0.489 mW/g

SAR(1 g) = 0.197 mW/g; SAR(10 g) = 0.0956 mW/g

Power Drift = -0.12 dB

**Area Scan (13x17x1):** Measurement grid: dx=10mm, dy=10mm

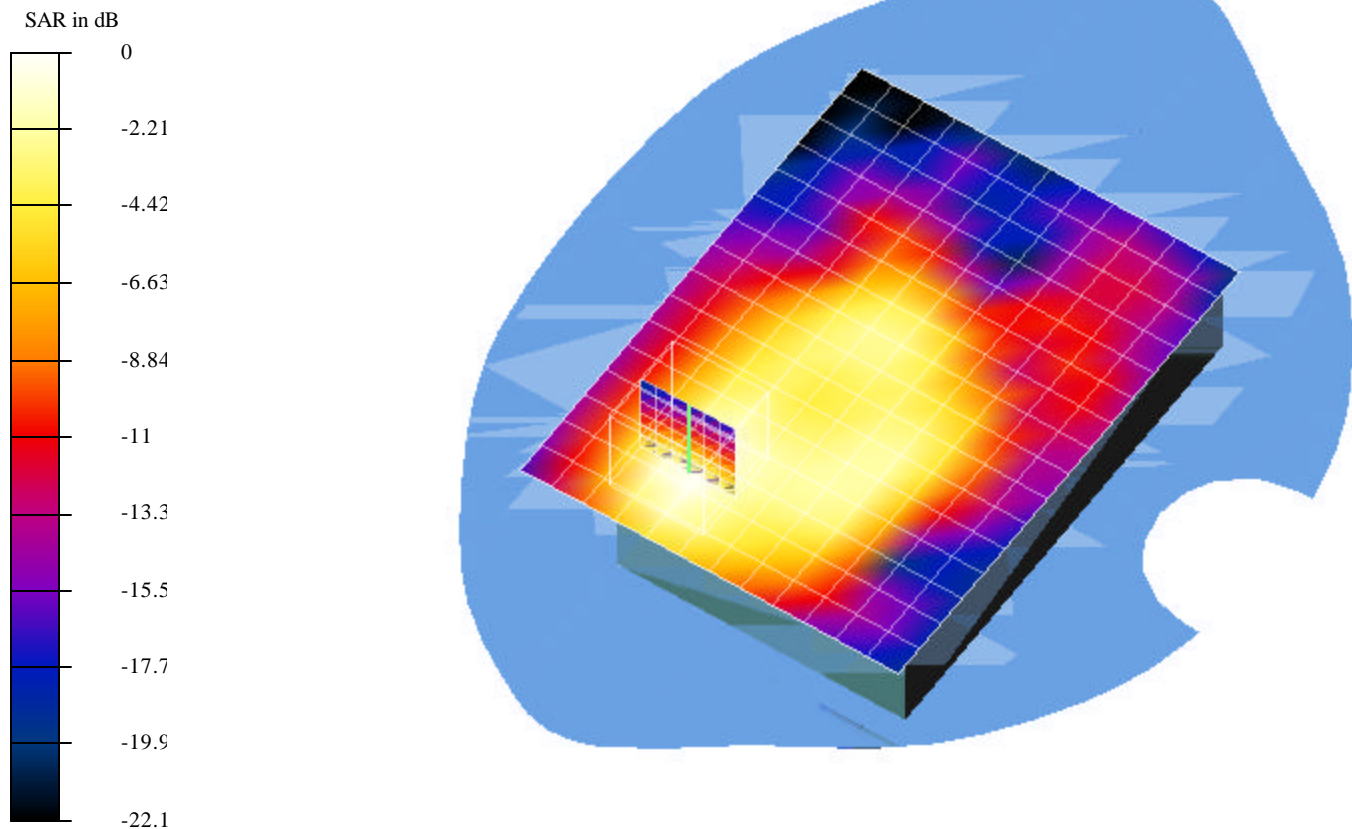

Test Laboratory: Compliance Certification Services

File Name: 3H-CH\_0.118 mW.da4

**DUT: Symbol Type & Serial Number: ViewPoint Telepack 2.4**

**Program: EUT Setup Configuration 1; Air temp 25 deg C & Liquid temp 23.5 deg C**

Communication System: FHSS; Frequency: 2480 MHz; Duty Cycle: 1:1

Medium: Muscle 2450 MHz ( $\sigma = 1.9613$  mho/m,  $\epsilon = 50.45$ ,  $\rho = 1000$  kg/m<sup>3</sup>)

Phantom section: FlatSection

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(4.7, 4.7, 4.7); Calibrated: 2/7/2003

- Sensor-Surface: 4mm (Mechanical Surface Detection)

- Electronics: DAE3 Sn427; Calibrated: 2/4/2003

- Phantom: SAM 2 - TP:1050

- Software: DASY4, V4.0 Build 51

**Zoom Scan (7x7x7)/Cube 1:** Measurement grid: dx=5mm, dy=5mm



Reference Value = 7.44 V/m

Peak SAR = 0.221 mW/g

SAR(1 g) = 0.118 mW/g; SAR(10 g) = 0.0681 mW/g



Power Drift = -0.12 dB

**Area Scan (13x17x1):** Measurement grid: dx=10mm, dy=10mm

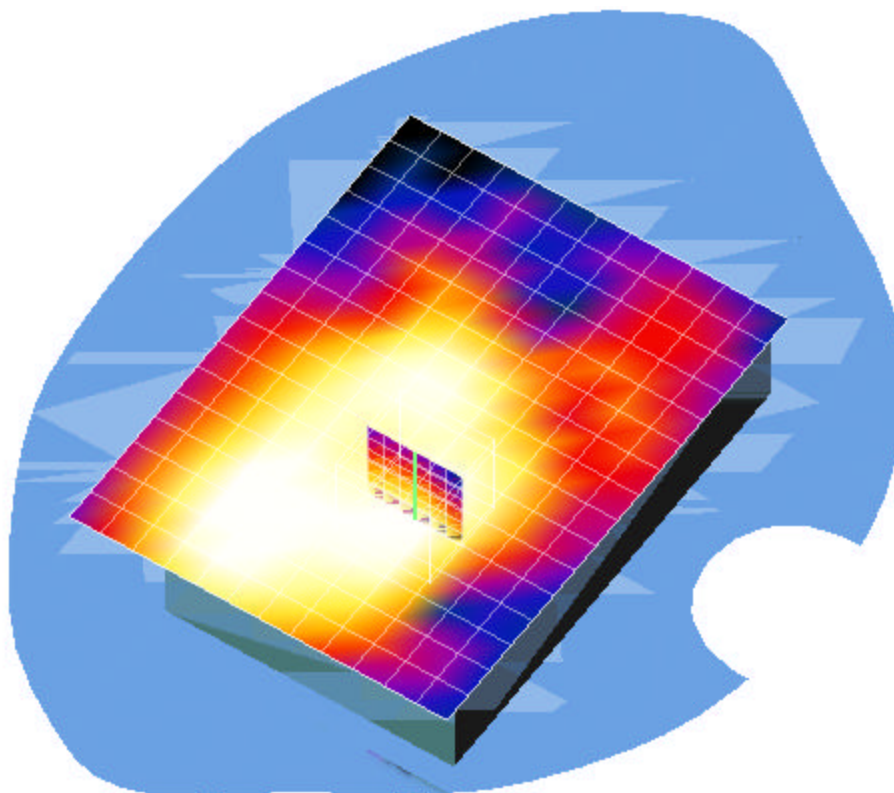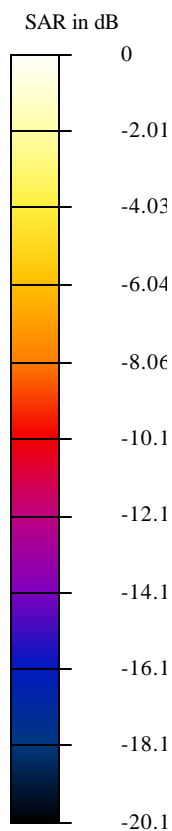

Test Laboratory: Compliance Certification Services  
File Name: 1L-CH\_0.29 mW.da4

### EUT Setup Configuration 2 (Front side)

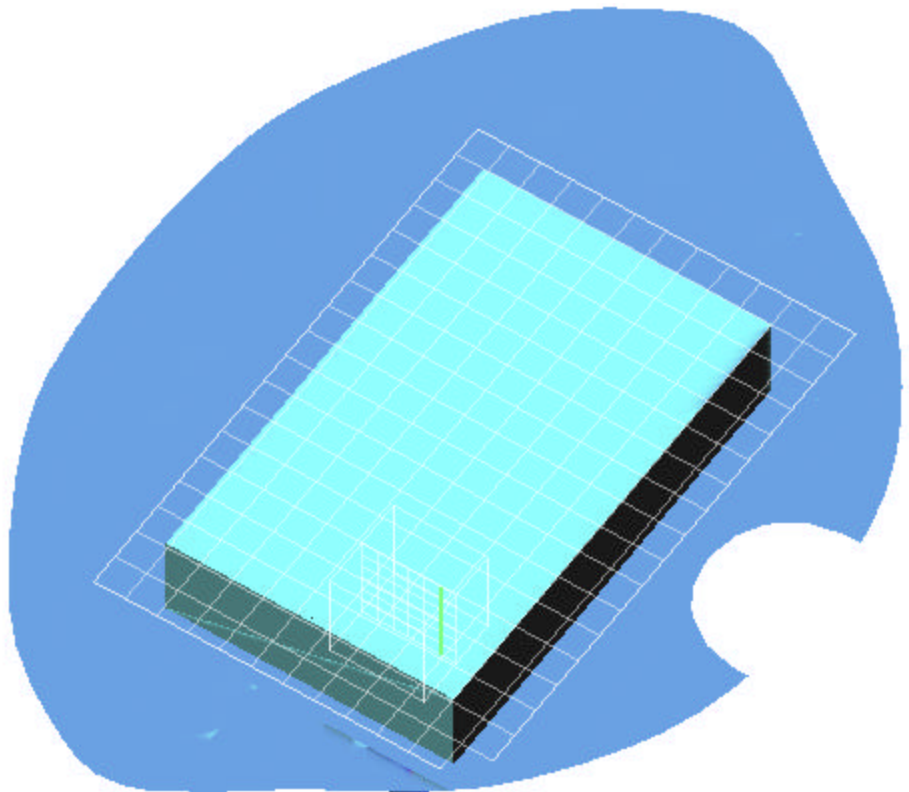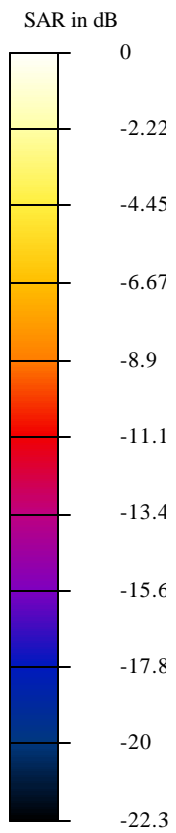

Test Laboratory: Compliance Certification Services  
 File Name: 1L-CH\_0.29 mW.da4

**DUT: Symbol Type & Serial Number: ViewPoint Telepack 2.4**  
**Program: EUT Setup Configuration 2; Air temp 25 deg C & Liquid temp 23.5 deg C**

Communication System: FHSS; Frequency: 2402 MHz; Duty Cycle: 1:1  
 Medium: Muscle 2450 MHz ( $\sigma = 1.9613$  mho/m,  $\epsilon = 50.45$ ,  $\rho = 1000$  kg/m<sup>3</sup>)  
 Phantom section: FlatSection

DASY4 Configuration:

- Probe: ET3DV6 - SN1577; ConvF(4.7, 4.7, 4.7); Calibrated: 2/7/2003
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn427; Calibrated: 2/4/2003
- Phantom: SAM 2 - TP:1050
- Software: DASY4, V4.0 Build 51

**Zoom Scan (7x7x7)/Cube 0:** Measurement grid: dx=5mm, dy=5mm

Reference Value = 3.29 V/m

Peak SAR = 0.721 mW/g

SAR(1 g) = 0.29 mW/g; SAR(10 g) = 0.123 mW/g

Power Drift = -0.09 dB

**Area Scan (13x19x1):** Measurement grid: dx=10mm, dy=10mm

