

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 15670            | 15865           |
| Channel Y | 16434            | 16415           |
| Channel Z | 15919            | 15447           |

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

|           | Average ( $\mu$ V) | min. Offset ( $\mu$ V) | max. Offset ( $\mu$ V) | Std. Deviation ( $\mu$ V) |
|-----------|--------------------|------------------------|------------------------|---------------------------|
| Channel X | 0.19               | -0.98                  | 1.40                   | 0.51                      |
| Channel Y | -0.58              | -2.05                  | 0.62                   | 0.61                      |
| Channel Z | -1.53              | -3.41                  | 0.30                   | 0.56                      |

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

|           | Zeroing (kOhm) | Measuring (MOhm) |
|-----------|----------------|------------------|
| Channel X | 200            | 200              |
| Channel Y | 200            | 200              |
| Channel Z | 200            | 200              |

#### 8. Low Battery Alarm Voltage (Typical values for information)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.9              |
| Supply (- Vcc) | -7.6              |

#### 9. Power Consumption (Typical values for information)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.01             | +6            | +14               |
| Supply (- Vcc) | -0.01             | -8            | -9                |



SCS

Schweizerischer Kalibrierdienst  
Service suisse d'étalonnage  
Servizio svizzero di taratura  
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Client **Sporton-CN (Auden)**

Certificate No: **EX3-3697\_Sep11**

## CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3697**

Calibration procedure(s) **QA CAL-01.v8, QA CAL-14.v3, QA CAL-23.v4, QA CAL-25.v4  
Calibration procedure for dosimetric E-field probes**

Calibration date: **September 2, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID              | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 31-Mar-11 (No. 217-01372)         | Apr-12                 |
| Power sensor E4412A        | MY41498087      | 31-Mar-11 (No. 217-01372)         | Apr-12                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 29-Mar-11 (No. 217-01369)         | Apr-12                 |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 29-Mar-11 (No. 217-01367)         | Apr-12                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 29-Mar-11 (No. 217-01370)         | Apr-12                 |
| Reference Probe ES3DV2     | SN: 3013        | 29-Dec-10 (No. ES3-3013_Dec10)    | Dec-11                 |
| DAE4                       | SN: 654         | 3-May-11 (No. DAE4-654_May11)     | May-12                 |
| Secondary Standards        | ID              | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Oct-09)  | In house check: Oct-11 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-10) | In house check: Oct-11 |

|                                                                                                                 |                              |                                      |                                                                                                    |
|-----------------------------------------------------------------------------------------------------------------|------------------------------|--------------------------------------|----------------------------------------------------------------------------------------------------|
| Calibrated by:                                                                                                  | Name<br><b>Katja Pokovic</b> | Function<br><b>Technical Manager</b> | Signature<br> |
| Approved by:                                                                                                    | Name<br><b>Niels Kuster</b>  | Function<br><b>Quality Manager</b>   | Signature<br> |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory. |                              |                                      | Issued: September 2, 2011                                                                          |



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|                          |                                                                                                                                                         |
|--------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                      | tissue simulating liquid                                                                                                                                |
| NORM <sub>x,y,z</sub>    | sensitivity in free space                                                                                                                               |
| ConvF                    | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                              |
| DCP                      | diode compression point                                                                                                                                 |
| CF                       | crest factor (1/duty_cycle) of the RF signal                                                                                                            |
| A, B, C                  | modulation dependent linearization parameters                                                                                                           |
| Polarization $\varphi$   | $\varphi$ rotation around probe axis                                                                                                                    |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\vartheta = 0$ is normal to probe axis |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

# Probe EX3DV4

## SN:3697

|               |                   |
|---------------|-------------------|
| Manufactured: | April 22, 2009    |
| Calibrated:   | September 2, 2011 |

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3697

### Basic Calibration Parameters

|                                                           | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|-----------------------------------------------------------|----------|----------|----------|-----------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 0.47     | 0.47     | 0.51     | ± 10.1 %  |
| DCP (mV) <sup>B</sup>                                     | 96.1     | 98.5     | 98.1     |           |

### Modulation Calibration Parameters

| UID   | Communication System Name | PAR  |   | A<br>dB | B<br>dB | C<br>dB | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-------|---------------------------|------|---|---------|---------|---------|----------|---------------------------|
| 10000 | CW                        | 0.00 | X | 0.00    | 0.00    | 1.00    | 109.5    | ±2.7 %                    |
|       |                           |      | Y | 0.00    | 0.00    | 1.00    | 113.5    |                           |
|       |                           |      | Z | 0.00    | 0.00    | 1.00    | 114.9    |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the  $E^2$ -field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3697

### Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750                  | 41.9                               | 0.89                            | 8.77    | 8.77    | 8.77    | 0.80  | 0.66       | ± 12.0 %    |
| 835                  | 41.5                               | 0.90                            | 8.45    | 8.45    | 8.45    | 0.78  | 0.66       | ± 12.0 %    |
| 900                  | 41.5                               | 0.97                            | 8.29    | 8.29    | 8.29    | 0.68  | 0.73       | ± 12.0 %    |
| 1450                 | 40.5                               | 1.20                            | 8.38    | 8.38    | 8.38    | 0.61  | 0.74       | ± 12.0 %    |
| 1750                 | 40.1                               | 1.37                            | 7.71    | 7.71    | 7.71    | 0.80  | 0.61       | ± 12.0 %    |
| 1900                 | 40.0                               | 1.40                            | 7.46    | 7.46    | 7.46    | 0.80  | 0.60       | ± 12.0 %    |
| 2000                 | 40.0                               | 1.40                            | 7.87    | 7.87    | 7.87    | 0.55  | 0.72       | ± 12.0 %    |
| 2300                 | 39.5                               | 1.67                            | 7.09    | 7.09    | 7.09    | 0.66  | 0.64       | ± 12.0 %    |
| 2450                 | 39.2                               | 1.80                            | 6.67    | 6.67    | 6.67    | 0.72  | 0.64       | ± 12.0 %    |
| 2600                 | 39.0                               | 1.96                            | 6.55    | 6.55    | 6.55    | 0.66  | 0.68       | ± 12.0 %    |
| 3500                 | 37.9                               | 2.91                            | 6.51    | 6.51    | 6.51    | 0.38  | 1.04       | ± 13.1 %    |
| 5200                 | 36.0                               | 4.66                            | 4.66    | 4.66    | 4.66    | 0.40  | 1.80       | ± 13.1 %    |
| 5500                 | 35.6                               | 4.96                            | 4.32    | 4.32    | 4.32    | 0.45  | 1.80       | ± 13.1 %    |
| 5600                 | 35.5                               | 5.07                            | 4.03    | 4.03    | 4.03    | 0.45  | 1.80       | ± 13.1 %    |
| 5800                 | 35.3                               | 5.27                            | 4.28    | 4.28    | 4.28    | 0.43  | 1.80       | ± 13.1 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## DASY/EASY - Parameters of Probe: EX3DV4- SN:3697

### Calibration Parameter Determined in Body Tissue Simulating Media


| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 750                  | 55.5                               | 0.96                            | 8.79    | 8.79    | 8.79    | 0.80  | 0.72       | ± 12.0 %    |
| 835                  | 55.2                               | 0.97                            | 8.67    | 8.67    | 8.67    | 0.80  | 0.69       | ± 12.0 %    |
| 900                  | 55.0                               | 1.05                            | 8.54    | 8.54    | 8.54    | 0.80  | 0.68       | ± 12.0 %    |
| 1450                 | 54.0                               | 1.30                            | 7.88    | 7.88    | 7.88    | 0.80  | 0.65       | ± 12.0 %    |
| 1750                 | 53.4                               | 1.49                            | 7.16    | 7.16    | 7.16    | 0.80  | 0.66       | ± 12.0 %    |
| 1900                 | 53.3                               | 1.52                            | 6.96    | 6.96    | 6.96    | 0.80  | 0.64       | ± 12.0 %    |
| 2000                 | 53.3                               | 1.52                            | 7.37    | 7.37    | 7.37    | 0.80  | 0.66       | ± 12.0 %    |
| 2300                 | 52.9                               | 1.81                            | 6.96    | 6.96    | 6.96    | 0.80  | 0.65       | ± 12.0 %    |
| 2450                 | 52.7                               | 1.95                            | 6.73    | 6.73    | 6.73    | 0.80  | 0.57       | ± 12.0 %    |
| 2600                 | 52.5                               | 2.16                            | 6.58    | 6.58    | 6.58    | 0.80  | 0.58       | ± 12.0 %    |
| 3500                 | 51.3                               | 3.31                            | 6.06    | 6.06    | 6.06    | 0.36  | 1.23       | ± 13.1 %    |
| 5200                 | 49.0                               | 5.30                            | 4.13    | 4.13    | 4.13    | 0.50  | 1.95       | ± 13.1 %    |
| 5500                 | 48.6                               | 5.65                            | 3.64    | 3.64    | 3.64    | 0.55  | 1.95       | ± 13.1 %    |
| 5600                 | 48.5                               | 5.77                            | 3.51    | 3.51    | 3.51    | 0.57  | 1.95       | ± 13.1 %    |
| 5800                 | 48.2                               | 6.00                            | 3.74    | 3.74    | 3.74    | 0.60  | 1.95       | ± 13.1 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

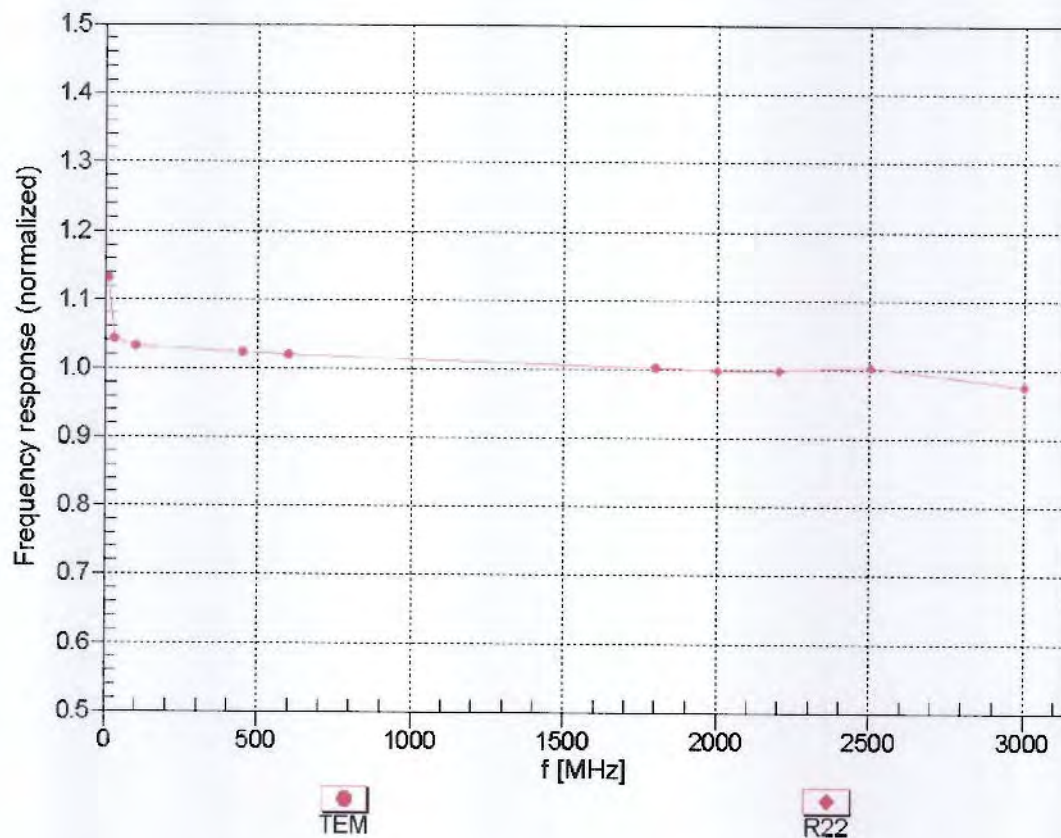



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

## Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

f=600 MHz,TEM


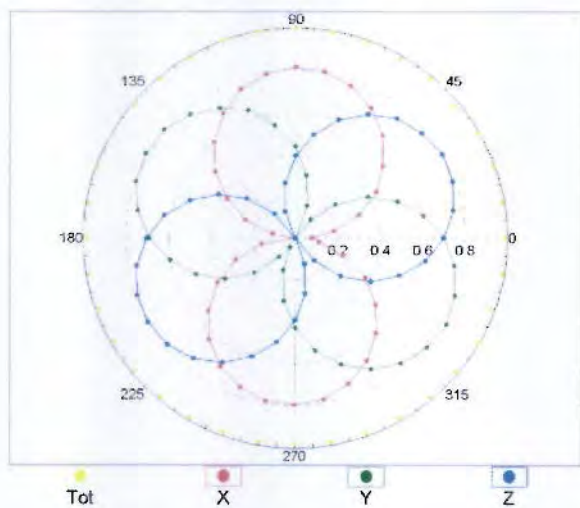


f=1800 MHz,R22

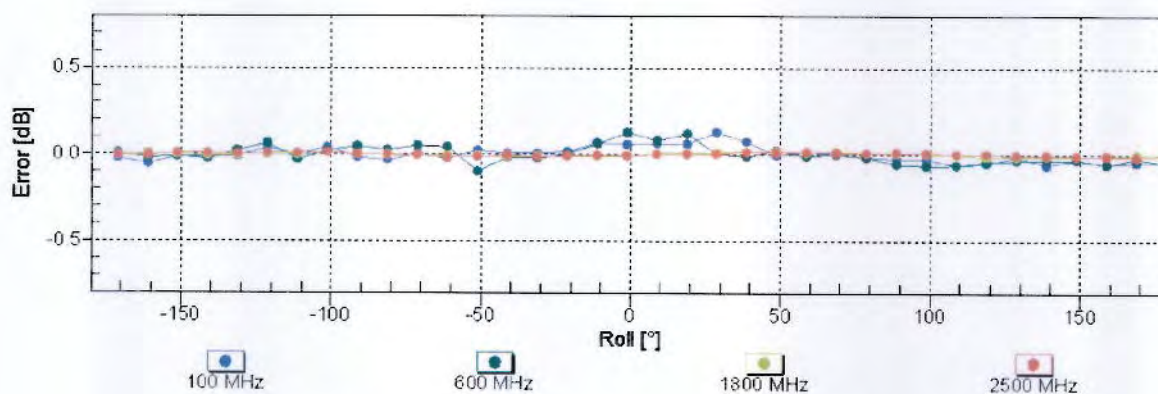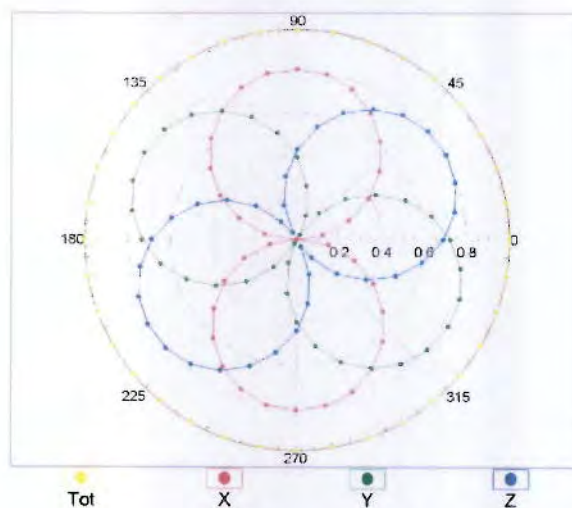


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

## Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell , $f = 900 \text{ MHz}$ )

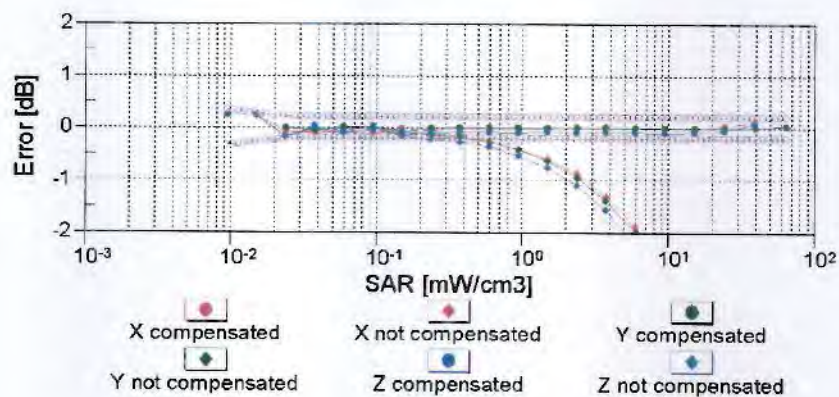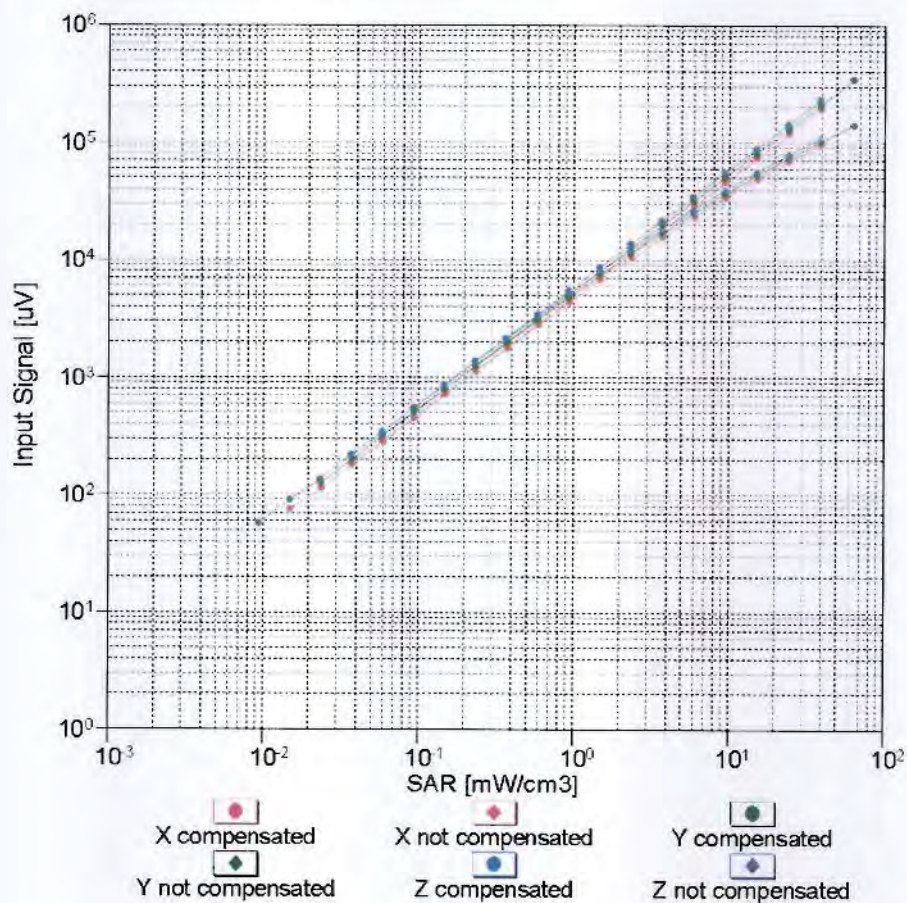



Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

## Conversion Factor Assessment

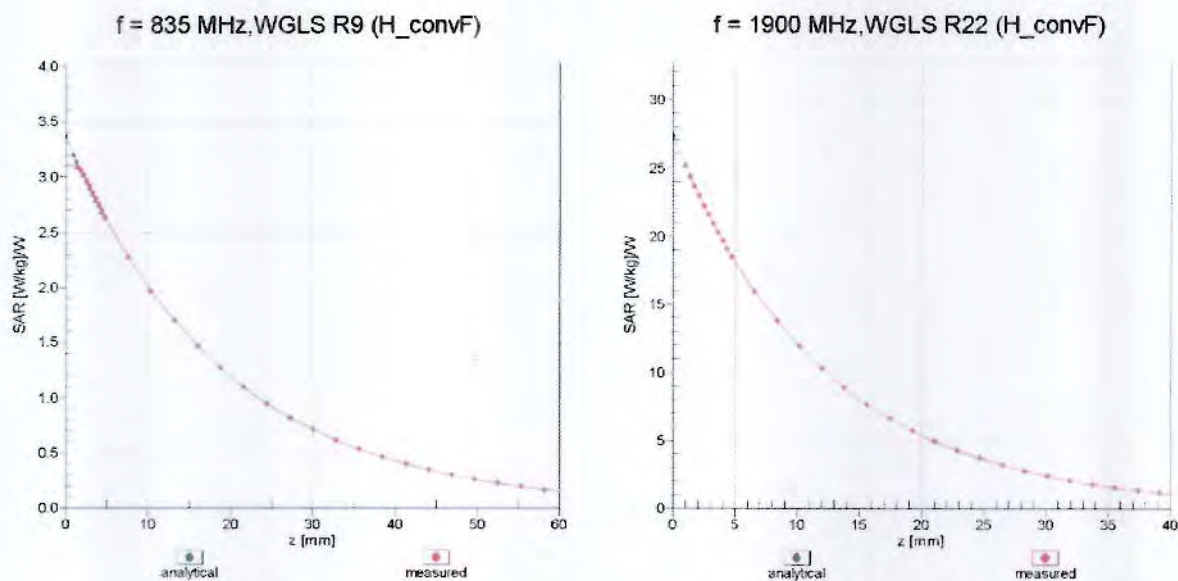

## Deviation from Isotropy in Liquid

Error ( $\phi, \theta$ ),  $f = 900 \text{ MHz}$

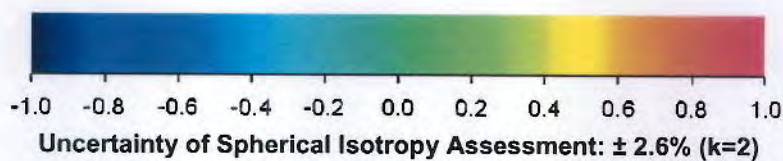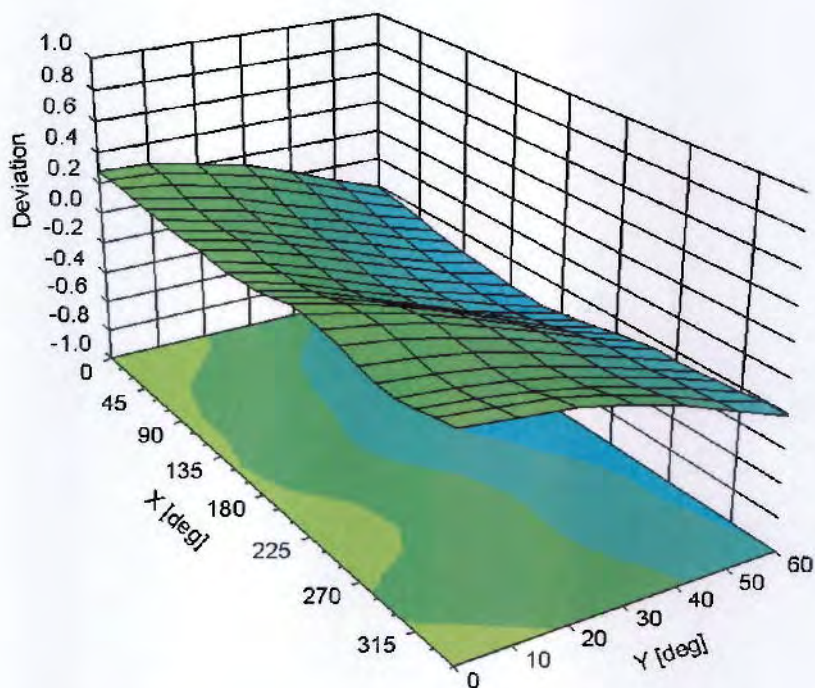

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3697

### Other Probe Parameters

|                                               |                |
|-----------------------------------------------|----------------|
| Sensor Arrangement                            | Triangular     |
| Connector Angle (°)                           | Not applicable |
| Mechanical Surface Detection Mode             | enabled        |
| Optical Surface Detection Mode                | disabled       |
| Probe Overall Length                          | 337 mm         |
| Probe Body Diameter                           | 10 mm          |
| Tip Length                                    | 9 mm           |
| Tip Diameter                                  | 2.5 mm         |
| Probe Tip to Sensor X Calibration Point       | 1 mm           |
| Probe Tip to Sensor Y Calibration Point       | 1 mm           |
| Probe Tip to Sensor Z Calibration Point       | 1 mm           |
| Recommended Measurement Distance from Surface | 2 mm           |



**Calibration Laboratory of**  
**Schmid & Partner**  
**Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Client **Sporton (Auden)**

Certificate No: **EX3-3731\_Sep10**

## CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3731**

Calibration procedure(s) **QA CAL-01.v6, QA CAL-14.v3, QA CAL-23.v3 and QA CAL-25.v2**  
**Calibration procedure for dosimetric E-field probes**

Calibration date: **September 20, 2010**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID #            | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 1-Apr-10 (No. 217-01136)          | Apr-11                 |
| Power sensor E4412A        | MY41495277      | 1-Apr-10 (No. 217-01136)          | Apr-11                 |
| Power sensor E4412A        | MY41498087      | 1-Apr-10 (No. 217-01136)          | Apr-11                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 30-Mar-10 (No. 217-01159)         | Mar-11                 |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 30-Mar-10 (No. 217-01161)         | Mar-11                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 30-Mar-10 (No. 217-01160)         | Mar-11                 |
| Reference Probe ES3DV2     | SN: 3013        | 30-Dec-09 (No. ES3-3013_Dec09)    | Dec-10                 |
| DAE4                       | SN: 660         | 20-Apr-10 (No. DAE4-660_Apr10)    | Apr-11                 |
| Secondary Standards        | ID #            | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Oct-09)  | In house check: Oct-11 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-09) | In house check: Oct-10 |

|                |                              |                                      |               |
|----------------|------------------------------|--------------------------------------|---------------|
| Calibrated by: | Name<br><b>Katja Pokovic</b> | Function<br><b>Technical Manager</b> | Signature<br> |
| Approved by:   | Name<br><b>Fin Bornholt</b>  | Function<br><b>R&amp;D Director</b>  | Signature<br> |

Issued: September 22, 2010

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



**S** Schweizerischer Kalibrierdienst  
**C** Service suisse d'étalonnage  
**S** Servizio svizzero di taratura  
**S** Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

## Glossary:

|                          |                                                                                                                                                         |
|--------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                      | tissue simulating liquid                                                                                                                                |
| NORM <sub>x,y,z</sub>    | sensitivity in free space                                                                                                                               |
| ConvF                    | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                              |
| DCP                      | diode compression point                                                                                                                                 |
| CF                       | crest factor (1/duty_cycle) of the RF signal                                                                                                            |
| A, B, C                  | modulation dependent linearization parameters                                                                                                           |
| Polarization $\varphi$   | $\varphi$ rotation around probe axis                                                                                                                    |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\vartheta = 0$ is normal to probe axis |

## Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

## Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>:** Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not effect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>:** DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; VR<sub>x,y,z</sub>:** A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters:** Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy):** in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset:** The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.



EX3DV4 SN:3731

September 20, 2010

# Probe EX3DV4

## SN:3731

|                  |                    |
|------------------|--------------------|
| Manufactured:    | October 19, 2009   |
| Last calibrated: | July 16, 2010      |
| Repaired:        | September 8, 2010  |
| Recalibrated:    | September 20, 2010 |

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

EX3DV4 SN:3731

September 20, 2010

**DASY/EASY - Parameters of Probe: EX3DV4 SN:3731**
**Basic Calibration Parameters**

|                                                           | Sensor X | Sensor Y | Sensor Z | Unc (k=2)    |
|-----------------------------------------------------------|----------|----------|----------|--------------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 0.51     | 0.53     | 0.56     | $\pm 10.1\%$ |
| DCP (mV) <sup>B</sup>                                     | 87.1     | 87.4     | 87.7     |              |

**Modulation Calibration Parameters**

| UID   | Communication System Name | PAR  |   | A<br>dB | B<br>dBuV | C    | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-------|---------------------------|------|---|---------|-----------|------|----------|---------------------------|
| 10000 | CW                        | 0.00 | X | 0.00    | 0.00      | 1.00 | 300      | $\pm 1.5\%$               |
|       |                           |      | Y | 0.00    | 0.00      | 1.00 | 300      |                           |
|       |                           |      | Z | 0.00    | 0.00      | 1.00 | 300      |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the maximum deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



EX3DV4 SN:3731

September 20, 2010

## DASY/EASY - Parameters of Probe: EX3DV4 SN:3731

### Calibration Parameter Determined in Head Tissue Simulating Media

| f [MHz] | Validity [MHz] <sup>c</sup> | Permittivity | Conductivity | ConvF X | ConvF Y | ConvF Z | Alpha | Depth Unc (k=2) |
|---------|-----------------------------|--------------|--------------|---------|---------|---------|-------|-----------------|
| 835     | ± 50 / ± 100                | 41.5 ± 5%    | 0.90 ± 5%    | 8.85    | 8.85    | 8.85    | 0.60  | 0.69 ± 11.0%    |
| 1900    | ± 50 / ± 100                | 40.0 ± 5%    | 1.40 ± 5%    | 7.46    | 7.46    | 7.46    | 0.75  | 0.60 ± 11.0%    |
| 2300    | ± 50 / ± 100                | 39.5 ± 5%    | 1.67 ± 5%    | 7.16    | 7.16    | 7.16    | 0.47  | 0.71 ± 11.0%    |
| 2600    | ± 50 / ± 100                | 39.0 ± 5%    | 1.96 ± 5%    | 6.88    | 6.88    | 6.88    | 0.31  | 0.95 ± 11.0%    |
| 3500    | ± 50 / ± 100                | 37.9 ± 5%    | 2.91 ± 5%    | 6.60    | 6.60    | 6.60    | 0.20  | 1.50 ± 13.1%    |
| 5200    | ± 50 / ± 100                | 36.0 ± 5%    | 4.66 ± 5%    | 4.83    | 4.83    | 4.83    | 0.35  | 1.90 ± 13.1%    |
| 5300    | ± 50 / ± 100                | 35.9 ± 5%    | 4.76 ± 5%    | 4.46    | 4.46    | 4.46    | 0.38  | 1.90 ± 13.1%    |
| 5500    | ± 50 / ± 100                | 35.6 ± 5%    | 4.96 ± 5%    | 4.46    | 4.46    | 4.46    | 0.42  | 1.90 ± 13.1%    |
| 5600    | ± 50 / ± 100                | 35.5 ± 5%    | 5.07 ± 5%    | 4.07    | 4.07    | 4.07    | 0.48  | 1.90 ± 13.1%    |
| 5800    | ± 50 / ± 100                | 35.3 ± 5%    | 5.27 ± 5%    | 4.22    | 4.22    | 4.22    | 0.50  | 1.90 ± 13.1%    |

<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.



EX3DV4 SN:3731

September 20, 2010

## DASY/EASY - Parameters of Probe: EX3DV4 SN:3731

### Calibration Parameter Determined in Body Tissue Simulating Media

| f [MHz] | Validity [MHz] <sup>c</sup> | Permittivity | Conductivity | ConvF X | ConvF Y | ConvF Z | Alpha | Depth Unc (k=2) |
|---------|-----------------------------|--------------|--------------|---------|---------|---------|-------|-----------------|
| 835     | ± 50 / ± 100                | 55.2 ± 5%    | 0.97 ± 5%    | 8.84    | 8.84    | 8.84    | 0.49  | 0.79 ± 11.0%    |
| 1900    | ± 50 / ± 100                | 53.3 ± 5%    | 1.52 ± 5%    | 7.13    | 7.13    | 7.13    | 0.65  | 0.66 ± 11.0%    |
| 2300    | ± 50 / ± 100                | 52.8 ± 5%    | 1.85 ± 5%    | 7.12    | 7.12    | 7.12    | 0.37  | 0.88 ± 11.0%    |
| 2600    | ± 50 / ± 100                | 52.5 ± 5%    | 2.16 ± 5%    | 6.85    | 6.85    | 6.85    | 0.32  | 0.97 ± 11.0%    |
| 3500    | ± 50 / ± 100                | 51.3 ± 5%    | 3.31 ± 5%    | 6.02    | 6.02    | 6.02    | 0.30  | 1.43 ± 13.1%    |
| 5200    | ± 50 / ± 100                | 49.0 ± 5%    | 5.30 ± 5%    | 3.87    | 3.87    | 3.87    | 0.60  | 1.95 ± 13.1%    |
| 5300    | ± 50 / ± 100                | 48.9 ± 5%    | 5.42 ± 5%    | 3.63    | 3.63    | 3.63    | 0.60  | 1.95 ± 13.1%    |
| 5500    | ± 50 / ± 100                | 48.6 ± 5%    | 5.65 ± 5%    | 3.44    | 3.44    | 3.44    | 0.63  | 1.95 ± 13.1%    |
| 5600    | ± 50 / ± 100                | 48.5 ± 5%    | 5.77 ± 5%    | 3.20    | 3.20    | 3.20    | 0.65  | 1.95 ± 13.1%    |
| 5800    | ± 50 / ± 100                | 48.2 ± 5%    | 6.00 ± 5%    | 3.55    | 3.55    | 3.55    | 0.60  | 1.95 ± 13.1%    |


<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

EX3DV4 SN:3731

September 20, 2010

## Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

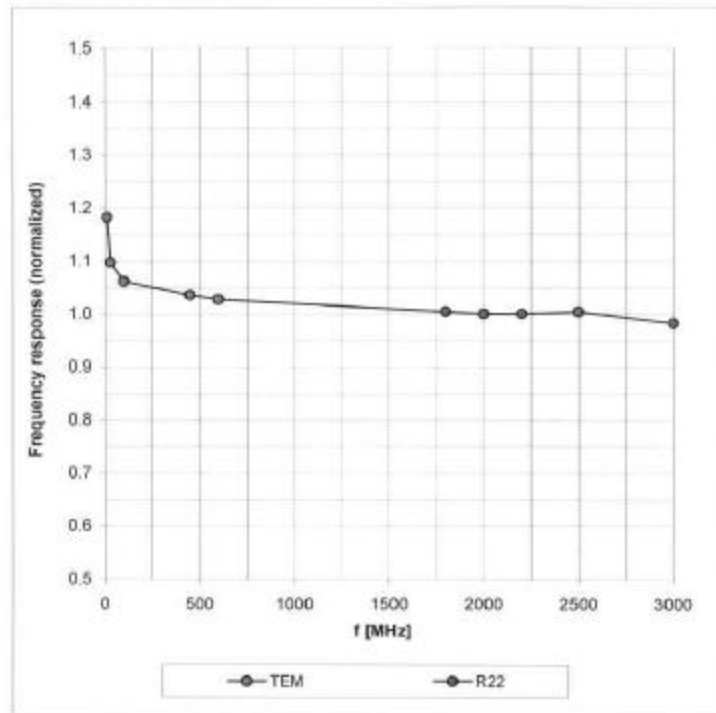


Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

EX3DV4 SN:3731

September 20, 2010

### Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

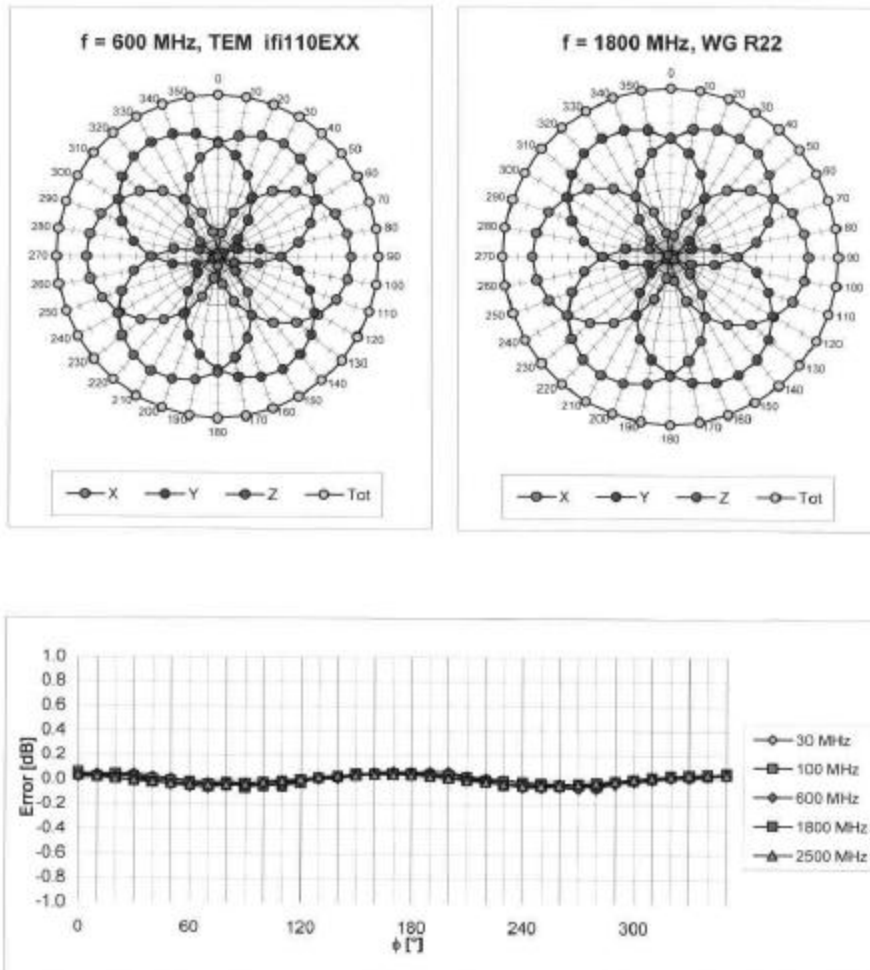


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

EX3DV4 SN:3731

September 20, 2010

### Dynamic Range f(SAR<sub>head</sub>) (Waveguide R22, f = 1800 MHz)

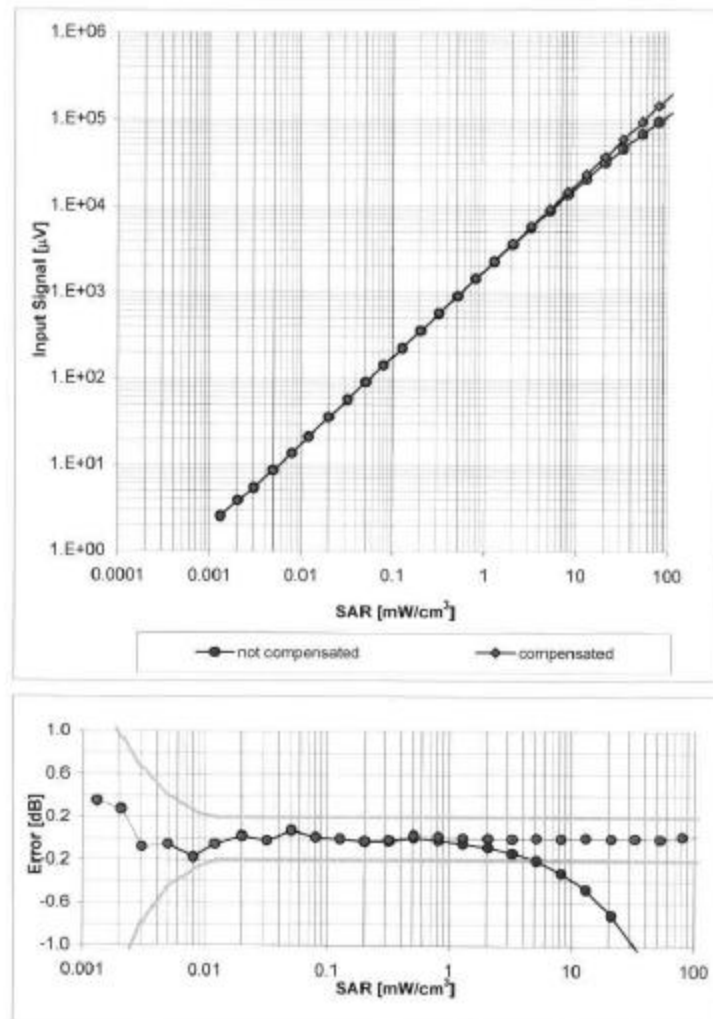


Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

EX3DV4 SN:3731


September 20, 2010

## Conversion Factor Assessment

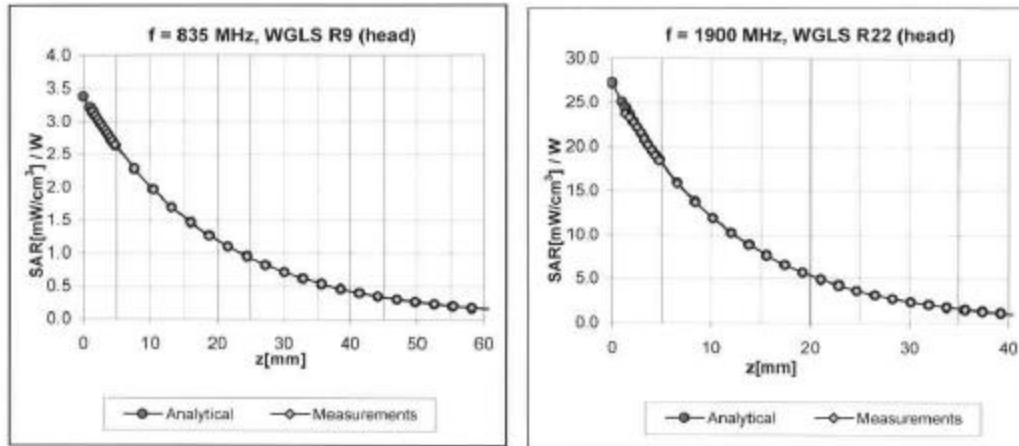

## Deviation from Isotropy in HSL

Error ( $\phi$ ,  $\theta$ ), f = 900 MHz

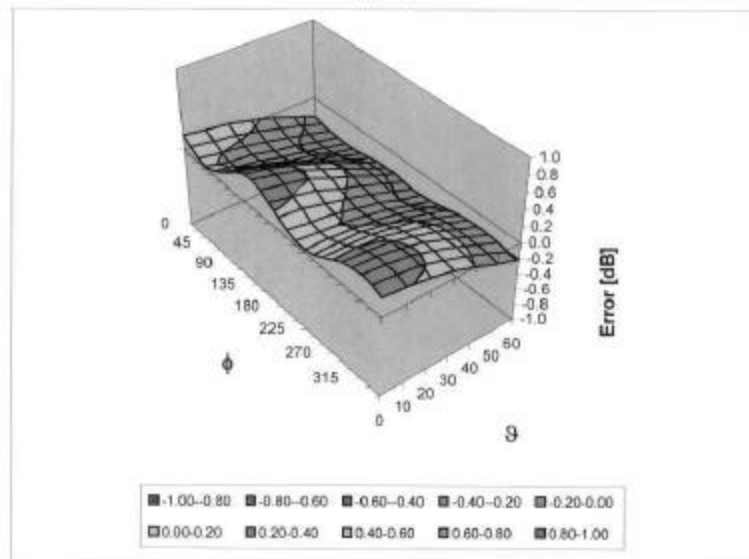

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  (k=2)



EX3DV4 SN:3731

September 20, 2010

### Other Probe Parameters

|                                               |                |
|-----------------------------------------------|----------------|
| Sensor Arrangement                            | Triangular     |
| Connector Angle (°)                           | Not applicable |
| Mechanical Surface Detection Mode             | enabled        |
| Optical Surface Detection Mode                | disabled       |
| Probe Overall Length                          | 337 mm         |
| Probe Body Diameter                           | 10 mm          |
| Tip Length                                    | 9 mm           |
| Tip Diameter                                  | 2.5 mm         |
| Probe Tip to Sensor X Calibration Point       | 1 mm           |
| Probe Tip to Sensor Y Calibration Point       | 1 mm           |
| Probe Tip to Sensor Z Calibration Point       | 1 mm           |
| Recommended Measurement Distance from Surface | 2 mm           |



Accredited by the Swiss Accreditation Service (SAS)  
 The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **TMC Shanghai (Auden)**

Certificate No: **EX3-3754\_Jan11**

## CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3754**

Calibration procedure(s) **GA CAL-01 v7, GA CAL-23 v4 and GA CAL-25 v3  
 Calibration procedure for document E-field probe**

Calibration date: **January 11, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID #            | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 1-Apr-10 (No. 217-01136)          | Apr-11                 |
| Power sensor E4412A        | MY41495277      | 1-Apr-10 (No. 217-01136)          | Apr-11                 |
| Power sensor E4412A        | MY41498087      | 1-Apr-10 (No. 217-01136)          | Apr-11                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 30-Mar-10 (No. 217-01159)         | Mar-11                 |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 30-Mar-10 (No. 217-01161)         | Mar-11                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 30-Mar-10 (No. 217-01160)         | Mar-11                 |
| Reference Probe ES3DV2     | SN: 3013        | 29-Dec-10 (No. ES3-3013_Dec10)    | Dec-11                 |
| DAE4                       | SN: 660         | 20-Apr-10 (No. DAE4-660_Apr10)    | Apr-11                 |
| Secondary Standards        | ID #            | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Oct-09)  | In house check: Oct-11 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-10) | In house check: Oct-11 |

|                |               |                   |                  |
|----------------|---------------|-------------------|------------------|
|                | <b>Name</b>   | <b>Function</b>   | <b>Signature</b> |
| Calibrated by: | Katja Pokovic | Technical Manager |                  |
| Approved by:   | Nils Kuster   | Quality Manager   |                  |

Issued: January 11, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

## Glossary:

|                          |                                                                                                                                                         |
|--------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                      | tissue simulating liquid                                                                                                                                |
| NORM <sub>x,y,z</sub>    | sensitivity in free space                                                                                                                               |
| ConvF                    | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                              |
| DCP                      | diode compression point                                                                                                                                 |
| CF                       | crest factor (1/duty_cycle) of the RF signal                                                                                                            |
| A, B, C                  | modulation dependent linearization parameters                                                                                                           |
| Polarization $\phi$      | $\phi$ rotation around probe axis                                                                                                                       |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\vartheta = 0$ is normal to probe axis |

## Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

## Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not effect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

# Probe EX3DV4

## SN:3754

|               |                  |
|---------------|------------------|
| Manufactured: | March 16, 2010   |
| Calibrated:   | January 11, 2011 |

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

**DASY/EASY - Parameters of Probe: EX3DV4 SN:3754****Basic Calibration Parameters**

|                                                           | Sensor X | Sensor Y | Sensor Z | Unc (k=2) |
|-----------------------------------------------------------|----------|----------|----------|-----------|
| Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup> | 0.44     | 0.49     | 0.50     | ± 10.1%   |
| DCP (mV) <sup>B</sup>                                     | 101.0    | 98.2     | 101.0    |           |

**Modulation Calibration Parameters**

| UID   | Communication System Name | PAR  |   | A<br>dB | B<br>dBuV | C    | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-------|---------------------------|------|---|---------|-----------|------|----------|---------------------------|
| 10000 | CW                        | 0.00 | X | 0.00    | 0.00      | 1.00 | 144.2    | ± 1.9 %                   |
|       |                           |      | Y | 0.00    | 0.00      | 1.00 | 113.1    |                           |
|       |                           |      | Z | 0.00    | 0.00      | 1.00 | 113.3    |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the maximum deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: EX3DV4 SN:3754

### Calibration Parameter Determined in Head Tissue Simulating Media

| f [MHz] | Validity [MHz] <sup>c</sup> | Permittivity | Conductivity | ConvF X | ConvF Y | ConvF Z | Alpha | Depth Unc (k=2) |
|---------|-----------------------------|--------------|--------------|---------|---------|---------|-------|-----------------|
| 835     | ± 50 / ± 100                | 41.5 ± 5%    | 0.90 ± 5%    | 8.71    | 8.71    | 8.71    | 0.48  | 0.77 ± 11.0%    |
| 900     | ± 50 / ± 100                | 41.5 ± 5%    | 0.97 ± 5%    | 8.63    | 8.63    | 8.63    | 0.76  | 0.60 ± 11.0%    |
| 1750    | ± 50 / ± 100                | 40.1 ± 5%    | 1.37 ± 5%    | 7.60    | 7.60    | 7.60    | 0.52  | 0.70 ± 11.0%    |
| 1900    | ± 50 / ± 100                | 40.0 ± 5%    | 1.40 ± 5%    | 7.38    | 7.38    | 7.38    | 0.70  | 0.60 ± 11.0%    |
| 2000    | ± 50 / ± 100                | 40.0 ± 5%    | 1.40 ± 5%    | 7.26    | 7.26    | 7.26    | 0.66  | 0.61 ± 11.0%    |
| 2300    | ± 50 / ± 100                | 39.5 ± 5%    | 1.67 ± 5%    | 7.01    | 7.01    | 7.01    | 0.64  | 0.61 ± 11.0%    |
| 2450    | ± 50 / ± 100                | 39.2 ± 5%    | 1.80 ± 5%    | 6.74    | 6.74    | 6.74    | 0.40  | 0.78 ± 11.0%    |
| 2600    | ± 50 / ± 100                | 39.0 ± 5%    | 1.96 ± 5%    | 6.63    | 6.63    | 6.63    | 0.29  | 1.02 ± 11.0%    |

<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.


**DASY/EASY - Parameters of Probe: EX3DV4 SN:3754****Calibration Parameter Determined in Body Tissue Simulating Media**

| <b>f [MHz]</b> | <b>Validity [MHz]<sup>c</sup></b> | <b>Permittivity</b> | <b>Conductivity</b> | <b>ConvF X</b> | <b>ConvF Y</b> | <b>ConvF Z</b> | <b>Alpha</b> | <b>Depth Unc (k=2)</b> |
|----------------|-----------------------------------|---------------------|---------------------|----------------|----------------|----------------|--------------|------------------------|
| 2300           | ± 50 / ± 100                      | 52.9 ± 5%           | 1.81 ± 5%           | 6.93           | 6.93           | 6.93           | 0.42         | 0.86 ± 11.0%           |
| 2450           | ± 50 / ± 100                      | 52.7 ± 5%           | 1.95 ± 5%           | 6.84           | 6.84           | 6.84           | 0.42         | 0.84 ± 11.0%           |
| 2600           | ± 50 / ± 100                      | 52.5 ± 5%           | 2.16 ± 5%           | 6.76           | 6.76           | 6.76           | 0.33         | 0.97 ± 11.0%           |

<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.



## Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

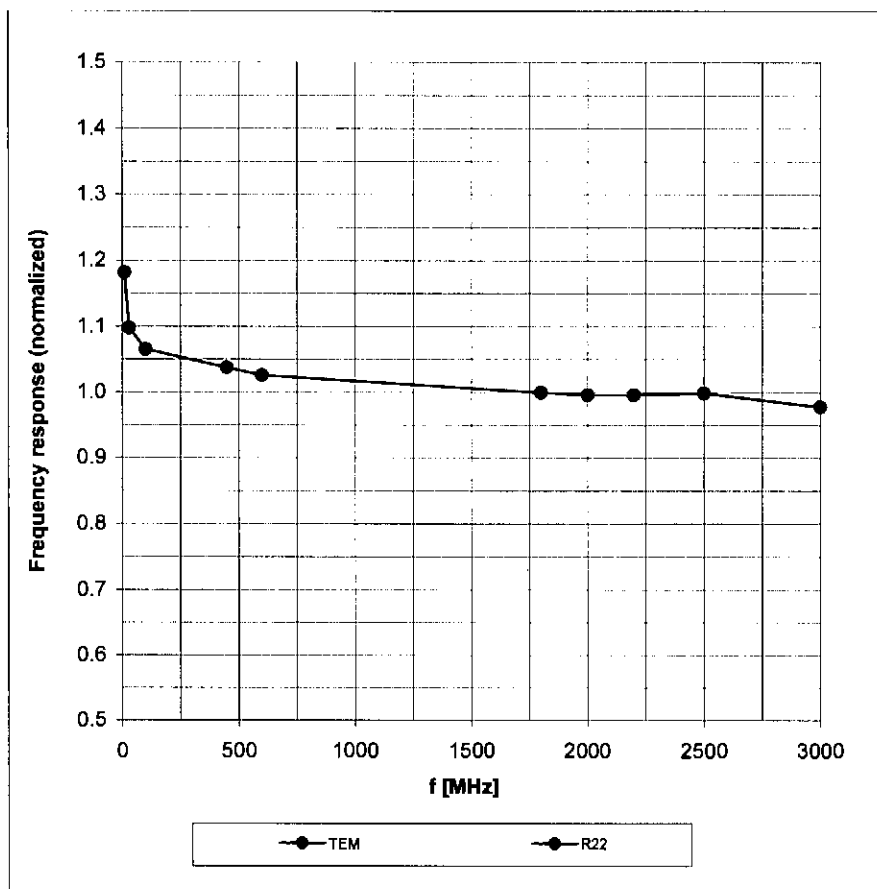



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

## Receiving Pattern ( $\phi$ ), $\vartheta = 0^\circ$

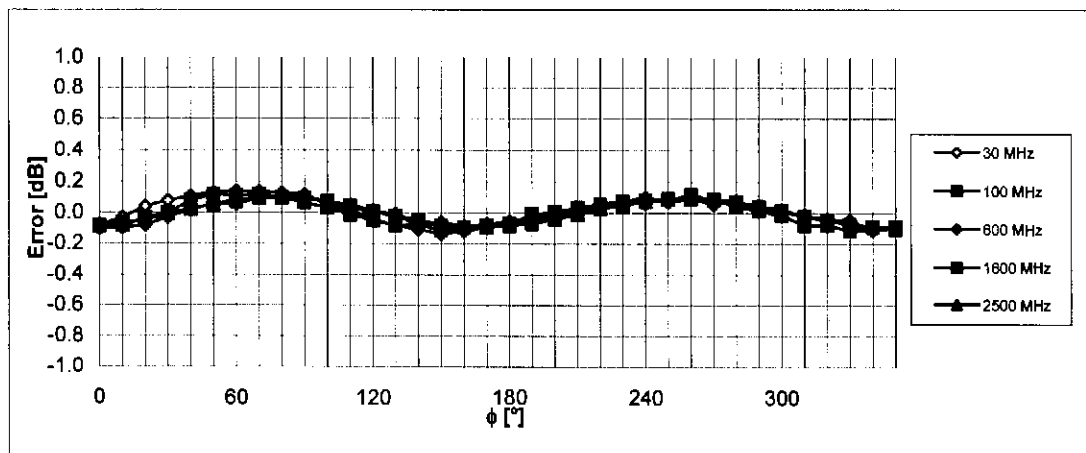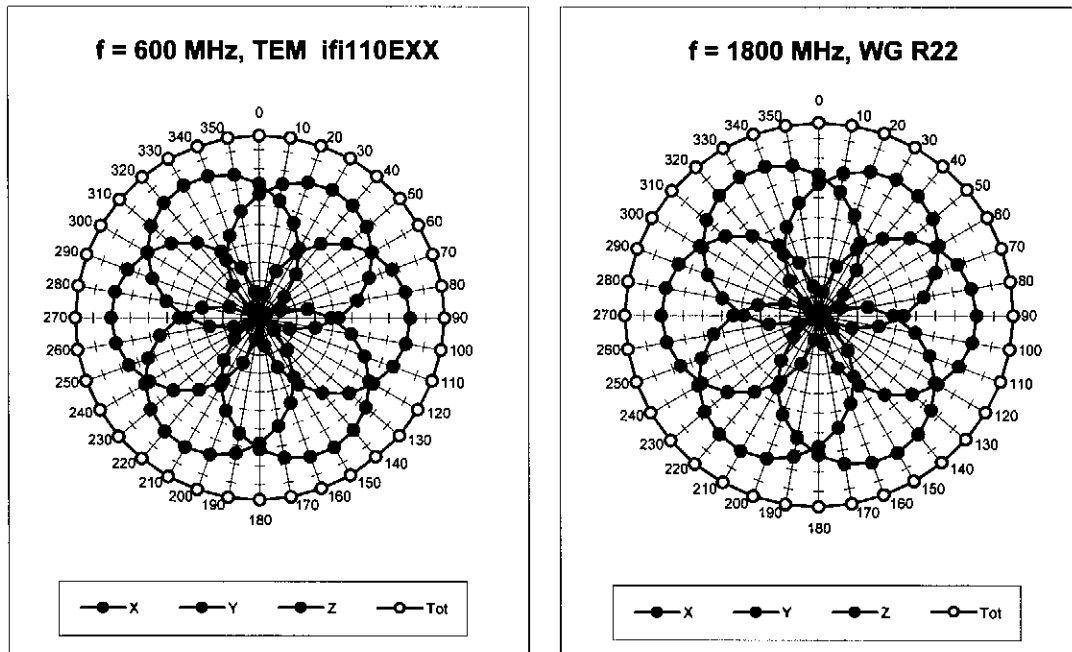



Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

# Dynamic Range f(SAR<sub>head</sub>) (TEM cell, f = 900 MHz)

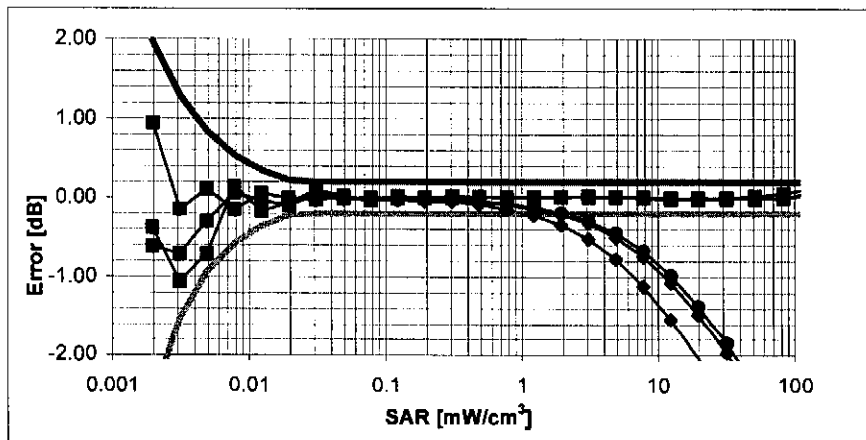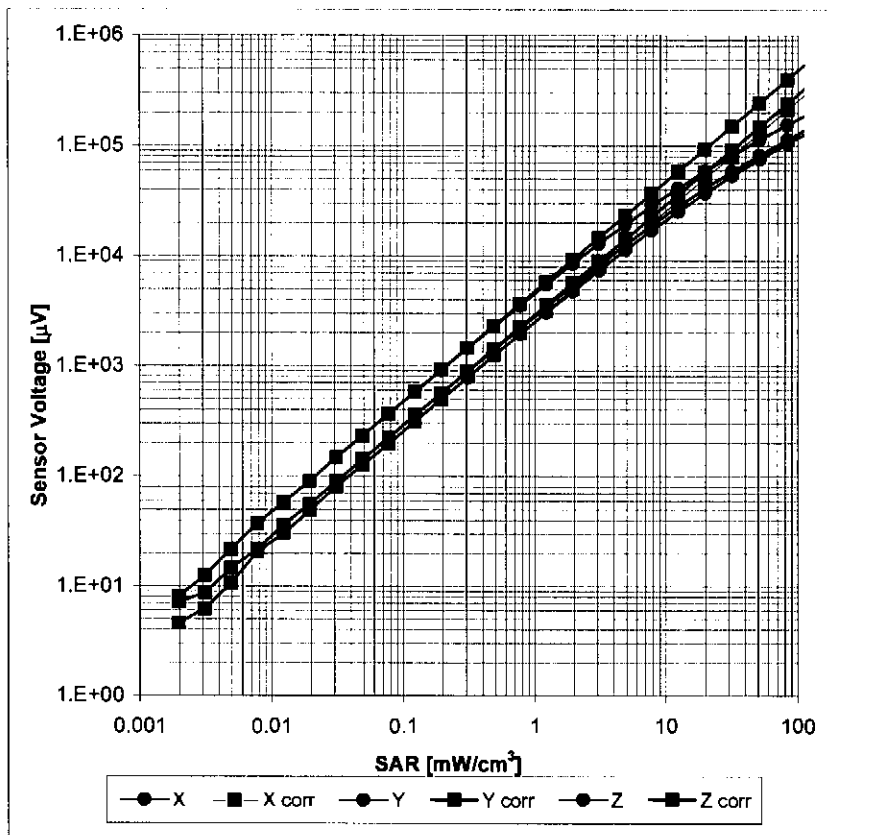


Uncertainty of Linearity Assessment:  $\pm 0.6\%$  (k=2)

## Conversion Factor Assessment

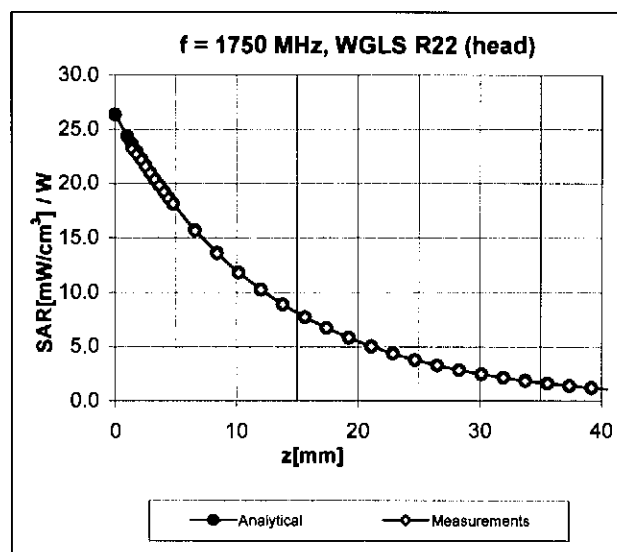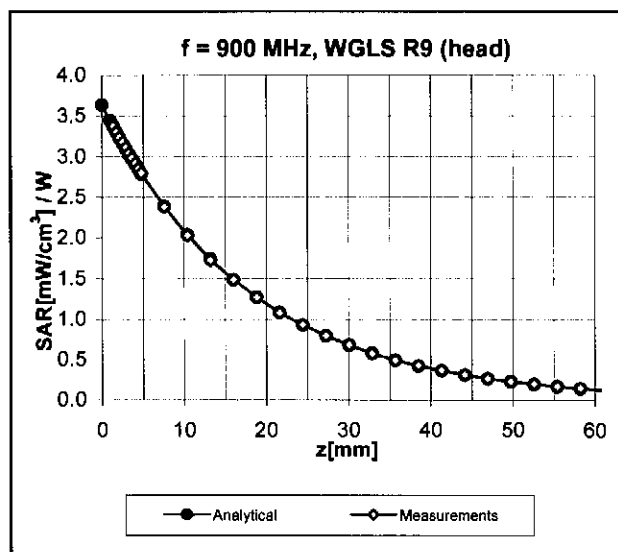

## Deviation from Isotropy in HSL

Error ( $\phi$ ,  $\theta$ ), f = 900 MHz

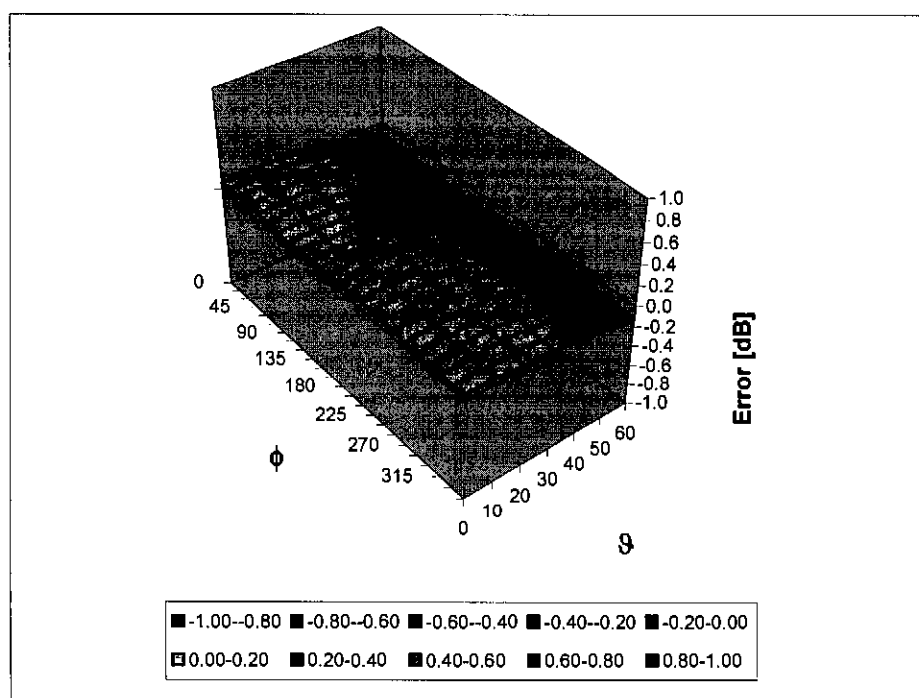

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  (k=2)

## Other Probe Parameters

|                                               |                |
|-----------------------------------------------|----------------|
| Sensor Arrangement                            | Triangular     |
| Connector Angle (°)                           | Not applicable |
| Mechanical Surface Detection Mode             | enabled        |
| Optical Surface Detection Mode                | disabled       |
| Probe Overall Length                          | 337 mm         |
| Probe Body Diameter                           | 10 mm          |
| Tip Length                                    | 9 mm           |
| Tip Diameter                                  | 2.5 mm         |
| Probe Tip to Sensor X Calibration Point       | 1 mm           |
| Probe Tip to Sensor Y Calibration Point       | 1 mm           |
| Probe Tip to Sensor Z Calibration Point       | 1 mm           |
| Recommended Measurement Distance from Surface | 2 mm           |



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

Client **Sporton (Auden)**

Certificate No: **EX3-3792\_Jun11**

## CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3792**

Calibration procedure(s) **QA CAL-01.v8, QA CAL-14.v3, QA CAL-23.v4, QA CAL-25.v4**  
**Calibration procedure for dosimetric E-field probes**

Calibration date: **June 20, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^{\circ}\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID              | Cal Date (Certificate No.)        | Scheduled Calibration  |
|----------------------------|-----------------|-----------------------------------|------------------------|
| Power meter E4419B         | GB41293874      | 31-Mar-11 (No. 217-01372)         | Apr-12                 |
| Power sensor E4412A        | MY41498087      | 31-Mar-11 (No. 217-01372)         | Apr-12                 |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 29-Mar-11 (No. 217-01369)         | Apr-12                 |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 29-Mar-11 (No. 217-01367)         | Apr-12                 |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 29-Mar-11 (No. 217-01370)         | Apr-12                 |
| Reference Probe ES3DV2     | SN: 3013        | 29-Dec-10 (No. ES3-3013_Dec10)    | Dec-11                 |
| DAE4                       | SN: 654         | 3-May-11 (No. DAE4-654_May11)     | May-12                 |
| Secondary Standards        | ID              | Check Date (in house)             | Scheduled Check        |
| RF generator HP 8648C      | US3642U01700    | 4-Aug-99 (in house check Oct-09)  | In house check: Oct-11 |
| Network Analyzer HP 8753E  | US37390585      | 18-Oct-01 (in house check Oct-10) | In house check: Oct-11 |

|                |                       |                               |               |
|----------------|-----------------------|-------------------------------|---------------|
| Calibrated by: | Name<br>Katja Pokovic | Function<br>Technical Manager | Signature<br> |
| Approved by:   | Niels Kuster          | Quality Manager               |               |

Issued: June 21, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA  
 Multilateral Agreement for the recognition of calibration certificates

### Glossary:

|                          |                                                                                                                                                         |
|--------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                      | tissue simulating liquid                                                                                                                                |
| NORM <sub>x,y,z</sub>    | sensitivity in free space                                                                                                                               |
| ConvF                    | sensitivity in TSL / NORM <sub>x,y,z</sub>                                                                                                              |
| DCP                      | diode compression point                                                                                                                                 |
| CF                       | crest factor (1/duty_cycle) of the RF signal                                                                                                            |
| A, B, C                  | modulation dependent linearization parameters                                                                                                           |
| Polarization $\varphi$   | $\varphi$ rotation around probe axis                                                                                                                    |
| Polarization $\vartheta$ | $\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center),<br>i.e., $\vartheta = 0$ is normal to probe axis |

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the  $E^2$ -field uncertainty inside TSL (see below **ConvF**).
- NORM(f)<sub>x,y,z</sub>** = NORM<sub>x,y,z</sub> \* frequency\_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of **ConvF**.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; VR<sub>x,y,z</sub>**: A, B, C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

# Probe EX3DV4

## SN:3792

Manufactured: April 5, 2011  
Calibrated: June 20, 2011

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3792

### Basic Calibration Parameters

|                                                    | Sensor X | Sensor Y | Sensor Z | Unc (k=2)     |
|----------------------------------------------------|----------|----------|----------|---------------|
| Norm ( $\mu\text{V}/(\text{V/m})^2$ ) <sup>A</sup> | 0.64     | 0.54     | 0.54     | $\pm 10.1 \%$ |
| DCP (mV) <sup>B</sup>                              | 97.9     | 98.9     | 99.8     |               |

### Modulation Calibration Parameters

| UID   | Communication System Name | PAR  |   | A<br>dB | B<br>dB | C<br>dB | VR<br>mV | Unc <sup>E</sup><br>(k=2) |
|-------|---------------------------|------|---|---------|---------|---------|----------|---------------------------|
| 10000 | CW                        | 0.00 | X | 0.00    | 0.00    | 1.00    | 134.2    | $\pm 2.7 \%$              |
|       |                           |      | Y | 0.00    | 0.00    | 1.00    | 123.8    |                           |
|       |                           |      | Z | 0.00    | 0.00    | 1.00    | 122.9    |                           |

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the  $E^2$ -field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3792

### Calibration Parameter Determined in Head Tissue Simulating Media

| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 835                  | 41.5                               | 0.90                            | 8.93    | 8.93    | 8.93    | 0.80  | 0.67       | ± 12.0 %    |
| 900                  | 41.5                               | 0.97                            | 8.69    | 8.69    | 8.69    | 0.75  | 0.71       | ± 12.0 %    |
| 1750                 | 40.1                               | 1.37                            | 8.06    | 8.06    | 8.06    | 0.75  | 0.62       | ± 12.0 %    |
| 1900                 | 40.0                               | 1.40                            | 7.76    | 7.76    | 7.76    | 0.76  | 0.60       | ± 12.0 %    |
| 2000                 | 40.0                               | 1.40                            | 7.68    | 7.68    | 7.68    | 0.80  | 0.57       | ± 12.0 %    |
| 2300                 | 39.5                               | 1.67                            | 7.27    | 7.27    | 7.27    | 0.73  | 0.61       | ± 12.0 %    |
| 2450                 | 39.2                               | 1.80                            | 6.92    | 6.92    | 6.92    | 0.70  | 0.62       | ± 12.0 %    |
| 2600                 | 39.0                               | 1.96                            | 6.85    | 6.85    | 6.85    | 0.62  | 0.68       | ± 12.0 %    |
| 3500                 | 37.9                               | 2.91                            | 6.74    | 6.74    | 6.74    | 0.34  | 1.03       | ± 13.1 %    |
| 5200                 | 36.0                               | 4.66                            | 4.95    | 4.95    | 4.95    | 0.35  | 1.80       | ± 13.1 %    |
| 5300                 | 35.9                               | 4.76                            | 4.71    | 4.71    | 4.71    | 0.35  | 1.80       | ± 13.1 %    |
| 5500                 | 35.6                               | 4.96                            | 4.66    | 4.66    | 4.66    | 0.40  | 1.80       | ± 13.1 %    |
| 5600                 | 35.5                               | 5.07                            | 4.23    | 4.23    | 4.23    | 0.45  | 1.80       | ± 13.1 %    |
| 5800                 | 35.3                               | 5.27                            | 4.42    | 4.42    | 4.42    | 0.43  | 1.80       | ± 13.1 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## DASY/EASY - Parameters of Probe: EX3DV4- SN:3792

### Calibration Parameter Determined in Body Tissue Simulating Media


| f (MHz) <sup>C</sup> | Relative Permittivity <sup>F</sup> | Conductivity (S/m) <sup>F</sup> | ConvF X | ConvF Y | ConvF Z | Alpha | Depth (mm) | Unct. (k=2) |
|----------------------|------------------------------------|---------------------------------|---------|---------|---------|-------|------------|-------------|
| 835                  | 55.2                               | 0.97                            | 9.02    | 9.02    | 9.02    | 0.80  | 0.72       | ± 12.0 %    |
| 900                  | 55.0                               | 1.05                            | 8.91    | 8.91    | 8.91    | 0.80  | 0.71       | ± 12.0 %    |
| 1750                 | 53.4                               | 1.49                            | 7.62    | 7.62    | 7.62    | 0.80  | 0.69       | ± 12.0 %    |
| 1900                 | 53.3                               | 1.52                            | 7.17    | 7.17    | 7.17    | 0.80  | 0.64       | ± 12.0 %    |
| 2000                 | 53.3                               | 1.52                            | 7.15    | 7.15    | 7.15    | 0.80  | 0.63       | ± 12.0 %    |
| 2300                 | 52.9                               | 1.81                            | 6.90    | 6.90    | 6.90    | 0.80  | 0.61       | ± 12.0 %    |
| 2450                 | 52.7                               | 1.95                            | 6.67    | 6.67    | 6.67    | 0.80  | 0.59       | ± 12.0 %    |
| 2600                 | 52.5                               | 2.16                            | 6.53    | 6.53    | 6.53    | 0.80  | 0.60       | ± 12.0 %    |
| 3500                 | 51.3                               | 3.31                            | 6.08    | 6.08    | 6.08    | 0.29  | 1.48       | ± 13.1 %    |
| 5200                 | 49.0                               | 5.30                            | 4.22    | 4.22    | 4.22    | 0.50  | 1.90       | ± 13.1 %    |
| 5300                 | 48.9                               | 5.42                            | 3.93    | 3.93    | 3.93    | 0.55  | 1.90       | ± 13.1 %    |
| 5500                 | 48.6                               | 5.65                            | 3.76    | 3.76    | 3.76    | 0.55  | 1.90       | ± 13.1 %    |
| 5600                 | 48.5                               | 5.77                            | 3.53    | 3.53    | 3.53    | 0.60  | 1.90       | ± 13.1 %    |
| 5800                 | 48.2                               | 6.00                            | 3.78    | 3.78    | 3.78    | 0.60  | 1.90       | ± 13.1 %    |

<sup>C</sup> Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

## Frequency Response of E-Field


(TEM-Cell: ifi110 EXX, Waveguide: R22)

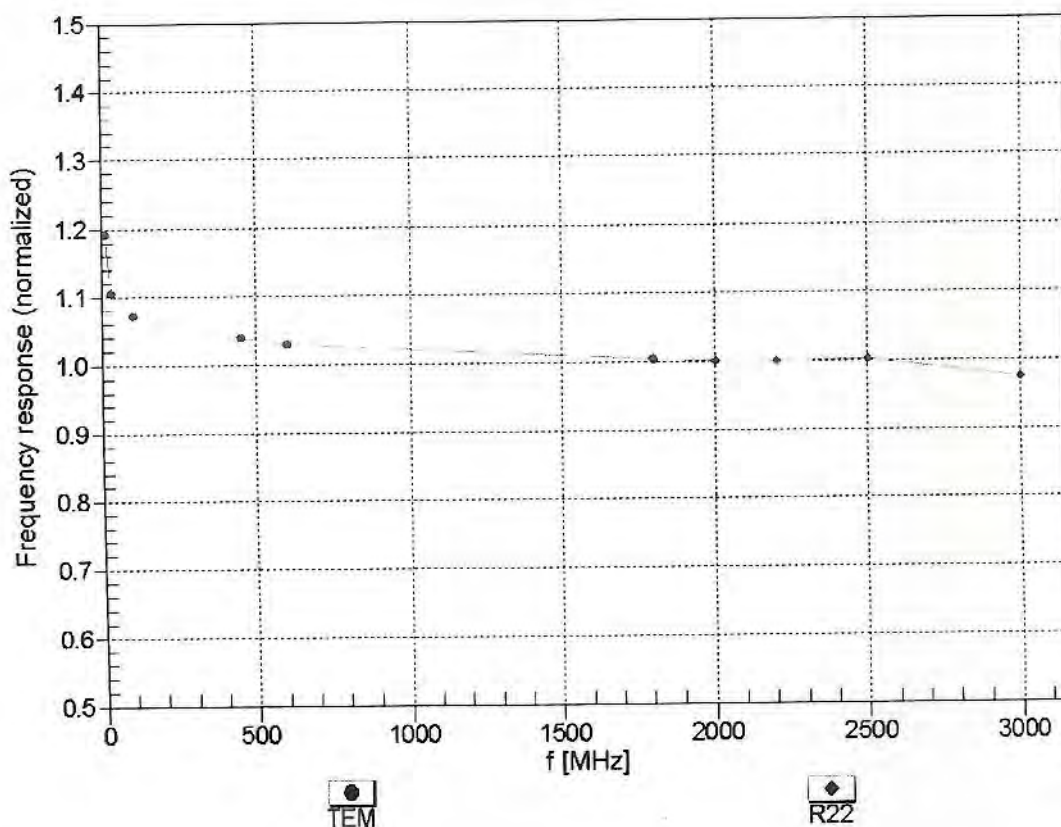



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

## Receiving Pattern ( $\phi$ ), $\vartheta = 0^\circ$

f=600 MHz,TEM


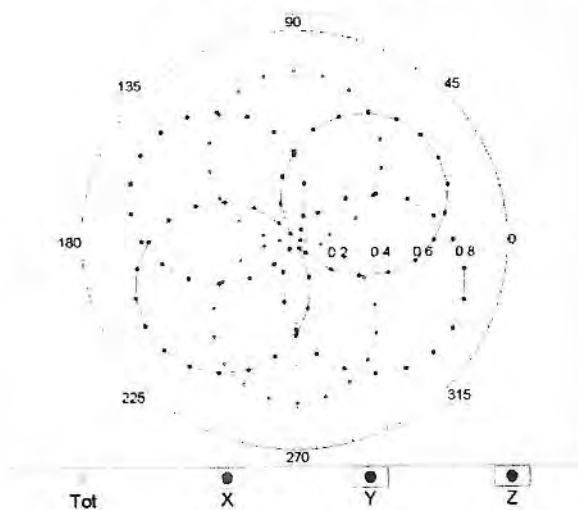


f=1800 MHz,R22

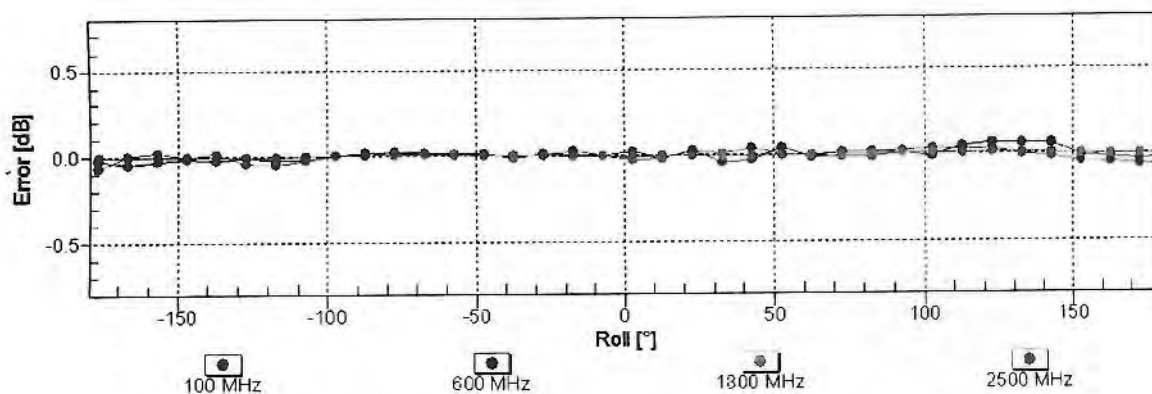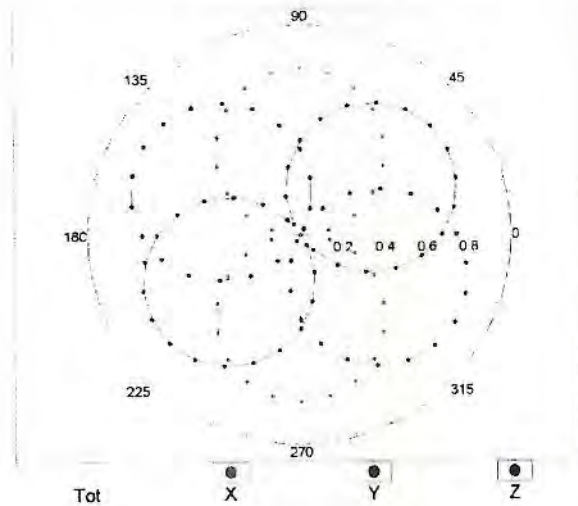


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )

# **Dynamic Range f(SAR<sub>head</sub>)** (TEM cell , f = 900 MHz)

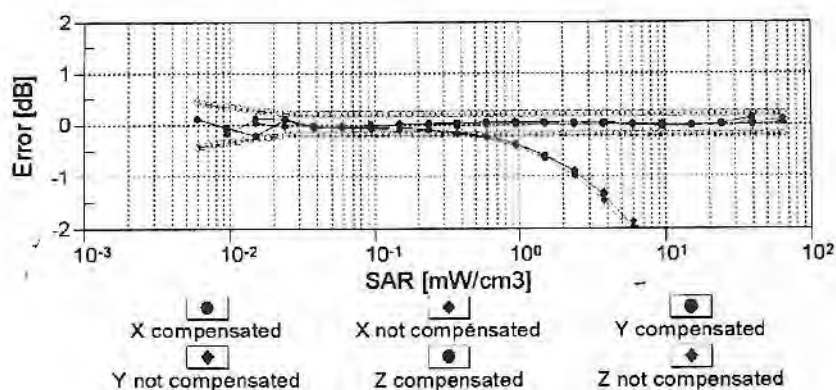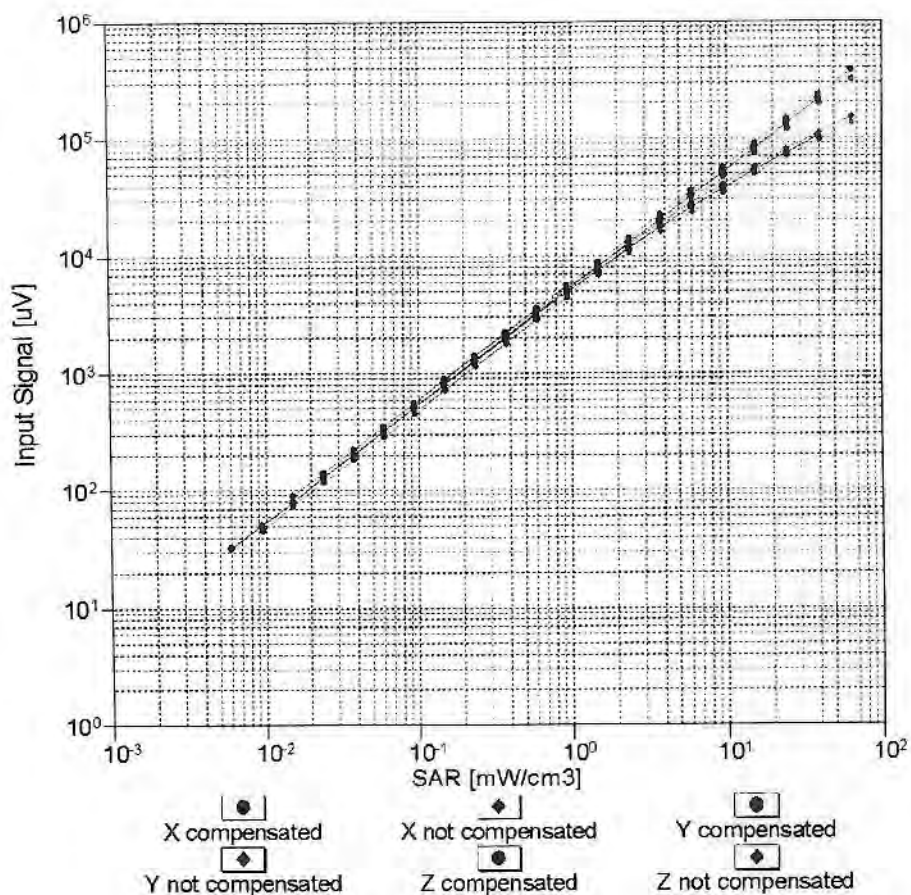



**Uncertainty of Linearity Assessment: ± 0.6% (k=2)**

## Conversion Factor Assessment

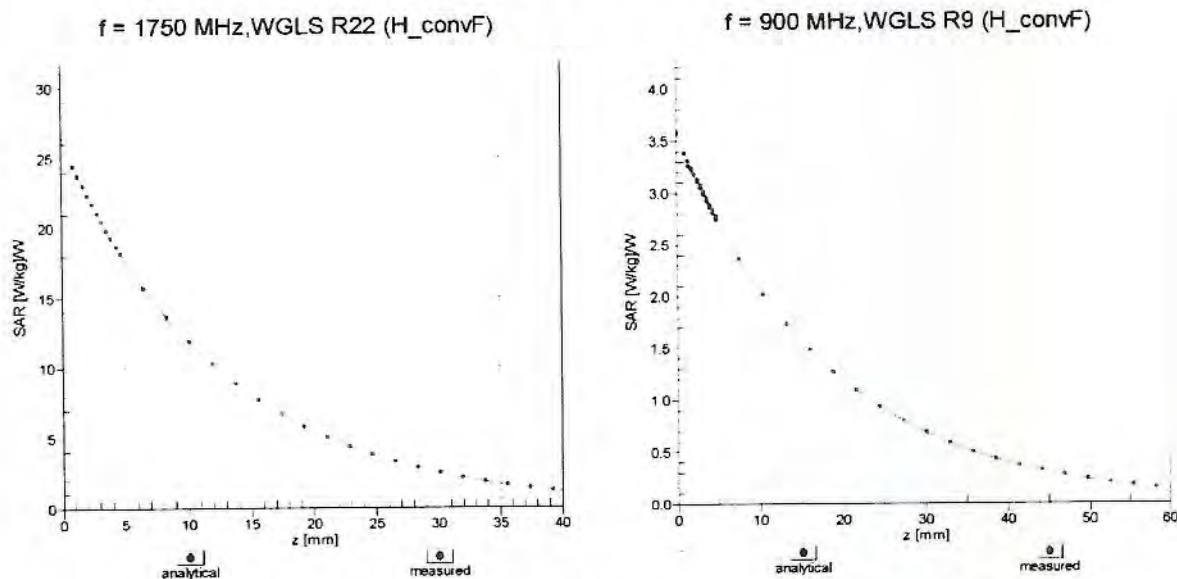

## Deviation from Isotropy in Liquid

Error ( $\phi, \theta$ ),  $f = 900 \text{ MHz}$

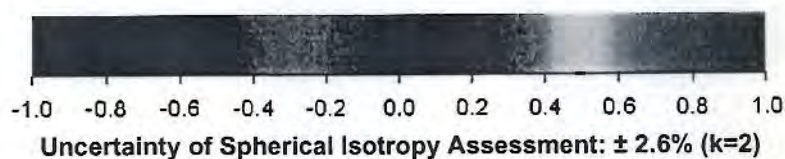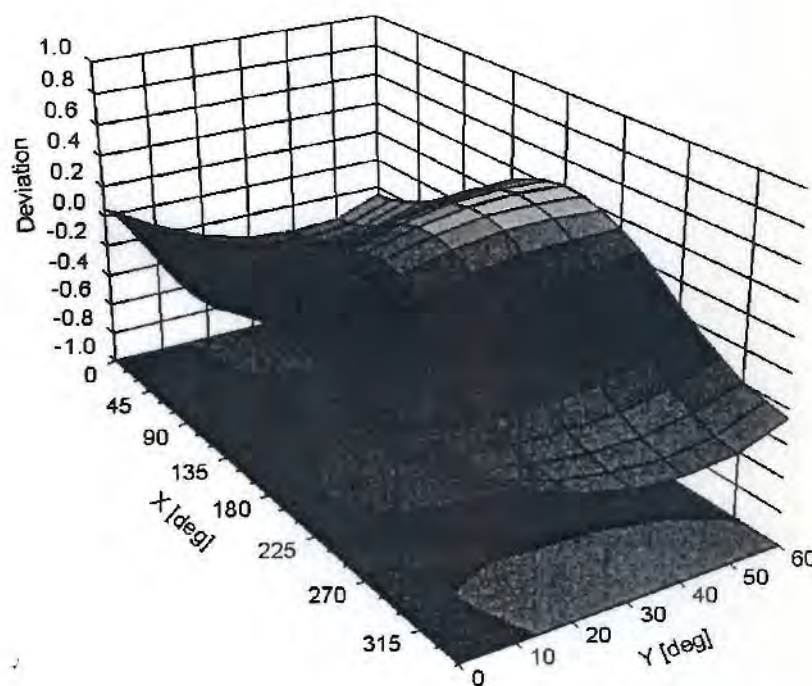

**DASY/EASY - Parameters of Probe: EX3DV4 - SN:3792****Other Probe Parameters**

|                                               |                |
|-----------------------------------------------|----------------|
| Sensor Arrangement                            | Triangular     |
| Connector Angle (°)                           | Not applicable |
| Mechanical Surface Detection Mode             | enabled        |
| Optical Surface Detection Mode                | disabled       |
| Probe Overall Length                          | 337 mm         |
| Probe Body Diameter                           | 10 mm          |
| Tip Length                                    | 9 mm           |
| Tip Diameter                                  | 2.5 mm         |
| Probe Tip to Sensor X Calibration Point       | 1 mm           |
| Probe Tip to Sensor Y Calibration Point       | 1 mm           |
| Probe Tip to Sensor Z Calibration Point       | 1 mm           |
| Recommended Measurement Distance from Surface | 2 mm           |