

System Check_Head_2450MHz

DUT: D2450V2 - SN929

Communication System: CW; Frequency: 2450.000 MHz; Duty Cycle: 1:1

Medium: HSL_2450_240227 Medium parameters used: $f = 2450.000$ MHz; $\sigma = 1.76$ S/m; $\epsilon_r = 38.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(7.12, 7.44, 7.23); Calibrated: 2023-05-24

- Sensor-Surface: 1.4 mm

- Electronics: DAE3 Sn577; Calibrated: 2023-09-14

- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2153; Section: Flat

- Measurement Software: 16.2.4.2524

- UID: CW

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.70 W/kg; SAR (10g) = 2.20 W/kg;


Pin=20.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.10 dB

SAR (1g) = 5.67 W/kg; SAR (8g) = 2.96 W/kg; SAR (10g) = 2.68 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 80.9 %

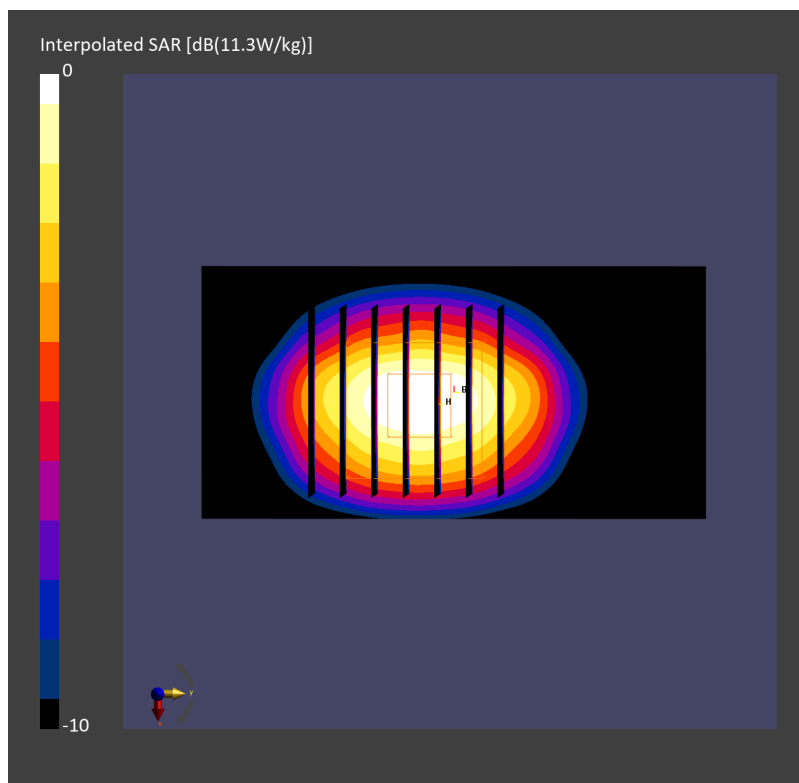

System Check_Head_5250MHz

DUT: D5GHzV2 - SN1171


Communication System: CW; Frequency: 5250.000 MHz; Duty Cycle: 1:1
Medium: HSL_5G_240226 Medium parameters used: $f= 5250.000$ MHz; $\sigma= 4.61$ S/m; $\epsilon_r = 35.4$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(5.45, 5.73, 5.49); Calibrated: 2023-05-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2023-09-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2153; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 6.10 W/kg; SAR (10g) = 1.88 W/kg;

Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = -0.04 dB
SAR (1g) = 7.33 W/kg; SAR (8g) = 2.64 W/kg; SAR (10g) = 2.28 W/kg
Smallest distance from peaks to all points 3 dB below = 7.4 mm
Ratio of SAR at M2 to SAR at M1 = 63.8 %

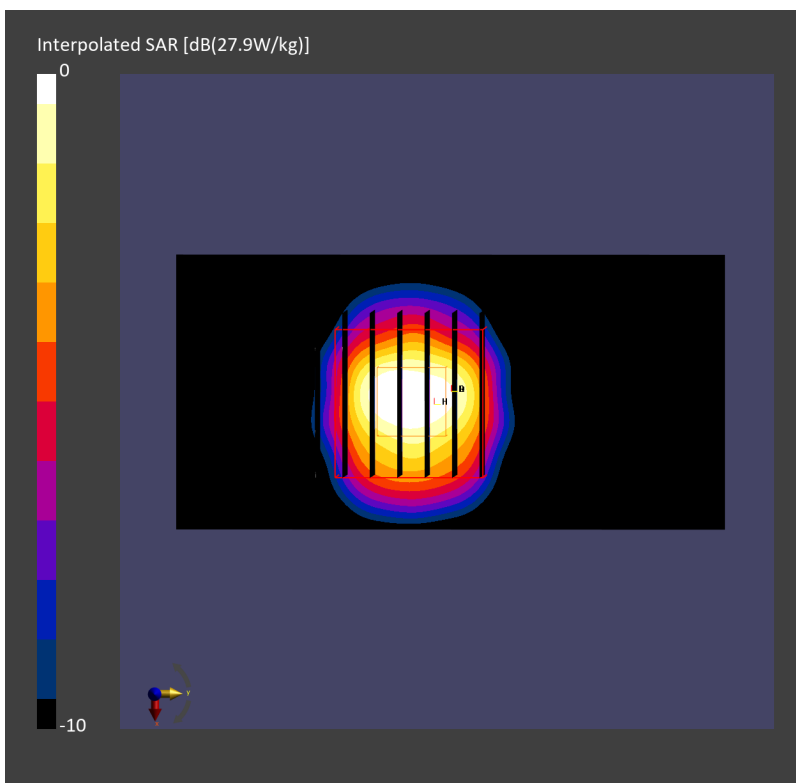

System Check_Head_5600MHz

DUT: D5GHzV2 - SN1171


Communication System: CW; Frequency: 5600.000 MHz; Duty Cycle: 1:1
Medium: HSL_5G_240226 Medium parameters used: $f= 5600.000$ MHz; $\sigma= 5.01$ S/m; $\epsilon_r = 34.8$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(4.75, 4.99, 4.76); Calibrated: 2023-05-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2023-09-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2153; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 6.48 W/kg; SAR (10g) = 1.94 W/kg;

Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = -0.10 dB
SAR (1g) = 7.67 W/kg; SAR (8g) = 2.66 W/kg; SAR (10g) = 2.29 W/kg
Smallest distance from peaks to all points 3 dB below = 7.9 mm
Ratio of SAR at M2 to SAR at M1 = 60.6 %

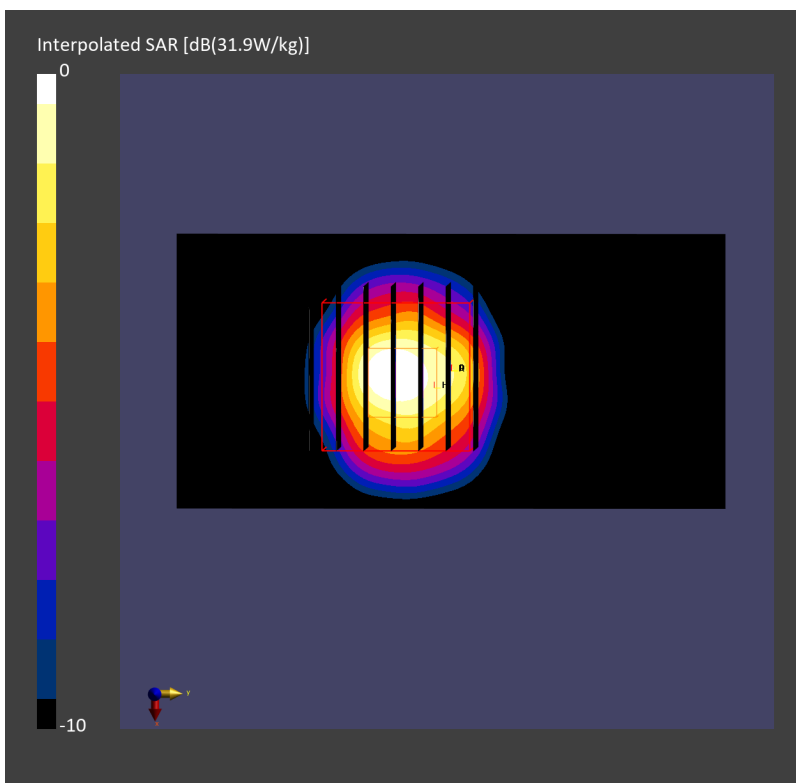

System Check_Head_5750MHz

DUT: D5GHzV2 - SN1171


Communication System: CW; Frequency: 5750.000 MHz; Duty Cycle: 1:1
Medium: HSL_5G_240226 Medium parameters used: $f= 5750.000$ MHz; $\sigma= 5.19$ S/m; $\epsilon_r = 34.5$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(4.96, 5.2, 5.0); Calibrated: 2023-05-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2023-09-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2153; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=20.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 6.09 W/kg; SAR (10g) = 1.86 W/kg;

Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = -0.07 dB
SAR (1g) = 7.35 W/kg; SAR (8g) = 2.52 W/kg; SAR (10g) = 2.28 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 59.4 %

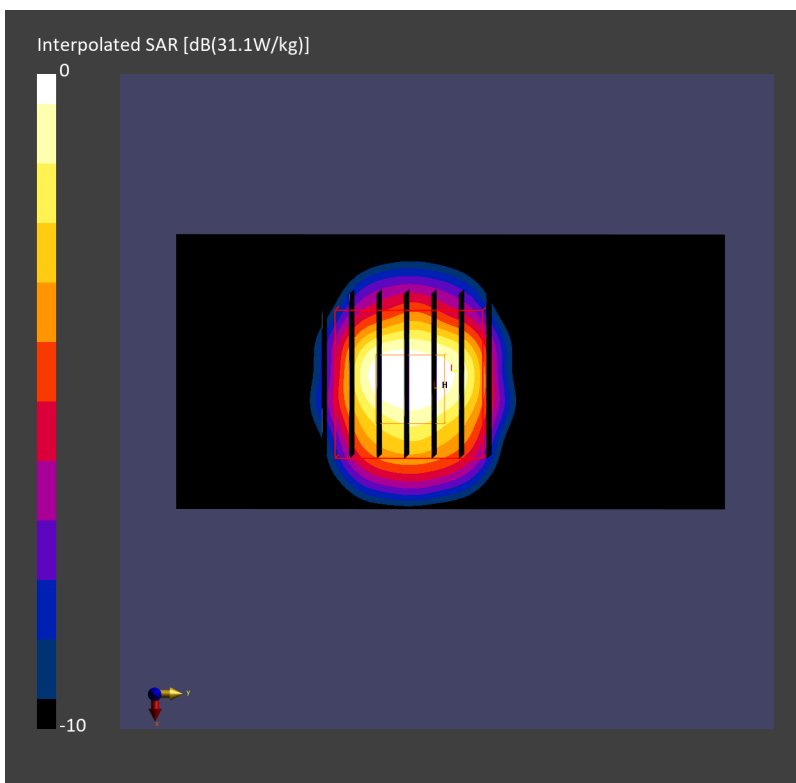

System Check_Head_5800MHz

DUT: D5GHzV2 - SN1128


Communication System: CW; Frequency: 5800.000 MHz; Duty Cycle: 1:1
Medium: HSL_5G_240531 Medium parameters used: $f= 5800.000$ MHz; $\sigma= 5.25$ S/m; $\epsilon_r = 36.2$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

DASY8 Configuration:

- Probe: EX3DV4 - SN3728; ConvF(4.46, 4.46, 4.46); Calibrated: 2024-03-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn699; Calibrated: 2024-02-13
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2155; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 10.0 mm x 10.0 mm
SAR (1g) = 3.46 W/kg; SAR (10g) = 1.09 W/kg;

Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = -0.17 dB
SAR (1g) = 3.93 W/kg; SAR (8g) = 1.42 W/kg; SAR (10g) = 1.20 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 61.1 %

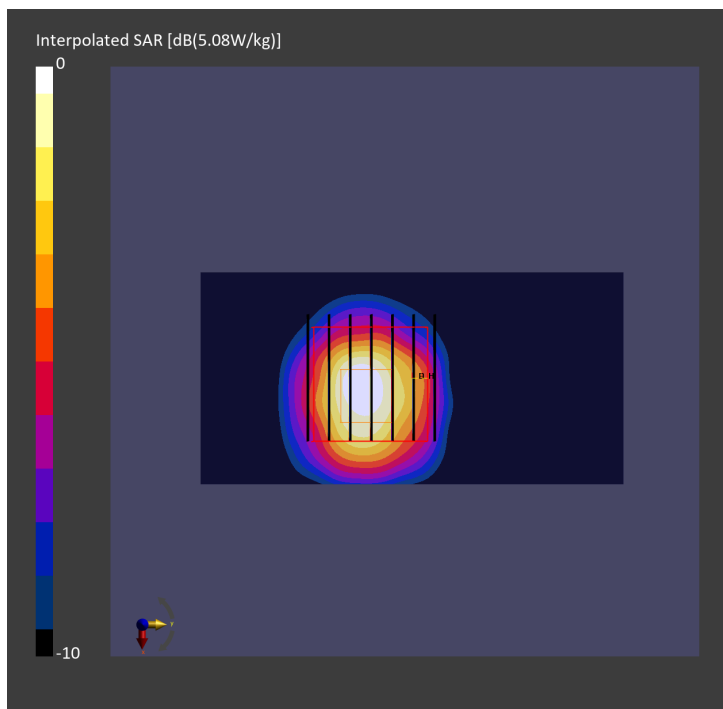

System Check_Head_6500MHz

DUT: D6.5GHzV2 - SN1083

Communication System: CW; Frequency: 6500.000 MHz; Duty Cycle: 1:1

Medium: HSL_6G_240226 Medium parameters used: $f=6500.000$ MHz; $\sigma=6.18$ S/m; $\epsilon_r=34.8$

Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7813; ConvF(5.15, 5.39, 5.13); Calibrated: 2023-05-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE3 Sn577; Calibrated: 2023-09-14
- Phantom: ELI V8.0 (20deg probe tilt); Serial: 2153; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW

Pin=20.0dBm/Area Scan (51.0 mm x 85.0 mm): Measurement Grid: 8.5 mm x 8.5 mm

SAR (1g) = 23.0 W/kg; SAR (10g) = 4.65 W/kg;

Pin=20.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 3.4 mm x 3.4 mm x 1.4 mm

Power Drift = -0.06 dB

SAR (1g) = 27.5 W/kg; SAR (8g) = 6.14 W/kg; SAR (10g) = 5.02 W/kg

Smallest distance from peaks to all points 3 dB below = 4.6 mm

Ratio of SAR at M2 to SAR at M1 = 49.6 %

psAPD (1.0cm², sq) = 275 [W/m²]; psAPD (4.0cm², sq) = 123 [W/m²]

