Report No. : ES/2008/40006 Page : 1 of 59

SAR TEST REPORT

Product Name	Wireless Data Collection Terminal	
Model No.	PA600	
FCC ID	HLEPA600BTGG	
Applicant	Unitech electronics co., ltd	
Address of Applicant	8FI.,No.118 Lane, 235, Pao-Chiao Rd., Hsin-Tien City, Taip	
	Hsien, Taiwan 231,R.O.C.	
Date of Receipt	2008.04.10	
Date of Test(s)	2008.04.16-2008.04.18	
Date of Issue	2008.05.22	

Standards:

FCC OET Bulletin 65 supplement C, ANSI/IEEE C95.1, C95.3, IEEE 1528

In the configuration tested, the EUT complied with the standards specified above. **Remarks:**

This report details the results of the testing carried out on one sample, the results contained in this test report do not relate to other samples of the same product. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report.

This report may only be reproduced and distributed in full. If the product in this report is used in any configuration other than that detailed in the report, the manufacturer must ensure the new system complies with all relevant standards. Any mention of SGS Taiwan Electronics & Communication Laboratory or testing done by SGS Taiwan Electronics & Communication Laboratory in connection with distribution or use of the product described in this report must be approved by SGS Taiwan Electronics & Communication Laboratory in writing.

Tested by	: <u>Ricky Huang</u>	Ricky Wrang	Date	: _	2008.05.22
	Sr. Engineer	Robert Chang			
Approved by	: Robert Chang Tech Manager	0	Date	:_	2008.05.22

Contents

1. General Information	
1.1 Testing Laboratory	3
1.2 Details of Applicant	3
1.3 Description of EUT	3
1.4 Test Environment	4
1.5 Operation description	4
1.6 The SAR Measurement System	5
1.7 System Components	6
1.8 SAR System Verification	7
1.9 Tissue Simulant Fluid for the Frequency Band	8
1.10 EVALUATION PROCEDURES	9
1.11 Test Standards and Limits	10
2. Summary of Results	12
3. Instruments List	14
4. Measurement values	15
GSM 850MHz	

PCS 1900MHz

WLAN802.11 b

WLAN802.11 g

5. System Verification

900MHz Body	35
1900MHz Body	36
2450MHz Body	37

6.APPENDIX

6.1. DAE & Probe Calibration certificate	38
6.2 Uncertainty Analysis	48
6.3 Phantom Description	49
6.4 System Validation from Original equipment supplier	50
6.5 Photographs of Test Setup	53
6.6 Photographs of EUT	56
6.7 Photographs of Battery	59

1. General Information

1.1 Testing Laboratory

SGS Taiwan Ltd. Electronics & Communication Laboratory		
5F, No. 134, Wukung Road, Wuku industrial zone		
Taipei county, Taiwan, R.O.C.		
Telephone	+886-2-2299-3279	
Fax	+886-2-2298-0488	
Internet http://www.tw.sgs.com/		

1.2 Details of Applicant

<u> </u>	
Name	Unitech electronics co., lte.
Address	8F.,No.118 Lane, 235, Pao-Chiao Rd., Hsin-Tien City, Taipei
	Hsien, Taiwan 231,R.O.C.
Telephone	02-8912-1122
Contact Person	Chris Yeh
E-mail	ChrisY@tw.ute.com

1.3 Description of EUT

Product Name	Wireless Data Collection Terminal			
Model Number	PA600			
Brand Name	unitech			
IMEI	355634007610527			
Mode of Operation	GSM,GPRS,EDGE,(900/1800/850/1900), WLAN802.11b/g			
Modulation mode	GMSK/ QPSK/8PSK/ OFDM			
Duty Cycle	GSM	GPRS(EDGE)	WLAN802.11 b/g	
	1/8	1/4	1	
Maximum RF Conducted	GSM 850	PCS 1900	WLAN802.11 b/g	
Power (Average)	32dbm	28.7dbm	14.83dbm	
TV Fraguency renge	GSM 850	PCS 1900	WLAN802.11 b/g	
TX Frequency range	824.2-848.8 MHz	1850.2-1909.8 MHz	2412-2472 MHz	

Report No. : ES/2008/40006

		Г	age : 4 of 59
Channel Number (ARFCN)	GSM 850	PCS 1900	WLAN802.11 b/g
	128-251	512-810	1-13
Antenna Type	Internal Antenna		
Antenna Gain	-1.98 ~ -4.53		
Definition	Production unit		
Max. SAR Measured (1 g)	0.273 W/kg (At GSM 1900 Channel 810_repeated with Bluetooth active)		

Note:

1. EGPRS mode was not measured because maximum averaged output power is 3 dB lower in EGPRS mode than in GPRS mode.

1.4 Test Environment

Ambient Temperature: 22.1° C Tissue Simulating Liquid: 21.7° C Relative Humidity: 62 %

1.5 Operation description

General:

- The EUT is controlled by using a Radio Communication Tester (R&S CMU200), and the communication between the EUT and the tester is established by air link. Measurements are performed respectively on the lowest, middle and highest channels of the operating band(s). The EUT is set to maximum power level during all tests, and at the beginning of each test the battery is fully charged.
- 2. During the SAR testing, the DASY4 system checks power drift by comparing the e-field strength of one specific location measured at the beginning with that measured at the end of the SAR testing.
- 3. Testing body-worn SAR with Headset with Bluetooth transmitter OFF by separating 1.5cm between the back of the EUT and the flat phantom in GPRS mode.
- 4. Testing body-worn SAR with Headset and with Bluetooth transmitter OFF by separating 1.5cm between the front of the EUT and the flat phantom in GPRS mode.
- 5. Testing body-worn SAR with Headset and with Bluetooth transmitter ON in GPRS mode at the body-worn worst case configuration.
- 6. For highest SAR configuration in this band repeated with external Memory card.

Report No. : ES/2008/40006 Page : 5 of 59

1.6 The SAR Measurement System

A photograph of the SAR measurement System is given in Fig. a. This SAR Measurement System uses a Computer-controlled 3-D stepper motor system (Speag Dasy 4 professional system). A Model EX3DV3 3526-field probe is used to determine the internal electric fields. The SAR can be obtained from the equation SAR= σ ($|Ei|^2$)/ ρ where σ and ρ are the conductivity and mass density of the tissue-simulant.

The DASY4 system for performing compliance tests consists of the following items:

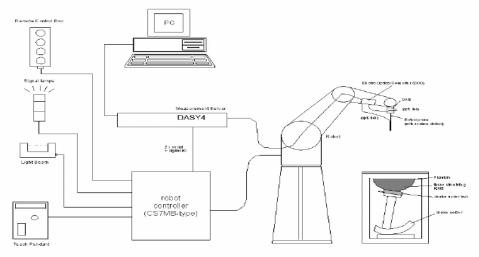


Fig. a The microwave circuit arrangement used for SAR system verification

- A standard high precision 6-axis robot (Stabile RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
 - A computer operating Windows 2000 or Windows XP.
 - DASY4 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.

Report No. : ES/2008/40006 Page : 6 of 59

- The SAM twin phantom enabling testing left-hand and right-hand usage.
- The device holder for hand-held mobile phones.
- Tissue simulating liquid mixed according to the given recipes.
- Validation dipole kits allowing to validate the proper functioning of the system.

1.7 System Components

EX3DV3 E-Field			
Construction	Symmetrical design with triangular core		
	Built-in shielding against static charges		
	PEEK enclosure material (resistant to organic		
	solvents, e.g., DGBE)		
Calibration	Basic Broad Band Calibration in air		
	Conversion Factors (CF) for		
	HSL850/1900/2450MHz Additional CF for		
	other liquids and frequencies upon request		
Frequency	10 MHz to $>$ 6 GHz, Linearity: \pm 0.2 dB (30 MHz to 6 GHz)		
Directivity	\pm 0.3 dB in HSL (rotation around probe axis)		
	\pm 0.5 dB in tissue material (rotation normal to probe axis)		
Dynamic Range	$10 \ \mu W/g \text{ to} > 100 \ m W/g$		
	Linearity: $\pm 0.2 \text{ dB}$ (noise: typically $< 1 \mu\text{W/g}$)		
Dimensions	Overall length: 330 mm (Tip: 20 mm)		
	Tip diameter: 2.5 mm (Body: 12 mm)		
	Typical distance from probe tip to dipole centers: 1 mm		
Application	High precision dosimetric measurements in any exposure scenario (e.g.,		
	very strong gradient fields). Only probe which enables compliance testing		
	for frequencies up to 6 GHz with precision of better 30%.		
SAM PHANTON	1 V4.0C		
Construction:	The shell corresponds to the specifications of the Specific Anthropomorphic		
	Mannequin (SAM) phantom defined in IEEE 1528-200X, CENELEC		
	50361 and IEC 62209.		
	It enables the dosimetric evaluation of left and right hand phone usage as		
	well as body mounted usage at the flat phantom region. A cover prevents		
	evaporation of the liquid. Reference markings on the phantom allow the		
	complete setup of all predefined phantom positions and measurement grids		
	by manually teaching three points with the robot.		
Shell Thickness:	2 ± 0.2 mm		
Filling Volume:	Approx. 25 liters		
Dimensions:	Height: 251 mm;		
	Length: 1000 mm;		
	Width: 500 mm		

EX3DV3 E-Field Probe

DEVICE HOLDER

Report No. : ES/2008/40006 Page : 7 of 59

Construction In combination with the Twin SAM Phantom V4.0/V4.0C or Twin SAM, the Mounting Device (made from POM) enables the rotation of the	
mounted transmitter in spherical coordinates, whereby the rotation point is the ear opening. The devices can be easily and accurately positioned according to IEC, IEEE, CENELEC, FCC or other specifications. The device holder can be locked at different phantom locations (left head, right head, flat phantom).	Device Holder

1.8 SAR System Verification

The microwave circuit arrangement for system verification is sketched in Fig. b. The daily system accuracy verification occurs within the flat section of the SAM phantom. A SAR measurement was performed to see if the measured SAR was within +/- 10% from the target SAR values. These tests were done at 850 & 1900 & 2450 MHz. The tests were conducted on the same days as the measurement of the DUT. The obtained results from the system accuracy verification are displayed in the table 1 (SAR values are normalized to 1W forward power delivered to the dipole). During the tests, the ambient temperature of the laboratory was in the range 22.1°C, the relative humidity was in the range 62% and the liquid depth above the ear reference points was above 15 cm in all the cases. It is seen that the system is operating within its specification, as the results are within acceptable tolerance of the reference values.




Fig.b The microwave circuit arrangement used for SAR system verification Agilent Model 8648D Signal Generator

- A. Mini circuits Model ZHL-42 Amplifier
- B. Agilent Model E4416A Power Meter
- C. Agilent Model 8481H Power Sensor
- D. Agilent Model 778D & 777D Dual directional coupling



Photograph of the dipole Antenna

E. Reference dipole antenna

Validation Kit	Frequency Hz	Target SAR (1g) (Pin=250mW)	Measured SAR (1g)	Variation	Measured Date
D900V2 S/N: 168	900 MHz (Body)	2.58m W/g	2.68 m W/g	3.8%	2008-04-16
D1900V2 S/N: 5d018	1900 MHz (Body)	9.55 m W/g	9.59 m W/g	0.1%	2008-04-17
D2450V2 S/N: 735	2450 MHz (Body)	12.9 m W/g	13 m W/g	0.7%	2008-04-18

Report No. : ES/2008/40006 Page · 8 of 59

Table 1. Results system validation

1.9 Tissue Simulant Fluid for the Frequency Band

The dielectric properties for this body-simulant fluid were measured by using the HP Model 85070D Dielectric Probe (rates frequency band 200 MHz to 20 GHz) in conjunction with HP 8753D Network Analyzer (30 KHz-6000 MHz) by using a procedure detailed in Section V. All dielectric parameters of tissue simulates were measured within 24 hours of SAR measurement. The depth of the tissue simulant in the ear reference point of the phantom was 15cm±5mm during all tests. (Fig .2)

Frequency	Tissue type	Measurement date/	Dielectric Parameters		
(MHz)		Limits	ρ	σ (S/m)	Simulated Tissue
					Temperature(° C)
900	Body	Measured, 2008.04.16	54.3	1.07	21.7
900	Dody	Recommended Limits	52.3-58.0	0.92-1.10	20-24
1900	Body	Measured, 2008.04.17	50.9	1.56	21.7
1900		Recommended Limits	50.6-56.0	1.38-1.60	20-24
2450	Podu	Measured, 2008.04.18	51.8	2.02	21.7
2130	Body	Recommended Limits	50.1-55.3	1.85-2.12	20-24

Table 2. Dielectric Parameters of Tissue Simulant Fluid

Band 850(Body) Frequency (MHz)	Channel	Target	Permittivity Measurement Date	Variation %	Target	Conductivity Measurement Date	Variation %
Low(824.2)	128		55.1	0.1		0.994	2.4
Mid(836.6)	190	55.2	55	0.3	0.97	1.0	3
High(848.8)	251		54.9	0.5		1.01	4.1

Table 3. Dielectric Parameters of Tissue Simulant Fluid (follow P1528 target value)

Report No. : ES/2008/40006 Page : 9 of 59

900Mhz(Body) 1900Mhz(Body) 2450Mhz (Body) Ingredient DGMBE Х 300.67 301.7 ml 632.68 716.56 698.3 ml Water 11.72 Х Sale 4.0 Preventol D-7 1.2 Х Х Cellulose Х Х Х X Х 600 g Sugar Total amount 1 L (1.0kg) 1 L (1.0kg) 1 L (1.0kg)

The composition of the brain tissue simulating liquid for 900 & 1900 & 2450 MHz is:

Table 4. Recipes for tissue simulating liquid

1.10 EVALUATION PROCEDURES

The entire evaluation of the spatial peak values is performed within the Post-processing engine (SEMCAD). The system always gives the maximum values for the 1 g and 10 g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- 1. The extraction of the measured data (grid and values) from the Zoom Scan.
- 2. The calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- 3. The generation of a high-resolution mesh within the measured volume
- 4. The interpolation of all measured values from the measurement grid to the high-resolution grid
- 5. The extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- 6. The calculation of the averaged SAR within masses of 1g and 10g.

The probe is calibrated at the center of the dipole sensors that is located 1 to 2.7mm away from the probe tip. During measurements, the probe stops shortly above the phantom surface, depending on the probe and the surface detecting system. Both distances are included as parameters in the probe configuration file. The software always knows exactly how far away the measured point is from the surface. As the probe cannot directly measure at the surface, the values between the deepest measured point and the surface must be extrapolated. The angle between the probe axis and the surface normal line is less than 30 degree.

In the Area Scan, the gradient of the interpolation function is evaluated to find all the extreme of the SAR distribution. The uncertainty on the locations of the extreme is less than 1/20 of the grid size. Only local maximum within -2 dB of the global maximum are searched and passed for the Cube Scan measurement. In the Cube Scan, the interpolation function is used to extrapolate the Peak SAR from the lowest measurement points to the inner phantom surface (the extrapolation distance). The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5mm.

The maximum search is automatically performed after each area scan measurement. It is based on splines in two or three dimensions. The procedure can find the maximum for most SAR distributions even with relatively large grid spacing. After the area scanning measurement, the probe is automatically moved to a position at the interpolated maximum. The following scan

Report No. : ES/2008/40006

Page : 10 of 59

can directly use this position for reference, e.g., for a finer resolution grid or the cube evaluations. The 1g and 10g peak evaluations are only available for the predefined cube 7x7x7 scans. The routines are verified and optimized for the grid dimensions used in these cube measurements. The measured volume of 30x30x30mm contains about 30g of tissue. The first procedure is an extrapolation (incl. Boundary correction) to get the points between the lowest measured plane and the surface. The next step uses 3D interpolation to get all points within the measured volume. In the last step, a 1g cube is placed numerically into the volume and its averaged SAR is calculated. This cube is the moved around until the highest averaged SAR is found. If the highest SAR is found at the edge of the measured volume, the system will issue a warning: higher SAR values might be found outside of the measured volume. In that case the cube measurement can be repeated, using the new interpolated maximum as the center.

1.11 Test Standards and Limits

According to FCC 47CFR §2.1093(d) The limits to be used for evaluation are based generally on criteria published by the American National Standards Institute (ANSI) for localized specific absorption rate ("SAR") in Section 4.2 of "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz," ANSI/IEEE C95.1–1992, Copyright 1992 by the Institute of Electrical and Electronics Engineers, Inc., New York, New York 10017. These criteria for SAR evaluation are similar to those recommended by the National Council on Radiation Protection and Measurements (NCRP) in "Biological Effects and Exposure Criteria for Radio frequency Electromagnetic Fields," NCRP Report No. 86, Section 17.4.5. Copyright NCRP, 1986, Bethesda, Maryland 20814. SAR is a measure of the rate of energy absorption due to exposure to an RF transmitting source. SAR values have been related to threshold levels for potential biological hazards. The criteria to be used are specified in paragraphs (d)(1) and (d)(2) of this section and shall apply for portable devices transmitting in the frequency range from 100 kHz to 6 GHz. Portable devices that transmit at frequencies above 6 GHz are to be evaluated in terms of the MPE limits specified in § 1.1310 of this chapter. Measurements and calculations to demonstrate compliance with MPE field strength or power density limits for devices operating above 6 GHz should be made at a minimum distance of 5 cm from the radiating source.

(1) Limits for Occupational/Controlled exposure: 0.4 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 8 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 20 W/kg, as averaged over an 10 grams of tissue (defined as a tissue volume in the shape of a cube). Occupational/Controlled limits apply when persons are exposed as a consequence of their employment provided these persons are fully aware of and exercise control over their exposure. Awareness of exposure can be accomplished by use of warning labels or by specific training or education through appropriate means, such as an RF safety program in a work environment.

Report No. : ES/2008/40006 Page : 11 of 59

(2) Limits for General Population/Uncontrolled exposure: 0.08 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 1.6 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 4 W/kg, as averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube). General Population/Uncontrolled limits apply when the general public may be exposed, or when persons that are exposed as a consequence of their employment may not be fully aware of the potential for exposure or do not exercise control over their exposure. Warning labels placed on consumer devices such as cellular telephones will not be sufficient reason to allow these devices to be evaluated subject to limits for occupational/controlled exposure in paragraph (d)(1) of this section.(Table .4)

Human Exposure	Uncontrolled Environment General Population	Controlled Environment Occupational
Spatial Peak SAR (Brain)	1.60 m W/g	8.00 m W/g
Spatial Average SAR (Whole Body)	0.08 m W/g	0.40 m W/g
Spatial Peak SAR (Hands/Feet/Ankle/Wrist)	4.00 m W/g	20.00 m W/g

Table .5 RF exposure limits

Notes:

1. Uncontrolled environments are defined as locations where there is potential exposure of

individuals who have no knowledge or control of their potential exposure.

2. Controlled environments are defined as locations where there is potential exposure of individuals who have knowledge of their potential exposure and can exercise control over their exposure.

Report No. : ES/2008/40006 Page : 12 of 59

2.Summary of Results

GSM 850 MHZ- testing in GPRS mode (uplink slot=2)

Body worn (testing in GPRS mode)
---------------------------------	---

Frequency	Channel	MHz	Conducted Output Measured(W/kg)		Amb.	Liquid
			Power (Average) 1g		Temp[°C]	Temp[°C]
850 MHz	128	824.2	31.7dbm	0.167	22.1	21.7
	190	836.6	31.9dbm	0.164	22.1	21.7
	251	848.8	32dbm	0.158	22.1	21.7

PCS 1900 MHZ- testing in GPRS mode (uplink slot=2)

				(" p"""""""""""""""""""""""""""""""""""					
Body worn (testing in GPRS mode)									
Frequency	Channel	MHz	Conducted Output	Measured(W/kg) Amb.		Liquid			
			Power (Average)	1g	Temp[°C]	Temp[°C]			
1900 MHz	512	1850.2	28.5dbm	0.208	22.1	21.7			
	661	1880.0	28.6dbm	0.191	22.1	21.7			
	810	1909.8	28.7dbm	0.242	22.1	21.7			
Body worn (to	Body worn (testing in GPRS mode)_repeated in EUT front to phantom								
Frequency	Channel	MHz	Conducted Output	Measured(W/kg)	Amb.	Liquid			
			Power (Average)	1g	Temp[°C]	Temp[°C]			
1900 MHz	810	1909.8	28.7dbm	0.014	22.1	21.7			
Body worn (to	esting in GI	PRS mod	e)_repeated with Me	mory card					
Frequency	Channel	MHz	Conducted Output	Measured(W/kg)	Amb.	Liquid			
			Power (Average)	1g	Temp[°C]	Temp[°C]			
1900 MHz	810	1909.8	28.7dbm	0.272	22.1	21.7			
Rody worn (t	esting in CI	PRS mod	Rody worn (testing in CPRS mode), repeated with Bluetooth active						

Body worll (testing in GPRS mode)_repeated with Bluetooth active							
Frequency	Channel	MHz	Conducted Output Measured(W/kg) A		Amb.	Liquid	
			Power (Average)	1g	Temp[°C]	Temp[°C]	
1900 MHz	810	1909.8	28.7dbm	0.273	22.1	21.7	

WLAN802.11b

Body worn							
Frequency	Channel	MHz	Conducted Output	Measured(W/kg)	Amb.	Liquid	
			Power (Average)	1g	Temp[°C]	Temp[°C]	
WLAN802.11b	WLAN802.11b 1 2412		14.83dbm	0.040	22.1	21.7	
	6	2437	14.39dbm	0.028	22.1	21.7	

Report No. : ES/2008/40006 Page : 13 of 59

	Page : 13 of 59					59	
	11	2462	13.55dbm	0.021	22.1	21.7	
Body worn _re	Body worn _repeated in EUT back to phantom						
Frequency	Channel	MHz	Conducted Output	Measured(W/kg)	Amb.	Liquid	
			Power (Average)	1g	Temp[°C]	Temp[°C]	
WLAN802.11b	1	2412	14.83dbm	0.0067	22.1	21.7	
Body worn _re	Body worn _repeated with Memory card						
Frequency	Channel	MHz	Conducted Output	Measured(W/kg)	Amb.	Liquid	
			Power (Average)	1g	Temp[°C]	Temp[°C]	
WLAN802.11b	1	2412	14.83dbm	0.038	22.1	21.7	
Body worn _re	peated witl	n Blueto	oth active				
Frequency	Channel	MHz	Conducted Output	Measured(W/kg)	Amb.	Liquid	
			Power (Average)	1g	Temp[°C]	Temp[°C]	
WLAN802.11b	1	2412	14.83dbm	0.038	22.1	21.7	

WLAN802.11g

Body worn							
Frequency	Channel	MHz	Conducted Output	Measured(W/kg)	Amb.	Liquid	
			Power (Average)	1g	Temp[°C]	Temp[°C]	
WLAN802.11g 1		2412	10.21dbm	0.029	22.1	21.7	
	6	2437	11.10dbm	0.020	22.1	21.7	
	11	2462	9.94dbm	0.015	22.1	21.7	

Note:SAR measurement results with transmitter at maximum output power.

Report No. : ES/2008/40006 Page : 14 of 59

3. Instruments List

Manufacturer	Device	Туре	Serial number	Date of last calibration
Schmid & Partner Engineering AG	Dosimetric E-Field Probe	EX3DV3	3526	Aug.29.2007
Schmid & Partner	900/1900/2450 MHz	D900V2	168	Apr.17.2007
	System Validation	D1900V2	5d018	Apr.23.2007
Engineering AG	Dipole	D2450N2	735	Apr.24.2007
Schmid & Partner Engineering AG	Data acquisition Electronics	DAE4	547	Oct.01.2007
Schmid & Partner Engineering AG	Software	DASY 4 V4.7 Build 55	N/A	Calibration isn't necessary
Schmid & Partner Engineering AG	Phantom	SAM	N/A	Calibration isn't necessary
Agilent	Network Analyzer	8753D	3410A05547	Nov.15.2007
Agilent	Dielectric Probe Kit	85070D	US01440168	Calibration isn't necessary
A = :1==+4	Deel dimentional complex	778D	50313	Aug.21.2007
Agilent	Dual-directional coupler	777D	50114	Aug.21.2007
Agilent	RF Signal Generator	8648D	3847M00432	May.22.2007
Agilent	Power Sensor	8481H	MY41091361	Jun.04.2007
R&S	Radio Communication Test	CMU200	113505	Aug.24.2007

Report No. : ES/2008/40006 Page : 15 of 59

4.Measurements

Date/Time: 2008/4/16 02:16:51

BODY_GSM850_CH128

DUT: PA600; IMEI:355634007610527

Communication System: GSM 850; Frequency: 824.2 MHz;Duty Cycle: 1:4 Medium: Muscle 900 MHz Medium parameters used (interpolated): f = 824.2 MHz; $\sigma = 0.994$ mho/m; $\epsilon_r = 55.1$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.177 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 6.32 V/m; Power Drift = 0.067 dB Peak SAR (extrapolated) = 0.217 W/kg

SAR(1 g) = 0.167 mW/g; SAR(10 g) = 0.125 mW/g

Maximum value of SAR (measured) = 0.177 mW/g

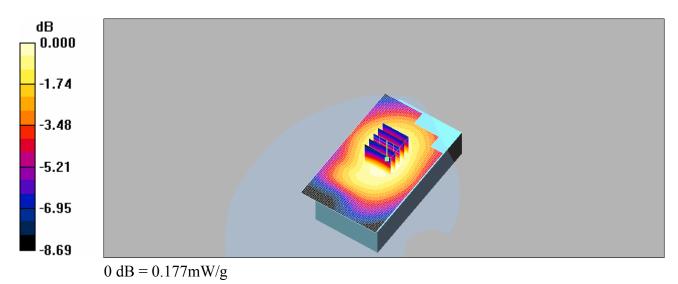

Report No. : ES/2008/40006 Page : 16 of 59 Date/Time: 2008/4/16 02:58:01

BODY_GSM850_CH190

DUT: PA600; IMEI:355634007610527

Communication System: GSM 850; Frequency: 836.6 MHz;Duty Cycle: 1:4 Medium: Muscle 900 MHz Medium parameters used: f = 837 MHz; $\sigma = 1$ mho/m; $\epsilon_r = 55$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.173 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 6.60 V/m; Power Drift = -0.053 dB Peak SAR (extrapolated) = 0.212 W/kg

SAR(1 g) = 0.164 mW/g; SAR(10 g) = 0.121 mW/g

Maximum value of SAR (measured) = 0.173 mW/g

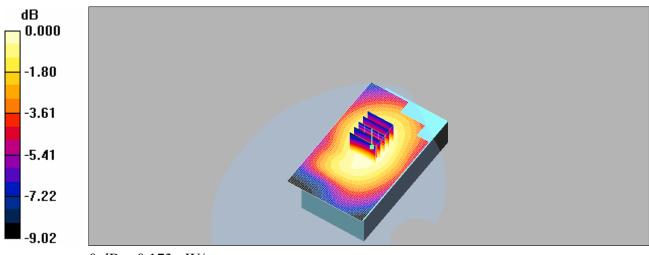

0 dB = 0.173 mW/g

Report No. : ES/2008/40006 Page : 17 of 59 Date/Time: 2008/4/16 03:26:44

BODY_GSM850_CH251

DUT: PA600; IMEI:355634007610527

Communication System: GSM 850; Frequency: 848.8 MHz;Duty Cycle: 1:4 Medium: Muscle 900 MHz Medium parameters used: f = 849 MHz; $\sigma = 1.01$ mho/m; $\epsilon_r = 54.9$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.165 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 6.68 V/m; Power Drift = -0.054 dB Peak SAR (extrapolated) = 0.210 W/kg

SAR(1 g) = 0.158 mW/g; SAR(10 g) = 0.117 mW/g

Maximum value of SAR (measured) = 0.167 mW/g

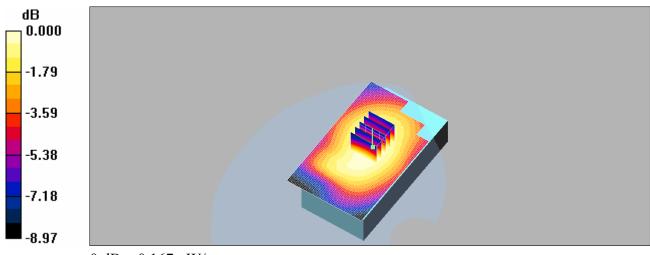

0 dB = 0.167 mW/g

Report No. : ES/2008/40006 Page : 18 of 59 \Date/Time: 2008/4/17 05:48:04

BODY_GSM1900_CH512

DUT: PA600; IMEI:355634007610527

Communication System: GSM1900; Frequency: 1850.2 MHz;Duty Cycle: 1:4 Medium: M1800 & 1900 Medium parameters used (interpolated): f = 1850.2 MHz; $\sigma = 1.52$ mho/m; $\varepsilon_r = 51.2$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.232 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 6.11 V/m; Power Drift = -0.080 dB Peak SAR (extrapolated) = 0.333 W/kg

SAR(1 g) = 0.208 mW/g; SAR(10 g) = 0.120 mW/g

Maximum value of SAR (measured) = 0.230 mW/g

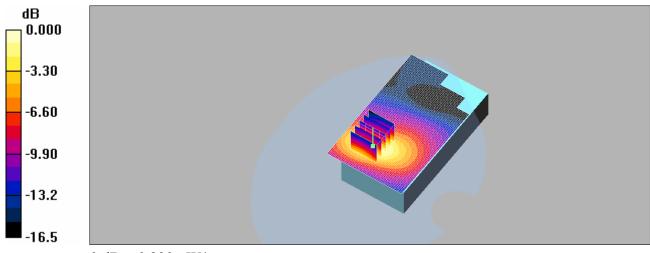

0 dB = 0.230 mW/g

Report No. : ES/2008/40006 Page : 19 of 59 Date/Time: 2008/4/17 06:29:10

BODY_GSM1900_CH661

DUT: PA600; IMEI:355634007610527

Communication System: GSM1900; Frequency: 1880 MHz;Duty Cycle: 1:4 Medium: M1800 & 1900 Medium parameters used (interpolated): f = 1880 MHz; $\sigma = 1.55$ mho/m; $\epsilon_r = 51$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.213 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 6.09 V/m; Power Drift = -0.040 dB Peak SAR (extrapolated) = 0.314 W/kg

SAR(1 g) = 0.191 mW/g; SAR(10 g) = 0.109 mW/g

Maximum value of SAR (measured) = 0.211 mW/g

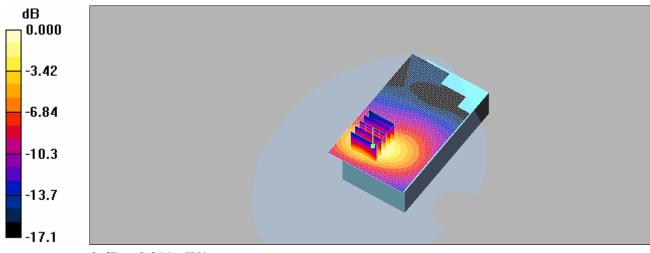

0 dB = 0.211 mW/g

Report No. : ES/2008/40006 Page : 20 of 59 Date/Time: 2008/4/17 07:01:43

BODY_GSM1900_CH810

DUT: PA600; IMEI:355634007610527


Communication System: GSM1900; Frequency: 1909.8 MHz;Duty Cycle: 1:4 Medium: M1800 & 1900 Medium parameters used: f = 1910 MHz; $\sigma = 1.57$ mho/m; $\epsilon_r = 50.9$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:

- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.271 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 7.25 V/m; Power Drift = 0.011 dB Peak SAR (extrapolated) = 0.390 W/kg **SAR(1 g) = 0.242 mW/g; SAR(10 g) = 0.138 mW/g** Maximum value of SAR (measured) = 0.268 mW/g

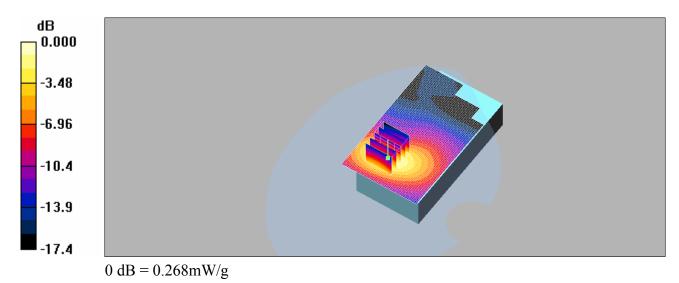

Report No. : ES/2008/40006 Page : 21 of 59 Date/Time: 2008/4/17 07:26:24

BODY_GSM1900_CH810_ repeated in EUT front to Phantom

DUT: PA600; IMEI:355634007610527

Communication System: GSM1900; Frequency: 1909.8 MHz;Duty Cycle: 1:4 Medium: M1800 & 1900 Medium parameters used: f = 1910 MHz; $\sigma = 1.57$ mho/m; $\epsilon_r = 50.9$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x131x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.016 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 2.62 V/m; Power Drift = -0.184 dB Peak SAR (extrapolated) = 0.023 W/kg

SAR(1 g) = 0.014 mW/g; SAR(10 g) = 0.009 mW/g

Maximum value of SAR (measured) = 0.016 mW/g

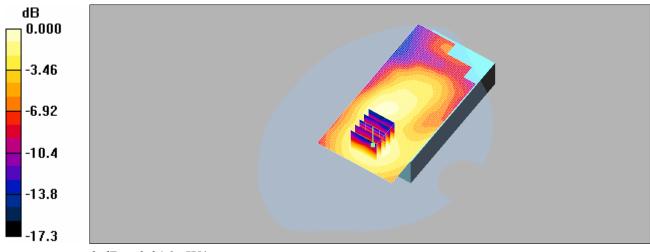

0 dB = 0.016 mW/g

Report No. : ES/2008/40006 Page : 22 of 59 Date/Time: 2008/4/17 08:13:20

BODY_GSM1900_CH810_repeated with Memory card

DUT: PA600; IMEI:355634007610527

Communication System: GSM1900; Frequency: 1909.8 MHz;Duty Cycle: 1:4 Medium: M1800 & 1900 Medium parameters used: f = 1910 MHz; $\sigma = 1.57$ mho/m; $\epsilon_r = 50.9$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.303 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 7.13 V/m; Power Drift = -0.016 dB Peak SAR (extrapolated) = 0.454 W/kg

SAR(1 g) = 0.272 mW/g; SAR(10 g) = 0.151 mW/g

Maximum value of SAR (measured) = 0.304 mW/g

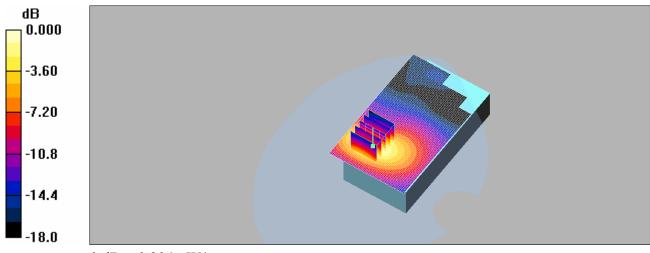

0 dB = 0.304 mW/g

Report No. : ES/2008/40006 Page : 23 of 59 Date/Time: 2008/4/17 08:58:48

BODY_GSM1900_CH810_repeated with Bluetooth active

DUT: PA600; IMEI:355634007610527

Communication System: GSM1900; Frequency: 1909.8 MHz;Duty Cycle: 1:4 Medium: M1800 & 1900 Medium parameters used: f = 1910 MHz; $\sigma = 1.57$ mho/m; $\epsilon_r = 50.9$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.304 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 7.43 V/m; Power Drift = -0.067 dB Peak SAR (extrapolated) = 0.459 W/kg

SAR(1 g) = 0.273 mW/g; SAR(10 g) = 0.152 mW/g

Maximum value of SAR (measured) = 0.303 mW/g

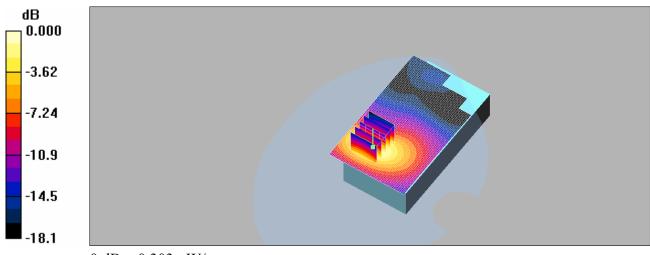

0 dB = 0.303 mW/g

Report No. : ES/2008/40006

Page : 24 of 59



Report No. : ES/2008/40006 Page : 25 of 59 Date/Time: 2008/4/18 15:16:15

BODY_WLAN802.11 b_CH1

DUT: PA600; IMEI:355634007610527

Communication System: Wireless LAN; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: Muscle 2450 Medium parameters used: f = 2412 MHz; $\sigma = 1.96$ mho/m; $\epsilon_r = 52.6$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.045 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 4.40 V/m; Power Drift = -0.172 dB Peak SAR (extrapolated) = 0.076 W/kg


SAR(1 g) = 0.040 mW/g; SAR(10 g) = 0.020 mW/g

Maximum value of SAR (measured) = 0.044 mW/g

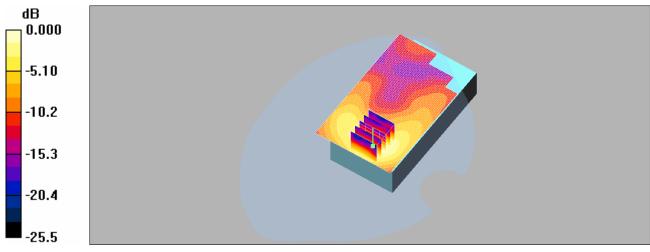

0 dB = 0.044 mW/g

Report No. : ES/2008/40006 Page : 26 of 59

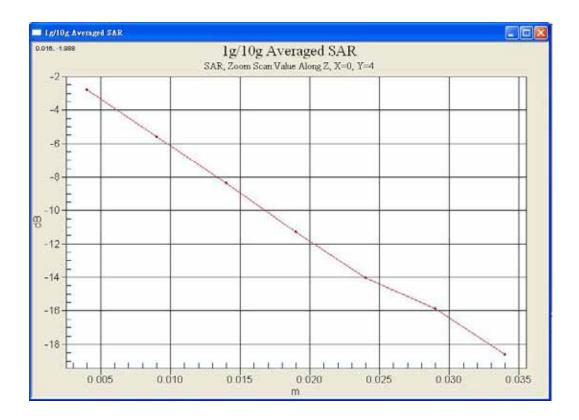

Report No. : ES/2008/40006 Page : 27 of 59 Date/Time: 2008/4/18 16:01:04

BODY_WLAN802.11 b_CH6

DUT: PA600; IMEI:355634007610527

Communication System: Wireless LAN; Frequency: 2437 MHz;Duty Cycle: 1:1 Medium: Muscle 2450 Medium parameters used: f = 2437 MHz; $\sigma = 1.99$ mho/m; $\epsilon_r = 52.1$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.031 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 3.48 V/m; Power Drift = -0.010 dB Peak SAR (extrapolated) = 0.056 W/kg

SAR(1 g) = 0.028 mW/g; SAR(10 g) = 0.014 mW/g

Maximum value of SAR (measured) = 0.031 mW/g

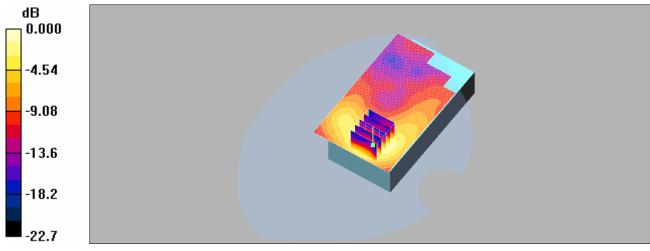

0 dB = 0.031 mW/g

Report No. : ES/2008/40006 Page : 28 of 59 Date/Time: 2008/4/18 16:49:18

BODY_WLAN802.11 b_CH11

DUT: PA600; IMEI:355634007610527

Communication System: Wireless LAN; Frequency: 2462 MHz;Duty Cycle: 1:1 Medium: Muscle 2450 Medium parameters used: f = 2462 MHz; $\sigma = 2.04$ mho/m; $\epsilon_r = 51.5$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.024 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 2.98 V/m; Power Drift = -0.143 dB Peak SAR (extrapolated) = 0.039 W/kg

SAR(1 g) = 0.021 mW/g; SAR(10 g) = 0.011 mW/g

Maximum value of SAR (measured) = 0.024 mW/g

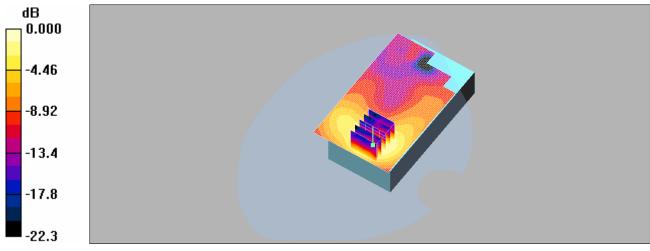

0 dB = 0.024 mW/g

Report No. : ES/2008/40006 Page : 29 of 59 Date/Time: 2008/4/18 19:52:13

BODY_WLAN802.11 b_CH1_repeated in EUT back to phantom

DUT: PA600; IMEI:355634007610527

Communication System: Wireless LAN; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: Muscle 2450 Medium parameters used: f = 2412 MHz; $\sigma = 1.96$ mho/m; $\epsilon_r = 52.6$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.008 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.56 V/m; Power Drift = 0.128 dB Peak SAR (extrapolated) = 0.013 W/kg

SAR(1 g) = 0.0067 mW/g; SAR(10 g) = 0.00382 mW/g

Maximum value of SAR (measured) = 0.007 mW/g

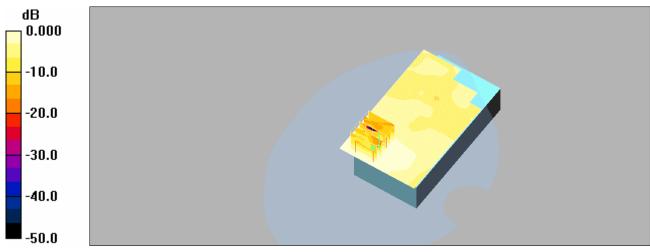

0 dB = 0.007 mW/g

Report No. : ES/2008/40006 Page : 30 of 59 Date/Time: 2008/4/18 20:36:30

BODY_WLAN802.11 b_CH1_repeated with Memory card

DUT: PA600; IMEI:355634007610527

Communication System: Wireless LAN; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: Muscle 2450 Medium parameters used: f = 2412 MHz; $\sigma = 1.96$ mho/m; $\epsilon_r = 52.6$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.042 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 3.61 V/m; Power Drift = -0.005 dB Peak SAR (extrapolated) = 0.076 W/kg

SAR(1 g) = 0.038 mW/g; SAR(10 g) = 0.020 mW/g

Maximum value of SAR (measured) = 0.043 mW/g

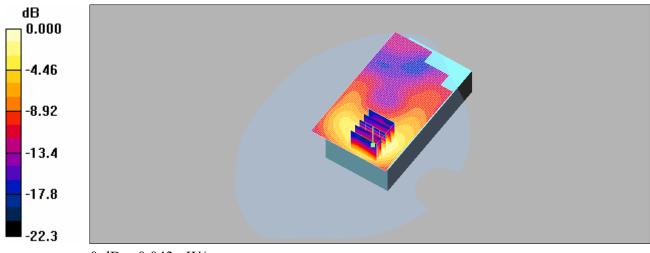

 $0 \, dB = 0.043 \, mW/g$

Report No. : ES/2008/40006 Page : 31 of 59 Date/Time: 2008/4/18 21:47:04

BODY_WLAN802.11 b_CH1_repeated with Bluetooth active

DUT: PA600; IMEI:355634007610527

Communication System: Wireless LAN; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: Muscle 2450 Medium parameters used: f = 2412 MHz; $\sigma = 1.96$ mho/m; $\epsilon_r = 52.6$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.044 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 3.72 V/m; Power Drift = -0.088 dB Peak SAR (extrapolated) = 0.074 W/kg

SAR(1 g) = 0.038 mW/g; SAR(10 g) = 0.020 mW/g

Maximum value of SAR (measured) = 0.043 mW/g

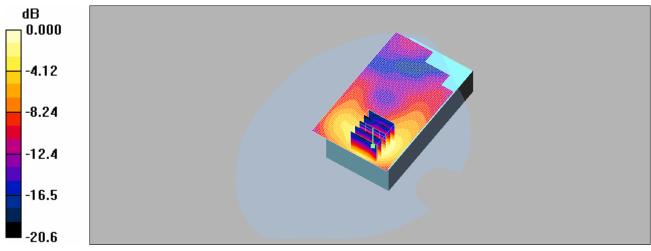

0 dB = 0.043 mW/g

Date/Time: 2008/4/18 17:38:27

Report No. : ES/2008/40006 Page : 32 of 59

BODY_WLAN802.11 g_CH1

DUT: PA600; IMEI:355634007610527

Communication System: Wireless LAN; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: Muscle 2450 Medium parameters used: f = 2412 MHz; $\sigma = 1.96$ mho/m; $\epsilon_r = 52.6$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.034 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 3.42 V/m; Power Drift = -0.062 dB Peak SAR (extrapolated) = 0.056 W/kg

SAR(1 g) = 0.029 mW/g; SAR(10 g) = 0.015 mW/g

Maximum value of SAR (measured) = 0.034 mW/g

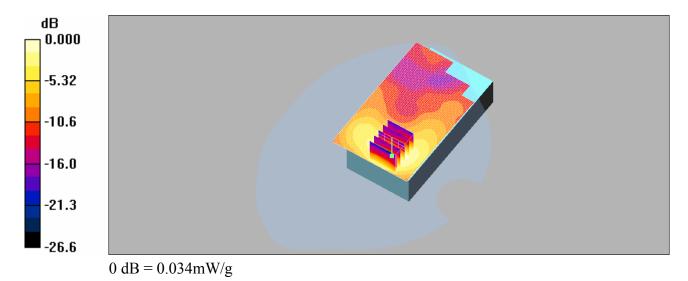

Report No. : ES/2008/40006 Page : 33 of 59 Date/Time: 2008/4/18 18:19:00

BODY_WLAN802.11 g_CH6

DUT: PA600; IMEI:355634007610527

Communication System: Wireless LAN; Frequency: 2437 MHz;Duty Cycle: 1:1 Medium: Muscle 2450 Medium parameters used: f = 2437 MHz; $\sigma = 1.99$ mho/m; $\epsilon_r = 52.1$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.023 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 2.83 V/m; Power Drift = -0.062 dB Peak SAR (extrapolated) = 0.040 W/kg

SAR(1 g) = 0.020 mW/g; SAR(10 g) = 0.010 mW/g

Maximum value of SAR (measured) = 0.023 mW/g

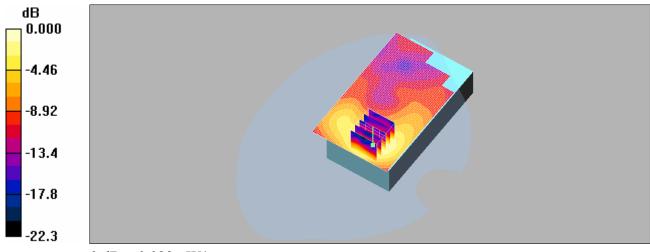

0 dB = 0.023 mW/g

Report No. : ES/2008/40006 Page : 34 of 59 Date/Time: 2008/4/18 19:03:49

BODY_WLAN802.11 g_CH11

DUT: PA600; IMEI:355634007610527

Communication System: Wireless LAN; Frequency: 2462 MHz;Duty Cycle: 1:1 Medium: Muscle 2450 Medium parameters used: f = 2462 MHz; $\sigma = 2.04$ mho/m; $\epsilon_r = 51.5$; $\rho = 1000$ kg/m³ Phantom section: Flat Section


DASY4 Configuration:

- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

BODY/Area Scan (61x111x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.017 mW/g

BODY/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 2.42 V/m; Power Drift = 0.020 dB Peak SAR (extrapolated) = 0.029 W/kg

SAR(1 g) = 0.015 mW/g; SAR(10 g) = 0.00759 mW/g

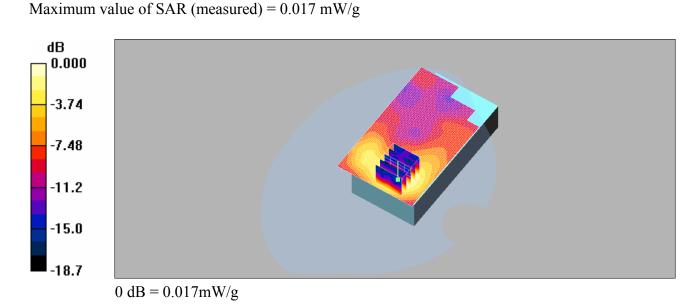

Report No. : ES/2008/40006 Page : 35 of 59

5.SAR System Performance Verification

Date/Time: 2008/4/16 01:23:51

DUT: Dipole 900 MHz; Type: D900V2; Serial: SN:168

Communication System: CW; Frequency: 900 MHz;Duty Cycle: 1:1 Medium: Muscle 900 MHz Medium parameters used: f = 900 MHz; $\sigma = 1.07$ mho/m; $\epsilon_r = 54.3$; $\rho = 1000$ kg/m³ Phantom section: Flat Section


DASY4 Configuration:

- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Pin=250mW/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 3.01 mW/g

Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 53.0 V/m; Power Drift = -0.010 dB Peak SAR (extrapolated) = 4.17 W/kg

SAR(1 g) = 2.68 mW/g; SAR(10 g) = 1.72 mW/g Maximum value of SAR (measured) = 3.00 mW/g

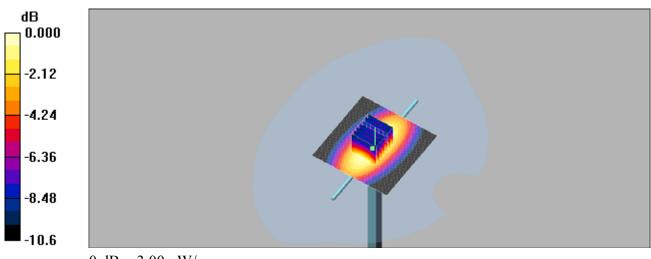

0 dB = 3.00 mW/g

Report No. : ES/2008/40006 Page : 36 of 59 Date/Time: 2008/4/17 04:56:32

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d018

Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: M1900 Medium parameters used (interpolated): f = 1900 MHz; $\sigma = 1.56$ mho/m; $\epsilon_r = 50.9$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY4 Configuration:


- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Pin=250mW/Area Scan (51x61x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 12.5 mW/g

Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 83.1 V/m; Power Drift = -0.019 dB Peak SAR (extrapolated) = 17.6 W/kg

SAR(1 g) = 9.59 mW/g; SAR(10 g) = 4.99 mW/g

Maximum value of SAR (measured) = 10.8 mW/g

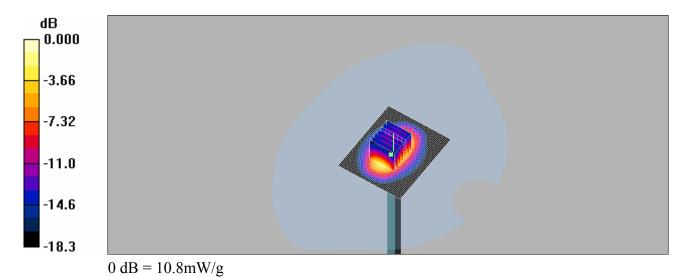

Report No. : ES/2008/40006 Page : 37 of 59 Date/Time: 2008/4/18 02:16:24

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 735

Communication System: CW; Frequency: 2450 MHz;Duty Cycle: 1:1 Medium: M 2450 Medium parameters used: f = 2450 MHz; $\sigma = 2.02$ mho/m; $\epsilon_r = 51.8$; $\rho = 1000$ kg/m³ Phantom section: Flat Section


DASY4 Configuration:

- Probe: EX3DV3 SN3526; Calibrated: 2007/8/29
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn547; Calibrated: 2007/10/1
- Phantom: SAM1; Type: SAM 4.0; Serial: TP:1419
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 176

Pin=250mW/Area Scan (51x61x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 17.1 mW/g

Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 86.3 V/m; Power Drift = -0.102 dB Peak SAR (extrapolated) = 27.5 W/kg

SAR(1 g) = 13 mW/g; SAR(10 g) = 5.89 mW/g Maximum value of SAR (measured) = 14.6 mW/g

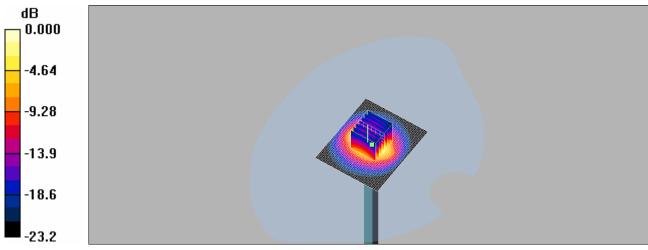

 $^{0 \}text{ dB} = 14.6 \text{mW/g}$

		6.Appendix	
AE & Probe Ca	libration ce	rtificate	
Calibration Laborator ichmid & Partner Engineering AG eughausstrasse 43, 8004 Zurici	504C3	ILCO MRA	S Schweizerischer Kalibrierdienst C Service suisse d'étalonnage Servizio svizzero di taratura S Swiss Calibration Service
ccredited by the Swiss Federal C he Swiss Accreditation Service luitilateral Agreement for the re	is one of the signatories	to the EA	tation No.: SCS 108
lient SGS (Auden)		Certifica	te No: DAE4-547_Oct07
CALIBRATION C	ERTIFICATE		
Doject	DAE4 - SD 000 D	04 BA - SN: 547	Contraction of the second
and bear	5724-55 000 5	04 DA - 511. 547	
Calibration procedure(s)	QA CAL-06.v12 Calibration proces	dure for the data acquisition	electronics (DAE)
Calibration date:	October 1, 2007		Lines Index Records
Condition of the calibrated item	In Tolerance		12 10 10 10 10 10 10 10 10 10 10 10 10 10
The measurements and the uncer	tainties with confidence pro	nal standards, which realize the physic obability are given on the following page facility: environment temperature (22	es and are part of the certificate.
Calibration Equipment used (M&T	E critical for calibration)		
Primary Standards	ID#	Cal Date (Calibrated by, Certificate N	
luke Process Calibrator Type 70 (eithley Multimeter Type 2001	2 SN: 6295803 SN: 0810278	13-Oct-06 (Elcal AG, No: 5492) 03-Oct-06 (Elcal AG, No: 5478)	0ct-07 0ct-07
econdary Standards	ID#	Check Date (in house)	Scheduled Check
Calibrator Box V1.1	SE UMS 006 AB 1004	25-Jun-07 (SPEAG, in house check)	In house check Jun-08
	Name Dominique Steffen	Function Technician	Signature D. Hoffin IN R. L. WIMM
Calibrated by:			

Report No. : ES/2008/40006 Page : 39 of 59

CALIBRATION CERTIFICATE Disect EX3DV3 - SN:3526 Calibration procedure(s) QA CAL-01.v6 Calibration procedure for dosimetric E-field probes Calibration date: August 29, 2007 Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.	fultilateral Agreement for the			
Silent SGS (Auden) Centificate No: EX3-3526_Aug07 CALIBRATION CERTIFICATE EX3DV3 - SN:3526 Object EX3DV3 - SN:3526 Calibration procedure(s) QA CAL-01:V6 Calibration procedure for dosimetric E-field probes Calibration date: August 29, 2007 Condition of the calibrated item In Tolerance This calibration centificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.		recognition of calibratio		
CALIBRATION CERTIFICATE Object EX3DV3 - SN:3526 Calibration procedure(s) QA CAL-01:v6 Calibration procedure for dosimetric E-field probes Calibration date: August 29, 2007 Condition of the calibrated item In Tolerance This calibration centificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.				
Calibration procedure(s) QA CAL-01.v6 Calibration procedure for dosimetric E-field probes Calibration date: August 29, 2007 Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (Si). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.	Client SGS (Auden)		Certificate No: E	EX3-3526_Aug07
Calibration procedure(s) QA CAL-01.v6 Calibration procedure for dosimetric E-field probes Calibration date: August 29, 2007 Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (Si). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.	CALIBRATION	CERTIFICAT	E	nie werden die
Calibration procedure for dosimetric E-field probes Calibration date: August 29, 2007 Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.	Object	EX3DV3 - SN:3	526	
Calibration procedure for dosimetric E-field probes Calibration date: August 29, 2007		01 01 01 0		
Calibration date: August 29, 2007 Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (Si). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.	Calibration procedure(s)	Concerning the second second second second	edure for dosimetric E-field probes	and the second
Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.		Common prov	source for occurrence is north propose	A STATUTE
Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			And the second sec	1. 1. 1. 1. 1. 1. 1. 1. 1. 1. 1. 1. 1. 1
Condition of the calibrated item In Tolerance This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.	Calibration date:	August 29, 200	7	
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.		magan sa, saa		
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.	Condition of the calibrated item	In Tolerance	State of the second state	and the second se
All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)*C and humidity < 70%.				The second se
All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)*C and humidity < 70%.				The second se
				The second se
	The measurements and the unc	ertainties with confidence	probability are given on the following pages and an	e part of the certificate.
Calibration Equipment used (M&TE critical for calibration)	The measurements and the unc	ertainties with confidence	probability are given on the following pages and an	e part of the certificate.
	The measurements and the unc	ertainties with confidence ucted in the closed laborat	probability are given on the following pages and ar ory facility: environment temperature $(22\pm 3)^{\circ}$ C an	e part of the certificate.
	The measurements and the unc All calibrations have been cond Calibration Equipment used (M	entainties with confidence ucted in the closed laborat KTE critical for calibration)	probability are given on the following pages and an ony facility: environment temperature (22 ± 3)°C an	e part of the certificate. d humidity < 70%.
	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards	entainties with confidence ucted in the closed laborat STE critical for calibration) IID #	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.)	e part of the certificate. d humidity < 70%. Scheduled Calibration
	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198	ertainties with confidence ucted in the closed laborat \$TE critical for calibration) ID # GB41293874	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)*C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08
Power sensor E4412A MY41498087 29-Mar-07 (METAS: No. 217-00670) Mar-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter E44198 Power sensor E4412A	ertainties with confidence ucted in the closed laborat kTE critical for calibration) IID # GB41293874 MY41495277	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)*C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-05
	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power mesor E4412A Power sensor E4412A	ertainties with confidence ucted in the closed laborat kTE critical for calibration) ID # GB41293874 MY41495087 MY41495087	probability are given on the following pages and an ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-06 Mar-06 Mar-08
Reference 3 dB Attenuator SN: \$5054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (M Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator	ertainties with confidence ucted in the closed laborat STE critical for calibration) aD # GB41293874 MY41495277 MY41495087 SN: S5054 (3c)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-05 Mar-08 Aug-08
Reference 3 dB Attenuator SN: S5054 (3c) 8-Aug-07 (METAS, No. 217-00716) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 d6 Attenuator Reference 20 d8 Attenuator	entainties with confidence ucted in the closed liaborat STE critical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: 55054 (3c) SN: 55056 (20b)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-06 Mar-08 Aug-08 Mar-08 Mar-08
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00710) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5129 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-08	The measurements and the unc All calibration Equipment used (Mi Calibration Equipment used (Mi Primary Standards Power meters E44198 Power sensor E4419A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # 0841293874 MY41495277 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55056 (20b) SN: 55129 (30b)	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cali Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00716) 8-Aug-07 (METAS, No. 217-0071) 8-Aug-07 (METAS, No. 217-00720)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-05
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00710) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5129 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power mensor E4412A Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator	ertainties with confidence ucted in the closed laborat STE critical for calibration) BD # GB41293874 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 3013	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00701) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Mar-08 Aug-08 Jan-08
Reference 3 dB Attenuator SN: S5054 (3c) 8-Aug-07 (METAS, No. 217-00716) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-06 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08 DAE4 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: 55054 (3c) SN: 55086 (20b) SN: 55086 (20b) SN: 55129 (30b) SN: 5514	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-0070) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. DAE4-654, Apr07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Aug-08 Jan-08 Apr-08
Reference 3 dB Attenuator SN: S5054 (3c) 8-Aug-07 (METAS, No. 217-00716) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00710) Mar-08 Reference 30 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-05 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Schedulad Check	The measurements and the unc All calibration Equipment used (Mi Calibration Equipment used (Mi Primary Standards Power meters E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: 55054 (30) SN: 55054 (30) SN: 55129 (30b) SN: 55129 (30b)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00710) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. E53-3013_Jan07) 29-Apr-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Jan-08 Aug-08 Jan-08 Aug-08 Scheduled Check
Beference 3 dB Attenuator SN: S5054 (3c) 8-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00710) Mar-08 Reference 30 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00710) Mar-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013, Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642001700 4-Aug-09 (SPEAG, in house check Nov-05) in house check Nov-05)	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator NP 8648C	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB41293874 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 654 ID # US3642U01700	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 9-Mar-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-05)	e part of the certificate d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Aug-08 Jan-08 Aug-05 Jan-08 Aug-08 Scheduled Check In house check: Nov-07
Reference 3 dB Attenuator SN: S5054 (3c) 8-Aug-07 (METAS, No. 217-00716) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00716) Mar-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00710) Mar-08 Reference 30 dB Attenuator SN: S5056 (20b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8649C US3542U01700 4-Aug-99 (SPEAG, in house check Nor-05) In house check: Nor-07 Network Analyzer HP 8753E 18-Oct-01 (SPEAG, in house check Oct-06) In house check: Oct-07	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator NP 8648C	entainties with confidence ucted in the closed laborat STE critical for calibration)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C en Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. CE3-3013_Jan07) 29-Agr-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Oct-06)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00710) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00710) Aug-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SN: S5129 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-06 Reference 90 dB Attenuator SN: S5139 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-06 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. E53-3013_Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check 8F generator HP 8648C US3642001700 4-Aug-90 (SPEAG, in house check Nor-05) In house check: Nor-07 Vetwork Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Oct-06) In house check: Oct-07 Name Function Signature Signature Signature	The measurements and the unc All calibration Equipment used (Mi Calibration Equipment used (Mi Primary Standards Power meters E44198 Power sensor E4419A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Regenerator HP 8648C Network Analyzer HP 8763E	ertainties with confidence ucted in the closed laborat STE critical for calibration) BB # GB41293874 MY41495277 MY41495087 SN: 55054 (30) SN: 55054 (30) SN: 55129 (30b) SN: 55129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585 Name	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00710) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. E53-3013_Jan07) 29-Apr-07 (SPEAG, No. DA54-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-06) 18-Oct-01 (SPEAG, in house check Nov-06) 18-Oct-01 (SPEAG, in house check Nov-06)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00710) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00710) Aug-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SN: S5129 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-06 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check 8F generator HP 8648C US3642001700 4-Aug-90 (SPEAG, in house check Nor-05) in house check: Nor-07 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Oct-06) In house check: Oct-07 Name Function Signature Signature Signature	The measurements and the unc All calibration Equipment used (Mi Calibration Equipment used (Mi Primary Standards Power meters E44198 Power sensor E4419A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Regenerator HP 8648C Network Analyzer HP 8763E	ertainties with confidence ucted in the closed laborat STE critical for calibration) BB # GB41293874 MY41495277 MY41495087 SN: 55054 (30) SN: 55054 (30) SN: 55129 (30b) SN: 55129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585 Name	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00710) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. E53-3013_Jan07) 29-Apr-07 (SPEAG, No. DA54-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-06) 18-Oct-01 (SPEAG, in house check Nov-06) 18-Oct-01 (SPEAG, in house check Nov-06)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07
Beference 3 dB Attenuator SN: S5054 (3c) 8 Aug-07 (METAS, No. 217-00716) Aug-08 Reference 20 dB Attenuator SN: S5056 (20c) 29-Mar-07 (METAS, No. 217-00716) Aug-08 Reference 30 dB Attenuator SN: S5056 (20c) 29-Mar-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013, Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check Fe generator HP IR648C US3542U01700 4-Aug-99 (SPEAG, in house check Nov-05) In house check: Nov-07 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-05) In house check: Cct-07 Calibrated by: Name Function Signature	The measurements and the unc All calibration Equipment used (M Calibration Equipment used (M Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator NP 8648C Network Analyzer NP 8753E Calibrated by:	ertainties with confidence ucted in the closed laborat IID # GB41233874 MY41485277 MY41485087 MY41485087 SN: 55086(20b) SN: 55086(20b) SN: 55129(30b) SN: 55129(30b) SN: 5513 ID # US3642U01700 US37300585 Name Kalja Pokovic	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 9-Mar-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 9-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAQ, No. 253-3013_Jan07) 20-Apr-07 (SPEAQ, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAQ, in house check Nor-06) 18-Oct-01 (SPEAQ, in house check Oct-06) Function Technical Managet	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07
Beference 3 dB Attenuator SN: S5054 (3c) 8 Aug-07 (METAS, No. 217-00710) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29 Mar-07 (METAS, No. 217-00710) Aug-08 Reference 30 dB Attenuator SN: S5056 (20b) 29 Mar-07 (METAS, No. 217-00710) Aug-08 Reference 30 dB Attenuator SN: S5059 (20b) 29 Mar-07 (METAS, No. 217-00710) Aug-08 Reference 30 dB Attenuator SN: S5129 (20b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 SN: S5129 (20b) SN: S13 4-Jan-07 (SPEAG, No. ES3-3013, Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check Reference HP 8648C US3642U01700 4-Aug-99 (SPEAG, in house check Nor-05) In house check: Nor-07 Vetwork Analyzer HP 8753E US3642U01700 4-Aug-99 (SPEAG, in house check Oct-06) In house check: Oct-07 Calibrated by: Name Function Signature	The measurements and the unc All calibration Equipment used (M Calibration Equipment used (M Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator NP 8648C Network Analyzer NP 8753E Calibrated by:	ertainties with confidence ucted in the closed laborat IID # GB41233874 MY41485277 MY41485087 MY41485087 SN: 55086(20b) SN: 55086(20b) SN: 55129(30b) SN: 55129(30b) SN: 5513 ID # US3642U01700 US37300585 Name Kalja Pokovic	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 9-Mar-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 9-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAQ, No. 253-3013_Jan07) 20-Apr-07 (SPEAQ, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAQ, in house check Nor-06) 18-Oct-01 (SPEAQ, in house check Oct-06) Function Technical Managet	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07
	The measurements and the unc All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter E44198 Power sensor E4412A	ertainties with confidence ucted in the closed laborat kTE critical for calibration) IID # GB41293874 MY41495277	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)*C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-06
Power sensor E4412A MY41498087 29-Mar-07 (METAS, No. 217-00670) Mar-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (M Primary Standards Power meter E44198 Power sensor E4412A	ertainties with confidence ucted in the closed laborat kTE critical for calibration) IID # GB41293874 MY41495277	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)*C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-05
	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power mesor E4412A Power sensor E4412A	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB41293874 MY41495087 MY41495087	probability are given on the following pages and an ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-06 Mar-06 Mar-08
	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power ensore E4412A Power sensor E4412A	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB41293874 MY41495087 MY41495087	probability are given on the following pages and an ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-06 Mar-06 Mar-08
Reference 3 dB Attenuator SN: \$5054 (3c) 8-Aug-07 (METAS, No. 217-00719) Aug-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (M Primary Standards Vower menter E44198 Power sensor E4412A Vower sensor E4412A Reference 3 dB Attenuator	ertainties with confidence ucted in the closed laborat STE critical for calibration) aD # GB41293874 MY41495277 MY41495277 SN: S5054 (3c)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-05 Mar-08 Aug-08
Reference 3 dB Attenuator SN: \$5054 (3c) 8-Aug-07 (METAS, No. 217-00719) Aug-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (M Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator	ertainties with confidence ucted in the closed laborat STE critical for calibration) aD # GB41293874 MY41495277 MY41495277 SN: S5054 (3c)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-05 Mar-08 Aug-08
Reference 3 dB Attenuator SN: \$5054 (3c) 8-Aug-07 (METAS, No. 217-00719) Aug-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (M Primary Standards Vower menter E44198 Power sensor E4412A Vower sensor E4412A Reference 3 dB Attenuator	ertainties with confidence ucted in the closed laborat STE critical for calibration) aD # GB41293874 MY41495277 MY41495277 SN: S5054 (3c)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-05 Mar-08 Aug-08
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 GB Attenuator Reference 20 dB Attenuator	entainties with confidence ucted in the closed liaborat STE critical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: 55054 (3c) SN: 55056 (20b)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-06 Mar-08 Aug-08 Mar-08 Mar-08
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00710) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08	The measurements and the unc All calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	entainties with confidence ucted in the closed liaborat STE critical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: 55054 (3c) SN: 55056 (20b)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-06 Mar-08 Aug-08 Mar-08 Mar-08
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00710) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08	The measurements and the unc All calibration Equipment used (Mi Calibration Equipment used (Mi Primary Standards Power meters 44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # 0841293874 MY41495277 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55056 (20b) SN: 55129 (30b)	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cali Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00716) 8-Aug-07 (METAS, No. 217-0071) 8-Aug-07 (METAS, No. 217-00720)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-05
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00710) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08	The measurements and the unc All calibration Equipment used (Mi Calibration Equipment used (Mi Primary Standards Power meters 44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # 0841293874 MY41495277 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55056 (20b) SN: 55129 (30b)	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cali Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00716) 8-Aug-07 (METAS, No. 217-0071) 8-Aug-07 (METAS, No. 217-00720)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-05
Reference 3 dB Attenuator SN: 55054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5129 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power sensor E4412A Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator	ertainties with confidence ucted in the closed laborat STE critical for calibration) BD # GB41293874 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 3013	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00701) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-05
Reference 3 dB Attenuator SN: 55054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5129 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power sensor E4412A Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator	ertainties with confidence ucted in the closed laborat STE critical for calibration) BD # GB41293874 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 3013	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00701) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Mar-08 Aug-08 Jan-08
Reference 3 dB Attenuator SN: 55054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08	The measurements and the uncellibration Equipment used (Mi Calibration Equipment used (Mi Primary Standards Power ensore E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2	ertainties with confidence ucted in the closed laborat STE critical for calibration) BD # GB41293874 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 3013	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00701) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Mar-08 Aug-08 Jan-08
Reference 3 dB Attenuator SN: 55054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08	The measurements and the uncellibration Equipment used (Mi Calibration Equipment used (Mi Primary Standards Power ensore E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2	ertainties with confidence ucted in the closed laborat STE critical for calibration) BD # GB41293874 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 3013	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00701) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Mar-08 Aug-08 Jan-08
Reference 3 dB Attenuator SN: 55054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5129 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power sensor E4412A Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator	ertainties with confidence ucted in the closed laborat STE critical for calibration) BD # GB41293874 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 3013	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-00701) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Mar-08 Aug-08 Jan-08
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00710) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-0071) Mar-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-06 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-06 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08 AAE SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meters E4412A Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: 55054 (3c) SN: 55086 (20b) SN: 55086 (20b) SN: 55129 (30b) SN: 5514	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 29-Mar-07 (METAS, No. 217-0070) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. DAE4-654, Apr07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Aug-08 Jan-08 Apr-08
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-0071) Mar-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-05 Reference 30 dB Attenuator SN: S5129 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-05 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08 AAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (In house) Scheduled Check	The measurements and the unc All calibration Equipment used (Mi Calibration Equipment used (Mi Primary Standards Power meters E44198 Power sensor E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: 55054 (30) SN: 55054 (30) SN: 55129 (30b) SN: 55129 (30b)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00710) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. E53-3013_Jan07) 29-Apr-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Jan-08 Aug-08 Jan-08 Aug-08 Scheduled Check
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-0071) Mar-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-05 Reference 30 dB Attenuator SN: S5129 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-05 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08 AAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (In house) Scheduled Check	The measurements and the unc All calibration Equipment used (Mi Calibration Equipment used (Mi Primary Standards Power meters E44198 Power sensor E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: 55054 (30) SN: 55054 (30) SN: 55129 (30b) SN: 55129 (30b)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00710) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. E53-3013_Jan07) 29-Apr-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Jan-08 Aug-08 Jan-08 Aug-08 Scheduled Check
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-0071) Mar-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-06 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-06 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013, Jan07) Jan-08 AE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654, Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check SF generator HP 8648C US3542U01700 4-Aug-99 (SPEAG, in house check Nor-05) In house check: Nor-07	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power ensore E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB41293874 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 654 ID # US3642U01700	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00710) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-05)	e part of the certificate d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Aug-08 Jan-08 Aug-05 Jan-08 Aug-08 Scheduled Check In house check: Nov-07
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-0071) Mar-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-06 Reference 30 dB Attenuator SN: S5129 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-06 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013, Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8649C US3542U01700 4-Aug-99 (SPEAG, in house check Nor-05) In house check: Nor-07	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Reference Probe ES3DV2	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB41293874 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 654 ID # US3642U01700	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00710) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-05)	e part of the certificate d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Aug-08 Jan-08 Aug-05 Jan-08 Aug-08 Scheduled Check In house check: Nov-07
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-0071) Mar-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-06 Reference 30 dB Attenuator SN: S5129 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-06 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013, Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8649C US3542U01700 4-Aug-99 (SPEAG, in house check Nor-05) In house check: Nor-07	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Reference Probe ES3DV2	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB41293874 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 654 ID # US3642U01700	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 9-Mar-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-05)	e part of the certificate d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Aug-08 Jan-08 Aug-05 Jan-08 Aug-08 Scheduled Check In house check: Nov-07
Reference 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00719) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-0071) Mar-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-06 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-06 Reference Probe ES3DV2 SN: 3013 4-Jan-07 (SPEAG, No. ES3-3013, Jan07) Jan-08 AE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654, Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check SF generator HP 8648C US3542U01700 4-Aug-99 (SPEAG, in house check Nor-05) In house check: Nor-07	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power ensore E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4	ertainties with confidence ucted in the closed laborat STE critical for calibration) ID # GB41293874 MY41495087 SN: 55054 (3c) SN: 55054 (3c) SN: 55129 (30b) SN: 55129 (30b) SN: 654 ID # US3642U01700	probability are given on the following pages and ar ony facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00719) 9-Mar-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-05)	e part of the certificate d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Mar-08 Aug-08 Aug-08 Jan-08 Aug-05 Jan-08 Aug-08 Scheduled Check In house check: Nov-07
Baference 3 dB Attenuator SN: S5054 (3c) 8-Aug-07 (METAS, No. 217-00716) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00671) Mar-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: S513 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-09 (SPEAG, in house check Nov-05) In house check: Nov-07 Network Analyzer HP 8753E 18-Oct-01 (SPEAG, in house check Oct-06) In house check: Oct-07	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator NP 8648C	entainties with confidence ucted in the closed laborat STE critical for calibration)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C en Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00710) 29-Mar-07 (METAS, No. 217-00710) 29-Mar-07 (METAS, No. 217-00710) 29-Mar-07 (METAS, No. 217-00671) 8-Aug-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Oct-06)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07
Batterence 3 dB Attenuator SN: S5054 (3c) B-Aug-07 (METAS, No. 217-00716) Aug-08 Reference 20 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00717) Mar-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SN: S5129 (30b) B-Aug-07 (METAS, No. 217-00720) Aug-06 Reference Probe ES3DV2 SN: S513 4-Jan-07 (SPEAG, No. ES3-3013_Jan077) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-09 (SPEAG, in house check Nor-05) In house check: Nor-07 Network Analyzer HP 8753E 18-Oct-01 (SPEAG, in house check Oct-06) In house check: Oct-07	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	entainties with confidence ucted in the closed laborat STE critical for calibration)	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C en Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00710) 29-Mar-07 (METAS, No. 217-00710) 29-Mar-07 (METAS, No. 217-00710) 29-Mar-07 (METAS, No. 217-00671) 8-Aug-07 (SPEAG, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-05) 18-Oct-01 (SPEAG, in house check Oct-06)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07
Bit SN: S5054 (3c) 8-Aug-07 (METAS, No. 217-00716) Aug-08 Reference 30 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00710) Aug-08 Reference 30 dB Attenuator SN: S5086 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SN: S5128 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: S013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator NP 8649C US3642001700 4-Aug-98 (SPEAG, in house check Nov-05) In house check: Nov-07 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Oct-06) In house check: Oct-07 Name Function Signature Signature Signature	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	ertainties with confidence ucted in the closed laborat STE critical for calibration) BB # GB41293874 MY41495277 MY41495087 SN: 55054 (30) SN: 55054 (30) SN: 55129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585 Name	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00710) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. E53-3013_Jan07) 29-Apr-07 (SPEAG, No. DA54-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-06) 16-Oct-01 (SPEAG, in house check Nov-06) 16-Oct-01 (SPEAG, in house check Nov-06)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07
Bit SN: S5054 (3c) 8-Aug-07 (METAS, No. 217-00710) Aug-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00710) Aug-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: S013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (SPEAG, in house check Nov-05) In house check: Nov-07 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Oct-06) In house check: Oct-07 Name Function Signature Signature Signature	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	ertainties with confidence ucted in the closed laborat STE critical for calibration) BB # GB41293874 MY41495277 MY41495087 SN: 55054 (30) SN: 55054 (30) SN: 55129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585 Name	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00710) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. E53-3013_Jan07) 29-Apr-07 (SPEAG, No. DA54-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-06) 16-Oct-01 (SPEAG, in house check Nov-06) 16-Oct-01 (SPEAG, in house check Nov-06)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07
Bit SN: S5054 (3c) 8-Aug-07 (METAS, No. 217-00710) Aug-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00710) Aug-08 Reference 30 dB Attenuator SN: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe ES3DV2 SN: S013 4-Jan-07 (SPEAG, No. ES3-3013_Jan07) Jan-08 DAE4 SN: 654 20-Apr-07 (SPEAG, No. DAE4-654_Apr07) Apr-08 Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-99 (SPEAG, in house check Nov-05) In house check: Nov-07 Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Oct-06) In house check: Oct-07 Name Function Signature Signature Signature	The measurements and the unc All calibrations have been cond Calibration Equipment used (Mi Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	ertainties with confidence ucted in the closed laborat STE critical for calibration) BB # GB41293874 MY41495277 MY41495087 SN: 55054 (30) SN: 55054 (30) SN: 55129 (30b) SN: 3013 SN: 654 ID # US3642U01700 US37390585 Name	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00710) 8-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAG, No. E53-3013_Jan07) 29-Apr-07 (SPEAG, No. DA54-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAG, in house check Nov-06) 16-Oct-01 (SPEAG, in house check Nov-06) 16-Oct-01 (SPEAG, in house check Nov-06)	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07
Reference 3 dB Attenuator SR: S5054 (3c) 8-Aug-07 (METAS, No. 217-00716) Aug-08 Reference 30 dB Attenuator SR: S5056 (20b) 29-Mar-07 (METAS, No. 217-00716) Aug-08 Reference 30 dB Attenuator SR: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SR: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe E53DV2 SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 DAE4 SN: S513 4-Jan-07 (SPEAG, No. E53-3013, Jan07) Jan-08 Secondary Standards ID # Check Date (in house) Scheduled Check Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-96 (SPEAG, in house check Nor-05) In house check: Nor-07 Network Analyzer HP 8753E US37390585 16-Oct-01 (SPEAG, in house check Oct-06) In house check: Oct-07 Name Function Signature Calibrated by: Name Function	The measurements and the unc All calibrations have been cond Calibration Equipment used (M Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E Calibrated by:	ertainties with confidence ucted in the closed laborat IID # GB41233874 MY41485277 MY41485087 MY41485087 SN: 55086(20b) SN: 55086(20b) SN: 55129(30b) SN: 55129(30b) SN: 55129(30b) SN: 654 ID # US3642U01700 US37300585 Name Katja Pokovic	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 9-Mar-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 9-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAQ, No. 233-0013_Jan07) 20-Apr-07 (SPEAQ, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAQ, in house check Nor-06) 18-Oct-01 (SPEAQ, in house check Oct-06) Function Technical Manager	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07
Reference 3 dB Attenuator SR: S5054 (3c) 8-Aug-07 (METAS, No. 217-00716) Aug-08 Reference 30 dB Attenuator SR: S5056 (20b) 29-Mar-07 (METAS, No. 217-00716) Aug-08 Reference 30 dB Attenuator SR: S5056 (20b) 29-Mar-07 (METAS, No. 217-00720) Aug-08 Reference 30 dB Attenuator SR: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 Reference Probe E53DV2 SN: S5129 (30b) 8-Aug-07 (METAS, No. 217-00720) Aug-08 DAE4 SN: S513 4-Jan-07 (SPEAG, No. E53-3013, Jan07) Jan-08 Secondary Standards ID # Check Date (in house) Scheduled Check Secondary Standards ID # Check Date (in house) Scheduled Check RF generator HP 8648C US3642U01700 4-Aug-96 (SPEAG, in house check Nor-05) In house check: Nor-07 Network Analyzer HP 8753E US37390585 16-Oct-01 (SPEAG, in house check Oct-06) In house check: Oct-07 Name Function Signature Calibrated by: Name Function	The measurements and the unc All calibrations have been cond Calibration Equipment used (M Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E Calibrated by:	ertainties with confidence ucted in the closed laborat IID # GB41233874 MY41485277 MY41485087 MY41485087 SN: 55086(20b) SN: 55086(20b) SN: 55129(30b) SN: 55129(30b) SN: 55129(30b) SN: 654 ID # US3642U01700 US37300585 Name Katja Pokovic	probability are given on the following pages and ar ory facility: environment temperature (22 ± 3)°C an Cal Date (Calibrated by, Certificate No.) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 29-Mar-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00670) 8-Aug-07 (METAS, No. 217-00671) 9-Mar-07 (METAS, No. 217-00671) 8-Aug-07 (METAS, No. 217-00671) 9-Aug-07 (METAS, No. 217-00720) 4-Jan-07 (SPEAQ, No. 233-0013_Jan07) 20-Apr-07 (SPEAQ, No. DAE4-654_Apr07) Check Date (in house) 4-Aug-09 (SPEAQ, in house check Nor-06) 18-Oct-01 (SPEAQ, in house check Oct-06) Function Technical Manager	e part of the certificate. d humidity < 70%. Scheduled Calibration Mar-08 Mar-08 Aug-08 Aug-08 Aug-08 Jan-08 Apr-08 Scheduled Check In house check: Nov-07 In house check: Oct-07

Calibration Laboratory of Schmid & Partner Engineering AG aughausstrasse 43, 8004 Zurich, Switzerla Zeug



SHISS

U

CRUBRAL S

S

S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

Globbally.	
TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
Polarization o	o rotation around probe axis
Polarization 9	9 rotation around an axis that is in the plane normal to probe axis (at
	measurement center), i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx, y, z does not effect the E2-field uncertainty inside TSL (see below ConvF)
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This ٠ linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx, y, z: DCP are numerical linearization parameters assessed based on the data of ٠ power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: EX3-3526_Aug07

Page 2 of 9

Report No. : ES/2008/40006 Page : 41 of 59

EX3DV3 SN:3526

August 29, 2007

Probe EX3DV3

SN:3526

Manufactured: Last calibrated: Recalibrated: March 19, 2004 August 25, 2006 August 29, 2007

Calibrated for DASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: EX3-3526_Aug07

Page 3 of 9

EX3DV3 SN:3526

August 29, 2007

DASY - Parameters of Probe: EX3DV3 SN:3526

Sensitivity in Free Space^A

Diode Compression^B

NormX	0.991 ± 10.1%	μV/(V/m) ²	DCP X	97 mV	
NormY	0.807 ± 10.1%	$\mu V/(V/m)^2$	DCP Y	96 mV	
NormZ	0.876 ± 10.1%	μV/(V/m) ²	DCP Z	97 mV	

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

Boundary Effect

TSL

900 MHz Typical SAR gradient: 5 % per mm

Sensor Cente	r to Phantom Surface Distance	2.0 mm	3.0 mm
SAR _{be} [%]	Without Correction Algorithm	1.5	0.5
SARee [%]	With Correction Algorithm	0.3	0.4

TSL 1810 MHz Typical SAR gradient: 10 % per mm

Sensor Cente	r to Phantom Surface Distance	2.0 mm	3.0 mm
SAR _{be} [%]	Without Correction Algorithm	3.0	1.5
SAR _{be} [%]	With Correction Algorithm	0.2	0.1

Sensor Offset

Probe Tip to Sensor Center

1.0 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

⁴ The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 8).

* Numerical linearization parameter: uncertainty not required.

Certificate No: EX3-3526_Aug07


Page 4 of 9

Report No. : ES/2008/40006 Page : 43 of 59

EX3DV3 SN:3526

August 29, 2007



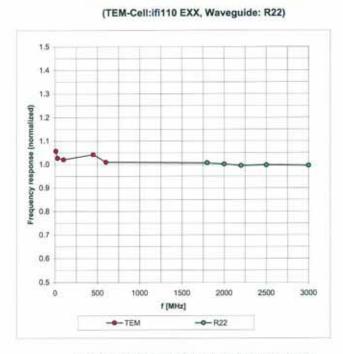


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: EX3-3526_Aug07


Page 5 of 9

EX3DV3 SN:3526

August 29, 2007

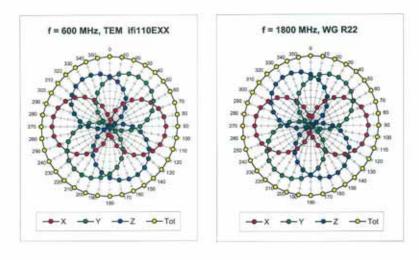

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

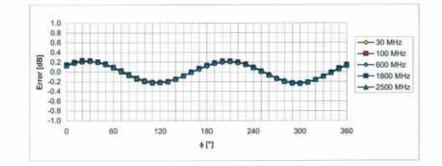


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: EX3-3526_Aug07

Page 6 of 9

Report No. : ES/2008/40006 Page : 45 of 59

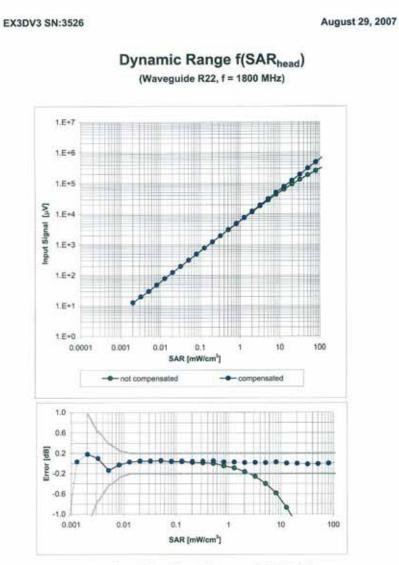


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: EX3-3526_Aug07

Page 7 of 9

EX3DV3 SN:3526

August 29, 2007

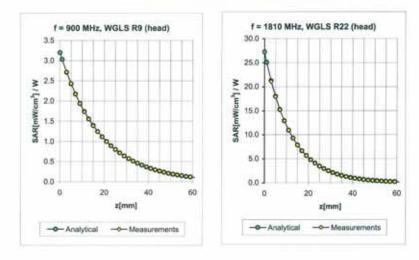


Conversion Factor Assessment

f [MHz]	Validity [MHz] ^c	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF	Uncertainty
900	± 50 / ± 100	Head	41.5±5%	0.97 ± 5%	0.50	0.80	11.48	± 11.0% (k=2)
1810	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.15	1.32	9.30	± 11.0% (k=2)
1950	± 50 / ± 100	Head	40.0 ± 5%	$1.40 \pm 5\%$	0.22	1.01	8.91	± 11.0% (k=2)
2450	± 507±100	Head	39.2 ± 5%	1.80 ± 5%	0.34	1.00	8.42	± 11.8% (k=2
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.50	0.80	10.93	± 11.0% (k=2
1810	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0,16	1.28	9.04	± 11.0% (k=2
1950	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.15	1.43	8.67	± 11.0% (k=2
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.38	1.00	8.08	± 11.8% (k=2

^C The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Certificate No: EX3-3526_Aug07

Report No. : ES/2008/40006 Page : 47 of 59

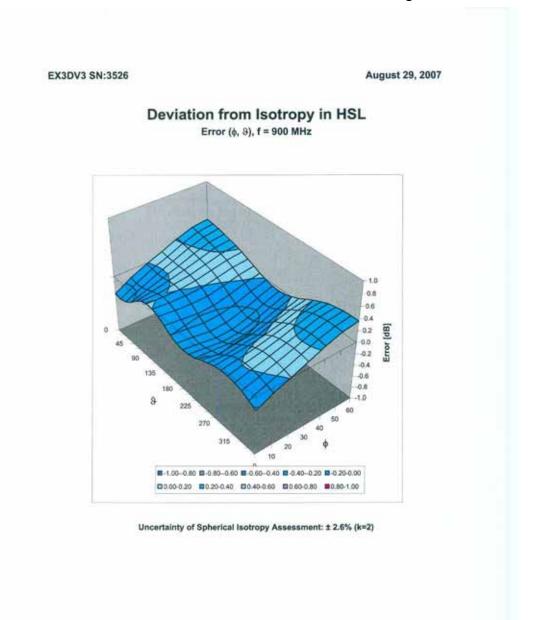

Certificate No: EX3-3526_Aug07

Page 9 of 9

ï

6.2 Uncertainty Analysis

1

Error Description	Uncertainty value	Prob. Dist.	Div.	$\begin{pmatrix} (c_i) \\ 1g \end{pmatrix}$	$\begin{pmatrix} (c_i) \\ 10g \end{pmatrix}$	Std. Unc. (1g)	Std. Unc. (10g)	$\left \begin{array}{c} (v_i) \\ v_{eff} \end{array} \right $
Measurement System			-					
Probe Calibration	$\pm 4.8\%$	N	1	1	1	$\pm 4.8\%$	$\pm 4.8\%$	∞
Axial Isotropy	±4.7 %	R	$\sqrt{3}$	0.7	0.7	$\pm 1.9\%$	$\pm 1.9 \%$	∞
Hemispherical Isotropy	$\pm 9.6 \%$	R	$\sqrt{3}$	0.7	0.7	$\pm 3.9\%$	$\pm 3.9\%$	∞
Boundary Effects	$\pm 1.0 \%$	R	$\sqrt{3}$	1	1	$\pm 0.6 \%$	$\pm 0.6 \%$	∞
Linearity	$\pm 4.7 \%$	R	$\sqrt{3}$	1	1	$\pm 2.7\%$	$\pm 2.7 \%$	∞
System Detection Limits	$\pm 1.0 \%$	R	$\sqrt{3}$	1	1	$\pm 0.6\%$	$\pm 0.6 \%$	∞
Readout Electronics	$\pm 1.0 \%$	N	1	1	1	$\pm 1.0\%$	$\pm 1.0 \%$	∞
Response Time	$\pm 0.8 \%$	R	$\sqrt{3}$	1	1	$\pm 0.5\%$	$\pm 0.5 \%$	∞
Integration Time	$\pm 2.6\%$	R	$\sqrt{3}$	1	1	$\pm 1.5 \%$	$\pm 1.5 \%$	∞
RF Ambient Conditions	$\pm 3.0 \%$	R	$\sqrt{3}$	1	1	±1.7%	±1.7 %	∞
Probe Positioner	$\pm 0.4\%$	R	$\sqrt{3}$	1	1	$\pm 0.2\%$	$\pm 0.2\%$	∞
Probe Positioning	$\pm 2.9\%$	R	$\sqrt{3}$	1	1	$\pm 1.7\%$	±1.7 %	∞
Max. SAR Eval.	$\pm 1.0 \%$	R	$\sqrt{3}$	1	1	$\pm 0.6\%$	$\pm 0.6\%$	∞
Test Sample Related								
Device Positioning	$\pm 2.9\%$	N	1	1	1	$\pm 2.9\%$	$\pm 2.9\%$	875
Device Holder	$\pm 3.6\%$	N	1	1	1	$\pm 3.6\%$	$\pm 3.6 \%$	5
Power Drift	$\pm 5.0 \%$	R	$\sqrt{3}$	1	1	$\pm 2.9\%$	$\pm 2.9 \%$	∞
Phantom and Setup								
Phantom Uncertainty	±4.0 %	R	$\sqrt{3}$	1	1	$\pm 2.3\%$	$\pm 2.3 \%$	∞
Liquid Conductivity (target)	$\pm 5.0 \%$	R	$\sqrt{3}$	0.64	0.43	$\pm 1.8 \%$	$\pm 1.2\%$	∞
Liquid Conductivity (meas.)	$\pm 2.5 \%$	N	1	0.64	0.43	$\pm 1.6 \%$	$\pm 1.1 \%$	∞
Liquid Permittivity (target)	$\pm 5.0 \%$	R	$\sqrt{3}$	0.6	0.49	$\pm 1.7 \%$	$\pm 1.4 \%$	∞
Liquid Permittivity (meas.)	$\pm 2.5 \%$	Ν	1	0.6	0.49	$\pm 1.5\%$	$\pm 1.2 \%$	∞
Combined Std. Uncertainty					1	$\pm 10.3 \%$	±10.0 %	331
Expanded STD Uncertain	ty					$\pm 20.6\%$	$\pm 20.1\%$	

6.3 Phantom Description

	8004 Zurich, Switzerland 00, Fax +41 1 245 9779	S	р	a	
info@speag.com, http	p://www.speag.com				

item	SAM Twin Phantom V4.0	
Type No	QD 000 P40 C	
Series No.	TP-1150 and higher	
Manufacturer	SPEAG Zeughausstrasse 43 CH-8004 Z0rich Switzerland	

Tests The series production process used allows the limitation to test of first articles. Complete tests were made on the pre-series Type No. QD 000 P40 AA, Serial No. TP-1001 and on the series first article Type No. QD 000 P40 BA, Serial No. TP-1006. Certain parameters have been retested using further series items (called samples) or are tested at each item.

Test	Requirement	Details	Units tested
Dimensions	Compliant with the geometry according to the CAD model.	IT'IS CAD File (*)	First article, Samples
Material thickness of shell	Compliant with the requirements according to the standards	2mm +/- 0.2mm in flat and specific areas of head section	First article, Samples, TP-1314 ff.
Material thickness at ERP	Compliant with the requirements according to the standards	6mm +/- 0.2mm at ERP	First article, All items
Material parameters	Dielectric parameters for required frequencies	300 MHz – 6 GHz: Relative permittivity < 5, Loss tangent < 0.05	Material samples
Material resistivity	The material has been tested to be compatible with the liquids defined in the standards if handled and cleaned according to the instructions. Observe technical Note for material compatibility.	DEGMBE based simulating liquids	Pre-series, First article, Material samples
Sagging	Compliant with the requirements according to the standards. Sagging of the flat section when filled with tissue simulating liquid.	< 1% typical < 0.8% if filled with 155mm of HSL900 and without DUT below	Prototypes, Sample testing

 Standards

 [1] CENELEC EN 50361

 [2] IEEE Std 1528-2003

 [3] IEC 62209 Part I

 [4] FCC OET Bulletin 65, Supplement C, Edition 01-01

 (*) The IT'IS CAD file is derived from [2] and is also within the tolerance requirements of the shapes of the other focuments

 the other documents.

Conformity Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of SAR measurements specified in standards [1] to [4].

07.07.2005

Date

Signature / Stamp

5 p ag 0

Schmid & Pagner Engineering AG 2703hausticess 43, 8054 Zuridi Switzeria Phone 141, 1345 8700 Par 44 v1 245 8779 Into Bapeag.com, http://www.speag.com

Doc No 881 - QD 000 P40 C - F

Page 1 (1)

6.4 System Validation from Original equipment supplier

DASY4 Validation Report for Body TSL

Date/Time: 17.04.2007 16:56:18

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 900 MHz; Type: D900V2; Serial: D900V2 - SN:168


Communication System: CW; Frequency: 900 MHz; Duty Cycle: 1:1 Medium: MSL U10BB; Medium parameters used: f = 900 MHz; $\sigma = 1.01$ mho/m; $\epsilon_r = 53$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 SN1507 (HF); ConvF(5.8, 5.8, 5.8); Calibrated: 19.10.2006
- · Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.01.2007
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin=250mW/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 54.8 V/m; Power Drift = 0.032 dB Peak SAR (extrapolated) = 3.58 W/kg SAR(1 g) = 2.58 mW/g; SAR(10 g) = 1.71 mW/g Maximum value of SAR (measured) = 2.77 mW/g

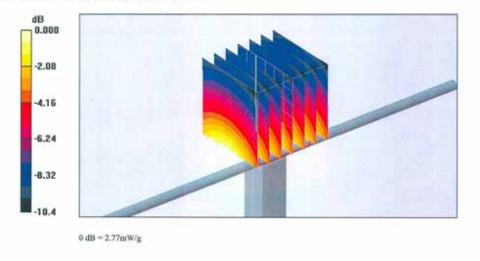

Certificate No: D900V2-168_Apr07

Report No. : ES/2008/40006 Page : 51 of 59

DASY4 Validation Report for Body TSL

Date/Time: 23.04.2007 16:11:04

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d018


Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1 Medium: MSL U10 BB; Medium parameters used: f = 1900 MHz; σ = 1.58 mho/m; ϵ_r = 52; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6 SN1507 (HF); ConvF(4.43, 4.43, 4.43); Calibrated: 19.10.2006
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.01.2007
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 88.3 V/m; Power Drift = 0.032 dB Peak SAR (extrapolated) = 15.7 W/kg SAR(1 g) = 9.55 mW/g; SAR(10 g) = 5.17 mW/g Maximum value of SAR (measured) = 10.7 mW/g

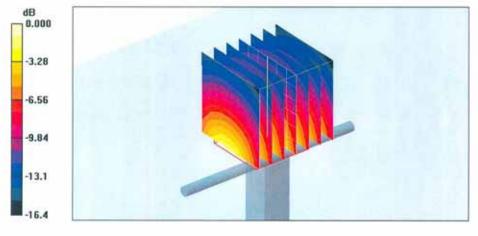

0 dB = 10.7mW/g

Certificate No: D1900V2-5d018_Apr07

DASY4 Validation Report for Body TSL

Date/Time: 24.04.2007 13:54:20

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN735


Communication System: CW-2450; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: MSL U10; Medium parameters used: f = 2450 MHz; σ = 1.92 mho/m; ϵ_r = 50.7; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025 (HF); ConvF(4.16, 4.16, 4.16); Calibrated: 19.10.2006
- · Sensor-Surface: 4mm (Mechanical Surface Detection)
- · Electronics: DAE4 Sn601; Calibrated: 30.01.2007
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA
- Measurement SW: DASY4, V4.7 Build 53; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 88.8 V/m; Power Drift = -0.060 dB Peak SAR (extrapolated) = 26.8 W/kg SAR(1 g) = 12.9 mW/g; SAR(10 g) = 5.95 mW/g Maximum value of SAR (measured) = 14.7 mW/g

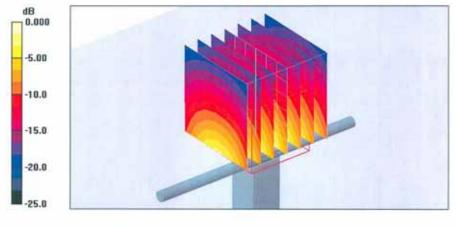

0 dB = 14.7 mW/g

Certificate No: D2450V2-735_Apr07

Report No. : ES/2008/40006 Page : 53 of 59

6.5 Photographs of Test Setup

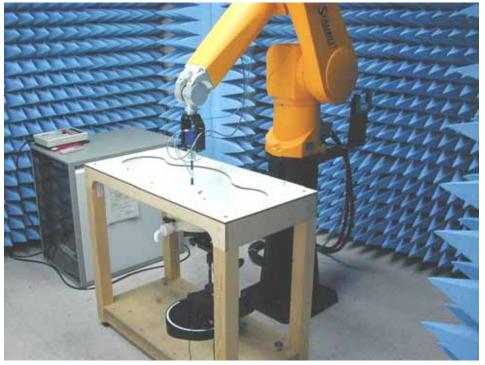


Fig.1 Photograph of the SAR measurement System

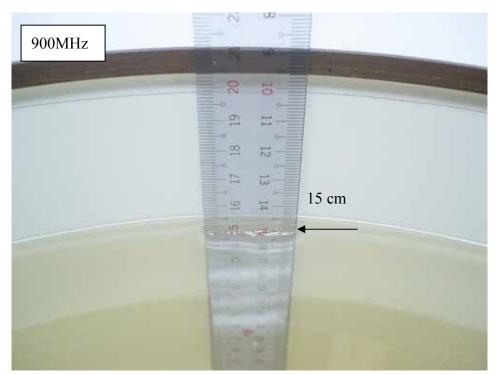


Fig.2.1 Photograph of the Tissue Simulant liquid depth 15cm for Flat position

Report No. : ES/2008/40006 Page : 54 of 59

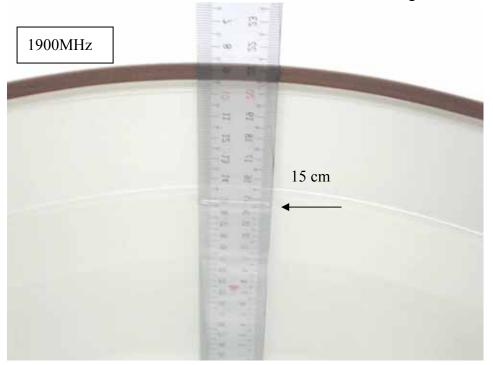


Fig.2.2 Photograph of the Tissue Simulant liquid depth 15cm for Flat position

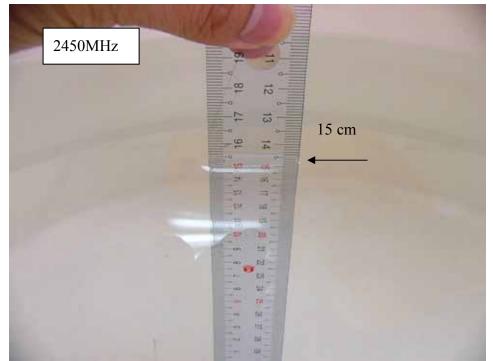


Fig.2.3 Photograph of the Tissue Simulant liquid depth 15cm for Flat position

Report No. : ES/2008/40006 Page : 55 of 59



Fig.3 Body worn- EUT back to flat phantom and distance between flat phantom and mobile phone is 1.5 cm



Fig.4 Body worn- EUT front to flat phantom and distance between flat phantom and mobile phone is 1.5 cm

Report No. : ES/2008/40006 Page : 56 of 59

6.6 Photographs of the EUT



Fig.5 Front view of device



Fig.6 Back view of device

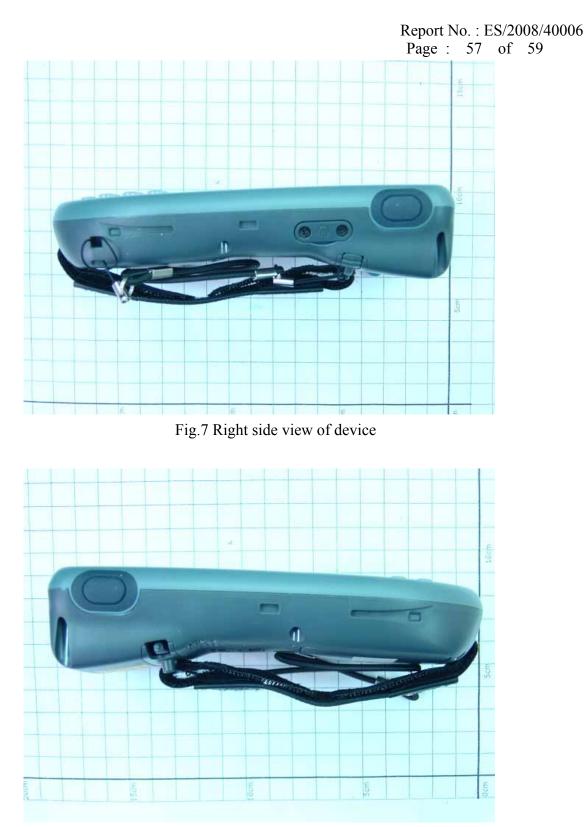


Fig.8 Left side view of device



Fig.9 AC Charger



Fig.10 Data cable

6.7 Photographs of the Battery



Fig.11 Front view of Battery



Fig.12 Back view of Battery

End of Report