

Contents

10.APPENDIX.....	120
10.1 Photographs of Test Setup.....	120
10.2. Photographs of the EUT	124

10.APPENDIX

10.1 Photographs of Test Setup

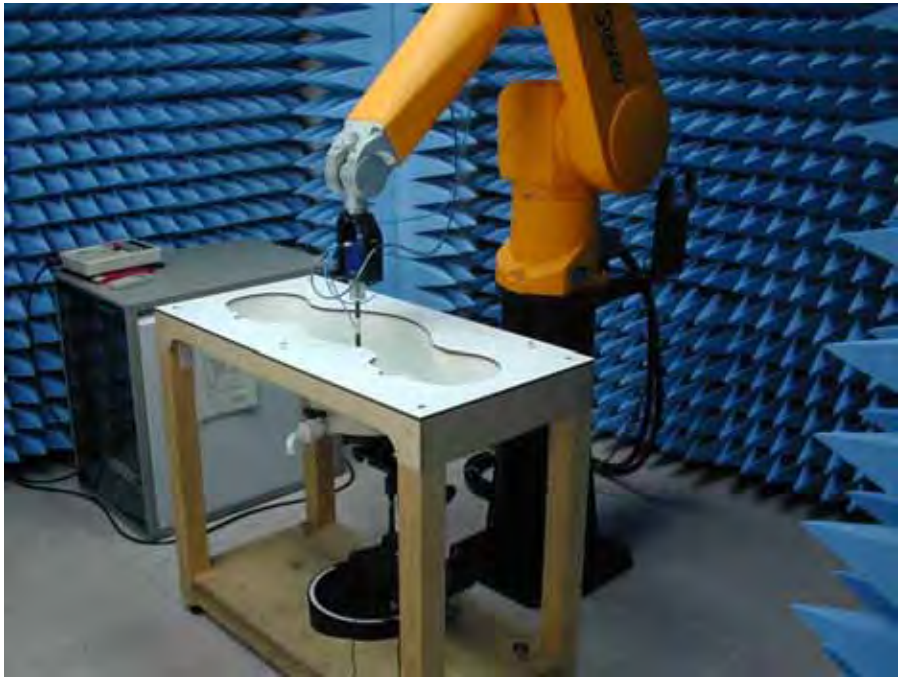


Fig.1 Photograph of the SAR measurement System

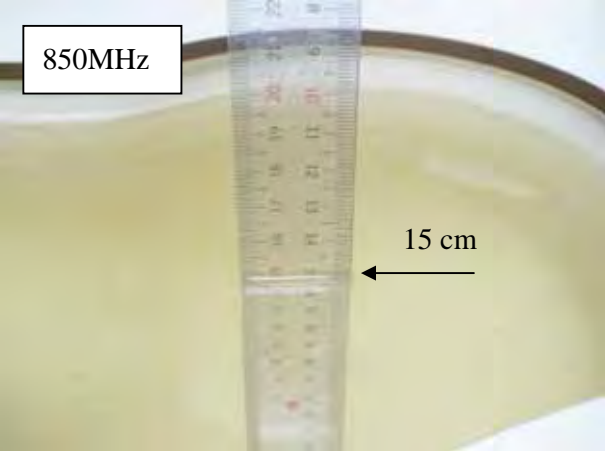


Fig.2.1 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Left-head Side

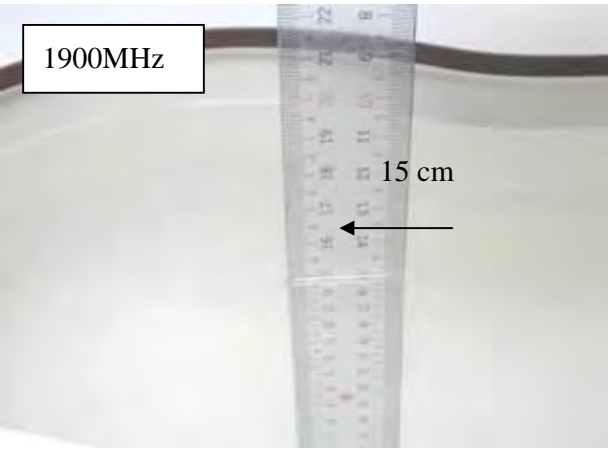


Fig.2.2 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Right-head Side

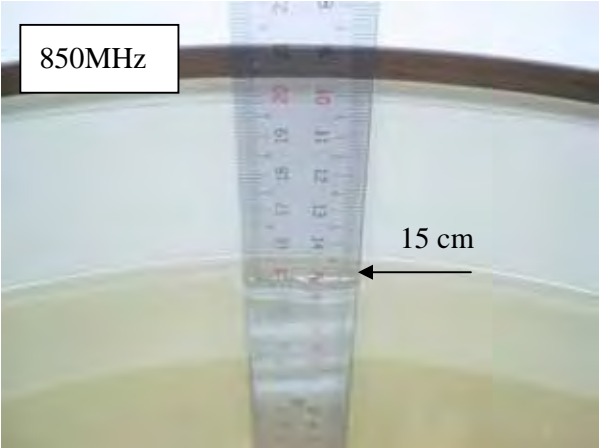


Fig.2.3 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

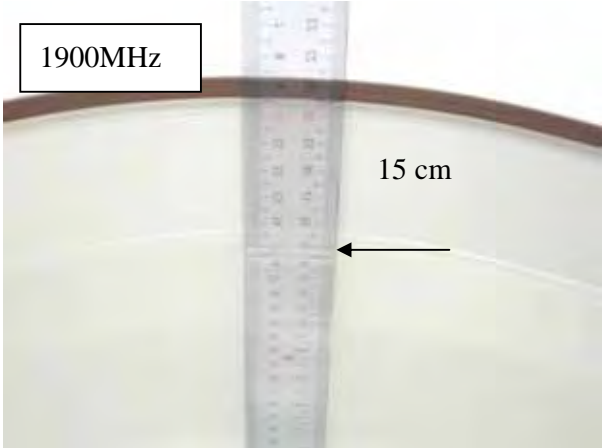


Fig.2.4 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

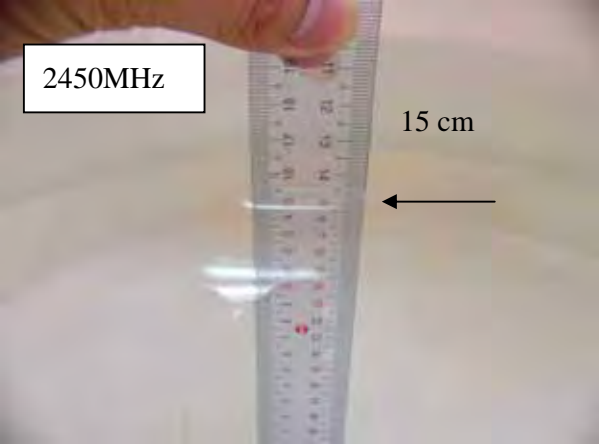


Fig.2.5 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)



Fig.3 Right Head Section / Cheek-Touch Position



Fig.4 Right Head Section / Ear-Tilt Position(15°)

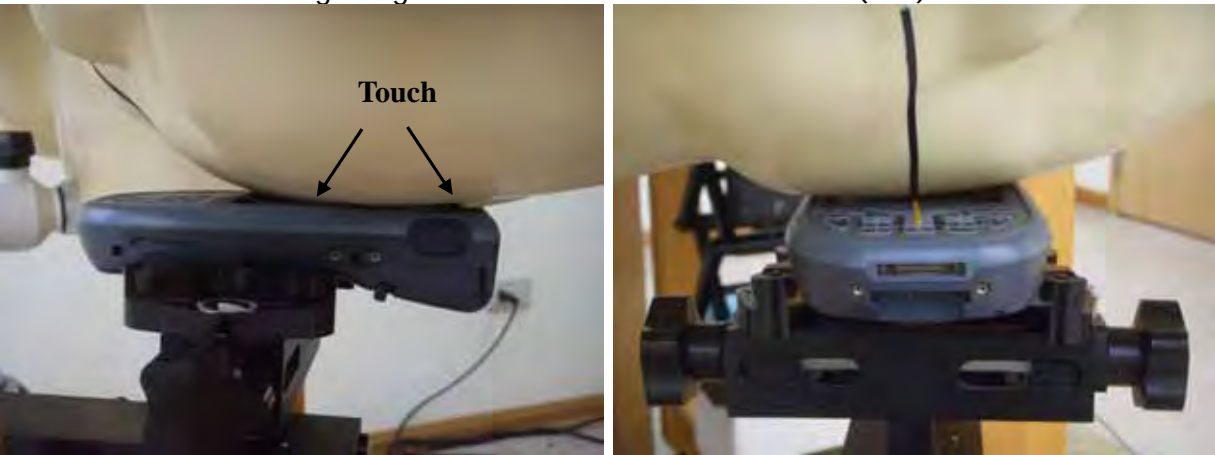


Fig.5 Left Head Section / Cheek-Touch Position



Fig.6 Left Head Section / Ear-Tilt Position(15°)



Fig.7 Body worn- EUT front to flat phantom and distance between flat phantom and mobile phone is 1.5 cm



Fig.8 Body worn- EUT back to flat phantom and distance between flat phantom and mobile phone is 1.5 cm

10.2. Photographs of the EUT



Fig.9 Front view of device



Fig.10 Back view of device



Fig.11 Right side view of device



Fig.12 Left side view of device

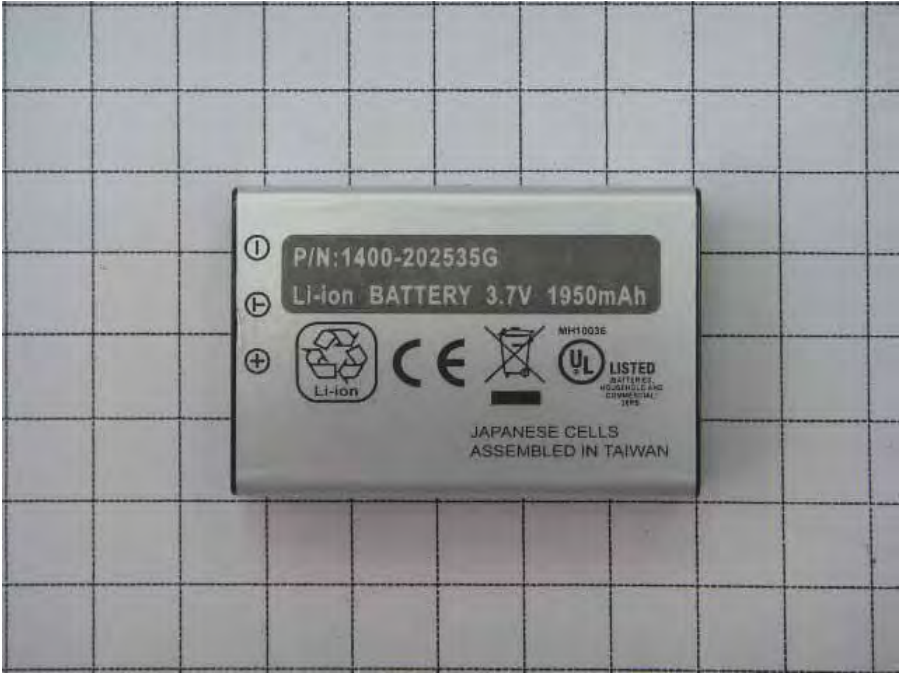


Fig.13 Front view of Battery



Fig.14 Back view of Battery



Fig.15 Charger

End of Report