SAR TEST REPORT

Equipment Under Test	802.11b/g/n RTL8191SE miniCard
Host Model Number	NAV50 , NAV60
FCC ID of WLAN module	HLZ-RTL8191SE
IC No. of WLAN module	1754F-RTL8191SE
Company Name	Acer Incorporated
Company Address	8F, 88,Sec,1,Hsin Tai Wu Rd. Hsichih Taipei Hsien 221
Date of Receipt	2010.01.27
Date of Test(s)	2010.02.04
Date of Issue	2010.02.24

Standards:

FCC OET 65 supplement C, IEEE /ANSI C95.1, C95.3, IEEE 1528, (KDB616217),RSS102

In the configuration tested, the EUT complied with the standards specified above. **Remarks**:

This report details the results of the testing carried out on one sample, the results contained in this test report do not relate to other samples of the same product. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report.

This report may only be reproduced and distributed in full. If the product in this report is used in any configuration other than that detailed in the report, the manufacturer must ensure the new system complies with all relevant standards. Any mention of SGS Taiwan Electronic & Communication Laboratory or testing done by SGS Taiwan Electronic & Communication Laboratory in connection with distribution or use of the product described in this report must be approved by SGS Taiwan Electronic & Communication Laboratory in writing.

×

		Andony	Wis			
Tested by	: Antony Wu	* *		Date	:	2010.02.24
	Engineer					
		Robert	Chang			
Approved by	: Robert Chang		0	Date	:	2010.02.24
	Tech Manager			_	_	

Contents

1.	General Information	. 3
	1.1 Testing Laboratory	. 3
	1.2 Details of Applicant	. 3
	1.3 Description of EUT	. 3
	1.4 Test Environment	. 6
	1.5 Operation description	. 6
	1.6 The SAR Measurement System	. 7
	1.7 System Components	. 8
	1.8 SAR System Verification	10
	1.9 Tissue Simulant Fluid for the Frequency Band	11
	1.10 Evaluation Procedures	12
	1.11 Test Standards and Limits	13
2.	Summary of Results	16
3.	Instruments List	17
4.	Measurements	18
5.	SAR System Performance Verification	23
6.	DAE & Probe Calibration certificate	24
7.	Uncertainty Analysis	34
8.	Phantom Description	36
9.	System Validation from Original equipment supplier	37

1. General Information

1.1 Testing Laboratory

SGS Taiwan Ltd. Electronics & Communication Laboratory			
134, Wu Kung Road, Wuku industrial zone			
Taipei county, Taiw	Taipei county, Taiwan, R.O.C.		
Telephone	+886-2-2299-3279		
Fax +886-2-2298-0488			
Internet <u>http://www.tw.sgs.com</u>			

1.2 Details of Applicant

Name	Acer Incorporated
Address	8F, 88,Sec,1,Hsin Tai Wu Rd. Hsichih Taipei Hsien 221

1.3 Description of EUT

EUT Name	802.11b/g/n RTL8191SE miniCard
Host Model Number	NAV50 , NAV60
Brand Name	Acer. Gateway, Packard Bell
FCC ID of WLAN	HLZ-RTL8191SE
IC No. of WLAN	1754F-RTL8191SE
Definition	Production unit
Mode of Operation	WLAN 802.11 b/g/n band

Duty Cycle	WLAN 802	11 b/g/n	
	1		
TX Frequency range	WLAN802.11 b/g/n(20M)	WLAN802.11n(40M)	
(MHz)	2412-2462	2422-2452	
Channel Number	WLAN802.11 b/g/n	WLAN802.11n(40M)	
(ARFCN)	1-11	3-9	
Power Supply	11.1Vdc re-charg	eable battery or	
	12Vdc by AC/D	C power adapter	
	WLAN8	02.11b	
	0.021W/kg		
	(WLAN802.11b _ CH1_ Configuration 1)		
	WLAN802.11g		
	0.00884W/kg		
Max. SAR Measured	(WLAN802.11g _ CH1_ Configuration 1)		
(1g)	WLAN802.11n (20M)		
	0.00777W/kg		
	(WLAN802.11n(20M) _	CH6_ Configuration 1)	
	WLAN802.11n(40M)		
	0.00877W/kg		
	(WLAN802.11n(40M) _	CH3_ Configuration 1)	

Note : 1. The 1-g SAR for the highest output channel is less than 0.8 W/kg, where the transmission band corresponding to all channels is ≤ 100 MHz, testing for the other channels is not required.

Report No. : ES/2010/10012 Page : 5 of 51

EUT Mode	Frequency (MHz)	СН	Peak Power (dBm)	Average Power (dBm)
WLAN802.11b	2412	1	18.11	15.24
	2437	6	17.62	15.08
	2462	11	17.72	15.05

2. WLAN802.11 b/g/n Conducted power :

EUT Mode	Frequency (MHz)	СН	Peak Power (dBm)	Average Power (dBm)
WLAN802.11g	2412	1	16.54	14.13
	2437	6	16.52	13.97
	2462	11	15.15	12.54

EUT Mode	Frequency (MHz)	СН	Peak Power (dBm)	Average Power (dBm)
WLAN802.11n (20M)	2412	1	16.39	13.77
	2437	6	16.48	13.90
(20101)	2462	11	15.07	12.68

EUT Mode	Frequency (MHz)	СН	Peak Power (dBm)	Average Power (dBm)
WLAN802.11n (40M)	2412	3	16.52	14.19
	2437	6	16.49	14.01
(40101)	2452	9	14.50	11.95

1.4 Test Environment

Ambient Temperature: 22±2° C Tissue Simulating Liquid: 22±2° C

1.5 Operation description

Use chipset specific software to control the EUT, and makes it transmit in maximum power. Measurements are performed respectively on the lowest, middle and highest channels of the operating band(s). The EUT is set to maximum power level during all tests, and at the beginning of each test the battery is fully charged.

- By comparing 802.11 b, 802.11g, 802.11H20 and 802.11H40 RF conducted average output power; if 802.11g/802.11H20/802.11H40 average output power is not 1/4 dB higher than 802.11b, 802.11g/802.11H20/802.11H40 modes are not required to be tested. (in this application, all 802.11g/802.11H20/802.11H40 tests are not necessary due to average power is not 1/4 dB higher than 802.11b)
- While testing 802.11b, SAR shall be measured at the middle channel if middle channel has the highest average power. If the measured SAR value is not greater than 0.8 W/kg, then low and high channel SAR measurement are not required.
- 3. When the maximum transmitter and antenna output power are \leq 60/f(GHz) (mW) SAR evaluation is typically not required for FCC or TCB approval (BT power= -1.99dBm)

The test configuration tested at the low, middle and high frequency channels, and then test of set in highest power. Finally, we will test it by dividing into 1 configuration:

Configuration 1: Laptop mode (WLAN/Main antenna -to-user separation distance is 113mm, so SAR test is required) (Appendix-Fig.3 & Fig.4)

1.6 The SAR Measurement System

A photograph of the SAR measurement System is given in Fig. a. This SAR Measurement System uses a Computer-controlled 3-D stepper motor system (SPEAG DASY 5 professional system). A Model ES3DV3 field probe is used to determine the internal electric fields. The SAR can be obtained from the equation SAR= σ ($|Ei|^2$)/ ρ where σ and ρ are the conductivity and mass density of the tissue-simulant.

The DASY5 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Staubli RX family) with controller, teach pendant and software. An arm extension is for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.

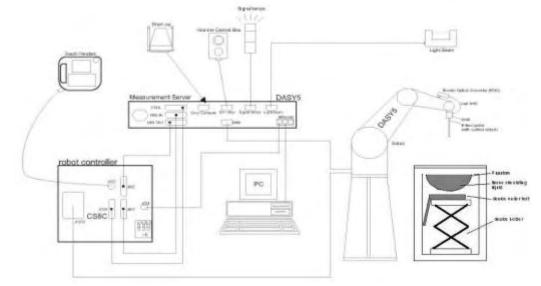


Fig.a The block diagram of SAR system

- The Electro-optical converter (EOC) performs the conversion between optical and electrical of the signals for the digital communication to the DAE and for the analog signal from the optical surface detection. The EOC is connected to the measurement server.
- The function of the measurement server is to perform the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
 - A computer operating Windows 2000 or Windows XP.
 - DASY5 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
 - The SAM twin phantom enabling testing left-hand and right-hand usage.
 - The device holder for handheld mobile phones.
 - Tissue simulating liquid mixed according to the given recipes.
 - Validation dipole kits allowing to validate the proper functioning of the system.

1.7 System Components

ES3DV3 E-Field Probe

Construction	Symmetrical design with triangular core	
	Built-in shielding against static charges	
	PEEK enclosure material (resistant to	
	organic solvents, e.g., DGBE)	
Calibration	Basic Broad Band Calibration in air	
	Conversion Factors (CF) for HSL2450 MHZ	
	Additional CF for other liquids and	
	frequencies upon request	
Frequency	10 MHz to $>$ 3 GHz, Linearity: \pm 0.6 dB (30 MHz to 6 GHz)	
Directivity	± 0.3 dB in HSL (rotation around probe axis)	
	± 0.5 dB in tissue material (rotation normal to probe axis)	

Dynamic Range	10 μW/g to > 100 mW/g
	Linearity: ± 0.6 dB (noise: typically < 1 µW/g)
Dimensions	Overall length: 330 mm (Tip: 10 mm)
	Tip diameter: 4 mm (Body: 10 mm)
	Typical distance from probe tip to dipole centers: 1 mm
Application	High precision dosimetric measurements in any exposure scenario
	(e.g., very strong gradient fields). Only probe which enables
	compliance testing for frequencies up to 6 GHz with precision of better
	30%.

SAM PHANTOM V4.0C

Construction	The shell corresponds to the specifications of the Specific						
	Anthropomorphic Mannequin (SAM)	phantom defined in IEEE					
	1528-200X, CENELEC 50361 and IEC 62209.						
	It enables the dosimetric evaluation	of left and right hand phone					
	usage as well as body mounted usa	ge at the flat phantom region. A					
	cover prevents evaporation of the liquid. Reference markings on the						
	phantom allow the complete setup	of all predefined phantom					
	positions and measurement grids by	y manually teaching three points					
	with the robot.						
Shell Thickness	2 ± 0.2 mm						
Filling Volume	Approx. 25 liters	(The second sec					
Dimensions	Height: 850 mm;						
	Length: 1000 mm;	N. III					
	Width: 500 mm	1					

DEVICE HOLDER

Construction	The device holder (Supporter) for	
	Notebook is made by POM	The second se
	(polyoxymethylene resin), which is	
	non-metal and non-conductive. The	
	height can be adjusted to fit varies	
	kind of notebooks.	
		Device Holder

1.8 SAR System Verification

The microwave circuit arrangement for system verification is sketched in Fig. b. The daily system accuracy verification occurs within the flat section of the SAM phantom. A SAR measurement was performed to see if the measured SAR was within +/- 5% from the target SAR values. These tests were done at 2450 MHz. The tests were conducted on the same days as the measurement of the DUT. The obtained results from the system accuracy verification are displayed in the table 1 (SAR values are normalized to 1W forward power delivered to the dipole). During the tests, the ambient temperature of the laboratory was in the range 22.1°C, the relative humidity was in the range 62% and the liquid depth above the ear reference points was above 15 cm in all the cases. It is seen that the system is operating within its specification, as the results are within acceptable tolerance of the reference values.




Fig.b The block diagram of system verification

Report No. : ES/2010/10012 Page : 11 of 51

- A. Agilent Model 8648D Signal Generator
- B. Mini circuits Model ZHL-42 Amplifier
- C. Agilent Model U2001B Power Sensor
- D. Agilent Model 777D Dual directional coupling
- E. Reference dipole antenna



Photograph of the dipole Antenna

Validation Kit	Frequency Hz	Target SAR (1g) (Pin=250mW)	Measured SAR (1g)	Measured Date
D2450V2 S/N: 727	2450 MHz (Body)	13.5m W/g	13.7mW/g	2010-02-04

Table 1. Results of system validation

1.9 Tissue Simulant Fluid for the Frequency Band

The dielectric properties for this body-simulant fluid were measured by using the Agilent Model 85070D Dielectric Probe (rates frequency band 200 MHz to 20 GHz) in conjunction with HP 8753D Network Analyzer (30 KHz-6000 MHz) by using a procedure detailed in Section V.

All dielectric parameters of tissue simulates were measured within 24 hours of SAR measurements. The depth of the tissue simulant in the ear reference point of the phantom was 15cm±5mm during all tests. (Fig .2)

Frequency	Tissue type	Measurement date/	Dielectric Parameters			
(MHz)		Limits	ρ	σ (S/m)	Simulated Tissue	
					Temperature(°C)	
	Pody	Measured, 2010.02.04	52.1	2.06	21.7	
2450 Body		Recommended Limits	51.68-57.12	1.88-2.09	20-24	

Table 2. Dielectric Parameters of Tissue Simulant Fluid

The composition of the body tissue simulating liquid is:

Ingredient	2450MHz (Body)
DGMBE	301.7ml
Water	698.3ml
Salt	Х
Preventol D-7	Х
Cellulose	Х
Sugar	Х
Total amount	1 L (1.0kg)

Table 3. Recipes for tissue simulating liquid

1.10 Evaluation Procedures

The entire evaluation of the spatial peak values is performed within the Post-processing engine (SEMCAD). The system always gives the maximum values for the 1 g and 10 g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- 1. The extraction of the measured data (grid and values) from the Zoom Scan.
- 2. The calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- 3. The generation of a high-resolution mesh within the measured volume
- 4. The interpolation of all measured values from the measurement grid to the high-resolution grid
- 5. The extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- 6. The calculation of the averaged SAR within masses of 1g and 10g. The probe is calibrated at the center of the dipole sensors that is located 1 to 2.7mm away from the probe tip. During measurements, the probe stops shortly above the phantom surface, depending on the probe and the surface detecting system. Both distances are included as parameters in the probe configuration file. The software always knows exactly how far away the measured point is from the surface. As the probe cannot directly measure at the surface, the values between the deepest measured point and the surface must be extrapolated. The angle between the probe axis and the surface normal

line is less than 30 degree.

In the Area Scan, the gradient of the interpolation function is evaluated to find all the extreme of the SAR distribution. The uncertainty on the locations of the extreme is less than 1/20 of the grid size. Only local maximum within –2 dB of the global maximum are searched and passed for the Cube Scan measurement. In the Cube Scan, the interpolation function is used to extrapolate the Peak SAR from the lowest measurement points to the inner phantom surface (the extrapolation distance). The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5mm. The maximum search is automatically performed after each area scan measurement. It is based on splines in two or three dimensions. The procedure can find the maximum for most SAR distributions even with relatively large grid spacing. After the area scanning measurement, the probe is automatically moved to a position at the interpolated maximum. The following scan can directly use this position for reference, e.g., for a finer resolution grid or the cube evaluations. The 1g and 10g peak evaluations are only available for the predefined cube 7x7x7 scans. The routines are verified and optimized for the grid dimensions used in these cube measurements.

The measured volume of 30x30x30mm contains about 30g of tissue.

The first procedure is an extrapolation (incl. Boundary correction) to get the points between the lowest measured plane and the surface. The next step uses 3D interpolation to get all points within the measured volume. In the last step, a 1g cube is placed numerically into the volume and its averaged SAR is calculated. This cube is the moved around until the highest averaged SAR is found. If the highest SAR is found at the edge of the measured volume, the system will issue a warning: higher SAR values might be found outside of the measured volume. In that case the cube measurement can be repeated, using the new interpolated maximum as the center.

1.11 Test Standards and Limits

According to FCC 47CFR §2.1093(d) The limits to be used for evaluation are based generally on criteria published by the American National Standards Institute (ANSI) for localized specific absorption rate ("SAR") in Section 4.2 of "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3

kHz to 300 GHz," ANSI/IEEE C95.1–1992, Copyright 1992 by the Institute of Electrical and Electronics Engineers, Inc., New York, New York 10017. These criteria for SAR evaluation are similar to those recommended by the National Council on Radiation Protection and Measurements (NCRP) in "Biological Effects and Exposure Criteria for Radio frequency Electromagnetic Fields," NCRP Report No. 86, Section 17.4.5. Copyright NCRP, 1986, Bethesda, Maryland 20814.

SAR is a measure of the rate of energy absorption due to exposure to an RF transmitting source. SAR values have been related to threshold levels for potential biological hazards. The criteria to be used are specified in paragraphs (d)(1) and (d)(2) of this section and shall apply for portable devices transmitting in the frequency range from 100 kHz to 6 GHz. Portable devices that transmit at frequencies above 6 GHz are to be evaluated in terms of the MPE limits specified in § 1.1310 of this chapter. Measurements and calculations to demonstrate compliance with MPE field strength or power density limits for devices operating above 6 GHz should be made at a minimum distance of 5 cm from the radiating source.

- (1) Limits for Occupational/Controlled exposure: 0.4 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 8 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 20 W/kg, as averaged over an 10 grams of tissue (defined as a tissue volume in the shape of a cube).
- (2) Occupational/Controlled limits apply when persons are exposed as a consequence of their employment provided these persons are fully aware of and exercise control over their exposure. Awareness of exposure can be accomplished by use of warning labels or by specific training or education through appropriate means, such as an RF safety program in a work environment.
- (3) Limits for General Population/Uncontrolled exposure: 0.08 W/kg as averaged over the whole-body and spatial peak SAR not exceeding 1.6 W/kg as averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube). Exceptions are the hands, wrists, feet and ankles where the spatial peak SAR shall not exceed 4 W/kg, as averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube). General Population/Uncontrolled limits apply when the general public may be exposed, or when persons that are exposed as a consequence of

their employment may not be fully aware of the potential for exposure or do not exercise control over their exposure. Warning labels placed on consumer devices such as cellular telephones will not be sufficient reason to allow these devices to be evaluated subject to limits for occupational/controlled exposure in paragraph (d)(1) of this section.(Table .4)

Human Exposure	Uncontrolled Environment General Population	Controlled Environment Occupational	
Spatial Peak SAR (Brain)	1.60 m W/g	8.00 m W/g	
Spatial Average SAR (Whole Body)	0.08 m W/g	0.40 m W/g	
Spatial Peak SAR (Hands/Feet/Ankle/Wrist)	4.00 m W/g	20.00 m W/g	

Table .4 RF exposure limits

Notes:

- 1. Uncontrolled environments are defined as locations where there is potential exposure of individuals who have no knowledge or control of their potential exposure.
- 2. Controlled environments are defined as locations where there is potential exposure of individuals who have knowledge of their potential exposure and can exercise control over their exposure.

2. Summary of Results

WLAN802.11 b

Configuration 1: Laptop mode						
Frequency	requency Channel MHz Conducted Output Measured(W/kg) Amb. Liquid				Liquid	
			Power (Average) 1g Temp[°C] Temp[°C			Temp[°C]
2450MHz	1	2412	15.24dBm	0.021	22.1	21.7

WLAN802.11 g

Configuration 1: Laptop mode						
Frequency	/ Channel MHz Conducted Output Measured(W/kg) Amb. Liquid				Liquid	
			Power (Average) 1g Temp[°C] Temp[°			Temp[°C]
2450MHz	1	2412	14.13dBm	0.00884	22.1	21.7

WLAN802.11 n(20M)

Configuration 1: Laptop mode						
Frequency	Channel MHz Conducted Output Measured(W/kg) Amb. Liquid				Liquid	
			Power (Average)	1g	Temp[°C]	Temp[°C]
2450MHz	6	2437	13.90dBm	0.00777	22.1	21.7

WLAN802.11 n(40M)

Configuration 1: Laptop mode						
Frequency	Channel MHz Conducted Output Measured(W/kg) Amb. Liquid				Liquid	
			Power (Average)1gTemp[°C]Temp[°C			Temp[°C]
2450MHz	3	2422	14.19dBm	0.00877	22.1	21.7

Note:

SAR measurement results with transmitter at maximum output power.

3. Instruments List

Manufacturer	Device	Туре	Serial number	Date of last calibration
Schmid & Partner Engineering AG	Dosimetric E-Field Probe	ES3DV3	3172	May.27.2009
Schmid & Partner Engineering AG	2450 MHz System Validation Dipole	D2450V2	727	Apr.27.2009
Schmid & Partner Engineering AG	Data acquisition Electronics	DAE4	856	May.26.2009
Schmid & Partner Engineering AG	Software	DASY 5 V5.0 Build125	N/A	Calibration not required
Schmid & Partner Engineering AG	Phantom	SAM	N/A	Calibration not required
Agilent	Network Analyzer	8753D	3410A05547	Mar.31.2009
Agilent	Dielectric Probe Kit	85070D	US01440168	Calibration not required
Agilent	Dual-directional coupler	777D 501		Aug.26.2009
Agilent	RF Signal Generator	8648D	3847M00432	May.25.2009
Agilent	Power Sensor	U2001B	MY48100169	Apr.23.2009

Report No. : ES/2010/10012 Page : 18 of 51

4. Measurements

Date/Time: 02/04/2010 07:26:39

Configuration 1_WLAN802.11b_CH1

DUT: NAV50;

Communication System: Wireless LAN; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: Body 2450 Medium parameters used: f = 2412 MHz; σ = 1.99 mho/m; ϵ_r = 52; ρ = 1000 kg/m³

Phantom section: Flat Section

- Probe: ES3DV3 SN3172; ConvF(4.02, 4.02, 4.02); Calibrated: 5/27/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn856; Calibrated: 5/26/2009
- Phantom: SAM1; Type: SAM;
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125


Body/Area Scan (61x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.024 mW/g

Body/Zoom Scan (7x7x7) (5x5x7)/Cube 0: Measurement grid: dx=8mm,

dy=8mm, dz=5mm Reference Value = 2.15 V/m; Power Drift = -0.054 dB Peak SAR (extrapolated) = 0.034 W/kg


SAR(1 g) = 0.021 mW/g; SAR(10 g) = 0.010 mW/g

Maximum value of SAR (measured) = 0.020 mW/g

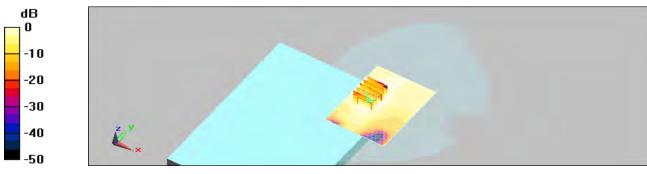

 $0 \, dB = 0.020 \, mW/g$

Report No. : ES/2010/10012 Page : 19 of 51

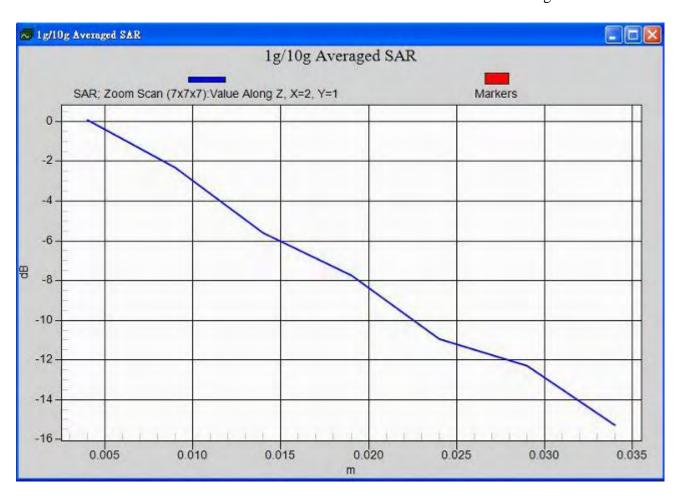

Report No. : ES/2010/10012 Page : 20 of 51

Date/Time: 02/04/2010 08:47:36

Configuration 1_WLAN802.11g_CH1

DUT: NAV50;

Communication System: Wireless LAN; Frequency: 2412 MHz;Duty Cycle: 1:1 Medium: Body 2450 Medium parameters used: f = 2412 MHz; σ = 1.99 mho/m; ϵ_r = 52; ρ = 1000 kg/m³ Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 SN3172; ConvF(4.02, 4.02, 4.02); Calibrated: 5/27/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn856; Calibrated: 5/26/2009
- Phantom: SAM1; Type: SAM;
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125


Body/Area Scan (61x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.00986 mW/g

Body/Zoom Scan (7x7x7) (5x5x7)/Cube 0: Measurement grid: dx=8mm,

dy=8mm, dz=5mm Reference Value = 1.22 V/m; Power Drift = 0.121 dB Peak SAR (extrapolated) = 0.036 W/kg

SAR(1 g) = 0.00884 mW/g; SAR(10 g) = 0.00409 mW/g

Maximum value of SAR (measured) = 0.010 mW/g

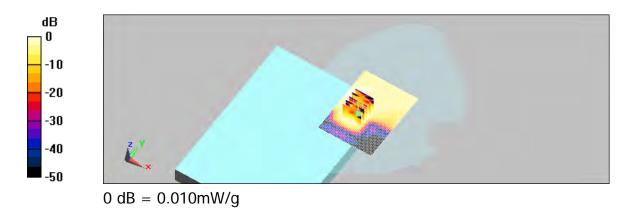

Report No. : ES/2010/10012 Page : 21 of 51

Date/Time: 02/04/2010 09:37:34

Configuration 1_WLAN802.11n(20M)_CH6

DUT: NAV50 ;

Communication System: Wireless LAN; Frequency: 2437 MHz;Duty Cycle: 1:1 Medium: Body 2450 Medium parameters used: f = 2437 MHz; σ = 2.04 mho/m; ϵ_r = 52.1; ρ = 1000 kg/m³ Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 SN3172; ConvF(4.02, 4.02, 4.02); Calibrated: 5/27/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn856; Calibrated: 5/26/2009
- Phantom: SAM1; Type: SAM;
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125


Body/Area Scan (61x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.00942 mW/g

Body/Zoom Scan (7x7x7) (5x5x7)/Cube 0: Measurement grid: dx=8mm,

dy=8mm, dz=5mm Reference Value = 1.16 V/m; Power Drift = -0.092 dB Peak SAR (extrapolated) = 0.013 W/kg

SAR(1 g) = 0.00777 mW/g; SAR(10 g) = 0.00359 mW/g

Maximum value of SAR (measured) = 0.00935 mW/g

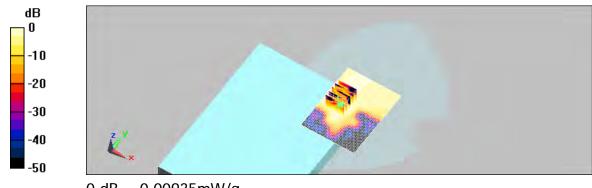

 $0 \, dB = 0.00935 mW/g$

Report No. : ES/2010/10012 Page : 22 of 51

Date/Time: 02/04/2010 10:31:07

Configuration 1_WLAN802.11n(40M)_CH3

DUT: NAV50 ;

Communication System: Wireless LAN; Frequency: 2422 MHz;Duty Cycle: 1:1 Medium: Body 2450 Medium parameters used: f = 2422 MHz; σ = 2.01 mho/m; ϵ_r = 52; ρ = 1000 kg/m³ Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 SN3172; ConvF(4.02, 4.02, 4.02); Calibrated: 5/27/2009
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn856; Calibrated: 5/26/2009
- Phantom: SAM1; Type: SAM;
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125


Body/Area Scan (61x81x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.010 mW/g

Body/Zoom Scan (7x7x7) (5x5x7)/Cube 0: Measurement grid: dx=8mm,

dy=8mm, dz=5mm Reference Value = 1.23 V/m; Power Drift = 0.147 dB Peak SAR (extrapolated) = 0.015 W/kg

SAR(1 g) = 0.00877 mW/g; SAR(10 g) = 0.0044 mW/g

Maximum value of SAR (measured) = 0.0097 mW/g

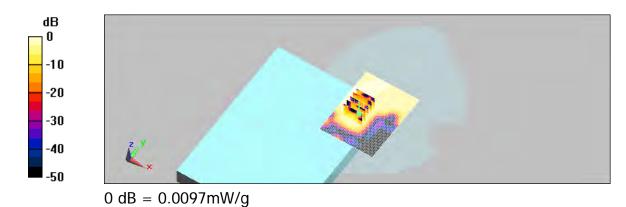

Report No. : ES/2010/10012 Page : 23 of 51

5. SAR System Performance Verification

Date/Time: 02/04/2010 06:12:13

DUT: Dipole 2450 MHz;

Communication System: CW; Frequency: 2450 MHz;Duty Cycle: 1:1 Medium: Body2450 Medium parameters used: f = 2450 MHz; σ = 2.06 mho/m; ϵ_r = 52.1; ρ = 1000 kg/m³ Phantom section: Flat Section

DASY5 Configuration:

- Probe: ES3DV3 SN3172; ConvF(4.02, 4.02, 4.02); Calibrated: 5/27/2009
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn856; Calibrated: 5/26/2009
- Phantom: SAM1; Type: SAM; Serial:
- Measurement SW: DASY5, V5.0 Build 125; SEMCAD X Version 13.4 Build 125


Pin=250mW/Area Scan (31x51x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 18.5 mW/g

Pin=250mW/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid:

dx=5mm, dy=5mm, dz=5mmReference Value = 95.6 V/m; Power Drift = -0.018 dB Peak SAR (extrapolated) = 36.4 W/kg

SAR(1 g) = 13.7 mW/g; SAR(10 g) = 5.6 mW/g

Maximum value of SAR (measured) = 17.8 mW/g

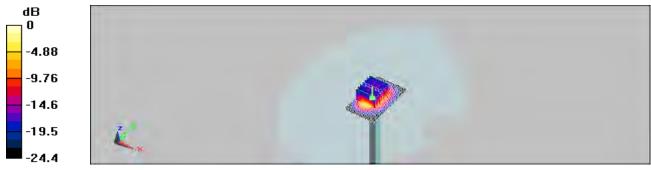

 $0 \, dB = 17.8 \, mW/g$

6. DAE & Probe Calibration certificate

ughausstrasse 43, 8004 Zurich,		BRATO BRATO	C Service subset of early mage Servicio svizzero di taratura S Swiss Calibration Service
ccredited by the Swiss Accreditation he Swiss Accreditation Service			ition No.: SCS 108
fultilateral Agreement for the rec	ognition of calibration c		
Client SGS (Auden)		Certificat	te No: DAE4-856_May09
CALIBRATION C	ERTIFICATE		
Object	DAE4 - SD 000 D	04 BJ - SN: 856	
Calibration procedure(s)	QA CAL-06.v12 Calibration proceed	lure for the data acquisition e	electronics (DAE)
Calibration date:	May 26, 2009		
Condition of the calibrated item	In Tolerance		
		nal standards, which realize the physic obability are given on the following page	
The measurements and the uncert All calibrations have been conduct	ainties with confidence pro		es and are part of the certificate.
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE	ainties with confidence pro	obability are given on the following page	es and are part of the certificate.
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702	eainties with confidence pro- ed in the closed laboratory E critical for calibration)	facility: environment temperature (22 Gal Date (Certificate No.) 30-Sep-08 (No: 7673)	es and are part of the certificate. ≥ 3)°C and humidity < 70%. Scheduled Calibration Sep-09
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001	ainties with confidence provide the closed laboratory E critical for calibration) ID # SN: 6295803 SN: 0810278	Cal Date (Certificate No.) 30-Sep-08 (No: 7673)	es and are part of the certificate. ± 3)°C and humidity < 70%. <u>Scheduled Calibration</u> Sep-09 Sep-09
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702	ainties with confidence pre- ed in the closed laboratory E critical for calibration) ID # 2 SN: 6295803 SN: 0810278 ID #	facility: environment temperature (22 Gal Date (Certificate No.) 30-Sep-08 (No: 7673)	es and are part of the certificate. ≥ 3)°C and humidity < 70%. Scheduled Calibration Sep-09
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	ainties with confidence pre- ed in the closed laboratory E critical for calibration) ID # 2 SN: 6295803 SN: 0810278 ID #	Cal Date (Certificate No.) 30-Sep-08 (No: 7673) 30-Sep-08 (No: 7670) Check Date (in house)	es and are part of the certificate. ± 3)°C and humidity < 70%. Scheduled Calibration Sep-09 Sep-09 Scheduled Check
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ainties with confidence pre- ed in the closed laboratory E critical for calibration) 2 SN: 6295803 SN: 0810278 1D # SE UMS 006 AB 1004 Name	Cal Date (Certificate No.) 30-Sep-08 (No: 7673) 30-Sep-08 (No: 7670) Check Date (in house) 06-Jun-08 (in house check)	es and are part of the certificate. ± 3)°C and humidity < 70%. Scheduled Calibration Sep-09 Sep-09 Scheduled Check
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	ainties with confidence pre- ed in the closed laboratory E critical for calibration) ID # 2 SN: 6295803 SN: 0810278 ID # SE UMS 006 AB 1004	bability are given on the following page facility: environment temperature (22 : <u>Cal Date (Certificate No.)</u> 30-Sep-08 (No: 7673) 30-Sep-08 (No: 7670) <u>Check Date (in house)</u> 06-Jun-08 (in house check)	es and are part of the certificate. £ 3)°C and humidity < 70%. <u>Scheduled Calibration</u> Sep-09 Sep-09 <u>Scheduled Check</u> In house check: Jun-09
The measurements and the uncert All calibrations have been conduct Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	ainties with confidence pre- ed in the closed laboratory E critical for calibration) 2 SN: 6295803 SN: 0810278 1D # SE UMS 006 AB 1004 Name	Cal Date (Certificate No.) 30-Sep-08 (No: 7673) 30-Sep-08 (No: 7670) Check Date (in house) 06-Jun-08 (in house check)	es and are part of the certificate. £ 3)°C and humidity < 70%. <u>Scheduled Calibration</u> Sep-09 Sep-09 <u>Scheduled Check</u> In house check: Jun-09

Certificate No: DAE4-856_May09

Page 1 of 5

alibration Laborator chmid & Partner Engineering AG eughausstrasse 43, 8004 Zuric		BALLER CONSTRUCTION OF THE STRUCTURE	Service suisse d'étalonnage Servizio svizzero di taratura
ccredited by the Swiss Accredita ne Swiss Accreditation Servic ultilateral Agreement for the r	e is one of the signatori	es to the EA	n No.: SCS 108
lient SGS (Auden)			o: ES3-3172_May09
CALIBRATION	CERTIFICAT	Έ	
Object	ES3DV3 - SN:3	172	
Calibration procedure(s)		and QA CAL-23.v3 edure for dosimetric E-field probe	S
Calibration date:	May 27, 2009		
	In Tolerance	tional standards, which realize the physical un probability are given on the following pages an	
Condition of the calibrated item This calibration certificate docum The measurements and the unco All calibrations have been condu	In Tolerance		nd are part of the certificate.
Condition of the calibrated item This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M&	In Tolerance	probability are given on the following pages an	nd are part of the certificate.
Condition of the calibrated item this calibration certificate docum the measurements and the unce UI calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E4419B	In Tolerance	probability are given on the following pages an ory facility: environment temperature (22 ± 3)°0 Cal Date (Certificate No.) 1-Apr-09 (No. 217-01030)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-10
Condition of the calibrated item This calibration certificate docum The measurements and the unco NI calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A	In Tolerance	probability are given on the following pages an ory facility: environment temperature (22 ± 3)°C Cal Date (Certificate No.) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-10 Apr-10
Condition of the calibrated item This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor E4412A Power sensor E4412A	In Tolerance	probability are given on the following pages an ory facility: environment temperature (22 ± 3)°(<u>Cal Date (Certificate No.)</u> 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-10 Apr-10 Apr-10
Condition of the calibrated item This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator	In Tolerance	probability are given on the following pages an ory facility: environment temperature (22 ± 3)°(Cal Date (Certificate No.) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01030) 31-Mar-09 (No. 217-01026)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-10 Apr-10 Apr-10 Mar-10 Mar-10
Condition of the calibrated item This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	In Tolerance ents the traceability to na ertainties with confidence cted in the closed laborat TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b)	probability are given on the following pages an ory facility: environment temperature (22 ± 3)°(Cal Date (Certificate No.) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028)	ad are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-10 Apr-10 Mar-10 Mar-10 Mar-10
Condition of the calibrated item This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	In Tolerance	Cal Date (Certificate No.) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027)	ad are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Mar-10
Condition of the calibrated item This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor E4412A Power sensor E4412A Power sensor E4412A Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator	In Tolerance ents the traceability to na ertainties with confidence cted in the closed laborat TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b)	probability are given on the following pages an ory facility: environment temperature (22 ± 3)°(Cal Date (Certificate No.) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028)	ad are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-10 Apr-10 Mar-10 Mar-10 Mar-10
Condition of the calibrated item This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	In Tolerance	Cal Date (Certificate No.) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01026) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01027) 2-Jan-09 (No. E33-3013_Jan09) 9-Sep-08 (No. DAE4-660_Sep08)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Jan-10 Sep-09
Condition of the calibrated item This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor E4412A Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	In Tolerance	Cal Date (Certificate No.) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01028) 32-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01028)	ad are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Jan-10
Condition of the calibrated item This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 90 dB Attenuator	In Tolerance thents the traceability to na ertainties with confidence cted in the closed laborat TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5086 (20b) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID #	cal Date (Certificate No.) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 2-Jan-09 (No. 217-01027) 2-Jan-09 (No. 217-01027) 2-Jan-09 (No. 217-01027) 2-Jan-09 (No. Apt-4660_Sep08) Check Date (in house)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Jan-10 Sep-09 Scheduled Check
Condition of the calibrated item This calibration certificate docum The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor E4412A Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	In Tolerance nents the traceability to na ertainties with confidence cted in the closed laborat TE critical for calibration) ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5129 (30b) SN: 3013 SN: 660 ID #	Cal Date (Certificate No.) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. ES3-3013_Jan09) 9-Sep-08 (No. DAE4-660_Sep08) Check Date (in house) 4-Aug-99 (in house check Oct-07)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-10 Apr-10 Mar-10 Mar-10 Jan-10 Sep-09 Scheduled Check In house check: Oct-09
Condition of the calibrated item This calibration certificate docum The measurements and the unce	In Tolerance nents the traceability to na ertainties with confidence cted in the closed laborat TE critical for calibration) ID # GB41293874 MY41495277 MY41495087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700 US37390585	cal Date (Certificate No.) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 1-Apr-09 (No. 217-01030) 31-Mar-09 (No. 217-01026) 31-Mar-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 2-Jan-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 2-Jan-09 (No. 217-01028) 31-Mar-09 (No. 217-01027) 2-Jan-09 (No. E33-3013_Jan09) 9-Sep-08 (No. DAE4-660_Sep08) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08)	nd are part of the certificate. C and humidity < 70%. Scheduled Calibration Apr-10 Apr-10 Mar-10 Mar-10 Mar-10 Jan-10 Sep-09 Scheduled Check In house check: Oct-09 In house check: Oct-09

Certificate No: ES3-3172_May09

Page 1 of 9

Report No. : ES/2010/10012 Page : 26 of 51

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



GWISS CRIBRIATION S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

 TSL
 tissue simulating liquid

 NORMx,y,z
 sensitivity in free space

 ConvF
 sensitivity in TSL / NORMx,y,z

 DCP
 diode compression point

 Polarization φ
 φ rotation around probe axis

 Polarization θ
 9 rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., θ = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx, y, z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx, y, z are only intermediate values, i.e., the uncertainties of NORMx, y, z does not effect the E²-field uncertainty inside TSL (see below *ConvF*).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ES3-3172_May09

Page 2 of 9

Report No. : ES/2010/10012 Page : 27 of 51

ES3DV3 SN:3172

May 27, 2009

Probe ES3DV3

SN:3172

Manufactured: Last calibrated: Recalibrated: January 23, 2008 June 23, 2008 May 27, 2009

Calibrated for DASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: ES3-3172_May09 Page 3 of 9

Report No. : ES/2010/10012 Page : 28 of 51

ES3DV3 SN:3172

May 27, 2009

DASY - Parameters of Probe: ES3DV3 SN:3172

Sensitivity in Free	e Space ^A		Diode C	ompression ^B
NormX	1.41 ± 10.1%	μ V/(V/m) ²	DCP X	94 mV
NormY	1.17 ± 10.1%	μ V/(V/m) ²	DCP Y	93 mV
NormZ	0.96 ± 10.1%	μ V/(V/m) ²	DCP Z	94 mV

Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

Boundary Effect

TSL 900 MHz Typical SAR gradient: 5 % per mm

Sensor Cente	er to Phantom Surface Distance	3.0 mm	4.0 mm
SAR _{be} [%]	Without Correction Algorithm	9.6	5.4
SAR _{be} [%]	With Correction Algorithm	0.9	0.7

TSL 1810 MHz Typical SAR gradient: 10 % per mm

Sensor Cente	er to Phantom Surface Distance	3.0 mm	4.0 mm	
SAR _{be} [%]	Without Correction Algorithm	9.2	5.4	
SAR _{be} [%]	With Correction Algorithm	0.7	0.4	

Sensor Offset

Probe Tip to Sensor Center

2.0 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 8).

^B Numerical linearization parameter: uncertainty not required.

Certificate No: ES3-3172_May09

Page 4 of 9


Report No. : ES/2010/10012 Page : 29 of 51

ES3DV3 SN:3172

May 27, 2009

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

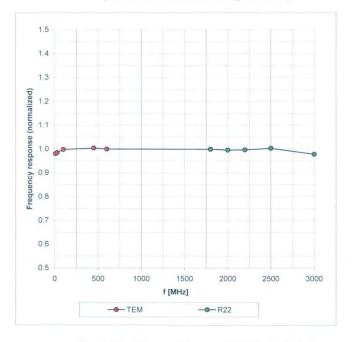


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: ES3-3172_May09 Page 5 of 9


Report No. : ES/2010/10012 Page : 30 of 51

ES3DV3 SN:3172

May 27, 2009

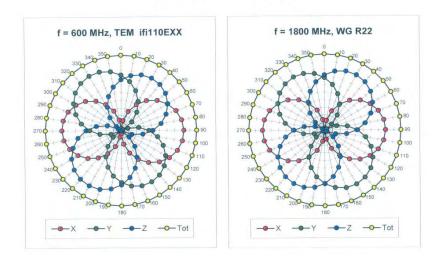

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

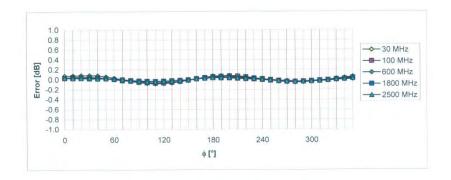


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: ES3-3172_May09

Page 6 of 9

Report No. : ES/2010/10012 Page : 31 of 51

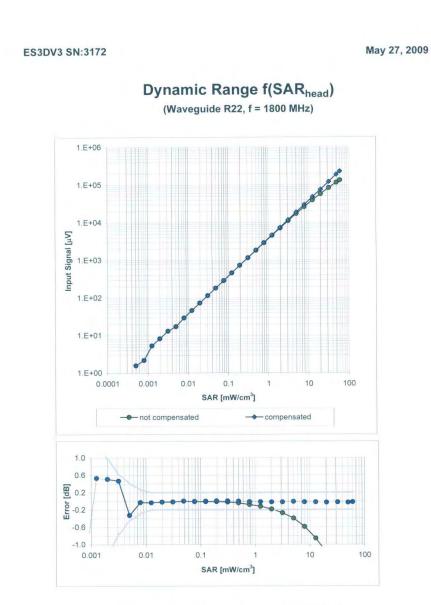


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: ES3-3172_May09

Page 7 of 9

ES3DV3 SN:3172

May 27, 2009

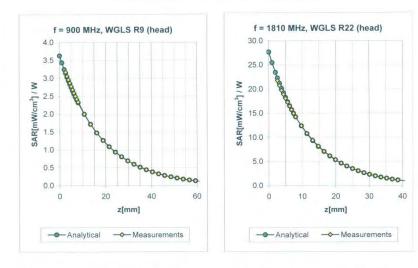

Conversion Factor Assessment


f [MHz]	Validity [MHz] ^C	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
835	± 50 / ± 100	Head	41.5 ± 5%	0.90 ± 5%	0.86	1.08	5.83 ± 11.0% (k=2)
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.87	1.08	5.65 ± 11.0% (k=2)
1750	± 50 / ± 100	Head	40.1 ± 5%	1.37 ± 5%	0.35	1.81	4.99 ± 11.0% (k=2)
1810	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.38	1.73	4.86 ± 11.0% (k=2)
1950	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.48	1.51	4.71 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1.80 ± 5%	0.41	1.78	4.33 ± 11.0% (k=2)
835	± 50 / ± 100	Body	55.2 ± 5%	0.97 ± 5%	0.78	1.15	5.81 ± 11.0% (k=2)
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.78	1.15	5.67 ± 11.0% (k=2)
1750	± 50 / ± 100	Body	53.4 ± 5%	1.49 ± 5%	0.45	1.75	4.69 ± 11.0% (k=2)
1810	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.33	2.23	4.54 ± 11.0% (k=2)
1950	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.27	2.99	4.53 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.40	1.40	4.02 ± 11.0% (k=2)

 $^{\rm C}$ The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Certificate No: ES3-3172_May09

Page 8 of 9

Report No. : ES/2010/10012 Page : 33 of 51

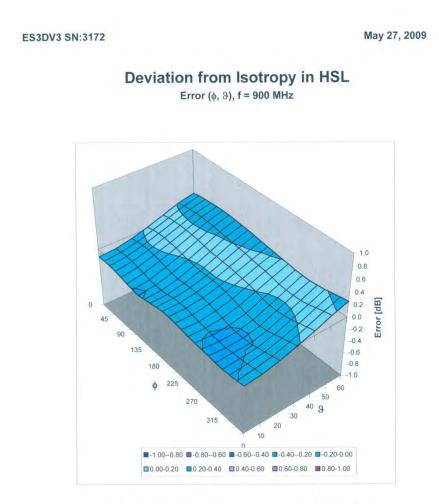

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Certificate No: ES3-3172_May09

Page 9 of 9

Report No. : ES/2010/10012 Page : 34 of 51

7. Uncertainty Analysis

Report No. : ES/2010/10012 Page : 35 of 51

Error Description	Uncertainty value	Prob. Dist.	Div.	$\begin{pmatrix} c_i \end{pmatrix}$ 1g	$\begin{pmatrix} c_i \\ 10g \end{pmatrix}$	Std. Unc. (1g)	Std. Unc. (10g)	$\begin{pmatrix} v_t \end{pmatrix}$ v_{eff}
Measurement System	12		1					
Probe Calibration	$\pm 5.9\%$	N	1	1	1	$\pm 5.9\%$	$\pm 5.9\%$	00
Axial Isotropy	$\pm 4.7\%$	R	$\sqrt{3}$	0.7	0.7	±1.9%	$\pm 1.9\%$	00
Hemispherical Isotropy	$\pm 9.6\%$	R	$\sqrt{3}$	0.7	0.7	$\pm 3.9\%$	$\pm 3.9\%$	00
Boundary Effects	±1.0%	R	$\sqrt{3}$	1	1	$\pm 0.6\%$	$\pm 0.6\%$	00
Linearity	$\pm 4.7\%$	R	$\sqrt{3}$	1	1	±2.7%	$\pm 2.7\%$	00
System Detection Limits	±1.0 %	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	00
Readout Electronics	$\pm 0.3\%$	N	1	1	1	$\pm 0.3\%$	$\pm 0.3\%$	00
Response Time	$\pm 0.8\%$	R	$\sqrt{3}$	1	1	$\pm 0.5\%$	±0.5%	00
Integration Time	$\pm 2.6\%$	R	$\sqrt{3}$	1	1	$\pm 1.5\%$	±1.5%	00
RF Ambient Noise	±3.0%	R	$\sqrt{3}$	1	1	$\pm 1.7\%$	$\pm 1.7\%$	00
RF Ambient Reflections	±3.0%	R	$\sqrt{3}$	1	1	±1.7%	$\pm 1.7\%$	00
Probe Positioner	$\pm 0.4\%$	R	$\sqrt{3}$	1	1	$\pm 0.2\%$	$\pm 0.2\%$	00
Probe Positioning	$\pm 2.9\%$	R	$\sqrt{3}$	1	1	±1.7%	$\pm 1.7\%$	00
Max. SAR Eval.	$\pm 1.0\%$	R	$\sqrt{3}$	1	1	±0.6%	±0.6%	00
Test Sample Related				1	1			1
Device Positioning	$\pm 2.9\%$	N	1	1	1	$\pm 2.9\%$	$\pm 2.9\%$	145
Device Holder	$\pm 3.6\%$	N	1	1	1	$\pm 3.6\%$	$\pm 3.6\%$	5
Power Drift	$\pm 5.0\%$	R	$\sqrt{3}$	1	1	$\pm 2.9\%$	$\pm 2.9\%$	00
Phantom and Setup			1200	1	1			1
Phantom Uncertainty	$\pm 4.0\%$	R	$\sqrt{3}$	1	1	$\pm 2.3\%$	$\pm 2.3\%$	00
Liquid Conductivity (target)	$\pm 5.0\%$	R	$\sqrt{3}$	0.64	0.43	±1.8%	$\pm 1.2\%$	00
Liquid Conductivity (meas.)	$\pm 2.5 \%$	N	1	0.64	0.43	$\pm 1.6\%$	$\pm 1.1 \%$	00
Liquid Permittivity (target)	$\pm 5.0\%$	R	$\sqrt{3}$	0.6	0.49	$\pm 1.7\%$	±1.4%	00
Liquid Permittivity (meas.)	$\pm 2.5 \%$	N	1	0.6	0.49	$\pm 1.5\%$	$\pm 1.2\%$	∞
Combined Std. Uncertainty						$\pm 10.9\%$	±10.7%	387
Expanded STD Uncertain	ty					$\pm 21.9\%$	$\pm 21.4\%$	

DASV5 Uncertainty Budget

Table 19.6: Worst-Case uncertainty budget for DASY5 assessed according to IEEE 1528 [1]. The budget is valid for the frequency range 300 MHz - 3 GHz and represents a worst-case analysis. For specific tests and configurations, the uncertainty could be considerable smaller.

g

8. Phantom Description

Schmid & Partner Engineering AG p S e а Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com. http://www.speag.com

Certificate of Conformity / First Article Inspection

ltern	SAM Twin Phantom V4.0	
Type No	QD 000 P40 C	
Series No	TP-1150 and higher	
Manufacturer	SPEAG Zeughausstasse 43 CH-8004 Zürich Switzetland	

Tests

The series production process used allows the limitation to test of first articles. Complete tests were made on the pre-series Type No. QD 000 P40 AA, Serial No. TP-1001 and on the series first article Type No. QD 000 P40 BA, Serial No. TP-1006. Certain parameters have been retested using further series items (called samples) or are tested at each item.

Test	Requirement	Details	Units tested
Dimensions	Compliant with the geometry according to the CAD model.	IT'IS CAD File (*)	First article, Samples
Material thickness of shell	Compliant with the requirements according to the standards	2mm +/- 0.2mm in flat and specific areas of head section	First article, Samples, TP-1314 ff.
Material thickness at ERP	Compliant with the requirements according to the standards	6mm +/- 0.2mm at ERP	First article, All items
Material parameters	Dielectric parameters for required frequencies	300 MHz – 6 GHz: Relative permittivity < 5, Loss tangent < 0.05	Material samples
Material resistivity	The material has been tested to be compatible with the liquids defined in the standards if handled and cleaned according to the instructions. Observe technical Note for material compatibility.	DEGMBE based simulating liquids	Pre-series, First article, Material samples
Sagging	Compliant with the requirements according to the standards. Sagging of the flat section when filled with tissue simulating liquid.	< 1% typical < 0.8% if filled with 155mm of HSL900 and without DUT below	Prototypes, Sample testing

Standards

- ndards CENELEC EN 50361 IEEE Std 1528-2003 IEC 62209 Part I FCC OET Bulletin 65, Supplement C, Edition 01-01 The IT'IS CAD file is derived from [2] and is also within the tolerance requirements of the shapes of the other documents. 12340

Conformity

Signature / Stamp

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of SAR measurements specified in standards [1] to [4].

Date	07.07.2005
the second second	10 / Jack 10 10 10 10

p 8 0 a Scient & Parser Engineering AQ Phone set 1, 200 Zurich, Cwitzerland Phone set 1, 205 9700 Fer 46 of 245 9779 Into Repear.com, http://www.spear.com

g

Doc No 881 - QD 000 P40 C - F

1(1).

Pege

9. System Validation from Original equipment supplier

ccredited by the Swiss Accred he Swiss Accreditation Service			No.: SCS 108
lultilateral Agreement for the m			
lient SGS (Auden)		Cartificate No	: D2450V2-727 Apr09
Sient 505 (Adden)		Certificate No	. D240042-121_Apros
CALIBRATION C	ERTIFICATE		
Object	D2450V2 - SN: 7	27	
Calibration procedure(s)	QA CAL-05.v7		
	Calibration proce	dure for dipole validation kits	
Calibration date:	April 27, 2009		
	. Transition and		
Condition of the calibrated item	In Tolerance		
	and the second se		
This calibration certificate docum	ents the traceability to nati	ional standards, which realize the physical uni	ts of measurements (SI).
		ional standards, which realize the physical uni robability are given on the following pages and	
The measurements and the unce	rtainties with confidence p		d are part of the certificate.
The measurements and the unce	rtainties with confidence p	robability are given on the following pages and	d are part of the certificate.
The measurements and the unce	rtainties with confidence p	robability are given on the following pages and	d are part of the certificate.
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M&	rtainties with confidence p	robability are given on the following pages and	d are part of the certificate.
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards	rtainties with confidence p cted in the closed laborato TE critical for calibration)	robability are given on the following pages and ry facility: environment temperature $(22 \pm 3)^\circ$ C	d are part of the certificate. C and humidity < 70%.
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Cal Date (Calibrated by, Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-09 Oct-09
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Reference 20 dB Attenuator	rtainties with confidence p cted in the closed laborato I'E critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g)	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C Cal Date (Calibrated by, Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 31-Mar-09 (No. 217-01025)	d are part of the certificate. C and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327	Cal Date (Calibrated by, Certificate No.) 08-Oct-08 (No. 217-00898) 031-Mar-09 (No. 217-01025) 31-Mar-09 (No. 217-01029)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025	Cal Date (Calibrated by, Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 03-Oct-08 (No. 217-0029) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. ES3-3025_Apr08)	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327	Cal Date (Calibrated by, Certificate No.) 08-Oct-08 (No. 217-00898) 031-Mar-09 (No. 217-01025) 31-Mar-09 (No. 217-01029)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards	rtainties with confidence p cted in the closed laborato IE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID #	Cal Date (Calibrated by, Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 03-Oct-08 (No. 217-0029) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. ES3-3025_Apr08)	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317	robability are given on the following pages and ry facility: environment temperature (22 ± 3)*C OB-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-01029) 31-Mar-09 (No. 217-01029) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. ES3-3025_Apr08) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09 Mar-10 Scheduled Check In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 100005	Cal Date (Calibrated by, Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 03-Mar-09 (No. 217-01025) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. ES3-3025_Apr08) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09 Mar-10 Scheduled Check In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317	robability are given on the following pages and ry facility: environment temperature (22 ± 3)*C OB-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-01029) 31-Mar-09 (No. 217-01029) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. ES3-3025_Apr08) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09 Mar-10 Scheduled Check In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 100005	Cal Date (Calibrated by, Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 03-Mar-09 (No. 217-01025) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. ES3-3025_Apr08) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09 Mar-10 Scheduled Check In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 100005	Cal Date (Calibrated by, Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 03-Mar-09 (No. 217-01025) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. ES3-3025_Apr08) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07)	d are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09 Mar-10 Scheduled Check In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 100005 US37390585 S4206	Cal Date (Calibrated by, Certificate No.) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 01-Mar-09 (No. 217-01025) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. E33-3025_Apr08) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08)	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09 Mar-10 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name	robability are given on the following pages and ry facility: environment temperature (22 ± 3)*C O8-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-01029) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. ES3-3025_Apr08) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08) Function	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09 Mar-10 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M&' Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by:	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name Jeton Kastrati	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C OB-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. ES3-3025_Apr08) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08) Function Laboratory Technician	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09 Mar-10 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M&' Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by:	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name	robability are given on the following pages and ry facility: environment temperature (22 ± 3)*C O8-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-01029) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. ES3-3025_Apr08) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08) Function	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09 Mar-10 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by:	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name Jeton Kastrati	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C OB-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. ES3-3025_Apr08) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08) Function Laboratory Technician	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09 Mar-10 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV2 DAE4 Secondary Standards	rtainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3025 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name Jeton Kastrati	robability are given on the following pages and ry facility: environment temperature (22 ± 3)°C OB-Oct-08 (No. 217-00898) 08-Oct-08 (No. 217-00898) 31-Mar-09 (No. 217-01029) 28-Apr-08 (No. ES3-3025_Apr08) 07-Mar-09 (No. DAE4-601_Mar09) Check Date (in house) 18-Oct-02 (in house check Oct-07) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-08) Function Laboratory Technician	d are part of the certificate. c and humidity < 70%. Scheduled Calibration Oct-09 Oct-09 Mar-10 Mar-10 Apr-09 Mar-10 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09

Report No. : ES/2010/10012 Page : 38 of 51

Calibration Laboratory of Schmid & Partner Engineering AG

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



SWISS

CRI BRATI

S Schweizerischer Kalibrierdienst
 Service suisse d'étalonnage
 Servizio svizzero di taratura
 S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D2450V2-727_Apr09

Page 2 of 9

Measurement Conditions

DASY Version	DASY5	V5.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.0 ± 6 %	1.82 mho/m ± 6 %
Head TSL temperature during test	(21.6 ± 0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.5 mW / g
SAR normalized	normalized to 1W	54.0 mW / g
SAR for nominal Head TSL parameters ¹	normalized to 1W	53.3 mW /g ± 17.0 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
	condition 250 mW input power	6.28 mW / g
SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured SAR normalized		6.28 mW / g 25.1 mW / g

¹ Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D2450V2-727_Apr09

Page 3 of 9

Body TSL parameters

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.4 ± 6 %	1.98 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C		

.

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.2 mW / g
SAR normalized	normalized to 1W	52.8 mW / g
SAR for nominal Body TSL parameters ²	normalized to 1W	52.8 mW /g ± 17.0 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
	condition 250 mW input power	6.18 mW / g
SAR averaged over 10 cm ³ (10 g) of Body TSL SAR measured SAR normalized		6.18 mW / g 24.7 mW / g
SAR measured	250 mW input power	

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D2450V2-727_Apr09

Page 4 of 9

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	55.1 Ω + 1.2 jΩ	
Return Loss	- 26.1 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.5 Ω + 3.3 jΩ	
Return Loss	- 29.6 dB	

General Antenna Parameters and Design

1.149 ns
_

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	January 09, 2003

Certificate No: D2450V2-727_Apr09

Page 5 of 9

Report No. : ES/2010/10012 Page : 42 of 51

DASY5 Validation Report for Head TSL

Date/Time: 27.04.2009 13:40:04

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN727


Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: HSL U10 BB Medium parameters used: f = 2450 MHz; σ = 1.82 mho/m; ϵ_r = 38; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC)

DASY5 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.4, 4.4, 4.4); Calibrated: 28.04.2008
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.4 Build 45

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

```
Reference Value = 100.3 V/m; Power Drift = 0.036 dB
Peak SAR (extrapolated) = 28.3 W/kg
SAR(1 g) = 13.5 mW/g; SAR(10 g) = 6.28 mW/g
Maximum value of SAR (measured) = 17.2 mW/g
```

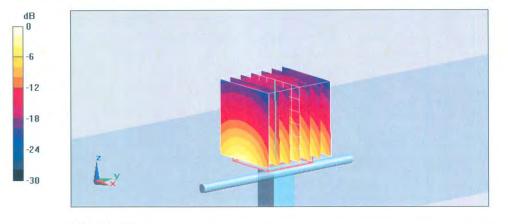


0 dB = 17.2 mW/g

Certificate No: D2450V2-727_Apr09

Page 6 of 9

Report No. : ES/2010/10012 Page : 43 of 51

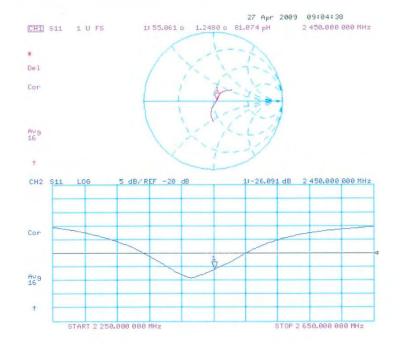

Impedance Measurement Plot for Head TSL

20. (F)

Certificate No: D2450V2-727_Apr09

Page 7 of 9

DASY5 Validation Report for Body TSL

Date/Time: 22.04.2009 13:12:14

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:727


Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: MSL U10 BB Medium parameters used: f = 2450 MHz; σ = 1.98 mho/m; ϵ_r = 54.4; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC)

DASY5 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.07, 4.07, 4.07); Calibrated: 28.04.2008
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 07.03.2009
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.4 Build 45

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


```
Reference Value = 96.9 \text{ V/m}; Power Drift = 0.031 \text{ dB}
Peak SAR (extrapolated) = 26.5 \text{ W/kg}
SAR(1 g) = 13.2 \text{ mW/g}; SAR(10 g) = 6.18 \text{ mW/g}
Maximum value of SAR (measured) = 17.3 \text{ mW/g}
```

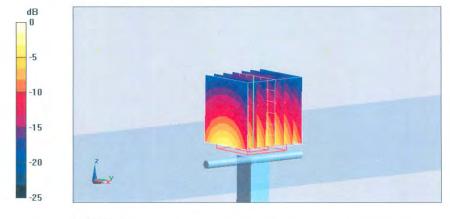

0 dB = 17.3 mW/g

Certificate No: D2450V2-727_Apr09

Page 8 of 9

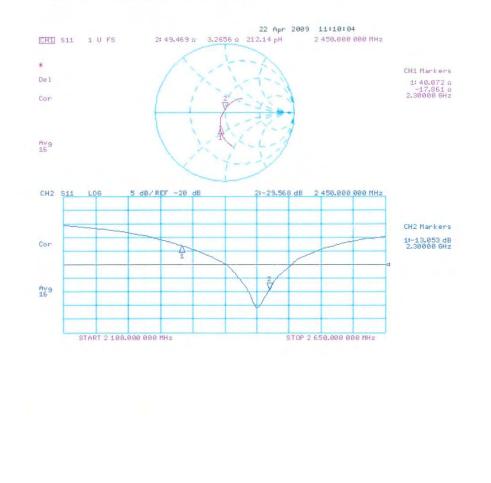

Impedance Measurement Plot for Body TSL

Certificate No: D2450V2-727_Apr09

Page 9 of 9

End of 1st part of report