

# Appendix C

# **Phantom Description**

Schmid & Partner Engineering AG

s e a D

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 info@speag.com, http://www.speag.com

### Certificate of Conformity / First Article Inspection

Item	Oval Flat Phantom ELI 5.0	
Type No	QD OVA 002 A	
Series No	1108 and higher	
Manufacturer	Untersee Composites Knebelstrasse 8, CH-8268 Mannenbach, Switzerland	

#### Tests

Complete tests were made on the prototype units QD OVA 001 A, pre-series units QD OVA 001 B as well as on some series units QD OVA 001 B. Some tests are made on all series units QD OVA 002 A.

Test	Requirement	Details	Units tested
Shape	Internal dimensions, depth and sagging are compatible with standards	Bottom elliptical 600 x 400 mm, Depth 190 mm, dimension compliant with [1] for f > 375 MHz	Prototypes
Material thickness	Bottom: 2.0mm +/- 0.2mm	dimension compliant with [3] for f > 800 MHz	all
Material parameters	rel. permittivity $2 - 5$ , loss tangent $\leq 0.05$ , at $f \leq 6$ GHz	rel. permittivity 3.5 +/- 0.5 loss tangent ≤ 0.05	Material samples
Material resistivity	Compatibility with tissue simulating liquids .	Compatible with SPEAG liquids. **	Phantoms, Material sample
Sagging	Sagging of the flat section in tolerance when filled with tissue simulating liquid.	within tolerance for filling height up to 155 mm	Prototypes, samples

Note: Compatibility restrictions apply certain liquid components mentioned in the standard, containing e.g. DGBE, DGMHE or Triton X-100. Observe technical note on material compatibility.

#### Standards

- [1] OET Bulletin 65, Supplement C, "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields", Edition 01-01 IEEE 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific
- [2] Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques, December 2003
- [3] IEC 62209-1 ed1.0, "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices - Human models, instrumentation, and procedures - Part 1:
- Procedure to determine the specific absorption rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)<sup>\*</sup>, 2005-02-18 IEC 62209–2 ed1.0, "Human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices Human models, instrumentation, and procedures Part 2: [4] Procedure to determine the specific absorption rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)<sup>a</sup>, 2010-03-30

## Conformity

Date

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of body-worn SAR measurements and system performance checks as specified in [1 - 4] and further standards

peag

Signature / Stamp

18 Partner-Engineering AG adestrosse 43, 8004 Vilch, Solation 441 44/2659708 Fext-46 6465 9779

Doc No 881 - QD OVA 002 A - A

25.7.2011

Page 1(1)

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488

www.sqs.com.tw



# System Validation from Original Equipment Supplier

credited by the Swiss Accreditation re Swiss Accreditation Service is utilateral Agreement for the rec	s one of the signatories	s to the EA	ccreditation No.: SCS 0108
lient SGS-TW (Auden	)	Certificate N	o: D2450V2-727_Apr20
	DTIFICATE		
CALIBRATION CI	ERTIFICATE		
Object	D2450V2 - SN:72	27	
Calibration procedure(s)	QA CAL-05.v11		
entraliant processis(e)		dure for SAR Validation Source	s between 0.7-3 GHz
D. (1. )	A		
Calibration date:	April 22, 2020		
All calibrations have been conducte	ad in the closed laborator	y facility: environment temperature (22 ± 3)	°C and humidity < 70%.
		y facility: environment temperature $(22 \pm 3)$	°C and humidity < 70%.
Calibration Equipment used (M&TE	critical for calibration)		
Calibration Equipment used (M&TE Primary Standards	critica) for calibration)	Cal Date (Certificate No.)	Scheduled Calibration
Calibration Equipment used (M&TE Primary Standards Power meter NRP	critical for calibration)	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101)	Scheduled Calibration Apr-21
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291	critical for calibration)	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101) 01-Apr-20 (No. 217-03100)	Scheduled Calibration
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291	critical for calibration)	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101)	Scheduled Calibration Apr-21 Apr-21
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator	critica) for calibration) ID # SN: 104778 SN: 103244 SN: 103245	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03101)	Scheduled Calibration Apr-21 Apr-21 Apr-21
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-201 Power sensor NRP-201 Reference 20 dB Attenuator Type-N mismatch combination	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k)	Cal Date (Certificate No.)   01-Apr-20 (No. 217-03100/03101)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03101)   31-Mar-20 (No. 217-03106)	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4	critica) for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 8H9394 (20k) SN: 310982 / 06327	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03101) 31-Mar-20 (No. 217-03106) 31-Mar-20 (No. 217-03104)	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Apr-21
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k) SN: 310924 (20k) SN: 31092 (20327 SN: 7349	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03101) 31-Mar-20 (No. 217-03106) 31-Mar-20 (No. 217-03104) 31-Dec-19 (No. EX3-7349_Dec19) 27-Dec-19 (No. DAE4-601_Dec19)	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Apr-21 Dec-20
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k) SN: 310982 / 06327 SN: 7349 SN: 7349 SN: 601	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03100) 31-Mar-20 (No. 217-03106) 31-Mar-20 (No. 217-03106) 31-Dec-19 (No. EX3-7349_Dec19)	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-201 Power sensor NRP-201 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 8H9394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601 ID #	Cal Date (Certificate No.) 01-Apr-20 (No. 217-03100/03101) 01-Apr-20 (No. 217-03100) 01-Apr-20 (No. 217-03101) 31-Mar-20 (No. 217-03106) 31-Mar-20 (No. 217-03104) 31-Dec-19 (No. EX3-7549_Dec19) 27-Dec-19 (No. DAE4-601_Dec19) Check Date (in house)	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k) SN: 31092 (06327 SN: 7349 SN: 601 ID # SN: GB39512475	Cal Date (Certificate No.)   01-Apr-20 (No. 217-03100/03101)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03101)   31-Mar-20 (No. 217-03104)   31-Dec-19 (No. EX3-7349_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house)   30-Oct-14 (in house check Feb-19)	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 3109245 SN: 310924 (208) SN: 31092 (208) SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783	Cal Date (Certificate No.)   01-Apr-20 (No. 217-03100/03101)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03101)   31-Mar-20 (No. 217-03106)   31-Mar-20 (No. 217-03104)   31-Dec-19 (No. EX3-7349_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house)   30-Oct-14 (in house check Feb-19)   07-Oct-15 (in house check Oct-18)	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-201 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06	critical for calibration) ID # SN: 104778 SN: 103245 SN: 103245 SN: 810394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601 ID # ID # SN: GB39512475 SN: US37292783 SN: MY41092317	Cal Date (Certificate No.)   01-Apr-20 (No. 217-03100/03101)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03101)   31-Mar-20 (No. 217-03105)   31-Mar-20 (No. 217-03104)   33-Dec-19 (No. EX3-7349_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house check Feb-19)   07-Oct-15 (in house check Cdc+18)   07-Oct-15 (in house check Cdc+18)	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20 In house check: Oct-20 In house check: Oct-20
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 103245 SN: 103924 (20k) SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: W374092317 SN: 100972	Cal Date (Certificate No.)   01-Apr-20 (No. 217-03100/03101)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03101)   31-Mar-20 (No. 217-03105)   31-Mar-20 (No. 217-03106)   31-Dec-19 (No. 217-03104)   31-Dec-19 (No. EX3-7549_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house)   30-Oct-14 (in house check Cet-18)   07-Oct-15 (in house check Oct-18)   15-Jun-15 (in house check Oct-18)	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20 In house check: Oct-20 In house check: Oct-20 In house check: Oct-20
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06 Natwork Analyzer Agilient E8358A	critical for calibration) ID # SN: 104778 SN: 103245 SN: 103245 SN: 8H0394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: 6B39512475 SN: 0837592783 SN: WY41092317 SN: 100972 SN: US41080477 Name	Cal Date (Certificate No.)   01-Apr-20 (No. 217-03100/03101)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03101)   31-Mar-20 (No. 217-03105)   31-Mar-20 (No. 217-03104)   31-Dec-19 (No. EX3-7349_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house check Feb-19)   07-Oct-15 (in house check Cdc+18)   07-Oct-15 (in house check Cdc+18)   15-Jun-15 (in house check Oct-18)   31-Mar-14 (in house check Oct-19)	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-201 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06	Critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k) SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: MY41092317 SN: 100972 SN: US41080477	Cal Date (Certificate No.)   01-Apr-20 (No. 217-03100/03101)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03101)   31-Mar-20 (No. 217-03106)   31-Mar-20 (No. 217-03104)   31-Dec-19 (No. EX3-7349_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house)   30-Oct-14 (in house check Feb-19)   07-Oct-15 (in house check Oct-18)   07-Oct-15 (in house check Oct-18)   15-Jun-15 (in house check Oct-19)	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer Aglient E8358A Calibrated by:	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k) SN: 31092 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: MY41092317 SN: US41080477 Name Jeffrey Katzmán	Cal Date (Certificate No.)   01-Apr-20 (No. 217-03100/03101)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03101)   31-Mar-20 (No. 217-03104)   31-Dec-19 (No. 217-03104)   31-Dec-19 (No. EX3-7349_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   27-Dec-15 (in house check Cet-18)   30-Oct-15 (in house check Cet-18)   07-Oct-15 (in house check Oct-18)   15-Jun-15 (in house check Oct-19)   Function   Laboratory Technician	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer Aglient E8358A	critical for calibration) ID # SN: 104778 SN: 103245 SN: 103245 SN: 8H0394 (20k) SN: 310982 / 06327 SN: 7349 SN: 601 ID # SN: 6B39512475 SN: 0837592783 SN: WY41092317 SN: 100972 SN: US41080477 Name	Cal Date (Certificate No.)   01-Apr-20 (No. 217-03100/03101)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03101)   31-Mar-20 (No. 217-03105)   31-Mar-20 (No. 217-03104)   31-Dec-19 (No. EX3-7349_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house check Feb-19)   07-Oct-15 (in house check Cdc+18)   07-Oct-15 (in house check Oct-18)   15-Jun-15 (in house check Oct-19)   Si-Mar-14 (in house check Oct-19)	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A RF generator R&S SMT-06 Natwork Analyzer Aglient E8358A Calibrated by:	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: BH9394 (20k) SN: 31092 / 06327 SN: 7349 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: MY41092317 SN: US41080477 Name Jeffrey Katzmán	Cal Date (Certificate No.)   01-Apr-20 (No. 217-03100/03101)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03100)   01-Apr-20 (No. 217-03101)   31-Mar-20 (No. 217-03104)   31-Dec-19 (No. 217-03104)   31-Dec-19 (No. EX3-7349_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   27-Dec-15 (in house check Cet-18)   30-Oct-15 (in house check Cet-18)   07-Oct-15 (in house check Oct-18)   15-Jun-15 (in house check Oct-19)   Function   Laboratory Technician	Scheduled Calibration Apr-21 Apr-21 Apr-21 Apr-21 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

Unless otherwise stated the results shown in this test report reter only to the sample(s) tested and such sample(s) are retained tor 90 days only. Mir#JAfabity i, the state methy mining test report reter only to the sample(s) tested and such sample(s) are retained tor 90 days only. Mir#JAfabity i, the state methy mining test report reter only to the sample(s) tested and such sample(s) are retained tor 90 days only. This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fulleest extent of the law. prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488

www.sqs.com.tw



**Calibration Laboratory of** Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst

Service suisse d'étalonnage C

Servizio svizzero di taratura S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

# Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

# Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatiala) Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

e) DASY4/5 System Handbook

# Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL; The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna. connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-727 Apr20

Page 2 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



#### **Measurement Conditions**

DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.6±6%	1.86 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

# SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.4 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.6 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL SAR measured	condition 250 mW input power	6.23 W/kg

Certificate No: D2450V2-727\_Apr20

Page 3 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時比樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents subject to Terms and Conditions for Electronic Documents at <u>http://www.sgs.com.tw/Terms-and-Conditions</u>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

```
www.sqs.com.tw
```



# Appendix (Additional assessments outside the scope of SCS 0108)

# Antenna Parameters with Head TSL

Impedance, transformed to feed point	56.0 $\Omega$ = 2.6 j $\Omega$
Return Loss	- 24.1 dB

## General Antenna Parameters and Design

Ins
1.149

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG

Certificate No: D2450V2-727 Apr20

Page 4 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

t (886-2) 2299-3279 台灣檢驗科技股份有限公司

f (886-2) 2298-0488

www.sqs.com.tw



## **DASY5 Validation Report for Head TSL**

Date: 22.04.2020

Test Laboratory: SPEAG, Zurich, Switzerland

# DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:727

Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz;  $\sigma = 1.86 \text{ S/m}$ ;  $\epsilon_r = 38.6$ ;  $\rho = 1000 \text{ kg/m}^3$ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(7.98, 7.98, 7.98) @ 2450 MHz; Calibrated: 31.12.2019
- Sensor-Surface: 1.4mm (Mechanical Surface Detection) 8
- Electronics: DAE4 Sn601; Calibrated: 27.12.2019
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

# Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 116.9 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 26.1 W/kg SAR(1 g) = 13.4 W/kg; SAR(10 g) = 6.23 W/kg Smallest distance from peaks to all points 3 dB below = 9 mm Ratio of SAR at M2 to SAR at M1 = 51.2% Maximum value of SAR (measured) = 21.9 W/kg



0 dB = 21.9 W/kg = 13.40 dBW/kg

Certificate No: D2450V2-727\_Apr20

Page 5 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law


No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488

www.sqs.com.tw



## Impedance Measurement Plot for Head TSL

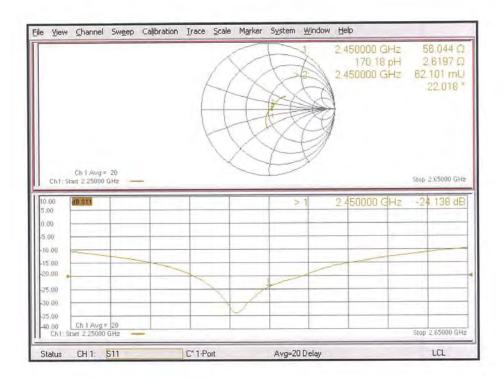

Certificate No: D2450V2-727\_Apr20

Page 6 of 6

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

t (886-2) 2299-3279 台灣檢驗科技股份有限公司

f (886-2) 2298-0488

www.sgs.com.tw



Engineering AG eughausstrasse 43, 8004 Zurich,	, Switzerland	34 2 19 19 31	Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
Accredited by the Swiss Accreditati The Swiss Accreditation Service Multilateral Agreement for the red	is one of the signatorie	es to the EA	Accreditation No.: SCS 0108
Client SGS-TW (Auder			No: D5GHzV2-1023_Jan20
CALIBRATION C	ERTIFICATI		
Object	D5GHzV2 - SN:1	1023	
Calibration procedure(s)	QA CAL-22.v4 Calibration Proce	edure for SAR Validation Source	es between 3-6 GHz
Calibration date:	January 28, 2020	0	
			and are part of the certificate.
alibration Equipment used (M&TE	critical for calibration)	ry facility: environment temperature (22 $\pm$ 3)	
alibration Equipment used (M&TE	E critical for calibration)	Cal Date (Certificate No.)	°C and humidity < 70%. Scheduled Calibration
alibration Equipment used (M&TE rimary Standards ower meter NRP	Critical for calibration)	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893)	°C and humidity < 70%. Scheduled Calibration Apr-20
alibration Equipment used (M&TE Imary Standards ower meter NRP ower sensor NRP-Z91	critical for calibration) ID # SN: 104778 SN: 103244	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892)	°C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20
alibration Equipment used (M&TE rimary Standards ower meter NRP ower sensor NRP-Z91 ower sensor NRP-Z91	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893)	C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20
alibration Equipment used (M&TE rimary Standards ower meter NRP ower sensor NRP-Z91 ower sensor NRP-Z91 leference 20 dB Attenuator	Critical for calibration)	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894)	C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Apr-20
alibration Equipment used (M&TE rimary Standards ower meter NRP ower sensor NRP-Z91 ower sensor NRP-Z91 leference 20 dB Attenuator ype-N mismatch combination	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 04-Apr-19 (No. 217-02895)	C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Apr-20 Apr-20 Apr-20
alibration Equipment used (M&TE rimary Standards ower meter NRP ower sensor NRP-Z91 ower sensor NRP-Z91 eference 20 dB Attenuator ype-N mismatch combination eference Probe EX3DV4	Critical for calibration)	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894)	C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Apr-20
alibration Equipment used (M&TE rimary Standards ower meter NRP ower sensor NRP-Z91 ower sensor NRP-Z91 leference 20 dB Attenuator ype-N mismatch combination leference Probe EX3DV4 AE4 econdary Standards	Critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047,2 / 06327 SN: 3503 SN: 601 ID #	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02895) 31-Dec-19 (No. EX3-3503_Dec19) 27-Dec-19 (No. DAE4-601_Dec19) Check Date (in house)	C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Scheduled Check
alibration Equipment used (M&TE imary Standards ower meter NRP ower sensor NRP-291 eference 20 dB Attenuator ype-N mismatch combination eference Probe EX3DV4 AE4 econdary Standards ower meter E4419B	Critical for calibration)	Cal Date (Certificate No.)   03-Apr-19 (No. 217-02892/02893)   03-Apr-19 (No. 217-02892)   03-Apr-19 (No. 217-02893)   04-Apr-19 (No. 217-02894)   04-Apr-19 (No. 217-02895)   31-Dec-19 (No. EX3-3503_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house)   30-Oct-14 (in house check Feb-19)	C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Check In house check: Oct-20
talibration Equipment used (M&TE rimary Standards ower meter NRP ower sensor NRP-Z91 ower sensor NRP-Z91 leference 20 dB Attenuator ype-N mismatch combination leference Probe EX3DV4 AE4 econdary Standards ower meter E4419B ower sensor HP 8481A	Critical for calibration)	Cal Date (Certificate No.)   03-Apr-19 (No. 217-02892/02893)   03-Apr-19 (No. 217-02892)   03-Apr-19 (No. 217-02893)   04-Apr-19 (No. 217-02894)   04-Apr-19 (No. 217-02895)   31-Dec-19 (No. EX3-3503_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house)   30-Oct-14 (in house check Feb-19)   07-Oct-15 (in house check Oct-18)	*C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
talibration Equipment used (M&TE rimary Standards ower meter NRP ower sensor NRP-Z91 ower sensor NRP-Z91 leference 20 dB Attenuator ype-N mismatch combination leference Probe EX3DV4 AE4 <u>econdary Standards</u> ower meter E4419B ower sensor HP 8481A ower sensor HP 8481A	Critical for calibration)	Cal Date (Certificate No.)   03-Apr-19 (No. 217-02892/02893)   03-Apr-19 (No. 217-02892)   03-Apr-19 (No. 217-02893)   04-Apr-19 (No. 217-02894)   04-Apr-19 (No. 217-02895)   31-Dec-19 (No. EX3-3503_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house)   30-Oct-14 (in house check Feb-19)   07-Oct-15 (in house check Oct-18)	C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20 In house check: Oct-20 In house check: Oct-20
alibration Equipment used (M&TE rimary Standards ower meter NRP ower sensor NRP-Z91 ower sensor NRP-Z91 eference 20 dB Attenuator ype-N mismatch combination eference Probe EX3DV4 AE4 econdary Standards ower meter E4419B ower sensor HP 8481A ower sensor HP 8481A ower sensor HP 8481A F generator R&S SMT-06	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3503 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: US37292783 SN: MY41092317 SN: 100972	Cal Date (Certificate No.)   03-Apr-19 (No. 217-02892/02893)   03-Apr-19 (No. 217-02892)   03-Apr-19 (No. 217-02893)   04-Apr-19 (No. 217-02894)   04-Apr-19 (No. 217-02895)   31-Dec-19 (No. 217-02895)   31-Dec-19 (No. 217-02895)   27-Dec-19 (No. DAE4-601_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house)   30-Oct-14 (in house check Feb-19)   07-Oct-15 (in house check Oct-18)   15-Jun-15 (in house check Oct-18)	*C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
Calibration Equipment used (M&TE rimary Standards lower meter NRP lower sensor NRP-Z91 leference 20 dB Attenuator ype-N mismatch combination leference Probe EX3DV4 IAE4 econdary Standards lower meter E4419B lower sensor HP 8481A ower sensor HP 8481A iver generator R&S SMT-06	Critical for calibration)	Cal Date (Certificate No.)   03-Apr-19 (No. 217-02892/02893)   03-Apr-19 (No. 217-02892)   03-Apr-19 (No. 217-02893)   04-Apr-19 (No. 217-02894)   04-Apr-19 (No. 217-02895)   31-Dec-19 (No. EX3-3503_Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house)   30-Oct-14 (in house check Feb-19)   07-Oct-15 (in house check Oct-18)	C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20 In house check: Oct-20 In house check: Oct-20
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator ype-N mismatch combination Reference Probe EX3DV4 PAE4 Recondary Standards Power meter E4419B Power sensor HP 8481A Power Senso	Critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3503 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: US3729778 SN: US3729778 SN: US37297778 SN: US37297778 SN: US37297777	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 04-Apr-19 (No. 217-02894) 04-Apr-19 (No. 217-02895) 31-Dec-19 (No. EX3-3503 Dec19) 27-Dec-19 (No. DAE4-601_Dec19) 27-Dec-19 (No. DAE4-601_Dec19) 07-Oct-15 (in house check Feb-19) 07-Oct-15 (in house check Cot-18) 07-Oct-15 (in house check Oct-18) 15-Jun-15 (in house check Oct-18) 31-Mar-14 (in house check Oct-19) Function	*C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
All calibrations have been conductor Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards Power sensor HP 8481A Power sensor HP	Critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047,2 / 06327 SN: 5047,2 / 06327 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: MY41092317 SN: US41080477	Cal Date (Certificate No.)   03-Apr-19 (No. 217-02892/02893)   03-Apr-19 (No. 217-02892)   03-Apr-19 (No. 217-02893)   04-Apr-19 (No. 217-02893)   04-Apr-19 (No. 217-02894)   04-Apr-19 (No. 217-02895)   31-Dec-19 (No. EX3-3503 Dec19)   27-Dec-19 (No. DAE4-601_Dec19)   Check Date (in house)   30-Oct-14 (in house check Feb-19)   07-Oct-15 (in house check Oct-18)   15-Jun-15 (in house check Oct-18)   31-Mar-14 (in house check Oct-19)	C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
Calibration Equipment used (M&TE Primary Standards Power meter NRP Power sensor NRP-291 Power sensor NRP-291 Reference 20 dB Attenuator ype-N mismatch combination Reference Probe EX3DV4 DAE4 Power meter E4419B Power sensor HP 8481A Power sen	Critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3503 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: US3729778 SN: US3729778 SN: US37297778 SN: US37297778 SN: US37297777	Cal Date (Certificate No.) 03-Apr-19 (No. 217-02892/02893) 03-Apr-19 (No. 217-02892) 03-Apr-19 (No. 217-02893) 04-Apr-19 (No. 217-02894) 04-Apr-19 (No. 217-02894) 04-Apr-19 (No. 217-02895) 31-Dec-19 (No. EX3-3503 Dec19) 27-Dec-19 (No. DAE4-601_Dec19) 27-Dec-19 (No. DAE4-601_Dec19) 07-Oct-15 (in house check Feb-19) 07-Oct-15 (in house check Cot-18) 07-Oct-15 (in house check Oct-18) 15-Jun-15 (in house check Oct-18) 31-Mar-14 (in house check Oct-19) Function	C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20
Calibration Equipment used (M&TE rrimary Standards Power meter NRP Power sensor NRP-Z91 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 20 dB Attenuator ype-N mismatch combination teleference Probe EX3DV4 PAE4 Recondary Standards Power meter E4419B Power sensor HP 8481A Power sensor HP 8481A Power sensor HP 8481A Pegenerator R&S SMT-06 Retwork Analyzer Agilent E8358A Calibrated by:	critical for calibration) ID # SN: 104778 SN: 103244 SN: 103245 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 3503 SN: 601 ID # SN: GB39512475 SN: US37292783 SN: W341092317 SN: 100972 SN: US41080477 Name Leif Klysner	Cal Date (Certificate No.)   03-Apr-19 (No. 217-02892/02893)   03-Apr-19 (No. 217-02892)   03-Apr-19 (No. 217-02893)   04-Apr-19 (No. 217-02894)   04-Apr-19 (No. 217-02895)   31-Dec-19 (No. 217-02895)   31-Dec-19 (No. 217-02895)   31-Dec-19 (No. 247-02895)   30-Oct-14 (In house)   Check Date (In house)   30-Oct-14 (In house check Feb-19)   07-Oct-15 (In house check Oct-18)   15-Jun-15 (In house check Oct-18)   31-Mar-14 (In house check Oct-18)	"C and humidity < 70%. Scheduled Calibration Apr-20 Apr-20 Apr-20 Apr-20 Apr-20 Dec-20 Dec-20 Scheduled Check In house check: Oct-20 In house check: Oct-20

Certificate No: D5GHzV2-1023\_Jan20

Page 1 of 9

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only. 除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份復製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This docume prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488

www.sgs.com.tw



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kallbrierdienst S Service suisse d'étalonnage

С Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

# Glassan

chossary.	
TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

# Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless C) communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

e) DASY4/5 System Handbook

### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated,
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D5GHzV2-1023 Jan20

Page 2 of 9

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction form exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



## **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.3
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5200 MHz ± 1 MHz 5300 MHz ± 1 MHz 5600 MHz ± 1 MHz 5800 MHz ± 1 MHz	

## Head TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.3 ± 6 %	4.49 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

# SAR result with Head TSL at 5200 MHz

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.05 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	80.1 W/kg ± 19.9 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSI	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL SAR measured	condition 100 mW input power	2.28 W/kg

Certificate No: D5GHzV2-1023 Jan20

Page 3 of 9

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u> and for electronic format documents issued by the Company subject to its General Conductors and every printed overlear, available on request of accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488

www.sqs.com.tw



#### Head TSL parameters at 5300 MHz The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.59 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

# SAR result with Head TSL at 5300 MHz

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.32 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	82.8 W/kg ± 19.9 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL SAR measured	condition 100 mW input power	2.35 W/kg

#### Head TSL parameters at 5600 MHz The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.89 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	السلا	

## SAR result with Head TSL at 5600 MHz

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.36 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	83.1 W/kg ± 19.9 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.37 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.5 W/kg ± 19.5 % (k=2)

Certificate No: D5GHzV2-1023\_Jan20

Page 4 of 9

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時比樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

t (886-2) 2299-3279 台灣檢驗科技股份有限公司

f (886-2) 2298-0488

www.sqs.com.tw



#### Head TSL parameters at 5800 MHz The following parameters and calculations were applied

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.5 ± 6 %	5.10 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	(1444)	

# SAR result with Head TSL at 5800 MHz

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.19 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	81.4 W/kg ± 19.9 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL SAR measured	condition 100 mW input power	2.29 W/kg

Certificate No: D5GHzV2-1023\_Jan20

Page 5 of 9

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留的天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a> and for electronic format documents issued by the Company subject to its General Conductors and every printed overlear, available on request of accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

t (886-2) 2299-3279 台灣檢驗科技股份有限公司

f (886-2) 2298-0488



# Appendix (Additional assessments outside the scope of SCS 0108)

# Antenna Parameters with Head TSL at 5200 MHz

Impedance, transformed to feed point	50.6 Ω - 8.0 jΩ	
Return Loss	- 22,0 dB	

Antenna Parameters with Head TSL at 5300 MHz

Impedance, transformed to feed point	52.4 Ω - 4.7 jΩ	
Return Loss	- 25.8 dB	

# Antenna Parameters with Head TSL at 5600 MHz

Impedance, transformed to feed point	55.9 Ω - 1.1 jΩ
Return Loss	- 25.0 dB

# Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	56.2 Ω + 2.9 jΩ	
Return Loss	- 23.8 dB	

# General Antenna Parameters and Design

Electrical Delay (one direction)	1.199 ns	
	1	

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG

Certificate No: D5GHzV2-1023 Jan20

Page 6 of 9

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



# **DASY5 Validation Report for Head TSL**

Date: 28.01.2020

Test Laboratory: SPEAG, Zurich, Switzerland

# DUT: Dipole D5GHzV2; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1023

Communication System: UID 0 - CW; Frequency: 5200 MHz, Frequency: 5300 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz Medium parameters used: f = 5200 MHz;  $\sigma$  = 4.49 S/m;  $\epsilon_r$  = 35.3;  $\rho$  = 1000 kg/m<sup>3</sup>, Medium parameters used: f = 5300 MHz;  $\sigma = 4.59 \text{ S/m}$ ;  $\varepsilon_r = 35.2$ ;  $\rho = 1000 \text{ kg/m}^3$ Medium parameters used: f = 5600 MHz;  $\sigma$  = 4.89 S/m;  $\epsilon_r$  = 34.8;  $\rho$  = 1000 kg/m<sup>3</sup>. Medium parameters used: f = 5800 MHz;  $\sigma = 5.1 \text{ S/m}$ ;  $\varepsilon_r = 34.5$ ;  $\rho = 1000 \text{ kg/m}^3$ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 SN3503; ConvF(5.8, 5.8, 5.8) @ 5200 MHz, ConvF(5.49, 5.49, 5.49) @ 5300 MHz, ConvF(5.1, 5.1, 5.1) @ 5600 MHz, ConvF(5.01, 5.01, 5.01) @ 5800 MHz; Calibrated: 31.12.2019
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.12.2019
- Phantom: Flat Phantom 5.0 (front); Type: QD 000 P50 AA; Serial: 1001
- DASY52 52.10.3(1513); SEMCAD X 14.6.13(7474)

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 77.00 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 28.9 W/kg SAR(1 g) = 8.05 W/kg; SAR(10 g) = 2.28 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 68.9% Maximum value of SAR (measured) = 18.6 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 77.20 V/m; Power Drift = -0.04 dB Peak SAR (extrapolated) = 30.2 W/kg SAR(1 g) = 8.32 W/kg; SAR(10 g) = 2.35 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 68.8% Maximum value of SAR (measured) = 19.4 W/kg

Certificate No: D5GHzV2-1023 Jan20

Page 7 of 9

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law


No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

f (886-2) 2298-0488



Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 77.04 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 31.6 W/kg SAR(1 g) = 8.36 W/kg; SAR(10 g) = 2.37 W/kg Smallest distance from peaks to all points 3 dB below = 7.4 mm Ratio of SAR at M2 to SAR at M1 = 67.1% Maximum value of SAR (measured) = 19.9 W/kg

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 75.51 V/m; Power Drift = -0.04 dB Peak SAR (extrapolated) = 33.1 W/kg SAR(1 g) = 8.19 W/kg; SAR(10 g) = 2.29 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 65.2% Maximum value of SAR (measured) = 19.8 W/kg

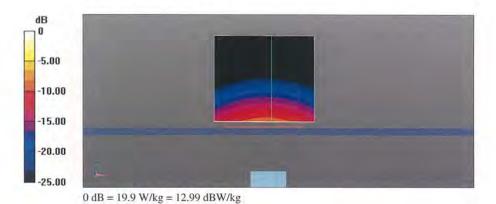

Certificate No: D5GHzV2-1023\_Jan20

Page 8 of 9

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

t (886-2) 2299-3279 台灣檢驗科技股份有限公司


f (886-2) 2298-0488

www.sgs.com.tw



Report No: ES/2020/C0014 Rev: 01 Page: 16 of 16

Impedance Measurement Plot for Head TSL

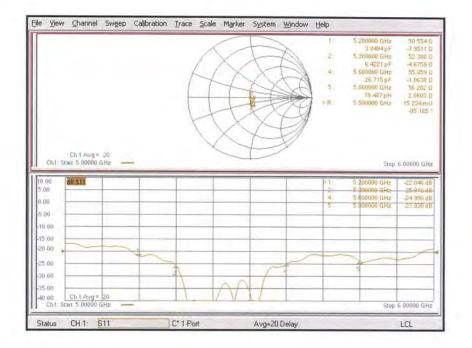

Certificate No: D5GHzV2-1023 Jan20

Page 9 of 9

# - End of report -

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.

除非另有說明,此報告結果僅對測試之樣品負責,同時此樣品僅保留90天。本報告未經本公司書面許可,不可部份複製。 This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <u>http://www.sgs.com.tw/Terms-and-Conditions</u> and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com.tw/Terms-and-Conditions">http://www.sgs.com.tw/Terms-and-Conditions</a>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

No.134,Wu Kung Road, New Taipei Industrial Park, Wuku District, New Taipei City, Taiwan/新北市五股區新北產業園區五工路 134 號

t (886-2) 2299-3279 台灣檢驗科技股份有限公司

f (886-2) 2298-0488

www.sgs.com.tw