

APPENDIX

10. Photographs of Test Setup



Fig.1 Photograph of the SAR Measurement System

Photograph of the Tissue Simulant Fluid Liquid Depth

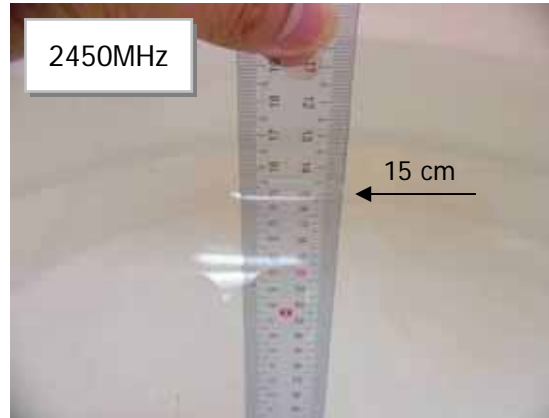


Fig.2. Flat (Body)

Body worn - distance between flat phantom and EUT is 0 mm

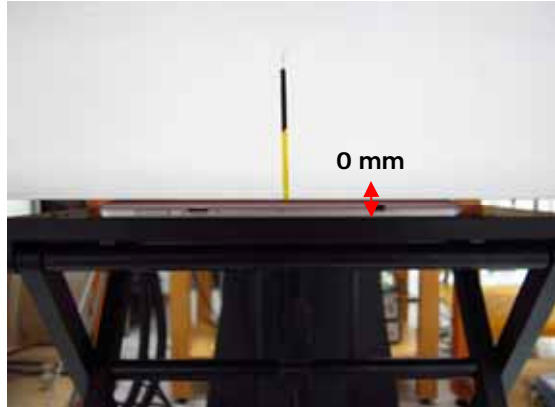


Fig.3 EUT Lap held mode to flat phantom

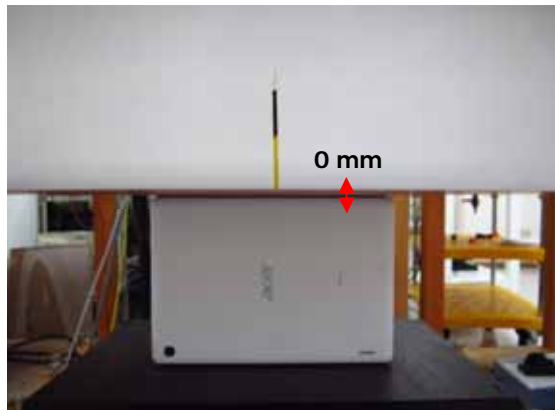


Fig.4 EUT Edge 1 to flat phantom

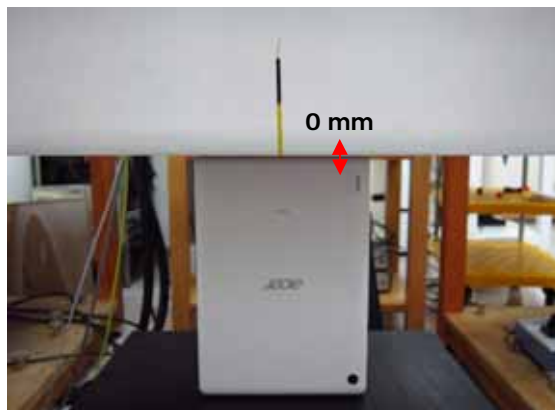


Fig.5 EUT Edge 3 to flat phantom

- End of 2nd part of report -