

### System Check\_Head\_2450MHz

#### DUT: D2450V2 - SN806

Communication System: CW; Frequency: 2450.000 MHz

Medium: HSL\_2450\_240421 Medium parameters used:  $f = 2450.000$  MHz;  $\sigma = 1.83$  S/m;  $\epsilon_r = 38.9$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7692; ConvF(7.59, 7.41, 8.57); Calibrated: 2023-07-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2023-09-13
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.65 W/kg; SAR (10g) = 1.22 W/kg;


**Pin=17.0dBm/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.62 W/kg; SAR (8g) = 1.35 W/kg; SAR (10g) = 1.22 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 80.8 %

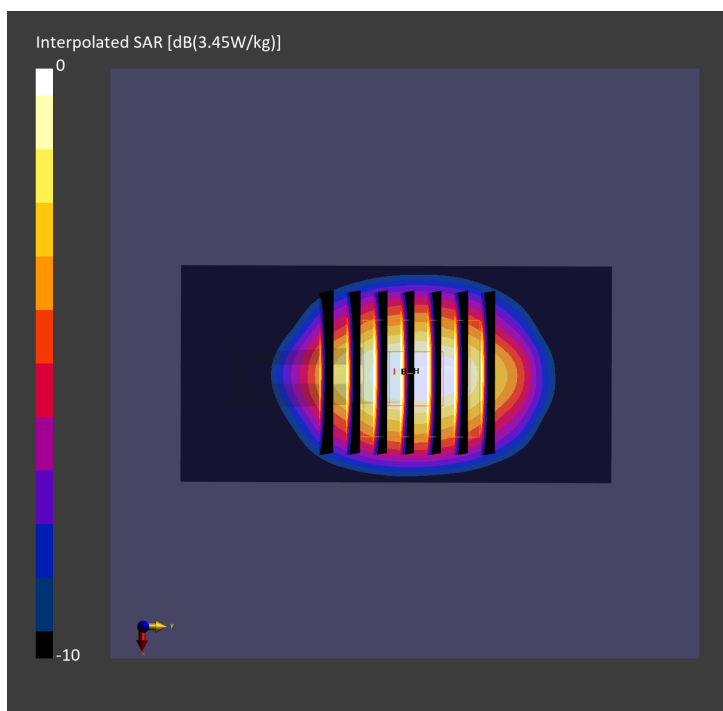

### System Check\_Head\_5250MHz

#### DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5250.000 MHz

Medium: HSL\_5250\_240421 Medium parameters used:  $f= 5250.000$  MHz;  $\sigma= 4.61$  S/m;  $\epsilon_r = 36.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7692; ConvF(5.84, 5.74, 6.7); Calibrated: 2023-07-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2023-09-13
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.11 W/kg; SAR (10g) = 1.16 W/kg;


**Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 4.23 W/kg; SAR (8g) = 1.40 W/kg; SAR (10g) = 1.20 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 65.4 %

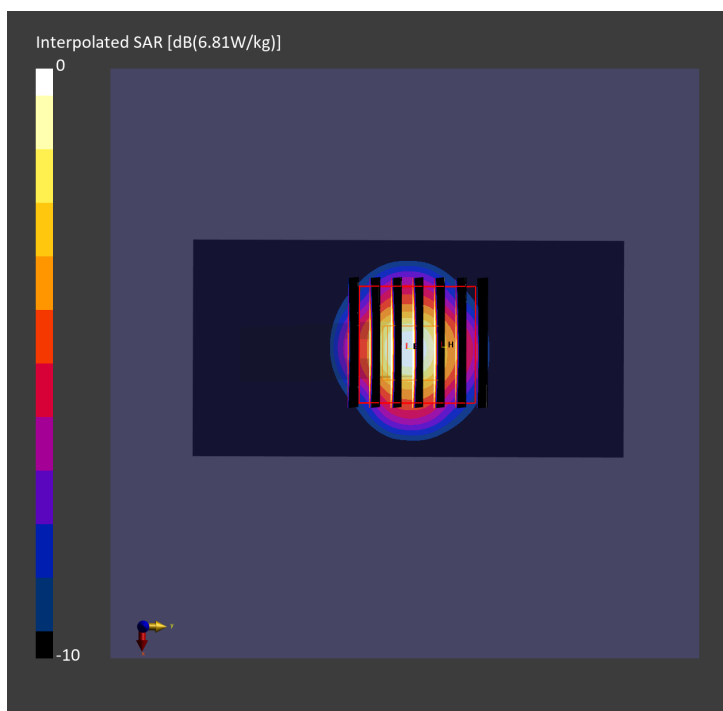

## System Check\_Head\_5600MHz

### DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5600.000 MHz

Medium: HSL\_5600\_240421 Medium parameters used:  $f=5600.000$  MHz;  $\sigma=4.94$  S/m;  $\epsilon_r=35.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7692; ConvF(5.09, 4.94, 5.73); Calibrated: 2023-07-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2023-09-13
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.41 W/kg; SAR (10g) = 1.23 W/kg;


**Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.07 dB

SAR (1g) = 4.46 W/kg; SAR (8g) = 1.49 W/kg; SAR (10g) = 1.28 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 62.7 %



### System Check\_Head\_5750MHz

#### DUT: D5GHzV2 - SN1006

Communication System: CW; Frequency: 5750.000 MHz

Medium: HSL\_5750\_240421 Medium parameters used:  $f = 5750.000$  MHz;  $\sigma = 5.08$  S/m;  $\epsilon_r = 35.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.2°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7692; ConvF(5.23, 5.12, 5.97); Calibrated: 2023-07-18
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1311; Calibrated: 2023-09-13
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1719; Section: Flat
- Measurement Software: 16.2.4.2524
- UID: CW, 0--

**Pin=17.0dBm/Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.91 W/kg; SAR (10g) = 1.09 W/kg;

**Pin=17.0dBm/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.05 dB

SAR (1g) = 4.05 W/kg; SAR (8g) = 1.33 W/kg; SAR (10g) = 1.14 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 61.6 %

