




## Calibration Certificate of DASY

### Impedance Measurement Plot for Head TSL



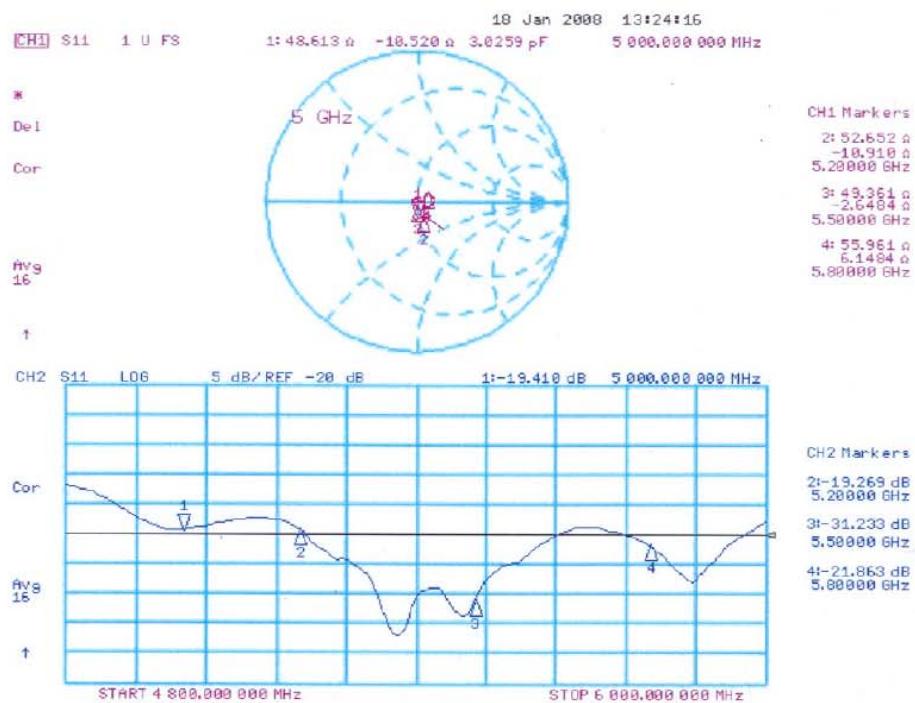

## Calibration Certificate of DASY

### DASY4 Validation Report for Body TSL

Date/Time: 24.01.2008 15:14:55

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole 5GHz; Type: D5GHz; Serial: D5GHzV2 - SN:1006

Communication System: CW-5GHz; Frequency: 5200 MHz, 5500 MHz, 5800 MHz; Duty Cycle: 1:1  
Medium: MSL 5800 MHz;

Medium parameters used:  $f = 5200 \text{ MHz}$ ;  $\sigma = 5.37 \text{ mho/m}$ ;  $\epsilon_r = 47.3$ ;  $\rho = 1000 \text{ kg/m}^3$

Medium parameters used:  $f = 5500 \text{ MHz}$ ;  $\sigma = 5.73 \text{ mho/m}$ ;  $\epsilon_r = 46.6$ ;  $\rho = 1000 \text{ kg/m}^3$

Medium parameters used:  $f = 5800 \text{ MHz}$ ;  $\sigma = 6.16 \text{ mho/m}$ ;  $\epsilon_r = 46.1$ ;  $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(4.96, 4.96, 4.96)ConvF(4.63, 4.63, 4.63)ConvF(4.76, 4.76, 4.76); Calibrated: 09.03.2007
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 03.01.2008
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

#### d=10mm, Pin=100mW, f=5200 MHz/Area Scan (61x61x1):

Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (interpolated) = 17.0 mW/g

#### d=10mm, Pin=100mW, f=5200 MHz/Zoom Scan (8x8x10), dist=2mm (8x8x10)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 48.5 V/m; Power Drift = -0.066 dB

Peak SAR (extrapolated) = 28.0 W/kg

SAR(1 g) = 7.77 mW/g; SAR(10 g) = 2.18 mW/g

Maximum value of SAR (measured) = 15.5 mW/g

#### d=10mm, Pin=100mW, f=5500 MHz/Zoom Scan (8x8x10), dist=2mm (8x8x10)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 47.2 V/m; Power Drift = -0.067 dB

Peak SAR (extrapolated) = 32.2 W/kg

SAR(1 g) = 8.12 mW/g; SAR(10 g) = 2.26 mW/g

Maximum value of SAR (measured) = 16.6 mW/g

#### d=10mm, Pin=100mW, f=5800 MHz/Zoom Scan (8x8x10), dist=2mm (8x8x10)/Cube 0:

Measurement grid: dx=4mm, dy=4mm, dz=2.5mm

Reference Value = 42.3 V/m; Power Drift = -0.131 dB


Peak SAR (extrapolated) = 28.9 W/kg

SAR(1 g) = 7.04 mW/g; SAR(10 g) = 1.95 mW/g

Maximum value of SAR (measured) = 14.5 mW/g



## Calibration Certificate of DASY

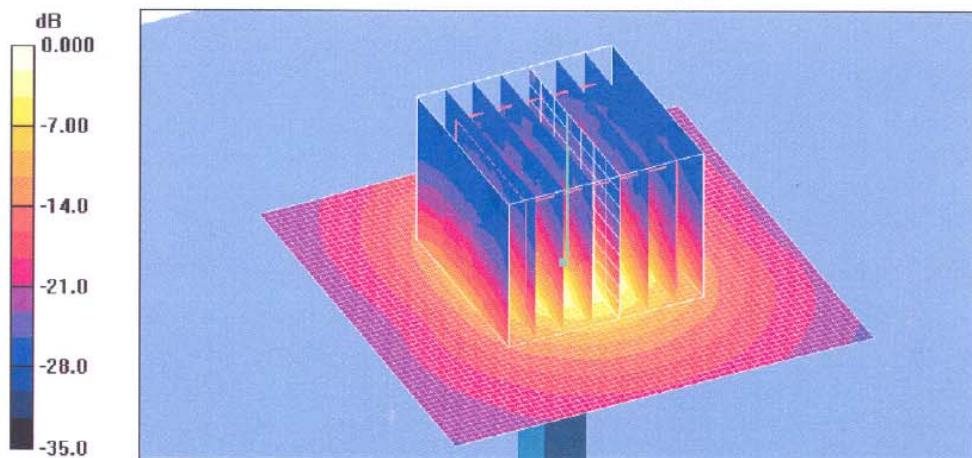


0 dB = 14.5mW/g



## Calibration Certificate of DASY

### Impedance Measurement Plot for Body TSL

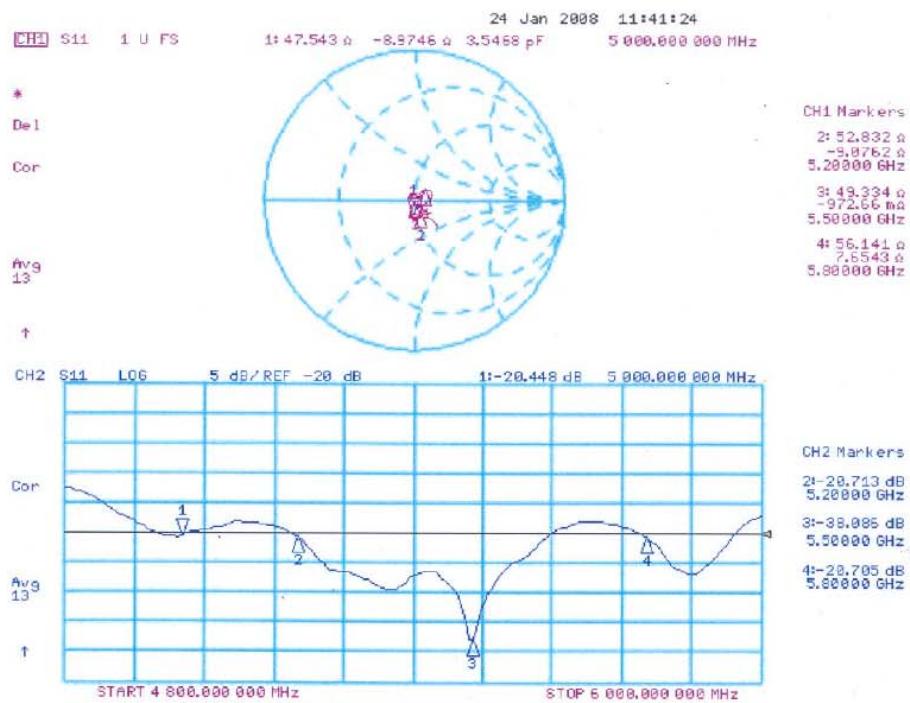



## Calibration Certificate of DASY

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client Sporton (Auden)

Certificate No: DAE4-778\_Sep08

### CALIBRATION CERTIFICATE

Object DAE4 - SD 000 D04 BG - SN: 778

Calibration procedure(s) QA CAL-06.v12  
Calibration procedure for the data acquisition electronics (DAE)

Calibration date: September 22, 2008

Condition of the calibrated item In Tolerance

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards                 | ID #               | Cal Date (Certificate No.) | Scheduled Calibration  |
|-----------------------------------|--------------------|----------------------------|------------------------|
| Fluke Process Calibrator Type 702 | SN: 6295803        | 04-Oct-07 (No: 6467)       | Oct-08                 |
| Keithley Multimeter Type 2001     | SN: 0810278        | 03-Oct-07 (No: 6465)       | Oct-08                 |
| Secondary Standards               | ID #               | Check Date (in house)      | Scheduled Check        |
| Calibrator Box V1.1               | SE UMS 006 AB 1004 | 06-Jun-08 (in house check) | In house check: Jun-09 |

Calibrated by: Name Andrea Guntli Function Technician Signature

Approved by: Name Fin Bornholt Function R&D Director Signature

Issued: September 22, 2008

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: DAE4-778\_Sep08

Page 1 of 5



## Calibration Certificate of DASY

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

### Glossary

|                 |                                                                                         |
|-----------------|-----------------------------------------------------------------------------------------|
| DAE             | data acquisition electronics                                                            |
| Connector angle | information used in DASY system to align probe sensor X to the robot coordinate system. |

### Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement*: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle*: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - *DC Voltage Measurement Linearity*: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - *Common mode sensitivity*: Influence of a positive or negative common mode voltage on the differential measurement.
  - *Channel separation*: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - *AD Converter Values with inputs shorted*: Values on the internal AD converter corresponding to zero input voltage
  - *Input Offset Measurement*: Output voltage and statistical results over a large number of zero voltage measurements.
  - *Input Offset Current*: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - *Input resistance*: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - *Low Battery Alarm Voltage*: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - *Power consumption*: Typical value for information. Supply currents in various operating modes.



## Calibration Certificate of DASY

### DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB =  $6.1\mu V$ , full range =  $-100...+300\text{ mV}$

Low Range: 1LSB =  $61\text{nV}$ , full range =  $-1.....+3\text{mV}$

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

| Calibration Factors | X                                | Y                                | Z                                |
|---------------------|----------------------------------|----------------------------------|----------------------------------|
| High Range          | $404.686 \pm 0.1\% (\text{k}=2)$ | $403.490 \pm 0.1\% (\text{k}=2)$ | $405.045 \pm 0.1\% (\text{k}=2)$ |
| Low Range           | $3.99455 \pm 0.7\% (\text{k}=2)$ | $3.96369 \pm 0.7\% (\text{k}=2)$ | $3.99417 \pm 0.7\% (\text{k}=2)$ |

### Connector Angle

|                                           |                         |
|-------------------------------------------|-------------------------|
| Connector Angle to be used in DASY system | $309^\circ \pm 1^\circ$ |
|-------------------------------------------|-------------------------|



## Calibration Certificate of DASY

### Appendix

#### 1. DC Voltage Linearity

| High Range        | Input (µV) | Reading (µV) | Error (%) |
|-------------------|------------|--------------|-----------|
| Channel X + Input | 200000     | 200000.3     | 0.00      |
| Channel X + Input | 20000      | 20004.24     | 0.02      |
| Channel X - Input | 20000      | -20002.46    | 0.01      |
| Channel Y + Input | 200000     | 200000.4     | 0.00      |
| Channel Y + Input | 20000      | 20002.60     | 0.01      |
| Channel Y - Input | 20000      | -20002.26    | 0.01      |
| Channel Z + Input | 200000     | 200000.6     | 0.00      |
| Channel Z + Input | 20000      | 20000.78     | 0.00      |
| Channel Z - Input | 20000      | -20005.75    | 0.03      |

| Low Range         | Input (µV) | Reading (µV) | Error (%) |
|-------------------|------------|--------------|-----------|
| Channel X + Input | 2000       | 2000         | 0.00      |
| Channel X + Input | 200        | 199.37       | -0.31     |
| Channel X - Input | 200        | -200.28      | 0.14      |
| Channel Y + Input | 2000       | 2000         | 0.00      |
| Channel Y + Input | 200        | 199.63       | -0.19     |
| Channel Y - Input | 200        | -200.88      | 0.44      |
| Channel Z + Input | 2000       | 2000.1       | 0.00      |
| Channel Z + Input | 200        | 198.60       | -0.70     |
| Channel Z - Input | 200        | -201.07      | 0.53      |

#### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Common mode<br>Input Voltage (mV) | High Range<br>Average Reading (µV) | Low Range<br>Average Reading (µV) |
|-----------|-----------------------------------|------------------------------------|-----------------------------------|
| Channel X | 200                               | -7.46                              | -6.40                             |
|           | -200                              | 10.00                              | 6.86                              |
| Channel Y | 200                               | -2.73                              | -2.45                             |
|           | -200                              | 0.84                               | 0.43                              |
| Channel Z | 200                               | -10.91                             | -10.94                            |
|           | -200                              | 7.89                               | 8.22                              |

#### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | Input Voltage (mV) | Channel X (µV) | Channel Y (µV) | Channel Z (µV) |
|-----------|--------------------|----------------|----------------|----------------|
| Channel X | 200                | -              | 3.08           | -1.34          |
| Channel Y | 200                | 1.18           | -              | 4.64           |
| Channel Z | 200                | -1.74          | 1.44           | -              |



## Calibration Certificate of DASY

### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

|           | High Range (LSB) | Low Range (LSB) |
|-----------|------------------|-----------------|
| Channel X | 16048            | 16021           |
| Channel Y | 16167            | 15166           |
| Channel Z | 16416            | 15977           |

### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10MΩ

|           | Average ( $\mu$ V) | min. Offset ( $\mu$ V) | max. Offset ( $\mu$ V) | Std. Deviation ( $\mu$ V) |
|-----------|--------------------|------------------------|------------------------|---------------------------|
| Channel X | -0.13              | -0.88                  | 0.92                   | 0.33                      |
| Channel Y | -0.88              | -2.47                  | 0.72                   | 0.55                      |
| Channel Z | -1.16              | -2.17                  | -0.19                  | 0.42                      |

### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

### 7. Input Resistance

|           | Zeroing (MΩ) | Measuring (MΩ) |
|-----------|--------------|----------------|
| Channel X | 0.2000       | 201.1          |
| Channel Y | 0.2000       | 201.0          |
| Channel Z | 0.2001       | 201.7          |

### 8. Low Battery Alarm Voltage (verified during pre test)

| Typical values | Alarm Level (VDC) |
|----------------|-------------------|
| Supply (+ Vcc) | +7.9              |
| Supply (- Vcc) | -7.6              |

### 9. Power Consumption (verified during pre test)

| Typical values | Switched off (mA) | Stand by (mA) | Transmitting (mA) |
|----------------|-------------------|---------------|-------------------|
| Supply (+ Vcc) | +0.0              | +6            | +14               |
| Supply (- Vcc) | -0.01             | -8            | -9                |



## Calibration Certificate of DASY

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client Sporton (Auden)

Certificate No: ET3-1788\_Sep08

### CALIBRATION CERTIFICATE

Object ET3DV6 - SN:1788

Calibration procedure(s) QA CAL-01.v6 and QA CAL-23.v3  
Calibration procedure for dosimetric E-field probes

Calibration date: September 23, 2008

Condition of the calibrated item In Tolerance

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID #            | Cal Date (Certificate No.)    | Scheduled Calibration |
|----------------------------|-----------------|-------------------------------|-----------------------|
| Power meter E4419B         | GB41293874      | 1-Apr-08 (No. 217-00788)      | Apr-09                |
| Power sensor E4412A        | MY41495277      | 1-Apr-08 (No. 217-00788)      | Apr-09                |
| Power sensor E4412A        | MY41498087      | 1-Apr-08 (No. 217-00788)      | Apr-09                |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 1-Jul-08 (No. 217-00865)      | Jul-09                |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 31-Mar-08 (No. 217-00787)     | Apr-09                |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 1-Jul-08 (No. 217-00866)      | Jul-09                |
| Reference Probe ES3DV2     | SN: 3013        | 2-Jan-08 (No. ES3-3013_Jan08) | Jan-09                |
| DAE4                       | SN: 660         | 9-Sep-08 (No. DAE4-660_Sep08) | Sep-09                |

| Secondary Standards       | ID #         | Check Date (in house)             | Scheduled Check        |
|---------------------------|--------------|-----------------------------------|------------------------|
| RF generator HP 8648C     | US3642U01700 | 4-Aug-99 (in house check Oct-07)  | In house check: Oct-09 |
| Network Analyzer HP 8753E | US37390585   | 18-Oct-01 (in house check Oct-07) | In house check: Oct-08 |

| Calibrated by: | Name          | Function          | Signature |
|----------------|---------------|-------------------|-----------|
|                | Katja Pokovic | Technical Manager |           |

| Approved by: | Name        | Function     | Signature |
|--------------|-------------|--------------|-----------|
|              | Fin Bomholt | R&D Director |           |

Issued: September 24, 2008

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



## Calibration Certificate of DASY

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

### Glossary:

|                        |                                                                                                                                                |
|------------------------|------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                    | tissue simulating liquid                                                                                                                       |
| NORMx,y,z              | sensitivity in free space                                                                                                                      |
| ConvF                  | sensitivity in TSL / NORMx,y,z                                                                                                                 |
| DCP                    | diode compression point                                                                                                                        |
| Polarization $\varphi$ | $\varphi$ rotation around probe axis                                                                                                           |
| Polarization $\theta$  | $\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis |

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- $NORMx,y,z$ : Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide).  $NORMx,y,z$  are only intermediate values, i.e., the uncertainties of  $NORMx,y,z$  does not effect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- $NORM(f)x,y,z = NORMx,y,z * frequency\_response$  (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- $DCPx,y,z$ : DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- *ConvF and Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to  $NORMx,y,z * ConvF$  whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- *Spherical isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.



ET3DV6 SN:1788

September 23, 2008

# Probe ET3DV6

## SN:1788

|                  |                    |
|------------------|--------------------|
| Manufactured:    | May 28, 2003       |
| Last calibrated: | September 26, 2007 |
| Recalibrated:    | September 23, 2008 |

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)



## Calibration Certificate of DASY

ET3DV6 SN:1788

September 23, 2008

### DASY - Parameters of Probe: ET3DV6 SN:1788

#### Sensitivity in Free Space<sup>A</sup>

|       |                   |                                     |
|-------|-------------------|-------------------------------------|
| NormX | $1.73 \pm 10.1\%$ | $\mu\text{V}/(\text{V}/\text{m})^2$ |
| NormY | $1.59 \pm 10.1\%$ | $\mu\text{V}/(\text{V}/\text{m})^2$ |
| NormZ | $1.72 \pm 10.1\%$ | $\mu\text{V}/(\text{V}/\text{m})^2$ |

#### Diode Compression<sup>B</sup>

|       |       |
|-------|-------|
| DCP X | 95 mV |
| DCP Y | 98 mV |
| DCP Z | 91 mV |

#### Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

#### Boundary Effect

TSL            900 MHz        Typical SAR gradient: 5 % per mm

|                                                         |        |        |
|---------------------------------------------------------|--------|--------|
| Sensor Center to Phantom Surface Distance               | 3.7 mm | 4.7 mm |
| SAR <sub>be</sub> [%]      Without Correction Algorithm | 10.6   | 6.8    |
| SAR <sub>be</sub> [%]      With Correction Algorithm    | 0.8    | 0.3    |

TSL            1750 MHz        Typical SAR gradient: 10 % per mm

|                                                         |        |        |
|---------------------------------------------------------|--------|--------|
| Sensor Center to Phantom Surface Distance               | 3.7 mm | 4.7 mm |
| SAR <sub>be</sub> [%]      Without Correction Algorithm | 8.8    | 4.9    |
| SAR <sub>be</sub> [%]      With Correction Algorithm    | 0.7    | 0.6    |

#### Sensor Offset

Probe Tip to Sensor Center            2.7 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 8).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.




ET3DV6 SN:1788

September 23, 2008

## Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

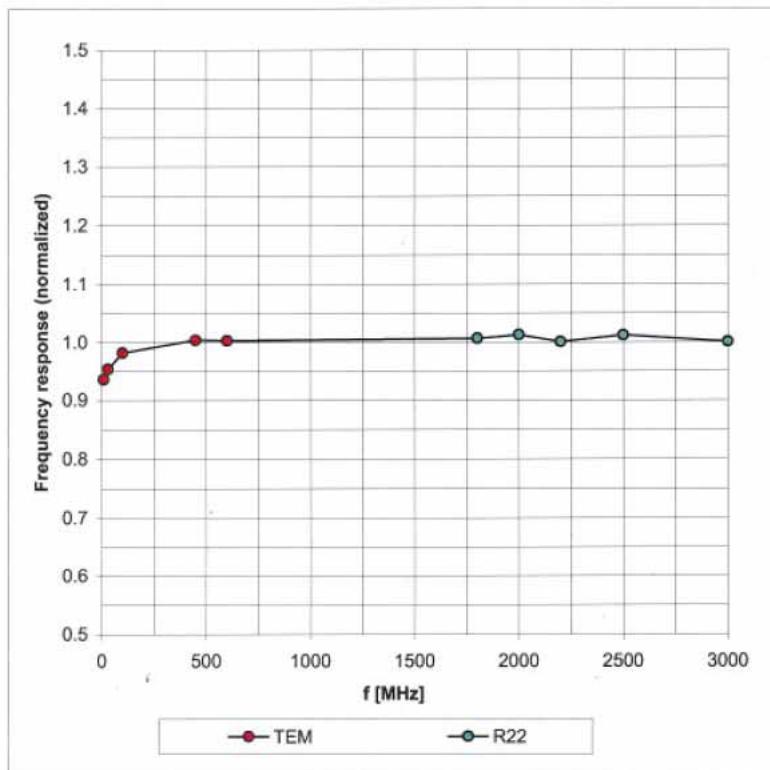

Uncertainty of Frequency Response of E-field:  $\pm 6.3\% (k=2)$





## Calibration Certificate of DASY

ET3DV6 SN:1788

September 23, 2008

### Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

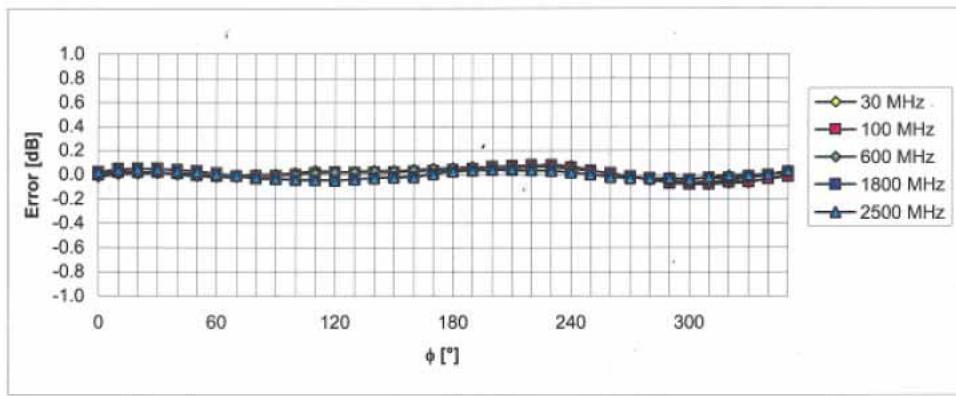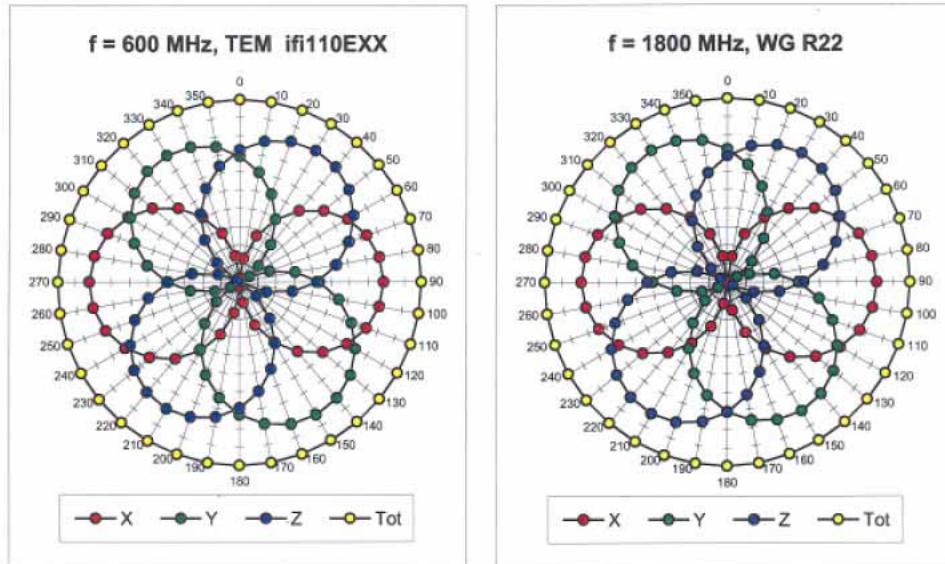

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )




## Calibration Certificate of DASY

ET3DV6 SN:1788

September 23, 2008

### Dynamic Range f(SAR<sub>head</sub>) (Waveguide R22, f = 1800 MHz)

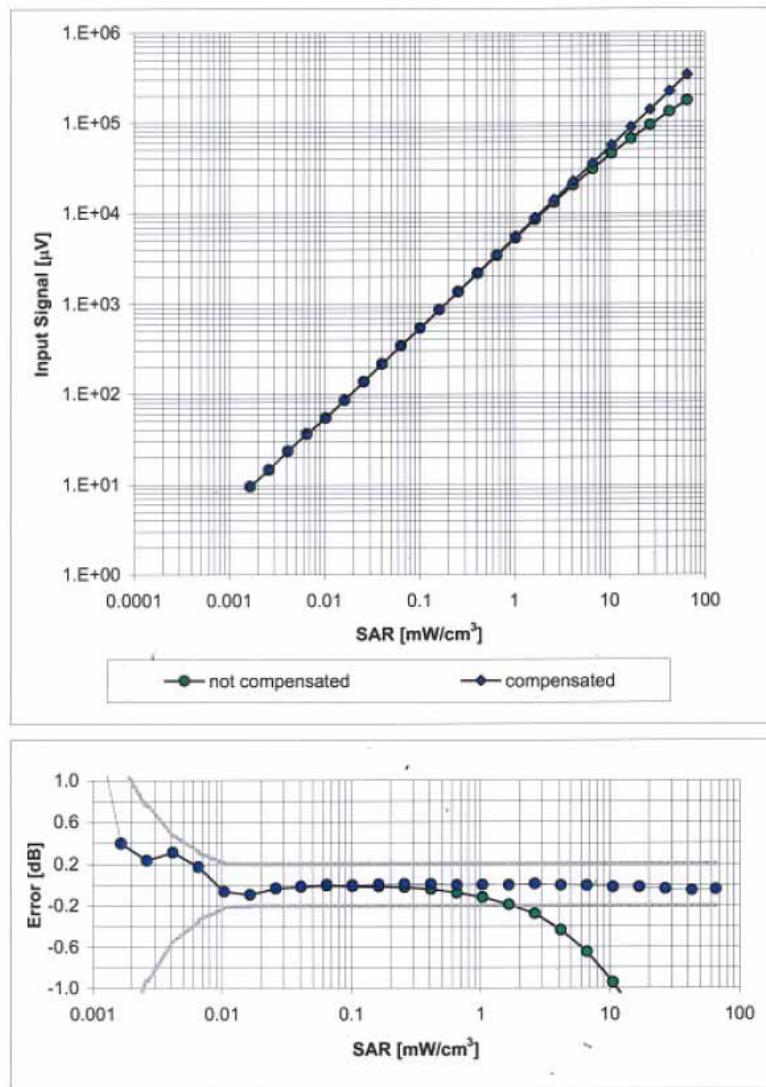


Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )



ET3DV6 SN:1788

September 23, 2008

## Conversion Factor Assessment

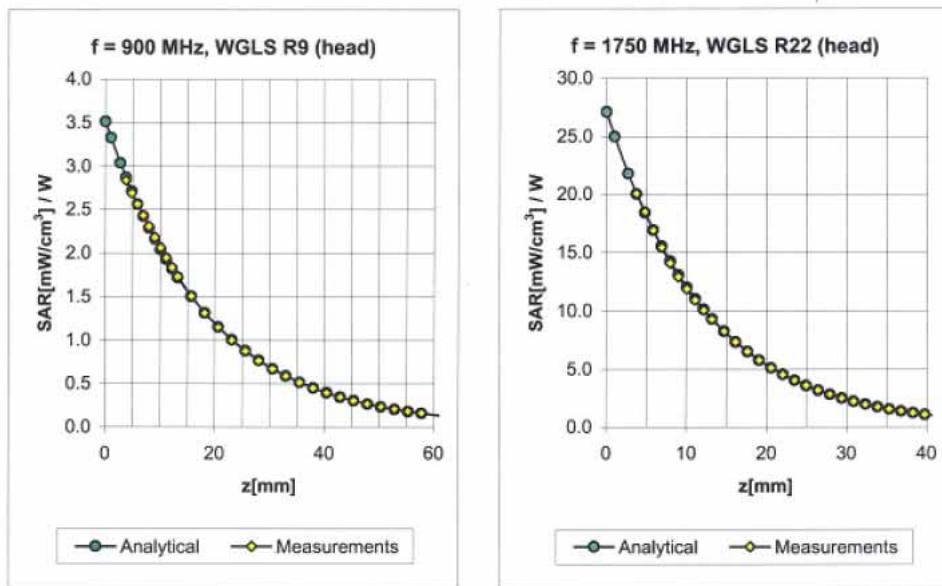

| f [MHz] | Validity [MHz] <sup>c</sup> | TSL  | Permittivity   | Conductivity   | Alpha | Depth | ConvF | Uncertainty        |
|---------|-----------------------------|------|----------------|----------------|-------|-------|-------|--------------------|
| 900     | $\pm 50 / \pm 100$          | Head | $41.5 \pm 5\%$ | $0.97 \pm 5\%$ | 0.44  | 2.65  | 6.55  | $\pm 11.0\% (k=2)$ |
| 1750    | $\pm 50 / \pm 100$          | Head | $40.1 \pm 5\%$ | $1.37 \pm 5\%$ | 0.68  | 1.98  | 5.59  | $\pm 11.0\% (k=2)$ |
| 1950    | $\pm 50 / \pm 100$          | Head | $40.0 \pm 5\%$ | $1.40 \pm 5\%$ | 0.75  | 1.75  | 5.13  | $\pm 11.0\% (k=2)$ |
| 2450    | $\pm 50 / \pm 100$          | Head | $39.2 \pm 5\%$ | $1.80 \pm 5\%$ | 0.80  | 1.45  | 4.68  | $\pm 11.0\% (k=2)$ |

|      |                    |      |                |                |      |      |      |                    |
|------|--------------------|------|----------------|----------------|------|------|------|--------------------|
| 900  | $\pm 50 / \pm 100$ | Body | $55.0 \pm 5\%$ | $1.05 \pm 5\%$ | 0.50 | 2.48 | 6.34 | $\pm 11.0\% (k=2)$ |
| 1750 | $\pm 50 / \pm 100$ | Body | $53.4 \pm 5\%$ | $1.49 \pm 5\%$ | 0.63 | 2.33 | 4.87 | $\pm 11.0\% (k=2)$ |
| 1950 | $\pm 50 / \pm 100$ | Body | $53.3 \pm 5\%$ | $1.52 \pm 5\%$ | 0.74 | 1.99 | 4.73 | $\pm 11.0\% (k=2)$ |
| 2450 | $\pm 50 / \pm 100$ | Body | $52.7 \pm 5\%$ | $1.95 \pm 5\%$ | 0.94 | 1.75 | 3.98 | $\pm 11.0\% (k=2)$ |

<sup>c</sup> The validity of  $\pm 100$  MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.




ET3DV6 SN:1788

September 23, 2008

### Deviation from Isotropy in HSL

Error ( $\phi, \theta$ ),  $f = 900$  MHz

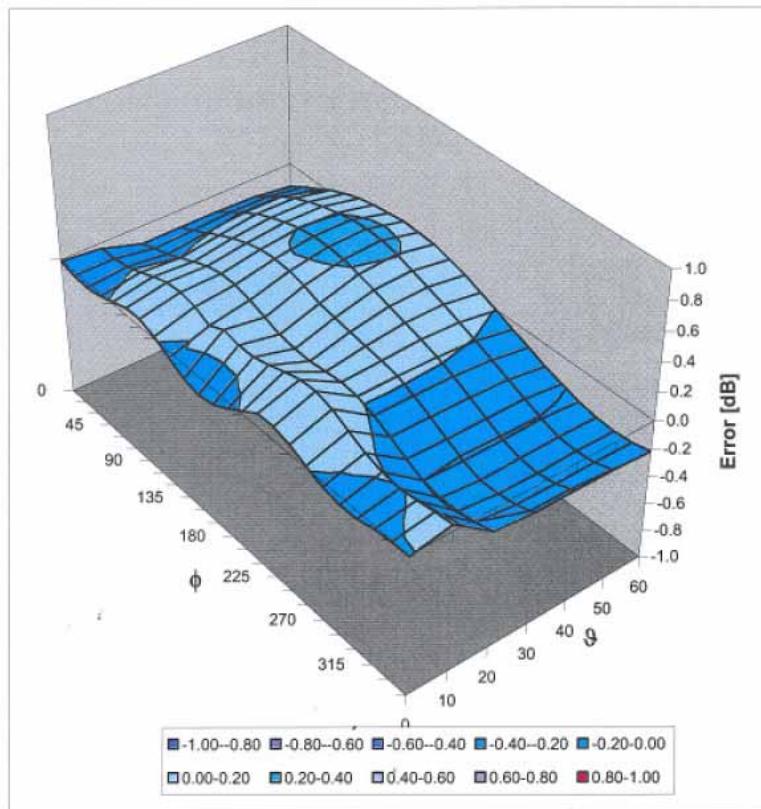

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  ( $k=2$ )



## Calibration Certificate of DASY

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client Sporton (Auden)

Certificate No: EX3-3514\_Jan08

### CALIBRATION CERTIFICATE

|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |                                                                                      |                                           |                          |
|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|-------------------------------------------|--------------------------|
| Object                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          | EX3DV3 - SN:3514                                                                     |                                           |                          |
| Calibration procedure(s)                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        | QA CAL-01.v6 and QA CAL.14.v3<br>Calibration procedure for dosimetric E-field probes |                                           |                          |
| Calibration date:                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               | January 31, 2008                                                                     |                                           |                          |
| Condition of the calibrated item                                                                                                                                                                                                                                                                                                                                                                                                                                                                                | In Tolerance                                                                         |                                           |                          |
| <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (<math>22 \pm 3</math>)°C and humidity &lt; 70%.</p> <p>Calibration Equipment used (M&amp;TE critical for calibration)</p> |                                                                                      |                                           |                          |
| Primary Standards                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               | ID #                                                                                 | Cal Date (Calibrated by, Certificate No.) | Scheduled Calibration    |
| Power meter E4419B                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              | GB41293874                                                                           | 29-Mar-07 (METAS, No. 217-00670)          | Mar-08                   |
| Power sensor E4412A                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             | MY41495277                                                                           | 29-Mar-07 (METAS, No. 217-00670)          | Mar-08                   |
| Power sensor E4412A                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             | MY41496087                                                                           | 29-Mar-07 (METAS, No. 217-00670)          | Mar-08                   |
| Reference 3 dB Attenuator                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       | SN: S5054 (3c)                                                                       | 8-Aug-07 (METAS, No. 217-00719)           | Aug-08                   |
| Reference 20 dB Attenuator                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      | SN: S5086 (20b)                                                                      | 29-Mar-07 (METAS, No. 217-00671)          | Mar-08                   |
| Reference 30 dB Attenuator                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      | SN: S5129 (30b)                                                                      | 8-Aug-07 (METAS, No. 217-00720)           | Aug-08                   |
| Reference Probe ES3DV2                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          | SN: 3013                                                                             | 2-Jan-08 (SPEAG, No. ES3-3013_Jan08)      | Jan-09                   |
| DAE4                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            | SN: 654                                                                              | 20-Apr-07 (SPEAG, No. DAE4-654_Apr07)     | Apr-08                   |
| Secondary Standards                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             | ID #                                                                                 | Check Date (in house)                     | Scheduled Check          |
| RF generator HP 8648C                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           | US3642U01700                                                                         | 4-Aug-99 (SPEAG, in house check Oct-07)   | In house check: Oct-09   |
| Network Analyzer HP 8753E                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       | US37390585                                                                           | 18-Oct-01 (SPEAG, in house check Oct-07)  | In house check: Oct-08   |
| Calibrated by:                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  | Name                                                                                 | Function                                  | Signature                |
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 | Katja Pokovic                                                                        | Technical Manager                         |                          |
| Approved by:                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    | Niels Kuster                                                                         | Quality Manager                           |                          |
| This calibration certificate shall not be reproduced except in full without written approval of the laboratory.                                                                                                                                                                                                                                                                                                                                                                                                 |                                                                                      |                                           | Issued: January 31, 2008 |

Certificate No: EX3-3514\_Jan08

Page 1 of 9



## Calibration Certificate of DASY

**Calibration Laboratory of**  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

### Glossary:

|                        |                                                                                                                                                |
|------------------------|------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                    | tissue simulating liquid                                                                                                                       |
| NORMx,y,z              | sensitivity in free space                                                                                                                      |
| ConvF                  | sensitivity in TSL / NORMx,y,z                                                                                                                 |
| DCP                    | diode compression point                                                                                                                        |
| Polarization $\varphi$ | $\varphi$ rotation around probe axis                                                                                                           |
| Polarization $\theta$  | $\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis |

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- *NORMx,y,z*: Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). *NORMx,y,z* are only intermediate values, i.e., the uncertainties of *NORMx,y,z* does not effect the  $E^2$ -field uncertainty inside TSL (see below *ConvF*).
- *NORM(f)x,y,z* = *NORMx,y,z* \* *frequency\_response* (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- *DCPx,y,z*: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- *ConvF and Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to *NORMx,y,z* \* *ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- *Spherical isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.



## ***Calibration Certificate of DASY***

---

**EX3DV3 SN:3514**

**January 31, 2008**

# **Probe EX3DV3**

## **SN:3514**

|                  |                   |
|------------------|-------------------|
| Manufactured:    | December 15, 2002 |
| Last calibrated: | February 21, 2007 |
| Recalibrated:    | January 31, 2008  |

**Calibrated for DASY Systems**

(Note: non-compatible with DASY2 system!)



## Calibration Certificate of DASY

EX3DV3 SN:3514

January 31, 2008

### DASY - Parameters of Probe: EX3DV3 SN:3514

#### Sensitivity in Free Space<sup>A</sup>

|       |                      |                                     |
|-------|----------------------|-------------------------------------|
| NormX | <b>0.650</b> ± 10.1% | $\mu\text{V}/(\text{V}/\text{m})^2$ |
| NormY | <b>0.690</b> ± 10.1% | $\mu\text{V}/(\text{V}/\text{m})^2$ |
| NormZ | <b>0.580</b> ± 10.1% | $\mu\text{V}/(\text{V}/\text{m})^2$ |

#### Diode Compression<sup>B</sup>

|       |              |
|-------|--------------|
| DCP X | <b>95</b> mV |
| DCP Y | <b>93</b> mV |
| DCP Z | <b>96</b> mV |

#### Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

#### Boundary Effect

TSL            2300 MHz        Typical SAR gradient: 10 % per mm

|                                                    |        |        |
|----------------------------------------------------|--------|--------|
| Sensor Center to Phantom Surface Distance          | 2.0 mm | 3.0 mm |
| SAR <sub>be</sub> [%] Without Correction Algorithm | 5.9    | 3.3    |
| SAR <sub>be</sub> [%] With Correction Algorithm    | 0.5    | 0.8    |

TSL            2600 MHz        Typical SAR gradient: 11 % per mm

|                                                    |        |        |
|----------------------------------------------------|--------|--------|
| Sensor Center to Phantom Surface Distance          | 2.0 mm | 3.0 mm |
| SAR <sub>be</sub> [%] Without Correction Algorithm | 6.3    | 3.4    |
| SAR <sub>be</sub> [%] With Correction Algorithm    | 0.1    | 0.3    |

#### Sensor Offset

Probe Tip to Sensor Center        **1.0** mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 8).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.




## Calibration Certificate of DASY

EX3DV3 SN:3514

January 31, 2008

### Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

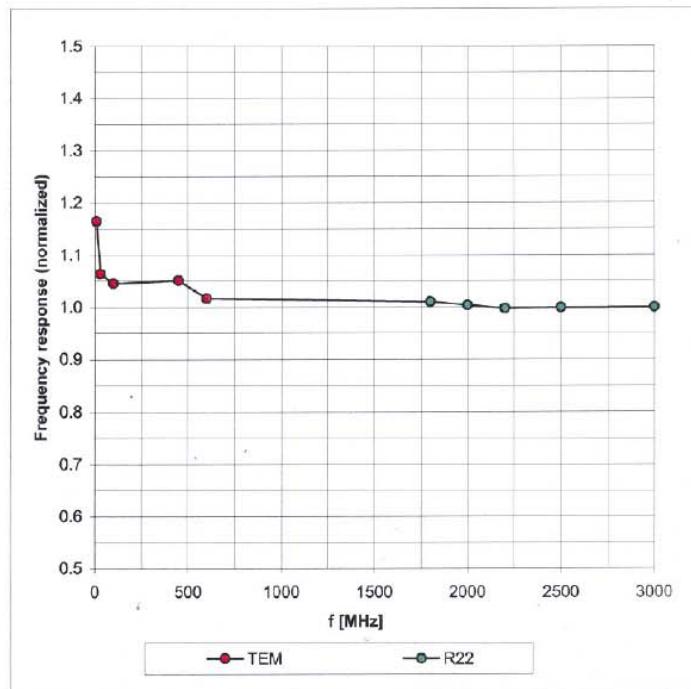

Uncertainty of Frequency Response of E-field:  $\pm 6.3\% \text{ (k=2)}$





## Calibration Certificate of DASY

EX3DV3 SN:3514

January 31, 2008

### Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

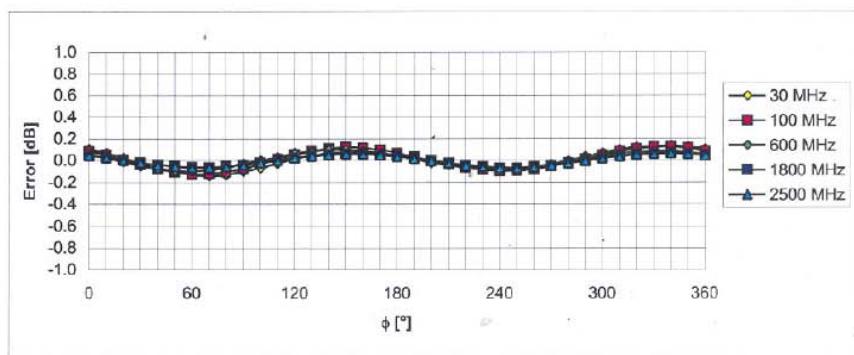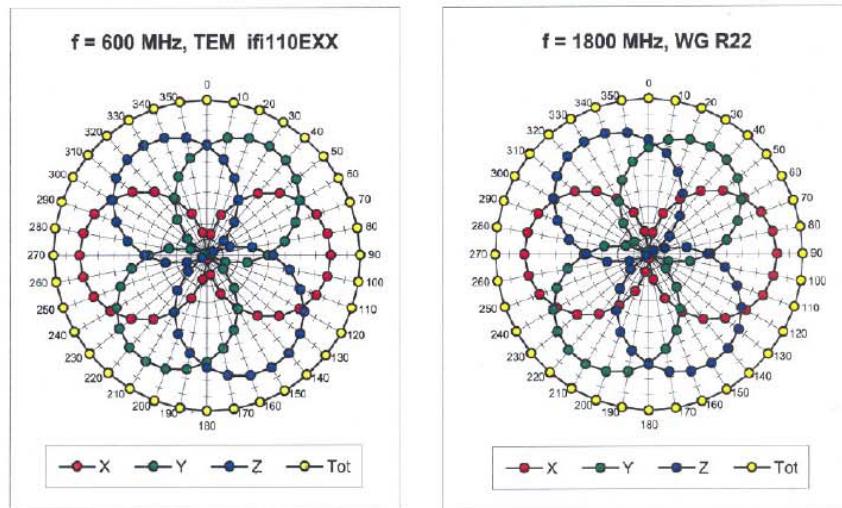

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )




## Calibration Certificate of DASY

EX3DV3 SN:3514

January 31, 2008

### Dynamic Range f(SAR<sub>head</sub>) (Waveguide R22, f = 1800 MHz)

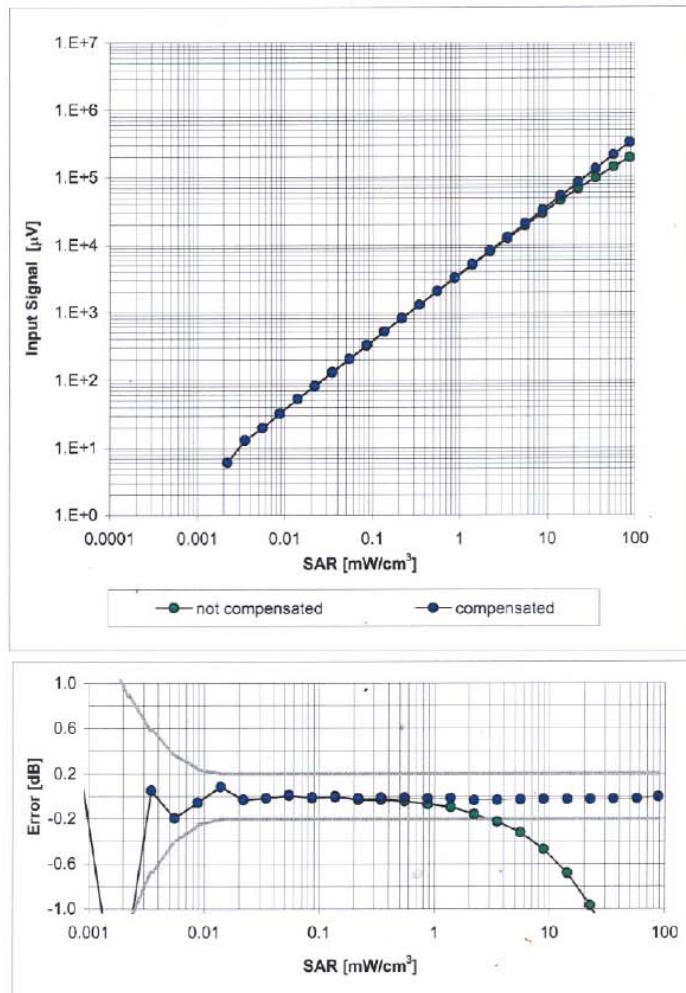

Uncertainty of Linearity Assessment: ± 0.6% (k=2)




## Calibration Certificate of DASY

EX3DV3 SN:3514

January 31, 2008

### Conversion Factor Assessment

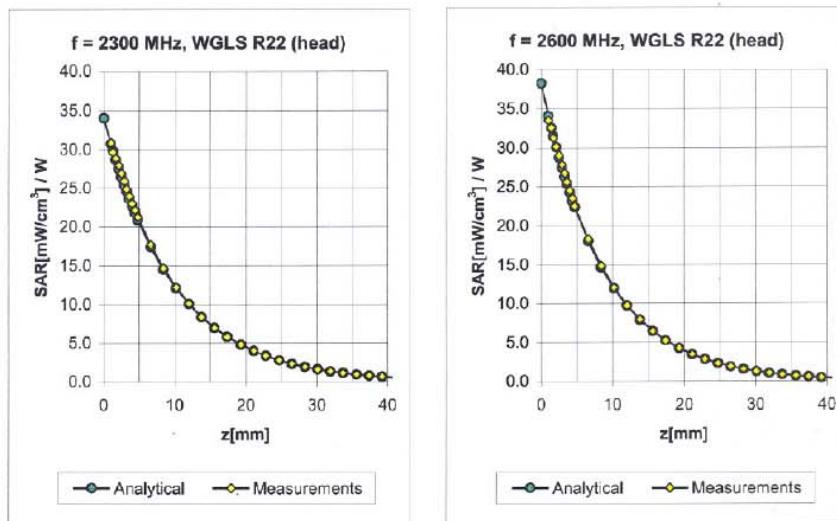

| f [MHz] | Validity [MHz] <sup>c</sup> | TSL  | Permittivity | Conductivity | Alpha | Depth | ConvF | Uncertainty   |
|---------|-----------------------------|------|--------------|--------------|-------|-------|-------|---------------|
| 2300    | ± 50 / ± 100                | Head | 39.4 ± 5%    | 1.71 ± 5%    | 0.76  | 0.52  | 7.73  | ± 11.8% (k=2) |
| 2600    | ± 50 / ± 100                | Head | 39.0 ± 5%    | 1.96 ± 5%    | 0.62  | 0.60  | 7.31  | ± 11.8% (k=2) |
| 3500    | ± 50 / ± 100                | Head | 37.9 ± 5%    | 2.91 ± 5%    | 0.36  | 1.03  | 7.09  | ± 13.1% (k=2) |
| 2300    | ± 50 / ± 100                | Body | 52.8 ± 5%    | 1.85 ± 5%    | 0.63  | 0.64  | 7.59  | ± 11.8% (k=2) |
| 2600    | ± 50 / ± 100                | Body | 52.5 ± 5%    | 2.16 ± 5%    | 0.52  | 0.76  | 6.91  | ± 11.8% (k=2) |
| 3500    | ± 50 / ± 100                | Body | 51.3 ± 5%    | 3.31 ± 5%    | 0.40  | 1.33  | 6.32  | ± 13.1% (k=2) |
| 5200    | ± 50 / ± 100                | Body | 49.0 ± 5%    | 5.30 ± 5%    | 0.35  | 1.70  | 4.34  | ± 13.1% (k=2) |
| 5300    | ± 50 / ± 100                | Body | 48.9 ± 5%    | 5.42 ± 5%    | 0.38  | 1.70  | 4.06  | ± 13.1% (k=2) |
| 5500    | ± 50 / ± 100                | Body | 48.6 ± 5%    | 5.65 ± 5%    | 0.43  | 1.70  | 3.98  | ± 13.1% (k=2) |
| 5600    | ± 50 / ± 100                | Body | 48.5 ± 5%    | 5.77 ± 5%    | 0.35  | 1.70  | 4.19  | ± 13.1% (k=2) |
| 5800    | ± 50 / ± 100                | Body | 48.2 ± 5%    | 6.00 ± 5%    | 0.30  | 1.70  | 4.20  | ± 13.1% (k=2) |

<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.




## Calibration Certificate of DASY

EX3DV3 SN:3514

January 31, 2008

### Deviation from Isotropy in HSL

Error ( $\phi, \theta$ ), f = 900 MHz

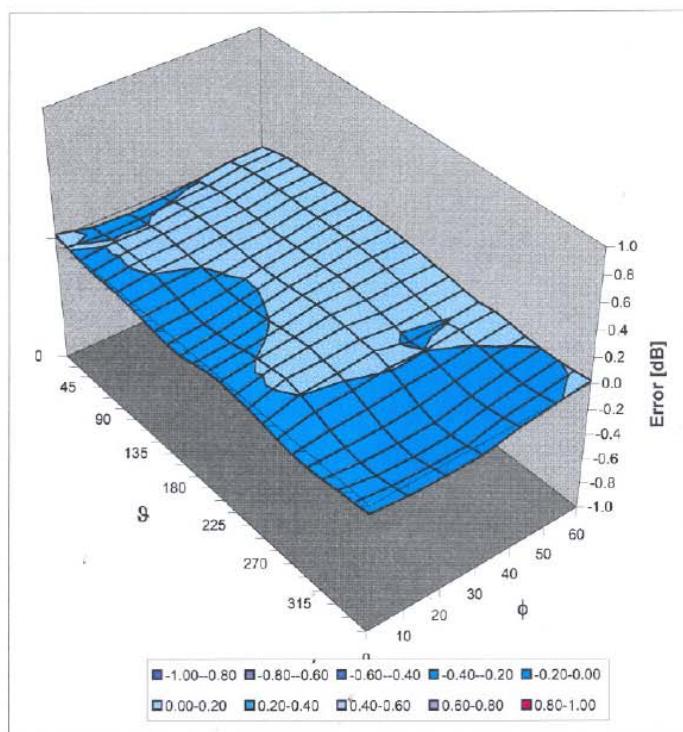

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  (k=2)



## Calibration Certificate of DASY

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client Sporton (Auden)

Certificate No: EX3-3514\_Jan09

### CALIBRATION CERTIFICATE

Object EX3DV3 - SN:3514

Calibration procedure(s) QA CAL-01.v6, QA CAL-14.v3 and QA CAL-23.v3  
Calibration procedure for dosimetric E-field probes

Calibration date: January 21, 2009

Condition of the calibrated item In Tolerance

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards          | ID #            | Cal Date (Certificate No.)    | Scheduled Calibration |
|----------------------------|-----------------|-------------------------------|-----------------------|
| Power meter E4419B         | GB41293874      | 1-Apr-08 (No. 217-00788)      | Apr-09                |
| Power sensor E4412A        | MY41495277      | 1-Apr-08 (No. 217-00788)      | Apr-09                |
| Power sensor E4412A        | MY41498087      | 1-Apr-08 (No. 217-00788)      | Apr-09                |
| Reference 3 dB Attenuator  | SN: S5054 (3c)  | 1-Jul-08 (No. 217-00865)      | Jul-09                |
| Reference 20 dB Attenuator | SN: S5086 (20b) | 31-Mar-08 (No. 217-00787)     | Apr-09                |
| Reference 30 dB Attenuator | SN: S5129 (30b) | 1-Jul-08 (No. 217-00866)      | Jul-09                |
| Reference Probe ES3DV2     | SN: 3013        | 2-Jan-09 (No. ES3-3013_Jan09) | Jan-10                |
| DAE4                       | SN: 660         | 9-Sep-08 (No. DAE4-660_Sep08) | Sep-09                |

| Secondary Standards       | ID #         | Check Date (in house)             | Scheduled Check        |
|---------------------------|--------------|-----------------------------------|------------------------|
| RF generator HP 8648C     | US3642U01700 | 4-Aug-99 (in house check Oct-07)  | In house check: Oct-09 |
| Network Analyzer HP 8753E | US37390585   | 18-Oct-01 (in house check Oct-08) | In house check: Oct-09 |

| Calibrated by: | Name          | Function          | Signature |
|----------------|---------------|-------------------|-----------|
|                | Katja Pokovic | Technical Manager |           |

| Approved by: | Name         | Function        | Signature |
|--------------|--------------|-----------------|-----------|
|              | Niels Kuster | Quality Manager |           |

Issued: January 21, 2009

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: EX3-3514\_Jan09

Page 1 of 9



## Calibration Certificate of DASY

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

### Glossary:

|                        |                                                                                                                                                |
|------------------------|------------------------------------------------------------------------------------------------------------------------------------------------|
| TSL                    | tissue simulating liquid                                                                                                                       |
| NORM $x,y,z$           | sensitivity in free space                                                                                                                      |
| ConvF                  | sensitivity in TSL / NORM $x,y,z$                                                                                                              |
| DCP                    | diode compression point                                                                                                                        |
| Polarization $\varphi$ | $\varphi$ rotation around probe axis                                                                                                           |
| Polarization $\theta$  | $\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis |

### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

### Methods Applied and Interpretation of Parameters:

- $NORMx,y,z$ : Assessed for E-field polarization  $\theta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide).  $NORMx,y,z$  are only intermediate values, i.e., the uncertainties of  $NORMx,y,z$  does not effect the  $E^2$ -field uncertainty inside TSL (see below ConvF).
- $NORM(f)x,y,z = NORMx,y,z * frequency\_response$  (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- $DCPx,y,z$ : DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- *ConvF and Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to  $NORMx,y,z * ConvF$  whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- *Spherical isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.



## **Calibration Certificate of DASY**

---

EX3DV3 SN:3514

January 21, 2009

# Probe EX3DV3

## SN:3514

|                  |                   |
|------------------|-------------------|
| Manufactured:    | December 15, 2002 |
| Last calibrated: | January 31, 2008  |
| Recalibrated:    | January 21, 2009  |

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)



## Calibration Certificate of DASY

EX3DV3 SN:3514

January 21, 2009

### DASY - Parameters of Probe: EX3DV3 SN:3514

#### Sensitivity in Free Space<sup>A</sup>

|       |                   |                                     |
|-------|-------------------|-------------------------------------|
| NormX | $0.66 \pm 10.1\%$ | $\mu\text{V}/(\text{V}/\text{m})^2$ |
| NormY | $0.70 \pm 10.1\%$ | $\mu\text{V}/(\text{V}/\text{m})^2$ |
| NormZ | $0.60 \pm 10.1\%$ | $\mu\text{V}/(\text{V}/\text{m})^2$ |

#### Diode Compression<sup>B</sup>

|       |       |
|-------|-------|
| DCP X | 91 mV |
| DCP Y | 94 mV |
| DCP Z | 95 mV |

#### Sensitivity in Tissue Simulating Liquid (Conversion Factors)

Please see Page 8.

#### Boundary Effect

TSL                    900 MHz                    Typical SAR gradient: 5 % per mm

|                                                         |        |        |
|---------------------------------------------------------|--------|--------|
| Sensor Center to Phantom Surface Distance               | 2.0 mm | 3.0 mm |
| SAR <sub>be</sub> [%]      Without Correction Algorithm | 7.7    | 4.4    |
| SAR <sub>be</sub> [%]      With Correction Algorithm    | 0.8    | 0.3    |

TSL                    1810 MHz                    Typical SAR gradient: 10 % per mm

|                                                         |        |        |
|---------------------------------------------------------|--------|--------|
| Sensor Center to Phantom Surface Distance               | 2.0 mm | 3.0 mm |
| SAR <sub>be</sub> [%]      Without Correction Algorithm | 6.2    | 3.4    |
| SAR <sub>be</sub> [%]      With Correction Algorithm    | 0.7    | 0.3    |

#### Sensor Offset

Probe Tip to Sensor Center                    1.0 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of NormX,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Page 8).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.




## Calibration Certificate of DASY

EX3DV3 SN:3514

January 21, 2009

### Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

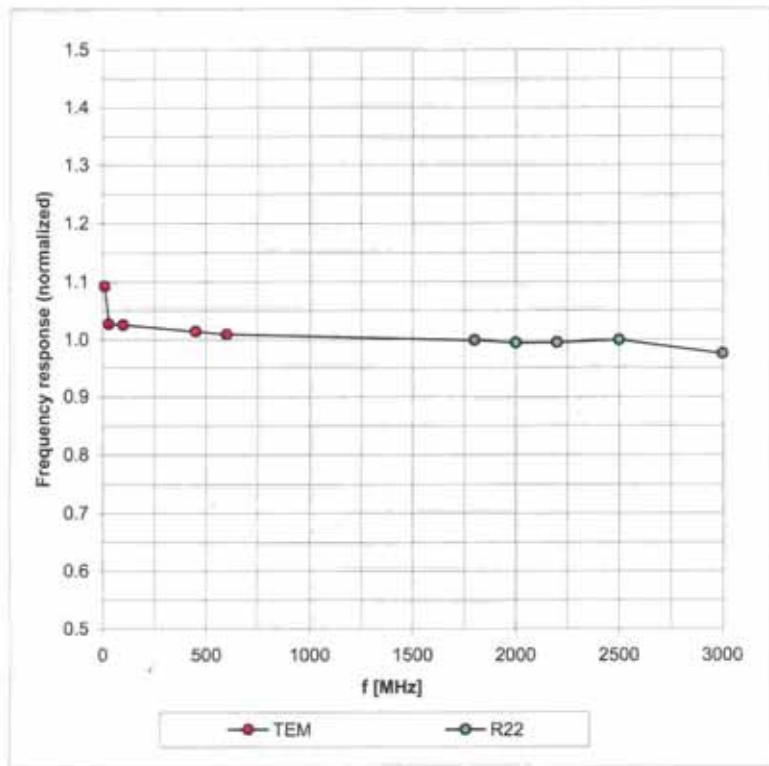

Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )





## Calibration Certificate of DASY

EX3DV3 SN:3514

January 21, 2009

### Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

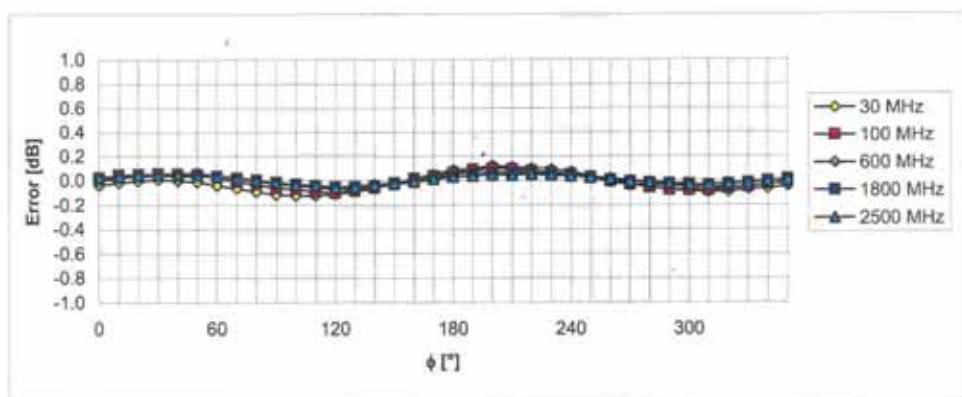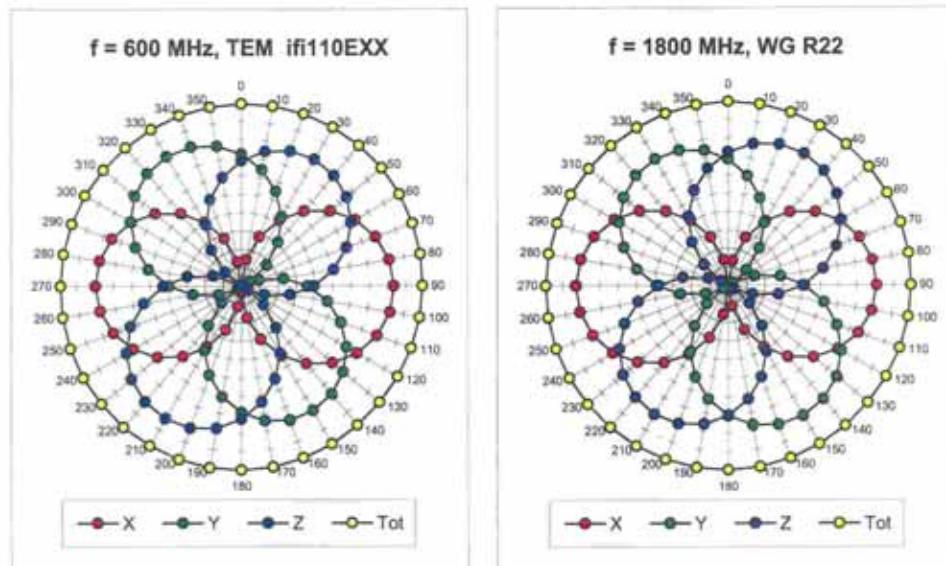

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )




## Calibration Certificate of DASY

EX3DV3 SN:3514

January 21, 2009

### Dynamic Range f(SAR<sub>head</sub>) (Waveguide R22, f = 1800 MHz)

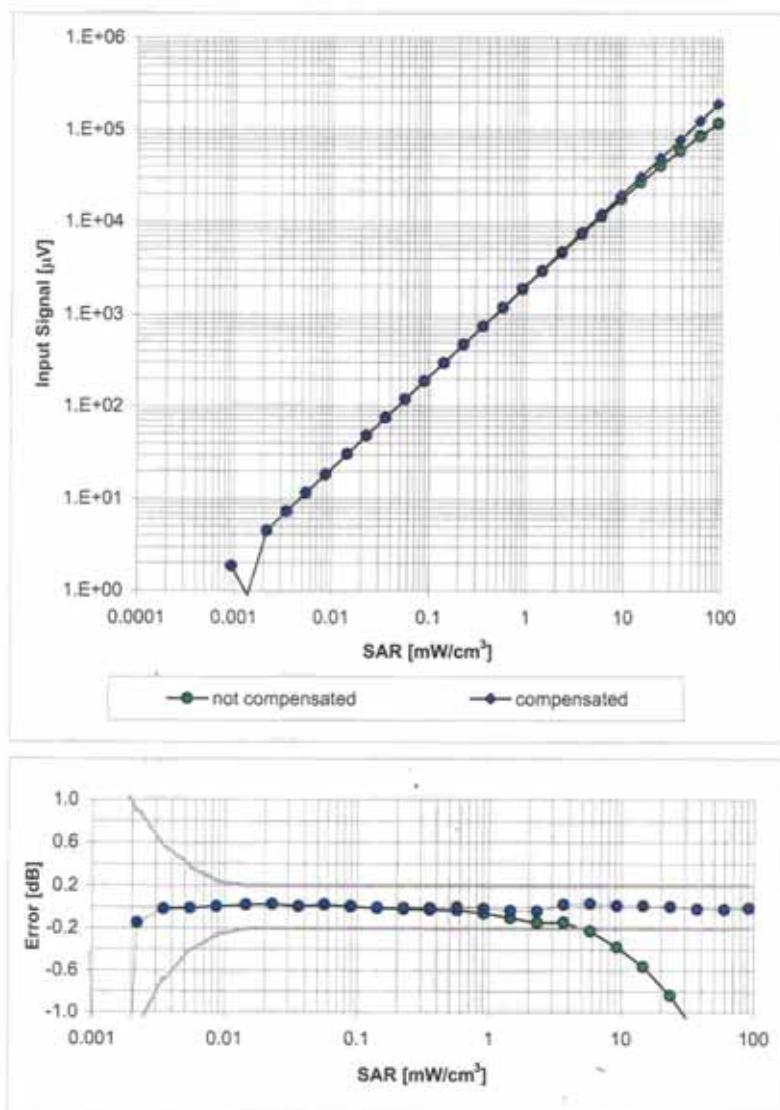

Uncertainty of Linearity Assessment: ± 0.6% (k=2)



## Calibration Certificate of DASY

EX3DV3 SN:3514

January 21, 2009

### Conversion Factor Assessment

| f [MHz] | Validity [MHz] <sup>c</sup> | TSL  | Permittivity | Conductivity | Alpha | Depth | ConvF Uncertainty  |
|---------|-----------------------------|------|--------------|--------------|-------|-------|--------------------|
| 900     | ± 50 / ± 100                | Head | 41.5 ± 5%    | 0.97 ± 5%    | 0.45  | 0.76  | 9.31 ± 11.0% (k=2) |
| 1810    | ± 50 / ± 100                | Head | 40.0 ± 5%    | 1.40 ± 5%    | 0.60  | 0.63  | 8.16 ± 11.0% (k=2) |
| 2300    | ± 50 / ± 100                | Head | 39.4 ± 5%    | 1.71 ± 5%    | 0.53  | 0.63  | 7.78 ± 11.0% (k=2) |
| 2600    | ± 50 / ± 100                | Head | 39.0 ± 5%    | 1.96 ± 5%    | 0.16  | 2.19  | 7.34 ± 11.0% (k=2) |
| 3500    | ± 50 / ± 100                | Head | 37.9 ± 5%    | 2.91 ± 5%    | 0.50  | 0.86  | 6.89 ± 13.1% (k=2) |
| 5200    | ± 50 / ± 100                | Head | 36.0 ± 5%    | 4.66 ± 5%    | 0.40  | 1.70  | 4.78 ± 13.1% (k=2) |
| 5300    | ± 50 / ± 100                | Head | 35.9 ± 5%    | 4.76 ± 5%    | 0.40  | 1.70  | 4.40 ± 13.1% (k=2) |
| 5500    | ± 50 / ± 100                | Head | 35.6 ± 5%    | 4.96 ± 5%    | 0.40  | 1.70  | 4.22 ± 13.1% (k=2) |
| 5600    | ± 50 / ± 100                | Head | 35.5 ± 5%    | 5.07 ± 5%    | 0.40  | 1.70  | 4.13 ± 13.1% (k=2) |
| 5800    | ± 50 / ± 100                | Head | 35.3 ± 5%    | 5.27 ± 5%    | 0.40  | 1.70  | 4.13 ± 13.1% (k=2) |
| 900     | ± 50 / ± 100                | Body | 55.0 ± 5%    | 1.05 ± 5%    | 0.42  | 0.76  | 9.41 ± 11.0% (k=2) |
| 1810    | ± 50 / ± 100                | Body | 53.3 ± 5%    | 1.52 ± 5%    | 0.85  | 0.56  | 8.18 ± 11.0% (k=2) |
| 2300    | ± 50 / ± 100                | Body | 52.8 ± 5%    | 1.85 ± 5%    | 0.18  | 4.17  | 7.60 ± 11.0% (k=2) |
| 2600    | ± 50 / ± 100                | Body | 52.5 ± 5%    | 2.16 ± 5%    | 0.34  | 1.14  | 7.20 ± 11.0% (k=2) |
| 3500    | ± 50 / ± 100                | Body | 51.3 ± 5%    | 3.31 ± 5%    | 0.53  | 0.81  | 6.40 ± 13.1% (k=2) |
| 5200    | ± 50 / ± 100                | Body | 49.0 ± 5%    | 5.30 ± 5%    | 0.45  | 1.75  | 4.29 ± 13.1% (k=2) |
| 5300    | ± 50 / ± 100                | Body | 48.9 ± 5%    | 5.42 ± 5%    | 0.45  | 1.75  | 3.94 ± 13.1% (k=2) |
| 5500    | ± 50 / ± 100                | Body | 48.6 ± 5%    | 5.65 ± 5%    | 0.45  | 1.75  | 3.88 ± 13.1% (k=2) |
| 5600    | ± 50 / ± 100                | Body | 48.5 ± 5%    | 5.77 ± 5%    | 0.45  | 1.75  | 3.89 ± 13.1% (k=2) |
| 5800    | ± 50 / ± 100                | Body | 48.2 ± 5%    | 6.00 ± 5%    | 0.45  | 1.75  | 3.85 ± 13.1% (k=2) |

<sup>c</sup> The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.




## Calibration Certificate of DASY

EX3DV3 SN:3514

January 21, 2009

### Deviation from Isotropy in HSL



Error ( $\phi, \theta$ ),  $f = 900$  MHz

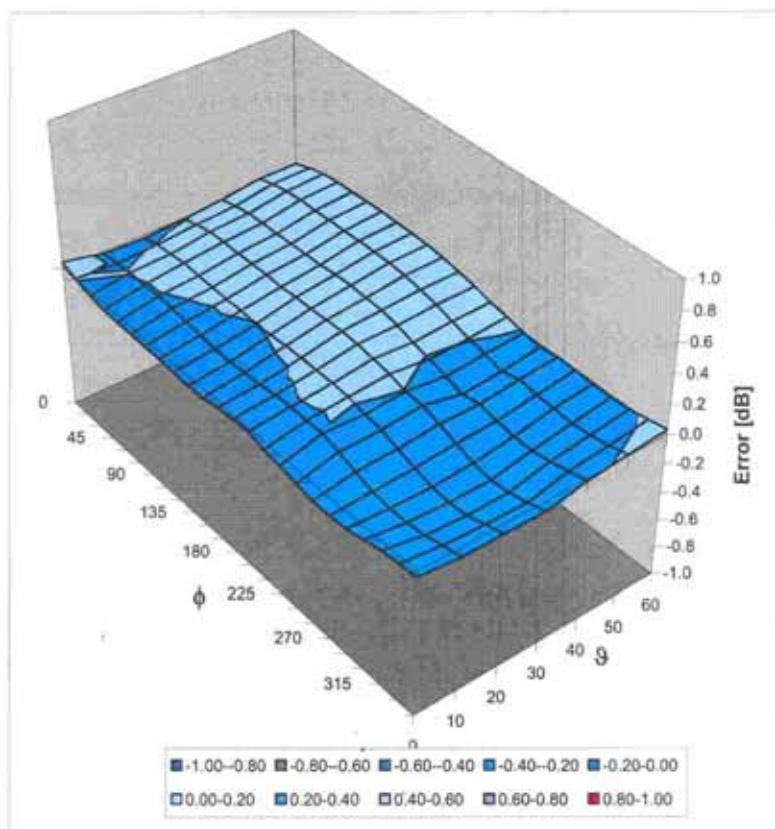

Uncertainty of Spherical Isotropy Assessment:  $\pm 2.6\%$  ( $k=2$ )




## Appendix D - Product Photos

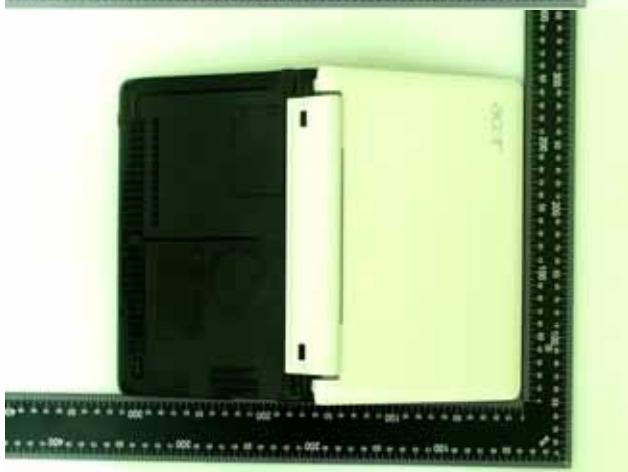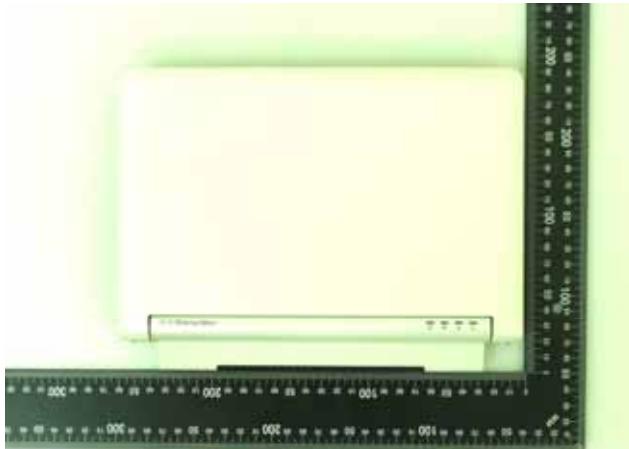

**Antenna Location :**



## Appendix E - Test Setup Photos

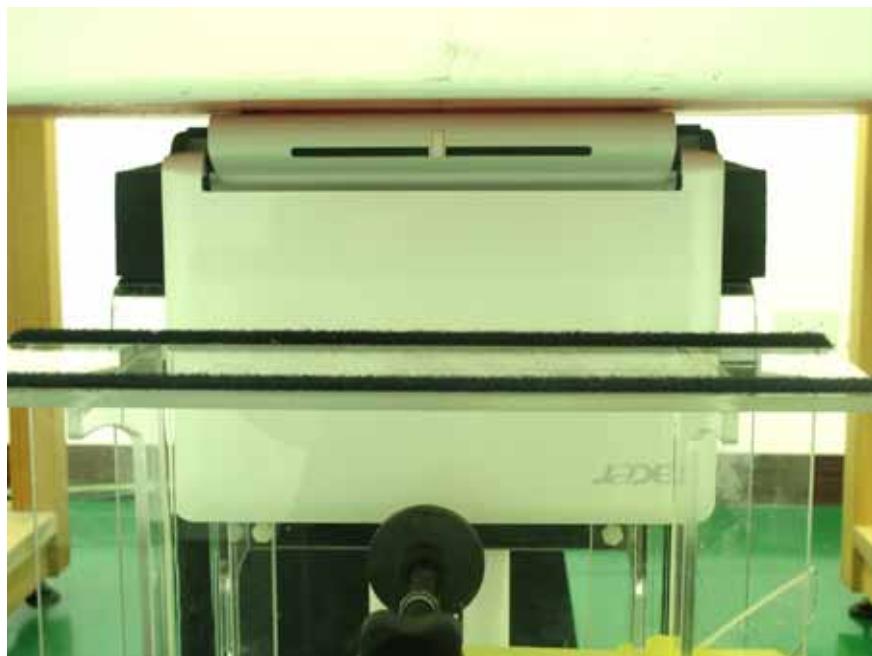

NB Bottom with 0cm Gap - Front View



NB Bottom with 0cm Gap - Side View