

Exhibit O: CDMA SAR Report - Part 3 of 3

FCC ID: HN22011B-2

APPENDIX C - SYSTEM VALIDATION

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

1800 MHz System Validation Dipole

Type:

D1800V2

Serial Number:

247

Place of Calibration:

Zurich

Date of Calibration:

June 20, 2001


Calibration Interval:

24 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:



Approved by:



DASY

Dipole Validation Kit

Type: D1800V2

Serial: 247

Manufactured: August 25, 1999

Calibrated: June 20, 2001

1. Measurement Conditions

The measurements were performed in the flat section of the new generic twin phantom filled with head simulating glycol solution of the following electrical parameters at 1800 MHz:

| | | |
|------------------------|-------------------|-----------|
| Relative Dielectricity | 40.0 | $\pm 5\%$ |
| Conductivity | 1.36 mho/m | $\pm 5\%$ |

The DASY3 System (Software version 3.1c) with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 5.57 at 1800 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was 250mW $\pm 3\%$. The results are normalized to 1W input power.

2. SAR Measurement

Standard SAR-measurements were performed with the phantom according to the measurement conditions described in section 1. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values are:

| | |
|--|-------------------|
| averaged over 1 cm ³ (1 g) of tissue: | 38.64 mW/g |
| averaged over 10 cm ³ (10 g) of tissue: | 20.08 mW/g |

Note: If the liquid parameters for validation are slightly different from the ones used for initial calibration, the SAR-values will be different as well. The estimated sensitivities of SAR-values and penetration depths to the liquid parameters are listed in the DASY Application Note 4: 'SAR Sensitivities'.

3. Dipole Impedance and return loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay: **1.208 ns** (one direction)
Transmission factor: **0.995** (voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 1800 MHz: $\text{Re}\{Z\} = 52.4 \Omega$

$\text{Im}\{Z\} = 0.7 \Omega$

Return Loss at 1800 MHz **-32.1 dB**

4. Measurement Conditions

The measurements were performed in the flat section of the new generic twin phantom filled with brain sugar-water solution of the following electrical parameters at 1800 MHz:

Relative Dielectricity **40.1** $\pm 5\%$
Conductivity **1.71 mho/m** $\pm 5\%$

The DASY3 System (Software version 3.1c) with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 5.63 at 1800 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was 250mW $\pm 3\%$. The results are normalized to 1W input power.

5. SAR Measurement

Standard SAR-measurements were performed with the phantom according to the measurement conditions described in section 4. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values are:

averaged over 1 cm³ (1 g) of tissue: **43.6 mW/g**

averaged over 10 cm³ (10 g) of tissue: **21.6 mW/g**

Note: If the liquid parameters for validation are slightly different from the ones used for initial calibration, the SAR-values will be different as well. The estimated sensitivities of SAR-values and penetration depths to the liquid parameters are listed in the DASY Application Note 4: 'SAR Sensitivities'.

6. Handling


The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Do not apply excessive force to the dipole arms, because they might bend. If the dipole arms have to be bent back, take care to release stress to the soldered connections near the feedpoint; they might come off.


After prolonged use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

20 Jun 2001 15:31:17

[CH1] S11 1 U FS 1: 52.408 Ω 0.7441 Ω 65.796 pH 1 800.000 000 MHz

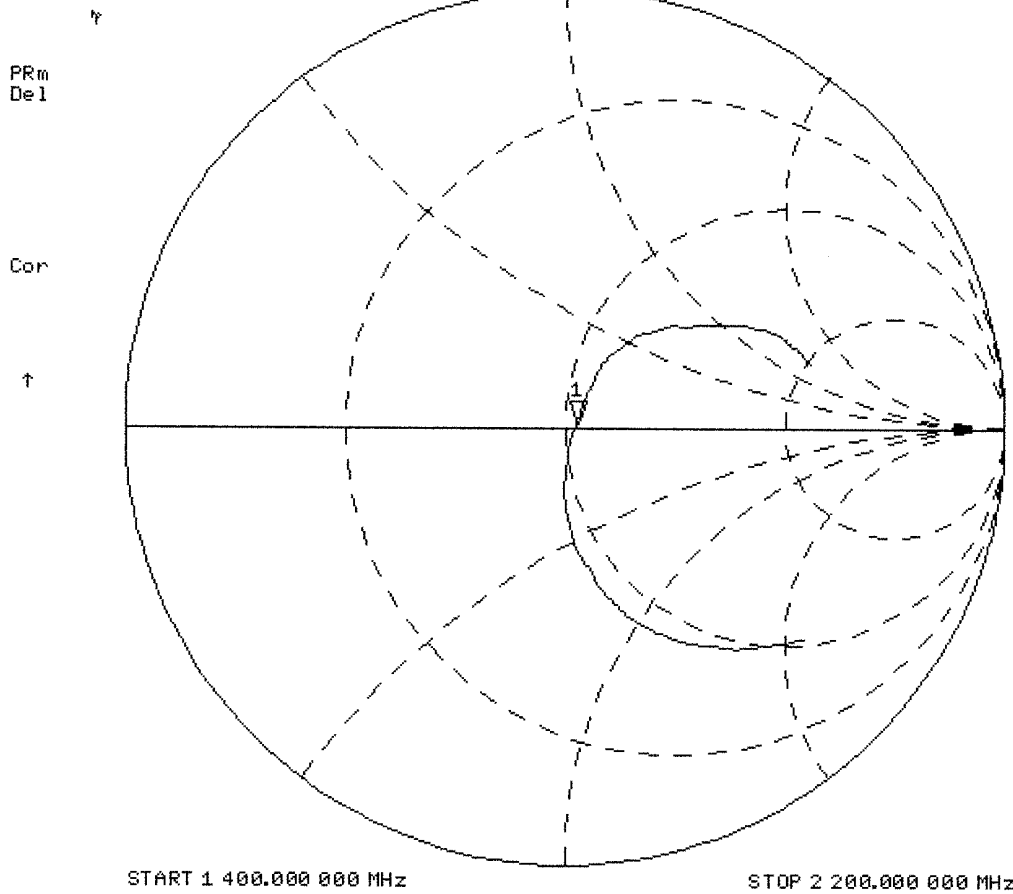


CH1 S11 LOG 5 dB/REF 0 dB 1:-32.107 dB 1 800.000 000 MHz

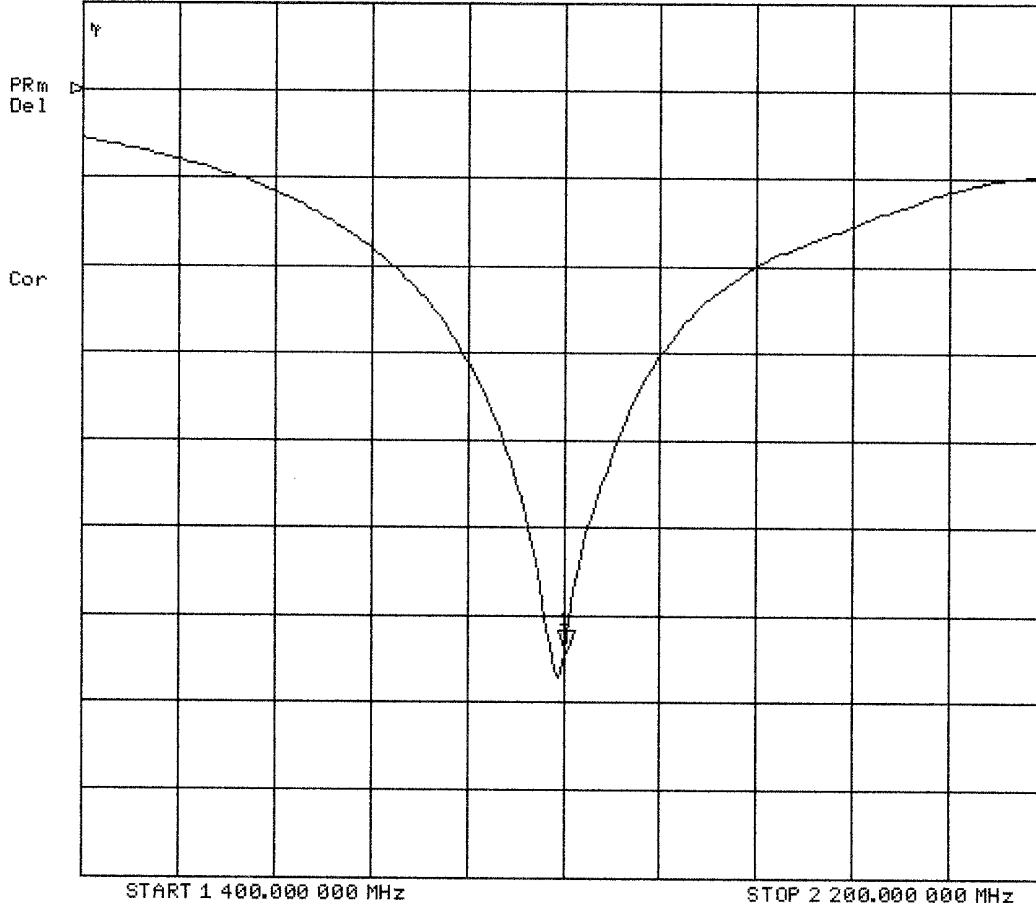

Validation Dipole D1800V2 SN:247, d = 10 mm

Frequency: 1800 MHz; Antenna Input Power: 250 [mW]
Generic Twin Phantom; Flat Section; Grid Spacing: Dx = 15.0, Dy = 15.0, Dz = 10.0
Probe: ET3DV6 - SN1507; ConvF(5.57,5.57,5.57); Crest factor: 1.0; IEEE1528 1800 MHz : $\sigma = 1.36 \text{ mho/m}$ $\epsilon_r = 40.0$ $\rho = 1.00 \text{ g/cm}^3$
Cubes (2): Peak: 18.2 mW/g $\pm 0.04 \text{ dB}$, SAR (1g): 9.66 mW/g $\pm 0.03 \text{ dB}$, SAR (10g): 5.02 mW/g $\pm 0.03 \text{ dB}$, (Worst-case extrapolation)
Penetration depth: 8.2 (7.6, 9.4) [mm]
Powerdrift: -0.01 dB

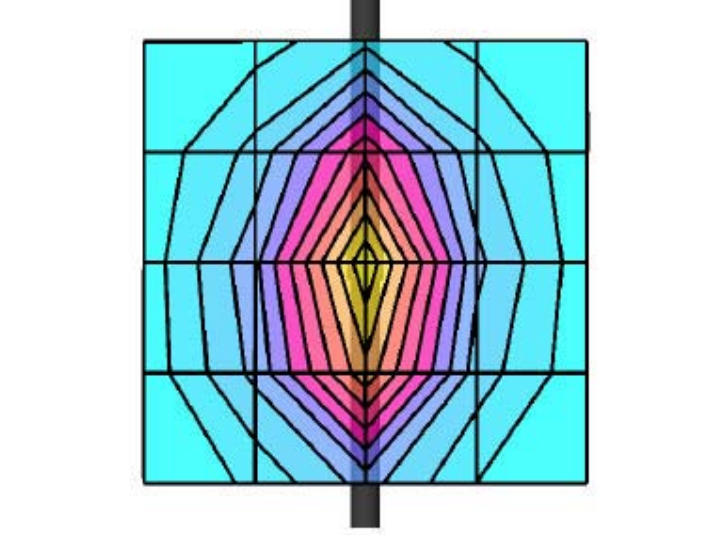

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

900 MHz System Validation Dipole

Type:

D900V2

Serial Number:

054

Place of Calibration:

Zurich

Date of Calibration:

June 20, 2001

Calibration Interval:

24 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

Rhonic Vohja

Approved by:

[Signature]

DASY

Dipole Validation Kit

Type: D900V2

Serial: 054

Manufactured: August 25, 1999
Calibrated: June 20, 2001

1. Measurement Conditions

The measurements were performed in the flat section of the new generic twin phantom filled with head simulating solution of the following electrical parameters at 900 MHz:

| | | |
|------------------------|-------------------|-----------|
| Relative Dielectricity | 42.4 | $\pm 5\%$ |
| Conductivity | 0.97 mho/m | $\pm 5\%$ |

The DASY3 System (Software version 3.1c) with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.27 at 900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was 250mW $\pm 3\%$. The results are normalized to 1W input power.

2. SAR Measurement

Standard SAR-measurements were performed with the phantom according to the measurement conditions described in section 1. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values are:

| | |
|--|-------------------|
| averaged over 1 cm ³ (1 g) of tissue: | 11.12 mW/g |
| averaged over 10 cm ³ (10 g) of tissue: | 7.04 mW/g |

Note: If the liquid parameters for validation are slightly different from the ones used for initial calibration, the SAR-values will be different as well.

5. SAR Measurement

Standard SAR-measurements were performed with the phantom according to the measurement conditions described in section 4. The results have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values are:

| | |
|--|-------------------|
| averaged over 1 cm ³ (1 g) of tissue: | 10.12 mW/g |
| averaged over 10 cm ³ (10 g) of tissue: | 6.52 mW/g |

Note: If the liquid parameters for validation are slightly different from the ones used for initial calibration, the SAR-values will be different as well.

6. Handling

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

Do not apply excessive force to the dipole arms, because they might bend. If the dipole arms have to be bent back, take care to release stress to the soldered connections near the feedpoint; they might come off.

After prolonged use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.


CHI S11 1 U FS 1: 51.324 Ω -478.52 $m\Omega$ 369.56 μF 900.000 000 MHz

γ

PRm
Del


Cor
Avg
16

↑

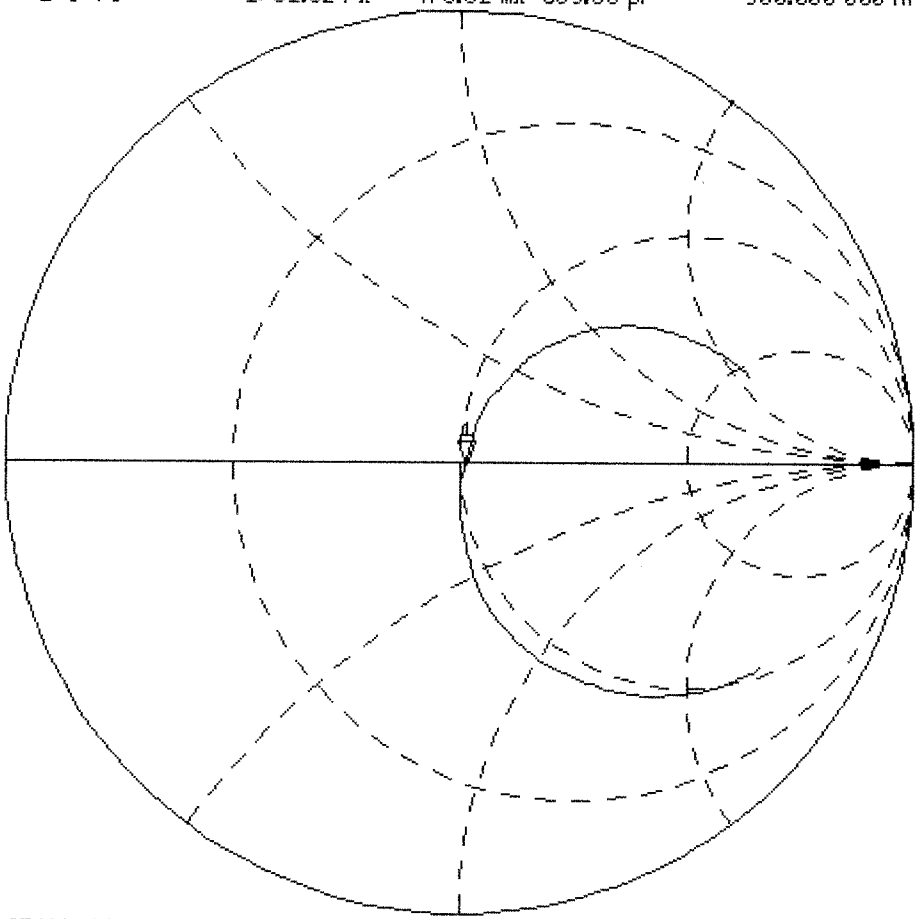

START 700.000 000 MHz

STOP 1 100.000 000 MHz

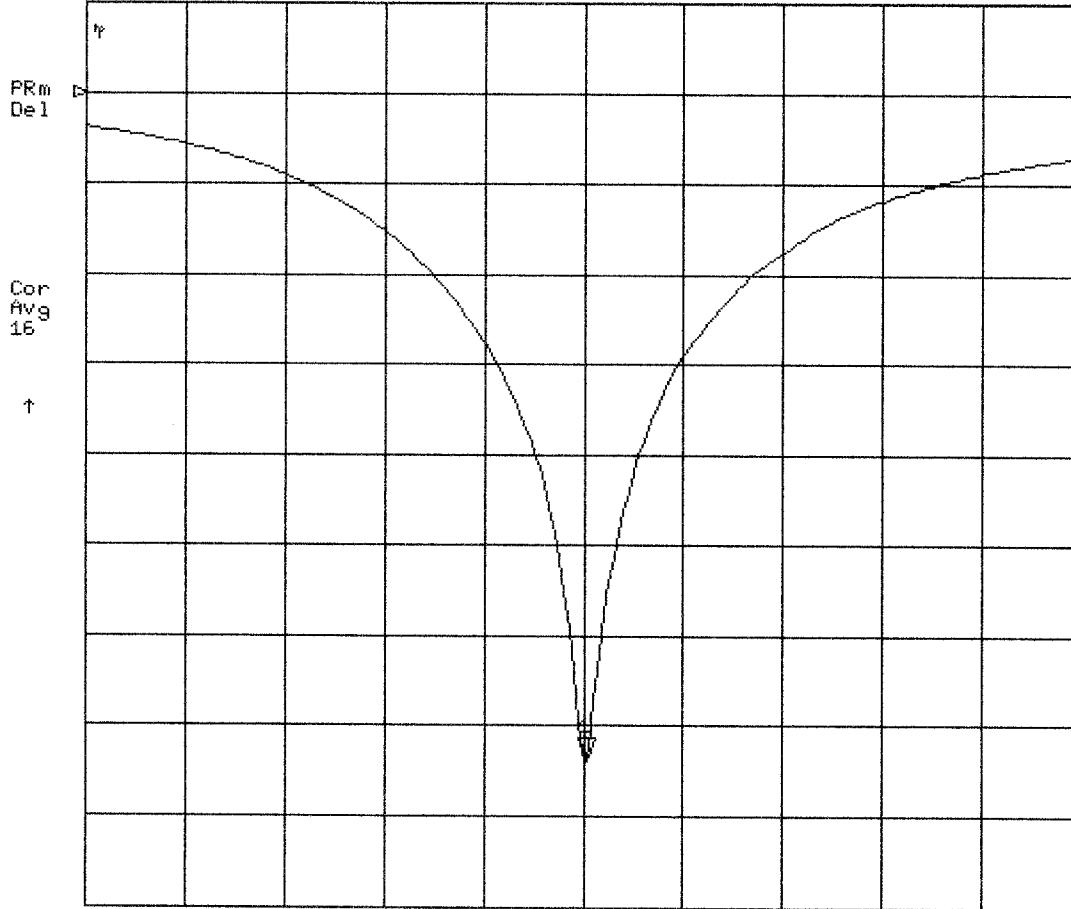


START 700.000 000 MHz

STOP 1 100.000 000 MHz

Validation Dipole D900V2 SN:054, d = 15 mm

Frequency: 900 MHz; Antenna Input Power: 250 [mW]
Generic Twin Phantom; Flat Section; Grid Spacing: Dx = 15.0, Dy = 15.0, Dz = 10.0
Probe: ET3DV6 - SN1507; ConvF(6.27,6.27,6.27); Crest factor: 1.0; IEEE1528 900 MHz: $\sigma = 0.97$ mho/m $\epsilon_r = 42.4$ $\rho = 1.00$ g/cm³
Cubes (2): Peak: 4.47 mW/g ± 0.05 dB, SAR (1g): 2.78 mW/g ± 0.04 dB, SAR (10g): 1.76 mW/g ± 0.02 dB, (Worst-case extrapolation)
Penetration depth: 11.5 (10.3, 13.2) [mm]
Powerdrift: -0.00 dB

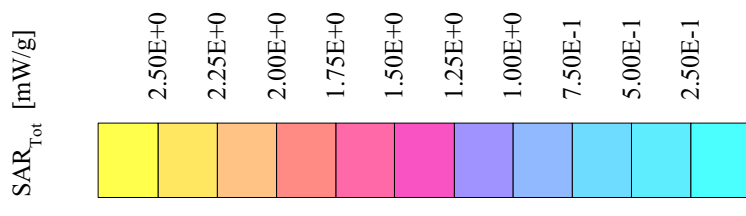

2450MHz SYSTEM VALIDATION DIPOLE

Type:

2450MHz Validation Dipole

Serial Number:

150

Place of Calibration:


Celltech Labs Inc.

Date of Calibration:


October 24, 2002

Celltech Research Inc. hereby certifies that this device has been calibrated on the date indicated above.

Calibrated by:

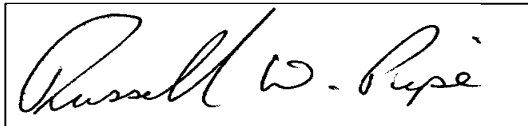

Approved by:

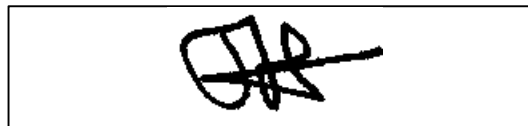


1. Dipole Construction & Electrical Characteristics

The validation dipole was constructed in accordance with the IEEE Std “Recommended Practice for Determining the Spatial-Peak Specific Absorption Rate (SAR) in the Human Body Due to Wireless Communications Devices: Experimental Techniques”. The electrical properties were measured using an HP 8753E Network Analyzer. The network analyzer was calibrated to the validation dipole N-type connector feed point using an HP85032E Type N calibration kit. The dipole was placed parallel to a planar phantom at a separation distance of 10.0mm from the simulating fluid using a loss-less dielectric spacer. The measured input impedance is:

Feed point impedance at 2450MHz
 $\text{Re}\{Z\} = 49.838\Omega$
 $\text{Im}\{Z\} = 0.2207\Omega$

Return Loss at 2450MHz
-49.398 dB

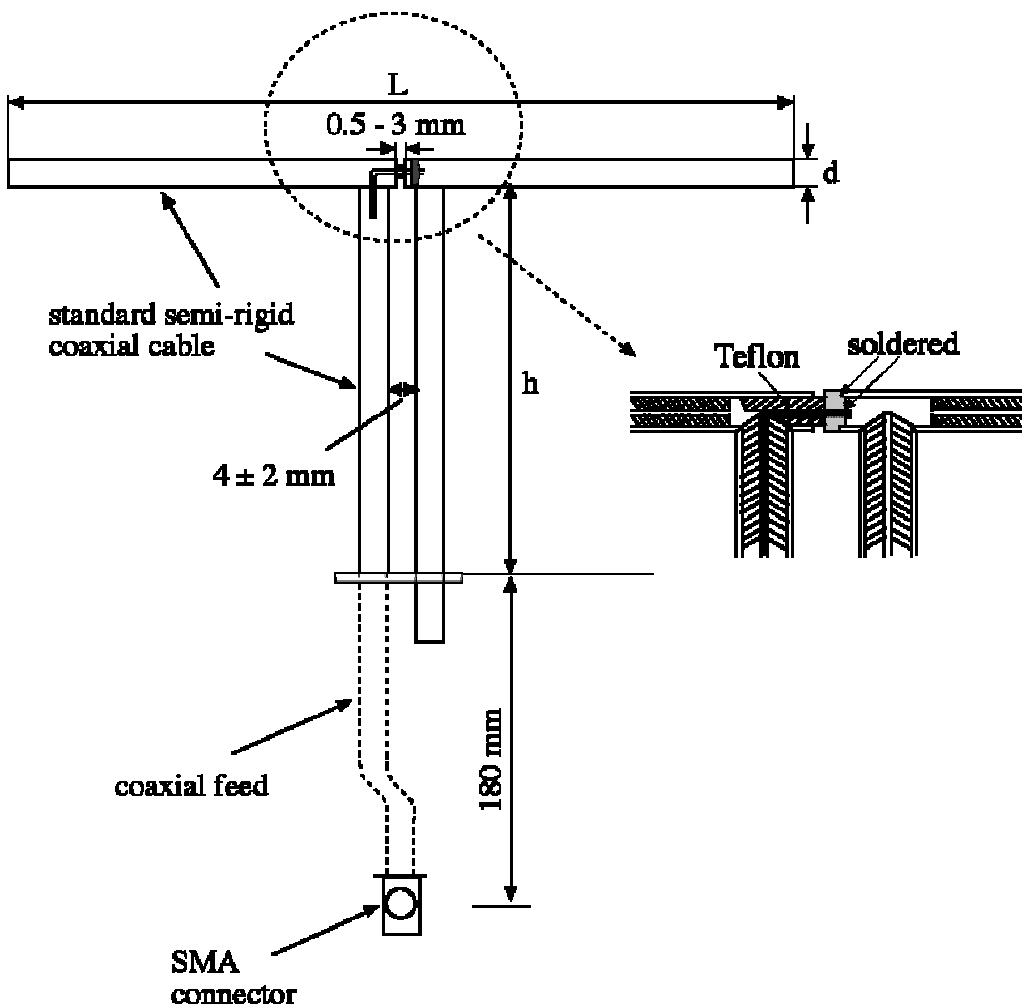

Validation Dipole Dimensions


| Frequency (MHz) | L (mm) | h (mm) | d (mm) |
|-----------------|--------|--------|--------|
| 300 | 420.0 | 250.0 | 6.2 |
| 450 | 288.0 | 167.0 | 6.2 |
| 835 | 161.0 | 89.8 | 3.6 |
| 900 | 149.0 | 83.3 | 3.6 |
| 1450 | 89.1 | 51.7 | 3.6 |
| 1800 | 72.0 | 41.7 | 3.6 |
| 1900 | 68.0 | 39.5 | 3.6 |
| 2000 | 64.5 | 37.5 | 3.6 |
| 2450 | 51.8 | 30.6 | 3.6 |
| 3000 | 41.5 | 25.0 | 3.6 |

2. Validation Phantom

The validation phantom is the SAM (Specific Anthropomorphic Mannequin) phantom manufactured by Schmid & Partner Engineering AG. The SAM phantom is a Fiberglass shell integrated in a wooden table. The shape of the shell corresponds to the phantom defined by SCC34-SC2. It enables the dosimetric evaluation of left and right hand phone usage as well as body mounted usage at the flat phantom region. A cover prevents evaporation of the liquid. Reference markings on the phantom allow the complete setup of all predefined phantom positions and measurement grids by manually teaching three points in the robot.

Shell Thickness: 2.0 ± 0.1 mm
Filling Volume: Approx. 20 liters
Dimensions: 50 cm (W) x 100 cm (L)

SAM Twin-Phantom

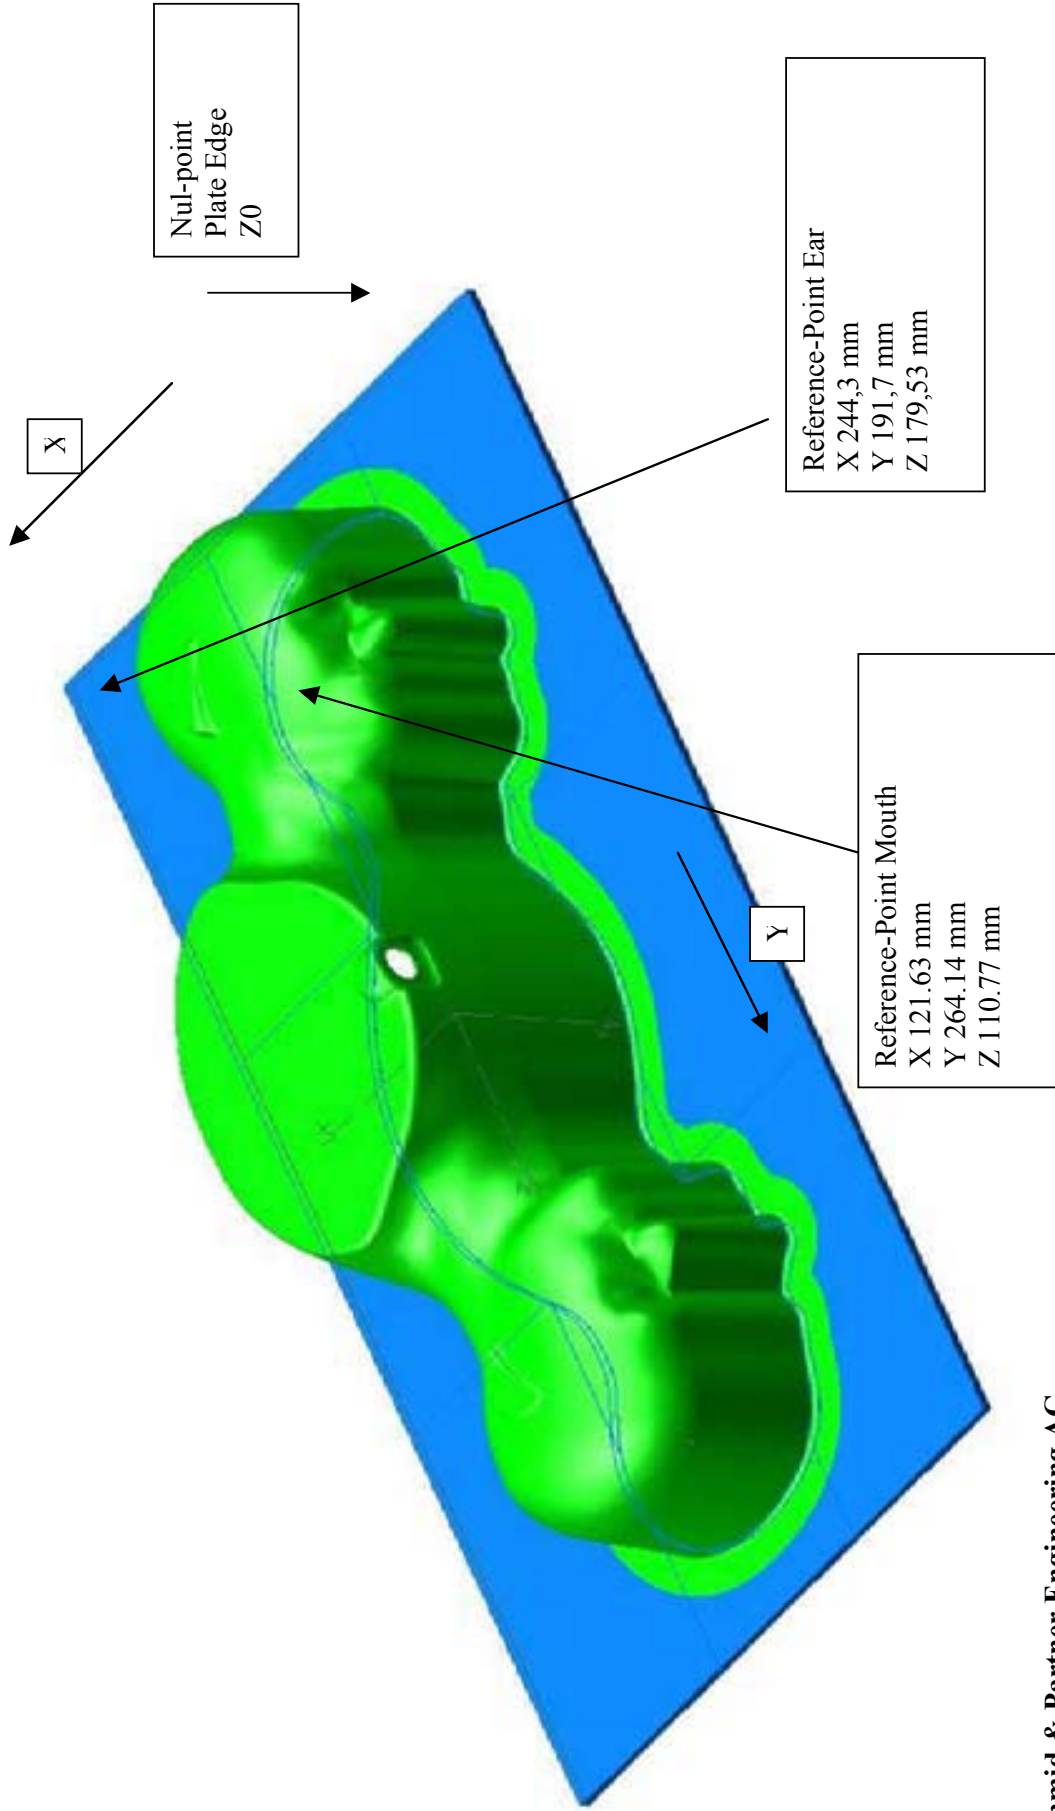

2450MHz Dipole Calibration



2450MHz Dipole Calibration



3. Measurement Conditions

The planar phantom was filled with brain simulating tissue having the following electrical parameters at 2450MHz:


| | |
|------------------------|------------|
| Relative Permittivity: | 36.8 |
| Conductivity: | 1.79 mho/m |
| Ambient Temperature: | 23.6°C |
| Fluid Temperature: | 23.8°C |
| Fluid Depth: | ≥ 15cm |

The 2450MHz simulating tissue consists of the following ingredients:

| Ingredient | Percentage by weight |
|---|---|
| Water | 55.20% |
| Glycol Monobutyl | 44.80% |
| Target Dielectric Parameters at 22°C | $\epsilon_r = 39.2$ (+/-10%) $\sigma = 1.80$ S/m (+/-5%) |

4. SAR Measurement

The SAR measurement was performed with the E-field probe in mechanical detection mode only. The setup and determination of the forward power into the dipole was performed using the following procedures.

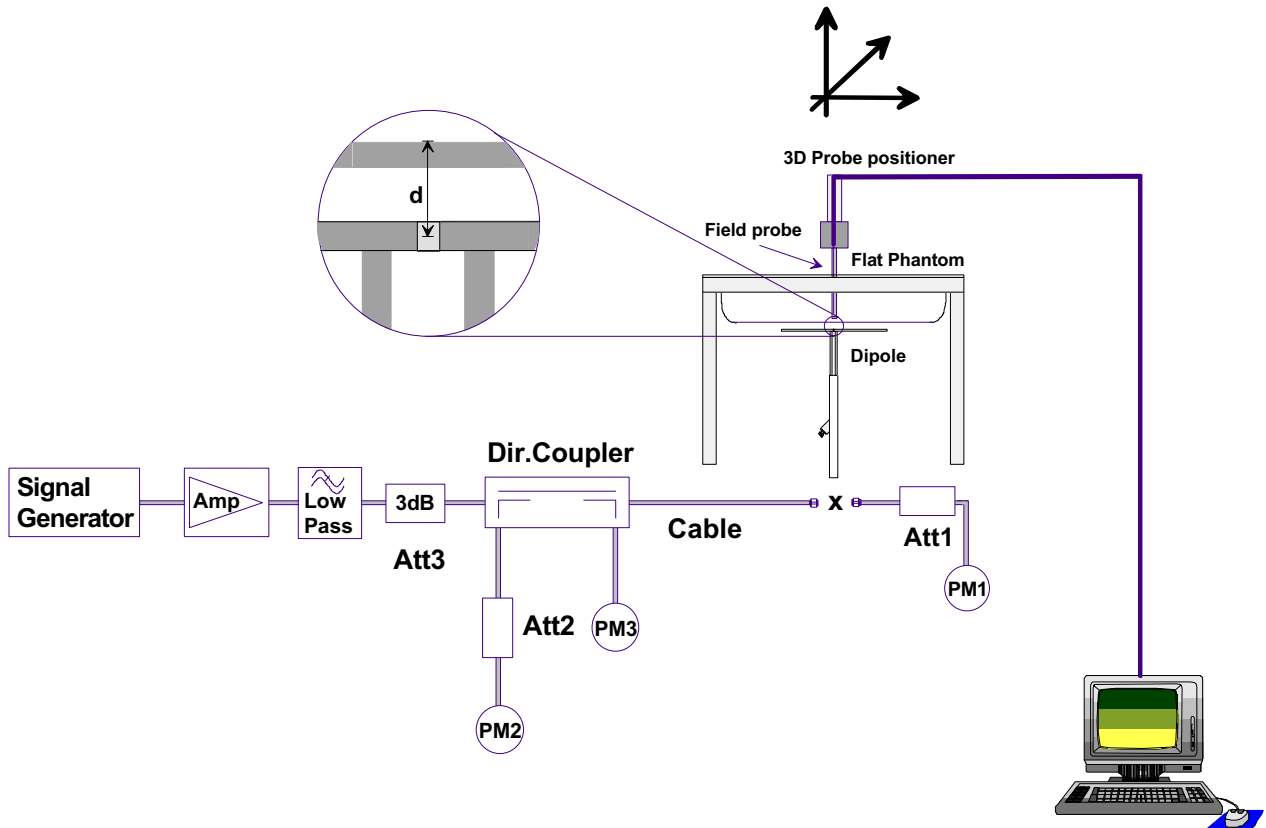

First, the power meter PM1 (including attenuator Att1) is connected to the cable to measure the forward power at the location of the dipole connector (X). The signal generator is adjusted for the desired forward power at the dipole connector (taking into account the attenuation of Att1) as read by power meter PM2. After connecting the cable to the dipole, the signal generator is readjusted for the same reading at power meter PM2. If the signal generator does not allow adjustment in 0.01dB steps, the remaining difference at PM2 must be taken into consideration. PM3 records the reflected power from the dipole to ensure that the value is not changed from the previous value. The reflected power should be 20dB below the forward power.

Ten SAR measurements were performed in order to achieve repeatability and to establish an average target value.

Validation Dipole SAR Test Results

| Validation Measurement | SAR @ 0.25W Input averaged over 1g | SAR @ 1W Input averaged over 1g | SAR @ 0.25W Input averaged over 10g | SAR @ 1W Input averaged over 10g | Peak SAR @ 0.25W Input |
|------------------------|------------------------------------|---------------------------------|-------------------------------------|----------------------------------|------------------------|
| Test 1 | 14.4 | 57.6 | 6.55 | 26.20 | 30.5 |
| Test 2 | 14.2 | 56.8 | 6.44 | 25.76 | 30.0 |
| Test 3 | 14.0 | 56.0 | 6.35 | 25.40 | 29.7 |
| Test 4 | 13.9 | 55.6 | 6.32 | 25.28 | 29.5 |
| Test 5 | 14.0 | 56.0 | 6.33 | 25.32 | 29.7 |
| Test 6 | 14.0 | 56.0 | 6.33 | 25.32 | 29.7 |
| Test 7 | 13.9 | 55.6 | 6.31 | 25.24 | 29.5 |
| Test 8 | 13.8 | 55.2 | 6.28 | 25.12 | 29.3 |
| Test 9 | 13.8 | 55.2 | 6.28 | 25.12 | 29.4 |
| Test10 | 14.0 | 56.0 | 6.33 | 25.32 | 29.7 |
| Average Value | 14.0 | 56.0 | 6.35 | 25.41 | 29.7 |

The results have been normalized to 1W (forward power) into the dipole.

Averaged over 1cm (1g) of tissue: 56.00 mW/g

Averaged over 10cm (10g) of tissue: 25.41 mW/g

24 Oct 2002 09:28:50


CH1 S11 1 U FS 1: 49.838 Ω 0.2207 Ω 14.337 pH 2 450.000 000 MHz

PRm

MARKER 1
2.45 GHz

Cor

↑

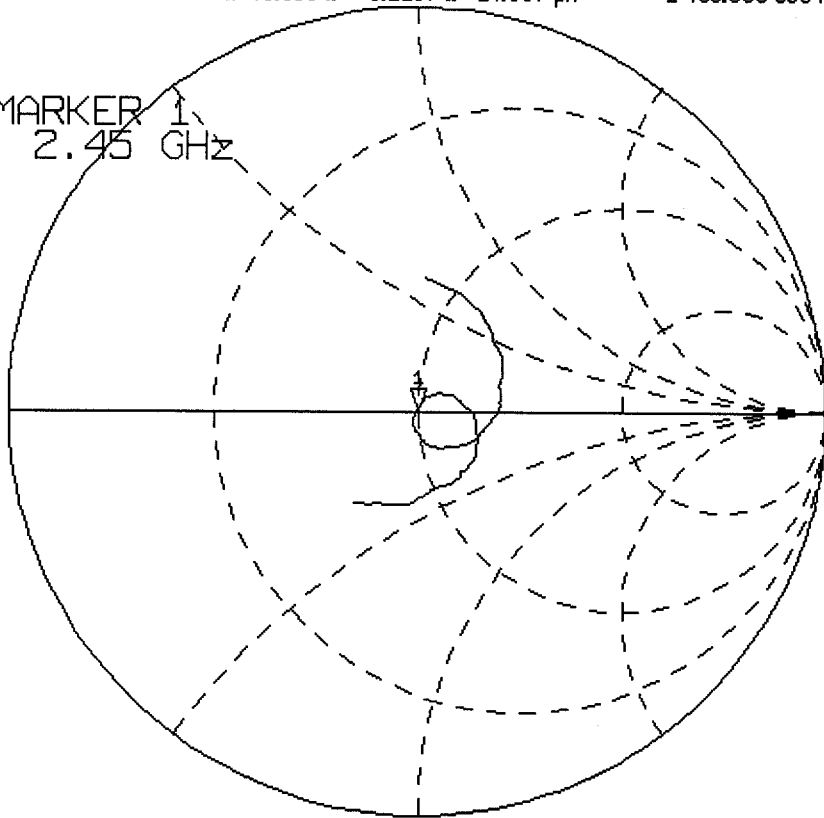


START 2 250.000 000 MHz

STOP 2 650.000 000 MHz

24 Oct 2002 09:28:12

CH1 S11 LOG 10 dB/REF 0 dB 11-49.398 dB 2 450.000 000 MHz

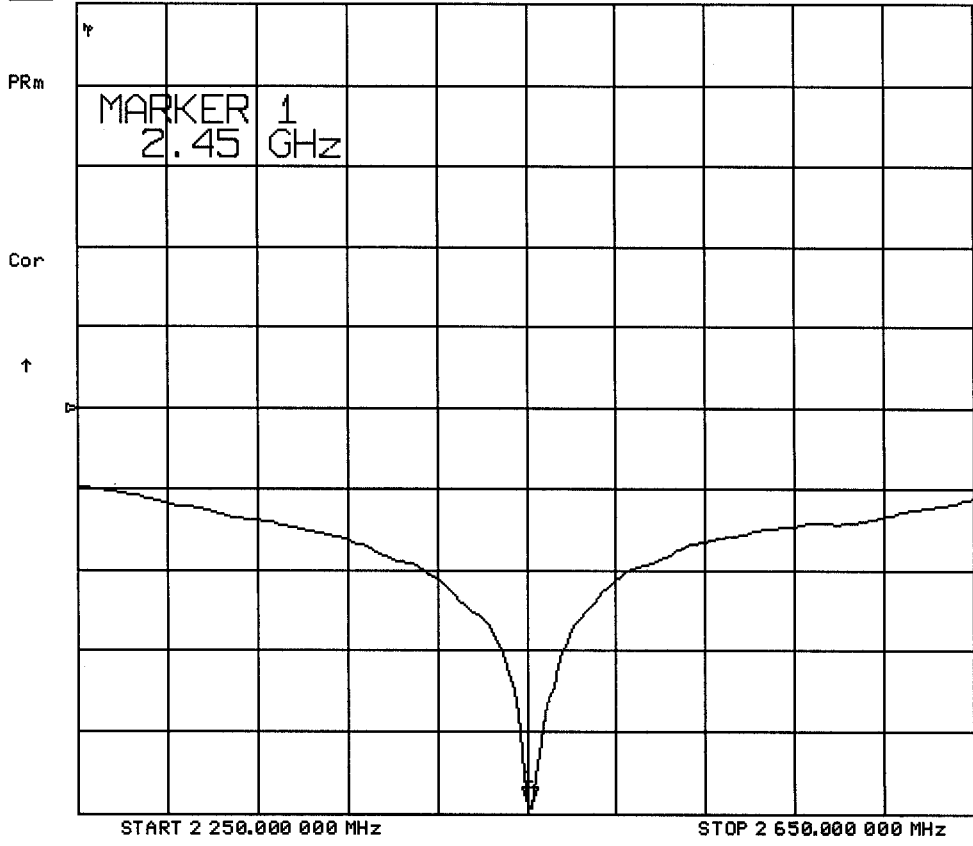

Dipole 2450MHz

SAM Phantom; Flat Section

Probe: ET3DV6 - SNI387; ConvF(4.70,4.70,4.70); Crest factor: 1.0; 2450 MHz Brain: $\sigma = 1.79 \text{ mho/m}$ $\epsilon_r = 36.8 \rho = 1.00 \text{ g/cm}^3$


Cubes (4): Peak: 29.7 mW/g $\pm 0.04 \text{ dB}$, SAR (1g): 14.0 mW/g $\pm 0.04 \text{ dB}$, SAR (10g): 6.35 mW/g $\pm 0.04 \text{ dB}$, (Worst-case extrapolation)

Penetration depth: 6.4 (6.1, 7.2) [mm]; Powerdrift: -0.04 dB


Ambient Temp.: 23.6°C; Fluid Temp.: 23.8°C

Forward Conducted Power: 250 mW

Calibration Date: October 24, 2002

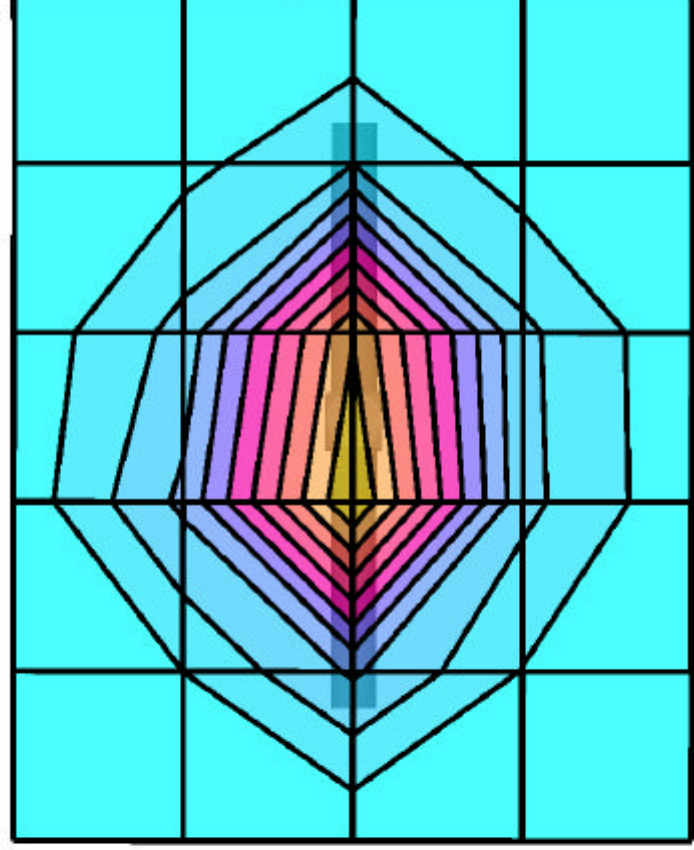

SAR_{tot} [mW/g]

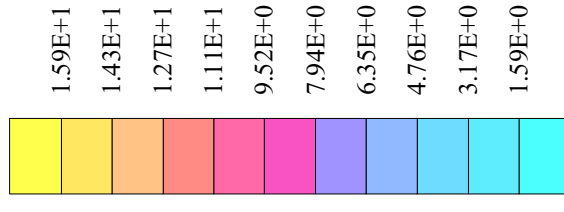

2450MHz System Validation

Measured Fluid Dielectric Parameters (Brain)

October 24, 2002

| Frequency | | ϵ' | ϵ'' |
|-------------|-----|-------------|--------------|
| 2.350000000 | GHz | 37.2108 | 12.9039 |
| 2.360000000 | GHz | 37.1695 | 12.9350 |
| 2.370000000 | GHz | 37.1398 | 12.9630 |
| 2.380000000 | GHz | 37.1057 | 12.9945 |
| 2.390000000 | GHz | 37.0746 | 13.0290 |
| 2.400000000 | GHz | 37.0424 | 13.0464 |
| 2.410000000 | GHz | 36.9746 | 13.0743 |
| 2.420000000 | GHz | 36.9322 | 13.1074 |
| 2.430000000 | GHz | 36.8908 | 13.1372 |
| 2.440000000 | GHz | 36.8449 | 13.1527 |
| 2.450000000 | GHz | 36.7983 | 13.1767 |
| 2.460000000 | GHz | 36.7651 | 13.2038 |
| 2.470000000 | GHz | 36.7300 | 13.2377 |
| 2.480000000 | GHz | 36.7004 | 13.2677 |
| 2.490000000 | GHz | 36.6658 | 13.2862 |
| 2.500000000 | GHz | 36.6120 | 13.2988 |
| 2.510000000 | GHz | 36.5655 | 13.3268 |
| 2.520000000 | GHz | 36.5147 | 13.3582 |
| 2.530000000 | GHz | 36.4743 | 13.3922 |
| 2.540000000 | GHz | 36.4044 | 13.4131 |
| 2.550000000 | GHz | 36.3807 | 13.4402 |

APPENDIX D - PROBE CALIBRATION

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79



Calibration Certificate

Dosimetric E-Field Probe

| | |
|-----------------------|-------------------------|
| Type: | ET3DV6 |
| Serial Number: | 1590 |
| Place of Calibration: | Zurich |
| Date of Calibration: | December 1, 2002 |
| Calibration Interval: | 12 months |

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

| | |
|----------------|--|
| Calibrated by: |  |
| Approved by: |  |

Probe ET3DV6

SN:1590

| | |
|-------------------|------------------|
| Manufactured: | March 19, 2001 |
| Last calibration: | April 26, 2002 |
| Recalibrated: | December 1, 2002 |

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

DASY - Parameters of Probe: ET3DV6 SN:1590

Sensitivity in Free Space

| | |
|-------|---|
| NormX | 1.75 $\mu\text{V}/(\text{V}/\text{m})^2$ |
| NormY | 1.89 $\mu\text{V}/(\text{V}/\text{m})^2$ |
| NormZ | 1.63 $\mu\text{V}/(\text{V}/\text{m})^2$ |

Diode Compression

| | | |
|-------|-----------|----|
| DCP X | 92 | mV |
| DCP Y | 92 | mV |
| DCP Z | 92 | mV |

Sensitivity in Tissue Simulating Liquid

| | | | |
|---------|------------------------------|-----------------------------|--|
| Head | 900 MHz | $\epsilon_r = 41.5 \pm 5\%$ | $\sigma = 0.97 \pm 5\% \text{ mho}/\text{m}$ |
| Head | 835 MHz | $\epsilon_r = 41.5 \pm 5\%$ | $\sigma = 0.90 \pm 5\% \text{ mho}/\text{m}$ |
| ConvF X | 6.9 $\pm 9.5\%$ (k=2) | | Boundary effect: |
| ConvF Y | 6.9 $\pm 9.5\%$ (k=2) | | Alpha 0.30 |
| ConvF Z | 6.9 $\pm 9.5\%$ (k=2) | | Depth 2.71 |
| Head | 1800 MHz | $\epsilon_r = 40.0 \pm 5\%$ | $\sigma = 1.40 \pm 5\% \text{ mho}/\text{m}$ |
| Head | 1900 MHz | $\epsilon_r = 40.0 \pm 5\%$ | $\sigma = 1.40 \pm 5\% \text{ mho}/\text{m}$ |
| ConvF X | 5.6 $\pm 9.5\%$ (k=2) | | Boundary effect: |
| ConvF Y | 5.6 $\pm 9.5\%$ (k=2) | | Alpha 0.42 |
| ConvF Z | 5.6 $\pm 9.5\%$ (k=2) | | Depth 2.56 |

Boundary Effect


| | | | |
|------|--|--|-------------|
| Head | 900 MHz | Typical SAR gradient: 5 % per mm | |
| | Probe Tip to Boundary | 1 mm | 2 mm |
| | SAR _{be} [%] Without Correction Algorithm | 8.7 | 5.0 |
| | SAR _{be} [%] With Correction Algorithm | 0.3 | 0.5 |
| Head | 1800 MHz | Typical SAR gradient: 10 % per mm | |
| | Probe Tip to Boundary | 1 mm | 2 mm |
| | SAR _{be} [%] Without Correction Algorithm | 10.7 | 7.4 |
| | SAR _{be} [%] With Correction Algorithm | 0.1 | 0.3 |

Sensor Offset


| | | |
|----------------------------|---------------------------------|----|
| Probe Tip to Sensor Center | 2.7 | mm |
| Optical Surface Detection | 1.2 \pm 0.2 | mm |

Receiving Pattern (ϕ), $\theta = 0^\circ$


f = 30 MHz, TEM cell ifi110

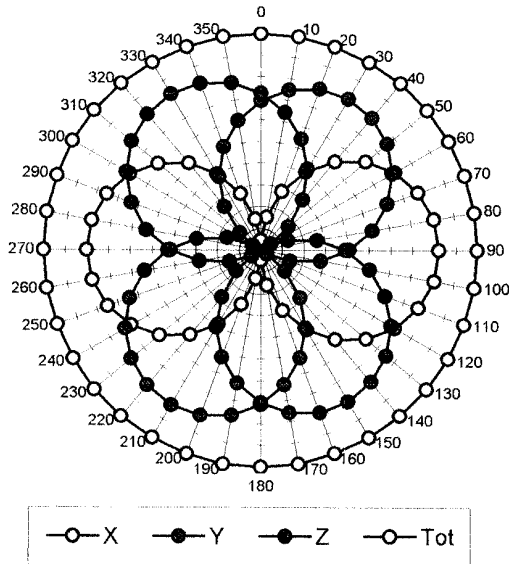


f = 100 MHz, TEM cell ifi110

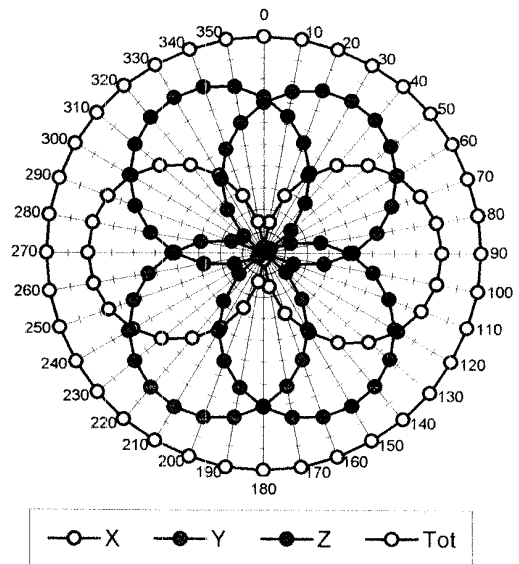


f = 300 MHz, TEM cell ifi110

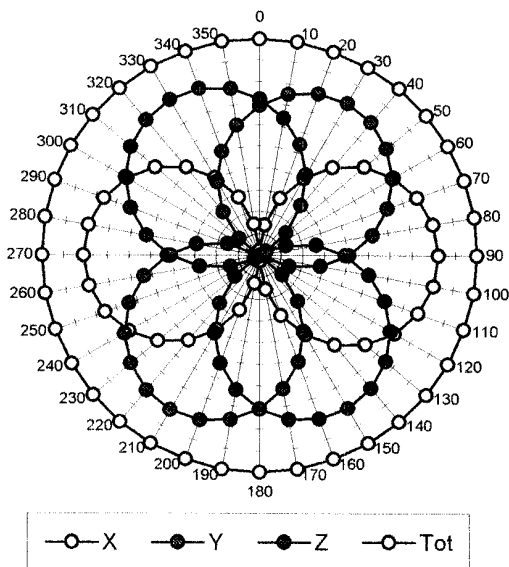


f = 900 MHz, TEM cell ifi110

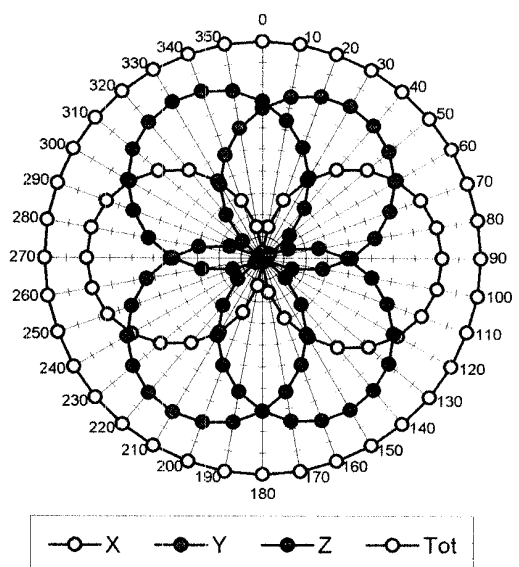

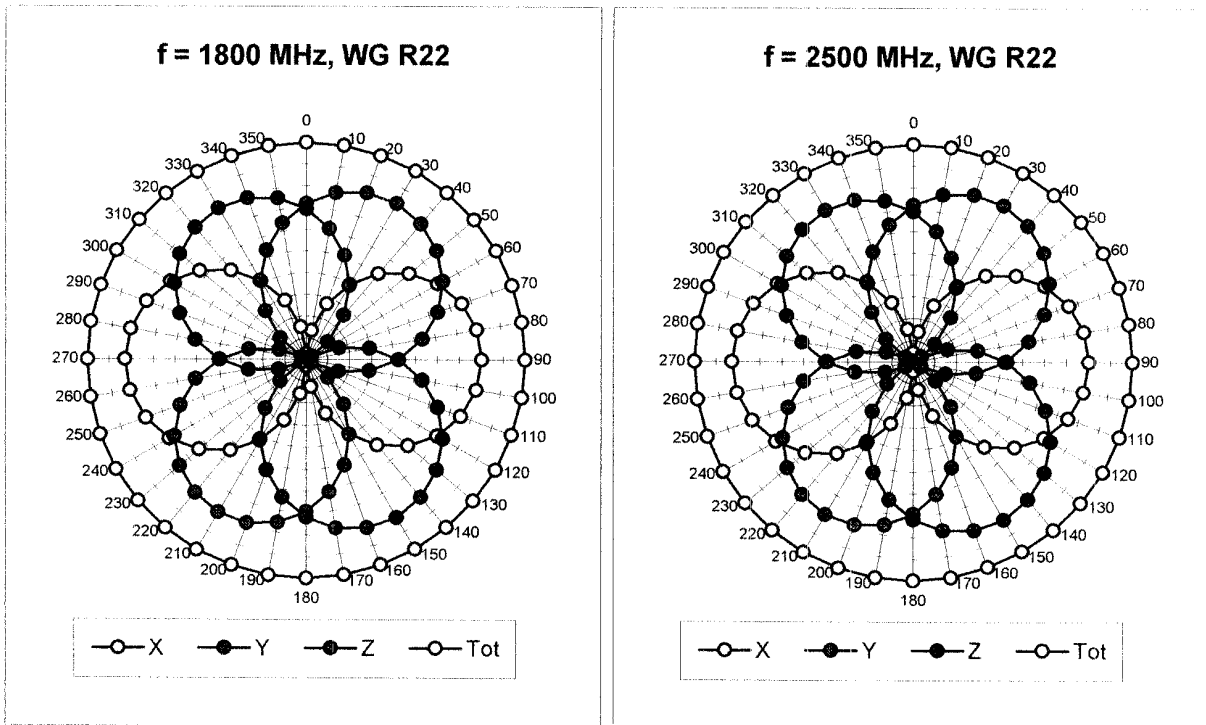


Isotropy Error (ϕ), $\theta = 0^\circ$


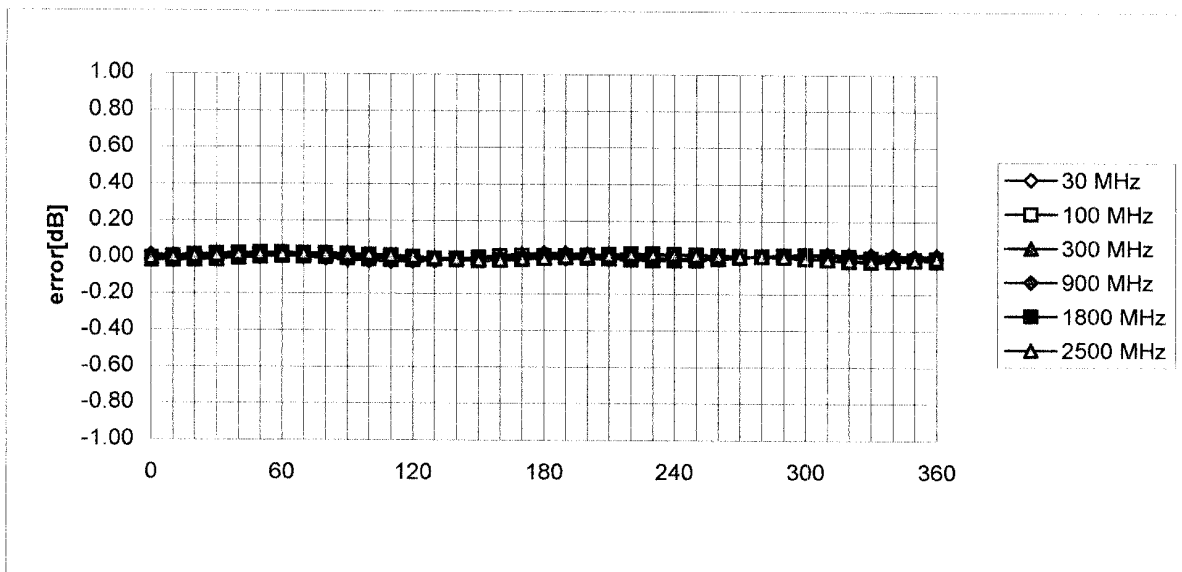


Frequency Response of E-Field


(TEM-Cell:ifi110, Waveguide R22)

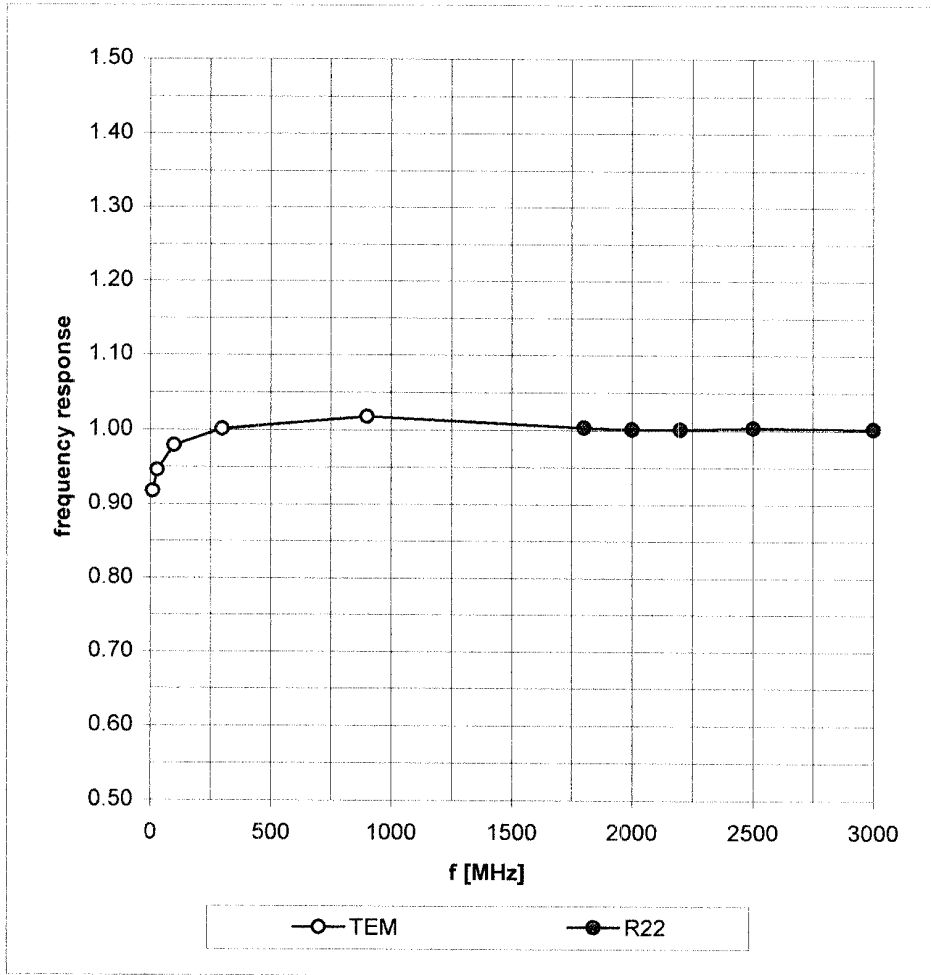

Dynamic Range f(SAR_{brain}) (Waveguide R22)

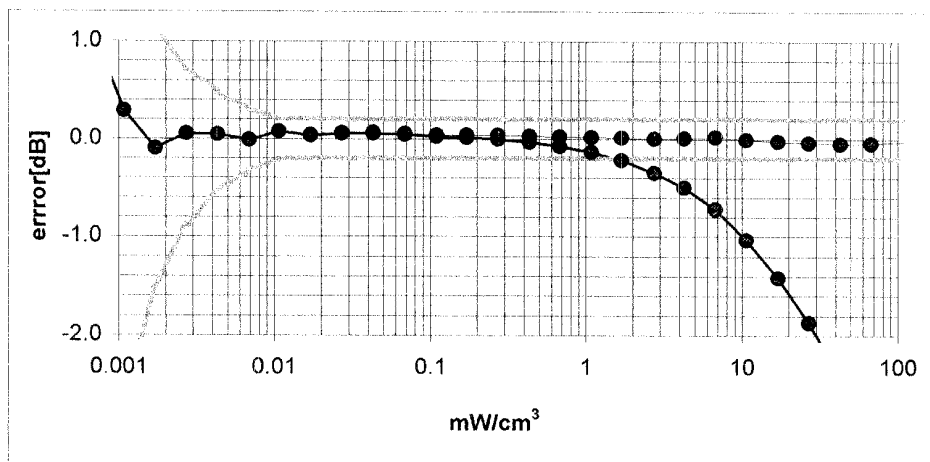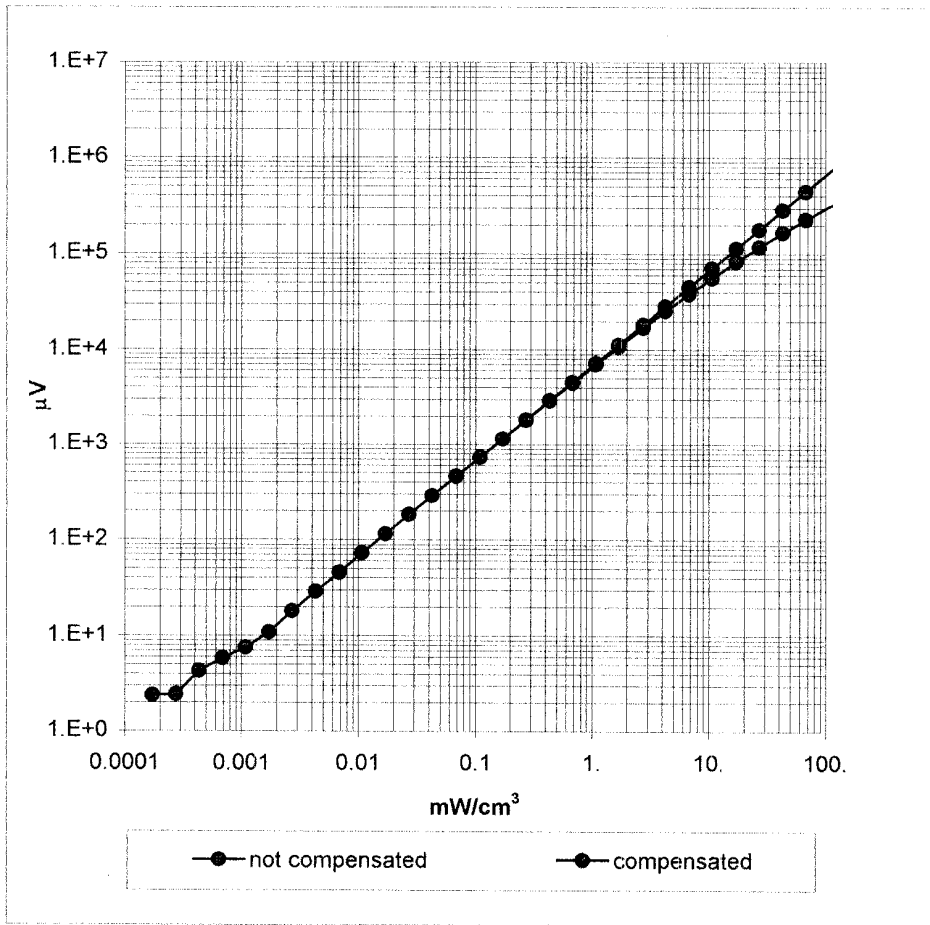


Conversion Factor Assessment

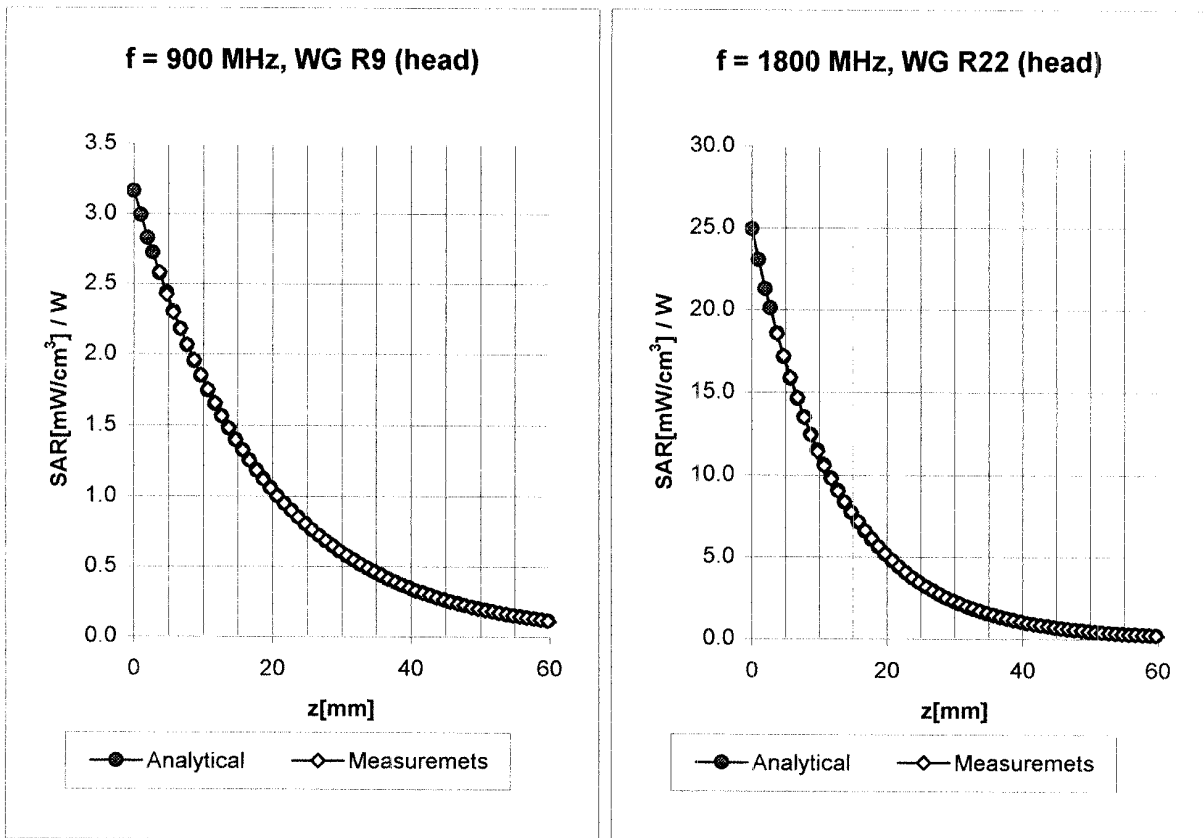

| | | | |
|-------------|-----------------|------------------------------|---------------------------------------|
| Head | 900 MHz | $\epsilon_r = 41.5 \pm 5\%$ | $\sigma = 0.97 \pm 5\% \text{ mho/m}$ |
| Head | 835 MHz | $\epsilon_r = 41.5 \pm 5\%$ | $\sigma = 0.90 \pm 5\% \text{ mho/m}$ |
| | ConvF X | 6.9 $\pm 9.5\%$ (k=2) | Boundary effect: |
| | ConvF Y | 6.9 $\pm 9.5\%$ (k=2) | Alpha 0.30 |
| | ConvF Z | 6.9 $\pm 9.5\%$ (k=2) | Depth 2.71 |
| | | | |
| Head | 1800 MHz | $\epsilon_r = 40.0 \pm 5\%$ | $\sigma = 1.40 \pm 5\% \text{ mho/m}$ |
| Head | 1900 MHz | $\epsilon_r = 40.0 \pm 5\%$ | $\sigma = 1.40 \pm 5\% \text{ mho/m}$ |
| | ConvF X | 5.6 $\pm 9.5\%$ (k=2) | Boundary effect: |
| | ConvF Y | 5.6 $\pm 9.5\%$ (k=2) | Alpha 0.42 |
| | ConvF Z | 5.6 $\pm 9.5\%$ (k=2) | Depth 2.56 |


Conversion Factor Assessment

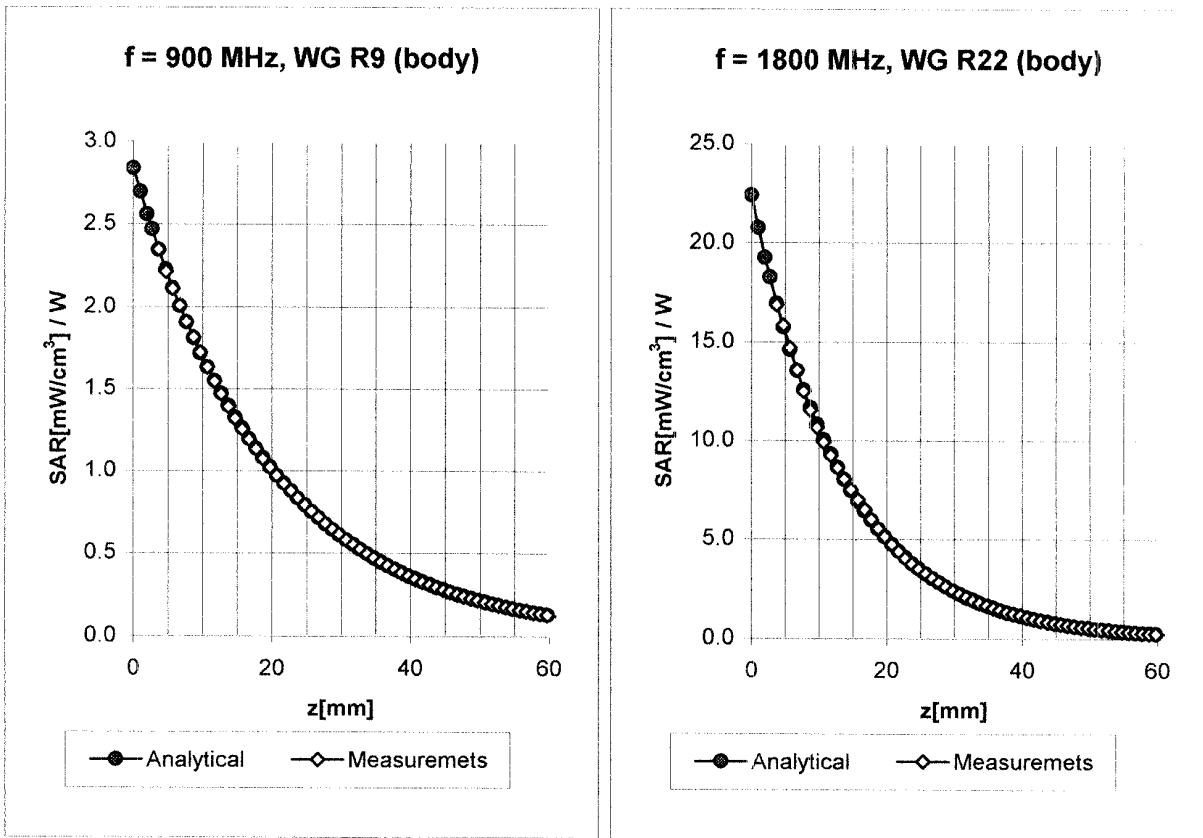

| | | | |
|-------------|-----------------|------------------------------|---------------------------------------|
| Body | 900 MHz | $\epsilon_r = 55.0 \pm 5\%$ | $\sigma = 1.05 \pm 5\% \text{ mho/m}$ |
| Body | 835 MHz | $\epsilon_r = 55.2 \pm 5\%$ | $\sigma = 0.97 \pm 5\% \text{ mho/m}$ |
| | ConvF X | 6.7 $\pm 9.5\%$ (k=2) | Boundary effect: |
| | ConvF Y | 6.7 $\pm 9.5\%$ (k=2) | Alpha 0.34 |
| | ConvF Z | 6.7 $\pm 9.5\%$ (k=2) | Depth 2.57 |
| | | | |
| Body | 1800 MHz | $\epsilon_r = 53.3 \pm 5\%$ | $\sigma = 1.52 \pm 5\% \text{ mho/m}$ |
| Body | 1900 MHz | $\epsilon_r = 53.3 \pm 5\%$ | $\sigma = 1.52 \pm 5\% \text{ mho/m}$ |
| | ConvF X | 5.3 $\pm 9.5\%$ (k=2) | Boundary effect: |
| | ConvF Y | 5.3 $\pm 9.5\%$ (k=2) | Alpha 0.52 |
| | ConvF Z | 5.3 $\pm 9.5\%$ (k=2) | Depth 2.46 |

Deviation from Isotropy in HSL

Error (θ, ϕ), $f = 900$ MHz

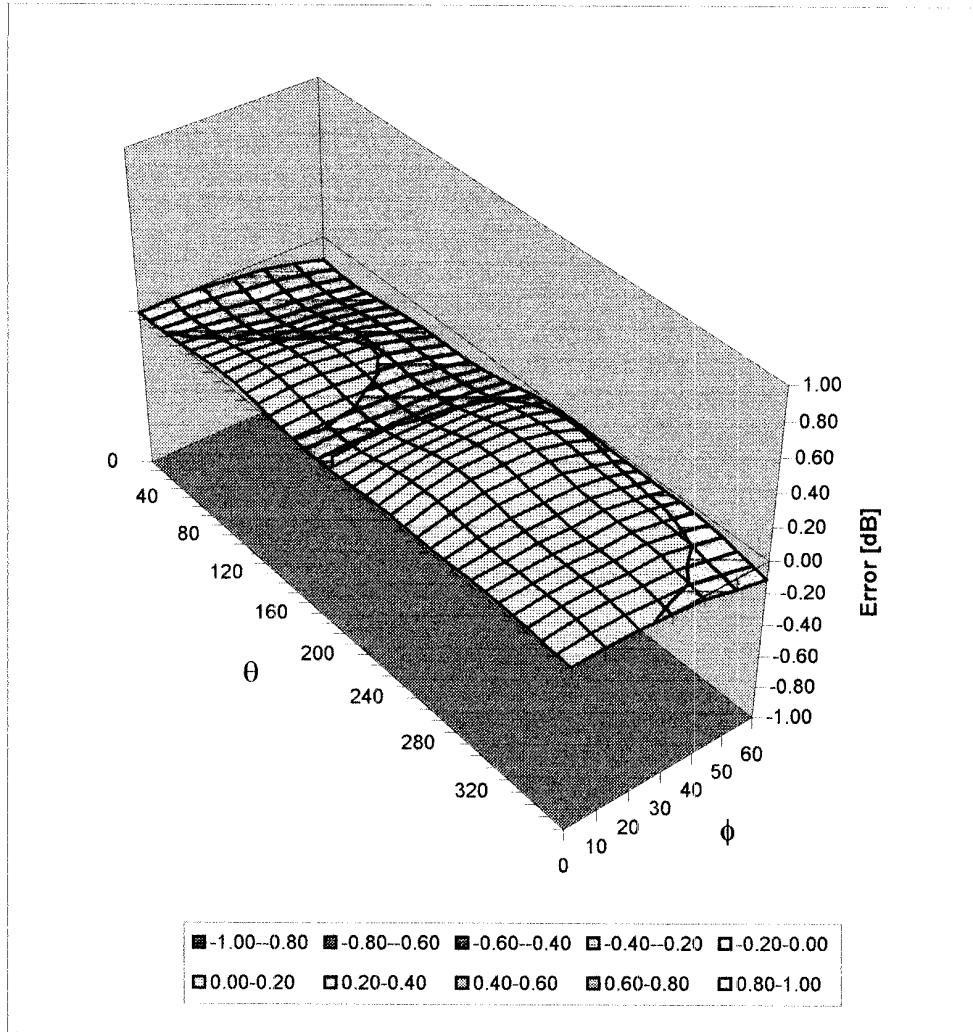

Additional Conversion Factors for Dosimetric E-Field Probe

Type:

ET3DV6

Serial Number:

1590

Place of Assessment:

Zurich

Date of Assessment:


May 1, 2002

Probe Calibration Date:

April 26, 2002

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Assessed by:



Dosimetric E-Field Probe ET3DV6 SN:1590

Conversion factor (\pm standard deviation)

| | | | |
|----------|-------|--------------|---|
| 150 MHz | ConvF | 9.4 \pm 8% | $\epsilon_r = 52.3$ $\sigma = 0.76$ mho/m (head tissue) |
| 300 MHz | ConvF | 8.2 \pm 8% | $\epsilon_r = 45.3$ $\sigma = 0.87$ mho/m (head tissue) |
| 450 MHz | ConvF | 7.8 \pm 8% | $\epsilon_r = 43.5$ $\sigma = 0.87$ mho/m (head tissue) |
| 150 MHz | ConvF | 9.1 \pm 8% | $\epsilon_r = 61.9$ $\sigma = 0.80$ mho/m (body tissue) |
| 450 MHz | ConvF | 7.9 \pm 8% | $\epsilon_r = 56.7$ $\sigma = 0.94$ mho/m (body tissue) |
| 2450 MHz | ConvF | 4.5 \pm 8% | $\epsilon_r = 39.2$ $\sigma = 1.80$ mho/m (head tissue) |
| 2450 MHz | ConvF | 4.1 \pm 8% | $\epsilon_r = 52.7$ $\sigma = 1.95$ mho/m (body tissue) |

APPENDIX E - MEASURED FLUID DIELECTRIC PARAMETERS

1800MHz System Performance Check

Measured Fluid Dielectric Parameters (Brain)

February 05, 2003

| Frequency | e' | e'' |
|-----------------|---------|---------|
| 1.700000000 GHz | 40.4061 | 13.8009 |
| 1.710000000 GHz | 40.3733 | 13.8098 |
| 1.720000000 GHz | 40.3382 | 13.8292 |
| 1.730000000 GHz | 40.3126 | 13.8524 |
| 1.740000000 GHz | 40.2715 | 13.9054 |
| 1.750000000 GHz | 40.2335 | 13.9505 |
| 1.760000000 GHz | 40.1868 | 13.9883 |
| 1.770000000 GHz | 40.1670 | 14.0289 |
| 1.780000000 GHz | 40.1124 | 14.0533 |
| 1.790000000 GHz | 40.0603 | 14.0852 |
| 1.800000000 GHz | 40.0190 | 14.1231 |
| 1.810000000 GHz | 39.9656 | 14.1531 |
| 1.820000000 GHz | 39.9030 | 14.1856 |
| 1.830000000 GHz | 39.8698 | 14.1952 |
| 1.840000000 GHz | 39.8129 | 14.2278 |
| 1.850000000 GHz | 39.7683 | 14.2444 |
| 1.860000000 GHz | 39.7407 | 14.2628 |
| 1.870000000 GHz | 39.6906 | 14.2859 |
| 1.880000000 GHz | 39.6470 | 14.3082 |
| 1.890000000 GHz | 39.6163 | 14.3403 |
| 1.900000000 GHz | 39.5770 | 14.3515 |

1900MHz EUT Evaluation (Head)

Measured Fluid Dielectric Parameters (Brain)

February 05, 2003

| Frequency | ϵ' | ϵ'' |
|-----------------|-------------|--------------|
| 1.780000000 GHz | 38.6873 | 12.9569 |
| 1.790000000 GHz | 38.6348 | 12.9971 |
| 1.800000000 GHz | 38.5879 | 13.0134 |
| 1.810000000 GHz | 38.5244 | 13.0453 |
| 1.820000000 GHz | 38.4633 | 13.0789 |
| 1.830000000 GHz | 38.4096 | 13.1026 |
| 1.840000000 GHz | 38.3629 | 13.1312 |
| 1.850000000 GHz | 38.3326 | 13.1358 |
| 1.860000000 GHz | 38.3044 | 13.1422 |
| 1.870000000 GHz | 38.2669 | 13.1657 |
| 1.880000000 GHz | 38.2332 | 13.1842 |
| 1.890000000 GHz | 38.2020 | 13.2099 |
| 1.900000000 GHz | 38.1546 | 13.2309 |
| 1.910000000 GHz | 38.1238 | 13.2536 |
| 1.920000000 GHz | 38.0701 | 13.2700 |
| 1.930000000 GHz | 38.0280 | 13.3084 |
| 1.940000000 GHz | 38.0164 | 13.3340 |
| 1.950000000 GHz | 37.9901 | 13.3571 |
| 1.960000000 GHz | 37.9699 | 13.3793 |
| 1.970000000 GHz | 37.9247 | 13.4055 |
| 1.980000000 GHz | 37.8975 | 13.4406 |

900MHz System Performance Check

Measured Fluid Dielectric Parameters (Brain)

February 05, 2003

| Frequency | ϵ' | ϵ'' |
|-----------------|-------------|--------------|
| 800.000000 MHz | 42.1740 | 19.7156 |
| 810.000000 MHz | 42.0933 | 19.7013 |
| 820.000000 MHz | 41.9317 | 19.6725 |
| 830.000000 MHz | 41.8074 | 19.6084 |
| 840.000000 MHz | 41.6626 | 19.5887 |
| 850.000000 MHz | 41.5291 | 19.5567 |
| 860.000000 MHz | 41.4146 | 19.5412 |
| 870.000000 MHz | 41.2620 | 19.4866 |
| 880.000000 MHz | 41.1726 | 19.4965 |
| 890.000000 MHz | 41.0479 | 19.4769 |
| 900.000000 MHz | 40.9714 | 19.3895 |
| 910.000000 MHz | 40.8670 | 19.3664 |
| 920.000000 MHz | 40.7501 | 19.2749 |
| 930.000000 MHz | 40.6708 | 19.2660 |
| 940.000000 MHz | 40.5484 | 19.2325 |
| 950.000000 MHz | 40.4001 | 19.2273 |
| 960.000000 MHz | 40.3158 | 19.2033 |
| 970.000000 MHz | 40.1948 | 19.1730 |
| 980.000000 MHz | 40.0876 | 19.1766 |
| 990.000000 MHz | 39.9922 | 19.1632 |
| 1.000000000 GHz | 39.9056 | 19.0976 |

835MHz EUT Evaluation (Head)

Measured Fluid Dielectric Parameters (Brain)

February 05, 2003

| Frequency | ϵ' | ϵ'' |
|-----------------------|----------------|----------------|
| 735.000000 MHz | 43.9057 | 20.3575 |
| 745.000000 MHz | 43.7600 | 20.3386 |
| 755.000000 MHz | 43.6378 | 20.2802 |
| 765.000000 MHz | 43.4930 | 20.2068 |
| 775.000000 MHz | 43.3777 | 20.1841 |
| 785.000000 MHz | 43.2591 | 20.1745 |
| 795.000000 MHz | 43.1569 | 20.1280 |
| 805.000000 MHz | 43.0713 | 20.0891 |
| 815.000000 MHz | 42.9442 | 20.0252 |
| 825.000000 MHz | 42.8254 | 20.0143 |
| 835.000000 MHz | 42.6693 | 19.9884 |
| 845.000000 MHz | 42.5414 | 19.9350 |
| 855.000000 MHz | 42.3724 | 19.9057 |
| 865.000000 MHz | 42.2461 | 19.8656 |
| 875.000000 MHz | 42.1132 | 19.8594 |
| 885.000000 MHz | 42.0308 | 19.8392 |
| 895.000000 MHz | 41.9503 | 19.7489 |
| 905.000000 MHz | 41.8650 | 19.7166 |
| 915.000000 MHz | 41.7337 | 19.6698 |
| 925.000000 MHz | 41.6408 | 19.6566 |
| 935.000000 MHz | 41.5240 | 19.6033 |

1800MHz System Performance Check

Measured Fluid Dielectric Parameters (Brain)

February 06, 2003

| Frequency | e' | e'' |
|-----------------|---------|---------|
| 1.700000000 GHz | 40.3798 | 13.6837 |
| 1.710000000 GHz | 40.3602 | 13.6951 |
| 1.720000000 GHz | 40.3428 | 13.7239 |
| 1.730000000 GHz | 40.3332 | 13.7635 |
| 1.740000000 GHz | 40.2970 | 13.8033 |
| 1.750000000 GHz | 40.2597 | 13.8594 |
| 1.760000000 GHz | 40.2399 | 13.9108 |
| 1.770000000 GHz | 40.1942 | 13.9531 |
| 1.780000000 GHz | 40.1424 | 13.9931 |
| 1.790000000 GHz | 40.1023 | 14.0196 |
| 1.800000000 GHz | 40.0392 | 14.0514 |
| 1.810000000 GHz | 39.9723 | 14.1044 |
| 1.820000000 GHz | 39.9305 | 14.1262 |
| 1.830000000 GHz | 39.8701 | 14.1601 |
| 1.840000000 GHz | 39.8256 | 14.2024 |
| 1.850000000 GHz | 39.7963 | 14.2136 |
| 1.860000000 GHz | 39.7578 | 14.2371 |
| 1.870000000 GHz | 39.6143 | 14.2698 |
| 1.880000000 GHz | 39.6860 | 14.3051 |
| 1.890000000 GHz | 39.6368 | 14.3388 |
| 1.900000000 GHz | 39.5979 | 14.3539 |

1900MHz EUT Evaluation (Body)

Measured Fluid Dielectric Parameters (Muscle)

February 06, 2003

| Frequency | ϵ' | ϵ'' |
|-----------------|-------------|--------------|
| 1.780000000 GHz | 52.7796 | 13.9878 |
| 1.790000000 GHz | 52.7309 | 14.0132 |
| 1.800000000 GHz | 52.7071 | 14.0612 |
| 1.810000000 GHz | 52.6554 | 14.0826 |
| 1.820000000 GHz | 52.6011 | 14.1030 |
| 1.830000000 GHz | 52.5695 | 14.1222 |
| 1.840000000 GHz | 52.5274 | 14.1438 |
| 1.850000000 GHz | 52.4862 | 14.1684 |
| 1.860000000 GHz | 52.4521 | 14.1907 |
| 1.870000000 GHz | 52.4158 | 14.2044 |
| 1.880000000 GHz | 52.3952 | 14.2296 |
| 1.890000000 GHz | 52.3583 | 14.2626 |
| 1.900000000 GHz | 52.3421 | 14.2806 |
| 1.910000000 GHz | 52.2986 | 14.3021 |
| 1.920000000 GHz | 52.2808 | 14.3184 |
| 1.930000000 GHz | 52.2599 | 14.3450 |
| 1.940000000 GHz | 52.2554 | 14.3601 |
| 1.950000000 GHz | 52.2385 | 14.3833 |
| 1.960000000 GHz | 52.2083 | 14.3903 |
| 1.970000000 GHz | 52.1897 | 14.4155 |
| 1.980000000 GHz | 52.1720 | 14.4436 |

900MHz System Performance Check

Measured Fluid Dielectric Parameters (Brain)

February 06, 2003

| Frequency | ϵ' | ϵ'' |
|-----------------|-------------|--------------|
| 800.000000 MHz | 42.2516 | 19.8355 |
| 810.000000 MHz | 42.1387 | 19.7978 |
| 820.000000 MHz | 42.0176 | 19.7745 |
| 830.000000 MHz | 41.8900 | 19.6955 |
| 840.000000 MHz | 41.7743 | 19.6998 |
| 850.000000 MHz | 41.6084 | 19.6252 |
| 860.000000 MHz | 41.5266 | 19.6111 |
| 870.000000 MHz | 41.3653 | 19.5597 |
| 880.000000 MHz | 41.2624 | 19.5538 |
| 890.000000 MHz | 41.1575 | 19.5290 |
| 900.000000 MHz | 41.0716 | 19.4246 |
| 910.000000 MHz | 40.9775 | 19.3990 |
| 920.000000 MHz | 40.8824 | 19.3600 |
| 930.000000 MHz | 40.7844 | 19.3181 |
| 940.000000 MHz | 40.6835 | 19.2880 |
| 950.000000 MHz | 40.5394 | 19.2632 |
| 960.000000 MHz | 40.4590 | 19.2477 |
| 970.000000 MHz | 40.3532 | 19.2035 |
| 980.000000 MHz | 40.2108 | 19.2099 |
| 990.000000 MHz | 40.1196 | 19.1911 |
| 1.000000000 GHz | 40.0367 | 19.1474 |

835MHz EUT Evaluation (Body)

Measured Fluid Dielectric Parameters (Muscle)

February 06, 2003

| Frequency | ϵ' | ϵ'' |
|----------------|-------------|--------------|
| 735.000000 MHz | 54.1219 | 21.2500 |
| 745.000000 MHz | 54.0580 | 21.2023 |
| 755.000000 MHz | 53.8874 | 21.1430 |
| 765.000000 MHz | 53.7792 | 21.0768 |
| 775.000000 MHz | 53.6616 | 21.0385 |
| 785.000000 MHz | 53.5728 | 21.0030 |
| 795.000000 MHz | 53.4847 | 20.9566 |
| 805.000000 MHz | 53.4224 | 20.9078 |
| 815.000000 MHz | 53.3484 | 20.8636 |
| 825.000000 MHz | 53.2422 | 20.8426 |
| 835.000000 MHz | 53.1222 | 20.8164 |
| 845.000000 MHz | 53.0085 | 20.7944 |
| 855.000000 MHz | 52.8885 | 20.7431 |
| 865.000000 MHz | 52.7609 | 20.7175 |
| 875.000000 MHz | 52.6412 | 20.7008 |
| 885.000000 MHz | 52.5292 | 20.6925 |
| 895.000000 MHz | 52.4905 | 20.6048 |
| 905.000000 MHz | 52.3781 | 20.5621 |
| 915.000000 MHz | 52.2834 | 20.5548 |
| 925.000000 MHz | 52.2066 | 20.5053 |
| 935.000000 MHz | 52.0883 | 20.4833 |

2450MHz System Performance Check

Measured Fluid Dielectric Parameters (Brain)

February 07, 2003

| Frequency | | ϵ' | ϵ'' |
|-------------|-----|-------------|--------------|
| 2.350000000 | GHz | 36.0271 | 13.4825 |
| 2.360000000 | GHz | 35.9858 | 13.5136 |
| 2.370000000 | GHz | 35.9561 | 13.5416 |
| 2.380000000 | GHz | 35.8820 | 13.5731 |
| 2.390000000 | GHz | 35.8409 | 13.6076 |
| 2.400000000 | GHz | 35.8087 | 13.6250 |
| 2.410000000 | GHz | 35.7851 | 13.6529 |
| 2.420000000 | GHz | 35.7485 | 13.6860 |
| 2.430000000 | GHz | 35.7071 | 13.7158 |
| 2.440000000 | GHz | 35.6612 | 13.7313 |
| 2.450000000 | GHz | 35.6146 | 13.7553 |
| 2.460000000 | GHz | 35.5814 | 13.7824 |
| 2.470000000 | GHz | 35.5463 | 13.8163 |
| 2.480000000 | GHz | 35.5167 | 13.8463 |
| 2.490000000 | GHz | 35.4821 | 13.8648 |
| 2.500000000 | GHz | 35.4283 | 13.8774 |
| 2.510000000 | GHz | 35.3818 | 13.9054 |
| 2.520000000 | GHz | 35.3310 | 13.9638 |
| 2.530000000 | GHz | 35.2906 | 13.9708 |
| 2.540000000 | GHz | 35.2207 | 13.9991 |
| 2.550000000 | GHz | 35.2970 | 14.0188 |

2450MHz EUT Evaluation (Body)

Measured Fluid Dielectric Parameters (Muscle)

February 07, 2003

| Frequency | ϵ' | ϵ'' |
|-----------------|-------------|--------------|
| 2.350000000 GHz | 48.1875 | 14.4457 |
| 2.360000000 GHz | 48.1641 | 14.5004 |
| 2.370000000 GHz | 48.1334 | 14.5432 |
| 2.380000000 GHz | 48.1113 | 14.5419 |
| 2.390000000 GHz | 48.0725 | 14.5613 |
| 2.400000000 GHz | 48.0341 | 14.5611 |
| 2.410000000 GHz | 47.9777 | 14.5897 |
| 2.420000000 GHz | 47.9240 | 14.6325 |
| 2.430000000 GHz | 47.8743 | 14.6652 |
| 2.440000000 GHz | 47.8417 | 14.7100 |
| 2.450000000 GHz | 47.7897 | 14.7756 |
| 2.460000000 GHz | 47.7626 | 14.8481 |
| 2.470000000 GHz | 47.7327 | 14.8916 |
| 2.480000000 GHz | 47.7271 | 14.9228 |
| 2.490000000 GHz | 47.6871 | 14.9452 |
| 2.500000000 GHz | 47.6706 | 14.9364 |
| 2.510000000 GHz | 47.6281 | 14.9757 |
| 2.520000000 GHz | 47.5699 | 14.9994 |
| 2.530000000 GHz | 47.5285 | 15.0253 |
| 2.540000000 GHz | 47.4758 | 15.0640 |
| 2.550000000 GHz | 47.4343 | 15.1240 |

2450MHz EUT Evaluation (Body)

Measured Fluid Dielectric Parameters (Muscle)

February 07, 2003

| Frequency | e' | e'' |
|-----------------|---------|---------|
| 2.350000000 GHz | 48.1875 | 14.4457 |
| 2.360000000 GHz | 48.1641 | 14.5004 |
| 2.370000000 GHz | 48.1334 | 14.5432 |
| 2.380000000 GHz | 48.1113 | 14.5419 |
| 2.390000000 GHz | 48.0725 | 14.5613 |
| 2.400000000 GHz | 48.0341 | 14.5611 |
| 2.410000000 GHz | 47.9777 | 14.5897 |
| 2.420000000 GHz | 47.9240 | 14.6325 |
| 2.430000000 GHz | 47.8743 | 14.6652 |
| 2.440000000 GHz | 47.8417 | 14.7100 |
| 2.450000000 GHz | 47.7897 | 14.7756 |
| 2.460000000 GHz | 47.7626 | 14.8481 |
| 2.470000000 GHz | 47.7327 | 14.8916 |
| 2.480000000 GHz | 47.7271 | 14.9228 |
| 2.490000000 GHz | 47.6871 | 14.9452 |
| 2.500000000 GHz | 47.6706 | 14.9364 |
| 2.510000000 GHz | 47.6281 | 14.9757 |
| 2.520000000 GHz | 47.5699 | 14.9994 |
| 2.530000000 GHz | 47.5285 | 15.0253 |
| 2.540000000 GHz | 47.4758 | 15.0640 |
| 2.550000000 GHz | 47.4343 | 15.1240 |

APPENDIX F - SAM PHANTOM CERTIFICATE OF CONFORMITY

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Certificate of conformity / First Article Inspection

| | |
|-----------------------|--|
| Item | SAM Twin Phantom V4.0 |
| Type No | QD 000 P40 BA |
| Series No | TP-1002 and higher |
| Manufacturer / Origin | Untersee Composites Hauptstr. 69 CH-8559 Fruthwilen Switzerland |

Tests

The series production process used allows the limitation to test of first articles. Complete tests were made on the pre-series Type No. QD 000 P40 AA, Serial No. TP-1001 and on the series first article Type No. QD 000 P40 BA, Serial No. TP-1006. Certain parameters have been retested using further series units (called samples).

| Test | Requirement | Details | Units tested |
|----------------------|---|--|---------------------------|
| Shape | Compliance with the geometry according to the CAD model. | IT'IS CAD File (*) | First article, Samples |
| Material thickness | Compliant with the requirements according to the standards | 2mm +/- 0.2mm in specific areas | First article, Samples |
| Material parameters | Dielectric parameters for required frequencies | 200 MHz – 3 GHz Relative permittivity < 5 Loss tangent < 0.05. | Material sample TP 104-5 |
| Material resistivity | The material has been tested to be compatible with the liquids defined in the standards | Liquid type HSL 1800 and others according to the standard. | Pre-series, First article |

Standards

- [1] CENELEC EN 50361
- [2] IEEE P1528-200x draft 6.5
- [3] IEC PT 62209 draft 0.9

(*) The IT'IS CAD file is derived from [2] and is also within the tolerance requirements of the shapes of [1] and [3].

Conformity

Based on the sample tests above, we certify that this item is in compliance with the uncertainty requirements of SAR measurements specified in standard [1] and draft standards [2] and [3].

Date 18.11.2001

Signature / Stamp



**Schmid & Partner
Engineering AG**



Zeughausstrasse 43, CH-8004 Zurich
Tel. +41 1 245 97 00, Fax +41 1 245 97 79

APPENDIX G - SAR TEST SETUP & EUT PHOTOGRAPHS

SAR TEST SETUP PHOTOGRAPHS
Single-Band External Stubby Antenna (P/N: 805-606-004)
Left Head Section / Cheek-Touch Position




SAR TEST SETUP PHOTOGRAPHS
Single-Band External Stubby Antenna (P/N: 805-606-004)
Left Head Section / Ear-Tilt Position



SAR TEST SETUP PHOTOGRAPHS
Single-Band External Stubby Antenna (P/N: 805-606-004)
Right Head Section / Cheek-Touch Position




SAR TEST SETUP PHOTOGRAPHS
Single-Band External Stubby Antenna (P/N: 805-606-004)
Right Head Section / Ear-Tilt Position

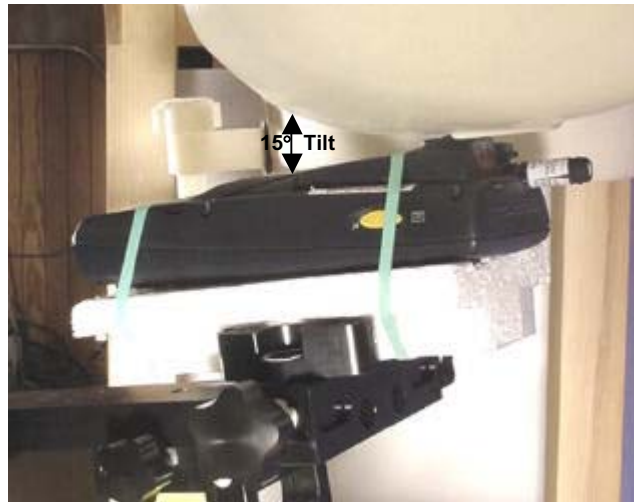

SAR TEST SETUP PHOTOGRAPHS
Dual-Band External Stubby Antenna (P/N: 805-606-002)
Left Head Section / Cheek-Touch Position




SAR TEST SETUP PHOTOGRAPHS
Dual-Band External Stubby Antenna (P/N: 805-606-002)
Left Head Section / Ear-Tilt Position

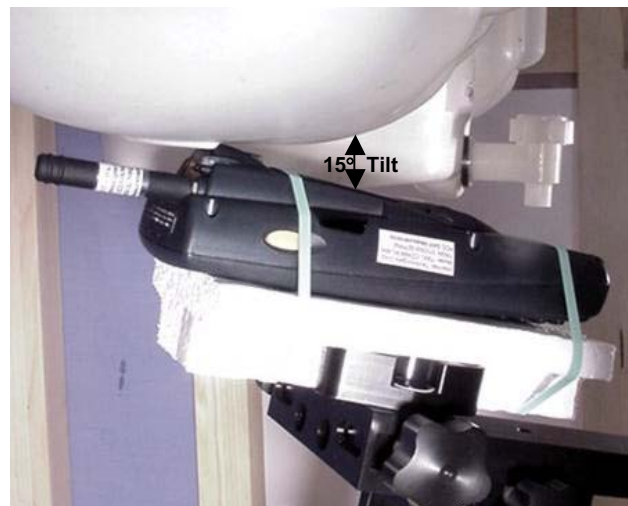

SAR TEST SETUP PHOTOGRAPHS
Dual-Band External Stubby Antenna (P/N: 805-606-002)
Right Head Section / Cheek-Touch Position



SAR TEST SETUP PHOTOGRAPHS
Dual-Band External Stubby Antenna (P/N: 805-606-002)
Right Head Section / Ear-Tilt Position

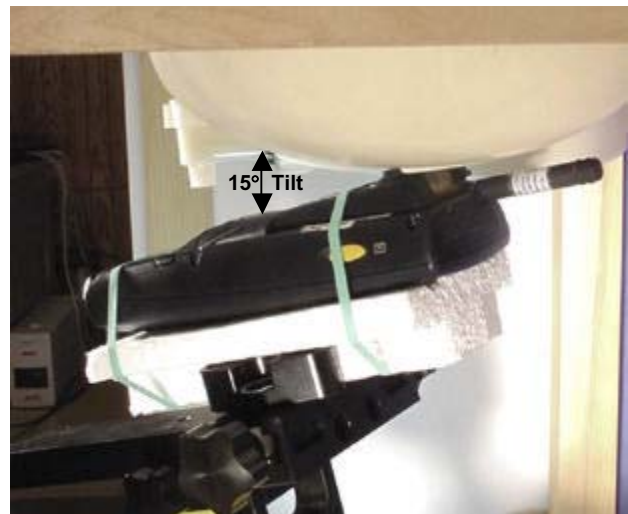

SAR TEST SETUP PHOTOGRAPHS
Single-Band External Stubby Antenna (P/N: 805-606-004)
Body-Worn / Back Side / 0.0cm Separation Distance



SAR TEST SETUP PHOTOGRAPHS
Single-Band External Stubby Antenna (P/N: 805-606-004)
Body-Worn / Right Side / 0.0cm Separation Distance



SAR TEST SETUP PHOTOGRAPHS
Single-Band External Stubby Antenna (P/N: 805-606-004
Body-Worn / Top Side / 1.5cm Separation Distance



SAR TEST SETUP PHOTOGRAPHS
Dual-Band External Stubby Antenna (P/N: 805-606-002)
Body-Worn / Back Side / 0.0cm Separation Distance



SAR TEST SETUP PHOTOGRAPHS
Dual-Band External Stubby Antenna (P/N: 805-606-002)
Body-Worn / Right Side / 0.0cm Separation Distance



SAR TEST SETUP PHOTOGRAPHS
Dual-Band External Stubby Antenna (P/N: 805-606-002)
Body-Worn / Top End / 1.5cm Separation Distance



SAR TEST SETUP PHOTOGRAPHS
Internal Patch Antenna
Body-Worn / Back Side / 0.0cm Separation Distance



SAR TEST SETUP PHOTOGRAPHS
Internal Patch Antenna
Body-Worn / Left Side / 0.0cm Separation Distance



SAR TEST SETUP PHOTOGRAPHS
Internal Patch Antenna
Body-Worn / Right Side / 0.0cm Separation Distance



EUT PHOTOGRAPHS
with Single-Band External Stubby Antenna (P/N: 805-606-004)



Front of EUT



Back of EUT



Single-Band Stubby Antenna (P/N: 805-606-004)



Left Side of EUT



Right Side of EUT

EUT PHOTOGRAPHS
with Dual-Band External Stubby Antenna (P/N: 805-606-002)



Front of EUT



Back of EUT



Dual-Band Stubby Antenna (P/N: 805-606-002)



Left Side of EUT



Right Side of EUT

EUT PHOTOGRAPHS



Battery Compartment



Lithium-Ion Battery



Lithium-Ion Battery