

# AGFA

## Medical Imaging *RDE*



From: [Jan Vercammen \(6233\) – MI/TSP-HW/Electronics](#)


Date: January 27, 2005



**Concerning: Foto's Drystar 5300 (FCC ID: HPL5365) – Part 1**


---



Overview of photo session :


1. page 2: VILIS mother PCB
2. page 3: Themis CPU PCB
3. page 4: 512Mbyte SDRAM module
4. page 5: printhead interface PCB
5. page 6: keypad PCB
6. page 7: RFID tag reader PCB
7. page 8: optical diode calibration module ODM PCB
8. page 9: LED light source for optical calibration
9. page 10: PCB
10. page 11 & 12: power supply unit A

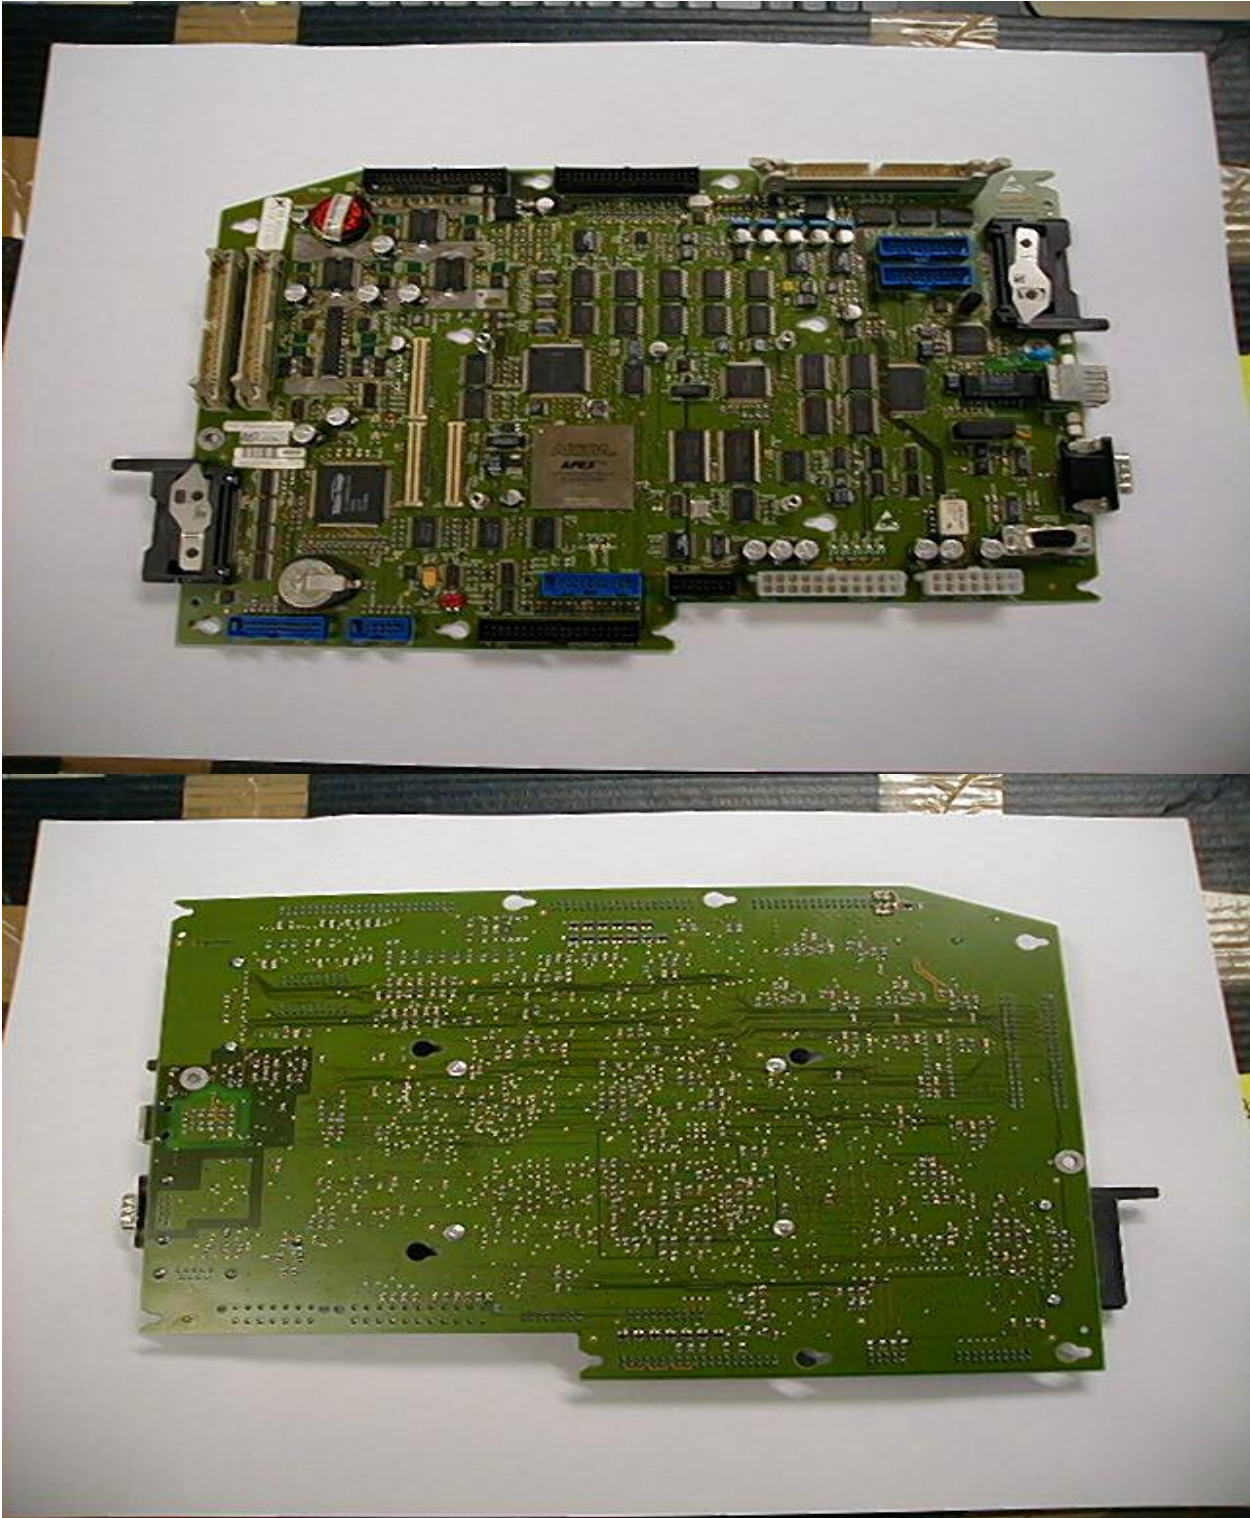

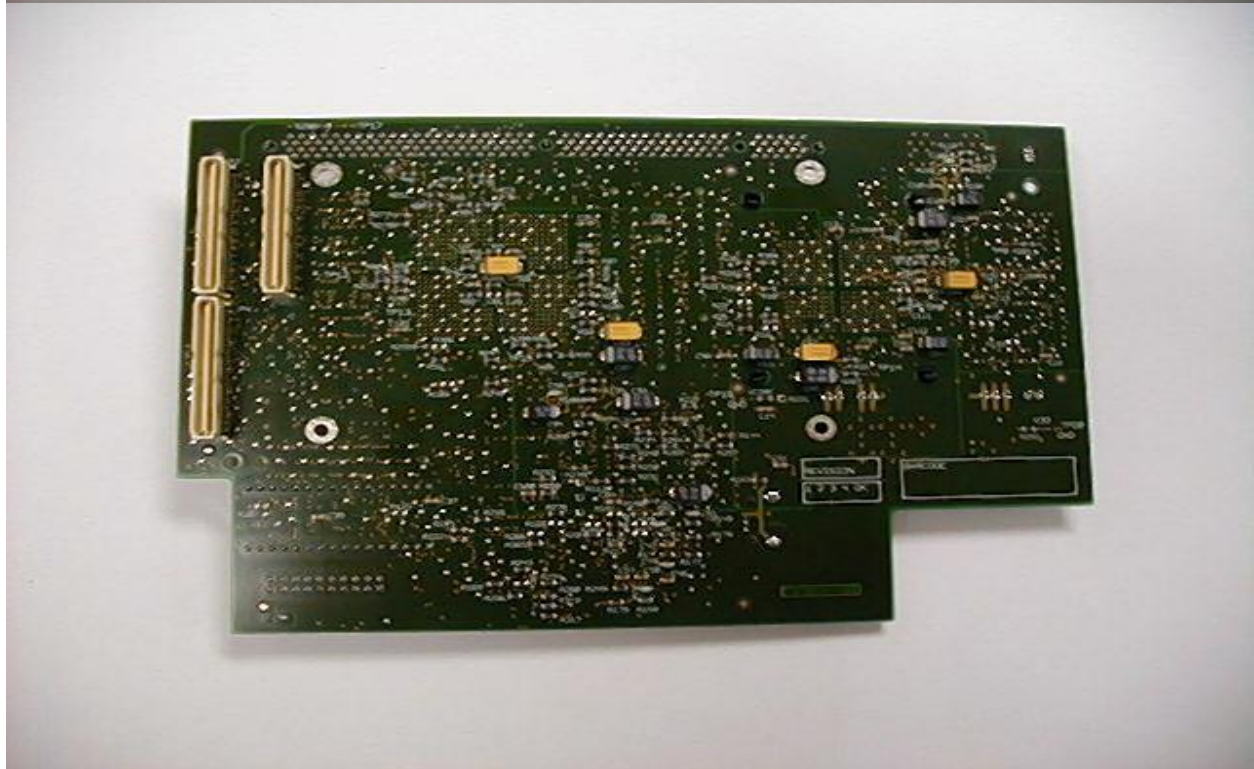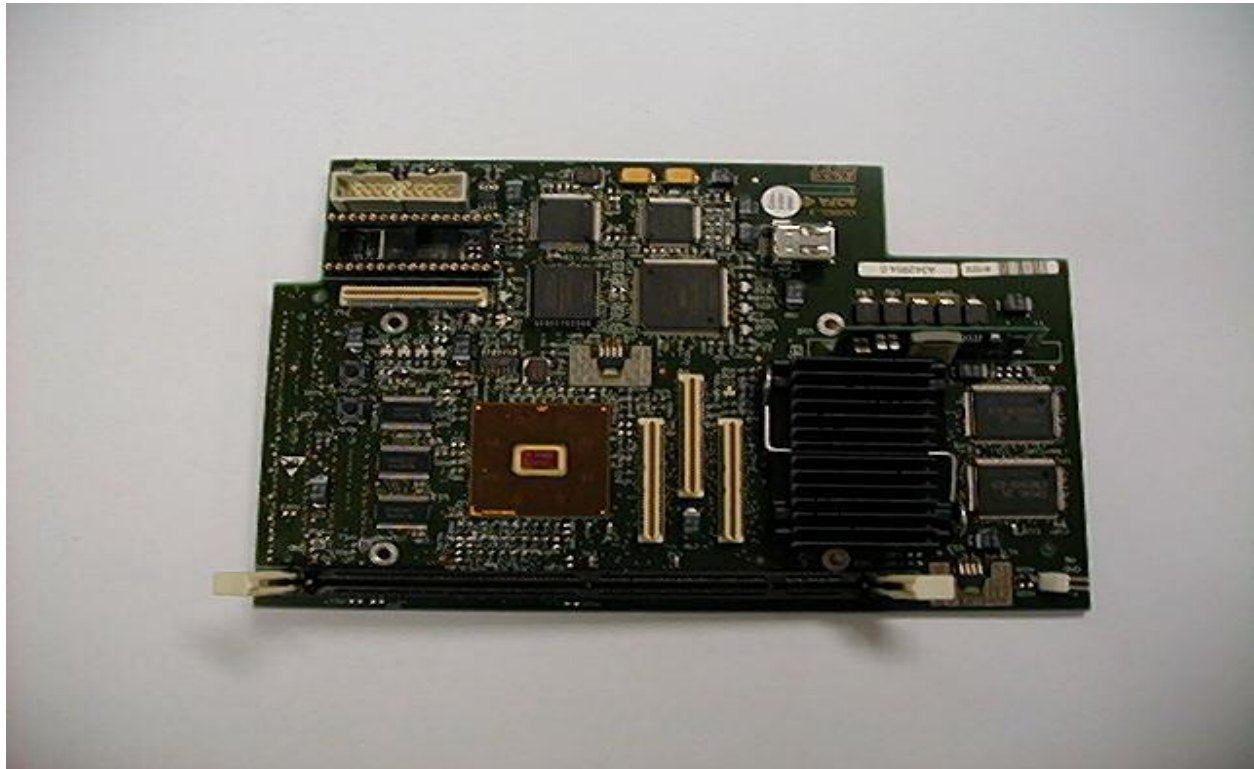


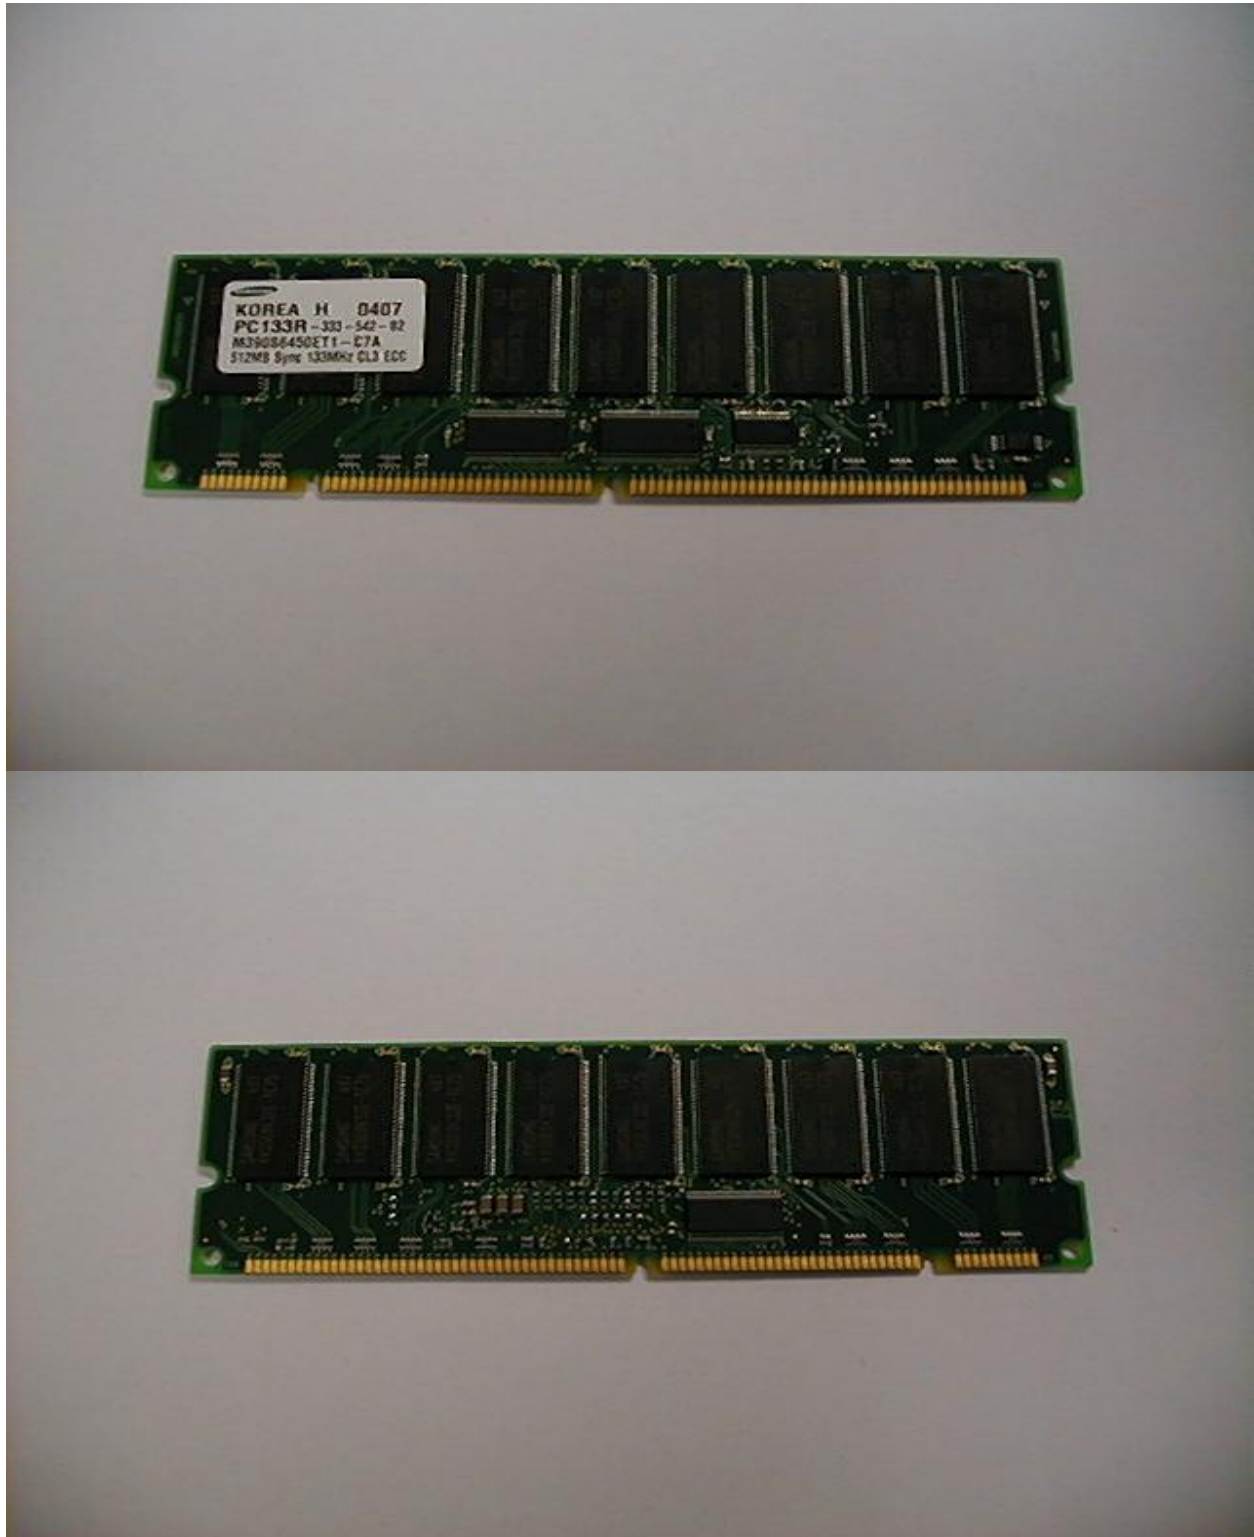

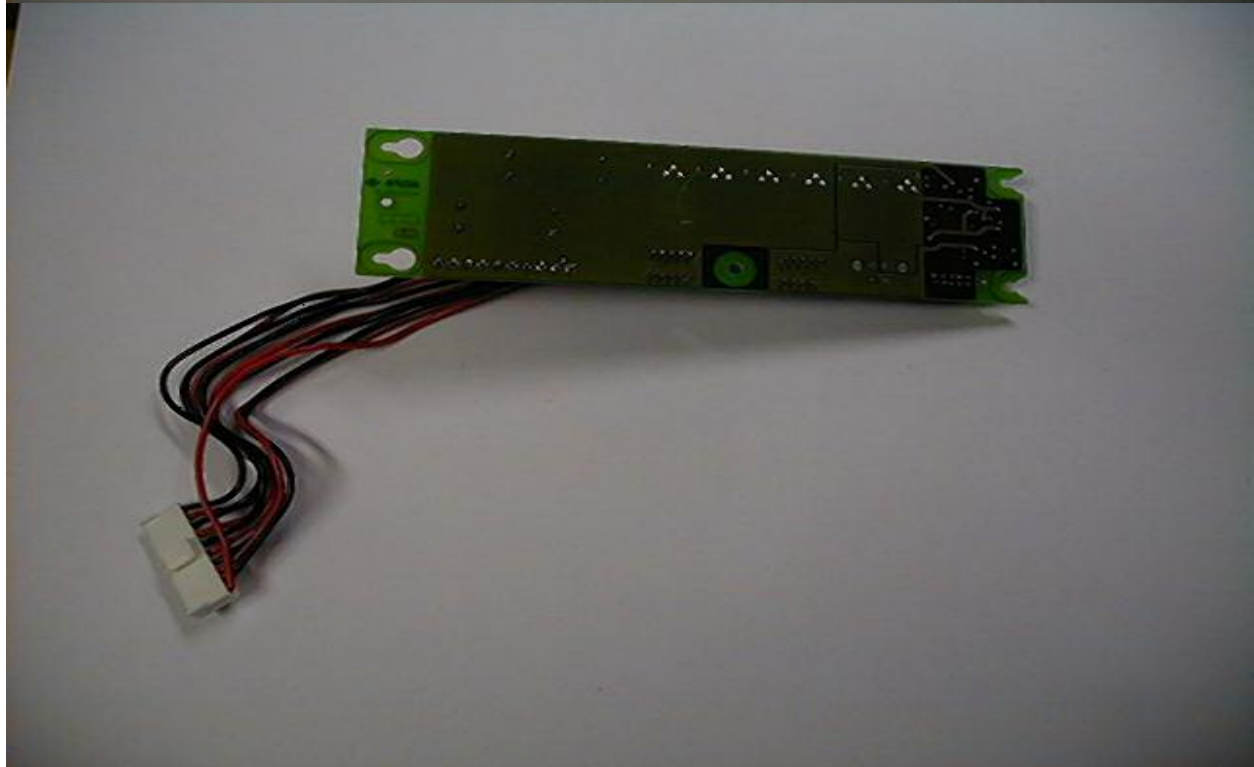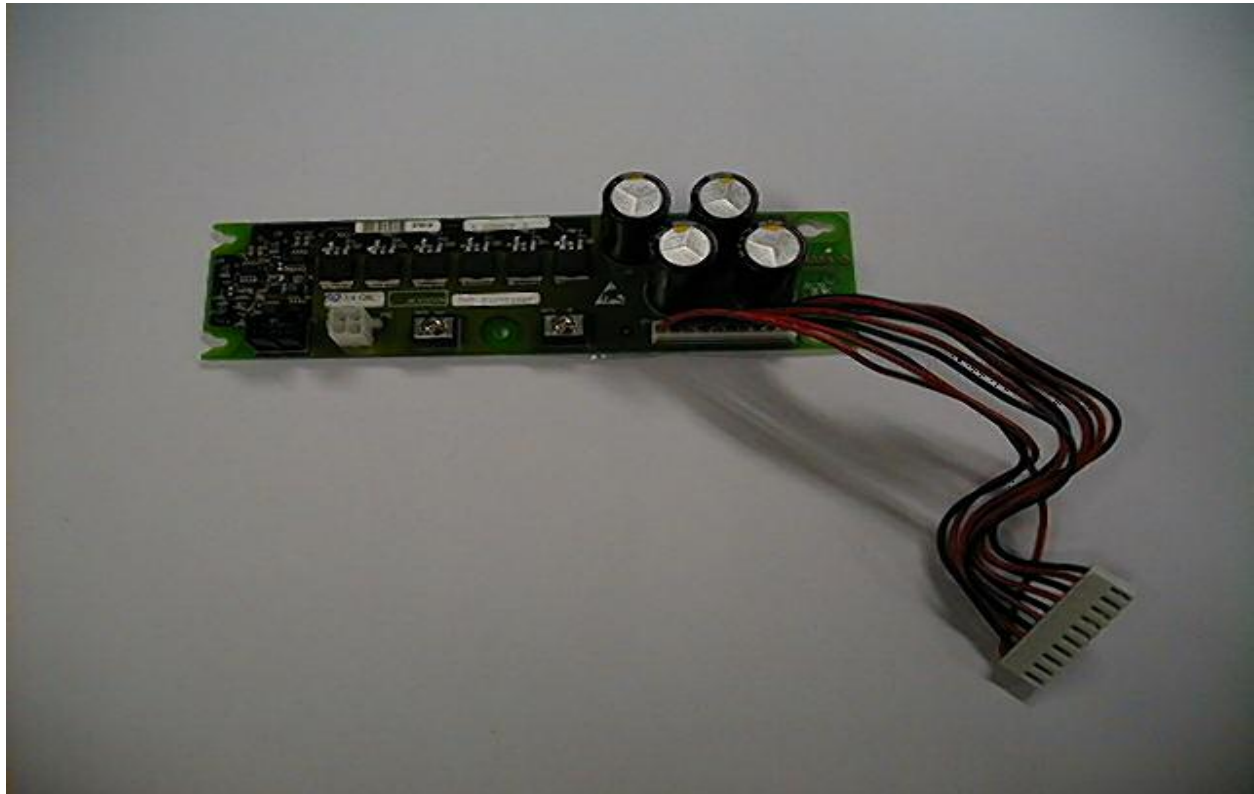



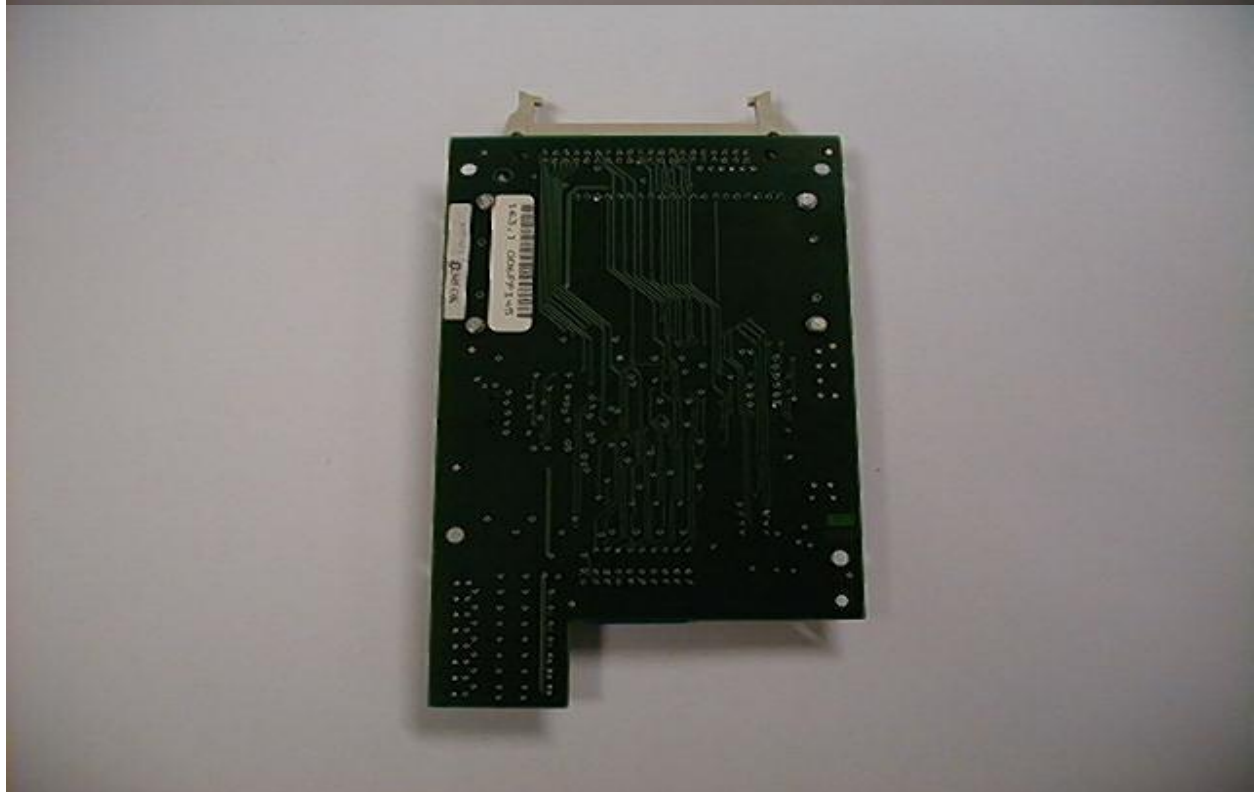




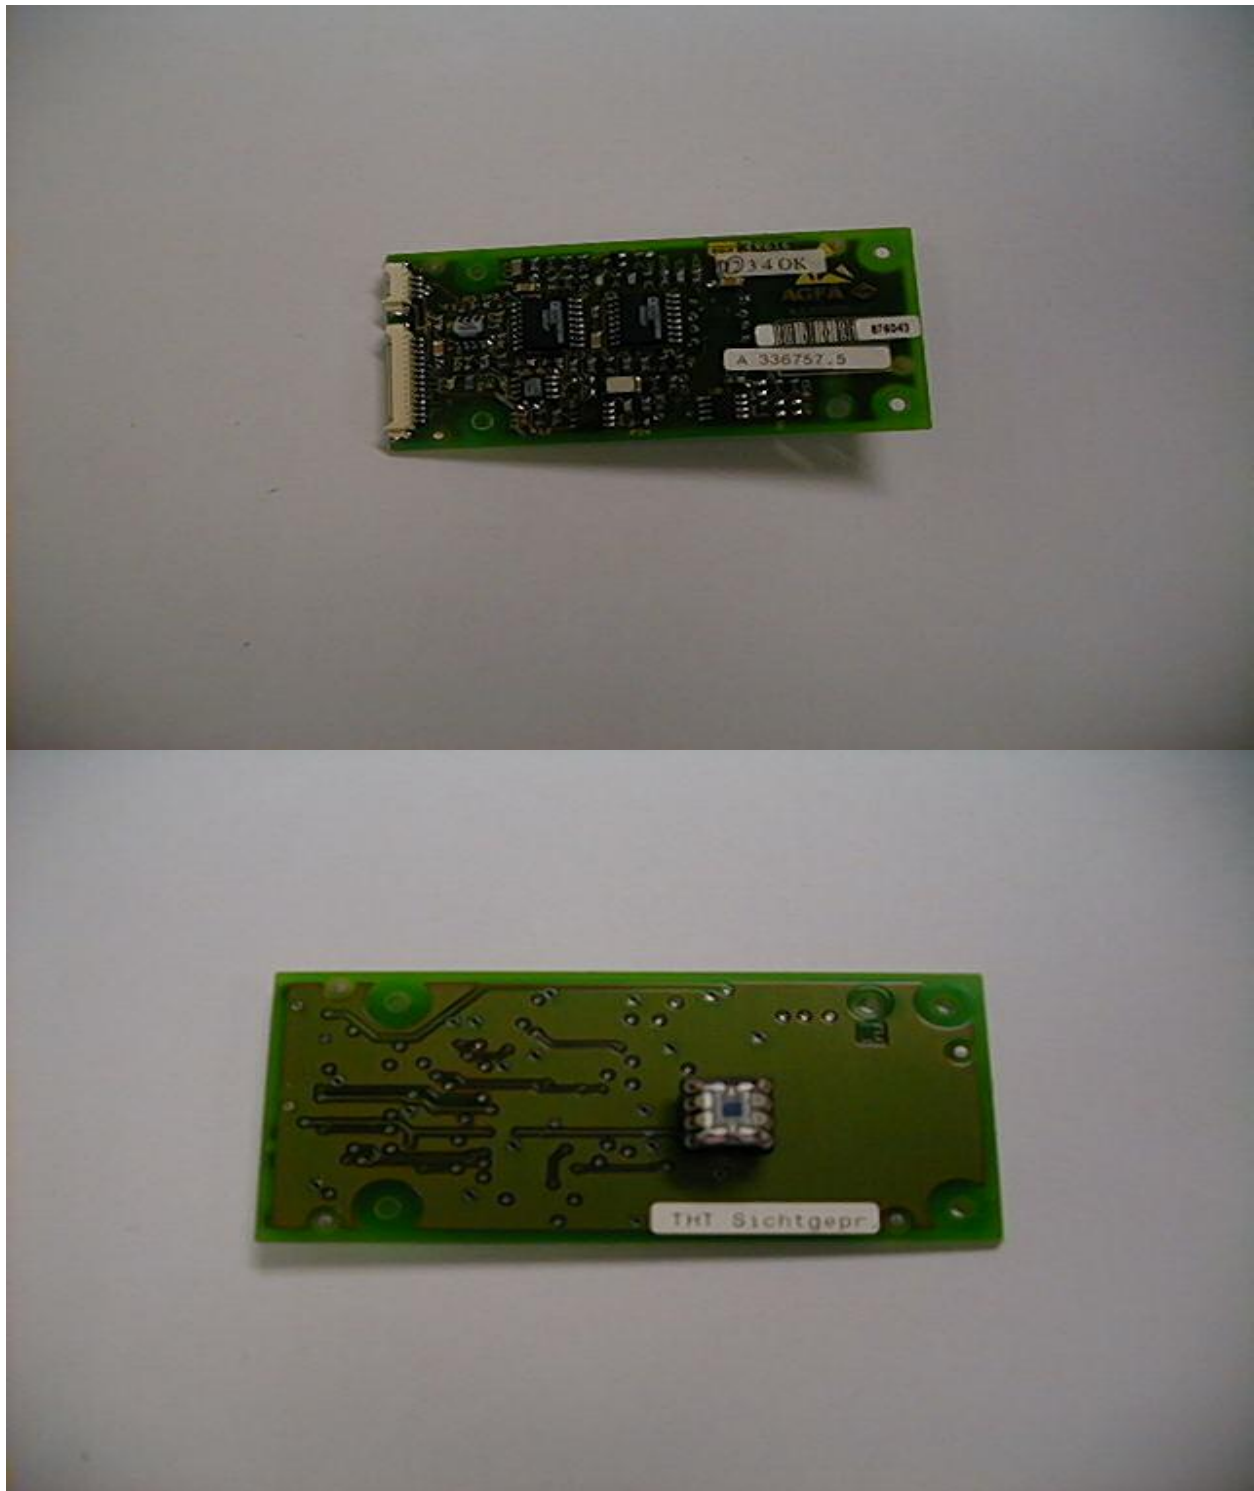



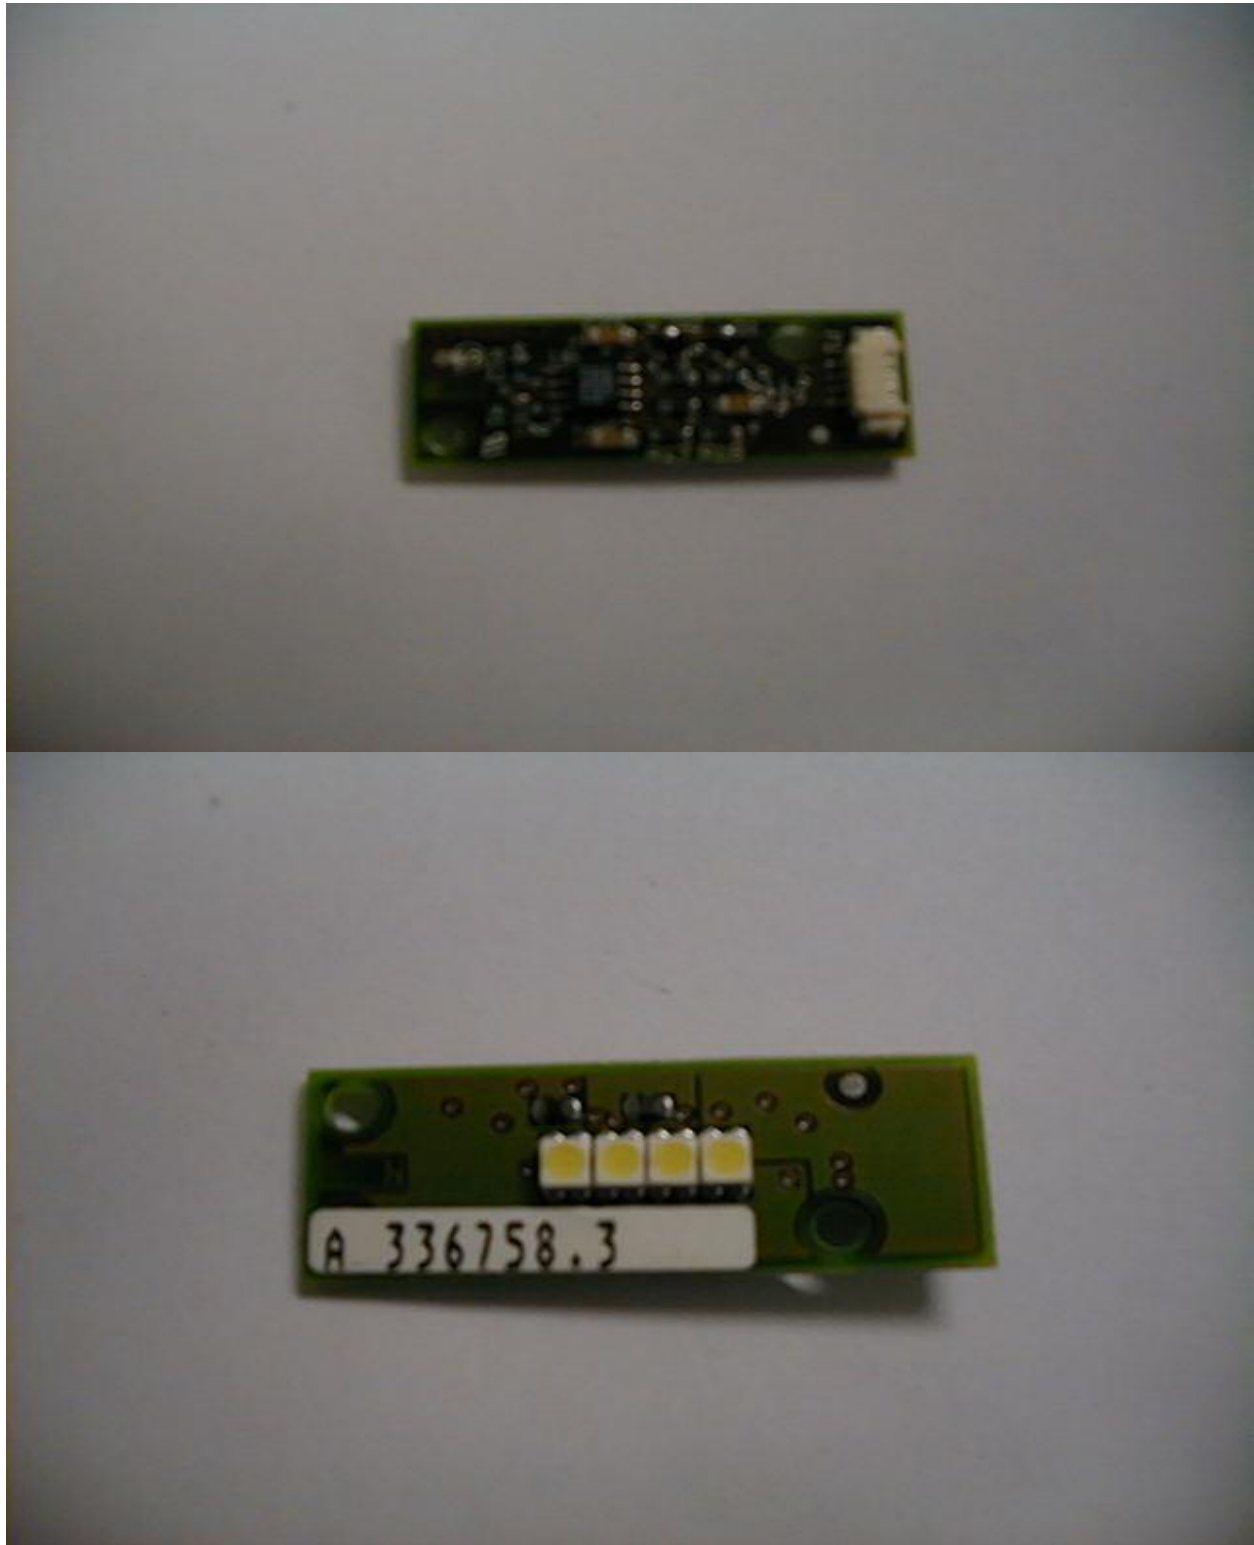

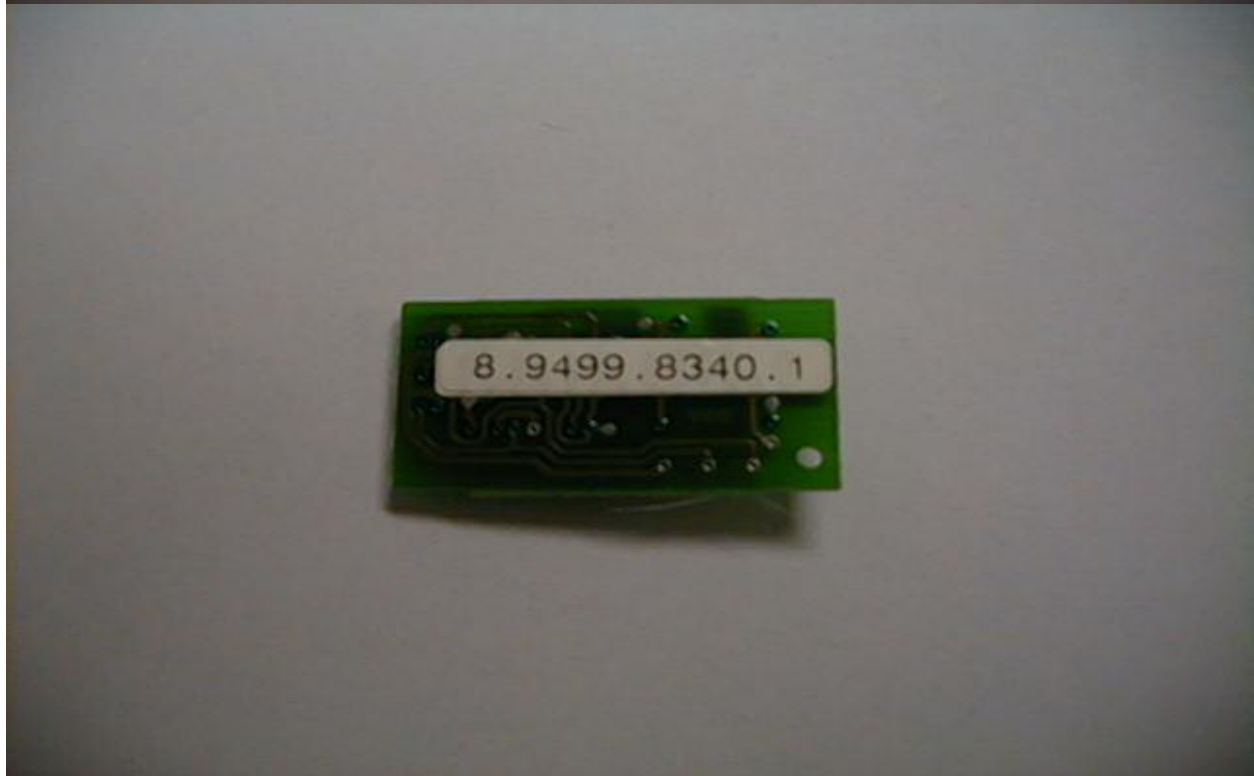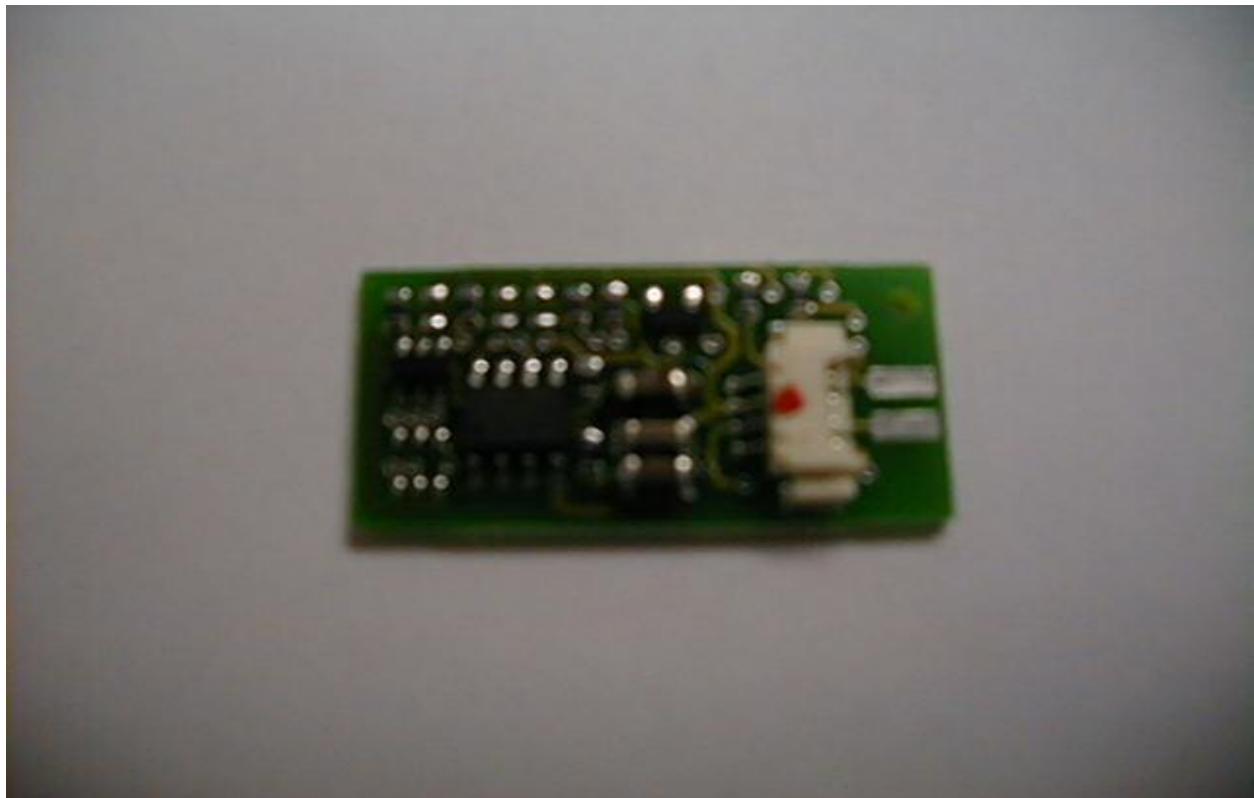





**END of Document**