



Medical Imaging *RDE*


From: [Jan Vercammen \(6233\) – MI/TSP-HW/Electronics](#)

Date: November 17, 2009

Concerning: Label position Drystar 5300 (FCC ID: HPL5365A)

Location of FCC ID label: at the **back** of the printer in the top left part is a type label.

The details of the label can be found in file **TypeLabelwithFCCID.doc**.

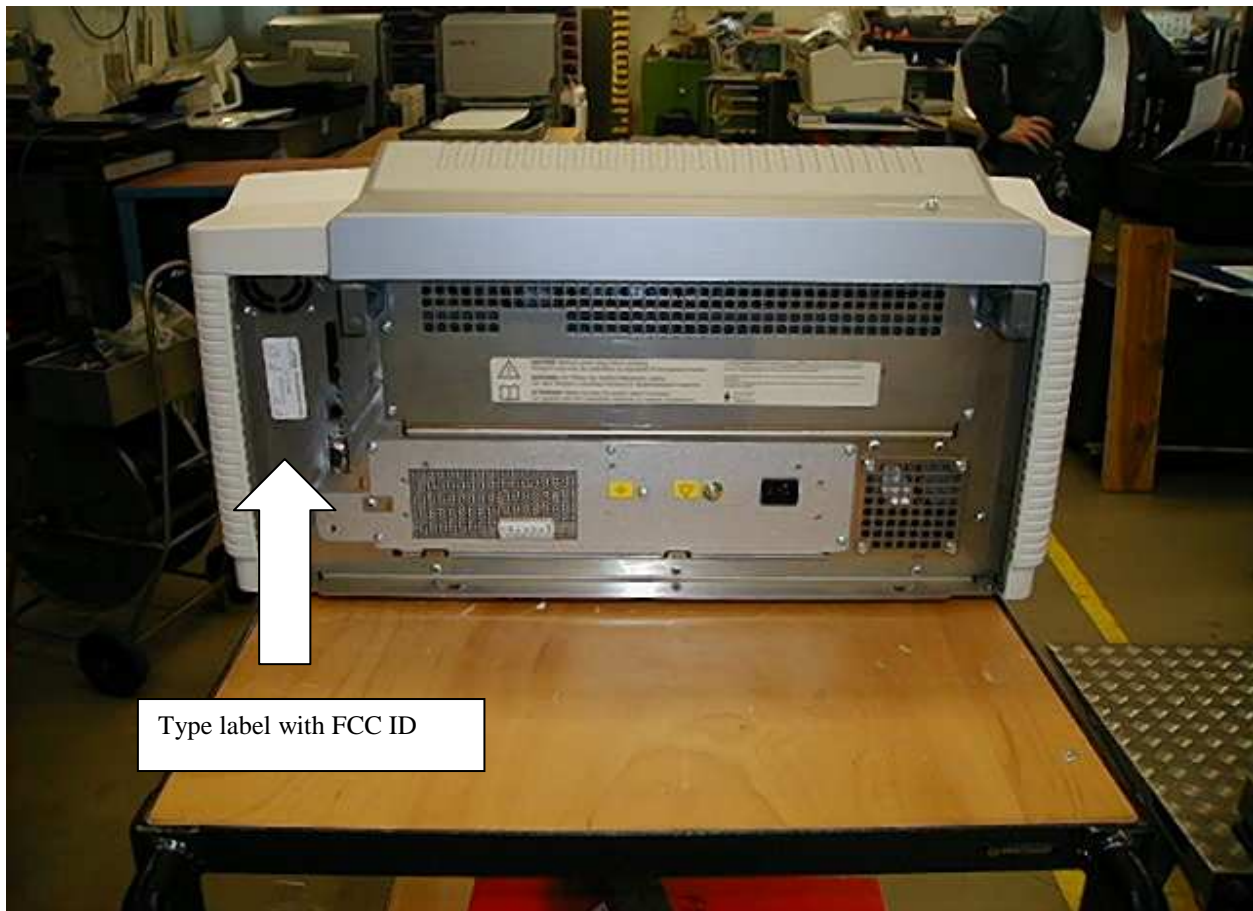

END of Document