

# Medical Imaging *RDE*

From: [Jan Vercammen \(6233\) – MI/TSP-HW/Electronics](#)

Date: August 29, 2007



## **Concerning: Foto's Drystar Axys (FCC ID: HPL5367) - PART 1**

---



Overview of photo session PART 1:

1. PART 1, page 2: DEVIL motherboard PCB
2. PART 1, page 3: THANOS PCB
3. PART 1, page 4: keypad
4. PART 1, page 5: RFID tag reader PCB
5. PART 1, page 6 & 7: front, left, back sides printer (right side similar to left side)
6. PART 2, page 2: top and bottom side of cassette
7. PART 2, page 3: electronics (Ebox) with and without shielding cover (note that this view is taken for DS5302, but both apparatus are very similar except for some minor details)
8. PART 2, page 4: left side without cover
9. PART 2, page 5 and 6: power supply unit


# Medical Imaging *RDE*

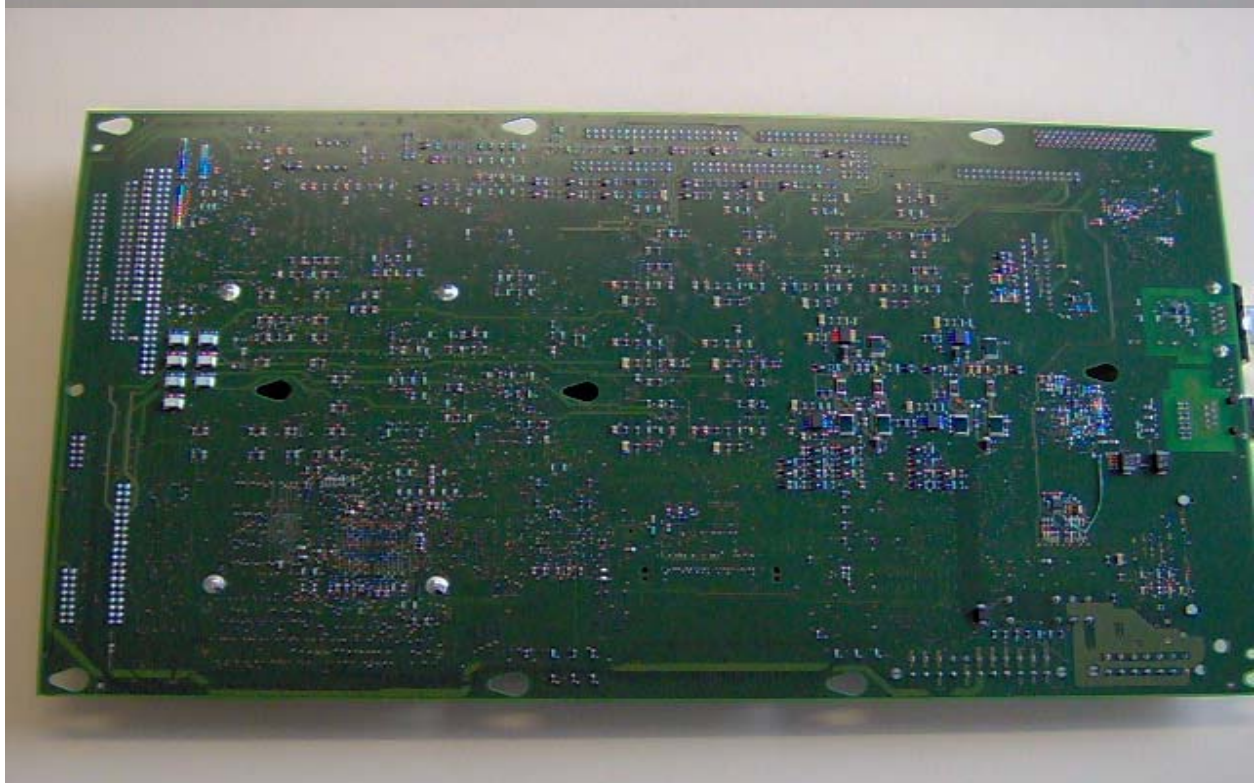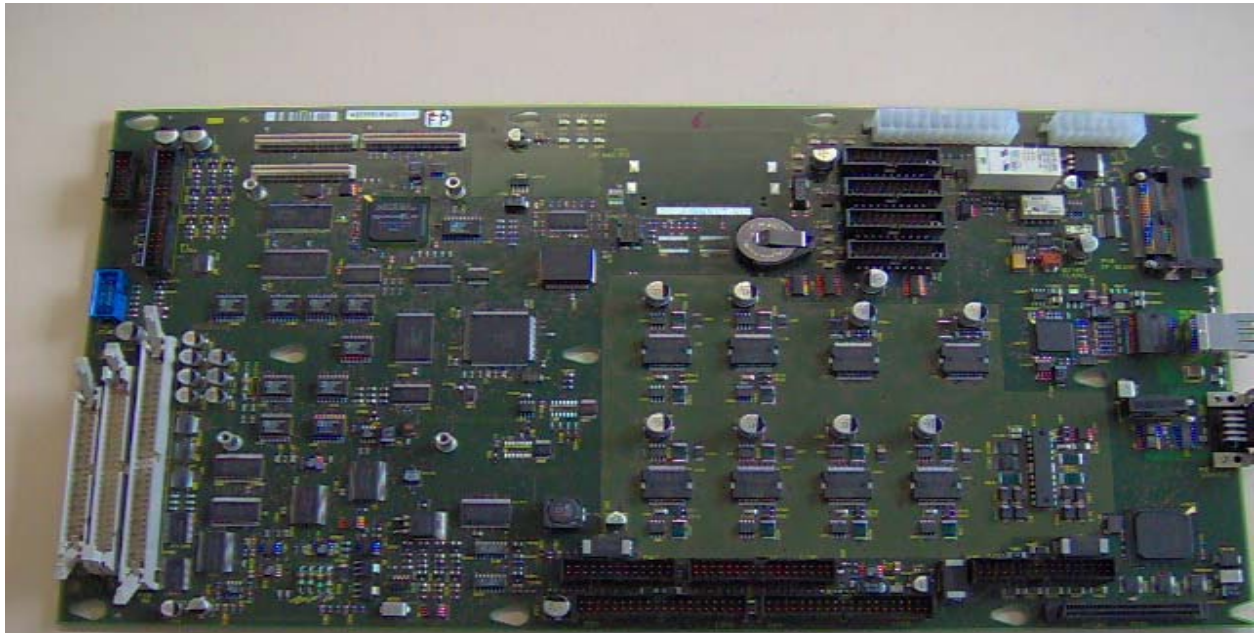

# Medical Imaging RDE

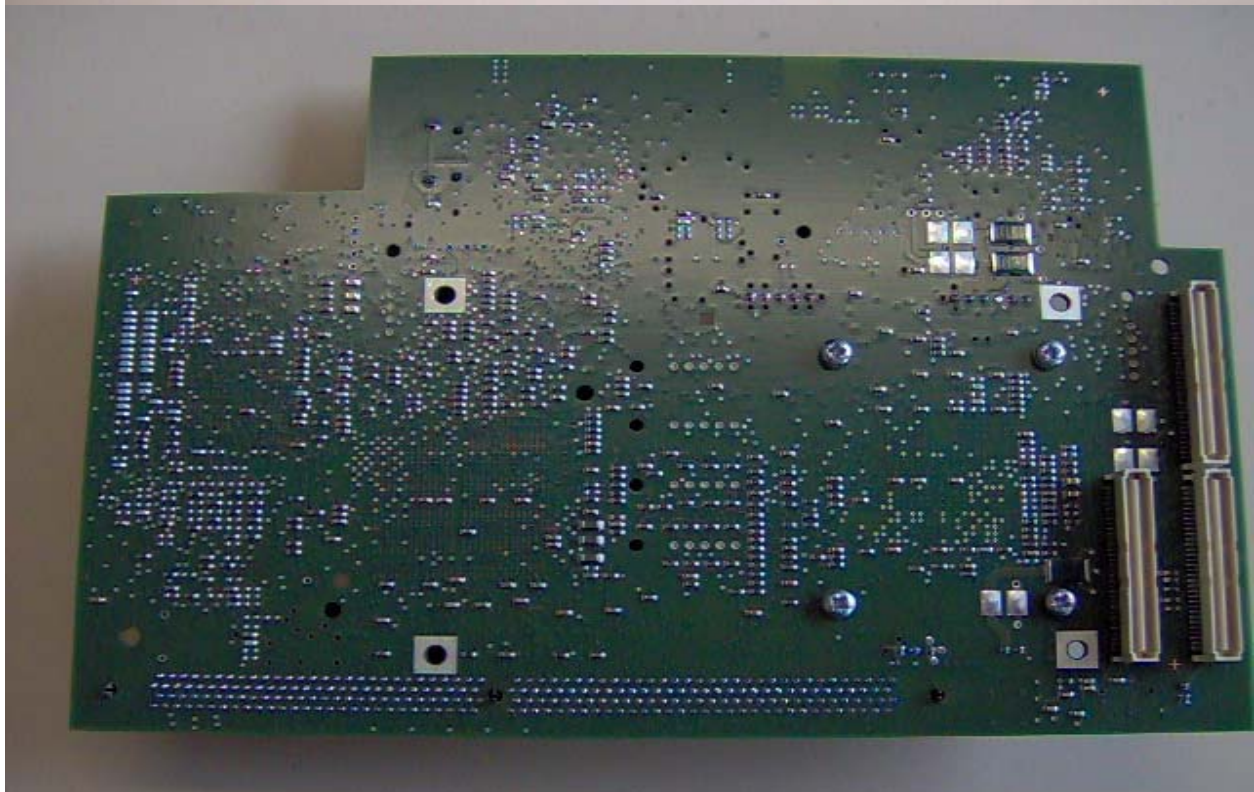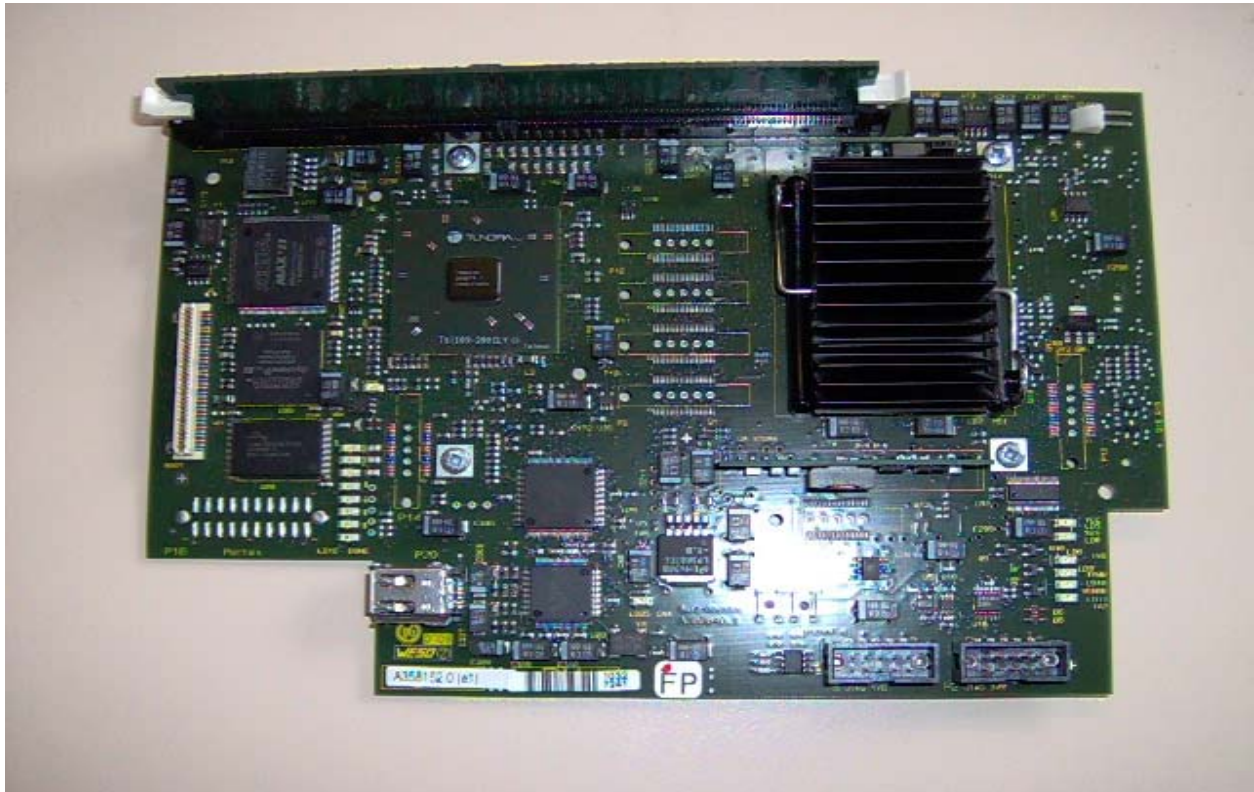

# Medical Imaging RDE

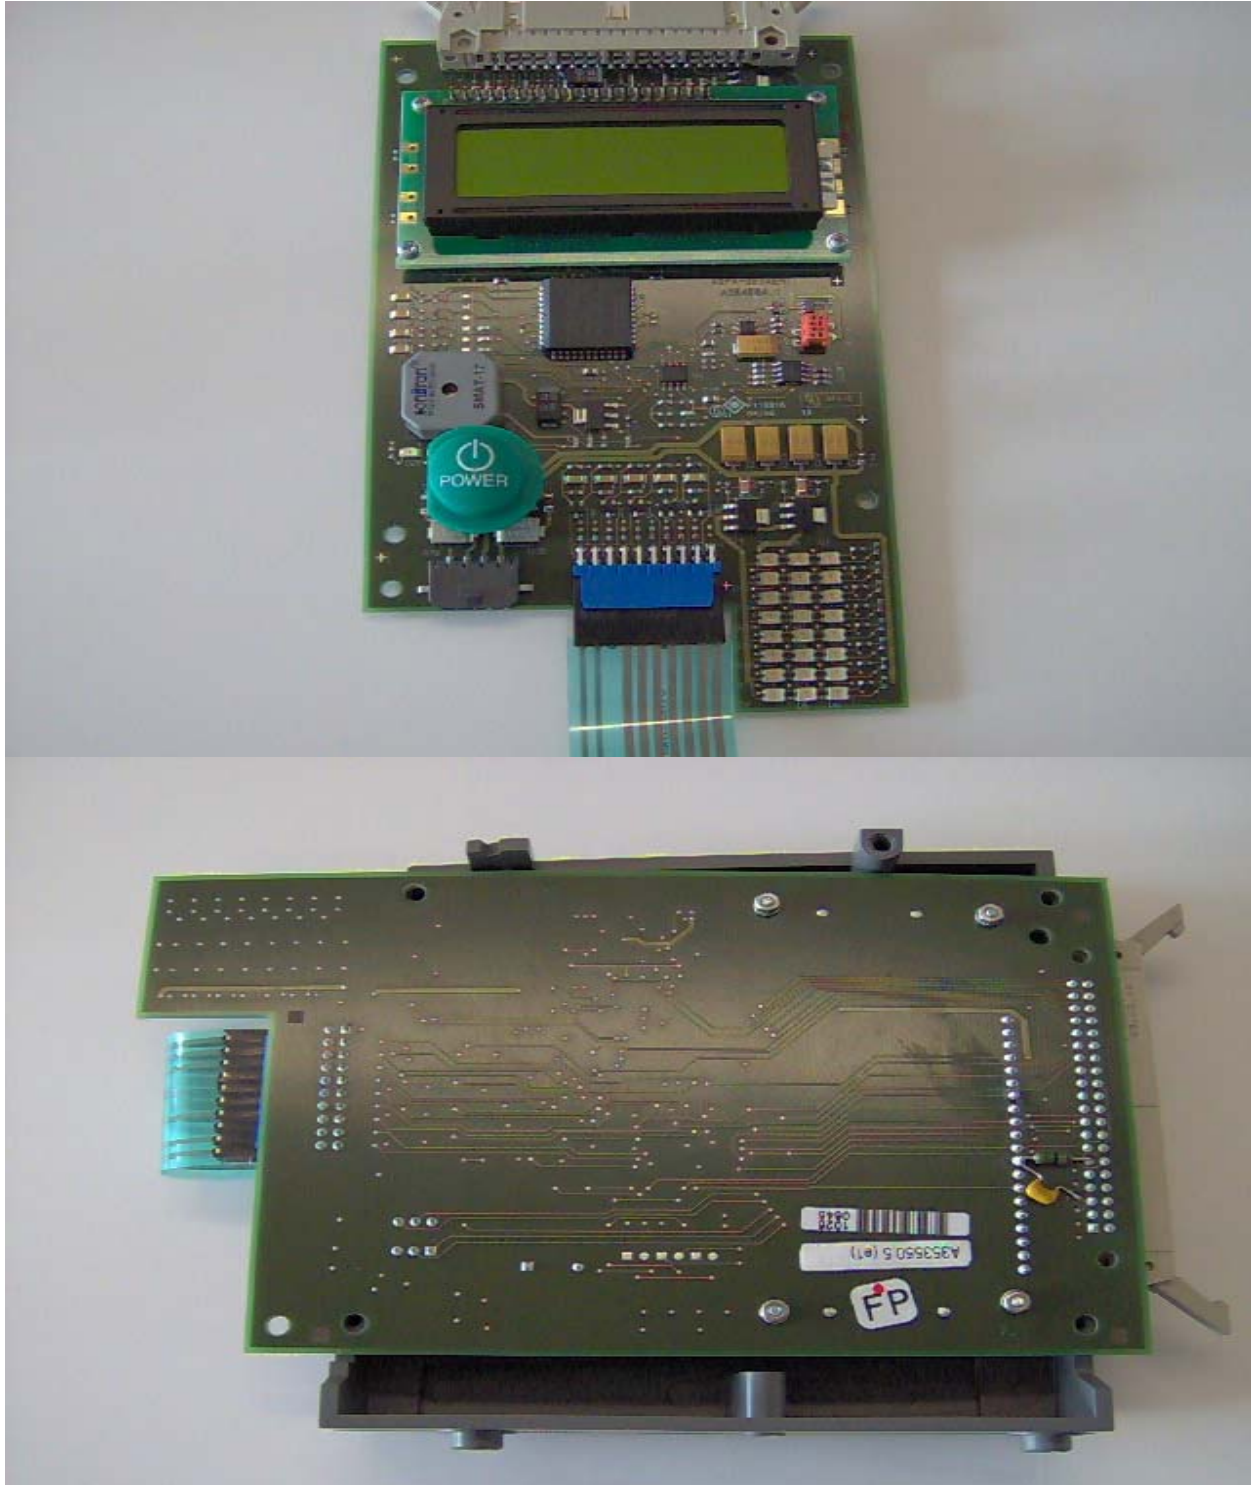

# Medical Imaging *RDE*



# Medical Imaging *RDE*



# Medical Imaging *RDE*



**END of Document – PART 1**