

Medical Imaging *RDE*


From: [Jan Vercammen \(6233\) – MI/TSP-HW/Electronics](#)

Date: September 7, 2007

Concerning: FCC ID position Drystar Axys (FCC ID: HPL5367)

Location of FCC ID label: at the **back** of the printer in the top left part is a type label.

The details of the label can be found in file TypeLabelwithFCCID.doc.

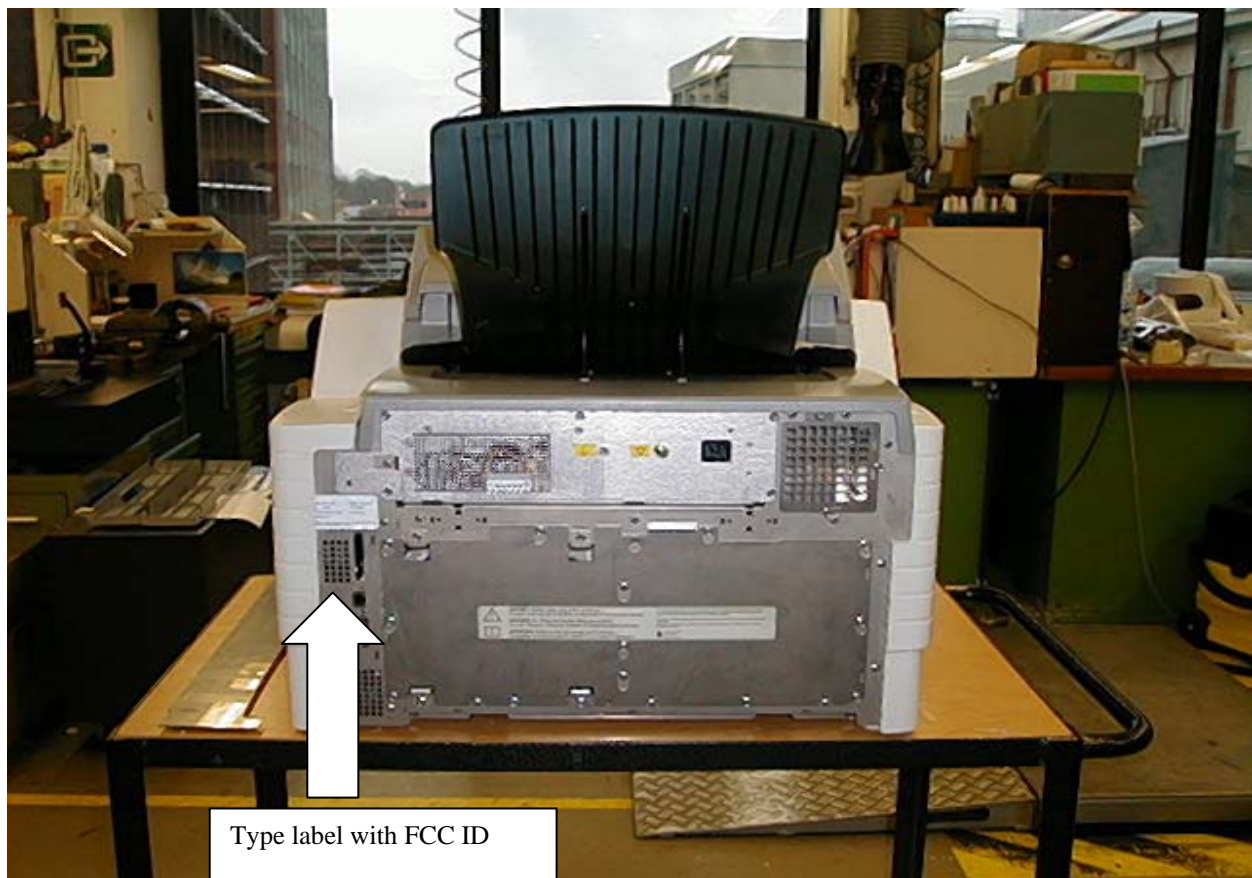

END of Document