

# Medical Imaging *RDE*

From: [Jan Vercaemmen \(6233\) – MI/TSP-HW/Electronics](#)


Date: November 16, 2009

**Concerning: FCC ID position Drystar Axys (FCC ID: HPL5367A)**

---

Location of FCC ID label: at the **back** of the printer in the top left part is a type label.

**The details of the label can be found in file TypeLabelwithFCCID.doc.**

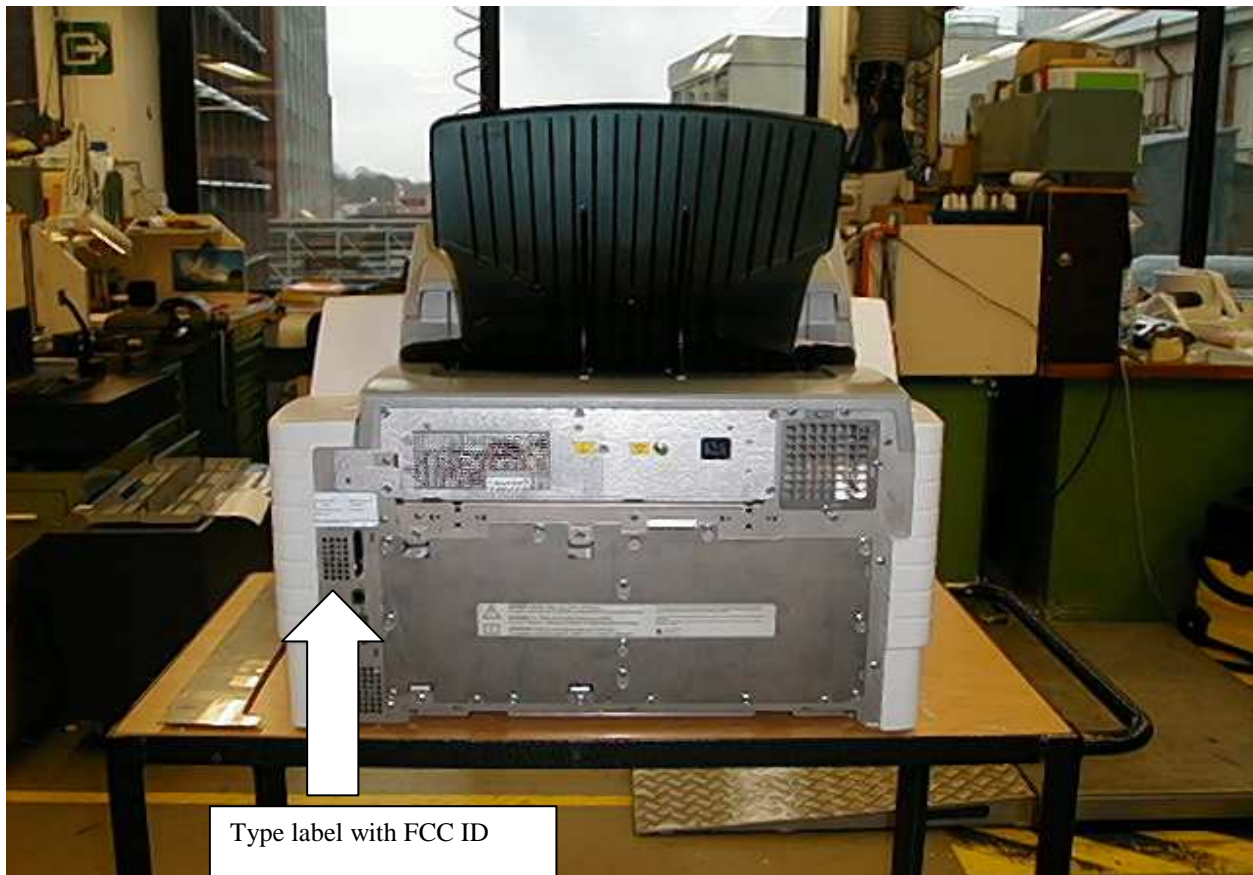

**END of Document**