



Specific Absorption Rate (SAR) Test Report

for

MICRO-STAR INT'L CO., LTD.

on the

Notebook

Report Number	: FA8N1310
Trade Name	: MSI
Model Name	: MS-N031, U120H(W/3.5G)
FCC ID	: I4L-N-F3507G
Date of Testing	: Nov. 21, 2008 ~ Nov. 28, 2008
Date of Report	: Feb. 13, 2009
Date of Review	: Feb. 13, 2009

The test results refer exclusively to the tested model/sample only.

- Without written approval of SPORTON INTERNATIONAL INC., the test report shall not be reproduced except in full.
- Report Version: Rev. 02

SPORTON INTERNATIONAL INC.

No. 52, Hwa Ya 1st Rd., Hwa Ya Technology Park, Kwei-Shan Hsiang, Tao Yuan Hsien, Taiwan, R.O.C.





Table of Contents

1.		nent of Compliance	
2.	Admir	nistration Data	
	2.1	Testing Laboratory	
	2.2	Applicant	4
	2.3	Manufacturer	4
	2.4	Application Details	4
3.	Gener	al Information	5
	3.1	Description of Device Under Test (DUT)	
	3.2	Basic Description of Accessories	
	3.3	Product Photos	
	3.4	Applied Standards	
	3.5	Device Category and SAR Limits	7
	3.6	Test Conditions	
		3.6.1 Ambient Condition	
		3.6.2 Test Configuration	
4.	Speci	fic Absorption Rate (SAR)	
	4.1	Introduction	
	4.2	SAR Definition	
5.	SAR N	Neasurement Setup	
•	5.1	DASY4 E-Field Probe System	
	•••	5.1.1 ET3DV6 E-Field Probe Specification	
		5.1.2 ET3DV6 E-Field Probe Calibration	
	5.2	DATA Acquisition Electronics (DAE)	
	5.3	Robot	
	5.4	Measurement Server	
	5.5	SAM Twin Phantom	
	5.6	Device Holder for SAM Twin Phantom	13
	5.7	Data Storage and Evaluation	14
		5.7.1 Data Storage	
		5.7.2 Data Evaluation	
	5.8	Test Equipment List	
6.	Tissu	e Simulating Liquids	
7.		tainty Assessment	
8.		Neasurement Evaluation	
0.	8.1	Purpose of System Performance check	
	8.2	System Setup	
	8.3	Validation Results	
9.		iption for DUT Testing Position	
		Irement Procedures	
10.	10.1	Spatial Peak SAR Evaluation	
	10.1	Scan Procedures	
	10.2	SAR Averaged Methods	
44		Fest Results	
11.	3AR I 11.1	Conducted Power	
	11.1	Test Records for Body SAR Test	
40		•	
		ences	29
		A - System Performance Check Data	
		B - SAR Measurement Data	
		C - Calibration Data	
Арр	pendix	D - Product Photos	

Appendix E - Test Setup Photos

Appendix F - FCC 3G SAR Measurement Procedures



1. <u>Statement of Compliance</u>

The Specific Absorption Rate (SAR) maximum results found during testing for the **MICRO-STAR INT'L CO., LTD. Notebook MSI MS-N031, U120H(W/3.5G)** are as follows (with expanded uncertainty 21.9%):

	GSM850	GSM1900	WCDMA Band V	WCDMA Band II
SAR	SAR	SAR	SAR	SAR
Position	(W/kg)	(W/kg)	(W/kg)	(W/kg)
Body	0.089	0.017	0.035	0.017

They are in compliance with Specific Absorption Rate (SAR) for general population/uncontrolled exposure limits specified in FCC 47 CFR part 2 (2.1093) and ANSI/IEEE C95.1-1999 and had been tested in accordance with the measurement methods and procedures specified in OET Bulletin 65 Supplement C (Edition 01-01).

Approved by

1 Wu Roy Wu

Manager



2. Administration Data

2.1 Testing Laboratory

Company Name :	Sporton International Inc.
Address :	No.52, Hwa-Ya 1 st RD., Hwa Ya Technology Park, Kwei-Shan Hsiang,
	TaoYuan Hsien, Taiwan, R.O.C.
Test Site :	SAR01-HY
Telephone Number :	886-3-327-3456
Fax Number :	886-3-328-4978

2.2 Applicant

Company Name :	MICRO-STAR INT'L CO., LTD.
Address :	No. 69, Lide St, Jhonghe City, Taipei County 235, Taiwan

2.3 Manufacturer

Company Name :	MICRO-STAR INT'L CO., LTD.
Address :	No. 69, Lide St, Jhonghe City, Taipei County 235, Taiwan

2.4 Application Details

Date of reception of application:	Nov. 13, 2008
Start of test :	Nov. 21, 2008
End of test :	Nov. 28, 2008



3. General Information

3.1 Description of Device Under Test (DUT)

Product Feature & Specification			
DUT Type :	JT Type : Notebook		
Trade Name :	MSI		
Model Name :	MS-N031, U120H(W/3.5G)		
FCC ID :	I4L-N-F3507G		
WWAN Module :	Sony Ericsson, F3507g		
Tx Frequency :	GSM 850 : 824 MHz ~ 849 MHz GSM 1900 : 1850 MHz ~ 1910 MHz WCDMA Band V : 824 MHz ~ 849 MHz WCDMA Band II : 1850 MHz ~ 1910 MHz		
Rx Frequency :	GSM 850 : 869 MHz ~ 894 MHz GSM 1900 : 1930 MHz ~ 1990 MHz WCDMA Band V : 869 MHz ~ 894 MHz WCDMA Band II : 1930 MHz ~ 1990 MHz		
Maximum Output Power to Antenna :	GSM 850 : 31.78 dBm GSM 1900 : 29.27 dBm WCDMA Band V : 22.53 dBm WCDMA Band II : 22.90 dBm		
Antenna Type : Fixed Internal			
HW Version :	1.3		
SW Version :	10B		
Type of Modulation :	GSM / GPRS : GMSK EDGE : 8PSK WCDMA : QPSK HSDPA : QPSK / 16QAM HSUPA : BPSK		
DUT Stage :	Identical Prototype		

Note: The DUT can not be used for simultaneous operation of WLAN and WWAN transmitters.



3.2 Basic Description of Accessories

	Brand Name	LI SHIN			
AC Adapter 1	Model Name	0225A2040			
	Power Rating	I/P:100-240Vac, 1.7A;			
	i ower Katilig	O/P: 20Vdc, 2A			
	AC Power Cord Type	1.82 meter non-shielded cable without ferrite core			
	Brand Name	DELTA			
	Model Name	ADP-40MH BDB			
AC Adapter 2	Power Rating	I/P:100-240Vac, 1.2A;			
		O/P: 20Vdc, 2A			
	AC Power Cord Type	1.9 meter shielded cable with ferrite core			
	Brand Name	MITAC			
Battery 1	Model Name	BTY-S12			
J	Power Rating	3.7Vdc, 2200mAh			
	Туре	6cells, Li-ion			
	Brand Name	STL			
Battery 2	Model Name	BTY-S12			
y _	Power Rating	3.7Vdc, 2600mAh			
	Туре	6cells, Li-ion			
	Brand Name	MITAC			
Battery 3	Model Name	BTY-S11			
Duttery	Power Rating	3.7Vdc, 2200mAh			
	Туре	3cells, Li-ion			
	Brand Name	STL			
Battery 4	Model Name	BTY-S11			
Dattery 4	Power Rating	3.7Vdc, 2200mAh			
	Туре	3cells, Li-ion			
	Brand Name	WellTop			
Battery 5	Model Name	BTY-S11			
Datter y 5	Power Rating	3.7Vdc, 2200mAh			
	Туре	3cells, Li-ion			
LCD Panel 1	Brand Name	Hannstar			
	Model Name	HSD100IFW1			
LCD Panel 2	Brand Name	СРТ			
	Model Name	CLAA102NA0ACW			
Camera 1	Brand Name	Bison			
	Model Name	BN29VDG8-000			
Camera 2	Brand Name	CHICONY			
	Model Name	CNF723121004442L			

Remark: Above EUT's information was declared by manufacturer. Please refer to the specifications of manufacturer or User's Manual for more detailed features description.

Test Report No : FA8N1310



3.3 Product Photos

Refer to Appendix D.

3.4 <u>Applied Standards</u>

The Specific Absorption Rate (SAR) testing specification, method and procedure for this Notebook is in accordance with the following standards:

47 CFR Part 2(2.1093) IEEE C95.1-1999 IEEE P1528-2003 OET Bulletin 65 Supplement C (Edition 01-01) Preliminary Guidance for Reviewing Applications for Certification of 3G Device. May 2006. KDB 941225 D01 v02

3.5 Device Category and SAR Limits

This device belongs to portable device category because its radiating structure is allowed to be used within 20 centimeters of the body of the user. Limit for General Population/Uncontrolled exposure should be applied for this device, it is 1.6 W/kg as averaged over any 1 gram of tissue.

3.6 Test Conditions

3.6.1 Ambient Condition

interent contanton			
Ambient Temperature	20-24		
Humidity	<60 %		

3.6.2 Test Configuration

The device was controlled by using a base station emulator Agilent E5515C. Communication between the device and the emulator was established by air link. The distance between the DUT and the antenna of the emulator is larger than 50 cm and the output power radiated from the emulator antenna is at least 30 dB smaller than the output power of DUT. The DUT was set from the emulator to radiate maximum output power during all tests.

Measurements were performed on the lowest, middle, and highest channel for each testing position. However, measurements were performed only on the middle channel if the SAR is below 3 dB of limit.

For SAR testing, EUT is in GPRS or WCDMA/HSPA link mode. In GPRS link mode, its crest factor is 4, because EUT is GPRS multi-slot class 10 device with 2 uplink slots. In WCDMA/HSPA link mode, its crest factor is 1.

The separation distance between WWAN and Bluetooth antenna is over 20 cm, so there is no simultaneous transmission SAR test requirement between WWAN and Bluetooth.



4. Specific Absorption Rate (SAR)

4.1 Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

4.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density.

). The equation description is as below:

$$\mathbf{SAR} = \frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$\mathbf{SAR} = C \, \frac{\delta T}{\delta t}$$

, where C is the specific head capacity, δT is the temperature rise and δt the exposure duration,

or related to the electrical field in the tissue by

$$\mathbf{SAR} = \frac{\sigma \left| E \right|^2}{\rho}$$

, where is the conductivity of the tissue, is the mass density of the tissue and E is the rms electrical field strength.

However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.



5. SAR Measurement Setup

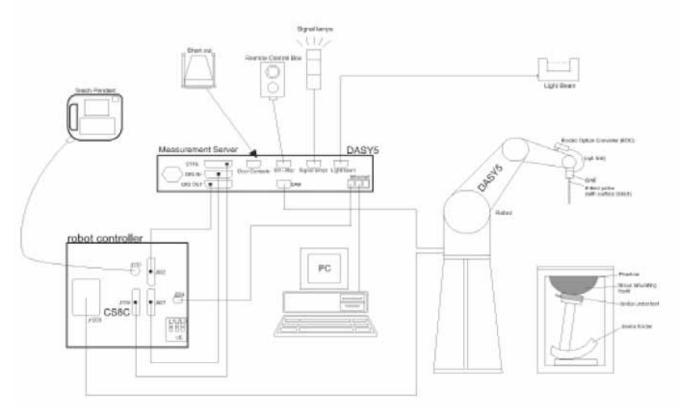


Fig. 5.1 DASY5 System

The DASY5 system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- A standard high precision 6-axis robot with controller, a teach pendant and software
- A data acquisition electronic (DAE) attached to the robot arm extension
- A dosimetric probe equipped with an optical surface detector system
- The electro-optical converter (ECO) performs the conversion between optical and electrical signals
- ➤ A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- A probe alignment unit which improves the accuracy of the probe positioning
- A computer operating Windows XP
- DASY5 software
- Remove control with teach pendant and additional circuitry for robot safety such as warming lamps, etc.
- The SAM twin phantom
- ➢ A device holder
- Tissue simulating liquid
- > Dipole for evaluating the proper functioning of the system

Some of the components are described in details in the following sub-sections.



5.1 DASY4 E-Field Probe System

The SAR measurement is conducted with the dosimetric probe ET3DV6 (manufactured by SPEAG). The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency. This probe has a built in optical surface detection system to prevent from collision with phantom.

5.1.1 ET3DV6 E-Field Probe Specification <FT3DV6>

<e13dv6></e13dv6>		
Construction	Symmetrical design with triangular core	
	Built-in optical fiber for surface detection system	
	Built-in shielding against static charges	
	PEEK enclosure material (resistant to organic solvents)	Contraction of the second s
Frequency	10 MHz to 3 GHz	
Directivity	\pm 0.2 dB in brain tissue (rotation around probe axis)	
-	\pm 0.4 dB in brain tissue (rotation perpendicular to	
	probe axis)	
Dynamic Range	5 µ W/g to 100mW/g; Linearity: ±0.2dB	
Surface Detection	± 0.2 mm repeatability in air and clear liquids on	
	reflecting surface	
Dimensions	Overall length: 330mm	States and States and I
	Tip length: 16mm	
	Body diameter: 12mm	
	Tip diameter: 6.8mm	
	Distance from probe tip to dipole centers: 2.7mm	
Application	General dosimetry up to 3GHz	
	Compliance tests for mobile phones and Wireless LAN	LILLS VIII CONTRACTOR
	Fast automatic scanning in arbitrary phantoms	
		Fig. 5.2 Probe Setup on Robot

5.1.2 ET3DV6 E-Field Probe Calibration

Each probe needs to be calibrated according to a dosimetric assessment procedure with accuracy better than \pm 10%. The spherical isotropy shall be evaluated and within \pm 0.25dB. The sensitivity parameters (NormX, NormY, and NormZ), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested. The calibration data are as below:

> ET3DV6 sn1788

Sensitivity	X axis : 1.73 μV		Y axis : 1.59 μV		Z axis : 1.72 μV	
Diode compression point	X axis : 95 mV		Y az	xis : 98 mV	Z axis : 91 mV	
Conversion factor (Body)	Frequency (MHz)	X axis		Y axis	Z axis	
	800~1000	6.34		6.34	6.34	
	1850~2050	4.73		4.73	4.73	
Boundary effect	Frequency (MHz)	Alp	oha	Depth		
(Body)	800~1000	0.50		2.48		
	1850~2050	0.7	74	1.99		

NOTE: The probe parameters have been calibrated by the SPEAG.



5.2 DATA Acquisition Electronics (DAE)

The data acquisition electronics (DAE4) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The mechanical probe mounting device includes two different sensor systems for frontal and sideways probe contacts. They are used for mechanical surface detection and probe collision detection.

The input impedance of the DAE4 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.

5.3 <u>Robot</u>

The DASY5 system uses the high precision robots TX90 XL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASY5 system, the CS8C robot controller version from Stäubli is used. The XL robot series have many features that are important for our application:

- High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- ➢ 6-axis controller

5.4 <u>Measurement Server</u>

The DASY5 measurement server is based on a PC/104 CPU board with 400 MHz CPU 128 MB chipdisk and 128 MB RAM.

Communication with the DAE4 electronic box the 16-bit AD-converter system for optical detection and digital I/O interface.

The measurement server performs all the real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operations.



5.5 <u>SAM Twin Phantom</u>

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- ➢ Left head
- Right head
- ➢ Flat phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

The phantom can be used with the following tissue simulating liquids:

- *Water-sugar based liquid
- *Glycol based liquids

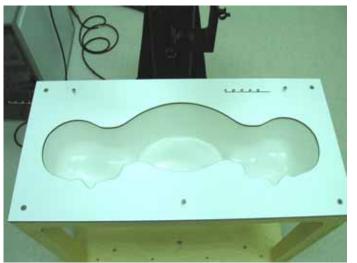


Fig. 5.3 Top View of Twin Phantom



Fig. 5.4 Bottom View of Twin Phantom



5.6 Device Holder for SAM Twin Phantom

The SAR in the Phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source in 5 mm distance, a positioning uncertainty of ± 0.5 mm would produce a SAR uncertainty of $\pm 20\%$. An accurate device position is therefore crucial for accurate and repeatable measurement. The position in which the devices must be measured, are defined by the standards.

The DASY5 device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation centers for both scales is the ear reference point (EPR).

Thus the device needs no repositioning when changing the angles.

The DASY5 device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity $_{\rm r}$ =3 and loss tangent δ = 0.02. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



Fig. 5.5 Device Holder



5.7 Data Storage and Evaluation

5.7.1 Data Storage

The DASY5 software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files with the extension .DA4. The post-processing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verification of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type (e.g., [V/m], [A/m], [mW/g]). Some of these units are not available in certain situations or give meaningless results, e.g., a SAR-output in a non-less media, will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

5.7.2 Data Evaluation

The DASY4 post-processing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software :

Probe parameters :	- Sensitivity	Norm _{<i>i</i>} , a_{i0} , a_{i1} , a_{i2}
	- Conversion factor	ConvF _i
	- Diode compression point	dcpi
Device parameters :	- Frequency	f
	- Crest factor	cf
Media parameters :	- Conductivity	
	- Density	

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY5 components. In the direct measuring mode of the multi-meter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power.



The formula for each channel can be given as :

$$Vi = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

with V_i = compensated signal of channel i (i = x, y, z) U_i = input signal of channel i (i = x, y, z) cf = crest factor of exciting field (DASY parameter) dcp_i = diode compression point (DASY parameter)

From the compensated input signals, the primary field data for each channel can be evaluated :

E-field probes : $E_i = \sqrt{\frac{V_i}{Norm_i ConvF}}$ **H-field probes** : $H_i = \sqrt{V_i} \frac{a_{i0+}a_{i1}f + a_{i2}f^2}{f}$ with V_i = compensated signal of channel *i* (*i* = x, y, z) *Norm*_i = sensor sensitivity of channel i (i = x, y, z) $\mu V/(V/m)^2$ for E-field Probes *ConvF* = sensitivity enhancement in solution a_{ii} = sensor sensitivity factors for H-field probes f = carrier frequency [GHz] E_i = electric field strength of channel *i* in V/m H_i = magnetic field strength of channel *i* in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$SAR = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

with

SAR = local specific absorption rate in mW/g*Etot* = total field strength in V/m= conductivity in [mho/m] or [Siemens/m] = equivalent tissue density in g/cm^3

* Note that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.

The power flow density is calculated assuming the excitation field to be a free space field.

$$P_{pwe} = \frac{E_{tot}^2}{3770}$$
 or $P_{pwe} = H_{tot}^2 \cdot 37.7$

 P_{pwe} = equivalent power density of a plane wave in mW/cm² with E_{tot} = total electric field strength in V/m H_{tot} = total magnetic field strength in A/m





5.8 <u>Test Equipment List</u>

Manufacturer	Name of Equipment	Type/Model	Serial Number	Calibration		
Manufacturer	Name of Equipment	Type/Iviodei	Serial Number	Last Cal.	Due Date	
SPEAG	Dosimetric E-Filed Probe	ET3DV6	1788	Sep. 23, 2008	Sep. 22, 2009	
SPEAG	835MHz System Validation Kit	D835V2	499	Mar. 17, 2008	Mar. 16, 2010	
SPEAG	1900MHz System Validation Kit	D1900V2	5d041	Mar. 28, 2008	Mar. 27, 2010	
SPEAG	Data Acquisition Electronics	DAE4	778	Sep. 22, 2008	Sep. 21, 2009	
SPEAG	Device Holder	N/A	N/A	NCR	NCR	
SPEAG	SAM Phantom	QD 000 P40 C	TP-1303	NCR	NCR	
SPEAG	SAM Phantom	QD 000 P40 C	TP-1446	NCR	NCR	
SPEAG	SAM Phantom	QD 000 P40 C	TP-1383	NCR	NCR	
SPEAG	ELI4 Phantom	QD 0VA 001 BA	1029	NCR	NCR	
Agilent	PNA Series Network Analyzer	E8358A	US40260131	Apr. 02, 2008	Apr. 01, 2009	
Agilent	Wireless Communication Test Set	E5515C	GB46311322	Dec. 22, 2006	Dec. 21, 2008	
R&S	Universal Radio Communication Tester	CMU200	114256	Dec.11, 2007	Dec. 10, 2008	
Agilent	Dielectric Probe Kit	85070D	US01440205	NCR	NCR	
Agilent	Dual Directional Coupler	778D	50422	NCR	NCR	
AR	Power Amplifier	5S1G4M2	0328767	NCR	NCR	
R&S	Power Meter	NRVD	101394	Oct. 20, 2008	Oct. 19, 2009	
R&S	Power Sensor	NRV-Z1	100130	Oct. 20, 2008	Oct. 19, 2009	

Table 5.1 Test Equipment List



6. <u>Tissue Simulating Liquids</u>

For the measurement of the field distribution inside the SAM phantom with DASY5, the phantom must be filled with around 25 liters of homogeneous tissue simulating liquid. The liquid height from the ear reference point (ERP) of the phantom to the liquid top surface is (head SAR)or from the flat phantom to the liquid top surface (body SAR) is 15.2cm.

The following ingredients for tissue simulating liquid are used:

- ▶ Water: deionized water (pure H₂0), resistivity \ge 16MΩ- as basis for the liquid
- Sugar: refined sugar in crystals, as available in food shops to reduce relative permittivity
- Salt: pure NaCl to increase conductivity
- Cellulose: Hydroxyethyl-cellulose, medium viscosity (75-125 mPa.s, 2% in water, 20°C), CAS#54290-to increase viscosity and to keep sugar in solution.
- Preservative: Preventol D-7 Bayer AG, D-51368 Leverkusen, CAS#55965-84-9- to prevent the spread of bacteria and molds.
- DGMBE: Deithlenglycol-monobuthyl ether (DGMBE), Fluka Chemie GmbH, CAS#112-34-5 – to reduce relative permittivity.

Table 6.1 gives the recipes for one liter of body tissue simulating liquid for frequency band 850MHz and 1900 MHz.

Ingredient	MSL-850	MSL-1900
Water	631.68 g	716.56 g
Cellulose	0 g	0 g
Salt	11.72 g	4.0 g
Preventol D-7	1.2 g	0 g
Sugar	600.0 g	0 g
DGMBE	0 g	300.67 g
Total amount	1 liter (1.3 kg)	1 liter (1.0 kg)
Dielectric Parameters at 22°	f=835 MHz	f= 1900 MHz
	$\varepsilon_{\rm r} = 55.2 \pm 5\%,$	$\epsilon_{\rm r} = 53.3 \pm 5 \%$,
	σ= 0.97±5% S/m	σ= 1.52±5% S/m

Table 6.1 Recipes for Tissue Simulating Liquid

The dielectric parameters of the liquids were verified prior to the SAR evaluation using an Agilent 85070D Dielectric Probe Kit and an Agilent Network Analyzer.



Band	Temperature	Frequency (MHz)	Conductivity (σ)	Permittivity (ε _r)	Measurement Date
		824.2	0.942	52.7	2
	21.5	836.4	0.954	52.6	Nov. 21, 2008
GSM850		848.8	0.967	52.5	
05111850		824.2	0.942	52.7	
	21.4	836.4	0.954	52.6	Nov. 28, 2008
		848.8	0.967	52.5	
		1850.2	1.48	51.1	
	21.1	1880.0	1.51	51.0	Nov. 22, 2008
GSM1900		1909.8	1.54	50.9	
0.51011900	21.2	1850.2	1.47	51.1	
		1880.0	1.50	51.0	Nov. 28, 2008
		1909.8	1.53	50.9	
		826.4	0.944	52.7	
WCDMA Band V	21.5	836.4	0.954	52.6	Nov. 22, 2008
		846.6	0.965	52.5	
		1852.4	1.48	51.1	
WCDMA Band II	21.1	1880.0	1.51	51.0	Nov. 22, 2008
		1907.6	1.54	50.9	

Table 6.2 shows the measuring results for muscle simulating liquid.

Table 6.2 Measuring Results for Simulating Liquid

The measuring data are consistent with $\epsilon_r = 55.2 \pm 5\%$ and $\sigma = 0.97 \pm 5\%$ for body GSM850 and WCDMA Band V, and $\epsilon_r = 53.3 \pm 5\%$ and $\sigma = 1.52 \pm 5\%$ for body GSM1900 and WCDMA Band II.





7. <u>Uncertainty Assessment</u>

The component of uncertainly may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainly by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance.

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience and knowledge of the behavior and properties of relevant materials and instruments, manufacture's specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in Table 7.1

Uncertainty Distributions	Normal	Rectangular	Triangular	U-shape
Multiplying factor ^(a)	$_{1/k}$ (b)	1/ 3	1/ 6	1/ 2

(a) standard uncertainty is determined as the product of the multiplying factor and the estimated range of variations in the measured quantity

(b) is the coverage factor

Table 7.1 Multiplying Factions for Various Distributions

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type B evaluation using the usual "root-sum-squares" (RSS) methods of combining standard deviations by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %. The DASY5 uncertainty Budget is showed in Table 7.2.



Error Description	Uncertainty Value ± %	Probability Distribution	Divisor	Ci (1g)	Standard Unc. (1g)	vi or Veff
Measurement Equipment						
Probe Calibration	±5.9 %	Normal	1	1	±5.9 %	∞
Axial Isotropy	±4.7 %	Rectangular	$\sqrt{3}$	0.7	±1.9 %	∞
Hemispherical Isotropy	±9.6 %	Rectangular	$\sqrt{3}$	0.7	±3.9 %	∞
Boundary Effects	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	∞
Linearity	±4.7 %	Rectangular	$\sqrt{3}$	1	±2.7 %	∞
System Detection Limits	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	∞
Readout Electronics	±0.3 %	Normal	1	1	±0.3 %	∞
Response Time	± 0.8 %	Rectangular	$\sqrt{3}$	1	±0.5 %	∞
Integration Time	±2.6 %	Rectangular	$\sqrt{3}$	1	±1.5 %	∞
RF Ambient Noise	±3.0 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
RF Ambient Reflections	±3.0 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
Probe Positioner	±0.4 %	Rectangular	$\sqrt{3}$	1	±0.2 %	∞
Probe Positioning	±2.9 %	Rectangular	$\sqrt{3}$	1	±1.7 %	∞
Max. SAR Eval.	±1.0 %	Rectangular	$\sqrt{3}$	1	±0.6 %	∞
Test Sample Related						
Device Positioning	±2.9 %	Normal	1	1	±2.9	145
Device Holder	±3.6 %	Normal	1	1	±3.6	5
Power Drift	±5.0 %	Rectangular	$\sqrt{3}$	1	±2.9	∞
Phantom and Setup						
Phantom Uncertainty	±4.0 %	Rectangular	$\sqrt{3}$	1	±2.3	∞
Liquid Conductivity (target)	±5.0 %	Rectangular	$\sqrt{3}$	0.64	± 1.8	∞
Liquid Conductivity (meas.)	±2.5 %	Normal	1	0.64	±1.6	∞
Liquid Permittivity (target)	±5.0 %	Rectangular	$\sqrt{3}$	0.6	±1.7	x
Liquid Permittivity (meas.)	±2.5 %	Normal	1	0.6	±1.5	x
Combined Standard Uncertainty					±10.9	387
Coverage Factor for 95 %		K=2				
Expanded uncertainty (Coverage factor = 2)					±21.9	

Table 7.2 Uncertainty Budget of DASY4



8. SAR Measurement Evaluation

Each DASY5 system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY5 software, enable the user to conduct the system performance check and system validation. System validation kit includes a dipole, tripod holder to fix it underneath the flat phantom and a corresponding distance holder.

8.1 <u>Purpose of System Performance check</u>

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

8.2 System Setup

In the simplified setup for system evaluation, the DUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave which comes from a signal generator at frequency 835 MHz and 1900 MHz. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

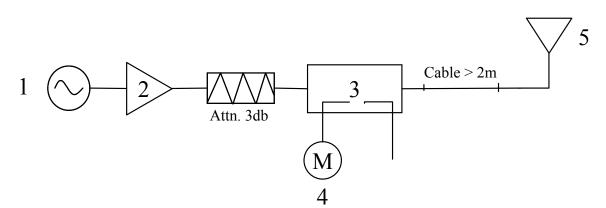


Fig. 8.1 System Setup for System Evaluation



- 1. Signal Generator
- 2. Amplifier
- 3. Directional Coupler
- 4. Power Meter
- 5. 835 MHz or 1900 MHz Dipole

The output power on dipole port must be calibrated to 20dBm (100mW) before dipole is connected.



Fig 8.2 Dipole Setup



8.3 Validation Results

Comparing to the original SAR value provided by SPEAG, the validation data should be within its specification of 10 %. Table 8.1 shows the target SAR and measured SAR after normalized to 1W input power.

Frequency	SAR	Target (W/kg)	Measurement data (W/kg)	Variation	Measurement Date
	SAR (1g)	9.52	9.44	-0.8 %	Nov. 21, 2008
835MHz	SAR (10g)	6.37	6.3	-1.1 %	1107.21,2008
	SAR (1g)	9.52	9.71	2.0 %	Nov. 28, 2008
	SAR (10g)	6.37	6.47	1.6 %	1100. 28, 2008
	SAR (1g)	40.1	40.1	0.0 %	Nov. 22, 2008
1900MHz	SAR (10g)	21.3	21.3	0.0 %	Nov. 22, 2008
	SAR (1g)	40.1	42.1	5.0 %	Nov 28 2000
	SAR (10g)	21.3	22.4	5.2 %	Nov. 28, 2008

Table 8.1 Target and Measurement Data Comparison

The table above indicates the system performance check can meet the variation criterion.



9. Description for DUT Testing Position

This DUT was tested in "Notebook Bottom with 0 cm Gap" position.

Remark: Please refer to Appendix E for the test setup photos.



10. Measurement Procedures

The measurement procedures are as follows:

- Linking DUT with base station emulator in middle channel
- Setting base station emulator to allow DUT to radiate maximum output power
- Measuring output power through RF cable and power meter
- Placing the DUT in the positions described in the last section
- Setting scan area, grid size and other setting on the DASY5 software
- > Taking data for the middle channel on each testing position
- Finding out the largest SAR result on these testing positions of each band
- Measuring output power and SAR results for the low and high channels in this worst case testing position

According to the OET Bulletin 65 Supplement C standard, the recommended procedure for assessing the peak spatial-average SAR value consists of the following steps:

- Power reference measurement
- Area scan
- Zoom scan
- > Power reference measurement

10.1 Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the OET Bulletin 65 Supplement C standard. It can be conducted for 1g and 10g, as well as for user-specific masses. The DASY5 software includes all numerical procedures necessary to evaluate the spatial peak SAR value.

The base for the evaluation is a "cube" measurement. The measured volume must include the 1g and 10g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan.

The entire evaluation of the spatial peak values is performed within the post-processing engine (SEMCAD). The system always gives the maximum values for the 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- extraction of the measured data (grid and values) from the Zoom Scan
- calculation of the SAR value at every measurement point based on all stored data (A/D values and measurement parameters)
- generation of a high-resolution mesh within the measured volume
- interpolation of all measured values form the measurement grid to the high-resolution grid
- extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- calculation of the averaged SAR within masses of 1g and 10g





10.2 <u>Scan Procedures</u>

First Area Scan is used to locate the approximate location(s) of the local peak SAR value(s). The measurement grid within an Area Scan is defined by the grid extent, grid step size and grid offset. Next, in order to determine the EM field distribution in a three-dimensional spatial extension, Zoom Scan is required. The Zoom Scan measures 5x5x7 points with step size 8, 8 and 5 mm. The Zoom Scan is performed around the highest E-field value to determine the averaged SAR-distribution over 1 g.

10.3 <u>SAR Averaged Methods</u>

In DASY5, the interpolation and extrapolation are both based on the modified Quadratic Shepard's method. The interpolation scheme combines a least-square fitted function method and a weighted average method which are the two basic types of computational interpolation and approximation.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1 g and 10 g cubes, the extrapolation distance should not be larger than 5 mm.



11. SAR Test Results

11.1 Conducted Power

Band Mada Channel		GSM 850 (dBm)		GSM 1900 (dBm)			
Mode	128	189	251	512	661	810	
GPRS 8	31.77	31.78	31.67	29.27	29.12	28.71	
GPRS 10	31.75	31.75	31.65	29.26	29.11	28.70	
EGPRS 8	26.85	26.91	26.87	26.12	26.19	25.79	
EGPRS 10	26.82	26.88	26.85	26.11	26.17	25.78	

	Band	V	CDMA Band (dBm)	V	WCDMA Band II (dBm)			
Mode		4132	4182	4233	9262	9400	9538	
12.2k	K	21.90	21.92	21.53	22.50	22.35	22.19	
	Subtest-1	22.51	22.53	22.13	22.90	22.80	22.26	
12.2K+HSDPA	Subtest-2	21.94	22.13	21.72	22.61	22.43	22.31	
12.2K7H5DFA	Subtest-3	21.80	22.01	21.56	22.40	22.19	22.07	
	Subtest-4	22.02	22.20	21.76	22.67	22.47	22.05	
	Subtest-1	21.85	21.88	21.48	22.25	22.02	21.93	
	Subtest-2	19.92	19.98	19.59	20.44	20.24	19.91	
12.2K+HSUPA	Subtest-3	21.02	21.14	20.68	21.40	21.21	20.98	
	Subtest-4	20.01	20.16	19.74	20.80	20.60	20.49	
	Subtest-5	21.76	21.71	21.43	22.23	22.11	21.91	





11.2 <u>Test Records for Body SAR Test</u>
--

Band	Chan.	Freq. (MHz)	Modulation Type	Battery	LCD	Camera	Measured 1g SAR (W/kg)	Limit (W/kg)	Result		
GSM850 (GPRS10)	189	836.4	GMSK	1	2	2	0.036	1.6	Pass		
GSM850 (GPRS10)	189	836.4	GMSK	2	2	2	0.034	1.6	Pass		
GSM850 (GPRS 10)	189	836.4	GMSK	3	2	2	0.056	1.6	Pass		
GSM850 (GPRS10)	189	836.4	GMSK	4	2	2	0.057	1.6	Pass		
GSM850 (GPRS10)	189	836.4	GMSK	5	2	2	0.056	1.6	Pass		
				R is Batt	ery 4, wł		d for all other test me				
GSM850 (GPRS10) 128 824.2 GMSK 4 2 2 0.032 1.6 Pass											
GSM850 (GPRS10)	251	848.8	GMSK	4	2	2	0.084	1.6	Pass		
GSM850 (GPRS10)	251	848.8	GMSK	4	1	1	0.089	1.6	Pass		
GSM1900 (GPRS10)	661	1880.0	GMSK	4	2	2	0.011	1.6	Pass		
GSM1900 (GPRS10)	512	1850.0	GMSK	4	2	2	0.00994	1.6	Pass		
GSM1900 (GPRS 10)	810	1909.8	GMSK	4	2	2	0.017	1.6	Pass		
GSM1900 (GPRS10)	810	1909.8	GMSK	4	1	1	0.013	1.6	Pass		
WCDMA Band V (RMK 12.2K)	4182	836.4	QPSK	4	2	2	0.034	1.6	Pass		
WCDMA Band V (HSDPA)	4182	836.4	QPSK	4	2	2	0.031	1.6	Pass		
WCDMA Band V (HSUPA)	4182	836.4	QPSK	4	2	2	0.026	1.6	Pass		
WCDMA Band V (RMC12.2K)	4132	826.4	QPSK	4	2	2	0.019	1.6	Pass		
WCDMA Band V (RMC12.2K)	4233	846.6	QPSK	4	2	2	0.035	1.6	Pass		
WCDMA Band II (RMC12.2K)	9400	1880.0	QPSK	4	2	2	0.017	1.6	Pass		
WCDMA Band II (HSDPA)	9400	1880.0	QPSK	4	2	2	0.012	1.6	Pass		
WCDMA Band II (HSUPA)	9400	1880.0	QPSK	4	2	2	0.011	1.6	Pass		
WCDMA Band II (RMC12.2K)	9262	1852.4	QPSK	4	2	2	0.00811	1.6	Pass		
WCDMA Band II (RMC12.2K)	9538	1907.6	QPSK	4	2	2	0.014	1.6	Pass		

Test Engineer : Jason Wang, Robert Liu, and A-Rod Chen



12.<u>References</u>

- [1] FCC 47 CFR Part 2 "Frequency Allocations and Radio Treaty Matters; General Rules and Regulations"
- [2] IEEE Std. P1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", April 21, 2003
- [3] Supplement C (Edition 01-01) to OET Bulletin 65 (Edition 97-01), "Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to RF Emissions", June 2001
- [4] IEEE Std. C95.1-1999, "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz", 1999
- [5] Robert J. Renka, "Multivariate Interpolation Of Large Sets Of Scattered Data", University of North Texas ACM Transactions on Mathematical Software, vol. 14, no. 2, June 1988, pp. 139-148
- [6] DASY5 System Handbook



Appendix A - System Performance Check Data

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/11/21

System Check_Body_835MHz_081121

DUT: Dipole 835 MHz


Communication System: CW; Frequency: 835 MHz;Duty Cycle: 1:1 Medium: MSL_850 Medium parameters used: f = 835 MHz; σ = 0.953 mho/m; ϵ_r = 52.6; ρ = 1000 kg/m³ Ambient Temperature : 22.4 ; Liquid Temperature : 21.5

DASY5 Configuration:

- Probe: ET3DV6 SN1788; ConvF(6.34, 6.34, 6.34); Calibrated: 2008/9/23
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2008/9/22
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.2 Build 87

Pin=100mW/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 1.03 mW/g

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 34.6 V/m; Power Drift = -0.028 dB Peak SAR (extrapolated) = 1.29 W/kg SAR(1 g) = 0.944 mW/g; SAR(10 g) = 0.630 mW/g Maximum value of SAR (measured) = 1.03 mW/g

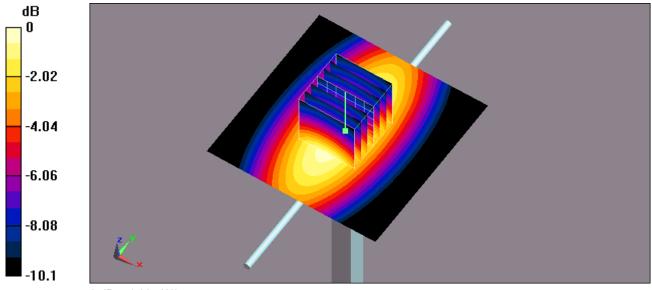

0 dB = 1.03mW/g



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/11/28

System Check_Body_835MHz_081128

DUT: Dipole 835 MHz


Communication System: CW; Frequency: 835 MHz;Duty Cycle: 1:1 Medium: MSL_850 Medium parameters used: f = 835 MHz; σ = 0.953 mho/m; ϵ_r = 52.6; ρ = 1000 kg/m³ Ambient Temperature : 22.4 ; Liquid Temperature : 21.4

DASY5 Configuration:

- Probe: ET3DV6 SN1788; ConvF(6.34, 6.34, 6.34); Calibrated: 2008/9/23
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2008/9/22
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.2 Build 87

Pin=100mW/Area Scan (61x61x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 1.05 mW/g

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 34.9 V/m; Power Drift = -0.000928 dB Peak SAR (extrapolated) = 1.32 W/kg SAR(1 g) = 0.971 mW/g; SAR(10 g) = 0.647 mW/g Maximum value of SAR (measured) = 1.06 mW/g

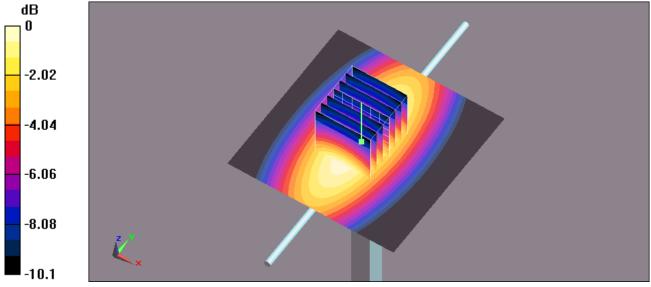

 $0 \, dB = 1.06 \, mW/g$



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/11/22

System Check_Body_1900MHz_081122

DUT: Dipole 1900 MHz


Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: MSL_1900 Medium parameters used: f = 1900 MHz; σ = 1.53 mho/m; ϵ_r = 51; ρ = 1000 kg/m³ Ambient Temperature : 22.7 ; Liquid Temperature : 21.1

DASY5 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.73, 4.73, 4.73); Calibrated: 2008/9/23
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2008/9/22
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.2 Build 87

Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 4.69 mW/g

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 57.7 V/m; Power Drift = -0.102 dB Peak SAR (extrapolated) = 7.12 W/kg SAR(1 g) = 4.01 mW/g; SAR(10 g) = 2.13 mW/g Maximum value of SAR (measured) = 4.52 mW/g

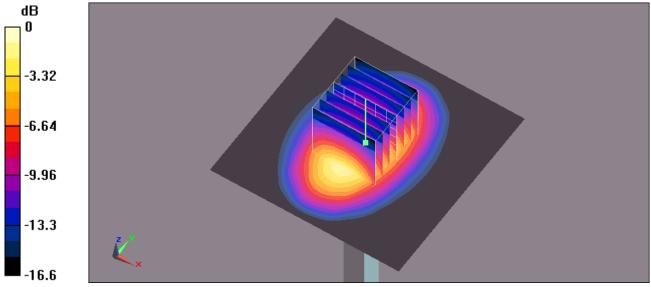

 $0 \, dB = 4.52 mW/g$



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/11/28

System Check_Body_1900MHz_081128

DUT: Dipole 1900 MHz


Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: MSL_1900 Medium parameters used: f = 1900 MHz; σ = 1.52 mho/m; ϵ_r = 50.9; ρ = 1000 kg/m³ Ambient Temperature : 22.5 ; Liquid Temperature : 21.2

DASY5 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.73, 4.73, 4.73); Calibrated: 2008/9/23
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2008/9/22
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.2 Build 87

Pin=100mW/Area Scan (91x91x1): Measurement grid: dx=10mm, dy=10mm Maximum value of SAR (interpolated) = 4.81 mW/g

Pin=100mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 58.9 V/m; Power Drift = -0.00786 dB Peak SAR (extrapolated) = 7.48 W/kg SAR(1 g) = 4.21 mW/g; SAR(10 g) = 2.24 mW/g Maximum value of SAR (measured) = 4.78 mW/g

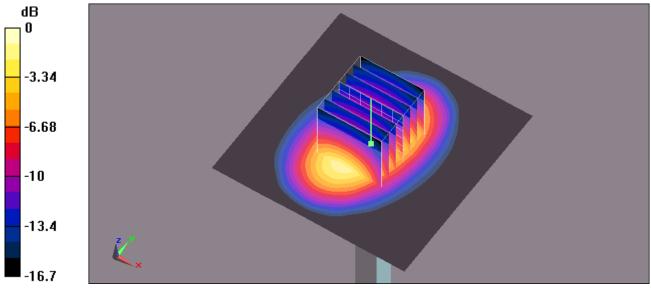

 $0 \, dB = 4.78 \, mW/g$



Appendix B - SAR Measurement Data

Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/11/28

Body_GSM850 Ch251_ NB Bottom With 0cm Gap_GPRS10_Battery 4_LCD 1_Camera 1

DUT: 8N1310-01


Communication System: GSM850; Frequency: 848.8 MHz;Duty Cycle: 1:4 Medium: MSL_850 Medium parameters used: f = 849 MHz; σ = 0.967 mho/m; ϵ_r = 52.5; ρ = 1000 kg/m³ Ambient Temperature : 22.4 ; Liquid Temperature : 21.4

DASY5 Configuration:

- Probe: ET3DV6 SN1788; ConvF(6.34, 6.34, 6.34); Calibrated: 2008/9/23
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2008/9/22
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.2 Build 87

Ch251/Area Scan (51x191x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.105 mW/g

Ch251/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 2.04 V/m; Power Drift = 0.115 dB Peak SAR (extrapolated) = 0.132 W/kg SAR(1 g) = 0.089 mW/g; SAR(10 g) = 0.059 mW/g Maximum value of SAR (measured) = 0.095 mW/g

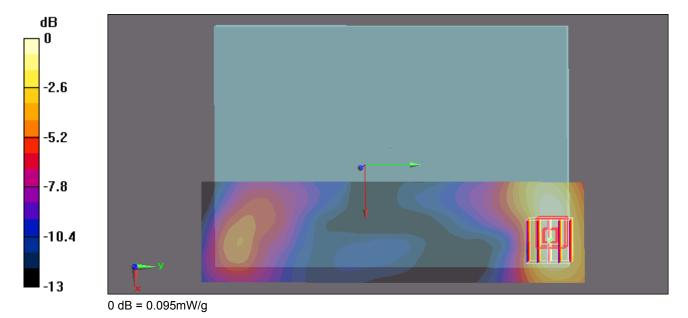



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab Date: 2008/11/22

Body_GSM1900 Ch810_NB Bottom With 0cm Gap_GPRS10_Battery 4_ LCD 2_Camera 2

DUT: 8N1310-01

Communication System: PCS; Frequency: 1909.8 MHz;Duty Cycle: 1:4 Medium: MSL_1900 Medium parameters used: f = 1910 MHz; σ = 1.54 mho/m; ϵ_r = 50.9; ρ = 1000 kg/m³ Ambient Temperature : 22.7 ; Liquid Temperature : 21.1


DASY5 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.73, 4.73, 4.73); Calibrated: 2008/9/23
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2008/9/22
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.2 Build 87

Ch810/Area Scan (51x191x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.020 mW/g

Ch810/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.53 V/m; Power Drift = -0.195 dB Peak SAR (extrapolated) = 0.030 W/kg SAR(1 g) = 0.017 mW/g; SAR(10 g) = 0.011 mW/g Maximum value of SAR (measured) = 0.018 mW/g

Ch810/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.53 V/m; Power Drift = -0.195 dB Peak SAR (extrapolated) = 0.021 W/kg SAR(1 g) = 0.015 mW/g; SAR(10 g) = 0.010 mW/g Maximum value of SAR (measured) = 0.015 mW/g

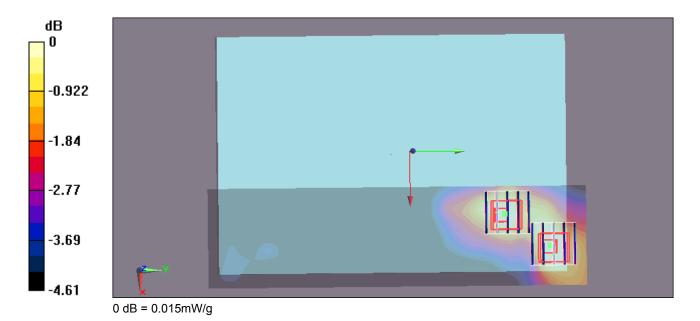



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab Date: 2008/11/22

Body_WCDMA850 Ch4233_NB Bottom With 0cm Gap_RMC12.2K_Battery 4_ LCD 2_Camera 2

DUT: 8N1310-01


Communication System: WCDMA; Frequency: 846.6 MHz;Duty Cycle: 1:1 Medium: MSL_850 Medium parameters used: f = 847 MHz; σ = 0.965 mho/m; ϵ_r = 52.5; ρ = 1000 kg/m³ Ambient Temperature : 22.4 ; Liquid Temperature : 21.5

DASY5 Configuration:

- Probe: ET3DV6 SN1788; ConvF(6.34, 6.34, 6.34); Calibrated: 2008/9/23
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2008/9/22
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.2 Build 87

Ch4233/Area Scan (51x191x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.037 mW/g

Ch4233/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.76 V/m; Power Drift = -0.117 dB Peak SAR (extrapolated) = 0.048 W/kg SAR(1 g) = 0.035 mW/g; SAR(10 g) = 0.024 mW/g Maximum value of SAR (measured) = 0.038 mW/g

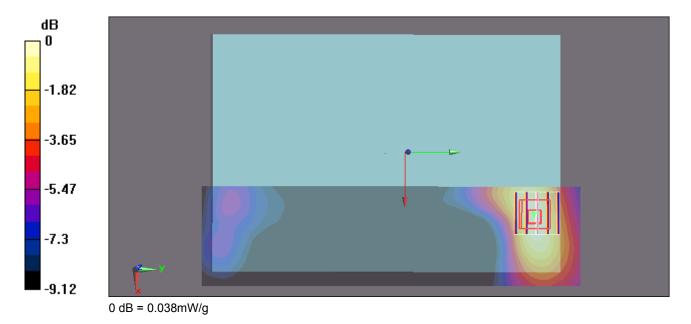



Body_WCDMA1900 Ch9400_NB Bottom With 0cm Gap_RMC12.2K_Battery 4_ LCD 2_Camera 2

DUT: 8N1310-01


Communication System: WCDMA; Frequency: 1880 MHz;Duty Cycle: 1:1 Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.51 mho/m; ϵ_r = 51; ρ = 1000 kg/m³ Ambient Temperature : 22.7 ; Liquid Temperature : 21.1

DASY5 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.73, 4.73, 4.73); Calibrated: 2008/9/23
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2008/9/22
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.2 Build 87

Ch9400/Area Scan (141x191x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.018 mW/g

Ch9400/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.38 V/m; Power Drift = 0.182 dB Peak SAR (extrapolated) = 0.026 W/kg SAR(1 g) = 0.017 mW/g; SAR(10 g) = 0.011 mW/g Maximum value of SAR (measured) = 0.018 mW/g

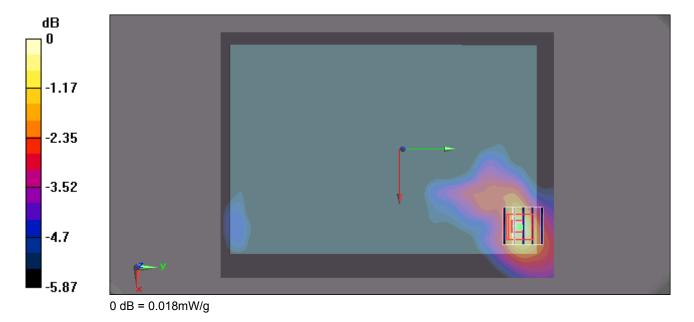



Body_GSM850 Ch251_ NB Bottom With 0cm Gap_GPRS10_Battery 4_ LCD 1_Camera 1_2D

DUT: 8N1310-01


Communication System: GSM850; Frequency: 848.8 MHz;Duty Cycle: 1:4 Medium: MSL_850 Medium parameters used: f = 849 MHz; σ = 0.967 mho/m; ϵ_r = 52.5; ρ = 1000 kg/m³ Ambient Temperature : 22.4 ; Liquid Temperature : 21.4

DASY5 Configuration:

- Probe: ET3DV6 SN1788; ConvF(6.34, 6.34, 6.34); Calibrated: 2008/9/23
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2008/9/22
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.2 Build 87

Ch251/Area Scan (51x191x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.105 mW/g

Ch251/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 2.04 V/m; Power Drift = 0.115 dB Peak SAR (extrapolated) = 0.132 W/kg SAR(1 g) = 0.089 mW/g; SAR(10 g) = 0.059 mW/g Maximum value of SAR (measured) = 0.095 mW/g

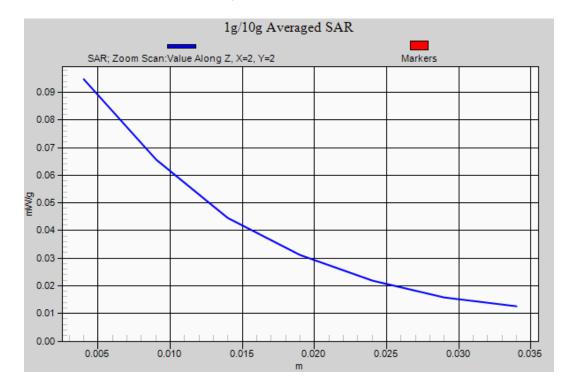



Body_GSM1900 Ch810_NB Bottom With 0cm Gap_GPRS10_Battery 4_ LCD 2_Camera 2_2D

DUT: 8N1310-01

Communication System: PCS; Frequency: 1909.8 MHz;Duty Cycle: 1:4 Medium: MSL_1900 Medium parameters used: f = 1910 MHz; σ = 1.54 mho/m; ϵ_r = 50.9; ρ = 1000 kg/m³ Ambient Temperature : 22.7 ; Liquid Temperature : 21.1


DASY5 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.73, 4.73, 4.73); Calibrated: 2008/9/23
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2008/9/22
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.2 Build 87

Ch810/Area Scan (51x191x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.020 mW/g

Ch810/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.53 V/m; Power Drift = -0.195 dB Peak SAR (extrapolated) = 0.030 W/kg SAR(1 g) = 0.017 mW/g; SAR(10 g) = 0.011 mW/g Maximum value of SAR (measured) = 0.018 mW/g

Ch810/Zoom Scan (5x5x7)/Cube 1: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.53 V/m; Power Drift = -0.195 dB Peak SAR (extrapolated) = 0.021 W/kg SAR(1 g) = 0.015 mW/g; SAR(10 g) = 0.010 mW/g Maximum value of SAR (measured) = 0.015 mW/g

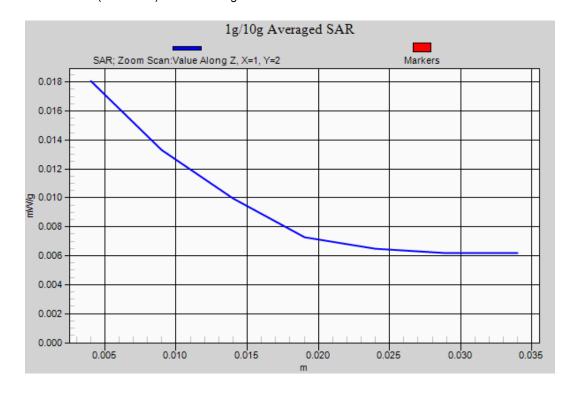



Body_WCDMA850 Ch4233_NB Bottom With 0cm Gap_RMC12.2K_Battery 4_ LCD 2_Camera 2_2D

DUT: 8N1310-01


Communication System: WCDMA; Frequency: 846.6 MHz;Duty Cycle: 1:1 Medium: MSL_850 Medium parameters used: f = 847 MHz; σ = 0.965 mho/m; ϵ_r = 52.5; ρ = 1000 kg/m³ Ambient Temperature : 22.4 ; Liquid Temperature : 21.5

DASY5 Configuration:

- Probe: ET3DV6 SN1788; ConvF(6.34, 6.34, 6.34); Calibrated: 2008/9/23
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2008/9/22
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.2 Build 87

Ch4233/Area Scan (51x191x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.037 mW/g

Ch4233/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm Reference Value = 1.76 V/m; Power Drift = -0.117 dB Peak SAR (extrapolated) = 0.048 W/kg SAR(1 g) = 0.035 mW/g; SAR(10 g) = 0.024 mW/g Maximum value of SAR (measured) = 0.038 mW/g

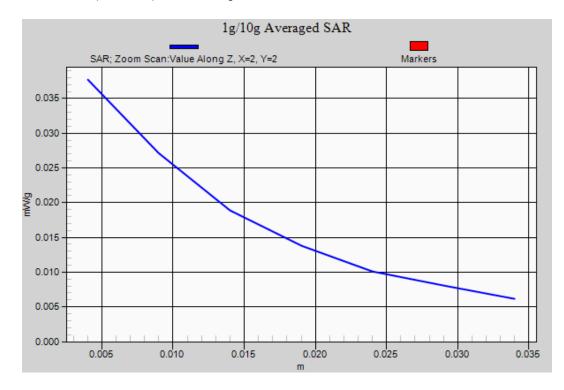



Test Laboratory: Sporton International Inc. SAR/HAC Testing Lab

Date: 2008/11/22

Body_WCDMA1900 Ch9400_NB Bottom With 0cm Gap_RMC12.2K_Battery 4_ LCD 2_Camera 2_2D

DUT: 8N1310-01

Communication System: WCDMA; Frequency: 1880 MHz;Duty Cycle: 1:1 Medium: MSL_1900 Medium parameters used: f = 1880 MHz; σ = 1.51 mho/m; ϵ_r = 51; ρ = 1000 kg/m³ Ambient Temperature : 22.7 ; Liquid Temperature : 21.1

DASY5 Configuration:

- Probe: ET3DV6 SN1788; ConvF(4.73, 4.73, 4.73); Calibrated: 2008/9/23
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn778; Calibrated: 2008/9/22
- Phantom: ELI 4.0; Type: QDOVA001BA; Serial: 1029
- Measurement SW: DASY5, V5.0 Build 120; SEMCAD X Version 13.2 Build 87


Ch9400/Area Scan (141x191x1): Measurement grid: dx=15mm, dy=15mm Maximum value of SAR (interpolated) = 0.018 mW/g

Ch9400/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 1.38 V/m; Power Drift = 0.182 dB

Peak SAR (extrapolated) = 0.026 W/kg SAR(1 g) = 0.017 mW/g; SAR(10 g) = 0.011 mW/g

Maximum value of SAR (measured) = 0.018 mW/g

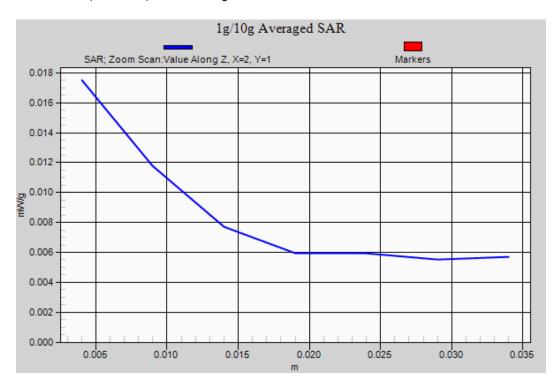



Appendix C – Calibration Data

	h, Switzerland	KIBRATE S S	wiss Calibration Service
credited by the Swiss Accred e Swiss Accreditation Servic Itilateral Agreement for the r	e is one of the signatorie		: SCS 108
lient Sporton (Aude	in)	Certificate No: D	835V2-499_Mar08
CALIBRATION	CERTIFICATE		
Dbject	D835V2 - SN: 49	9	
Calibration procedure(s)	QA CAL-05.v7 Calibration proce	dure for dipole validation kits	
Calibration date:	March 17, 2008		
Condition of the calibrated item	In Tolerance		
The measurements and the unce	ertainties with confidence proceed in the closed laborator	onal standards, which realize the physical units of robability are given on the following pages and are y facility: environment temperature (22 ± 3)°C and	e part of the certificate.
The measurements and the unce	ertainties with confidence proceed in the closed laborator	robability are given on the following pages and are	e part of the certificate.
he measurements and the unce all calibrations have been conduct calibration Equipment used (M& trimary Standards	rtainties with confidence protected in the closed laborator TE critical for calibration)	robability are given on the following pages and an y facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.)	e part of the certificate. d humidity < 70%. Scheduled Calibration
The measurements and the unce of calibrations have been conduct calibration Equipment used (M& Primary Standards Prower meter EPM-442A	rtainties with confidence proceed in the closed laborator TE critical for calibration)	robability are given on the following pages and an y facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	rtainties with confidence proceed in the closed laborator TE critical for calibration) ID # GB37480704 US37292783	robability are given on the following pages and are y facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	rtainties with confidence provided in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g)	robability are given on the following pages and are y fadility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718)	e part of the certificate d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2	rtainties with confidence proceed in the closed laborator TE critical for calibration) ID # GB37480704 US37292783	robability are given on the following pages and are y facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Prower sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4	rtainties with confidence provided in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025	robability are given on the following pages and are y facility: environment temperature (22 ± 3)*C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-09
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	rtainties with confidence provided in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909	robability are given on the following pages and are y fadility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-09 Sep-08
The measurements and the unce all calibrations have been conduct calibration Equipment used (M&T trimary Standards tower meter EPM-442A tower sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 VAE4 Secondary Standards tower sensor HP 8481A	ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID #	robability are given on the following pages and are y facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # ID # MY41092317	Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09
The measurements and the unce All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	ID # ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # MY41092317 100005	robability are given on the following pages and are y facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 04-Aug-99 (SPEAG, in house check Oct-07)	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # MY41092317 I00005 US37390585 S4206 IUS37390585 S4206 IUS37292783 IUS37390585 S4206 IUS37390585	robability are given on the following pages and are y facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 04-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07)	e part of the certificate d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Reference 2robe ES3DV2 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by:	ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # MY41092317 100005 US37390585 S4206 Name	robability are given on the following pages and are y facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00736) 07-Aug-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 04-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) Function	e part of the certificate. d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09
The measurements and the unce	ID # ID # GB37480704 US37292783 SN: 5086 (20g) SN: 3025 SN 909 ID # MY41092317 100005 US37390585 S4206 Name Claudio Leubler	robability are given on the following pages and are ty facility: environment temperature (22 ± 3)°C and Cal Date (Calibrated by, Certificate No.) 04-Oct-07 (METAS, No. 217-00736) 04-Oct-07 (METAS, No. 217-00718) 01-Mar-08 (SPEAG, No. 217-00718) 01-Mar-08 (SPEAG, No. 253-3025_Mar08) 03-Sep-07 (SPEAG, No. DAE4-909_Sep07) Check Date (in house) 18-Oct-02 (SPEAG, in house check Oct-07) 04-Aug-99 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) 18-Oct-01 (SPEAG, in house check Oct-07) Function Laboratory Technician	e part of the certificate d humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Aug-08 Mar-09 Sep-08 Scheduled Check In house check: Oct-09 In house check: Oct-09 In house check: Oct-09



Calibration Laboratory of Schmid & Partner

Engineering AG





S

S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage

С Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions; Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- · Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D835V2-499 Mar08

Page 2 of 9



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V4.9	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	44
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.5 ± 6 %	0.90 mho/m ± 6 %
Head TSL temperature during test	(22.0 ± 0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.29 mW/g
SAR normalized	normalized to 1W	9.16 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	9.16 mW / g ± 17.0 % (k=2)

SAR measured	250 mW input power	1.50 mW/g
SAR normalized	normalized to 1W	6.00 mW/g
SAR for nominal Head TSL parameters 1	 normalized to 1W 	6.00 mW / g ± 16.5 % (k=2)

.

1 Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D835V2-499_Mar08

Page 3 of 9

Body TSL parameters The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.0 ± 6 %	1.00 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C		2122.0

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.46 mW/g
SAR normalized	normalized to 1W	9.84 mW / g
SAR for nominal Body TSL parameters 2	normalized to 1W	9.52 mW/g±17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.63 mW / g
SAR normalized	normalized to 1W	6.52 mW / g
SAR for nominal Body TSL parameters 2	normalized to 1W	6.37 mW / g ± 16.5 % (k=2)

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D835V2-499_Mar08

Page 4 of 9



Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.9 Ω - 2.3 jΩ
Return Loss	- 28.9 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.2 Ω - 3.3 jΩ	
Return Loss	- 29.3 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.392 ns	

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	July 10, 2003

Certificate No: D835V2-499_Mar08

Page 5 of 9





DASY4 Validation Report for Head TSL

Date/Time: 17.03.2008 11:32:45

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:499


Communication System: CW-835; Frequency: 835 MHz; Duty Cycle: 1:1 Medium: HSL 900 MHz; Medium parameters used: f = 835 MHz; σ = 0.9 mho/m; ε_r = 41.5; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(6.09, 6.09, 6.09); Calibrated: 01.03.2008
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 03.09.2007
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

Unnamed procedure/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 54.9 V/m; Power Drift = -0.005 dB Peak SAR (extrapolated) = 3.34 W/kg SAR(1 g) = 2.29 mW/g; SAR(10 g) = 1.5 mW/g Maximum value of SAR (measured) = 2.58 mW/g

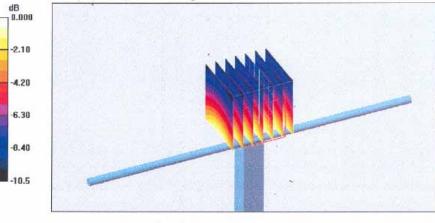


 $0 \, dB = 2.58 \, mW/g$

Certificate No: D835V2-499_Mar08

Page 6 of 9





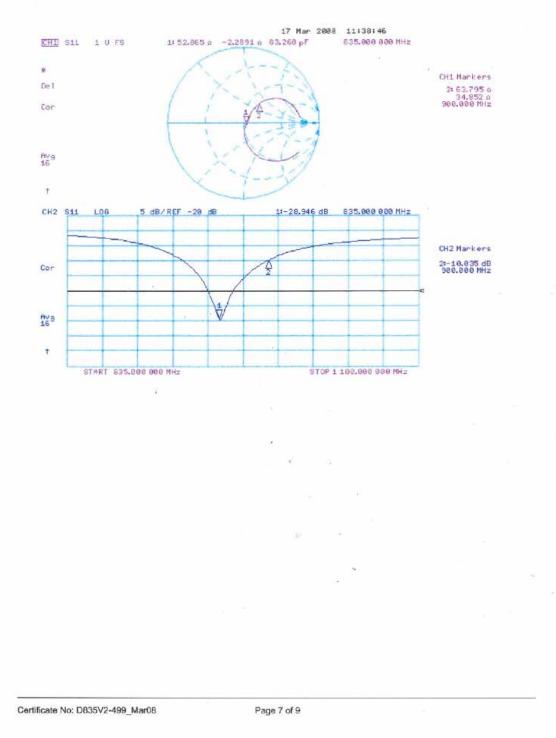

Date/Time: 10.03.2008 12:48:36



DASY4 Validation Report for Body TSL


Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:499

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium: MSL900; Medium parameters used: f = 835 MHz; $\sigma = 1$ mho/m; $\epsilon_r = 54$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)


DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(5.85, 5.85, 5.85); Calibrated: 01.03.2008
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 03.09.2007
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

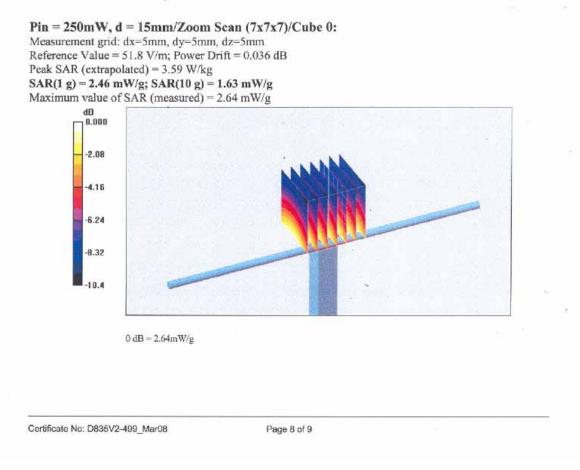



Impedance Measurement Plot for Body TSL

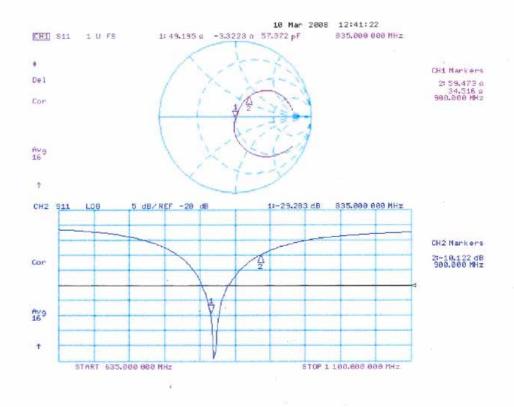

Certificate No: D835V2-499_Mar08

Page 9 of 9



Calibration Laborator Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurio	π.		ichweizerischer Kalibrierdienst ervice suisse d'étalonnage ervizio svizzero di taratura wiss Calibration Service
Accredited by the Swiss Federal (The Swiss Accreditation Servic	지수는 것 같은 것 같은 것이 같은 것 같은 것 같은 것이 같이 많이 많이 했다.		a: SCS 108
Multilateral Agreement for the r	. 그가 요즘 아무렇게 한 것을 가락하게 다 가격을 했다.		
Client Sporton (Aude			01900V2-5d041_Mar08
CALIBRATION			
Object	D1900V2 - SN: 5	d041	
- Dijedi	0100072 - 514. 0		
Calibration procedure(s)	QA CAL-05.v7 Calibration proce	dure for dipole validation kits	
Calibration date:	March 18, 2008		
Condition of the calibrated item	In Tolerance		
	cted in the closed laborator	robability are given on the following pages and arry facility: environment temperature $(22 \pm 3)^{\circ}$ C and	
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	04-Oct-07 (METAS, No. 217-00736)	Oct-08
Power sensor HP 8481A	US37292783	04-Oct-07 (METAS, No. 217-00736)	Oct-08
Reference 20 dB Attenuator	SN: 5086 (20g)	07-Aug-07 (METAS, No 217-00718)	Aug-08
Reference 10 dB Attenuator Reference Probe ES3DV2	SN: 5047.2 (10r)	07-Aug-07 (METAS, No 217-00718)	Aug-08
DAE4	SN: 3025 SN 909	01-Mar-08 (SPEAG, No. ES3-3025_Mar08) 3-Sep-08 (SPEAG, No. DAE4-909_Sep07)	Mar-09 Sep-07
DAL-	014 000	3-3ep-06 (SPENG, No. DRE4-ada_3ep01)	36p-07
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (SPEAG, in house check Oct-07)	In house check: Oct-08
RF generator R&S SMT-06	100005	4-Aug-99 (SPEAG, in house check Oct-07)	In house check: Oct-09
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (SPEAG, in house check Oct-07)	In house check: Oct-08
Power meter EPM-442A	GB37480704	04-Oct-07 (METAS, No. 217-00736)	Oct-08
		-	
Calibrated by:	Name Marcel Fehr	Function Laboratory Technician	Signature
Approved by:	Kalja Pokovic	Technical Manager	Jolan Katy
This calibration certificate shall no	ot be reproduced except in	full without written approval of the laboratory.	Issued: March 18, 2008

Certificate No: D1900V2-5d041_Mar08

Page 1 of 9



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S

S

Schweizerischer Kalibrierdienst

C Service suisse d'étalonnage

Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D1900V2-5d041_Mar08

Page 2 of 9



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY4	V4.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	¥.
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	1.47 mho/m ± 6 %
Head TSL temperature during test	(21.1 ± 0.2) °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	condition	
SAR measured	250 mW input power	10.1 mW/g
SAR normalized	normalized to 1W	40.4 mW / g
SAR for nominal Head TSL parameters 1	normalized to 1W	39.5 mW / g ± 17.0 % (k=2)
24 D	Que d'Alere	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
	Condition 250 mW input power	5.20 mW / g
SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured SAR normalized		5.20 mW / g 20.8 mW / g

¹ Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D1900V2-5d041_Mar08

Page 3 of 9



Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	51.6 ± 6 %	1.57 mho/m ± 6 %
Body TSL temperature during test	(21.4±0.2) °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.4 mW / g
SAR normalized	normalized to 1W	41.6 mW/g
SAR for nominal Body TSL parameters 2	normalized to 1W	40.1 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.44 mW / g
SAR normalized	normalized to 1W	21.8 mW/g
SAR for nominal Body TSL parameters ²	normalized to 1W	21.3 mW / g ± 16.5 % (k=2)

² Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

Certificate No: D1900V2-5d041_Mar08

Page 4 of 9



Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.0 Ω + 5.1 jΩ	
Return Loss	- 24.2 dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.0 Ω + 6.1 jΩ	
Return Loss	- 23.6 dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.199 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	July 04, 2003	

Certificate No: D1900V2-5d041_Mar08

Page 5 of 9



DASY4 Validation Report for Head TSL

Date/Time: 18.03.2008 12:05:10

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d041


Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: HSL U10 BB; Medium parameters used: f = 1900 MHz; σ = 1.47 mho/m; ϵ_r = 40.2; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.9, 4.9, 4.9); Calibrated: 01.03.2008
- · Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 03.09.2007
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 91.7 V/m; Power Drift = 0.013 dB Peak SAR (extrapolated) = 19.1 W/kg SAR(1 g) = 10.1 mW/g; SAR(10 g) = 5.2 mW/g Maximum value of SAR (measured) = 11.8 mW/g

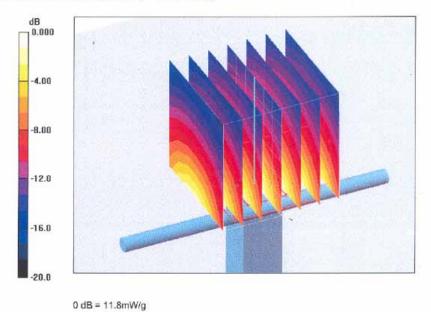


Certificate No: D1900V2-5d041_Mar08

Page 6 of 9



Impedance Measurement Plot for Head TSL

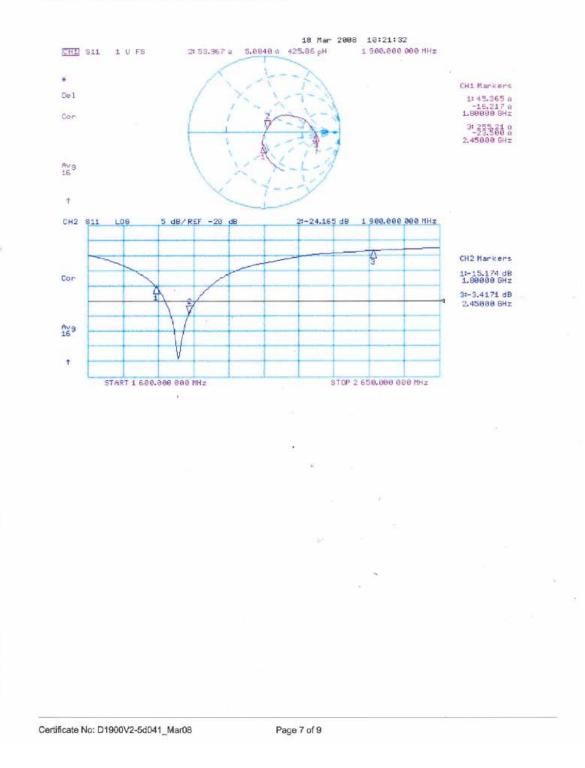



DASY4 Validation Report for Body TSL

Date/Time: 14.03.2008 13:22:24

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d041


Communication System: CW; Frequency: 1900 MHz;Duty Cycle: 1:1 Medium: MSL U10 BB; Medium parameters used: f = 1900 MHz; σ = 1.57 mho/m; ϵ_r = 51.7; ρ = 1000 kg/m³ Phantom section: Flat Section Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ES3DV2 SN3025; ConvF(4.5, 4.5, 4.5); Calibrated: 01.03.2008
- Sensor-Surface: 3.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn909; Calibrated: 03.09.2007
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; ;
- Measurement SW: DASY4, V4.7 Build 55; Postprocessing SW: SEMCAD, V1.8 Build 172

Pin = 250 mW; d = 10 mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 89.7 V/m; Power Drift = 0.004 dB Peak SAR (extrapolated) = 18.6 W/kg SAR(1 g) = 10.4 mW/g; SAR(10 g) = 5.44 mW/g Maximum value of SAR (measured) = 12.0 mW/g

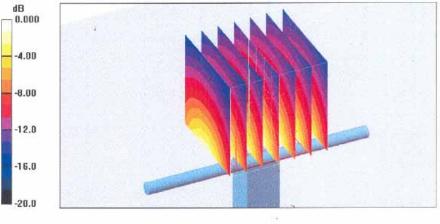


0 dB = 12.0mW/g

Certificate No: D1900V2-5d041_Mar08

Page 8 of 9



Impedance Measurement Plot for Body TSL

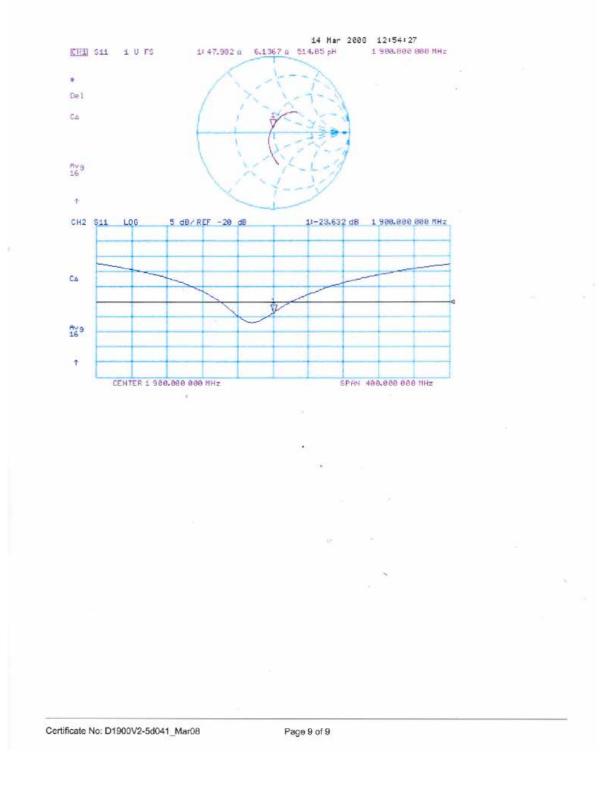



Schmid & Partner Engineering AG eughausstrasse 43, 8004 Zurich,	of Switzerland		z) c	Schweizerischer Kalibrierdie Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service	nst
ccredited by the Swiss Accreditation he Swiss Accreditation Service in fulfilateral Agreement for the reco	s one of the signatories	to the EA	Accreditation N	o.: SCS 108	
lient Sporton (Auden)			Certificate No:	DAE4-778_Sep08	
CALIBRATION C	ERTIFICATE				100
Dbject	DAE4 - SD 000 D	04 BG - SN: 778		Monte S. V.	
Calibration procedure(s)	QA CAL-06.v12 Calibration proces	dure for the data acqui	sition electro	onics (DAE)	
Calibration date:	September 22, 20	800			
Condition of the calibrated item This calibration certificate documen The measurements and the uncerta All calibrations have been conducte	ainties with confidence pr	obability are given on the follow	wing pages and a	are part of the certificate.	
This calibration certificate documen The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE	its the traceability to natio ainties with confidence pr ed in the closed laboratory critical for calibration)	obability are given on the follow	wing pages and a	are part of the certificate. and humidity < 70%.	
This calibration certificate documen The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards	Its the traceability to natio ainties with confidence pr ed in the closed laboratory critical for calibration)	obability are given on the follow y facility: environment tempera Cal Date (Certificate No.)	wing pages and a	are part of the certificate. and humidity < 70%. Scheduled Calibration	
This calibration certificate documen The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702	Its the traceability to natio ainties with confidence pr ed in the closed laboratory critical for calibration)	obability are given on the follow	wing pages and a	are part of the certificate. and humidity < 70%.	
This calibration certificate documen The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001	ts the traceability to natio ainties with confidence pr ed in the closed laboratory critical for calibration) ID # SN: 6295603	Cal Date (Certificate No.) 04-Oct-07 (No: 6467)	wing pages and a	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-08	
This calibration certificate documen The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	ts the traceability to natio ainties with confidence pr ed in the closed laboratory critical for calibration) 1D # SN: 6295603 SN: 0810278	Cal Date (Certificate No.) 04-Oct-07 (No: 6465)	wing pages and a	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-08 Oct-08	
This calibration certificate documen The measurements and the uncerta	Its the traceability to natio antices with confidence pr ed in the closed laboratory critical for calibration) ID # SN: 6295603 SN: 0810278 ID # SE UMS 006 AB 1004	obability are given on the follow y facility: environment tempera <u>Cal Date (Certificate No.)</u> 04-Oct-07 (No: 6467) 03-Oct-07 (No: 6465) <u>Check Date (in house)</u> 06-Jun-08 (in house check)	wing pages and a	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Scheduled Check In house check: Jun-09 Circature	
This calibration certificate documen The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards	Its the traceability to natio antices with confidence pr ed in the closed laboratory critical for calibration) ID # SN: 6295603 SN: 0810278 ID #	Cal Date (Certificate No.) 04-Oct-07 (No: 6465) 03-Oct-07 (No: 6465) Check Date (in house)	wing pages and a	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Scheduled Check In house check: Jun-09 Circature	
This calibration certificate documen The measurements and the uncerta All calibrations have been conducte Calibration Equipment used (M&TE Primary Standards Fluke Process Calibrator Type 702 Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V1.1	Its the traceability to natio anties with confidence pr ed in the closed laboratory critical for calibration) ID # SN: 6295603 SN: 0810278 ID # SE UMS 006 AB 1004	obability are given on the follow y facility: environment tempera <u>Cal Date (Certificate No.)</u> 04-Oct-07 (No: 6467) 03-Oct-07 (No: 6465) <u>Check Date (in house)</u> 06-Jun-08 (in house check) Function.	wing pages and a	are part of the certificate. and humidity < 70%. Scheduled Calibration Oct-08 Oct-08 Scheduled Check In house check: Jun-09	



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





- S Schweizerischer Kalibrierdienst
- C Service suisse d'étalonnage
- Servizio svizzero di taratura Suiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE Connector angle

data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a
 result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-778_Sep08

Page 2 of 5

1.16



DC Voltage Measurement

A/D - Converter Resi	olution nominal			
High Range:	1LSB =	6.1µV.	full range =	-100+300 mV
Low Range:	1LSB =	61nV .	full range =	-1+3mV
DASY measurement	parameters: Aut	to Zero Time: 3	sec; Measuring	time: 3 sec

Calibration Factors	x	Y	z
High Range	404.686 ± 0.1% (k=2)	403.490 ± 0.1% (k=2)	405.045 ± 0.1% (k=2)
Low Range	3.99455 ± 0.7% (k=2)	3.96369 ± 0.7% (k=2)	3.99417 ± 0.7% (k=2)

Connector Angle

Connector Angle to be used in DASY system	309 ° ± 1 °
---	-------------

Certificate No: DAE4-778_Sep08

Page 3 of 5



Appendix

1.	DC	Voltage	Linearity
	~~	* ortago	Linoany

High Range	Input (µV)	Reading (µV)	Error (%)
Channel X + Input	200000	200000.3	0.00
Channel X + Input	20000	20004.24	0.02
Channel X - Input	20000	-20002.46	0.01
Channel Y + Input	200000	200000.4	0.00
Channel Y + Input	20000	20002.60	0.01
Channel Y - Input	20000	-20002.26	0.01
Channel Z + Input	200000	200000.6	0.00
Channel Z + Input	20000	20000.78	0.00
Channel Z - Input	20000	-20005.75	0.03
Low Range	Input (µV)	Reading (µV)	Error (%)
Channel X + Input	2000	2000	0.00
Channel X + Input	200	199.37	-0.31
Channel X - Input	200	-200.28	0.14
Channel Y + Input	2000	2000	0.00
Channel Y + Input	200	199.63	-0.19
Channel Y - Input	200	-200.88	0.44
Channel Z + Input	2000	2000.1	0.00
Channel Z + Input	200	198.60	-0.70

2. Common mode sensitivity

- Input

Channel Z

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (µV)
Channel X	200	-7.46	-6.40
	- 200	10.00	6.86
Channel Y	200	-2.73	-2.45
	- 200	0.84	0.43
Channel Z	200	-10.91	-10.94
	- 200	7.89	8,22

200

-201.07

0.53

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200		3.08	-1.34
Channel Y	200	1.18		4.64
Channel Z	200	-1.74	1,44	

Certificate No: DAE4-778_Sep08

Page 4 of 5



4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16048	16021
Channel Y	16167	15166
Channel Z	16416	15977

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input 10M $\!\Omega$

	Average (µV)	min. Offset (µV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	-0.13	-0.88	0.92	0.33
Channel Y	-0.88	-2.47	0.72	0.55
Channel Z	-1,16	-2.17	-0.19	0.42

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance

	Zeroing (MOhm)	Measuring (MOhm)
Channel X	0.2000	201.1
Channel Y	0.2000	201.0
Channel Z	0.2001	201.7

8. Low Battery Alarm Voltage (verified during pre test)

Typical values	Alarm Level (VDC)		
Supply (+ Vcc)	•	+7.9	
Supply (- Vcc)	3	-7.6	

9. Power Consumption (verified during pre test)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.0	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE4-778_Sep08

Page 5 of 5



Test Report No : FA8N1310

Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



 S
 Schweizerischer Kalibrierdienst

 C
 Service suisse d'étalonnage

 Servizio svizzero di taratura

 S wiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client Sporton (Auden)

Certificate No: ET3-1788_Sep08

Accreditation No.: SCS 108

Object	ET3DV6 - SN:1	788	
Calibration procedure(s)		and QA CAL-23.v3 edure for dosimetric E-field probe	S
Calibration date:	September 23, 2	2008	
Condition of the calibrated item	In Tolerance		
		bry facility: environment temperature $(22 \pm 3)^{\circ}$	C and humidity < 70%.
Calibration Equipment used (M&T	E critical for calibration)		
	E critical for calibration)	Cal Date (Certificate No.)	Scheduled Calibration
rimary Standards	ĩ	Cal Date (Certificate No.) 1-Apr-08 (No. 217-00788)	Scheduled Calibration Apr-09
rimary Standards ower meter E4419B	ID #	and the second	and the set of provide and the set of the set
rimary Standards ower meter E4419B ower sensor E4412A	ID # GB41293874	1-Apr-08 (No. 217-00788)	Apr-09
rimary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A	ID # GB41293874 MY41495277	1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788)	Apr-09 Apr-09
rimary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A leference 3 dB Attenuator	ID # GB41293874 MY41495277 MY41498087	1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788)	Apr-09 Apr-09 Apr-09
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c)	1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00865)	Apr-09 Apr-09 Apr-09 Jul-09
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b)	1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00865) 31-Mar-08 (No. 217-00787)	Apr-09 Apr-09 Apr-09 Jul-09 Apr-09
rimary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A teference 3 dB Attenuator teference 20 dB Attenuator teference 30 dB Attenuator teference Probe ES3DV2	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b)	1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00865) 31-Mar-08 (No. 217-00787) 1-Jul-08 (No. 217-00866)	Apr-09 Apr-09 Apr-09 Jul-09 Apr-09 Jul-09
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID #	1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00865) 31-Mar-08 (No. 217-00866) 2-Jan-08 (No. ES3-3013_Jan08) 9-Sep-08 (No. DAE4-660_Sep08) Check Date (in house)	Apr-09 Apr-09 Apr-09 Jul-09 Apr-09 Jul-09 Jan-09 Sep-09 Scheduled Check
rimary Standards ower meter E4419B ower sensor E4412A ower sensor E4412A telerence 3 dB Attenuator telerence 20 dB Attenuator telerence 30 dB Attenuator telerence Probe ES3DV2 tAE4 econdary Standards	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 660	1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00865) 31-Mar-08 (No. 217-00866) 2-Jan-08 (No. ES3-3013_Jan08) 9-Sep-08 (No. DAE4-660_Sep08)	Apr-09 Apr-09 Apr-09 Jul-09 Apr-09 Jul-09 Jan-09 Sep-09 Scheduled Check In house check: Oct-09
rimary Standards ower meter E44198 ower sensor E4412A ower sensor E4412A telerence 3 dB Attenuator telerence 20 dB Attenuator telerence 30 dB Attenuator telerence Probe ES3DV2 AE4 econdary Standards F generator HP 8648C	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID #	1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00865) 31-Mar-08 (No. 217-00866) 2-Jan-08 (No. ES3-3013_Jan08) 9-Sep-08 (No. DAE4-660_Sep08) Check Date (in house)	Apr-09 Apr-09 Apr-09 Jul-09 Apr-09 Jul-09 Jan-09 Sep-09 Scheduled Check
Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700	1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00865) 31-Mar-08 (No. 217-00866) 2-Jan-08 (No. 217-00866) 2-Jan-08 (No. ES3-3013_Jan08) 9-Sep-08 (No. DAE4-660_Sep08) Check Date (in house) 4-Aug-99 (in house check Oct-07)	Apr-09 Apr-09 Apr-09 Jul-09 Apr-09 Jul-09 Jan-09 Sep-09 Scheduled Check In house check: Oct-09
Primary Standards Power meter E44198 Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700 US37390585	1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00865) 31-Mar-08 (No. 217-00866) 2-Jan-08 (No. 217-00866) 2-Jan-08 (No. ES3-3013_Jan08) 9-Sep-08 (No. DAE4-660_Sep08) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-07)	Apr-09 Apr-09 Apr-09 Jul-09 Apr-09 Jul-09 Jan-09 Sep-09 Scheduled Check In house check: Oct-09 In house check: Oct-08
Calibration Equipment used (M&T Primary Standards Power meter E4419B Power sensor E4412A Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference 90 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E Calibrated by:	ID # GB41293874 MY41495277 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 660 ID # US3642U01700 US37390585 Name	1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Apr-08 (No. 217-00788) 1-Jul-08 (No. 217-00865) 31-Mar-08 (No. 217-00866) 2-Jan-08 (No. 217-00866) 2-Jan-08 (No. ES3-3013_Jan08) 9-Sep-08 (No. DAE4-660_Sep08) Check Date (in house) 4-Aug-99 (in house check Oct-07) 18-Oct-01 (in house check Oct-07) Function	Apr-09 Apr-09 Apr-09 Jul-09 Apr-09 Jul-09 Jan-09 Sep-09 Scheduled Check In house check: Oct-09 In house check: Oct-08

Certificate No: ET3-1788_Sep08

Page 1 of 9



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





- S Schweizerischer Kalibrierdienst Service suisse d'étalonnage
- C Service suisse d'etalonnage Servizio svizzero di taratura

S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
Polarization ϕ	φ rotation around probe axis
Polarization 9	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx, y, z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx, y, z are only intermediate values, i.e., the uncertainties of NORMx, y, z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This
 linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of
 the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: ET3-1788_Sep08

Page 2 of 9



September 23, 2008

Probe ET3DV6

SN:1788

Manufactured: Last calibrated: Recalibrated:

ī.

May 28, 2003 September 26, 2007 September 23, 2008

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

÷

Certificate No: ET3-1788 Sep08

Page 3 of 9



September 23, 2008

DASY - Parameters of Probe: ET3DV6 SN:1788

Sensitivity in Free	e Space ^A		Diode C	compression ^B
NormX	1.73 ± 10.1%	μ V/(V/m) ²	DCP X	95 mV
NormY	1.59 ± 10.1%	μ V/(V/m) ²	DCP Y	98 mV
NormZ	1.72 ± 10.1%	μV/(V/m) ²	DCP Z	91 mV
Sensitivity in Tiss	ue Simulating Li	quid (Convers	ion Factors)	
Please see Page 8.				

Boundary Effect

TSL

900 MHz Typical SAR gradient: 5 % per mm

Sensor Cente	er to Phantom Surface Distance	3.7 mm	4.7 mm
SAR _{be} [%]	Without Correction Algorithm	10.6	6.8
SAR _{be} [%]	With Correction Algorithm	0.8	0.3

TSL 1750 MHz Typical SAR gradient: 10 % per mm

Sensor Cente	r to Phantom Surface Distance	3.7 mm	4.7 mm
SAR _{be} [%]	Without Correction Algorithm	8.8	4.9
SAR _{be} [%]	With Correction Algorithm	0.7	0.6

Sensor Offset

Probe Tip to Sensor Center

2.7 mm

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Page 8).


⁸ Numerical linearization parameter: uncertainty not required.

Certificate No: ET3-1788_Sep08

Page 4 of 9



September 23, 2008

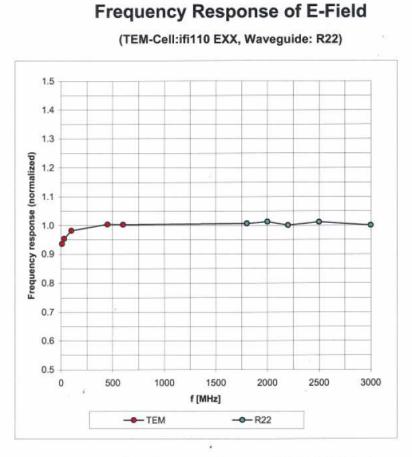


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: ET3-1788_Sep08


Page 5 of 9



September 23, 2008

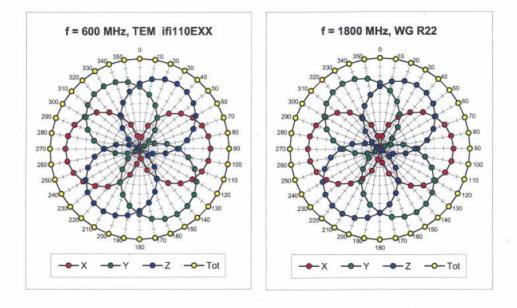

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

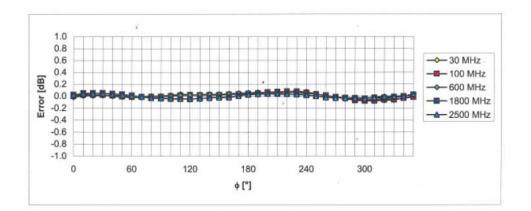


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: ET3-1788_Sep08

Page 6 of 9



September 23, 2008

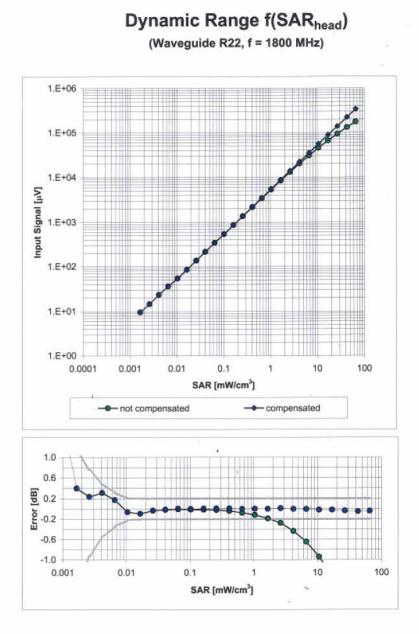


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: ET3-1788_Sep08

Page 7 of 9



September 23, 2008

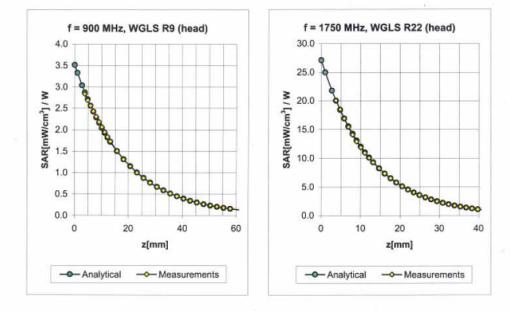

Conversion Factor Assessment

f [MHz]	Validity [MHz] ^c	TSL	Permittivity	Conductivity	Alpha	Depth	ConvF Uncertainty
900	± 50 / ± 100	Head	41.5 ± 5%	0.97 ± 5%	0.44	2.65	6.55 ± 11.0% (k=2)
1750	± 50 / ± 100	Head	40.1 ± 5%	1.37 ± 5%	0.68	1.98	5.59 ± 11.0% (k=2)
1950	± 50 / ± 100	Head	40.0 ± 5%	1.40 ± 5%	0.75	1.75	5.13 ± 11.0% (k=2)
2450	± 50 / ± 100	Head	39.2 ± 5%	1.80 ± 5%	0.80	1.45	4.68 ± 11.0% (k=2)
				÷			
900	± 50 / ± 100	Body	55.0 ± 5%	1.05 ± 5%	0.50	. 2.48	6.34 ± 11.0% (k=2)
1750	± 50 / ± 100	Body	53.4 ± 5%	1.49 ± 5%	0.63	2.33	4.87 ± 11.0% (k=2)
1950	± 50 / ± 100	Body	53.3 ± 5%	1.52 ± 5%	0.74	1.99	4.73 ± 11.0% (k=2)
2450	± 50 / ± 100	Body	52.7 ± 5%	1.95 ± 5%	0.94	1.75	3.98 ± 11.0% (k=2)


^C The validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

Certificate No: ET3-1788_Sep08


Page 8 of 9



September 23, 2008



Error (\, \,), f = 900 MHz

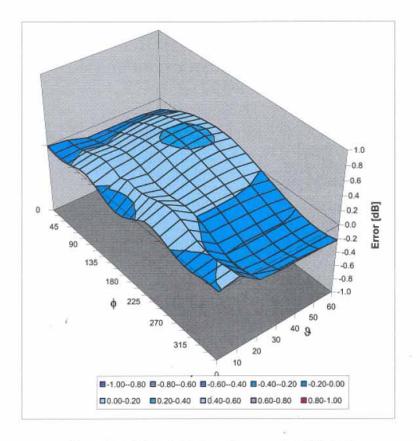

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Page 9 of 9