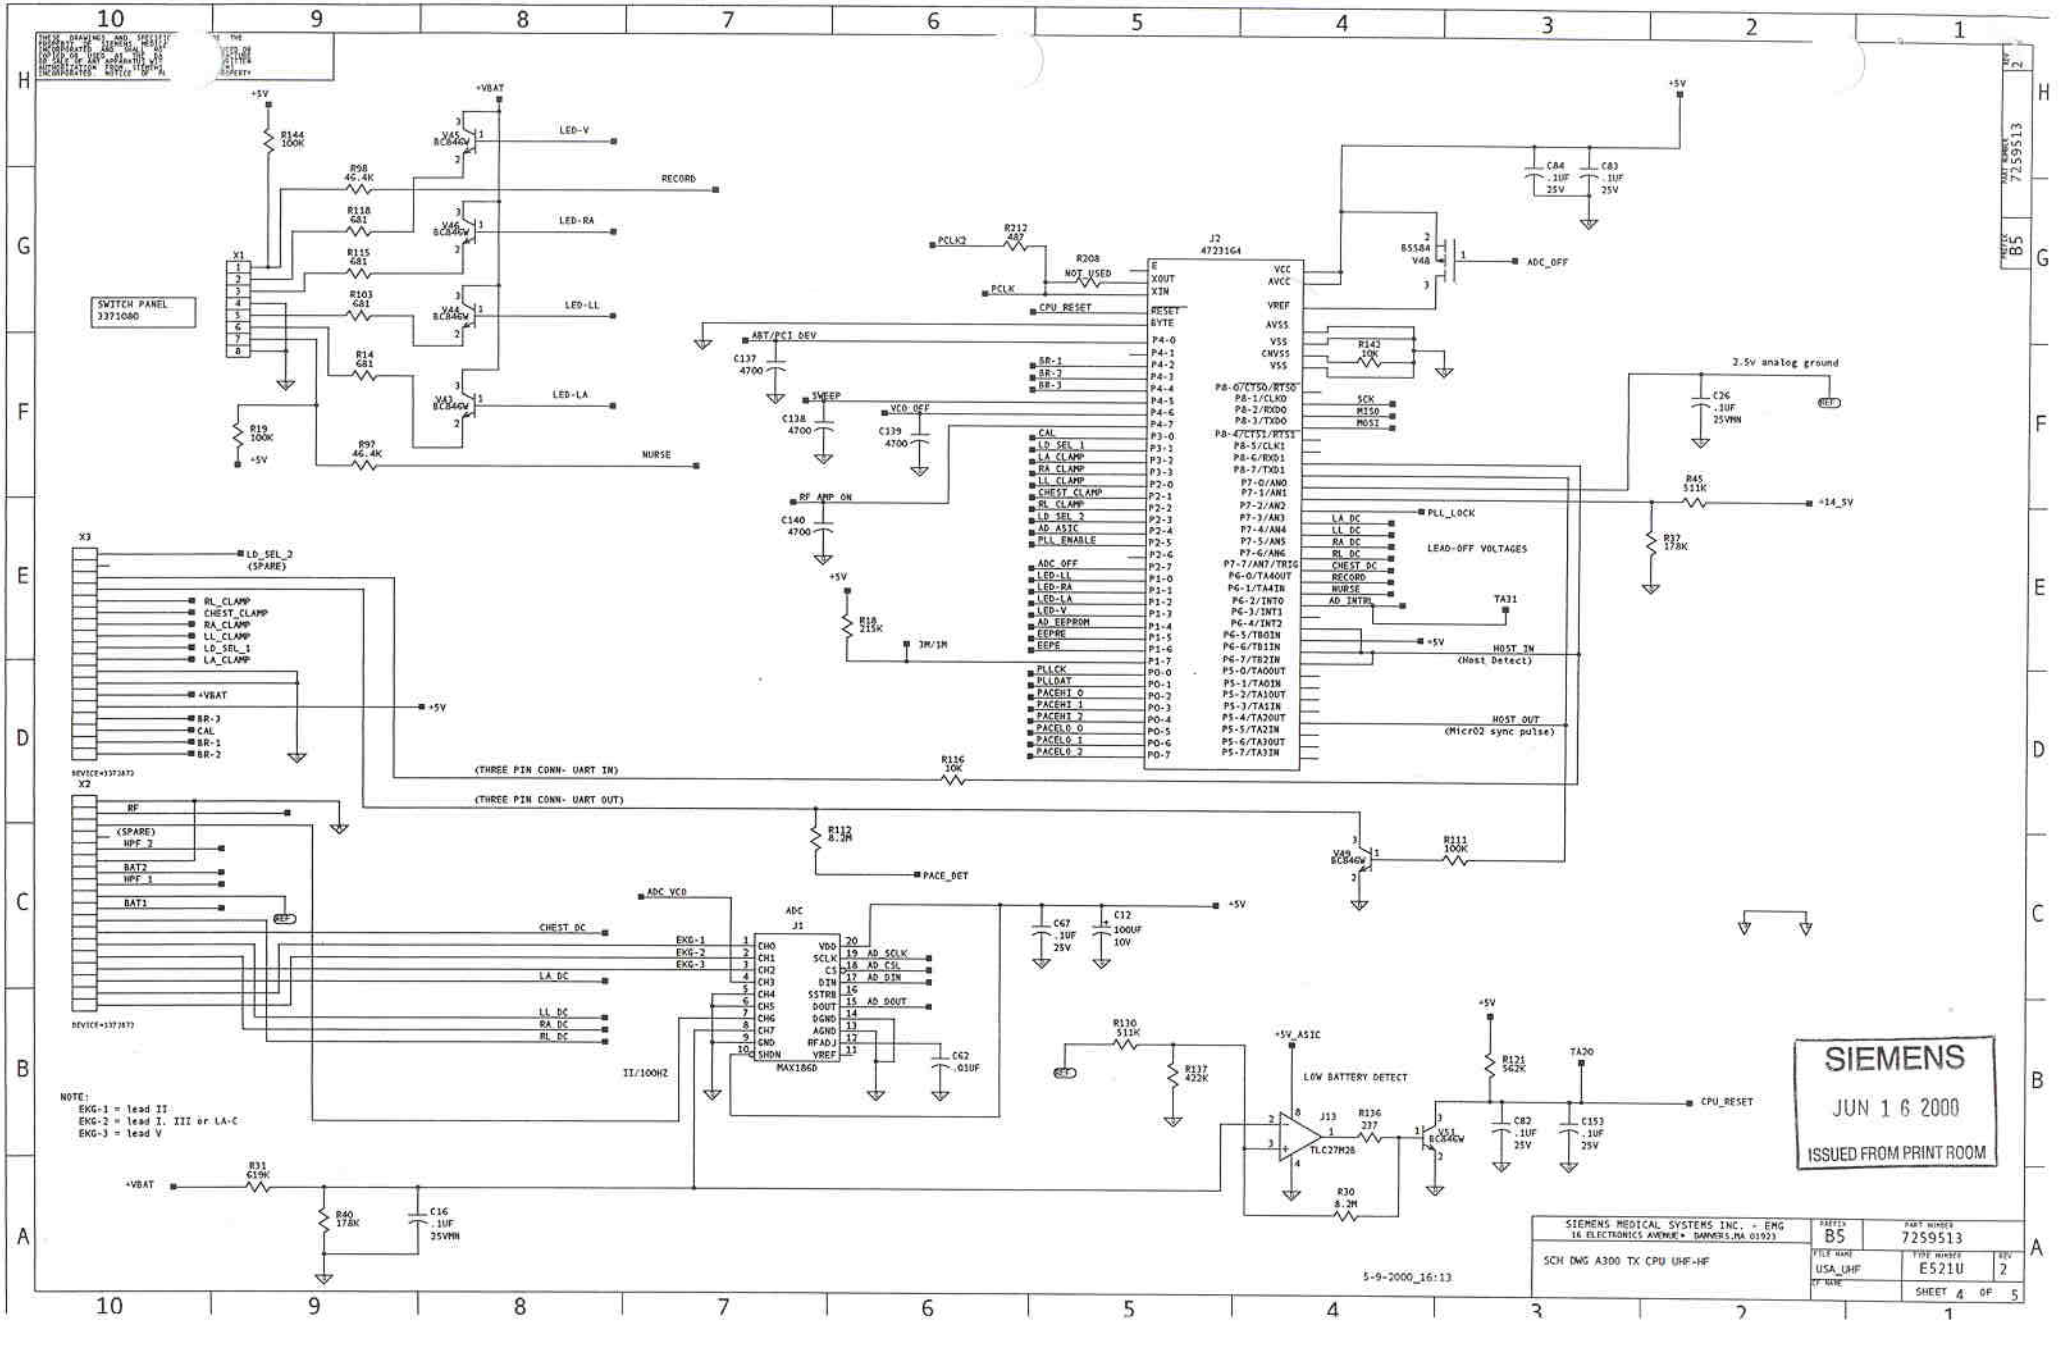
SWITCH PANEL
3371080
LED-V
RECORD
LED-RA
LED-LL
LED-LA
NURSE
J2
472316G4
ADC_OFF
2.5V analog ground
+14_5V
PLL_LOCK
LEAD-OFF VOLTAGES
HOST_IN
(Host Detect)
HOST_OUT
(Micro2 sync pulse)
(THREE PIN CONN- UART IN)
(THREE PIN CONN- UART OUT)
PACE_DET
ADC
J1
MAX186D
LOW BATTERY DETECT
CPU_RESET
NOTE:
EKG-1 = lead II
EKG-2 = lead I, III or LA-C
EKG-3 = lead V
SIEMENS
JUN 16 2000
ISSUED FROM PRINT ROOM
SIEMENS MEDICAL SYSTEMS INC. - EMG
16 ELECTRONICS AVENUE • DANVERS,MA 01923
SCH DWG A300 TX CPU UHF-HF
PREFIX B5
PART NUMBER 7259513
FILE NAME USA_UHF
TYPE NUMBER E521U
REV 2
SHEET 4 OF 5
5-9-2000_16:13