

## System Check\_Head\_750MHz

**DUT:D750V3 - SN:1087**

Communication System: ; Frequency: 750.000

Medium: HSL. Medium parameters used:  $f= 750.000$  MHz;  $\sigma= 0.925$  S/m;  $\epsilon_r = 42.4$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(10.97, 10.97, 10.97); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.444 W/kg; SAR (10g) = 0.296 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 0.436 W/kg; SAR (10g) = 0.284 W/kg;

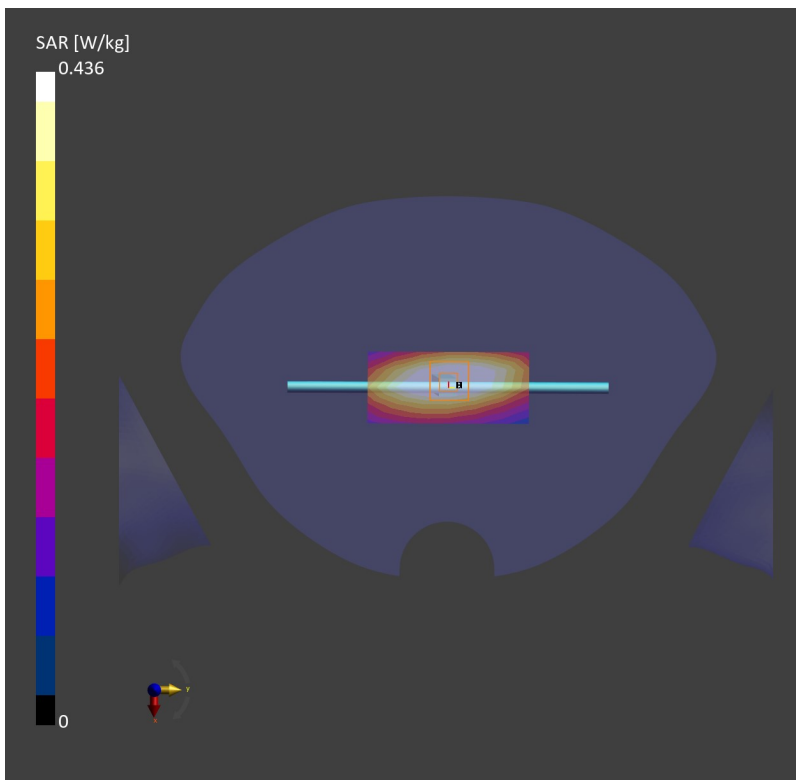

## System Check\_Head\_835MHz

### DUT:D835V2 - SN:4d091

Communication System: ; Frequency: 835.000

Medium: HSL. Medium parameters used:  $f = 835.000$  MHz;  $\sigma = 0.915$  S/m;  $\epsilon_r = 41.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(10.67, 10.67, 10.67); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.506 W/kg; SAR (10g) = 0.333 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 0.500 W/kg; SAR (10g) = 0.323 W/kg;

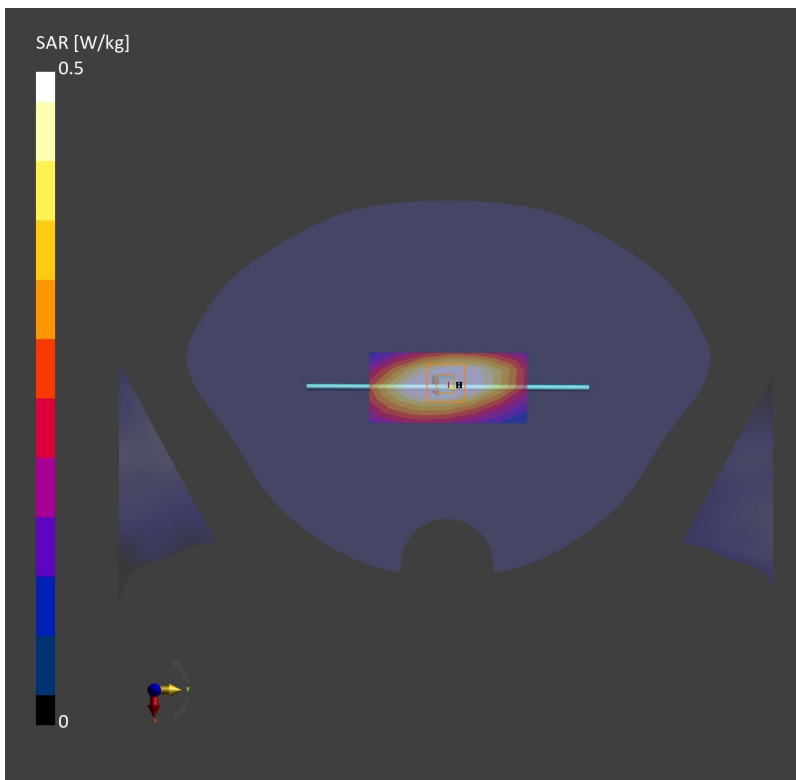

## System Check\_Head\_1750MHz

### DUT:D1750V2 - SN:1090

Communication System: ; Frequency: 1750.000

Medium: HSL. Medium parameters used:  $f= 1750.000$  MHz;  $\sigma= 1.38$  S/m;  $\epsilon_r = 40.2$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.31, 9.31, 9.31); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.92 W/kg; SAR (10g) = 1.04 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.88 W/kg; SAR (10g) = 0.988 W/kg;

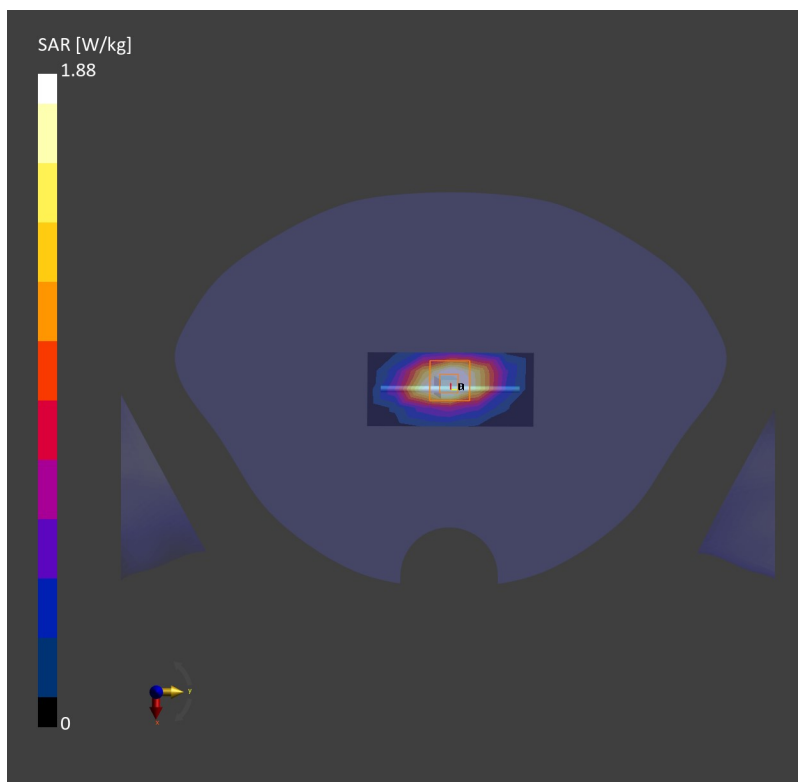

## System Check\_Head\_1900MHz

### DUT:D1900V2 - SN:5d118

Communication System: ; Frequency: 1900.000

Medium: HSL. Medium parameters used:  $f= 1900.000$  MHz;  $\sigma= 1.45$  S/m;  $\epsilon_r = 39.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.89, 8.89, 8.89); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.10 W/kg; SAR (10g) = 1.11 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.08 W/kg; SAR (10g) = 1.07 W/kg;

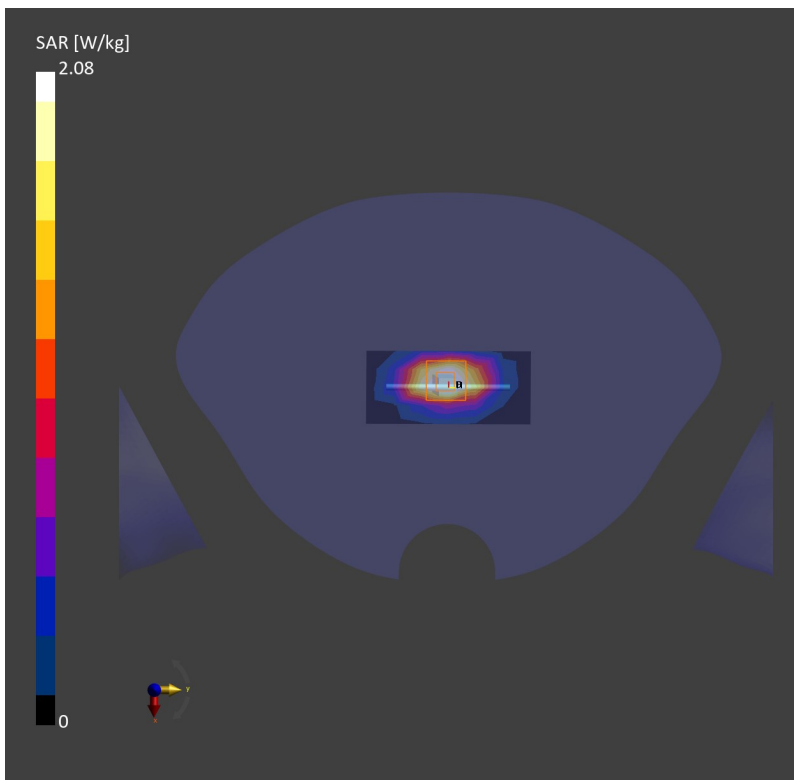

## System Check\_Head\_2450MHz

**DUT:D2450V2 - SN:1040**

Communication System: ; Frequency: 2450.000

Medium: HSL. Medium parameters used:  $f= 2450.000$  MHz;  $\sigma= 1.85$  S/m;  $\epsilon_r = 39.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.38, 8.38, 8.38); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.69 W/kg; SAR (10g) = 1.24 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.68 W/kg; SAR (10g) = 1.24 W/kg;

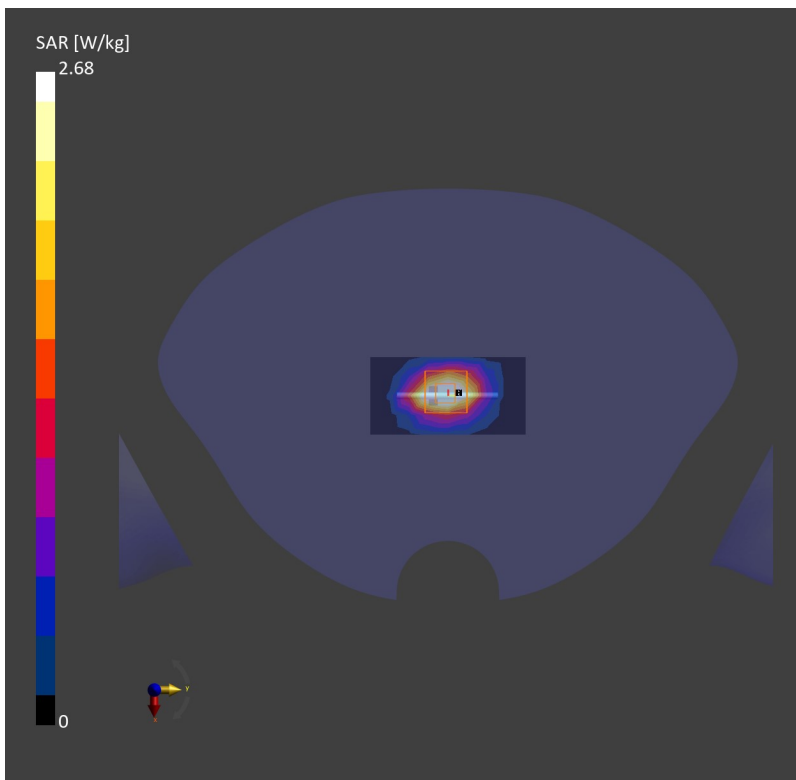

## System Check\_Head\_2600MHz

### DUT:D2600V2 - SN:1061

Communication System: ; Frequency: 2600.000

Medium: HSL. Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 1.93$  S/m;  $\epsilon_r = 39.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.1, 8.1, 8.1); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.67 W/kg; SAR (10g) = 1.23 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.69 W/kg; SAR (10g) = 1.18 W/kg;

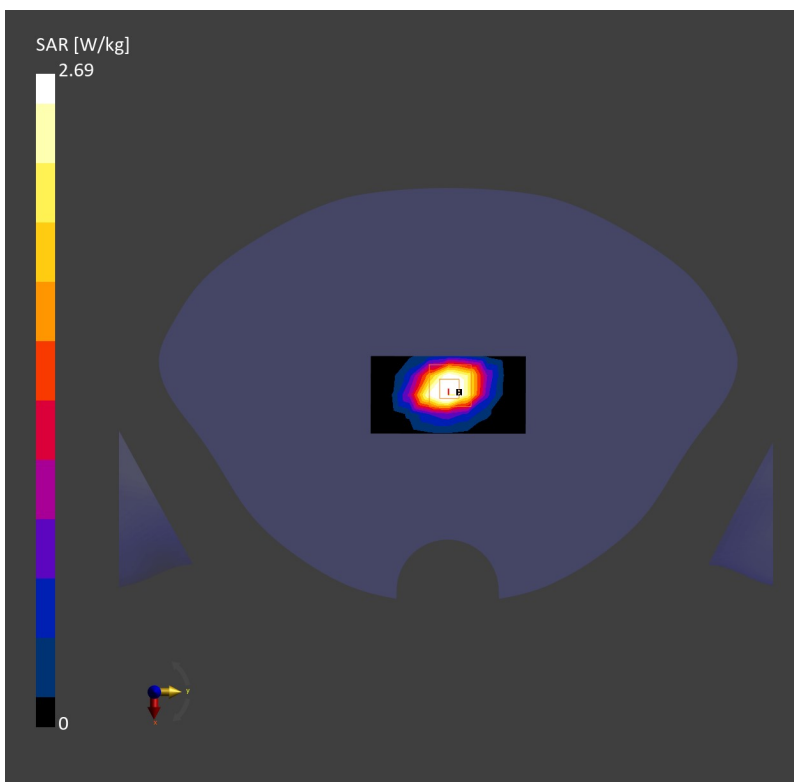

## System Check\_Head\_3500MHz

### DUT:D3500V2 - SN:1037

Communication System: ; Frequency: 3500.000

Medium: HSL. Medium parameters used:  $f= 3500.000$  MHz;  $\sigma= 2.80$  S/m;  $\epsilon_r = 39.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.68, 7.68, 7.68); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.17 W/kg; SAR (10g) = 1.23 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.20 W/kg;

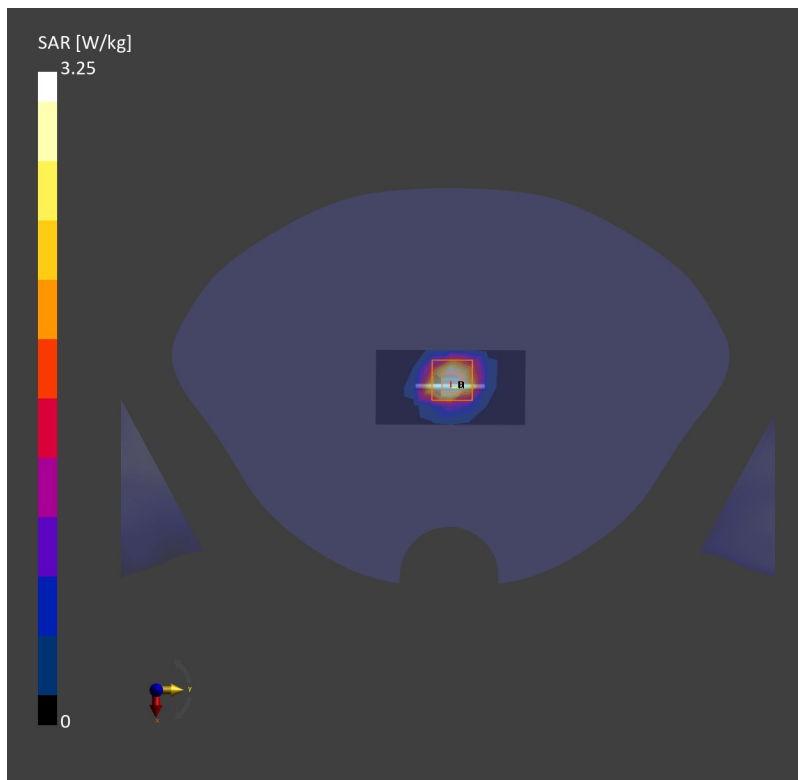

## System Check\_Head\_3700MHz

### DUT:D3700V2 - SN:1008

Communication System: ; Frequency: 3700.000

Medium: HSL. Medium parameters used:  $f= 3700.000$  MHz;  $\sigma= 2.98$  S/m;  $\epsilon_r = 38.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.61, 7.61, 7.61); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.29 W/kg; SAR (10g) = 1.22 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.31 W/kg; SAR (10g) = 1.21 W/kg;

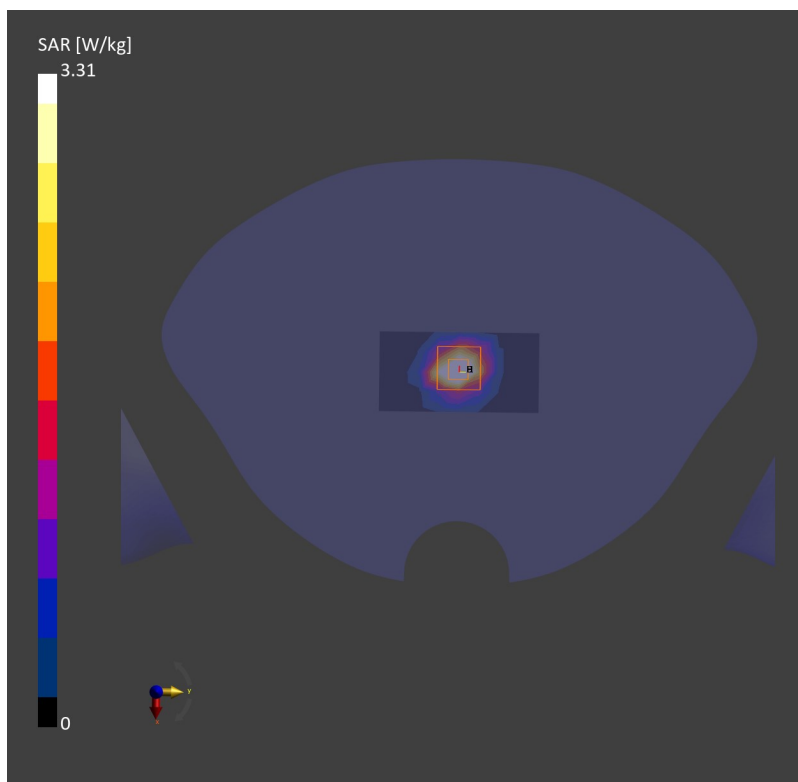



## System Check\_Head\_3900MHz

### DUT:D3900V2 - SN:1048

Communication System: ; Frequency: 3900.000

Medium: HSL. Medium parameters used:  $f= 3900.000$  MHz;  $\sigma= 3.28$  S/m;  $\epsilon_r = 37.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.31, 7.31, 7.31); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.27 W/kg; SAR (10g) = 1.16 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.16 W/kg;

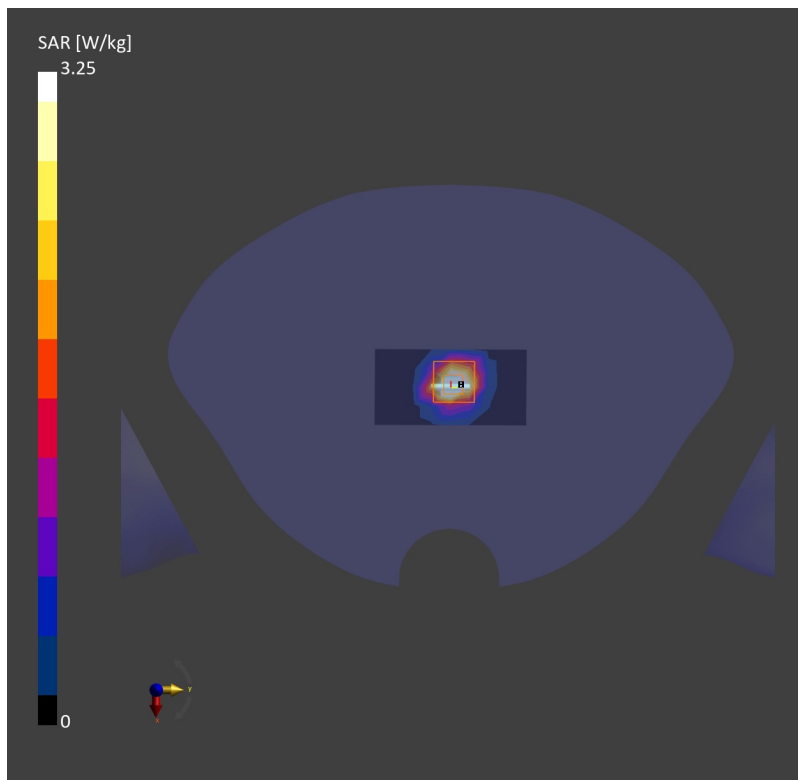

## System Check\_Head\_5250MHz

### DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5250.000

Medium: HSL. Medium parameters used:  $f = 5250.000$  MHz;  $\sigma = 4.56$  S/m;  $\epsilon_r = 35.0$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.18, 6.18, 6.18); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.51 W/kg; SAR (10g) = 1.00 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.82 W/kg; SAR (10g) = 1.09 W/kg;

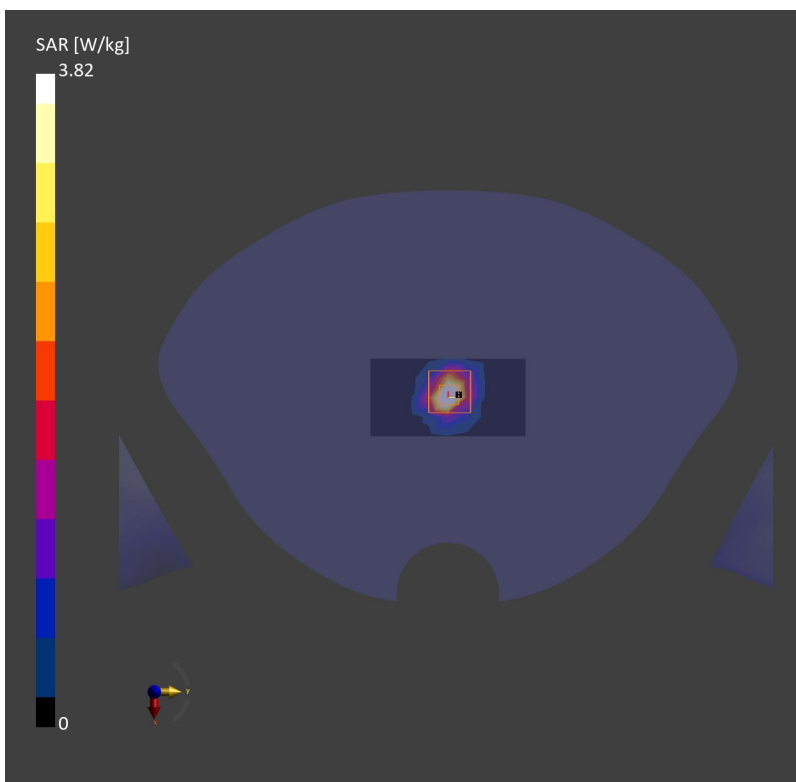

## System Check\_Head\_5600MHz

### DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5600.000

Medium: HSL. Medium parameters used:  $f= 5600.000$  MHz;  $\sigma= 4.95$  S/m;  $\epsilon_r = 34.4$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.39, 5.39, 5.39); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.82 W/kg; SAR (10g) = 1.08 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.97 W/kg; SAR (10g) = 1.12 W/kg;

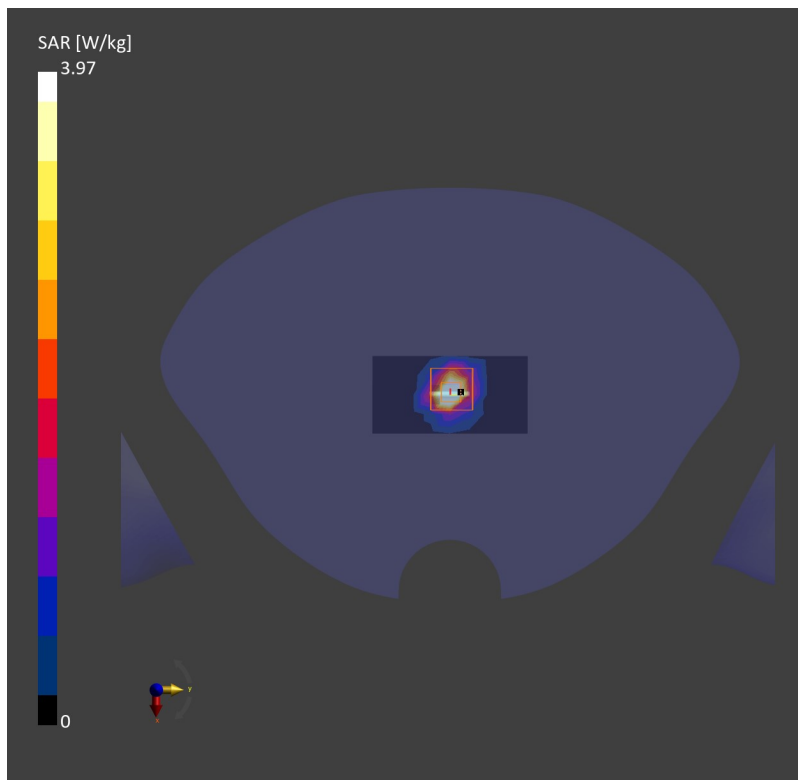

## System Check\_Head\_5750MHz

### DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5750.000

Medium: HSL. Medium parameters used:  $f= 5750.000$  MHz;  $\sigma= 5.12$  S/m;  $\epsilon_r = 34.1$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.57, 5.57, 5.57); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.42 W/kg; SAR (10g) = 0.976 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.82 W/kg; SAR (10g) = 1.09 W/kg;

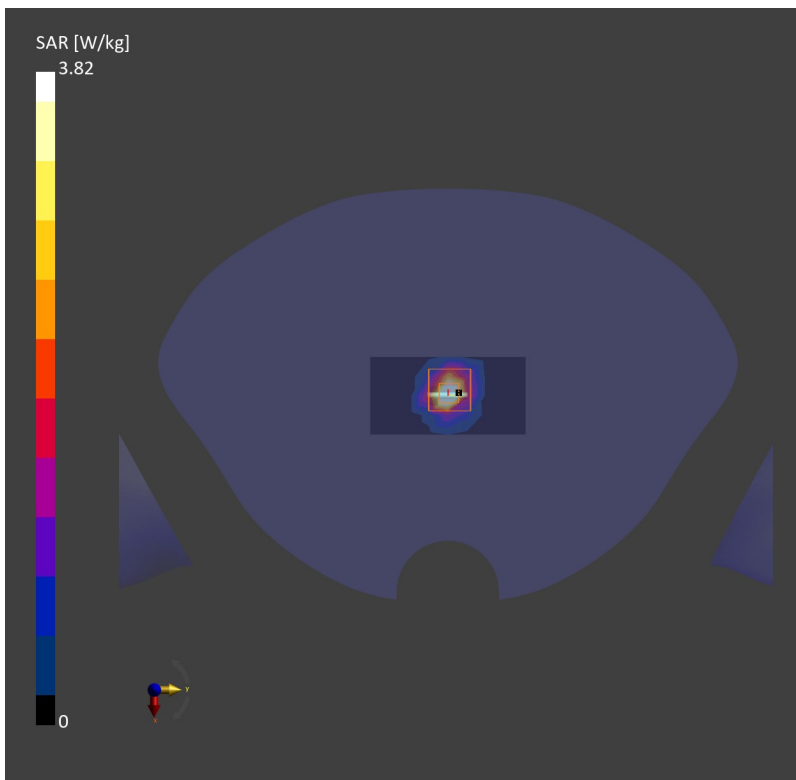

## System Check\_Head\_750MHz

**DUT:D750V3 - SN:1087**

Communication System: ; Frequency: 750.000

Medium: HSL. Medium parameters used:  $f= 750.000$  MHz;  $\sigma= 0.926$  S/m;  $\epsilon_r = 42.4$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(10.97, 10.97, 10.97); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.443 W/kg; SAR (10g) = 0.295 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 0.437 W/kg; SAR (10g) = 0.284 W/kg;

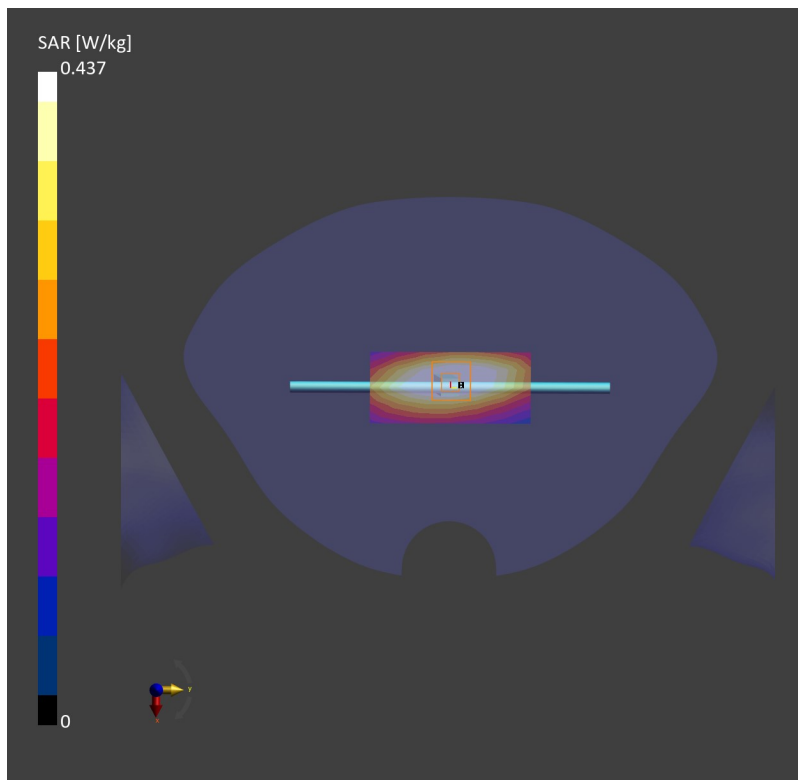

## System Check\_Head\_835MHz

### DUT:D835V2 - SN:4d091

Communication System: ; Frequency: 835.000

Medium: HSL. Medium parameters used:  $f = 835.000$  MHz;  $\sigma = 0.934$  S/m;  $\epsilon_r = 41.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(10.67, 10.67, 10.67); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.517 W/kg; SAR (10g) = 0.339 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.09 dB

SAR (1g) = 0.501 W/kg; SAR (10g) = 0.330 W/kg;

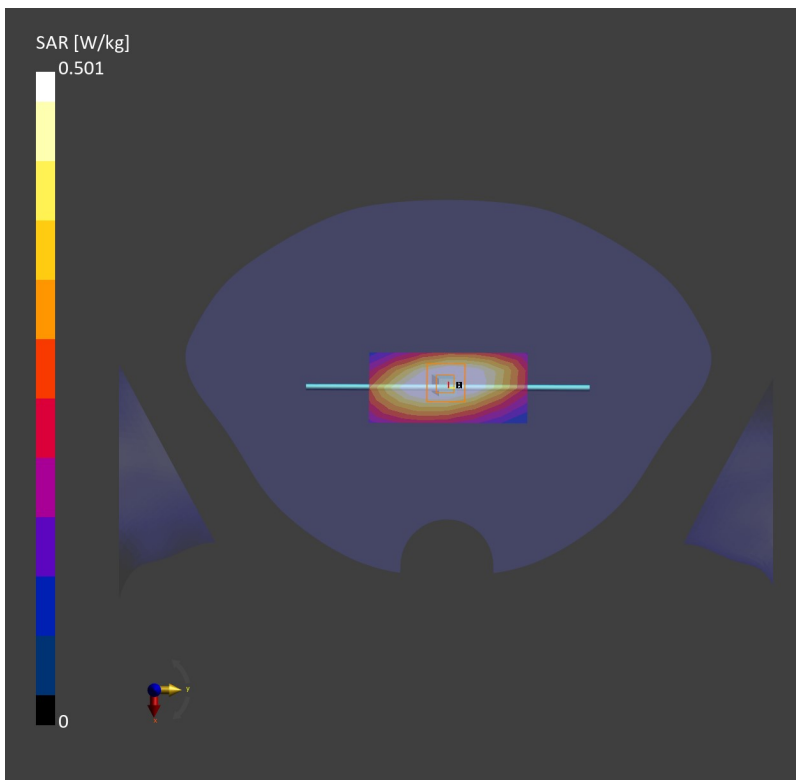

## System Check\_Head\_1750MHz

### DUT:D1750V2 - SN:1090

Communication System: ; Frequency: 1750.000

Medium: HSL. Medium parameters used:  $f= 1750.000$  MHz;  $\sigma= 1.38$  S/m;  $\epsilon_r = 40.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.31, 9.31, 9.31); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.92 W/kg; SAR (10g) = 1.04 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.990 W/kg;

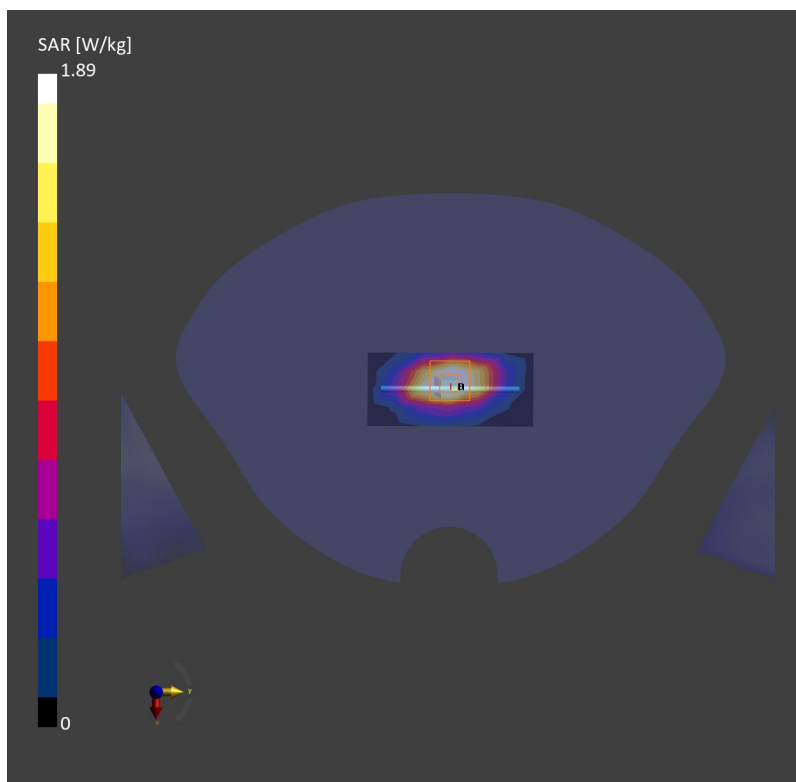

## System Check\_Head\_1900MHz

### DUT:D1900V2 - SN:5d118

Communication System: ; Frequency: 1900.000

Medium: HSL. Medium parameters used:  $f= 1900.000$  MHz;  $\sigma= 1.45$  S/m;  $\epsilon_r = 40.0$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.89, 8.89, 8.89); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.11 W/kg; SAR (10g) = 1.11 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.03 dB

SAR (1g) = 2.04 W/kg; SAR (10g) = 1.05 W/kg;

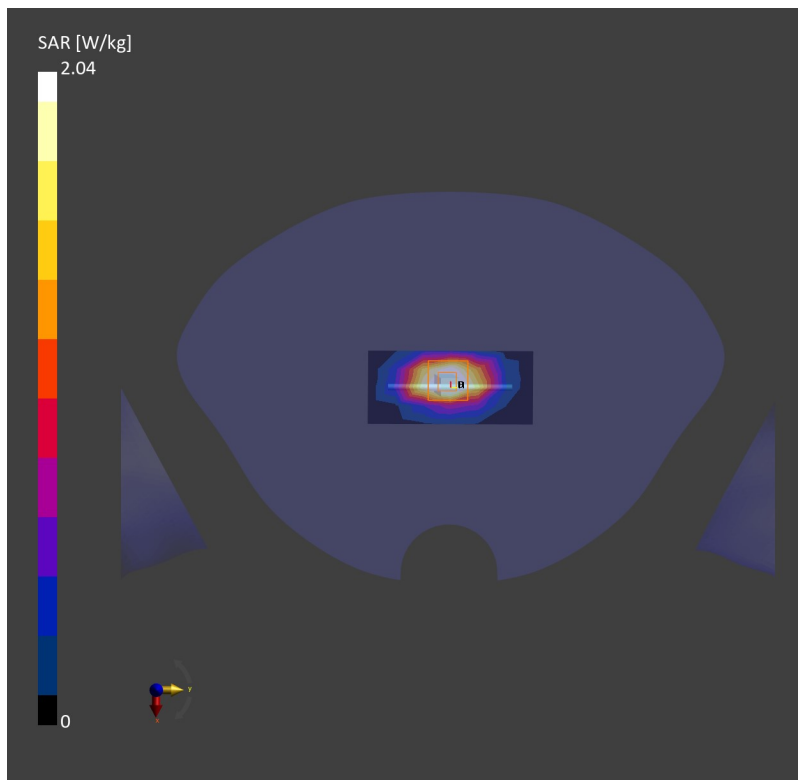



## System Check\_Head\_2450MHz

### DUT:D2450V2 - SN:1040

Communication System: ; Frequency: 2450.000

Medium: HSL. Medium parameters used:  $f = 2450.000$  MHz;  $\sigma = 1.86$  S/m;  $\epsilon_r = 38.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.38, 8.38, 8.38); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.67 W/kg; SAR (10g) = 1.23 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.66 W/kg; SAR (10g) = 1.23 W/kg;

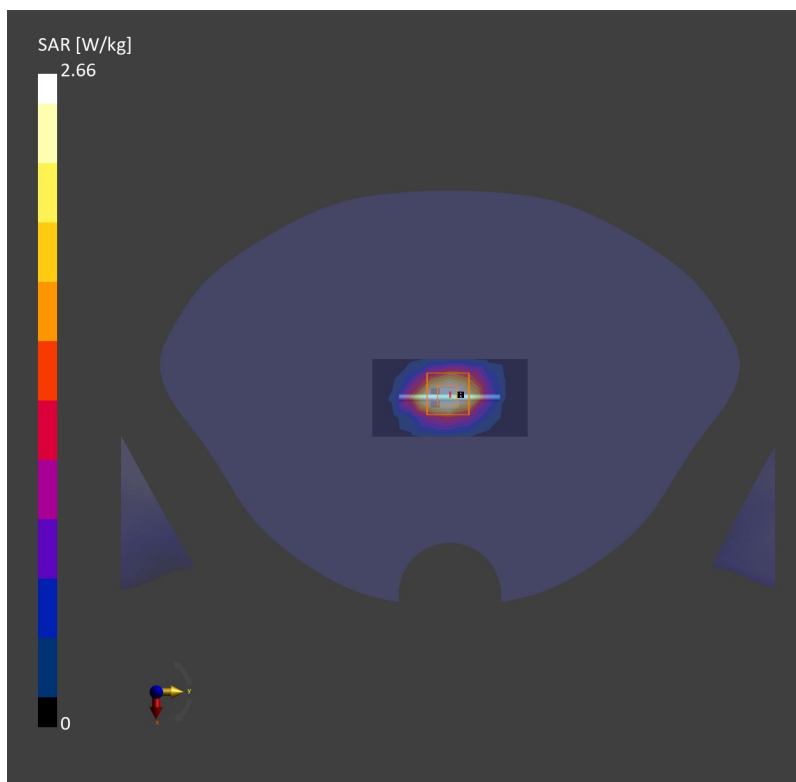

## System Check\_Head\_2600MHz

### DUT:D2600V2 - SN:1061

Communication System: ; Frequency: 2600.000

Medium: HSL. Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 1.94$  S/m;  $\epsilon_r = 39.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.1, 8.1, 8.1); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.67 W/kg; SAR (10g) = 1.23 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.73 W/kg; SAR (10g) = 1.19 W/kg;

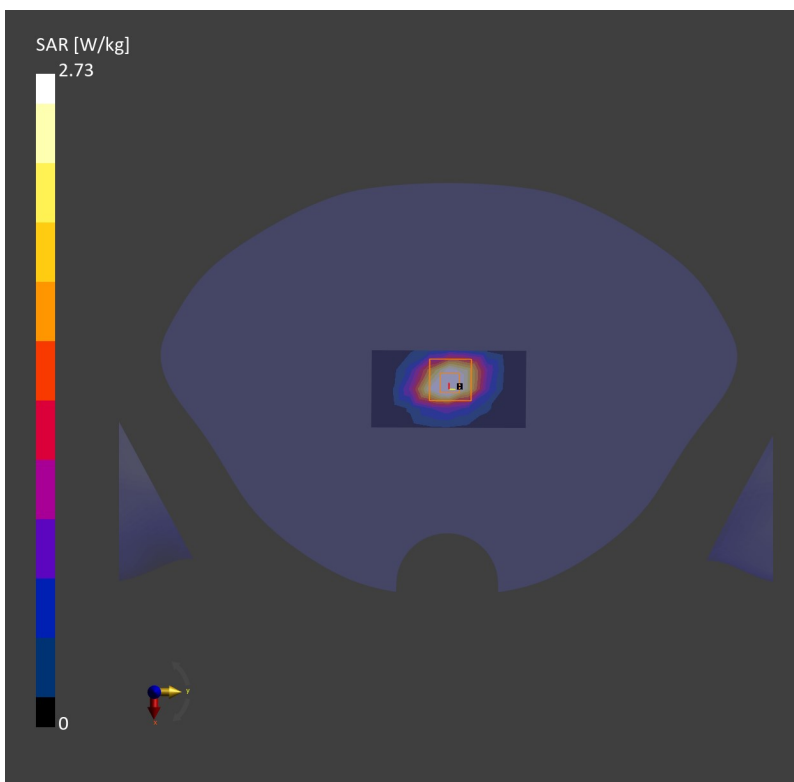

## System Check\_Head\_3500MHz

### DUT:D3500V2 - SN:1037

Communication System: ; Frequency: 3500.000

Medium: HSL. Medium parameters used:  $f = 3500.000$  MHz;  $\sigma = 2.81$  S/m;  $\epsilon_r = 39.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.68, 7.68, 7.68); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.20 W/kg; SAR (10g) = 1.24 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.17 W/kg; SAR (10g) = 1.20 W/kg;

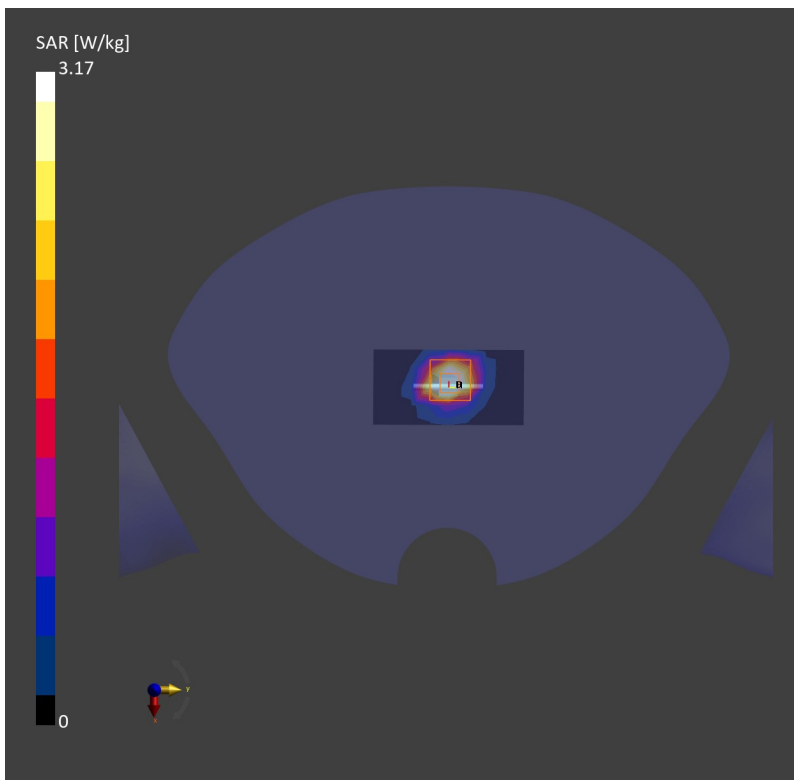

## System Check\_Head\_3700MHz

### DUT:D3700V2 - SN:1008

Communication System: ; Frequency: 3700.000

Medium: HSL. Medium parameters used:  $f= 3700.000$  MHz;  $\sigma= 2.99$  S/m;  $\epsilon_r = 38.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.61, 7.61, 7.61); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.20 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.31 W/kg; SAR (10g) = 1.22 W/kg;

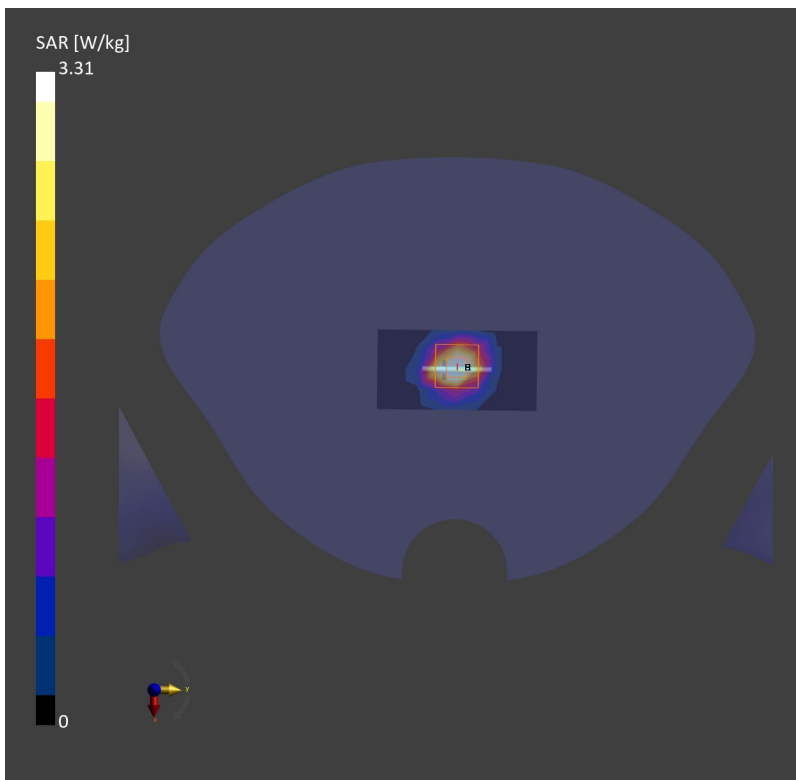

## System Check\_Head\_3900MHz

### DUT:D3900V2 - SN:1048

Communication System: ; Frequency: 3900.000

Medium: HSL. Medium parameters used:  $f= 3900.000$  MHz;  $\sigma= 3.25$  S/m;  $\epsilon_r = 37.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.31, 7.31, 7.31); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.21 W/kg; SAR (10g) = 1.14 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.27 W/kg; SAR (10g) = 1.14 W/kg;

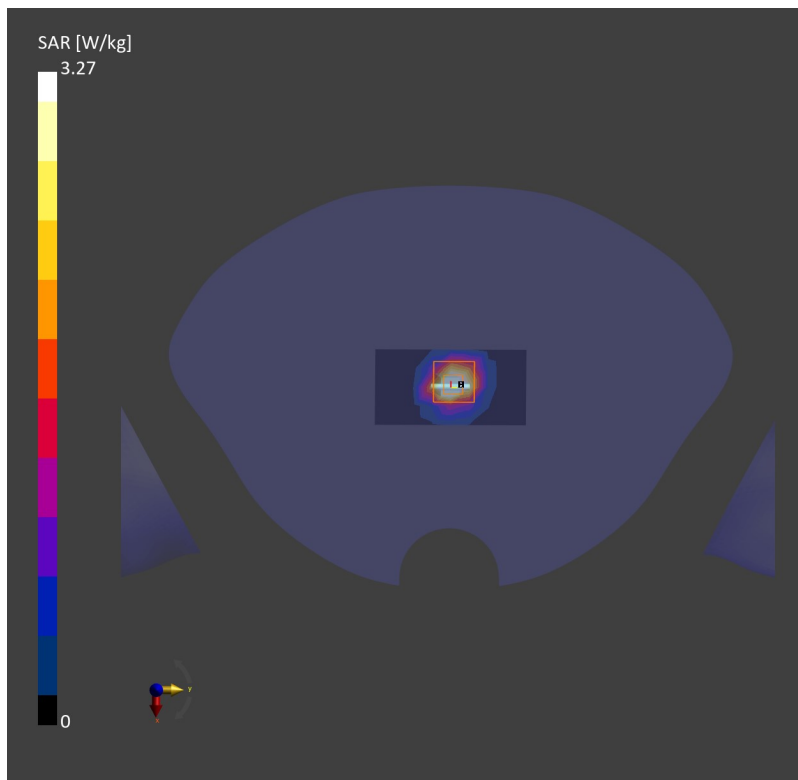

## System Check\_Head\_5250MHz

### DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5250.000

Medium: HSL. Medium parameters used:  $f = 5250.000$  MHz;  $\sigma = 4.73$  S/m;  $\epsilon_r = 36.0$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.18, 6.18, 6.18); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.61 W/kg; SAR (10g) = 1.03 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.85 W/kg; SAR (10g) = 1.09 W/kg;

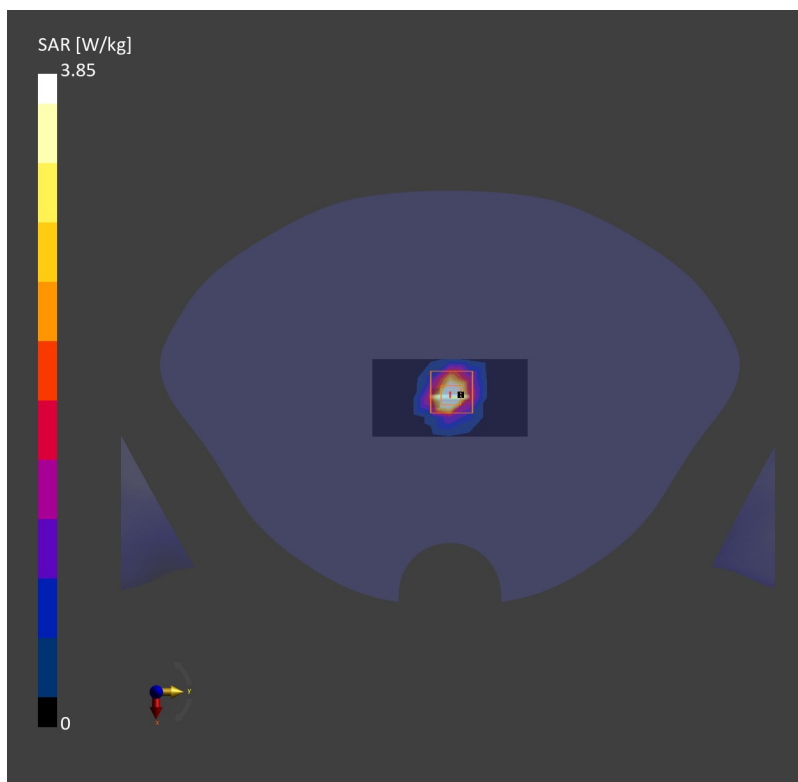

## System Check\_Head\_5600MHz

### DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5600.000

Medium: HSL. Medium parameters used:  $f= 5600.000$  MHz;  $\sigma= 5.15$  S/m;  $\epsilon_r = 35.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.39, 5.39, 5.39); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 4.04 W/kg; SAR (10g) = 1.14 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 4.15 W/kg; SAR (10g) = 1.17 W/kg;

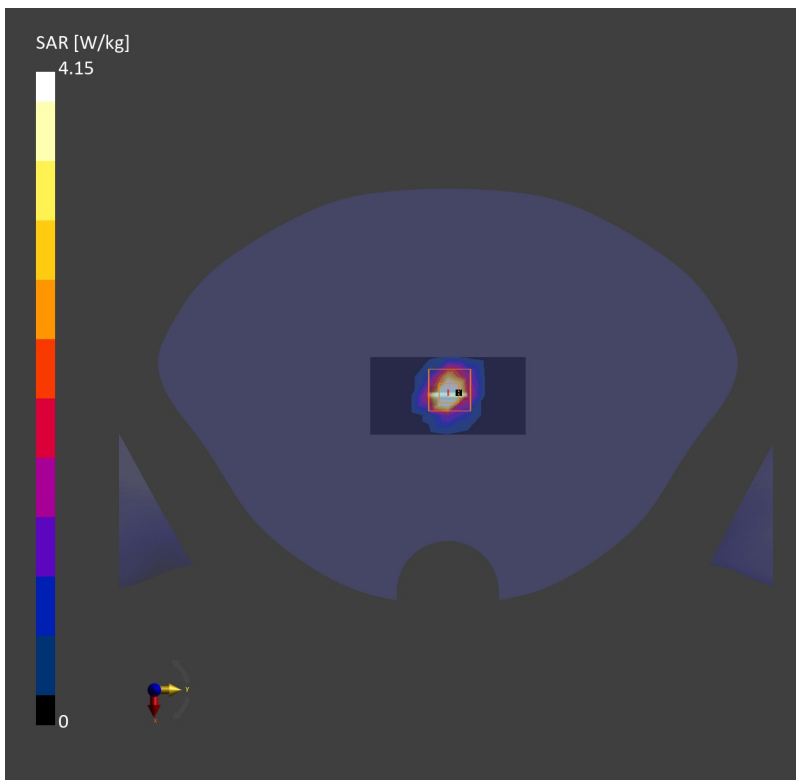

## System Check\_Head\_5750MHz

### DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5750.000

Medium: HSL. Medium parameters used:  $f= 5750.000$  MHz;  $\sigma= 5.32$  S/m;  $\epsilon_r = 35.0$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.57, 5.57, 5.57); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.54 W/kg; SAR (10g) = 1.01 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.76 W/kg; SAR (10g) = 1.09 W/kg;

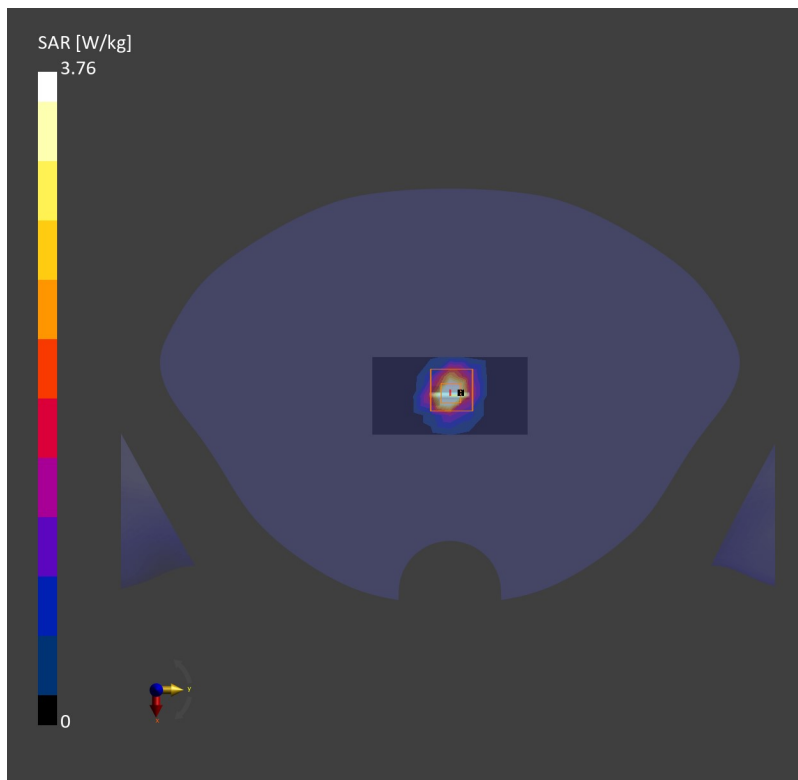



## System Check\_Head\_2600MHz

### DUT:D2600V2 - SN:1061

Communication System: ; Frequency: 2600.000

Medium: HSL. Medium parameters used:  $f = 2600.000$  MHz;  $\sigma = 1.95$  S/m;  $\epsilon_r = 39.1$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(8.1, 8.1, 8.1); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.71 W/kg; SAR (10g) = 1.24 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.66 W/kg; SAR (10g) = 1.20 W/kg;

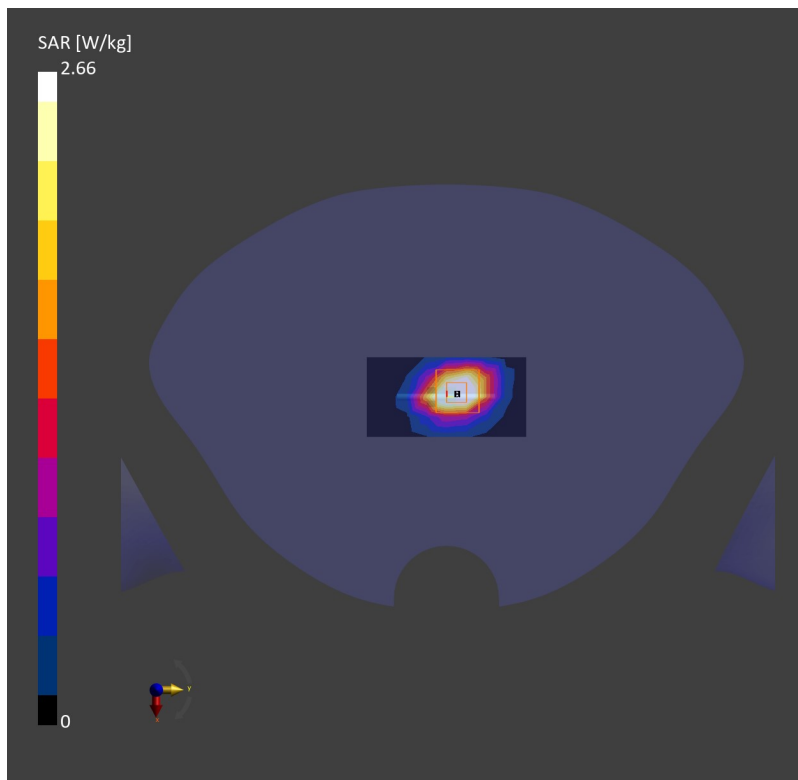

## System Check\_Head\_835MHz

**DUT: D835V2-SN:4d091**

Communication System: ; Frequency: 835.000

Medium: HSL. Medium parameters used:  $f= 835.000$  MHz;  $\sigma= 0.911$  S/m;  $\epsilon_r = 41.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(10.67, 10.67, 10.67); Calibrated: 2023-01-26
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1358; Calibrated: 2023-02-21
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: cDASY6 V6.6.0.13926

**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.467 W/kg; SAR (10g) = 0.311 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.03 dB

SAR (1g) = 0.472 W/kg; SAR (10g) = 0.306 W/kg;

