

## System Check\_1750MHz

### D1750V2-SN:1137

Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1  
Medium: HSL Medium parameters used:  $f = 1750.0$  MHz;  $\sigma = 1.32$  S/m;  $\epsilon_r = 41.6$   
Ambient Temperature: 23.1°C; Liquid Temperature: 22.3°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(8.58, 8.58, 8.58); Calibrated: 2023/6/6
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2023/1/25
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

**Area Scan (40.0 mm x 120.0 mm):** Measurement Grid: 5.0 mm x 15.0 mm  
SAR (1g) = 8.80 W/kg; SAR (10g) = 4.78 W/kg;


**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 8.79 W/kg; SAR (10g) = 4.53 W/kg

Smallest distance from peaks to all points 3 dB below = 10.8 mm

Ratio of SAR at M2 to SAR at M1 = 83.3 %

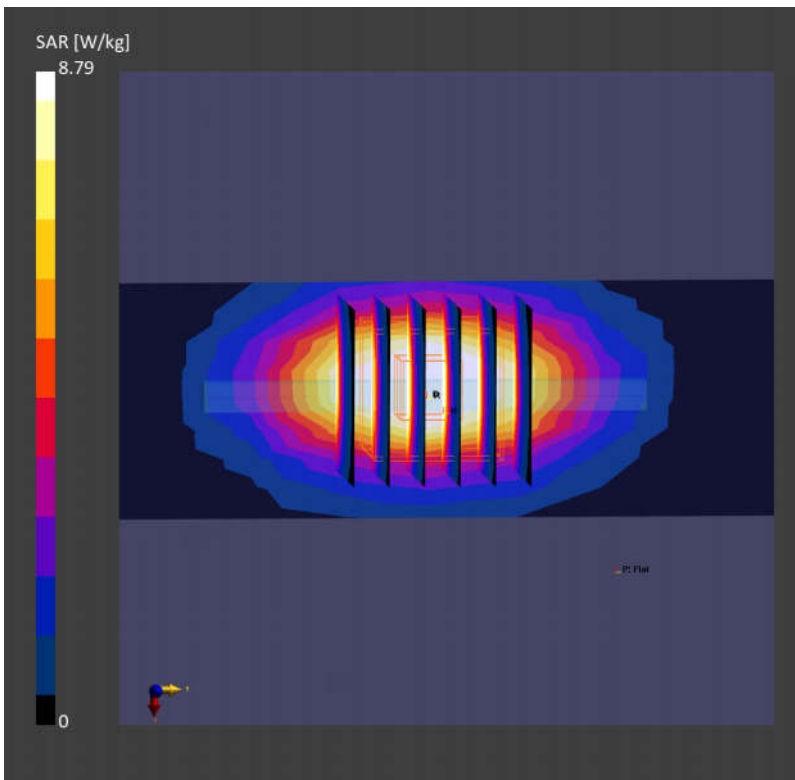

## System Check\_1900MHz

### D1900V2-SN:5d182

Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1  
Medium: HSL Medium parameters used:  $f = 1900.0$  MHz;  $\sigma = 1.45$  S/m;  $\epsilon_r = 41.3$   
Ambient Temperature: 23.2°C; Liquid Temperature: 22.1°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(8.29, 8.29, 8.29); Calibrated: 2023/6/6
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2023/1/25
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

**Area Scan (40.0 mm x 120.0 mm):** Measurement Grid: 5.0 mm x 15.0 mm  
SAR (1g) = 10.9 W/kg; SAR (10g) = 5.70 W/kg;


**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 10.5 W/kg; SAR (10g) = 5.41 W/kg

Smallest distance from peaks to all points 3 dB below = 9.7 mm

Ratio of SAR at M2 to SAR at M1 = 82.6 %

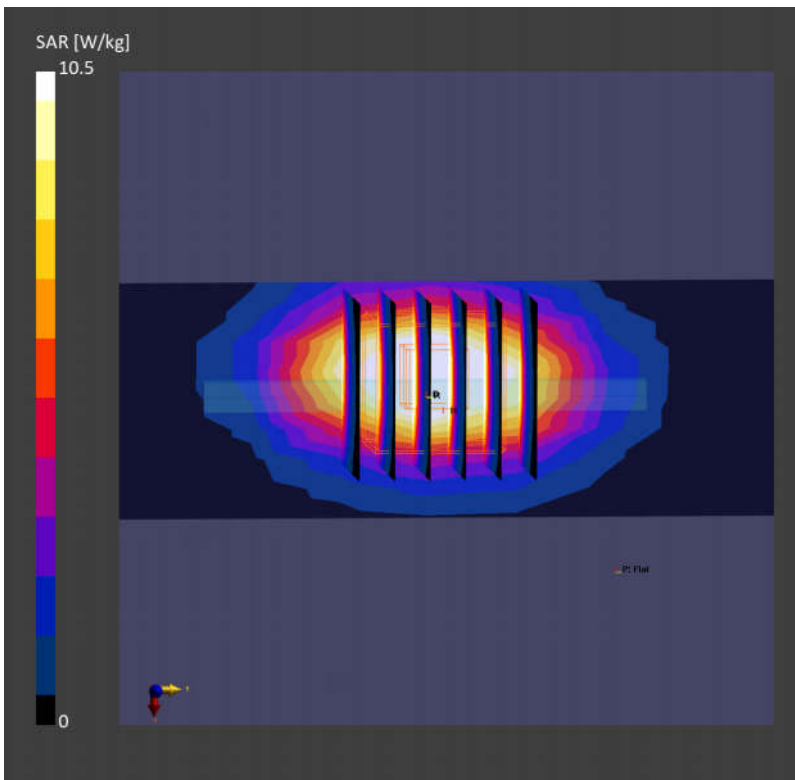

Date: 2024/5/4

## System Check\_2600MHz

### D2600V2-SN:1070

Communication System: CW; Frequency: 2600.0 MHz; Duty Cycle: 1:1  
Medium: HSL Medium parameters used:  $f = 2600.0$  MHz;  $\sigma = 1.91$  S/m;  $\epsilon_r = 40.3$   
Ambient Temperature: 23.6°C; Liquid Temperature: 22.5°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.55, 7.55, 7.55); Calibrated: 2023/6/6
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2023/1/25
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 5.0 mm x 10.0 mm  
SAR (1g) = 13.9 W/kg; SAR (10g) = 6.32 W/kg;


**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 13.4 W/kg; SAR (10g) = 5.82 W/kg

Smallest distance from peaks to all points 3 dB below = 9.0 mm

Ratio of SAR at M2 to SAR at M1 = 77.1 %

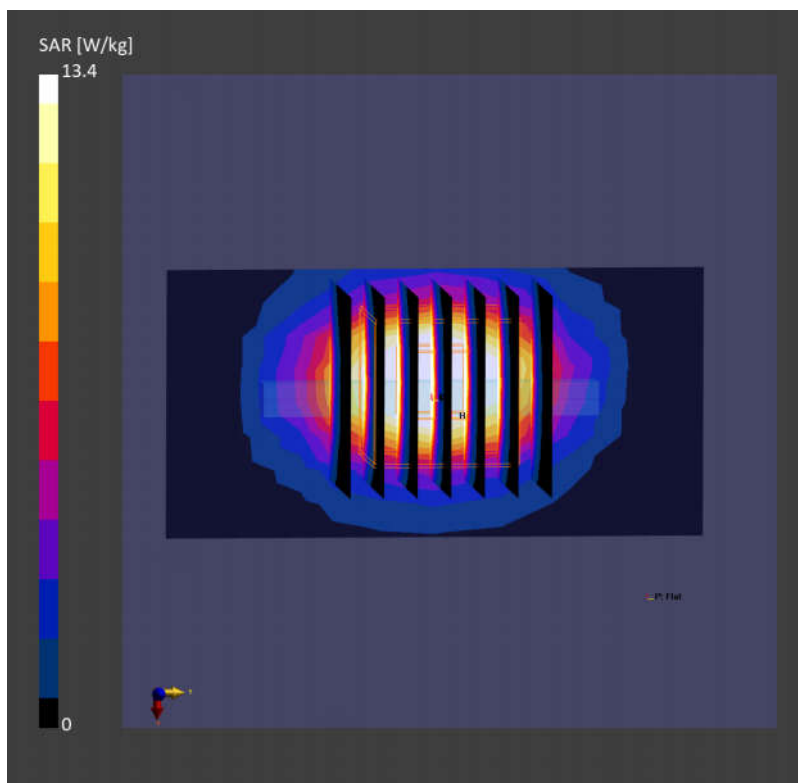

Date: 2024/5/5

## System Check\_3500MHz

### D3500V2-SN:1076

Communication System: CW; Frequency: 3500.0 MHz; Duty Cycle: 1:1  
Medium: HSL Medium parameters used:  $f = 3500.0$  MHz;  $\sigma = 2.88$  S/m;  $\epsilon_r = 39.1$   
Ambient Temperature: 23.2°C; Liquid Temperature: 22.4°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(6.78, 6.78, 6.78); Calibrated: 2023/6/6
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn715; Calibrated: 2023/1/25
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 5.0 mm x 10.0 mm  
SAR (1g) = 6.47 W/kg; SAR (10g) = 2.51 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 6.31 W/kg; SAR (10g) = 2.35 W/kg

Smallest distance from peaks to all points 3 dB below = 8.1 mm

Ratio of SAR at M2 to SAR at M1 = 75.9 %

