

## System Check\_Head\_750MHz

**DUT:D750V3 - SN:1087**

Communication System: ; Frequency: 750.000

Medium: HSL. Medium parameters used:  $f= 750.000$  MHz;  $\sigma= 0.898$  S/m;  $\epsilon_r = 42.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.34, 10.73, 9.7); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.445 W/kg; SAR (10g) = 0.295 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.03 dB

SAR (1g) = 0.430 W/kg; SAR (10g) = 0.285 W/kg;

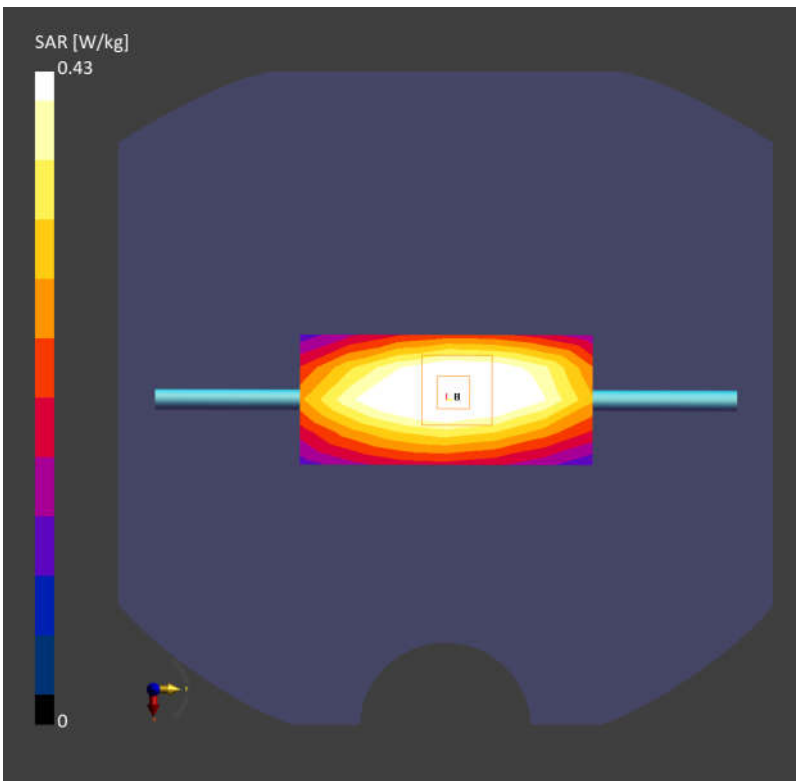

## System Check\_Head\_835MHz

**DUT:D835V2 - SN:4d091**

Communication System: ; Frequency: 835.000

Medium: HSL. Medium parameters used:  $f= 835.000$  MHz;  $\sigma= 0.928$  S/m;  $\epsilon_r = 42.1$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.26, 10.67, 9.28); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.508 W/kg; SAR (10g) = 0.333 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.06 dB

SAR (1g) = 0.502 W/kg; SAR (10g) = 0.329 W/kg;

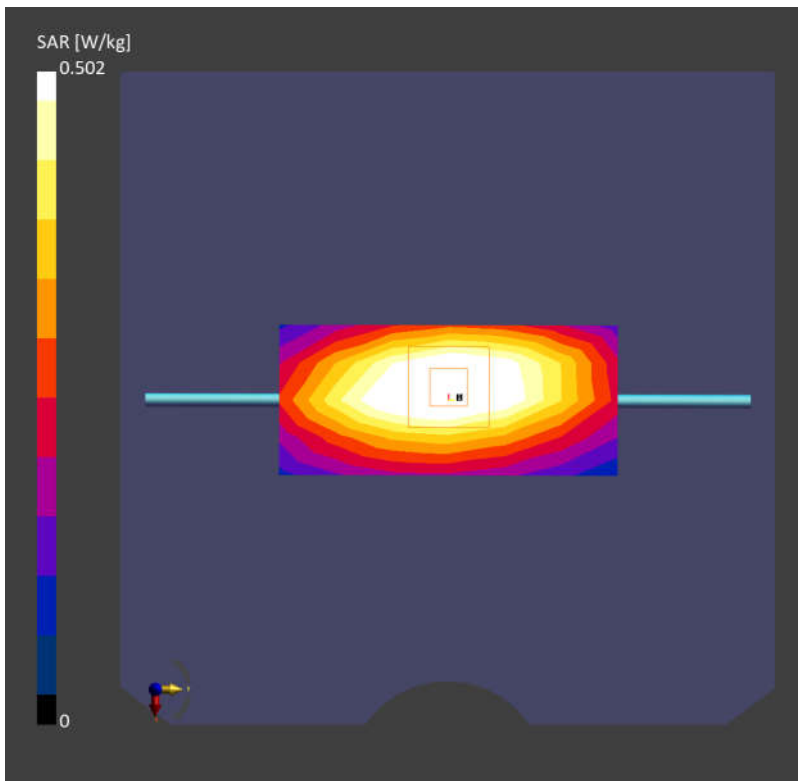

## System Check\_Head\_1750MHz

**DUT:D1750V2 - SN:1090**

Communication System: ; Frequency: 1750.000

Medium: HSL. Medium parameters used:  $f= 1750.000$  MHz;  $\sigma= 1.36$  S/m;  $\epsilon_r = 40.9$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.87, 9.06, 8.09); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.80 W/kg; SAR (10g) = 1.00 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 1.95 W/kg; SAR (10g) = 1.01 W/kg;

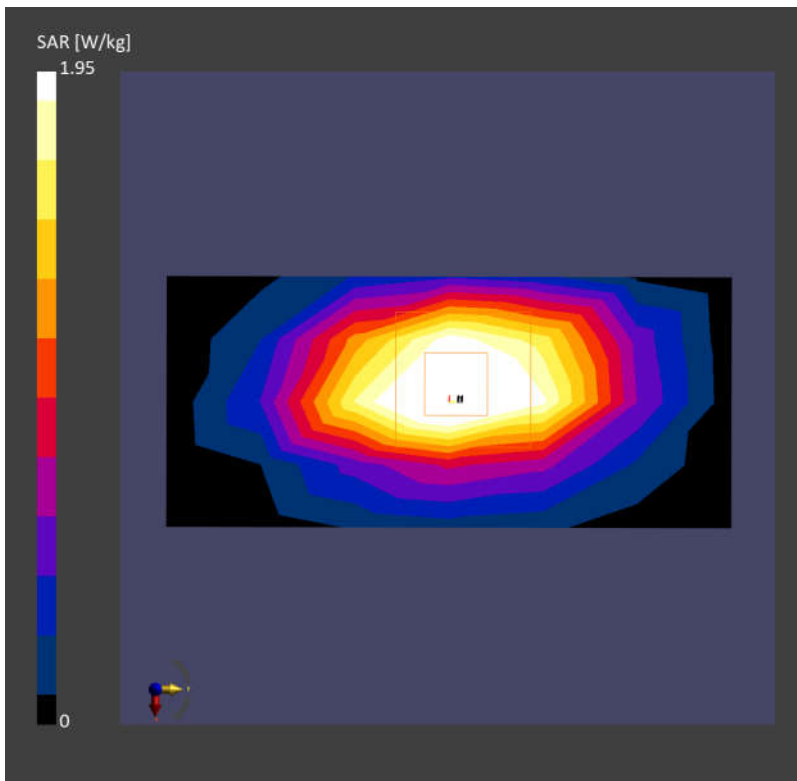

## System Check\_Head\_1900MHz

**DUT:D1900V2 - SN:5d118**

Communication System: ; Frequency: 1900.000

Medium: HSL. Medium parameters used:  $f= 1900.000$  MHz;  $\sigma= 1.46$  S/m;  $\epsilon_r = 40.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.77, 8.97, 7.88); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.79 W/kg; SAR (10g) = 0.947 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.02 dB

SAR (1g) = 1.81 W/kg; SAR (10g) = 1.03 W/kg;

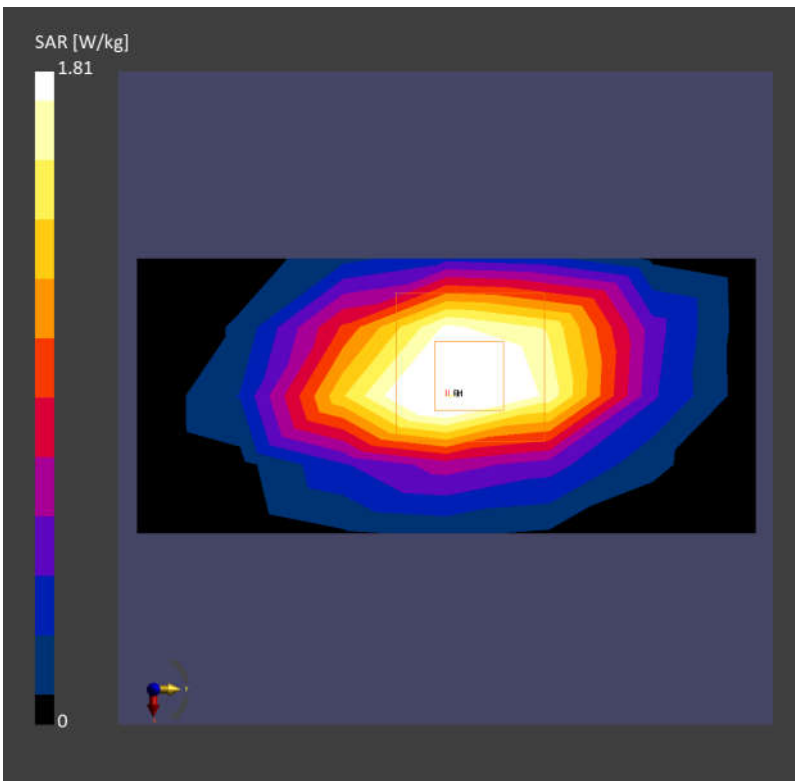

## System Check\_Head\_2300MHz

**DUT:D2300V2- SN:1055**

Communication System: ; Frequency: 2300.000

Medium: HSL. Medium parameters used:  $f= 2300.000$  MHz;  $\sigma= 1.72$  S/m;  $\epsilon_r = 38.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.57, 8.73, 7.66); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.61 W/kg; SAR (10g) = 1.27 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.05 dB

SAR (1g) = 2.54 W/kg; SAR (10g) = 1.23 W/kg;

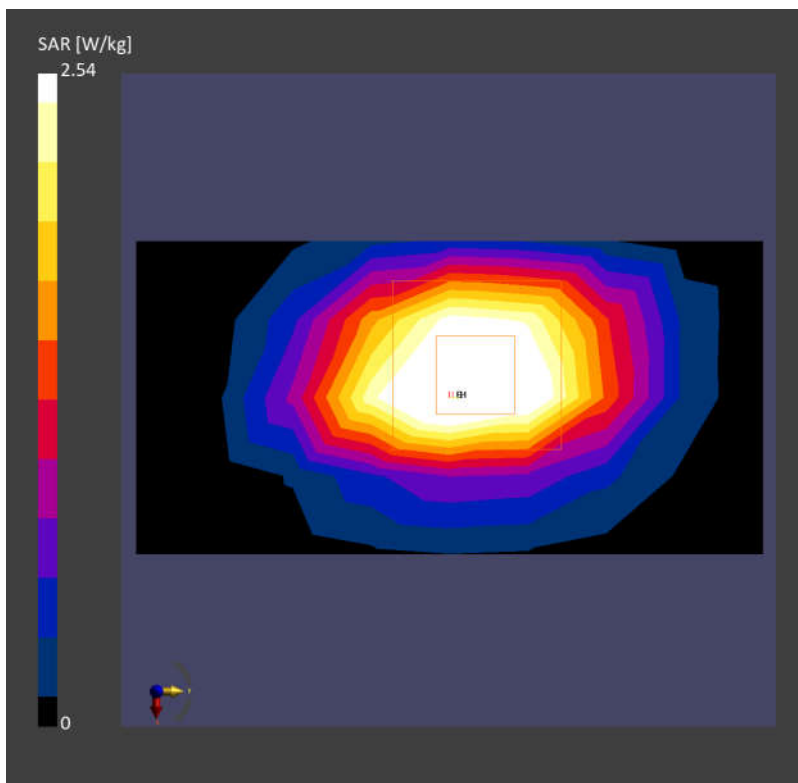

## System Check\_Head\_2450MHz

**DUT:D2450V2 - SN:1040**

Communication System: ; Frequency: 2450.000

Medium: HSL. Medium parameters used:  $f= 2450.000$  MHz;  $\sigma= 1.87$  S/m;  $\epsilon_r = 40.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.47, 8.61, 7.55); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.73 W/kg; SAR (10g) = 1.29 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.65 W/kg; SAR (10g) = 1.26 W/kg;

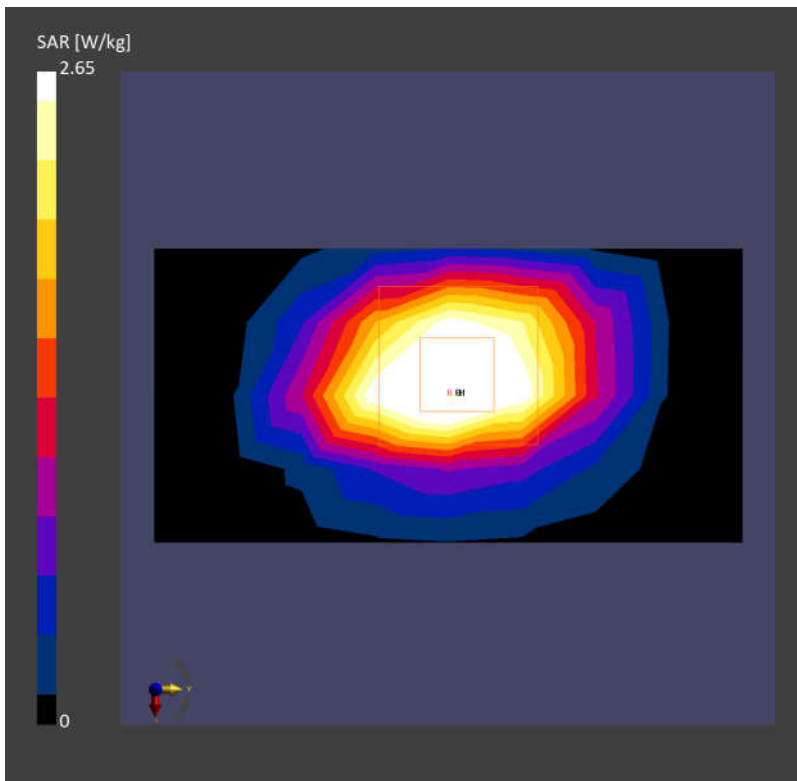

## System Check\_Head\_2600MHz

**DUT:D2600V2 - SN:1112**

Communication System: ; Frequency: 2600.000

Medium: HSL. Medium parameters used:  $f= 2600.000$  MHz;  $\sigma= 1.98$  S/m;  $\epsilon_r = 40.6$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.3, 8.44, 7.37); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.73 W/kg; SAR (10g) = 1.27 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.66 W/kg; SAR (10g) = 1.21 W/kg;

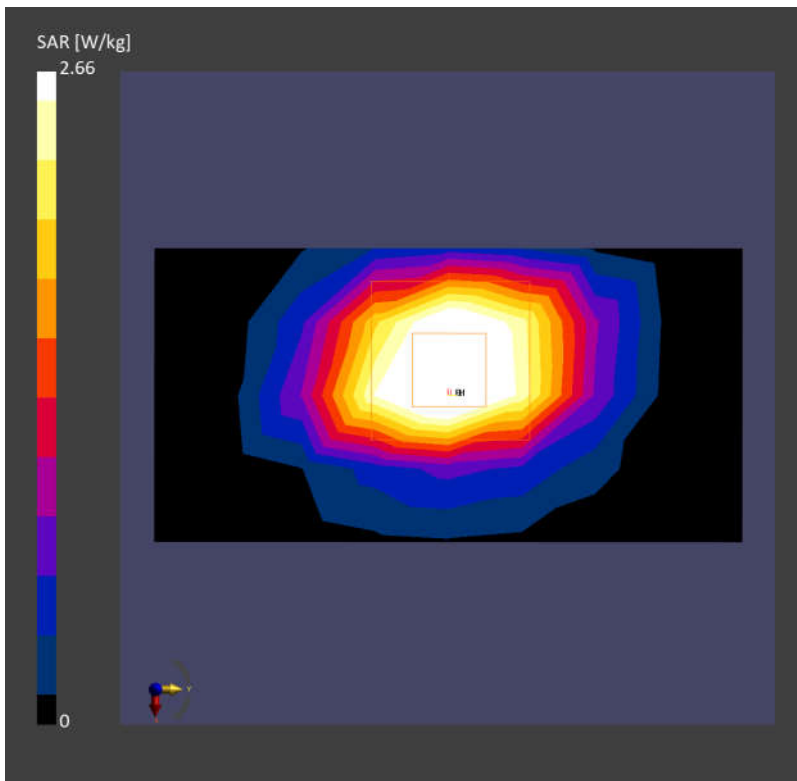

## System Check\_Head\_3500MHz

**DUT:D3500V2 - SN:1037**

Communication System: ; Frequency: 3500.000

Medium: HSL. Medium parameters used:  $f= 3500.000$  MHz;  $\sigma= 2.88$  S/m;  $\epsilon_r = 38.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.99, 8.16, 7.09); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.11 W/kg; SAR (10g) = 1.22 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.13 W/kg; SAR (10g) = 1.19 W/kg;

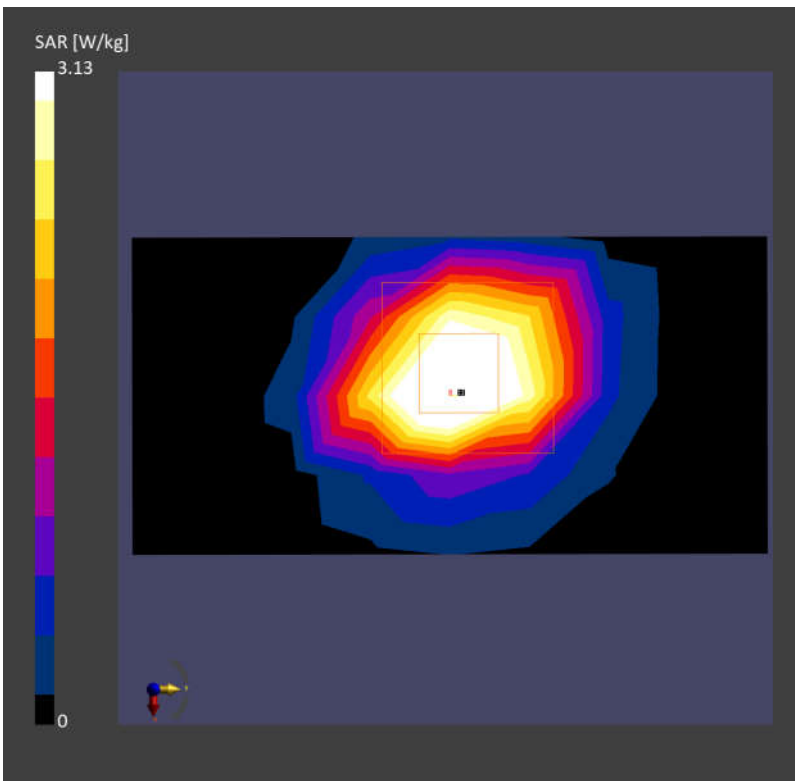



## System Check\_Head\_3700MHz

**DUT:D3700V2 - SN:1008**

Communication System: ; Frequency: 3700.000

Medium: HSL. Medium parameters used:  $f= 3700.000$  MHz;  $\sigma= 3.08$  S/m;  $\epsilon_r = 38.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.89, 8.06, 7.01); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.29 W/kg; SAR (10g) = 1.23 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.24 W/kg; SAR (10g) = 1.22 W/kg;

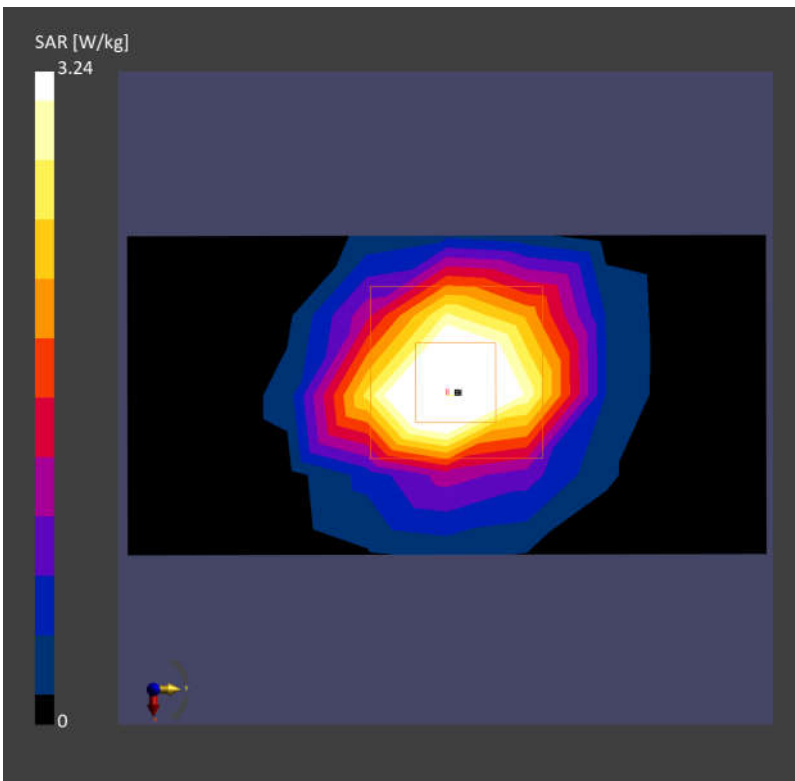

## System Check\_Head\_3900MHz

**DUT:D3900V2 - SN:1048**

Communication System: ; Frequency: 3900.000

Medium: HSL. Medium parameters used:  $f= 3900.000$  MHz;  $\sigma= 3.28$  S/m;  $\epsilon_r = 37.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.83, 7.98, 6.94); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.24 W/kg; SAR (10g) = 1.18 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.06 dB

SAR (1g) = 3.21 W/kg; SAR (10g) = 1.16 W/kg;

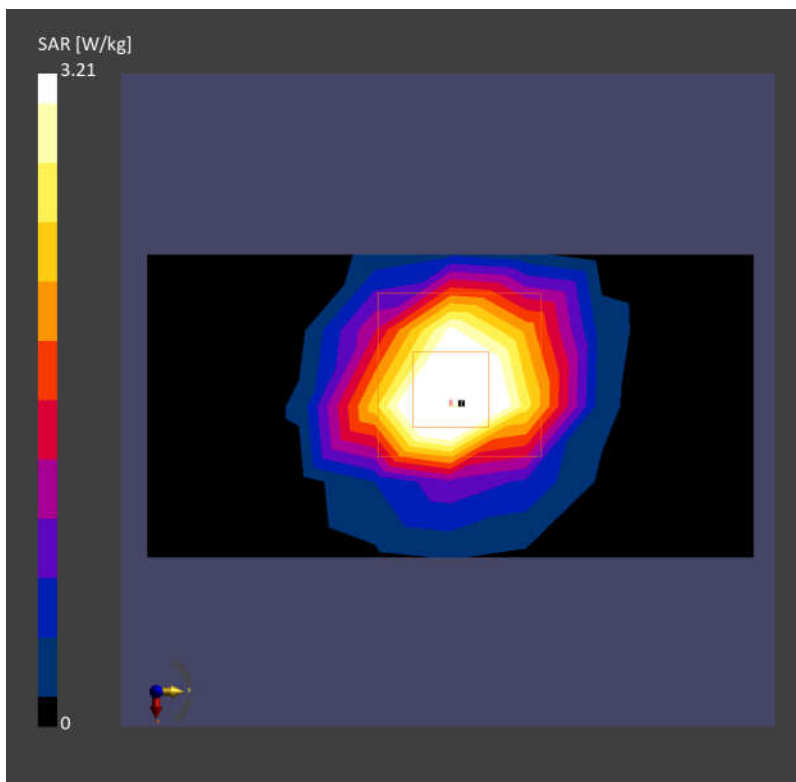

## System Check\_Head\_5250MHz

### DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5250.000

Medium: HSL. Medium parameters used:  $f= 5250.000$  MHz;  $\sigma= 4.59$  S/m;  $\epsilon_r = 36.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.84, 6.82, 5.88); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.37 W/kg; SAR (10g) = 1.06 W/kg;

**Zoom Scan (24.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 3.79 W/kg; SAR (10g) = 1.14 W/kg;

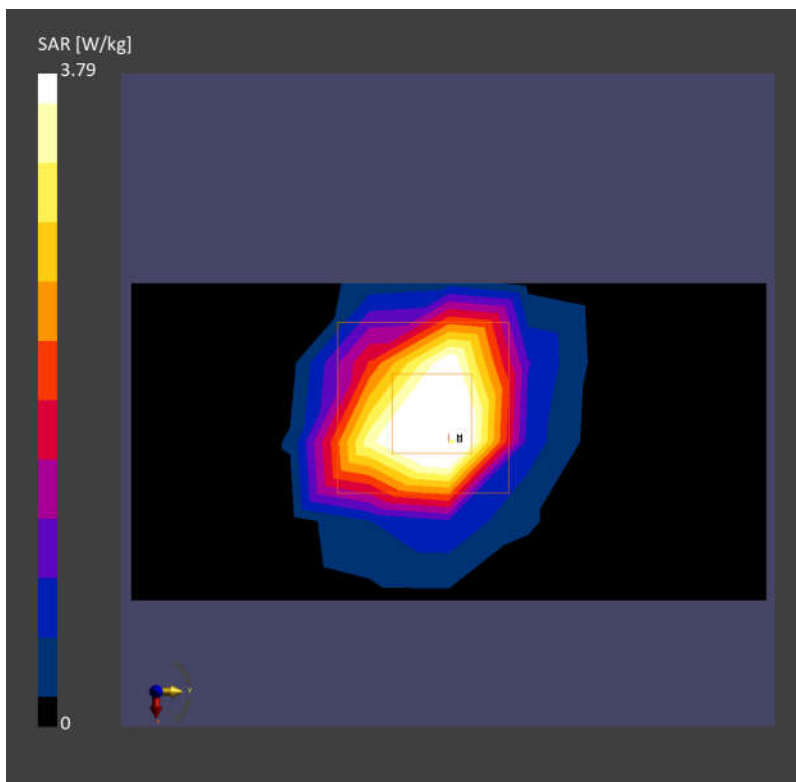

## System Check\_Head\_5600MHz

**DUT:D5GHzV2 - SN:1113**

Communication System: ; Frequency: 5600.000

Medium: HSL. Medium parameters used:  $f= 5600.000$  MHz;  $\sigma= 4.96$  S/m;  $\epsilon_r = 35.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(4.83, 5.71, 4.9); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.90 W/kg; SAR (10g) = 1.16 W/kg;

**Zoom Scan (24.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 4.01 W/kg; SAR (10g) = 1.14 W/kg;

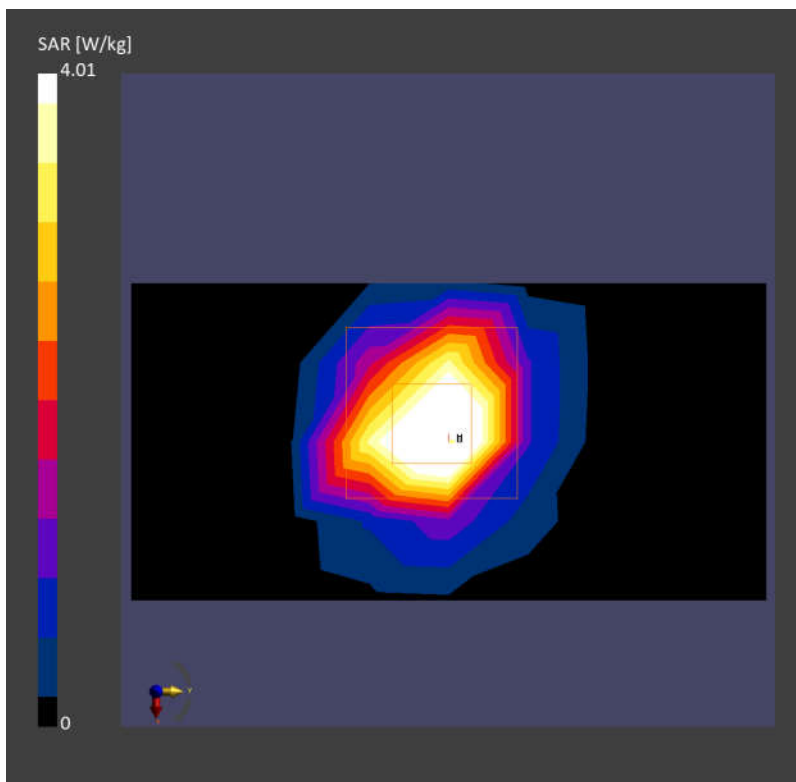

## System Check\_Head\_5750MHz

**DUT:D5GHzV2 - SN:1113**

Communication System: ; Frequency: 5750.000

Medium: HSL. Medium parameters used:  $f= 5750.000$  MHz;  $\sigma= 5.14$  S/m;  $\epsilon_r = 35.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.03, 5.88, 5.16); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.49 W/kg; SAR (10g) = 1.04 W/kg;

**Zoom Scan (24.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.77 W/kg; SAR (10g) = 1.13 W/kg;

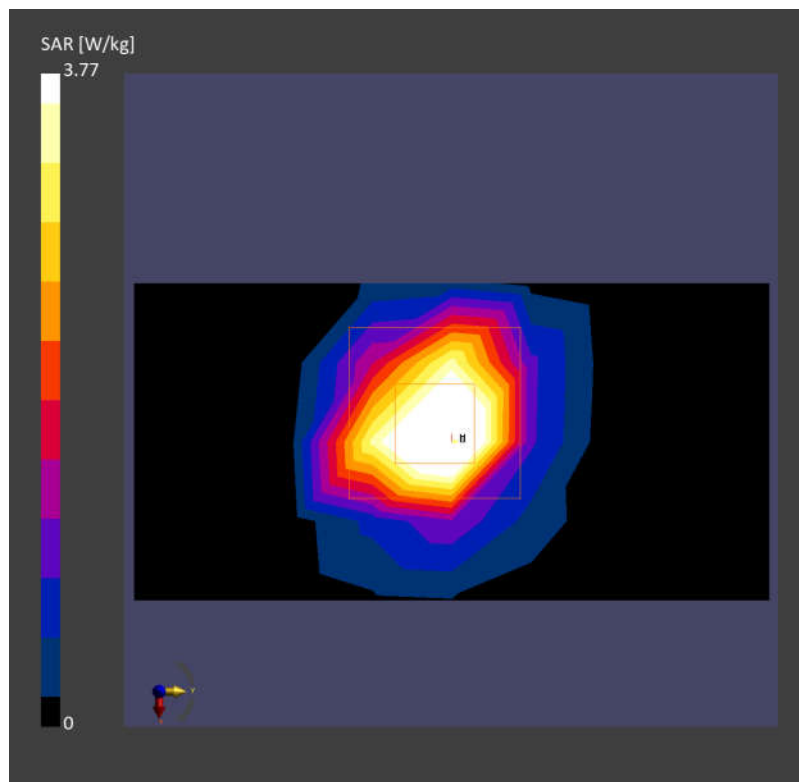

## System Check\_Head\_750MHz

**DUT:D750V3 - SN:1087**

Communication System: ; Frequency: 750.000

Medium: HSL. Medium parameters used:  $f= 750.000$  MHz;  $\sigma= 0.872$  S/m;  $\epsilon_r = 41.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.34, 10.73, 9.7); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.420 W/kg; SAR (10g) = 0.279 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.418 W/kg; SAR (10g) = 0.277 W/kg;

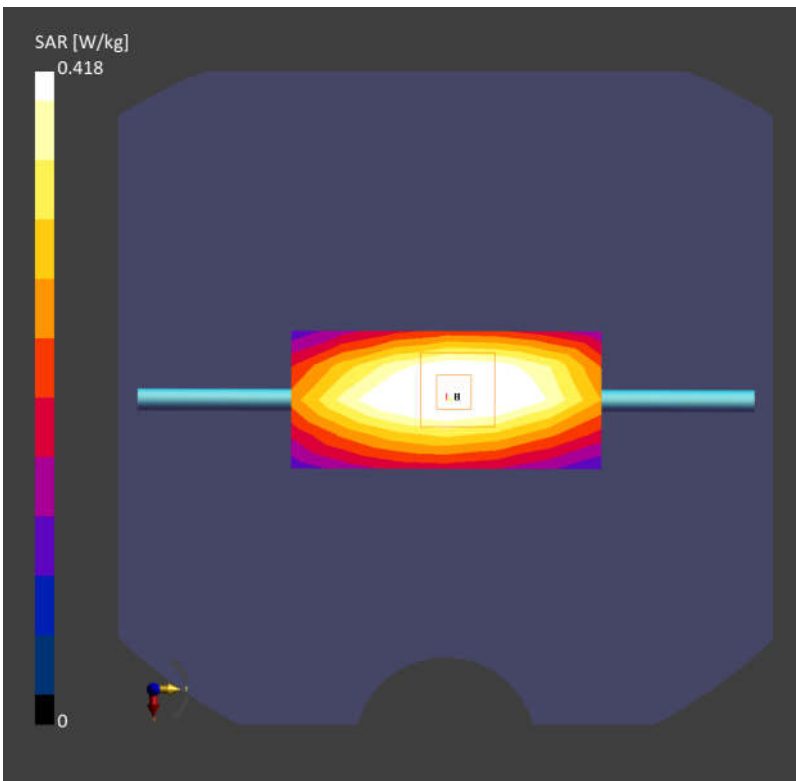

## System Check\_Head\_835MHz

**DUT:D835V2 - SN:4d091**

Communication System: ; Frequency: 835.000

Medium: HSL. Medium parameters used:  $f= 835.000$  MHz;  $\sigma= 0.920$  S/m;  $\epsilon_r = 40.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.26, 10.67, 9.28); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.503 W/kg; SAR (10g) = 0.330 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 0.497 W/kg; SAR (10g) = 0.325 W/kg;

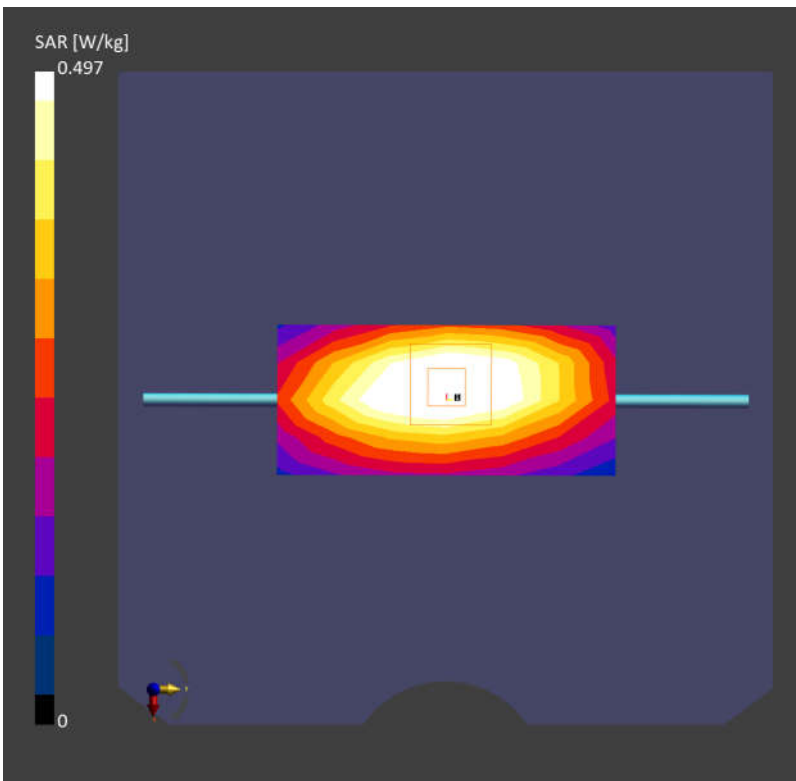

## System Check\_Head\_1750MHz

**DUT:D1750V2 - SN:1090**

Communication System: ; Frequency: 1750.000

Medium: HSL. Medium parameters used:  $f= 1750.000$  MHz;  $\sigma= 1.39$  S/m;  $\epsilon_r = 38.5$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.87, 9.06, 8.09); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.86 W/kg; SAR (10g) = 1.01 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.92 W/kg; SAR (10g) = 1.00 W/kg;

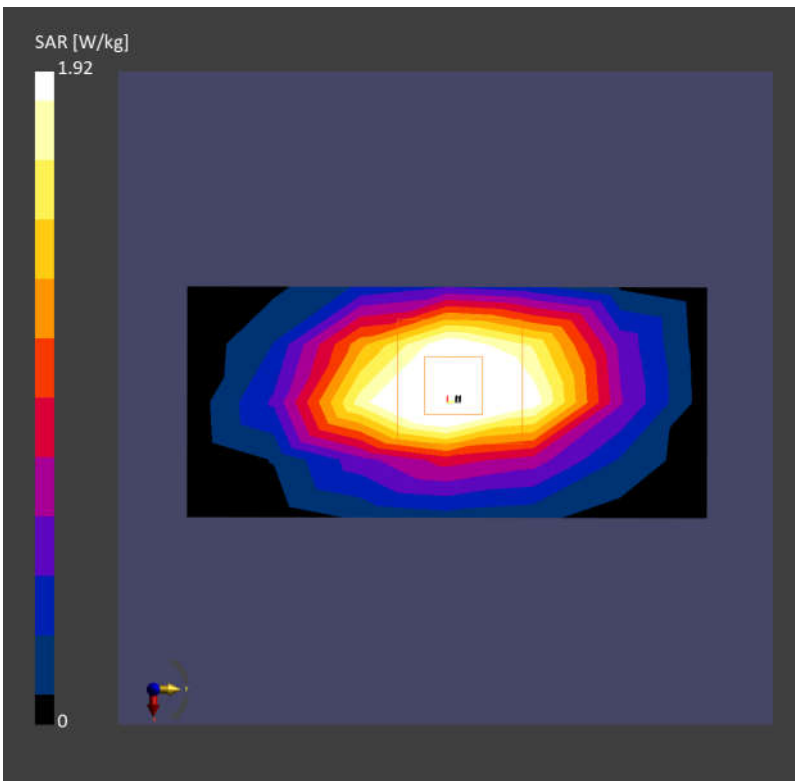



## System Check\_Head\_1900MHz

**DUT:D1900V2 - SN:5d118**

Communication System: ; Frequency: 1900.000

Medium: HSL. Medium parameters used:  $f= 1900.000$  MHz;  $\sigma= 1.45$  S/m;  $\epsilon_r = 39.9$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.77, 8.97, 7.88); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.00 W/kg; SAR (10g) = 1.05 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.12 dB

SAR (1g) = 1.89 W/kg; SAR (10g) = 1.05 W/kg;

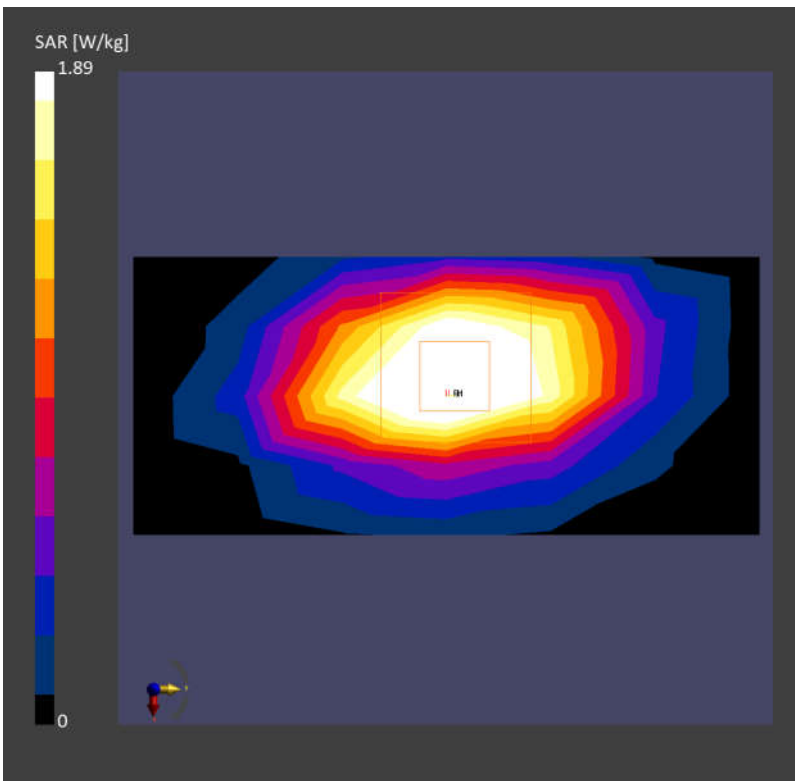

## System Check\_Head\_2300MHz

**DUT:D2300V2 - SN:1055**

Communication System: ; Frequency: 2300.000

Medium: HSL. Medium parameters used:  $f= 2300.000$  MHz;  $\sigma= 1.71$  S/m;  $\epsilon_r = 39.5$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.57, 8.73, 7.66); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.55 W/kg; SAR (10g) = 1.24 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 2.47 W/kg; SAR (10g) = 1.20 W/kg;

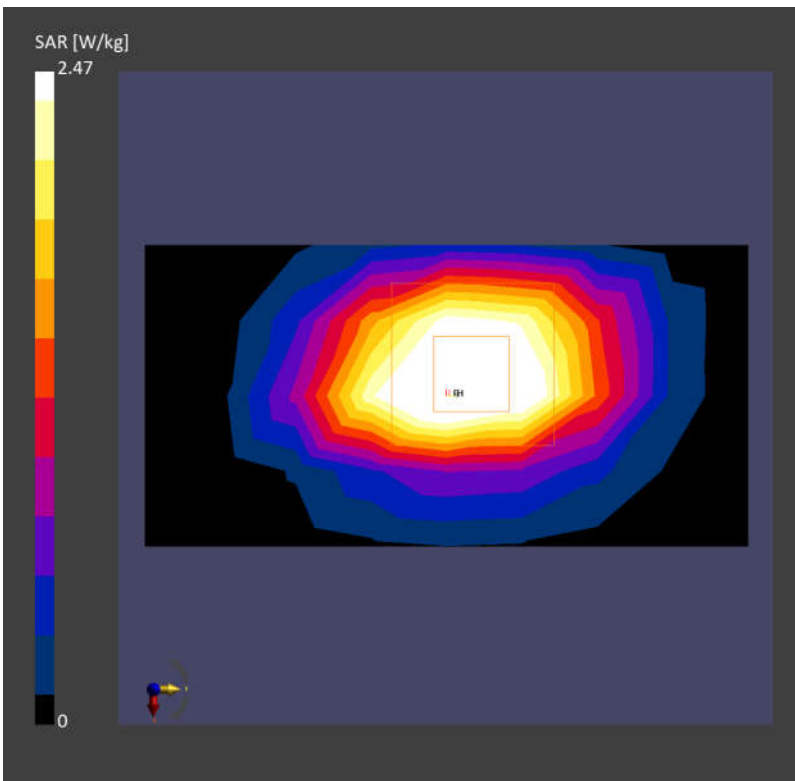

## System Check\_Head\_2450MHz

**DUT:D2450V2 - SN:1040**

Communication System: ; Frequency: 2450.000

Medium: HSL. Medium parameters used:  $f= 2450.000$  MHz;  $\sigma= 1.84$  S/m;  $\epsilon_r = 38.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.47, 8.61, 7.55); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.70 W/kg; SAR (10g) = 1.28 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.61 W/kg; SAR (10g) = 1.24 W/kg;

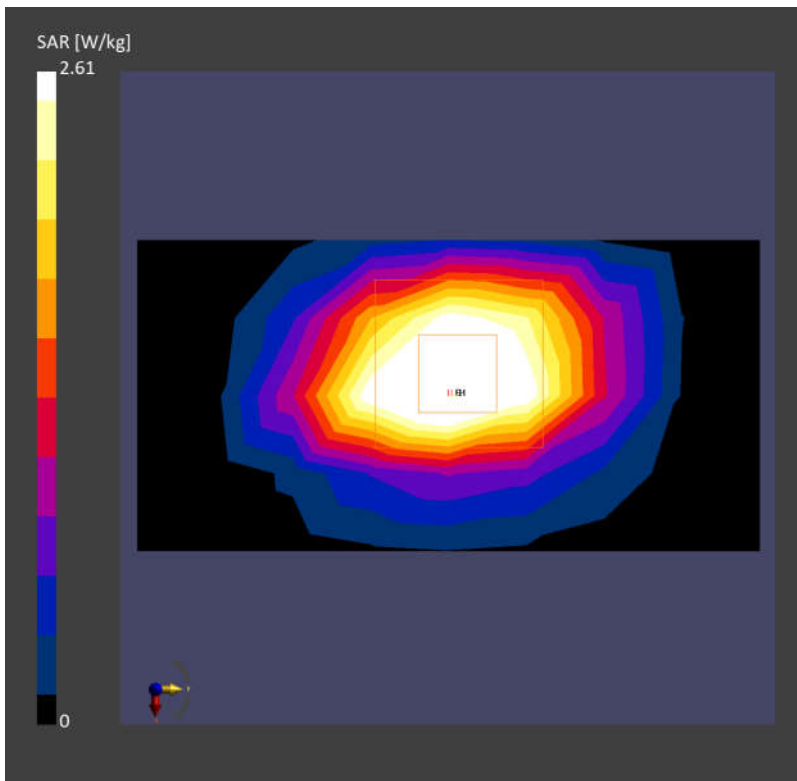

## System Check\_Head\_2600MHz

**DUT:D2600V2 - SN:1112**

Communication System: ; Frequency: 2600.000

Medium: HSL. Medium parameters used:  $f= 2600.000$  MHz;  $\sigma= 1.94$  S/m;  $\epsilon_r = 37.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.3, 8.44, 7.37); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.69 W/kg; SAR (10g) = 1.24 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.04 dB

SAR (1g) = 2.62 W/kg; SAR (10g) = 1.19 W/kg;

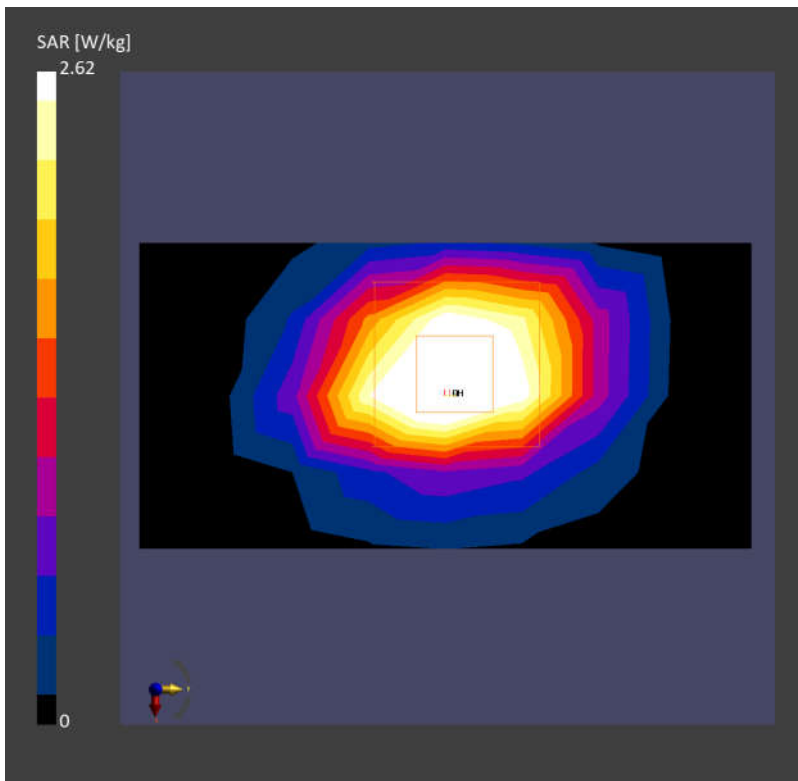

## System Check\_Head\_3500MHz

**DUT:D3500V2 - SN:1037**

Communication System: ; Frequency: 3500.000

Medium: HSL. Medium parameters used:  $f= 3500.000$  MHz;  $\sigma= 2.79$  S/m;  $\epsilon_r = 39.6$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.99, 8.16, 7.09); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.03 W/kg; SAR (10g) = 1.18 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.18 W/kg; SAR (10g) = 1.25 W/kg;

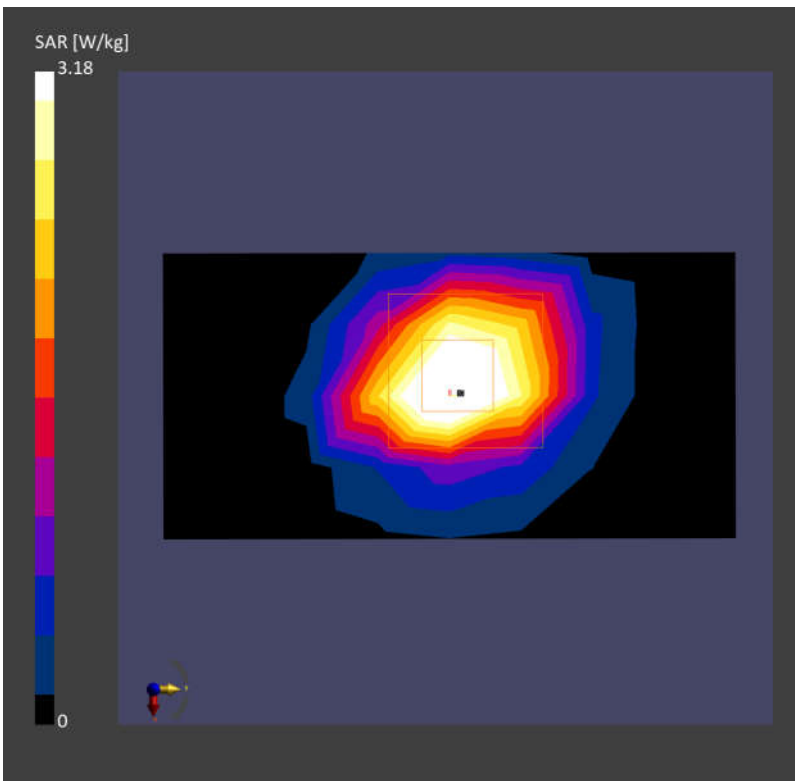

## System Check\_Head\_3700MHz

**DUT:D3700V2 - SN:1008**

Communication System: ; Frequency: 3700.000

Medium: HSL. Medium parameters used:  $f= 3700.000$  MHz;  $\sigma= 2.99$  S/m;  $\epsilon_r = 38.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.89, 8.06, 7.01); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.18 W/kg; SAR (10g) = 1.19 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.14 W/kg; SAR (10g) = 1.18 W/kg;

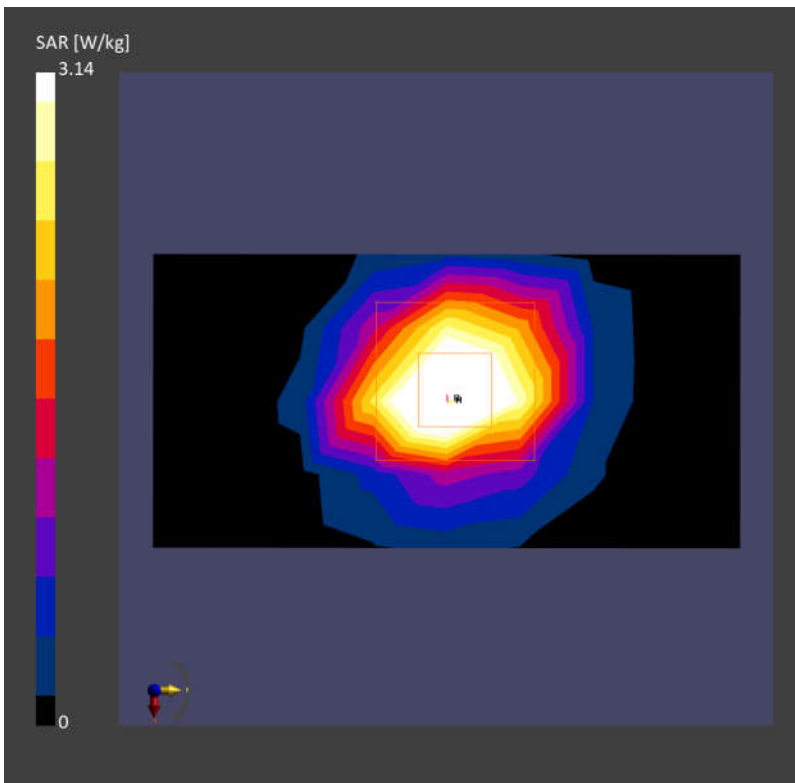

## System Check\_Head\_3900MHz

**DUT:D3900V2 - SN:1048**

Communication System: ; Frequency: 3900.000

Medium: HSL. Medium parameters used:  $f= 3900.000$  MHz;  $\sigma= 3.19$  S/m;  $\epsilon_r = 38.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.83, 7.98, 6.94); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.24 W/kg; SAR (10g) = 1.18 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.06 dB

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.13 W/kg;

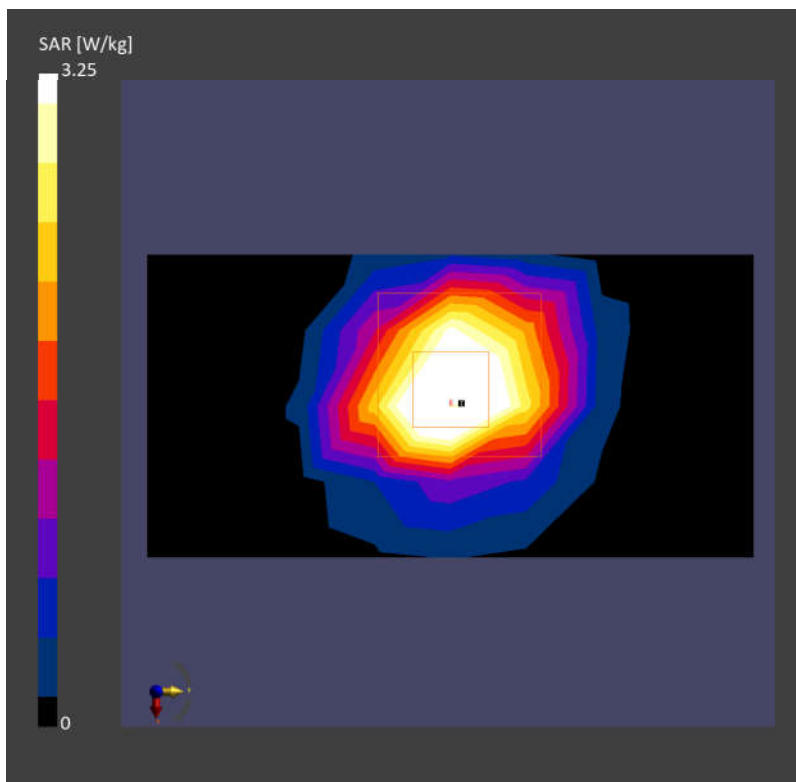

## System Check\_Head\_5250MHz

### DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5250.000

Medium: HSL. Medium parameters used:  $f= 5250.000$  MHz;  $\sigma= 4.67$  S/m;  $\epsilon_r = 36.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.84, 6.82, 5.88); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.37 W/kg; SAR (10g) = 1.06 W/kg;

**Zoom Scan (24.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 3.84 W/kg; SAR (10g) = 1.17 W/kg;

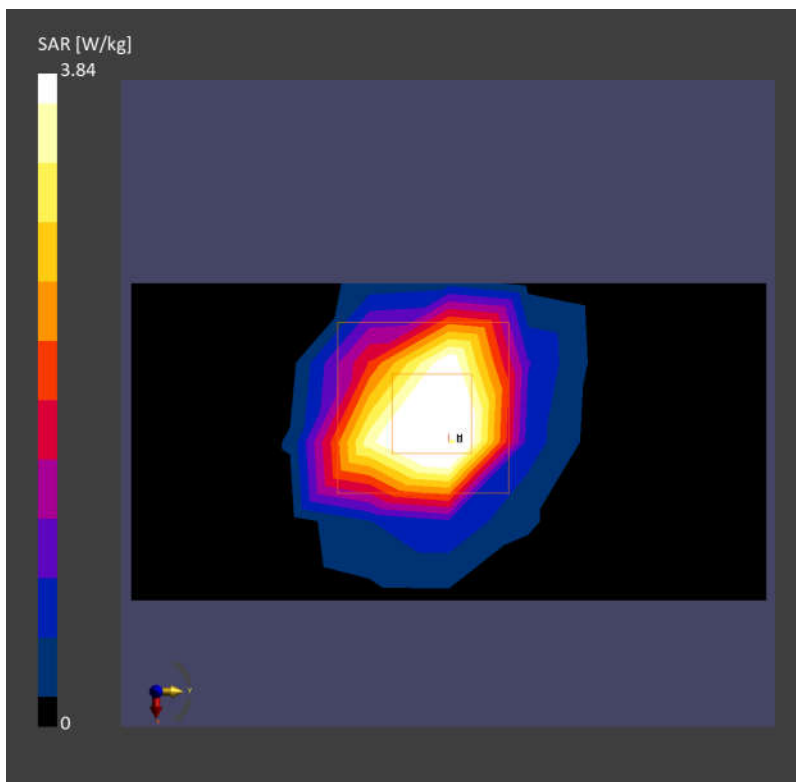



## System Check\_Head\_5600MHz

**DUT:D5GHzV2 - SN:1113**

Communication System: ; Frequency: 5600.000

Medium: HSL. Medium parameters used:  $f= 5600.000$  MHz;  $\sigma= 5.07$  S/m;  $\epsilon_r = 36.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(4.83, 5.71, 4.9); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.90 W/kg; SAR (10g) = 1.16 W/kg;

**Zoom Scan (24.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 4.11 W/kg; SAR (10g) = 1.18 W/kg;

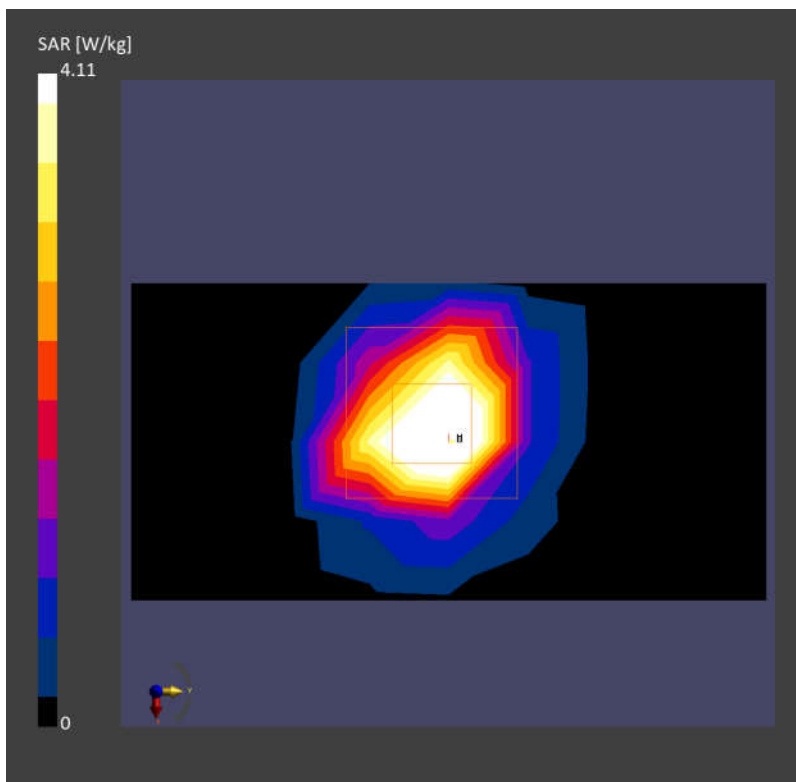

## System Check\_Head\_5750MHz

**DUT:D5GHzV2 - SN:1113**

Communication System: ; Frequency: 5750.000

Medium: HSL. Medium parameters used:  $f= 5750.000$  MHz;  $\sigma= 5.25$  S/m;  $\epsilon_r = 35.8$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.03, 5.88, 5.16); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.49 W/kg; SAR (10g) = 1.04 W/kg;

**Zoom Scan (24.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.79 W/kg; SAR (10g) = 1.14 W/kg;

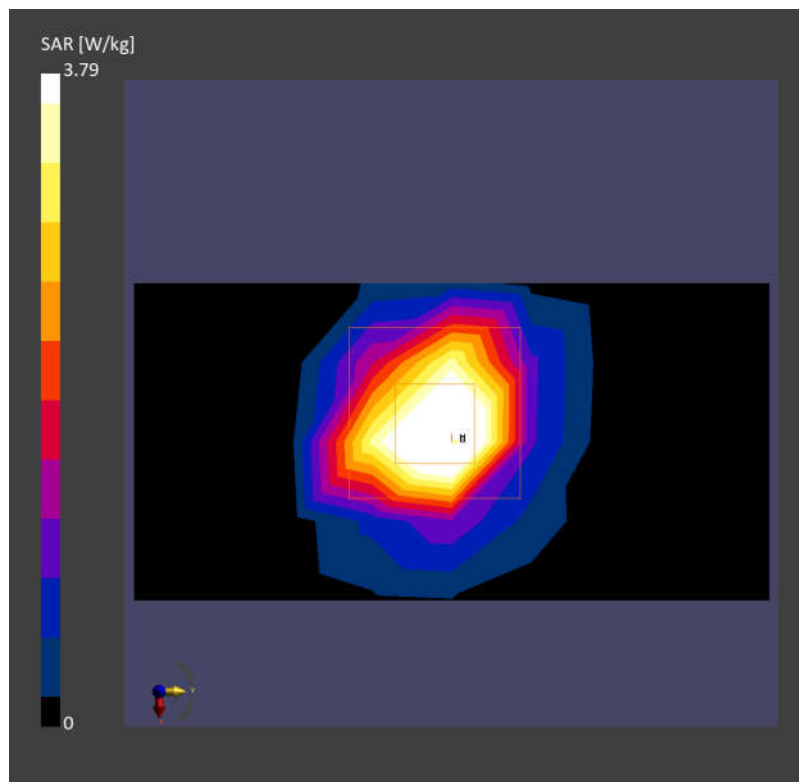

## System Check\_Head\_750MHz

**DUT:D750V3 - SN:1087**

Communication System: ; Frequency: 750.000

Medium: HSL. Medium parameters used:  $f= 750.000$  MHz;  $\sigma= 0.925$  S/m;  $\epsilon_r = 42.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.34, 10.73, 9.7); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.421 W/kg; SAR (10g) = 0.280 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.418 W/kg; SAR (10g) = 0.276 W/kg;

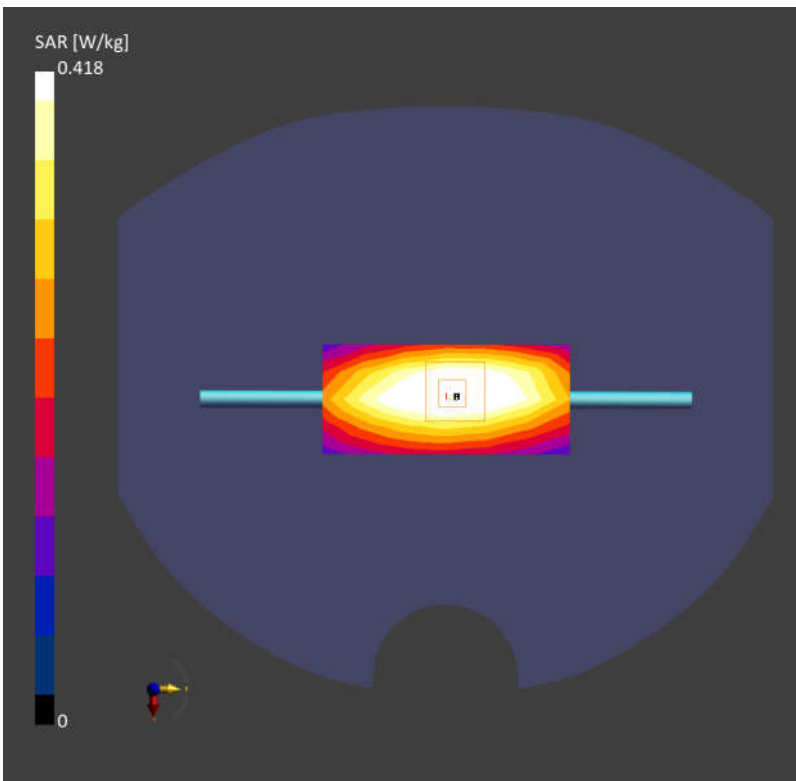

## System Check\_Head\_835MHz

**DUT:D835V2 - SN:4d091**

Communication System: ; Frequency: 835.000

Medium: HSL. Medium parameters used:  $f= 835.000$  MHz;  $\sigma= 0.911$  S/m;  $\epsilon_r = 42.7$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(9.26, 10.67, 9.28); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.499 W/kg; SAR (10g) = 0.328 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 0.493 W/kg; SAR (10g) = 0.322 W/kg;

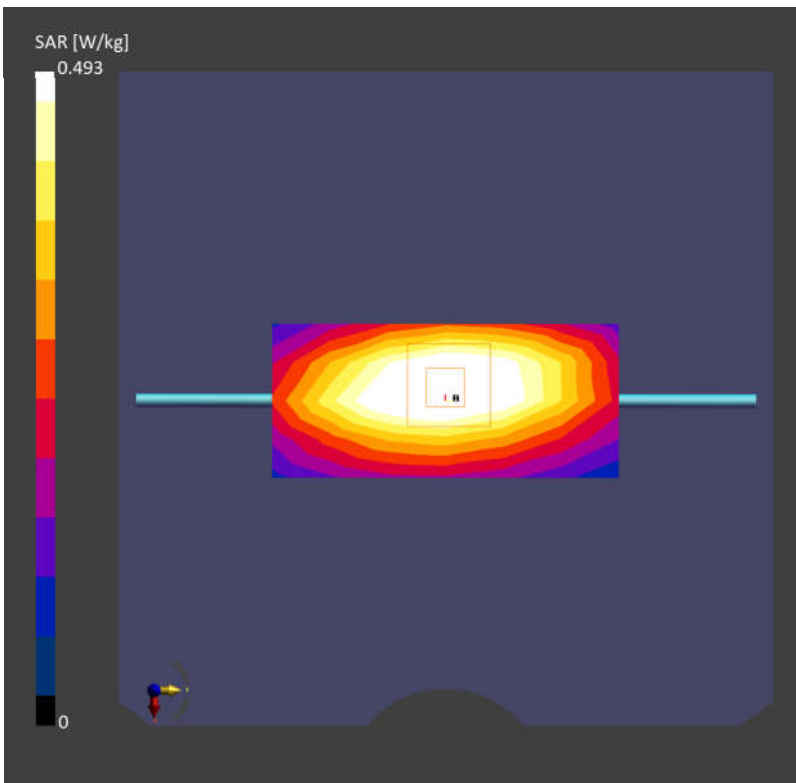

## System Check\_Head\_1750MHz

**DUT:D1750V2 - SN:1090**

Communication System: ; Frequency: 1750.000

Medium: HSL. Medium parameters used:  $f= 1750.000$  MHz;  $\sigma= 1.38$  S/m;  $\epsilon_r = 40.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.87, 9.06, 8.09); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.99 W/kg; SAR (10g) = 1.07 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.97 W/kg; SAR (10g) = 1.05 W/kg;

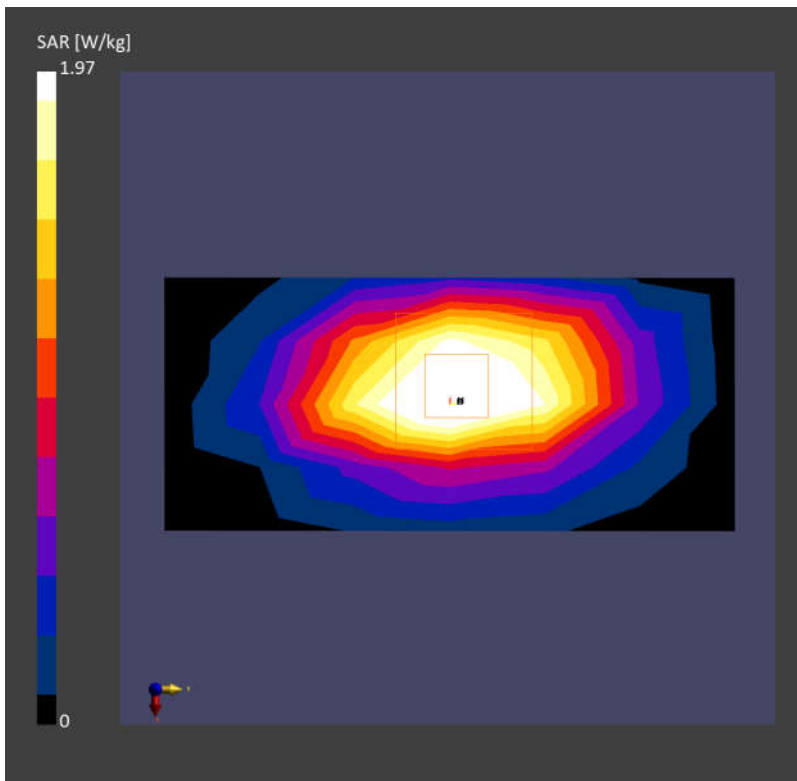

## System Check\_Head\_1900MHz

**DUT:D1900V2 - SN:5d118**

Communication System: ; Frequency: 1900.000

Medium: HSL. Medium parameters used:  $f= 1900.000$  MHz;  $\sigma= 1.40$  S/m;  $\epsilon_r = 41.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.77, 8.97, 7.88); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.70 W/kg; SAR (10g) = 0.900 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.07 dB

SAR (1g) = 1.81 W/kg; SAR (10g) = 1.07 W/kg;

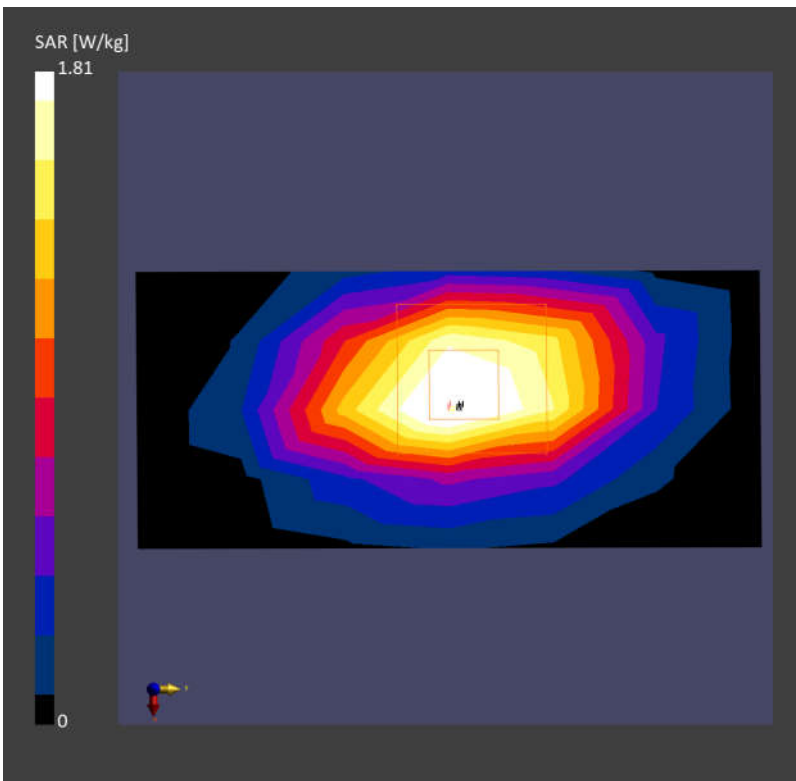

## System Check\_Head\_2300MHz

**DUT:D2300V2 - SN:1055**

Communication System: ; Frequency: 2300.000

Medium: HSL. Medium parameters used:  $f= 2300.000$  MHz;  $\sigma= 1.74$  S/m;  $\epsilon_r = 39.3$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.57, 8.73, 7.66); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.55 W/kg; SAR (10g) = 1.24 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 2.47 W/kg; SAR (10g) = 1.20 W/kg;

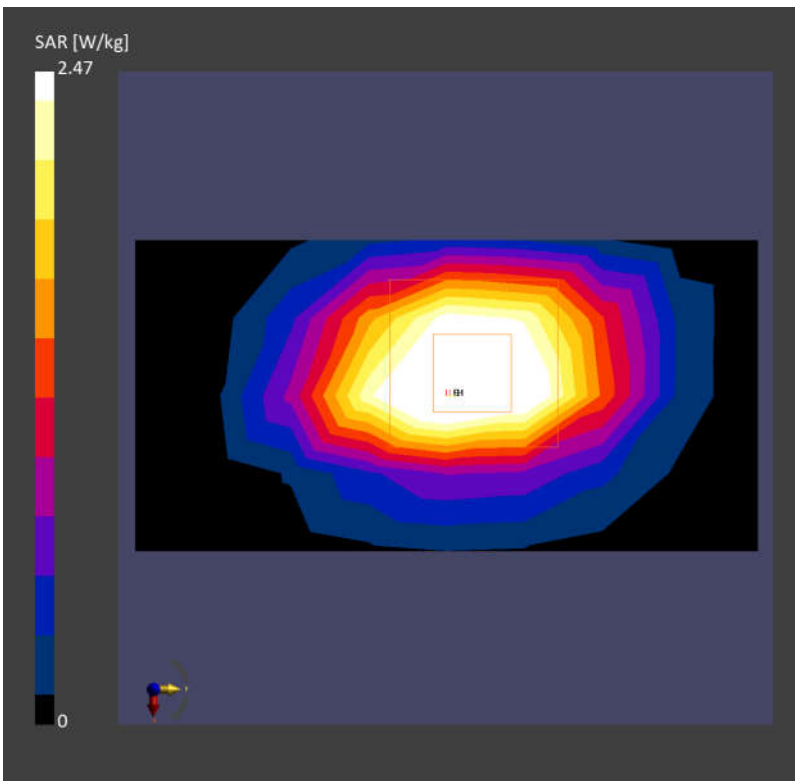

## System Check\_Head\_2450MHz

**DUT:D2450V2 - SN:1040**

Communication System: ; Frequency: 2450.000

Medium: HSL. Medium parameters used:  $f= 2450.000$  MHz;  $\sigma= 1.79$  S/m;  $\epsilon_r = 40.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.47, 8.61, 7.55); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.63 W/kg; SAR (10g) = 1.25 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 2.54 W/kg; SAR (10g) = 1.21 W/kg;

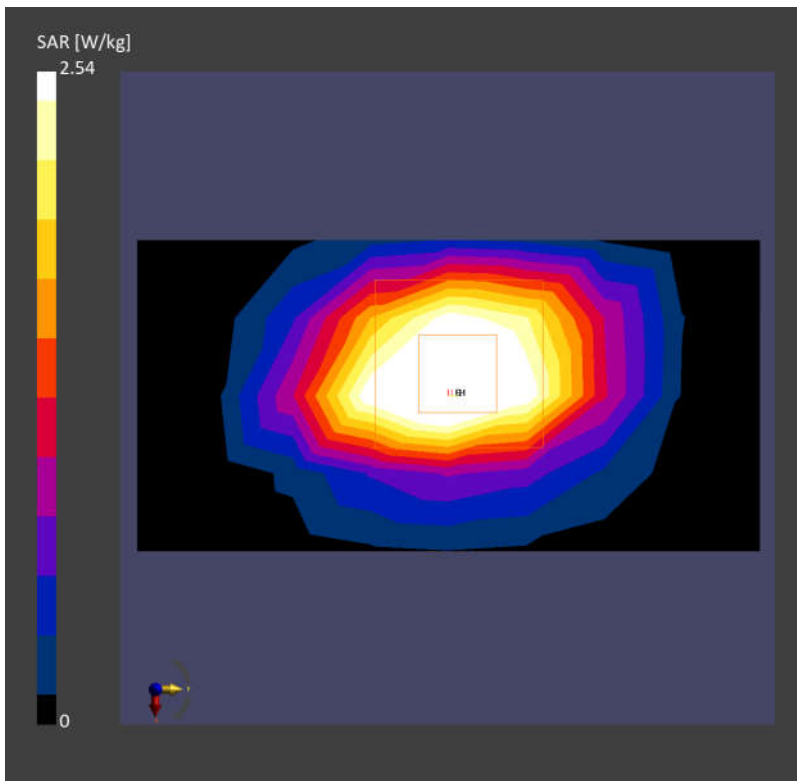



## System Check\_Head\_2600MHz

**DUT:D2600V2 - SN:1112**

Communication System: ; Frequency: 2600.000

Medium: HSL. Medium parameters used:  $f= 2600.000$  MHz;  $\sigma= 1.93$  S/m;  $\epsilon_r = 39.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.3, 8.44, 7.37); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.68 W/kg; SAR (10g) = 1.21 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.02 dB

SAR (1g) = 2.69 W/kg; SAR (10g) = 1.19 W/kg;

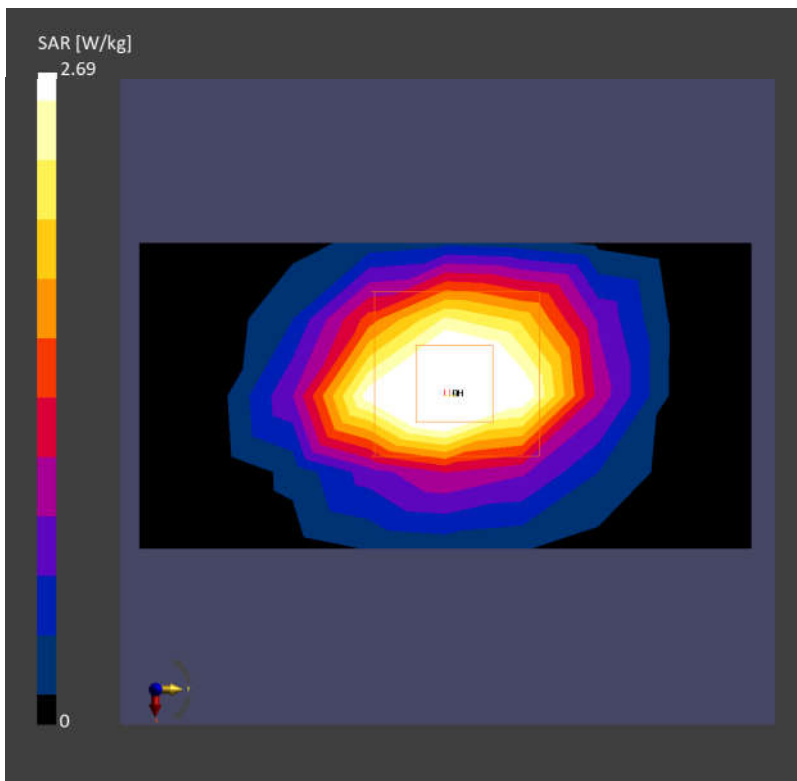

## System Check\_Head\_3500MHz

**DUT:D3500V2 - SN:1037**

Communication System: ; Frequency: 3500.000

Medium: HSL. Medium parameters used:  $f= 3500.000$  MHz;  $\sigma= 2.85$  S/m;  $\epsilon_r = 38.6$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.99, 8.16, 7.09); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.10 W/kg; SAR (10g) = 1.21 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.16 W/kg; SAR (10g) = 1.18 W/kg;

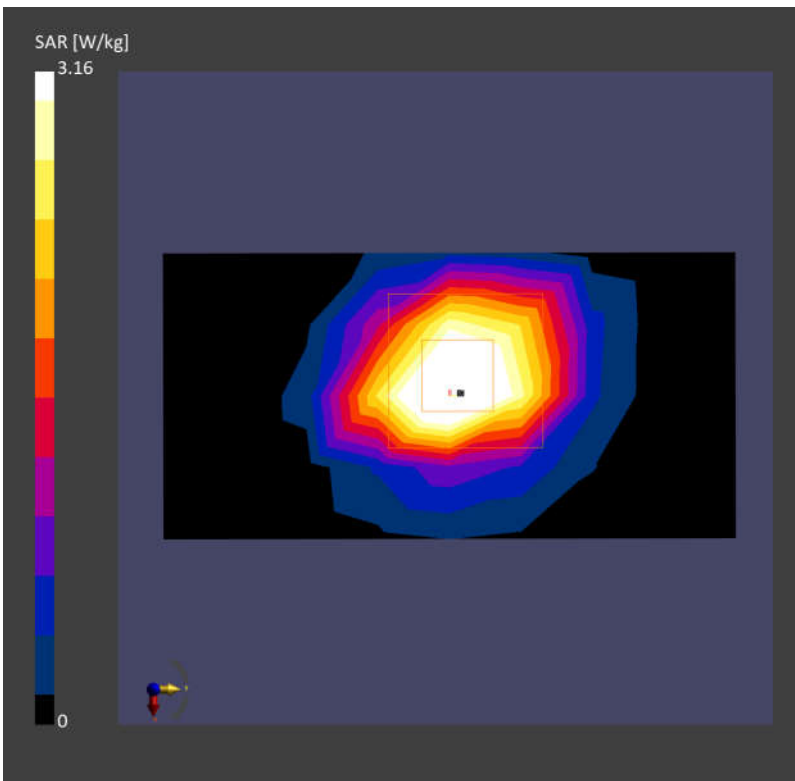

## System Check\_Head\_3700MHz

**DUT:D3700V2 - SN:1008**

Communication System: ; Frequency: 3700.000

Medium: HSL. Medium parameters used:  $f= 3700.000$  MHz;  $\sigma= 2.98$  S/m;  $\epsilon_r = 38.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.89, 8.06, 7.01); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.18 W/kg; SAR (10g) = 1.19 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.01 dB

SAR (1g) = 3.24 W/kg; SAR (10g) = 1.22 W/kg;

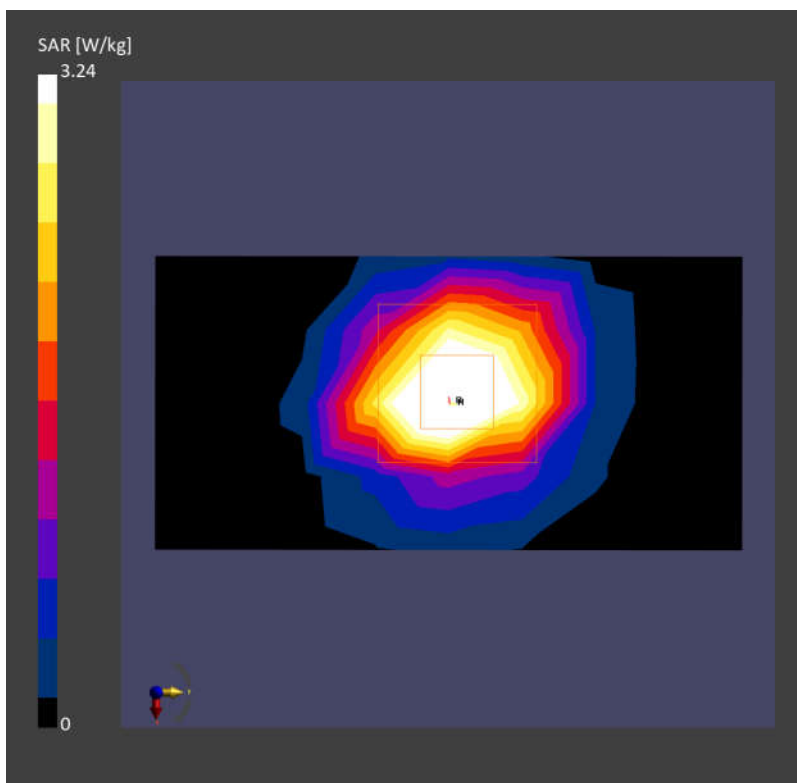

## System Check\_Head\_3900MHz

**DUT:D3900V2 - SN:1048**

Communication System: ; Frequency: 3900.000

Medium: HSL. Medium parameters used:  $f= 3900.000$  MHz;  $\sigma= 3.18$  S/m;  $\epsilon_r = 38.3$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(6.83, 7.98, 6.94); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.24 W/kg; SAR (10g) = 1.18 W/kg;

**Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.06 dB

SAR (1g) = 3.26 W/kg; SAR (10g) = 1.19 W/kg;

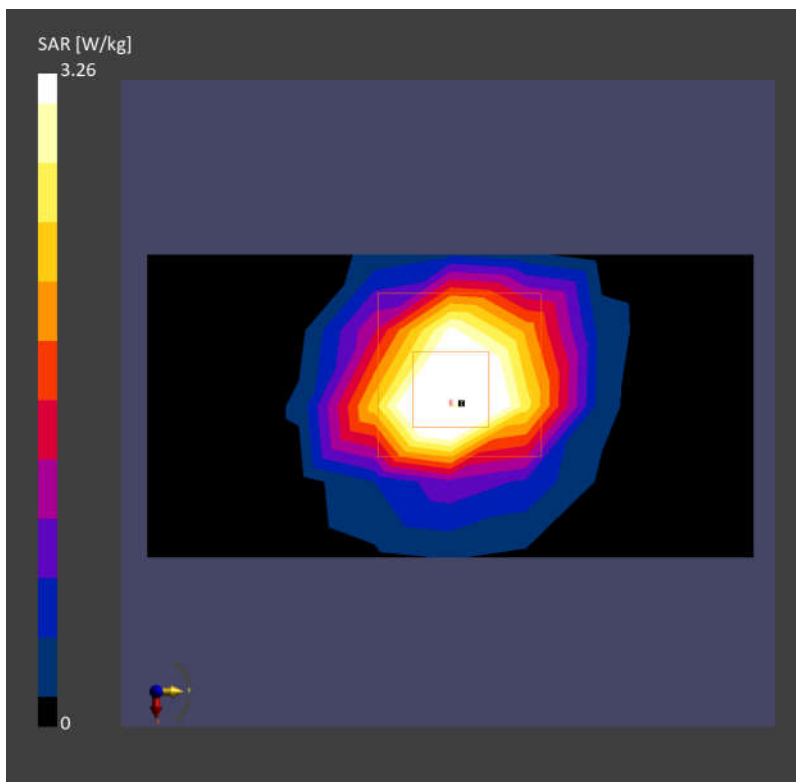

## System Check\_Head\_5250MHz

### DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5250.000

Medium: HSL. Medium parameters used:  $f= 5250.000$  MHz;  $\sigma= 4.57$  S/m;  $\epsilon_r = 35.5$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.84, 6.82, 5.88); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.37 W/kg; SAR (10g) = 1.06 W/kg;

**Zoom Scan (24.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.03 dB

SAR (1g) = 3.81 W/kg; SAR (10g) = 1.21 W/kg;

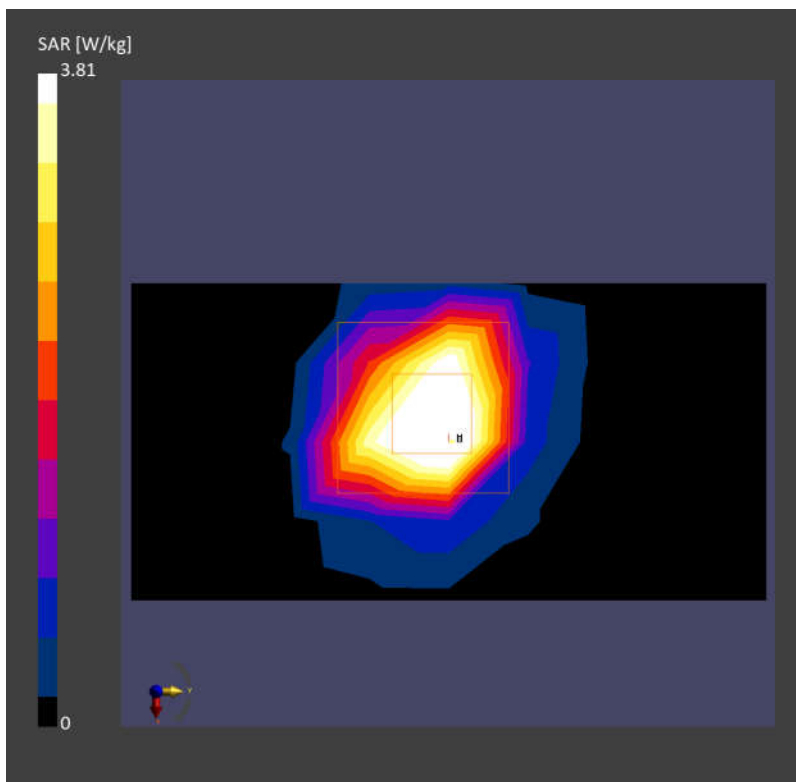

## System Check\_Head\_5600MHz

**DUT:D5GHzV2 - SN:1113**

Communication System: ; Frequency: 5600.000

Medium: HSL. Medium parameters used:  $f= 5600.000$  MHz;  $\sigma= 4.95$  S/m;  $\epsilon_r = 34.8$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(4.83, 5.71, 4.9); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.90 W/kg; SAR (10g) = 1.16 W/kg;

**Zoom Scan (24.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 4.05 W/kg; SAR (10g) = 1.11 W/kg;

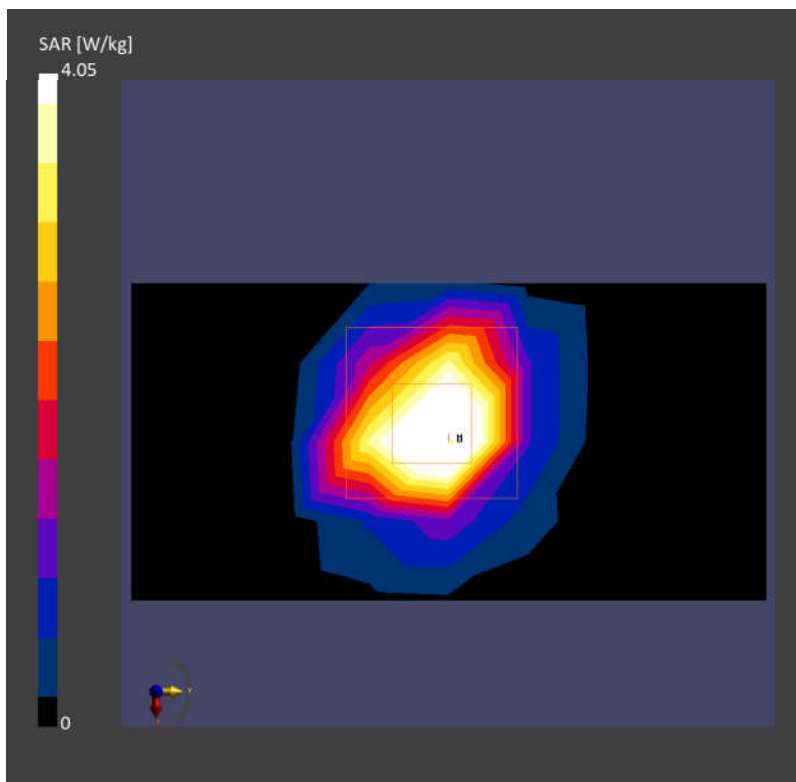

## System Check\_Head\_5750MHz

**DUT:D5GHzV2 - SN:1113**

Communication System: ; Frequency: 5750.000

Medium: HSL. Medium parameters used:  $f= 5750.000$  MHz;  $\sigma= 5.13$  S/m;  $\epsilon_r = 34.6$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(5.03, 5.88, 5.16); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.49 W/kg; SAR (10g) = 1.04 W/kg;

**Zoom Scan (24.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.82 W/kg; SAR (10g) = 1.15 W/kg;

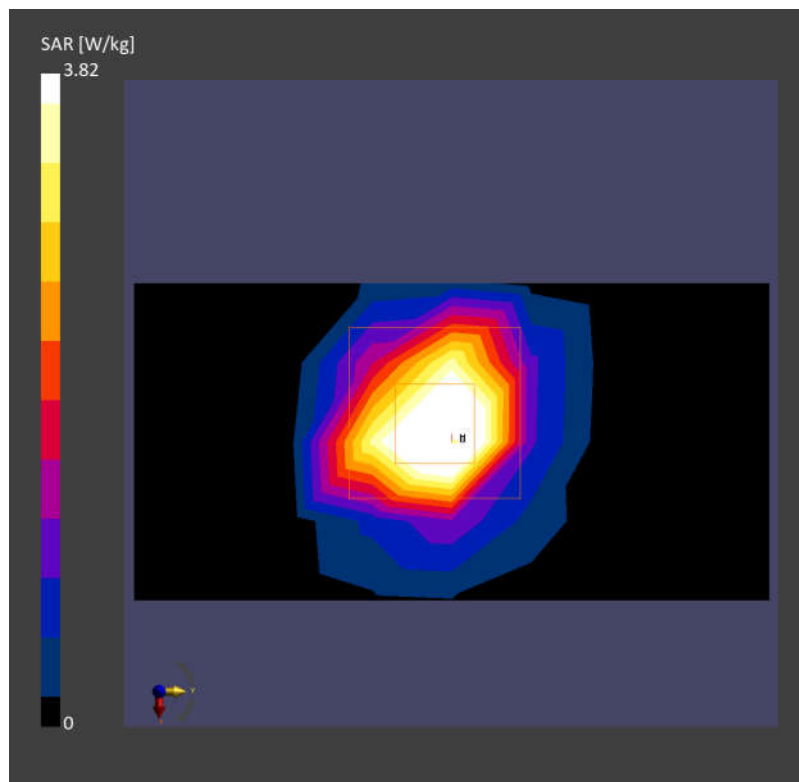

## System Check\_Head\_750MHz

**DUT:D750V3 - SN:1087**

Communication System: ; Frequency: 750.0

Medium: HSL. Medium parameters used:  $f= 750.0$  MHz;  $\sigma= 0.883$  S/m;  $\epsilon_r = 41.4$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(10.19, 10.19, 10.19); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.392 W/kg; SAR (10g) = 0.264 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.01 dB

SAR (1g) = 0.398 W/kg; SAR (10g) = 0.261 W/kg;

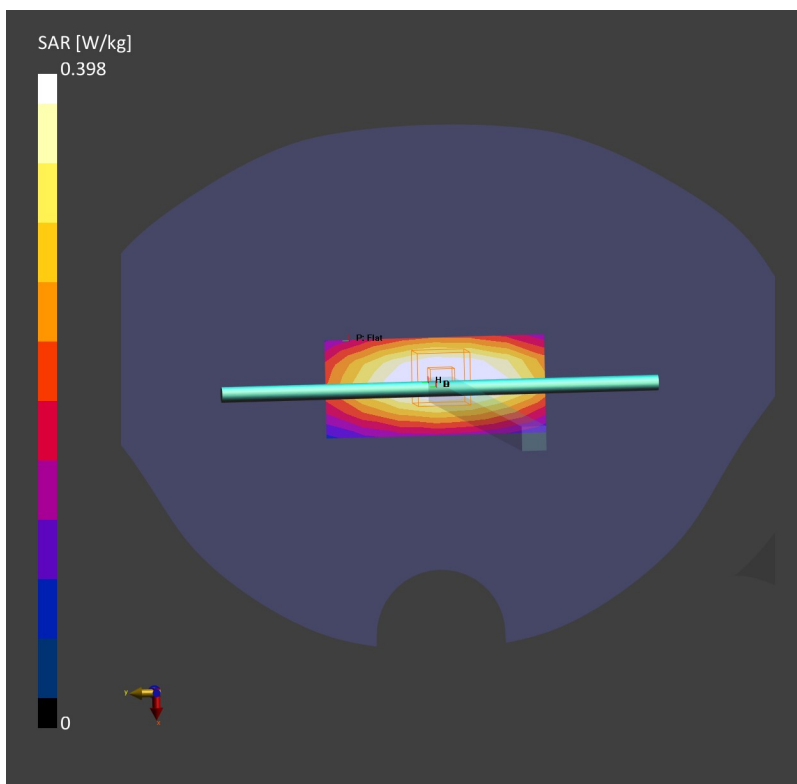



## System Check\_Head\_835MHz

**DUT:D835V2 - SN:4d091**

Communication System: ; Frequency: 835.000

Medium: HSL. Medium parameters used:  $f= 835.000$  MHz;  $\sigma= 0.912$  S/m;  $\epsilon_r = 41.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(9.78, 9.78, 9.78); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 0.501 W/kg; SAR (10g) = 0.316 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 0.502 W/kg; SAR (10g) = 0.329 W/kg;

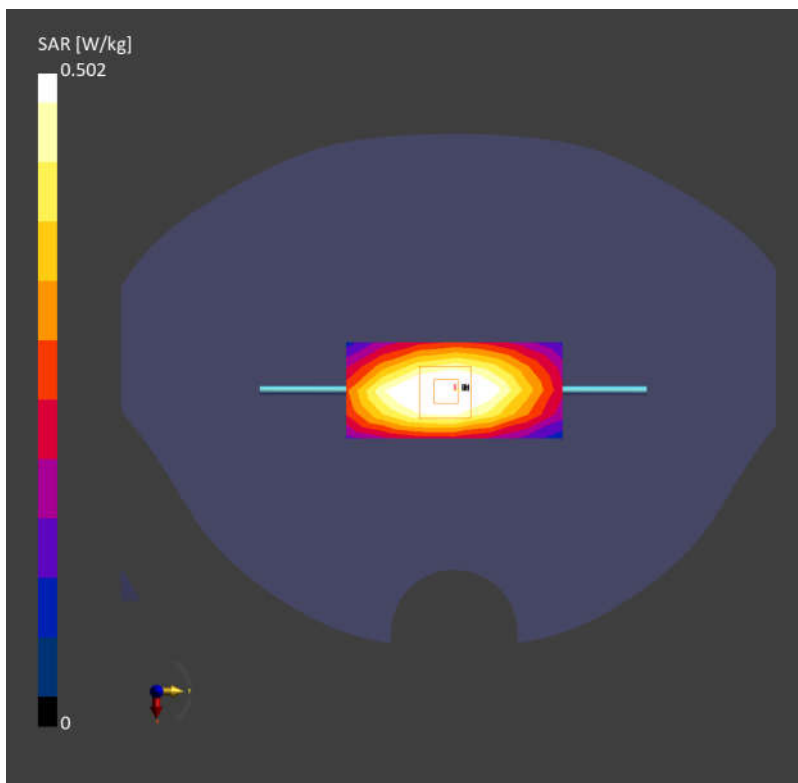

## System Check\_Head\_1750MHz

**DUT:D1750V2 - SN:1090**

Communication System: ; Frequency: 1750.000

Medium: HSL. Medium parameters used:  $f= 1750.000$  MHz;  $\sigma= 1.32$  S/m;  $\epsilon_r = 40.3$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.78, 8.78, 8.78); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 1.91 W/kg; SAR (10g) = 1.03 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.01 dB

SAR (1g) = 1.93 W/kg; SAR (10g) = 1.05 W/kg;

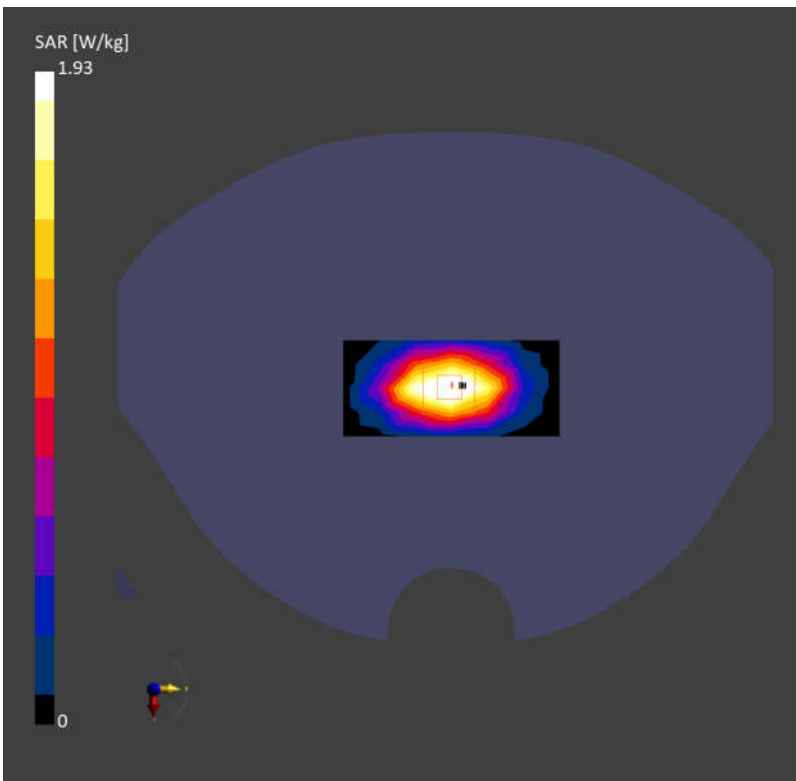

## System Check\_Head\_1900MHz

**DUT:D1900V2 - SN:5d118**

Communication System: ; Frequency: 1900.000

Medium: HSL. Medium parameters used:  $f= 1900.000$  MHz;  $\sigma= 1.41$  S/m;  $\epsilon_r = 40.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.46, 8.46, 8.46); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 2.09 W/kg; SAR (10g) = 1.08 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.08 W/kg; SAR (10g) = 1.10 W/kg;

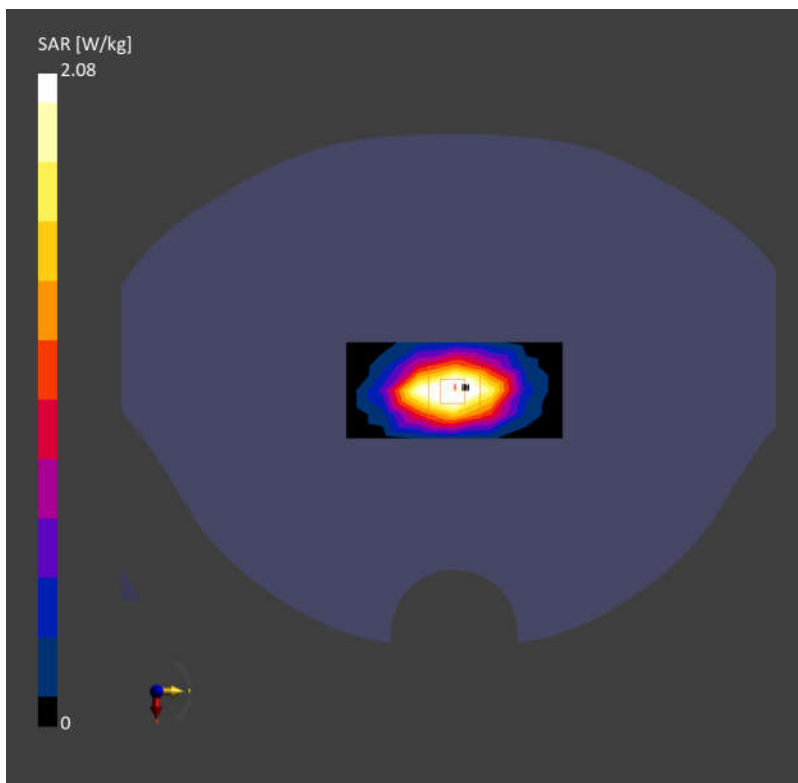

## System Check\_Head\_2300MHz

**DUT:D2300V2 - SN:1055**

Communication System: ; Frequency: 2300.000

Medium: HSL. Medium parameters used:  $f= 2300.000$  MHz;  $\sigma= 1.72$  S/m;  $\epsilon_r = 37.8$

Ambient Temperature: 23.1°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.18, 8.18, 8.18); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.31 W/kg; SAR (10g) = 1.11 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.31 W/kg; SAR (10g) = 1.11 W/kg;

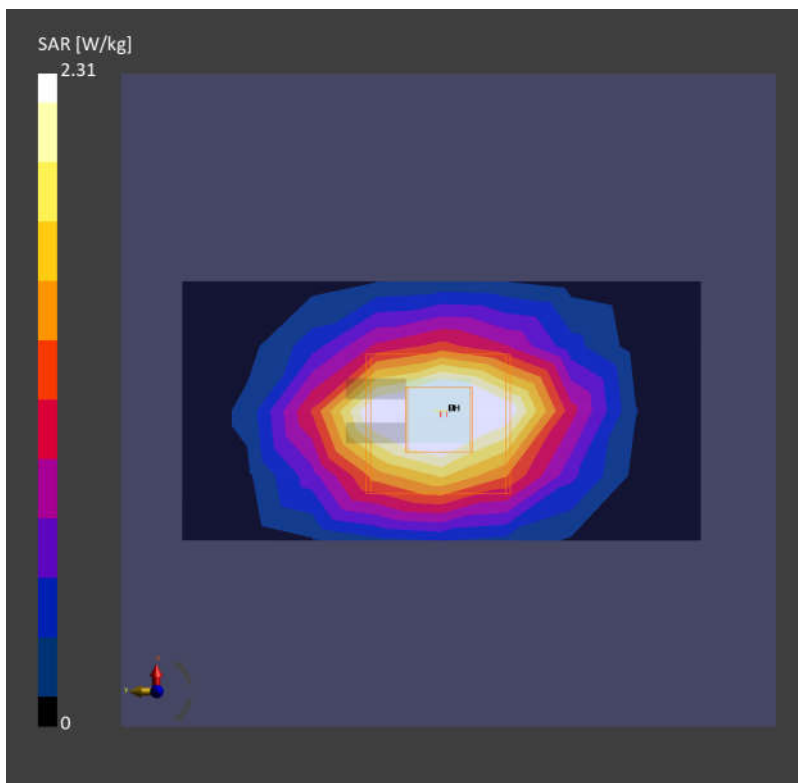

## System Check\_Head\_2450MHz

### DUT:D2450V2 - SN:1040

Communication System: ; Frequency: 2450.000

Medium: HSL. Medium parameters used:  $f= 2450.000$  MHz;  $\sigma= 1.86$  S/m;  $\epsilon_r = 38.6$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

### DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.03, 8.03, 8.03); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.61 W/kg; SAR (10g) = 1.21 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.55 W/kg; SAR (10g) = 1.19 W/kg;

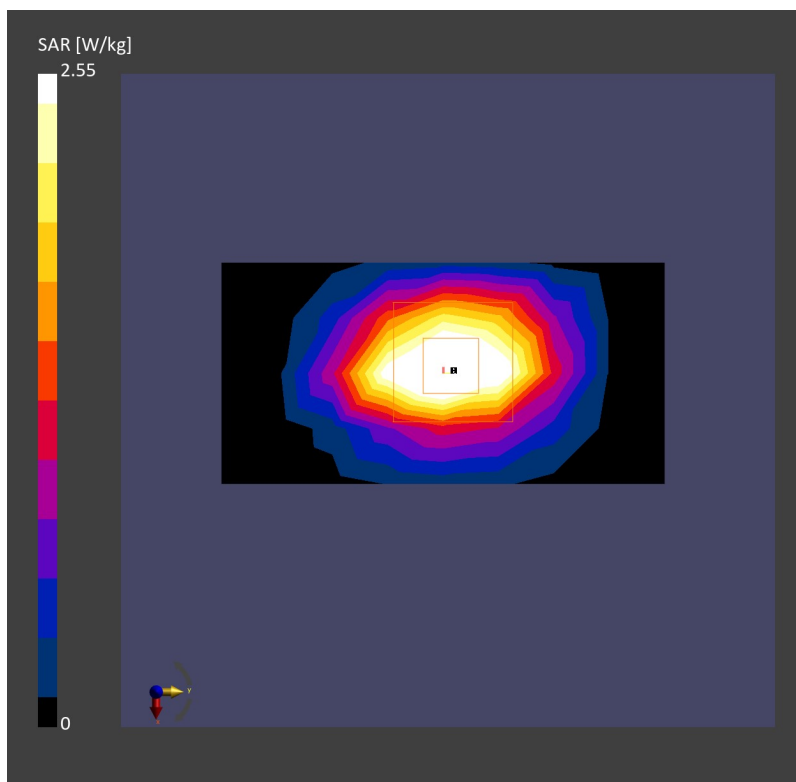

## System Check\_Head\_2600MHz

**DUT:D2600V2 - SN:1112**

Communication System: ; Frequency: 2600.000

Medium: HSL. Medium parameters used:  $f= 2600.000$  MHz;  $\sigma= 1.88$  S/m;  $\epsilon_r = 39.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(8.02, 8.02, 8.02); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 12.0 mm

SAR (1g) = 2.55 W/kg; SAR (10g) = 1.14 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.68 W/kg; SAR (10g) = 1.22 W/kg;

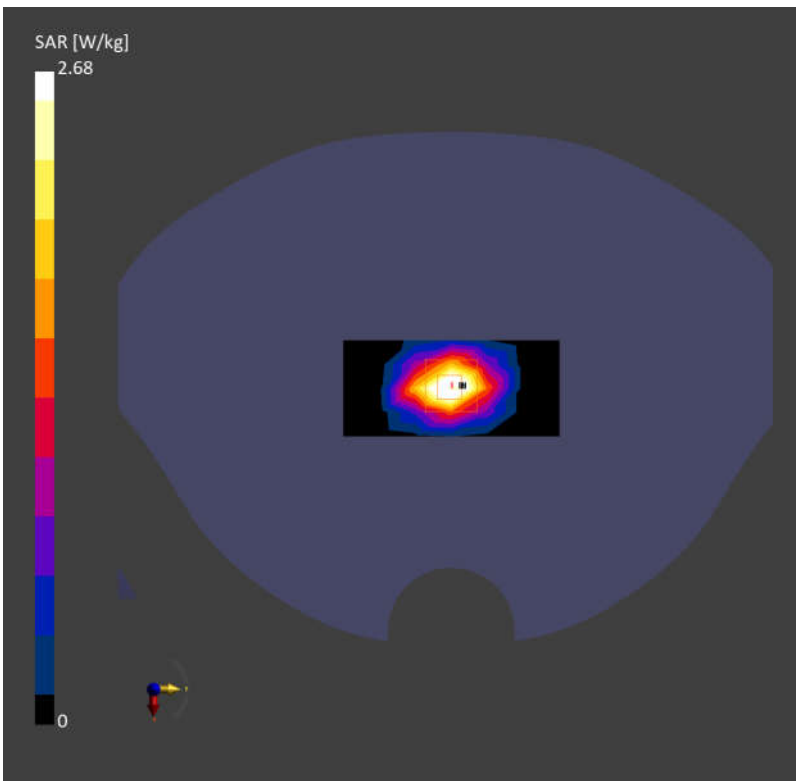

## System Check\_Head\_3500MHz

**DUT:D3500V2 - SN:1037**

Communication System: ; Frequency: 3500.000

Medium: HSL. Medium parameters used:  $f= 3500.000$  MHz;  $\sigma= 2.81$  S/m;  $\epsilon_r = 38.7$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.11, 7.11, 7.11); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.34 W/kg; SAR (10g) = 1.27 W/kg;

**Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.39 W/kg; SAR (10g) = 1.33 W/kg;

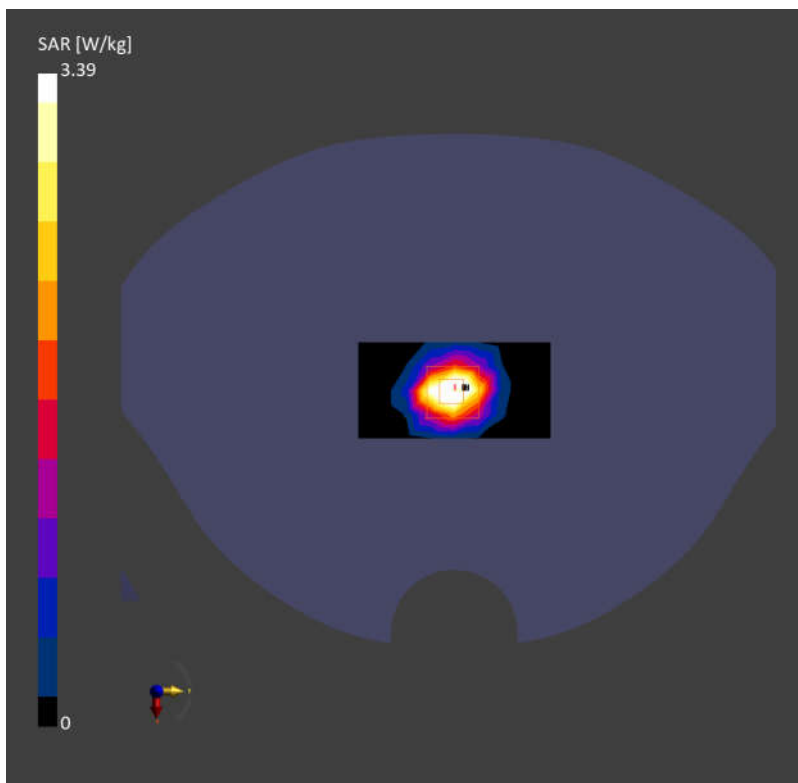

## System Check\_Head\_3700MHz

**DUT:D3700V2 - SN:1008**

Communication System: ; Frequency: 3700.000

Medium: HSL. Medium parameters used:  $f= 3700.000$  MHz;  $\sigma= 2.99$  S/m;  $\epsilon_r = 38.4$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(7.1, 7.1, 7.1); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.25 W/kg; SAR (10g) = 1.21 W/kg;

**Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.00 dB

SAR (1g) = 3.34 W/kg; SAR (10g) = 1.28 W/kg;

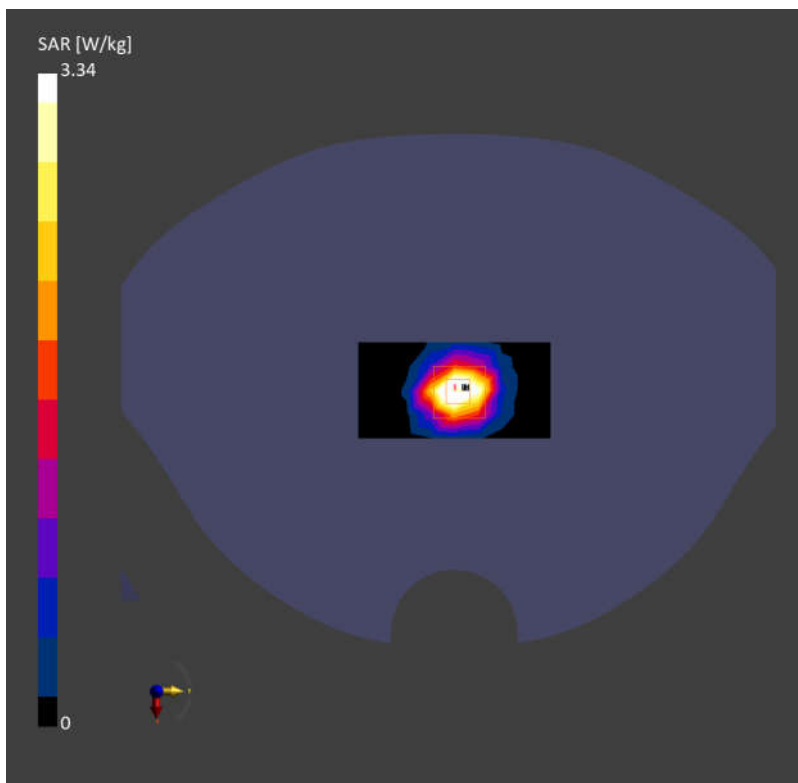



## System Check\_Head\_3900MHz

**DUT:D3900V2 - SN:1048**

Communication System: ; Frequency: 3900.000

Medium: HSL. Medium parameters used:  $f= 3900.000$  MHz;  $\sigma= 3.18$  S/m;  $\epsilon_r = 38.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(6.74, 6.74, 6.74); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.34 W/kg; SAR (10g) = 1.19 W/kg;

**Zoom Scan (24.0 mm x 24.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = -0.02 dB

SAR (1g) = 3.51 W/kg; SAR (10g) = 1.29 W/kg;

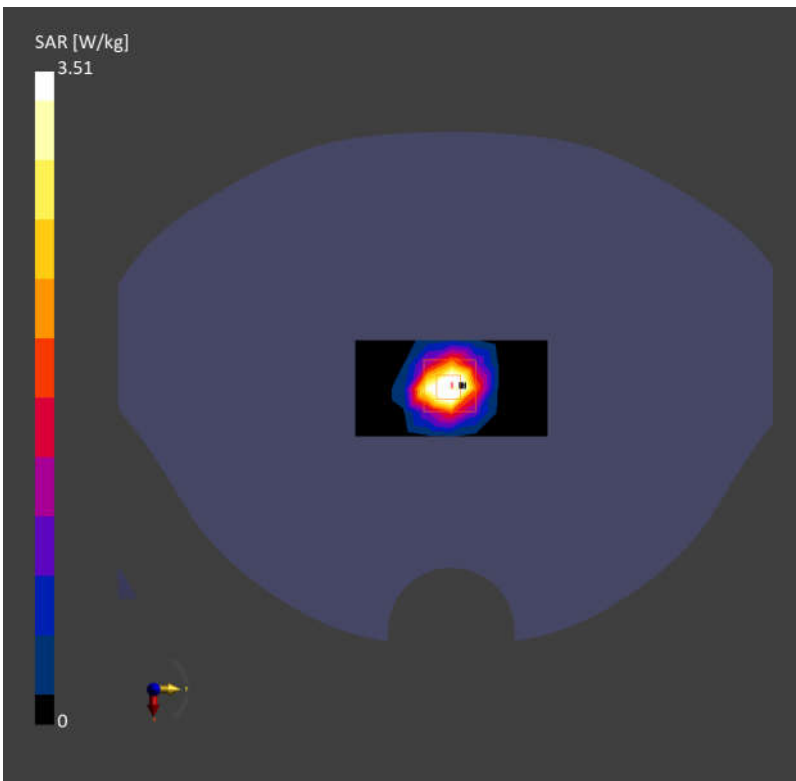

## System Check\_Head\_5250MHz

### DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5250.000

Medium: HSL. Medium parameters used:  $f= 5250.000$  MHz;  $\sigma= 4.59$  S/m;  $\epsilon_r = 35.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.73, 5.73, 5.73); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.30 W/kg; SAR (10g) = 0.977 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.02 dB

SAR (1g) = 3.87 W/kg; SAR (10g) = 1.09 W/kg;

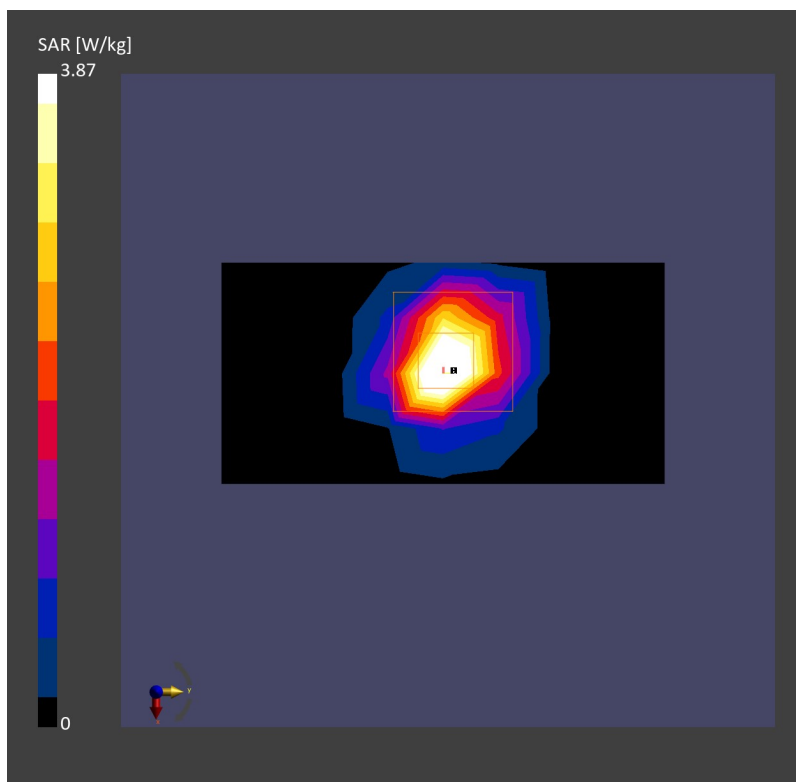

## System Check\_Head\_5600MHz

### DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5600.000

Medium: HSL. Medium parameters used:  $f= 5600.000$  MHz;  $\sigma= 5.05$  S/m;  $\epsilon_r = 35.0$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.10, 5.10, 5.10); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.64 W/kg; SAR (10g) = 1.06 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.88 W/kg; SAR (10g) = 1.11 W/kg;

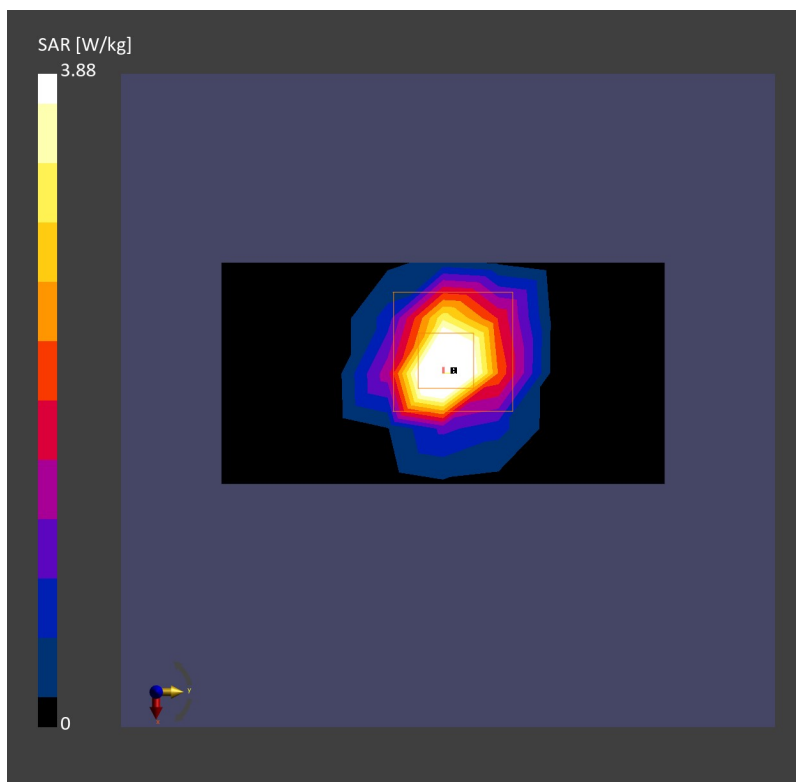

## System Check\_Head\_5750MHz

### DUT:D5GHzV2 - SN:1113

Communication System: ; Frequency: 5750.000

Medium: HSL. Medium parameters used:  $f= 5750.000$  MHz;  $\sigma= 5.15$  S/m;  $\epsilon_r = 34.7$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.8°C

#### DASY6 Configuration:

- Probe: EX3DV4 - SN7764; ConvF(5.32, 5.32, 5.32); Calibrated: 2023-10-05
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn690; Calibrated: 2023-06-20
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2022
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 3.27 W/kg; SAR (10g) = 0.960 W/kg;

**Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm):** Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm

Power Drift = 0.01 dB

SAR (1g) = 3.79 W/kg; SAR (10g) = 1.08 W/kg;

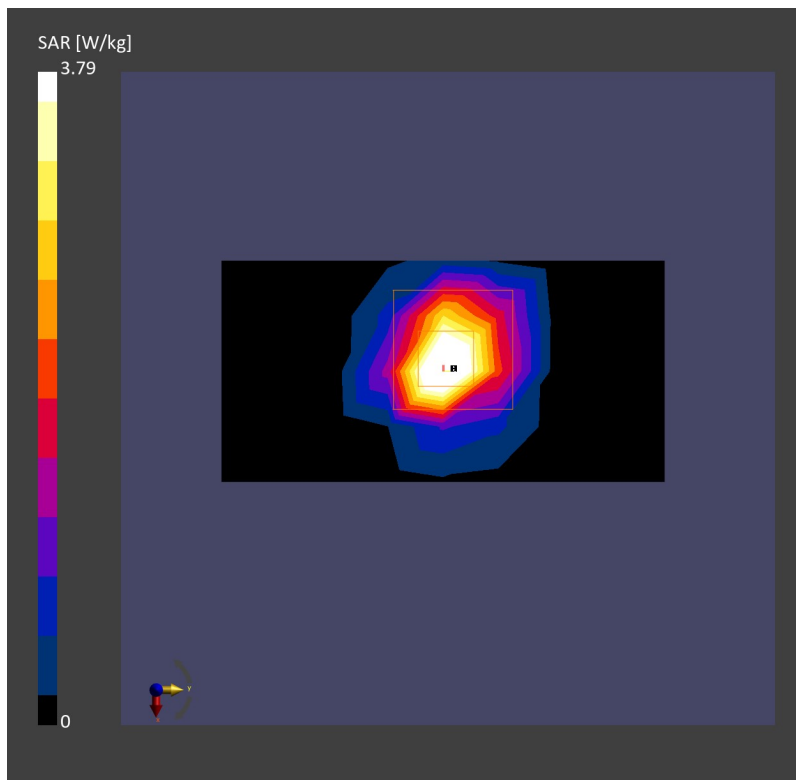

## System Check\_Head\_750MHz

**DUT: D750V3 - SN:1087**

Communication System: ; Frequency: 750.000

Medium: HSL. Medium parameters used:  $f= 750.000$  MHz;  $\sigma= 0.900$  S/m;  $\epsilon_r = 41.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(10.17, 10.07, 10.45); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1303; Calibrated: 2023-11-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.446 W/kg; SAR (10g) = 0.296 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.02 dB

SAR (1g) = 0.444 W/kg; SAR (10g) = 0.297 W/kg;

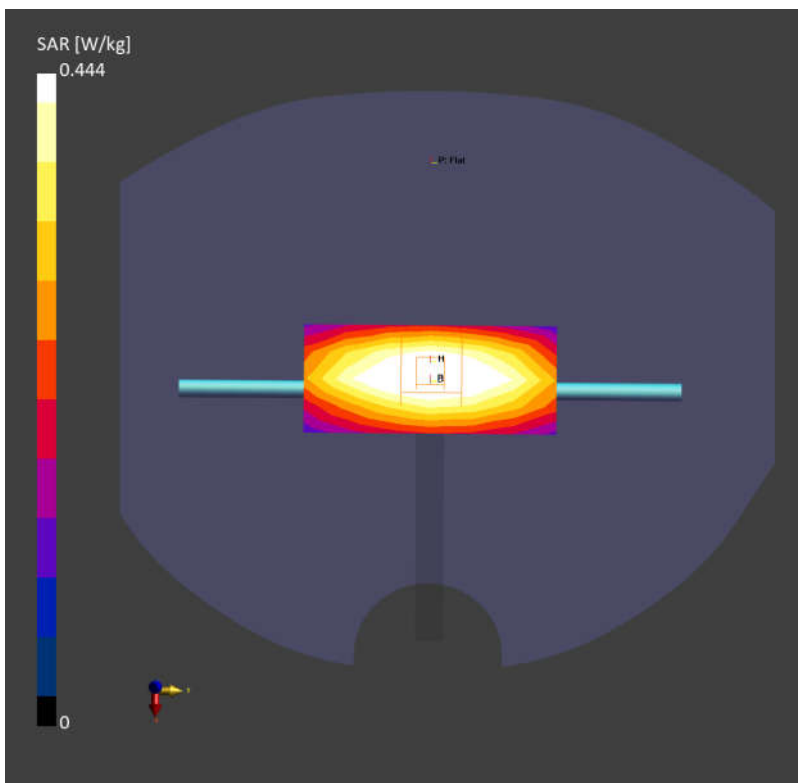

## System Check\_Head\_835MHz

**DUT: D835V2 - SN:4d091**

Communication System: ; Frequency: 835.000

Medium: HSL. Medium parameters used:  $f= 835.000$  MHz;  $\sigma= 0.902$  S/m;  $\epsilon_r = 41.2$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.8°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(10.13, 10.02, 10.22); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1303; Calibrated: 2023-11-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 0.488 W/kg; SAR (10g) = 0.320 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.03 dB

SAR (1g) = 0.486 W/kg; SAR (10g) = 0.322 W/kg;

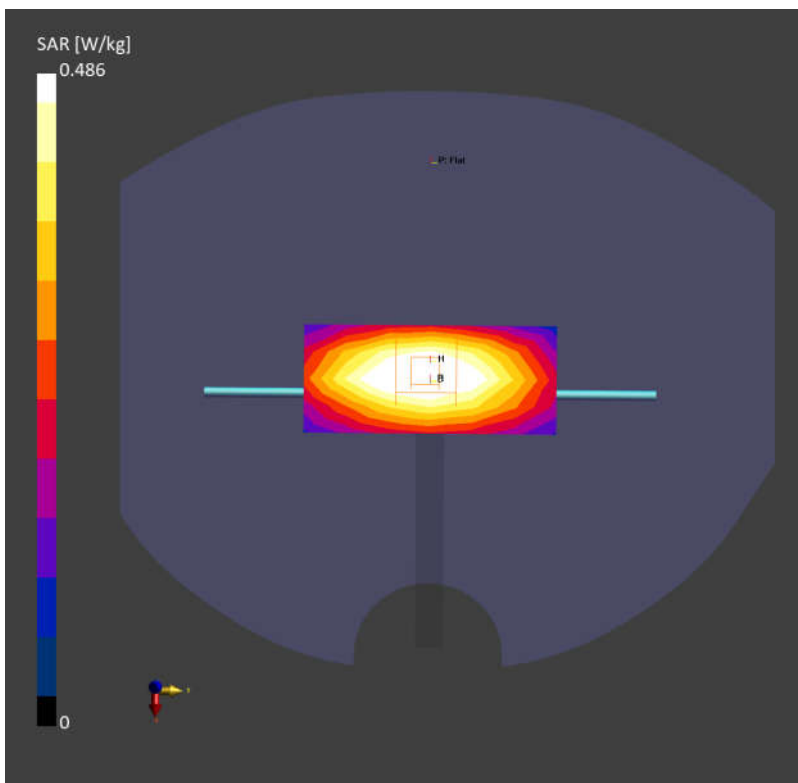

## System Check\_Head\_1750MHz

**DUT: D1750V2 - SN:1090**

Communication System: ; Frequency: 1750.0

Medium: HSL. Medium parameters used:  $f= 1750.0$  MHz;  $\sigma= 1.40$  S/m;  $\epsilon_r = 40.7$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(8.79, 8.61, 8.89); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1303; Calibrated: 2023-11-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 1.89 W/kg; SAR (10g) = 1.03 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = -0.03 dB

SAR (1g) = 1.89 W/kg; SAR (10g) = 0.993 W/kg;

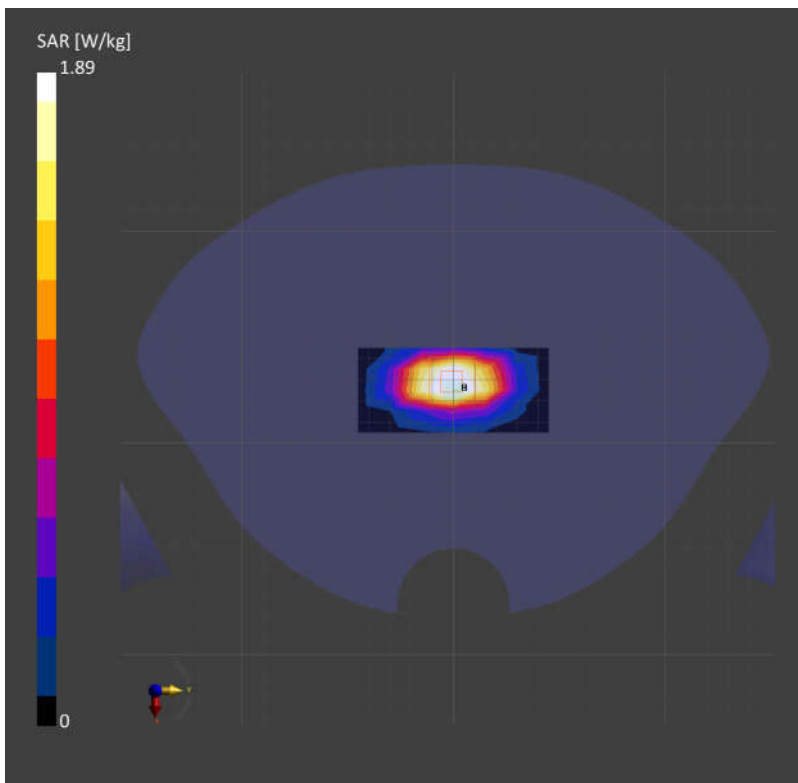

## System Check\_Head\_1900MHz

**DUT: D1900V2 - SN:5d118**

Communication System: ; Frequency: 1900.000

Medium: HSL. Medium parameters used:  $f= 1900.000$  MHz;  $\sigma= 1.40$  S/m;  $\epsilon_r = 39.0$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(8.41, 8.15, 8.28); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1303; Calibrated: 2023-11-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 15.0 mm x 15.0 mm

SAR (1g) = 2.06 W/kg; SAR (10g) = 1.06 W/kg;

**Zoom Scan (32.0 mm x 32.0 mm x 30.0 mm):** Measurement Grid: 8.0 mm x 8.0 mm x 5.0 mm

Power Drift = 0.05 dB

SAR (1g) = 2.07 W/kg; SAR (10g) = 1.08 W/kg;

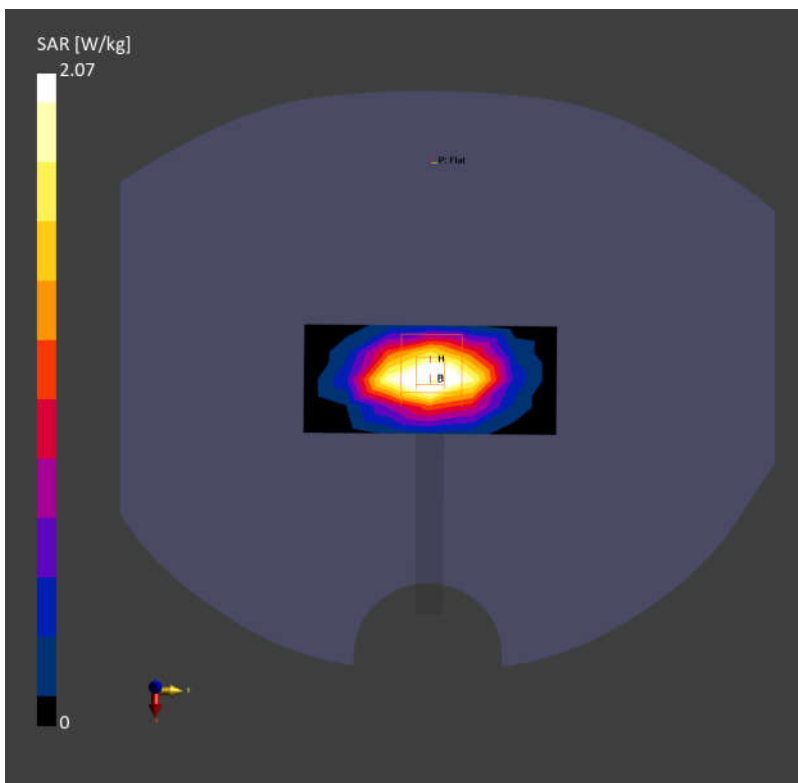



## System Check\_Head\_2600MHz

**DUT: D2600V2 - SN:1112**

Communication System: ; Frequency: 2600.000

Medium: HSL. Medium parameters used:  $f= 2600.000$  MHz;  $\sigma= 1.93$  S/m;  $\epsilon_r = 38.2$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7627; ConvF(7.54, 7.41, 7.52); Calibrated: 2023-06-06
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1303; Calibrated: 2023-11-20
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1644
- Measurement Software: cDASY6 V6.6.0.13926


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 12.0 mm x 12.0 mm

SAR (1g) = 2.81 W/kg; SAR (10g) = 1.26 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 5.0 mm

Power Drift = -0.01 dB

SAR (1g) = 2.82 W/kg; SAR (10g) = 1.28 W/kg;

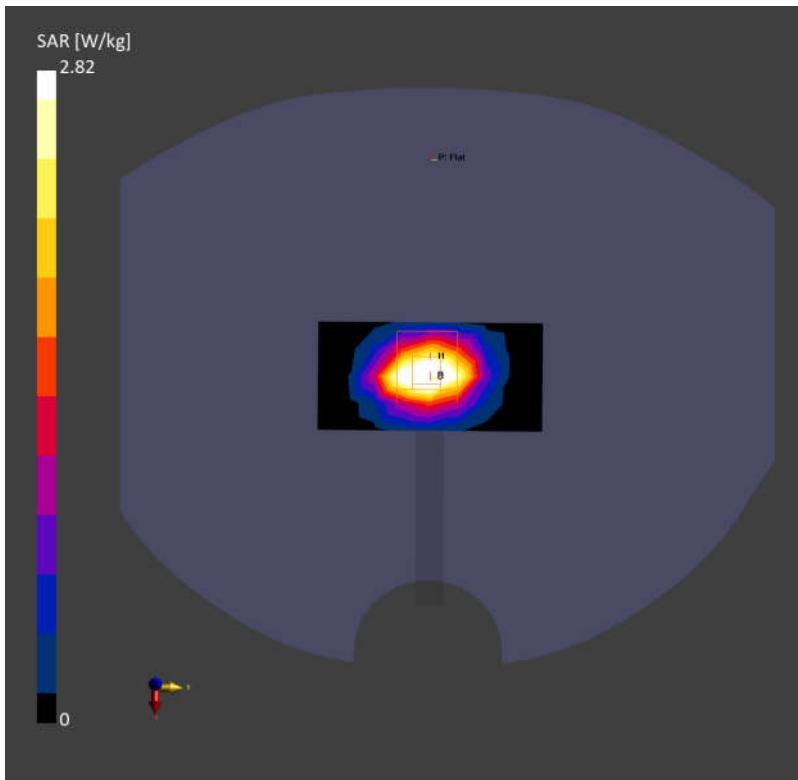

## System Check\_Head\_2450MHz

**DUT:D2450V2 - SN:1040**

Communication System: ; Frequency: 2450.000

Medium: HSL. Medium parameters used:  $f= 2450.000$  MHz;  $\sigma= 1.82$  S/m;  $\epsilon_r = 39.2$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.47, 8.61, 7.55); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448


**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.75 W/kg; SAR (10g) = 1.28 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = 0.09 dB

SAR (1g) = 2.70 W/kg; SAR (10g) = 1.29 W/kg;

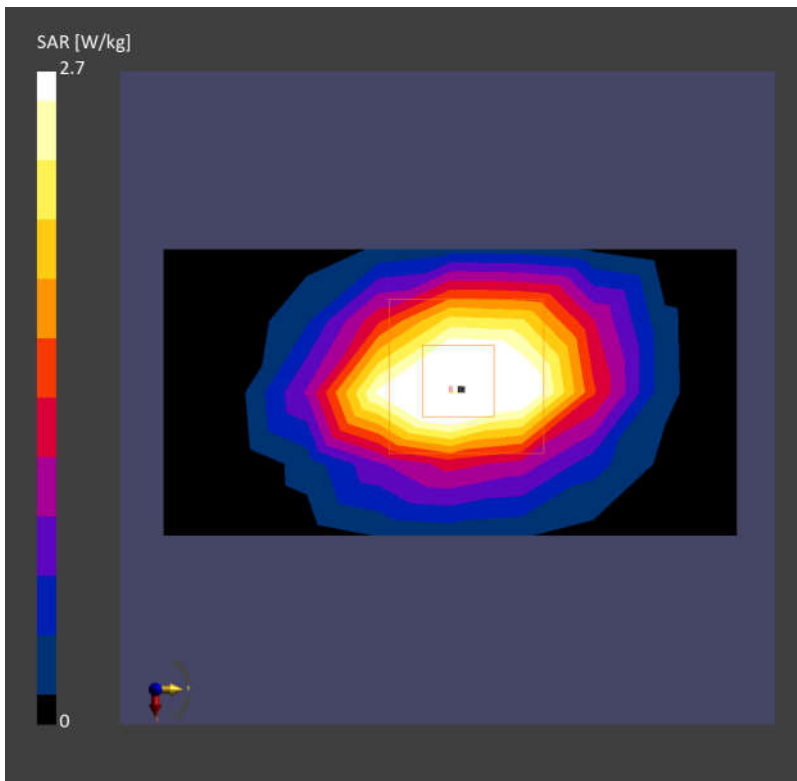

## System Check\_Head\_2600MHz

**DUT:D2600V2 - SN:1112**

Communication System: ; Frequency: 2600.000

Medium: HSL. Medium parameters used:  $f= 2600.000$  MHz;  $\sigma= 1.93$  S/m;  $\epsilon_r = 39.0$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.9°C

DASY6 Configuration:

- Probe: EX3DV4 - SN7706; ConvF(7.3, 8.44, 7.37); Calibrated: 2024-01-24
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1649; Calibrated: 2023-04-24
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2024
- Measurement Software: 16.2.4.2448

**Area Scan (40.0 mm x 80.0 mm):** Measurement Grid: 10.0 mm x 10.0 mm

SAR (1g) = 2.84 W/kg; SAR (10g) = 1.31 W/kg;

**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.75 W/kg; SAR (10g) = 1.27 W/kg;

